



**Off-Base Drinking Water Sample Results,  
Combined Level 2 and Level 4 Laboratory Report,  
Electronic Data Deliverable, Data Validation Report,  
and the Sample Location Figure, SDG 320-31468-1**

*Naval Air Warfare Center Warminster  
Warminster, Pennsylvania*

August 2019

N62269\_001142  
WARMINSTER\_NAWC  
SSIC 5000-33c

**LABORATORY DATA PACKAGE, 320-31468-1, NAS WILLOW GROVE NAWC**  
**WARMINSTER PA**  
09/22/2017  
TESTAMERICA LABORATORIES INC

Approved for public release: distribution unlimited.

## ANALYTICAL REPORT

Job Number: 320-31468-1

Job Description: Warminster: PFAS, NAS JRB Willow Grove

For:  
Tetra Tech, Inc.  
234 Mall Boulevard  
Suite 260  
King of Prussia, PA 19406  
Attention: Andy Frebowitz



Approved for release.  
David R Alltucker  
Project Manager I  
9/22/2017 2:47 PM

---

David R Alltucker, Project Manager I  
880 Riverside Parkway, West Sacramento, CA, 95605  
(916)374-4383  
david.alltucker@testamericainc.com  
09/22/2017

# Table of Contents

Cover Title Page . . . . .	1
Data Summaries . . . . .	4
Definitions . . . . .	4
Case Narrative . . . . .	5
Detection Summary . . . . .	6
Client Sample Results . . . . .	9
Default Detection Limits . . . . .	17
Surrogate Summary . . . . .	18
QC Sample Results . . . . .	19
QC Association . . . . .	21
Chronicle . . . . .	23
Certification Summary . . . . .	27
Method Summary . . . . .	28
Sample Summary . . . . .	29
Manual Integration Summary . . . . .	30
Reagent Traceability . . . . .	39
COAs . . . . .	50
Organic Sample Data . . . . .	99
LCMS . . . . .	99
Method 537 DOD . . . . .	99
Method 537 DOD QC Summary . . . . .	100
Method 537 DOD Sample Data . . . . .	118
Standards Data . . . . .	281
Method 537 DOD ICAL Data . . . . .	281
Method 537 DOD CCAL Data . . . . .	329
Raw QC Data . . . . .	403

# Table of Contents

Method 537 DOD Blank Data .....	403
Method 537 DOD LCS/LCSD Data .....	413
Method 537 DOD Run Logs .....	449
Method 537 DOD Prep Data .....	454
Shipping and Receiving Documents .....	473
Client Chain of Custody .....	474
Sample Receipt Checklist .....	476

# Definitions/Glossary

Client: Tetra Tech, Inc.  
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-31468-1

## Qualifiers

### LCMS

Qualifier	Qualifier Description
Q	One or more quality control criteria failed.
U	Undetected at the Limit of Detection.
J	Estimated: The analyte was positively identified; the quantitation is an estimation
M	Manual integrated compound.

## Glossary

Abbreviation	These commonly used abbreviations may or may not be present in this report.
α	Listed under the "D" column to designate that the result is reported on a dry weight basis
%R	Percent Recovery
CFL	Contains Free Liquid
CNF	Contains No Free Liquid
DER	Duplicate Error Ratio (normalized absolute difference)
Dil Fac	Dilution Factor
DL	Detection Limit (DoD/DOE)
DL, RA, RE, IN	Indicates a Dilution, Re-analysis, Re-extraction, or additional Initial metals/anion analysis of the sample
DLC	Decision Level Concentration (Radiochemistry)
EDL	Estimated Detection Limit (Dioxin)
LOD	Limit of Detection (DoD/DOE)
LOQ	Limit of Quantitation (DoD/DOE)
MDA	Minimum Detectable Activity (Radiochemistry)
MDC	Minimum Detectable Concentration (Radiochemistry)
MDL	Method Detection Limit
ML	Minimum Level (Dioxin)
NC	Not Calculated
ND	Not Detected at the reporting limit (or MDL or EDL if shown)
PQL	Practical Quantitation Limit
QC	Quality Control
RER	Relative Error Ratio (Radiochemistry)
RL	Reporting Limit or Requested Limit (Radiochemistry)
RPD	Relative Percent Difference, a measure of the relative difference between two points
TEF	Toxicity Equivalent Factor (Dioxin)
TEQ	Toxicity Equivalent Quotient (Dioxin)

**Job Narrative  
320-31468-1**

**Receipt**

The samples were received on 9/12/2017 2:21 PM; the samples arrived in good condition, properly preserved and, where required, on ice. The temperatures of the 2 coolers at receipt time were 1.5° C and 2.1° C.

**Receipt Exceptions**

The container label for the following samples did not match the information listed on the Chain-of-Custody (COC):  
NAWC-091117-RW-106 (320-31468-1), NAWC-091117-FRB-106 (320-31468-2), NAWC-091117-RW-060 (320-31468-3),  
NAWC-091117-FRB-060 (320-31468-4), NAWC-091117-RW-314 (320-31468-5), NAWC-091117-FRB-314 (320-31468-6),  
NAWC-091117-RW-258 (320-31468-7), NAWC-091117-FRB-258 (320-31468-8), NAWC-091117-RW-048 (320-31468-9),  
NAWC-091117-FRB-048 (320-31468-10), NAWC-091117-RW-145 (320-31468-11), NAWC-091117-FRB-145 (320-31468-12),  
NAWC-091117-RW-317 (320-31468-13), NAWC-091117-FRB-317 (320-31468-14), NAWC-091117-RW-319 (320-31468-15),  
NAWC-091117-FRB-319 (320-31468-16), NAWC-091117-RW-321 (320-31468-17), NAWC-091117-FRB-321 (320-31468-18),  
NAWC-091117-RW-010 (320-31468-19), NAWC-091117-FRB-010 (320-31468-20), NAWC-091117-RW-162 (320-31468-21),  
NAWC-091117-FRB-162 (320-31468-22) and WGNA-091117-DUP09 (320-31468-23). The container labels list WGNA-, while the COC lists NAWC-. The samples were logged in according to the CoC.

**LCMS**

Method(s) 537: The first level standard from the initial calibration curve is used to evaluate the tune criteria. The instrument mass windows are set at +/- 0.5amu; therefore, detection of the analyte serves as verification that the assigned mass is within +/- 0.5amu of the true value, which meets the DoD/DOE QSM tune criterion.

Method(s) 537: Surrogate recovery for the following samples was outside control limits: NAWC-091117-RW-106 (320-31468-1), NAWC-091117-RW-319 (320-31468-15) and (MB 320-184385/1-A). Re-analysis was performed with concurring results. The original analysis has been reported.

No additional analytical or quality issues were noted, other than those described above or in the Definitions/Glossary page.

**Organic Prep**

Method(s) 537: Insufficient sample volume was available to perform a matrix spike/matrix spike duplicate (MS/MSD) associated with preparation batch 320-184382.

Method(s) 537: Insufficient sample volume was available to perform a matrix spike/matrix spike duplicate (MS/MSD) associated with preparation batch 320-184385.

Method(s) 537: The following samples: NAWC-091117-RW-106 (320-31468-1) and NAWC-091117-RW-319 (320-31468-15) were decanted prior to preparation due to particulates in the sample.

No additional analytical or quality issues were noted, other than those described above or in the Definitions/Glossary page.

# Detection Summary

Client: Tetra Tech, Inc.  
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-31468-1

## Client Sample ID: NAWC-091117-RW-106

Lab Sample ID: 320-31468-1

Analyte	Result	Qualifier	LOQ	DL	Unit	Dil Fac	D	Method	Prep Type
Perfluorooctanesulfonic acid (PFOS)	17	J M	40	6.7	ng/L	1		537	Total/NA
Perfluorooctanoic acid (PFOA)	20		20	2.8	ng/L	1		537	Total/NA
Perfluorohexanesulfonic acid (PFHxS)	8.9	J	30	5.4	ng/L	1		537	Total/NA
Perfluoroheptanoic acid (PFHpA)	8.1	J	9.9	1.9	ng/L	1		537	Total/NA

## Client Sample ID: NAWC-091117-FRB-106

Lab Sample ID: 320-31468-2

No Detections.

## Client Sample ID: NAWC-091117-RW-060

Lab Sample ID: 320-31468-3

Analyte	Result	Qualifier	LOQ	DL	Unit	Dil Fac	D	Method	Prep Type
Perfluorooctanesulfonic acid (PFOS)	27	J M	38	6.5	ng/L	1		537	Total/NA
Perfluorooctanoic acid (PFOA)	17	J	19	2.7	ng/L	1		537	Total/NA
Perfluorohexanesulfonic acid (PFHxS)	9.9	J	29	5.3	ng/L	1		537	Total/NA
Perfluoroheptanoic acid (PFHpA)	3.9	J	9.6	1.8	ng/L	1		537	Total/NA

## Client Sample ID: NAWC-091117-FRB-060

Lab Sample ID: 320-31468-4

No Detections.

## Client Sample ID: NAWC-091117-RW-314

Lab Sample ID: 320-31468-5

Analyte	Result	Qualifier	LOQ	DL	Unit	Dil Fac	D	Method	Prep Type
Perfluorooctanesulfonic acid (PFOS)	15	J M	38	6.5	ng/L	1		537	Total/NA
Perfluorooctanoic acid (PFOA)	17	J	19	2.7	ng/L	1		537	Total/NA
Perfluoroheptanoic acid (PFHpA)	4.4	J	9.5	1.8	ng/L	1		537	Total/NA

## Client Sample ID: NAWC-091117-FRB-314

Lab Sample ID: 320-31468-6

No Detections.

## Client Sample ID: NAWC-091117-RW-258

Lab Sample ID: 320-31468-7

Analyte	Result	Qualifier	LOQ	DL	Unit	Dil Fac	D	Method	Prep Type
Perfluorooctanesulfonic acid (PFOS)	18	J M	37	6.4	ng/L	1		537	Total/NA
Perfluorooctanoic acid (PFOA)	21		19	2.6	ng/L	1		537	Total/NA
Perfluorononanoic acid (PFNA)	12	J	22	7.5	ng/L	1		537	Total/NA
Perfluoroheptanoic acid (PFHpA)	7.7	J	9.4	1.8	ng/L	1		537	Total/NA

## Client Sample ID: NAWC-091117-FRB-258

Lab Sample ID: 320-31468-8

No Detections.

## Client Sample ID: NAWC-091117-RW-048

Lab Sample ID: 320-31468-9

Analyte	Result	Qualifier	LOQ	DL	Unit	Dil Fac	D	Method	Prep Type
Perfluorooctanoic acid (PFOA)	4.5	J M	19	2.7	ng/L	1		537	Total/NA

## Client Sample ID: NAWC-091117-FRB-048

Lab Sample ID: 320-31468-10

No Detections.

This Detection Summary does not include radiochemical test results.

TestAmerica Sacramento



# Detection Summary

Client: Tetra Tech, Inc.  
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-31468-1

## Client Sample ID: NAWC-091117-RW-145

Lab Sample ID: 320-31468-11

Analyte	Result	Qualifier	LOQ	DL	Unit	Dil Fac	D	Method	Prep Type
Perfluorooctanesulfonic acid (PFOS)	19	J M	37	6.3	ng/L	1		537	Total/NA
Perfluorooctanoic acid (PFOA)	20		19	2.6	ng/L	1		537	Total/NA
Perfluorohexanesulfonic acid (PFHxS)	7.3	J	28	5.1	ng/L	1		537	Total/NA
Perfluoroheptanoic acid (PFHpA)	5.6	J	9.3	1.8	ng/L	1		537	Total/NA

## Client Sample ID: NAWC-091117-FRB-145

Lab Sample ID: 320-31468-12

No Detections.

## Client Sample ID: NAWC-091117-RW-317

Lab Sample ID: 320-31468-13

Analyte	Result	Qualifier	LOQ	DL	Unit	Dil Fac	D	Method	Prep Type
Perfluorooctanesulfonic acid (PFOS)	49	M	38	6.4	ng/L	1		537	Total/NA
Perfluorooctanoic acid (PFOA)	21		19	2.7	ng/L	1		537	Total/NA
Perfluorohexanesulfonic acid (PFHxS)	34		28	5.2	ng/L	1		537	Total/NA
Perfluoroheptanoic acid (PFHpA)	8.1	J	9.5	1.8	ng/L	1		537	Total/NA

## Client Sample ID: NAWC-091117-FRB-317

Lab Sample ID: 320-31468-14

No Detections.

## Client Sample ID: NAWC-091117-RW-319

Lab Sample ID: 320-31468-15

Analyte	Result	Qualifier	LOQ	DL	Unit	Dil Fac	D	Method	Prep Type
Perfluorooctanesulfonic acid (PFOS)	43	M	40	6.8	ng/L	1		537	Total/NA
Perfluorooctanoic acid (PFOA)	44		20	2.8	ng/L	1		537	Total/NA
Perfluorononanoic acid (PFNA)	9.7	J	24	8.0	ng/L	1		537	Total/NA
Perfluorohexanesulfonic acid (PFHxS)	8.0	J	30	5.5	ng/L	1		537	Total/NA
Perfluoroheptanoic acid (PFHpA)	15	M	10	1.9	ng/L	1		537	Total/NA

## Client Sample ID: NAWC-091117-FRB-319

Lab Sample ID: 320-31468-16

No Detections.

## Client Sample ID: NAWC-091117-RW-321

Lab Sample ID: 320-31468-17

Analyte	Result	Qualifier	LOQ	DL	Unit	Dil Fac	D	Method	Prep Type
Perfluorooctanesulfonic acid (PFOS)	7.5	J M	38	6.5	ng/L	1		537	Total/NA
Perfluorooctanoic acid (PFOA)	6.9	J	19	2.7	ng/L	1		537	Total/NA
Perfluoroheptanoic acid (PFHpA)	1.8	J	9.5	1.8	ng/L	1		537	Total/NA

## Client Sample ID: NAWC-091117-FRB-321

Lab Sample ID: 320-31468-18

No Detections.

## Client Sample ID: NAWC-091117-RW-010

Lab Sample ID: 320-31468-19

Analyte	Result	Qualifier	LOQ	DL	Unit	Dil Fac	D	Method	Prep Type
Perfluorooctanesulfonic acid (PFOS)	30	J M	39	6.7	ng/L	1		537	Total/NA
Perfluorooctanoic acid (PFOA)	12	J	20	2.7	ng/L	1		537	Total/NA
Perfluorohexanesulfonic acid (PFHxS)	17	J	29	5.4	ng/L	1		537	Total/NA

This Detection Summary does not include radiochemical test results.

TestAmerica Sacramento

# Detection Summary

Client: Tetra Tech, Inc.  
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-31468-1

## Client Sample ID: NAWC-091117-RW-010 (Continued)

Lab Sample ID: 320-31468-19

Analyte	Result	Qualifier	LOQ	DL	Unit	Dil Fac	D	Method	Prep Type
Perfluoroheptanoic acid (PFHpA)	5.4	J	9.8	1.9	ng/L	1		537	Total/NA

## Client Sample ID: NAWC-091117-FRB-010

Lab Sample ID: 320-31468-20

No Detections.

## Client Sample ID: NAWC-091117-RW-162

Lab Sample ID: 320-31468-21

Analyte	Result	Qualifier	LOQ	DL	Unit	Dil Fac	D	Method	Prep Type
Perfluorooctanesulfonic acid (PFOS)	33	J M	38	6.5	ng/L	1		537	Total/NA
Perfluorooctanoic acid (PFOA)	15	J	19	2.7	ng/L	1		537	Total/NA
Perfluorohexanesulfonic acid (PFHxS)	13	J	29	5.2	ng/L	1		537	Total/NA
Perfluoroheptanoic acid (PFHpA)	5.4	J	9.5	1.8	ng/L	1		537	Total/NA

## Client Sample ID: NAWC-091117-FRB-162

Lab Sample ID: 320-31468-22

No Detections.

## Client Sample ID: WGNA-091117-DUP09

Lab Sample ID: 320-31468-23

Analyte	Result	Qualifier	LOQ	DL	Unit	Dil Fac	D	Method	Prep Type
Perfluorooctanoic acid (PFOA)	4.5	J	19	2.7	ng/L	1		537	Total/NA

This Detection Summary does not include radiochemical test results.

TestAmerica Sacramento

# Client Sample Results

Client: Tetra Tech, Inc.  
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-31468-1

## Client Sample ID: NAWC-091117-RW-106

Date Collected: 09/11/17 09:40

Date Received: 09/12/17 14:21

## Lab Sample ID: 320-31468-1

Matrix: Water

### Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
<b>Perfluorooctanesulfonic acid (PFOS)</b>	<b>17</b>	<b>J M</b>	40	6.7	ng/L		09/14/17 09:17	09/20/17 04:49	1
<b>Perfluorooctanoic acid (PFOA)</b>	<b>20</b>		20	2.8	ng/L		09/14/17 09:17	09/20/17 04:49	1
Perfluorononanoic acid (PFNA)	20	U	24	7.9	ng/L		09/14/17 09:17	09/20/17 04:49	1
<b>Perfluorohexanesulfonic acid (PFHxS)</b>	<b>8.9</b>	<b>J</b>	30	5.4	ng/L		09/14/17 09:17	09/20/17 04:49	1
<b>Perfluoroheptanoic acid (PFHpA)</b>	<b>8.1</b>	<b>J</b>	9.9	1.9	ng/L		09/14/17 09:17	09/20/17 04:49	1
Perfluorobutanesulfonic acid (PFBS)	36	U	89	16	ng/L		09/14/17 09:17	09/20/17 04:49	1
<b>Surrogate</b>	<b>%Recovery</b>	<b>Qualifier</b>	<b>Limits</b>				<b>Prepared</b>	<b>Analyzed</b>	<b>Dil Fac</b>
13C2 PFHxA	67	Q	70 - 130				09/14/17 09:17	09/20/17 04:49	1
13C2 PFDA	100		70 - 130				09/14/17 09:17	09/20/17 04:49	1

## Client Sample ID: NAWC-091117-FRB-106

Date Collected: 09/11/17 09:35

Date Received: 09/12/17 14:21

## Lab Sample ID: 320-31468-2

Matrix: Water

### Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	15	U	39	6.6	ng/L		09/14/17 09:17	09/20/17 04:54	1
Perfluorooctanoic acid (PFOA)	7.7	U	19	2.7	ng/L		09/14/17 09:17	09/20/17 04:54	1
Perfluorononanoic acid (PFNA)	19	U	23	7.7	ng/L		09/14/17 09:17	09/20/17 04:54	1
Perfluorohexanesulfonic acid (PFHxS)	12	U	29	5.3	ng/L		09/14/17 09:17	09/20/17 04:54	1
Perfluoroheptanoic acid (PFHpA)	3.9	U	9.7	1.8	ng/L		09/14/17 09:17	09/20/17 04:54	1
Perfluorobutanesulfonic acid (PFBS)	35	U	87	16	ng/L		09/14/17 09:17	09/20/17 04:54	1
<b>Surrogate</b>	<b>%Recovery</b>	<b>Qualifier</b>	<b>Limits</b>				<b>Prepared</b>	<b>Analyzed</b>	<b>Dil Fac</b>
13C2 PFHxA	82		70 - 130				09/14/17 09:17	09/20/17 04:54	1
13C2 PFDA	105		70 - 130				09/14/17 09:17	09/20/17 04:54	1

## Client Sample ID: NAWC-091117-RW-060

Date Collected: 09/11/17 09:55

Date Received: 09/12/17 14:21

## Lab Sample ID: 320-31468-3

Matrix: Water

### Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
<b>Perfluorooctanesulfonic acid (PFOS)</b>	<b>27</b>	<b>J M</b>	38	6.5	ng/L		09/14/17 09:17	09/20/17 04:59	1
<b>Perfluorooctanoic acid (PFOA)</b>	<b>17</b>	<b>J</b>	19	2.7	ng/L		09/14/17 09:17	09/20/17 04:59	1
Perfluorononanoic acid (PFNA)	19	U	23	7.6	ng/L		09/14/17 09:17	09/20/17 04:59	1
<b>Perfluorohexanesulfonic acid (PFHxS)</b>	<b>9.9</b>	<b>J</b>	29	5.3	ng/L		09/14/17 09:17	09/20/17 04:59	1
<b>Perfluoroheptanoic acid (PFHpA)</b>	<b>3.9</b>	<b>J</b>	9.6	1.8	ng/L		09/14/17 09:17	09/20/17 04:59	1
Perfluorobutanesulfonic acid (PFBS)	34	U	86	15	ng/L		09/14/17 09:17	09/20/17 04:59	1
<b>Surrogate</b>	<b>%Recovery</b>	<b>Qualifier</b>	<b>Limits</b>				<b>Prepared</b>	<b>Analyzed</b>	<b>Dil Fac</b>
13C2 PFHxA	71		70 - 130				09/14/17 09:17	09/20/17 04:59	1
13C2 PFDA	114		70 - 130				09/14/17 09:17	09/20/17 04:59	1

# Client Sample Results

Client: Tetra Tech, Inc.  
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-31468-1

**Client Sample ID: NAWC-091117-FRB-060**

**Lab Sample ID: 320-31468-4**

**Date Collected: 09/11/17 09:50**

**Matrix: Water**

**Date Received: 09/12/17 14:21**

**Method: 537 - Perfluorinated Alkyl Acids (LC/MS)**

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	15	U	38	6.5	ng/L		09/14/17 09:17	09/20/17 05:04	1
Perfluorooctanoic acid (PFOA)	7.7	U	19	2.7	ng/L		09/14/17 09:17	09/20/17 05:04	1
Perfluorononanoic acid (PFNA)	19	U	23	7.7	ng/L		09/14/17 09:17	09/20/17 05:04	1
Perfluorohexanesulfonic acid (PFHxS)	12	U	29	5.3	ng/L		09/14/17 09:17	09/20/17 05:04	1
Perfluoroheptanoic acid (PFHpA)	3.8	U	9.6	1.8	ng/L		09/14/17 09:17	09/20/17 05:04	1
Perfluorobutanesulfonic acid (PFBS)	35	U	87	15	ng/L		09/14/17 09:17	09/20/17 05:04	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	86		70 - 130	09/14/17 09:17	09/20/17 05:04	1
13C2 PFDA	107		70 - 130	09/14/17 09:17	09/20/17 05:04	1

**Client Sample ID: NAWC-091117-RW-314**

**Lab Sample ID: 320-31468-5**

**Date Collected: 09/11/17 10:25**

**Matrix: Water**

**Date Received: 09/12/17 14:21**

**Method: 537 - Perfluorinated Alkyl Acids (LC/MS)**

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	15	J M	38	6.5	ng/L		09/14/17 09:17	09/20/17 05:08	1
Perfluorooctanoic acid (PFOA)	17	J	19	2.7	ng/L		09/14/17 09:17	09/20/17 05:08	1
Perfluorononanoic acid (PFNA)	19	U	23	7.6	ng/L		09/14/17 09:17	09/20/17 05:08	1
Perfluorohexanesulfonic acid (PFHxS)	11	U	29	5.2	ng/L		09/14/17 09:17	09/20/17 05:08	1
Perfluoroheptanoic acid (PFHpA)	4.4	J	9.5	1.8	ng/L		09/14/17 09:17	09/20/17 05:08	1
Perfluorobutanesulfonic acid (PFBS)	34	U	86	15	ng/L		09/14/17 09:17	09/20/17 05:08	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	72		70 - 130	09/14/17 09:17	09/20/17 05:08	1
13C2 PFDA	104		70 - 130	09/14/17 09:17	09/20/17 05:08	1

**Client Sample ID: NAWC-091117-FRB-314**

**Lab Sample ID: 320-31468-6**

**Date Collected: 09/11/17 10:20**

**Matrix: Water**

**Date Received: 09/12/17 14:21**

**Method: 537 - Perfluorinated Alkyl Acids (LC/MS)**

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	15	U	38	6.4	ng/L		09/14/17 09:17	09/20/17 05:13	1
Perfluorooctanoic acid (PFOA)	7.5	U	19	2.6	ng/L		09/14/17 09:17	09/20/17 05:13	1
Perfluorononanoic acid (PFNA)	19	U	23	7.5	ng/L		09/14/17 09:17	09/20/17 05:13	1
Perfluorohexanesulfonic acid (PFHxS)	11	U	28	5.2	ng/L		09/14/17 09:17	09/20/17 05:13	1
Perfluoroheptanoic acid (PFHpA)	3.8	U	9.4	1.8	ng/L		09/14/17 09:17	09/20/17 05:13	1
Perfluorobutanesulfonic acid (PFBS)	34	U	85	15	ng/L		09/14/17 09:17	09/20/17 05:13	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	82		70 - 130	09/14/17 09:17	09/20/17 05:13	1
13C2 PFDA	102		70 - 130	09/14/17 09:17	09/20/17 05:13	1

# Client Sample Results

Client: Tetra Tech, Inc.  
 Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-31468-1

**Client Sample ID: NAWC-091117-RW-258**

**Lab Sample ID: 320-31468-7**

**Date Collected: 09/11/17 11:00**

**Matrix: Water**

**Date Received: 09/12/17 14:21**

**Method: 537 - Perfluorinated Alkyl Acids (LC/MS)**

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	18	J M	37	6.4	ng/L		09/14/17 09:17	09/20/17 05:18	1
Perfluorooctanoic acid (PFOA)	21		19	2.6	ng/L		09/14/17 09:17	09/20/17 05:18	1
Perfluorononanoic acid (PFNA)	12	J	22	7.5	ng/L		09/14/17 09:17	09/20/17 05:18	1
Perfluorohexanesulfonic acid (PFHxS)	11	U	28	5.1	ng/L		09/14/17 09:17	09/20/17 05:18	1
Perfluoroheptanoic acid (PFHpA)	7.7	J	9.4	1.8	ng/L		09/14/17 09:17	09/20/17 05:18	1
Perfluorobutanesulfonic acid (PFBS)	34	U	84	15	ng/L		09/14/17 09:17	09/20/17 05:18	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	72		70 - 130	09/14/17 09:17	09/20/17 05:18	1
13C2 PFDA	98		70 - 130	09/14/17 09:17	09/20/17 05:18	1

**Client Sample ID: NAWC-091117-FRB-258**

**Lab Sample ID: 320-31468-8**

**Date Collected: 09/11/17 10:55**

**Matrix: Water**

**Date Received: 09/12/17 14:21**

**Method: 537 - Perfluorinated Alkyl Acids (LC/MS)**

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	15	U	38	6.5	ng/L		09/14/17 09:17	09/20/17 05:32	1
Perfluorooctanoic acid (PFOA)	7.6	U	19	2.7	ng/L		09/14/17 09:17	09/20/17 05:32	1
Perfluorononanoic acid (PFNA)	19	U	23	7.6	ng/L		09/14/17 09:17	09/20/17 05:32	1
Perfluorohexanesulfonic acid (PFHxS)	11	U	29	5.3	ng/L		09/14/17 09:17	09/20/17 05:32	1
Perfluoroheptanoic acid (PFHpA)	3.8	U	9.6	1.8	ng/L		09/14/17 09:17	09/20/17 05:32	1
Perfluorobutanesulfonic acid (PFBS)	34	U	86	15	ng/L		09/14/17 09:17	09/20/17 05:32	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	86		70 - 130	09/14/17 09:17	09/20/17 05:32	1
13C2 PFDA	101		70 - 130	09/14/17 09:17	09/20/17 05:32	1

**Client Sample ID: NAWC-091117-RW-048**

**Lab Sample ID: 320-31468-9**

**Date Collected: 09/11/17 13:05**

**Matrix: Water**

**Date Received: 09/12/17 14:21**

**Method: 537 - Perfluorinated Alkyl Acids (LC/MS)**

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	15	U M	38	6.4	ng/L		09/14/17 09:17	09/20/17 05:37	1
Perfluorooctanoic acid (PFOA)	4.5	J M	19	2.7	ng/L		09/14/17 09:17	09/20/17 05:37	1
Perfluorononanoic acid (PFNA)	19	U	23	7.6	ng/L		09/14/17 09:17	09/20/17 05:37	1
Perfluorohexanesulfonic acid (PFHxS)	11	U	28	5.2	ng/L		09/14/17 09:17	09/20/17 05:37	1
Perfluoroheptanoic acid (PFHpA)	3.8	U	9.5	1.8	ng/L		09/14/17 09:17	09/20/17 05:37	1
Perfluorobutanesulfonic acid (PFBS)	34	U	85	15	ng/L		09/14/17 09:17	09/20/17 05:37	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	74		70 - 130	09/14/17 09:17	09/20/17 05:37	1
13C2 PFDA	111		70 - 130	09/14/17 09:17	09/20/17 05:37	1

# Client Sample Results

Client: Tetra Tech, Inc.  
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-31468-1

**Client Sample ID: NAWC-091117-FRB-048**

**Lab Sample ID: 320-31468-10**

**Date Collected: 09/11/17 13:00**

**Matrix: Water**

**Date Received: 09/12/17 14:21**

**Method: 537 - Perfluorinated Alkyl Acids (LC/MS)**

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	15	U	37	6.4	ng/L		09/14/17 09:17	09/20/17 05:42	1
Perfluorooctanoic acid (PFOA)	7.5	U	19	2.6	ng/L		09/14/17 09:17	09/20/17 05:42	1
Perfluorononanoic acid (PFNA)	19	U	22	7.5	ng/L		09/14/17 09:17	09/20/17 05:42	1
Perfluorohexanesulfonic acid (PFHxS)	11	U	28	5.2	ng/L		09/14/17 09:17	09/20/17 05:42	1
Perfluoroheptanoic acid (PFHpA)	3.7	U	9.4	1.8	ng/L		09/14/17 09:17	09/20/17 05:42	1
Perfluorobutanesulfonic acid (PFBS)	34	U	84	15	ng/L		09/14/17 09:17	09/20/17 05:42	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	84		70 - 130	09/14/17 09:17	09/20/17 05:42	1
13C2 PFDA	102		70 - 130	09/14/17 09:17	09/20/17 05:42	1

**Client Sample ID: NAWC-091117-RW-145**

**Lab Sample ID: 320-31468-11**

**Date Collected: 09/11/17 13:35**

**Matrix: Water**

**Date Received: 09/12/17 14:21**

**Method: 537 - Perfluorinated Alkyl Acids (LC/MS)**

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	19	J M	37	6.3	ng/L		09/14/17 09:17	09/20/17 05:46	1
Perfluorooctanoic acid (PFOA)	20		19	2.6	ng/L		09/14/17 09:17	09/20/17 05:46	1
Perfluorononanoic acid (PFNA)	19	U	22	7.4	ng/L		09/14/17 09:17	09/20/17 05:46	1
Perfluorohexanesulfonic acid (PFHxS)	7.3	J	28	5.1	ng/L		09/14/17 09:17	09/20/17 05:46	1
Perfluoroheptanoic acid (PFHpA)	5.6	J	9.3	1.8	ng/L		09/14/17 09:17	09/20/17 05:46	1
Perfluorobutanesulfonic acid (PFBS)	33	U	84	15	ng/L		09/14/17 09:17	09/20/17 05:46	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	74		70 - 130	09/14/17 09:17	09/20/17 05:46	1
13C2 PFDA	115		70 - 130	09/14/17 09:17	09/20/17 05:46	1

**Client Sample ID: NAWC-091117-FRB-145**

**Lab Sample ID: 320-31468-12**

**Date Collected: 09/11/17 13:30**

**Matrix: Water**

**Date Received: 09/12/17 14:21**

**Method: 537 - Perfluorinated Alkyl Acids (LC/MS)**

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	15	U	38	6.4	ng/L		09/14/17 09:17	09/20/17 05:51	1
Perfluorooctanoic acid (PFOA)	7.5	U	19	2.6	ng/L		09/14/17 09:17	09/20/17 05:51	1
Perfluorononanoic acid (PFNA)	19	U	23	7.5	ng/L		09/14/17 09:17	09/20/17 05:51	1
Perfluorohexanesulfonic acid (PFHxS)	11	U	28	5.2	ng/L		09/14/17 09:17	09/20/17 05:51	1
Perfluoroheptanoic acid (PFHpA)	3.8	U	9.4	1.8	ng/L		09/14/17 09:17	09/20/17 05:51	1
Perfluorobutanesulfonic acid (PFBS)	34	U	85	15	ng/L		09/14/17 09:17	09/20/17 05:51	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	83		70 - 130	09/14/17 09:17	09/20/17 05:51	1
13C2 PFDA	100		70 - 130	09/14/17 09:17	09/20/17 05:51	1

# Client Sample Results

Client: Tetra Tech, Inc.  
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-31468-1

**Client Sample ID: NAWC-091117-RW-317**

**Lab Sample ID: 320-31468-13**

Date Collected: 09/11/17 14:00

Matrix: Water

Date Received: 09/12/17 14:21

**Method: 537 - Perfluorinated Alkyl Acids (LC/MS)**

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	49	M	38	6.4	ng/L	-	09/14/17 09:17	09/20/17 05:56	1
Perfluorooctanoic acid (PFOA)	21		19	2.7	ng/L		09/14/17 09:17	09/20/17 05:56	1
Perfluorononanoic acid (PFNA)	19	U	23	7.6	ng/L		09/14/17 09:17	09/20/17 05:56	1
Perfluorohexanesulfonic acid (PFHxS)	34		28	5.2	ng/L		09/14/17 09:17	09/20/17 05:56	1
Perfluoroheptanoic acid (PFHpA)	8.1	J	9.5	1.8	ng/L		09/14/17 09:17	09/20/17 05:56	1
Perfluorobutanesulfonic acid (PFBS)	34	U	85	15	ng/L		09/14/17 09:17	09/20/17 05:56	1
<b>Surrogate</b>	<b>%Recovery</b>	<b>Qualifier</b>	<b>Limits</b>				<b>Prepared</b>	<b>Analyzed</b>	<b>Dil Fac</b>
13C2 PFHxA	78		70 - 130				09/14/17 09:17	09/20/17 05:56	1
13C2 PFDA	116		70 - 130				09/14/17 09:17	09/20/17 05:56	1

**Client Sample ID: NAWC-091117-FRB-317**

**Lab Sample ID: 320-31468-14**

Date Collected: 09/11/17 13:55

Matrix: Water

Date Received: 09/12/17 14:21

**Method: 537 - Perfluorinated Alkyl Acids (LC/MS)**

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	16	U	39	6.7	ng/L	-	09/14/17 09:17	09/20/17 06:01	1
Perfluorooctanoic acid (PFOA)	7.9	U	20	2.8	ng/L		09/14/17 09:17	09/20/17 06:01	1
Perfluorononanoic acid (PFNA)	20	U	24	7.9	ng/L		09/14/17 09:17	09/20/17 06:01	1
Perfluorohexanesulfonic acid (PFHxS)	12	U	29	5.4	ng/L		09/14/17 09:17	09/20/17 06:01	1
Perfluoroheptanoic acid (PFHpA)	3.9	U	9.8	1.9	ng/L		09/14/17 09:17	09/20/17 06:01	1
Perfluorobutanesulfonic acid (PFBS)	35	U	88	16	ng/L		09/14/17 09:17	09/20/17 06:01	1
<b>Surrogate</b>	<b>%Recovery</b>	<b>Qualifier</b>	<b>Limits</b>				<b>Prepared</b>	<b>Analyzed</b>	<b>Dil Fac</b>
13C2 PFHxA	83		70 - 130				09/14/17 09:17	09/20/17 06:01	1
13C2 PFDA	97		70 - 130				09/14/17 09:17	09/20/17 06:01	1

**Client Sample ID: NAWC-091117-RW-319**

**Lab Sample ID: 320-31468-15**

Date Collected: 09/11/17 14:25

Matrix: Water

Date Received: 09/12/17 14:21

**Method: 537 - Perfluorinated Alkyl Acids (LC/MS)**

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	43	M	40	6.8	ng/L	-	09/14/17 09:17	09/20/17 06:05	1
Perfluorooctanoic acid (PFOA)	44		20	2.8	ng/L		09/14/17 09:17	09/20/17 06:05	1
Perfluorononanoic acid (PFNA)	9.7	J	24	8.0	ng/L		09/14/17 09:17	09/20/17 06:05	1
Perfluorohexanesulfonic acid (PFHxS)	8.0	J	30	5.5	ng/L		09/14/17 09:17	09/20/17 06:05	1
Perfluoroheptanoic acid (PFHpA)	15	M	10	1.9	ng/L		09/14/17 09:17	09/20/17 06:05	1
Perfluorobutanesulfonic acid (PFBS)	36	U	90	16	ng/L		09/14/17 09:17	09/20/17 06:05	1
<b>Surrogate</b>	<b>%Recovery</b>	<b>Qualifier</b>	<b>Limits</b>				<b>Prepared</b>	<b>Analyzed</b>	<b>Dil Fac</b>
13C2 PFHxA	61	Q	70 - 130				09/14/17 09:17	09/20/17 06:05	1
13C2 PFDA	83		70 - 130				09/14/17 09:17	09/20/17 06:05	1



# Client Sample Results

Client: Tetra Tech, Inc.  
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-31468-1

**Client Sample ID: NAWC-091117-FRB-319**

**Lab Sample ID: 320-31468-16**

**Date Collected: 09/11/17 14:40**

**Matrix: Water**

**Date Received: 09/12/17 14:21**

**Method: 537 - Perfluorinated Alkyl Acids (LC/MS)**

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	15	U	37	6.4	ng/L		09/14/17 09:17	09/20/17 06:10	1
Perfluorooctanoic acid (PFOA)	7.5	U	19	2.6	ng/L		09/14/17 09:17	09/20/17 06:10	1
Perfluorononanoic acid (PFNA)	19	U	22	7.5	ng/L		09/14/17 09:17	09/20/17 06:10	1
Perfluorohexanesulfonic acid (PFHxS)	11	U	28	5.2	ng/L		09/14/17 09:17	09/20/17 06:10	1
Perfluoroheptanoic acid (PFHpA)	3.7	U	9.4	1.8	ng/L		09/14/17 09:17	09/20/17 06:10	1
Perfluorobutanesulfonic acid (PFBS)	34	U	84	15	ng/L		09/14/17 09:17	09/20/17 06:10	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	82		70 - 130	09/14/17 09:17	09/20/17 06:10	1
13C2 PFDA	124		70 - 130	09/14/17 09:17	09/20/17 06:10	1

**Client Sample ID: NAWC-091117-RW-321**

**Lab Sample ID: 320-31468-17**

**Date Collected: 09/11/17 15:10**

**Matrix: Water**

**Date Received: 09/12/17 14:21**

**Method: 537 - Perfluorinated Alkyl Acids (LC/MS)**

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
<b>Perfluorooctanesulfonic acid (PFOS)</b>	<b>7.5</b>	<b>J M</b>	38	6.5	ng/L		09/14/17 09:17	09/20/17 06:15	1
<b>Perfluorooctanoic acid (PFOA)</b>	<b>6.9</b>	<b>J</b>	19	2.7	ng/L		09/14/17 09:17	09/20/17 06:15	1
Perfluorononanoic acid (PFNA)	19	U	23	7.6	ng/L		09/14/17 09:17	09/20/17 06:15	1
Perfluorohexanesulfonic acid (PFHxS)	11	U	29	5.2	ng/L		09/14/17 09:17	09/20/17 06:15	1
<b>Perfluoroheptanoic acid (PFHpA)</b>	<b>1.8</b>	<b>J</b>	9.5	1.8	ng/L		09/14/17 09:17	09/20/17 06:15	1
Perfluorobutanesulfonic acid (PFBS)	34	U	86	15	ng/L		09/14/17 09:17	09/20/17 06:15	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	76		70 - 130	09/14/17 09:17	09/20/17 06:15	1
13C2 PFDA	106		70 - 130	09/14/17 09:17	09/20/17 06:15	1

**Client Sample ID: NAWC-091117-FRB-321**

**Lab Sample ID: 320-31468-18**

**Date Collected: 09/11/17 15:05**

**Matrix: Water**

**Date Received: 09/12/17 14:21**

**Method: 537 - Perfluorinated Alkyl Acids (LC/MS)**

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	15	U	38	6.5	ng/L		09/14/17 09:17	09/20/17 06:29	1
Perfluorooctanoic acid (PFOA)	7.6	U	19	2.7	ng/L		09/14/17 09:17	09/20/17 06:29	1
Perfluorononanoic acid (PFNA)	19	U	23	7.6	ng/L		09/14/17 09:17	09/20/17 06:29	1
Perfluorohexanesulfonic acid (PFHxS)	11	U	28	5.2	ng/L		09/14/17 09:17	09/20/17 06:29	1
Perfluoroheptanoic acid (PFHpA)	3.8	U	9.5	1.8	ng/L		09/14/17 09:17	09/20/17 06:29	1
Perfluorobutanesulfonic acid (PFBS)	34	U	85	15	ng/L		09/14/17 09:17	09/20/17 06:29	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	84		70 - 130	09/14/17 09:17	09/20/17 06:29	1
13C2 PFDA	104		70 - 130	09/14/17 09:17	09/20/17 06:29	1



# Client Sample Results

Client: Tetra Tech, Inc.  
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-31468-1

**Client Sample ID: NAWC-091117-RW-010**

**Lab Sample ID: 320-31468-19**

**Date Collected: 09/11/17 15:45**

**Matrix: Water**

**Date Received: 09/12/17 14:21**

**Method: 537 - Perfluorinated Alkyl Acids (LC/MS)**

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	30	J M	39	6.7	ng/L	-	09/14/17 09:17	09/20/17 06:34	1
Perfluorooctanoic acid (PFOA)	12	J	20	2.7	ng/L	-	09/14/17 09:17	09/20/17 06:34	1
Perfluorononanoic acid (PFNA)	20	U	24	7.9	ng/L	-	09/14/17 09:17	09/20/17 06:34	1
Perfluorohexanesulfonic acid (PFHxS)	17	J	29	5.4	ng/L	-	09/14/17 09:17	09/20/17 06:34	1
Perfluoroheptanoic acid (PFHpA)	5.4	J	9.8	1.9	ng/L	-	09/14/17 09:17	09/20/17 06:34	1
Perfluorobutanesulfonic acid (PFBS)	35	U	88	16	ng/L	-	09/14/17 09:17	09/20/17 06:34	1
<b>Surrogate</b>	<b>%Recovery</b>	<b>Qualifier</b>	<b>Limits</b>				<b>Prepared</b>	<b>Analyzed</b>	<b>Dil Fac</b>
13C2 PFHxA	75		70 - 130				09/14/17 09:17	09/20/17 06:34	1
13C2 PFDA	104		70 - 130				09/14/17 09:17	09/20/17 06:34	1

**Client Sample ID: NAWC-091117-FRB-010**

**Lab Sample ID: 320-31468-20**

**Date Collected: 09/11/17 15:40**

**Matrix: Water**

**Date Received: 09/12/17 14:21**

**Method: 537 - Perfluorinated Alkyl Acids (LC/MS)**

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	15	U	38	6.5	ng/L	-	09/14/17 09:17	09/20/17 06:39	1
Perfluorooctanoic acid (PFOA)	7.7	U	19	2.7	ng/L	-	09/14/17 09:17	09/20/17 06:39	1
Perfluorononanoic acid (PFNA)	19	U	23	7.7	ng/L	-	09/14/17 09:17	09/20/17 06:39	1
Perfluorohexanesulfonic acid (PFHxS)	12	U	29	5.3	ng/L	-	09/14/17 09:17	09/20/17 06:39	1
Perfluoroheptanoic acid (PFHpA)	3.8	U	9.6	1.8	ng/L	-	09/14/17 09:17	09/20/17 06:39	1
Perfluorobutanesulfonic acid (PFBS)	35	U	87	15	ng/L	-	09/14/17 09:17	09/20/17 06:39	1
<b>Surrogate</b>	<b>%Recovery</b>	<b>Qualifier</b>	<b>Limits</b>				<b>Prepared</b>	<b>Analyzed</b>	<b>Dil Fac</b>
13C2 PFHxA	83		70 - 130				09/14/17 09:17	09/20/17 06:39	1
13C2 PFDA	97		70 - 130				09/14/17 09:17	09/20/17 06:39	1

**Client Sample ID: NAWC-091117-RW-162**

**Lab Sample ID: 320-31468-21**

**Date Collected: 09/11/17 11:20**

**Matrix: Water**

**Date Received: 09/12/17 14:21**

**Method: 537 - Perfluorinated Alkyl Acids (LC/MS)**

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	33	J M	38	6.5	ng/L	-	09/14/17 09:29	09/20/17 04:11	1
Perfluorooctanoic acid (PFOA)	15	J	19	2.7	ng/L	-	09/14/17 09:29	09/20/17 04:11	1
Perfluorononanoic acid (PFNA)	19	U	23	7.6	ng/L	-	09/14/17 09:29	09/20/17 04:11	1
Perfluorohexanesulfonic acid (PFHxS)	13	J	29	5.2	ng/L	-	09/14/17 09:29	09/20/17 04:11	1
Perfluoroheptanoic acid (PFHpA)	5.4	J	9.5	1.8	ng/L	-	09/14/17 09:29	09/20/17 04:11	1
Perfluorobutanesulfonic acid (PFBS)	34	U	86	15	ng/L	-	09/14/17 09:29	09/20/17 04:11	1
<b>Surrogate</b>	<b>%Recovery</b>	<b>Qualifier</b>	<b>Limits</b>				<b>Prepared</b>	<b>Analyzed</b>	<b>Dil Fac</b>
13C2 PFHxA	78		70 - 130				09/14/17 09:29	09/20/17 04:11	1
13C2 PFDA	111		70 - 130				09/14/17 09:29	09/20/17 04:11	1

# Client Sample Results

Client: Tetra Tech, Inc.  
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-31468-1

**Client Sample ID: NAWC-091117-FRB-162**

**Lab Sample ID: 320-31468-22**

**Date Collected: 09/11/17 11:15**

**Matrix: Water**

**Date Received: 09/12/17 14:21**

**Method: 537 - Perfluorinated Alkyl Acids (LC/MS)**

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	16	U	40	6.9	ng/L		09/14/17 09:29	09/20/17 04:16	1
Perfluorooctanoic acid (PFOA)	8.1	U	20	2.8	ng/L		09/14/17 09:29	09/20/17 04:16	1
Perfluorononanoic acid (PFNA)	20	U	24	8.1	ng/L		09/14/17 09:29	09/20/17 04:16	1
Perfluorohexanesulfonic acid (PFHxS)	12	U	30	5.6	ng/L		09/14/17 09:29	09/20/17 04:16	1
Perfluoroheptanoic acid (PFHpA)	4.0	U	10	1.9	ng/L		09/14/17 09:29	09/20/17 04:16	1
Perfluorobutanesulfonic acid (PFBS)	36	U	91	16	ng/L		09/14/17 09:29	09/20/17 04:16	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	91		70 - 130	09/14/17 09:29	09/20/17 04:16	1
13C2 PFDA	129		70 - 130	09/14/17 09:29	09/20/17 04:16	1

**Client Sample ID: WGNA-091117-DUP09**

**Lab Sample ID: 320-31468-23**

**Date Collected: 09/11/17 07:00**

**Matrix: Water**

**Date Received: 09/12/17 14:21**

**Method: 537 - Perfluorinated Alkyl Acids (LC/MS)**

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	15	U M	38	6.5	ng/L		09/14/17 09:29	09/20/17 04:21	1
<b>Perfluorooctanoic acid (PFOA)</b>	<b>4.5</b>	<b>J</b>	19	2.7	ng/L		09/14/17 09:29	09/20/17 04:21	1
Perfluorononanoic acid (PFNA)	19	U	23	7.7	ng/L		09/14/17 09:29	09/20/17 04:21	1
Perfluorohexanesulfonic acid (PFHxS)	12	U	29	5.3	ng/L		09/14/17 09:29	09/20/17 04:21	1
Perfluoroheptanoic acid (PFHpA)	3.8	U M	9.6	1.8	ng/L		09/14/17 09:29	09/20/17 04:21	1
Perfluorobutanesulfonic acid (PFBS)	35	U	87	15	ng/L		09/14/17 09:29	09/20/17 04:21	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	75		70 - 130	09/14/17 09:29	09/20/17 04:21	1
13C2 PFDA	125		70 - 130	09/14/17 09:29	09/20/17 04:21	1

# Default Detection Limits

Client: Tetra Tech, Inc.  
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-31468-1

## Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Prep: 537

Analyte	LOQ	DL	Units	Method
Perfluorobutanesulfonic acid (PFBS)	90	16	ng/L	537
Perfluoroheptanoic acid (PFHpA)	10	1.9	ng/L	537
Perfluorohexanesulfonic acid (PFHxS)	30	5.5	ng/L	537
Perfluorononanoic acid (PFNA)	24	8.0	ng/L	537
Perfluorooctanesulfonic acid (PFOS)	40	6.8	ng/L	537
Perfluorooctanoic acid (PFOA)	20	2.8	ng/L	537

# Surrogate Summary

Client: Tetra Tech, Inc.  
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-31468-1

## Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Matrix: Water

Prep Type: Total/NA

Lab Sample ID	Client Sample ID	Percent Surrogate Recovery (Acceptance Limits)	
		3C2 PFHx (70-130)	3C2 PFD <sub>A</sub> (70-130)
320-31468-1	NAWC-091117-RW-106	67 Q	100
320-31468-2	NAWC-091117-FRB-106	82	105
320-31468-3	NAWC-091117-RW-060	71	114
320-31468-4	NAWC-091117-FRB-060	86	107
320-31468-5	NAWC-091117-RW-314	72	104
320-31468-6	NAWC-091117-FRB-314	82	102
320-31468-7	NAWC-091117-RW-258	72	98
320-31468-8	NAWC-091117-FRB-258	86	101
320-31468-9	NAWC-091117-RW-048	74	111
320-31468-10	NAWC-091117-FRB-048	84	102
320-31468-11	NAWC-091117-RW-145	74	115
320-31468-12	NAWC-091117-FRB-145	83	100
320-31468-13	NAWC-091117-RW-317	78	116
320-31468-14	NAWC-091117-FRB-317	83	97
320-31468-15	NAWC-091117-RW-319	61 Q	83
320-31468-16	NAWC-091117-FRB-319	82	124
320-31468-17	NAWC-091117-RW-321	76	106
320-31468-18	NAWC-091117-FRB-321	84	104
320-31468-19	NAWC-091117-RW-010	75	104
320-31468-20	NAWC-091117-FRB-010	83	97
320-31468-21	NAWC-091117-RW-162	78	111
320-31468-22	NAWC-091117-FRB-162	91	129
320-31468-23	WGNA-091117-DUP09	75	125
LCS 320-184382/2-A	Lab Control Sample	91	115
LCSD 320-184382/3-A	Lab Control Sample Dup	86	110
LLCS 320-184385/2-A	Lab Control Sample	90	113
LLCSD 320-184385/3-A	Lab Control Sample Dup	93	124
MB 320-184382/1-A	Method Blank	90	111
MB 320-184385/1-A	Method Blank	87	143 Q

### Surrogate Legend

13C2 PFHxA = 13C2 PFHxA

13C2 PFDA = 13C2 PFDA

# QC Sample Results

Client: Tetra Tech, Inc.  
 Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-31468-1

## Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

**Lab Sample ID: MB 320-184382/1-A**  
**Matrix: Water**  
**Analysis Batch: 185407**

**Client Sample ID: Method Blank**  
**Prep Type: Total/NA**  
**Prep Batch: 184382**

Analyte	MB	MB	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
	Result	Qualifier							
Perfluorooctanesulfonic acid (PFOS)	16	U	40	6.8	ng/L		09/14/17 09:17	09/20/17 04:35	1
Perfluorooctanoic acid (PFOA)	8.0	U	20	2.8	ng/L		09/14/17 09:17	09/20/17 04:35	1
Perfluorononanoic acid (PFNA)	20	U	24	8.0	ng/L		09/14/17 09:17	09/20/17 04:35	1
Perfluorohexanesulfonic acid (PFHxS)	12	U	30	5.5	ng/L		09/14/17 09:17	09/20/17 04:35	1
Perfluoroheptanoic acid (PFHpA)	4.0	U	10	1.9	ng/L		09/14/17 09:17	09/20/17 04:35	1
Perfluorobutanesulfonic acid (PFBS)	36	U	90	16	ng/L		09/14/17 09:17	09/20/17 04:35	1

Surrogate	MB	MB	Limits	Prepared	Analyzed	Dil Fac
	%Recovery	Qualifier				
13C2 PFHxA	90		70 - 130	09/14/17 09:17	09/20/17 04:35	1
13C2 PFDA	111		70 - 130	09/14/17 09:17	09/20/17 04:35	1

**Lab Sample ID: LCS 320-184382/2-A**  
**Matrix: Water**  
**Analysis Batch: 185407**

**Client Sample ID: Lab Control Sample**  
**Prep Type: Total/NA**  
**Prep Batch: 184382**  
**%Rec. Limits**

Analyte	Spike Added	LCS Result	LCS Qualifier	Unit	D	%Rec	%Rec. Limits
Perfluorooctanoic acid (PFOA)	111	103		ng/L		93	70 - 130
Perfluorononanoic acid (PFNA)	111	99.7		ng/L		90	70 - 130
Perfluorohexanesulfonic acid (PFHxS)	167	150		ng/L		90	70 - 130
Perfluoroheptanoic acid (PFHpA)	55.6	50.5		ng/L		91	70 - 130
Perfluorobutanesulfonic acid (PFBS)	500	408		ng/L		82	70 - 130

Surrogate	LCS	LCS	Limits
	%Recovery	Qualifier	
13C2 PFHxA	91		70 - 130
13C2 PFDA	115		70 - 130

**Lab Sample ID: LCSD 320-184382/3-A**  
**Matrix: Water**  
**Analysis Batch: 185407**

**Client Sample ID: Lab Control Sample Dup**  
**Prep Type: Total/NA**  
**Prep Batch: 184382**  
**%Rec. RPD**

Analyte	Spike Added	LCSD Result	LCSD Qualifier	Unit	D	%Rec	%Rec. Limits	RPD	RPD Limit
Perfluorooctanoic acid (PFOA)	111	96.8		ng/L		87	70 - 130	7	30
Perfluorononanoic acid (PFNA)	111	93.6		ng/L		84	70 - 130	6	30
Perfluorohexanesulfonic acid (PFHxS)	167	143		ng/L		86	70 - 130	5	30
Perfluoroheptanoic acid (PFHpA)	55.6	48.7		ng/L		88	70 - 130	3	30
Perfluorobutanesulfonic acid (PFBS)	500	403		ng/L		81	70 - 130	1	30

Surrogate	LCSD	LCSD	Limits
	%Recovery	Qualifier	
13C2 PFHxA	86		70 - 130
13C2 PFDA	110		70 - 130

# QC Sample Results

Client: Tetra Tech, Inc.  
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-31468-1

## Method: 537 - Perfluorinated Alkyl Acids (LC/MS) (Continued)

**Lab Sample ID: MB 320-184385/1-A**  
**Matrix: Water**  
**Analysis Batch: 185406**

**Client Sample ID: Method Blank**  
**Prep Type: Total/NA**  
**Prep Batch: 184385**

Analyte	MB	MB	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
	Result	Qualifier							
Perfluorooctanesulfonic acid (PFOS)	16	U	40	6.8	ng/L		09/14/17 09:29	09/20/17 03:57	1
Perfluorooctanoic acid (PFOA)	8.0	U	20	2.8	ng/L		09/14/17 09:29	09/20/17 03:57	1
Perfluorononanoic acid (PFNA)	20	U	24	8.0	ng/L		09/14/17 09:29	09/20/17 03:57	1
Perfluorohexanesulfonic acid (PFHxS)	12	U	30	5.5	ng/L		09/14/17 09:29	09/20/17 03:57	1
Perfluoroheptanoic acid (PFHpA)	4.0	U	10	1.9	ng/L		09/14/17 09:29	09/20/17 03:57	1
Perfluorobutanesulfonic acid (PFBS)	36	U	90	16	ng/L		09/14/17 09:29	09/20/17 03:57	1
Surrogate	MB	MB	Limits			D	Prepared	Analyzed	Dil Fac
	%Recovery	Qualifier							
13C2 PFHxA	87		70 - 130				09/14/17 09:29	09/20/17 03:57	1
13C2 PFDA	143	Q	70 - 130				09/14/17 09:29	09/20/17 03:57	1

**Lab Sample ID: LLCS 320-184385/2-A**  
**Matrix: Water**  
**Analysis Batch: 185406**

**Client Sample ID: Lab Control Sample**  
**Prep Type: Total/NA**  
**Prep Batch: 184385**

Analyte	Spike Added	LLCS	LLCS	Unit	D	%Rec	%Rec.	Limits
		Result	Qualifier					
Perfluorooctanesulfonic acid (PFOS)	40.0	36.6	J M	ng/L		91		50 - 150
Perfluorooctanoic acid (PFOA)	20.0	18.4	J	ng/L		92		50 - 150
Perfluorononanoic acid (PFNA)	20.0	18.5	J	ng/L		93		50 - 150
Perfluorohexanesulfonic acid (PFHxS)	30.0	28.9	J	ng/L		96		50 - 150
Perfluoroheptanoic acid (PFHpA)	10.0	10.2		ng/L		102		50 - 150
Perfluorobutanesulfonic acid (PFBS)	90.0	86.1	J	ng/L		96		50 - 150
Surrogate	LLCS	LLCS	Limits			D	%Rec	Limits
	%Recovery	Qualifier						
13C2 PFHxA	90		70 - 130					
13C2 PFDA	113		70 - 130					

**Lab Sample ID: LLCSD 320-184385/3-A**  
**Matrix: Water**  
**Analysis Batch: 185406**

**Client Sample ID: Lab Control Sample Dup**  
**Prep Type: Total/NA**  
**Prep Batch: 184385**

Analyte	Spike Added	LLCSD	LLCSD	Unit	D	%Rec	%Rec.	Limits	RPD	RPD
		Result	Qualifier						RPD	Limit
Perfluorooctanesulfonic acid (PFOS)	40.0	36.2	J M	ng/L		90		50 - 150	1	50
Perfluorooctanoic acid (PFOA)	20.0	18.7	J	ng/L		93		50 - 150	1	50
Perfluorononanoic acid (PFNA)	20.0	19.0	J	ng/L		95		50 - 150	3	50
Perfluorohexanesulfonic acid (PFHxS)	30.0	29.4	J	ng/L		98		50 - 150	2	50
Perfluoroheptanoic acid (PFHpA)	10.0	10.8		ng/L		108		50 - 150	6	50
Perfluorobutanesulfonic acid (PFBS)	90.0	89.0	J	ng/L		99		50 - 150	3	50
Surrogate	LLCSD	LLCSD	Limits			D	%Rec	Limits		
	%Recovery	Qualifier								
13C2 PFHxA	93		70 - 130							
13C2 PFDA	124		70 - 130							

TestAmerica Sacramento

# QC Association Summary

Client: Tetra Tech, Inc.  
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-31468-1

## LCMS

### Prep Batch: 184382

Lab Sample ID	Client Sample ID	Prep Type	Matrix	Method	Prep Batch
320-31468-1	NAWC-091117-RW-106	Total/NA	Water	537	
320-31468-2	NAWC-091117-FRB-106	Total/NA	Water	537	
320-31468-3	NAWC-091117-RW-060	Total/NA	Water	537	
320-31468-4	NAWC-091117-FRB-060	Total/NA	Water	537	
320-31468-5	NAWC-091117-RW-314	Total/NA	Water	537	
320-31468-6	NAWC-091117-FRB-314	Total/NA	Water	537	
320-31468-7	NAWC-091117-RW-258	Total/NA	Water	537	
320-31468-8	NAWC-091117-FRB-258	Total/NA	Water	537	
320-31468-9	NAWC-091117-RW-048	Total/NA	Water	537	
320-31468-10	NAWC-091117-FRB-048	Total/NA	Water	537	
320-31468-11	NAWC-091117-RW-145	Total/NA	Water	537	
320-31468-12	NAWC-091117-FRB-145	Total/NA	Water	537	
320-31468-13	NAWC-091117-RW-317	Total/NA	Water	537	
320-31468-14	NAWC-091117-FRB-317	Total/NA	Water	537	
320-31468-15	NAWC-091117-RW-319	Total/NA	Water	537	
320-31468-16	NAWC-091117-FRB-319	Total/NA	Water	537	
320-31468-17	NAWC-091117-RW-321	Total/NA	Water	537	
320-31468-18	NAWC-091117-FRB-321	Total/NA	Water	537	
320-31468-19	NAWC-091117-RW-010	Total/NA	Water	537	
320-31468-20	NAWC-091117-FRB-010	Total/NA	Water	537	
MB 320-184382/1-A	Method Blank	Total/NA	Water	537	
LCS 320-184382/2-A	Lab Control Sample	Total/NA	Water	537	
LCSD 320-184382/3-A	Lab Control Sample Dup	Total/NA	Water	537	

### Prep Batch: 184385

Lab Sample ID	Client Sample ID	Prep Type	Matrix	Method	Prep Batch
320-31468-21	NAWC-091117-RW-162	Total/NA	Water	537	
320-31468-22	NAWC-091117-FRB-162	Total/NA	Water	537	
320-31468-23	WGNA-091117-DUP09	Total/NA	Water	537	
MB 320-184385/1-A	Method Blank	Total/NA	Water	537	
LLCS 320-184385/2-A	Lab Control Sample	Total/NA	Water	537	
LLCSD 320-184385/3-A	Lab Control Sample Dup	Total/NA	Water	537	

### Analysis Batch: 185406

Lab Sample ID	Client Sample ID	Prep Type	Matrix	Method	Prep Batch
320-31468-21	NAWC-091117-RW-162	Total/NA	Water	537	184385
320-31468-22	NAWC-091117-FRB-162	Total/NA	Water	537	184385
320-31468-23	WGNA-091117-DUP09	Total/NA	Water	537	184385
MB 320-184385/1-A	Method Blank	Total/NA	Water	537	184385
LLCS 320-184385/2-A	Lab Control Sample	Total/NA	Water	537	184385
LLCSD 320-184385/3-A	Lab Control Sample Dup	Total/NA	Water	537	184385

### Analysis Batch: 185407

Lab Sample ID	Client Sample ID	Prep Type	Matrix	Method	Prep Batch
320-31468-1	NAWC-091117-RW-106	Total/NA	Water	537	184382
320-31468-2	NAWC-091117-FRB-106	Total/NA	Water	537	184382
320-31468-3	NAWC-091117-RW-060	Total/NA	Water	537	184382
320-31468-4	NAWC-091117-FRB-060	Total/NA	Water	537	184382
320-31468-5	NAWC-091117-RW-314	Total/NA	Water	537	184382
320-31468-6	NAWC-091117-FRB-314	Total/NA	Water	537	184382
320-31468-7	NAWC-091117-RW-258	Total/NA	Water	537	184382

TestAmerica Sacramento

# QC Association Summary

Client: Tetra Tech, Inc.  
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-31468-1

## LCMS (Continued)

### Analysis Batch: 185407 (Continued)

Lab Sample ID	Client Sample ID	Prep Type	Matrix	Method	Prep Batch
MB 320-184382/1-A	Method Blank	Total/NA	Water	537	184382
LCS 320-184382/2-A	Lab Control Sample	Total/NA	Water	537	184382
LCSD 320-184382/3-A	Lab Control Sample Dup	Total/NA	Water	537	184382

### Analysis Batch: 185408

Lab Sample ID	Client Sample ID	Prep Type	Matrix	Method	Prep Batch
320-31468-8	NAWC-091117-FRB-258	Total/NA	Water	537	184382
320-31468-9	NAWC-091117-RW-048	Total/NA	Water	537	184382
320-31468-10	NAWC-091117-FRB-048	Total/NA	Water	537	184382
320-31468-11	NAWC-091117-RW-145	Total/NA	Water	537	184382
320-31468-12	NAWC-091117-FRB-145	Total/NA	Water	537	184382
320-31468-13	NAWC-091117-RW-317	Total/NA	Water	537	184382
320-31468-14	NAWC-091117-FRB-317	Total/NA	Water	537	184382
320-31468-15	NAWC-091117-RW-319	Total/NA	Water	537	184382
320-31468-16	NAWC-091117-FRB-319	Total/NA	Water	537	184382
320-31468-17	NAWC-091117-RW-321	Total/NA	Water	537	184382

### Analysis Batch: 185409

Lab Sample ID	Client Sample ID	Prep Type	Matrix	Method	Prep Batch
320-31468-18	NAWC-091117-FRB-321	Total/NA	Water	537	184382
320-31468-19	NAWC-091117-RW-010	Total/NA	Water	537	184382
320-31468-20	NAWC-091117-FRB-010	Total/NA	Water	537	184382



# Lab Chronicle

Client: Tetra Tech, Inc.  
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-31468-1

## Client Sample ID: NAWC-091117-RW-106

Date Collected: 09/11/17 09:40

Date Received: 09/12/17 14:21

## Lab Sample ID: 320-31468-1

Matrix: Water

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			184382	09/14/17 09:17	NS1	TAL SAC
Total/NA	Analysis	537		1	185407	09/20/17 04:49	JRB	TAL SAC

## Client Sample ID: NAWC-091117-FRB-106

Date Collected: 09/11/17 09:35

Date Received: 09/12/17 14:21

## Lab Sample ID: 320-31468-2

Matrix: Water

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			184382	09/14/17 09:17	NS1	TAL SAC
Total/NA	Analysis	537		1	185407	09/20/17 04:54	JRB	TAL SAC

## Client Sample ID: NAWC-091117-RW-060

Date Collected: 09/11/17 09:55

Date Received: 09/12/17 14:21

## Lab Sample ID: 320-31468-3

Matrix: Water

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			184382	09/14/17 09:17	NS1	TAL SAC
Total/NA	Analysis	537		1	185407	09/20/17 04:59	JRB	TAL SAC

## Client Sample ID: NAWC-091117-FRB-060

Date Collected: 09/11/17 09:50

Date Received: 09/12/17 14:21

## Lab Sample ID: 320-31468-4

Matrix: Water

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			184382	09/14/17 09:17	NS1	TAL SAC
Total/NA	Analysis	537		1	185407	09/20/17 05:04	JRB	TAL SAC

## Client Sample ID: NAWC-091117-RW-314

Date Collected: 09/11/17 10:25

Date Received: 09/12/17 14:21

## Lab Sample ID: 320-31468-5

Matrix: Water

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			184382	09/14/17 09:17	NS1	TAL SAC
Total/NA	Analysis	537		1	185407	09/20/17 05:08	JRB	TAL SAC

## Client Sample ID: NAWC-091117-FRB-314

Date Collected: 09/11/17 10:20

Date Received: 09/12/17 14:21

## Lab Sample ID: 320-31468-6

Matrix: Water

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			184382	09/14/17 09:17	NS1	TAL SAC
Total/NA	Analysis	537		1	185407	09/20/17 05:13	JRB	TAL SAC

TestAmerica Sacramento

# Lab Chronicle

Client: Tetra Tech, Inc.  
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-31468-1

**Client Sample ID: NAWC-091117-RW-258**

**Lab Sample ID: 320-31468-7**

Date Collected: 09/11/17 11:00

Matrix: Water

Date Received: 09/12/17 14:21

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			184382	09/14/17 09:17	NS1	TAL SAC
Total/NA	Analysis	537		1	185407	09/20/17 05:18	JRB	TAL SAC

**Client Sample ID: NAWC-091117-FRB-258**

**Lab Sample ID: 320-31468-8**

Date Collected: 09/11/17 10:55

Matrix: Water

Date Received: 09/12/17 14:21

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			184382	09/14/17 09:17	NS1	TAL SAC
Total/NA	Analysis	537		1	185408	09/20/17 05:32	JRB	TAL SAC

**Client Sample ID: NAWC-091117-RW-048**

**Lab Sample ID: 320-31468-9**

Date Collected: 09/11/17 13:05

Matrix: Water

Date Received: 09/12/17 14:21

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			184382	09/14/17 09:17	NS1	TAL SAC
Total/NA	Analysis	537		1	185408	09/20/17 05:37	JRB	TAL SAC

**Client Sample ID: NAWC-091117-FRB-048**

**Lab Sample ID: 320-31468-10**

Date Collected: 09/11/17 13:00

Matrix: Water

Date Received: 09/12/17 14:21

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			184382	09/14/17 09:17	NS1	TAL SAC
Total/NA	Analysis	537		1	185408	09/20/17 05:42	JRB	TAL SAC

**Client Sample ID: NAWC-091117-RW-145**

**Lab Sample ID: 320-31468-11**

Date Collected: 09/11/17 13:35

Matrix: Water

Date Received: 09/12/17 14:21

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			184382	09/14/17 09:17	NS1	TAL SAC
Total/NA	Analysis	537		1	185408	09/20/17 05:46	JRB	TAL SAC

**Client Sample ID: NAWC-091117-FRB-145**

**Lab Sample ID: 320-31468-12**

Date Collected: 09/11/17 13:30

Matrix: Water

Date Received: 09/12/17 14:21

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			184382	09/14/17 09:17	NS1	TAL SAC
Total/NA	Analysis	537		1	185408	09/20/17 05:51	JRB	TAL SAC

TestAmerica Sacramento

# Lab Chronicle

Client: Tetra Tech, Inc.  
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-31468-1

**Client Sample ID: NAWC-091117-RW-317**

**Lab Sample ID: 320-31468-13**

Date Collected: 09/11/17 14:00

Matrix: Water

Date Received: 09/12/17 14:21

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			184382	09/14/17 09:17	NS1	TAL SAC
Total/NA	Analysis	537		1	185408	09/20/17 05:56	JRB	TAL SAC

**Client Sample ID: NAWC-091117-FRB-317**

**Lab Sample ID: 320-31468-14**

Date Collected: 09/11/17 13:55

Matrix: Water

Date Received: 09/12/17 14:21

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			184382	09/14/17 09:17	NS1	TAL SAC
Total/NA	Analysis	537		1	185408	09/20/17 06:01	JRB	TAL SAC

**Client Sample ID: NAWC-091117-RW-319**

**Lab Sample ID: 320-31468-15**

Date Collected: 09/11/17 14:25

Matrix: Water

Date Received: 09/12/17 14:21

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			184382	09/14/17 09:17	NS1	TAL SAC
Total/NA	Analysis	537		1	185408	09/20/17 06:05	JRB	TAL SAC

**Client Sample ID: NAWC-091117-FRB-319**

**Lab Sample ID: 320-31468-16**

Date Collected: 09/11/17 14:40

Matrix: Water

Date Received: 09/12/17 14:21

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			184382	09/14/17 09:17	NS1	TAL SAC
Total/NA	Analysis	537		1	185408	09/20/17 06:10	JRB	TAL SAC

**Client Sample ID: NAWC-091117-RW-321**

**Lab Sample ID: 320-31468-17**

Date Collected: 09/11/17 15:10

Matrix: Water

Date Received: 09/12/17 14:21

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			184382	09/14/17 09:17	NS1	TAL SAC
Total/NA	Analysis	537		1	185408	09/20/17 06:15	JRB	TAL SAC

**Client Sample ID: NAWC-091117-FRB-321**

**Lab Sample ID: 320-31468-18**

Date Collected: 09/11/17 15:05

Matrix: Water

Date Received: 09/12/17 14:21

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			184382	09/14/17 09:17	NS1	TAL SAC
Total/NA	Analysis	537		1	185409	09/20/17 06:29	JRB	TAL SAC

TestAmerica Sacramento

# Lab Chronicle

Client: Tetra Tech, Inc.  
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-31468-1

**Client Sample ID: NAWC-091117-RW-010**

**Lab Sample ID: 320-31468-19**

**Date Collected: 09/11/17 15:45**

**Matrix: Water**

**Date Received: 09/12/17 14:21**

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			184382	09/14/17 09:17	NS1	TAL SAC
Total/NA	Analysis	537		1	185409	09/20/17 06:34	JRB	TAL SAC

**Client Sample ID: NAWC-091117-FRB-010**

**Lab Sample ID: 320-31468-20**

**Date Collected: 09/11/17 15:40**

**Matrix: Water**

**Date Received: 09/12/17 14:21**

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			184382	09/14/17 09:17	NS1	TAL SAC
Total/NA	Analysis	537		1	185409	09/20/17 06:39	JRB	TAL SAC

**Client Sample ID: NAWC-091117-RW-162**

**Lab Sample ID: 320-31468-21**

**Date Collected: 09/11/17 11:20**

**Matrix: Water**

**Date Received: 09/12/17 14:21**

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			184385	09/14/17 09:29	CCB	TAL SAC
Total/NA	Analysis	537		1	185406	09/20/17 04:11	JRB	TAL SAC

**Client Sample ID: NAWC-091117-FRB-162**

**Lab Sample ID: 320-31468-22**

**Date Collected: 09/11/17 11:15**

**Matrix: Water**

**Date Received: 09/12/17 14:21**

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			184385	09/14/17 09:29	CCB	TAL SAC
Total/NA	Analysis	537		1	185406	09/20/17 04:16	JRB	TAL SAC

**Client Sample ID: WGNA-091117-DUP09**

**Lab Sample ID: 320-31468-23**

**Date Collected: 09/11/17 07:00**

**Matrix: Water**

**Date Received: 09/12/17 14:21**

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			184385	09/14/17 09:29	CCB	TAL SAC
Total/NA	Analysis	537		1	185406	09/20/17 04:21	JRB	TAL SAC

**Laboratory References:**

TAL SAC = TestAmerica Sacramento, 880 Riverside Parkway, West Sacramento, CA 95605, TEL (916)373-5600

# Accreditation/Certification Summary

Client: Tetra Tech, Inc.  
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-31468-1

## Laboratory: TestAmerica Sacramento

Unless otherwise noted, all analytes for this laboratory were covered under each accreditation/certification below.

Authority	Program	EPA Region	Identification Number	Expiration Date
Oregon	NELAP	10	4040	01-28-18

The following analytes are included in this report, but accreditation/certification is not offered by the governing authority:

Analysis Method	Prep Method	Matrix	Analyte
537	537	Water	Perfluorobutanesulfonic acid (PFBS)
537	537	Water	Perfluoroheptanoic acid (PFHpA)
537	537	Water	Perfluorohexanesulfonic acid (PFHxS)
537	537	Water	Perfluorononanoic acid (PFNA)
537	537	Water	Perfluorooctanesulfonic acid (PFOS)
537	537	Water	Perfluorooctanoic acid (PFOA)

# Method Summary

Client: Tetra Tech, Inc.  
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-31468-1

---

---

<b>Method</b>	<b>Method Description</b>	<b>Protocol</b>	<b>Laboratory</b>
537	Perfluorinated Alkyl Acids (LC/MS)	EPA	TAL SAC

**Protocol References:**

EPA = US Environmental Protection Agency

**Laboratory References:**

TAL SAC = TestAmerica Sacramento, 880 Riverside Parkway, West Sacramento, CA 95605, TEL (916)373-5600

# Sample Summary

Client: Tetra Tech, Inc.

TestAmerica Job ID: 320-31468-1

Project/Site: Warminster: PFAS, NAS JRB Willow Grove

Lab Sample ID	Client Sample ID	Matrix	Collected	Received
320-31468-1	NAWC-091117-RW-106	Water	09/11/17 09:40	09/12/17 14:21
320-31468-2	NAWC-091117-FRB-106	Water	09/11/17 09:35	09/12/17 14:21
320-31468-3	NAWC-091117-RW-060	Water	09/11/17 09:55	09/12/17 14:21
320-31468-4	NAWC-091117-FRB-060	Water	09/11/17 09:50	09/12/17 14:21
320-31468-5	NAWC-091117-RW-314	Water	09/11/17 10:25	09/12/17 14:21
320-31468-6	NAWC-091117-FRB-314	Water	09/11/17 10:20	09/12/17 14:21
320-31468-7	NAWC-091117-RW-258	Water	09/11/17 11:00	09/12/17 14:21
320-31468-8	NAWC-091117-FRB-258	Water	09/11/17 10:55	09/12/17 14:21
320-31468-9	NAWC-091117-RW-048	Water	09/11/17 13:05	09/12/17 14:21
320-31468-10	NAWC-091117-FRB-048	Water	09/11/17 13:00	09/12/17 14:21
320-31468-11	NAWC-091117-RW-145	Water	09/11/17 13:35	09/12/17 14:21
320-31468-12	NAWC-091117-FRB-145	Water	09/11/17 13:30	09/12/17 14:21
320-31468-13	NAWC-091117-RW-317	Water	09/11/17 14:00	09/12/17 14:21
320-31468-14	NAWC-091117-FRB-317	Water	09/11/17 13:55	09/12/17 14:21
320-31468-15	NAWC-091117-RW-319	Water	09/11/17 14:25	09/12/17 14:21
320-31468-16	NAWC-091117-FRB-319	Water	09/11/17 14:40	09/12/17 14:21
320-31468-17	NAWC-091117-RW-321	Water	09/11/17 15:10	09/12/17 14:21
320-31468-18	NAWC-091117-FRB-321	Water	09/11/17 15:05	09/12/17 14:21
320-31468-19	NAWC-091117-RW-010	Water	09/11/17 15:45	09/12/17 14:21
320-31468-20	NAWC-091117-FRB-010	Water	09/11/17 15:40	09/12/17 14:21
320-31468-21	NAWC-091117-RW-162	Water	09/11/17 11:20	09/12/17 14:21
320-31468-22	NAWC-091117-FRB-162	Water	09/11/17 11:15	09/12/17 14:21
320-31468-23	WGNA-091117-DUP09	Water	09/11/17 07:00	09/12/17 14:21

LCMS MANUAL INTEGRATION SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1

SDG No.: \_\_\_\_\_

Instrument ID: A8\_N Analysis Batch Number: 185329

Lab Sample ID: IC 320-185329/4 Client Sample ID: \_\_\_\_\_

Date Analyzed: 09/20/17 02:56 Lab File ID: 2017.09.19\_537ICAL\_004.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.11	Missed Peak	barnettj	09/20/17 10:03

Lab Sample ID: IC 320-185329/5 Client Sample ID: \_\_\_\_\_

Date Analyzed: 09/20/17 03:00 Lab File ID: 2017.09.19\_537ICAL\_005.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.11	Missed Peak	barnettj	09/20/17 10:04

Lab Sample ID: IC 320-185329/6 Client Sample ID: \_\_\_\_\_

Date Analyzed: 09/20/17 03:05 Lab File ID: 2017.09.19\_537ICAL\_006.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.10	Missed Peak	barnettj	09/20/17 10:05

Lab Sample ID: IC 320-185329/7 ICISAV Client Sample ID: \_\_\_\_\_

Date Analyzed: 09/20/17 03:10 Lab File ID: 2017.09.19\_537ICAL\_007.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.11	Missed Peak	barnettj	09/20/17 10:05



LCMS MANUAL INTEGRATION SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1

SDG No.: \_\_\_\_\_

Instrument ID: A8\_N Analysis Batch Number: 185329

Lab Sample ID: IC 320-185329/8 Client Sample ID: \_\_\_\_\_

Date Analyzed: 09/20/17 03:15 Lab File ID: 2017.09.19\_537ICAL\_008.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.11	Missed Peak	barnettj	09/20/17 10:06

Lab Sample ID: IC 320-185329/9 Client Sample ID: \_\_\_\_\_

Date Analyzed: 09/20/17 03:19 Lab File ID: 2017.09.19\_537ICAL\_009.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.11	Missed Peak	barnettj	09/20/17 10:07

Lab Sample ID: CCVL 320-185329/11 Client Sample ID: \_\_\_\_\_

Date Analyzed: 09/20/17 03:29 Lab File ID: 2017.09.19\_537ICAL\_011.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.10	Missed Peak	barnettj	09/20/17 10:10

Lab Sample ID: ICV 320-185329/13 Client Sample ID: \_\_\_\_\_

Date Analyzed: 09/20/17 03:38 Lab File ID: 2017.09.19\_537ICAL\_013.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.11	Missed Peak	barnettj	09/20/17 10:11

LCMS MANUAL INTEGRATION SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1

SDG No.: \_\_\_\_\_

Instrument ID: A8\_N Analysis Batch Number: 185406

Lab Sample ID: CCV 320-185406/1 CCVIS Client Sample ID: \_\_\_\_\_

Date Analyzed: 09/20/17 03:48 Lab File ID: 2017.09.19\_537A\_001.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.11	Missed Peak	barnettj	09/20/17 11:35

Lab Sample ID: LLCS 320-184385/2-A Client Sample ID: \_\_\_\_\_

Date Analyzed: 09/20/17 04:02 Lab File ID: 2017.09.19\_537A\_004.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.10	Missed Peak	barnettj	09/20/17 11:39

Lab Sample ID: LLCSD 320-184385/3-A Client Sample ID: \_\_\_\_\_

Date Analyzed: 09/20/17 04:07 Lab File ID: 2017.09.19\_537A\_005.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.10	Missed Peak	barnettj	09/20/17 11:40

Lab Sample ID: 320-31468-21 Client Sample ID: NAWC-091117-RW-162

Date Analyzed: 09/20/17 04:11 Lab File ID: 2017.09.19\_537A\_006.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.10	Missed Peak	barnettj	09/20/17 11:41

LCMS MANUAL INTEGRATION SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1

SDG No.: \_\_\_\_\_

Instrument ID: A8\_N Analysis Batch Number: 185406

Lab Sample ID: 320-31468-23 Client Sample ID: WGNA-091117-DUP09

Date Analyzed: 09/20/17 04:21 Lab File ID: 2017.09.19\_537A\_008.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluoroheptanoic acid (PFHpA)	1.66	Missed Peak	barnettj	09/20/17 11:42
Perfluorooctanesulfonic acid (PFOS)	2.01	Missed Peak	barnettj	09/20/17 11:41

Lab Sample ID: CCV 320-185406/9 CCVIS Client Sample ID: \_\_\_\_\_

Date Analyzed: 09/20/17 04:26 Lab File ID: 2017.09.19\_537A\_009.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.10	Missed Peak	barnettj	09/20/17 11:35

LCMS MANUAL INTEGRATION SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1

SDG No.: \_\_\_\_\_

Instrument ID: A8\_N Analysis Batch Number: 185407

Lab Sample ID: CCV 320-185407/9 CCVIS Client Sample ID: \_\_\_\_\_

Date Analyzed: 09/20/17 04:26 Lab File ID: 2017.09.19\_537A\_009.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.10	Missed Peak	barnettj	09/20/17 11:35

Lab Sample ID: LCS 320-184382/2-A Client Sample ID: \_\_\_\_\_

Date Analyzed: 09/20/17 04:40 Lab File ID: 2017.09.19\_537A\_012.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.09	Missed Peak	barnettj	09/20/17 13:22

Lab Sample ID: LCSD 320-184382/3-A Client Sample ID: \_\_\_\_\_

Date Analyzed: 09/20/17 04:45 Lab File ID: 2017.09.19\_537A\_013.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.10	Missed Peak	barnettj	09/20/17 13:23

Lab Sample ID: 320-31468-1 Client Sample ID: NAWC-091117-RW-106

Date Analyzed: 09/20/17 04:49 Lab File ID: 2017.09.19\_537A\_014.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.10	Missed Peak	barnettj	09/20/17 13:24

LCMS MANUAL INTEGRATION SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1

SDG No.: \_\_\_\_\_

Instrument ID: A8\_N Analysis Batch Number: 185407

Lab Sample ID: 320-31468-3 Client Sample ID: NAWC-091117-RW-060

Date Analyzed: 09/20/17 04:59 Lab File ID: 2017.09.19\_537A\_016.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.10	Missed Peak	barnettj	09/20/17 13:25

Lab Sample ID: 320-31468-5 Client Sample ID: NAWC-091117-RW-314

Date Analyzed: 09/20/17 05:08 Lab File ID: 2017.09.19\_537A\_018.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.10	Missed Peak	barnettj	09/20/17 13:26

Lab Sample ID: 320-31468-7 Client Sample ID: NAWC-091117-RW-258

Date Analyzed: 09/20/17 05:18 Lab File ID: 2017.09.19\_537A\_020.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.10	Missed Peak	barnettj	09/20/17 13:27

Lab Sample ID: CCV 320-185407/21 CCVIS Client Sample ID: \_\_\_\_\_

Date Analyzed: 09/20/17 05:23 Lab File ID: 2017.09.19\_537A\_021.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.10	Missed Peak	barnettj	09/20/17 13:27

LCMS MANUAL INTEGRATION SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1

SDG No.: \_\_\_\_\_

Instrument ID: A8\_N Analysis Batch Number: 185408

Lab Sample ID: CCV 320-185408/21 CCVIS Client Sample ID: \_\_\_\_\_

Date Analyzed: 09/20/17 05:23 Lab File ID: 2017.09.19\_537A\_021.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.10	Missed Peak	barnettj	09/20/17 13:27

Lab Sample ID: 320-31468-9 Client Sample ID: NAWC-091117-RW-048

Date Analyzed: 09/20/17 05:37 Lab File ID: 2017.09.19\_537A\_024.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanoic acid (PFOA)	1.85	Baseline	barnettj	09/20/17 13:30
Perfluorooctanesulfonic acid (PFOS)	2.01	Missed Peak	barnettj	09/20/17 13:30

Lab Sample ID: 320-31468-11 Client Sample ID: NAWC-091117-RW-145

Date Analyzed: 09/20/17 05:46 Lab File ID: 2017.09.19\_537A\_026.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.10	Missed Peak	barnettj	09/20/17 13:31

Lab Sample ID: 320-31468-13 Client Sample ID: NAWC-091117-RW-317

Date Analyzed: 09/20/17 05:56 Lab File ID: 2017.09.19\_537A\_028.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.09	Missed Peak	barnettj	09/20/17 13:32

LCMS MANUAL INTEGRATION SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1

SDG No.: \_\_\_\_\_

Instrument ID: A8\_N Analysis Batch Number: 185408

Lab Sample ID: 320-31468-15 Client Sample ID: NAWC-091117-RW-319

Date Analyzed: 09/20/17 06:05 Lab File ID: 2017.09.19\_537A\_030.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluoroheptanoic acid (PFHpA)	1.66	Baseline	barnettj	09/20/17 13:33
Perfluorooctanesulfonic acid (PFOS)	2.09	Missed Peak	barnettj	09/20/17 13:33

Lab Sample ID: 320-31468-17 Client Sample ID: NAWC-091117-RW-321

Date Analyzed: 09/20/17 06:15 Lab File ID: 2017.09.19\_537A\_032.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.09	Missed Peak	barnettj	09/20/17 13:34

LCMS MANUAL INTEGRATION SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1

SDG No.: \_\_\_\_\_

Instrument ID: A8\_N Analysis Batch Number: 185409

Lab Sample ID: 320-31468-19 Client Sample ID: NAWC-091117-RW-010

Date Analyzed: 09/20/17 06:34 Lab File ID: 2017.09.19\_537A\_036.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.09	Missed Peak	barnettj	09/20/17 13:36

Lab Sample ID: CCV 320-185409/38 CCVIS Client Sample ID: \_\_\_\_\_

Date Analyzed: 09/20/17 06:43 Lab File ID: 2017.09.19\_537A\_038.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.09	Missed Peak	barnettj	09/20/17 13:35



REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-31468-1

SDG No.: \_\_\_\_\_

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration		
					Reagent ID	Volume Added				
<b>LC537-HSP_00023</b>	02/10/18	08/10/17	Methanol, Lot 141039	20000 uL	LC537SPIM_00023	277.8 uL	Perfluorobutane Sulfonate	1250.1 ng/mL		
							Perfluorobutanesulfonic acid (PFBS)	1250.1 ng/mL		
							Perfluoroheptanoic acid (PFHpA)	138.923 ng/mL		
							Perfluorohexanesulfonic acid (PFHxS)	416.76 ng/mL		
							Perfluorononanoic acid (PFNA)	277.827 ng/mL		
							Perfluorooctanoic acid (PFOA)	278.01 ng/mL		
.LC537SPIM_00023	02/10/18	08/10/17	Methanol, Lot 104453	10000 uL	LC537-PFBS_00008	450 uL	Perfluorobutane Sulfonate	90 ug/mL		
							Perfluorobutanesulfonic acid (PFBS)	90 ug/mL		
							LC537-PFHpA_00015	100 uL	Perfluoroheptanoic acid (PFHpA)	10.0016 ug/mL
							LC537-PFHxS_00010	150 uL	Perfluorohexanesulfonic acid (PFHxS)	30.0043 ug/mL
							LC537-PFNA_00013	200 uL	Perfluorononanoic acid (PFNA)	20.002 ug/mL
							LC537-PFOA_00013	200 uL	Perfluorooctanoic acid (PFOA)	20.0151 ug/mL
..LC537-PFOS_00008	02/10/18	08/10/17	Methanol, Lot 090285	49.6 mL	LC537_PFOS_00002	0.0992 g	Perfluorobutane Sulfonate	2 mg/mL		
							Perfluorobutanesulfonic acid (PFBS)	2 mg/mL		
...LC537_PFOS_00002	04/01/18	Sigma, Lot MKBP8842V			(Purchased Reagent)		Perfluorobutane Sulfonate	1 g/g		
							Perfluorobutanesulfonic acid (PFBS)	1 g/g		
..LC537-PFHpA_00015	02/10/18	08/10/17	Methanol, Lot 090285	48.7 mL	LC537_PFHpA_00002	0.0492 g	Perfluoroheptanoic acid (PFHpA)	1.00016 mg/mL		
							...LC537_PFHpA_00002	04/01/18	Aldrich, Lot BCBM2579V	
..LC537-PFHxS_00010	02/10/18	08/10/17	Methanol, Lot 090285	55.92 mL	LC537_PFHxS_00002	0.123 g	Perfluorohexanesulfonic acid (PFHxS)	2.00029 mg/mL		
							...LC537_PFHxS_00002	04/01/18	Sigma, Lot BCBL3545V	
..LC537-PFNA_00013	02/10/18	08/10/17	Methanol, Lot 090285	62.3 mL	LC537 PFNA_00002	0.0647 g	Perfluorononanoic acid (PFNA)	1000.1 ug/mL		
							...LC537 PFNA_00002	04/01/18	TCI America, Lot QN44F	
..LC537-PFOA_00013	02/10/18	08/10/17	Methanol, Lot 090285	22.76 mL	LC537 PFOA_00003	0.0228 g	Perfluorooctanoic acid (PFOA)	1.00076 mg/mL		
							...LC537 PFOA_00003	10/31/23	SIGMA ALDRICH, Lot BCBS1198V	
..LC537-PFOS_00008	02/10/18	08/10/17	Methanol, Lot 090285	44.43 mL	LC537_PFOS_00003	0.0488 g	Perfluorooctanesulfonic acid (PFOS)	1.00016 mg/mL		
							...LC537_PFOS_00003	04/17/19	sigma alrich, Lot SZBE107XV	
<b>LC537-ICV_00028</b>	01/05/18	08/02/17	MeOH/H2O, Lot 067374	10 mL	LC537-IS_00045	1000 uL	13C2-PFOA	10 ng/mL		
							13C4 PFOS	28.68 ng/mL		
.LC537-IS_00045	01/05/18	07/05/17	Methanol, Lot 090285	30000 uL	LCM2PFOA_00007	60 uL	13C2-PFOA	0.1 ug/mL		
							LCMPFOS_00019	180 uL	13C4 PFOS	0.2868 ug/mL
..LCM2PFOA_00007	02/12/21	Wellington Laboratories, Lot M2PFOA0216			(Purchased Reagent)		13C2-PFOA	50 ug/mL		

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-31468-1

SDG No.: \_\_\_\_\_

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
..LCMPFOS 00019	08/03/21	Wellington Laboratories, Lot MPFOS0816			(Purchased Reagent)		13C4 PFOS	47.8 ug/mL
LC537-ICV_00028	01/05/18	08/02/17	MeOH/H2O, Lot 067374	10 mL	LC537-SU_00046	1000 uL	13C2 PFDA	10 ng/mL
							13C2 PFHxA	10 ng/mL
					LC537ICIM_00019	20 uL	Perfluorobutanesulfonic acid (PFBS)	100.119 ng/mL
							Perfluoroheptanoic acid (PFHpA)	9.99613 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	20.0761 ng/mL
							Perfluorononanoic acid (PFNA)	20.1272 ng/mL
							Perfluorooctanoic acid (PFOA)	20.4843 ng/mL
				Perfluorooctanesulfonic acid (PFOS)	19.698 ng/mL			
.LC537-SU_00046	01/05/18	07/05/17	Methanol, Lot 104453	30000 uL	LCMPFDA 00012	60 uL	13C2 PFDA	0.1 ug/mL
					LCMPFHxA 00013	60 uL	13C2 PFHxA	0.1 ug/mL
..LCMPFDA 00012	09/30/21	Wellington Laboratories, Lot MPFDA0916			(Purchased Reagent)		13C2 PFDA	50 ug/mL
..LCMPFHxA 00013	04/08/21	Wellington Laboratories, Lot MPFHxA0416			(Purchased Reagent)		13C2 PFHxA	50 ug/mL
.LC537ICIM_00019	01/25/18	08/01/17	Methanol, Lot 090285	25 mL	LC537-PFBS2_00008	0.6 mL	Perfluorobutanesulfonic acid (PFBS)	50.0597 ug/mL
					LC537-PFHpA2_00011	0.061 mL	Perfluoroheptanoic acid (PFHpA)	4.99806 ug/mL
					LC537-PFHxS2_00008	0.122 mL	Perfluorohexanesulfonic acid (PFHxS)	10.038 ug/mL
					LC537-PFNA2_00009	0.126 mL	Perfluorononanoic acid (PFNA)	10.0636 ug/mL
					LC537-PFOA2_00010	0.122 mL	Perfluorooctanoic acid (PFOA)	10.2421 ug/mL
					LC537-PFOS2_00010	0.124 mL	Perfluorooctanesulfonic acid (PFOS)	9.849 ug/mL
..LC537-PFBS2_00008	01/25/18	07/25/17	Methanol, Lot 090285	20 mL	LC537_PFBS2_00002	0.0418 g	Perfluorobutanesulfonic acid (PFBS)	2085.82 ug/mL
...LC537_PFBS2_00002	09/08/22	Santa Cruz Biotechnology, Lot F0917			(Purchased Reagent)		Perfluorobutanesulfonic acid (PFBS)	0.998 g/g
..LC537-PFHpA2_00011	01/25/18	07/25/17	Methanol, Lot 09092	31 mL	LC537_PFHpA2_00002	0.0635 g	Perfluoroheptanoic acid (PFHpA)	2048.39 ug/mL
...LC537_PFHpA2_00002	06/13/22	Afla Aesar, Lot 10200390			(Purchased Reagent)		Perfluoroheptanoic acid (PFHpA)	1 g/g
..LC537-PFHxS2_00008	01/25/18	07/25/17	Methanol, Lot 090285	21 mL	LC537_PFHxS2_00002	0.0475 g	Perfluorohexanesulfonic acid (PFHxS)	2056.98 ug/mL
...LC537_PFHxS2_00002	06/08/22	Santa Cruz Biotechnology, Lot G2516			(Purchased Reagent)		Perfluorohexanesulfonic acid (PFHxS)	0.9094 g/g
..LC537-PFNA2_00009	01/25/18	07/25/17	Methanol, Lot 090285	21 mL	LC537 PFNA2_00002	0.0421 g	Perfluorononanoic acid (PFNA)	1996.74 ug/mL
...LC537_PFNA2_00002	06/14/22	Aldrich, Lot MKCC0699			(Purchased Reagent)		Perfluorononanoic acid (PFNA)	0.996 g/g
..LC537-PFOA2_00010	01/25/18	08/01/17	Methanol, Lot 090285	20 mL	LC537 PFOA2_00002	0.0424 g	Perfluorooctanoic acid (PFOA)	2098.8 ug/mL
...LC537_PFOA2_00002	06/09/22	Afla Aesar, Lot 10199078			(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	0.99 g/g
..LC537-PFOS2_00010	01/25/18	08/01/17	Methanol, Lot 090285	22 mL	LC537_PFOS2_00002	0.0561 g	Perfluorooctanesulfonic acid (PFOS)	1985.68 ug/mL
...LC537_PFOS2_00002	06/14/22	Sigma, Lot BCBQ0108V			(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	0.7787 g/g
LC537-IS_00047	02/04/18	08/04/17	Methanol, Lot 090285	30000 uL	LCM2PFOA 00007	60 uL	13C2-PFOA	0.1 ug/mL
					LCMPFOS 00021	180 uL	13C4 PFOS	0.2868 ug/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-31468-1

SDG No.: \_\_\_\_\_

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration		
					Reagent ID	Volume Added				
.LCM2PFOA_00007	02/12/21		Wellington Laboratories, Lot M2PFOA0216			(Purchased Reagent)	13C2-PFOA	50 ug/mL		
.LCMPFOS_00021	12/12/21		Wellington Laboratories, Lot MPFOS1216			(Purchased Reagent)	13C4 PFOS	47.8 ug/mL		
LC537-L1_00020	02/04/18	08/14/17	MeOH/H2O, Lot 090285	5 mL	LC537-IS_00048	500 uL	13C2-PFOA	10 ng/mL		
							13C4 PFOS	28.68 ng/mL		
							Perfluorobutanesulfonic acid (PFBS)	9.0018 ng/mL		
							Perfluoroheptanoic acid (PFHpA)	1.00036 ng/mL		
					LC537-MSP_00029	60 uL	Perfluorohexanesulfonic acid (PFHxS)	3.00103 ng/mL		
							Perfluorononanoic acid (PFNA)	2.0006 ng/mL		
							Perfluorooctanoic acid (PFOA)	2.00191 ng/mL		
							Perfluorooctanesulfonic acid (PFOS)	4.00146 ng/mL		
LC537-SU_00049	500 uL	13C2 PFDA	10 ng/mL							
		13C2 PFHxA	10 ng/mL							
.LC537-IS_00048	02/04/18	08/04/17	Methanol, Lot 090285	30000 uL	LCM2PFOA_00007	60 uL	13C2-PFOA	0.1 ug/mL		
					LCMPFOS_00021	180 uL	13C4 PFOS	0.2868 ug/mL		
..LCM2PFOA_00007	02/12/21		Wellington Laboratories, Lot M2PFOA0216			(Purchased Reagent)	13C2-PFOA	50 ug/mL		
..LCMPFOS_00021	12/12/21		Wellington Laboratories, Lot MPFOS1216			(Purchased Reagent)	13C4 PFOS	47.8 ug/mL		
.LC537-MSP_00029	02/10/18	08/10/17	Methanol, Lot 141039	20000 uL	LC537SPIM_00023	166.7 uL	Perfluorobutanesulfonic acid (PFBS)	750.15 ng/mL		
							Perfluoroheptanoic acid (PFHpA)	83.3637 ng/mL		
							Perfluorohexanesulfonic acid (PFHxS)	250.086 ng/mL		
							Perfluorononanoic acid (PFNA)	166.716 ng/mL		
							Perfluorooctanoic acid (PFOA)	166.826 ng/mL		
							Perfluorooctanesulfonic acid (PFOS)	333.455 ng/mL		
..LC537SPIM_00023	02/10/18	08/10/17	Methanol, Lot 104453	10000 uL	LC537-PFBS_00008	450 uL	Perfluorobutanesulfonic acid (PFBS)	90 ug/mL		
							LC537-PFHpA_00015	100 uL	Perfluoroheptanoic acid (PFHpA)	10.0016 ug/mL
							LC537-PFHxS_00010	150 uL	Perfluorohexanesulfonic acid (PFHxS)	30.0043 ug/mL
							LC537-PFNA_00013	200 uL	Perfluorononanoic acid (PFNA)	20.002 ug/mL
							LC537-PFOA_00013	200 uL	Perfluorooctanoic acid (PFOA)	20.0151 ug/mL
							LC537-PFOS_00008	400 uL	Perfluorooctanesulfonic acid (PFOS)	40.0066 ug/mL
...LC537-PFBS_00008	02/10/18	08/10/17	Methanol, Lot 090285	49.6 mL	LC537_PFBS_00002	0.0992 g	Perfluorobutanesulfonic acid (PFBS)	2 mg/mL		
....LC537_PFBS_00002	04/01/18		Sigma, Lot MKBP8842V			(Purchased Reagent)	Perfluorobutanesulfonic acid (PFBS)	1 g/g		
...LC537-PFHpA_00015	02/10/18	08/10/17	Methanol, Lot 090285	48.7 mL	LC537_PFHpA_00002	0.0492 g	Perfluoroheptanoic acid (PFHpA)	1.00016 mg/mL		
....LC537_PFHpA_00002	04/01/18		Aldrich, Lot BCBM2579V			(Purchased Reagent)	Perfluoroheptanoic acid (PFHpA)	0.99 g/g		

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-31468-1

SDG No.: \_\_\_\_\_

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
...LC537-PFHxS_00010	02/10/18	08/10/17	Methanol, Lot 090285	55.92 mL	LC537_PFHxS_00002	0.123 g	Perfluorohexanesulfonic acid (PFHxS)	2.00029 mg/mL
....LC537_PFHxS_00002	04/01/18		Sigma, Lot BCBL3545V		(Purchased Reagent)		Perfluorohexanesulfonic acid (PFHxS)	0.9094 g/g
...LC537-PFNA 00013	02/10/18	08/10/17	Methanol, Lot 090285	62.3 mL	LC537 PFNA_00002	0.0647 g	Perfluorononanoic acid (PFNA)	1000.1 ug/mL
...LC537 PFNA 00002	04/01/18		TCI America, Lot QN44F		(Purchased Reagent)		Perfluorononanoic acid (PFNA)	0.963 g/g
...LC537-PFOA 00013	02/10/18	08/10/17	Methanol, Lot 090285	22.76 mL	LC537 PFOA_00003	0.0228 g	Perfluorooctanoic acid (PFOA)	1.00076 mg/mL
...LC537 PFOA 00003	10/31/23		SIGMA ALDRICH, Lot BCBS1198V		(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	0.999 g/g
...LC537-PFOS_00008	02/10/18	08/10/17	Methanol, Lot 090285	44.43 mL	LC537_PFOS_00003	0.0488 g	Perfluorooctanesulfonic acid (PFOS)	1.00016 mg/mL
....LC537_PFOS_00003	04/17/19		sigma alrich, Lot SZBE107XV		(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	0.9106 g/g
.LC537-SU_00049	02/04/18	08/04/17	Methanol, Lot 104453	30000 uL	LCMPFDA 00012	60 uL	13C2 PFDA	0.1 ug/mL
					LCMPFHxA 00013	60 uL	13C2 PFHxA	0.1 ug/mL
..LCMPFDA 00012	09/30/21		Wellington Laboratories, Lot MPFDA0916		(Purchased Reagent)		13C2 PFDA	50 ug/mL
..LCMPFHxA 00013	04/08/21		Wellington Laboratories, Lot MPFHxA0416		(Purchased Reagent)		13C2 PFHxA	50 ug/mL
<b>LC537-L2_00020</b>	02/04/18	08/14/17	MeOH/H2O, Lot 090285	5 mL	LC537-HSP_00025	80 uL	Perfluorobutanesulfonic acid (PFBS)	20.0016 ng/mL
							Perfluoroheptanoic acid (PFHpA)	2.22277 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	6.66817 ng/mL
							Perfluorononanoic acid (PFNA)	4.44524 ng/mL
							Perfluorooctanoic acid (PFOA)	4.44816 ng/mL
							Perfluorooctanesulfonic acid (PFOS)	8.89106 ng/mL
					LC537-IS_00048	500 uL	13C2-PFOA	10 ng/mL
							13C4 PFOS	28.68 ng/mL
					LC537-SU_00049	500 uL	13C2 PFDA	10 ng/mL
							13C2 PFHxA	10 ng/mL
.LC537-HSP_00025	02/10/18	08/10/17	Methanol, Lot 141039	20000 uL	LC537SPIM_00023	277.8 uL	Perfluorobutanesulfonic acid (PFBS)	1250.1 ng/mL
							Perfluoroheptanoic acid (PFHpA)	138.923 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	416.76 ng/mL
							Perfluorononanoic acid (PFNA)	277.827 ng/mL
							Perfluorooctanoic acid (PFOA)	278.01 ng/mL
							Perfluorooctanesulfonic acid (PFOS)	555.691 ng/mL
..LC537SPIM_00023	02/10/18	08/10/17	Methanol, Lot 104453	10000 uL	LC537-PFBS_00008	450 uL	Perfluorobutanesulfonic acid (PFBS)	90 ug/mL
					LC537-PFHxA_00015	100 uL	Perfluoroheptanoic acid (PFHpA)	10.0016 ug/mL
					LC537-PFHxS_00010	150 uL	Perfluorohexanesulfonic acid (PFHxS)	30.0043 ug/mL
					LC537-PFNA_00013	200 uL	Perfluorononanoic acid (PFNA)	20.002 ug/mL
					LC537-PFOA_00013	200 uL	Perfluorooctanoic acid (PFOA)	20.0151 ug/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-31468-1

SDG No.:

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
					LC537-PFOS_00008	400 uL	Perfluorooctanesulfonic acid (PFOS)	40.0066 ug/mL
...LC537-PFBS_00008	02/10/18	08/10/17	Methanol, Lot 090285	49.6 mL	LC537_PFB_00002	0.0992 g	Perfluorobutanesulfonic acid (PFBS)	2 mg/mL
....LC537_PFB_00002	04/01/18		Sigma, Lot MKBP8842V		(Purchased Reagent)		Perfluorobutanesulfonic acid (PFBS)	1 g/g
...LC537-PFHpA_00015	02/10/18	08/10/17	Methanol, Lot 090285	48.7 mL	LC537_PFHpA_00002	0.0492 g	Perfluoroheptanoic acid (PFHpA)	1.00016 mg/mL
....LC537_PFHpA_00002	04/01/18		Aldrich, Lot BCM2579V		(Purchased Reagent)		Perfluoroheptanoic acid (PFHpA)	0.99 g/g
...LC537-PFHxS_00010	02/10/18	08/10/17	Methanol, Lot 090285	55.92 mL	LC537_PFHxS_00002	0.123 g	Perfluorohexanesulfonic acid (PFHxS)	2.00029 mg/mL
....LC537_PFHxS_00002	04/01/18		Sigma, Lot BCBL3545V		(Purchased Reagent)		Perfluorohexanesulfonic acid (PFHxS)	0.9094 g/g
...LC537-PFNA_00013	02/10/18	08/10/17	Methanol, Lot 090285	62.3 mL	LC537 PFNA_00002	0.0647 g	Perfluorononanoic acid (PFNA)	1000.1 ug/mL
....LC537 PFNA_00002	04/01/18		TCI America, Lot QN44F		(Purchased Reagent)		Perfluorononanoic acid (PFNA)	0.963 g/g
...LC537-PFOA_00013	02/10/18	08/10/17	Methanol, Lot 090285	22.76 mL	LC537_PFOA_00003	0.0228 g	Perfluorooctanoic acid (PFOA)	1.00076 mg/mL
....LC537_PFOA_00003	10/31/23		SIGMA ALDRICH, Lot BCBS1198V		(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	0.999 g/g
...LC537-PFOS_00008	02/10/18	08/10/17	Methanol, Lot 090285	44.43 mL	LC537_PFOS_00003	0.0488 g	Perfluorooctanesulfonic acid (PFOS)	1.00016 mg/mL
....LC537_PFOS_00003	04/17/19		sigma alrich, Lot SZBE107XV		(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	0.9106 g/g
.LC537-IS_00048	02/04/18	08/04/17	Methanol, Lot 090285	30000 uL	LCM2PFOA_00007	60 uL	13C2-PFOA	0.1 ug/mL
					LCMPFOS_00021	180 uL	13C4 PFOS	0.2868 ug/mL
..LCM2PFOA_00007	02/12/21		Wellington Laboratories, Lot M2PFOA0216		(Purchased Reagent)		13C2-PFOA	50 ug/mL
..LCMPFOS_00021	12/12/21		Wellington Laboratories, Lot MPFOS1216		(Purchased Reagent)		13C4 PFOS	47.8 ug/mL
.LC537-SU_00049	02/04/18	08/04/17	Methanol, Lot 104453	30000 uL	LCMPFDA_00012	60 uL	13C2 PFDA	0.1 ug/mL
					LCMPFHxA_00013	60 uL	13C2 PFHxA	0.1 ug/mL
..LCMPFDA_00012	09/30/21		Wellington Laboratories, Lot MPFDA0916		(Purchased Reagent)		13C2 PFDA	50 ug/mL
..LCMPFHxA_00013	04/08/21		Wellington Laboratories, Lot MPFHxA0416		(Purchased Reagent)		13C2 PFHxA	50 ug/mL
<b>LC537-L3_00023</b>	02/04/18	08/14/17	MeOH/H2O, Lot 090285	5 mL	LC537-HSP_00025	180 uL	Perfluorobutanesulfonic acid (PFBS)	45.0036 ng/mL
							Perfluoroheptanoic acid (PFHpA)	5.00122 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	15.0034 ng/mL
							Perfluorononanoic acid (PFNA)	10.0018 ng/mL
							Perfluorooctanoic acid (PFOA)	10.0084 ng/mL
							Perfluorooctanesulfonic acid (PFOS)	20.0049 ng/mL
					LC537-IS_00048	500 uL	13C2-PFOA	10 ng/mL
							13C4 PFOS	28.68 ng/mL
					LC537-SU_00049	500 uL	13C2 PFDA	10 ng/mL
							13C2 PFHxA	10 ng/mL
.LC537-HSP_00025	02/10/18	08/10/17	Methanol, Lot 141039	20000 uL	LC537SPIM_00023	277.8 uL	Perfluorobutanesulfonic acid (PFBS)	1250.1 ng/mL
							Perfluoroheptanoic acid (PFHpA)	138.923 ng/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-31468-1

SDG No.: \_\_\_\_\_

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration	
					Reagent ID	Volume Added			
							Perfluorohexanesulfonic acid (PFHxS)	416.76 ng/mL	
							Perfluorononanoic acid (PFNA)	277.827 ng/mL	
							Perfluorooctanoic acid (PFOA)	278.01 ng/mL	
							Perfluorooctanesulfonic acid (PFOS)	555.691 ng/mL	
..LC537SPIM_00023	02/10/18	08/10/17	Methanol, Lot 104453	10000 uL	LC537-PFBS_00008	450 uL	Perfluorobutanesulfonic acid (PFBS)	90 ug/mL	
						LC537-PFHpA_00015	100 uL	Perfluoroheptanoic acid (PFHpA)	10.0016 ug/mL
						LC537-PFHxS_00010	150 uL	Perfluorohexanesulfonic acid (PFHxS)	30.0043 ug/mL
						LC537-PFNA_00013	200 uL	Perfluorononanoic acid (PFNA)	20.002 ug/mL
						LC537-PFOA_00013	200 uL	Perfluorooctanoic acid (PFOA)	20.0151 ug/mL
						LC537-PFOS_00008	400 uL	Perfluorooctanesulfonic acid (PFOS)	40.0066 ug/mL
...LC537-PFBS_00008	02/10/18	08/10/17	Methanol, Lot 090285	49.6 mL	LC537_PFBS_00002	0.0992 g	Perfluorobutanesulfonic acid (PFBS)	2 mg/mL	
....LC537_PFBS_00002	04/01/18		Sigma, Lot MKBP8842V		(Purchased Reagent)		Perfluorobutanesulfonic acid (PFBS)	1 g/g	
...LC537-PFHpA_00015	02/10/18	08/10/17	Methanol, Lot 090285	48.7 mL	LC537_PFHpA_00002	0.0492 g	Perfluoroheptanoic acid (PFHpA)	1.00016 mg/mL	
....LC537_PFHpA_00002	04/01/18		Aldrich, Lot BCBM2579V		(Purchased Reagent)		Perfluoroheptanoic acid (PFHpA)	0.99 g/g	
...LC537-PFHxS_00010	02/10/18	08/10/17	Methanol, Lot 090285	55.92 mL	LC537_PFHxS_00002	0.123 g	Perfluorohexanesulfonic acid (PFHxS)	2.00029 mg/mL	
....LC537_PFHxS_00002	04/01/18		Sigma, Lot BCBL3545V		(Purchased Reagent)		Perfluorohexanesulfonic acid (PFHxS)	0.9094 g/g	
...LC537-PFNA_00013	02/10/18	08/10/17	Methanol, Lot 090285	62.3 mL	LC537 PFNA_00002	0.0647 g	Perfluorononanoic acid (PFNA)	1000.1 ug/mL	
....LC537 PFNA_00002	04/01/18		TCI America, Lot QN44F		(Purchased Reagent)		Perfluorononanoic acid (PFNA)	0.963 g/g	
...LC537-PFOA_00013	02/10/18	08/10/17	Methanol, Lot 090285	22.76 mL	LC537 PFOA_00003	0.0228 g	Perfluorooctanoic acid (PFOA)	1.00076 mg/mL	
....LC537 PFOA_00003	10/31/23		SIGMA ALDRICH, Lot BCBS1198V		(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	0.999 g/g	
...LC537-PFOS_00008	02/10/18	08/10/17	Methanol, Lot 090285	44.43 mL	LC537_PFOS_00003	0.0488 g	Perfluorooctanesulfonic acid (PFOS)	1.00016 mg/mL	
....LC537_PFOS_00003	04/17/19		sigma alrich, Lot SZBE107XV		(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	0.9106 g/g	
.LC537-IS_00048	02/04/18	08/04/17	Methanol, Lot 090285	30000 uL	LCM2PFOA_00007	60 uL	13C2-PFOA	0.1 ug/mL	
					LCMPFOS_00021	180 uL	13C4 PFOS	0.2868 ug/mL	
..LCM2PFOA_00007	02/12/21		Wellington Laboratories, Lot M2PFOA0216		(Purchased Reagent)		13C2-PFOA	50 ug/mL	
..LCMPFOS_00021	12/12/21		Wellington Laboratories, Lot MPFOS1216		(Purchased Reagent)		13C4 PFOS	47.8 ug/mL	
.LC537-SU_00049	02/04/18	08/04/17	Methanol, Lot 104453	30000 uL	LCMPFDA_00012	60 uL	13C2 PFDA	0.1 ug/mL	
					LCMPFHxA_00013	60 uL	13C2 PFHxA	0.1 ug/mL	
..LCMPFDA_00012	09/30/21		Wellington Laboratories, Lot MPFDA0916		(Purchased Reagent)		13C2 PFDA	50 ug/mL	
..LCMPFHxA_00013	04/08/21		Wellington Laboratories, Lot MPFHxA0416		(Purchased Reagent)		13C2 PFHxA	50 ug/mL	
<b>LC537-L4_00020</b>	02/04/18	08/14/17	MeOH/H2O, Lot 090285	5 mL	LC537-HSP_00025	360 uL	Perfluorobutanesulfonic acid (PFBS)	90.0072 ng/mL	
							Perfluoroheptanoic acid (PFHpA)	10.0024 ng/mL	

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-31468-1

SDG No.: \_\_\_\_\_

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration		
					Reagent ID	Volume Added				
							Perfluorohexanesulfonic acid (PFHxS)	30.0067 ng/mL		
							Perfluorononanoic acid (PFNA)	20.0036 ng/mL		
							Perfluorooctanoic acid (PFOA)	20.0167 ng/mL		
							Perfluorooctanesulfonic acid (PFOS)	40.0098 ng/mL		
							LC537-IS_00048	500 uL	13C2-PFOA	10 ng/mL
									13C4 PFOS	28.68 ng/mL
..LC537-HSP_00025	02/10/18	08/10/17	Methanol, Lot 141039	20000 uL	LC537SPIM_00023	277.8 uL	13C2 PFDA	10 ng/mL		
							13C2 PFHxA	10 ng/mL		
							Perfluorobutanesulfonic acid (PFBS)	1250.1 ng/mL		
							Perfluoroheptanoic acid (PFHpA)	138.923 ng/mL		
							Perfluorohexanesulfonic acid (PFHxS)	416.76 ng/mL		
							Perfluorononanoic acid (PFNA)	277.827 ng/mL		
Perfluorooctanoic acid (PFOA)	278.01 ng/mL									
Perfluorooctanesulfonic acid (PFOS)	555.691 ng/mL									
..LC537SPIM_00023	02/10/18	08/10/17	Methanol, Lot 104453	10000 uL	LC537-PFBS_00008	450 uL	Perfluorobutanesulfonic acid (PFBS)	90 ug/mL		
							LC537-PFHpA_00015	100 uL	Perfluoroheptanoic acid (PFHpA)	10.0016 ug/mL
							LC537-PFHxS_00010	150 uL	Perfluorohexanesulfonic acid (PFHxS)	30.0043 ug/mL
							LC537-PFNA_00013	200 uL	Perfluorononanoic acid (PFNA)	20.002 ug/mL
							LC537-PFOA_00013	200 uL	Perfluorooctanoic acid (PFOA)	20.0151 ug/mL
							LC537-PFOS_00008	400 uL	Perfluorooctanesulfonic acid (PFOS)	40.0066 ug/mL
...LC537-PFBS_00008	02/10/18	08/10/17	Methanol, Lot 090285	49.6 mL	LC537_PFBS_00002	0.0992 g	Perfluorobutanesulfonic acid (PFBS)	2 mg/mL		
....LC537_PFBS_00002	04/01/18	Sigma, Lot MKBP8842V			(Purchased Reagent)		Perfluorobutanesulfonic acid (PFBS)	1 g/g		
...LC537-PFHpA_00015	02/10/18	08/10/17	Methanol, Lot 090285	48.7 mL	LC537_PFHpA_00002	0.0492 g	Perfluoroheptanoic acid (PFHpA)	1.00016 mg/mL		
....LC537_PFHpA_00002	04/01/18	Aldrich, Lot BCBM2579V			(Purchased Reagent)		Perfluoroheptanoic acid (PFHpA)	0.99 g/g		
...LC537-PFHxS_00010	02/10/18	08/10/17	Methanol, Lot 090285	55.92 mL	LC537_PFHxS_00002	0.123 g	Perfluorohexanesulfonic acid (PFHxS)	2.00029 mg/mL		
....LC537_PFHxS_00002	04/01/18	Sigma, Lot BCBL3545V			(Purchased Reagent)		Perfluorohexanesulfonic acid (PFHxS)	0.9094 g/g		
...LC537-PFNA_00013	02/10/18	08/10/17	Methanol, Lot 090285	62.3 mL	LC537 PFNA_00002	0.0647 g	Perfluorononanoic acid (PFNA)	1000.1 ug/mL		
....LC537 PFNA_00002	04/01/18	TCI America, Lot QN44F			(Purchased Reagent)		Perfluorononanoic acid (PFNA)	0.963 g/g		
...LC537-PFOA_00013	02/10/18	08/10/17	Methanol, Lot 090285	22.76 mL	LC537 PFOA_00003	0.0228 g	Perfluorooctanoic acid (PFOA)	1.00076 mg/mL		
....LC537 PFOA_00003	10/31/23	SIGMA ALDRICH, Lot BCBS1198V			(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	0.999 g/g		
...LC537-PFOS_00008	02/10/18	08/10/17	Methanol, Lot 090285	44.43 mL	LC537_PFOS_00003	0.0488 g	Perfluorooctanesulfonic acid (PFOS)	1.00016 mg/mL		
....LC537_PFOS_00003	04/17/19	sigma alrich, Lot SZBE107XV			(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	0.9106 g/g		

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-31468-1

SDG No.: \_\_\_\_\_

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
.LC537-IS_00048	02/04/18	08/04/17	Methanol, Lot 090285	30000 uL	LCM2PFOA_00007	60 uL	13C2-PFOA	0.1 ug/mL
					LCMPFOS_00021	180 uL	13C4 PFOS	0.2868 ug/mL
..LCM2PFOA_00007	02/12/21	Wellington Laboratories, Lot M2PFOA0216			(Purchased Reagent)		13C2-PFOA	50 ug/mL
..LCMPFOS_00021	12/12/21	Wellington Laboratories, Lot MPFOS1216			(Purchased Reagent)		13C4 PFOS	47.8 ug/mL
.LC537-SU_00049	02/04/18	08/04/17	Methanol, Lot 104453	30000 uL	LCMPFDA_00012	60 uL	13C2 PFDA	0.1 ug/mL
					LCMPFHxA_00013	60 uL	13C2 PFHxA	0.1 ug/mL
..LCMPFDA_00012	09/30/21	Wellington Laboratories, Lot MPFDA0916			(Purchased Reagent)		13C2 PFDA	50 ug/mL
..LCMPFHxA_00013	04/08/21	Wellington Laboratories, Lot MPFHxA0416			(Purchased Reagent)		13C2 PFHxA	50 ug/mL
<b>LC537-L5_00024</b>	02/04/18	08/14/17	MeOH/H2O, Lot 090285	5 mL	LC537-HSP_00025	540 uL	Perfluorobutanesulfonic acid (PFBS)	135.011 ng/mL
							Perfluoroheptanoic acid (PFHpA)	15.0037 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	45.0101 ng/mL
							Perfluorononanoic acid (PFNA)	30.0053 ng/mL
							Perfluorooctanoic acid (PFOA)	30.0251 ng/mL
							Perfluorooctanesulfonic acid (PFOS)	60.0146 ng/mL
					LC537-IS_00048	500 uL	13C2-PFOA	10 ng/mL
							13C4 PFOS	28.68 ng/mL
					LC537-SU_00049	500 uL	13C2 PFDA	10 ng/mL
							13C2 PFHxA	10 ng/mL
.LC537-HSP_00025	02/10/18	08/10/17	Methanol, Lot 141039	20000 uL	LC537SPIM_00023	277.8 uL	Perfluorobutanesulfonic acid (PFBS)	1250.1 ng/mL
							Perfluoroheptanoic acid (PFHpA)	138.923 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	416.76 ng/mL
							Perfluorononanoic acid (PFNA)	277.827 ng/mL
							Perfluorooctanoic acid (PFOA)	278.01 ng/mL
							Perfluorooctanesulfonic acid (PFOS)	555.691 ng/mL
..LC537SPIM_00023	02/10/18	08/10/17	Methanol, Lot 104453	10000 uL	LC537-PFBS_00008	450 uL	Perfluorobutanesulfonic acid (PFBS)	90 ug/mL
					LC537-PFHpA_00015	100 uL	Perfluoroheptanoic acid (PFHpA)	10.0016 ug/mL
					LC537-PFHxS_00010	150 uL	Perfluorohexanesulfonic acid (PFHxS)	30.0043 ug/mL
					LC537-PFNA_00013	200 uL	Perfluorononanoic acid (PFNA)	20.002 ug/mL
					LC537-PFOA_00013	200 uL	Perfluorooctanoic acid (PFOA)	20.0151 ug/mL
					LC537-PFOS_00008	400 uL	Perfluorooctanesulfonic acid (PFOS)	40.0066 ug/mL
...LC537-PFBS_00008	02/10/18	08/10/17	Methanol, Lot 090285	49.6 mL	LC537_PFBS_00002	0.0992 g	Perfluorobutanesulfonic acid (PFBS)	2 mg/mL
....LC537_PFBS_00002	04/01/18	Sigma, Lot MKBP8842V			(Purchased Reagent)		Perfluorobutanesulfonic acid (PFBS)	1 g/g
..LC537-PFHpA_00015	02/10/18	08/10/17	Methanol, Lot 090285	48.7 mL	LC537_PFHpA_00002	0.0492 g	Perfluoroheptanoic acid (PFHpA)	1.00016 mg/mL



REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-31468-1

SDG No.: \_\_\_\_\_

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
....LC537_PFHpA_00002	04/01/18		Aldrich, Lot BCM2579V		(Purchased Reagent)		Perfluoroheptanoic acid (PFHpA)	0.99 g/g
...LC537-PFHxS_00010	02/10/18	08/10/17	Methanol, Lot 090285	55.92 mL	LC537_PFHxS_00002	0.123 g	Perfluorohexanesulfonic acid (PFHxS)	2.00029 mg/mL
....LC537_PFHxS_00002	04/01/18		Sigma, Lot BCBL3545V		(Purchased Reagent)		Perfluorohexanesulfonic acid (PFHxS)	0.9094 g/g
...LC537-PFNA_00013	02/10/18	08/10/17	Methanol, Lot 090285	62.3 mL	LC537_PFNA_00002	0.0647 g	Perfluorononanoic acid (PFNA)	1000.1 ug/mL
....LC537 PFNA_00002	04/01/18		TCI America, Lot QN44F		(Purchased Reagent)		Perfluorononanoic acid (PFNA)	0.963 g/g
...LC537-PFOA_00013	02/10/18	08/10/17	Methanol, Lot 090285	22.76 mL	LC537_PFOA_00003	0.0228 g	Perfluorooctanoic acid (PFOA)	1.00076 mg/mL
....LC537_PFOA_00003	10/31/23		SIGMA ALDRICH, Lot BCBS1198V		(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	0.999 g/g
...LC537-PFOS_00008	02/10/18	08/10/17	Methanol, Lot 090285	44.43 mL	LC537_PFOS_00003	0.0488 g	Perfluorooctanesulfonic acid (PFOS)	1.00016 mg/mL
....LC537_PFOS_00003	04/17/19		sigma alrich, Lot SZBE107XV		(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	0.9106 g/g
.LC537-IS_00048	02/04/18	08/04/17	Methanol, Lot 090285	30000 uL	LCM2PFOA_00007	60 uL	13C2-PFOA	0.1 ug/mL
..LCM2PFOA_00007	02/12/21		Wellington Laboratories, Lot M2PFOA0216		(Purchased Reagent)		13C2-PFOA	50 ug/mL
..LCMPFOS_00021	12/12/21		Wellington Laboratories, Lot MPFOS1216		(Purchased Reagent)		13C4 PFOS	47.8 ug/mL
.LC537-SU_00049	02/04/18	08/04/17	Methanol, Lot 104453	30000 uL	LCMPFDA_00012	60 uL	13C2 PFDA	0.1 ug/mL
..LCMPFDA_00012	09/30/21		Wellington Laboratories, Lot MPFDA0916		(Purchased Reagent)		13C2 PFDA	50 ug/mL
..LCMPFHxA_00013	04/08/21		Wellington Laboratories, Lot MPFHxA0416		(Purchased Reagent)		13C2 PFHxA	50 ug/mL
<b>LC537-L6_00020</b>	02/04/18	08/14/17	MeOH/H2O, Lot 090285	5 mL	LC537-HSP_00025	720 uL	Perfluorobutanesulfonic acid (PFBS)	180.014 ng/mL
							Perfluoroheptanoic acid (PFHpA)	20.0049 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	60.0135 ng/mL
							Perfluorononanoic acid (PFNA)	40.0071 ng/mL
							Perfluorooctanoic acid (PFOA)	40.0334 ng/mL
							Perfluorooctanesulfonic acid (PFOS)	80.0195 ng/mL
					LC537-IS_00048	500 uL	13C2-PFOA	10 ng/mL
							13C4 PFOS	28.68 ng/mL
					LC537-SU_00049	500 uL	13C2 PFDA	10 ng/mL
							13C2 PFHxA	10 ng/mL
.LC537-HSP_00025	02/10/18	08/10/17	Methanol, Lot 141039	20000 uL	LC537SPIM_00023	277.8 uL	Perfluorobutanesulfonic acid (PFBS)	1250.1 ng/mL
							Perfluoroheptanoic acid (PFHpA)	138.923 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	416.76 ng/mL
							Perfluorononanoic acid (PFNA)	277.827 ng/mL
							Perfluorooctanoic acid (PFOA)	278.01 ng/mL
							Perfluorooctanesulfonic acid (PFOS)	555.691 ng/mL
..LC537SPIM_00023	02/10/18	08/10/17	Methanol, Lot 104453	10000 uL	LC537-PFBS_00008	450 uL	Perfluorobutanesulfonic acid (PFBS)	90 ug/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-31468-1

SDG No.: \_\_\_\_\_

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
					LC537-PFHpA_00015	100 uL	Perfluoroheptanoic acid (PFHpA)	10.0016 ug/mL
					LC537-PFHxS_00010	150 uL	Perfluorohexanesulfonic acid (PFHxS)	30.0043 ug/mL
					LC537-PFNA_00013	200 uL	Perfluorononanoic acid (PFNA)	20.002 ug/mL
					LC537-PFOA_00013	200 uL	Perfluorooctanoic acid (PFOA)	20.0151 ug/mL
					LC537-PFOS_00008	400 uL	Perfluorooctanesulfonic acid (PFOS)	40.0066 ug/mL
...LC537-PFBS_00008	02/10/18	08/10/17	Methanol, Lot 090285	49.6 mL	LC537_PFBS_00002	0.0992 g	Perfluorobutanesulfonic acid (PFBS)	2 mg/mL
....LC537_PFBS_00002	04/01/18	Sigma, Lot MKBP8842V			(Purchased Reagent)		Perfluorobutanesulfonic acid (PFBS)	1 g/g
...LC537-PFHpA_00015	02/10/18	08/10/17	Methanol, Lot 090285	48.7 mL	LC537_PFHpA_00002	0.0492 g	Perfluoroheptanoic acid (PFHpA)	1.00016 mg/mL
....LC537_PFHpA_00002	04/01/18	Aldrich, Lot BCM2579V			(Purchased Reagent)		Perfluoroheptanoic acid (PFHpA)	0.99 g/g
...LC537-PFHxS_00010	02/10/18	08/10/17	Methanol, Lot 090285	55.92 mL	LC537_PFHxS_00002	0.123 g	Perfluorohexanesulfonic acid (PFHxS)	2.00029 mg/mL
....LC537_PFHxS_00002	04/01/18	Sigma, Lot BCBL3545V			(Purchased Reagent)		Perfluorohexanesulfonic acid (PFHxS)	0.9094 g/g
...LC537-PFNA_00013	02/10/18	08/10/17	Methanol, Lot 090285	62.3 mL	LC537_PFNA_00002	0.0647 g	Perfluorononanoic acid (PFNA)	1000.1 ug/mL
....LC537_PFNA_00002	04/01/18	TCI America, Lot QN44F			(Purchased Reagent)		Perfluorononanoic acid (PFNA)	0.963 g/g
...LC537-PFOA_00013	02/10/18	08/10/17	Methanol, Lot 090285	22.76 mL	LC537_PFOA_00003	0.0228 g	Perfluorooctanoic acid (PFOA)	1.00076 mg/mL
....LC537_PFOA_00003	10/31/23	SIGMA ALDRICH, Lot BCBS1198V			(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	0.999 g/g
...LC537-PFOS_00008	02/10/18	08/10/17	Methanol, Lot 090285	44.43 mL	LC537_PFOS_00003	0.0488 g	Perfluorooctanesulfonic acid (PFOS)	1.00016 mg/mL
....LC537_PFOS_00003	04/17/19	sigma alrich, Lot SZBE107XV			(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	0.9106 g/g
.LC537-IS_00048	02/04/18	08/04/17	Methanol, Lot 090285	30000 uL	LCM2PFOA_00007	60 uL	13C2-PFOA	0.1 ug/mL
..LCM2PFOA_00007	02/12/21	Wellington Laboratories, Lot M2PFOA0216			LCMPFOS_00021	180 uL	13C4 PFOS	0.2868 ug/mL
..LCMPFOS_00021	12/12/21	Wellington Laboratories, Lot MPFOS1216			(Purchased Reagent)		13C2-PFOA	50 ug/mL
.LC537-SU_00049	02/04/18	08/04/17	Methanol, Lot 104453	30000 uL	LCMPFDA_00012	60 uL	13C4 PFOS	47.8 ug/mL
..LCMPFDA_00012	09/30/21	Wellington Laboratories, Lot MPFDA0916			LCMPFHxA_00013	60 uL	13C2 PFDA	0.1 ug/mL
..LCMPFHxA_00013	04/08/21	Wellington Laboratories, Lot MPFHxA0416			(Purchased Reagent)		13C2 PFDA	50 ug/mL
..LCMPFHxA_00013	04/08/21	Wellington Laboratories, Lot MPFHxA0416			(Purchased Reagent)		13C2 PFHxA	50 ug/mL
<b>LC537-LSP_00025</b>	02/10/18	08/10/17	Methanol, Lot 090285	20000 uL	LC537SPIM_00023	50 uL	Perfluorobutane Sulfonate	225 ng/mL
							Perfluorobutanesulfonic acid (PFBS)	225 ng/mL
							Perfluoroheptanoic acid (PFHpA)	25.0041 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	75.0109 ng/mL
							Perfluorononanoic acid (PFNA)	50.0049 ng/mL
							Perfluorooctanoic acid (PFOA)	50.0378 ng/mL
							Perfluorooctanesulfonic acid (PFOS)	100.016 ng/mL
.LC537SPIM_00023	02/10/18	08/10/17	Methanol, Lot 104453	10000 uL	LC537-PFBS_00008	450 uL	Perfluorobutane Sulfonate	90 ug/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-31468-1

SDG No.: \_\_\_\_\_

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
							Perfluorobutanesulfonic acid (PFBS)	90 ug/mL
					LC537-PFHpA_00015	100 uL	Perfluoroheptanoic acid (PFHpA)	10.0016 ug/mL
					LC537-PFHxS_00010	150 uL	Perfluorohexanesulfonic acid (PFHxS)	30.0043 ug/mL
					LC537-PFNA_00013	200 uL	Perfluorononanoic acid (PFNA)	20.002 ug/mL
					LC537-PFOA_00013	200 uL	Perfluorooctanoic acid (PFOA)	20.0151 ug/mL
					LC537-PFOS_00008	400 uL	Perfluorooctanesulfonic acid (PFOS)	40.0066 ug/mL
..LC537-PFBS_00008	02/10/18	08/10/17	Methanol, Lot 090285	49.6 mL	LC537_PFBS_00002	0.0992 g	Perfluorobutane Sulfonate	2 mg/mL
							Perfluorobutanesulfonic acid (PFBS)	2 mg/mL
...LC537_PFBS_00002	04/01/18		Sigma, Lot MKBP8842V		(Purchased Reagent)		Perfluorobutane Sulfonate	1 g/g
							Perfluorobutanesulfonic acid (PFBS)	1 g/g
..LC537-PFHpA_00015	02/10/18	08/10/17	Methanol, Lot 090285	48.7 mL	LC537_PFHpA_00002	0.0492 g	Perfluoroheptanoic acid (PFHpA)	1.00016 mg/mL
...LC537_PFHpA_00002	04/01/18		Aldrich, Lot BCBM2579V		(Purchased Reagent)		Perfluoroheptanoic acid (PFHpA)	0.99 g/g
..LC537-PFHxS_00010	02/10/18	08/10/17	Methanol, Lot 090285	55.92 mL	LC537_PFHxS_00002	0.123 g	Perfluorohexanesulfonic acid (PFHxS)	2.00029 mg/mL
...LC537_PFHxS_00002	04/01/18		Sigma, Lot BCBL3545V		(Purchased Reagent)		Perfluorohexanesulfonic acid (PFHxS)	0.9094 g/g
..LC537-PFNA_00013	02/10/18	08/10/17	Methanol, Lot 090285	62.3 mL	LC537 PFNA_00002	0.0647 g	Perfluorononanoic acid (PFNA)	1000.1 ug/mL
...LC537 PFNA_00002	04/01/18		TCI America, Lot QN44F		(Purchased Reagent)		Perfluorononanoic acid (PFNA)	0.963 g/g
..LC537-PFOA_00013	02/10/18	08/10/17	Methanol, Lot 090285	22.76 mL	LC537 PFOA_00003	0.0228 g	Perfluorooctanoic acid (PFOA)	1.00076 mg/mL
...LC537 PFOA_00003	10/31/23		SIGMA ALDRICH, Lot BCBS1198V		(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	0.999 g/g
..LC537-PFOS_00008	02/10/18	08/10/17	Methanol, Lot 090285	44.43 mL	LC537_PFOS_00003	0.0488 g	Perfluorooctanesulfonic acid (PFOS)	1.00016 mg/mL
...LC537_PFOS_00003	04/17/19		sigma alrich, Lot SZBE107XV		(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	0.9106 g/g
<b>LC537-SU_00048</b>	02/04/18	08/04/17	Methanol, Lot 104453	30000 uL	LCMPFDA_00012	60 uL	13C2 PFDA	0.1 ug/mL
					LCMPFHxA_00013	60 uL	13C2 PFHxA	0.1 ug/mL
.LCMPFDA_00012	09/30/21		Wellington Laboratories, Lot MPFDA0916		(Purchased Reagent)		13C2 PFDA	50 ug/mL
.LCMPFHxA_00013	04/08/21		Wellington Laboratories, Lot MPFHxA0416		(Purchased Reagent)		13C2 PFHxA	50 ug/mL

Reagent

---

**LC537\_PFB\_S\_00002**

4/1/15 SPV

3050 Spruce Street, Saint Louis, MO 63103, USA

Website: www.sigmaaldrich.com

Email USA: techserv@sial.com


Outside USA: eurtechserv@sial.com

## Certificate of Analysis

Product Name:

Nonafluorobutane-1-sulfonic acid - 97%

**Product Number:** 562629  
**Batch Number:** MKBP8842V  
**Brand:** ALDRICH  
**CAS Number:** 375-73-5  
**MDL Number:** MFCD01320794  
**Formula:** C4HF9O3S  
**Formula Weight:** 300.10 g/mol  
**Storage Temperature:** Store at 2 - 8 °C  
**Quality Release Date:** 11 OCT 2013



PFBS

Test	Specification	Result
Appearance (Color)	Colorless	Colorless
Appearance (Form)	Liquid	Liquid
Infrared Spectrum	Conforms to Structure	Conforms
Fluorine NMR Spectrum	Conforms to Structure	Conforms
Purity (Titration by NaOH)	96.5 - 103.5 %	101.6 %

Jamie Gleason, Manager  
 Quality Control  
 Milwaukee, Wisconsin US


Sigma-Aldrich warrants, that at the time of the quality release or subsequent retest date this product conformed to the information contained in this publication. The current Specification sheet may be available at Sigma-Aldrich.com. For further inquiries, please contact Technical Service. Purchaser must determine the suitability of the product for its particular use. See reverse side of invoice or packing slip for additional terms and conditions of sale.

Reagent

---

**LC537\_PFB2\_00002**

F: 6.8.17 SW



# CERTIFICATE OF ANALYSIS

The Power to Question

Catalog Number: sc-236187  
Lot Number: F0917  
Product Name: Nonafluorobutane-1-sulfonic acid  
CAS Number: 375-73-5  
Molecular Formula:  $C_4HF_9O_3S$   
Molecular Weight: 300.10

Test	Specification	Result
Appearance	Colorless liquid	Complies
Identification (19F-NMR)	Conforms to structure	Complies
Purity (Sodium Hydroxide Titration)	$\geq 97\%$	101.3%
Infrared Spectrum	Conforms to structure	Complies

Reagent

---

**LC537\_PFHpA\_00002**



R: 4/1/15 4V

### Certificate of Analysis

**Product Name:** PERFLUOROHEPTANOIC ACID  
 99 %  
**Product Number:** 342041  
**Batch Number:** BCBM2579V  
**Brand:** Aldrich  
**CAS Number:** 375-85-9  
**Formula:**  $CF_3(CF_2)_5CO_2H$   
**Formula Weight:** 364.06  
**Quality Release Date:** 06 DEC 2013  
**Recommended Retest Date:** OCT 2018

PFHpA

TEST	SPECIFICATION	RESULT
APPEARANCE (COLOR)	COLORLESS OR WHITE	WHITE
APPEARANCE (FORM)	LIQUID OR SOLID	SOLID
TITRATION	98.5 - 101.5 %	99.8 %
TITRATION (METHOD)	-	BACK TITRATION
PURITY (GC AREA %)	≥ 98.5 %	99.5 %
INFRARED SPECTRUM	CONFORMS TO STRUCTURE	CONFORMS

Dr. Claudia Geitner  
 Manager Quality Control  
 Buchs, Switzerland

Sigma-Aldrich warrants that at the time of the quality release or subsequent retest date this product conformed to the information contained in this publication. The current specification sheet may be available at Sigma-Aldrich.com. For further inquiries, please contact Technical Service. Purchaser must determine the suitability of the product for its particular use. See reverse side of invoice or packing slip for additional terms and conditions of sale.

Reagent

---

**LC537\_PFHpA2\_00002**

# Certificate of analysis

r:6.13.17 SW

Product No.: A12092  
Product: Perfluoroheptanoic acid, 98+%  
Lot No.: 10200390

PFHe A

Appearance: White fused solid  
Water Content (Karl-Fischer): 0.30%  
Melting Point: 32.0-34.3°C  
Assay (Aqueous acid-base titration): 99.7%  
Identification (FTIR): Conforms

This document has been electronically generated and does not require a signature.

Order our products online [www.alfa.com](http://www.alfa.com)

**ThermoFisher**  
SCIENTIFIC

Reagent

---

**LC537\_PFHxS\_00002**

r: 4/1/15 stw

### Certificate of Analysis

**Product Name:** TRIDECAFLUOROHEXANE-1-SULFONIC ACID POTASSIUM SALT  
 >= 98.0 % T

**Product Number:** 50929

**Batch Number:** BCBL3545V

**Brand:** Aldrich

**CAS Number:** 3871-99-6

**Formula:** C<sub>6</sub>F<sub>13</sub>KO<sub>3</sub>S

**Formula Weight:** 438.20

**Quality Release Date:** 20 JUN 2013

PFH<sub>13</sub>S-K

TEST	SPECIFICATION	RESULT
APPEARANCE (COLOR)	WHITE TO FAINT BEIGE	WHITE
APPEARANCE (FORM)	POWDER OR CRYSTALS	POWDER
TITRATION (ION EXCHANGE)	≥ 98.0 %	99.5 %
INFRARED SPECTRUM	CONFORMS TO STRUCTURE	CONFORMS

Dr. Claudia Geitner  
Manager Quality Control  
Buchs, Switzerland

$$MW_{corr} = \frac{(k_{form}) - (k) + (H)}{438.20 (k_{form})} = \frac{(438.20 - 3910 + 101)}{438.20 (k_{form})} = 0.91307 \text{ (anion form)}$$

$$Purity = 90.94 \% \text{ w/m.w correction}$$

stw 4/1/15

Sigma-Aldrich warrants that at the time of the quality release or subsequent retest date this product conformed to the information contained in this publication. The current specification sheet may be available at Sigma-Aldrich.com. For further inquiries, please contact Technical Service. Purchaser must determine the suitability of the product for its particular use. See reverse side of invoice or packing slip for additional terms and conditions of sale.

Reagent

---

**LC537\_PFHxS2\_00002**

n: 6-8-17 SKJ




The Future of Science

# CERTIFICATE OF ANALYSIS

Catalog Number: sc-237289  
 Lot Number: G2516  
 Product Name: Tridecafluorohexane-1-sulfonic acid potassium salt  
 CAS Number: 3871-99-6  
 Molecular Formula:  $C_6F_{13}KO_3S$   
 Molecular Weight: 438.20

Test	Specification	Result
Appearance	White to faint beige powder or crystals	White powder
Identification (Infrared Spectrum)	Consistent with structure	Complies
Purity (Titration, Ion Exchange)	≥ 98.0%	100.4%

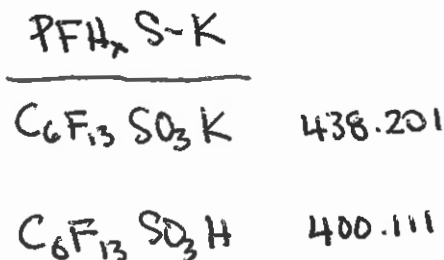

MW correction =  $\frac{400.11}{438.201} = 0.91307$  PFH<sub>13</sub>S  
 CAS# 355-46-4

Purity  $\frac{1}{9}$  MW correction = 90.9%

*This document was produced electronically and is valid without a signature.*

Reagent

---

**LC537\_PENA\_00002**



R: 4/1/15 SKV



### Certificate of Analysis

Apr 2, 2015 (JST)

TOKYO CHEMICAL INDUSTRY CO.,LTD.  
4-10-1 Nihonbashi-Honcho, Chuo-ku, Tokyo 103-0023 Japan

Chemical Name: Heptadecafluorononanoic Acid		
Product Number: H0843 CAS: 375-95-1	Lot: QN44F	

Tests	Results	Specifications
Purity(GC)	96.3 %	min. 95.0 %
Purity(Neutralization titration)	98.1 %	min. 95.0 %
Melting point	63.3 deg-C	62.0 to 67.0 deg-C

TCI Lot numbers are 4-5 characters in length.  
Characters listed after the first 4-5 characters are control numbers for internal purpose only.

**Customer service:**

TCI AMERICA  
Tel: +1-800-423-8616 / +1-503-283-1681  
Fax: +1-888-520-1075 / +1-503-283-1987  
E-mail: Sales-US@TCIchemicals.com

PFNA

Reagent

---

**LC537\_PFN2\_00002**

P: 6.14.17 SKW

3050 Spruce Street, Saint Louis, MO 63103, USA

Website: [www.sigmaaldrich.com](http://www.sigmaaldrich.com)


Email USA: [techserv@sial.com](mailto:techserv@sial.com)

Outside USA: [eurtechserv@sial.com](mailto:eurtechserv@sial.com)

## Certificate of Analysis

Product Name:  
Perfluorononanoic acid - 97%

Product Number: 394459  
Batch Number: MKCC0699  
Brand: ALDRICH  
CAS Number: 375-95-1  
MDL Number: MFCD00039605  
Formula: C9HF17O2  
Formula Weight: 464.08 g/mol  
Quality Release Date: 07 DEC 2016



Test	Specification	Result
Appearance (Color)	White to Off-White	White
Appearance (Form)	Powder or Crystals or Crystalline Chunk(s) or Granule or Flakes or Solid	Powder
Infrared Spectrum	Conforms to Structure	Conforms
GC (area %)	≥ 96.5 %	98.2 %

Michael Grady, Manager  
Quality Control  
Milwaukee, WI US

PFNA

Sigma-Aldrich warrants, that at the time of the quality release or subsequent retest date this product conformed to the information contained in this publication. The current Specification sheet may be available at Sigma-Aldrich.com. For further inquiries, please contact Technical Service. Purchaser must determine the suitability of the product for its particular use. See reverse side of Invoice or packing slip for additional terms and conditions of sale.

Reagent

---

**LC537\_PFOA\_00003**

P: 11/30/16 SKV  
PFA


**SIGMA-ALDRICH**

3050 Spruce Street, Saint Louis, MO 63103 USA  
Email USA: techserv@sial.com Outside USA: eurtechserv@sial.com

## Certificate of Analysis

**Product Name:** PENTADECAFLUOROOCCTANOIC ACID  
analytical standard  
**Product Number:** 33824  
**Batch Number:** BCBS1198V  
**Brand:** Sigma-Aldrich  
**CAS Number:** 335-67-1  
**Formula:**  $\text{CF}_3(\text{CF}_2)_6\text{COOH}$   
**Formula Weight:** 414.07  
**Expiration Date:** OCT 2023  
**Quality Release Date:** 12 MAY 2016

TEST	SPECIFICATION	RESULT
PURITY (HPLC AREA %)	≥ 98.0%	100.0%
IDENTIFICATION (LC-MS)	IDENTITY CONFORMS	CONFORMS

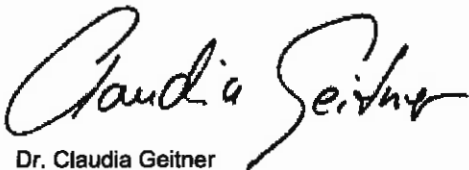

Dr. Claudia Geitner  
Manager Quality Control  
Buchs, Switzerland

Sigma-Aldrich warrants that at the time of the quality release or subsequent retest date this product conformed to the information contained in this publication. The current specification sheet may be available at Sigma-Aldrich.com. For further inquiries, please contact Technical Service. Purchaser must determine the suitability of the product for its particular use. See reverse side of invoice or packing slip for additional terms and conditions of sale.

Reagent

---

**LC537\_PFOA2\_00002**

# Certificate of analysis

P: 6/21/17 SW ✓

Product No.: L08862  
Product: Perfluorooctanoic acid, 95%  
Lot No.: 10199078

PFOA

Appearance: White powder  
Water Content (Karl-Fischer): 1.30%  
Melting Point: 47.6-54.0°C  
Assay (Aqueous acid-base titration): 98.4%  
Assay (GC Silyl Deriv): 97.2%

This document has been electronically generated and does not require a signature.

Order our products online [www.alfa.com](http://www.alfa.com)

**ThermoFisher**  
SCIENTIFIC

Reagent

---

**LC537\_PFOs\_00003**



n: 11/30/16 SV  
PFOS

**SIGMA-ALDRICH**

**CERTIFICATE OF ANALYSIS**

Sigma-Aldrich Laborchemikalien GmbH D-30918 Seelze  
Telefon: +49 5137 8238-150

Seelze, 22.04.2014/524107/14/08646

Order-No.:

Customer-No.:

Order-Code:

Quantity:

Production Date: 17.Apr.2014

Expiry Date: 17.Apr.2019

Article/Product: 33829

Batch : SZBE107XV

Heptadecafluorooctanesulfonic acid potassium salt OEKANAL®

**Reference Material (RM)**

**1. General Information**

Formula: C<sub>8</sub>F<sub>17</sub>KO<sub>3</sub>S

CAS-No.: [2795-39-3]

Usage : PFOS

Molar mass: 538.22 g/Mole

Recomm. storage temp.: roomtemp.

The estimated uncertainty of a single measurement of the assay can be expected to be 0.5 % relative (confidence level = 95%, n= 6) whereby the assay measurements are calculated by 100% minus found impurities.

**2. Batch Analysis**

Identity

Assay (LC-MS)

Date of Analysis

complying

98 %

22.Apr.2014

**3. Advice and Remarks**

- The expiry date is based on the current knowledge and holds only for proper storage conditions in the originally closed flasks/ packages.
- Whenever the container is opened for removal of aliquot portions of the substance, the person handling the substance must assure, that the integrity of the substance is maintained and proper records of all its handlings are kept. Special care has to be taken to avoid any contamination or adulteration of the substance.
- We herewith confirm that the delivery is effected according to the technical delivery conditions agreed.
- Particular properties of the products or the suitability for a particular area of application are not assured.
- We guarantee a proper quality within our General Conditions of Sales.

Sigma-Aldrich Laborchemikalien GmbH  
Quality Management SA-LC

Reagent

---

**LC537\_PFO2\_00002**

R: 6.14.17 SKV

**Certificate of Analysis**


**Product Name:** HEPTADECAFLUOROOCATANESULFONIC ACID TETRAETHYLAMMONIUM SALT  
 98 %  
**Product Number:** 365289  
**Batch Number:** BCBQ0108V  
**Brand:** Aldrich  
**CAS Number:** 56773-42-3  
**Formula:**  $CF_3(CF_2)_6CF_2SO_3N(C_2H_5)_4$   
**Formula Weight:** 629.37  
**Quality Release Date:** 11 JUN 2015

TEST	SPECIFICATION	RESULT
APPEARANCE (COLOR)	WHITE TO OFF WHITE	OFF-WHITE
APPEARANCE (FORM)	POWDER OR POWDER WITH CHUNK(S)	POWDER
CARBON CONTENT	29.77 % - 31.29 %	29.97 %
INFRARED SPECTRUM	CONFORMS TO STRUCTURE	CONFORMS

*Claudia Geitner*  
 Dr. Claudia Geitner  
 Manager Quality Control  
 Buchs, Switzerland

MW correction:  $\frac{500.125}{629.37} = 0.7946$

Purity & MW correction = 77.37%



	$C_8 F_{17} SO_3^+ H$	$C_8 H_{20} N$
C = 12.011	96.088	96.088
F = 18.998	322.966	—
S = 32.066	32.066	—
O = 16.000	47.997	20.60
H = 1.008	1.008	14.007
N = 14.007	—	—
	<hr/>	<hr/>
	500.125	130.255

Reagent

---

**LCM2PFOA\_00007**

P: 5/11/17 SKV




# WELLINGTON LABORATORIES

## CERTIFICATE OF ANALYSIS DOCUMENTATION

**PRODUCT CODE:** M2PFOA  
**COMPOUND:** Perfluoro-n-[1,2-<sup>13</sup>C<sub>2</sub>]octanoic acid

**LOT NUMBER:** M2PFOA0216

**STRUCTURE:** **CAS #:** Not available

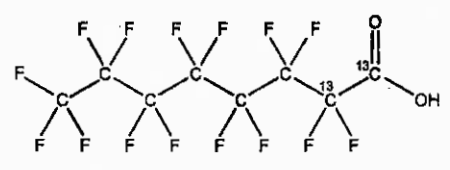

**MOLECULAR FORMULA:** <sup>13</sup>C<sub>2</sub><sup>12</sup>C<sub>6</sub>HF<sub>16</sub>O<sub>2</sub>  
**CONCENTRATION:** 50 ± 2.5 µg/ml

**MOLECULAR WEIGHT:** 416.05  
**SOLVENT(S):** Methanol  
Water (<1%)

**CHEMICAL PURITY:** >98%  
**LAST TESTED:** (mm/dd/yyyy) 02/12/2016  
**EXPIRY DATE:** (mm/dd/yyyy) 02/12/2021

**ISOTOPIC PURITY:** ≥99%<sup>13</sup>C  
(1,2-<sup>13</sup>C<sub>2</sub>)

**RECOMMENDED STORAGE:** Store ampoule in a cool, dark place

**DOCUMENTATION/ DATA ATTACHED:**

- Figure 1: LC/MS Data (TIC and Mass Spectrum)
- Figure 2: LC/MS/MS Data (Selected MRM Transitions)

**ADDITIONAL INFORMATION:**

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent conversion of the carboxylic acid to the methyl ester.

**FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE**

**Certified By:**   
B.G. Chittim

**Date:** 02/24/2016  
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA  
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

### **INTENDED USE:**

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

### **HAZARDS:**

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

### **SYNTHESIS / CHARACTERIZATION:**

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

### **HOMOGENEITY:**

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

### **UNCERTAINTY:**

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty,  $u_c(y)$ , of a value  $y$  and the uncertainty of the independent parameters  $x_1, x_2, \dots, x_n$  on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where  $x$  is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of  $\pm 5\%$  (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

### **TRACEABILITY:**

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

### **EXPIRY DATE / PERIOD OF VALIDITY:**


Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

### **LIMITED WARRANTY:**

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



### **QUALITY MANAGEMENT:**

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



\*\*For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at [www.well-labs.com](http://www.well-labs.com) or contact us directly at [info@well-labs.com](mailto:info@well-labs.com)\*\*

**Figure 1: M2PFOA; LC/MS Data (TIC and Mass Spectrum)**

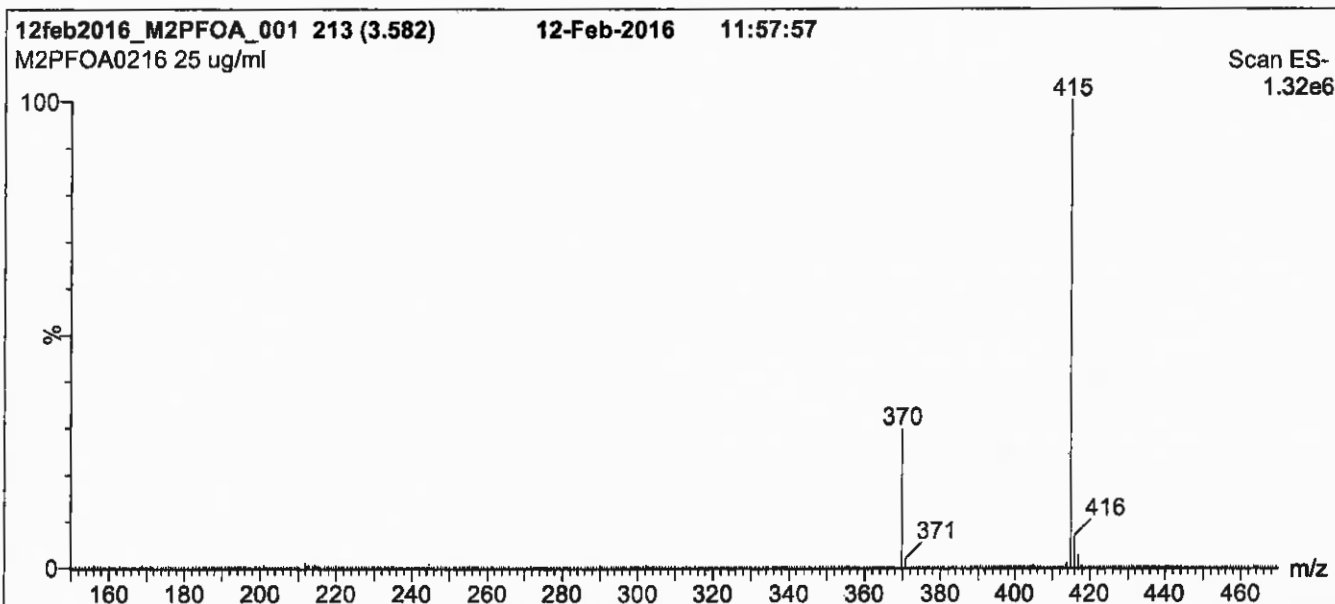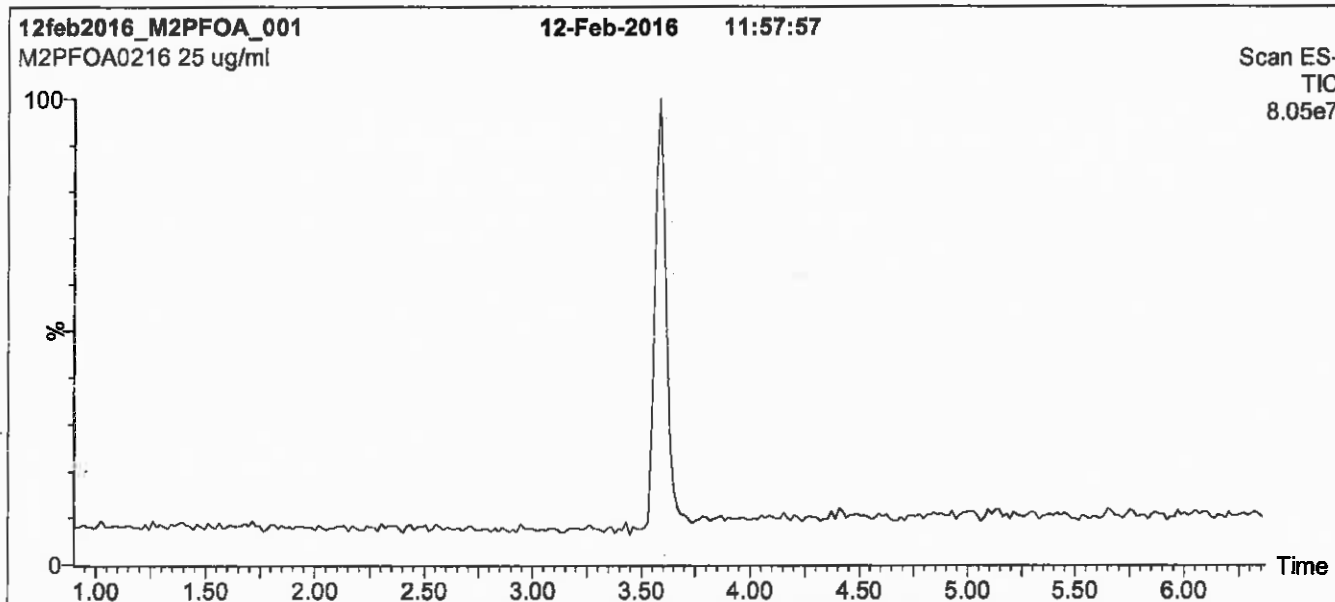

**Conditions for Figure 1:**

**LC:** Waters Acquity Ultra Performance LC  
**MS:** Micromass Quattro *micro* API MS

**Chromatographic Conditions**

Column: Acquity UPLC BEH Shield RP<sub>18</sub>  
1.7  $\mu$ m, 2.1 x 100 mm


Mobile phase: Gradient  
Start: 50% (80:20 MeOH:ACN) / 50% H<sub>2</sub>O  
(both with 10 mM NH<sub>4</sub>OAc buffer)  
Ramp to 90% organic over 7.5 min and hold for 1.5 min  
before returning to initial conditions in 0.5 min.  
Time: 10 min

Flow: 300  $\mu$ l/min

**MS Parameters**

Experiment: Full Scan (150 - 850 amu)  
Source: Electrospray (negative)  
Capillary Voltage (kV) = 3.00  
Cone Voltage (V) = 15.00  
Cone Gas Flow (l/hr) = 100  
Desolvation Gas Flow (l/hr) = 750

**Figure 2: M2PFOA; LC/MS/MS Data (Selected MRM Transitions)**



**Conditions for Figure 2:**

Injection: Direct loop injection  
 10  $\mu\text{l}$  (500 ng/ml M2PFOA)

Mobile phase: Isocratic 80% MeOH / 20% H<sub>2</sub>O

Flow: 300  $\mu\text{l}/\text{min}$

**MS Parameters**

Collision Gas (mbar) = 3.39e-3  
 Collision Energy (eV) = 10



Reagent

---

**LCMPFDA\_00012**

R: SBC 12/21/16



814255

ID: LCMPPFDA\_00012

Exp: 09/30/21 Prpd: SBC

13C2-Perfluorodecanoic acid



# WELLINGTON LABORATORIES

## CERTIFICATE OF ANALYSIS DOCUMENTATION

**PRODUCT CODE:** MPFDA      **LOT NUMBER:** MPFDA0916  
**COMPOUND:** Perfluoro-n-[1,2-<sup>13</sup>C<sub>2</sub>]decanoic acid

**STRUCTURE:**      **CAS #:** Not available



**MOLECULAR FORMULA:** <sup>13</sup>C<sub>2</sub><sup>12</sup>C<sub>8</sub>HF<sub>19</sub>O<sub>2</sub>  
**CONCENTRATION:** 50 ± 2.5 µg/ml

**MOLECULAR WEIGHT:** 516.07  
**SOLVENT(S):** Methanol  
Water (<1%)

**CHEMICAL PURITY:** >98%

**ISOTOPIC PURITY:** ≥99% <sup>13</sup>C  
(1,2-<sup>13</sup>C<sub>2</sub>)

**LAST TESTED:** (mm/dd/yyyy) 09/30/2016

**EXPIRY DATE:** (mm/dd/yyyy) 09/30/2021

**RECOMMENDED STORAGE:** Store ampoule in a cool, dark place

### DOCUMENTATION/ DATA ATTACHED:

Figure 1: LC/MS Data (TIC and Mass Spectrum)

Figure 2: LC/MS/MS Data (Selected MRM Transitions)

### ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent conversion of the carboxylic acid to the methyl ester.
- Contains < 0.1% of <sup>13</sup>C<sub>1</sub>-PFNA.

**FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE**

Certified By:   
B.G. Chríttim

Date: 10/07/2016  
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA  
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

### **INTENDED USE:**

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

### **HAZARDS:**

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

### **SYNTHESIS / CHARACTERIZATION:**

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

### **HOMOGENEITY:**

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

### **UNCERTAINTY:**

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty,  $u_c(y)$ , of a value  $y$  and the uncertainty of the independent parameters  $x_1, x_2, \dots, x_n$  on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where  $x$  is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of  $\pm 5\%$  (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

### **TRACEABILITY:**

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

### **EXPIRY DATE / PERIOD OF VALIDITY:**

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

### **LIMITED WARRANTY:**

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



### **QUALITY MANAGEMENT:**

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



\*\*For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at [www.well-labs.com](http://www.well-labs.com) or contact us directly at [info@well-labs.com](mailto:info@well-labs.com)\*\*

**Figure 1: MPFDA; LC/MS Data (TIC and Mass Spectrum)**



**Conditions for Figure 1:**

**LC:** Waters Acquity Ultra Performance LC  
**MS:** Micromass Quattro *micro* API MS

**Chromatographic Conditions**


Column: Acquity UPLC BEH Shield RP<sub>18</sub>  
1.7  $\mu$ m, 2.1 x 100 mm  
Mobile phase: Gradient  
Start: 50% (80:20 MeOH:ACN) / 50% H<sub>2</sub>O  
(both with 10 mM NH<sub>4</sub>OAc buffer)  
Ramp to 90% organic over 7 min and hold for 1.5 min  
before returning to initial conditions in 0.5 min.  
Time: 10 min

Flow: 300  $\mu$ l/min

**MS Parameters**

Experiment: Full Scan (225 - 850 amu)  
Source: Electrospray (negative)  
Capillary Voltage (kV) = 2.00  
Cone Voltage (V) = 15.00  
Cone Gas Flow (l/hr) = 50  
Desolvation Gas Flow (l/hr) = 750

**Figure 2: MPFDA; LC/MS/MS Data (Selected MRM Transitions)**

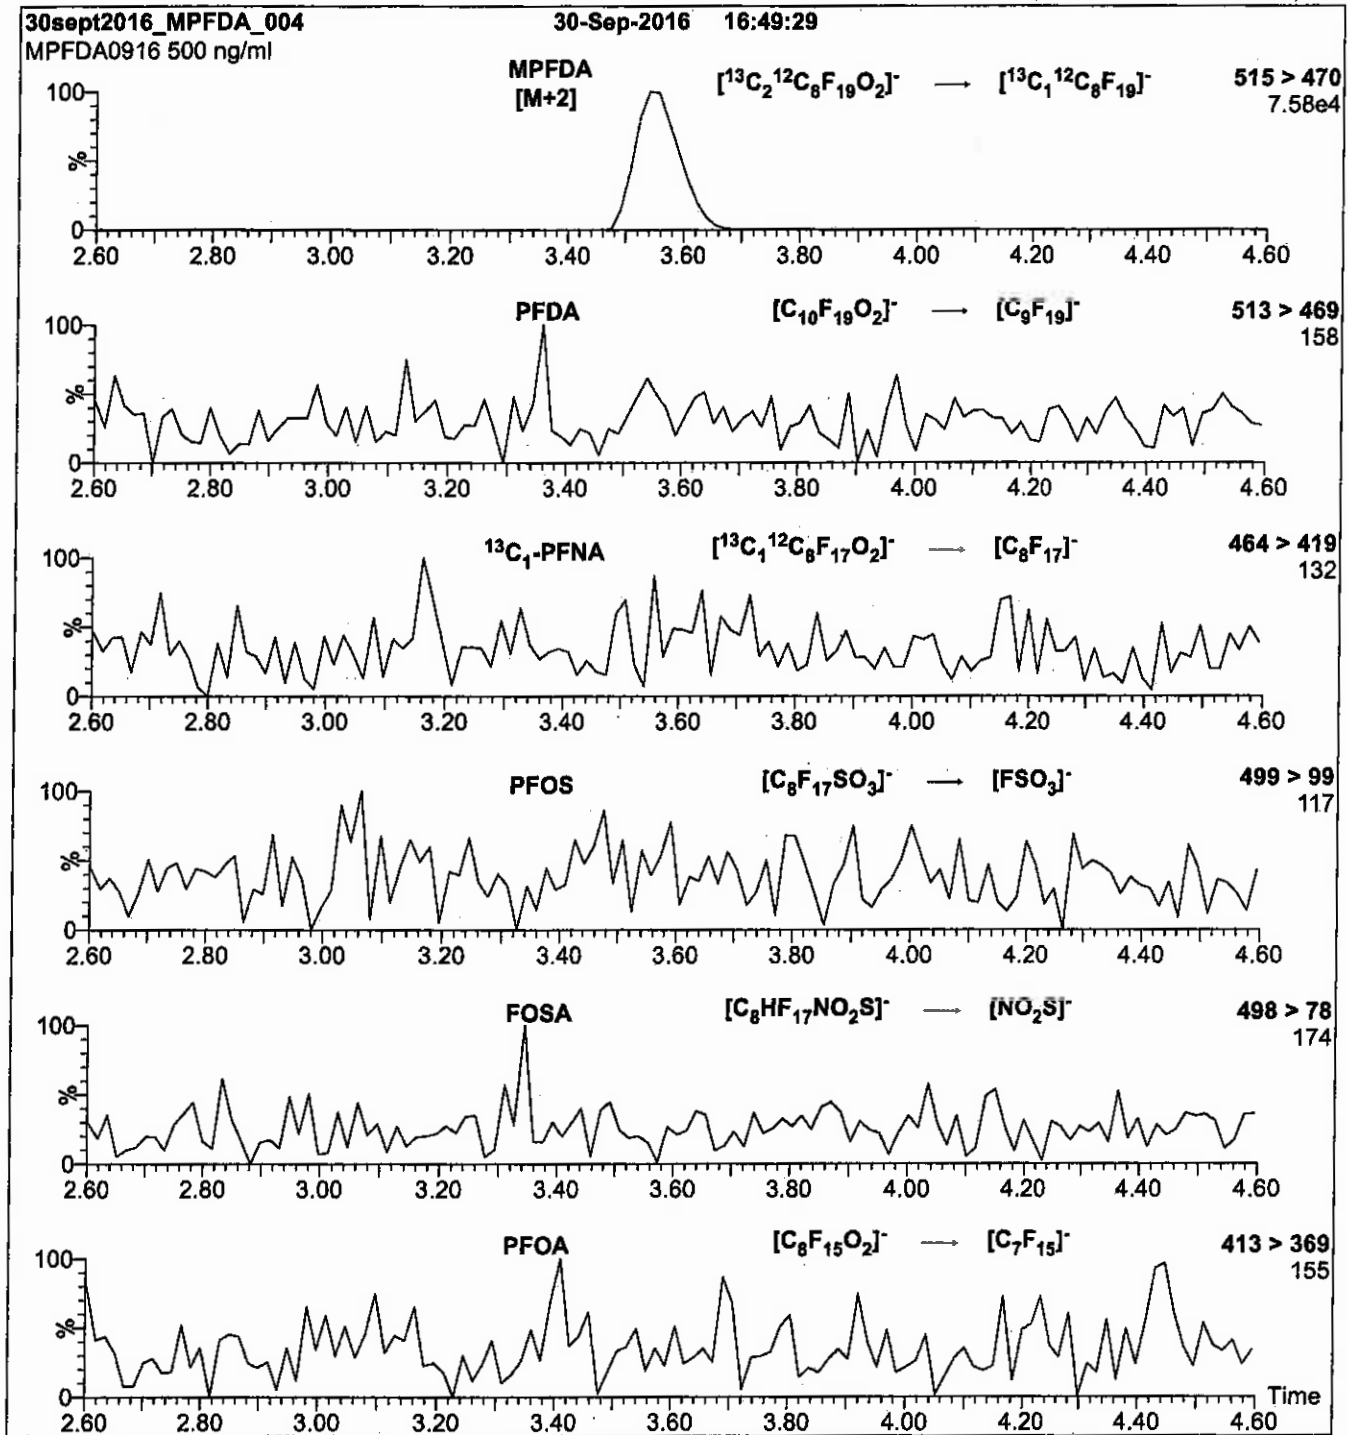

**Conditions for Figure 2:**

Injection: Direct loop injection  
10  $\mu$ l (500 ng/ml MPFDA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H<sub>2</sub>O  
(both with 10 mM NH<sub>4</sub>OAc buffer)

Flow: 300  $\mu$ l/min

**MS Parameters**

Collision Gas (mbar) = 3.31e-3  
Collision Energy (eV) = 13

Reagent

---

**LCMPFHxA\_00013**

R: SBC 12/21/16



814258  
ID: LCMPFHxA\_00013  
Exp: 04/08/21 Ppdt. SBC  
13C2-Perfluorohexanoic ac



# WELLINGTON LABORATORIES


## CERTIFICATE OF ANALYSIS DOCUMENTATION

**PRODUCT CODE:** MPFHxA  
**COMPOUND:** Perfluoro-n-[1,2-<sup>13</sup>C<sub>2</sub>]hexanoic acid

**LOT NUMBER:** MPFHxA0416

**STRUCTURE:**

**CAS #:** Not available



**MOLECULAR FORMULA:** <sup>13</sup>C<sub>2</sub><sup>12</sup>C<sub>4</sub>HF<sub>11</sub>O<sub>2</sub>  
**CONCENTRATION:** 50 ± 2.5 µg/ml

**MOLECULAR WEIGHT:** 316.04  
**SOLVENT(S):** Methanol  
Water (<1%)

**CHEMICAL PURITY:** >98%

**ISOTOPIC PURITY:** ≥99%<sup>13</sup>C  
(1,2-<sup>13</sup>C<sub>2</sub>)

**LAST TESTED:** (mm/dd/yyyy) 04/08/2016

**EXPIRY DATE:** (mm/dd/yyyy) 04/08/2021

**RECOMMENDED STORAGE:** Store ampoule in a cool, dark place

**DOCUMENTATION/ DATA ATTACHED:**

- Figure 1: LC/MS Data (TIC and Mass Spectrum)
- Figure 2: LC/MS/MS Data (Selected MRM Transitions)

**ADDITIONAL INFORMATION:**

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent conversion of the carboxylic acid to the methyl ester.
- Contains < 0.1% of perfluoro-n-hexanoic acid and ~ 0.3% of perfluoro-n-octanoic acid.

**FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE**

**Certified By:**   
B.G. Chittim

**Date:** 04/29/2016  
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA  
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

### **INTENDED USE:**

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

### **HAZARDS:**

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

### **SYNTHESIS / CHARACTERIZATION:**

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

### **HOMOGENEITY:**

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

### **UNCERTAINTY:**

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty,  $u_c(y)$ , of a value  $y$  and the uncertainty of the independent parameters  $x_1, x_2, \dots, x_n$  on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where  $x$  is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of  $\pm 5\%$  (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

### **TRACEABILITY:**

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

### **EXPIRY DATE / PERIOD OF VALIDITY:**

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

### **LIMITED WARRANTY:**

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.

### **QUALITY MANAGEMENT:**



This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



\*\*For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at [www.well-labs.com](http://www.well-labs.com) or contact us directly at [info@well-labs.com](mailto:info@well-labs.com)\*\*



**Figure 1: MPFHxA; LC/MS Data (TIC and Mass Spectrum)**



**Conditions for Figure 1:**

**LC:** Waters Acquity Ultra Performance LC  
**MS:** Micromass Quattro *micro* API MS

**Chromatographic Conditions**

Column: Acquity UPLC BEH Shield RP<sub>18</sub>  
1.7  $\mu$ m, 2.1 x 100 mm

Mobile phase: Gradient  
Start: 50% (80:20 MeOH:ACN) / 50% H<sub>2</sub>O  
(both with 10 mM NH<sub>4</sub>OAc buffer)  
Ramp to 90% organic over 7.5 min and hold for 1.5 min  
before returning to initial conditions over 0.5 min.  
Time: 10 min


Flow: 300  $\mu$ l/min

**MS Parameters**

Experiment: Full Scan (150 - 850 amu)

Source: Electrospray (negative)  
Capillary Voltage (kV) = 2.00  
Cone Voltage (V) = 15.00  
Cone Gas Flow (l/hr) = 100  
Desolvation Gas Flow (l/hr) = 750

**Figure 2: MPFHxA; LC/MS/MS Data (Selected MRM Transitions)**

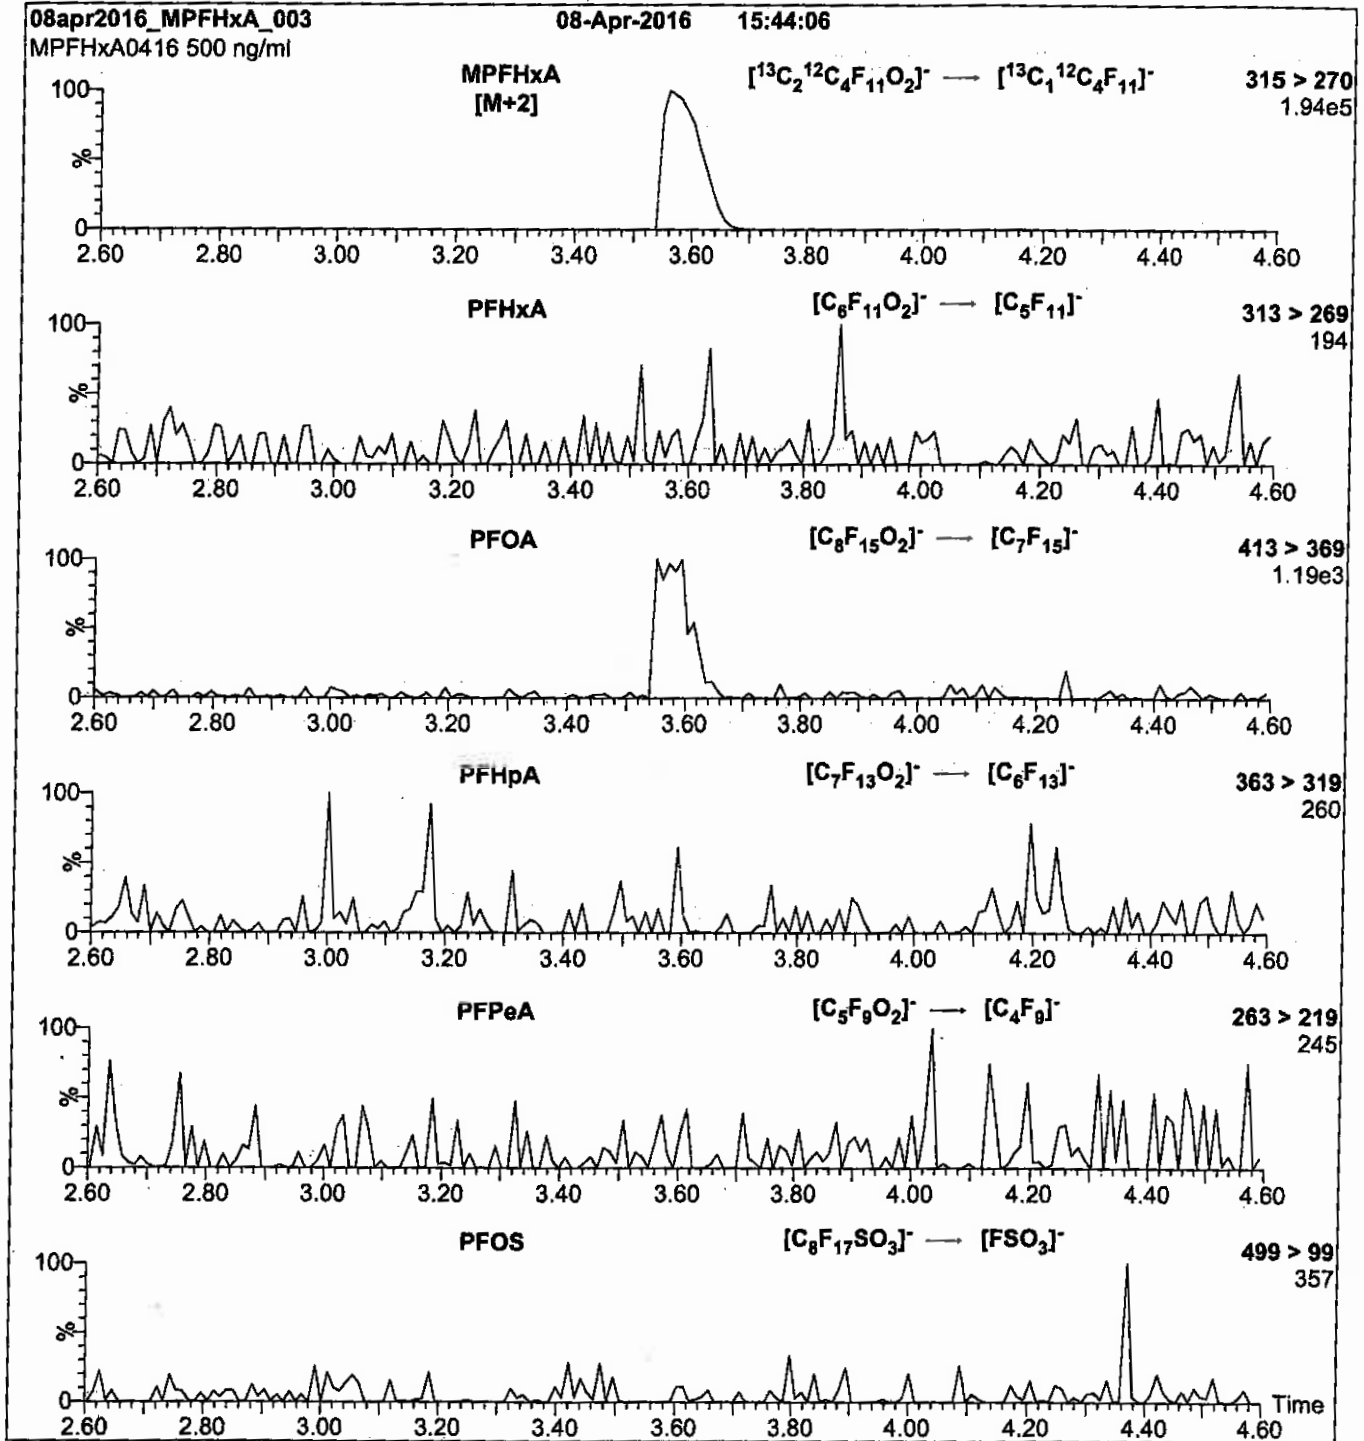

**Conditions for Figure 2:**

Injection: Direct loop injection  
10  $\mu$ l (500 ng/ml MPFHxA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H<sub>2</sub>O  
(both with 10 mM NH<sub>4</sub>OAc buffer)

Flow: 300  $\mu$ l/min

**MS Parameters**

Collision Gas (mbar) = 3.39e-3  
Collision Energy (eV) = 10

Reagent

---

**LCMPFOS\_00019**

R: SBC 12/21/16



814253  
ID: LCMPFOS\_00019  
Exp: 08/03/21 Ppfd: SBC  
13C4-Perfluorooctanesulfo




# WELLINGTON LABORATORIES

## CERTIFICATE OF ANALYSIS DOCUMENTATION

**PRODUCT CODE:** MPFOS      **LOT NUMBER:** MPFOS0816  
**COMPOUND:** Sodium perfluoro-1-[1,2,3,4-<sup>13</sup>C<sub>4</sub>]octanesulfonate

**STRUCTURE:**      **CAS #:** Not available



<b>MOLECULAR FORMULA:</b>	<sup>13</sup> C <sub>4</sub> <sup>12</sup> C <sub>4</sub> F <sub>17</sub> SO <sub>3</sub> Na	<b>MOLECULAR WEIGHT:</b>	526.08
<b>CONCENTRATION:</b>	50.0 ± 2.5 µg/ml (Na salt) 47.8 ± 2.4 µg/ml (MPFOS anion)	<b>SOLVENT(S):</b>	Methanol
<b>CHEMICAL PURITY:</b>	>98%	<b>ISOTOPIC PURITY:</b>	≥99% <sup>13</sup> C (1,2,3,4- <sup>13</sup> C <sub>4</sub> )
<b>LAST TESTED:</b> (mm/dd/yyyy)	08/03/2016		
<b>EXPIRY DATE:</b> (mm/dd/yyyy)	08/03/2021		
<b>RECOMMENDED STORAGE:</b>	Store ampoule in a cool, dark place		


**DOCUMENTATION/ DATA ATTACHED:**

Figure 1: LC/MS Data (TIC and Mass Spectrum)  
Figure 2: LC/MS/MS Data (Selected MRM Transitions)

**ADDITIONAL INFORMATION:**

- See page 2 for further details.
- Contains ~ 0.8% Sodium perfluoro-1-[1,2,3-<sup>13</sup>C<sub>3</sub>]heptanesulfonate.

**FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE**

**Certified By:**   
B.G. Chittim      **Date:** 08/05/2016  
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA  
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

### **INTENDED USE:**

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

### **HAZARDS:**

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

### **SYNTHESIS / CHARACTERIZATION:**

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

### **HOMOGENEITY:**

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

### **UNCERTAINTY:**

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty,  $u_c(y)$ , of a value  $y$  and the uncertainty of the independent parameters  $x_1, x_2, \dots, x_n$  on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where  $x$  is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of  $\pm 5\%$  (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

### **TRACEABILITY:**

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

### **EXPIRY DATE / PERIOD OF VALIDITY:**


Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

### **LIMITED WARRANTY:**

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



### **QUALITY MANAGEMENT:**

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



\*\*For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at [www.well-labs.com](http://www.well-labs.com) or contact us directly at [info@well-labs.com](mailto:info@well-labs.com)\*\*

**Figure 1: MPFOS; LC/MS Data (TIC and Mass Spectrum)**



**Conditions for Figure 1:**

**LC:** Waters Acquity Ultra Performance LC  
**MS:** Micromass Quattro *micro* API MS

**Chromatographic Conditions**

**Column:** Acquity UPLC BEH Shield RP<sub>18</sub>  
 1.7  $\mu$ m, 2.1 x 100 mm

**Mobile phase:** Gradient  
 Start: 45% (80:20 MeOH:ACN) / 55% H<sub>2</sub>O  
 (both with 10 mM NH<sub>4</sub>OAc buffer)  
 Ramp to 90% organic over 7 min and hold for 1.5 min  
 before returning to initial conditions in 0.5 min.  
 Time: 10 min


**Flow:** 300  $\mu$ l/min

**MS Parameters**

**Experiment:** Full Scan (225 - 850 amu)

**Source:** Electrospray (negative)  
 Capillary Voltage (kV) = 3.00  
 Cone Voltage (V) = 60.00  
 Cone Gas Flow (l/hr) = 50  
 Desolvation Gas Flow (l/hr) = 750

**Figure 2: MPFOS; LC/MS/MS Data (Selected MRM Transitions)**

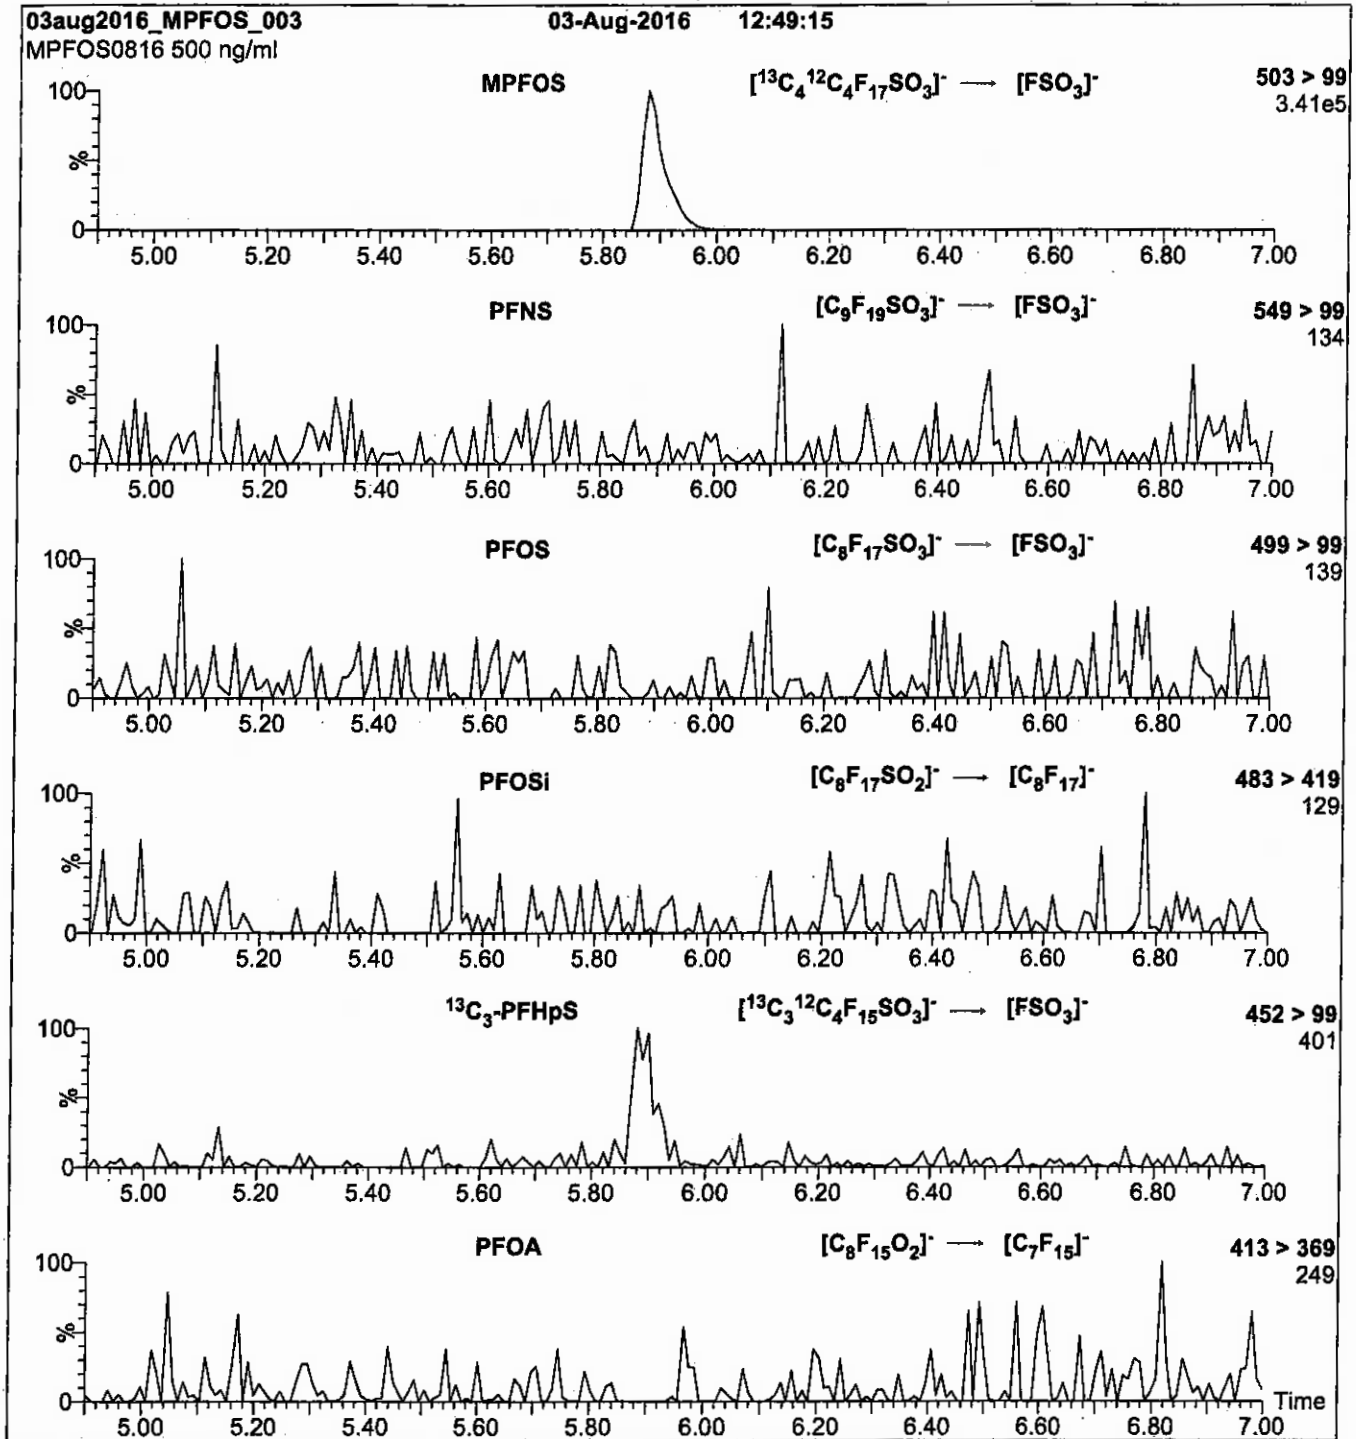

**Conditions for Figure 2:**

Injection: Direct loop injection  
10  $\mu\text{l}$  (500 ng/ml MPFOS)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20%  $\text{H}_2\text{O}$   
(both with 10 mM  $\text{NH}_4\text{OAc}$  buffer)

Flow: 300  $\mu\text{l}/\text{min}$

**MS Parameters**

Collision Gas (mbar) = 3.46e-3  
Collision Energy (eV) = 40

Reagent

---

**LCMPFOS\_00021**



r: 5/6/17 SKV




# WELLINGTON LABORATORIES

## CERTIFICATE OF ANALYSIS DOCUMENTATION

**PRODUCT CODE:** MPFOS **LOT NUMBER:** MPFOS1216  
**COMPOUND:** Sodium perfluoro-1-[1,2,3,4-<sup>13</sup>C<sub>4</sub>]octanesulfonate

**STRUCTURE:** **CAS #:** Not available



<b>MOLECULAR FORMULA:</b>	<sup>13</sup> C <sub>4</sub> <sup>12</sup> C <sub>4</sub> F <sub>17</sub> SO <sub>3</sub> Na	<b>MOLECULAR WEIGHT:</b>	526.08
<b>CONCENTRATION:</b>	50.0 ± 2.5 µg/ml (Na salt) 47.8 ± 2.4 µg/ml (MPFOS anion)	<b>SOLVENT(S):</b>	Methanol
<b>CHEMICAL PURITY:</b>	>98%	<b>ISOTOPIC PURITY:</b>	≥99% <sup>13</sup> C (1,2,3,4- <sup>13</sup> C <sub>4</sub> )
<b>LAST TESTED:</b> (mm/dd/yyyy)	12/12/2016		
<b>EXPIRY DATE:</b> (mm/dd/yyyy)	12/12/2021		
<b>RECOMMENDED STORAGE:</b>	Store ampoule in a cool, dark place		


**DOCUMENTATION/ DATA ATTACHED:**

- Figure 1: LC/MS Data (TIC and Mass Spectrum)
- Figure 2: LC/MS/MS Data (Selected MRM Transitions)

**ADDITIONAL INFORMATION:**

- See page 2 for further details.
- Contains ~ 0.8% Sodium perfluoro-1-[1,2,3-<sup>13</sup>C<sub>3</sub>]heptanesulfonate.

**FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE**

**Certified By:**   
 B.G. Chittim **Date:** 12/14/2016  
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA  
 519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

### **INTENDED USE:**

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

### **HAZARDS:**

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

### **SYNTHESIS / CHARACTERIZATION:**

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

### **HOMOGENEITY:**

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

### **UNCERTAINTY:**

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty,  $u_c(y)$ , of a value  $y$  and the uncertainty of the independent parameters  $x_1, x_2, \dots, x_n$  on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where  $x$  is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of  $\pm 5\%$  (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

### **TRACEABILITY:**

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

### **EXPIRY DATE / PERIOD OF VALIDITY:**


Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

### **LIMITED WARRANTY:**

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



### **QUALITY MANAGEMENT:**

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



\*\*For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at [www.well-labs.com](http://www.well-labs.com) or contact us directly at [info@well-labs.com](mailto:info@well-labs.com)\*\*

**Figure 1: MPFOS; LC/MS Data (TIC and Mass Spectrum)**



**Conditions for Figure 1:**

**LC:** Waters Acquity Ultra Performance LC  
**MS:** Micromass Quattro *micro* API MS

**Chromatographic Conditions**

**Column:** Acquity UPLC BEH Shield RP<sub>18</sub>  
 1.7  $\mu$ m, 2.1 x 100 mm

**Mobile phase:** Gradient  
 Start: 50% (80:20 MeOH:ACN) / 50% H<sub>2</sub>O  
 (both with 10 mM NH<sub>4</sub>OAc buffer)  
 Ramp to 85% organic over 7.5 min and hold for 1.5 min  
 before returning to initial conditions in 0.5 min.  
 Time: 10 min


**Flow:** 300  $\mu$ l/min

**MS Parameters**

**Experiment:** Full Scan (150 - 850 amu)

**Source:** Electrospray (negative)  
 Capillary Voltage (kV) = 3.00  
 Cone Voltage (V) = 60.00  
 Cone Gas Flow (l/hr) = 50  
 Desolvation Gas Flow (l/hr) = 750

**Figure 2: MPFOS; LC/MS/MS Data (Selected MRM Transitions)**



**Conditions for Figure 2:**

**Injection:** Direct loop injection  
10  $\mu\text{l}$  (500 ng/ml MPFOS)

**Mobile phase:** Isocratic 80% (80:20 MeOH:ACN) / 20%  $\text{H}_2\text{O}$   
(both with 10 mM  $\text{NH}_4\text{OAc}$  buffer)

**Flow:** 300  $\mu\text{l}/\text{min}$

**MS Parameters**

Collision Gas (mbar) = 3.35e-3  
Collision Energy (eV) = 40

# Method 537 DOD

---

Perfluorinated Alkyl Acids (LC/MS)  
by Method 537 DOD

FORM II  
LCMS SURROGATE RECOVERY

Lab Name: TestAmerica Sacramento

Job No.: 320-31468-1

SDG No.: \_\_\_\_\_

Matrix: Water

Level: Low

GC Column (1): GeminiC18 3 ID: 3 (mm)

Client Sample ID	Lab Sample ID	PFHxA #	PFDA #
NAWC-091117-RW-106	320-31468-1	67 Q	100
NAWC-091117-FRB-106	320-31468-2	82	105
NAWC-091117-RW-060	320-31468-3	71	114
NAWC-091117-FRB-060	320-31468-4	86	107
NAWC-091117-RW-314	320-31468-5	72	104
NAWC-091117-FRB-314	320-31468-6	82	102
NAWC-091117-RW-258	320-31468-7	72	98
NAWC-091117-FRB-258	320-31468-8	86	101
NAWC-091117-RW-048	320-31468-9	74	111
NAWC-091117-FRB-048	320-31468-10	84	102
NAWC-091117-RW-145	320-31468-11	74	115
NAWC-091117-FRB-145	320-31468-12	83	100
NAWC-091117-RW-317	320-31468-13	78	116
NAWC-091117-FRB-317	320-31468-14	83	97
NAWC-091117-RW-319	320-31468-15	61 Q	83
NAWC-091117-FRB-319	320-31468-16	82	124
NAWC-091117-RW-321	320-31468-17	76	106
NAWC-091117-FRB-321	320-31468-18	84	104
NAWC-091117-RW-010	320-31468-19	75	104
NAWC-091117-FRB-010	320-31468-20	83	97
NAWC-091117-RW-162	320-31468-21	78	111
NAWC-091117-FRB-162	320-31468-22	91	129
WGNA-091117-DUP09	320-31468-23	75	125
	MB 320-184382/1-A	90	111
	MB 320-184385/1-A	87	143 Q
	LCS 320-184382/2-A	91	115
	LCSD 320-184382/3-A	86	110
	LLCS 320-184385/2-A	90	113

PFHxA = 13C2 PFHxA  
PFDA = 13C2 PFDA

QC LIMITS  
70-130  
70-130

# Column to be used to flag recovery values

FORM II  
LCMS SURROGATE RECOVERY

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1

SDG No.: \_\_\_\_\_

Matrix: Water Level: Low

GC Column (1): GeminiC18 3 ID: 3 (mm)

Client Sample ID	Lab Sample ID	PFHxA #	PFDA #
	LLCSD 320-184385/3-A	93	124

PFHxA = 13C2 PFHxA  
PFDA = 13C2 PFDA

QC LIMITS  
70-130  
70-130

# Column to be used to flag recovery values

FORM II 537

FORM III  
LCMS LAB CONTROL SAMPLE RECOVERY

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Matrix: Water Level: Low Lab File ID: 2017.09.19\_537A\_012.d  
 Lab ID: LCS 320-184382/2-A Client ID: \_\_\_\_\_

COMPOUND	SPIKE ADDED (ng/L)	LCS CONCENTRATION (ng/L)	LCS % REC	QC LIMITS REC	#
Perfluorooctanesulfonic acid (PFOS)	222	198	89	70-130	M
Perfluorooctanoic acid (PFOA)	111	103	93	70-130	
Perfluorononanoic acid (PFNA)	111	99.7	90	70-130	
Perfluorohexanesulfonic acid (PFHxS)	167	150	90	70-130	
Perfluoroheptanoic acid (PFHpA)	55.6	50.5	91	70-130	
Perfluorobutanesulfonic acid (PFBS)	500	408	82	70-130	

# Column to be used to flag recovery and RPD values



FORM III  
LCMS LAB CONTROL SAMPLE DUPLICATE RECOVERY

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1

SDG No.: \_\_\_\_\_

Matrix: Water Level: Low Lab File ID: 2017.09.19\_537A\_013.d

Lab ID: LCSD 320-184382/3-A Client ID: \_\_\_\_\_

COMPOUND	SPIKE ADDED (ng/L)	LCSD CONCENTRATION (ng/L)	LCSD % REC	% RPD	QC LIMITS		#
					RPD	REC	
Perfluorooctanesulfonic acid (PFOS)	222	188	84	5	30	70-130	M
Perfluorooctanoic acid (PFOA)	111	96.8	87	7	30	70-130	
Perfluorononanoic acid (PFNA)	111	93.6	84	6	30	70-130	
Perfluorohexanesulfonic acid (PFHxS)	167	143	86	5	30	70-130	
Perfluoroheptanoic acid (PFHpA)	55.6	48.7	88	3	30	70-130	
Perfluorobutanesulfonic acid (PFBS)	500	403	81	1	30	70-130	

# Column to be used to flag recovery and RPD values

FORM III  
LCMS LOW LEVEL CONTROL SAMPLE RECOVERY

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Matrix: Water Level: Low Lab File ID: 2017.09.19\_537A\_004.d  
 Lab ID: LLCS 320-184385/2-A Client ID: \_\_\_\_\_

COMPOUND	SPIKE ADDED (ng/L)	LLCS CONCENTRATION (ng/L)	LLCS % REC	QC LIMITS REC	#
Perfluorooctanesulfonic acid (PFOS)	40.0	36.6 J	91	50-150	M
Perfluorooctanoic acid (PFOA)	20.0	18.4 J	92	50-150	
Perfluorononanoic acid (PFNA)	20.0	18.5 J	93	50-150	
Perfluorohexanesulfonic acid (PFHxS)	30.0	28.9 J	96	50-150	
Perfluoroheptanoic acid (PFHpA)	10.0	10.2	102	50-150	
Perfluorobutanesulfonic acid (PFBS)	90.0	86.1 J	96	50-150	

# Column to be used to flag recovery and RPD values

FORM III  
LCMS LOW LEVEL CONTROL STANDARD DUPLICATE RECOVERY

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Matrix: Water Level: Low Lab File ID: 2017.09.19\_537A\_005.d  
 Lab ID: LLCSD 320-184385/3-A Client ID: \_\_\_\_\_

COMPOUND	SPIKE ADDED (ng/L)	LLCSD CONCENTRATION (ng/L)	LLCSD % REC	% RPD	QC LIMITS		#
					RPD	REC	
Perfluorooctanesulfonic acid (PFOS)	40.0	36.2 J	90	1	50	50-150	M
Perfluorooctanoic acid (PFOA)	20.0	18.7 J	93	1	50	50-150	
Perfluorononanoic acid (PFNA)	20.0	19.0 J	95	3	50	50-150	
Perfluorohexanesulfonic acid (PFHxS)	30.0	29.4 J	98	2	50	50-150	
Perfluoroheptanoic acid (PFHpA)	10.0	10.8	108	6	50	50-150	
Perfluorobutanesulfonic acid (PFBS)	90.0	89.0 J	99	3	50	50-150	

# Column to be used to flag recovery and RPD values

FORM IV  
LCMS METHOD BLANK SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-31468-1

SDG No.: \_\_\_\_\_

Lab File ID: 2017.09.19\_537A\_011.d

Lab Sample ID: MB 320-184382/1-A

Matrix: Water

Date Extracted: 09/14/2017 09:17

Instrument ID: A8\_N

Date Analyzed: 09/20/2017 04:35

Level: (Low/Med) Low

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES:

CLIENT SAMPLE ID	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED
	LCS 320-184382/2-A	2017.09.19_537A_012.d	09/20/2017 04:40
	LCSD 320-184382/3-A	2017.09.19_537A_013.d	09/20/2017 04:45
NAWC-091117-RW-106	320-31468-1	2017.09.19_537A_014.d	09/20/2017 04:49
NAWC-091117-FRB-106	320-31468-2	2017.09.19_537A_015.d	09/20/2017 04:54
NAWC-091117-RW-060	320-31468-3	2017.09.19_537A_016.d	09/20/2017 04:59
NAWC-091117-FRB-060	320-31468-4	2017.09.19_537A_017.d	09/20/2017 05:04
NAWC-091117-RW-314	320-31468-5	2017.09.19_537A_018.d	09/20/2017 05:08
NAWC-091117-FRB-314	320-31468-6	2017.09.19_537A_019.d	09/20/2017 05:13
NAWC-091117-RW-258	320-31468-7	2017.09.19_537A_020.d	09/20/2017 05:18
NAWC-091117-FRB-258	320-31468-8	2017.09.19_537A_023.d	09/20/2017 05:32
NAWC-091117-RW-048	320-31468-9	2017.09.19_537A_024.d	09/20/2017 05:37
NAWC-091117-FRB-048	320-31468-10	2017.09.19_537A_025.d	09/20/2017 05:42
NAWC-091117-RW-145	320-31468-11	2017.09.19_537A_026.d	09/20/2017 05:46
NAWC-091117-FRB-145	320-31468-12	2017.09.19_537A_027.d	09/20/2017 05:51
NAWC-091117-RW-317	320-31468-13	2017.09.19_537A_028.d	09/20/2017 05:56
NAWC-091117-FRB-317	320-31468-14	2017.09.19_537A_029.d	09/20/2017 06:01
NAWC-091117-RW-319	320-31468-15	2017.09.19_537A_030.d	09/20/2017 06:05
NAWC-091117-FRB-319	320-31468-16	2017.09.19_537A_031.d	09/20/2017 06:10
NAWC-091117-RW-321	320-31468-17	2017.09.19_537A_032.d	09/20/2017 06:15
NAWC-091117-FRB-321	320-31468-18	2017.09.19_537A_035.d	09/20/2017 06:29
NAWC-091117-RW-010	320-31468-19	2017.09.19_537A_036.d	09/20/2017 06:34
NAWC-091117-FRB-010	320-31468-20	2017.09.19_537A_037.d	09/20/2017 06:39

FORM IV  
LCMS METHOD BLANK SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Lab File ID: 2017.09.19\_537A\_003.d Lab Sample ID: MB 320-184385/1-A  
 Matrix: Water Date Extracted: 09/14/2017 09:29  
 Instrument ID: A8\_N Date Analyzed: 09/20/2017 03:57  
 Level: (Low/Med) Low

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES:

CLIENT SAMPLE ID	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED
	LLCS 320-184385/2-A	2017.09.19_537A_004.d	09/20/2017 04:02
	LLCSD 320-184385/3-A	2017.09.19_537A_005.d	09/20/2017 04:07
NAWC-091117-RW-162	320-31468-21	2017.09.19_537A_006.d	09/20/2017 04:11
NAWC-091117-FRB-162	320-31468-22	2017.09.19_537A_007.d	09/20/2017 04:16
WGNA-091117-DUP09	320-31468-23	2017.09.19_537A_008.d	09/20/2017 04:21

FORM VIII  
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Instrument ID: A8\_N Calibration Start Date: 09/20/2017 02:56  
 GC Column: GeminiC18 3x100 ID: 3(mm) Calibration End Date: 09/20/2017 03:19  
 Calibration ID: 34457

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
INITIAL CALIBRATION MEAN AREA AND MEAN RT	2116635	1.86	5570738	2.11		
UPPER LIMIT	3174953	2.36	8356107	2.61		
LOWER LIMIT	1058318	1.36	2785369	1.61		
LAB SAMPLE ID	CLIENT SAMPLE ID					
CCVL 320-185329/11	2252465	1.85	5723538	2.10		
ICV 320-185329/13	2616480	1.85	7294448	2.10		
CCV 320-185406/1 CCVIS	1946548	1.85	5210623	2.10		
MB 320-184385/1-A	2539018	1.85	6194895	2.10		
LLCS 320-184385/2-A	2322795	1.85	5655681	2.10		
LLCSD 320-184385/3-A	2191521	1.84	5502551	2.09		
320-31468-21	NAWC-091117-RW-162	2350014	1.84	5861531	2.10	
320-31468-22	NAWC-091117-FRB-162	2344211	1.85	6003115	2.10	
320-31468-23	WGNA-091117-DUP09	2370526	1.85	6043874	2.10	
CCV 320-185406/9 CCVIS	2062556	1.85	5491922	2.10		
CCV 320-185407/9 CCVIS	2062556	1.85	5491922	2.10		
MB 320-184382/1-A	2402894	1.85	5785526	2.10		
LCS 320-184382/2-A	2181509	1.84	5704391	2.09		
LCSD 320-184382/3-A	2332217	1.85	5855728	2.10		
320-31468-1	NAWC-091117-RW-106	2290728	1.84	5860369	2.09	
320-31468-2	NAWC-091117-FRB-106	2577088	1.84	6073981	2.09	
320-31468-3	NAWC-091117-RW-060	2387971	1.85	6309998	2.10	
320-31468-4	NAWC-091117-FRB-060	2308276	1.85	5696853	2.10	
320-31468-5	NAWC-091117-RW-314	2570115	1.85	6192393	2.10	
320-31468-6	NAWC-091117-FRB-314	2574796	1.85	6281693	2.10	
320-31468-7	NAWC-091117-RW-258	2394768	1.84	6099250	2.10	
CCV 320-185407/21 CCVIS	2036337	1.85	5320724	2.10		
CCV 320-185408/21 CCVIS	2036337	1.85	5320724	2.10		
320-31468-8	NAWC-091117-FRB-258	2497710	1.85	6286206	2.10	
320-31468-9	NAWC-091117-RW-048	2501111	1.85	6308482	2.10	
320-31468-10	NAWC-091117-FRB-048	2637228	1.85	6282400	2.10	
320-31468-11	NAWC-091117-RW-145	2432580	1.84	6418340	2.10	
320-31468-12	NAWC-091117-FRB-145	2685353	1.84	6382119	2.10	

13PFOA = 13C2-PFOA

PFOS = 13C4 PFOS

Area Limit = 50%-150% of internal standard area

RT Limit = ± 0.5 minutes of internal standard RT

# Column used to flag values outside QC limits

FORM VIII  
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Instrument ID: A8\_N Calibration Start Date: 09/20/2017 02:56  
 GC Column: GeminiC18 3x100 ID: 3(mm) Calibration End Date: 09/20/2017 03:19  
 Calibration ID: 34457

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
INITIAL CALIBRATION MEAN AREA AND MEAN RT	2116635	1.86	5570738	2.11		
UPPER LIMIT	3174953	2.36	8356107	2.61		
LOWER LIMIT	1058318	1.36	2785369	1.61		
LAB SAMPLE ID	CLIENT SAMPLE ID					
320-31468-13	NAWC-091117-RW-317	2501311	1.84	6642891	2.09	
320-31468-14	NAWC-091117-FRB-317	2631497	1.84	6447036	2.09	
320-31468-15	NAWC-091117-RW-319	2337114	1.84	6427066	2.09	
320-31468-16	NAWC-091117-FRB-319	2681945	1.84	6402518	2.09	
320-31468-17	NAWC-091117-RW-321	2557163	1.84	6417541	2.09	
CCV 320-185408/33 CCVIS		2192291	1.84	5605406	2.09	
CCV 320-185409/33 CCVIS		2192291	1.84	5605406	2.09	
320-31468-18	NAWC-091117-FRB-321	2584590	1.84	6389473	2.10	
320-31468-19	NAWC-091117-RW-010	2457461	1.84	6222745	2.09	
320-31468-20	NAWC-091117-FRB-010	2679499	1.84	6439213	2.09	
CCV 320-185409/38 CCVIS		2137164	1.84	5388320	2.09	

13PFOA = 13C2-PFOA  
 PFOS = 13C4 PFOS

Area Limit = 50%-150% of internal standard area  
 RT Limit = ± 0.5 minutes of internal standard RT

# Column used to flag values outside QC limits

FORM VIII  
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Sample No.: CCV 320-185406/1 Date Analyzed: 09/20/2017 03:48  
 Instrument ID: A8\_N GC Column: GeminiC18 3x100 ID: 3 (mm)  
 Lab File ID (Standard): 2017.09.19\_537A\_001 Heated Purge: (Y/N) N  
 Calibration ID: 34457

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	1946548	1.85	5210623	2.10		
UPPER LIMIT	2725167	2.35	7294872	2.60		
LOWER LIMIT	1362584	1.35	3647436	1.60		
LAB SAMPLE ID	CLIENT SAMPLE ID					
MB 320-184385/1-A		2539018	1.85	6194895	2.10	
LLCS 320-184385/2-A		2322795	1.85	5655681	2.10	
LLCSD 320-184385/3-A		2191521	1.84	5502551	2.09	
320-31468-21	NAWC-091117-RW-162	2350014	1.84	5861531	2.10	
320-31468-22	NAWC-091117-FRB-162	2344211	1.85	6003115	2.10	
320-31468-23	WGNA-091117-DUP09	2370526	1.85	6043874	2.10	

13PFOA = 13C2-PFOA  
 13PFOA = 13C2-PFOA  
 PFOS = 13C4 PFOS  
 PFOS = 13C4 PFOS  
 Area Limit = 70%-140% of internal standard area  
 RT Limit = ± 0.5 minutes of internal standard RT

# Column used to flag values outside QC limits



FORM VIII  
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Sample No.: CCV 320-185406/9 Date Analyzed: 09/20/2017 04:26  
 Instrument ID: A8\_N GC Column: GeminiC18 3x100 ID: 3 (mm)  
 Lab File ID (Standard): 2017.09.19\_537A\_009 Heated Purge: (Y/N) N  
 Calibration ID: 34457

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	2062556	1.85	5491922	2.10		
UPPER LIMIT	2887578	2.35	7688691	2.60		
LOWER LIMIT	1443789	1.35	3844345	1.60		
LAB SAMPLE ID	CLIENT SAMPLE ID					
MB 320-184385/1-A		2539018	1.85	6194895	2.10	
LLCS 320-184385/2-A		2322795	1.85	5655681	2.10	
LLCSD 320-184385/3-A		2191521	1.84	5502551	2.09	
320-31468-21	NAWC-091117-RW-162	2350014	1.84	5861531	2.10	
320-31468-22	NAWC-091117-FRB-162	2344211	1.85	6003115	2.10	
320-31468-23	WGNA-091117-DUP09	2370526	1.85	6043874	2.10	

13PFOA = 13C2-PFOA  
 13PFOA = 13C2-PFOA  
 PFOS = 13C4 PFOS  
 PFOS = 13C4 PFOS  
 Area Limit = 70%-140% of internal standard area  
 RT Limit = ± 0.5 minutes of internal standard RT

# Column used to flag values outside QC limits

FORM VIII  
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Sample No.: CCV 320-185407/9 Date Analyzed: 09/20/2017 04:26  
 Instrument ID: A8\_N GC Column: GeminiC18 3x100 ID: 3 (mm)  
 Lab File ID (Standard): 2017.09.19\_537A\_009 Heated Purge: (Y/N) N  
 Calibration ID: 34457

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	2062556	1.85	5491922	2.10		
UPPER LIMIT	2887578	2.35	7688691	2.60		
LOWER LIMIT	1443789	1.35	3844345	1.60		
LAB SAMPLE ID	CLIENT SAMPLE ID					
MB 320-184382/1-A		2402894	1.85	5785526	2.10	
LCS 320-184382/2-A		2181509	1.84	5704391	2.09	
LCSD 320-184382/3-A		2332217	1.85	5855728	2.10	
320-31468-1	NAWC-091117-RW-106	2290728	1.84	5860369	2.09	
320-31468-2	NAWC-091117-FRB-106	2577088	1.84	6073981	2.09	
320-31468-3	NAWC-091117-RW-060	2387971	1.85	6309998	2.10	
320-31468-4	NAWC-091117-FRB-060	2308276	1.85	5696853	2.10	
320-31468-5	NAWC-091117-RW-314	2570115	1.85	6192393	2.10	
320-31468-6	NAWC-091117-FRB-314	2574796	1.85	6281693	2.10	
320-31468-7	NAWC-091117-RW-258	2394768	1.84	6099250	2.10	

13PFOA = 13C2-PFOA  
 13PFOA = 13C2-PFOA  
 PFOS = 13C4 PFOS  
 PFOS = 13C4 PFOS  
 Area Limit = 70%-140% of internal standard area  
 RT Limit = ± 0.5 minutes of internal standard RT

# Column used to flag values outside QC limits

FORM VIII  
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Sample No.: CCV 320-185407/21 Date Analyzed: 09/20/2017 05:23  
 Instrument ID: A8\_N GC Column: GeminiC18 3x100 ID: 3 (mm)  
 Lab File ID (Standard): 2017.09.19\_537A\_021 Heated Purge: (Y/N) N  
 Calibration ID: 34457

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	2036337	1.85	5320724	2.10		
UPPER LIMIT	2850872	2.35	7449014	2.60		
LOWER LIMIT	1425436	1.35	3724507	1.60		
LAB SAMPLE ID	CLIENT SAMPLE ID					
MB 320-184382/1-A		2402894	1.85	5785526	2.10	
LCS 320-184382/2-A		2181509	1.84	5704391	2.09	
LCSD 320-184382/3-A		2332217	1.85	5855728	2.10	
320-31468-1	NAWC-091117-RW-106	2290728	1.84	5860369	2.09	
320-31468-2	NAWC-091117-FRB-106	2577088	1.84	6073981	2.09	
320-31468-3	NAWC-091117-RW-060	2387971	1.85	6309998	2.10	
320-31468-4	NAWC-091117-FRB-060	2308276	1.85	5696853	2.10	
320-31468-5	NAWC-091117-RW-314	2570115	1.85	6192393	2.10	
320-31468-6	NAWC-091117-FRB-314	2574796	1.85	6281693	2.10	
320-31468-7	NAWC-091117-RW-258	2394768	1.84	6099250	2.10	

13PFOA = 13C2-PFOA  
 13PFOA = 13C2-PFOA  
 PFOS = 13C4 PFOS  
 PFOS = 13C4 PFOS  
 Area Limit = 70%-140% of internal standard area  
 RT Limit = ± 0.5 minutes of internal standard RT

# Column used to flag values outside QC limits

FORM VIII  
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Sample No.: CCV 320-185408/21 Date Analyzed: 09/20/2017 05:23  
 Instrument ID: A8\_N GC Column: GeminiC18 3x100 ID: 3 (mm)  
 Lab File ID (Standard): 2017.09.19\_537A\_021 Heated Purge: (Y/N) N  
 Calibration ID: 34457

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	2036337	1.85	5320724	2.10		
UPPER LIMIT	2850872	2.35	7449014	2.60		
LOWER LIMIT	1425436	1.35	3724507	1.60		
LAB SAMPLE ID	CLIENT SAMPLE ID					
320-31468-8	NAWC-091117-FRB-258	2497710	1.85	6286206	2.10	
320-31468-9	NAWC-091117-RW-048	2501111	1.85	6308482	2.10	
320-31468-10	NAWC-091117-FRB-048	2637228	1.85	6282400	2.10	
320-31468-11	NAWC-091117-RW-145	2432580	1.84	6418340	2.10	
320-31468-12	NAWC-091117-FRB-145	2685353	1.84	6382119	2.10	
320-31468-13	NAWC-091117-RW-317	2501311	1.84	6642891	2.09	
320-31468-14	NAWC-091117-FRB-317	2631497	1.84	6447036	2.09	
320-31468-15	NAWC-091117-RW-319	2337114	1.84	6427066	2.09	
320-31468-16	NAWC-091117-FRB-319	2681945	1.84	6402518	2.09	
320-31468-17	NAWC-091117-RW-321	2557163	1.84	6417541	2.09	

13PFOA = 13C2-PFOA  
 13PFOA = 13C2-PFOA  
 PFOS = 13C4 PFOS  
 PFOS = 13C4 PFOS  
 Area Limit = 70%-140% of internal standard area  
 RT Limit = ± 0.5 minutes of internal standard RT

# Column used to flag values outside QC limits

FORM VIII  
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Sample No.: CCV 320-185408/33 Date Analyzed: 09/20/2017 06:20  
 Instrument ID: A8\_N GC Column: GeminiC18 3x100 ID: 3 (mm)  
 Lab File ID (Standard): 2017.09.19\_537A\_033 Heated Purge: (Y/N) N  
 Calibration ID: 34457

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	2192291	1.84	5605406	2.09		
UPPER LIMIT	3069207	2.34	7847568	2.59		
LOWER LIMIT	1534604	1.34	3923784	1.59		
LAB SAMPLE ID	CLIENT SAMPLE ID					
320-31468-8	NAWC-091117-FRB-258	2497710	1.85	6286206	2.10	
320-31468-9	NAWC-091117-RW-048	2501111	1.85	6308482	2.10	
320-31468-10	NAWC-091117-FRB-048	2637228	1.85	6282400	2.10	
320-31468-11	NAWC-091117-RW-145	2432580	1.84	6418340	2.10	
320-31468-12	NAWC-091117-FRB-145	2685353	1.84	6382119	2.10	
320-31468-13	NAWC-091117-RW-317	2501311	1.84	6642891	2.09	
320-31468-14	NAWC-091117-FRB-317	2631497	1.84	6447036	2.09	
320-31468-15	NAWC-091117-RW-319	2337114	1.84	6427066	2.09	
320-31468-16	NAWC-091117-FRB-319	2681945	1.84	6402518	2.09	
320-31468-17	NAWC-091117-RW-321	2557163	1.84	6417541	2.09	

13PFOA = 13C2-PFOA  
 13PFOA = 13C2-PFOA  
 PFOS = 13C4 PFOS  
 PFOS = 13C4 PFOS  
 Area Limit = 70%-140% of internal standard area  
 RT Limit = ± 0.5 minutes of internal standard RT

# Column used to flag values outside QC limits

FORM VIII  
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Sample No.: CCV 320-185409/33 Date Analyzed: 09/20/2017 06:20  
 Instrument ID: A8\_N GC Column: GeminiC18 3x100 ID: 3 (mm)  
 Lab File ID (Standard): 2017.09.19\_537A\_033 Heated Purge: (Y/N) N  
 Calibration ID: 34457

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	2192291	1.84	5605406	2.09		
UPPER LIMIT	3069207	2.34	7847568	2.59		
LOWER LIMIT	1534604	1.34	3923784	1.59		
LAB SAMPLE ID	CLIENT SAMPLE ID					
320-31468-18	NAWC-091117-FRB-321	2584590	1.84	6389473	2.10	
320-31468-19	NAWC-091117-RW-010	2457461	1.84	6222745	2.09	
320-31468-20	NAWC-091117-FRB-010	2679499	1.84	6439213	2.09	

13PFOA = 13C2-PFOA  
 13PFOA = 13C2-PFOA  
 PFOS = 13C4 PFOS  
 PFOS = 13C4 PFOS  
 Area Limit = 70%-140% of internal standard area  
 RT Limit = ± 0.5 minutes of internal standard RT

# Column used to flag values outside QC limits

FORM VIII  
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Sample No.: CCV 320-185409/38 Date Analyzed: 09/20/2017 06:43  
 Instrument ID: A8\_N GC Column: GeminiC18 3x100 ID: 3 (mm)  
 Lab File ID (Standard): 2017.09.19\_537A\_038 Heated Purge: (Y/N) N  
 Calibration ID: 34457

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	2137164	1.84	5388320	2.09		
UPPER LIMIT	2992030	2.34	7543648	2.59		
LOWER LIMIT	1496015	1.34	3771824	1.59		
LAB SAMPLE ID	CLIENT SAMPLE ID					
320-31468-18	NAWC-091117-FRB-321	2584590	1.84	6389473	2.10	
320-31468-19	NAWC-091117-RW-010	2457461	1.84	6222745	2.09	
320-31468-20	NAWC-091117-FRB-010	2679499	1.84	6439213	2.09	

13PFOA = 13C2-PFOA  
 13PFOA = 13C2-PFOA  
 PFOS = 13C4 PFOS  
 PFOS = 13C4 PFOS  
 Area Limit = 70%-140% of internal standard area  
 RT Limit = ± 0.5 minutes of internal standard RT

# Column used to flag values outside QC limits

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-RW-106 Lab Sample ID: 320-31468-1  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_014.d  
 Analysis Method: 537 Date Collected: 09/11/2017 09:40  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 252.7(mL) Date Analyzed: 09/20/2017 04:49  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185407 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	17	J M	40	16	6.7
335-67-1	Perfluorooctanoic acid (PFOA)	20		20	7.9	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	7.9
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	8.9	J	30	12	5.4
375-85-9	Perfluoroheptanoic acid (PFHpA)	8.1	J	9.9	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	89	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	67	Q	70-130
STL00996	13C2 PFDA	100		70-130



TestAmerica Sacramento  
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_014.d  
 Lims ID: 320-31468-A-1-A  
 Client ID: NAWC-091117-RW-106  
 Sample Type: Client  
 Inject. Date: 20-Sep-2017 04:49:53 ALS Bottle#: 10 Worklist Smp#: 14  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: 320-31468-a-1-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:27 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d  
 Column 1 : Det: EXP1  
 Process Host: XAWRK008

First Level Reviewer: barnettj Date: 20-Sep-2017 13:25:00

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.396	1.402	-0.006	1.000	445923	1.81		90.3	
298.90 > 99.00	1.396	1.402	-0.006	1.000	285893		1.56(0.00-0.00)	313	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.517	1.524	-0.007	1.000	1807817	6.74		5539	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.662	1.668	-0.006	1.000	751914	2.25		117	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.662	1.668	-0.006	1.000	443249	2.05		45.2	
* 6 13C2-PFOA									
415.00 > 370.00	1.844	1.855	-0.011		2290728	10.0		6413	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.844	1.856	-0.012	1.000	1089742	5.17		40.5	
413.00 > 169.00	1.844	1.856	-0.012	1.000	597923		1.82(0.00-0.00)	1171	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.102	2.094	0.008	1.000	819625	4.31		144	M
499.00 > 99.00	2.102	2.094	0.008	1.000	150970		5.43(0.00-0.00)	98.4	M
* 7 13C4 PFOS									
503.00 > 80.00	2.094	2.108	-0.014		5860369	28.7		1986	
9 Perfluorononanoic acid									
463.00 > 419.00	2.109	2.116	-0.007	1.000	132853	0.9327		3.7	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.276	2.282	-0.006	1.000	1271468	9.95		11161	

## QC Flag Legend

Review Flags

M - Manually Integrated

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_014.d

Injection Date: 20-Sep-2017 04:49:53

Instrument ID: A8\_N

Lims ID: 320-31468-A-1-A

Lab Sample ID: 320-31468-1

Client ID: NAWC-091117-RW-106

Operator ID: SACINSTLCMS01

ALS Bottle#: 10

Worklist Smp#: 14

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537\_A8\_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




\* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

\* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento  
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_014.d  
 Lims ID: 320-31468-A-1-A  
 Client ID: NAWC-091117-RW-106  
 Sample Type: Client  
 Inject. Date: 20-Sep-2017 04:49:53 ALS Bottle#: 10 Worklist Smp#: 14  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: 320-31468-a-1-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:27 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d  
 Column 1 : Det: EXP1  
 Process Host: XAWRK008

First Level Reviewer: barnettj Date: 20-Sep-2017 13:25:00

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	6.74	67.35
\$ 10 13C2 PFDA	10.0	9.95	99.51

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_014.d  
Injection Date: 20-Sep-2017 04:49:53 Instrument ID: A8\_N  
Lims ID: 320-31468-A-1-A Lab Sample ID: 320-31468-1  
Client ID: NAWC-091117-RW-106  
Operator ID: SACINSTLCMS01 ALS Bottle#: 10 Worklist Smp#: 14  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.10  
Area: 819625  
Amount: 4.305199  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 13:24:06  
Audit Action: Assigned Compound ID

Audit Reason: Missed Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_014.d  
Injection Date: 20-Sep-2017 04:49:53 Instrument ID: A8\_N  
Lims ID: 320-31468-A-1-A Lab Sample ID: 320-31468-1  
Client ID: NAWC-091117-RW-106  
Operator ID: SACINSTLCMS01 ALS Bottle#: 10 Worklist Smp#: 14  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.10  
Area: 150970  
Amount: 4.305199  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 13:24:39

Audit Action: Manually Integrated

Audit Reason: Missed Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_014.d  
Injection Date: 20-Sep-2017 04:49:53 Instrument ID: A8\_N  
Lims ID: 320-31468-A-1-A Lab Sample ID: 320-31468-1  
Client ID: NAWC-091117-RW-106  
Operator ID: SACINSTLCMS01 ALS Bottle#: 10 Worklist Smp#: 14  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.10  
Area: 819625  
Amount: 4.305199  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 13:24:39

Audit Action: Manually Integrated

Audit Reason: Missed Peak



FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-FRB-106 Lab Sample ID: 320-31468-2  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_015.d  
 Analysis Method: 537 Date Collected: 09/11/2017 09:35  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 258.9(mL) Date Analyzed: 09/20/2017 04:54  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185407 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	39	15	6.6
335-67-1	Perfluorooctanoic acid (PFOA)	7.7	U	19	7.7	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.7
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	29	12	5.3
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.9	U	9.7	3.9	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	35	U	87	35	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	82		70-130
STL00996	13C2 PFDA	105		70-130

TestAmerica Sacramento  
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_015.d  
 Lims ID: 320-31468-A-2-A  
 Client ID: NAWC-091117-FRB-106  
 Sample Type: Client  
 Inject. Date: 20-Sep-2017 04:54:39 ALS Bottle#: 11 Worklist Smp#: 15  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: 320-31468-a-2-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:27 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d

Column 1 : Det: EXP1  
 Process Host: XAWRK008

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
\$ 2 13C2 PFHxA	315.00 > 270.00	1.517	1.524	-0.007	1.000	2466570	8.17	8648	
* 6 13C2-PFOA	415.00 > 370.00	1.844	1.855	-0.011		2577088	10.0	8143	
* 7 13C4 PFOS	503.00 > 80.00	2.094	2.108	-0.014		6073981	28.7	4791	
\$ 10 13C2 PFDA	515.00 > 470.00	2.276	2.282	-0.006	1.000	1515069	10.5	12848	

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_015.d

Injection Date: 20-Sep-2017 04:54:39

Instrument ID: A8\_N

Lims ID: 320-31468-A-2-A

Lab Sample ID: 320-31468-2

Client ID: NAWC-091117-FRB-106

Operator ID: SACINSTLCMS01

ALS Bottle#: 11

Worklist Smp#: 15




Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537\_A8\_N

Limit Group: LC 537 ICAL




1 Perfluorobutanesulfonic acid (ND) 1 Perfluorobutanesulfonic acid (ND) \$ 2 13C2 PFHxA






3 Perfluorohexanesulfonic acid (ND) 4 Perfluoroheptanoic acid (ND) \* 6 13C2-PFOA




5 Perfluorooctanoic acid (ND) 5 Perfluorooctanoic acid (ND) 8 Perfluorooctane sulfonic acid (ND)



8 Perfluorooctane sulfonic acid (ND) \* 7 13C4 PFOS 9 Perfluorononanoic acid (ND)



\$ 10 13C2 PFDA



TestAmerica Sacramento  
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_015.d  
 Lims ID: 320-31468-A-2-A  
 Client ID: NAWC-091117-FRB-106  
 Sample Type: Client  
 Inject. Date: 20-Sep-2017 04:54:39 ALS Bottle#: 11 Worklist Smp#: 15  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: 320-31468-a-2-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:27 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d

Column 1 : Det: EXP1  
 Process Host: XAWRK008

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	8.17	81.68
\$ 10 13C2 PFDA	10.0	10.5	105.40

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-RW-060 Lab Sample ID: 320-31468-3  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_016.d  
 Analysis Method: 537 Date Collected: 09/11/2017 09:55  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 261.7(mL) Date Analyzed: 09/20/2017 04:59  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185407 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	27	J M	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	17	J	19	7.6	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	9.9	J	29	11	5.3
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.9	J	9.6	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	86	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	71		70-130
STL00996	13C2 PFDA	114		70-130

TestAmerica Sacramento  
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_016.d  
 Lims ID: 320-31468-A-3-A  
 Client ID: NAWC-091117-RW-060  
 Sample Type: Client  
 Inject. Date: 20-Sep-2017 04:59:25 ALS Bottle#: 12 Worklist Smp#: 16  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: 320-31468-a-3-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:27 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d  
 Column 1 : Det: EXP1  
 Process Host: XAWRK008

First Level Reviewer: barnettj Date: 20-Sep-2017 13:25:45

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.404	1.402	0.002	1.000	329313	1.24		106	
298.90 > 99.00	1.404	1.402	0.002	1.000	203453		1.62(0.00-0.00)	343	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.525	1.524	0.001	1.000	1998146	7.14		6791	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.669	1.668	0.001	1.000	931087	2.58		173	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.669	1.668	0.001	1.000	232151	1.03		27.0	
* 6 13C2-PFOA									
415.00 > 370.00	1.851	1.855	-0.004		2387971	10.0		6917	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.851	1.856	-0.005	1.000	984268	4.48		37.8	
413.00 > 169.00	1.851	1.856	-0.005	1.000	572729		1.72(0.00-0.00)	1341	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.102	2.094	0.008	1.000	1433665	6.99		278	M
499.00 > 99.00	2.102	2.094	0.008	1.000	253386		5.66(0.00-0.00)	174	M
* 7 13C4 PFOS									
503.00 > 80.00	2.102	2.108	-0.006		6309998	28.7		2529	
9 Perfluorononanoic acid									
463.00 > 419.00	2.109	2.116	-0.007	1.000	76359	0.5142		2.3	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.276	2.282	-0.006	1.000	1511967	11.4		12776	

## QC Flag Legend

### Review Flags

M - Manually Integrated



TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_016.d

Injection Date: 20-Sep-2017 04:59:25

Instrument ID: A8\_N

Lims ID: 320-31468-A-3-A

Lab Sample ID: 320-31468-3

Client ID: NAWC-091117-RW-060

Operator ID: SACINSTLCMS01

ALS Bottle#: 12

Worklist Smp#: 16

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537\_A8\_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




\* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

\* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento  
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_016.d  
 Lims ID: 320-31468-A-3-A  
 Client ID: NAWC-091117-RW-060  
 Sample Type: Client  
 Inject. Date: 20-Sep-2017 04:59:25 ALS Bottle#: 12 Worklist Smp#: 16  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: 320-31468-a-3-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:27 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d  
 Column 1 : Det: EXP1  
 Process Host: XAWRK008

First Level Reviewer: barnettj Date: 20-Sep-2017 13:25:45

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	7.14	71.41
\$ 10 13C2 PFDA	10.0	11.4	113.52

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_016.d  
Injection Date: 20-Sep-2017 04:59:25 Instrument ID: A8\_N  
Lims ID: 320-31468-A-3-A Lab Sample ID: 320-31468-3  
Client ID: NAWC-091117-RW-060  
Operator ID: SACINSTLCMS01 ALS Bottle#: 12 Worklist Smp#: 16  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.10  
Area: 1433665  
Amount: 6.993932  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 13:25:14  
Audit Action: Assigned Compound ID

Audit Reason: Missed Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_016.d  
Injection Date: 20-Sep-2017 04:59:25 Instrument ID: A8\_N  
Lims ID: 320-31468-A-3-A Lab Sample ID: 320-31468-3  
Client ID: NAWC-091117-RW-060  
Operator ID: SACINSTLCMS01 ALS Bottle#: 12 Worklist Smp#: 16  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.10  
Area: 253386  
Amount: 6.993932  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 13:25:29

Audit Action: Manually Integrated

Audit Reason: Missed Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_016.d  
Injection Date: 20-Sep-2017 04:59:25 Instrument ID: A8\_N  
Lims ID: 320-31468-A-3-A Lab Sample ID: 320-31468-3  
Client ID: NAWC-091117-RW-060  
Operator ID: SACINSTLCMS01 ALS Bottle#: 12 Worklist Smp#: 16  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.10  
Area: 1433665  
Amount: 6.993932  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 13:25:29

Audit Action: Manually Integrated

Audit Reason: Missed Peak

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-FRB-060 Lab Sample ID: 320-31468-4  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_017.d  
 Analysis Method: 537 Date Collected: 09/11/2017 09:50  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 259.9(mL) Date Analyzed: 09/20/2017 05:04  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185407 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	7.7	U	19	7.7	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.7
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	29	12	5.3
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	U	9.6	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	35	U	87	35	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	86		70-130
STL00996	13C2 PFDA	107		70-130

TestAmerica Sacramento  
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_017.d  
 Lims ID: 320-31468-A-4-A  
 Client ID: NAWC-091117-FRB-060  
 Sample Type: Client  
 Inject. Date: 20-Sep-2017 05:04:12 ALS Bottle#: 13 Worklist Smp#: 17  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: 320-31468-a-4-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:27 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d

Column 1 : Det: EXP1  
 Process Host: XAWRK008

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
\$ 2 13C2 PFHxA	315.00 > 270.00	1.517	1.524	-0.007	1.000	2314636	8.56	7504	
* 6 13C2-PFOA	415.00 > 370.00	1.851	1.855	-0.004		2308276	10.0	6492	
* 7 13C4 PFOS	503.00 > 80.00	2.102	2.108	-0.006		5696853	28.7	4726	
\$ 10 13C2 PFDA	515.00 > 470.00	2.276	2.282	-0.006	1.000	1381748	10.7	12044	



TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_017.d

Injection Date: 20-Sep-2017 05:04:12

Instrument ID: A8\_N

Lims ID: 320-31468-A-4-A

Lab Sample ID: 320-31468-4

Client ID: NAWC-091117-FRB-060

Operator ID: SACINSTLCMS01

ALS Bottle#: 13

Worklist Smp#: 17

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537\_A8\_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid (ND)

1 Perfluorobutanesulfonic acid (ND)




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid (ND)

4 Perfluoroheptanoic acid (ND)




\* 6 13C2-PFOA



5 Perfluorooctanoic acid (ND)

5 Perfluorooctanoic acid (ND)




8 Perfluorooctane sulfonic acid (ND)




8 Perfluorooctane sulfonic acid (ND)

\* 7 13C4 PFOS

9 Perfluorononanoic acid (ND)



\$ 10 13C2 PFDA



TestAmerica Sacramento  
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_017.d  
 Lims ID: 320-31468-A-4-A  
 Client ID: NAWC-091117-FRB-060  
 Sample Type: Client  
 Inject. Date: 20-Sep-2017 05:04:12 ALS Bottle#: 13 Worklist Smp#: 17  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: 320-31468-a-4-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:27 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d

Column 1 : Det: EXP1  
 Process Host: XAWRK008

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	8.56	85.58
\$ 10 13C2 PFDA	10.0	10.7	107.32

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-RW-314 Lab Sample ID: 320-31468-5  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_018.d  
 Analysis Method: 537 Date Collected: 09/11/2017 10:25  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 262.7(mL) Date Analyzed: 09/20/2017 05:08  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185407 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	J M	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	17	J	19	7.6	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	29	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.4	J	9.5	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	86	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	72		70-130
STL00996	13C2 PFDA	104		70-130

TestAmerica Sacramento  
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_018.d  
 Lims ID: 320-31468-A-5-A  
 Client ID: NAWC-091117-RW-314  
 Sample Type: Client  
 Inject. Date: 20-Sep-2017 05:08:57 ALS Bottle#: 14 Worklist Smp#: 18  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: 320-31468-a-5-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:27 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d  
 Column 1 : Det: EXP1  
 Process Host: XAWRK008

First Level Reviewer: barnettj Date: 20-Sep-2017 13:26:37

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.396	1.402	-0.006	1.000	250880	0.9600		247	
298.90 > 99.00	1.396	1.402	-0.006	1.000	163774		1.53(0.00-0.00)	340	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.517	1.524	-0.007	1.000	2181599	7.24		7787	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.662	1.668	-0.006	1.000	290467	0.8212		130	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.662	1.668	-0.006	1.000	280493	1.16		47.2	
* 6 13C2-PFOA									
415.00 > 370.00	1.851	1.855	-0.004		2570115	10.0		8557	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.851	1.856	-0.005	1.000	1064334	4.50		46.3	
413.00 > 169.00	1.851	1.856	-0.005	1.000	589803		1.80(0.00-0.00)	1430	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.102	2.094	0.008	1.000	796790	3.96		246	M
499.00 > 99.00	2.102	2.094	0.008	1.000	127095		6.27(0.00-0.00)	96.4	M
* 7 13C4 PFOS									
503.00 > 80.00	2.102	2.108	-0.006		6192393	28.7		4275	
9 Perfluorononanoic acid									
463.00 > 419.00	2.109	2.116	-0.007	1.000	67671	0.4234		2.1	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.276	2.282	-0.006	1.000	1485346	10.4		13583	

## QC Flag Legend

### Review Flags

M - Manually Integrated

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_018.d

Injection Date: 20-Sep-2017 05:08:57

Instrument ID: A8\_N

Lims ID: 320-31468-A-5-A

Lab Sample ID: 320-31468-5

Client ID: NAWC-091117-RW-314

Operator ID: SACINSTLCMS01

ALS Bottle#: 14

Worklist Smp#: 18

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537\_A8\_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




\* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

\* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA





TestAmerica Sacramento  
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_018.d  
 Lims ID: 320-31468-A-5-A  
 Client ID: NAWC-091117-RW-314  
 Sample Type: Client  
 Inject. Date: 20-Sep-2017 05:08:57 ALS Bottle#: 14 Worklist Smp#: 18  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: 320-31468-a-5-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:27 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d  
 Column 1 : Det: EXP1  
 Process Host: XAWRK008

First Level Reviewer: barnettj Date: 20-Sep-2017 13:26:37

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	7.24	72.44
\$ 10 13C2 PFDA	10.0	10.4	103.61

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_018.d  
Injection Date: 20-Sep-2017 05:08:57 Instrument ID: A8\_N  
Lims ID: 320-31468-A-5-A Lab Sample ID: 320-31468-5  
Client ID: NAWC-091117-RW-314  
Operator ID: SACINSTLCMS01 ALS Bottle#: 14 Worklist Smp#: 18  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.10  
Area: 796790  
Amount: 3.960849  
Amount Units: ng/ml



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_018.d  
Injection Date: 20-Sep-2017 05:08:57 Instrument ID: A8\_N  
Lims ID: 320-31468-A-5-A Lab Sample ID: 320-31468-5  
Client ID: NAWC-091117-RW-314  
Operator ID: SACINSTLCMS01 ALS Bottle#: 14 Worklist Smp#: 18  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.10  
Area: 127095  
Amount: 3.960849  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 13:26:19

Audit Action: Manually Integrated

Audit Reason: Missed Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_018.d  
Injection Date: 20-Sep-2017 05:08:57 Instrument ID: A8\_N  
Lims ID: 320-31468-A-5-A Lab Sample ID: 320-31468-5  
Client ID: NAWC-091117-RW-314  
Operator ID: SACINSTLCMS01 ALS Bottle#: 14 Worklist Smp#: 18  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.10  
Area: 796790  
Amount: 3.960849  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 13:26:19

Audit Action: Manually Integrated

Audit Reason: Missed Peak

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-FRB-314 Lab Sample ID: 320-31468-6  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_019.d  
 Analysis Method: 537 Date Collected: 09/11/2017 10:20  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 265.6(mL) Date Analyzed: 09/20/2017 05:13  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185407 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	38	15	6.4
335-67-1	Perfluorooctanoic acid (PFOA)	7.5	U	19	7.5	2.6
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.5
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	U	9.4	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	85	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	82		70-130
STL00996	13C2 PFDA	102		70-130

TestAmerica Sacramento  
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_019.d  
 Lims ID: 320-31468-A-6-A  
 Client ID: NAWC-091117-FRB-314  
 Sample Type: Client  
 Inject. Date: 20-Sep-2017 05:13:41 ALS Bottle#: 15 Worklist Smp#: 19  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: 320-31468-a-6-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:27 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d

Column 1 : Det: EXP1  
 Process Host: XAWRK008

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
\$ 2 13C2 PFHxA	315.00 > 270.00	1.517	1.524	-0.007	1.000	2484950	8.24	7713	
* 6 13C2-PFOA	415.00 > 370.00	1.851	1.855	-0.004		2574796	10.0	8898	
* 7 13C4 PFOS	503.00 > 80.00	2.102	2.108	-0.006		6281693	28.7	4780	
\$ 10 13C2 PFDA	515.00 > 470.00	2.276	2.282	-0.006	1.000	1469522	10.2	13059	

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_019.d

Injection Date: 20-Sep-2017 05:13:41

Instrument ID: A8\_N

Lims ID: 320-31468-A-6-A

Lab Sample ID: 320-31468-6

Client ID: NAWC-091117-FRB-314

Operator ID: SACINSTLCMS01

ALS Bottle#: 15

Worklist Smp#: 19




Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537\_A8\_N

Limit Group: LC 537 ICAL




1 Perfluorobutanesulfonic acid (ND) 1 Perfluorobutanesulfonic acid (ND) \$ 2 13C2 PFHxA






3 Perfluorohexanesulfonic acid (ND) 4 Perfluoroheptanoic acid (ND) \* 6 13C2-PFOA




5 Perfluorooctanoic acid (ND) 5 Perfluorooctanoic acid (ND) 8 Perfluorooctane sulfonic acid (ND)



8 Perfluorooctane sulfonic acid (ND) \* 7 13C4 PFOS 9 Perfluorononanoic acid (ND)



\$ 10 13C2 PFDA





TestAmerica Sacramento  
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_019.d  
 Lims ID: 320-31468-A-6-A  
 Client ID: NAWC-091117-FRB-314  
 Sample Type: Client  
 Inject. Date: 20-Sep-2017 05:13:41 ALS Bottle#: 15 Worklist Smp#: 19  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: 320-31468-a-6-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:27 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d

Column 1 : Det: EXP1  
 Process Host: XAWRK008

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	8.24	82.36
\$ 10 13C2 PFDA	10.0	10.2	102.32

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-RW-258 Lab Sample ID: 320-31468-7  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_020.d  
 Analysis Method: 537 Date Collected: 09/11/2017 11:00  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 267(mL) Date Analyzed: 09/20/2017 05:18  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185407 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	18	J M	37	15	6.4
335-67-1	Perfluorooctanoic acid (PFOA)	21		19	7.5	2.6
375-95-1	Perfluorononanoic acid (PFNA)	12	J	22	19	7.5
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.1
375-85-9	Perfluoroheptanoic acid (PFHpA)	7.7	J	9.4	3.7	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	84	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	72		70-130
STL00996	13C2 PFDA	98		70-130

TestAmerica Sacramento  
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_020.d  
 Lims ID: 320-31468-A-7-A  
 Client ID: NAWC-091117-RW-258  
 Sample Type: Client  
 Inject. Date: 20-Sep-2017 05:18:26 ALS Bottle#: 16 Worklist Smp#: 20  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: 320-31468-a-7-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:27 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d  
 Column 1 : Det: EXP1  
 Process Host: XAWRK008

First Level Reviewer: barnettj Date: 20-Sep-2017 13:27:28

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.396	1.402	-0.006	1.000	552745	2.15		116	
298.90 > 99.00	1.396	1.402	-0.006	1.000	368552		1.50(0.00-0.00)	521	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.517	1.524	-0.007	1.000	2009631	7.16		6723	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.662	1.668	-0.006	1.000	177340	0.5090		21.9	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.662	1.668	-0.006	1.000	464818	2.06		47.3	
* 6 13C2-PFOA									
415.00 > 370.00	1.844	1.855	-0.011		2394768	10.0		6111	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.851	1.856	-0.005	1.000	1236417	5.62		43.0	
413.00 > 169.00	1.851	1.856	-0.005	1.000	713019		1.73(0.00-0.00)	1494	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.102	2.094	0.008	1.000	951609	4.80		133	M
499.00 > 99.00	2.102	2.094	0.008	1.000	167546		5.68(0.00-0.00)	122	M
* 7 13C4 PFOS									
503.00 > 80.00	2.102	2.108	-0.006		6099250	28.7		1418	
9 Perfluorononanoic acid									
463.00 > 419.00	2.109	2.116	-0.007	1.000	492236	3.31		12.9	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.276	2.282	-0.006	1.000	1302376	9.75		10415	

## QC Flag Legend

Review Flags

M - Manually Integrated

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_020.d

Injection Date: 20-Sep-2017 05:18:26

Instrument ID: A8\_N

Lims ID: 320-31468-A-7-A

Lab Sample ID: 320-31468-7

Client ID: NAWC-091117-RW-258

Operator ID: SACINSTLCMS01

ALS Bottle#: 16

Worklist Smp#: 20

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537\_A8\_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




\* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

\* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento  
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_020.d  
 Lims ID: 320-31468-A-7-A  
 Client ID: NAWC-091117-RW-258  
 Sample Type: Client  
 Inject. Date: 20-Sep-2017 05:18:26 ALS Bottle#: 16 Worklist Smp#: 20  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: 320-31468-a-7-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:27 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d  
 Column 1 : Det: EXP1  
 Process Host: XAWRK008

First Level Reviewer: barnettj Date: 20-Sep-2017 13:27:28

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	7.16	71.62
\$ 10 13C2 PFDA	10.0	9.75	97.50

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_020.d  
Injection Date: 20-Sep-2017 05:18:26 Instrument ID: A8\_N  
Lims ID: 320-31468-A-7-A Lab Sample ID: 320-31468-7  
Client ID: NAWC-091117-RW-258  
Operator ID: SACINSTLCMS01 ALS Bottle#: 16 Worklist Smp#: 20  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.10  
Area: 951609  
Amount: 4.802696  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 13:26:49  
Audit Action: Assigned Compound ID

Audit Reason: Missed Peak



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_020.d  
Injection Date: 20-Sep-2017 05:18:26 Instrument ID: A8\_N  
Lims ID: 320-31468-A-7-A Lab Sample ID: 320-31468-7  
Client ID: NAWC-091117-RW-258  
Operator ID: SACINSTLCMS01 ALS Bottle#: 16 Worklist Smp#: 20  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.10  
Area: 167546  
Amount: 4.802696  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 13:27:08

Audit Action: Manually Integrated

Audit Reason: Missed Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_020.d  
Injection Date: 20-Sep-2017 05:18:26 Instrument ID: A8\_N  
Lims ID: 320-31468-A-7-A Lab Sample ID: 320-31468-7  
Client ID: NAWC-091117-RW-258  
Operator ID: SACINSTLCMS01 ALS Bottle#: 16 Worklist Smp#: 20  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.10  
Area: 951609  
Amount: 4.802696  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 13:27:08

Audit Action: Manually Integrated

Audit Reason: Missed Peak

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-FRB-258 Lab Sample ID: 320-31468-8  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_023.d  
 Analysis Method: 537 Date Collected: 09/11/2017 10:55  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 261.6(mL) Date Analyzed: 09/20/2017 05:32  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	7.6	U	19	7.6	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	29	11	5.3
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	U	9.6	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	86	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	86		70-130
STL00996	13C2 PFDA	101		70-130

TestAmerica Sacramento  
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_023.d  
 Lims ID: 320-31468-A-8-A  
 Client ID: NAWC-091117-FRB-258  
 Sample Type: Client  
 Inject. Date: 20-Sep-2017 05:32:39 ALS Bottle#: 17 Worklist Smp#: 23  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: 320-31468-a-8-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:40 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d

Column 1 : Det: EXP1  
 Process Host: XAWRK008

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
\$ 2 13C2 PFHxA	315.00 > 270.00	1.525	1.524	0.001	1.000	2503772	8.55	8235	
* 6 13C2-PFOA	415.00 > 370.00	1.851	1.855	-0.004		2497710	10.0	7601	
* 7 13C4 PFOS	503.00 > 80.00	2.102	2.108	-0.006		6286206	28.7	5807	
\$ 10 13C2 PFDA	515.00 > 470.00	2.276	2.282	-0.006	1.000	1412493	10.1	11685	

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_023.d

Injection Date: 20-Sep-2017 05:32:39

Instrument ID: A8\_N

Lims ID: 320-31468-A-8-A

Lab Sample ID: 320-31468-8

Client ID: NAWC-091117-FRB-258

Operator ID: SACINSTLCMS01

ALS Bottle#: 17

Worklist Smp#: 23

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537\_A8\_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid (ND)

1 Perfluorobutanesulfonic acid (ND)




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid (ND)

4 Perfluoroheptanoic acid (ND)




\* 6 13C2-PFOA



5 Perfluorooctanoic acid (ND)

5 Perfluorooctanoic acid (ND)




8 Perfluorooctane sulfonic acid (ND)




8 Perfluorooctane sulfonic acid (ND)

\* 7 13C4 PFOS

9 Perfluorononanoic acid (ND)



\$ 10 13C2 PFDA



TestAmerica Sacramento  
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_023.d  
 Lims ID: 320-31468-A-8-A  
 Client ID: NAWC-091117-FRB-258  
 Sample Type: Client  
 Inject. Date: 20-Sep-2017 05:32:39 ALS Bottle#: 17 Worklist Smp#: 23  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: 320-31468-a-8-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:40 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d

Column 1 : Det: EXP1  
 Process Host: XAWRK008

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	8.55	85.55
\$ 10 13C2 PFDA	10.0	10.1	101.39

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-RW-048 Lab Sample ID: 320-31468-9  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_024.d  
 Analysis Method: 537 Date Collected: 09/11/2017 13:05  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 263.9(mL) Date Analyzed: 09/20/2017 05:37  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U M	38	15	6.4
335-67-1	Perfluorooctanoic acid (PFOA)	4.5	J M	19	7.6	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	U	9.5	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	85	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	74		70-130
STL00996	13C2 PFDA	111		70-130



TestAmerica Sacramento  
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_024.d  
 Lims ID: 320-31468-A-9-A  
 Client ID: NAWC-091117-RW-048  
 Sample Type: Client  
 Inject. Date: 20-Sep-2017 05:37:24 ALS Bottle#: 18 Worklist Smp#: 24  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: 320-31468-a-9-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:40 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d  
 Column 1 : Det: EXP1  
 Process Host: XAWRK008

First Level Reviewer: barnettj Date: 20-Sep-2017 13:30:43

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.396	1.402	-0.006	1.000	129290	0.4852		115	
298.90 > 99.00	1.404	1.402	0.002	1.005	78316		1.65(0.00-0.00)	145	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.517	1.524	-0.007	1.000	2173184	7.42		7198	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.662	1.668	-0.006	1.000	193757	0.5377		70.0	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.669	1.668	0.001	1.000	70158	0.2979		10.4	
* 6 13C2-PFOA									
415.00 > 370.00	1.851	1.855	-0.004		2501111	10.0		7114	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.851	1.856	-0.005	1.000	275068	1.20		11.3	M
413.00 > 169.00	1.851	1.856	-0.005	1.000	164373		1.67(0.00-0.00)	445	M
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.011	2.094	-0.083	1.000	279841	1.37		68.4	M
499.00 > 99.00	2.102	2.094	0.008	1.045	37395		7.48(0.00-0.00)	17.5	M
* 7 13C4 PFOS									
503.00 > 80.00	2.102	2.108	-0.006		6308482	28.7		3157	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.276	2.282	-0.006	1.000	1549878	11.1		12048	

## QC Flag Legend

Review Flags

M - Manually Integrated

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_024.d

Injection Date: 20-Sep-2017 05:37:24

Instrument ID: A8\_N

Lims ID: 320-31468-A-9-A

Lab Sample ID: 320-31468-9

Client ID: NAWC-091117-RW-048

Operator ID: SACINSTLCMS01

ALS Bottle#: 18

Worklist Smp#: 24

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537\_A8\_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




\* 6 13C2-PFOA



5 Perfluorooctanoic acid (M)

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid

\* 7 13C4 PFOS

9 Perfluorononanoic acid (ND)



\$ 10 13C2 PFDA



TestAmerica Sacramento  
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_024.d  
 Lims ID: 320-31468-A-9-A  
 Client ID: NAWC-091117-RW-048  
 Sample Type: Client  
 Inject. Date: 20-Sep-2017 05:37:24 ALS Bottle#: 18 Worklist Smp#: 24  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: 320-31468-a-9-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:40 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d  
 Column 1 : Det: EXP1  
 Process Host: XAWRK008

First Level Reviewer: barnettj Date: 20-Sep-2017 13:30:43

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	7.42	74.15
\$ 10 13C2 PFDA	10.0	11.1	111.10

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_024.d  
Injection Date: 20-Sep-2017 05:37:24 Instrument ID: A8\_N  
Lims ID: 320-31468-A-9-A Lab Sample ID: 320-31468-9  
Client ID: NAWC-091117-RW-048  
Operator ID: SACINSTLCMS01 ALS Bottle#: 18 Worklist Smp#: 24  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1


Signal: 1

Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results



RT: 2.01  
Area: 279841  
Amount: 1.365493  
Amount Units: ng/ml

Reviewer: barnettj, 20-Sep-2017 13:29:45  
Audit Action: Assigned Compound ID

Audit Reason: Missed Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_024.d  
Injection Date: 20-Sep-2017 05:37:24 Instrument ID: A8\_N  
Lims ID: 320-31468-A-9-A Lab Sample ID: 320-31468-9  
Client ID: NAWC-091117-RW-048  
Operator ID: SACINSTLCMS01 ALS Bottle#: 18 Worklist Smp#: 24  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.01  
Area: 279841  
Amount: 1.365493  
Amount Units: ng/ml



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_024.d  
Injection Date: 20-Sep-2017 05:37:24 Instrument ID: A8\_N  
Lims ID: 320-31468-A-9-A Lab Sample ID: 320-31468-9  
Client ID: NAWC-091117-RW-048  
Operator ID: SACINSTLCMS01 ALS Bottle#: 18 Worklist Smp#: 24  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

5 Perfluorooctanoic acid, CAS: 335-67-1

Signal: 1


RT: 1.85  
Area: 300140  
Amount: 1.305155  
Amount Units: ng/ml

Processing Integration Results



RT: 1.85  
Area: 275068  
Amount: 1.196130  
Amount Units: ng/ml

Manual Integration Results



Reviewer: barnettj, 20-Sep-2017 13:30:29  
Audit Action: Manually Integrated

Audit Reason: Baseline



FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-FRB-048 Lab Sample ID: 320-31468-10  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_025.d  
 Analysis Method: 537 Date Collected: 09/11/2017 13:00  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 266.7(mL) Date Analyzed: 09/20/2017 05:42  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	37	15	6.4
335-67-1	Perfluorooctanoic acid (PFOA)	7.5	U	19	7.5	2.6
375-95-1	Perfluorononanoic acid (PFNA)	19	U	22	19	7.5
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.7	U	9.4	3.7	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	84	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	84		70-130
STL00996	13C2 PFDA	102		70-130

TestAmerica Sacramento  
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_025.d  
 Lims ID: 320-31468-A-10-A  
 Client ID: NAWC-091117-FRB-048  
 Sample Type: Client  
 Inject. Date: 20-Sep-2017 05:42:08 ALS Bottle#: 19 Worklist Smp#: 25  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: 320-31468-a-10-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:40 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d

Column 1 : Det: EXP1  
 Process Host: XAWRK008

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
\$ 2 13C2 PFHxA	315.00 > 270.00	1.525	1.524	0.001	1.000	2582511	8.36	11939	
* 6 13C2-PFOA	415.00 > 370.00	1.851	1.855	-0.004		2637228	10.0	9674	
* 7 13C4 PFOS	503.00 > 80.00	2.102	2.108	-0.006		6282400	28.7	5776	
\$ 10 13C2 PFDA	515.00 > 470.00	2.276	2.282	-0.006	1.000	1493987	10.2	14231	

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_025.d

Injection Date: 20-Sep-2017 05:42:08

Instrument ID: A8\_N

Lims ID: 320-31468-A-10-A

Lab Sample ID: 320-31468-10

Client ID: NAWC-091117-FRB-048

Operator ID: SACINSTLCMS01

ALS Bottle#: 19

Worklist Smp#: 25




Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537\_A8\_N

Limit Group: LC 537 ICAL




1 Perfluorobutanesulfonic acid (ND) 1 Perfluorobutanesulfonic acid (ND) \$ 2 13C2 PFHxA






3 Perfluorohexanesulfonic acid (ND) 4 Perfluoroheptanoic acid (ND) \* 6 13C2-PFOA




5 Perfluorooctanoic acid (ND) 5 Perfluorooctanoic acid (ND) 8 Perfluorooctane sulfonic acid (ND)



8 Perfluorooctane sulfonic acid (ND) \* 7 13C4 PFOS 9 Perfluorononanoic acid (ND)



\$ 10 13C2 PFDA



TestAmerica Sacramento  
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_025.d  
 Lims ID: 320-31468-A-10-A  
 Client ID: NAWC-091117-FRB-048  
 Sample Type: Client  
 Inject. Date: 20-Sep-2017 05:42:08 ALS Bottle#: 19 Worklist Smp#: 25  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: 320-31468-a-10-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:40 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d

Column 1 : Det: EXP1  
 Process Host: XAWRK008

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	8.36	83.57
\$ 10 13C2 PFDA	10.0	10.2	101.56

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-RW-145 Lab Sample ID: 320-31468-11  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_026.d  
 Analysis Method: 537 Date Collected: 09/11/2017 13:35  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 269(mL) Date Analyzed: 09/20/2017 05:46  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	19	J M	37	15	6.3
335-67-1	Perfluorooctanoic acid (PFOA)	20		19	7.4	2.6
375-95-1	Perfluorononanoic acid (PFNA)	19	U	22	19	7.4
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	7.3	J	28	11	5.1
375-85-9	Perfluoroheptanoic acid (PFHpA)	5.6	J	9.3	3.7	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	33	U	84	33	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	74		70-130
STL00996	13C2 PFDA	115		70-130

TestAmerica Sacramento  
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_026.d  
 Lims ID: 320-31468-A-11-A  
 Client ID: NAWC-091117-RW-145  
 Sample Type: Client  
 Inject. Date: 20-Sep-2017 05:46:54 ALS Bottle#: 20 Worklist Smp#: 26  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: 320-31468-a-11-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:40 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d  
 Column 1 : Det: EXP1  
 Process Host: XAWRK008

First Level Reviewer: barnettj Date: 20-Sep-2017 13:31:53

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.396	1.402	-0.006	1.000	567761	2.10		433	
298.90 > 99.00	1.396	1.402	-0.006	1.000	385160		1.47(0.00-0.00)	721	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.517	1.524	-0.007	1.000	2113985	7.42		9156	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.662	1.668	-0.006	1.000	716159	1.95		256	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.662	1.668	-0.006	1.000	345512	1.51		50.9	
* 6 13C2-PFOA									
415.00 > 370.00	1.844	1.855	-0.011		2432580	10.0		8596	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.851	1.856	-0.005	1.000	1226316	5.48		50.1	
413.00 > 169.00	1.851	1.856	-0.005	1.000	692549		1.77(0.00-0.00)	1700	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.102	2.094	0.008	1.000	1075193	5.16		242	M
499.00 > 99.00	2.102	2.094	0.008	1.000	185051		5.81(0.00-0.00)	111	M
* 7 13C4 PFOS									
503.00 > 80.00	2.102	2.108	-0.006		6418340	28.7		3283	
9 Perfluorononanoic acid									
463.00 > 419.00	2.109	2.116	-0.007	1.000	119085	0.7872		3.2	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.276	2.282	-0.006	1.000	1567134	11.5		14160	

## QC Flag Legend

### Review Flags

M - Manually Integrated



TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_026.d

Injection Date: 20-Sep-2017 05:46:54

Instrument ID: A8\_N

Lims ID: 320-31468-A-11-A

Lab Sample ID: 320-31468-11

Client ID: NAWC-091117-RW-145

Operator ID: SACINSTLCMS01

ALS Bottle#: 20

Worklist Smp#: 26

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537\_A8\_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




\* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

\* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento  
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_026.d  
 Lims ID: 320-31468-A-11-A  
 Client ID: NAWC-091117-RW-145  
 Sample Type: Client  
 Inject. Date: 20-Sep-2017 05:46:54 ALS Bottle#: 20 Worklist Smp#: 26  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: 320-31468-a-11-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:40 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d  
 Column 1 : Det: EXP1  
 Process Host: XAWRK008

First Level Reviewer: barnettj Date: 20-Sep-2017 13:31:53

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	7.42	74.16
\$ 10 13C2 PFDA	10.0	11.5	115.50

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_026.d  
Injection Date: 20-Sep-2017 05:46:54 Instrument ID: A8\_N  
Lims ID: 320-31468-A-11-A Lab Sample ID: 320-31468-11  
Client ID: NAWC-091117-RW-145  
Operator ID: SACINSTLCMS01 ALS Bottle#: 20 Worklist Smp#: 26  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.10  
Area: 1075193  
Amount: 5.156638  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 13:31:06  
Audit Action: Assigned Compound ID

Audit Reason: Missed Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_026.d  
Injection Date: 20-Sep-2017 05:46:54 Instrument ID: A8\_N  
Lims ID: 320-31468-A-11-A Lab Sample ID: 320-31468-11  
Client ID: NAWC-091117-RW-145  
Operator ID: SACINSTLCMS01 ALS Bottle#: 20 Worklist Smp#: 26  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1


Signal: 2

Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results



RT: 2.10  
Area: 185051  
Amount: 5.156638  
Amount Units: ng/ml

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_026.d  
Injection Date: 20-Sep-2017 05:46:54 Instrument ID: A8\_N  
Lims ID: 320-31468-A-11-A Lab Sample ID: 320-31468-11  
Client ID: NAWC-091117-RW-145  
Operator ID: SACINSTLCMS01 ALS Bottle#: 20 Worklist Smp#: 26  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.10  
Area: 1075193  
Amount: 5.156638  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 13:31:34

Audit Action: Manually Integrated

Audit Reason: Missed Peak

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-FRB-145 Lab Sample ID: 320-31468-12  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_027.d  
 Analysis Method: 537 Date Collected: 09/11/2017 13:30  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 265.6(mL) Date Analyzed: 09/20/2017 05:51  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	38	15	6.4
335-67-1	Perfluorooctanoic acid (PFOA)	7.5	U	19	7.5	2.6
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.5
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	U	9.4	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	85	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	83		70-130
STL00996	13C2 PFDA	100		70-130

TestAmerica Sacramento  
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_027.d  
 Lims ID: 320-31468-A-12-A  
 Client ID: NAWC-091117-FRB-145  
 Sample Type: Client  
 Inject. Date: 20-Sep-2017 05:51:39 ALS Bottle#: 21 Worklist Smp#: 27  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: 320-31468-a-12-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:40 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d

Column 1 : Det: EXP1  
 Process Host: XAWRK008

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
\$ 2 13C2 PFHxA	315.00 > 270.00	1.517	1.524	-0.007	1.000	2597327	8.25	7410	
* 6 13C2-PFOA	415.00 > 370.00	1.844	1.855	-0.011		2685353	10.0	7292	
* 7 13C4 PFOS	503.00 > 80.00	2.102	2.108	-0.006		6382119	28.7	5232	
\$ 10 13C2 PFDA	515.00 > 470.00	2.276	2.282	-0.006	1.000	1495513	9.98	12664	



TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_027.d

Injection Date: 20-Sep-2017 05:51:39

Instrument ID: A8\_N

Lims ID: 320-31468-A-12-A

Lab Sample ID: 320-31468-12

Client ID: NAWC-091117-FRB-145

Operator ID: SACINSTLCMS01

ALS Bottle#: 21

Worklist Smp#: 27




Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537\_A8\_N

Limit Group: LC 537 ICAL




1 Perfluorobutanesulfonic acid (ND) 1 Perfluorobutanesulfonic acid (ND) \$ 2 13C2 PFHxA






3 Perfluorohexanesulfonic acid (ND) 4 Perfluoroheptanoic acid (ND) \* 6 13C2-PFOA




5 Perfluorooctanoic acid (ND) 5 Perfluorooctanoic acid (ND) 8 Perfluorooctane sulfonic acid (ND)



8 Perfluorooctane sulfonic acid (ND) \* 7 13C4 PFOS 9 Perfluorononanoic acid (ND)



\$ 10 13C2 PFDA



TestAmerica Sacramento  
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_027.d  
 Lims ID: 320-31468-A-12-A  
 Client ID: NAWC-091117-FRB-145  
 Sample Type: Client  
 Inject. Date: 20-Sep-2017 05:51:39 ALS Bottle#: 21 Worklist Smp#: 27  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: 320-31468-a-12-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:40 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d

Column 1 : Det: EXP1  
 Process Host: XAWRK008

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	8.25	82.54
\$ 10 13C2 PFDA	10.0	9.98	99.85

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-RW-317 Lab Sample ID: 320-31468-13  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_028.d  
 Analysis Method: 537 Date Collected: 09/11/2017 14:00  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 263.7(mL) Date Analyzed: 09/20/2017 05:56  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	49	M	38	15	6.4
335-67-1	Perfluorooctanoic acid (PFOA)	21		19	7.6	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	34		28	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	8.1	J	9.5	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	85	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	78		70-130
STL00996	13C2 PFDA	116		70-130

TestAmerica Sacramento  
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_028.d  
 Lims ID: 320-31468-A-13-A  
 Client ID: NAWC-091117-RW-317  
 Sample Type: Client  
 Inject. Date: 20-Sep-2017 05:56:24 ALS Bottle#: 22 Worklist Smp#: 28  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: 320-31468-a-13-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:40 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d  
 Column 1 : Det: EXP1  
 Process Host: XAWRK008

First Level Reviewer: barnettj Date: 20-Sep-2017 13:32:39

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.396	1.402	-0.006	1.000	423770	1.51		473	
298.90 > 99.00	1.396	1.402	-0.006	1.000	283395		1.50(0.00-0.00)	594	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.517	1.524	-0.007	1.000	2297413	7.84		9945	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.662	1.668	-0.006	1.000	3392154	8.94		1675	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.662	1.668	-0.006	1.000	504743	2.14		83.8	
* 6 13C2-PFOA									
415.00 > 370.00	1.844	1.855	-0.011		2501311	10.0		10469	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.844	1.856	-0.012	1.000	1283721	5.58		57.0	
413.00 > 169.00	1.844	1.856	-0.012	1.000	747350		1.72(0.00-0.00)	2178	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.094	2.094	0.0	1.000	2793177	12.9		866	M
499.00 > 99.00	2.094	2.094	0.0	1.000	581181		4.81(0.00-0.00)	426	M
* 7 13C4 PFOS									
503.00 > 80.00	2.094	2.108	-0.014		6642891	28.7		4014	
9 Perfluorononanoic acid									
463.00 > 419.00	2.102	2.116	-0.014	1.000	116563	0.7494		3.8	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.269	2.282	-0.014	1.000	1615910	11.6		14563	

## QC Flag Legend

### Review Flags

M - Manually Integrated

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_028.d

Injection Date: 20-Sep-2017 05:56:24

Instrument ID: A8\_N

Lims ID: 320-31468-A-13-A

Lab Sample ID: 320-31468-13

Client ID: NAWC-091117-RW-317

Operator ID: SACINSTLCMS01

ALS Bottle#: 22

Worklist Smp#: 28

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537\_A8\_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




\* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

\* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA





TestAmerica Sacramento  
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_028.d  
 Lims ID: 320-31468-A-13-A  
 Client ID: NAWC-091117-RW-317  
 Sample Type: Client  
 Inject. Date: 20-Sep-2017 05:56:24 ALS Bottle#: 22 Worklist Smp#: 28  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: 320-31468-a-13-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:40 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d  
 Column 1 : Det: EXP1  
 Process Host: XAWRK008

First Level Reviewer: barnettj Date: 20-Sep-2017 13:32:39

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	7.84	78.39
\$ 10 13C2 PFDA	10.0	11.6	115.82

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_028.d  
Injection Date: 20-Sep-2017 05:56:24 Instrument ID: A8\_N  
Lims ID: 320-31468-A-13-A Lab Sample ID: 320-31468-13  
Client ID: NAWC-091117-RW-317  
Operator ID: SACINSTLCMS01 ALS Bottle#: 22 Worklist Smp#: 28  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.09  
Area: 2793177  
Amount: 12.943278  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 13:32:06  
Audit Action: Assigned Compound ID

Audit Reason: Missed Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_028.d  
Injection Date: 20-Sep-2017 05:56:24 Instrument ID: A8\_N  
Lims ID: 320-31468-A-13-A Lab Sample ID: 320-31468-13  
Client ID: NAWC-091117-RW-317  
Operator ID: SACINSTLCMS01 ALS Bottle#: 22 Worklist Smp#: 28  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.09  
Area: 581181  
Amount: 12.943278  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 13:32:23

Audit Action: Manually Integrated

Audit Reason: Missed Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_028.d  
Injection Date: 20-Sep-2017 05:56:24 Instrument ID: A8\_N  
Lims ID: 320-31468-A-13-A Lab Sample ID: 320-31468-13  
Client ID: NAWC-091117-RW-317  
Operator ID: SACINSTLCMS01 ALS Bottle#: 22 Worklist Smp#: 28  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.09  
Area: 2793177  
Amount: 12.943278  
Amount Units: ng/ml



FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-FRB-317 Lab Sample ID: 320-31468-14  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_029.d  
 Analysis Method: 537 Date Collected: 09/11/2017 13:55  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 254.4(mL) Date Analyzed: 09/20/2017 06:01  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	39	16	6.7
335-67-1	Perfluorooctanoic acid (PFOA)	7.9	U	20	7.9	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	7.9
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	29	12	5.4
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.9	U	9.8	3.9	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	35	U	88	35	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	83		70-130
STL00996	13C2 PFDA	97		70-130

TestAmerica Sacramento  
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_029.d  
 Lims ID: 320-31468-A-14-A  
 Client ID: NAWC-091117-FRB-317  
 Sample Type: Client  
 Inject. Date: 20-Sep-2017 06:01:09 ALS Bottle#: 23 Worklist Smp#: 29  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: 320-31468-a-14-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:40 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d

Column 1 : Det: EXP1  
 Process Host: XAWRK008

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
\$ 2 13C2 PFHxA	315.00 > 270.00	1.517	1.524	-0.007	1.000	2564042	8.32	7618	
* 6 13C2-PFOA	415.00 > 370.00	1.844	1.855	-0.011		2631497	10.0	6270	
* 7 13C4 PFOS	503.00 > 80.00	2.094	2.108	-0.014		6447036	28.7	4595	
\$ 10 13C2 PFDA	515.00 > 470.00	2.276	2.282	-0.006	1.000	1417849	9.66	11667	

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_029.d

Injection Date: 20-Sep-2017 06:01:09

Instrument ID: A8\_N

Lims ID: 320-31468-A-14-A

Lab Sample ID: 320-31468-14

Client ID: NAWC-091117-FRB-317

Operator ID: SACINSTLCMS01

ALS Bottle#: 23

Worklist Smp#: 29




Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537\_A8\_N

Limit Group: LC 537 ICAL




1 Perfluorobutanesulfonic acid (ND) 1 Perfluorobutanesulfonic acid (ND) \$ 2 13C2 PFHxA






3 Perfluorohexanesulfonic acid (ND) 4 Perfluoroheptanoic acid (ND) \* 6 13C2-PFOA




5 Perfluorooctanoic acid (ND) 5 Perfluorooctanoic acid (ND) 8 Perfluorooctane sulfonic acid (ND)



8 Perfluorooctane sulfonic acid (ND) \* 7 13C4 PFOS 9 Perfluorononanoic acid (ND)



\$ 10 13C2 PFDA





TestAmerica Sacramento  
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_029.d  
 Lims ID: 320-31468-A-14-A  
 Client ID: NAWC-091117-FRB-317  
 Sample Type: Client  
 Inject. Date: 20-Sep-2017 06:01:09 ALS Bottle#: 23 Worklist Smp#: 29  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: 320-31468-a-14-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:40 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d

Column 1 : Det: EXP1  
 Process Host: XAWRK008

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	8.32	83.15
\$ 10 13C2 PFDA	10.0	9.66	96.60

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-RW-319 Lab Sample ID: 320-31468-15  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_030.d  
 Analysis Method: 537 Date Collected: 09/11/2017 14:25  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 251(mL) Date Analyzed: 09/20/2017 06:05  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	43	M	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	44		20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	9.7	J	24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	8.0	J	30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	15	M	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	61	Q	70-130
STL00996	13C2 PFDA	83		70-130

TestAmerica Sacramento  
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_030.d  
 Lims ID: 320-31468-A-15-A  
 Client ID: NAWC-091117-RW-319  
 Sample Type: Client  
 Inject. Date: 20-Sep-2017 06:05:54 ALS Bottle#: 24 Worklist Smp#: 30  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: 320-31468-a-15-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:40 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d  
 Column 1 : Det: EXP1  
 Process Host: XAWRK008

First Level Reviewer: barnettj Date: 20-Sep-2017 13:33:58

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.396	1.402	-0.006	1.000	397316	1.47		27.0	
298.90 > 99.00	1.396	1.402	-0.006	1.000	270675		1.47(0.00-0.00)	96.2	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.517	1.524	-0.007	1.000	1659318	6.06		6829	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.662	1.668	-0.006	1.000	738145	2.01		57.9	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.662	1.668	-0.006	1.000	841612	3.82		39.4	M
* 6 13C2-PFOA									
415.00 > 370.00	1.844	1.855	-0.011		2337114	10.0		7816	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.844	1.856	-0.012	1.000	2350073	10.9		68.2	
413.00 > 169.00	1.844	1.856	-0.012	1.000	1279688		1.84(0.00-0.00)	1339	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.094	2.094	0.0	1.000	2231766	10.7		196	M
499.00 > 99.00	2.094	2.094	0.0	1.000	417752		5.34(0.00-0.00)	153	M
* 7 13C4 PFOS									
503.00 > 80.00	2.094	2.108	-0.014		6427066	28.7		1199	
9 Perfluorononanoic acid									
463.00 > 419.00	2.102	2.116	-0.014	1.000	353011	2.43		9.8	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.276	2.282	-0.006	1.000	1080740	8.29		7633	

## QC Flag Legend

Review Flags

M - Manually Integrated

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_030.d

Injection Date: 20-Sep-2017 06:05:54

Instrument ID: A8\_N

Lims ID: 320-31468-A-15-A

Lab Sample ID: 320-31468-15

Client ID: NAWC-091117-RW-319

Operator ID: SACINSTLCMS01

ALS Bottle#: 24

Worklist Smp#: 30

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537\_A8\_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid (M)




\* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

\* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento  
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_030.d  
 Lims ID: 320-31468-A-15-A  
 Client ID: NAWC-091117-RW-319  
 Sample Type: Client  
 Inject. Date: 20-Sep-2017 06:05:54 ALS Bottle#: 24 Worklist Smp#: 30  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: 320-31468-a-15-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:40 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d  
 Column 1 : Det: EXP1  
 Process Host: XAWRK008

First Level Reviewer: barnettj Date: 20-Sep-2017 13:33:58

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	6.06	60.59
\$ 10 13C2 PFDA	10.0	8.29	82.91

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_030.d  
Injection Date: 20-Sep-2017 06:05:54 Instrument ID: A8\_N  
Lims ID: 320-31468-A-15-A Lab Sample ID: 320-31468-15  
Client ID: NAWC-091117-RW-319  
Operator ID: SACINSTLCMS01 ALS Bottle#: 24 Worklist Smp#: 30  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.09  
Area: 2231766  
Amount: 10.689044  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 13:32:54  
Audit Action: Assigned Compound ID

Audit Reason: Missed Peak



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_030.d  
Injection Date: 20-Sep-2017 06:05:54 Instrument ID: A8\_N  
Lims ID: 320-31468-A-15-A Lab Sample ID: 320-31468-15  
Client ID: NAWC-091117-RW-319  
Operator ID: SACINSTLCMS01 ALS Bottle#: 24 Worklist Smp#: 30  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.09  
Area: 417752  
Amount: 10.689044  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 13:33:23

Audit Action: Manually Integrated

Audit Reason: Missed Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_030.d  
Injection Date: 20-Sep-2017 06:05:54 Instrument ID: A8\_N  
Lims ID: 320-31468-A-15-A Lab Sample ID: 320-31468-15  
Client ID: NAWC-091117-RW-319  
Operator ID: SACINSTLCMS01 ALS Bottle#: 24 Worklist Smp#: 30  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.09  
Area: 2231766  
Amount: 10.689044  
Amount Units: ng/ml



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_030.d  
Injection Date: 20-Sep-2017 06:05:54 Instrument ID: A8\_N  
Lims ID: 320-31468-A-15-A Lab Sample ID: 320-31468-15  
Client ID: NAWC-091117-RW-319  
Operator ID: SACINSTLCMS01 ALS Bottle#: 24 Worklist Smp#: 30  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

4 Perfluoroheptanoic acid, CAS: 375-85-9

Signal: 1


RT: 1.66  
Area: 1024374  
Amount: 4.654142  
Amount Units: ng/ml

Processing Integration Results



RT: 1.66  
Area: 841612  
Amount: 3.823781  
Amount Units: ng/ml

Manual Integration Results



FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-FRB-319 Lab Sample ID: 320-31468-16  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_031.d  
 Analysis Method: 537 Date Collected: 09/11/2017 14:40  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 266.7(mL) Date Analyzed: 09/20/2017 06:10  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	37	15	6.4
335-67-1	Perfluorooctanoic acid (PFOA)	7.5	U	19	7.5	2.6
375-95-1	Perfluorononanoic acid (PFNA)	19	U	22	19	7.5
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.7	U	9.4	3.7	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	84	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	82		70-130
STL00996	13C2 PFDA	124		70-130

TestAmerica Sacramento  
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_031.d  
 Lims ID: 320-31468-A-16-A  
 Client ID: NAWC-091117-FRB-319  
 Sample Type: Client  
 Inject. Date: 20-Sep-2017 06:10:38 ALS Bottle#: 25 Worklist Smp#: 31  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: 320-31468-a-16-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:40 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d

Column 1 : Det: EXP1  
 Process Host: XAWRK008

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
\$ 2 13C2 PFHxA	315.00 > 270.00	1.517	1.524	-0.007	1.000	2592322	8.25	12244	
* 6 13C2-PFOA	415.00 > 370.00	1.844	1.855	-0.011		2681945	10.0	10809	
* 7 13C4 PFOS	503.00 > 80.00	2.094	2.108	-0.014		6402518	28.7	2879	
\$ 10 13C2 PFDA	515.00 > 470.00	2.269	2.282	-0.014	1.000	1848418	12.4	14579	

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_031.d

Injection Date: 20-Sep-2017 06:10:38

Instrument ID: A8\_N

Lims ID: 320-31468-A-16-A

Lab Sample ID: 320-31468-16

Client ID: NAWC-091117-FRB-319

Operator ID: SACINSTLCMS01

ALS Bottle#: 25

Worklist Smp#: 31




Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537\_A8\_N

Limit Group: LC 537 ICAL




1 Perfluorobutanesulfonic acid (ND) 1 Perfluorobutanesulfonic acid (ND) \$ 2 13C2 PFHxA






3 Perfluorohexanesulfonic acid (ND) 4 Perfluoroheptanoic acid (ND) \* 6 13C2-PFOA




5 Perfluorooctanoic acid (ND) 5 Perfluorooctanoic acid (ND) 8 Perfluorooctane sulfonic acid (ND)



8 Perfluorooctane sulfonic acid (ND) \* 7 13C4 PFOS 9 Perfluorononanoic acid (ND)



\$ 10 13C2 PFDA



TestAmerica Sacramento  
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_031.d  
 Lims ID: 320-31468-A-16-A  
 Client ID: NAWC-091117-FRB-319  
 Sample Type: Client  
 Inject. Date: 20-Sep-2017 06:10:38 ALS Bottle#: 25 Worklist Smp#: 31  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: 320-31468-a-16-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:40 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d

Column 1 : Det: EXP1  
 Process Host: XAWRK008

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	8.25	82.49
\$ 10 13C2 PFDA	10.0	12.4	123.56



FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-RW-321 Lab Sample ID: 320-31468-17  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_032.d  
 Analysis Method: 537 Date Collected: 09/11/2017 15:10  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 262 (mL) Date Analyzed: 09/20/2017 06:15  
 Con. Extract Vol.: 1.0 (mL) Dilution Factor: 1  
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	7.5	J M	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	6.9	J	19	7.6	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	29	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	1.8	J	9.5	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	86	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	76		70-130
STL00996	13C2 PFDA	106		70-130

TestAmerica Sacramento  
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_032.d  
 Lims ID: 320-31468-A-17-A  
 Client ID: NAWC-091117-RW-321  
 Sample Type: Client  
 Inject. Date: 20-Sep-2017 06:15:23 ALS Bottle#: 26 Worklist Smp#: 32  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: 320-31468-a-17-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:40 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d  
 Column 1 : Det: EXP1  
 Process Host: XAWRK008

First Level Reviewer: barnettj Date: 20-Sep-2017 13:35:12

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.396	1.402	-0.006	1.000	537564	1.99		545	
298.90 > 99.00	1.396	1.402	-0.006	1.000	359056		1.50(0.00-0.00)	733	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.517	1.524	-0.007	1.000	2284128	7.62		7844	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.662	1.668	-0.006	1.000	351682	0.9594		172	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.662	1.668	-0.006	1.000	114016	0.4734		18.2	
* 6 13C2-PFOA									
415.00 > 370.00	1.844	1.855	-0.011		2557163	10.0		7561	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.844	1.856	-0.012	1.000	426788	1.82		17.3	
413.00 > 169.00	1.844	1.856	-0.012	1.000	239562		1.78(0.00-0.00)	731	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.094	2.094	0.0	1.000	407127	1.95		118	M
499.00 > 99.00	2.086	2.094	-0.008	0.996	69980		5.82(0.00-0.00)	46.7	M
* 7 13C4 PFOS									
503.00 > 80.00	2.086	2.108	-0.022		6417541	28.7		3401	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.269	2.282	-0.014	1.000	1518990	10.6		12431	

## QC Flag Legend

Review Flags

M - Manually Integrated

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_032.d

Injection Date: 20-Sep-2017 06:15:23

Instrument ID: A8\_N

Lims ID: 320-31468-A-17-A

Lab Sample ID: 320-31468-17

Client ID: NAWC-091117-RW-321

Operator ID: SACINSTLCMS01

ALS Bottle#: 26

Worklist Smp#: 32

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537\_A8\_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




\* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid

\* 7 13C4 PFOS

9 Perfluorononanoic acid (ND)



\$ 10 13C2 PFDA



TestAmerica Sacramento  
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_032.d  
 Lims ID: 320-31468-A-17-A  
 Client ID: NAWC-091117-RW-321  
 Sample Type: Client  
 Inject. Date: 20-Sep-2017 06:15:23 ALS Bottle#: 26 Worklist Smp#: 32  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: 320-31468-a-17-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:40 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d  
 Column 1 : Det: EXP1  
 Process Host: XAWRK008

First Level Reviewer: barnettj Date: 20-Sep-2017 13:35:12

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	7.62	76.23
\$ 10 13C2 PFDA	10.0	10.6	106.50

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_032.d  
Injection Date: 20-Sep-2017 06:15:23 Instrument ID: A8\_N  
Lims ID: 320-31468-A-17-A Lab Sample ID: 320-31468-17  
Client ID: NAWC-091117-RW-321  
Operator ID: SACINSTLCMS01 ALS Bottle#: 26 Worklist Smp#: 32  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.09  
Area: 407127  
Amount: 1.952829  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 13:34:11  
Audit Action: Assigned Compound ID

Audit Reason: Missed Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_032.d  
Injection Date: 20-Sep-2017 06:15:23 Instrument ID: A8\_N  
Lims ID: 320-31468-A-17-A Lab Sample ID: 320-31468-17  
Client ID: NAWC-091117-RW-321  
Operator ID: SACINSTLCMS01 ALS Bottle#: 26 Worklist Smp#: 32  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.09  
Area: 407127  
Amount: 1.952829  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 13:34:26

Audit Action: Manually Integrated

Audit Reason: Missed Peak



FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-FRB-321 Lab Sample ID: 320-31468-18  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_035.d  
 Analysis Method: 537 Date Collected: 09/11/2017 15:05  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 263.5 (mL) Date Analyzed: 09/20/2017 06:29  
 Con. Extract Vol.: 1.0 (mL) Dilution Factor: 1  
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185409 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	7.6	U	19	7.6	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	U	9.5	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	85	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	84		70-130
STL00996	13C2 PFDA	104		70-130

TestAmerica Sacramento  
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_035.d  
 Lims ID: 320-31468-A-18-A  
 Client ID: NAWC-091117-FRB-321  
 Sample Type: Client  
 Inject. Date: 20-Sep-2017 06:29:34 ALS Bottle#: 27 Worklist Smp#: 35  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: 320-31468-a-18-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:04:03 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d

Column 1 : Det: EXP1  
 Process Host: XAWRK008

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
\$ 2 13C2 PFHxA	315.00 > 270.00	1.517	1.524	-0.007	1.000	2547329	8.41	12696	
* 6 13C2-PFOA	415.00 > 370.00	1.844	1.855	-0.011		2584590	10.0	9451	
* 7 13C4 PFOS	503.00 > 80.00	2.102	2.108	-0.006		6389473	28.7	5451	
\$ 10 13C2 PFDA	515.00 > 470.00	2.276	2.282	-0.006	1.000	1503347	10.4	13102	

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_035.d

Injection Date: 20-Sep-2017 06:29:34

Instrument ID: A8\_N

Lims ID: 320-31468-A-18-A

Lab Sample ID: 320-31468-18

Client ID: NAWC-091117-FRB-321

Operator ID: SACINSTLCMS01

ALS Bottle#: 27

Worklist Smp#: 35




Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537\_A8\_N

Limit Group: LC 537 ICAL




1 Perfluorobutanesulfonic acid (ND) 1 Perfluorobutanesulfonic acid (ND) \$ 2 13C2 PFHxA






3 Perfluorohexanesulfonic acid (ND) 4 Perfluoroheptanoic acid (ND) \* 6 13C2-PFOA




5 Perfluorooctanoic acid (ND) 5 Perfluorooctanoic acid (ND) 8 Perfluorooctane sulfonic acid (ND)



8 Perfluorooctane sulfonic acid (ND) \* 7 13C4 PFOS 9 Perfluorononanoic acid (ND)



\$ 10 13C2 PFDA



TestAmerica Sacramento  
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_035.d  
 Lims ID: 320-31468-A-18-A  
 Client ID: NAWC-091117-FRB-321  
 Sample Type: Client  
 Inject. Date: 20-Sep-2017 06:29:34 ALS Bottle#: 27 Worklist Smp#: 35  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: 320-31468-a-18-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:04:03 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d

Column 1 : Det: EXP1  
 Process Host: XAWRK008

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	8.41	84.11
\$ 10 13C2 PFDA	10.0	10.4	104.28

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-RW-010 Lab Sample ID: 320-31468-19  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_036.d  
 Analysis Method: 537 Date Collected: 09/11/2017 15:45  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 254.7(mL) Date Analyzed: 09/20/2017 06:34  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185409 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	30	J M	39	16	6.7
335-67-1	Perfluorooctanoic acid (PFOA)	12	J	20	7.9	2.7
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	7.9
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	17	J	29	12	5.4
375-85-9	Perfluoroheptanoic acid (PFHpA)	5.4	J	9.8	3.9	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	35	U	88	35	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	75		70-130
STL00996	13C2 PFDA	104		70-130

TestAmerica Sacramento  
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_036.d  
 Lims ID: 320-31468-A-19-A  
 Client ID: NAWC-091117-RW-010  
 Sample Type: Client  
 Inject. Date: 20-Sep-2017 06:34:19 ALS Bottle#: 28 Worklist Smp#: 36  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: 320-31468-a-19-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:04:03 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d  
 Column 1 : Det: EXP1  
 Process Host: XAWRK008

First Level Reviewer: barnettj Date: 20-Sep-2017 13:36:37

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.396	1.402	-0.006	1.000	232581	0.8855		89.9	
298.90 > 99.00	1.396	1.402	-0.006	1.000	144041		1.61(0.00-0.00)	289	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.517	1.524	-0.007	1.000	2150655	7.47		7539	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.662	1.668	-0.006	1.000	1567295	4.41		426	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.662	1.668	-0.006	1.000	320048	1.38		43.1	
* 6 13C2-PFOA									
415.00 > 370.00	1.844	1.855	-0.011		2457461	10.0		7641	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.844	1.856	-0.012	1.000	675652	2.99		34.9	
413.00 > 169.00	1.844	1.856	-0.012	1.000	761627		0.89(0.00-0.00)	2039	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.094	2.094	0.0	1.000	1566703	7.75		387	M
499.00 > 99.00	2.094	2.094	0.0	1.000	314157		4.99(0.00-0.00)	218	M
* 7 13C4 PFOS									
503.00 > 80.00	2.094	2.108	-0.014		6222745	28.7		2488	
9 Perfluorononanoic acid									
463.00 > 419.00	2.102	2.116	-0.014	1.000	113269	0.7412		4.2	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.269	2.282	-0.014	1.000	1421514	10.4		13236	

## QC Flag Legend

Review Flags

M - Manually Integrated



TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_036.d

Injection Date: 20-Sep-2017 06:34:19

Instrument ID: A8\_N

Lims ID: 320-31468-A-19-A

Lab Sample ID: 320-31468-19

Client ID: NAWC-091117-RW-010

Operator ID: SACINSTLCMS01

ALS Bottle#: 28

Worklist Smp#: 36

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537\_A8\_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




\* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

\* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento  
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_036.d  
 Lims ID: 320-31468-A-19-A  
 Client ID: NAWC-091117-RW-010  
 Sample Type: Client  
 Inject. Date: 20-Sep-2017 06:34:19 ALS Bottle#: 28 Worklist Smp#: 36  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: 320-31468-a-19-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:04:03 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d  
 Column 1 : Det: EXP1  
 Process Host: XAWRK008

First Level Reviewer: barnettj Date: 20-Sep-2017 13:36:37

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	7.47	74.69
\$ 10 13C2 PFDA	10.0	10.4	103.71

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_036.d  
Injection Date: 20-Sep-2017 06:34:19 Instrument ID: A8\_N  
Lims ID: 320-31468-A-19-A Lab Sample ID: 320-31468-19  
Client ID: NAWC-091117-RW-010  
Operator ID: SACINSTLCMS01 ALS Bottle#: 28 Worklist Smp#: 36  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.09  
Area: 1566703  
Amount: 7.750106  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 13:35:57  
Audit Action: Assigned Compound ID

Audit Reason: Missed Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_036.d  
Injection Date: 20-Sep-2017 06:34:19 Instrument ID: A8\_N  
Lims ID: 320-31468-A-19-A Lab Sample ID: 320-31468-19  
Client ID: NAWC-091117-RW-010  
Operator ID: SACINSTLCMS01 ALS Bottle#: 28 Worklist Smp#: 36  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.09  
Area: 314157  
Amount: 7.750106  
Amount Units: ng/ml



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_036.d  
Injection Date: 20-Sep-2017 06:34:19 Instrument ID: A8\_N  
Lims ID: 320-31468-A-19-A Lab Sample ID: 320-31468-19  
Client ID: NAWC-091117-RW-010  
Operator ID: SACINSTLCMS01 ALS Bottle#: 28 Worklist Smp#: 36  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.09  
Area: 1566703  
Amount: 7.750106  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 13:36:29

Audit Action: Manually Integrated

Audit Reason: Missed Peak

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-FRB-010 Lab Sample ID: 320-31468-20  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_037.d  
 Analysis Method: 537 Date Collected: 09/11/2017 15:40  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 259.8(mL) Date Analyzed: 09/20/2017 06:39  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185409 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	7.7	U	19	7.7	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.7
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	29	12	5.3
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	U	9.6	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	35	U	87	35	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	83		70-130
STL00996	13C2 PFDA	97		70-130

TestAmerica Sacramento  
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_037.d  
 Lims ID: 320-31468-A-20-A  
 Client ID: NAWC-091117-FRB-010  
 Sample Type: Client  
 Inject. Date: 20-Sep-2017 06:39:04 ALS Bottle#: 29 Worklist Smp#: 37  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: 320-31468-a-20-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:04:03 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d

Column 1 : Det: EXP1  
 Process Host: XAWRK008

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
\$ 2 13C2 PFHxA	315.00 > 270.00	1.517	1.524	-0.007	1.000	2615176	8.33	7861	
* 6 13C2-PFOA	415.00 > 370.00	1.844	1.855	-0.011		2679499	10.0	7233	
* 7 13C4 PFOS	503.00 > 80.00	2.094	2.108	-0.014		6439213	28.7	5873	
\$ 10 13C2 PFDA	515.00 > 470.00	2.276	2.282	-0.006	1.000	1452775	9.72	11751	



TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_037.d

Injection Date: 20-Sep-2017 06:39:04

Instrument ID: A8\_N

Lims ID: 320-31468-A-20-A

Lab Sample ID: 320-31468-20

Client ID: NAWC-091117-FRB-010

Operator ID: SACINSTLCMS01

ALS Bottle#: 29

Worklist Smp#: 37


Injection Vol: 2.0 ul

Dil. Factor: 1.0000


Method: 537\_A8\_N

Limit Group: LC 537 ICAL


1 Perfluorobutanesulfonic acid (ND) 1 Perfluorobutanesulfonic acid (ND) \$ 2 13C2 PFHxA




3 Perfluorohexanesulfonic acid (ND) 4 Perfluoroheptanoic acid (ND) \* 6 13C2-PFOA




5 Perfluorooctanoic acid (ND) 5 Perfluorooctanoic acid (ND) 8 Perfluorooctane sulfonic acid (ND)



8 Perfluorooctane sulfonic acid (ND) \* 7 13C4 PFOS 9 Perfluorononanoic acid (ND)



\$ 10 13C2 PFDA



TestAmerica Sacramento  
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_037.d  
 Lims ID: 320-31468-A-20-A  
 Client ID: NAWC-091117-FRB-010  
 Sample Type: Client  
 Inject. Date: 20-Sep-2017 06:39:04 ALS Bottle#: 29 Worklist Smp#: 37  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: 320-31468-a-20-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:04:03 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d

Column 1 : Det: EXP1  
 Process Host: XAWRK008

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	8.33	83.29
\$ 10 13C2 PFDA	10.0	9.72	97.20

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-RW-162 Lab Sample ID: 320-31468-21  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_006.d  
 Analysis Method: 537 Date Collected: 09/11/2017 11:20  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:29  
 Sample wt/vol: 262.9(mL) Date Analyzed: 09/20/2017 04:11  
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185406 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	33	J M	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	15	J	19	7.6	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	13	J	29	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	5.4	J	9.5	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	86	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	78		70-130
STL00996	13C2 PFDA	111		70-130

TestAmerica Sacramento  
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_006.d  
 Lims ID: 320-31468-A-21-A  
 Client ID: NAWC-091117-RW-162  
 Sample Type: Client  
 Inject. Date: 20-Sep-2017 04:11:58 ALS Bottle#: 4 Worklist Smp#: 6  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: 320-31468-a-21-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:15 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d  
 Column 1 : Det: EXP1  
 Process Host: XAWRK008

First Level Reviewer: barnettj Date: 20-Sep-2017 11:41:21

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.396	1.402	-0.006	1.000	385864	1.56		318	
298.90 > 99.00	1.396	1.402	-0.006	1.000	264037		1.46(0.00-0.00)	365	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.517	1.524	-0.007	1.000	2139566	7.77		6462	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.662	1.668	-0.006	1.000	1123421	3.36		447	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.662	1.668	-0.006	1.000	313203	1.42		52.4	
* 6 13C2-PFOA									
415.00 > 370.00	1.844	1.855	-0.011		2350014	10.0		7578	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.844	1.856	-0.012	1.000	834136	3.86		31.0	
413.00 > 169.00	1.844	1.856	-0.012	1.000	487680		1.71(0.00-0.00)	1188	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.102	2.094	0.008	1.000	1664423	8.74		602	M
499.00 > 99.00	2.094	2.094	0.0	0.996	314742		5.29(0.00-0.00)	202	M
* 7 13C4 PFOS									
503.00 > 80.00	2.102	2.108	-0.006		5861531	28.7		3126	
9 Perfluorononanoic acid									
463.00 > 419.00	2.109	2.116	-0.007	1.000	59012	0.4038		1.6	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.276	2.282	-0.006	1.000	1459907	11.1		11113	

## QC Flag Legend

### Review Flags

M - Manually Integrated

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_006.d

Injection Date: 20-Sep-2017 04:11:58

Instrument ID: A8\_N

Lims ID: 320-31468-A-21-A

Lab Sample ID: 320-31468-21

Client ID: NAWC-091117-RW-162

Operator ID: SACINSTLCMS01

ALS Bottle#: 4

Worklist Smp#: 6

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537\_A8\_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




\* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

\* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA





TestAmerica Sacramento  
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_006.d  
 Lims ID: 320-31468-A-21-A  
 Client ID: NAWC-091117-RW-162  
 Sample Type: Client  
 Inject. Date: 20-Sep-2017 04:11:58 ALS Bottle#: 4 Worklist Smp#: 6  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: 320-31468-a-21-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:15 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d  
 Column 1 : Det: EXP1  
 Process Host: XAWRK008

First Level Reviewer: barnettj Date: 20-Sep-2017 11:41:21

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	7.77	77.70
\$ 10 13C2 PFDA	10.0	11.1	111.38

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_006.d  
Injection Date: 20-Sep-2017 04:11:58 Instrument ID: A8\_N  
Lims ID: 320-31468-A-21-A Lab Sample ID: 320-31468-21  
Client ID: NAWC-091117-RW-162  
Operator ID: SACINSTLCMS01 ALS Bottle#: 4 Worklist Smp#: 6  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.10  
Area: 1664423  
Amount: 8.740889  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 11:40:53  
Audit Action: Assigned Compound ID

Audit Reason: Missed Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_006.d  
Injection Date: 20-Sep-2017 04:11:58 Instrument ID: A8\_N  
Lims ID: 320-31468-A-21-A Lab Sample ID: 320-31468-21  
Client ID: NAWC-091117-RW-162  
Operator ID: SACINSTLCMS01 ALS Bottle#: 4 Worklist Smp#: 6  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.09  
Area: 314742  
Amount: 8.740889  
Amount Units: ng/ml



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_006.d  
Injection Date: 20-Sep-2017 04:11:58 Instrument ID: A8\_N  
Lims ID: 320-31468-A-21-A Lab Sample ID: 320-31468-21  
Client ID: NAWC-091117-RW-162  
Operator ID: SACINSTLCMS01 ALS Bottle#: 4 Worklist Smp#: 6  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.10  
Area: 1664423  
Amount: 8.740889  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 11:41:13

Audit Action: Manually Integrated

Audit Reason: Missed Peak

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-FRB-162 Lab Sample ID: 320-31468-22  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_007.d  
 Analysis Method: 537 Date Collected: 09/11/2017 11:15  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:29  
 Sample wt/vol: 247.3(mL) Date Analyzed: 09/20/2017 04:16  
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185406 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	40	16	6.9
335-67-1	Perfluorooctanoic acid (PFOA)	8.1	U	20	8.1	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	8.1
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	30	12	5.6
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.0	U	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	91	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	91		70-130
STL00996	13C2 PFDA	129		70-130

TestAmerica Sacramento  
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_007.d  
 Lims ID: 320-31468-A-22-A  
 Client ID: NAWC-091117-FRB-162  
 Sample Type: Client  
 Inject. Date: 20-Sep-2017 04:16:44 ALS Bottle#: 5 Worklist Smp#: 7  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: 320-31468-a-22-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:15 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d

Column 1 : Det: EXP1  
 Process Host: XAWRK008

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
\$ 2 13C2 PFHxA	315.00 > 270.00	1.525	1.524	0.001	1.000	2495701	9.09	10298	
* 6 13C2-PFOA	415.00 > 370.00	1.851	1.855	-0.004		2344211	10.0	9710	
* 7 13C4 PFOS	503.00 > 80.00	2.102	2.108	-0.006		6003115	28.7	5528	
\$ 10 13C2 PFDA	515.00 > 470.00	2.276	2.282	-0.006	1.000	1683971	12.9	15545	

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_007.d

Injection Date: 20-Sep-2017 04:16:44

Instrument ID: A8\_N

Lims ID: 320-31468-A-22-A

Lab Sample ID: 320-31468-22

Client ID: NAWC-091117-FRB-162

Operator ID: SACINSTLCMS01

ALS Bottle#: 5

Worklist Smp#: 7

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537\_A8\_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid (ND)

1 Perfluorobutanesulfonic acid (ND)




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid (ND)

4 Perfluoroheptanoic acid (ND)




\* 6 13C2-PFOA



5 Perfluorooctanoic acid (ND)

5 Perfluorooctanoic acid (ND)




8 Perfluorooctane sulfonic acid (ND)




8 Perfluorooctane sulfonic acid (ND)

\* 7 13C4 PFOS

9 Perfluorononanoic acid (ND)



\$ 10 13C2 PFDA





TestAmerica Sacramento  
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_007.d  
 Lims ID: 320-31468-A-22-A  
 Client ID: NAWC-091117-FRB-162  
 Sample Type: Client  
 Inject. Date: 20-Sep-2017 04:16:44 ALS Bottle#: 5 Worklist Smp#: 7  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: 320-31468-a-22-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:15 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d

Column 1 : Det: EXP1  
 Process Host: XAWRK008

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	9.09	90.86
\$ 10 13C2 PFDA	10.0	12.9	128.79

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: WGNA-091117-DUP09 Lab Sample ID: 320-31468-23  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_008.d  
 Analysis Method: 537 Date Collected: 09/11/2017 07:00  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:29  
 Sample wt/vol: 260 (mL) Date Analyzed: 09/20/2017 04:21  
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1  
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185406 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U M	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	4.5	J	19	7.7	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.7
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	29	12	5.3
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	U M	9.6	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	35	U	87	35	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	75		70-130
STL00996	13C2 PFDA	125		70-130

TestAmerica Sacramento  
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_008.d  
 Lims ID: 320-31468-A-23-A  
 Client ID: WGNA-091117-DUP09  
 Sample Type: Client  
 Inject. Date: 20-Sep-2017 04:21:29 ALS Bottle#: 6 Worklist Smp#: 8  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: 320-31468-a-23-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:15 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d  
 Column 1 : Det: EXP1  
 Process Host: XAWRK008

First Level Reviewer: barnettj Date: 20-Sep-2017 13:22:04

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.396	1.402	-0.006	1.000	122321	0.4791		94.3	
298.90 > 99.00	1.396	1.402	-0.006	1.000	79684		1.54(0.00-0.00)	118	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.517	1.524	-0.007	1.000	2071902	7.46		6005	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.662	1.668	-0.006	1.000	180233	0.5221		71.9	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.662	1.668	-0.006	1.000	72735	0.3258		11.4	M
* 6 13C2-PFOA									
415.00 > 370.00	1.851	1.855	-0.004		2370526	10.0		6529	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.851	1.856	-0.005	1.000	256372	1.18		9.8	
413.00 > 169.00	1.851	1.856	-0.005	1.000	149545		1.71(0.00-0.00)	337	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.011	2.094	-0.083	1.000	264838	1.35		69.4	M
499.00 > 99.00	2.102	2.094	0.008	1.045	31078		8.52(0.00-0.00)	12.2	M
* 7 13C4 PFOS									
503.00 > 80.00	2.102	2.108	-0.006		6043874	28.7		2959	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.276	2.282	-0.006	1.000	1646412	12.5		12979	

## QC Flag Legend

Review Flags

M - Manually Integrated

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_008.d

Injection Date: 20-Sep-2017 04:21:29

Instrument ID: A8\_N

Lims ID: 320-31468-A-23-A

Lab Sample ID: 320-31468-23

Client ID: WGNA-091117-DUP09

Operator ID: SACINSTLCMS01

ALS Bottle#: 6

Worklist Smp#: 8

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537\_A8\_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid (M)




\* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid

\* 7 13C4 PFOS

9 Perfluorononanoic acid (ND)



\$ 10 13C2 PFDA



TestAmerica Sacramento  
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_008.d  
 Lims ID: 320-31468-A-23-A  
 Client ID: WGNA-091117-DUP09  
 Sample Type: Client  
 Inject. Date: 20-Sep-2017 04:21:29 ALS Bottle#: 6 Worklist Smp#: 8  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: 320-31468-a-23-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:15 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d  
 Column 1 : Det: EXP1  
 Process Host: XAWRK008

First Level Reviewer: barnettj Date: 20-Sep-2017 13:22:04

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	7.46	74.59
\$ 10 13C2 PFDA	10.0	12.5	124.52

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_008.d  
Injection Date: 20-Sep-2017 04:21:29 Instrument ID: A8\_N  
Lims ID: 320-31468-A-23-A Lab Sample ID: 320-31468-23  
Client ID: WGNA-091117-DUP09  
Operator ID: SACINSTLCMS01 ALS Bottle#: 6 Worklist Smp#: 8  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1


Signal: 1

Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results



RT: 2.01  
Area: 264838  
Amount: 1.348863  
Amount Units: ng/ml



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_008.d  
Injection Date: 20-Sep-2017 04:21:29 Instrument ID: A8\_N  
Lims ID: 320-31468-A-23-A Lab Sample ID: 320-31468-23  
Client ID: WGNA-091117-DUP09  
Operator ID: SACINSTLCMS01 ALS Bottle#: 6 Worklist Smp#: 8  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1


Signal: 1

Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results



RT: 2.01  
Area: 264838  
Amount: 1.348863  
Amount Units: ng/ml

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_008.d  
Injection Date: 20-Sep-2017 04:21:29 Instrument ID: A8\_N  
Lims ID: 320-31468-A-23-A Lab Sample ID: 320-31468-23  
Client ID: WGNA-091117-DUP09  
Operator ID: SACINSTLCMS01 ALS Bottle#: 6 Worklist Smp#: 8  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

4 Perfluoroheptanoic acid, CAS: 375-85-9

Signal: 1


Not Detected  
Expected RT: 1.67

Processing Integration Results



Manual Integration Results

RT: 1.66  
Area: 72735  
Amount: 0.325806  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 11:42:06  
Audit Action: Manually Integrated

Audit Reason: Missed Peak

FORM VI  
LCMS BY INTERNAL STANDARD - INITIAL CALIBRATION DATA  
CURVE EVALUATION

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1 Analy Batch No.: 185329

SDG No.: \_\_\_\_\_

Instrument ID: A8\_N GC Column: GeminiC18 3 ID: 3(mm) Heated Purge: (Y/N) N

Calibration Start Date: 09/20/2017 02:56 Calibration End Date: 09/20/2017 03:19 Calibration ID: 34457

Calibration Files:

LEVEL:	LAB SAMPLE ID:	LAB FILE ID:
Level 1	IC 320-185329/4	2017.09.19_537ICAL_004.d
Level 2	IC 320-185329/5	2017.09.19_537ICAL_005.d
Level 3	IC 320-185329/6	2017.09.19_537ICAL_006.d
Level 4	IC 320-185329/7	2017.09.19_537ICAL_007.d
Level 5	IC 320-185329/8	2017.09.19_537ICAL_008.d
Level 6	IC 320-185329/9	2017.09.19_537ICAL_009.d

ANALYTE	RRF					CURVE TYPE	COEFFICIENT			#	MIN RRF	%RSD	#	MAX %RSD	R <sup>2</sup> OR COD	#	MIN R <sup>2</sup> OR COD
	LVL 1 LVL 6	LVL 2	LVL 3	LVL 4	LVL 5		B	M1	M2								
Perfluorobutanesulfonic acid (PFBS)	1.1549 0.7675	1.2218	1.1299	0.9825	0.8671	QuaF		1.2127	-0.002495					1.0000			0.9600
Perfluoroheptanoic acid (PFHpA)	0.9156 0.9157	1.0104	0.9599	0.9323	0.9167	Ave		0.9418			4.0		30.0				
Perfluorohexanesulfonic acid (PFHxS)	1.6240 1.5024	1.7562	1.6778	1.6725	1.5962	Ave		1.6382			5.3		30.0				
Perfluorooctanoic acid (PFOA)	0.8827 0.9310	0.9355	0.9297	0.9101	0.9278	Ave		0.9195			2.2		30.0				
Perfluorooctanesulfonic acid (PFOS)	0.8786 0.9472	0.9205	0.9514	0.9450	0.9475	Ave		0.9317			3.0		30.0				
Perfluorononanoic acid (PFNA)	0.6171 0.6192	0.6458	0.6231	0.6183	0.6076	Ave		0.6218			2.1		30.0				
13C2 PFHxA	1.1170 1.2085	1.1856	1.1778	1.1659	1.1757	Ave		1.1718			2.6		30.0				
13C2 PFDA	0.5262 0.5719	0.5663	0.5603	0.5520	0.5699	Ave		0.5578			3.1		30.0				

Note: The M1 coefficient is the same as Ave RRF for an Ave curve type.

FORM VI  
 LCMS BY INTERNAL STANDARD - INITIAL CALIBRATION DATA  
 RESPONSE AND CONCENTRATION

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1 Analy Batch No.: 185329

SDG No.: \_\_\_\_\_

Instrument ID: A8\_N GC Column: GeminiC18 3 ID: 3(mm) Heated Purge: (Y/N) N

Calibration Start Date: 09/20/2017 02:56 Calibration End Date: 09/20/2017 03:19 Calibration ID: 34457

Calibration Files:

LEVEL:	LAB SAMPLE ID:	LAB FILE ID:
Level 1	IC 320-185329/4	2017.09.19_537ICAL_004.d
Level 2	IC 320-185329/5	2017.09.19_537ICAL_005.d
Level 3	IC 320-185329/6	2017.09.19_537ICAL_006.d
Level 4	IC 320-185329/7	2017.09.19_537ICAL_007.d
Level 5	IC 320-185329/8	2017.09.19_537ICAL_008.d
Level 6	IC 320-185329/9	2017.09.19_537ICAL_009.d

ANALYTE	IS REF	CURVE TYPE	RESPONSE					CONCENTRATION (NG/ML)				
			LVL 1 LVL 6	LVL 2	LVL 3	LVL 4	LVL 5	LVL 1 LVL 6	LVL 2	LVL 3	LVL 4	LVL 5
Perfluorobutanesulfonic acid (PFBS)	PFOS	QuaF	2072419 26277877	5031340	9714039	16708415	22246597	9.00 180	20.0	45.0	90.0	135
Perfluoroheptanoic acid (PFHpA)	13PF OA	Ave	202553 3731330	492336	996370	1954380	2871658	1.00 20.0	2.22	5.00	10.0	15.0
Perfluorohexanesulfonic acid (PFHxS)	PFOS	Ave	971572 17148552	2411042	4809005	9481986	13653533	3.00 60.0	6.67	15.0	30.0	45.0
Perfluorooctanoic acid (PFOA)	13PF OA	Ave	390753 7591950	912252	1931186	3817782	5816384	2.00 40.0	4.45	10.0	20.0	30.0
Perfluorooctanesulfonic acid (PFOS)	PFOS	Ave	700862 14414630	1684976	3635963	7143258	10806665	4.00 80.0	8.89	20.0	40.0	60.0
Perfluorononanoic acid (PFNA)	13PF OA	Ave	273016 5046017	629304	1293375	2592159	3806555	2.00 40.0	4.45	10.0	20.0	30.0
13C2 PFHxA	13PF OA	Ave	2470192 2461679	2599092	2444565	2443470	2454801	10.0 10.0	10.0	10.0	10.0	10.0
13C2 PFDA	13PF OA	Ave	1163662 1164862	1241510	1162968	1156914	1189895	10.0 10.0	10.0	10.0	10.0	10.0

Curve Type Legend:

Ave = Average ISTD
QuaF = Quadratic ISTD forced zero

FORM VI  
 LCMS BY INTERNAL STANDARD - INITIAL CALIBRATION DATA  
 READBACK PERCENT ERROR

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1 Analy Batch No.: 185329

SDG No.: \_\_\_\_\_


Instrument ID: A8\_N GC Column: GeminiC18 3 ID: 3(mm) Heated Purge: (Y/N) N


Calibration Start Date: 09/20/2017 02:56 Calibration End Date: 09/20/2017 03:19 Calibration ID: 34457

Calibration Files:

LEVEL:	LAB SAMPLE ID:	LAB FILE ID:
Level 1	IC 320-185329/4	2017.09.19_537ICAL_004.d
Level 2	IC 320-185329/5	2017.09.19_537ICAL_005.d
Level 3	IC 320-185329/6	2017.09.19_537ICAL_006.d
Level 4	IC 320-185329/7	2017.09.19_537ICAL_007.d
Level 5	IC 320-185329/8	2017.09.19_537ICAL_008.d
Level 6	IC 320-185329/9	2017.09.19_537ICAL_009.d

ANALYTE	PERCENT ERROR						PERCENT ERROR LIMIT					
	LVL 1 #	LVL 2 #	LVL 3 #	LVL 4 #	LVL 5 #	LVL 6 #	LVL 1	LVL 2	LVL 3	LVL 4	LVL 5	LVL 6
Perfluorobutanesulfonic acid (PFBS)	-3.0	5.3	3.0	-0.7	-1.6	1.3	50	30	30	30	30	30
Perfluoroheptanoic acid (PFHpA)	-2.8	7.3	1.9	-1.0	-2.7	-2.8	50	30	30	30	30	30
Perfluorohexanesulfonic acid (PFHxS)	-0.9	7.2	2.4	2.1	-2.6	-8.3	50	30	30	30	30	30
Perfluorooctanoic acid (PFOA)	-4.0	1.7	1.1	-1.0	0.9	1.3	50	30	30	30	30	30
Perfluorooctanesulfonic acid (PFOS)	-5.7	-1.2	2.1	1.4	1.7	1.7	50	30	30	30	30	30
Perfluorononanoic acid (PFNA)	-0.8	3.8	0.2	-0.6	-2.3	-0.4	50	30	30	30	30	30
13C2 PFHxA	-4.7	1.2	0.5	-0.5	0.3	3.1	30	30	30	30	30	30
13C2 PFDA	-5.7	1.5	0.5	-1.0	2.2	2.5	30	30	30	30	30	30

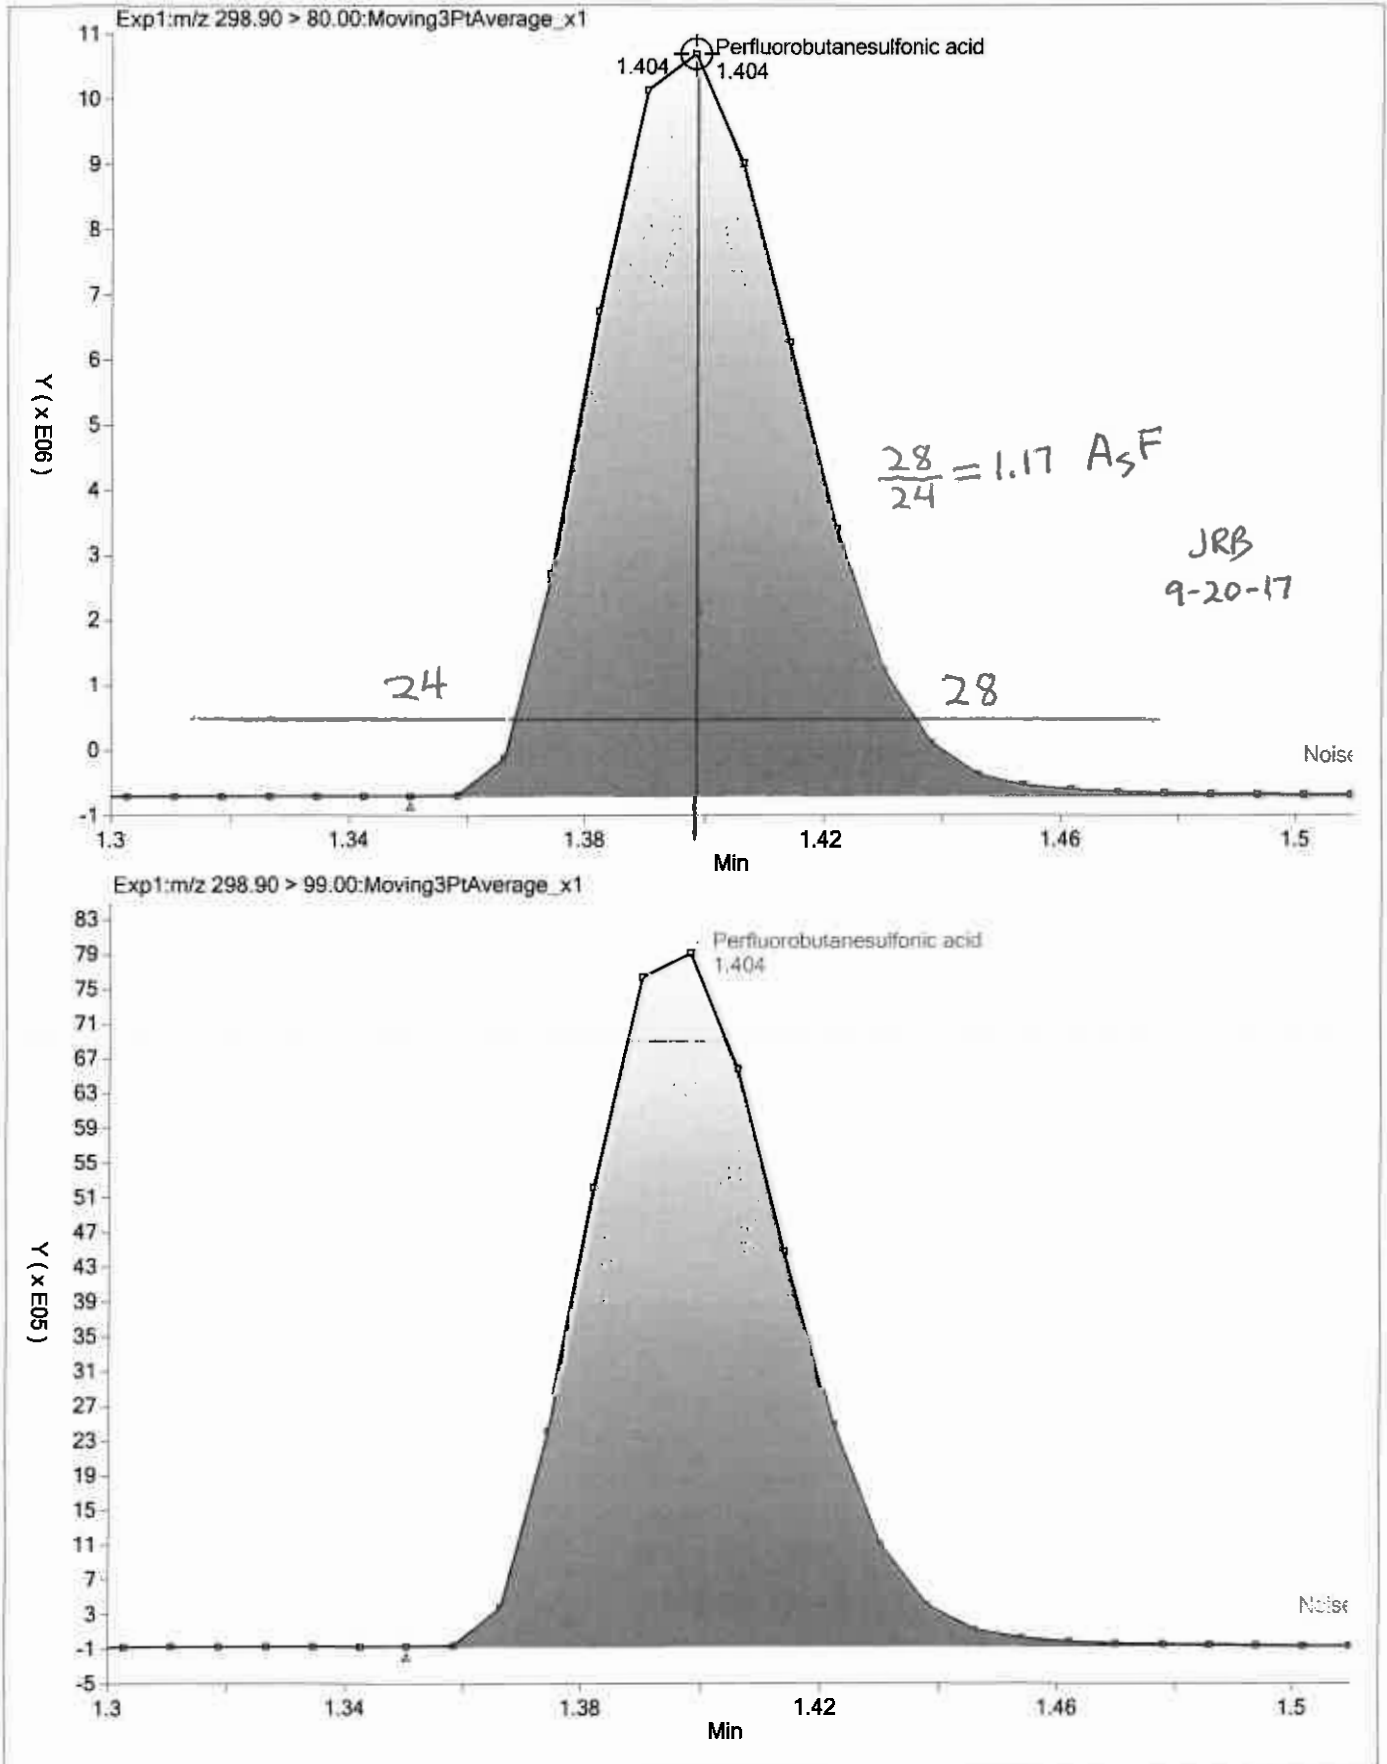



TestAmerica Laboratories  
Istd/Surrogate Recovery Report

Worklist Name: 19SEP2017\_537\_ICAL      Worklist Num: 48154  
 Instrument: A8\_N      Method: 537\_A8\_N  
 Batch Directory: \\ChromNa\Sacramento\ChromData\A8\_N\20170919-48154.b  
 Limit Group: LC 537 ICAL  
 Analysis Type: SemiVOA  
 Inj Volume: 2.00      Inj Vol Units: ul

Lims Batch: 185329  
 CCV IS Mode: Select Ical Level, Cal Level: 3  
 Non-Cal IS Mode: Last Ccal Sample

\$ 2 13C2 PFHxA  
 \$ 10 13C2 PFDA

Lab ID	Inj Date	\$ 2	\$ 10	* 6 13C2-PFOA	* 7 13C4 PFOS
	IS Std			1939425 1.94	5718230 2.17
# 1 RB	20-Sep-2017 02:41:50			2065918 106.5 1.86	5411709 94.6 2.11
# 2 RB	20-Sep-2017 02:46:34			2077017 107.1 1.85	5614007 98.2 2.11
	IS Std			2075431 1.85	5478893 2.10
# 3 RB	20-Sep-2017 02:51:19			1999632 96.3 1.85	5340682 97.5 2.11
	IS Std				
# 4 IC L1	20-Sep-2017 02:56:02	1.53 95.33	2.28 94.34	2211369> 100.0* 1.85	5717338> 100.0* 2.11
# 5 IC L2	20-Sep-2017 03:00:47	1.53 101.20	2.28 101.50	2192240> 99.1* 1.86	5904759> 103.3* 2.11
# 6 IC L3	20-Sep-2017 03:05:32	1.52 100.50	2.28 100.50	2075481> 93.9* 1.85	5478893> 95.8* 2.10
# 7 IC L4	20-Sep-2017 03:10:16	1.53 99.50	2.28 98.97	2095801> 94.8* 1.86	5418565> 94.8* 2.11
# 8 IC L5	20-Sep-2017 03:15:01	1.53 100.30	2.28 102.20	2087979> 94.4* 1.86	5450221> 95.3* 2.11
# 9 IC L6	20-Sep-2017 03:19:48	1.53 103.10	2.28 102.50	2036942> 92.1* 1.85	5454650> 95.4* 2.11
	IS Std			2075481 1.85	5478893 2.10
#10 RB	20-Sep-2017 03:24:33			2085152 100.5 1.85	5726961 104.5 2.10
	IS Std			2095801 1.86	5418565 2.11
#11 CCVL	20-Sep-2017 03:29:17	1.52 97.20	2.28 102.10	2252465 107.5 1.85	5723538 105.6 2.10
	IS Std			2252465 1.85	5723538 2.10
#12 RB	20-Sep-2017 03:34:02			2077507 92.2 1.85	5580721 97.5 2.10
	IS Std			2095801 1.86	5418565 2.11
#13 ICV	20-Sep-2017 03:38:46	1.53 99.40	2.28 103.60	2616480 124.8 1.85	7294448 134.6 2.10
	IS Std			1963439 1.85	5207540 2.11
#14 RB	20-Sep-2017 03:43:31			1963439 100.0 1.85	5207540 100.0 2.11

13C2-PFOA

$$RPD = \frac{2211369 - 2036942}{2211369 + 2036942} = 8.2$$

13C4-PFOS

$$RPD = \frac{5904759 - 5418565}{5904759 + 5418565} = 8.6$$

JRB

9-20-17



TestAmerica Sacramento  
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_004.d  
 Lims ID: IC L1  
 Client ID:  
 Sample Type: IC Calib Level: 1  
 Inject. Date: 20-Sep-2017 02:56:02 ALS Bottle#: 1 Worklist Smp#: 4  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: L1\_537  
 Misc. Info.: Plate: 1 Rack: 1  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Sublist: chrom-537\_A8\_N\*sub1  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170919-48154.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 10:35:29 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d

Column 1 : Det: EXP1  
 Process Host: XAWRK008

First Level Reviewer: barnettj Date: 20-Sep-2017 10:03:54

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.404	1.402	0.002	1.000	2072419	8.73		6405	
298.90 > 99.00	1.404	1.402	0.002	1.000	1455019		1.42(0.00-0.00)	3941	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.525	1.524	0.001	1.000	2470192	9.53		11139	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.669	1.668	0.001	1.000	971572	2.98		3003	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.669	1.668	0.001	1.000	202553	0.9726		61.6	
* 6 13C2-PFOA									
415.00 > 370.00	1.851	1.855	-0.004		2211369	10.0		9755	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.859	1.856	0.003	1.000	390753	1.92		17.1	
413.00 > 169.00	1.859	1.856	0.003	1.000	208681		1.87(0.00-0.00)	858	
* 7 13C4 PFOS									
503.00 > 80.00	2.109	2.108	0.001		5717338	28.7		8554	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.109	2.109	0.0	1.000	700862	3.77		668	M
499.00 > 99.00	2.109	2.109	0.0	1.000	152073		4.61(0.00-0.00)	192	M
9 Perfluorononanoic acid									
463.00 > 419.00	2.117	2.116	0.001	1.000	273016	1.99		41.2	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.284	2.282	0.002	1.000	1163662	9.43		9791	

**QC Flag Legend**

Review Flags

M - Manually Integrated

**Reagents:**

LC537-L1\_00020

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_004.d

Injection Date: 20-Sep-2017 02:56:02

Instrument ID: A8\_N

Lims ID: IC L1

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 1

Worklist Smp#: 4

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537\_A8\_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




\* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




\* 7 13C4 PFOS




8 Perfluorooctane sulfonic acid (M)

8 Perfluorooctane sulfonic acid (M)

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_004.d  
Injection Date: 20-Sep-2017 02:56:02 Instrument ID: A8\_N  
Lims ID: IC L1  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 1 Worklist Smp#: 4  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.11

Processing Integration Results



Manual Integration Results

RT: 2.11  
Area: 700862  
Amount: 3.773476  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 10:02:54  
Audit Action: Assigned Compound ID

Audit Reason: Missed Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_004.d  
Injection Date: 20-Sep-2017 02:56:02 Instrument ID: A8\_N  
Lims ID: IC L1  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 1 Worklist Smp#: 4  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected  
Expected RT: 2.11

Processing Integration Results



RT: 2.11  
Area: 152073  
Amount: 3.773476  
Amount Units: ng/ml

Manual Integration Results



Reviewer: barnettj, 20-Sep-2017 10:03:37

Audit Action: Manually Integrated

Audit Reason: Missed Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_004.d  
Injection Date: 20-Sep-2017 02:56:02 Instrument ID: A8\_N  
Lims ID: IC L1  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 1 Worklist Smp#: 4  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1


Signal: 1

Not Detected  
Expected RT: 2.11

Processing Integration Results



Manual Integration Results



RT: 2.11  
Area: 700862  
Amount: 3.773476  
Amount Units: ng/ml

TestAmerica Sacramento  
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_005.d  
 Lims ID: IC L2  
 Client ID:  
 Sample Type: IC Calib Level: 2  
 Inject. Date: 20-Sep-2017 03:00:47 ALS Bottle#: 2 Worklist Smp#: 5  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: L2\_537  
 Misc. Info.: Plate: 1 Rack: 1  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Sublist: chrom-537\_A8\_N\*sub1  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170919-48154.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 10:35:30 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d  
 Column 1 : Det: EXP1  
 Process Host: XAWRK008

First Level Reviewer: barnettj Date: 20-Sep-2017 10:04:59

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.404	1.402	0.002	1.000	5031340	21.1		7563	
298.90 > 99.00	1.404	1.402	0.002	1.000	3464667		1.45(0.00-0.00)	5263	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.525	1.524	0.001	1.000	2599092	10.1		7997	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.669	1.668	0.001	1.000	492336	2.38		155	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.669	1.668	0.001	1.000	2411042	7.15		4372	
* 6 13C2-PFOA									
415.00 > 370.00	1.859	1.855	0.004		2192240	10.0		6795	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.859	1.856	0.003	1.000	912252	4.53		39.5	
413.00 > 169.00	1.859	1.856	0.003	1.000	481504		1.89(0.00-0.00)	1816	
* 7 13C4 PFOS									
503.00 > 80.00	2.109	2.108	0.001		5904759	28.7		8529	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.109	2.109	0.0	1.000	1684976	8.78		1115	M
499.00 > 99.00	2.109	2.109	0.0	1.000	369952		4.55(0.00-0.00)	447	M
9 Perfluorononanoic acid									
463.00 > 419.00	2.117	2.116	0.001	1.000	629304	4.62		87.1	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.284	2.282	0.002	1.000	1241510	10.2		10447	



**QC Flag Legend**

Review Flags

M - Manually Integrated

**Reagents:**

LC537-L2\_00020

Amount Added: 1.00

Units: mL

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_005.d

Injection Date: 20-Sep-2017 03:00:47

Instrument ID: A8\_N

Lims ID: IC L2

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 2

Worklist Smp#: 5

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537\_A8\_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



4 Perfluoroheptanoic acid

3 Perfluorohexanesulfonic acid




\* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




\* 7 13C4 PFOS




8 Perfluorooctane sulfonic acid (M)

8 Perfluorooctane sulfonic acid (M)

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_005.d  
Injection Date: 20-Sep-2017 03:00:47 Instrument ID: A8\_N  
Lims ID: IC L2  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 2 Worklist Smp#: 5  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.11

Processing Integration Results



Manual Integration Results

RT: 2.11  
Area: 1684976  
Amount: 8.784044  
Amount Units: ng/ml



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_005.d  
Injection Date: 20-Sep-2017 03:00:47 Instrument ID: A8\_N  
Lims ID: IC L2  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 2 Worklist Smp#: 5  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected  
Expected RT: 2.11

Processing Integration Results



Manual Integration Results

RT: 2.11  
Area: 369952  
Amount: 8.784044  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 10:04:48

Audit Action: Manually Integrated

Audit Reason: Missed Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_005.d  
Injection Date: 20-Sep-2017 03:00:47 Instrument ID: A8\_N  
Lims ID: IC L2  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 2 Worklist Smp#: 5  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1


Signal: 1

Not Detected  
Expected RT: 2.11

Processing Integration Results



Manual Integration Results



RT: 2.11  
Area: 1684976  
Amount: 8.784044  
Amount Units: ng/ml

TestAmerica Sacramento  
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_006.d  
 Lims ID: IC L3  
 Client ID:  
 Sample Type: IC Calib Level: 3  
 Inject. Date: 20-Sep-2017 03:05:32 ALS Bottle#: 3 Worklist Smp#: 6  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: L3\_537  
 Misc. Info.: Plate: 1 Rack: 1  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Sublist: chrom-537\_A8\_N\*sub1  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170919-48154.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 10:35:31 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d

Column 1 : Det: EXP1  
 Process Host: XAWRK008

First Level Reviewer: barnettj Date: 20-Sep-2017 10:05:28

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.396	1.402	-0.006	1.000	9714039	46.3		7320	
298.90 > 99.00	1.396	1.402	-0.006	1.000	6860395		1.42(0.00-0.00)	6049	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.517	1.524	-0.007	1.000	2444565	10.1		7634	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.662	1.668	-0.006	1.000	4809005	15.4		5113	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.662	1.668	-0.006	1.000	996370	5.10		304	
* 6 13C2-PFOA									
415.00 > 370.00	1.851	1.855	-0.004		2075481	10.0		7307	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.851	1.856	-0.005	1.000	1931186	10.1		80.1	
413.00 > 169.00	1.851	1.856	-0.005	1.000	1010441		1.91(0.00-0.00)	3393	
* 7 13C4 PFOS									
503.00 > 80.00	2.102	2.108	-0.006		5478893	28.7		7009	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.102	2.109	-0.007	1.000	3635963	20.4		4871	M
499.00 > 99.00	2.102	2.109	-0.007	1.000	723199		5.03(0.00-0.00)	729	M
9 Perfluorononanoic acid									
463.00 > 419.00	2.109	2.116	-0.007	1.000	1293375	10.0		234	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.276	2.282	-0.006	1.000	1162968	10.0		8493	

**QC Flag Legend**

Review Flags

M - Manually Integrated

**Reagents:**

LC537-L3\_00023

Amount Added: 1.00

Units: mL



TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_006.d

Injection Date: 20-Sep-2017 03:05:32

Instrument ID: A8\_N

Lims ID: IC L3

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 3

Worklist Smp#: 6

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537\_A8\_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




\* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




\* 7 13C4 PFOS




8 Perfluorooctane sulfonic acid (M)

8 Perfluorooctane sulfonic acid (M)

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_006.d  
Injection Date: 20-Sep-2017 03:05:32 Instrument ID: A8\_N  
Lims ID: IC L3  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 3 Worklist Smp#: 6  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.11

Processing Integration Results



Manual Integration Results

RT: 2.10  
Area: 3635963  
Amount: 20.428176  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 10:05:06  
Audit Action: Assigned Compound ID

Audit Reason: Missed Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_006.d  
Injection Date: 20-Sep-2017 03:05:32 Instrument ID: A8\_N  
Lims ID: IC L3  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 3 Worklist Smp#: 6  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected  
Expected RT: 2.11

Processing Integration Results



Manual Integration Results

RT: 2.10  
Area: 723199  
Amount: 20.428176  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 10:05:21

Audit Action: Manually Integrated

Audit Reason: Missed Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_006.d  
Injection Date: 20-Sep-2017 03:05:32 Instrument ID: A8\_N  
Lims ID: IC L3  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 3 Worklist Smp#: 6  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1


Signal: 1

Not Detected  
Expected RT: 2.11

Processing Integration Results



Manual Integration Results



RT: 2.10  
Area: 3635963  
Amount: 20.428176  
Amount Units: ng/ml

TestAmerica Sacramento  
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_007.d  
 Lims ID: IC L4  
 Client ID:  
 Sample Type: ICISAV Calib Level: 4  
 Inject. Date: 20-Sep-2017 03:10:16 ALS Bottle#: 4 Worklist Smp#: 7  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: L4\_537  
 Misc. Info.: Plate: 1 Rack: 1  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Sublist: chrom-537\_A8\_N\*sub1

Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170919-48154.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 10:35:32 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d

Column 1 : Det: EXP1  
 Process Host: XAWRK008

First Level Reviewer: barnettj Date: 20-Sep-2017 10:06:05

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.404	1.402	0.002	1.000	16708415	89.3		6528	
298.90 > 99.00	1.404	1.402	0.002	1.000	12155594		1.37(0.00-0.00)	6466	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.525	1.524	0.001	1.000	2443470	9.95		7571	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.669	1.668	0.001	1.000	1954380	9.90		573	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.669	1.668	0.001	1.000	9481986	30.6		5903	
* 6 13C2-PFOA									
415.00 > 370.00	1.859	1.855	0.004		2095801	10.0		7193	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.859	1.856	0.003	1.000	3817782	19.8		156	
413.00 > 169.00	1.859	1.856	0.003	1.000	2029912		1.88(0.00-0.00)	6086	
* 7 13C4 PFOS									
503.00 > 80.00	2.109	2.108	0.001		5418565	28.7		8070	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.109	2.109	0.0	1.000	7143258	40.6		5401	M
499.00 > 99.00	2.109	2.109	0.0	1.000	1480190		4.83(0.00-0.00)	1160	M
9 Perfluorononanoic acid									
463.00 > 419.00	2.117	2.116	0.001	1.000	2592159	19.9		433	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.284	2.282	0.002	1.000	1156914	9.90		8203	

**QC Flag Legend**

Review Flags

M - Manually Integrated

**Reagents:**

LC537-L4\_00020

Amount Added: 1.00

Units: mL

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_007.d

Injection Date: 20-Sep-2017 03:10:16

Instrument ID: A8\_N

Lims ID: IC L4

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 4

Worklist Smp#: 7

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537\_A8\_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



4 Perfluoroheptanoic acid

3 Perfluorohexanesulfonic acid




\* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




\* 7 13C4 PFOS



8 Perfluorooctane sulfonic acid (M)


8 Perfluorooctane sulfonic acid (M)

9 Perfluorononanoic acid





\$ 10 13C2 PFDA



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_007.d  
Injection Date: 20-Sep-2017 03:10:16 Instrument ID: A8\_N  
Lims ID: IC L4  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 4 Worklist Smp#: 7  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1


Signal: 1

Not Detected  
Expected RT: 2.11

Processing Integration Results



Manual Integration Results



RT: 2.11  
Area: 7143258  
Amount: 40.580278  
Amount Units: ng/ml

Reviewer: barnettj, 20-Sep-2017 10:05:35  
Audit Action: Assigned Compound ID

Audit Reason: Missed Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_007.d  
Injection Date: 20-Sep-2017 03:10:16 Instrument ID: A8\_N  
Lims ID: IC L4  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 4 Worklist Smp#: 7  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected  
Expected RT: 2.11

Processing Integration Results



Manual Integration Results

RT: 2.11  
Area: 1480190  
Amount: 40.580278  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 10:05:50

Audit Action: Manually Integrated

Audit Reason: Missed Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_007.d  
Injection Date: 20-Sep-2017 03:10:16 Instrument ID: A8\_N  
Lims ID: IC L4  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 4 Worklist Smp#: 7  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.11

Processing Integration Results



Manual Integration Results

RT: 2.11  
Area: 7143258  
Amount: 40.580278  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 10:05:50

Audit Action: Manually Integrated

Audit Reason: Missed Peak

TestAmerica Sacramento  
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_008.d  
 Lims ID: IC L5  
 Client ID:  
 Sample Type: IC Calib Level: 5  
 Inject. Date: 20-Sep-2017 03:15:01 ALS Bottle#: 5 Worklist Smp#: 8  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: L5\_537  
 Misc. Info.: Plate: 1 Rack: 1  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Sublist: chrom-537\_A8\_N\*sub1  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170919-48154.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 10:35:33 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d

Column 1 : Det: EXP1  
 Process Host: XAWRK008

First Level Reviewer: barnettj Date: 20-Sep-2017 10:06:40

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.404	1.402	0.002	1.000	22246597	132.8		7166	
298.90 > 99.00	1.404	1.402	0.002	1.000	16593473		1.34(0.00-0.00)	7174	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.525	1.524	0.001	1.000	2454801	10.0		9700	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.669	1.668	0.001	1.000	13653533	43.9		6726	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.669	1.668	0.001	1.000	2871658	14.6		836	
* 6 13C2-PFOA									
415.00 > 370.00	1.859	1.855	0.004		2087979	10.0		8636	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.859	1.856	0.003	1.000	5816384	30.3		226	
413.00 > 169.00	1.859	1.856	0.003	1.000	3025635		1.92(0.00-0.00)	7093	
* 7 13C4 PFOS									
503.00 > 80.00	2.109	2.108	0.001		5450221	28.7		7142	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.109	2.109	0.0	1.000	10806665	61.0		6680	M
499.00 > 99.00	2.109	2.109	0.0	1.000	2283151		4.73(0.00-0.00)	1726	M
9 Perfluorononanoic acid									
463.00 > 419.00	2.117	2.116	0.001	1.000	3806555	29.3		645	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.284	2.282	0.002	1.000	1189895	10.2		10440	

**QC Flag Legend**

Review Flags

M - Manually Integrated

**Reagents:**

LC537-L5\_00024

Amount Added: 1.00

Units: mL

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_008.d

Injection Date: 20-Sep-2017 03:15:01

Instrument ID: A8\_N

Lims ID: IC L5

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 5

Worklist Smp#: 8

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537\_A8\_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




\* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




\* 7 13C4 PFOS




8 Perfluorooctane sulfonic acid (M)

8 Perfluorooctane sulfonic acid (M)

9 Perfluorononanoic acid



\$ 10 13C2 PFDA





TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_008.d  
Injection Date: 20-Sep-2017 03:15:01 Instrument ID: A8\_N  
Lims ID: IC L5  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 5 Worklist Smp#: 8  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.11

Processing Integration Results



Manual Integration Results

RT: 2.11  
Area: 10806665  
Amount: 61.035224  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 10:06:19  
Audit Action: Assigned Compound ID

Audit Reason: Missed Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_008.d  
Injection Date: 20-Sep-2017 03:15:01 Instrument ID: A8\_N  
Lims ID: IC L5  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 5 Worklist Smp#: 8  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected  
Expected RT: 2.11

Processing Integration Results



Manual Integration Results

RT: 2.11  
Area: 2283151  
Amount: 61.035224  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 10:06:32

Audit Action: Manually Integrated

Audit Reason: Missed Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_008.d  
Injection Date: 20-Sep-2017 03:15:01 Instrument ID: A8\_N  
Lims ID: IC L5  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 5 Worklist Smp#: 8  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.11

Processing Integration Results



Manual Integration Results

RT: 2.11  
Area: 10806665  
Amount: 61.035224  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 10:06:32

Audit Action: Manually Integrated

Audit Reason: Missed Peak

TestAmerica Sacramento  
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d  
 Lims ID: IC L6  
 Client ID:  
 Sample Type: IC Calib Level: 6  
 Inject. Date: 20-Sep-2017 03:19:48 ALS Bottle#: 6 Worklist Smp#: 9  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: L6\_537  
 Misc. Info.: Plate: 1 Rack: 1  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Sublist: chrom-537\_A8\_N\*sub1

Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170919-48154.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 10:35:34 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d

Column 1 : Det: EXP1  
 Process Host: XAWRK008

First Level Reviewer: barnettj Date: 20-Sep-2017 10:07:38

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.404	1.402	0.002	1.000	26277877	182.3		5148	
298.90 > 99.00	1.404	1.402	0.002	1.000	20065753		1.31(0.00-0.00)	5796	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.525	1.524	0.001	1.000	2461679	10.3		8448	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.669	1.668	0.001	1.000	3731330	19.5		999	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.669	1.668	0.001	1.000	17148552	55.0		5562	
* 6 13C2-PFOA									
415.00 > 370.00	1.851	1.855	-0.004		2036942	10.0		7709	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.851	1.856	-0.005	1.000	7591950	40.5		298	
413.00 > 169.00	1.851	1.856	-0.005	1.000	4055944		1.87(0.00-0.00)	6840	
* 7 13C4 PFOS									
503.00 > 80.00	2.109	2.108	0.001		5454650	28.7		5153	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.109	2.109	0.0	1.000	14414630	81.3		7141	M
499.00 > 99.00	2.102	2.109	-0.007	0.996	3087448		4.67(0.00-0.00)	1891	M
9 Perfluorononanoic acid									
463.00 > 419.00	2.117	2.116	0.001	1.000	5046017	39.8		666	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.284	2.282	0.002	1.000	1164862	10.3		8578	

**QC Flag Legend**

Review Flags

M - Manually Integrated

**Reagents:**

LC537-L6\_00020

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d

Injection Date: 20-Sep-2017 03:19:48

Instrument ID: A8\_N

Lims ID: IC L6

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 6

Worklist Smp#: 9

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537\_A8\_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



4 Perfluoroheptanoic acid

3 Perfluorohexanesulfonic acid




\* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




\* 7 13C4 PFOS




8 Perfluorooctane sulfonic acid (M)

8 Perfluorooctane sulfonic acid (M)

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d  
Injection Date: 20-Sep-2017 03:19:48 Instrument ID: A8\_N  
Lims ID: IC L6  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 6 Worklist Smp#: 9  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.11

Processing Integration Results



Manual Integration Results

RT: 2.11  
Area: 14414630  
Amount: 81.346632  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 10:06:49  
Audit Action: Assigned Compound ID

Audit Reason: Missed Peak



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d  
Injection Date: 20-Sep-2017 03:19:48 Instrument ID: A8\_N  
Lims ID: IC L6  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 6 Worklist Smp#: 9  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected  
Expected RT: 2.11

Processing Integration Results



Manual Integration Results

RT: 2.10  
Area: 3087448  
Amount: 81.346632  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 10:07:12

Audit Action: Manually Integrated

Audit Reason: Missed Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d  
Injection Date: 20-Sep-2017 03:19:48 Instrument ID: A8\_N  
Lims ID: IC L6  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 6 Worklist Smp#: 9  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.11

Processing Integration Results



Manual Integration Results

RT: 2.11  
Area: 14414630  
Amount: 81.346632  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 10:07:12

Audit Action: Manually Integrated

Audit Reason: Missed Peak

FORM VII  
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Lab Sample ID: CCVL 320-185329/11 Calibration Date: 09/20/2017 03:29  
 Instrument ID: A8\_N Calib Start Date: 09/20/2017 02:56  
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 09/20/2017 03:19  
 Lab File ID: 2017.09.19\_537ICAL\_011.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		1.235		21.3	20.0	6.5	50.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9418	0.9779		2.31	2.22	3.8	50.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.638	1.762		7.17	6.67	7.6	50.0
Perfluorooctanoic acid (PFOA)	Ave	0.9195	0.9059		4.38	4.45	-1.5	50.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9317	0.9490		9.06	8.89	1.9	50.0
Perfluorononanoic acid (PFNA)	Ave	0.6218	0.6352		4.54	4.45	2.2	50.0
13C2 PFHxA	Ave	1.172	1.139		9.72	10.0	-2.8	30.0
13C2 PFDA	Ave	0.5578	0.5694		10.2	10.0	2.1	30.0

TestAmerica Sacramento  
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_011.d  
 Lims ID: CCVL  
 Client ID:  
 Sample Type: CCVL  
 Inject. Date: 20-Sep-2017 03:29:17 ALS Bottle#: 2 Worklist Smp#: 11  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: CCV L2  
 Misc. Info.: Plate: 1 Rack: 1  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Sublist: chrom-537\_A8\_N\*sub1  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170919-48154.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 10:35:36 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d  
 Column 1 : Det: EXP1  
 Process Host: XAWRK008

First Level Reviewer: barnettj Date: 20-Sep-2017 10:10:45

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.396	1.402	-0.006	1.000	4928523	21.3		8745	
298.90 > 99.00	1.396	1.402	-0.006	1.000	3609505		1.37(0.00-0.00)	6187	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.517	1.524	-0.007	1.000	2565324	9.72		10005	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.662	1.668	-0.006	1.000	2344621	7.17		4423	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.662	1.668	-0.006	1.000	489617	2.31		144	
* 6 13C2-PFOA									
415.00 > 370.00	1.851	1.855	-0.004		2252465	10.0		8774	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.851	1.856	-0.005	1.000	907626	4.38		34.8	
413.00 > 169.00	1.851	1.856	-0.005	1.000	489379		1.85(0.00-0.00)	2088	
* 7 13C4 PFOS									
503.00 > 80.00	2.102	2.108	-0.006		5723538	28.7		6648	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.102	2.109	-0.007	1.000	1683920	9.06		2776	M
499.00 > 99.00	2.102	2.109	-0.007	1.000	342465		4.92(0.00-0.00)	388	M
9 Perfluorononanoic acid									
463.00 > 419.00	2.109	2.116	-0.007	1.000	636035	4.54		88.8	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.276	2.282	-0.006	1.000	1282617	10.2		10770	

**QC Flag Legend**

Review Flags

M - Manually Integrated

**Reagents:**

LC537-L2\_00020




Amount Added: 1.00

Units: mL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




\* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




\* 7 13C4 PFOS




8 Perfluorooctane sulfonic acid (M)

8 Perfluorooctane sulfonic acid (M)

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_011.d  
Injection Date: 20-Sep-2017 03:29:17 Instrument ID: A8\_N  
Lims ID: CCVL  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 2 Worklist Smp#: 11  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.11

Processing Integration Results



RT: 2.10  
Area: 1683920  
Amount: 9.056489  
Amount Units: ng/ml

Manual Integration Results



Reviewer: barnettj, 20-Sep-2017 10:10:03  
Audit Action: Assigned Compound ID

Audit Reason: Missed Peak



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_011.d  
Injection Date: 20-Sep-2017 03:29:17 Instrument ID: A8\_N  
Lims ID: CCVL  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 2 Worklist Smp#: 11  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected  
Expected RT: 2.11

Processing Integration Results



Manual Integration Results

RT: 2.10  
Area: 342465  
Amount: 9.056489  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 10:10:20

Audit Action: Manually Integrated

Audit Reason: Missed Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_011.d  
Injection Date: 20-Sep-2017 03:29:17 Instrument ID: A8\_N  
Lims ID: CCVL  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 2 Worklist Smp#: 11  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.11

Processing Integration Results



RT: 2.10  
Area: 1683920  
Amount: 9.056489  
Amount Units: ng/ml

Manual Integration Results



Reviewer: barnettj, 20-Sep-2017 10:10:20

Audit Action: Manually Integrated

Audit Reason: Missed Peak

FORM VII  
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Lab Sample ID: ICV 320-185329/13 Calibration Date: 09/20/2017 03:38  
 Instrument ID: A8\_N Calib Start Date: 09/20/2017 02:56  
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 09/20/2017 03:19  
 Lab File ID: 2017.09.19\_537ICAL\_013.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		0.9069		92.5	100	-7.7	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9418	0.9703		10.3	10.0	3.0	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.638	1.860		22.8	20.1	13.5	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9195	0.9535		21.2	20.5	3.7	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9317	1.134		24.0	19.7	21.8	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6218	0.7173		23.2	20.1	15.3	30.0
13C2 PFHxA	Ave	1.172	1.165		9.94	10.0	-0.6	30.0
13C2 PFDA	Ave	0.5578	0.5781		10.4	10.0	3.6	30.0

TestAmerica Sacramento  
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_013.d  
 Lims ID: ICV  
 Client ID:  
 Sample Type: ICV  
 Inject. Date: 20-Sep-2017 03:38:46 ALS Bottle#: 7 Worklist Smp#: 13  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: ICV  
 Misc. Info.: Plate: 1 Rack: 1  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Sublist:

Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170919-48154.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 10:35:38 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last Ical File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d

Column 1 : Det: EXP1  
 Process Host: XAWRK008

First Level Reviewer: barnettj Date: 20-Sep-2017 10:35:23

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.404	1.402	0.002	1.000	23093305	92.5		5826	
298.90 > 99.00	1.404	1.402	0.002	1.000	17724893		1.30(0.00-0.00)	6513	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.525	1.524	0.001	1.000	3047368	9.94		9351	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.669	1.668	0.001	1.000	9496803	22.8		6818	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.669	1.668	0.001	1.000	2537716	10.3		696	
* 6 13C2-PFOA									
415.00 > 370.00	1.851	1.855	-0.004		2616480	10.0		7926	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.851	1.856	-0.005	1.000	5110686	21.2		193	
413.00 > 169.00	1.851	1.856	-0.005	1.000	2741837		1.86(0.00-0.00)	6488	
* 7 13C4 PFOS									
503.00 > 80.00	2.102	2.108	-0.006		7294448	28.7		6378	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.109	2.109	0.0	1.000	5683706	24.0		5285	M
499.00 > 99.00	2.102	2.109	-0.007	0.996	1038148		5.47(0.00-0.00)	913	M
9 Perfluorononanoic acid									
463.00 > 419.00	2.117	2.116	0.001	1.000	3777210	23.2		739	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.276	2.282	-0.006	1.000	1512622	10.4		11751	

**QC Flag Legend**

Review Flags

M - Manually Integrated

**Reagents:**

LC537-ICV\_00028




Amount Added: 1.00

Units: mL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




\* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




\* 7 13C4 PFOS




8 Perfluorooctane sulfonic acid (M)

8 Perfluorooctane sulfonic acid (M)

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_013.d  
Injection Date: 20-Sep-2017 03:38:46 Instrument ID: A8\_N  
Lims ID: ICV  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 7 Worklist Smp#: 13  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1


Signal: 1

Not Detected  
Expected RT: 2.11

Processing Integration Results



Manual Integration Results



RT: 2.11  
Area: 5683706  
Amount: 23.985133  
Amount Units: ng/ml



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_013.d  
Injection Date: 20-Sep-2017 03:38:46 Instrument ID: A8\_N  
Lims ID: ICV  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 7 Worklist Smp#: 13  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected  
Expected RT: 2.11

Processing Integration Results



Manual Integration Results

RT: 2.10  
Area: 1038148  
Amount: 23.985133  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 10:11:07

Audit Action: Manually Integrated

Audit Reason: Missed Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_013.d  
Injection Date: 20-Sep-2017 03:38:46 Instrument ID: A8\_N  
Lims ID: ICV  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 7 Worklist Smp#: 13  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.11

Processing Integration Results



Manual Integration Results

RT: 2.11  
Area: 5683706  
Amount: 23.985133  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 10:11:07

Audit Action: Manually Integrated

Audit Reason: Missed Peak

FORM VII  
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Lab Sample ID: CCV 320-185406/1 Calibration Date: 09/20/2017 03:48  
 Instrument ID: A8\_N Calib Start Date: 09/20/2017 02:56  
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 09/20/2017 03:19  
 Lab File ID: 2017.09.19\_537A\_001.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		0.8903		139	135	2.7	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9418	0.9394		15.0	15.0	-0.3	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.638	1.592		43.7	45.0	-2.8	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9195	0.9540		31.2	30.0	3.8	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9317	0.9465		61.0	60.0	1.6	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6218	0.6196		29.9	30.0	-0.4	30.0
13C2 PFHxA	Ave	1.172	1.202		10.3	10.0	2.5	30.0
13C2 PFDA	Ave	0.5578	0.5820		10.4	10.0	4.3	30.0

TestAmerica Sacramento  
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_001.d  
 Lims ID: CCV L5  
 Client ID:  
 Sample Type: CCVIS  
 Inject. Date: 20-Sep-2017 03:48:15 ALS Bottle#: 5 Worklist Smp#: 1  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: CCV L5  
 Misc. Info.: Plate: 1 Rack: 1  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Sublist: chrom-537\_A8\_N\*sub1  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:15 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d  
 Column 1 : Det: EXP1  
 Process Host: XAWRK008

First Level Reviewer: barnettj Date: 20-Sep-2017 11:35:38

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.404	1.402	0.002	1.000	21839023	138.7		6131	
298.90 > 99.00	1.404	1.402	0.002	1.000	16362037		1.33(0.00-0.00)	6056	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.525	1.524	0.001	1.000	2339020	10.3		8153	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.669	1.668	0.001	1.000	13015051	43.7		5956	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.669	1.668	0.001	1.000	2743469	15.0		769	
* 6 13C2-PFOA									
415.00 > 370.00	1.851	1.855	-0.004		1946548	10.0		7453	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.851	1.856	-0.005	1.000	5575494	31.2		198	
413.00 > 169.00	1.851	1.856	-0.005	1.000	2950512		1.89(0.00-0.00)	6884	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.109	2.094	0.015	1.000	10320110	61.0		7836	M
499.00 > 99.00	2.102	2.094	0.008	0.996	2127833		4.85(0.00-0.00)	1537	M
* 7 13C4 PFOS									
503.00 > 80.00	2.102	2.108	-0.006		5210623	28.7		6119	
9 Perfluorononanoic acid									
463.00 > 419.00	2.117	2.116	0.001	1.000	3618914	29.9		629	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.284	2.282	0.002	1.000	1132831	10.4		9353	

**QC Flag Legend**

Review Flags

M - Manually Integrated

**Reagents:**

LC537-L5\_00024

Amount Added: 1.00

Units: mL

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_001.d

Injection Date: 20-Sep-2017 03:48:15

Instrument ID: A8\_N

Lims ID: CCV L5

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 5

Worklist Smp#: 1

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537\_A8\_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




\* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

\* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_001.d  
Injection Date: 20-Sep-2017 03:48:15 Instrument ID: A8\_N  
Lims ID: CCV L5  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 5 Worklist Smp#: 1  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.11  
Area: 10320110  
Amount: 60.967395  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 11:35:16  
Audit Action: Assigned Compound ID

Audit Reason: Missed Peak



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_001.d  
Injection Date: 20-Sep-2017 03:48:15 Instrument ID: A8\_N  
Lims ID: CCV L5  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 5 Worklist Smp#: 1  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.10  
Area: 2127833  
Amount: 60.967395  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 11:35:32

Audit Action: Manually Integrated

Audit Reason: Missed Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_001.d  
Injection Date: 20-Sep-2017 03:48:15 Instrument ID: A8\_N  
Lims ID: CCV L5  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 5 Worklist Smp#: 1  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.11  
Area: 10320110  
Amount: 60.967395  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 11:35:32

Audit Action: Manually Integrated

Audit Reason: Missed Peak

FORM VII  
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Lab Sample ID: CCV 320-185406/9 Calibration Date: 09/20/2017 04:26  
 Instrument ID: A8\_N Calib Start Date: 09/20/2017 02:56  
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 09/20/2017 03:19  
 Lab File ID: 2017.09.19\_537A\_009.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		1.115		45.7	45.0	1.5	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9418	0.9367		4.97	5.00	-0.5	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.638	1.690		15.5	15.0	3.2	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9195	0.8864		9.65	10.0	-3.6	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9317	0.9189		19.7	20.0	-1.4	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6218	0.6261		10.1	10.0	0.7	30.0
13C2 PFHxA	Ave	1.172	1.146		9.78	10.0	-2.2	30.0
13C2 PFDA	Ave	0.5578	0.5476		9.82	10.0	-1.8	30.0

FORM VII  
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Lab Sample ID: CCV 320-185407/9 Calibration Date: 09/20/2017 04:26  
 Instrument ID: A8\_N Calib Start Date: 09/20/2017 02:56  
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 09/20/2017 03:19  
 Lab File ID: 2017.09.19\_537A\_009.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		1.115		45.7	45.0	1.5	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9418	0.9367		4.97	5.00	-0.5	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.638	1.690		15.5	15.0	3.2	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9195	0.8864		9.65	10.0	-3.6	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9317	0.9189		19.7	20.0	-1.4	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6218	0.6261		10.1	10.0	0.7	30.0
13C2 PFHxA	Ave	1.172	1.146		9.78	10.0	-2.2	30.0
13C2 PFDA	Ave	0.5578	0.5476		9.82	10.0	-1.8	30.0

TestAmerica Sacramento  
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_009.d  
 Lims ID: CCV L3  
 Client ID:  
 Sample Type: CCVIS  
 Inject. Date: 20-Sep-2017 04:26:13 ALS Bottle#: 3 Worklist Smp#: 9  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: CCV L3  
 Misc. Info.: Plate: 1 Rack: 1  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Sublist: chrom-537\_A8\_N\*sub1  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:27 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d  
 Column 1 : Det: EXP1  
 Process Host: XAWRK008

First Level Reviewer: barnettj Date: 20-Sep-2017 11:36:54

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.396	1.402	-0.006	1.000	9610287	45.7		8080	
298.90 > 99.00	1.396	1.402	-0.006	1.000	6797456		1.41(0.00-0.00)	6657	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.517	1.524	-0.007	1.000	2364296	9.78		8397	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.662	1.668	-0.006	1.000	4855313	15.5		5746	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.662	1.668	-0.006	1.000	966278	4.97		273	
* 6 13C2-PFOA									
415.00 > 370.00	1.851	1.855	-0.004		2062556	10.0		7669	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.851	1.856	-0.005	1.000	1829795	9.65		75.1	
413.00 > 169.00	1.851	1.856	-0.005	1.000	964810		1.90(0.00-0.00)	3563	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.102	2.094	0.008	1.000	3519854	19.7		4625	M
499.00 > 99.00	2.102	2.094	0.008	1.000	719367		4.89(0.00-0.00)	633	M
* 7 13C4 PFOS									
503.00 > 80.00	2.102	2.108	-0.006		5491922	28.7		5669	
9 Perfluorononanoic acid									
463.00 > 419.00	2.109	2.116	-0.007	1.000	1291624	10.1		129	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.276	2.282	-0.006	1.000	1129404	9.82		8258	

**QC Flag Legend**

Review Flags

M - Manually Integrated

**Reagents:**

LC537-L3\_00023

Amount Added: 1.00

Units: mL

TestAmerica Sacramento  
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_009.d  
 Lims ID: CCV L3  
 Client ID:  
 Sample Type: CCVIS  
 Inject. Date: 20-Sep-2017 04:26:13 ALS Bottle#: 3 Worklist Smp#: 9  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: CCV L3  
 Misc. Info.: Plate: 1 Rack: 1  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Sublist: chrom-537\_A8\_N\*sub1  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:27 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d  
 Column 1 : Det: EXP1  
 Process Host: XAWRK008

First Level Reviewer: barnettj Date: 20-Sep-2017 11:36:54

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.396	1.402	-0.006	1.000	9610287	45.7		8080	
298.90 > 99.00	1.396	1.402	-0.006	1.000	6797456		1.41(0.00-0.00)	6657	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.517	1.524	-0.007	1.000	2364296	9.78		8397	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.662	1.668	-0.006	1.000	4855313	15.5		5746	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.662	1.668	-0.006	1.000	966278	4.97		273	
* 6 13C2-PFOA									
415.00 > 370.00	1.851	1.855	-0.004		2062556	10.0		7669	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.851	1.856	-0.005	1.000	1829795	9.65		75.1	
413.00 > 169.00	1.851	1.856	-0.005	1.000	964810		1.90(0.00-0.00)	3563	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.102	2.094	0.008	1.000	3519854	19.7		4625	M
499.00 > 99.00	2.102	2.094	0.008	1.000	719367		4.89(0.00-0.00)	633	M
* 7 13C4 PFOS									
503.00 > 80.00	2.102	2.108	-0.006		5491922	28.7		5669	
9 Perfluorononanoic acid									
463.00 > 419.00	2.109	2.116	-0.007	1.000	1291624	10.1		129	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.276	2.282	-0.006	1.000	1129404	9.82		8258	

**QC Flag Legend**

Review Flags

M - Manually Integrated

**Reagents:**

LC537-L3\_00023

Amount Added: 1.00

Units: mL



TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_009.d

Injection Date: 20-Sep-2017 04:26:13

Instrument ID: A8\_N

Lims ID: CCV L3

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 3

Worklist Smp#: 9

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537\_A8\_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




\* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

\* 7 13C4 PFOS

9 Perfluorononanoic acid






\$ 10 13C2 PFDA



1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




\* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

\* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_009.d  
Injection Date: 20-Sep-2017 04:26:13 Instrument ID: A8\_N  
Lims ID: CCV L3  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 3 Worklist Smp#: 9  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.10  
Area: 3519854  
Amount: 19.728917  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 11:35:43  
Audit Action: Assigned Compound ID

Audit Reason: Missed Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_009.d  
Injection Date: 20-Sep-2017 04:26:13 Instrument ID: A8\_N  
Lims ID: CCV L3  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 3 Worklist Smp#: 9  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.10  
Area: 719367  
Amount: 19.728917  
Amount Units: ng/ml



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_009.d  
Injection Date: 20-Sep-2017 04:26:13 Instrument ID: A8\_N  
Lims ID: CCV L3  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 3 Worklist Smp#: 9  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.10  
Area: 3519854  
Amount: 19.728917  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 11:35:55

Audit Action: Manually Integrated

Audit Reason: Missed Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_009.d  
Injection Date: 20-Sep-2017 04:26:13 Instrument ID: A8\_N  
Lims ID: CCV L3  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 3 Worklist Smp#: 9  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.10  
Area: 3519854  
Amount: 19.728917  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 11:35:43  
Audit Action: Assigned Compound ID

Audit Reason: Missed Peak



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_009.d  
Injection Date: 20-Sep-2017 04:26:13 Instrument ID: A8\_N  
Lims ID: CCV L3  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 3 Worklist Smp#: 9  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.10  
Area: 719367  
Amount: 19.728917  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 11:35:55

Audit Action: Manually Integrated

Audit Reason: Missed Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_009.d  
Injection Date: 20-Sep-2017 04:26:13 Instrument ID: A8\_N  
Lims ID: CCV L3  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 3 Worklist Smp#: 9  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.10  
Area: 3519854  
Amount: 19.728917  
Amount Units: ng/ml



FORM VII  
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Lab Sample ID: CCV 320-185407/21 Calibration Date: 09/20/2017 05:23  
 Instrument ID: A8\_N Calib Start Date: 09/20/2017 02:56  
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 09/20/2017 03:19  
 Lab File ID: 2017.09.19\_537A\_021.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		0.8709		134	135	-0.9	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9418	0.9425		15.0	15.0	0.0	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.638	1.605		44.1	45.0	-2.0	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9195	0.9201		30.0	30.0	0.0	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9317	0.9641		62.1	60.0	3.5	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6218	0.6242		30.1	30.0	0.4	30.0
13C2 PFHxA	Ave	1.172	1.175		10.0	10.0	0.3	30.0
13C2 PFDA	Ave	0.5578	0.5501		9.86	10.0	-1.4	30.0

FORM VII  
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Lab Sample ID: CCV 320-185408/21 Calibration Date: 09/20/2017 05:23  
 Instrument ID: A8\_N Calib Start Date: 09/20/2017 02:56  
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 09/20/2017 03:19  
 Lab File ID: 2017.09.19\_537A\_021.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		0.8709		134	135	-0.9	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9418	0.9425		15.0	15.0	0.0	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.638	1.605		44.1	45.0	-2.0	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9195	0.9201		30.0	30.0	0.0	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9317	0.9641		62.1	60.0	3.5	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6218	0.6242		30.1	30.0	0.4	30.0
13C2 PFHxA	Ave	1.172	1.175		10.0	10.0	0.3	30.0
13C2 PFDA	Ave	0.5578	0.5501		9.86	10.0	-1.4	30.0

TestAmerica Sacramento  
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_021.d  
 Lims ID: CCV L5  
 Client ID:  
 Sample Type: CCVIS  
 Inject. Date: 20-Sep-2017 05:23:10 ALS Bottle#: 5 Worklist Smp#: 21  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: CCV L5  
 Misc. Info.: Plate: 1 Rack: 1  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Sublist: chrom-537\_A8\_N\*sub1  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:40 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last Ical File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d  
 Column 1 : Det: EXP1  
 Process Host: XAWRK008

First Level Reviewer: barnettj Date: 20-Sep-2017 13:29:15

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.404	1.402	0.002	1.000	21814395	133.8		5029	
298.90 > 99.00	1.404	1.402	0.002	1.000	16334817		1.34(0.00-0.00)	5515	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.525	1.524	0.001	1.000	2392461	10.0		8065	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.669	1.668	0.001	1.000	13406173	44.1		5377	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.669	1.668	0.001	1.000	2879520	15.0		716	
* 6 13C2-PFOA									
415.00 > 370.00	1.851	1.855	-0.004		2036337	10.0		7634	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.851	1.856	-0.005	1.000	5625754	30.0		197	
413.00 > 169.00	1.851	1.856	-0.005	1.000	3000908		1.87(0.00-0.00)	6318	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.102	2.094	0.008	1.000	10734107	62.1		6191	M
499.00 > 99.00	2.102	2.094	0.008	1.000	2235008		4.80(0.00-0.00)	1485	M
* 7 13C4 PFOS									
503.00 > 80.00	2.102	2.108	-0.006		5320724	28.7		5650	
9 Perfluorononanoic acid									
463.00 > 419.00	2.109	2.116	-0.007	1.000	3814151	30.1		450	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.276	2.282	-0.006	1.000	1120086	9.86		8867	

**QC Flag Legend**

Review Flags

M - Manually Integrated

**Reagents:**

LC537-L5\_00024

Amount Added: 1.00

Units: mL

TestAmerica Sacramento  
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_021.d  
 Lims ID: CCV L5  
 Client ID:  
 Sample Type: CCVIS  
 Inject. Date: 20-Sep-2017 05:23:10 ALS Bottle#: 5 Worklist Smp#: 21  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: CCV L5  
 Misc. Info.: Plate: 1 Rack: 1  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Sublist: chrom-537\_A8\_N\*sub1  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:40 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d  
 Column 1 : Det: EXP1  
 Process Host: XAWRK008

First Level Reviewer: barnettj Date: 20-Sep-2017 13:29:15

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.404	1.402	0.002	1.000	21814395	133.8		5029	
298.90 > 99.00	1.404	1.402	0.002	1.000	16334817		1.34(0.00-0.00)	5515	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.525	1.524	0.001	1.000	2392461	10.0		8065	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.669	1.668	0.001	1.000	13406173	44.1		5377	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.669	1.668	0.001	1.000	2879520	15.0		716	
* 6 13C2-PFOA									
415.00 > 370.00	1.851	1.855	-0.004		2036337	10.0		7634	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.851	1.856	-0.005	1.000	5625754	30.0		197	
413.00 > 169.00	1.851	1.856	-0.005	1.000	3000908		1.87(0.00-0.00)	6318	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.102	2.094	0.008	1.000	10734107	62.1		6191	M
499.00 > 99.00	2.102	2.094	0.008	1.000	2235008		4.80(0.00-0.00)	1485	M
* 7 13C4 PFOS									
503.00 > 80.00	2.102	2.108	-0.006		5320724	28.7		5650	
9 Perfluorononanoic acid									
463.00 > 419.00	2.109	2.116	-0.007	1.000	3814151	30.1		450	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.276	2.282	-0.006	1.000	1120086	9.86		8867	

**QC Flag Legend**

Review Flags

M - Manually Integrated

**Reagents:**

LC537-L5\_00024

Amount Added: 1.00

Units: mL



TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_021.d

Injection Date: 20-Sep-2017 05:23:10

Instrument ID: A8\_N

Lims ID: CCV L5

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 5

Worklist Smp#: 21

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537\_A8\_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




\* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

\* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_021.d

Injection Date: 20-Sep-2017 05:23:10

Instrument ID: A8\_N

Lims ID: CCV L5

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 5

Worklist Smp#: 21

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537\_A8\_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




\* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

\* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_021.d  
Injection Date: 20-Sep-2017 05:23:10 Instrument ID: A8\_N  
Lims ID: CCV L5  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 5 Worklist Smp#: 21  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.10  
Area: 10734107  
Amount: 62.100937  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 13:27:35  
Audit Action: Assigned Compound ID

Audit Reason: Missed Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_021.d  
Injection Date: 20-Sep-2017 05:23:10 Instrument ID: A8\_N  
Lims ID: CCV L5  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 5 Worklist Smp#: 21  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected  
Expected RT: 2.09

Processing Integration Results



RT: 2.10  
Area: 2235008  
Amount: 62.100937  
Amount Units: ng/ml

Manual Integration Results



Reviewer: barnettj, 20-Sep-2017 13:27:56

Audit Action: Manually Integrated

Audit Reason: Missed Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_021.d  
Injection Date: 20-Sep-2017 05:23:10 Instrument ID: A8\_N  
Lims ID: CCV L5  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 5 Worklist Smp#: 21  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.09

Processing Integration Results



RT: 2.10  
Area: 10734107  
Amount: 62.100937  
Amount Units: ng/ml

Manual Integration Results



Reviewer: barnettj, 20-Sep-2017 13:27:56

Audit Action: Manually Integrated

Audit Reason: Missed Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_021.d  
Injection Date: 20-Sep-2017 05:23:10 Instrument ID: A8\_N  
Lims ID: CCV L5  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 5 Worklist Smp#: 21  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1


Signal: 1

Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results



RT: 2.10  
Area: 10734107  
Amount: 62.100937  
Amount Units: ng/ml



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_021.d  
Injection Date: 20-Sep-2017 05:23:10 Instrument ID: A8\_N  
Lims ID: CCV L5  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 5 Worklist Smp#: 21  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.10  
Area: 2235008  
Amount: 62.100937  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 13:27:56

Audit Action: Manually Integrated

Audit Reason: Missed Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_021.d  
Injection Date: 20-Sep-2017 05:23:10 Instrument ID: A8\_N  
Lims ID: CCV L5  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 5 Worklist Smp#: 21  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.09

Processing Integration Results



RT: 2.10  
Area: 10734107  
Amount: 62.100937  
Amount Units: ng/ml

Manual Integration Results



Reviewer: barnettj, 20-Sep-2017 13:27:56

Audit Action: Manually Integrated

Audit Reason: Missed Peak

FORM VII  
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Lab Sample ID: CCV 320-185408/33 Calibration Date: 09/20/2017 06:20  
 Instrument ID: A8\_N Calib Start Date: 09/20/2017 02:56  
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 09/20/2017 03:19  
 Lab File ID: 2017.09.19\_537A\_033.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		1.118		45.8	45.0	1.8	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9418	0.9457		5.02	5.00	0.4	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.638	1.760		16.1	15.0	7.4	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9195	0.8821		9.60	10.0	-4.1	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9317	0.9386		20.2	20.0	0.7	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6218	0.6156		9.90	10.0	-1.0	30.0
13C2 PFHxA	Ave	1.172	1.175		10.0	10.0	0.3	30.0
13C2 PFDA	Ave	0.5578	0.5469		9.81	10.0	-1.9	30.0

FORM VII  
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Lab Sample ID: CCV 320-185409/33 Calibration Date: 09/20/2017 06:20  
 Instrument ID: A8\_N Calib Start Date: 09/20/2017 02:56  
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 09/20/2017 03:19  
 Lab File ID: 2017.09.19\_537A\_033.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		1.118		45.8	45.0	1.8	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9418	0.9457		5.02	5.00	0.4	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.638	1.760		16.1	15.0	7.4	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9195	0.8821		9.60	10.0	-4.1	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9317	0.9386		20.2	20.0	0.7	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6218	0.6156		9.90	10.0	-1.0	30.0
13C2 PFHxA	Ave	1.172	1.175		10.0	10.0	0.3	30.0
13C2 PFDA	Ave	0.5578	0.5469		9.81	10.0	-1.9	30.0

TestAmerica Sacramento  
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_033.d  
 Lims ID: CCV L3  
 Client ID:  
 Sample Type: CCVIS  
 Inject. Date: 20-Sep-2017 06:20:06 ALS Bottle#: 3 Worklist Smp#: 33  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: CCV L3  
 Misc. Info.: Plate: 1 Rack: 1  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Sublist: chrom-537\_A8\_N\*sub1  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:04:03 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d  
 Column 1 : Det: EXP1  
 Process Host: XAWRK008

First Level Reviewer: barnettj Date: 20-Sep-2017 13:29:34

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.396	1.402	-0.006	1.000	9834882	45.8		5462	
298.90 > 99.00	1.396	1.402	-0.006	1.000	7111289		1.38(0.00-0.00)	5098	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.517	1.524	-0.007	1.000	2576920	10.0		7756	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.654	1.668	-0.014	1.000	5160786	16.1		4495	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.654	1.668	-0.014	1.000	1036861	5.02		264	
* 6 13C2-PFOA									
415.00 > 370.00	1.836	1.855	-0.019		2192291	10.0		6757	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.844	1.856	-0.012	1.000	1935350	9.60		69.6	
413.00 > 169.00	1.844	1.856	-0.012	1.000	1039881		1.86(0.00-0.00)	3456	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.094	2.094	0.0	1.000	3669732	20.2		3098	
499.00 > 99.00	2.086	2.094	-0.008	0.996	749613		4.90(0.00-0.00)	568	
* 7 13C4 PFOS									
503.00 > 80.00	2.086	2.108	-0.022		5605406	28.7		3887	
9 Perfluorononanoic acid									
463.00 > 419.00	2.102	2.116	-0.014	1.000	1349736	9.90		138	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.269	2.282	-0.014	1.000	1199046	9.81		8373	

Reagents:

LC537-L3\_00023

Amount Added: 1.00

Units: mL

TestAmerica Sacramento  
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_033.d  
 Lims ID: CCV L3  
 Client ID:  
 Sample Type: CCVIS  
 Inject. Date: 20-Sep-2017 06:20:06 ALS Bottle#: 3 Worklist Smp#: 33  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: CCV L3  
 Misc. Info.: Plate: 1 Rack: 1  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Sublist: chrom-537\_A8\_N\*sub1  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:04:03 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d  
 Column 1 : Det: EXP1  
 Process Host: XAWRK008

First Level Reviewer: barnettj Date: 20-Sep-2017 13:29:34

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.396	1.402	-0.006	1.000	9834882	45.8		5462	
298.90 > 99.00	1.396	1.402	-0.006	1.000	7111289		1.38(0.00-0.00)	5098	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.517	1.524	-0.007	1.000	2576920	10.0		7756	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.654	1.668	-0.014	1.000	5160786	16.1		4495	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.654	1.668	-0.014	1.000	1036861	5.02		264	
* 6 13C2-PFOA									
415.00 > 370.00	1.836	1.855	-0.019		2192291	10.0		6757	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.844	1.856	-0.012	1.000	1935350	9.60		69.6	
413.00 > 169.00	1.844	1.856	-0.012	1.000	1039881		1.86(0.00-0.00)	3456	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.094	2.094	0.0	1.000	3669732	20.2		3098	
499.00 > 99.00	2.086	2.094	-0.008	0.996	749613		4.90(0.00-0.00)	568	
* 7 13C4 PFOS									
503.00 > 80.00	2.086	2.108	-0.022		5605406	28.7		3887	
9 Perfluorononanoic acid									
463.00 > 419.00	2.102	2.116	-0.014	1.000	1349736	9.90		138	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.269	2.282	-0.014	1.000	1199046	9.81		8373	

**Reagents:**

LC537-L3\_00023

Amount Added: 1.00

Units: mL



TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_033.d

Injection Date: 20-Sep-2017 06:20:06

Instrument ID: A8\_N

Lims ID: CCV L3

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 3

Worklist Smp#: 33

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537\_A8\_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




\* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid




8 Perfluorooctane sulfonic acid

\* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_033.d

Injection Date: 20-Sep-2017 06:20:06

Instrument ID: A8\_N

Lims ID: CCV L3

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 3

Worklist Smp#: 33

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537\_A8\_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




\* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid




8 Perfluorooctane sulfonic acid

\* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



FORM VII  
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Lab Sample ID: CCV 320-185409/38 Calibration Date: 09/20/2017 06:43  
 Instrument ID: A8\_N Calib Start Date: 09/20/2017 02:56  
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 09/20/2017 03:19  
 Lab File ID: 2017.09.19\_537A\_038.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		0.8765		135	135	0.1	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9418	0.8948		14.3	15.0	-5.0	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.638	1.596		43.9	45.0	-2.6	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9195	0.8826		28.8	30.0	-4.0	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9317	0.9548		61.5	60.0	2.5	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6218	0.5935		28.6	30.0	-4.6	30.0
13C2 PFHxA	Ave	1.172	1.209		10.3	10.0	3.2	30.0
13C2 PFDA	Ave	0.5578	0.5368		9.62	10.0	-3.8	30.0

TestAmerica Sacramento  
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_038.d  
 Lims ID: CCV L5  
 Client ID:  
 Sample Type: CCVIS  
 Inject. Date: 20-Sep-2017 06:43:50 ALS Bottle#: 5 Worklist Smp#: 38  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: CCV L5  
 Misc. Info.: Plate: 1 Rack: 1  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Sublist: chrom-537\_A8\_N\*sub1  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:04:14 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d  
 Column 1 : Det: EXP1  
 Process Host: XAWRK008

First Level Reviewer: barnettj Date: 20-Sep-2017 13:35:45

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.396	1.402	-0.006	1.000	22232213	135.2		5349	
298.90 > 99.00	1.396	1.402	-0.006	1.000	16661218		1.33(0.00-0.00)	5354	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.517	1.524	-0.007	1.000	2583322	10.3		8977	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.662	1.668	-0.006	1.000	13497139	43.9		5454	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.662	1.668	-0.006	1.000	2869181	14.3		737	
* 6 13C2-PFOA									
415.00 > 370.00	1.844	1.855	-0.011		2137164	10.0		6904	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.844	1.856	-0.012	1.000	5663334	28.8		195	
413.00 > 169.00	1.844	1.856	-0.012	1.000	3095220		1.83(0.00-0.00)	6277	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.094	2.094	0.0	1.000	10765898	61.5		5899	M
499.00 > 99.00	2.094	2.094	0.0	1.000	2244815		4.80(0.00-0.00)	1522	M
* 7 13C4 PFOS									
503.00 > 80.00	2.094	2.108	-0.014		5388320	28.7		4770	
9 Perfluorononanoic acid									
463.00 > 419.00	2.102	2.116	-0.014	1.000	3805767	28.6		458	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.269	2.282	-0.014	1.000	1147213	9.62		9670	

**QC Flag Legend**

Review Flags

M - Manually Integrated

**Reagents:**

LC537-L5\_00024




Amount Added: 1.00

Units: mL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




\* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)



8 Perfluorooctane sulfonic acid (M)


\* 7 13C4 PFOS

9 Perfluorononanoic acid





\$ 10 13C2 PFDA



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_038.d  
Injection Date: 20-Sep-2017 06:43:50 Instrument ID: A8\_N  
Lims ID: CCV L5  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 5 Worklist Smp#: 38  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1


Signal: 1

Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results



RT: 2.09  
Area: 10765898  
Amount: 61.503502  
Amount Units: ng/ml

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_038.d  
Injection Date: 20-Sep-2017 06:43:50 Instrument ID: A8\_N  
Lims ID: CCV L5  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 5 Worklist Smp#: 38  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.09  
Area: 2244815  
Amount: 61.503502  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 13:35:38

Audit Action: Manually Integrated

Audit Reason: Missed Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_038.d  
Injection Date: 20-Sep-2017 06:43:50 Instrument ID: A8\_N  
Lims ID: CCV L5  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 5 Worklist Smp#: 38  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.09

Processing Integration Results



RT: 2.09  
Area: 10765898  
Amount: 61.503502  
Amount Units: ng/ml

Manual Integration Results



Reviewer: barnettj, 20-Sep-2017 13:35:38

Audit Action: Manually Integrated

Audit Reason: Missed Peak

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: \_\_\_\_\_ Lab Sample ID: MB 320-184382/1-A  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_011.d  
 Analysis Method: 537 Date Collected: \_\_\_\_\_  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 250 (mL) Date Analyzed: 09/20/2017 04:35  
 Con. Extract Vol.: 1.0 (mL) Dilution Factor: 1  
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185407 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	8.0	U	20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.0	U	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	90		70-130
STL00996	13C2 PFDA	111		70-130

TestAmerica Sacramento  
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_011.d  
 Lims ID: MB 320-184382/1-A  
 Client ID:  
 Sample Type: MB  
 Inject. Date: 20-Sep-2017 04:35:41 ALS Bottle#: 7 Worklist Smp#: 11  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: mb 320-184382/1-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:27 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d

Column 1 : Det: EXP1  
 Process Host: XAWRK008

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
\$ 2 13C2 PFHxA	315.00 > 270.00	1.517	1.524	-0.007	1.000	2529619	8.98	9517	
* 6 13C2-PFOA	415.00 > 370.00	1.851	1.855	-0.004		2402894	10.0	7956	
* 7 13C4 PFOS	503.00 > 80.00	2.102	2.108	-0.006		5785526	28.7	5282	
\$ 10 13C2 PFDA	515.00 > 470.00	2.276	2.282	-0.006	1.000	1483741	11.1	15054	

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_011.d

Injection Date: 20-Sep-2017 04:35:41

Instrument ID: A8\_N

Lims ID: MB 320-184382/1-A

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 7

Worklist Smp#: 11

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537\_A8\_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid (ND)

1 Perfluorobutanesulfonic acid (ND)




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid (ND)

4 Perfluoroheptanoic acid (ND)




\* 6 13C2-PFOA



5 Perfluorooctanoic acid (ND)

5 Perfluorooctanoic acid (ND)




8 Perfluorooctane sulfonic acid (ND)




8 Perfluorooctane sulfonic acid (ND)

\* 7 13C4 PFOS

9 Perfluorononanoic acid (ND)



\$ 10 13C2 PFDA





TestAmerica Sacramento  
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_011.d  
 Lims ID: MB 320-184382/1-A  
 Client ID:  
 Sample Type: MB  
 Inject. Date: 20-Sep-2017 04:35:41 ALS Bottle#: 7 Worklist Smp#: 11  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: mb 320-184382/1-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:27 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d

Column 1 : Det: EXP1  
 Process Host: XAWRK008

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	8.98	89.84
\$ 10 13C2 PFDA	10.0	11.1	110.70

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: \_\_\_\_\_ Lab Sample ID: MB 320-184385/1-A  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_003.d  
 Analysis Method: 537 Date Collected: \_\_\_\_\_  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:29  
 Sample wt/vol: 250 (mL) Date Analyzed: 09/20/2017 03:57  
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1  
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185406 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	8.0	U	20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.0	U	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	87		70-130
STL00996	13C2 PFDA	143	Q	70-130

TestAmerica Sacramento  
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_003.d  
 Lims ID: MB 320-184385/1-A  
 Client ID:  
 Sample Type: MB  
 Inject. Date: 20-Sep-2017 03:57:43 ALS Bottle#: 1 Worklist Smp#: 3  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: mb 320-184385/1-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:15 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d

Column 1 : Det: EXP1  
 Process Host: XAWRK008

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
\$ 2 13C2 PFHxA	315.00 > 270.00	1.525	1.524	0.001	1.000	2581279	8.68	9673	
* 6 13C2-PFOA	415.00 > 370.00	1.851	1.855	-0.004		2539018	10.0	10228	
* 7 13C4 PFOS	503.00 > 80.00	2.102	2.108	-0.006		6194895	28.7	1245	
\$ 10 13C2 PFDA	515.00 > 470.00	2.276	2.282	-0.006	1.000	2031171	14.3	15568	

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_003.d

Injection Date: 20-Sep-2017 03:57:43

Instrument ID: A8\_N

Lims ID: MB 320-184385/1-A

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 1

Worklist Smp#: 3

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537\_A8\_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid (ND)

1 Perfluorobutanesulfonic acid (ND)




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid (ND)

4 Perfluoroheptanoic acid (ND)




\* 6 13C2-PFOA



5 Perfluorooctanoic acid (ND)

5 Perfluorooctanoic acid (ND)




8 Perfluorooctane sulfonic acid (ND)




8 Perfluorooctane sulfonic acid (ND)

\* 7 13C4 PFOS

9 Perfluorononanoic acid (ND)



\$ 10 13C2 PFDA



TestAmerica Sacramento  
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_003.d  
 Lims ID: MB 320-184385/1-A  
 Client ID:  
 Sample Type: MB  
 Inject. Date: 20-Sep-2017 03:57:43 ALS Bottle#: 1 Worklist Smp#: 3  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: mb 320-184385/1-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:15 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d

Column 1 : Det: EXP1  
 Process Host: XAWRK008

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	8.68	86.76
\$ 10 13C2 PFDA	10.0	14.3	143.42

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: \_\_\_\_\_ Lab Sample ID: LCS 320-184382/2-A  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_012.d  
 Analysis Method: 537 Date Collected: \_\_\_\_\_  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 250 (mL) Date Analyzed: 09/20/2017 04:40  
 Con. Extract Vol.: 1.0 (mL) Dilution Factor: 1  
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185407 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	198	M	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	103		20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	99.7		24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	150		30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	50.5		10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	408		90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	91		70-130
STL00996	13C2 PFDA	115		70-130

TestAmerica Sacramento  
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_012.d  
 Lims ID: LCS 320-184382/2-A  
 Client ID:  
 Sample Type: LCS  
 Inject. Date: 20-Sep-2017 04:40:25 ALS Bottle#: 8 Worklist Smp#: 12  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: lcs 320-184382/2-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:27 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d  
 Column 1 : Det: EXP1  
 Process Host: XAWRK008

First Level Reviewer: barnettj Date: 20-Sep-2017 13:23:08

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.396	1.402	-0.006	1.000	19434859	102.0		5516	
298.90 > 99.00	1.396	1.402	-0.006	1.000	14542305		1.34(0.00-0.00)	5620	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.517	1.524	-0.007	1.000	2316253	9.06		7239	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.662	1.668	-0.006	1.000	12226141	37.5		5745	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.662	1.668	-0.006	1.000	2591545	12.6		674	
* 6 13C2-PFOA									
415.00 > 370.00	1.844	1.855	-0.011		2181509	10.0		6687	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.844	1.856	-0.012	1.000	5187286	25.9		231	
413.00 > 169.00	1.844	1.856	-0.012	1.000	2697593		1.92(0.00-0.00)	5632	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.094	2.094	0.0	1.000	9183709	49.6		7671	M
499.00 > 99.00	2.094	2.094	0.0	1.000	1906144		4.82(0.00-0.00)	1302	M
* 7 13C4 PFOS									
503.00 > 80.00	2.094	2.108	-0.014		5704391	28.7		4962	
9 Perfluorononanoic acid									
463.00 > 419.00	2.109	2.116	-0.007	1.000	3381160	24.9		150	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.276	2.282	-0.006	1.000	1393646	11.5		12330	



## QC Flag Legend




Review Flags

M - Manually Integrated

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




\* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

\* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento  
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_012.d  
 Lims ID: LCS 320-184382/2-A  
 Client ID:  
 Sample Type: LCS  
 Inject. Date: 20-Sep-2017 04:40:25 ALS Bottle#: 8 Worklist Smp#: 12  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: lcs 320-184382/2-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:27 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d  
 Column 1 : Det: EXP1  
 Process Host: XAWRK008

First Level Reviewer: barnettj Date: 20-Sep-2017 13:23:08

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	9.06	90.61
\$ 10 13C2 PFDA	10.0	11.5	114.54

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_012.d  
Injection Date: 20-Sep-2017 04:40:25 Instrument ID: A8\_N  
Lims ID: LCS 320-184382/2-A  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 8 Worklist Smp#: 12  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.09  
Area: 9183709  
Amount: 49.557774  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 13:22:15  
Audit Action: Assigned Compound ID

Audit Reason: Missed Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_012.d  
Injection Date: 20-Sep-2017 04:40:25 Instrument ID: A8\_N  
Lims ID: LCS 320-184382/2-A  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 8 Worklist Smp#: 12  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.09  
Area: 1906144  
Amount: 49.557774  
Amount Units: ng/ml



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_012.d  
Injection Date: 20-Sep-2017 04:40:25 Instrument ID: A8\_N  
Lims ID: LCS 320-184382/2-A  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 8 Worklist Smp#: 12  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.09  
Area: 9183709  
Amount: 49.557774  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 13:22:42

Audit Action: Manually Integrated

Audit Reason: Missed Peak

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: \_\_\_\_\_ Lab Sample ID: LCSD 320-184382/3-A  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_013.d  
 Analysis Method: 537 Date Collected: \_\_\_\_\_  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 250 (mL) Date Analyzed: 09/20/2017 04:45  
 Con. Extract Vol.: 1.0 (mL) Dilution Factor: 1  
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185407 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	188	M	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	96.8		20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	93.6		24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	143		30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	48.7		10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	403		90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	86		70-130
STL00996	13C2 PFDA	110		70-130



TestAmerica Sacramento  
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_013.d  
 Lims ID: LCSD 320-184382/3-A  
 Client ID:  
 Sample Type: LCSD  
 Inject. Date: 20-Sep-2017 04:45:09 ALS Bottle#: 9 Worklist Smp#: 13  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: lcsd 320-184382/3-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:27 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d  
 Column 1 : Det: EXP1  
 Process Host: XAWRK008

First Level Reviewer: barnettj Date: 20-Sep-2017 13:23:56

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.404	1.402	0.002	1.000	19788378	100.8		5456	
298.90 > 99.00	1.396	1.402	-0.006	0.995	14893459		1.33(0.00-0.00)	5463	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.517	1.524	-0.007	1.000	2340027	8.56		8090	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.662	1.668	-0.006	1.000	11991969	35.9		5992	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.662	1.668	-0.006	1.000	2675370	12.2		721	
* 6 13C2-PFOA									
415.00 > 370.00	1.851	1.855	-0.004		2332217	10.0		8234	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.851	1.856	-0.005	1.000	5187121	24.2		244	
413.00 > 169.00	1.851	1.856	-0.005	1.000	2753051		1.88(0.00-0.00)	6050	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.102	2.094	0.008	1.000	8927546	46.9		7277	M
499.00 > 99.00	2.102	2.094	0.008	1.000	1856917		4.81(0.00-0.00)	1363	M
* 7 13C4 PFOS									
503.00 > 80.00	2.102	2.108	-0.006		5855728	28.7		5973	
9 Perfluorononanoic acid									
463.00 > 419.00	2.109	2.116	-0.007	1.000	3392058	23.4		140	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.276	2.282	-0.006	1.000	1426596	11.0		11069	

## QC Flag Legend

Review Flags

M - Manually Integrated

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_013.d

Injection Date: 20-Sep-2017 04:45:09

Instrument ID: A8\_N

Lims ID: LCSD 320-184382/3-A

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 9

Worklist Smp#: 13

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537\_A8\_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




\* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

\* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento  
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_013.d  
 Lims ID: LCSD 320-184382/3-A  
 Client ID:  
 Sample Type: LCSD  
 Inject. Date: 20-Sep-2017 04:45:09 ALS Bottle#: 9 Worklist Smp#: 13  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: lcsd 320-184382/3-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:27 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d  
 Column 1 : Det: EXP1  
 Process Host: XAWRK008

First Level Reviewer: barnettj Date: 20-Sep-2017 13:23:56

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	8.56	85.63
\$ 10 13C2 PFDA	10.0	11.0	109.67

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_013.d  
Injection Date: 20-Sep-2017 04:45:09 Instrument ID: A8\_N  
Lims ID: LCSD 320-184382/3-A  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 9 Worklist Smp#: 13  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.10  
Area: 8927546  
Amount: 46.930390  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 13:23:18  
Audit Action: Assigned Compound ID

Audit Reason: Missed Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_013.d  
Injection Date: 20-Sep-2017 04:45:09 Instrument ID: A8\_N  
Lims ID: LCSD 320-184382/3-A  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 9 Worklist Smp#: 13  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.10  
Area: 1856917  
Amount: 46.930390  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 13:23:34

Audit Action: Manually Integrated

Audit Reason: Missed Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_013.d  
Injection Date: 20-Sep-2017 04:45:09 Instrument ID: A8\_N  
Lims ID: LCSD 320-184382/3-A  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 9 Worklist Smp#: 13  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.10  
Area: 8927546  
Amount: 46.930390  
Amount Units: ng/ml





FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: \_\_\_\_\_ Lab Sample ID: LLCS 320-184385/2-A  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_004.d  
 Analysis Method: 537 Date Collected: \_\_\_\_\_  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:29  
 Sample wt/vol: 250 (mL) Date Analyzed: 09/20/2017 04:02  
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1  
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185406 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	36.6	J M	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	18.4	J	20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	18.5	J	24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	28.9	J	30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	10.2		10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	86.1	J	90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	90		70-130
STL00996	13C2 PFDA	113		70-130

TestAmerica Sacramento  
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_004.d  
 Lims ID: LLCS 320-184385/2-A  
 Client ID:  
 Sample Type: LLCS  
 Inject. Date: 20-Sep-2017 04:02:28 ALS Bottle#: 2 Worklist Smp#: 4  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: llcs 320-184385/2-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:15 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d  
 Column 1 : Det: EXP1  
 Process Host: XAWRK008

First Level Reviewer: barnettj Date: 20-Sep-2017 11:39:54

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.396	1.402	-0.006	1.000	4920070	21.5		5963	
298.90 > 99.00	1.396	1.402	-0.006	1.000	3493700		1.41(0.00-0.00)	3416	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.517	1.524	-0.007	1.000	2444028	8.98		7563	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.662	1.668	-0.006	1.000	2334552	7.23		3934	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.662	1.668	-0.006	1.000	555411	2.54		148	
* 6 13C2-PFOA									
415.00 > 370.00	1.851	1.855	-0.004		2322795	10.0		7571	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.851	1.856	-0.005	1.000	983366	4.60		48.8	
413.00 > 169.00	1.851	1.856	-0.005	1.000	501816		1.96(0.00-0.00)	1668	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.102	2.094	0.008	1.000	1679680	9.14		1224	M
499.00 > 99.00	2.102	2.094	0.008	1.000	358008		4.69(0.00-0.00)	285	M
* 7 13C4 PFOS									
503.00 > 80.00	2.102	2.108	-0.006		5655681	28.7		5134	
9 Perfluorononanoic acid									
463.00 > 419.00	2.109	2.116	-0.007	1.000	669429	4.63		14.6	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.276	2.282	-0.006	1.000	1458473	11.3		13717	

## QC Flag Legend

Review Flags

M - Manually Integrated

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_004.d

Injection Date: 20-Sep-2017 04:02:28

Instrument ID: A8\_N

Lims ID: LLCS 320-184385/2-A

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 2

Worklist Smp#: 4

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537\_A8\_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




\* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

\* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento  
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_004.d  
 Lims ID: LLCS 320-184385/2-A  
 Client ID:  
 Sample Type: LLCS  
 Inject. Date: 20-Sep-2017 04:02:28 ALS Bottle#: 2 Worklist Smp#: 4  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: llcs 320-184385/2-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:15 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d  
 Column 1 : Det: EXP1  
 Process Host: XAWRK008

First Level Reviewer: barnettj Date: 20-Sep-2017 11:39:54

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	8.98	89.80
\$ 10 13C2 PFDA	10.0	11.3	112.57

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_004.d  
Injection Date: 20-Sep-2017 04:02:28 Instrument ID: A8\_N  
Lims ID: LLCS 320-184385/2-A  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 2 Worklist Smp#: 4  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.09

Processing Integration Results



RT: 2.10  
Area: 1679680  
Amount: 9.142071  
Amount Units: ng/ml

Manual Integration Results



Reviewer: barnettj, 20-Sep-2017 11:39:20  
Audit Action: Assigned Compound ID

Audit Reason: Missed Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_004.d  
Injection Date: 20-Sep-2017 04:02:28 Instrument ID: A8\_N  
Lims ID: LLCS 320-184385/2-A  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 2 Worklist Smp#: 4  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.10  
Area: 358008  
Amount: 9.142071  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 11:39:36

Audit Action: Manually Integrated

Audit Reason: Missed Peak



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_004.d  
Injection Date: 20-Sep-2017 04:02:28 Instrument ID: A8\_N  
Lims ID: LLCS 320-184385/2-A  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 2 Worklist Smp#: 4  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.10  
Area: 1679680  
Amount: 9.142071  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 11:39:36

Audit Action: Manually Integrated

Audit Reason: Missed Peak

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: \_\_\_\_\_ Lab Sample ID: LLCSD 320-184385/3-A  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_005.d  
 Analysis Method: 537 Date Collected: \_\_\_\_\_  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:29  
 Sample wt/vol: 250 (mL) Date Analyzed: 09/20/2017 04:07  
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1  
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185406 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	36.2	J M	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	18.7	J	20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	19.0	J	24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	29.4	J	30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	10.8		10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	89.0	J	90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	93		70-130
STL00996	13C2 PFDA	124		70-130

TestAmerica Sacramento  
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_005.d  
 Lims ID: LLCSD 320-184385/3-A  
 Client ID:  
 Sample Type: LLCSD  
 Inject. Date: 20-Sep-2017 04:07:13 ALS Bottle#: 3 Worklist Smp#: 5  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: llcsd 320-184385/3-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:15 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d  
 Column 1 : Det: EXP1  
 Process Host: XAWRK008

First Level Reviewer: barnettj Date: 20-Sep-2017 11:40:48

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.396	1.402	-0.006	1.000	4940789	22.3		5684	
298.90 > 99.00	1.396	1.402	-0.006	1.000	3361171		1.47(0.00-0.00)	3312	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.517	1.524	-0.007	1.000	2376283	9.25		8068	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.662	1.668	-0.006	1.000	2307781	7.34		3660	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.662	1.668	-0.006	1.000	558601	2.71		156	
* 6 13C2-PFOA									
415.00 > 370.00	1.844	1.855	-0.011		2191521	10.0		7552	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.844	1.856	-0.012	1.000	940343	4.67		44.4	
413.00 > 169.00	1.844	1.856	-0.012	1.000	514934		1.83(0.00-0.00)	1806	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.102	2.094	0.008	1.000	1617344	9.05		800	M
499.00 > 99.00	2.094	2.094	0.0	0.996	344536		4.69(0.00-0.00)	279	M
* 7 13C4 PFOS									
503.00 > 80.00	2.094	2.108	-0.014		5502551	28.7		4491	
9 Perfluorononanoic acid									
463.00 > 419.00	2.109	2.116	-0.007	1.000	648339	4.76		15.3	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.269	2.282	-0.014	1.000	1511214	12.4		11405	

## QC Flag Legend

Review Flags

M - Manually Integrated

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_005.d

Injection Date: 20-Sep-2017 04:07:13

Instrument ID: A8\_N

Lims ID: LLCSD 320-184385/3-A

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 3

Worklist Smp#: 5

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537\_A8\_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




\* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

\* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento  
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_005.d  
 Lims ID: LLCSD 320-184385/3-A  
 Client ID:  
 Sample Type: LLCSD  
 Inject. Date: 20-Sep-2017 04:07:13 ALS Bottle#: 3 Worklist Smp#: 5  
 Injection Vol: 2.0 ul Dil. Factor: 1.0000  
 Sample Info: llcsd 320-184385/3-a  
 Misc. Info.: Plate: 1 Rack: 2  
 Operator ID: SACINSTLCMS01 Instrument ID: A8\_N  
 Method: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\537\_A8\_N.m  
 Limit Group: LC 537 ICAL  
 Last Update: 20-Sep-2017 14:03:15 Calib Date: 20-Sep-2017 03:19:48  
 Integrator: Picker  
 Quant Method: Internal Standard Quant By: Initial Calibration  
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8\_N\20170919-48154.b\2017.09.19\_537ICAL\_009.d  
 Column 1 : Det: EXP1  
 Process Host: XAWRK008

First Level Reviewer: barnettj Date: 20-Sep-2017 11:40:48

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	9.25	92.54
\$ 10 13C2 PFDA	10.0	12.4	123.63

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_005.d  
Injection Date: 20-Sep-2017 04:07:13 Instrument ID: A8\_N  
Lims ID: LLCSD 320-184385/3-A  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 3 Worklist Smp#: 5  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.10  
Area: 1617344  
Amount: 9.047765  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 11:40:01  
Audit Action: Assigned Compound ID

Audit Reason: Missed Peak



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_005.d  
Injection Date: 20-Sep-2017 04:07:13 Instrument ID: A8\_N  
Lims ID: LLCSD 320-184385/3-A  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 3 Worklist Smp#: 5  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.09  
Area: 344536  
Amount: 9.047765  
Amount Units: ng/ml



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b\2017.09.19\_537A\_005.d  
Injection Date: 20-Sep-2017 04:07:13 Instrument ID: A8\_N  
Lims ID: LLCSD 320-184385/3-A  
Client ID:  
Operator ID: SACINSTLCMS01 ALS Bottle#: 3 Worklist Smp#: 5  
Injection Vol: 2.0 ul Dil. Factor: 1.0000  
Method: 537\_A8\_N Limit Group: LC 537 ICAL  
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected  
Expected RT: 2.09

Processing Integration Results



Manual Integration Results

RT: 2.10  
Area: 1617344  
Amount: 9.047765  
Amount Units: ng/ml



Reviewer: barnettj, 20-Sep-2017 11:40:29

Audit Action: Manually Integrated

Audit Reason: Missed Peak

LCMS ANALYSIS RUN LOG

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1

SDG No.: \_\_\_\_\_

Instrument ID: A8\_N Start Date: 09/20/2017 02:56

Analysis Batch Number: 185329 End Date: 09/20/2017 03:38

LAB SAMPLE ID	CLIENT SAMPLE ID	DATE ANALYZED	DILUTION FACTOR	LAB FILE ID	COLUMN ID
IC 320-185329/4		09/20/2017 02:56	1	2017.09.19_537I CAL 004.d	GeminiC18 3x100 3(mm)
IC 320-185329/5		09/20/2017 03:00	1	2017.09.19_537I CAL 005.d	GeminiC18 3x100 3(mm)
IC 320-185329/6		09/20/2017 03:05	1	2017.09.19_537I CAL 006.d	GeminiC18 3x100 3(mm)
IC 320-185329/7 ICISAV		09/20/2017 03:10	1	2017.09.19_537I CAL 007.d	GeminiC18 3x100 3(mm)
IC 320-185329/8		09/20/2017 03:15	1	2017.09.19_537I CAL 008.d	GeminiC18 3x100 3(mm)
IC 320-185329/9		09/20/2017 03:19	1	2017.09.19_537I CAL 009.d	GeminiC18 3x100 3(mm)
ZZZZZ		09/20/2017 03:24	1		GeminiC18 3x100 3(mm)
CCVL 320-185329/11		09/20/2017 03:29	1	2017.09.19_537I CAL 011.d	GeminiC18 3x100 3(mm)
ZZZZZ		09/20/2017 03:34	1		GeminiC18 3x100 3(mm)
ICV 320-185329/13		09/20/2017 03:38	1	2017.09.19_537I CAL 013.d	GeminiC18 3x100 3(mm)

LCMS ANALYSIS RUN LOG

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1

SDG No.: \_\_\_\_\_

Instrument ID: A8\_N Start Date: 09/20/2017 03:48

Analysis Batch Number: 185406 End Date: 09/20/2017 04:26

LAB SAMPLE ID	CLIENT SAMPLE ID	DATE ANALYZED	DILUTION FACTOR	LAB FILE ID	COLUMN ID
CCV 320-185406/1 CCVIS		09/20/2017 03:48	1	2017.09.19_537A 001.d	GeminiC18 3x100 3(mm)
ZZZZZ		09/20/2017 03:52	1		GeminiC18 3x100 3(mm)
MB 320-184385/1-A		09/20/2017 03:57	1	2017.09.19_537A 003.d	GeminiC18 3x100 3(mm)
LLCS 320-184385/2-A		09/20/2017 04:02	1	2017.09.19_537A 004.d	GeminiC18 3x100 3(mm)
LLCSD 320-184385/3-A		09/20/2017 04:07	1	2017.09.19_537A 005.d	GeminiC18 3x100 3(mm)
320-31468-21		09/20/2017 04:11	1	2017.09.19_537A 006.d	GeminiC18 3x100 3(mm)
320-31468-22		09/20/2017 04:16	1	2017.09.19_537A 007.d	GeminiC18 3x100 3(mm)
320-31468-23		09/20/2017 04:21	1	2017.09.19_537A 008.d	GeminiC18 3x100 3(mm)
CCV 320-185406/9 CCVIS		09/20/2017 04:26	1	2017.09.19_537A 009.d	GeminiC18 3x100 3(mm)

LCMS ANALYSIS RUN LOG

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1

SDG No.: \_\_\_\_\_

Instrument ID: A8\_N Start Date: 09/20/2017 04:26

Analysis Batch Number: 185407 End Date: 09/20/2017 05:23

LAB SAMPLE ID	CLIENT SAMPLE ID	DATE ANALYZED	DILUTION FACTOR	LAB FILE ID	COLUMN ID
CCV 320-185407/9 CCVIS ZZZZZ		09/20/2017 04:26	1	2017.09.19_537A 009.d	GeminiC18 3x100 3(mm)
MB 320-184382/1-A		09/20/2017 04:35	1	2017.09.19_537A 011.d	GeminiC18 3x100 3(mm)
LCS 320-184382/2-A		09/20/2017 04:40	1	2017.09.19_537A 012.d	GeminiC18 3x100 3(mm)
LCSD 320-184382/3-A		09/20/2017 04:45	1	2017.09.19_537A 013.d	GeminiC18 3x100 3(mm)
320-31468-1		09/20/2017 04:49	1	2017.09.19_537A 014.d	GeminiC18 3x100 3(mm)
320-31468-2		09/20/2017 04:54	1	2017.09.19_537A 015.d	GeminiC18 3x100 3(mm)
320-31468-3		09/20/2017 04:59	1	2017.09.19_537A 016.d	GeminiC18 3x100 3(mm)
320-31468-4		09/20/2017 05:04	1	2017.09.19_537A 017.d	GeminiC18 3x100 3(mm)
320-31468-5		09/20/2017 05:08	1	2017.09.19_537A 018.d	GeminiC18 3x100 3(mm)
320-31468-6		09/20/2017 05:13	1	2017.09.19_537A 019.d	GeminiC18 3x100 3(mm)
320-31468-7		09/20/2017 05:18	1	2017.09.19_537A 020.d	GeminiC18 3x100 3(mm)
CCV 320-185407/21 CCVIS		09/20/2017 05:23	1	2017.09.19_537A 021.d	GeminiC18 3x100 3(mm)

LCMS ANALYSIS RUN LOG

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1

SDG No.: \_\_\_\_\_

Instrument ID: A8\_N Start Date: 09/20/2017 05:23

Analysis Batch Number: 185408 End Date: 09/20/2017 06:20

LAB SAMPLE ID	CLIENT SAMPLE ID	DATE ANALYZED	DILUTION FACTOR	LAB FILE ID	COLUMN ID
CCV 320-185408/21 CCVIS		09/20/2017 05:23	1	2017.09.19_537A 021.d	GeminiC18 3x100 3(mm)
ZZZZZ		09/20/2017 05:27	1		GeminiC18 3x100 3(mm)
320-31468-8		09/20/2017 05:32	1	2017.09.19_537A 023.d	GeminiC18 3x100 3(mm)
320-31468-9		09/20/2017 05:37	1	2017.09.19_537A 024.d	GeminiC18 3x100 3(mm)
320-31468-10		09/20/2017 05:42	1	2017.09.19_537A 025.d	GeminiC18 3x100 3(mm)
320-31468-11		09/20/2017 05:46	1	2017.09.19_537A 026.d	GeminiC18 3x100 3(mm)
320-31468-12		09/20/2017 05:51	1	2017.09.19_537A 027.d	GeminiC18 3x100 3(mm)
320-31468-13		09/20/2017 05:56	1	2017.09.19_537A 028.d	GeminiC18 3x100 3(mm)
320-31468-14		09/20/2017 06:01	1	2017.09.19_537A 029.d	GeminiC18 3x100 3(mm)
320-31468-15		09/20/2017 06:05	1	2017.09.19_537A 030.d	GeminiC18 3x100 3(mm)
320-31468-16		09/20/2017 06:10	1	2017.09.19_537A 031.d	GeminiC18 3x100 3(mm)
320-31468-17		09/20/2017 06:15	1	2017.09.19_537A 032.d	GeminiC18 3x100 3(mm)
CCV 320-185408/33 CCVIS		09/20/2017 06:20	1	2017.09.19_537A 033.d	GeminiC18 3x100 3(mm)

LCMS ANALYSIS RUN LOG

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1

SDG No.: \_\_\_\_\_

Instrument ID: A8\_N Start Date: 09/20/2017 06:20

Analysis Batch Number: 185409 End Date: 09/20/2017 06:43

LAB SAMPLE ID	CLIENT SAMPLE ID	DATE ANALYZED	DILUTION FACTOR	LAB FILE ID	COLUMN ID
CCV 320-185409/33 CCVIS		09/20/2017 06:20	1	2017.09.19_537A 033.d	GeminiC18 3x100 3(mm)
ZZZZZ		09/20/2017 06:24	1		GeminiC18 3x100 3(mm)
320-31468-18		09/20/2017 06:29	1	2017.09.19_537A 035.d	GeminiC18 3x100 3(mm)
320-31468-19		09/20/2017 06:34	1	2017.09.19_537A 036.d	GeminiC18 3x100 3(mm)
320-31468-20		09/20/2017 06:39	1	2017.09.19_537A 037.d	GeminiC18 3x100 3(mm)
CCV 320-185409/38 CCVIS		09/20/2017 06:43	1	2017.09.19_537A 038.d	GeminiC18 3x100 3(mm)

LCMS BATCH WORKSHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1

SDG No.: \_\_\_\_\_

Batch Number: 184382 Batch Start Date: 09/14/17 09:16 Batch Analyst: Sharifi, Nooshin

Batch Method: 537 Batch End Date: 09/18/17 16:50

Lab Sample ID	Client Sample ID	Method Chain	Basis	GrossWeight	TareWeight	InitialAmount	FinalAmount	ReceivedpH	LC537-HSP 00023
MB 320-184382/1		537, 537				250 mL	1.0 mL	7 SU	
LCS 320-184382/2		537, 537				250 mL	1.0 mL	7 SU	100 uL
LCSD 320-184382/3		537, 537				250 mL	1.0 mL	7 SU	100 uL
320-31468-A-1	NAWC-091117-RW-106	537, 537	T	279.32 g	26.60 g	252.7 mL	1.0 mL	7 SU	
320-31468-A-2	NAWC-091117-FRB-106	537, 537	T	286.63 g	27.74 g	258.9 mL	1.0 mL	7 SU	
320-31468-A-3	NAWC-091117-RW-060	537, 537	T	289.73 g	28.04 g	261.7 mL	1.0 mL	7 SU	
320-31468-A-4	NAWC-091117-FRB-060	537, 537	T	287.72 g	27.79 g	259.9 mL	1.0 mL	7 SU	
320-31468-A-5	NAWC-091117-RW-314	537, 537	T	290.32 g	27.61 g	262.7 mL	1.0 mL	7 SU	
320-31468-A-6	NAWC-091117-FRB-314	537, 537	T	293.04 g	27.48 g	265.6 mL	1.0 mL	7 SU	
320-31468-A-7	NAWC-091117-RW-258	537, 537	T	294.63 g	27.68 g	267 mL	1.0 mL	7 SU	
320-31468-A-8	NAWC-091117-FRB-258	537, 537	T	289.24 g	27.66 g	261.6 mL	1.0 mL	7 SU	
320-31468-A-9	NAWC-091117-RW-048	537, 537	T	291.43 g	27.53 g	263.9 mL	1.0 mL	7 SU	
320-31468-A-10	NAWC-091117-FRB-048	537, 537	T	294.51 g	27.81 g	266.7 mL	1.0 mL	7 SU	
320-31468-A-11	NAWC-091117-RW-145	537, 537	T	296.76 g	27.74 g	269 mL	1.0 mL	7 SU	
320-31468-A-12	NAWC-091117-FRB-145	537, 537	T	293.17 g	27.53 g	265.6 mL	1.0 mL	7 SU	
320-31468-A-13	NAWC-091117-RW-317	537, 537	T	291.04 g	27.35 g	263.7 mL	1.0 mL	7 SU	
320-31468-A-14	NAWC-091117-FRB-317	537, 537	T	281.96 g	27.52 g	254.4 mL	1.0 mL	7 SU	
320-31468-A-15	NAWC-091117-RW-319	537, 537	T	278.29 g	27.27 g	251 mL	1.0 mL	7 SU	
320-31468-A-16	NAWC-091117-FRB-319	537, 537	T	294.18 g	27.53 g	266.7 mL	1.0 mL	7 SU	
320-31468-A-17	NAWC-091117-RW-321	537, 537	T	289.71 g	27.73 g	262 mL	1.0 mL	7 SU	
320-31468-A-18	NAWC-091117-FRB-321	537, 537	T	291.10 g	27.64 g	263.5 mL	1.0 mL	7 SU	
320-31468-A-19	NAWC-091117-RW-010	537, 537	T	283.27 g	28.59 g	254.7 mL	1.0 mL	7 SU	

The pound sign (#) in the amount added field denotes that the reagent was used undiluted. All calculations are performed using the stated concentration for this reagent.



LCMS BATCH WORKSHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1

SDG No.: \_\_\_\_\_

Batch Number: 184382 Batch Start Date: 09/14/17 09:16 Batch Analyst: Sharifi, Nooshin

Batch Method: 537 Batch End Date: 09/18/17 16:50

Lab Sample ID	Client Sample ID	Method Chain	Basis	GrossWeight	TareWeight	InitialAmount	FinalAmount	ReceivedpH	LC537-HSP 00023
320-31468-A-20	NAWC-091117-FRB-010	537, 537	T	287.79 g	27.95 g	259.8 mL	1.0 mL	7 SU	

Lab Sample ID	Client Sample ID	Method Chain	Basis	LC537-IS 00047	LC537-SU 00048	AnalysisComment			
MB 320-184382/1		537, 537		100 uL	100 uL	CH ND			
LCS 320-184382/2		537, 537		100 uL	100 uL	CH ND			
LCSD 320-184382/3		537, 537		100 uL	100 uL	CH ND			
320-31468-A-1	NAWC-091117-RW-106	537, 537	T	100 uL	100 uL	CH ND			
320-31468-A-2	NAWC-091117-FRB-106	537, 537	T	100 uL	100 uL	CH ND			
320-31468-A-3	NAWC-091117-RW-060	537, 537	T	100 uL	100 uL	CH ND			
320-31468-A-4	NAWC-091117-FRB-060	537, 537	T	100 uL	100 uL	CH ND			
320-31468-A-5	NAWC-091117-RW-314	537, 537	T	100 uL	100 uL	CH ND			
320-31468-A-6	NAWC-091117-FRB-314	537, 537	T	100 uL	100 uL	CH ND			
320-31468-A-7	NAWC-091117-RW-258	537, 537	T	100 uL	100 uL	CH ND			
320-31468-A-8	NAWC-091117-FRB-258	537, 537	T	100 uL	100 uL	CH ND			
320-31468-A-9	NAWC-091117-RW-048	537, 537	T	100 uL	100 uL	CH ND			
320-31468-A-10	NAWC-091117-FRB-048	537, 537	T	100 uL	100 uL	CH ND			
320-31468-A-11	NAWC-091117-RW-145	537, 537	T	100 uL	100 uL	CH ND			
320-31468-A-12	NAWC-091117-FRB-145	537, 537	T	100 uL	100 uL	CH ND			
320-31468-A-13	NAWC-091117-RW-317	537, 537	T	100 uL	100 uL	CH ND			
320-31468-A-14	NAWC-091117-FRB-317	537, 537	T	100 uL	100 uL	CH ND			
320-31468-A-15	NAWC-091117-RW-319	537, 537	T	100 uL	100 uL	CH ND			
320-31468-A-16	NAWC-091117-FRB-319	537, 537	T	100 uL	100 uL	CH ND			

The pound sign (#) in the amount added field denotes that the reagent was used undiluted. All calculations are performed using the stated concentration for this reagent.

LCMS BATCH WORKSHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1

SDG No.: \_\_\_\_\_

Batch Number: 184382 Batch Start Date: 09/14/17 09:16 Batch Analyst: Sharifi, Nooshin

Batch Method: 537 Batch End Date: 09/18/17 16:50

Lab Sample ID	Client Sample ID	Method Chain	Basis	LC537-IS 00047	LC537-SU 00048	AnalysisComment			
320-31468-A-17	NAWC-091117-RW-321	537, 537	T	100 uL	100 uL	CH ND			
320-31468-A-18	NAWC-091117-FRB-321	537, 537	T	100 uL	100 uL	CH ND			
320-31468-A-19	NAWC-091117-RW-010	537, 537	T	100 uL	100 uL	CH ND			
320-31468-A-20	NAWC-091117-FRB-010	537, 537	T	100 uL	100 uL	CH ND			

Batch Notes	
Batch Comment	IS: 1002957 BD: CCB FV: VPM AL:VPM
Manifold ID	1,3
Methanol ID	1021237
Pipette ID	H14930F
Analyst ID - IS Reagent Drop	VPM
Analyst ID - IS Reagent Drop Witness	TWL
Analyst ID - SU Reagent Drop	NSH
Analyst ID - SU Reagent Drop Witness	AAR
Analyst ID - TA Reagent Drop	NSH
Analyst ID - TA Reagent Drop Witness	AAR
SPE Cartridge ID	6357081-05
Trizma ID	SLBR4303V
Reagent Water ID	9/13/17

Basis	Basis Description
T	Total/NA

The pound sign (#) in the amount added field denotes that the reagent was used undiluted. All calculations are performed using the stated concentration for this reagent.

LCMS BATCH WORKSHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1

SDG No.: \_\_\_\_\_

Batch Number: 184385 Batch Start Date: 09/14/17 09:29 Batch Analyst: Branscum, Cassie

Batch Method: 537 Batch End Date: 09/15/17 14:40

Lab Sample ID	Client Sample ID	Method Chain	Basis	GrossWeight	TareWeight	InitialAmount	FinalAmount	ReceivedpH	LC537-IS 00047
MB 320-184385/1		537, 537				250 mL	1.00 mL	7 SU	100 uL
LLCS 320-184385/2		537, 537				250 mL	1.00 mL	7 SU	100 uL
LLCSD 320-184385/3		537, 537				250 mL	1.00 mL	7 SU	100 uL
320-31468-A-21	NAWC-091117-RW-1 62	537, 537	T	291.25 g	28.32 g	262.9 mL	1.00 mL	7 SU	100 uL
320-31468-A-22	NAWC-091117-FRB- 162	537, 537	T	275.14 g	27.84 g	247.3 mL	1.00 mL	7 SU	100 uL
320-31468-A-23	WGNA-091117-DUP0 9	537, 537	T	287.92 g	27.88 g	260 mL	1.00 mL	7 SU	100 uL

Lab Sample ID	Client Sample ID	Method Chain	Basis	LC537-LSP 00025	LC537-SU 00048	AnalysisComment			
MB 320-184385/1		537, 537			100 uL	ch nd			
LLCS 320-184385/2		537, 537		100 uL	100 uL	ch nd			
LLCSD 320-184385/3		537, 537		100 uL	100 uL	ch nd			
320-31468-A-21	NAWC-091117-RW-1 62	537, 537	T		100 uL	ch nd			
320-31468-A-22	NAWC-091117-FRB- 162	537, 537	T		100 uL	ch nd			
320-31468-A-23	WGNA-091117-DUP0 9	537, 537	T		100 uL	ch nd			

The pound sign (#) in the amount added field denotes that the reagent was used undiluted. All calculations are performed using the stated concentration for this reagent.

LCMS BATCH WORKSHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1

SDG No.: \_\_\_\_\_

Batch Number: 184385 Batch Start Date: 09/14/17 09:29 Batch Analyst: Branscum, Cassie

Batch Method: 537 Batch End Date: 09/15/17 14:40

Batch Notes	
Batch Comment	IS:1002957 BD:CCB FV: CCB AL:VPM
Manifold ID	9
Methanol ID	1021243
Pipette ID	H14930F
Analyst ID - IS Reagent Drop	VPM
Analyst ID - IS Reagent Drop Witness	NSH
Analyst ID - SU Reagent Drop	CCB
Analyst ID - SU Reagent Drop Witness	HJA
Analyst ID - TA Reagent Drop	CCB
Analyst ID - TA Reagent Drop Witness	HJA
SPE Cartridge ID	6357081-06
Trizma ID	SLBR4303V
Reagent Water ID	9/13/17

Basis	Basis Description
T	Total/NA

The pound sign (#) in the amount added field denotes that the reagent was used undiluted. All calculations are performed using the stated concentration for this reagent.

A8

Job No: 31468 Instrument ID & Date: 9-20-17 ICAL Batch: 185329  
 Extraction Batch: 184382, 184385 Worklist #: 48169, 48188 TALS Batch: 185406, 185407, 185408, 185409, 185468

Review Items	-- Level 1 --			Level 2
	Yes	No	N/A	
<b>Initial Calibration</b>				
1. Is ICAL verified and locked in Chrom & TALS?	✓			✓
2. Is ICV properly linked in TALS?	✓			✓
<b>Continuing Calibration</b>				
1. Low-range CCV injected at start of analytical run? CCV injected after every 10 samples and at the end of the analytical run and alternated between Low-range, Mid-range and High-range?	✓			✓
2. If sequence was not after an ICAL was a low and mid range CCV injected at the start of the analytical run?			✓	
3. Native compounds and surrogates in control? Low-range within ±50% of true value Mid and High-range within ±30% of true value	✓			✓
4. Internal Standard areas in control? Areas ≥ 50% of average area of the ICAL and 70-140% of the most recent CCV.	✓			✓
<b>Client Samples &amp; QC Sample Results</b>				
1. Were preparation and analysis done within holding times?	✓			✓
2. Are Chromatograms reviewed and spectra verified?	✓			✓
3. Are positive results within calibration range?	✓			✓
4. Dilutions due to target cpds? _____ Dilutions due to non-targets? _____			✓	
5. All target compounds in MB < 1/3 RL? (Requires NCM if "no.")	✓			✓
6. Are target constituents in LCS/LCSD within method control limits?	✓			✓
7. Internal Standard areas in control for all samples and QC reported? ±50% from the average area of the ICAL and 70-140% of the most recent CCV	✓			✓
8. Do results (e.g., dilutions/trip blanks) make sense?	✓			✓
9. Are MS/MSD recoveries and RPDs within method control limits?			✓	
10. Are all QC samples properly linked in TALS?	✓			✓
11. All manual integrations appropriate and completely documented?	✓			✓
12. Are nonconformances documented as NCMs?	✓			✓
13. Are all Chrom graphics uploaded?	✓			✓

1<sup>st</sup> Level Reviewer / Date: JRB 9-20-17 2<sup>nd</sup> Level Reviewer / Date: Sub 9/22/17

NCM # and Comments: 101636

A8

Instrument ID & Date: 9-20-17 Worklist#: 48154

ICAL Batch: 185329, 185330 Calibration ID number: 34457

Review Items	--- Level 1 ---			Level 2
	Yes	No	N/A	
<b>Initial Calibration</b>				
1. Mass calibration, as needed, verified by full scan of PFC stock standard. All PFC ions used for quantitation are within 0.3 m/z of true mass?	✓			✓
2. Responses increase with increasing concentration?	✓			✓
3. Fit used (circle): <u>Average</u> Linear (1/x <sup>2</sup> ) Linear <u>Quadratic</u> (6 points minimum)				
4. Meets fit criteria? Intercept ≤ ½ RL RSD ≤ 30% for Average R <sup>2</sup> ≥ 0.990 for Linear R <sup>2</sup> ≥ 0.990 for Quadratic NOTE: "Force through Zero" must be used and weighted if needed	✓			✓
5. If quadratic fit used the curve does not "bend over".	✓			✓
6. Feed calibration points into the calculated curve. Are points ≤MRL within ±50% of true value? Are points >MRL within ±30% of true value?	✓			✓
7. Any carryover from the high calibration point must be ≤ 1/3 RL	✓			✓
8. Asymmetry check meets criteria for the first two eluting peaks? (0.8 - 1.5).	✓			✓
9. Is the asymmetry check scanned and linked in TALS to the calibration point?	✓			✓
10. Is ICV (2 <sup>nd</sup> source) ± 30% of true value?	✓			✓
11. Is ICV (2 <sup>nd</sup> source) internal standards ±50% of average area of the ICAL?	✓			✓
12. ICAL locked in Chrom and uploaded to TALS?	✓			✓
13. ICAL locked in TALS and scanned?				✓

1<sup>st</sup> Level Reviewer / Date: MWJ for JRB  
9/22/17

2<sup>nd</sup> Level Reviewer / Date: MWJ  
9/22/17

NCM # and Comments: \_\_\_\_\_  
\_\_\_\_\_  
\_\_\_\_\_  
\_\_\_\_\_

TestAmerica Laboratories  
Worklist QC Batch Report

Worklist Name: 20SEP2017\_537A  
Instrument Name: A8\_N  
Data Directory: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48169.b  
QC Batching: Enabled

Worklist Number: 48169  
Chrom Method: 537\_A8\_N  
Limit Group Batching: Enabled

QC Batch: 1	LC 537 ICAL Raw Batch: 185406
# 1 CCV L5	# 1 CCV L5
# 2 RB	# 2 RB
# 3 MB 320-184385/1-A	# 3 MB 320-184385/1-A
# 4 LLCS 320-184385/2-A	# 4 LLCS 320-184385/2-A
# 5 LLCSD 320-184385/3-A	# 5 LLCSD 320-184385/3-A
# 6 320-31468-A-21-A	# 6 320-31468-A-21-A
# 7 320-31468-A-22-A	# 7 320-31468-A-22-A
# 8 320-31468-A-23-A	# 8 320-31468-A-23-A
# 9 CCV L3	# 9 CCV L3

QC Batch: 2	LC 537 ICAL Raw Batch: 185407
# 9 CCV L3	# 9 CCV L3
#10 RB	#10 RB
#11 MB 320-184382/1-A	#11 MB 320-184382/1-A
#12 LCS 320-184382/2-A	#12 LCS 320-184382/2-A
#13 LCSD 320-184382/3-A	#13 LCSD 320-184382/3-A
#14 320-31468-A-1-A	#14 320-31468-A-1-A
#15 320-31468-A-2-A	#15 320-31468-A-2-A
#16 320-31468-A-3-A	#16 320-31468-A-3-A
#17 320-31468-A-4-A	#17 320-31468-A-4-A
#18 320-31468-A-5-A	#18 320-31468-A-5-A
#19 320-31468-A-6-A	#19 320-31468-A-6-A
#20 320-31468-A-7-A	#20 320-31468-A-7-A
#21 CCV L5	#21 CCV L5

QC Batch: 3	LC 537 ICAL Raw Batch: 185408
#21 CCV L5	#21 CCV L5
#22 RB	#22 RB
#23 320-31468-A-8-A	#23 320-31468-A-8-A
#24 320-31468-A-9-A	#24 320-31468-A-9-A
#25 320-31468-A-10-A	#25 320-31468-A-10-A
#26 320-31468-A-11-A	#26 320-31468-A-11-A
#27 320-31468-A-12-A	#27 320-31468-A-12-A
#28 320-31468-A-13-A	#28 320-31468-A-13-A
#29 320-31468-A-14-A	#29 320-31468-A-14-A
#30 320-31468-A-15-A	#30 320-31468-A-15-A
#31 320-31468-A-16-A	#31 320-31468-A-16-A
#32 320-31468-A-17-A	#32 320-31468-A-17-A
#33 CCV L3	#33 CCV L3

QC Batch: 4	LC 537 ICAL Raw Batch: 185409
#33 CCV L3	#33 CCV L3
#34 RB	#34 RB
#35 320-31468-A-18-A	#35 320-31468-A-18-A
#36 320-31468-A-19-A	#36 320-31468-A-19-A
#37 320-31468-A-20-A	#37 320-31468-A-20-A
#38 CCV L5	#38 CCV L5

TestAmerica Laboratories  
 Worklist QC Batch Report

Worklist Name: 20SEP2017\_537D                      Worklist Number: 48188  
 Instrument Name: A8\_N                                  Chrom Method: 537\_A8\_N  
 Data Directory: \\ChromNa\Sacramento\ChromData\A8\_N\20170920-48188.b  
 QC Batching: Enabled                                  Limit Group Batching: Enabled

QC Batch: 1	LC 537 ICAL Raw Batch: 185468
# 1 CCV L3	# 1 CCV L3
# 2 RB	# 2 RB
# 3 320-31468-A-1-A	# 3 320-31468-A-1-A
# 4 320-31468-A-15-A	# 4 320-31468-A-15-A
# 5 320-31489-A-9-A	# 5 320-31489-A-9-A
# 6 RINSE	# 6 RINSE
# 7 MB 320-184385/1-A	# 7 MB 320-184385/1-A
# 8 320-31489-A-13-A	# 8 320-31489-A-13-A
# 9 CCV L5	# 9 CCV L5
#10 RB	#10 RB



17

AB 9/19/17

# Aqueous Extraction Analysis Sheet







(To Accompany Samples to Instruments)

Batch Number: 320-184385  
 Method Code: 320-537\_Prep-320

Analyst: Branscum, Cassie

Batch Open: 9/14/2017 9:29:00AM  
 Batch End: 9/15/2017 2:40:00PM

## Extraction of Perfluorinated Alkyl Acids

Input Sample Lab ID (Analytical Method)	SDG (Job #)	GrossWt TareWt	InitAmnt FinAmnt	Rcvd	PHs Adj1 Adj2	Due Date	Analytical TAT	Div Rank	Comments	Output Sample Lab ID
1 MB~320-184385/1 N/A	N/A		250 mL	7		N/A	N/A	N/A	ch nd <b>RI</b>	
			1.00 mL							
2 LLCS~320-184385/2 N/A	N/A		250 mL	7		N/A	N/A	N/A	ch nd	
			1.00 mL							
3 LLCSD~320-184385/3 N/A	N/A		250 mL	7		N/A	N/A	N/A	ch nd	
			1.00 mL							
320-31468-A-21 (537_DOD5)	N/A (320-31468-1)	291.25 g	262.9 mL	7		9/16/17	16_Days	4	ch nd	
		28.32 g	1.00 mL							
320-31468-A-22 (537_DOD5)	N/A (320-31468-1)	275.14 g	247.3 mL	7		9/16/17	16_Days	4	ch nd	
		27.84 g	1.00 mL							
6 320-31468-A-23 (537_DOD5)	N/A (320-31468-1)	287.92 g	260 mL	7		9/16/17	16_Days	4	ch nd	
		27.88 g	1.00 mL							

Page 463 of 476

# Aqueous Extraction Analysis Sheet

(To Accompany Samples to Instruments)

Batch Number: 320-184385

Analyst: Branscum, Cassie

Batch Open: 9/14/2017 9:29:00AM

Method Code: 320-537\_Prep-320

Batch End: 9/15/2017 2:40:00PM

## Batch Notes

Manifold ID 9

Trizma ID SLBR4303V

SPE Cartridge ID 6357081-06

Methanol ID 1021243

Reagent Water ID 9/13/17

Pipette ID H14930F

Analyst ID - TA Reagent Drop CCB

Analyst ID - TA Reagent Drop HJA

Witness

Analyst ID - SU Reagent Drop CCB

Analyst ID - SU Reagent Drop HJA

Witness

Analyst ID - IS Reagent Drop VPM

Analyst ID - IS Reagent Drop NSH

Witness

Batch Comment IS:1002957 BD:CCB FV: CCB AL:VPM

## Comments

Page 464 of 476

# Aqueous Extraction Analysis Sheet

(To Accompany Samples to Instruments)

Batch Number: 320-184385

Analyst: Branscum, Cassie

Batch Open: 9/14/2017 9:29:00AM

Method Code: 320-537\_Prep-320

Batch End:

## Reagent Additions Worksheet

Lab ID	Reagent Code	Amount Added	Final Amount	By	Witness
MB 320-184385/1	LC537-SU_00048	100 uL	1.00 mL	CAB 9-14-17	HSA 9-14-17
LLCS 320-184385/2	LC537-LSP_00025	100 uL	1.00 mL	↓	↓
LLCS 320-184385/2	LC537-SU_00048	100 uL	1.00 mL		
LLCSD 320-184385/3	LC537-LSP_00025	100 uL	1.00 mL		
LLCSD 320-184385/3	LC537-SU_00048	100 uL	1.00 mL		
320-31468-A-21	LC537-SU_00048	100 uL	1.00 mL		
320-31468-A-22	LC537-SU_00048	100 uL	1.00 mL		
320-31468-A-23	LC537-SU_00048	100 uL	1.00 mL		

Page 465 of 476

### Other Reagents:

Reagent	Amount/Units	Lot#:

Preparation Batch Number(s): 320-184385 Test: 537-Prep

Earliest Holding Time: 9-25-17

	1 <sup>st</sup> Level Reviewer	2 <sup>nd</sup> Level Reviewer
<b>Sample List Tab</b>		
Samples identified to the correct method	✓	✓
All necessary NCMs filed (including holding time)	✓	✓
Method/sample/login/QAS checked and correct	✓	✓
<b>Worksheet Tab</b>		
All samples properly preserved	✓	✓
Weights in anticipated range and not targeted	✓	✓
All additional test requirements performed, documented, and uploaded to TALS correctly (e.g. final amount, initial amount, turbidity, and CI Check)	✓	✓
The pH is transcribed correctly in TALS	✓	✓
All additional information transcribed into TALS is correct and raw data is attached	✓	✓
Comments are transcribed correctly in TALS	✓	✓
<b>Reagents Tab</b>		
All necessary reagents not expired and entered into TALS	✓	✓
All spike amounts correct and added to necessary samples and QC	✓	✓
<b>Batch Information</b>		
Date and time accurate and entered into TALS correctly	✓	✓
All necessary 'batch information' complete and entered into TALS correctly	✓	✓

1<sup>st</sup> Level Reviewer: JW

Date: 9/15/17

2<sup>nd</sup> Level Reviewer: VPM

Date: 9/15/17

Comments: \_\_\_\_\_

19

# Aqueous Extraction Analysis Sheet

AB 9/19/17

(To Accompany Samples to Instruments)

Batch Number: 320-184382

Analyst: Sharifi, Nooshin

Batch Open: 9/14/2017 9:16:00AM

Method Code: 320-537\_Prep-320

Batch End: 9/18/2017 4:50:00PM

## Extraction of Perfluorinated Alkyl Acids

Input Sample Lab ID (Analytical Method)	SDG (Job #)	GrossWt TareWt	InitAmnt FinAmnt	Rcvd	PHs Adj1 Adj2	Due Date	Analytical TAT	Div Rank	Comments	Output Sample Lab ID
1 MB-320-184382/1 N/A	N/A		250 mL	7		N/A	N/A	N/A	CH ND	
			1.0 mL							
2 LCS-320-184382/2 N/A	N/A		250 mL	7		N/A	N/A	N/A	CH ND	
			1.0 mL							
3 LCSD-320-184382/3 N/A	N/A		250 mL	7		N/A	N/A	N/A	CH ND	
			1.0 mL							
4 320-31468-A-1 (537_DOD5)	N/A (320-31468-1)	279.32 g	252.7 mL	7		9/16/17	16_Days	4	CH ND RI	
		26.60 g	1.0 mL							
5 320-31468-A-2 (537_DOD5)	N/A (320-31468-1)	286.63 g	258.9 mL	7		9/16/17	16_Days	4	CH ND	
		27.74 g	1.0 mL							
6 320-31468-A-3 (537_DOD5)	N/A (320-31468-1)	289.73 g	261.7 mL	7		9/16/17	16_Days	4	CH ND	
		28.04 g	1.0 mL							
7 320-31468-A-4 (537_DOD5)	N/A (320-31468-1)	287.72 g	259.9 mL	7		9/16/17	16_Days	4	CH ND	
		27.79 g	1.0 mL							
8 320-31468-A-5 (537_DOD5)	N/A (320-31468-1)	290.32 g	262.7 mL	7		9/16/17	16_Days	4	CH ND	
		27.61 g	1.0 mL							
9 320-31468-A-6 (537_DOD5)	N/A (320-31468-1)	293.04 g	265.6 mL	7		9/16/17	16_Days	4	CH ND	
		27.48 g	1.0 mL							
10 320-31468-A-7 (537_DOD5)	N/A (320-31468-1)	294.63 g	267 mL	7		9/16/17	16_Days	4	CH ND	
		27.68 g	1.0 mL							

Page 467 of 476

# Aqueous Extraction Analysis Sheet

(To Accompany Samples to Instruments)













Batch Number: 320-184382

Analyst: Sharifi, Nooshin

Batch Open: 9/14/2017 9:16:00AM

Method Code: 320-537\_Prep-320

Batch End:

11	320-31468-A-8 (537_DOD5)	N/A (320-31468-1)	289.24 g	1.0 mL	7		9/16/17	16_Days	4	CH ND	
12	320-31468-A-9 (537_DOD5)	N/A (320-31468-1)	291.43 g	1.0 mL	7		9/16/17	16_Days	4	CH ND	
13	320-31468-A-10 (537_DOD5)	N/A (320-31468-1)	294.51 g	1.0 mL	7		9/16/17	16_Days	4	CH ND	
14	320-31468-A-11 (537_DOD5)	N/A (320-31468-1)	296.76 g	1.0 mL	7		9/16/17	16_Days	4	CH ND	
15	320-31468-A-12 (537_DOD5)	N/A (320-31468-1)	293.17 g	1.0 mL	7		9/16/17	16_Days	4	CH ND	
16	320-31468-A-13 (537_DOD5)	N/A (320-31468-1)	291.04 g	1.0 mL	7		9/16/17	16_Days	4	CH ND	
17	320-31468-A-14 (537_DOD5)	N/A (320-31468-1)	281.96 g	1.0 mL	7		9/16/17	16_Days	4	CH ND	
18	320-31468-A-15 (537_DOD5)	N/A (320-31468-1)	278.29 g	1.0 mL	7		9/16/17	16_Days	4	CH ND	RI 
19	320-31468-A-16 (537_DOD5)	N/A (320-31468-1)	294.18 g	1.0 mL	7		9/16/17	16_Days	4	CH ND	
20	320-31468-A-17 (537_DOD5)	N/A (320-31468-1)	289.71 g	1.0 mL	7		9/16/17	16_Days	4	CH ND	
21	320-31468-A-18 (537_DOD5)	N/A (320-31468-1)	291.10 g	1.0 mL	7		9/16/17	16_Days	4	CH ND	
22	320-31468-A-19 (537_DOD5)	N/A (320-31468-1)	283.27 g	1.0 mL	7		9/16/17	16_Days	4	CH ND	

Page 468 of 476

# Aqueous Extraction Analysis Sheet

(To Accompany Samples to Instruments)

Batch Number: 320-184382


Analyst: Sharifi, Nooshin

Batch Open: 9/14/2017 9:16:00AM

Method Code: 320-537\_Prep-320

Batch End:

23

320-31468-A-20 (537_DOD5)	N/A (320-31468-1)	287.79 g		7		9/16/17	16_Days	4	CH ND	
		1.0 mL								

## Batch Notes

Manifold ID 1,3

Trizma ID SLBR4303V

SPE Cartridge ID 6357081-025

Methanol ID 1021237

Reagent Water ID 9/13/17

Pipette ID H14930F

Analyst ID - TA Reagent Drop NSH

Analyst ID - TA Reagent Drop Witness CCB ABH 9/15/17  
AAR

Analyst ID - SU Reagent Drop NSH

Analyst ID - SU Reagent Drop Witness CCB ABH 9/15/17  
AAR

Analyst ID - IS Reagent Drop VPM

Analyst ID - IS Reagent Drop Witness TWL

Batch Comment IS: 1002957      BD: CCB      FV: VPM      AL: VPM

## Comments

Page 469 of 476

# Aqueous Extraction Analysis Sheet

(To Accompany Samples to Instruments)

Batch Number: 320-184382

Analyst: Sharifi, Nooshin

Batch Open: 9/14/2017 9:16:00AM

Method Code: 320-537\_Prep-320

Batch End:

## Reagent Additions Worksheet

Lab ID	Reagent Code	Amount Added	Final Amount	By	Witness
MB 320-184382/1	LC537-SU_00048	100 uL	1.0 mL	NSH 9/14/17	AAK 9/14/17
LCS 320-184382/2	LC537-HSP_00023	100 uL	1.0 mL		
LCS 320-184382/2	LC537-SU_00048	100 uL	1.0 mL		
LCSD 320-184382/3	LC537-HSP_00023	100 uL	1.0 mL		
LCSD 320-184382/3	LC537-SU_00048	100 uL	1.0 mL		
320-31468-A-1	LC537-SU_00048	100 uL	1.0 mL		
320-31468-A-2	LC537-SU_00048	100 uL	1.0 mL		
320-31468-A-3	LC537-SU_00048	100 uL	1.0 mL		
320-31468-A-4	LC537-SU_00048	100 uL	1.0 mL		
320-31468-A-5	LC537-SU_00048	100 uL	1.0 mL		
320-31468-A-6	LC537-SU_00048	100 uL	1.0 mL		
320-31468-A-7	LC537-SU_00048	100 uL	1.0 mL		
320-31468-A-8	LC537-SU_00048	100 uL	1.0 mL		
320-31468-A-9	LC537-SU_00048	100 uL	1.0 mL		
320-31468-A-10	LC537-SU_00048	100 uL	1.0 mL		
320-31468-A-11	LC537-SU_00048	100 uL	1.0 mL		
320-31468-A-12	LC537-SU_00048	100 uL	1.0 mL		
320-31468-A-13	LC537-SU_00048	100 uL	1.0 mL		

Page 470 of 476



# Aqueous Extraction Analysis Sheet

(To Accompany Samples to Instruments)

Batch Number: 320-184382

Analyst: Sharifi, Nooshin

Batch Open: 9/14/2017 9:16:00AM

Method Code: 320-537\_Prep-320

Batch End:

320-31468-A-14	LC537-SU_00048	100 uL	1.0 mL	NSA 9/14/17	AAR 9/14/17
320-31468-A-15	LC537-SU_00048	100 uL	1.0 mL		
320-31468-A-16	LC537-SU_00048	100 uL	1.0 mL		
320-31468-A-17	LC537-SU_00048	100 uL	1.0 mL		
320-31468-A-18	LC537-SU_00048	100 uL	1.0 mL		
320-31468-A-19	LC537-SU_00048	100 uL	1.0 mL		
320-31468-A-20	LC537-SU_00048	100 uL	1.0 mL		

### Other Reagents:

Reagent	Amount/Units	Lot#:

Page 471 of 476

Preparation Batch Number(s): 184382 Test: 537  
 Earliest Holding Time: 9/25/17

<b>Sample List Tab</b>		1 <sup>st</sup> Level Reviewer	2 <sup>nd</sup> Level Reviewer
Samples identified to the correct method		✓	✓
All necessary NCMs filed (including holding time)		✓	✓
Method/sample/login/QAS checked and correct		✓	✓
<b>Worksheet Tab</b>		1 <sup>st</sup> Level Reviewer	2 <sup>nd</sup> Level Reviewer
All samples properly preserved		✓	✓
Weights in anticipated range and not targeted		✓	✓
All additional test requirements performed, documented, and uploaded to TALS correctly (e.g. final amount, initial amount, turbidity, and CI Check)		✓	✓
The pH is transcribed correctly in TALS		✓	✓
All additional information transcribed into TALS is correct and raw data is attached		✓	✓
Comments are transcribed correctly in TALS		✓	✓
<b>Reagents Tab</b>		1 <sup>st</sup> Level Reviewer	2 <sup>nd</sup> Level Reviewer
All necessary reagents not expired and entered into TALS		✓	✓
All spike amounts correct and added to necessary samples and QC		✓	✓
<b>Batch Information</b>		1 <sup>st</sup> Level Reviewer	2 <sup>nd</sup> Level Reviewer
Date and time accurate and entered into TALS correctly		✓	✓
All necessary 'batch information' complete and entered into TALS correctly		✓	✓

1<sup>st</sup> Level Reviewer: ABH Date: 9/18/17  
 2<sup>nd</sup> Level Reviewer: VPM Date: 9/18/17  
 Comments: \_\_\_\_\_

# Shipping and Receiving Documents

**TestAmerica Sacramento**

880 Riverside Parkway  
West Sacramento, CA 95605-1500  
phone 916.373.5600 fax 303.467.7248

**Chain of Custody Record**



THE LEADER IN ENVIRONMENTAL TESTING.

**TestAmerica Laboratories, Inc.**

Regulatory Program:  DW  NPDES  RCRA  Other:

<b>Client Contact</b>		<b>Project Manager:</b> Andy Frebowitz		<b>Site Contact:</b> Mary Kay Bond		<b>Date:</b> 9/11/2017		<b>COC No:</b>															
TetraTech		Tel/Fax: 610.382.1170		Lab Contact: Dave Alltucker		Carrier: FedEx		1 of 2 COCs															
234 Mall Boulevard Suite 260		<table border="1"> <tr> <th colspan="2">Analysis Turnaround Time</th> </tr> <tr> <td><input type="checkbox"/> CALENDAR DAYS</td> <td><input type="checkbox"/> WORKING DAYS</td> </tr> <tr> <td colspan="2">TAT if different from Below 21</td> </tr> <tr> <td><input type="checkbox"/> 2 weeks</td> <td></td> </tr> <tr> <td><input type="checkbox"/> 1 week</td> <td></td> </tr> <tr> <td><input type="checkbox"/> 2 days</td> <td></td> </tr> <tr> <td><input type="checkbox"/> 1 day</td> <td></td> </tr> </table>								Analysis Turnaround Time		<input type="checkbox"/> CALENDAR DAYS	<input type="checkbox"/> WORKING DAYS	TAT if different from Below 21		<input type="checkbox"/> 2 weeks		<input type="checkbox"/> 1 week		<input type="checkbox"/> 2 days		<input type="checkbox"/> 1 day	
Analysis Turnaround Time																							
<input type="checkbox"/> CALENDAR DAYS	<input type="checkbox"/> WORKING DAYS																						
TAT if different from Below 21																							
<input type="checkbox"/> 2 weeks																							
<input type="checkbox"/> 1 week																							
<input type="checkbox"/> 2 days																							
<input type="checkbox"/> 1 day																							
King of Prussia, PA 19406																							
610-382-1174																							
610-491-9688																							
Project Name: WE04																							
Site: WE04																							
P O # 1132358 (through EarthToxics)																							



Sample Identification	Sample Date	Sample Time	Sample Type (C=Comp, G=Grab)	Matrix	# of Cont.	Filtered Sample (Y/N)	Perform MS / MSD (Y/N)	EPA 537 UCMR3	Sample Specific Notes:									
NAWC-091117-RW-106	9/11/2017	09:40	G	DW	2	N	N	Y										
NAWC-091117-FRB-106	9/11/2017	09:35	G	DW	2	N	N	Y	Field Reagent Blank									
NAWC-091117-RW-060	9/11/2017	09:55	G	DW	2	N	N	Y										
NAWC-091117-FRB-060	9/11/2017	09:50	G	DW	2	N	N	Y	Field Reagent Blank									
NAWC-091117-RW-314	9/11/2017	10:25	G	DW	2	N	N	Y										
NAWC-091117-FRB-314	9/11/2017	10:20	G	DW	2	N	N	Y	Field Reagent Blank									
NAWC-091117-RW-258	9/11/2017	11:00	G	DW	2	N	N	Y										
NAWC-091117-FRB-258	9/11/2017	10:55	G	DW	2	N	N	Y	Field Reagent Blank									
NAWC-091117-RW-048	9/11/2017	13:05	G	DW	2	N	N	Y										
NAWC-091117-FRB-048	9/11/2017	13:00	G	DW	2	N	N	Y	Field Reagent Blank									
NAWC-091117-RW-145	9/11/2017	13:35	G	DW	2	N	N	Y										
NAWC-091117-FRB-145	9/11/2017	13:30	G	DW	2	N	N	Y	Field Reagent Blank									

Page 474 of 476

<b>Preservation Used:</b> 1= Ice, 2= HCl; 3= H2SO4; 4=HNO3; 5=NaOH; 6= Other: Trizma		<b>Sample Disposal ( A fee may be assessed if samples are retained longer than 1 month)</b>	
<b>Possible Hazard Identification:</b> Are any samples from a listed EPA Hazardous Waste? Please List any EPA Waste Codes for the sample in the <input type="checkbox"/> Non-Hazard <input type="checkbox"/> Flammable <input type="checkbox"/> Skin Irritant <input type="checkbox"/> Poison B <input type="checkbox"/> Unknown		<input type="checkbox"/> Return to Client <input type="checkbox"/> Disposal by Lab <input type="checkbox"/> Archive for _____ Months	

**Fed Ex Tracking: 770221957389**

Custody Seals Intact:  Yes  No      Custody Seal No.: \_\_\_\_\_      Cooler Temp. (°C): Obs'd: 15      Corr'd: \_\_\_\_\_      Therm ID No.: AK-1

Relinquished by: <u>Mary Kay Bond</u>	Company: Tetra Tech	Date/Time: 9/11/2017 18:00	Received by: <u>[Signature]</u>	Company: <u>[Signature]</u>	Date/Time: 9/12/17 930
Relinquished by:	Company:	Date/Time:	Received by:	Company:	Date/Time:
Relinquished by:	Company:	Date/Time:	Received in Laboratory by:	Company:	Date/Time:

*All labeled WGN - at 9-12-17*



# Login Sample Receipt Checklist

Client: Tetra Tech, Inc.

Job Number: 320-31468-1

**Login Number: 31468**  
**List Number: 1**  
**Creator: Edman, Connor M**

**List Source: TestAmerica Sacramento**

Question	Answer	Comment
Radioactivity wasn't checked or is <=/ background as measured by a survey meter.	True	
The cooler's custody seal, if present, is intact.	True	
Sample custody seals, if present, are intact.	N/A	
The cooler or samples do not appear to have been compromised or tampered with.	True	
Samples were received on ice.	True	
Cooler Temperature is acceptable.	True	
Cooler Temperature is recorded.	True	
COC is present.	True	
COC is filled out in ink and legible.	True	
COC is filled out with all pertinent information.	True	
Is the Field Sampler's name present on COC?	True	
There are no discrepancies between the containers received and the COC.	False	IDs on containers do not match the COC. Logged in per COC.
Samples are received within Holding Time (excluding tests with immediate HTs)	True	
Sample containers have legible labels.	True	
Containers are not broken or leaking.	True	
Sample collection date/times are provided.	True	
Appropriate sample containers are used.	True	
Sample bottles are completely filled.	True	
Sample Preservation Verified.	N/A	
There is sufficient vol. for all requested analyses, incl. any requested MS/MSDs	True	
Containers requiring zero headspace have no headspace or bubble is <6mm (1/4").	True	
Multiphasic samples are not present.	True	
Samples do not require splitting or compositing.	True	
Residual Chlorine Checked.	N/A	

"NAWC-091117-RW-106","537","RES","320-31468-1","TALSAC","1763-23-1","Perfluorooctanesulfonic acid (PFOS)","17","ng/L","J M","6.7","DL","","TRG","","","40","LOQ","YES","-99","","252.7","1.0","16",""  
"NAWC-091117-RW-106","537","RES","320-31468-1","TALSAC","335-67-1","Perfluorooctanoic acid (PFOA)","20","ng/L","","2.8","DL","","TRG","","","20","LOQ","YES","-99","","252.7","1.0","7.9",""  
"NAWC-091117-RW-106","537","RES","320-31468-1","TALSAC","355-46-4","Perfluorohexanesulfonic acid (PFHxS)","8.9","ng/L","J","5.4","DL","","TRG","","","30","LOQ","YES","-99","","252.7","1.0","12",""  
"NAWC-091117-RW-106","537","RES","320-31468-1","TALSAC","375-73-5","Perfluorobutanesulfonic acid (PFBS)","36","ng/L","U","16","DL","","TRG","","","89","LOQ","YES","-99","","252.7","1.0","36",""  
"NAWC-091117-RW-106","537","RES","320-31468-1","TALSAC","375-85-9","Perfluoroheptanoic acid (PFHpA)","8.1","ng/L","J","1.9","DL","","TRG","","","9.9","LOQ","YES","-99","","252.7","1.0","4.0",""  
"NAWC-091117-RW-106","537","RES","320-31468-1","TALSAC","375-95-1","Perfluorononanoic acid (PFNA)","20","ng/L","U","7.9","DL","","TRG","","","24","LOQ","YES","-99","","252.7","1.0","20",""  
"NAWC-091117-RW-106","537","RES","320-31468-1","TALSAC","STL00993","13C2  
PFHxA","27","ng/L","Q","-99","DL","","SURR","67","","-99","LOQ","YES","39.6","","252.7","1.0","0",""  
"NAWC-091117-RW-106","537","RES","320-31468-1","TALSAC","STL00996","13C2  
PFDA","39","ng/L","","-99","DL","","SURR","100","","-99","LOQ","YES","39.6","","252.7","1.0","0",""  
"NAWC-091117-FRB-048","537","RES","320-31468-10","TALSAC","1763-23-1","Perfluorooctanesulfonic acid (PFOS)","15","ng/L","U","6.4","DL","","TRG","","","37","LOQ","YES","-99","","266.7","1.0","15",""  
"NAWC-091117-FRB-048","537","RES","320-31468-10","TALSAC","335-67-1","Perfluorooctanoic acid (PFOA)","7.5","ng/L","U","2.6","DL","","TRG","","","19","LOQ","YES","-99","","266.7","1.0","7.5",""  
"NAWC-091117-FRB-048","537","RES","320-31468-10","TALSAC","355-46-4","Perfluorohexanesulfonic acid (PFHxS)","11","ng/L","U","5.2","DL","","TRG","","","28","LOQ","YES","-99","","266.7","1.0","11",""  
"NAWC-091117-FRB-048","537","RES","320-31468-10","TALSAC","375-73-5","Perfluorobutanesulfonic acid (PFBS)","34","ng/L","U","15","DL","","TRG","","","84","LOQ","YES","-99","","266.7","1.0","34",""  
"NAWC-091117-FRB-048","537","RES","320-31468-10","TALSAC","375-85-9","Perfluoroheptanoic acid (PFHpA)","3.7","ng/L","U","1.8","DL","","TRG","","","9.4","LOQ","YES","-99","","266.7","1.0","3.7",""  
"NAWC-091117-FRB-048","537","RES","320-31468-10","TALSAC","375-95-1","Perfluorononanoic acid (PFNA)","19","ng/L","U","7.5","DL","","TRG","","","22","LOQ","YES","-99","","266.7","1.0","19",""  
"NAWC-091117-FRB-048","537","RES","320-31468-10","TALSAC","STL00993","13C2  
PFHxA","31","ng/L","","-99","DL","","SURR","84","","-99","LOQ","YES","37.5","","266.7","1.0","0",""  
"NAWC-091117-FRB-048","537","RES","320-31468-10","TALSAC","STL00996","13C2  
PFDA","38","ng/L","","-99","DL","","SURR","102","","-99","LOQ","YES","37.5","","266.7","1.0","0",""  
"NAWC-091117-RW-145","537","RES","320-31468-11","TALSAC","1763-23-1","Perfluorooctanesulfonic acid (PFOS)","19","ng/L","J M","6.3","DL","","TRG","","","37","LOQ","YES","-99","","269","1.0","15",""  
"NAWC-091117-RW-145","537","RES","320-31468-11","TALSAC","335-67-1","Perfluorooctanoic acid (PFOA)","20","ng/L","","2.6","DL","","TRG","","","19","LOQ","YES","-99","","269","1.0","7.4",""  
"NAWC-091117-RW-145","537","RES","320-31468-11","TALSAC","355-46-4","Perfluorohexanesulfonic acid (PFHxS)","7.3","ng/L","J","5.1","DL","","TRG","","","28","LOQ","YES","-99","","269","1.0","11",""  
"NAWC-091117-RW-145","537","RES","320-31468-11","TALSAC","375-73-5","Perfluorobutanesulfonic acid (PFBS)","33","ng/L","U","15","DL","","TRG","","","84","LOQ","YES","-99","","269","1.0","33",""  
"NAWC-091117-RW-145","537","RES","320-31468-11","TALSAC","375-85-9","Perfluoroheptanoic acid (PFHpA)","5.6","ng/L","J","1.8","DL","","TRG","","","9.3","LOQ","YES","-99","","269","1.0","3.7",""  
"NAWC-091117-RW-145","537","RES","320-31468-11","TALSAC","375-95-1","Perfluorononanoic acid (PFNA)","19","ng/L","U","7.4","DL","","TRG","","","22","LOQ","YES","-99","","269","1.0","19",""  
"NAWC-091117-RW-145","537","RES","320-31468-11","TALSAC","STL00993","13C2  
PFHxA","28","ng/L","","-99","DL","","SURR","74","","-99","LOQ","YES","37.2","","269","1.0","0",""  
"NAWC-091117-RW-145","537","RES","320-31468-11","TALSAC","STL00996","13C2  
PFDA","43","ng/L","","-99","DL","","SURR","115","","-99","LOQ","YES","37.2","","269","1.0","0",""  
"NAWC-091117-FRB-145","537","RES","320-31468-12","TALSAC","1763-23-1","Perfluorooctanesulfonic acid (PFOS)","15","ng/L","U","6.4","DL","","TRG","","","38","LOQ","YES","-99","","265.6","1.0","15",""  
"NAWC-091117-FRB-145","537","RES","320-31468-12","TALSAC","335-67-1","Perfluorooctanoic acid (PFOA)","7.5","ng/L","U","2.6","DL","","TRG","","","19","LOQ","YES","-99","","265.6","1.0","7.5",""  
"NAWC-091117-FRB-145","537","RES","320-31468-12","TALSAC","355-46-4","Perfluorohexanesulfonic acid

(PFHxS),"11","ng/L","U","5.2","DL","","TRG","","","28","LOQ","YES","-99","","265.6","1.0","11",""  
"NAWC-091117-FRB-145","537","RES","320-31468-12","TALSAC","375-73-5","Perfluorobutanesulfonic acid  
(PFBS)","34","ng/L","U","15","DL","","TRG","","","85","LOQ","YES","-99","","265.6","1.0","34",""  
"NAWC-091117-FRB-145","537","RES","320-31468-12","TALSAC","375-85-9","Perfluoroheptanoic acid  
(PFHpA)","3.8","ng/L","U","1.8","DL","","TRG","","","9.4","LOQ","YES","-99","","265.6","1.0","3.8",""  
"NAWC-091117-FRB-145","537","RES","320-31468-12","TALSAC","375-95-1","Perfluorononanoic acid  
(PFNA)","19","ng/L","U","7.5","DL","","TRG","","","23","LOQ","YES","-99","","265.6","1.0","19",""  
"NAWC-091117-FRB-145","537","RES","320-31468-12","TALSAC","STL00993","13C2  
PFHxA","31","ng/L","","-99","DL","","SURR","83","","-99","LOQ","YES","37.7","","265.6","1.0","0",""  
"NAWC-091117-FRB-145","537","RES","320-31468-12","TALSAC","STL00996","13C2  
PFDA","38","ng/L","","-99","DL","","SURR","100","","-99","LOQ","YES","37.7","","265.6","1.0","0",""  
"NAWC-091117-RW-317","537","RES","320-31468-13","TALSAC","1763-23-1","Perfluorooctanesulfonic acid  
(PFOS)","49","ng/L","M","6.4","DL","","TRG","","","38","LOQ","YES","-99","","263.7","1.0","15",""  
"NAWC-091117-RW-317","537","RES","320-31468-13","TALSAC","335-67-1","Perfluorooctanoic acid  
(PFOA)","21","ng/L","","2.7","DL","","TRG","","","19","LOQ","YES","-99","","263.7","1.0","7.6",""  
"NAWC-091117-RW-317","537","RES","320-31468-13","TALSAC","355-46-4","Perfluorohexanesulfonic acid  
(PFHxS)","34","ng/L","","5.2","DL","","TRG","","","28","LOQ","YES","-99","","263.7","1.0","11",""  
"NAWC-091117-RW-317","537","RES","320-31468-13","TALSAC","375-73-5","Perfluorobutanesulfonic acid  
(PFBS)","34","ng/L","U","15","DL","","TRG","","","85","LOQ","YES","-99","","263.7","1.0","34",""  
"NAWC-091117-RW-317","537","RES","320-31468-13","TALSAC","375-85-9","Perfluoroheptanoic acid  
(PFHpA)","8.1","ng/L","J","1.8","DL","","TRG","","","9.5","LOQ","YES","-99","","263.7","1.0","3.8",""  
"NAWC-091117-RW-317","537","RES","320-31468-13","TALSAC","375-95-1","Perfluorononanoic acid  
(PFNA)","19","ng/L","U","7.6","DL","","TRG","","","23","LOQ","YES","-99","","263.7","1.0","19",""  
"NAWC-091117-RW-317","537","RES","320-31468-13","TALSAC","STL00993","13C2  
PFHxA","30","ng/L","","-99","DL","","SURR","78","","-99","LOQ","YES","37.9","","263.7","1.0","0",""  
"NAWC-091117-RW-317","537","RES","320-31468-13","TALSAC","STL00996","13C2  
PFDA","44","ng/L","","-99","DL","","SURR","116","","-99","LOQ","YES","37.9","","263.7","1.0","0",""  
"NAWC-091117-FRB-317","537","RES","320-31468-14","TALSAC","1763-23-1","Perfluorooctanesulfonic acid  
(PFOS)","16","ng/L","U","6.7","DL","","TRG","","","39","LOQ","YES","-99","","254.4","1.0","16",""  
"NAWC-091117-FRB-317","537","RES","320-31468-14","TALSAC","335-67-1","Perfluorooctanoic acid  
(PFOA)","7.9","ng/L","U","2.8","DL","","TRG","","","20","LOQ","YES","-99","","254.4","1.0","7.9",""  
"NAWC-091117-FRB-317","537","RES","320-31468-14","TALSAC","355-46-4","Perfluorohexanesulfonic acid  
(PFHxS)","12","ng/L","U","5.4","DL","","TRG","","","29","LOQ","YES","-99","","254.4","1.0","12",""  
"NAWC-091117-FRB-317","537","RES","320-31468-14","TALSAC","375-73-5","Perfluorobutanesulfonic acid  
(PFBS)","35","ng/L","U","16","DL","","TRG","","","88","LOQ","YES","-99","","254.4","1.0","35",""  
"NAWC-091117-FRB-317","537","RES","320-31468-14","TALSAC","375-85-9","Perfluoroheptanoic acid  
(PFHpA)","3.9","ng/L","U","1.9","DL","","TRG","","","9.8","LOQ","YES","-99","","254.4","1.0","3.9",""  
"NAWC-091117-FRB-317","537","RES","320-31468-14","TALSAC","375-95-1","Perfluorononanoic acid  
(PFNA)","20","ng/L","U","7.9","DL","","TRG","","","24","LOQ","YES","-99","","254.4","1.0","20",""  
"NAWC-091117-FRB-317","537","RES","320-31468-14","TALSAC","STL00993","13C2  
PFHxA","33","ng/L","","-99","DL","","SURR","83","","-99","LOQ","YES","39.3","","254.4","1.0","0",""  
"NAWC-091117-FRB-317","537","RES","320-31468-14","TALSAC","STL00996","13C2  
PFDA","38","ng/L","","-99","DL","","SURR","97","","-99","LOQ","YES","39.3","","254.4","1.0","0",""  
"NAWC-091117-RW-319","537","RES","320-31468-15","TALSAC","1763-23-1","Perfluorooctanesulfonic acid  
(PFOS)","43","ng/L","M","6.8","DL","","TRG","","","40","LOQ","YES","-99","","251","1.0","16",""  
"NAWC-091117-RW-319","537","RES","320-31468-15","TALSAC","335-67-1","Perfluorooctanoic acid  
(PFOA)","44","ng/L","","2.8","DL","","TRG","","","20","LOQ","YES","-99","","251","1.0","8.0",""  
"NAWC-091117-RW-319","537","RES","320-31468-15","TALSAC","355-46-4","Perfluorohexanesulfonic acid  
(PFHxS)","8.0","ng/L","J","5.5","DL","","TRG","","","30","LOQ","YES","-99","","251","1.0","12",""  
"NAWC-091117-RW-319","537","RES","320-31468-15","TALSAC","375-73-5","Perfluorobutanesulfonic acid  
(PFBS)","36","ng/L","U","16","DL","","TRG","","","90","LOQ","YES","-99","","251","1.0","36",""  
"NAWC-091117-RW-319","537","RES","320-31468-15","TALSAC","375-85-9","Perfluoroheptanoic acid  
(PFHpA)","15","ng/L","M","1.9","DL","","TRG","","","10","LOQ","YES","-99","","251","1.0","4.0",""  
"NAWC-091117-RW-319","537","RES","320-31468-15","TALSAC","375-95-1","Perfluorononanoic acid



(PFNA),"9.7","ng/L","J","8.0","DL","","TRG","","","24","LOQ","YES",-99","","251","1.0","20","","  
"NAWC-091117-RW-319","537","RES","320-31468-15","TALSAC","STL00993","13C2  
PFHxA","24","ng/L","Q",-99,"DL","","SURR","61","","-99","LOQ","YES","39.8","","251","1.0","0","","  
"NAWC-091117-RW-319","537","RES","320-31468-15","TALSAC","STL00996","13C2  
PFDA","33","ng/L","","-99","DL","","SURR","83","","-99","LOQ","YES","39.8","","251","1.0","0","","  
"NAWC-091117-FRB-319","537","RES","320-31468-16","TALSAC","1763-23-1","Perfluorooctanesulfonic acid  
(PFOS)","15","ng/L","U","6.4","DL","","TRG","","","37","LOQ","YES",-99","","266.7","1.0","15","","  
"NAWC-091117-FRB-319","537","RES","320-31468-16","TALSAC","335-67-1","Perfluorooctanoic acid  
(PFOA)","7.5","ng/L","U","2.6","DL","","TRG","","","19","LOQ","YES",-99","","266.7","1.0","7.5","","  
"NAWC-091117-FRB-319","537","RES","320-31468-16","TALSAC","355-46-4","Perfluorohexanesulfonic acid  
(PFHxS)","11","ng/L","U","5.2","DL","","TRG","","","28","LOQ","YES",-99","","266.7","1.0","11","","  
"NAWC-091117-FRB-319","537","RES","320-31468-16","TALSAC","375-73-5","Perfluorobutanesulfonic acid  
(PFBS)","34","ng/L","U","15","DL","","TRG","","","84","LOQ","YES",-99","","266.7","1.0","34","","  
"NAWC-091117-FRB-319","537","RES","320-31468-16","TALSAC","375-85-9","Perfluoroheptanoic acid  
(PFHpA)","3.7","ng/L","U","1.8","DL","","TRG","","","9.4","LOQ","YES",-99","","266.7","1.0","3.7","","  
"NAWC-091117-FRB-319","537","RES","320-31468-16","TALSAC","375-95-1","Perfluorononanoic acid  
(PFNA)","19","ng/L","U","7.5","DL","","TRG","","","22","LOQ","YES",-99","","266.7","1.0","19","","  
"NAWC-091117-FRB-319","537","RES","320-31468-16","TALSAC","STL00993","13C2  
PFHxA","31","ng/L","","-99","DL","","SURR","82","","-99","LOQ","YES","37.5","","266.7","1.0","0","","  
"NAWC-091117-FRB-319","537","RES","320-31468-16","TALSAC","STL00996","13C2  
PFDA","46","ng/L","","-99","DL","","SURR","124","","-99","LOQ","YES","37.5","","266.7","1.0","0","","  
"NAWC-091117-RW-321","537","RES","320-31468-17","TALSAC","1763-23-1","Perfluorooctanesulfonic acid  
(PFOS)","7.5","ng/L","J M","6.5","DL","","TRG","","","38","LOQ","YES",-99","","262","1.0","15","","  
"NAWC-091117-RW-321","537","RES","320-31468-17","TALSAC","335-67-1","Perfluorooctanoic acid  
(PFOA)","6.9","ng/L","J","2.7","DL","","TRG","","","19","LOQ","YES",-99","","262","1.0","7.6","","  
"NAWC-091117-RW-321","537","RES","320-31468-17","TALSAC","355-46-4","Perfluorohexanesulfonic acid  
(PFHxS)","11","ng/L","U","5.2","DL","","TRG","","","29","LOQ","YES",-99","","262","1.0","11","","  
"NAWC-091117-RW-321","537","RES","320-31468-17","TALSAC","375-73-5","Perfluorobutanesulfonic acid  
(PFBS)","34","ng/L","U","15","DL","","TRG","","","86","LOQ","YES",-99","","262","1.0","34","","  
"NAWC-091117-RW-321","537","RES","320-31468-17","TALSAC","375-85-9","Perfluoroheptanoic acid  
(PFHpA)","1.8","ng/L","J","1.8","DL","","TRG","","","9.5","LOQ","YES",-99","","262","1.0","3.8","","  
"NAWC-091117-RW-321","537","RES","320-31468-17","TALSAC","375-95-1","Perfluorononanoic acid  
(PFNA)","19","ng/L","U","7.6","DL","","TRG","","","23","LOQ","YES",-99","","262","1.0","19","","  
"NAWC-091117-RW-321","537","RES","320-31468-17","TALSAC","STL00993","13C2  
PFHxA","29","ng/L","","-99","DL","","SURR","76","","-99","LOQ","YES","38.2","","262","1.0","0","","  
"NAWC-091117-RW-321","537","RES","320-31468-17","TALSAC","STL00996","13C2  
PFDA","41","ng/L","","-99","DL","","SURR","106","","-99","LOQ","YES","38.2","","262","1.0","0","","  
"NAWC-091117-FRB-321","537","RES","320-31468-18","TALSAC","1763-23-1","Perfluorooctanesulfonic acid  
(PFOS)","15","ng/L","U","6.5","DL","","TRG","","","38","LOQ","YES",-99","","263.5","1.0","15","","  
"NAWC-091117-FRB-321","537","RES","320-31468-18","TALSAC","335-67-1","Perfluorooctanoic acid  
(PFOA)","7.6","ng/L","U","2.7","DL","","TRG","","","19","LOQ","YES",-99","","263.5","1.0","7.6","","  
"NAWC-091117-FRB-321","537","RES","320-31468-18","TALSAC","355-46-4","Perfluorohexanesulfonic acid  
(PFHxS)","11","ng/L","U","5.2","DL","","TRG","","","28","LOQ","YES",-99","","263.5","1.0","11","","  
"NAWC-091117-FRB-321","537","RES","320-31468-18","TALSAC","375-73-5","Perfluorobutanesulfonic acid  
(PFBS)","34","ng/L","U","15","DL","","TRG","","","85","LOQ","YES",-99","","263.5","1.0","34","","  
"NAWC-091117-FRB-321","537","RES","320-31468-18","TALSAC","375-85-9","Perfluoroheptanoic acid  
(PFHpA)","3.8","ng/L","U","1.8","DL","","TRG","","","9.5","LOQ","YES",-99","","263.5","1.0","3.8","","  
"NAWC-091117-FRB-321","537","RES","320-31468-18","TALSAC","375-95-1","Perfluorononanoic acid  
(PFNA)","19","ng/L","U","7.6","DL","","TRG","","","23","LOQ","YES",-99","","263.5","1.0","19","","  
"NAWC-091117-FRB-321","537","RES","320-31468-18","TALSAC","STL00993","13C2  
PFHxA","32","ng/L","","-99","DL","","SURR","84","","-99","LOQ","YES","38.0","","263.5","1.0","0","","  
"NAWC-091117-FRB-321","537","RES","320-31468-18","TALSAC","STL00996","13C2  
PFDA","40","ng/L","","-99","DL","","SURR","104","","-99","LOQ","YES","38.0","","263.5","1.0","0","","  
"NAWC-091117-RW-010","537","RES","320-31468-19","TALSAC","1763-23-1","Perfluorooctanesulfonic acid

(PFOS),"30","ng/L","J M","6.7","DL","","TRG","","","39","LOQ","YES",-99","","254.7","1.0","16","","  
"NAWC-091117-RW-010","537","RES","320-31468-19","TALSAC","335-67-1","Perfluorooctanoic acid  
(PFOA),"12","ng/L","J","2.7","DL","","TRG","","","20","LOQ","YES",-99","","254.7","1.0","7.9","","  
"NAWC-091117-RW-010","537","RES","320-31468-19","TALSAC","355-46-4","Perfluorohexanesulfonic acid  
(PFHxS),"17","ng/L","J","5.4","DL","","TRG","","","29","LOQ","YES",-99","","254.7","1.0","12","","  
"NAWC-091117-RW-010","537","RES","320-31468-19","TALSAC","375-73-5","Perfluorobutanesulfonic acid  
(PFBS),"35","ng/L","U","16","DL","","TRG","","","88","LOQ","YES",-99","","254.7","1.0","35","","  
"NAWC-091117-RW-010","537","RES","320-31468-19","TALSAC","375-85-9","Perfluoroheptanoic acid  
(PFHpA),"5.4","ng/L","J","1.9","DL","","TRG","","","9.8","LOQ","YES",-99","","254.7","1.0","3.9","","  
"NAWC-091117-RW-010","537","RES","320-31468-19","TALSAC","375-95-1","Perfluorononanoic acid  
(PFNA),"20","ng/L","U","7.9","DL","","TRG","","","24","LOQ","YES",-99","","254.7","1.0","20","","  
"NAWC-091117-RW-010","537","RES","320-31468-19","TALSAC","STL00993","13C2  
PFHxA","29","ng/L","","-99","DL","","SURR","75","","-99","LOQ","YES","39.3","","254.7","1.0","0","","  
"NAWC-091117-RW-010","537","RES","320-31468-19","TALSAC","STL00996","13C2  
PFDA","41","ng/L","","-99","DL","","SURR","104","","-99","LOQ","YES","39.3","","254.7","1.0","0","","  
"NAWC-091117-FRB-106","537","RES","320-31468-2","TALSAC","1763-23-1","Perfluorooctanesulfonic acid  
(PFOS),"15","ng/L","U","6.6","DL","","TRG","","","39","LOQ","YES",-99","","258.9","1.0","15","","  
"NAWC-091117-FRB-106","537","RES","320-31468-2","TALSAC","335-67-1","Perfluorooctanoic acid  
(PFOA),"7.7","ng/L","U","2.7","DL","","TRG","","","19","LOQ","YES",-99","","258.9","1.0","7.7","","  
"NAWC-091117-FRB-106","537","RES","320-31468-2","TALSAC","355-46-4","Perfluorohexanesulfonic acid  
(PFHxS),"12","ng/L","U","5.3","DL","","TRG","","","29","LOQ","YES",-99","","258.9","1.0","12","","  
"NAWC-091117-FRB-106","537","RES","320-31468-2","TALSAC","375-73-5","Perfluorobutanesulfonic acid  
(PFBS),"35","ng/L","U","16","DL","","TRG","","","87","LOQ","YES",-99","","258.9","1.0","35","","  
"NAWC-091117-FRB-106","537","RES","320-31468-2","TALSAC","375-85-9","Perfluoroheptanoic acid  
(PFHpA),"3.9","ng/L","U","1.8","DL","","TRG","","","9.7","LOQ","YES",-99","","258.9","1.0","3.9","","  
"NAWC-091117-FRB-106","537","RES","320-31468-2","TALSAC","375-95-1","Perfluorononanoic acid  
(PFNA),"19","ng/L","U","7.7","DL","","TRG","","","23","LOQ","YES",-99","","258.9","1.0","19","","  
"NAWC-091117-FRB-106","537","RES","320-31468-2","TALSAC","STL00993","13C2  
PFHxA","32","ng/L","","-99","DL","","SURR","82","","-99","LOQ","YES","38.6","","258.9","1.0","0","","  
"NAWC-091117-FRB-106","537","RES","320-31468-2","TALSAC","STL00996","13C2  
PFDA","41","ng/L","","-99","DL","","SURR","105","","-99","LOQ","YES","38.6","","258.9","1.0","0","","  
"NAWC-091117-FRB-010","537","RES","320-31468-20","TALSAC","1763-23-1","Perfluorooctanesulfonic acid  
(PFOS),"15","ng/L","U","6.5","DL","","TRG","","","38","LOQ","YES",-99","","259.8","1.0","15","","  
"NAWC-091117-FRB-010","537","RES","320-31468-20","TALSAC","335-67-1","Perfluorooctanoic acid  
(PFOA),"7.7","ng/L","U","2.7","DL","","TRG","","","19","LOQ","YES",-99","","259.8","1.0","7.7","","  
"NAWC-091117-FRB-010","537","RES","320-31468-20","TALSAC","355-46-4","Perfluorohexanesulfonic acid  
(PFHxS),"12","ng/L","U","5.3","DL","","TRG","","","29","LOQ","YES",-99","","259.8","1.0","12","","  
"NAWC-091117-FRB-010","537","RES","320-31468-20","TALSAC","375-73-5","Perfluorobutanesulfonic acid  
(PFBS),"35","ng/L","U","15","DL","","TRG","","","87","LOQ","YES",-99","","259.8","1.0","35","","  
"NAWC-091117-FRB-010","537","RES","320-31468-20","TALSAC","375-85-9","Perfluoroheptanoic acid  
(PFHpA),"3.8","ng/L","U","1.8","DL","","TRG","","","9.6","LOQ","YES",-99","","259.8","1.0","3.8","","  
"NAWC-091117-FRB-010","537","RES","320-31468-20","TALSAC","375-95-1","Perfluorononanoic acid  
(PFNA),"19","ng/L","U","7.7","DL","","TRG","","","23","LOQ","YES",-99","","259.8","1.0","19","","  
"NAWC-091117-FRB-010","537","RES","320-31468-20","TALSAC","STL00993","13C2  
PFHxA","32","ng/L","","-99","DL","","SURR","83","","-99","LOQ","YES","38.5","","259.8","1.0","0","","  
"NAWC-091117-FRB-010","537","RES","320-31468-20","TALSAC","STL00996","13C2  
PFDA","37","ng/L","","-99","DL","","SURR","97","","-99","LOQ","YES","38.5","","259.8","1.0","0","","  
"NAWC-091117-RW-162","537","RES","320-31468-21","TALSAC","1763-23-1","Perfluorooctanesulfonic acid  
(PFOS),"33","ng/L","J M","6.5","DL","","TRG","","","38","LOQ","YES",-99","","262.9","1.00","15","","  
"NAWC-091117-RW-162","537","RES","320-31468-21","TALSAC","335-67-1","Perfluorooctanoic acid  
(PFOA),"15","ng/L","J","2.7","DL","","TRG","","","19","LOQ","YES",-99","","262.9","1.00","7.6","","  
"NAWC-091117-RW-162","537","RES","320-31468-21","TALSAC","355-46-4","Perfluorohexanesulfonic acid  
(PFHxS),"13","ng/L","J","5.2","DL","","TRG","","","29","LOQ","YES",-99","","262.9","1.00","11","","  
"NAWC-091117-RW-162","537","RES","320-31468-21","TALSAC","375-73-5","Perfluorobutanesulfonic acid

(PFBS)", "34", "ng/L", "U", "15", "DL", "", "TRG", "", "", "86", "LOQ", "YES", "-99", "", "262.9", "1.00", "34", ""  
"NAWC-091117-RW-162", "537", "RES", "320-31468-21", "TALSAC", "375-85-9", "Perfluoroheptanoic acid  
(PFHpA)", "5.4", "ng/L", "J", "1.8", "DL", "", "TRG", "", "", "9.5", "LOQ", "YES", "-99", "", "262.9", "1.00", "3.8", ""  
"NAWC-091117-RW-162", "537", "RES", "320-31468-21", "TALSAC", "375-95-1", "Perfluorononanoic acid  
(PFNA)", "19", "ng/L", "U", "7.6", "DL", "", "TRG", "", "", "23", "LOQ", "YES", "-99", "", "262.9", "1.00", "19", ""  
"NAWC-091117-RW-162", "537", "RES", "320-31468-21", "TALSAC", "STL00993", "13C2  
PFHxA", "30", "ng/L", "", "-99", "DL", "", "SURR", "78", "", "-99", "LOQ", "YES", "38.0", "", "262.9", "1.00", "0", ""  
"NAWC-091117-RW-162", "537", "RES", "320-31468-21", "TALSAC", "STL00996", "13C2  
PFDA", "42", "ng/L", "", "-99", "DL", "", "SURR", "111", "", "-99", "LOQ", "YES", "38.0", "", "262.9", "1.00", "0", ""  
"NAWC-091117-FRB-162", "537", "RES", "320-31468-22", "TALSAC", "1763-23-1", "Perfluorooctanesulfonic acid  
(PFOS)", "16", "ng/L", "U", "6.9", "DL", "", "TRG", "", "", "40", "LOQ", "YES", "-99", "", "247.3", "1.00", "16", ""  
"NAWC-091117-FRB-162", "537", "RES", "320-31468-22", "TALSAC", "335-67-1", "Perfluorooctanoic acid  
(PFOA)", "8.1", "ng/L", "U", "2.8", "DL", "", "TRG", "", "", "20", "LOQ", "YES", "-99", "", "247.3", "1.00", "8.1", ""  
"NAWC-091117-FRB-162", "537", "RES", "320-31468-22", "TALSAC", "355-46-4", "Perfluorohexanesulfonic acid  
(PFHxS)", "12", "ng/L", "U", "5.6", "DL", "", "TRG", "", "", "30", "LOQ", "YES", "-99", "", "247.3", "1.00", "12", ""  
"NAWC-091117-FRB-162", "537", "RES", "320-31468-22", "TALSAC", "375-73-5", "Perfluorobutanesulfonic acid  
(PFBS)", "36", "ng/L", "U", "16", "DL", "", "TRG", "", "", "91", "LOQ", "YES", "-99", "", "247.3", "1.00", "36", ""  
"NAWC-091117-FRB-162", "537", "RES", "320-31468-22", "TALSAC", "375-85-9", "Perfluoroheptanoic acid  
(PFHpA)", "4.0", "ng/L", "U", "1.9", "DL", "", "TRG", "", "", "10", "LOQ", "YES", "-99", "", "247.3", "1.00", "4.0", ""  
"NAWC-091117-FRB-162", "537", "RES", "320-31468-22", "TALSAC", "375-95-1", "Perfluorononanoic acid  
(PFNA)", "20", "ng/L", "U", "8.1", "DL", "", "TRG", "", "", "24", "LOQ", "YES", "-99", "", "247.3", "1.00", "20", ""  
"NAWC-091117-FRB-162", "537", "RES", "320-31468-22", "TALSAC", "STL00993", "13C2  
PFHxA", "37", "ng/L", "", "-99", "DL", "", "SURR", "91", "", "-99", "LOQ", "YES", "40.4", "", "247.3", "1.00", "0", ""  
"NAWC-091117-FRB-162", "537", "RES", "320-31468-22", "TALSAC", "STL00996", "13C2  
PFDA", "52", "ng/L", "", "-99", "DL", "", "SURR", "129", "", "-99", "LOQ", "YES", "40.4", "", "247.3", "1.00", "0", ""  
"WGNA-091117-DUP09", "537", "RES", "320-31468-23", "TALSAC", "1763-23-1", "Perfluorooctanesulfonic acid  
(PFOS)", "15", "ng/L", "U M", "6.5", "DL", "", "TRG", "", "", "38", "LOQ", "YES", "-99", "", "260", "1.00", "15", ""  
"WGNA-091117-DUP09", "537", "RES", "320-31468-23", "TALSAC", "335-67-1", "Perfluorooctanoic acid  
(PFOA)", "4.5", "ng/L", "J", "2.7", "DL", "", "TRG", "", "", "19", "LOQ", "YES", "-99", "", "260", "1.00", "7.7", ""  
"WGNA-091117-DUP09", "537", "RES", "320-31468-23", "TALSAC", "355-46-4", "Perfluorohexanesulfonic acid  
(PFHxS)", "12", "ng/L", "U", "5.3", "DL", "", "TRG", "", "", "29", "LOQ", "YES", "-99", "", "260", "1.00", "12", ""  
"WGNA-091117-DUP09", "537", "RES", "320-31468-23", "TALSAC", "375-73-5", "Perfluorobutanesulfonic acid  
(PFBS)", "35", "ng/L", "U", "15", "DL", "", "TRG", "", "", "87", "LOQ", "YES", "-99", "", "260", "1.00", "35", ""  
"WGNA-091117-DUP09", "537", "RES", "320-31468-23", "TALSAC", "375-85-9", "Perfluoroheptanoic acid  
(PFHpA)", "3.8", "ng/L", "U M", "1.8", "DL", "", "TRG", "", "", "9.6", "LOQ", "YES", "-99", "", "260", "1.00", "3.8", ""  
"WGNA-091117-DUP09", "537", "RES", "320-31468-23", "TALSAC", "375-95-1", "Perfluorononanoic acid  
(PFNA)", "19", "ng/L", "U", "7.7", "DL", "", "TRG", "", "", "23", "LOQ", "YES", "-99", "", "260", "1.00", "19", ""  
"WGNA-091117-DUP09", "537", "RES", "320-31468-23", "TALSAC", "STL00993", "13C2  
PFHxA", "29", "ng/L", "", "-99", "DL", "", "SURR", "75", "", "-99", "LOQ", "YES", "38.5", "", "260", "1.00", "0", ""  
"WGNA-091117-DUP09", "537", "RES", "320-31468-23", "TALSAC", "STL00996", "13C2  
PFDA", "48", "ng/L", "", "-99", "DL", "", "SURR", "125", "", "-99", "LOQ", "YES", "38.5", "", "260", "1.00", "0", ""  
"NAWC-091117-RW-060", "537", "RES", "320-31468-3", "TALSAC", "1763-23-1", "Perfluorooctanesulfonic acid  
(PFOS)", "27", "ng/L", "J M", "6.5", "DL", "", "TRG", "", "", "38", "LOQ", "YES", "-99", "", "261.7", "1.0", "15", ""  
"NAWC-091117-RW-060", "537", "RES", "320-31468-3", "TALSAC", "335-67-1", "Perfluorooctanoic acid  
(PFOA)", "17", "ng/L", "J", "2.7", "DL", "", "TRG", "", "", "19", "LOQ", "YES", "-99", "", "261.7", "1.0", "7.6", ""  
"NAWC-091117-RW-060", "537", "RES", "320-31468-3", "TALSAC", "355-46-4", "Perfluorohexanesulfonic acid  
(PFHxS)", "9.9", "ng/L", "J", "5.3", "DL", "", "TRG", "", "", "29", "LOQ", "YES", "-99", "", "261.7", "1.0", "11", ""  
"NAWC-091117-RW-060", "537", "RES", "320-31468-3", "TALSAC", "375-73-5", "Perfluorobutanesulfonic acid  
(PFBS)", "34", "ng/L", "U", "15", "DL", "", "TRG", "", "", "86", "LOQ", "YES", "-99", "", "261.7", "1.0", "34", ""  
"NAWC-091117-RW-060", "537", "RES", "320-31468-3", "TALSAC", "375-85-9", "Perfluoroheptanoic acid  
(PFHpA)", "3.9", "ng/L", "J", "1.8", "DL", "", "TRG", "", "", "9.6", "LOQ", "YES", "-99", "", "261.7", "1.0", "3.8", ""  
"NAWC-091117-RW-060", "537", "RES", "320-31468-3", "TALSAC", "375-95-1", "Perfluorononanoic acid  
(PFNA)", "19", "ng/L", "U", "7.6", "DL", "", "TRG", "", "", "23", "LOQ", "YES", "-99", "", "261.7", "1.0", "19", ""  
"NAWC-091117-RW-060", "537", "RES", "320-31468-3", "TALSAC", "STL00993", "13C2

PFHxA,"27","ng/L","",-99,"DL","","SURR","71","",-99,"LOQ","YES","38.2","","261.7","1.0","0",""  
"NAWC-091117-RW-060","537","RES","320-31468-3","TALSAC","STL00996","13C2  
PFDA,"43","ng/L","",-99,"DL","","SURR","114","",-99,"LOQ","YES","38.2","","261.7","1.0","0",""  
"NAWC-091117-FRB-060","537","RES","320-31468-4","TALSAC","1763-23-1","Perfluorooctanesulfonic acid  
(PFOS)","15","ng/L","U","6.5","DL","","TRG","","","38","LOQ","YES","-99","","259.9","1.0","15",""  
"NAWC-091117-FRB-060","537","RES","320-31468-4","TALSAC","335-67-1","Perfluorooctanoic acid  
(PFOA)","7.7","ng/L","U","2.7","DL","","TRG","","","19","LOQ","YES","-99","","259.9","1.0","7.7",""  
"NAWC-091117-FRB-060","537","RES","320-31468-4","TALSAC","355-46-4","Perfluorohexanesulfonic acid  
(PFHxS)","12","ng/L","U","5.3","DL","","TRG","","","29","LOQ","YES","-99","","259.9","1.0","12",""  
"NAWC-091117-FRB-060","537","RES","320-31468-4","TALSAC","375-73-5","Perfluorobutanesulfonic acid  
(PFBS)","35","ng/L","U","15","DL","","TRG","","","87","LOQ","YES","-99","","259.9","1.0","35",""  
"NAWC-091117-FRB-060","537","RES","320-31468-4","TALSAC","375-85-9","Perfluoroheptanoic acid  
(PFHpA)","3.8","ng/L","U","1.8","DL","","TRG","","","9.6","LOQ","YES","-99","","259.9","1.0","3.8",""  
"NAWC-091117-FRB-060","537","RES","320-31468-4","TALSAC","375-95-1","Perfluorononanoic acid  
(PFNA)","19","ng/L","U","7.7","DL","","TRG","","","23","LOQ","YES","-99","","259.9","1.0","19",""  
"NAWC-091117-FRB-060","537","RES","320-31468-4","TALSAC","STL00993","13C2  
PFHxA,"33","ng/L","",-99,"DL","","SURR","86","",-99,"LOQ","YES","38.5","","259.9","1.0","0",""  
"NAWC-091117-FRB-060","537","RES","320-31468-4","TALSAC","STL00996","13C2  
PFDA,"41","ng/L","",-99,"DL","","SURR","107","",-99,"LOQ","YES","38.5","","259.9","1.0","0",""  
"NAWC-091117-RW-314","537","RES","320-31468-5","TALSAC","1763-23-1","Perfluorooctanesulfonic acid  
(PFOS)","15","ng/L","J M","6.5","DL","","TRG","","","38","LOQ","YES","-99","","262.7","1.0","15",""  
"NAWC-091117-RW-314","537","RES","320-31468-5","TALSAC","335-67-1","Perfluorooctanoic acid  
(PFOA)","17","ng/L","J","2.7","DL","","TRG","","","19","LOQ","YES","-99","","262.7","1.0","7.6",""  
"NAWC-091117-RW-314","537","RES","320-31468-5","TALSAC","355-46-4","Perfluorohexanesulfonic acid  
(PFHxS)","11","ng/L","U","5.2","DL","","TRG","","","29","LOQ","YES","-99","","262.7","1.0","11",""  
"NAWC-091117-RW-314","537","RES","320-31468-5","TALSAC","375-73-5","Perfluorobutanesulfonic acid  
(PFBS)","34","ng/L","U","15","DL","","TRG","","","86","LOQ","YES","-99","","262.7","1.0","34",""  
"NAWC-091117-RW-314","537","RES","320-31468-5","TALSAC","375-85-9","Perfluoroheptanoic acid  
(PFHpA)","4.4","ng/L","J","1.8","DL","","TRG","","","9.5","LOQ","YES","-99","","262.7","1.0","3.8",""  
"NAWC-091117-RW-314","537","RES","320-31468-5","TALSAC","375-95-1","Perfluorononanoic acid  
(PFNA)","19","ng/L","U","7.6","DL","","TRG","","","23","LOQ","YES","-99","","262.7","1.0","19",""  
"NAWC-091117-RW-314","537","RES","320-31468-5","TALSAC","STL00993","13C2  
PFHxA,"28","ng/L","",-99,"DL","","SURR","72","",-99,"LOQ","YES","38.1","","262.7","1.0","0",""  
"NAWC-091117-RW-314","537","RES","320-31468-5","TALSAC","STL00996","13C2  
PFDA,"39","ng/L","",-99,"DL","","SURR","104","",-99,"LOQ","YES","38.1","","262.7","1.0","0",""  
"NAWC-091117-FRB-314","537","RES","320-31468-6","TALSAC","1763-23-1","Perfluorooctanesulfonic acid  
(PFOS)","15","ng/L","U","6.4","DL","","TRG","","","38","LOQ","YES","-99","","265.6","1.0","15",""  
"NAWC-091117-FRB-314","537","RES","320-31468-6","TALSAC","335-67-1","Perfluorooctanoic acid  
(PFOA)","7.5","ng/L","U","2.6","DL","","TRG","","","19","LOQ","YES","-99","","265.6","1.0","7.5",""  
"NAWC-091117-FRB-314","537","RES","320-31468-6","TALSAC","355-46-4","Perfluorohexanesulfonic acid  
(PFHxS)","11","ng/L","U","5.2","DL","","TRG","","","28","LOQ","YES","-99","","265.6","1.0","11",""  
"NAWC-091117-FRB-314","537","RES","320-31468-6","TALSAC","375-73-5","Perfluorobutanesulfonic acid  
(PFBS)","34","ng/L","U","15","DL","","TRG","","","85","LOQ","YES","-99","","265.6","1.0","34",""  
"NAWC-091117-FRB-314","537","RES","320-31468-6","TALSAC","375-85-9","Perfluoroheptanoic acid  
(PFHpA)","3.8","ng/L","U","1.8","DL","","TRG","","","9.4","LOQ","YES","-99","","265.6","1.0","3.8",""  
"NAWC-091117-FRB-314","537","RES","320-31468-6","TALSAC","375-95-1","Perfluorononanoic acid  
(PFNA)","19","ng/L","U","7.5","DL","","TRG","","","23","LOQ","YES","-99","","265.6","1.0","19",""  
"NAWC-091117-FRB-314","537","RES","320-31468-6","TALSAC","STL00993","13C2  
PFHxA,"31","ng/L","",-99,"DL","","SURR","82","",-99,"LOQ","YES","37.7","","265.6","1.0","0",""  
"NAWC-091117-FRB-314","537","RES","320-31468-6","TALSAC","STL00996","13C2  
PFDA,"39","ng/L","",-99,"DL","","SURR","102","",-99,"LOQ","YES","37.7","","265.6","1.0","0",""  
"NAWC-091117-RW-258","537","RES","320-31468-7","TALSAC","1763-23-1","Perfluorooctanesulfonic acid  
(PFOS)","18","ng/L","J M","6.4","DL","","TRG","","","37","LOQ","YES","-99","","267","1.0","15",""  
"NAWC-091117-RW-258","537","RES","320-31468-7","TALSAC","335-67-1","Perfluorooctanoic acid

(PFOA)", "21", "ng/L", "", "2.6", "DL", "", "TRG", "", "", "19", "LOQ", "YES", "-99", "", "267", "1.0", "7.5", ""  
"NAWC-091117-RW-258", "537", "RES", "320-31468-7", "TALSAC", "355-46-4", "Perfluorohexanesulfonic acid  
(PFHxS)", "11", "ng/L", "U", "5.1", "DL", "", "TRG", "", "", "28", "LOQ", "YES", "-99", "", "267", "1.0", "11", ""  
"NAWC-091117-RW-258", "537", "RES", "320-31468-7", "TALSAC", "375-73-5", "Perfluorobutanesulfonic acid  
(PFBS)", "34", "ng/L", "U", "15", "DL", "", "TRG", "", "", "84", "LOQ", "YES", "-99", "", "267", "1.0", "34", ""  
"NAWC-091117-RW-258", "537", "RES", "320-31468-7", "TALSAC", "375-85-9", "Perfluoroheptanoic acid  
(PFHpA)", "7.7", "ng/L", "J", "1.8", "DL", "", "TRG", "", "", "9.4", "LOQ", "YES", "-99", "", "267", "1.0", "3.7", ""  
"NAWC-091117-RW-258", "537", "RES", "320-31468-7", "TALSAC", "375-95-1", "Perfluorononanoic acid  
(PFNA)", "12", "ng/L", "J", "7.5", "DL", "", "TRG", "", "", "22", "LOQ", "YES", "-99", "", "267", "1.0", "19", ""  
"NAWC-091117-RW-258", "537", "RES", "320-31468-7", "TALSAC", "STL00993", "13C2  
PFHxA", "27", "ng/L", "", "-99", "DL", "", "SURR", "72", "", "-99", "LOQ", "YES", "37.5", "", "267", "1.0", "0", ""  
"NAWC-091117-RW-258", "537", "RES", "320-31468-7", "TALSAC", "STL00996", "13C2  
PFDA", "37", "ng/L", "", "-99", "DL", "", "SURR", "98", "", "-99", "LOQ", "YES", "37.5", "", "267", "1.0", "0", ""  
"NAWC-091117-FRB-258", "537", "RES", "320-31468-8", "TALSAC", "1763-23-1", "Perfluorooctanesulfonic acid  
(PFOS)", "15", "ng/L", "U", "6.5", "DL", "", "TRG", "", "", "38", "LOQ", "YES", "-99", "", "261.6", "1.0", "15", ""  
"NAWC-091117-FRB-258", "537", "RES", "320-31468-8", "TALSAC", "335-67-1", "Perfluorooctanoic acid  
(PFOA)", "7.6", "ng/L", "U", "2.7", "DL", "", "TRG", "", "", "19", "LOQ", "YES", "-99", "", "261.6", "1.0", "7.6", ""  
"NAWC-091117-FRB-258", "537", "RES", "320-31468-8", "TALSAC", "355-46-4", "Perfluorohexanesulfonic acid  
(PFHxS)", "11", "ng/L", "U", "5.3", "DL", "", "TRG", "", "", "29", "LOQ", "YES", "-99", "", "261.6", "1.0", "11", ""  
"NAWC-091117-FRB-258", "537", "RES", "320-31468-8", "TALSAC", "375-73-5", "Perfluorobutanesulfonic acid  
(PFBS)", "34", "ng/L", "U", "15", "DL", "", "TRG", "", "", "86", "LOQ", "YES", "-99", "", "261.6", "1.0", "34", ""  
"NAWC-091117-FRB-258", "537", "RES", "320-31468-8", "TALSAC", "375-85-9", "Perfluoroheptanoic acid  
(PFHpA)", "3.8", "ng/L", "U", "1.8", "DL", "", "TRG", "", "", "9.6", "LOQ", "YES", "-99", "", "261.6", "1.0", "3.8", ""  
"NAWC-091117-FRB-258", "537", "RES", "320-31468-8", "TALSAC", "375-95-1", "Perfluorononanoic acid  
(PFNA)", "19", "ng/L", "U", "7.6", "DL", "", "TRG", "", "", "23", "LOQ", "YES", "-99", "", "261.6", "1.0", "19", ""  
"NAWC-091117-FRB-258", "537", "RES", "320-31468-8", "TALSAC", "STL00993", "13C2  
PFHxA", "33", "ng/L", "", "-99", "DL", "", "SURR", "86", "", "-99", "LOQ", "YES", "38.2", "", "261.6", "1.0", "0", ""  
"NAWC-091117-FRB-258", "537", "RES", "320-31468-8", "TALSAC", "STL00996", "13C2  
PFDA", "39", "ng/L", "", "-99", "DL", "", "SURR", "101", "", "-99", "LOQ", "YES", "38.2", "", "261.6", "1.0", "0", ""  
"NAWC-091117-RW-048", "537", "RES", "320-31468-9", "TALSAC", "1763-23-1", "Perfluorooctanesulfonic acid  
(PFOS)", "15", "ng/L", "U M", "6.4", "DL", "", "TRG", "", "", "38", "LOQ", "YES", "-99", "", "263.9", "1.0", "15", ""  
"NAWC-091117-RW-048", "537", "RES", "320-31468-9", "TALSAC", "335-67-1", "Perfluorooctanoic acid  
(PFOA)", "4.5", "ng/L", "J M", "2.7", "DL", "", "TRG", "", "", "19", "LOQ", "YES", "-99", "", "263.9", "1.0", "7.6", ""  
"NAWC-091117-RW-048", "537", "RES", "320-31468-9", "TALSAC", "355-46-4", "Perfluorohexanesulfonic acid  
(PFHxS)", "11", "ng/L", "U", "5.2", "DL", "", "TRG", "", "", "28", "LOQ", "YES", "-99", "", "263.9", "1.0", "11", ""  
"NAWC-091117-RW-048", "537", "RES", "320-31468-9", "TALSAC", "375-73-5", "Perfluorobutanesulfonic acid  
(PFBS)", "34", "ng/L", "U", "15", "DL", "", "TRG", "", "", "85", "LOQ", "YES", "-99", "", "263.9", "1.0", "34", ""  
"NAWC-091117-RW-048", "537", "RES", "320-31468-9", "TALSAC", "375-85-9", "Perfluoroheptanoic acid  
(PFHpA)", "3.8", "ng/L", "U", "1.8", "DL", "", "TRG", "", "", "9.5", "LOQ", "YES", "-99", "", "263.9", "1.0", "3.8", ""  
"NAWC-091117-RW-048", "537", "RES", "320-31468-9", "TALSAC", "375-95-1", "Perfluorononanoic acid  
(PFNA)", "19", "ng/L", "U", "7.6", "DL", "", "TRG", "", "", "23", "LOQ", "YES", "-99", "", "263.9", "1.0", "19", ""  
"NAWC-091117-RW-048", "537", "RES", "320-31468-9", "TALSAC", "STL00993", "13C2  
PFHxA", "28", "ng/L", "", "-99", "DL", "", "SURR", "74", "", "-99", "LOQ", "YES", "37.9", "", "263.9", "1.0", "0", ""  
"NAWC-091117-RW-048", "537", "RES", "320-31468-9", "TALSAC", "STL00996", "13C2  
PFDA", "42", "ng/L", "", "-99", "DL", "", "SURR", "111", "", "-99", "LOQ", "YES", "37.9", "", "263.9", "1.0", "0", ""  
"LCS 320-184382/2-A", "537", "RES", "LCS 320-184382/2-A", "TALSAC", "1763-23-1", "Perfluorooctanesulfonic acid  
(PFOS)", "198", "ng/L", "M", "6.8", "DL", "", "SPK", "89", "", "40", "LOQ", "YES", "222", "", "250", "1.0", "16", ""  
"LCS 320-184382/2-A", "537", "RES", "LCS 320-184382/2-A", "TALSAC", "335-67-1", "Perfluorooctanoic acid  
(PFOA)", "103", "ng/L", "", "2.8", "DL", "", "SPK", "93", "", "20", "LOQ", "YES", "111", "", "250", "1.0", "8.0", ""  
"LCS 320-184382/2-A", "537", "RES", "LCS 320-184382/2-A", "TALSAC", "355-46-4", "Perfluorohexanesulfonic acid  
(PFHxS)", "150", "ng/L", "", "5.5", "DL", "", "SPK", "90", "", "30", "LOQ", "YES", "167", "", "250", "1.0", "12", ""  
"LCS 320-184382/2-A", "537", "RES", "LCS 320-184382/2-A", "TALSAC", "375-73-5", "Perfluorobutanesulfonic acid  
(PFBS)", "408", "ng/L", "", "16", "DL", "", "SPK", "82", "", "90", "LOQ", "YES", "500", "", "250", "1.0", "36", ""  
"LCS 320-184382/2-A", "537", "RES", "LCS 320-184382/2-A", "TALSAC", "375-85-9", "Perfluoroheptanoic acid

(PFHpA),"50.5","ng/L","", "1.9","DL","", "SPK","91","", "10","LOQ","YES","55.6","", "250","1.0","4.0",""  
"LCS 320-184382/2-A","537","RES","LCS 320-184382/2-A","TALSAC","375-95-1","Perfluorononanoic acid  
(PFNA),"99.7","ng/L","", "8.0","DL","", "SPK","90","", "24","LOQ","YES","111","", "250","1.0","20",""  
"LCS 320-184382/2-A","537","RES","LCS 320-184382/2-A","TALSAC","STL00993","13C2  
PFHxA","36.2","ng/L","", "-99","DL","", "SURR","91","", "-99","LOQ","YES","40.0","", "250","1.0","0",""  
"LCS 320-184382/2-A","537","RES","LCS 320-184382/2-A","TALSAC","STL00996","13C2  
PFDA","45.8","ng/L","", "-99","DL","", "SURR","115","", "-99","LOQ","YES","40.0","", "250","1.0","0",""  
"LCSD 320-184382/3-A","537","RES","LCSD 320-184382/3-A","TALSAC","1763-23-1","Perfluorooctanesulfonic  
acid (PFOS),"188","ng/L","M","6.8","DL","", "SPK","84","5","40","LOQ","YES","222","LCS 320-184382/2-  
A","250","1.0","16",""  
"LCSD 320-184382/3-A","537","RES","LCSD 320-184382/3-A","TALSAC","335-67-1","Perfluorooctanoic acid  
(PFOA),"96.8","ng/L","", "2.8","DL","", "SPK","87","7","20","LOQ","YES","111","LCS 320-184382/2-  
A","250","1.0","8.0",""  
"LCSD 320-184382/3-A","537","RES","LCSD 320-184382/3-A","TALSAC","355-46-4","Perfluorohexanesulfonic  
acid (PFHxS),"143","ng/L","", "5.5","DL","", "SPK","86","5","30","LOQ","YES","167","LCS 320-184382/2-  
A","250","1.0","12",""  
"LCSD 320-184382/3-A","537","RES","LCSD 320-184382/3-A","TALSAC","375-73-5","Perfluorobutanesulfonic acid  
(PFBS),"403","ng/L","", "16","DL","", "SPK","81","1","90","LOQ","YES","500","LCS 320-184382/2-  
A","250","1.0","36",""  
"LCSD 320-184382/3-A","537","RES","LCSD 320-184382/3-A","TALSAC","375-85-9","Perfluoroheptanoic acid  
(PFHpA),"48.7","ng/L","", "1.9","DL","", "SPK","88","3","10","LOQ","YES","55.6","LCS 320-184382/2-  
A","250","1.0","4.0",""  
"LCSD 320-184382/3-A","537","RES","LCSD 320-184382/3-A","TALSAC","375-95-1","Perfluorononanoic acid  
(PFNA),"93.6","ng/L","", "8.0","DL","", "SPK","84","6","24","LOQ","YES","111","LCS 320-184382/2-  
A","250","1.0","20",""  
"LCSD 320-184382/3-A","537","RES","LCSD 320-184382/3-A","TALSAC","STL00993","13C2  
PFHxA","34.3","ng/L","", "-99","DL","", "SURR","86","", "-99","LOQ","YES","40.0","LCS 320-184382/2-  
A","250","1.0","0",""  
"LCSD 320-184382/3-A","537","RES","LCSD 320-184382/3-A","TALSAC","STL00996","13C2  
PFDA","43.9","ng/L","", "-99","DL","", "SURR","110","", "-99","LOQ","YES","40.0","LCS 320-184382/2-  
A","250","1.0","0",""  
"LLCS 320-184385/2-A","537","RES","LLCS 320-184385/2-A","TALSAC","1763-23-1","Perfluorooctanesulfonic  
acid (PFOS),"36.6","ng/L","J M","6.8","DL","", "SPK","91","", "40","LOQ","YES","40.0","", "250","1.00","16",""  
"LLCS 320-184385/2-A","537","RES","LLCS 320-184385/2-A","TALSAC","335-67-1","Perfluorooctanoic acid  
(PFOA),"18.4","ng/L","J","2.8","DL","", "SPK","92","", "20","LOQ","YES","20.0","", "250","1.00","8.0",""  
"LLCS 320-184385/2-A","537","RES","LLCS 320-184385/2-A","TALSAC","355-46-4","Perfluorohexanesulfonic acid  
(PFHxS),"28.9","ng/L","J","5.5","DL","", "SPK","96","", "30","LOQ","YES","30.0","", "250","1.00","12",""  
"LLCS 320-184385/2-A","537","RES","LLCS 320-184385/2-A","TALSAC","375-73-5","Perfluorobutanesulfonic acid  
(PFBS),"86.1","ng/L","J","16","DL","", "SPK","96","", "90","LOQ","YES","90.0","", "250","1.00","36",""  
"LLCS 320-184385/2-A","537","RES","LLCS 320-184385/2-A","TALSAC","375-85-9","Perfluoroheptanoic acid  
(PFHpA),"10.2","ng/L","", "1.9","DL","", "SPK","102","", "10","LOQ","YES","10.0","", "250","1.00","4.0",""  
"LLCS 320-184385/2-A","537","RES","LLCS 320-184385/2-A","TALSAC","375-95-1","Perfluorononanoic acid  
(PFNA),"18.5","ng/L","J","8.0","DL","", "SPK","93","", "24","LOQ","YES","20.0","", "250","1.00","20",""  
"LLCS 320-184385/2-A","537","RES","LLCS 320-184385/2-A","TALSAC","STL00993","13C2  
PFHxA","35.9","ng/L","", "-99","DL","", "SURR","90","", "-99","LOQ","YES","40.0","", "250","1.00","0",""  
"LLCS 320-184385/2-A","537","RES","LLCS 320-184385/2-A","TALSAC","STL00996","13C2  
PFDA","45.0","ng/L","", "-99","DL","", "SURR","113","", "-99","LOQ","YES","40.0","", "250","1.00","0",""  
"LLCSD 320-184385/3-A","537","RES","LLCSD 320-184385/3-A","TALSAC","1763-23-1","Perfluorooctanesulfonic  
acid (PFOS),"36.2","ng/L","J M","6.8","DL","", "SPK","90","1","40","LOQ","YES","40.0","LLCS 320-184385/2-  
A","250","1.00","16",""  
"LLCSD 320-184385/3-A","537","RES","LLCSD 320-184385/3-A","TALSAC","335-67-1","Perfluorooctanoic acid  
(PFOA),"18.7","ng/L","J","2.8","DL","", "SPK","93","1","20","LOQ","YES","20.0","LLCS 320-184385/2-  
A","250","1.00","8.0",""  
"LLCSD 320-184385/3-A","537","RES","LLCSD 320-184385/3-A","TALSAC","355-46-4","Perfluorohexanesulfonic

acid (PFHxS)", "29.4", "ng/L", "J", "5.5", "DL", "", "SPK", "98", "2", "30", "LOQ", "YES", "30.0", "LLCS 320-184385/2-A", "250", "1.00", "12", ""

"LLCSD 320-184385/3-A", "537", "RES", "LLCSD 320-184385/3-A", "TALSAC", "375-73-5", "Perfluorobutanesulfonic acid (PFBS)", "89.0", "ng/L", "J", "16", "DL", "", "SPK", "99", "3", "90", "LOQ", "YES", "90.0", "LLCS 320-184385/2-A", "250", "1.00", "36", ""

"LLCSD 320-184385/3-A", "537", "RES", "LLCSD 320-184385/3-A", "TALSAC", "375-85-9", "Perfluoroheptanoic acid (PFHpA)", "10.8", "ng/L", "", "1.9", "DL", "", "SPK", "108", "6", "10", "LOQ", "YES", "10.0", "LLCS 320-184385/2-A", "250", "1.00", "4.0", ""

"LLCSD 320-184385/3-A", "537", "RES", "LLCSD 320-184385/3-A", "TALSAC", "375-95-1", "Perfluorononanoic acid (PFNA)", "19.0", "ng/L", "J", "8.0", "DL", "", "SPK", "95", "3", "24", "LOQ", "YES", "20.0", "LLCS 320-184385/2-A", "250", "1.00", "20", ""

"LLCSD 320-184385/3-A", "537", "RES", "LLCSD 320-184385/3-A", "TALSAC", "STL00993", "13C2 PFHxA", "37.0", "ng/L", "", "-99", "DL", "", "SURR", "93", "3", "-99", "LOQ", "YES", "40.0", "LLCS 320-184385/2-A", "250", "1.00", "0", ""

"LLCSD 320-184385/3-A", "537", "RES", "LLCSD 320-184385/3-A", "TALSAC", "STL00996", "13C2 PFDA", "49.5", "ng/L", "", "-99", "DL", "", "SURR", "124", "9", "-99", "LOQ", "YES", "40.0", "LLCS 320-184385/2-A", "250", "1.00", "0", ""

"MB 320-184382/1-A", "537", "RES", "MB 320-184382/1-A", "TALSAC", "1763-23-1", "Perfluorooctanesulfonic acid (PFOS)", "16", "ng/L", "U", "6.8", "DL", "", "TRG", "", "", "40", "LOQ", "YES", "-99", "", "250", "1.0", "16", ""

"MB 320-184382/1-A", "537", "RES", "MB 320-184382/1-A", "TALSAC", "335-67-1", "Perfluorooctanoic acid (PFOA)", "8.0", "ng/L", "U", "2.8", "DL", "", "TRG", "", "", "20", "LOQ", "YES", "-99", "", "250", "1.0", "8.0", ""

"MB 320-184382/1-A", "537", "RES", "MB 320-184382/1-A", "TALSAC", "355-46-4", "Perfluorohexanesulfonic acid (PFHxS)", "12", "ng/L", "U", "5.5", "DL", "", "TRG", "", "", "30", "LOQ", "YES", "-99", "", "250", "1.0", "12", ""

"MB 320-184382/1-A", "537", "RES", "MB 320-184382/1-A", "TALSAC", "375-73-5", "Perfluorobutanesulfonic acid (PFBS)", "36", "ng/L", "U", "16", "DL", "", "TRG", "", "", "90", "LOQ", "YES", "-99", "", "250", "1.0", "36", ""

"MB 320-184382/1-A", "537", "RES", "MB 320-184382/1-A", "TALSAC", "375-85-9", "Perfluoroheptanoic acid (PFHpA)", "4.0", "ng/L", "U", "1.9", "DL", "", "TRG", "", "", "10", "LOQ", "YES", "-99", "", "250", "1.0", "4.0", ""

"MB 320-184382/1-A", "537", "RES", "MB 320-184382/1-A", "TALSAC", "375-95-1", "Perfluorononanoic acid (PFNA)", "20", "ng/L", "U", "8.0", "DL", "", "TRG", "", "", "24", "LOQ", "YES", "-99", "", "250", "1.0", "20", ""

"MB 320-184382/1-A", "537", "RES", "MB 320-184382/1-A", "TALSAC", "STL00993", "13C2 PFHxA", "35.9", "ng/L", "", "-99", "DL", "", "SURR", "90", "", "-99", "LOQ", "YES", "40.0", "", "250", "1.0", "0", ""

"MB 320-184382/1-A", "537", "RES", "MB 320-184382/1-A", "TALSAC", "STL00996", "13C2 PFDA", "44.3", "ng/L", "", "-99", "DL", "", "SURR", "111", "", "-99", "LOQ", "YES", "40.0", "", "250", "1.0", "0", ""

"MB 320-184385/1-A", "537", "RES", "MB 320-184385/1-A", "TALSAC", "1763-23-1", "Perfluorooctanesulfonic acid (PFOS)", "16", "ng/L", "U", "6.8", "DL", "", "TRG", "", "", "40", "LOQ", "YES", "-99", "", "250", "1.00", "16", ""

"MB 320-184385/1-A", "537", "RES", "MB 320-184385/1-A", "TALSAC", "335-67-1", "Perfluorooctanoic acid (PFOA)", "8.0", "ng/L", "U", "2.8", "DL", "", "TRG", "", "", "20", "LOQ", "YES", "-99", "", "250", "1.00", "8.0", ""

"MB 320-184385/1-A", "537", "RES", "MB 320-184385/1-A", "TALSAC", "355-46-4", "Perfluorohexanesulfonic acid (PFHxS)", "12", "ng/L", "U", "5.5", "DL", "", "TRG", "", "", "30", "LOQ", "YES", "-99", "", "250", "1.00", "12", ""

"MB 320-184385/1-A", "537", "RES", "MB 320-184385/1-A", "TALSAC", "375-73-5", "Perfluorobutanesulfonic acid (PFBS)", "36", "ng/L", "U", "16", "DL", "", "TRG", "", "", "90", "LOQ", "YES", "-99", "", "250", "1.00", "36", ""

"MB 320-184385/1-A", "537", "RES", "MB 320-184385/1-A", "TALSAC", "375-85-9", "Perfluoroheptanoic acid (PFHpA)", "4.0", "ng/L", "U", "1.9", "DL", "", "TRG", "", "", "10", "LOQ", "YES", "-99", "", "250", "1.00", "4.0", ""

"MB 320-184385/1-A", "537", "RES", "MB 320-184385/1-A", "TALSAC", "375-95-1", "Perfluorononanoic acid (PFNA)", "20", "ng/L", "U", "8.0", "DL", "", "TRG", "", "", "24", "LOQ", "YES", "-99", "", "250", "1.00", "20", ""

"MB 320-184385/1-A", "537", "RES", "MB 320-184385/1-A", "TALSAC", "STL00993", "13C2 PFHxA", "34.7", "ng/L", "", "-99", "DL", "", "SURR", "87", "", "-99", "LOQ", "YES", "40.0", "", "250", "1.00", "0", ""

"MB 320-184385/1-A", "537", "RES", "MB 320-184385/1-A", "TALSAC", "STL00996", "13C2 PFDA", "57.4", "ng/L", "Q", "-99", "DL", "", "SURR", "143", "", "-99", "LOQ", "YES", "40.0", "", "250", "1.00", "0", ""

"Unknown", "Unknown", "NAWC-091117-RW-106", "09/11/2017 09:40", "AQ", "320-31468-1", "NM", "", "2.1", "537", "METHOD", "RES", "09/14/2017 09:17", "09/20/2017 04:49", "TALSAC", "COA", "WET", "NA", "1", "NA", "NA", "", "100", "320-184382", "320-184382", "NA", "320-185407", "320-31468-1", "09/12/2017 14:21", "09/13/2017 10:20", ""

"Unknown", "Unknown", "NAWC-091117-FRB-048", "09/11/2017 13:00", "AQ", "320-31468-



10","FB",,"2.1","537","METHOD","RES","09/14/2017 09:17","09/20/2017  
05:42","TALSAC","COA","WET","NA","1","NA","NA",,"100","320-184382","320-184382","NA","320-  
185408","320-31468-1","09/12/2017 14:21","09/13/2017 10:20",,"  
"Unknown","Unknown","NAWC-091117-RW-145","09/11/2017 13:35","AQ","320-31468-  
11","NM",,"2.1","537","METHOD","RES","09/14/2017 09:17","09/20/2017  
05:46","TALSAC","COA","WET","NA","1","NA","NA",,"100","320-184382","320-184382","NA","320-  
185408","320-31468-1","09/12/2017 14:21","09/13/2017 10:20",,"  
"Unknown","Unknown","NAWC-091117-FRB-145","09/11/2017 13:30","AQ","320-31468-  
12","FB",,"2.1","537","METHOD","RES","09/14/2017 09:17","09/20/2017  
05:51","TALSAC","COA","WET","NA","1","NA","NA",,"100","320-184382","320-184382","NA","320-  
185408","320-31468-1","09/12/2017 14:21","09/13/2017 10:20",,"  
"Unknown","Unknown","NAWC-091117-RW-317","09/11/2017 14:00","AQ","320-31468-  
13","NM",,"2.1","537","METHOD","RES","09/14/2017 09:17","09/20/2017  
05:56","TALSAC","COA","WET","NA","1","NA","NA",,"100","320-184382","320-184382","NA","320-  
185408","320-31468-1","09/12/2017 14:21","09/13/2017 10:20",,"  
"Unknown","Unknown","NAWC-091117-FRB-317","09/11/2017 13:55","AQ","320-31468-  
14","FB",,"2.1","537","METHOD","RES","09/14/2017 09:17","09/20/2017  
06:01","TALSAC","COA","WET","NA","1","NA","NA",,"100","320-184382","320-184382","NA","320-  
185408","320-31468-1","09/12/2017 14:21","09/13/2017 10:20",,"  
"Unknown","Unknown","NAWC-091117-RW-319","09/11/2017 14:25","AQ","320-31468-  
15","NM",,"2.1","537","METHOD","RES","09/14/2017 09:17","09/20/2017  
06:05","TALSAC","COA","WET","NA","1","NA","NA",,"100","320-184382","320-184382","NA","320-  
185408","320-31468-1","09/12/2017 14:21","09/13/2017 10:20",,"  
"Unknown","Unknown","NAWC-091117-FRB-319","09/11/2017 14:40","AQ","320-31468-  
16","FB",,"2.1","537","METHOD","RES","09/14/2017 09:17","09/20/2017  
06:10","TALSAC","COA","WET","NA","1","NA","NA",,"100","320-184382","320-184382","NA","320-  
185408","320-31468-1","09/12/2017 14:21","09/13/2017 10:20",,"  
"Unknown","Unknown","NAWC-091117-RW-321","09/11/2017 15:10","AQ","320-31468-  
17","NM",,"2.1","537","METHOD","RES","09/14/2017 09:17","09/20/2017  
06:15","TALSAC","COA","WET","NA","1","NA","NA",,"100","320-184382","320-184382","NA","320-  
185408","320-31468-1","09/12/2017 14:21","09/13/2017 10:20",,"  
"Unknown","Unknown","NAWC-091117-FRB-321","09/11/2017 15:05","AQ","320-31468-  
18","FB",,"2.1","537","METHOD","RES","09/14/2017 09:17","09/20/2017  
06:29","TALSAC","COA","WET","NA","1","NA","NA",,"100","320-184382","320-184382","NA","320-  
185409","320-31468-1","09/12/2017 14:21","09/13/2017 10:20",,"  
"Unknown","Unknown","NAWC-091117-RW-010","09/11/2017 15:45","AQ","320-31468-  
19","NM",,"2.1","537","METHOD","RES","09/14/2017 09:17","09/20/2017  
06:34","TALSAC","COA","WET","NA","1","NA","NA",,"100","320-184382","320-184382","NA","320-  
185409","320-31468-1","09/12/2017 14:21","09/13/2017 10:20",,"  
"Unknown","Unknown","NAWC-091117-FRB-106","09/11/2017 09:35","AQ","320-31468-  
2","FB",,"2.1","537","METHOD","RES","09/14/2017 09:17","09/20/2017  
04:54","TALSAC","COA","WET","NA","1","NA","NA",,"100","320-184382","320-184382","NA","320-  
185407","320-31468-1","09/12/2017 14:21","09/13/2017 10:20",,"  
"Unknown","Unknown","NAWC-091117-FRB-010","09/11/2017 15:40","AQ","320-31468-  
20","FB",,"2.1","537","METHOD","RES","09/14/2017 09:17","09/20/2017  
06:39","TALSAC","COA","WET","NA","1","NA","NA",,"100","320-184382","320-184382","NA","320-  
185409","320-31468-1","09/12/2017 14:21","09/13/2017 10:20",,"  
"Unknown","Unknown","NAWC-091117-RW-162","09/11/2017 11:20","AQ","320-31468-  
21","NM",,"2.1","537","METHOD","RES","09/14/2017 09:29","09/20/2017  
04:11","TALSAC","COA","WET","NA","1","NA","NA",,"100","320-184385","320-184385","NA","320-  
185406","320-31468-1","09/12/2017 14:21","09/13/2017 10:20",,"  
"Unknown","Unknown","NAWC-091117-FRB-162","09/11/2017 11:15","AQ","320-31468-  
22","FB",,"2.1","537","METHOD","RES","09/14/2017 09:29","09/20/2017  
04:16","TALSAC","COA","WET","NA","1","NA","NA",,"100","320-184385","320-184385","NA","320-



185406","320-31468-1","09/12/2017 14:21","09/13/2017 10:20",""  
"Unknown","Unknown","WGNA-091117-DUP09","09/11/2017 07:00","AQ","320-31468-  
23","FD","","2.1","537","METHOD","RES","09/14/2017 09:29","09/20/2017  
04:21","TALSAC","COA","WET","NA","1","NA","NA","","100","320-184385","320-184385","NA","320-  
185406","320-31468-1","09/12/2017 14:21","09/13/2017 10:20",""  
"Unknown","Unknown","NAWC-091117-RW-060","09/11/2017 09:55","AQ","320-31468-  
3","NM","","2.1","537","METHOD","RES","09/14/2017 09:17","09/20/2017  
04:59","TALSAC","COA","WET","NA","1","NA","NA","","100","320-184382","320-184382","NA","320-  
185407","320-31468-1","09/12/2017 14:21","09/13/2017 10:20",""  
"Unknown","Unknown","NAWC-091117-FRB-060","09/11/2017 09:50","AQ","320-31468-  
4","FB","","2.1","537","METHOD","RES","09/14/2017 09:17","09/20/2017  
05:04","TALSAC","COA","WET","NA","1","NA","NA","","100","320-184382","320-184382","NA","320-  
185407","320-31468-1","09/12/2017 14:21","09/13/2017 10:20",""  
"Unknown","Unknown","NAWC-091117-RW-314","09/11/2017 10:25","AQ","320-31468-  
5","NM","","2.1","537","METHOD","RES","09/14/2017 09:17","09/20/2017  
05:08","TALSAC","COA","WET","NA","1","NA","NA","","100","320-184382","320-184382","NA","320-  
185407","320-31468-1","09/12/2017 14:21","09/13/2017 10:20",""  
"Unknown","Unknown","NAWC-091117-FRB-314","09/11/2017 10:20","AQ","320-31468-  
6","FB","","2.1","537","METHOD","RES","09/14/2017 09:17","09/20/2017  
05:13","TALSAC","COA","WET","NA","1","NA","NA","","100","320-184382","320-184382","NA","320-  
185407","320-31468-1","09/12/2017 14:21","09/13/2017 10:20",""  
"Unknown","Unknown","NAWC-091117-RW-258","09/11/2017 11:00","AQ","320-31468-  
7","NM","","2.1","537","METHOD","RES","09/14/2017 09:17","09/20/2017  
05:18","TALSAC","COA","WET","NA","1","NA","NA","","100","320-184382","320-184382","NA","320-  
185407","320-31468-1","09/12/2017 14:21","09/13/2017 10:20",""  
"Unknown","Unknown","NAWC-091117-FRB-258","09/11/2017 10:55","AQ","320-31468-  
8","FB","","2.1","537","METHOD","RES","09/14/2017 09:17","09/20/2017  
05:32","TALSAC","COA","WET","NA","1","NA","NA","","100","320-184382","320-184382","NA","320-  
185408","320-31468-1","09/12/2017 14:21","09/13/2017 10:20",""  
"Unknown","Unknown","NAWC-091117-RW-048","09/11/2017 13:05","AQ","320-31468-  
9","NM","","2.1","537","METHOD","RES","09/14/2017 09:17","09/20/2017  
05:37","TALSAC","COA","WET","NA","1","NA","NA","","100","320-184382","320-184382","NA","320-  
185408","320-31468-1","09/12/2017 14:21","09/13/2017 10:20",""  
"Unknown","Unknown","LCS 320-184382/2-A","","AQ","LCS 320-184382/2-  
A","LCS","",-99","537","METHOD","RES","09/14/2017 09:17","09/20/2017  
04:40","TALSAC","COA","WET","NA","1","NA","NA","","100","320-184382","320-184382","NA","320-  
185407","320-31468-1","09/14/2017 09:17","09/13/2017 10:20",""  
"Unknown","Unknown","LCSD 320-184382/3-A","","AQ","LCSD 320-184382/3-  
A","LCSD","",-99","537","METHOD","RES","09/14/2017 09:17","09/20/2017  
04:45","TALSAC","COA","WET","NA","1","NA","NA","","100","320-184382","320-184382","NA","320-  
185407","320-31468-1","09/14/2017 09:17","09/13/2017 10:20",""  
"Unknown","Unknown","LLCS 320-184385/2-A","","AQ","LLCS 320-184385/2-  
A","LCS","",-99","537","METHOD","RES","09/14/2017 09:29","09/20/2017  
04:02","TALSAC","COA","WET","NA","1","NA","NA","","100","320-184385","320-184385","NA","320-  
185406","320-31468-1","09/14/2017 09:29","09/13/2017 10:20",""  
"Unknown","Unknown","LLCSD 320-184385/3-A","","AQ","LLCSD 320-184385/3-  
A","LCSD","",-99","537","METHOD","RES","09/14/2017 09:29","09/20/2017  
04:07","TALSAC","COA","WET","NA","1","NA","NA","","100","320-184385","320-184385","NA","320-  
185406","320-31468-1","09/14/2017 09:29","09/13/2017 10:20",""  
"Unknown","Unknown","MB 320-184382/1-A","","AQ","MB 320-184382/1-  
A","MB","",-99","537","METHOD","RES","09/14/2017 09:17","09/20/2017  
04:35","TALSAC","COA","WET","NA","1","NA","NA","","100","320-184382","320-184382","NA","320-  
185407","320-31468-1","09/14/2017 09:17","09/13/2017 10:20",""  
"Unknown","Unknown","MB 320-184385/1-A","","AQ","MB 320-184385/1-

A,"MB",,"-99","537","METHOD","RES","09/14/2017 09:29","09/20/2017  
03:57","TALSAC","COA","WET","NA","1","NA","NA",,"100","320-184385","320-184385","NA","320-  
185406","320-31468-1","09/14/2017 09:29","09/13/2017 10:20",,""



TO: A. FREBOWITZ DATE: OCTOBER 16, 2017  
FROM: TERRI L. SOLOMON COPIES: DV FILE  
SUBJECT: ORGANIC DATA VALIDATION –POLYFLUOROALKYL SUBSTANCES (PFAS)  
NAS JRB WILLOW GROVE  
SAMPLE DELIVERY GROUP (SDG) 320-31468-1

SAMPLES: 11/Field Reagent Blank (FRB)  
NAWC-091117-FRB-106 NAWC-091117-FRB-048  
NAWC-091117-FRB-010 NAWC-091117-FRB-145  
NAWC-091117-FRB-317 NAWC-091117-FRB-319  
NAWC-091117-FRB-321 NAWC-091117-FRB-060  
NAWC-091117-FRB-162 NAWC-091117-FRB-258  
NAWC-091117-FRB-314  
  
12/Drinking Water  
NAWC-091117-RW-106 NAWC-091117-RW-048  
NAWC-091117-RW-010 NAWC-091117-RW-145  
NAWC-091117-RW-317 NAWC-091117-RW-319  
NAWC-091117-RW-321 NAWC-091117-RW-060  
NAWC-091117-RW-162 NAWC-091117-RW-258  
NAWC-091117-RW-314 NAWC-091117-DUP09

Overview

The sample set for NAS JRB Willow Grove, SDG 320-31468-1, consisted of twelve (12) drinking water samples and eleven (11) FRB samples. All samples were analyzed for select polyfluorinated alkyl acids including pentadecafluorooctanoic acid (PFOA), perfluorobutane sulfonic acid (PFBS), perfluoroheptanoic acid (PFHpA), perfluorohexanesulfonic acid (PFHxS), perfluorononanoic acid (PFNA) and perfluorooctane sulfonic acid (PFOS). One (1) field duplicate sample pair, NAWC-091117-RW-048 / NAWC-091117-DUP09, was included in this SDG.

The samples were collected by Tetra Tech on September 11, 2017 and analyzed by TestAmerica-Sacramento. All sample analyses were conducted in accordance with EPA Method 537 version 1.1 analytical and reporting protocols.

The data contained in this SDG was validated with regard to the following parameters: data completeness, holding times, initial/continuing calibrations, laboratory method/FRBs, surrogate spike recoveries, laboratory control sample / laboratory control sample duplicate results, internal standard areas and recoveries, chromatographic resolution, analyte identification, analyte quantitation, and detection limits. Areas of concern are listed below.

Major

None.

Minor

The following surrogate recoveries were below the 70% quality control limit. The samples were reanalyzed by the laboratory with similar recoveries and the original analysis was reported. The detected and nondetected results reported in the affected samples were qualified as estimated (J) and (UJ), respectively.

TO: A. FREBOWITZ  
SDG: 320-31468-1

PAGE 2

<u>Sample</u>	<u>Surrogate</u>
NAWC-091117-RW-106	13C2 Perfluorohexanoic acid
NAWC-091117-RW-319	13C2 Perfluorohexanoic acid

Detected results reported below the limit of quantitation (LOQ) but above the detection limit (DL) were qualified as estimated, (J).

### **Notes**

It was stated in the case narrative that none of the sample IDs matched the chain of custody. The laboratory logged the samples in for analyses using the chain of custody IDs which begin with NAWC. The validator changed the sample ID to NAWC for field duplicate 091117-DUP09 per the project manager.

Samples with detections and their associated FRBs are summarized below. No detected results were present in any FRBs.

<u>Sample</u>	<u>Associated FRB</u>
NAWC-091117-RW-106	NAWC-091117-FRB-106
NAWC-091117-RW-048	NAWC-091117-FRB-048
NAWC-091117-RW-010	NAWC-091117-FRB-010
NAWC-091117-RW-145	NAWC-091117-FRB-145
NAWC-091117-RW-317	NAWC-091117-FRB-317
NAWC-091117-RW-319	NAWC-091117-FRB-319
NAWC-091117-RW-321	NAWC-091117-FRB-321
NAWC-091117-RW-060	NAWC-091117-FRB-060
NAWC-091117-RW-162	NAWC-091117-FRB-162
NAWC-091117-RW-258	NAWC-091117-FRB-258
NAWC-091117-RW-314	NAWC-091117-FRB-314
NAWC-091117-DUP09	NAWC-091117-FRB-048

Non-detected results were reported to the Limit of Detection (LOD).

The buffering agent Trizma was added to all drinking water samples.

### **Executive Summary**

**Laboratory Performance:** Two surrogate recoveries were below the quality control limit in two samples.

**Other Factors Affecting Data Quality:** Results below the RL were estimated.

The data for these analyses were reviewed with reference to the Environmental Protection Agency document EPA/600/R-08/092, Method 537, "Determination of Selected Perfluorinated Alkyl Acids in Drinking Water by Solid Phase Extraction and Liquid Chromatography/Tandem Mass Spectrometry (LC/MS/MS)", (September 2009) and the US EPA National Functional Guidelines for Organic Data Review (January 2017) as applicable. The text of this report has been formulated to address only those areas affecting data quality.

TO: A. FREBOWITZ  
SDG: 320-31468-1

PAGE 3



---

Tetra Tech, Inc.  
Terri L. Solomon  
Chemist/Data Validator



---

Tetra Tech, Inc.  
Joseph A. Samchuck  
Data Validation Manager

Attachments:

Appendix A – Qualified Analytical Results  
Appendix B – Results as Reported by the Laboratory  
Appendix C – Support Documentation

### Data Qualifier Definitions

The following definitions provide brief explanations of the validation qualifiers assigned to results in the data review process.

<b>U</b>	The analyte was analyzed for, but was not detected at a level greater than or equal to the level of the adjusted method detection limit for sample and method.
<b>J</b>	The analyte was positively identified and the associated numerical value is the approximate concentration of the analyte in the sample (due either to the quality of the data generated because certain quality control criteria were not met, or the concentration of the analyte was below the reporting limit).
<b>J+</b>	The result is an estimated quantity, but the result may be biased high.
<b>J-</b>	The result is an estimated quantity, but the result may be biased low.
<b>UJ</b>	The analyte was analyzed for, but was not detected. The reported detection limit is approximate and may be inaccurate or imprecise.
<b>R</b>	The sample result (detected) is unusable due to the quality of the data generated because certain criteria were not met. The analyte may or may not be present in the sample.
<b>UR</b>	The sample result (nondetected) is unusable due to the quality of the data generated because certain criteria were not met. The analyte may or may not be present in the sample.

**Appendix A**

Qualified Analytical Results

**Qualifier Codes:**

- A = Lab Blank Contamination
- B = Field Blank Contamination
- C = Calibration Noncompliance (i.e., % RSDs, %Ds, ICVs, CCVs, RRFs, etc.)
- C01 = GC/MS Tuning Noncompliance
- D = MS/MSD Recovery Noncompliance
- E = LCS/LCSD Recovery Noncompliance
- F = Lab Duplicate Imprecision
- G = Field Duplicate Imprecision
- H = Holding Time Exceedance
- I = ICP Serial Dilution Noncompliance
- J = ICP PDS Recovery Noncompliance; MSA's  $r < 0.995$
- K = ICP Interference - includes ICS % R Noncompliance
- L = Instrument Calibration Range Exceedance
- M = Sample Preservation Noncompliance
- N = Internal Standard Noncompliance
- N01 = Internal Standard Recovery Noncompliance Dioxins
- N02 = Recovery Standard Noncompliance Dioxins
- N03 = Clean-up Standard Noncompliance Dioxins
- O = Poor Instrument Performance (i.e., base-time drifting)
- P = Uncertainty near detection limit ( $< 2 \times$  IDL for inorganics and  $<$ CRQL for organics)
- Q = Other problems (can encompass a number of issues; i.e.chromatography,interferences, etc.)
- R = Surrogates Recovery Noncompliance
- S = Pesticide/PCB Resolution
- T = % Breakdown Noncompliance for DDT and Endrin
- U = RPD between columns/detectors  $>40\%$  for positive results determined via GC/HPLC
- V = Non-linear calibrations; correlation coefficient  $r < 0.995$
- W = EMPC result
- X = Signal to noise response drop
- Y = Percent solids  $<30\%$
- Z = Uncertainty at 2 standard deviations is greater than sample activity
- Z1 = Tentatively Identified Compound considered presumptively present
- Z2 = Tentatively Identified Compound column bleed
- Z3 = Tentatively Identified Compound aldol condensate
- Z4 = Sample activity is less than the at uncertainty at 3 standard deviations and greater than the MDC
- Z5 = Sample activity is less than the at uncertainty at 3 standard deviations and less than the MDC



<b>PROJ_NO: 08005-WE04</b> <b>SDG: 320-31468-1</b> <b>FRACTION: PFAS</b> <b>MEDIA: WATER</b>	NSAMPLE	NAWC-091117-DUP09			NAWC-091117-FRB-010			NAWC-091117-FRB-048			NAWC-091117-FRB-060		
	LAB_ID	320-31468-23			320-31468-20			320-31468-10			320-31468-4		
	SAMP_DATE	9/11/2017			9/11/2017			9/11/2017			9/11/2017		
	QC_TYPE	FD			FB			FB			FB		
	UNITS	NG/L			NG/L			NG/L			NG/L		
	PCT_SOLIDS	0.0			0.0			0.0			0.0		
	DUP_OF	NAWC-091117-RW-048											
PARAMETER	RESULT	VQL	QLCD	RESULT	VQL	QLCD	RESULT	VQL	QLCD	RESULT	VQL	QLCD	
PENTADECAFLUOROOCTANOIC ACID	4.5	J	P	7.7	U		7.5	U		7.7	U		
PERFLUOROBUTANESULFONIC ACID	35	U		35	U		34	U		35	U		
PERFLUOROHEPTANOIC ACID	3.8	U		3.8	U		3.7	U		3.8	U		
PERFLUOROHXANESULFONIC ACID	12	U		12	U		11	U		12	U		
PERFLUORONONANOIC ACID	19	U		19	U		19	U		19	U		
PERFLUOROOCTANE SULFONIC ACID	15	U		15	U		15	U		15	U		

<b>PROJ_NO: 08005-WE04</b> <b>SDG: 320-31468-1</b> <b>FRACTION: PFAS</b> <b>MEDIA: WATER</b>	NSAMPLE	NAWC-091117-FRB-106			NAWC-091117-FRB-145			NAWC-091117-FRB-162			NAWC-091117-FRB-258		
	LAB_ID	320-31468-2			320-31468-12			320-31468-22			320-31468-8		
	SAMP_DATE	9/11/2017			9/11/2017			9/11/2017			9/11/2017		
	QC_TYPE	FB			FB			FB			FB		
	UNITS	NG/L			NG/L			NG/L			NG/L		
	PCT_SOLIDS	0.0			0.0			0.0			0.0		
	DUP_OF												
PARAMETER	RESULT	VQL	QLCD	RESULT	VQL	QLCD	RESULT	VQL	QLCD	RESULT	VQL	QLCD	
PENTADECAFLUOROOCTANOIC ACID	7.7	U		7.5	U		8.1	U		7.6	U		
PERFLUOROBUTANESULFONIC ACID	35	U		34	U		36	U		34	U		
PERFLUOROHEPTANOIC ACID	3.9	U		3.8	U		4	U		3.8	U		
PERFLUOROHXANESULFONIC ACID	12	U		11	U		12	U		11	U		
PERFLUORONONANOIC ACID	19	U		19	U		20	U		19	U		
PERFLUOROOCTANE SULFONIC ACID	15	U		15	U		16	U		15	U		

<b>PROJ_NO: 08005-WE04</b> <b>SDG: 320-31468-1</b> <b>FRACTION: PFAS</b> <b>MEDIA: WATER</b>	NSAMPLE	NAWC-091117-FRB-314			NAWC-091117-FRB-317			NAWC-091117-FRB-319			NAWC-091117-FRB-321		
	LAB_ID	320-31468-6			320-31468-14			320-31468-16			320-31468-18		
	SAMP_DATE	9/11/2017			9/11/2017			9/11/2017			9/11/2017		
	QC_TYPE	FB			FB			FB			FB		
	UNITS	NG/L			NG/L			NG/L			NG/L		
	PCT_SOLIDS	0.0			0.0			0.0			0.0		
	DUP_OF												
PARAMETER	RESULT	VQL	QLCD	RESULT	VQL	QLCD	RESULT	VQL	QLCD	RESULT	VQL	QLCD	
PENTADECAFLUOROOCTANOIC ACID	7.5	U		7.9	U		7.5	U		7.6	U		
PERFLUOROBUTANESULFONIC ACID	34	U		35	U		34	U		34	U		
PERFLUOROHEPTANOIC ACID	3.8	U		3.9	U		3.7	U		3.8	U		
PERFLUOROHXANESULFONIC ACID	11	U		12	U		11	U		11	U		
PERFLUORONONANOIC ACID	19	U		20	U		19	U		19	U		
PERFLUOROOCTANE SULFONIC ACID	15	U		16	U		15	U		15	U		

<b>PROJ_NO: 08005-WE04</b> <b>SDG: 320-31468-1</b> <b>FRACTION: PFAS</b> <b>MEDIA: WATER</b>	NSAMPLE	NAWC-091117-RW-010			NAWC-091117-RW-048			NAWC-091117-RW-060			NAWC-091117-RW-106		
	LAB_ID	320-31468-19			320-31468-9			320-31468-3			320-31468-1		
	SAMP_DATE	9/11/2017			9/11/2017			9/11/2017			9/11/2017		
	QC_TYPE	NM			NM			NM			NM		
	UNITS	NG/L			NG/L			NG/L			NG/L		
	PCT_SOLIDS	0.0			0.0			0.0			0.0		
	DUP_OF				NAWC-091117-RW-048								
PARAMETER	RESULT	VQL	QLCD	RESULT	VQL	QLCD	RESULT	VQL	QLCD	RESULT	VQL	QLCD	
PENTADECAFLUOROOCTANOIC ACID	12	J	P	4.5	J	P	17	J	P	20	J	R	
PERFLUOROBUTANESULFONIC ACID	35	U		34	U		34	U		36	UJ	R	
PERFLUOROHEPTANOIC ACID	5.4	J	P	3.8	U		3.9	J	P	8.1	J	PR	
PERFLUOROHXANESULFONIC ACID	17	J	P	11	U		9.9	J	P	8.9	J	PR	
PERFLUORONONANOIC ACID	20	U		19	U		19	U		20	UJ	R	
PERFLUOROOCTANE SULFONIC ACID	30	J		15	U		27	J	P	17	J	PR	

<b>PROJ_NO: 08005-WE04</b> <b>SDG: 320-31468-1</b> <b>FRACTION: PFAS</b> <b>MEDIA: WATER</b>	NSAMPLE	NAWC-091117-RW-145			NAWC-091117-RW-162			NAWC-091117-RW-258			NAWC-091117-RW-314		
	LAB_ID	320-31468-11			320-31468-21			320-31468-7			320-31468-5		
	SAMP_DATE	9/11/2017			9/11/2017			9/11/2017			9/11/2017		
	QC_TYPE	NM			NM			NM			NM		
	UNITS	NG/L			NG/L			NG/L			NG/L		
	PCT_SOLIDS	0.0			0.0			0.0			0.0		
	DUP_OF												
PARAMETER	RESULT	VQL	QLCD	RESULT	VQL	QLCD	RESULT	VQL	QLCD	RESULT	VQL	QLCD	
PENTADECAFLUOROOCTANOIC ACID	20			15 J	P		21			17 J	P		
PERFLUOROBUTANESULFONIC ACID	33 U			34 U			34 U			34 U			
PERFLUOROHEPTANOIC ACID	5.6 J	P		5.4 J	P		7.7 J	P		4.4 J	P		
PERFLUOROHXANESULFONIC ACID	7.3 J	P		13 J	P		11 U			11 U			
PERFLUORONONANOIC ACID	19 U			19 U			12 J	P		19 U			
PERFLUOROOCTANE SULFONIC ACID	19 J	P		33 J	P		18 J	P		15 J	P		

<b>PROJ_NO: 08005-WE04</b> <b>SDG: 320-31468-1</b> <b>FRACTION: PFAS</b> <b>MEDIA: WATER</b>	NSAMPLE	NAWC-091117-RW-317			NAWC-091117-RW-319			NAWC-091117-RW-321		
	LAB_ID	320-31468-13			320-31468-15			320-31468-17		
	SAMP_DATE	9/11/2017			9/11/2017			9/11/2017		
	QC_TYPE	NM			NM			NM		
	UNITS	NG/L			NG/L			NG/L		
	PCT_SOLIDS	0.0			0.0			0.0		
	DUP_OF									
PARAMETER	RESULT	VQL	QLCD	RESULT	VQL	QLCD	RESULT	VQL	QLCD	
PENTADECAFLUOROOCTANOIC ACID	21			44 J	R		6.9 J	P		
PERFLUOROBUTANESULFONIC ACID	34 U			36 UJ	R		34 U			
PERFLUOROHEPTANOIC ACID	8.1 J	P		15 J	R		1.8 J	P		
PERFLUOROHXANESULFONIC ACID	34			8 J	PR		11 U			
PERFLUORONONANOIC ACID	19 U			9.7 J	PR		19 U			
PERFLUOROOCTANE SULFONIC ACID	49			43 J	R		7.5 J	P		

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-RW-106 Lab Sample ID: 320-31468-1  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_014.d  
 Analysis Method: 537 Date Collected: 09/11/2017 09:40  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 252.7(mL) Date Analyzed: 09/20/2017 04:49  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185407 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	17	J <del>M</del>	40	16	6.7
335-67-1	Perfluorooctanoic acid (PFOA)	20	J	20	7.9	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	<del>U</del> JJ	24	20	7.9
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	8.9	J	30	12	5.4
375-85-9	Perfluoroheptanoic acid (PFHpA)	8.1	J	9.9	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	<del>U</del> JJ	89	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	67	Q	70-130
STL00996	13C2 PFDA	100		70-130

*Steve L. Salzman*  
10/06/2017

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-FRB-106 Lab Sample ID: 320-31468-2  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_015.d  
 Analysis Method: 537 Date Collected: 09/11/2017 09:35  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 258.9(mL) Date Analyzed: 09/20/2017 04:54  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185407 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	39	15	6.6
335-67-1	Perfluorooctanoic acid (PFOA)	7.7	U	19	7.7	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.7
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	29	12	5.3
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.9	U	9.7	3.9	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	35	U	87	35	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	82		70-130
STL00996	13C2 PFDA	105		70-130

*Ali J. Salem*  
10/06/2017



FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-RW-060 Lab Sample ID: 320-31468-3  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_016.d  
 Analysis Method: 537 Date Collected: 09/11/2017 09:55  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 261.7(mL) Date Analyzed: 09/20/2017 04:59  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185407 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	27	J <del>M</del>	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	17	J	19	7.6	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	9.9	J	29	11	5.3
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.9	J	9.6	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	86	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	71		70-130
STL00996	13C2 PFDA	114		70-130

*Ali L. Salem*  
10/06/2017

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-FRB-060 Lab Sample ID: 320-31468-4  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_017.d  
 Analysis Method: 537 Date Collected: 09/11/2017 09:50  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 259.9(mL) Date Analyzed: 09/20/2017 05:04  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185407 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	7.7	U	19	7.7	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.7
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	29	12	5.3
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	U	9.6	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	35	U	87	35	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	86		70-130
STL00996	13C2 PFDA	107		70-130

*Asim J. Salaman*  
10/06/2017

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-RW-314 Lab Sample ID: 320-31468-5  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_018.d  
 Analysis Method: 537 Date Collected: 09/11/2017 10:25  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 262.7(mL) Date Analyzed: 09/20/2017 05:08  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185407 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	J <del>M</del>	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	17	J	19	7.6	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	29	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.4	J	9.5	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	86	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	72		70-130
STL00996	13C2 PFDA	104		70-130

*Wesley L. Selman*  
10/06/2017

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-FRB-314 Lab Sample ID: 320-31468-6  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_019.d  
 Analysis Method: 537 Date Collected: 09/11/2017 10:20  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 265.6(mL) Date Analyzed: 09/20/2017 05:13  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185407 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	38	15	6.4
335-67-1	Perfluorooctanoic acid (PFOA)	7.5	U	19	7.5	2.6
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.5
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	U	9.4	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	85	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	82		70-130
STL00996	13C2 PFDA	102		70-130

*Ali L. Salaman*  
10/06/2017

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-RW-258 Lab Sample ID: 320-31468-7  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_020.d  
 Analysis Method: 537 Date Collected: 09/11/2017 11:00  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 267(mL) Date Analyzed: 09/20/2017 05:18  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185407 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	18	J <del>M</del>	37	15	6.4
335-67-1	Perfluorooctanoic acid (PFOA)	21		19	7.5	2.6
375-95-1	Perfluorononanoic acid (PFNA)	12	J	22	19	7.5
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.1
375-85-9	Perfluoroheptanoic acid (PFHpA)	7.7	J	9.4	3.7	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	84	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	72		70-130
STL00996	13C2 PFDA	98		70-130

*Ali L. Salem*  
10/06/2017

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-FRB-258 Lab Sample ID: 320-31468-8  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_023.d  
 Analysis Method: 537 Date Collected: 09/11/2017 10:55  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 261.6(mL) Date Analyzed: 09/20/2017 05:32  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	7.6	U	19	7.6	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	29	11	5.3
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	U	9.6	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	86	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	86		70-130
STL00996	13C2 PFDA	101		70-130

*Amir L. Salaman*  
10/06/2017

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-RW-048 Lab Sample ID: 320-31468-9  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_024.d  
 Analysis Method: 537 Date Collected: 09/11/2017 13:05  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 263.9(mL) Date Analyzed: 09/20/2017 05:37  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U <del>M</del>	38	15	6.4
335-67-1	Perfluorooctanoic acid (PFOA)	4.5	J <del>M</del>	19	7.6	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	U	9.5	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	85	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	74		70-130
STL00996	13C2 PFDA	111		70-130

*Amir L. Selman*  
10/06/2017

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-FRB-048 Lab Sample ID: 320-31468-10  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_025.d  
 Analysis Method: 537 Date Collected: 09/11/2017 13:00  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 266.7(mL) Date Analyzed: 09/20/2017 05:42  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	37	15	6.4
335-67-1	Perfluorooctanoic acid (PFOA)	7.5	U	19	7.5	2.6
375-95-1	Perfluorononanoic acid (PFNA)	19	U	22	19	7.5
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.7	U	9.4	3.7	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	84	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	84		70-130
STL00996	13C2 PFDA	102		70-130

*Atari L. Selman*  
10/06/2017



FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-RW-145 Lab Sample ID: 320-31468-11  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_026.d  
 Analysis Method: 537 Date Collected: 09/11/2017 13:35  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 269(mL) Date Analyzed: 09/20/2017 05:46  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	19	J <del>M</del>	37	15	6.3
335-67-1	Perfluorooctanoic acid (PFOA)	20		19	7.4	2.6
375-95-1	Perfluorononanoic acid (PFNA)	19	U	22	19	7.4
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	7.3	J	28	11	5.1
375-85-9	Perfluoroheptanoic acid (PFHpA)	5.6	J	9.3	3.7	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	33	U	84	33	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	74		70-130
STL00996	13C2 PFDA	115		70-130

*Wesley L. Selman*  
10/06/2017

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-FRB-145 Lab Sample ID: 320-31468-12  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_027.d  
 Analysis Method: 537 Date Collected: 09/11/2017 13:30  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 265.6(mL) Date Analyzed: 09/20/2017 05:51  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	38	15	6.4
335-67-1	Perfluorooctanoic acid (PFOA)	7.5	U	19	7.5	2.6
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.5
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	U	9.4	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	85	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	83		70-130
STL00996	13C2 PFDA	100		70-130

*Wesley L. Salzman*  
10/06/2017

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-RW-317 Lab Sample ID: 320-31468-13  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_028.d  
 Analysis Method: 537 Date Collected: 09/11/2017 14:00  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 263.7(mL) Date Analyzed: 09/20/2017 05:56  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	49	<del>M</del>	38	15	6.4
335-67-1	Perfluorooctanoic acid (PFOA)	21		19	7.6	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	34		28	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	8.1	J	9.5	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	85	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	78		70-130
STL00996	13C2 PFDA	116		70-130

*Amir L. Salem*  
10/06/2017

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-FRB-317 Lab Sample ID: 320-31468-14  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_029.d  
 Analysis Method: 537 Date Collected: 09/11/2017 13:55  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 254.4(mL) Date Analyzed: 09/20/2017 06:01  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	39	16	6.7
335-67-1	Perfluorooctanoic acid (PFOA)	7.9	U	20	7.9	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	7.9
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	29	12	5.4
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.9	U	9.8	3.9	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	35	U	88	35	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	83		70-130
STL00996	13C2 PFDA	97		70-130

*Staci L. Selman*  
10/06/2017

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-RW-319 Lab Sample ID: 320-31468-15  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_030.d  
 Analysis Method: 537 Date Collected: 09/11/2017 14:25  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 251(mL) Date Analyzed: 09/20/2017 06:05  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	43	<del>M</del> J	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	44	J	20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	9.7	J	24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	8.0	J	30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	15	<del>M</del> J	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	<del>U</del> JJ	90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	61	Q	70-130
STL00996	13C2 PFDA	83		70-130

*Wesley J. Salaman*  
10/06/2017

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-FRB-319 Lab Sample ID: 320-31468-16  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_031.d  
 Analysis Method: 537 Date Collected: 09/11/2017 14:40  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 266.7(mL) Date Analyzed: 09/20/2017 06:10  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	37	15	6.4
335-67-1	Perfluorooctanoic acid (PFOA)	7.5	U	19	7.5	2.6
375-95-1	Perfluorononanoic acid (PFNA)	19	U	22	19	7.5
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.7	U	9.4	3.7	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	84	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	82		70-130
STL00996	13C2 PFDA	124		70-130

*W. L. Selman*  
10/06/2017

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-RW-321 Lab Sample ID: 320-31468-17  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_032.d  
 Analysis Method: 537 Date Collected: 09/11/2017 15:10  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 262 (mL) Date Analyzed: 09/20/2017 06:15  
 Con. Extract Vol.: 1.0 (mL) Dilution Factor: 1  
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	7.5	J <del>M</del>	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	6.9	J	19	7.6	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	29	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	1.8	J	9.5	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	86	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	76		70-130
STL00996	13C2 PFDA	106		70-130

*Steve L. Selman*  
10/06/2017

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-FRB-321 Lab Sample ID: 320-31468-18  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_035.d  
 Analysis Method: 537 Date Collected: 09/11/2017 15:05  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 263.5 (mL) Date Analyzed: 09/20/2017 06:29  
 Con. Extract Vol.: 1.0 (mL) Dilution Factor: 1  
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185409 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	7.6	U	19	7.6	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	U	9.5	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	85	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	84		70-130
STL00996	13C2 PFDA	104		70-130

*Wesley L. Salomon*  
10/06/2017



FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-RW-010 Lab Sample ID: 320-31468-19  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_036.d  
 Analysis Method: 537 Date Collected: 09/11/2017 15:45  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 254.7(mL) Date Analyzed: 09/20/2017 06:34  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185409 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	30	J <del>M</del>	39	16	6.7
335-67-1	Perfluorooctanoic acid (PFOA)	12	J	20	7.9	2.7
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	7.9
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	17	J	29	12	5.4
375-85-9	Perfluoroheptanoic acid (PFHpA)	5.4	J	9.8	3.9	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	35	U	88	35	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	75		70-130
STL00996	13C2 PFDA	104		70-130

*Wesley L. Selman*  
10/06/2017

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-FRB-010 Lab Sample ID: 320-31468-20  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_037.d  
 Analysis Method: 537 Date Collected: 09/11/2017 15:40  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 259.8(mL) Date Analyzed: 09/20/2017 06:39  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185409 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	7.7	U	19	7.7	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.7
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	29	12	5.3
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	U	9.6	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	35	U	87	35	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	83		70-130
STL00996	13C2 PFDA	97		70-130

*Steve L. Selman*  
10/06/2017

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-RW-162 Lab Sample ID: 320-31468-21  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_006.d  
 Analysis Method: 537 Date Collected: 09/11/2017 11:20  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:29  
 Sample wt/vol: 262.9(mL) Date Analyzed: 09/20/2017 04:11  
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185406 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	33	J <del>M</del>	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	15	J	19	7.6	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	13	J	29	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	5.4	J	9.5	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	86	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	78		70-130
STL00996	13C2 PFDA	111		70-130

*Reza L. Saleman*  
10/06/2017

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-FRB-162 Lab Sample ID: 320-31468-22  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_007.d  
 Analysis Method: 537 Date Collected: 09/11/2017 11:15  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:29  
 Sample wt/vol: 247.3(mL) Date Analyzed: 09/20/2017 04:16  
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185406 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	40	16	6.9
335-67-1	Perfluorooctanoic acid (PFOA)	8.1	U	20	8.1	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	8.1
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	30	12	5.6
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.0	U	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	91	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	91		70-130
STL00996	13C2 PFDA	129		70-130

*Steve L. Salzman*  
10/06/2017

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: NAWC  
 Client Sample ID: WGNA-091117-DUP09 Lab Sample ID: 320-31468-23  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_008.d  
 Analysis Method: 537 Date Collected: 09/11/2017 07:00  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:29  
 Sample wt/vol: 260 (mL) Date Analyzed: 09/20/2017 04:21  
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1  
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185406 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U <del>M</del>	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	4.5	J	19	7.7	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.7
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	29	12	5.3
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	U <del>M</del>	9.6	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	35	U	87	35	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	75		70-130
STL00996	13C2 PFDA	125		70-130

*Wesley L. Selman*  
10/06/2017

**Appendix B**

Results as Reported by the Laboratory

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-RW-106 Lab Sample ID: 320-31468-1  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_014.d  
 Analysis Method: 537 Date Collected: 09/11/2017 09:40  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 252.7(mL) Date Analyzed: 09/20/2017 04:49  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185407 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	17	J M	40	16	6.7
335-67-1	Perfluorooctanoic acid (PFOA)	20		20	7.9	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	7.9
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	8.9	J	30	12	5.4
375-85-9	Perfluoroheptanoic acid (PFHpA)	8.1	J	9.9	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	89	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	67	Q	70-130
STL00996	13C2 PFDA	100		70-130

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-FRB-106 Lab Sample ID: 320-31468-2  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_015.d  
 Analysis Method: 537 Date Collected: 09/11/2017 09:35  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 258.9(mL) Date Analyzed: 09/20/2017 04:54  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185407 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	39	15	6.6
335-67-1	Perfluorooctanoic acid (PFOA)	7.7	U	19	7.7	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.7
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	29	12	5.3
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.9	U	9.7	3.9	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	35	U	87	35	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	82		70-130
STL00996	13C2 PFDA	105		70-130



FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-RW-060 Lab Sample ID: 320-31468-3  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_016.d  
 Analysis Method: 537 Date Collected: 09/11/2017 09:55  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 261.7(mL) Date Analyzed: 09/20/2017 04:59  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185407 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	27	J M	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	17	J	19	7.6	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	9.9	J	29	11	5.3
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.9	J	9.6	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	86	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	71		70-130
STL00996	13C2 PFDA	114		70-130

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-FRB-060 Lab Sample ID: 320-31468-4  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_017.d  
 Analysis Method: 537 Date Collected: 09/11/2017 09:50  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 259.9(mL) Date Analyzed: 09/20/2017 05:04  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185407 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	7.7	U	19	7.7	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.7
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	29	12	5.3
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	U	9.6	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	35	U	87	35	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	86		70-130
STL00996	13C2 PFDA	107		70-130

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-RW-314 Lab Sample ID: 320-31468-5  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_018.d  
 Analysis Method: 537 Date Collected: 09/11/2017 10:25  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 262.7(mL) Date Analyzed: 09/20/2017 05:08  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185407 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	J M	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	17	J	19	7.6	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	29	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.4	J	9.5	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	86	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	72		70-130
STL00996	13C2 PFDA	104		70-130

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-FRB-314 Lab Sample ID: 320-31468-6  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_019.d  
 Analysis Method: 537 Date Collected: 09/11/2017 10:20  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 265.6(mL) Date Analyzed: 09/20/2017 05:13  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185407 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	38	15	6.4
335-67-1	Perfluorooctanoic acid (PFOA)	7.5	U	19	7.5	2.6
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.5
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	U	9.4	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	85	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	82		70-130
STL00996	13C2 PFDA	102		70-130

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-RW-258 Lab Sample ID: 320-31468-7  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_020.d  
 Analysis Method: 537 Date Collected: 09/11/2017 11:00  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 267(mL) Date Analyzed: 09/20/2017 05:18  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185407 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	18	J M	37	15	6.4
335-67-1	Perfluorooctanoic acid (PFOA)	21		19	7.5	2.6
375-95-1	Perfluorononanoic acid (PFNA)	12	J	22	19	7.5
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.1
375-85-9	Perfluoroheptanoic acid (PFHpA)	7.7	J	9.4	3.7	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	84	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	72		70-130
STL00996	13C2 PFDA	98		70-130

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-FRB-258 Lab Sample ID: 320-31468-8  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_023.d  
 Analysis Method: 537 Date Collected: 09/11/2017 10:55  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 261.6(mL) Date Analyzed: 09/20/2017 05:32  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	7.6	U	19	7.6	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	29	11	5.3
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	U	9.6	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	86	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	86		70-130
STL00996	13C2 PFDA	101		70-130

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-RW-048 Lab Sample ID: 320-31468-9  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_024.d  
 Analysis Method: 537 Date Collected: 09/11/2017 13:05  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 263.9(mL) Date Analyzed: 09/20/2017 05:37  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U M	38	15	6.4
335-67-1	Perfluorooctanoic acid (PFOA)	4.5	J M	19	7.6	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	U	9.5	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	85	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	74		70-130
STL00996	13C2 PFDA	111		70-130

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-FRB-048 Lab Sample ID: 320-31468-10  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_025.d  
 Analysis Method: 537 Date Collected: 09/11/2017 13:00  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 266.7(mL) Date Analyzed: 09/20/2017 05:42  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	37	15	6.4
335-67-1	Perfluorooctanoic acid (PFOA)	7.5	U	19	7.5	2.6
375-95-1	Perfluorononanoic acid (PFNA)	19	U	22	19	7.5
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.7	U	9.4	3.7	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	84	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	84		70-130
STL00996	13C2 PFDA	102		70-130



FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-RW-145 Lab Sample ID: 320-31468-11  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_026.d  
 Analysis Method: 537 Date Collected: 09/11/2017 13:35  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 269(mL) Date Analyzed: 09/20/2017 05:46  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	19	J M	37	15	6.3
335-67-1	Perfluorooctanoic acid (PFOA)	20		19	7.4	2.6
375-95-1	Perfluorononanoic acid (PFNA)	19	U	22	19	7.4
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	7.3	J	28	11	5.1
375-85-9	Perfluoroheptanoic acid (PFHpA)	5.6	J	9.3	3.7	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	33	U	84	33	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	74		70-130
STL00996	13C2 PFDA	115		70-130

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-FRB-145 Lab Sample ID: 320-31468-12  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_027.d  
 Analysis Method: 537 Date Collected: 09/11/2017 13:30  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 265.6(mL) Date Analyzed: 09/20/2017 05:51  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	38	15	6.4
335-67-1	Perfluorooctanoic acid (PFOA)	7.5	U	19	7.5	2.6
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.5
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	U	9.4	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	85	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	83		70-130
STL00996	13C2 PFDA	100		70-130

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-RW-317 Lab Sample ID: 320-31468-13  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_028.d  
 Analysis Method: 537 Date Collected: 09/11/2017 14:00  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 263.7(mL) Date Analyzed: 09/20/2017 05:56  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	49	M	38	15	6.4
335-67-1	Perfluorooctanoic acid (PFOA)	21		19	7.6	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	34		28	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	8.1	J	9.5	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	85	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	78		70-130
STL00996	13C2 PFDA	116		70-130

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-FRB-317 Lab Sample ID: 320-31468-14  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_029.d  
 Analysis Method: 537 Date Collected: 09/11/2017 13:55  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 254.4(mL) Date Analyzed: 09/20/2017 06:01  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	39	16	6.7
335-67-1	Perfluorooctanoic acid (PFOA)	7.9	U	20	7.9	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	7.9
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	29	12	5.4
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.9	U	9.8	3.9	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	35	U	88	35	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	83		70-130
STL00996	13C2 PFDA	97		70-130

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-RW-319 Lab Sample ID: 320-31468-15  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_030.d  
 Analysis Method: 537 Date Collected: 09/11/2017 14:25  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 251(mL) Date Analyzed: 09/20/2017 06:05  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	43	M	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	44		20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	9.7	J	24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	8.0	J	30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	15	M	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	61	Q	70-130
STL00996	13C2 PFDA	83		70-130

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-FRB-319 Lab Sample ID: 320-31468-16  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_031.d  
 Analysis Method: 537 Date Collected: 09/11/2017 14:40  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 266.7(mL) Date Analyzed: 09/20/2017 06:10  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	37	15	6.4
335-67-1	Perfluorooctanoic acid (PFOA)	7.5	U	19	7.5	2.6
375-95-1	Perfluorononanoic acid (PFNA)	19	U	22	19	7.5
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.7	U	9.4	3.7	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	84	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	82		70-130
STL00996	13C2 PFDA	124		70-130

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-RW-321 Lab Sample ID: 320-31468-17  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_032.d  
 Analysis Method: 537 Date Collected: 09/11/2017 15:10  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 262 (mL) Date Analyzed: 09/20/2017 06:15  
 Con. Extract Vol.: 1.0 (mL) Dilution Factor: 1  
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	7.5	J M	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	6.9	J	19	7.6	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	29	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	1.8	J	9.5	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	86	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	76		70-130
STL00996	13C2 PFDA	106		70-130

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-FRB-321 Lab Sample ID: 320-31468-18  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_035.d  
 Analysis Method: 537 Date Collected: 09/11/2017 15:05  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 263.5 (mL) Date Analyzed: 09/20/2017 06:29  
 Con. Extract Vol.: 1.0 (mL) Dilution Factor: 1  
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185409 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	7.6	U	19	7.6	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	U	9.5	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	85	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	84		70-130
STL00996	13C2 PFDA	104		70-130



FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-RW-010 Lab Sample ID: 320-31468-19  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_036.d  
 Analysis Method: 537 Date Collected: 09/11/2017 15:45  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 254.7(mL) Date Analyzed: 09/20/2017 06:34  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185409 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	30	J M	39	16	6.7
335-67-1	Perfluorooctanoic acid (PFOA)	12	J	20	7.9	2.7
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	7.9
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	17	J	29	12	5.4
375-85-9	Perfluoroheptanoic acid (PFHpA)	5.4	J	9.8	3.9	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	35	U	88	35	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	75		70-130
STL00996	13C2 PFDA	104		70-130

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-FRB-010 Lab Sample ID: 320-31468-20  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_037.d  
 Analysis Method: 537 Date Collected: 09/11/2017 15:40  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 259.8(mL) Date Analyzed: 09/20/2017 06:39  
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185409 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	7.7	U	19	7.7	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.7
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	29	12	5.3
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	U	9.6	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	35	U	87	35	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	83		70-130
STL00996	13C2 PFDA	97		70-130

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-RW-162 Lab Sample ID: 320-31468-21  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_006.d  
 Analysis Method: 537 Date Collected: 09/11/2017 11:20  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:29  
 Sample wt/vol: 262.9(mL) Date Analyzed: 09/20/2017 04:11  
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185406 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	33	J M	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	15	J	19	7.6	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	13	J	29	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	5.4	J	9.5	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	86	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	78		70-130
STL00996	13C2 PFDA	111		70-130

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: NAWC-091117-FRB-162 Lab Sample ID: 320-31468-22  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_007.d  
 Analysis Method: 537 Date Collected: 09/11/2017 11:15  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:29  
 Sample wt/vol: 247.3(mL) Date Analyzed: 09/20/2017 04:16  
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1  
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185406 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	40	16	6.9
335-67-1	Perfluorooctanoic acid (PFOA)	8.1	U	20	8.1	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	8.1
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	30	12	5.6
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.0	U	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	91	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	91		70-130
STL00996	13C2 PFDA	129		70-130

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: NAWC  
 Client Sample ID: ~~WCNA~~-091117-DUP09 Lab Sample ID: 320-31468-23  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_008.d  
 Analysis Method: 537 Date Collected: 09/11/2017 07:00  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:29  
 Sample wt/vol: 260 (mL) Date Analyzed: 09/20/2017 04:21  
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1  
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185406 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U M	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	4.5	J	19	7.7	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.7
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	29	12	5.3
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	U M	9.6	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	35	U	87	35	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	75		70-130
STL00996	13C2 PFDA	125		70-130

*Thomas J. Selman*  
10/06/2017

**Appendix C**


Support Documentation

<b>ANALYTE</b>	<b>ORIGINAL</b>	<b>DUPLICATE</b>	<b>RL</b>	<b>RPD</b>	<b>RPD &gt; 50%</b>	<b>ORIGINAL SAMPLE CONC &gt;2xRL</b>	<b>DUPLICATE SAMPLE CONC &gt;2xRL</b>	<b>DIFFERENCE &gt;2xRL</b>		
Perfluorooctanoic acid (PFOA)	091117-RW-048	DUP09	4.5	4.5	19	0.000	FALSE	FALSE	FALSE	FALSE

**Chain of Custody Record**

TestAmerica Laboratories, Inc.

Regulatory Program:  DW  NPDES  RCRA  Other:

<b>Client Contact</b>			<b>Project Manager:</b> Andy Frebowitz			<b>Site Contact:</b> Mary Kay Bond			<b>Date:</b> 9/11/2017			<b>COC No.:</b>					
TetraTech			Tel/Fax: 610.382.1170			Lab Contact: Dave Alltucker			Carrier: FedEx			1 of 2 COCs					
234 Mall Boulevard Suite 260			<b>Analysis Turnaround Time</b>			<input type="checkbox"/> CALENDAR DAYS <input type="checkbox"/> WORKING DAYS TAT if different from Below 21 <input type="checkbox"/> 2 weeks <input type="checkbox"/> 1 week <input type="checkbox"/> 2 days <input type="checkbox"/> 1 day			Filtered Sample (Y/N) Perform MS / MSD (Y/N) EPA 537 UCMR3			 320-31468 Chain of Custody			Sampler: Mary Kay Bond		
King of Prussia, PA 19406			For Lab Use Only:														
610-382-1174			Walk-in Client:														
610-491-9688			Lab Sampling:														
Project Name: WE04			Job / SDG No.:														
Site: WE04																	
P O # 1132358 (through EarthToxics)																	
Sample Identification		Sample Date	Sample Time	Sample Type (C=Comp, G=Grab)	Matrix	# of Cont.	Filtered Sample (Y/N)	Perform MS / MSD (Y/N)	EPA 537 UCMR3	Sample Specific Notes:							
NAWC-091117-RW-106		9/11/2017	09:40	G	DW	2	N	N	Y								
NAWC-091117-FRB-106		9/11/2017	09:35	G	DW	2	N	N	Y	Field Reagent Blank							
NAWC-091117-RW-060		9/11/2017	09:55	G	DW	2	N	N	Y								
NAWC-091117-FRB-060		9/11/2017	09:50	G	DW	2	N	N	Y	Field Reagent Blank							
NAWC-091117-RW-314		9/11/2017	10:25	G	DW	2	N	N	Y								
NAWC-091117-FRB-314		9/11/2017	10:20	G	DW	2	N	N	Y	Field Reagent Blank							
NAWC-091117-RW-258		9/11/2017	11:00	G	DW	2	N	N	Y								
NAWC-091117-FRB-258		9/11/2017	10:55	G	DW	2	N	N	Y	Field Reagent Blank							
NAWC-091117-RW-048		9/11/2017	13:05	G	DW	2	N	N	Y								
NAWC-091117-FRB-048		9/11/2017	13:00	G	DW	2	N	N	Y	Field Reagent Blank							
NAWC-091117-RW-145		9/11/2017	13:35	G	DW	2	N	N	Y								
NAWC-091117-FRB-145		9/11/2017	13:30	G	DW	2	N	N	Y	Field Reagent Blank							
<b>Preservation Used:</b> 1= Ice, 2= HCl; 3= H2SO4; 4=HNO3; 5=NaOH; 6= Other: Trizma																	
<b>Possible Hazard Identification:</b> Are any samples from a listed EPA Hazardous Waste? Please List any EPA Waste Codes for the sample in the												<b>Sample Disposal ( A fee may be assessed if samples are retained longer than 1 month)</b> <input type="checkbox"/> Return to Client <input type="checkbox"/> Disposal by Lab <input type="checkbox"/> Archive for _____ Months					
<input type="checkbox"/> Non-Hazard <input type="checkbox"/> Flammable <input type="checkbox"/> Skin Irritant <input type="checkbox"/> Poison B <input type="checkbox"/> Unknown																	
<b>Fed Ex Tracking: 770221957389</b>																	
Custody Seals Intact: <input type="checkbox"/> Yes <input type="checkbox"/> No			Custody Seal No.:			Cooler Temp. (°C): Obs'd: 1-5			Corr'd: -			Therm ID No.: AR-1					
Relinquished by: <i>Mary Kay Bond</i>			Company: Tetra Tech			Date/Time: 9/11/2017 18:00			Received by: <i>[Signature]</i>			Company: <i>Telus</i>					
Relinquished by:			Company:			Date/Time:			Received by:			Date/Time: 9/12/17 930					
Relinquished by:			Company:			Date/Time:			Received in Laboratory by:			Date/Time:					

Page 474 of 476

All labeled WGN -  
 at 9-12-17



**TestAmerica Sacramento**

880 Riverside Parkway  
 West Sacramento, CA 95605-1500  
 phone 916.373.5600 fax 303.467.7248

**Chain of Custody Record**



**TestAmerica Laboratories, Inc.**

**Regulatory Program:**  DW  NPDES  RCRA  Other:

<b>Client Contact</b>		<b>Project Manager:</b> Andy Frebowitz		<b>Site Contact:</b> Mary Kay Bond		<b>Date:</b> 9/11/2017		<b>COC No.:</b>	
TetraTech 234 Mall Boulevard Suite 260 King of Prussia, PA 19406 610-382-1174 610-491-9688		Tel/Fax: 610.382.1170		Lab Contact: Dave Alltucker		Carrier: FedEx		2 of 2 COCs	
Project Name: WE04 Site: WE04 P O # 1132358 (through EarthToxics)		<b>Analysis Turnaround Time</b>		Filtered Sample (Y/N) Perform MS/MSD (Y/N) EPA 537 UCMR3				Sampler: Mary Kay Bond For Lab Use Only: Walk-in Client: Lab Sampling: Job / SDG No.:	
		<input type="checkbox"/> CALENDAR DAYS <input type="checkbox"/> WORKING DAYS TAT if different from Below 21 <input type="checkbox"/> 2 weeks <input type="checkbox"/> 1 week <input type="checkbox"/> 2 days <input type="checkbox"/> 1 day							

Page 475 of 476

Sample Identification	Sample Date	Sample Time	Sample Type (C=Comp, G=Grab)	Matrix	# of Cont.	Filtered Sample (Y/N)	Perform MS/MSD (Y/N)	EPA 537 UCMR3	Sample Specific Notes:
NAWC-091117-RW-317	9/11/2017	14:00	G	DW	2	N	N	Y	
NAWC-091117-FRB-317	9/11/2017	13:55	G	DW	2	N	N	Y	Field Reagent Blank
NAWC-091117-RW-319	9/11/2017	14:25	G	DW	2	N	N	Y	
NAWC-091117-FRB-319	9/11/2017	14:40	G	DW	2	N	N	Y	Field Reagent Blank
NAWC-091117-RW-321	9/11/2017	15:10	G	DW	2	N	N	Y	
NAWC-091117-FRB-321	9/11/2017	15:05	G	DW	2	N	N	Y	Field Reagent Blank
NAWC-091117-RW-010	9/11/2017	15:45	G	DW	2	N	N	Y	
NAWC-091117-FRB-010	9/11/2017	15:40	G	DW	2	N	N	Y	Field Reagent Blank
NAWC-091117-RW-162	9/11/2017	11:20	G	DW	2	N	N	Y	
NAWC-091117-FRB-162	9/11/2017	11:15	G	DW	2	N	N	Y	Field Reagent Blank
WGNA-091117-DUP09	9/11/2017	07:00	G	DW	2	N	N	Y	Duplicate

<b>Preservation Used:</b> 1= Ice, 2= HCl; 3= H2SO4; 4=HNO3; 5=NaOH; 6= Other: Trizma		<b>Sample Disposal ( A fee may be assessed if samples are retained longer than 1 month)</b>	
<b>Possible Hazard Identification:</b> Comments Section if the lab is to dispose of the sample.		<input type="checkbox"/> Return to Client <input type="checkbox"/> Disposal by Lab <input type="checkbox"/> Archive for _____ Months	
<input type="checkbox"/> Non-Hazard <input type="checkbox"/> Flammable <input type="checkbox"/> Skin Irritant <input type="checkbox"/> Poison B <input type="checkbox"/> Unknown			

**Fed Ex Tracking: 770221957389**

Custody Seals Intact: <input type="checkbox"/> Yes <input type="checkbox"/> No		Custody Seal No.:		Cooler Temp. (°C): Obs'd: <u>1.9</u> Corr'd: <u>    </u>		Therm ID No.: <u>AK-1</u>	
Relinquished by: <i>Mary Kay Bond</i>	Company: Tetra Tech	Date/Time: 9/11/2017 18:00	Received by: <i>[Signature]</i>	Company: <i>TAG</i>	Date/Time: 9/11/2017 9:30		
Relinquished by:	Company:	Date/Time:	Received by:	Company:	Date/Time:		
Relinquished by:	Company:	Date/Time:	Received in Laboratory by:	Company:	Date/Time:		

**Job Narrative  
320-31468-1**

**Receipt**

The samples were received on 9/12/2017 2:21 PM; the samples arrived in good condition, properly preserved and, where required, on ice. The temperatures of the 2 coolers at receipt time were 1.5° C and 2.1° C.

**Receipt Exceptions**

The container label for the following samples did not match the information listed on the Chain-of-Custody (COC):  
NAWC-091117-RW-106 (320-31468-1), NAWC-091117-FRB-106 (320-31468-2), NAWC-091117-RW-060 (320-31468-3),  
NAWC-091117-FRB-060 (320-31468-4), NAWC-091117-RW-314 (320-31468-5), NAWC-091117-FRB-314 (320-31468-6),  
NAWC-091117-RW-258 (320-31468-7), NAWC-091117-FRB-258 (320-31468-8), NAWC-091117-RW-048 (320-31468-9),  
NAWC-091117-FRB-048 (320-31468-10), NAWC-091117-RW-145 (320-31468-11), NAWC-091117-FRB-145 (320-31468-12),  
NAWC-091117-RW-317 (320-31468-13), NAWC-091117-FRB-317 (320-31468-14), NAWC-091117-RW-319 (320-31468-15),  
NAWC-091117-FRB-319 (320-31468-16), NAWC-091117-RW-321 (320-31468-17), NAWC-091117-FRB-321 (320-31468-18),  
NAWC-091117-RW-010 (320-31468-19), NAWC-091117-FRB-010 (320-31468-20), NAWC-091117-RW-162 (320-31468-21),  
NAWC-091117-FRB-162 (320-31468-22) and WGNA-091117-DUP09 (320-31468-23). The container labels list WGNA-, while the COC lists NAWC-. The samples were logged in according to the CoC.

**LCMS**

Method(s) 537: The first level standard from the initial calibration curve is used to evaluate the tune criteria. The instrument mass windows are set at +/- 0.5amu; therefore, detection of the analyte serves as verification that the assigned mass is within +/- 0.5amu of the true value, which meets the DoD/DOE QSM tune criterion.

Method(s) 537: Surrogate recovery for the following samples was outside control limits: NAWC-091117-RW-106 (320-31468-1), NAWC-091117-RW-319 (320-31468-15) and (MB 320-184385/1-A). Re-analysis was performed with concurring results. The original analysis has been reported.

No additional analytical or quality issues were noted, other than those described above or in the Definitions/Glossary page.

**Organic Prep**

Method(s) 537: Insufficient sample volume was available to perform a matrix spike/matrix spike duplicate (MS/MSD) associated with preparation batch 320-184382.

Method(s) 537: Insufficient sample volume was available to perform a matrix spike/matrix spike duplicate (MS/MSD) associated with preparation batch 320-184385.

Method(s) 537: The following samples: NAWC-091117-RW-106 (320-31468-1) and NAWC-091117-RW-319 (320-31468-15) were decanted prior to preparation due to particulates in the sample.

No additional analytical or quality issues were noted, other than those described above or in the Definitions/Glossary page.

# Method Summary

Client: Tetra Tech, Inc.  
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-31468-1

---

---

<b>Method</b>	<b>Method Description</b>	<b>Protocol</b>	<b>Laboratory</b>
537	Perfluorinated Alkyl Acids (LC/MS)	EPA	TAL SAC

**Protocol References:**

EPA = US Environmental Protection Agency

**Laboratory References:**

TAL SAC = TestAmerica Sacramento, 880 Riverside Parkway, West Sacramento, CA 95605, TEL (916)373-5600

# Sample Summary

Client: Tetra Tech, Inc.

TestAmerica Job ID: 320-31468-1

Project/Site: Warminster: PFAS, NAS JRB Willow Grove

Lab Sample ID	Client Sample ID	Matrix	Collected	Received
320-31468-1	NAWC-091117-RW-106	Water	09/11/17 09:40	09/12/17 14:21
320-31468-2	NAWC-091117-FRB-106	Water	09/11/17 09:35	09/12/17 14:21
320-31468-3	NAWC-091117-RW-060	Water	09/11/17 09:55	09/12/17 14:21
320-31468-4	NAWC-091117-FRB-060	Water	09/11/17 09:50	09/12/17 14:21
320-31468-5	NAWC-091117-RW-314	Water	09/11/17 10:25	09/12/17 14:21
320-31468-6	NAWC-091117-FRB-314	Water	09/11/17 10:20	09/12/17 14:21
320-31468-7	NAWC-091117-RW-258	Water	09/11/17 11:00	09/12/17 14:21
320-31468-8	NAWC-091117-FRB-258	Water	09/11/17 10:55	09/12/17 14:21
320-31468-9	NAWC-091117-RW-048	Water	09/11/17 13:05	09/12/17 14:21
320-31468-10	NAWC-091117-FRB-048	Water	09/11/17 13:00	09/12/17 14:21
320-31468-11	NAWC-091117-RW-145	Water	09/11/17 13:35	09/12/17 14:21
320-31468-12	NAWC-091117-FRB-145	Water	09/11/17 13:30	09/12/17 14:21
320-31468-13	NAWC-091117-RW-317	Water	09/11/17 14:00	09/12/17 14:21
320-31468-14	NAWC-091117-FRB-317	Water	09/11/17 13:55	09/12/17 14:21
320-31468-15	NAWC-091117-RW-319	Water	09/11/17 14:25	09/12/17 14:21
320-31468-16	NAWC-091117-FRB-319	Water	09/11/17 14:40	09/12/17 14:21
320-31468-17	NAWC-091117-RW-321	Water	09/11/17 15:10	09/12/17 14:21
320-31468-18	NAWC-091117-FRB-321	Water	09/11/17 15:05	09/12/17 14:21
320-31468-19	NAWC-091117-RW-010	Water	09/11/17 15:45	09/12/17 14:21
320-31468-20	NAWC-091117-FRB-010	Water	09/11/17 15:40	09/12/17 14:21
320-31468-21	NAWC-091117-RW-162	Water	09/11/17 11:20	09/12/17 14:21
320-31468-22	NAWC-091117-FRB-162	Water	09/11/17 11:15	09/12/17 14:21
320-31468-23	WGNA-091117-DUP09	Water	09/11/17 07:00	09/12/17 14:21

FORM II  
LCMS SURROGATE RECOVERY

Lab Name: TestAmerica Sacramento

Job No.: 320-31468-1

SDG No.: \_\_\_\_\_

Matrix: Water

Level: Low

GC Column (1): GeminiC18 3 ID: 3 (mm)

Client Sample ID	Lab Sample ID	PFHxA #	PFDA #
NAWC-091117-RW-106	320-31468-1	67 Q	100
NAWC-091117-FRB-106	320-31468-2	82	105
NAWC-091117-RW-060	320-31468-3	71	114
NAWC-091117-FRB-060	320-31468-4	86	107
NAWC-091117-RW-314	320-31468-5	72	104
NAWC-091117-FRB-314	320-31468-6	82	102
NAWC-091117-RW-258	320-31468-7	72	98
NAWC-091117-FRB-258	320-31468-8	86	101
NAWC-091117-RW-048	320-31468-9	74	111
NAWC-091117-FRB-048	320-31468-10	84	102
NAWC-091117-RW-145	320-31468-11	74	115
NAWC-091117-FRB-145	320-31468-12	83	100
NAWC-091117-RW-317	320-31468-13	78	116
NAWC-091117-FRB-317	320-31468-14	83	97
NAWC-091117-RW-319	320-31468-15	61 Q	83
NAWC-091117-FRB-319	320-31468-16	82	124
NAWC-091117-RW-321	320-31468-17	76	106
NAWC-091117-FRB-321	320-31468-18	84	104
NAWC-091117-RW-010	320-31468-19	75	104
NAWC-091117-FRB-010	320-31468-20	83	97
NAWC-091117-RW-162	320-31468-21	78	111
NAWC-091117-FRB-162	320-31468-22	91	129
WGNA-091117-DUP09	320-31468-23	75	125
	MB 320-184382/1-A	90	111
	MB 320-184385/1-A	87	143 Q
	LCS 320-184382/2-A	91	115
	LCSD 320-184382/3-A	86	110
	LLCS 320-184385/2-A	90	113

PFHxA = 13C2 PFHxA  
PFDA = 13C2 PFDA

QC LIMITS  
70-130  
70-130

# Column to be used to flag recovery values

FORM II  
LCMS SURROGATE RECOVERY

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1

SDG No.: \_\_\_\_\_

Matrix: Water Level: Low

GC Column (1): GeminiC18 3 ID: 3 (mm)

Client Sample ID	Lab Sample ID	PFHxA #	PFDA #
	LLCSD 320-184385/3-A	93	124

PFHxA = 13C2 PFHxA  
PFDA = 13C2 PFDA

QC LIMITS  
70-130  
70-130

# Column to be used to flag recovery values

FORM II 537

FORM III  
LCMS LAB CONTROL SAMPLE RECOVERY

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Matrix: Water Level: Low Lab File ID: 2017.09.19\_537A\_012.d  
 Lab ID: LCS 320-184382/2-A Client ID: \_\_\_\_\_

COMPOUND	SPIKE ADDED (ng/L)	LCS CONCENTRATION (ng/L)	LCS % REC	QC LIMITS REC	#
Perfluorooctanesulfonic acid (PFOS)	222	198	89	70-130	M
Perfluorooctanoic acid (PFOA)	111	103	93	70-130	
Perfluorononanoic acid (PFNA)	111	99.7	90	70-130	
Perfluorohexanesulfonic acid (PFHxS)	167	150	90	70-130	
Perfluoroheptanoic acid (PFHpA)	55.6	50.5	91	70-130	
Perfluorobutanesulfonic acid (PFBS)	500	408	82	70-130	

# Column to be used to flag recovery and RPD values

FORM III  
LCMS LAB CONTROL SAMPLE DUPLICATE RECOVERY

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1

SDG No.: \_\_\_\_\_

Matrix: Water Level: Low Lab File ID: 2017.09.19\_537A\_013.d

Lab ID: LCSD 320-184382/3-A Client ID: \_\_\_\_\_

COMPOUND	SPIKE ADDED (ng/L)	LCSD CONCENTRATION (ng/L)	LCSD % REC	% RPD	QC LIMITS		#
					RPD	REC	
Perfluorooctanesulfonic acid (PFOS)	222	188	84	5	30	70-130	M
Perfluorooctanoic acid (PFOA)	111	96.8	87	7	30	70-130	
Perfluorononanoic acid (PFNA)	111	93.6	84	6	30	70-130	
Perfluorohexanesulfonic acid (PFHxS)	167	143	86	5	30	70-130	
Perfluoroheptanoic acid (PFHpA)	55.6	48.7	88	3	30	70-130	
Perfluorobutanesulfonic acid (PFBS)	500	403	81	1	30	70-130	

# Column to be used to flag recovery and RPD values



FORM III  
LCMS LOW LEVEL CONTROL SAMPLE RECOVERY

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1

SDG No.: \_\_\_\_\_

Matrix: Water Level: Low Lab File ID: 2017.09.19\_537A\_004.d

Lab ID: LLCS 320-184385/2-A Client ID: \_\_\_\_\_

COMPOUND	SPIKE ADDED (ng/L)	LLCS CONCENTRATION (ng/L)	LLCS % REC	QC LIMITS REC	#
Perfluorooctanesulfonic acid (PFOS)	40.0	36.6 J	91	50-150	M
Perfluorooctanoic acid (PFOA)	20.0	18.4 J	92	50-150	
Perfluorononanoic acid (PFNA)	20.0	18.5 J	93	50-150	
Perfluorohexanesulfonic acid (PFHxS)	30.0	28.9 J	96	50-150	
Perfluoroheptanoic acid (PFHpA)	10.0	10.2	102	50-150	
Perfluorobutanesulfonic acid (PFBS)	90.0	86.1 J	96	50-150	

# Column to be used to flag recovery and RPD values

FORM III  
LCMS LOW LEVEL CONTROL STANDARD DUPLICATE RECOVERY

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1

SDG No.: \_\_\_\_\_

Matrix: Water Level: Low Lab File ID: 2017.09.19\_537A\_005.d

Lab ID: LLCSD 320-184385/3-A Client ID: \_\_\_\_\_

COMPOUND	SPIKE ADDED (ng/L)	LLCSD CONCENTRATION (ng/L)	LLCSD % REC	% RPD	QC LIMITS		#
					RPD	REC	
Perfluorooctanesulfonic acid (PFOS)	40.0	36.2 J	90	1	50	50-150	M
Perfluorooctanoic acid (PFOA)	20.0	18.7 J	93	1	50	50-150	
Perfluorononanoic acid (PFNA)	20.0	19.0 J	95	3	50	50-150	
Perfluorohexanesulfonic acid (PFHxS)	30.0	29.4 J	98	2	50	50-150	
Perfluoroheptanoic acid (PFHpA)	10.0	10.8	108	6	50	50-150	
Perfluorobutanesulfonic acid (PFBS)	90.0	89.0 J	99	3	50	50-150	

# Column to be used to flag recovery and RPD values

FORM IV  
LCMS METHOD BLANK SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Lab File ID: 2017.09.19\_537A\_011.d Lab Sample ID: MB 320-184382/1-A  
 Matrix: Water Date Extracted: 09/14/2017 09:17  
 Instrument ID: A8\_N Date Analyzed: 09/20/2017 04:35  
 Level: (Low/Med) Low

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES:

CLIENT SAMPLE ID	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED
	LCS 320-184382/2-A	2017.09.19_537A_012.d	09/20/2017 04:40
	LCSD 320-184382/3-A	2017.09.19_537A_013.d	09/20/2017 04:45
NAWC-091117-RW-106	320-31468-1	2017.09.19_537A_014.d	09/20/2017 04:49
NAWC-091117-FRB-106	320-31468-2	2017.09.19_537A_015.d	09/20/2017 04:54
NAWC-091117-RW-060	320-31468-3	2017.09.19_537A_016.d	09/20/2017 04:59
NAWC-091117-FRB-060	320-31468-4	2017.09.19_537A_017.d	09/20/2017 05:04
NAWC-091117-RW-314	320-31468-5	2017.09.19_537A_018.d	09/20/2017 05:08
NAWC-091117-FRB-314	320-31468-6	2017.09.19_537A_019.d	09/20/2017 05:13
NAWC-091117-RW-258	320-31468-7	2017.09.19_537A_020.d	09/20/2017 05:18
NAWC-091117-FRB-258	320-31468-8	2017.09.19_537A_023.d	09/20/2017 05:32
NAWC-091117-RW-048	320-31468-9	2017.09.19_537A_024.d	09/20/2017 05:37
NAWC-091117-FRB-048	320-31468-10	2017.09.19_537A_025.d	09/20/2017 05:42
NAWC-091117-RW-145	320-31468-11	2017.09.19_537A_026.d	09/20/2017 05:46
NAWC-091117-FRB-145	320-31468-12	2017.09.19_537A_027.d	09/20/2017 05:51
NAWC-091117-RW-317	320-31468-13	2017.09.19_537A_028.d	09/20/2017 05:56
NAWC-091117-FRB-317	320-31468-14	2017.09.19_537A_029.d	09/20/2017 06:01
NAWC-091117-RW-319	320-31468-15	2017.09.19_537A_030.d	09/20/2017 06:05
NAWC-091117-FRB-319	320-31468-16	2017.09.19_537A_031.d	09/20/2017 06:10
NAWC-091117-RW-321	320-31468-17	2017.09.19_537A_032.d	09/20/2017 06:15
NAWC-091117-FRB-321	320-31468-18	2017.09.19_537A_035.d	09/20/2017 06:29
NAWC-091117-RW-010	320-31468-19	2017.09.19_537A_036.d	09/20/2017 06:34
NAWC-091117-FRB-010	320-31468-20	2017.09.19_537A_037.d	09/20/2017 06:39

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: \_\_\_\_\_ Lab Sample ID: MB 320-184382/1-A  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_011.d  
 Analysis Method: 537 Date Collected: \_\_\_\_\_  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:17  
 Sample wt/vol: 250 (mL) Date Analyzed: 09/20/2017 04:35  
 Con. Extract Vol.: 1.0 (mL) Dilution Factor: 1  
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185407 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	8.0	U	20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.0	U	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	90		70-130
STL00996	13C2 PFDA	111		70-130

FORM IV  
LCMS METHOD BLANK SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Lab File ID: 2017.09.19\_537A\_003.d Lab Sample ID: MB 320-184385/1-A  
 Matrix: Water Date Extracted: 09/14/2017 09:29  
 Instrument ID: A8\_N Date Analyzed: 09/20/2017 03:57  
 Level: (Low/Med) Low

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES:

CLIENT SAMPLE ID	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED
	LLCS 320-184385/2-A	2017.09.19_537A_004.d	09/20/2017 04:02
	LLCSD 320-184385/3-A	2017.09.19_537A_005.d	09/20/2017 04:07
NAWC-091117-RW-162	320-31468-21	2017.09.19_537A_006.d	09/20/2017 04:11
NAWC-091117-FRB-162	320-31468-22	2017.09.19_537A_007.d	09/20/2017 04:16
WGNA-091117-DUP09	320-31468-23	2017.09.19_537A_008.d	09/20/2017 04:21

FORM I  
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Client Sample ID: \_\_\_\_\_ Lab Sample ID: MB 320-184385/1-A  
 Matrix: Water Lab File ID: 2017.09.19\_537A\_003.d  
 Analysis Method: 537 Date Collected: \_\_\_\_\_  
 Extraction Method: 537 Date Extracted: 09/14/2017 09:29  
 Sample wt/vol: 250 (mL) Date Analyzed: 09/20/2017 03:57  
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1  
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)  
 % Moisture: \_\_\_\_\_ GPC Cleanup: (Y/N) N  
 Analysis Batch No.: 185406 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	8.0	U	20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.0	U	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	87		70-130
STL00996	13C2 PFDA	143	Q	70-130

FORM VIII  
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Instrument ID: A8\_N Calibration Start Date: 09/20/2017 02:56  
 GC Column: GeminiC18 3x100 ID: 3(mm) Calibration End Date: 09/20/2017 03:19  
 Calibration ID: 34457

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
INITIAL CALIBRATION MEAN AREA AND MEAN RT	2116635	1.86	5570738	2.11		
UPPER LIMIT	3174953	2.36	8356107	2.61		
LOWER LIMIT	1058318	1.36	2785369	1.61		
LAB SAMPLE ID	CLIENT SAMPLE ID					
CCVL 320-185329/11		2252465	1.85	5723538	2.10	
ICV 320-185329/13		2616480	1.85	7294448	2.10	
CCV 320-185406/1 CCVIS		1946548	1.85	5210623	2.10	
MB 320-184385/1-A		2539018	1.85	6194895	2.10	
LLCS 320-184385/2-A		2322795	1.85	5655681	2.10	
LLCSD 320-184385/3-A		2191521	1.84	5502551	2.09	
320-31468-21	NAWC-091117-RW-162	2350014	1.84	5861531	2.10	
320-31468-22	NAWC-091117-FRB-162	2344211	1.85	6003115	2.10	
320-31468-23	WGNA-091117-DUP09	2370526	1.85	6043874	2.10	
CCV 320-185406/9 CCVIS		2062556	1.85	5491922	2.10	
CCV 320-185407/9 CCVIS		2062556	1.85	5491922	2.10	
MB 320-184382/1-A		2402894	1.85	5785526	2.10	
LCS 320-184382/2-A		2181509	1.84	5704391	2.09	
LCSD 320-184382/3-A		2332217	1.85	5855728	2.10	
320-31468-1	NAWC-091117-RW-106	2290728	1.84	5860369	2.09	
320-31468-2	NAWC-091117-FRB-106	2577088	1.84	6073981	2.09	
320-31468-3	NAWC-091117-RW-060	2387971	1.85	6309998	2.10	
320-31468-4	NAWC-091117-FRB-060	2308276	1.85	5696853	2.10	
320-31468-5	NAWC-091117-RW-314	2570115	1.85	6192393	2.10	
320-31468-6	NAWC-091117-FRB-314	2574796	1.85	6281693	2.10	
320-31468-7	NAWC-091117-RW-258	2394768	1.84	6099250	2.10	
CCV 320-185407/21 CCVIS		2036337	1.85	5320724	2.10	
CCV 320-185408/21 CCVIS		2036337	1.85	5320724	2.10	
320-31468-8	NAWC-091117-FRB-258	2497710	1.85	6286206	2.10	
320-31468-9	NAWC-091117-RW-048	2501111	1.85	6308482	2.10	
320-31468-10	NAWC-091117-FRB-048	2637228	1.85	6282400	2.10	
320-31468-11	NAWC-091117-RW-145	2432580	1.84	6418340	2.10	
320-31468-12	NAWC-091117-FRB-145	2685353	1.84	6382119	2.10	

13PFOA = 13C2-PFOA

PFOS = 13C4 PFOS

Area Limit = 50%-150% of internal standard area

RT Limit = ± 0.5 minutes of internal standard RT

# Column used to flag values outside QC limits

FORM VIII  
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Instrument ID: A8\_N Calibration Start Date: 09/20/2017 02:56  
 GC Column: GeminiC18 3x100 ID: 3(mm) Calibration End Date: 09/20/2017 03:19  
 Calibration ID: 34457

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
INITIAL CALIBRATION MEAN AREA AND MEAN RT	2116635	1.86	5570738	2.11		
UPPER LIMIT	3174953	2.36	8356107	2.61		
LOWER LIMIT	1058318	1.36	2785369	1.61		
LAB SAMPLE ID	CLIENT SAMPLE ID					
320-31468-13	NAWC-091117-RW-317	2501311	1.84	6642891	2.09	
320-31468-14	NAWC-091117-FRB-317	2631497	1.84	6447036	2.09	
320-31468-15	NAWC-091117-RW-319	2337114	1.84	6427066	2.09	
320-31468-16	NAWC-091117-FRB-319	2681945	1.84	6402518	2.09	
320-31468-17	NAWC-091117-RW-321	2557163	1.84	6417541	2.09	
CCV 320-185408/33 CCVIS		2192291	1.84	5605406	2.09	
CCV 320-185409/33 CCVIS		2192291	1.84	5605406	2.09	
320-31468-18	NAWC-091117-FRB-321	2584590	1.84	6389473	2.10	
320-31468-19	NAWC-091117-RW-010	2457461	1.84	6222745	2.09	
320-31468-20	NAWC-091117-FRB-010	2679499	1.84	6439213	2.09	
CCV 320-185409/38 CCVIS		2137164	1.84	5388320	2.09	

13PFOA = 13C2-PFOA  
 PFOS = 13C4 PFOS

Area Limit = 50%-150% of internal standard area  
 RT Limit = ± 0.5 minutes of internal standard RT

# Column used to flag values outside QC limits



FORM VIII  
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Sample No.: CCV 320-185406/1 Date Analyzed: 09/20/2017 03:48  
 Instrument ID: A8\_N GC Column: GeminiC18 3x100 ID: 3 (mm)  
 Lab File ID (Standard): 2017.09.19\_537A\_001 Heated Purge: (Y/N) N  
 Calibration ID: 34457

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	1946548	1.85	5210623	2.10		
UPPER LIMIT	2725167	2.35	7294872	2.60		
LOWER LIMIT	1362584	1.35	3647436	1.60		
LAB SAMPLE ID	CLIENT SAMPLE ID					
MB 320-184385/1-A		2539018	1.85	6194895	2.10	
LLCS 320-184385/2-A		2322795	1.85	5655681	2.10	
LLCSD 320-184385/3-A		2191521	1.84	5502551	2.09	
320-31468-21	NAWC-091117-RW-162	2350014	1.84	5861531	2.10	
320-31468-22	NAWC-091117-FRB-162	2344211	1.85	6003115	2.10	
320-31468-23	WGNA-091117-DUP09	2370526	1.85	6043874	2.10	

13PFOA = 13C2-PFOA  
 13PFOA = 13C2-PFOA  
 PFOS = 13C4 PFOS  
 PFOS = 13C4 PFOS  
 Area Limit = 70%-140% of internal standard area  
 RT Limit = ± 0.5 minutes of internal standard RT

# Column used to flag values outside QC limits

FORM VIII  
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Sample No.: CCV 320-185406/9 Date Analyzed: 09/20/2017 04:26  
 Instrument ID: A8\_N GC Column: GeminiC18 3x100 ID: 3 (mm)  
 Lab File ID (Standard): 2017.09.19\_537A\_009 Heated Purge: (Y/N) N  
 Calibration ID: 34457

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
<u>12/24 HOUR STD</u>	2062556	1.85	5491922	2.10		
UPPER LIMIT	2887578	2.35	7688691	2.60		
LOWER LIMIT	1443789	1.35	3844345	1.60		
LAB SAMPLE ID	CLIENT SAMPLE ID					
MB 320-184385/1-A		2539018	1.85	6194895	2.10	
LLCS 320-184385/2-A		2322795	1.85	5655681	2.10	
LLCSD 320-184385/3-A		2191521	1.84	5502551	2.09	
320-31468-21	NAWC-091117-RW-162	2350014	1.84	5861531	2.10	
320-31468-22	NAWC-091117-FRB-162	2344211	1.85	6003115	2.10	
320-31468-23	WGNA-091117-DUP09	2370526	1.85	6043874	2.10	

13PFOA = 13C2-PFOA  
 13PFOA = 13C2-PFOA  
 PFOS = 13C4 PFOS  
 PFOS = 13C4 PFOS  
 Area Limit = 70%-140% of internal standard area  
 RT Limit = ± 0.5 minutes of internal standard RT

# Column used to flag values outside QC limits

FORM VIII  
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Sample No.: CCV 320-185407/9 Date Analyzed: 09/20/2017 04:26  
 Instrument ID: A8\_N GC Column: GeminiC18 3x100 ID: 3 (mm)  
 Lab File ID (Standard): 2017.09.19\_537A\_009 Heated Purge: (Y/N) N  
 Calibration ID: 34457

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	2062556	1.85	5491922	2.10		
UPPER LIMIT	2887578	2.35	7688691	2.60		
LOWER LIMIT	1443789	1.35	3844345	1.60		
LAB SAMPLE ID	CLIENT SAMPLE ID					
MB 320-184382/1-A		2402894	1.85	5785526	2.10	
LCS 320-184382/2-A		2181509	1.84	5704391	2.09	
LCSD 320-184382/3-A		2332217	1.85	5855728	2.10	
320-31468-1	NAWC-091117-RW-106	2290728	1.84	5860369	2.09	
320-31468-2	NAWC-091117-FRB-106	2577088	1.84	6073981	2.09	
320-31468-3	NAWC-091117-RW-060	2387971	1.85	6309998	2.10	
320-31468-4	NAWC-091117-FRB-060	2308276	1.85	5696853	2.10	
320-31468-5	NAWC-091117-RW-314	2570115	1.85	6192393	2.10	
320-31468-6	NAWC-091117-FRB-314	2574796	1.85	6281693	2.10	
320-31468-7	NAWC-091117-RW-258	2394768	1.84	6099250	2.10	

13PFOA = 13C2-PFOA  
 13PFOA = 13C2-PFOA  
 PFOS = 13C4 PFOS  
 PFOS = 13C4 PFOS  
 Area Limit = 70%-140% of internal standard area  
 RT Limit = ± 0.5 minutes of internal standard RT

# Column used to flag values outside QC limits

FORM VIII  
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Sample No.: CCV 320-185407/21 Date Analyzed: 09/20/2017 05:23  
 Instrument ID: A8\_N GC Column: GeminiC18 3x100 ID: 3 (mm)  
 Lab File ID (Standard): 2017.09.19\_537A\_021 Heated Purge: (Y/N) N  
 Calibration ID: 34457

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	2036337	1.85	5320724	2.10		
UPPER LIMIT	2850872	2.35	7449014	2.60		
LOWER LIMIT	1425436	1.35	3724507	1.60		
LAB SAMPLE ID	CLIENT SAMPLE ID					
MB 320-184382/1-A		2402894	1.85	5785526	2.10	
LCS 320-184382/2-A		2181509	1.84	5704391	2.09	
LCSD 320-184382/3-A		2332217	1.85	5855728	2.10	
320-31468-1	NAWC-091117-RW-106	2290728	1.84	5860369	2.09	
320-31468-2	NAWC-091117-FRB-106	2577088	1.84	6073981	2.09	
320-31468-3	NAWC-091117-RW-060	2387971	1.85	6309998	2.10	
320-31468-4	NAWC-091117-FRB-060	2308276	1.85	5696853	2.10	
320-31468-5	NAWC-091117-RW-314	2570115	1.85	6192393	2.10	
320-31468-6	NAWC-091117-FRB-314	2574796	1.85	6281693	2.10	
320-31468-7	NAWC-091117-RW-258	2394768	1.84	6099250	2.10	

13PFOA = 13C2-PFOA  
 13PFOA = 13C2-PFOA  
 PFOS = 13C4 PFOS  
 PFOS = 13C4 PFOS  
 Area Limit = 70%-140% of internal standard area  
 RT Limit = ± 0.5 minutes of internal standard RT

# Column used to flag values outside QC limits

FORM VIII  
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Sample No.: CCV 320-185408/21 Date Analyzed: 09/20/2017 05:23  
 Instrument ID: A8\_N GC Column: GeminiC18 3x100 ID: 3 (mm)  
 Lab File ID (Standard): 2017.09.19\_537A\_021 Heated Purge: (Y/N) N  
 Calibration ID: 34457

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	2036337	1.85	5320724	2.10		
UPPER LIMIT	2850872	2.35	7449014	2.60		
LOWER LIMIT	1425436	1.35	3724507	1.60		
LAB SAMPLE ID	CLIENT SAMPLE ID					
320-31468-8	NAWC-091117-FRB-258	2497710	1.85	6286206	2.10	
320-31468-9	NAWC-091117-RW-048	2501111	1.85	6308482	2.10	
320-31468-10	NAWC-091117-FRB-048	2637228	1.85	6282400	2.10	
320-31468-11	NAWC-091117-RW-145	2432580	1.84	6418340	2.10	
320-31468-12	NAWC-091117-FRB-145	2685353	1.84	6382119	2.10	
320-31468-13	NAWC-091117-RW-317	2501311	1.84	6642891	2.09	
320-31468-14	NAWC-091117-FRB-317	2631497	1.84	6447036	2.09	
320-31468-15	NAWC-091117-RW-319	2337114	1.84	6427066	2.09	
320-31468-16	NAWC-091117-FRB-319	2681945	1.84	6402518	2.09	
320-31468-17	NAWC-091117-RW-321	2557163	1.84	6417541	2.09	

13PFOA = 13C2-PFOA  
 13PFOA = 13C2-PFOA  
 PFOS = 13C4 PFOS  
 PFOS = 13C4 PFOS  
 Area Limit = 70%-140% of internal standard area  
 RT Limit = ± 0.5 minutes of internal standard RT

# Column used to flag values outside QC limits

FORM VIII  
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Sample No.: CCV 320-185408/33 Date Analyzed: 09/20/2017 06:20  
 Instrument ID: A8\_N GC Column: GeminiC18 3x100 ID: 3 (mm)  
 Lab File ID (Standard): 2017.09.19\_537A\_033 Heated Purge: (Y/N) N  
 Calibration ID: 34457

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	2192291	1.84	5605406	2.09		
UPPER LIMIT	3069207	2.34	7847568	2.59		
LOWER LIMIT	1534604	1.34	3923784	1.59		
LAB SAMPLE ID	CLIENT SAMPLE ID					
320-31468-8	NAWC-091117-FRB-258	2497710	1.85	6286206	2.10	
320-31468-9	NAWC-091117-RW-048	2501111	1.85	6308482	2.10	
320-31468-10	NAWC-091117-FRB-048	2637228	1.85	6282400	2.10	
320-31468-11	NAWC-091117-RW-145	2432580	1.84	6418340	2.10	
320-31468-12	NAWC-091117-FRB-145	2685353	1.84	6382119	2.10	
320-31468-13	NAWC-091117-RW-317	2501311	1.84	6642891	2.09	
320-31468-14	NAWC-091117-FRB-317	2631497	1.84	6447036	2.09	
320-31468-15	NAWC-091117-RW-319	2337114	1.84	6427066	2.09	
320-31468-16	NAWC-091117-FRB-319	2681945	1.84	6402518	2.09	
320-31468-17	NAWC-091117-RW-321	2557163	1.84	6417541	2.09	

13PFOA = 13C2-PFOA  
 13PFOA = 13C2-PFOA  
 PFOS = 13C4 PFOS  
 PFOS = 13C4 PFOS  
 Area Limit = 70%-140% of internal standard area  
 RT Limit = ± 0.5 minutes of internal standard RT

# Column used to flag values outside QC limits

FORM VIII  
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Sample No.: CCV 320-185409/33 Date Analyzed: 09/20/2017 06:20  
 Instrument ID: A8\_N GC Column: GeminiC18 3x100 ID: 3 (mm)  
 Lab File ID (Standard): 2017.09.19\_537A\_033 Heated Purge: (Y/N) N  
 Calibration ID: 34457

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	2192291	1.84	5605406	2.09		
UPPER LIMIT	3069207	2.34	7847568	2.59		
LOWER LIMIT	1534604	1.34	3923784	1.59		
LAB SAMPLE ID	CLIENT SAMPLE ID					
320-31468-18	NAWC-091117-FRB-321	2584590	1.84	6389473	2.10	
320-31468-19	NAWC-091117-RW-010	2457461	1.84	6222745	2.09	
320-31468-20	NAWC-091117-FRB-010	2679499	1.84	6439213	2.09	

13PFOA = 13C2-PFOA  
 13PFOA = 13C2-PFOA  
 PFOS = 13C4 PFOS  
 PFOS = 13C4 PFOS  
 Area Limit = 70%-140% of internal standard area  
 RT Limit = ± 0.5 minutes of internal standard RT

# Column used to flag values outside QC limits

FORM VIII  
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Sample No.: CCV 320-185409/38 Date Analyzed: 09/20/2017 06:43  
 Instrument ID: A8\_N GC Column: GeminiC18 3x100 ID: 3 (mm)  
 Lab File ID (Standard): 2017.09.19\_537A\_038 Heated Purge: (Y/N) N  
 Calibration ID: 34457

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	2137164	1.84	5388320	2.09		
UPPER LIMIT	2992030	2.34	7543648	2.59		
LOWER LIMIT	1496015	1.34	3771824	1.59		
LAB SAMPLE ID	CLIENT SAMPLE ID					
320-31468-18	NAWC-091117-FRB-321	2584590	1.84	6389473	2.10	
320-31468-19	NAWC-091117-RW-010	2457461	1.84	6222745	2.09	
320-31468-20	NAWC-091117-FRB-010	2679499	1.84	6439213	2.09	

13PFOA = 13C2-PFOA  
 13PFOA = 13C2-PFOA  
 PFOS = 13C4 PFOS  
 PFOS = 13C4 PFOS  
 Area Limit = 70%-140% of internal standard area  
 RT Limit = ± 0.5 minutes of internal standard RT

# Column used to flag values outside QC limits



FORM VI  
LCMS BY INTERNAL STANDARD - INITIAL CALIBRATION DATA  
CURVE EVALUATION

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1 Analy Batch No.: 185329

SDG No.: \_\_\_\_\_

Instrument ID: A8\_N GC Column: GeminiC18 3 ID: 3(mm) Heated Purge: (Y/N) N

Calibration Start Date: 09/20/2017 02:56 Calibration End Date: 09/20/2017 03:19 Calibration ID: 34457

Calibration Files:

LEVEL:	LAB SAMPLE ID:	LAB FILE ID:
Level 1	IC 320-185329/4	2017.09.19_537ICAL_004.d
Level 2	IC 320-185329/5	2017.09.19_537ICAL_005.d
Level 3	IC 320-185329/6	2017.09.19_537ICAL_006.d
Level 4	IC 320-185329/7	2017.09.19_537ICAL_007.d
Level 5	IC 320-185329/8	2017.09.19_537ICAL_008.d
Level 6	IC 320-185329/9	2017.09.19_537ICAL_009.d

ANALYTE	RRF					CURVE TYPE	COEFFICIENT			#	MIN RRF	%RSD	#	MAX %RSD	R <sup>2</sup> OR COD	#	MIN R <sup>2</sup> OR COD
	LVL 1 LVL 6	LVL 2	LVL 3	LVL 4	LVL 5		B	M1	M2								
Perfluorobutanesulfonic acid (PFBS)	1.1549 0.7675	1.2218	1.1299	0.9825	0.8671	QuaF		1.2127	-0.002495					1.0000			0.9600
Perfluoroheptanoic acid (PFHpA)	0.9156 0.9157	1.0104	0.9599	0.9323	0.9167	Ave		0.9418			4.0		30.0				
Perfluorohexanesulfonic acid (PFHxS)	1.6240 1.5024	1.7562	1.6778	1.6725	1.5962	Ave		1.6382			5.3		30.0				
Perfluorooctanoic acid (PFOA)	0.8827 0.9310	0.9355	0.9297	0.9101	0.9278	Ave		0.9195			2.2		30.0				
Perfluorooctanesulfonic acid (PFOS)	0.8786 0.9472	0.9205	0.9514	0.9450	0.9475	Ave		0.9317			3.0		30.0				
Perfluorononanoic acid (PFNA)	0.6171 0.6192	0.6458	0.6231	0.6183	0.6076	Ave		0.6218			2.1		30.0				
13C2 PFHxA	1.1170 1.2085	1.1856	1.1778	1.1659	1.1757	Ave		1.1718			2.6		30.0				
13C2 PFDA	0.5262 0.5719	0.5663	0.5603	0.5520	0.5699	Ave		0.5578			3.1		30.0				

Note: The M1 coefficient is the same as Ave RRF for an Ave curve type.

FORM VI  
 LCMS BY INTERNAL STANDARD - INITIAL CALIBRATION DATA  
 RESPONSE AND CONCENTRATION

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1 Analy Batch No.: 185329

SDG No.: \_\_\_\_\_

Instrument ID: A8\_N GC Column: GeminiC18 3 ID: 3(mm) Heated Purge: (Y/N) N

Calibration Start Date: 09/20/2017 02:56 Calibration End Date: 09/20/2017 03:19 Calibration ID: 34457

Calibration Files:

LEVEL:	LAB SAMPLE ID:	LAB FILE ID:
Level 1	IC 320-185329/4	2017.09.19_537ICAL_004.d
Level 2	IC 320-185329/5	2017.09.19_537ICAL_005.d
Level 3	IC 320-185329/6	2017.09.19_537ICAL_006.d
Level 4	IC 320-185329/7	2017.09.19_537ICAL_007.d
Level 5	IC 320-185329/8	2017.09.19_537ICAL_008.d
Level 6	IC 320-185329/9	2017.09.19_537ICAL_009.d

ANALYTE	IS REF	CURVE TYPE	RESPONSE					CONCENTRATION (NG/ML)				
			LVL 1 LVL 6	LVL 2	LVL 3	LVL 4	LVL 5	LVL 1 LVL 6	LVL 2	LVL 3	LVL 4	LVL 5
Perfluorobutanesulfonic acid (PFBS)	PFOS	QuaF	2072419 26277877	5031340	9714039	16708415	22246597	9.00 180	20.0	45.0	90.0	135
Perfluoroheptanoic acid (PFHpA)	13PF OA	Ave	202553 3731330	492336	996370	1954380	2871658	1.00 20.0	2.22	5.00	10.0	15.0
Perfluorohexanesulfonic acid (PFHxS)	PFOS	Ave	971572 17148552	2411042	4809005	9481986	13653533	3.00 60.0	6.67	15.0	30.0	45.0
Perfluorooctanoic acid (PFOA)	13PF OA	Ave	390753 7591950	912252	1931186	3817782	5816384	2.00 40.0	4.45	10.0	20.0	30.0
Perfluorooctanesulfonic acid (PFOS)	PFOS	Ave	700862 14414630	1684976	3635963	7143258	10806665	4.00 80.0	8.89	20.0	40.0	60.0
Perfluorononanoic acid (PFNA)	13PF OA	Ave	273016 5046017	629304	1293375	2592159	3806555	2.00 40.0	4.45	10.0	20.0	30.0
13C2 PFHxA	13PF OA	Ave	2470192 2461679	2599092	2444565	2443470	2454801	10.0 10.0	10.0	10.0	10.0	10.0
13C2 PFDA	13PF OA	Ave	1163662 1164862	1241510	1162968	1156914	1189895	10.0 10.0	10.0	10.0	10.0	10.0

Curve Type Legend:

Ave = Average ISTD
QuaF = Quadratic ISTD forced zero

FORM VI  
 LCMS BY INTERNAL STANDARD - INITIAL CALIBRATION DATA  
 READBACK PERCENT ERROR

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1 Analy Batch No.: 185329

SDG No.: \_\_\_\_\_


Instrument ID: A8\_N GC Column: GeminiC18 3 ID: 3(mm) Heated Purge: (Y/N) N


Calibration Start Date: 09/20/2017 02:56 Calibration End Date: 09/20/2017 03:19 Calibration ID: 34457

Calibration Files:

LEVEL:	LAB SAMPLE ID:	LAB FILE ID:
Level 1	IC 320-185329/4	2017.09.19_537ICAL_004.d
Level 2	IC 320-185329/5	2017.09.19_537ICAL_005.d
Level 3	IC 320-185329/6	2017.09.19_537ICAL_006.d
Level 4	IC 320-185329/7	2017.09.19_537ICAL_007.d
Level 5	IC 320-185329/8	2017.09.19_537ICAL_008.d
Level 6	IC 320-185329/9	2017.09.19_537ICAL_009.d

ANALYTE	PERCENT ERROR						PERCENT ERROR LIMIT					
	LVL 1 #	LVL 2 #	LVL 3 #	LVL 4 #	LVL 5 #	LVL 6 #	LVL 1	LVL 2	LVL 3	LVL 4	LVL 5	LVL 6
Perfluorobutanesulfonic acid (PFBS)	-3.0	5.3	3.0	-0.7	-1.6	1.3	50	30	30	30	30	30
Perfluoroheptanoic acid (PFHpA)	-2.8	7.3	1.9	-1.0	-2.7	-2.8	50	30	30	30	30	30
Perfluorohexanesulfonic acid (PFHxS)	-0.9	7.2	2.4	2.1	-2.6	-8.3	50	30	30	30	30	30
Perfluorooctanoic acid (PFOA)	-4.0	1.7	1.1	-1.0	0.9	1.3	50	30	30	30	30	30
Perfluorooctanesulfonic acid (PFOS)	-5.7	-1.2	2.1	1.4	1.7	1.7	50	30	30	30	30	30
Perfluorononanoic acid (PFNA)	-0.8	3.8	0.2	-0.6	-2.3	-0.4	50	30	30	30	30	30
13C2 PFHxA	-4.7	1.2	0.5	-0.5	0.3	3.1	30	30	30	30	30	30
13C2 PFDA	-5.7	1.5	0.5	-1.0	2.2	2.5	30	30	30	30	30	30





FORM VII  
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Lab Sample ID: CCVL 320-185329/11 Calibration Date: 09/20/2017 03:29  
 Instrument ID: A8\_N Calib Start Date: 09/20/2017 02:56  
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 09/20/2017 03:19  
 Lab File ID: 2017.09.19\_537ICAL\_011.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		1.235		21.3	20.0	6.5	50.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9418	0.9779		2.31	2.22	3.8	50.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.638	1.762		7.17	6.67	7.6	50.0
Perfluorooctanoic acid (PFOA)	Ave	0.9195	0.9059		4.38	4.45	-1.5	50.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9317	0.9490		9.06	8.89	1.9	50.0
Perfluorononanoic acid (PFNA)	Ave	0.6218	0.6352		4.54	4.45	2.2	50.0
13C2 PFHxA	Ave	1.172	1.139		9.72	10.0	-2.8	30.0
13C2 PFDA	Ave	0.5578	0.5694		10.2	10.0	2.1	30.0

FORM VII  
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Lab Sample ID: ICV 320-185329/13 Calibration Date: 09/20/2017 03:38  
 Instrument ID: A8\_N Calib Start Date: 09/20/2017 02:56  
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 09/20/2017 03:19  
 Lab File ID: 2017.09.19\_537ICAL\_013.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		0.9069		92.5	100	-7.7	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9418	0.9703		10.3	10.0	3.0	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.638	1.860		22.8	20.1	13.5	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9195	0.9535		21.2	20.5	3.7	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9317	1.134		24.0	19.7	21.8	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6218	0.7173		23.2	20.1	15.3	30.0
13C2 PFHxA	Ave	1.172	1.165		9.94	10.0	-0.6	30.0
13C2 PFDA	Ave	0.5578	0.5781		10.4	10.0	3.6	30.0

FORM VII  
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Lab Sample ID: CCV 320-185406/1 Calibration Date: 09/20/2017 03:48  
 Instrument ID: A8\_N Calib Start Date: 09/20/2017 02:56  
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 09/20/2017 03:19  
 Lab File ID: 2017.09.19\_537A\_001.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		0.8903		139	135	2.7	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9418	0.9394		15.0	15.0	-0.3	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.638	1.592		43.7	45.0	-2.8	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9195	0.9540		31.2	30.0	3.8	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9317	0.9465		61.0	60.0	1.6	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6218	0.6196		29.9	30.0	-0.4	30.0
13C2 PFHxA	Ave	1.172	1.202		10.3	10.0	2.5	30.0
13C2 PFDA	Ave	0.5578	0.5820		10.4	10.0	4.3	30.0



FORM VII  
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Lab Sample ID: CCV 320-185406/9 Calibration Date: 09/20/2017 04:26  
 Instrument ID: A8\_N Calib Start Date: 09/20/2017 02:56  
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 09/20/2017 03:19  
 Lab File ID: 2017.09.19\_537A\_009.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		1.115		45.7	45.0	1.5	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9418	0.9367		4.97	5.00	-0.5	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.638	1.690		15.5	15.0	3.2	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9195	0.8864		9.65	10.0	-3.6	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9317	0.9189		19.7	20.0	-1.4	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6218	0.6261		10.1	10.0	0.7	30.0
13C2 PFHxA	Ave	1.172	1.146		9.78	10.0	-2.2	30.0
13C2 PFDA	Ave	0.5578	0.5476		9.82	10.0	-1.8	30.0

FORM VII  
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Lab Sample ID: CCV 320-185407/9 Calibration Date: 09/20/2017 04:26  
 Instrument ID: A8\_N Calib Start Date: 09/20/2017 02:56  
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 09/20/2017 03:19  
 Lab File ID: 2017.09.19\_537A\_009.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		1.115		45.7	45.0	1.5	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9418	0.9367		4.97	5.00	-0.5	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.638	1.690		15.5	15.0	3.2	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9195	0.8864		9.65	10.0	-3.6	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9317	0.9189		19.7	20.0	-1.4	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6218	0.6261		10.1	10.0	0.7	30.0
13C2 PFHxA	Ave	1.172	1.146		9.78	10.0	-2.2	30.0
13C2 PFDA	Ave	0.5578	0.5476		9.82	10.0	-1.8	30.0

FORM VII  
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Lab Sample ID: CCV 320-185407/21 Calibration Date: 09/20/2017 05:23  
 Instrument ID: A8\_N Calib Start Date: 09/20/2017 02:56  
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 09/20/2017 03:19  
 Lab File ID: 2017.09.19\_537A\_021.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		0.8709		134	135	-0.9	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9418	0.9425		15.0	15.0	0.0	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.638	1.605		44.1	45.0	-2.0	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9195	0.9201		30.0	30.0	0.0	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9317	0.9641		62.1	60.0	3.5	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6218	0.6242		30.1	30.0	0.4	30.0
13C2 PFHxA	Ave	1.172	1.175		10.0	10.0	0.3	30.0
13C2 PFDA	Ave	0.5578	0.5501		9.86	10.0	-1.4	30.0

FORM VII  
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Lab Sample ID: CCV 320-185408/21 Calibration Date: 09/20/2017 05:23  
 Instrument ID: A8\_N Calib Start Date: 09/20/2017 02:56  
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 09/20/2017 03:19  
 Lab File ID: 2017.09.19\_537A\_021.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		0.8709		134	135	-0.9	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9418	0.9425		15.0	15.0	0.0	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.638	1.605		44.1	45.0	-2.0	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9195	0.9201		30.0	30.0	0.0	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9317	0.9641		62.1	60.0	3.5	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6218	0.6242		30.1	30.0	0.4	30.0
13C2 PFHxA	Ave	1.172	1.175		10.0	10.0	0.3	30.0
13C2 PFDA	Ave	0.5578	0.5501		9.86	10.0	-1.4	30.0

FORM VII  
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Lab Sample ID: CCV 320-185408/33 Calibration Date: 09/20/2017 06:20  
 Instrument ID: A8\_N Calib Start Date: 09/20/2017 02:56  
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 09/20/2017 03:19  
 Lab File ID: 2017.09.19\_537A\_033.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		1.118		45.8	45.0	1.8	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9418	0.9457		5.02	5.00	0.4	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.638	1.760		16.1	15.0	7.4	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9195	0.8821		9.60	10.0	-4.1	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9317	0.9386		20.2	20.0	0.7	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6218	0.6156		9.90	10.0	-1.0	30.0
13C2 PFHxA	Ave	1.172	1.175		10.0	10.0	0.3	30.0
13C2 PFDA	Ave	0.5578	0.5469		9.81	10.0	-1.9	30.0

FORM VII  
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Lab Sample ID: CCV 320-185409/33 Calibration Date: 09/20/2017 06:20  
 Instrument ID: A8\_N Calib Start Date: 09/20/2017 02:56  
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 09/20/2017 03:19  
 Lab File ID: 2017.09.19\_537A\_033.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		1.118		45.8	45.0	1.8	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9418	0.9457		5.02	5.00	0.4	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.638	1.760		16.1	15.0	7.4	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9195	0.8821		9.60	10.0	-4.1	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9317	0.9386		20.2	20.0	0.7	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6218	0.6156		9.90	10.0	-1.0	30.0
13C2 PFHxA	Ave	1.172	1.175		10.0	10.0	0.3	30.0
13C2 PFDA	Ave	0.5578	0.5469		9.81	10.0	-1.9	30.0

FORM VII  
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1  
 SDG No.: \_\_\_\_\_  
 Lab Sample ID: CCV 320-185409/38 Calibration Date: 09/20/2017 06:43  
 Instrument ID: A8\_N Calib Start Date: 09/20/2017 02:56  
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 09/20/2017 03:19  
 Lab File ID: 2017.09.19\_537A\_038.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		0.8765		135	135	0.1	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9418	0.8948		14.3	15.0	-5.0	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.638	1.596		43.9	45.0	-2.6	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9195	0.8826		28.8	30.0	-4.0	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9317	0.9548		61.5	60.0	2.5	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6218	0.5935		28.6	30.0	-4.6	30.0
13C2 PFHxA	Ave	1.172	1.209		10.3	10.0	3.2	30.0
13C2 PFDA	Ave	0.5578	0.5368		9.62	10.0	-3.8	30.0

LCMS ANALYSIS RUN LOG

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1

SDG No.: \_\_\_\_\_

Instrument ID: A8\_N Start Date: 09/20/2017 02:56

Analysis Batch Number: 185329 End Date: 09/20/2017 03:38

LAB SAMPLE ID	CLIENT SAMPLE ID	DATE ANALYZED	DILUTION FACTOR	LAB FILE ID	COLUMN ID
IC 320-185329/4		09/20/2017 02:56	1	2017.09.19_537I CAL 004.d	GeminiC18 3x100 3(mm)
IC 320-185329/5		09/20/2017 03:00	1	2017.09.19_537I CAL 005.d	GeminiC18 3x100 3(mm)
IC 320-185329/6		09/20/2017 03:05	1	2017.09.19_537I CAL 006.d	GeminiC18 3x100 3(mm)
IC 320-185329/7 ICISAV		09/20/2017 03:10	1	2017.09.19_537I CAL 007.d	GeminiC18 3x100 3(mm)
IC 320-185329/8		09/20/2017 03:15	1	2017.09.19_537I CAL 008.d	GeminiC18 3x100 3(mm)
IC 320-185329/9		09/20/2017 03:19	1	2017.09.19_537I CAL 009.d	GeminiC18 3x100 3(mm)
ZZZZZ		09/20/2017 03:24	1		GeminiC18 3x100 3(mm)
CCVL 320-185329/11		09/20/2017 03:29	1	2017.09.19_537I CAL 011.d	GeminiC18 3x100 3(mm)
ZZZZZ		09/20/2017 03:34	1		GeminiC18 3x100 3(mm)
ICV 320-185329/13		09/20/2017 03:38	1	2017.09.19_537I CAL 013.d	GeminiC18 3x100 3(mm)



LCMS ANALYSIS RUN LOG

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1

SDG No.: \_\_\_\_\_

Instrument ID: A8\_N Start Date: 09/20/2017 03:48

Analysis Batch Number: 185406 End Date: 09/20/2017 04:26

LAB SAMPLE ID	CLIENT SAMPLE ID	DATE ANALYZED	DILUTION FACTOR	LAB FILE ID	COLUMN ID
CCV 320-185406/1 CCVIS		09/20/2017 03:48	1	2017.09.19_537A 001.d	GeminiC18 3x100 3(mm)
ZZZZZ		09/20/2017 03:52	1		GeminiC18 3x100 3(mm)
MB 320-184385/1-A		09/20/2017 03:57	1	2017.09.19_537A 003.d	GeminiC18 3x100 3(mm)
LLCS 320-184385/2-A		09/20/2017 04:02	1	2017.09.19_537A 004.d	GeminiC18 3x100 3(mm)
LLCSD 320-184385/3-A		09/20/2017 04:07	1	2017.09.19_537A 005.d	GeminiC18 3x100 3(mm)
320-31468-21		09/20/2017 04:11	1	2017.09.19_537A 006.d	GeminiC18 3x100 3(mm)
320-31468-22		09/20/2017 04:16	1	2017.09.19_537A 007.d	GeminiC18 3x100 3(mm)
320-31468-23		09/20/2017 04:21	1	2017.09.19_537A 008.d	GeminiC18 3x100 3(mm)
CCV 320-185406/9 CCVIS		09/20/2017 04:26	1	2017.09.19_537A 009.d	GeminiC18 3x100 3(mm)

LCMS ANALYSIS RUN LOG

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1

SDG No.: \_\_\_\_\_

Instrument ID: A8\_N Start Date: 09/20/2017 04:26

Analysis Batch Number: 185407 End Date: 09/20/2017 05:23

LAB SAMPLE ID	CLIENT SAMPLE ID	DATE ANALYZED	DILUTION FACTOR	LAB FILE ID	COLUMN ID
CCV 320-185407/9 CCVIS ZZZZZ		09/20/2017 04:26	1	2017.09.19_537A 009.d	GeminiC18 3x100 3(mm)
MB 320-184382/1-A		09/20/2017 04:35	1	2017.09.19_537A 011.d	GeminiC18 3x100 3(mm)
LCS 320-184382/2-A		09/20/2017 04:40	1	2017.09.19_537A 012.d	GeminiC18 3x100 3(mm)
LCSD 320-184382/3-A		09/20/2017 04:45	1	2017.09.19_537A 013.d	GeminiC18 3x100 3(mm)
320-31468-1		09/20/2017 04:49	1	2017.09.19_537A 014.d	GeminiC18 3x100 3(mm)
320-31468-2		09/20/2017 04:54	1	2017.09.19_537A 015.d	GeminiC18 3x100 3(mm)
320-31468-3		09/20/2017 04:59	1	2017.09.19_537A 016.d	GeminiC18 3x100 3(mm)
320-31468-4		09/20/2017 05:04	1	2017.09.19_537A 017.d	GeminiC18 3x100 3(mm)
320-31468-5		09/20/2017 05:08	1	2017.09.19_537A 018.d	GeminiC18 3x100 3(mm)
320-31468-6		09/20/2017 05:13	1	2017.09.19_537A 019.d	GeminiC18 3x100 3(mm)
320-31468-7		09/20/2017 05:18	1	2017.09.19_537A 020.d	GeminiC18 3x100 3(mm)
CCV 320-185407/21 CCVIS		09/20/2017 05:23	1	2017.09.19_537A 021.d	GeminiC18 3x100 3(mm)

LCMS ANALYSIS RUN LOG

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1

SDG No.: \_\_\_\_\_

Instrument ID: A8\_N Start Date: 09/20/2017 05:23

Analysis Batch Number: 185408 End Date: 09/20/2017 06:20

LAB SAMPLE ID	CLIENT SAMPLE ID	DATE ANALYZED	DILUTION FACTOR	LAB FILE ID	COLUMN ID
CCV 320-185408/21 CCVIS		09/20/2017 05:23	1	2017.09.19_537A 021.d	GeminiC18 3x100 3(mm)
ZZZZZ		09/20/2017 05:27	1		GeminiC18 3x100 3(mm)
320-31468-8		09/20/2017 05:32	1	2017.09.19_537A 023.d	GeminiC18 3x100 3(mm)
320-31468-9		09/20/2017 05:37	1	2017.09.19_537A 024.d	GeminiC18 3x100 3(mm)
320-31468-10		09/20/2017 05:42	1	2017.09.19_537A 025.d	GeminiC18 3x100 3(mm)
320-31468-11		09/20/2017 05:46	1	2017.09.19_537A 026.d	GeminiC18 3x100 3(mm)
320-31468-12		09/20/2017 05:51	1	2017.09.19_537A 027.d	GeminiC18 3x100 3(mm)
320-31468-13		09/20/2017 05:56	1	2017.09.19_537A 028.d	GeminiC18 3x100 3(mm)
320-31468-14		09/20/2017 06:01	1	2017.09.19_537A 029.d	GeminiC18 3x100 3(mm)
320-31468-15		09/20/2017 06:05	1	2017.09.19_537A 030.d	GeminiC18 3x100 3(mm)
320-31468-16		09/20/2017 06:10	1	2017.09.19_537A 031.d	GeminiC18 3x100 3(mm)
320-31468-17		09/20/2017 06:15	1	2017.09.19_537A 032.d	GeminiC18 3x100 3(mm)
CCV 320-185408/33 CCVIS		09/20/2017 06:20	1	2017.09.19_537A 033.d	GeminiC18 3x100 3(mm)

LCMS ANALYSIS RUN LOG

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1

SDG No.: \_\_\_\_\_

Instrument ID: A8\_N Start Date: 09/20/2017 06:20

Analysis Batch Number: 185409 End Date: 09/20/2017 06:43

LAB SAMPLE ID	CLIENT SAMPLE ID	DATE ANALYZED	DILUTION FACTOR	LAB FILE ID	COLUMN ID
CCV 320-185409/33 CCVIS		09/20/2017 06:20	1	2017.09.19_537A 033.d	GeminiC18 3x100 3(mm)
ZZZZZ		09/20/2017 06:24	1		GeminiC18 3x100 3(mm)
320-31468-18		09/20/2017 06:29	1	2017.09.19_537A 035.d	GeminiC18 3x100 3(mm)
320-31468-19		09/20/2017 06:34	1	2017.09.19_537A 036.d	GeminiC18 3x100 3(mm)
320-31468-20		09/20/2017 06:39	1	2017.09.19_537A 037.d	GeminiC18 3x100 3(mm)
CCV 320-185409/38 CCVIS		09/20/2017 06:43	1	2017.09.19_537A 038.d	GeminiC18 3x100 3(mm)

LCMS BATCH WORKSHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1

SDG No.: \_\_\_\_\_

Batch Number: 184382 Batch Start Date: 09/14/17 09:16 Batch Analyst: Sharifi, Nooshin

Batch Method: 537 Batch End Date: 09/18/17 16:50

Lab Sample ID	Client Sample ID	Method Chain	Basis	GrossWeight	TareWeight	InitialAmount	FinalAmount	ReceivedpH	LC537-HSP 00023
MB 320-184382/1		537, 537				250 mL	1.0 mL	7 SU	
LCS 320-184382/2		537, 537				250 mL	1.0 mL	7 SU	100 uL
LCSD 320-184382/3		537, 537				250 mL	1.0 mL	7 SU	100 uL
320-31468-A-1	NAWC-091117-RW-106	537, 537	T	279.32 g	26.60 g	252.7 mL	1.0 mL	7 SU	
320-31468-A-2	NAWC-091117-FRB-106	537, 537	T	286.63 g	27.74 g	258.9 mL	1.0 mL	7 SU	
320-31468-A-3	NAWC-091117-RW-060	537, 537	T	289.73 g	28.04 g	261.7 mL	1.0 mL	7 SU	
320-31468-A-4	NAWC-091117-FRB-060	537, 537	T	287.72 g	27.79 g	259.9 mL	1.0 mL	7 SU	
320-31468-A-5	NAWC-091117-RW-314	537, 537	T	290.32 g	27.61 g	262.7 mL	1.0 mL	7 SU	
320-31468-A-6	NAWC-091117-FRB-314	537, 537	T	293.04 g	27.48 g	265.6 mL	1.0 mL	7 SU	
320-31468-A-7	NAWC-091117-RW-258	537, 537	T	294.63 g	27.68 g	267 mL	1.0 mL	7 SU	
320-31468-A-8	NAWC-091117-FRB-258	537, 537	T	289.24 g	27.66 g	261.6 mL	1.0 mL	7 SU	
320-31468-A-9	NAWC-091117-RW-048	537, 537	T	291.43 g	27.53 g	263.9 mL	1.0 mL	7 SU	
320-31468-A-10	NAWC-091117-FRB-048	537, 537	T	294.51 g	27.81 g	266.7 mL	1.0 mL	7 SU	
320-31468-A-11	NAWC-091117-RW-145	537, 537	T	296.76 g	27.74 g	269 mL	1.0 mL	7 SU	
320-31468-A-12	NAWC-091117-FRB-145	537, 537	T	293.17 g	27.53 g	265.6 mL	1.0 mL	7 SU	
320-31468-A-13	NAWC-091117-RW-317	537, 537	T	291.04 g	27.35 g	263.7 mL	1.0 mL	7 SU	
320-31468-A-14	NAWC-091117-FRB-317	537, 537	T	281.96 g	27.52 g	254.4 mL	1.0 mL	7 SU	
320-31468-A-15	NAWC-091117-RW-319	537, 537	T	278.29 g	27.27 g	251 mL	1.0 mL	7 SU	
320-31468-A-16	NAWC-091117-FRB-319	537, 537	T	294.18 g	27.53 g	266.7 mL	1.0 mL	7 SU	
320-31468-A-17	NAWC-091117-RW-321	537, 537	T	289.71 g	27.73 g	262 mL	1.0 mL	7 SU	
320-31468-A-18	NAWC-091117-FRB-321	537, 537	T	291.10 g	27.64 g	263.5 mL	1.0 mL	7 SU	
320-31468-A-19	NAWC-091117-RW-010	537, 537	T	283.27 g	28.59 g	254.7 mL	1.0 mL	7 SU	

The pound sign (#) in the amount added field denotes that the reagent was used undiluted. All calculations are performed using the stated concentration for this reagent.

LCMS BATCH WORKSHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1

SDG No.: \_\_\_\_\_

Batch Number: 184382 Batch Start Date: 09/14/17 09:16 Batch Analyst: Sharifi, Nooshin

Batch Method: 537 Batch End Date: 09/18/17 16:50

Lab Sample ID	Client Sample ID	Method Chain	Basis	GrossWeight	TareWeight	InitialAmount	FinalAmount	ReceivedpH	LC537-HSP 00023
320-31468-A-20	NAWC-091117-FRB-010	537, 537	T	287.79 g	27.95 g	259.8 mL	1.0 mL	7 SU	

Lab Sample ID	Client Sample ID	Method Chain	Basis	LC537-IS 00047	LC537-SU 00048	AnalysisComment			
MB 320-184382/1		537, 537		100 uL	100 uL	CH ND			
LCS 320-184382/2		537, 537		100 uL	100 uL	CH ND			
LCSD 320-184382/3		537, 537		100 uL	100 uL	CH ND			
320-31468-A-1	NAWC-091117-RW-106	537, 537	T	100 uL	100 uL	CH ND			
320-31468-A-2	NAWC-091117-FRB-106	537, 537	T	100 uL	100 uL	CH ND			
320-31468-A-3	NAWC-091117-RW-060	537, 537	T	100 uL	100 uL	CH ND			
320-31468-A-4	NAWC-091117-FRB-060	537, 537	T	100 uL	100 uL	CH ND			
320-31468-A-5	NAWC-091117-RW-314	537, 537	T	100 uL	100 uL	CH ND			
320-31468-A-6	NAWC-091117-FRB-314	537, 537	T	100 uL	100 uL	CH ND			
320-31468-A-7	NAWC-091117-RW-258	537, 537	T	100 uL	100 uL	CH ND			
320-31468-A-8	NAWC-091117-FRB-258	537, 537	T	100 uL	100 uL	CH ND			
320-31468-A-9	NAWC-091117-RW-048	537, 537	T	100 uL	100 uL	CH ND			
320-31468-A-10	NAWC-091117-FRB-048	537, 537	T	100 uL	100 uL	CH ND			
320-31468-A-11	NAWC-091117-RW-145	537, 537	T	100 uL	100 uL	CH ND			
320-31468-A-12	NAWC-091117-FRB-145	537, 537	T	100 uL	100 uL	CH ND			
320-31468-A-13	NAWC-091117-RW-317	537, 537	T	100 uL	100 uL	CH ND			
320-31468-A-14	NAWC-091117-FRB-317	537, 537	T	100 uL	100 uL	CH ND			
320-31468-A-15	NAWC-091117-RW-319	537, 537	T	100 uL	100 uL	CH ND			
320-31468-A-16	NAWC-091117-FRB-319	537, 537	T	100 uL	100 uL	CH ND			

The pound sign (#) in the amount added field denotes that the reagent was used undiluted. All calculations are performed using the stated concentration for this reagent.

LCMS BATCH WORKSHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1

SDG No.: \_\_\_\_\_

Batch Number: 184382 Batch Start Date: 09/14/17 09:16 Batch Analyst: Sharifi, Nooshin

Batch Method: 537 Batch End Date: 09/18/17 16:50

Lab Sample ID	Client Sample ID	Method Chain	Basis	LC537-IS 00047	LC537-SU 00048	AnalysisComment			
320-31468-A-17	NAWC-091117-RW-321	537, 537	T	100 uL	100 uL	CH ND			
320-31468-A-18	NAWC-091117-FRB-321	537, 537	T	100 uL	100 uL	CH ND			
320-31468-A-19	NAWC-091117-RW-010	537, 537	T	100 uL	100 uL	CH ND			
320-31468-A-20	NAWC-091117-FRB-010	537, 537	T	100 uL	100 uL	CH ND			

Batch Notes	
Batch Comment	IS: 1002957 BD: CCB FV: VPM AL:VPM
Manifold ID	1,3
Methanol ID	1021237
Pipette ID	H14930F
Analyst ID - IS Reagent Drop	VPM
Analyst ID - IS Reagent Drop Witness	TWL
Analyst ID - SU Reagent Drop	NSH
Analyst ID - SU Reagent Drop Witness	AAR
Analyst ID - TA Reagent Drop	NSH
Analyst ID - TA Reagent Drop Witness	AAR
SPE Cartridge ID	6357081-05
Trizma ID	SLBR4303V
Reagent Water ID	9/13/17

Basis	Basis Description
T	Total/NA

The pound sign (#) in the amount added field denotes that the reagent was used undiluted. All calculations are performed using the stated concentration for this reagent.

LCMS BATCH WORKSHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1

SDG No.: \_\_\_\_\_

Batch Number: 184385 Batch Start Date: 09/14/17 09:29 Batch Analyst: Branscum, Cassie

Batch Method: 537 Batch End Date: 09/15/17 14:40

Lab Sample ID	Client Sample ID	Method Chain	Basis	GrossWeight	TareWeight	InitialAmount	FinalAmount	ReceivedpH	LC537-IS 00047
MB 320-184385/1		537, 537				250 mL	1.00 mL	7 SU	100 uL
LLCS 320-184385/2		537, 537				250 mL	1.00 mL	7 SU	100 uL
LLCSD 320-184385/3		537, 537				250 mL	1.00 mL	7 SU	100 uL
320-31468-A-21	NAWC-091117-RW-1 62	537, 537	T	291.25 g	28.32 g	262.9 mL	1.00 mL	7 SU	100 uL
320-31468-A-22	NAWC-091117-FRB- 162	537, 537	T	275.14 g	27.84 g	247.3 mL	1.00 mL	7 SU	100 uL
320-31468-A-23	WGNA-091117-DUP0 9	537, 537	T	287.92 g	27.88 g	260 mL	1.00 mL	7 SU	100 uL

Lab Sample ID	Client Sample ID	Method Chain	Basis	LC537-LSP 00025	LC537-SU 00048	AnalysisComment			
MB 320-184385/1		537, 537			100 uL	ch nd			
LLCS 320-184385/2		537, 537		100 uL	100 uL	ch nd			
LLCSD 320-184385/3		537, 537		100 uL	100 uL	ch nd			
320-31468-A-21	NAWC-091117-RW-1 62	537, 537	T		100 uL	ch nd			
320-31468-A-22	NAWC-091117-FRB- 162	537, 537	T		100 uL	ch nd			
320-31468-A-23	WGNA-091117-DUP0 9	537, 537	T		100 uL	ch nd			

The pound sign (#) in the amount added field denotes that the reagent was used undiluted. All calculations are performed using the stated concentration for this reagent.



LCMS BATCH WORKSHEET

Lab Name: TestAmerica Sacramento Job No.: 320-31468-1

SDG No.: \_\_\_\_\_

Batch Number: 184385 Batch Start Date: 09/14/17 09:29 Batch Analyst: Branscum, Cassie

Batch Method: 537 Batch End Date: 09/15/17 14:40

Batch Notes	
Batch Comment	IS:1002957 BD:CCB FV: CCB AL:VPM
Manifold ID	9
Methanol ID	1021243
Pipette ID	H14930F
Analyst ID - IS Reagent Drop	VPM
Analyst ID - IS Reagent Drop Witness	NSH
Analyst ID - SU Reagent Drop	CCB
Analyst ID - SU Reagent Drop Witness	HJA
Analyst ID - TA Reagent Drop	CCB
Analyst ID - TA Reagent Drop Witness	HJA
SPE Cartridge ID	6357081-06
Trizma ID	SLBR4303V
Reagent Water ID	9/13/17

Basis	Basis Description
T	Total/NA

The pound sign (#) in the amount added field denotes that the reagent was used undiluted. All calculations are performed using the stated concentration for this reagent.

PFAS Calibration Calculations:

Initial Calibration 9/20/2017  
 Instrument A8\_N

Perfluorohexanesulfonic acid

Analyte Concentration	Analyte Response	Internal Standard Response	Internal Standard Amount	RRF	Reported RRF
3	971572	5717338	28.7	1.62571	1.624
6.67	2411042	5904759	28.7	1.75695	1.7562
15	4809005	5478893	28.7	1.67940	1.6778
30	9481986	5418565	28.7	1.67408	1.6725
45	13653533	5450221	28.7	1.59772	1.5962
60	17148552	5454650	28.7	1.50380	1.5024
Average				1.63961	1.6382
Standard Deviation				0.0859	
RSD				0.0524	
%RSD				5.24164	5.3

Continuing Calibration 09/20/2017 @ 3:48  
 A8\_N

Perfluorohexanesulfonic acid

Analyte Concentration	Analyte Response	Internal Standard Response	Internal Standard Amount	RRF	%D	Reported RRF	Reported %D
45	13015051	5210623	28.7	1.5930	-2.756925	1.592	-2.8

Willow Grove  
SDG 320-31468-1

Sample Identification NAWC-091117-RW-106

Compound Perfluorohexanesulfonic acid

Compound Area 751914

Internal Standard Amount (ng) 28.7

Dilution Factor 1

Internal Standard Area 5860369

Average RRF 1.6382

Sample Volume(ml) 252.7

Volume Extract (ml) 1


Injection Volume (µl) 1

µl to ml 1000.00

Concentration 8.90 ng/L



C:\AI\Projects\112008005\WE04\F.S.DR.03\NAWC\_201901.mxd MKB 1/24/2019

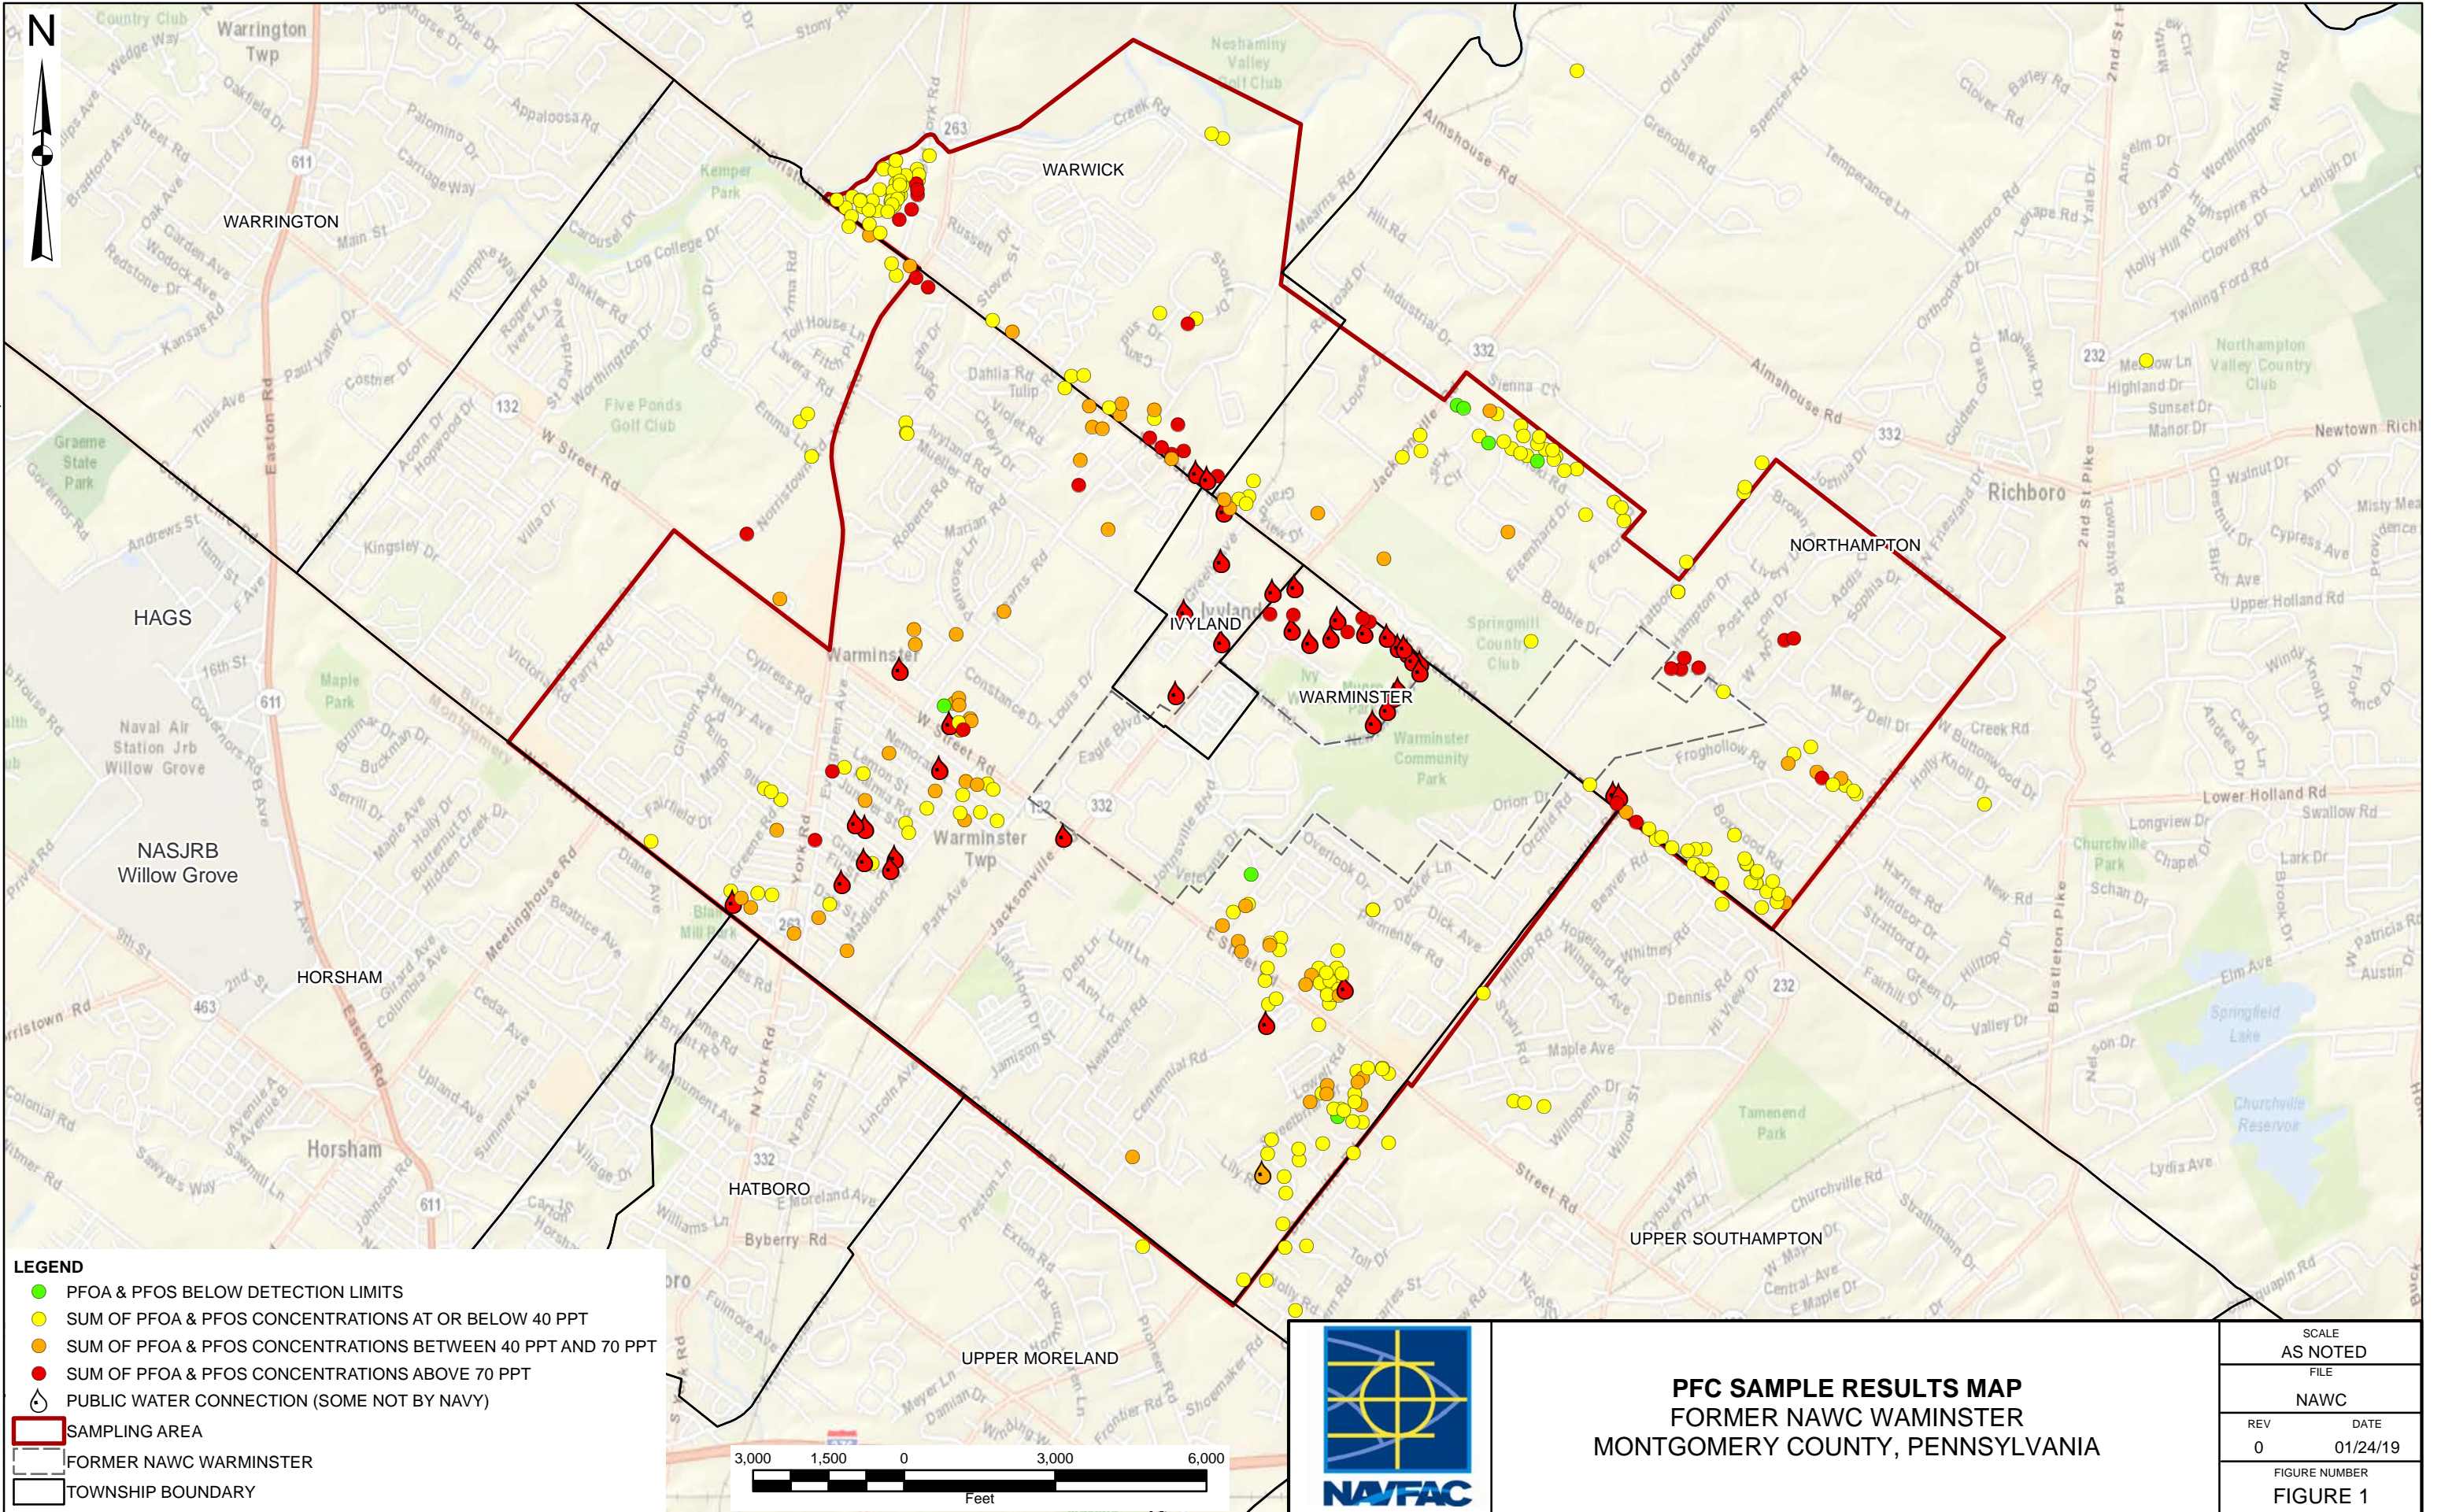

**LEGEND**

- PFOA & PFOS BELOW DETECTION LIMITS
- SUM OF PFOA & PFOS CONCENTRATIONS AT OR BELOW 40 PPT
- SUM OF PFOA & PFOS CONCENTRATIONS BETWEEN 40 PPT AND 70 PPT
- SUM OF PFOA & PFOS CONCENTRATIONS ABOVE 70 PPT
- 👉 PUBLIC WATER CONNECTION (SOME NOT BY NAVY)
- SAMPLING AREA
- FORMER NAWC WARRINSTER
- TOWNSHIP BOUNDARY



**PFC SAMPLE RESULTS MAP**  
**FORMER NAWC WARRINSTER**  
**MONTGOMERY COUNTY, PENNSYLVANIA**

SCALE AS NOTED	
FILE	
NAWC	
REV 0	DATE 01/24/19
FIGURE NUMBER	
FIGURE 1	