



**Off-Base Drinking Water Sample Results,
Combined Level 2 and Level 4 Laboratory Report,
Electronic Data Deliverable, Data Validation Report,
and the Sample Location Figure, SDG 320-34917-1**

*Naval Air Warfare Center Warminster
Warminster, Pennsylvania*

August 2019

N62269_001162
WARMINSTER_NAWC
SSIC 5000-33c

**LABORATORY DATA PACKAGE, 320-34917-1, NAS WILLOW GROVE NAWC
WARMINSTER PA**
01/24/2018
TESTAMERICA LABORATORIES INC

Approved for public release: distribution unlimited.

ANALYTICAL REPORT

Job Number: 320-34917-1

Job Description: Warminster: PFAS, NAS JRB Willow Grove

For:
Tetra Tech, Inc.
234 Mall Boulevard
Suite 260
King of Prussia, PA 19406
Attention: Andy Frebowitz



Approved for release.
David R. Alltucker
Project Manager I
1/24/2018 2:07 PM

David R Alltucker, Project Manager I
880 Riverside Parkway, West Sacramento, CA, 95605
(916)374-4383
david.alltucker@testamericainc.com
01/24/2018

Table of Contents

Cover Title Page	1
Data Summaries	4
Definitions	4
Case Narrative	5
Detection Summary	6
Client Sample Results	8
Default Detection Limits	13
Surrogate Summary	14
QC Sample Results	15
QC Association	17
Chronicle	18
Certification Summary	21
Method Summary	22
Sample Summary	23
Manual Integration Summary	24
Reagent Traceability	28
COAs	38
Organic Sample Data	92
LCMS	92
Method 537 DOD	92
Method 537 DOD QC Summary	93
Method 537 DOD Sample Data	103
Standards Data	189
Method 537 DOD ICAL Data	189
Method 537 DOD CCAL Data	228
Raw QC Data	271

Table of Contents

Method 537 DOD Blank Data	271
Method 537 DOD LCS/LCSD Data	276
Method 537 DOD MS/MSD Data	281
Method 537 DOD Run Logs	295
Method 537 DOD Prep Data	298
Shipping and Receiving Documents	327
Client Chain of Custody	328
Sample Receipt Checklist	329

Definitions/Glossary

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-34917-1

Qualifiers

LCMS

Qualifier	Qualifier Description
U	Undetected at the Limit of Detection.
J	Estimated: The analyte was positively identified; the quantitation is an estimation
M	Manual integrated compound.

Glossary

Abbreviation	These commonly used abbreviations may or may not be present in this report.
α	Listed under the "D" column to designate that the result is reported on a dry weight basis
%R	Percent Recovery
CFL	Contains Free Liquid
CNF	Contains No Free Liquid
DER	Duplicate Error Ratio (normalized absolute difference)
Dil Fac	Dilution Factor
DL	Detection Limit (DoD/DOE)
DL, RA, RE, IN	Indicates a Dilution, Re-analysis, Re-extraction, or additional Initial metals/anion analysis of the sample
DLC	Decision Level Concentration (Radiochemistry)
EDL	Estimated Detection Limit (Dioxin)
LOD	Limit of Detection (DoD/DOE)
LOQ	Limit of Quantitation (DoD/DOE)
MDA	Minimum Detectable Activity (Radiochemistry)
MDC	Minimum Detectable Concentration (Radiochemistry)
MDL	Method Detection Limit
ML	Minimum Level (Dioxin)
NC	Not Calculated
ND	Not Detected at the reporting limit (or MDL or EDL if shown)
PQL	Practical Quantitation Limit
QC	Quality Control
RER	Relative Error Ratio (Radiochemistry)
RL	Reporting Limit or Requested Limit (Radiochemistry)
RPD	Relative Percent Difference, a measure of the relative difference between two points
TEF	Toxicity Equivalent Factor (Dioxin)
TEQ	Toxicity Equivalent Quotient (Dioxin)

Detection Summary

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-34917-1

Client Sample ID: WGNA-010818-RW-0344

Lab Sample ID: 320-34917-1

Analyte	Result	Qualifier	LOQ	DL	Unit	Dil Fac	D	Method	Prep Type
Perfluorooctanesulfonic acid (PFOS)	32	J	40	6.8	ng/L	1		537	Total/NA
Perfluorooctanoic acid (PFOA)	24		20	2.8	ng/L	1		537	Total/NA
Perfluorononanoic acid (PFNA)	32		24	8.0	ng/L	1		537	Total/NA
Perfluorohexanesulfonic acid (PFHxS)	18	J	30	5.5	ng/L	1		537	Total/NA
Perfluoroheptanoic acid (PFHpA)	6.4	J	10	1.9	ng/L	1		537	Total/NA

Client Sample ID: WGNA-010818-FRB-0344

Lab Sample ID: 320-34917-2

No Detections.

Client Sample ID: WGNA-010818-RW-3957

Lab Sample ID: 320-34917-3

Analyte	Result	Qualifier	LOQ	DL	Unit	Dil Fac	D	Method	Prep Type
Perfluorooctanesulfonic acid (PFOS)	18	J	39	6.6	ng/L	1		537	Total/NA
Perfluorooctanoic acid (PFOA)	15	J	19	2.7	ng/L	1		537	Total/NA
Perfluorohexanesulfonic acid (PFHxS)	6.5	J	29	5.3	ng/L	1		537	Total/NA
Perfluoroheptanoic acid (PFHpA)	3.8	J	9.7	1.8	ng/L	1		537	Total/NA

Client Sample ID: WGNA-010818-FRB-3957

Lab Sample ID: 320-34917-4

No Detections.

Client Sample ID: WGNA-010818-DUP-16

Lab Sample ID: 320-34917-5

Analyte	Result	Qualifier	LOQ	DL	Unit	Dil Fac	D	Method	Prep Type
Perfluorooctanesulfonic acid (PFOS)	25	J	38	6.5	ng/L	1		537	Total/NA
Perfluorooctanoic acid (PFOA)	21		19	2.7	ng/L	1		537	Total/NA
Perfluorohexanesulfonic acid (PFHxS)	8.0	J	29	5.2	ng/L	1		537	Total/NA
Perfluoroheptanoic acid (PFHpA)	6.2	J	9.5	1.8	ng/L	1		537	Total/NA

Client Sample ID: WGNA-010818-RW-3178

Lab Sample ID: 320-34917-6

Analyte	Result	Qualifier	LOQ	DL	Unit	Dil Fac	D	Method	Prep Type
Perfluorooctanesulfonic acid (PFOS)	16	J	42	7.1	ng/L	1		537	Total/NA
Perfluorooctanoic acid (PFOA)	9.8	J	21	2.9	ng/L	1		537	Total/NA
Perfluorohexanesulfonic acid (PFHxS)	7.0	J	31	5.7	ng/L	1		537	Total/NA
Perfluoroheptanoic acid (PFHpA)	2.8	J	10	2.0	ng/L	1		537	Total/NA

Client Sample ID: WGNA-010818-FRB-3178

Lab Sample ID: 320-34917-7

No Detections.

Client Sample ID: NAWC-010818-RW-141

Lab Sample ID: 320-34917-8

Analyte	Result	Qualifier	LOQ	DL	Unit	Dil Fac	D	Method	Prep Type
Perfluorooctanesulfonic acid (PFOS)	24	J	39	6.6	ng/L	1		537	Total/NA
Perfluorooctanoic acid (PFOA)	15	J	19	2.7	ng/L	1		537	Total/NA
Perfluorohexanesulfonic acid (PFHxS)	16	J	29	5.3	ng/L	1		537	Total/NA
Perfluoroheptanoic acid (PFHpA)	7.6	J	9.7	1.8	ng/L	1		537	Total/NA

This Detection Summary does not include radiochemical test results.

TestAmerica Sacramento

Detection Summary

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-34917-1

Client Sample ID: NAWC-010818-FRB-141

Lab Sample ID: 320-34917-9

No Detections.

Client Sample ID: WGNA-010818-RW-4024

Lab Sample ID: 320-34917-10

Analyte	Result	Qualifier	LOQ	DL	Unit	Dil Fac	D	Method	Prep Type
Perfluorooctanesulfonic acid (PFOS)	18	J M	40	6.8	ng/L	1		537	Total/NA
Perfluorooctanoic acid (PFOA)	12	J	20	2.8	ng/L	1		537	Total/NA
Perfluoroheptanoic acid (PFHpA)	3.6	J	10	1.9	ng/L	1		537	Total/NA

Client Sample ID: WGNA-010818-FRB-4024

Lab Sample ID: 320-34917-11

No Detections.

Client Sample ID: WGNA-010818-RW-4844

Lab Sample ID: 320-34917-12

Analyte	Result	Qualifier	LOQ	DL	Unit	Dil Fac	D	Method	Prep Type
Perfluorooctanesulfonic acid (PFOS)	7.9	J M	39	6.7	ng/L	1		537	Total/NA
Perfluorooctanoic acid (PFOA)	14	J	20	2.8	ng/L	1		537	Total/NA
Perfluoroheptanoic acid (PFHpA)	7.1	J	9.9	1.9	ng/L	1		537	Total/NA

Client Sample ID: WGNA-010818-FRB-4844

Lab Sample ID: 320-34917-13

No Detections.

Client Sample ID: WGNA-010818-RW-0404

Lab Sample ID: 320-34917-14

Analyte	Result	Qualifier	LOQ	DL	Unit	Dil Fac	D	Method	Prep Type
Perfluorooctanesulfonic acid (PFOS)	26	J M	40	6.8	ng/L	1		537	Total/NA
Perfluorooctanoic acid (PFOA)	21		20	2.8	ng/L	1		537	Total/NA
Perfluorohexanesulfonic acid (PFHxS)	8.3	J	30	5.5	ng/L	1		537	Total/NA
Perfluoroheptanoic acid (PFHpA)	6.3	J	10	1.9	ng/L	1		537	Total/NA

Client Sample ID: WGNA-010818-FRB-0404

Lab Sample ID: 320-34917-15

No Detections.

This Detection Summary does not include radiochemical test results.

TestAmerica Sacramento

Client Sample Results

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-34917-1

Client Sample ID: WGNA-010818-RW-0344

Lab Sample ID: 320-34917-1

Date Collected: 01/08/18 08:10

Matrix: Water

Date Received: 01/09/18 10:30

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	32	J	40	6.8	ng/L		01/17/18 10:50	01/20/18 19:11	1
Perfluorooctanoic acid (PFOA)	24		20	2.8	ng/L		01/17/18 10:50	01/20/18 19:11	1
Perfluorononanoic acid (PFNA)	32		24	8.0	ng/L		01/17/18 10:50	01/20/18 19:11	1
Perfluorohexanesulfonic acid (PFHxS)	18	J	30	5.5	ng/L		01/17/18 10:50	01/20/18 19:11	1
Perfluoroheptanoic acid (PFHpA)	6.4	J	10	1.9	ng/L		01/17/18 10:50	01/20/18 19:11	1
Perfluorobutanesulfonic acid (PFBS)	36	U	90	16	ng/L		01/17/18 10:50	01/20/18 19:11	1
Surrogate	%Recovery	Qualifier	Limits				Prepared	Analyzed	Dil Fac
13C2 PFHxA	91		70 - 130				01/17/18 10:50	01/20/18 19:11	1
13C2 PFDA	93		70 - 130				01/17/18 10:50	01/20/18 19:11	1

Client Sample ID: WGNA-010818-FRB-0344

Lab Sample ID: 320-34917-2

Date Collected: 01/08/18 08:05

Matrix: Water

Date Received: 01/09/18 10:30

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	16	U	39	6.7	ng/L		01/17/18 10:50	01/20/18 19:15	1
Perfluorooctanoic acid (PFOA)	7.9	U	20	2.8	ng/L		01/17/18 10:50	01/20/18 19:15	1
Perfluorononanoic acid (PFNA)	20	U	24	7.9	ng/L		01/17/18 10:50	01/20/18 19:15	1
Perfluorohexanesulfonic acid (PFHxS)	12	U	30	5.4	ng/L		01/17/18 10:50	01/20/18 19:15	1
Perfluoroheptanoic acid (PFHpA)	3.9	U	9.9	1.9	ng/L		01/17/18 10:50	01/20/18 19:15	1
Perfluorobutanesulfonic acid (PFBS)	36	U	89	16	ng/L		01/17/18 10:50	01/20/18 19:15	1
Surrogate	%Recovery	Qualifier	Limits				Prepared	Analyzed	Dil Fac
13C2 PFHxA	97		70 - 130				01/17/18 10:50	01/20/18 19:15	1
13C2 PFDA	98		70 - 130				01/17/18 10:50	01/20/18 19:15	1

Client Sample ID: WGNA-010818-RW-3957

Lab Sample ID: 320-34917-3

Date Collected: 01/08/18 08:40

Matrix: Water

Date Received: 01/09/18 10:30

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	18	J	39	6.6	ng/L		01/17/18 10:50	01/20/18 19:20	1
Perfluorooctanoic acid (PFOA)	15	J	19	2.7	ng/L		01/17/18 10:50	01/20/18 19:20	1
Perfluorononanoic acid (PFNA)	19	U M	23	7.8	ng/L		01/17/18 10:50	01/20/18 19:20	1
Perfluorohexanesulfonic acid (PFHxS)	6.5	J	29	5.3	ng/L		01/17/18 10:50	01/20/18 19:20	1
Perfluoroheptanoic acid (PFHpA)	3.8	J	9.7	1.8	ng/L		01/17/18 10:50	01/20/18 19:20	1
Perfluorobutanesulfonic acid (PFBS)	35	U	87	16	ng/L		01/17/18 10:50	01/20/18 19:20	1
Surrogate	%Recovery	Qualifier	Limits				Prepared	Analyzed	Dil Fac
13C2 PFHxA	91		70 - 130				01/17/18 10:50	01/20/18 19:20	1
13C2 PFDA	104		70 - 130				01/17/18 10:50	01/20/18 19:20	1

Client Sample Results

Client: Tetra Tech, Inc.
 Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-34917-1

Client Sample ID: WGNA-010818-FRB-3957

Lab Sample ID: 320-34917-4

Date Collected: 01/08/18 08:35

Matrix: Water

Date Received: 01/09/18 10:30

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	16	U	39	6.6	ng/L		01/17/18 10:50	01/20/18 19:25	1
Perfluorooctanoic acid (PFOA)	7.8	U	20	2.7	ng/L		01/17/18 10:50	01/20/18 19:25	1
Perfluorononanoic acid (PFNA)	20	U	23	7.8	ng/L		01/17/18 10:50	01/20/18 19:25	1
Perfluorohexanesulfonic acid (PFHxS)	12	U	29	5.4	ng/L		01/17/18 10:50	01/20/18 19:25	1
Perfluoroheptanoic acid (PFHpA)	3.9	U	9.8	1.9	ng/L		01/17/18 10:50	01/20/18 19:25	1
Perfluorobutanesulfonic acid (PFBS)	35	U	88	16	ng/L		01/17/18 10:50	01/20/18 19:25	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	96		70 - 130	01/17/18 10:50	01/20/18 19:25	1
13C2 PFDA	98		70 - 130	01/17/18 10:50	01/20/18 19:25	1

Client Sample ID: WGNA-010818-DUP-16

Lab Sample ID: 320-34917-5

Date Collected: 01/08/18 07:00

Matrix: Water

Date Received: 01/09/18 10:30

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	25	J	38	6.5	ng/L		01/17/18 10:50	01/20/18 19:29	1
Perfluorooctanoic acid (PFOA)	21		19	2.7	ng/L		01/17/18 10:50	01/20/18 19:29	1
Perfluorononanoic acid (PFNA)	19	U	23	7.6	ng/L		01/17/18 10:50	01/20/18 19:29	1
Perfluorohexanesulfonic acid (PFHxS)	8.0	J	29	5.2	ng/L		01/17/18 10:50	01/20/18 19:29	1
Perfluoroheptanoic acid (PFHpA)	6.2	J	9.5	1.8	ng/L		01/17/18 10:50	01/20/18 19:29	1
Perfluorobutanesulfonic acid (PFBS)	34	U	86	15	ng/L		01/17/18 10:50	01/20/18 19:29	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	96		70 - 130	01/17/18 10:50	01/20/18 19:29	1
13C2 PFDA	109		70 - 130	01/17/18 10:50	01/20/18 19:29	1

Client Sample ID: WGNA-010818-RW-3178

Lab Sample ID: 320-34917-6

Date Collected: 01/08/18 10:10

Matrix: Water

Date Received: 01/09/18 10:30

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	16	J	42	7.1	ng/L		01/17/18 10:50	01/20/18 19:34	1
Perfluorooctanoic acid (PFOA)	9.8	J	21	2.9	ng/L		01/17/18 10:50	01/20/18 19:34	1
Perfluorononanoic acid (PFNA)	21	U	25	8.4	ng/L		01/17/18 10:50	01/20/18 19:34	1
Perfluorohexanesulfonic acid (PFHxS)	7.0	J	31	5.7	ng/L		01/17/18 10:50	01/20/18 19:34	1
Perfluoroheptanoic acid (PFHpA)	2.8	J	10	2.0	ng/L		01/17/18 10:50	01/20/18 19:34	1
Perfluorobutanesulfonic acid (PFBS)	38	U	94	17	ng/L		01/17/18 10:50	01/20/18 19:34	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	90		70 - 130	01/17/18 10:50	01/20/18 19:34	1
13C2 PFDA	102		70 - 130	01/17/18 10:50	01/20/18 19:34	1

Client Sample Results

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-34917-1

Client Sample ID: WGNA-010818-FRB-3178

Lab Sample ID: 320-34917-7

Date Collected: 01/08/18 10:05

Matrix: Water

Date Received: 01/09/18 10:30

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	16	U	39	6.6	ng/L		01/17/18 10:50	01/20/18 19:39	1
Perfluorooctanoic acid (PFOA)	7.8	U	19	2.7	ng/L		01/17/18 10:50	01/20/18 19:39	1
Perfluorononanoic acid (PFNA)	19	U	23	7.8	ng/L		01/17/18 10:50	01/20/18 19:39	1
Perfluorohexanesulfonic acid (PFHxS)	12	U	29	5.4	ng/L		01/17/18 10:50	01/20/18 19:39	1
Perfluoroheptanoic acid (PFHpA)	3.9	U	9.7	1.9	ng/L		01/17/18 10:50	01/20/18 19:39	1
Perfluorobutanesulfonic acid (PFBS)	35	U	88	16	ng/L		01/17/18 10:50	01/20/18 19:39	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	98		70 - 130	01/17/18 10:50	01/20/18 19:39	1
13C2 PFDA	103		70 - 130	01/17/18 10:50	01/20/18 19:39	1

Client Sample ID: NAWC-010818-RW-141

Lab Sample ID: 320-34917-8

Date Collected: 01/08/18 11:10

Matrix: Water

Date Received: 01/09/18 10:30

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	24	J	39	6.6	ng/L		01/17/18 10:50	01/20/18 19:43	1
Perfluorooctanoic acid (PFOA)	15	J	19	2.7	ng/L		01/17/18 10:50	01/20/18 19:43	1
Perfluorononanoic acid (PFNA)	19	U	23	7.8	ng/L		01/17/18 10:50	01/20/18 19:43	1
Perfluorohexanesulfonic acid (PFHxS)	16	J	29	5.3	ng/L		01/17/18 10:50	01/20/18 19:43	1
Perfluoroheptanoic acid (PFHpA)	7.6	J	9.7	1.8	ng/L		01/17/18 10:50	01/20/18 19:43	1
Perfluorobutanesulfonic acid (PFBS)	35	U	87	16	ng/L		01/17/18 10:50	01/20/18 19:43	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	88		70 - 130	01/17/18 10:50	01/20/18 19:43	1
13C2 PFDA	96		70 - 130	01/17/18 10:50	01/20/18 19:43	1

Client Sample ID: NAWC-010818-FRB-141

Lab Sample ID: 320-34917-9

Date Collected: 01/08/18 11:05

Matrix: Water

Date Received: 01/09/18 10:30

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	15	U	38	6.4	ng/L		01/17/18 10:50	01/24/18 05:15	1
Perfluorooctanoic acid (PFOA)	7.5	U	19	2.6	ng/L		01/17/18 10:50	01/24/18 05:15	1
Perfluorononanoic acid (PFNA)	19	U	23	7.5	ng/L		01/17/18 10:50	01/24/18 05:15	1
Perfluorohexanesulfonic acid (PFHxS)	11	U	28	5.2	ng/L		01/17/18 10:50	01/24/18 05:15	1
Perfluoroheptanoic acid (PFHpA)	3.8	U	9.4	1.8	ng/L		01/17/18 10:50	01/24/18 05:15	1
Perfluorobutanesulfonic acid (PFBS)	34	U	85	15	ng/L		01/17/18 10:50	01/24/18 05:15	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	95		70 - 130	01/17/18 10:50	01/24/18 05:15	1
13C2 PFDA	99		70 - 130	01/17/18 10:50	01/24/18 05:15	1

Client Sample Results

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-34917-1

Client Sample ID: WGNA-010818-RW-4024

Lab Sample ID: 320-34917-10

Date Collected: 01/08/18 11:40

Matrix: Water

Date Received: 01/09/18 10:30

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	18	J M	40	6.8	ng/L		01/17/18 10:50	01/24/18 05:19	1
Perfluorooctanoic acid (PFOA)	12	J	20	2.8	ng/L		01/17/18 10:50	01/24/18 05:19	1
Perfluorononanoic acid (PFNA)	20	U	24	8.0	ng/L		01/17/18 10:50	01/24/18 05:19	1
Perfluorohexanesulfonic acid (PFHxS)	12	U	30	5.5	ng/L		01/17/18 10:50	01/24/18 05:19	1
Perfluoroheptanoic acid (PFHpA)	3.6	J	10	1.9	ng/L		01/17/18 10:50	01/24/18 05:19	1
Perfluorobutanesulfonic acid (PFBS)	36	U	90	16	ng/L		01/17/18 10:50	01/24/18 05:19	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	71		70 - 130	01/17/18 10:50	01/24/18 05:19	1
13C2 PFDA	93		70 - 130	01/17/18 10:50	01/24/18 05:19	1

Client Sample ID: WGNA-010818-FRB-4024

Lab Sample ID: 320-34917-11

Date Collected: 01/08/18 11:35

Matrix: Water

Date Received: 01/09/18 10:30

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	16	U	39	6.6	ng/L		01/17/18 10:50	01/24/18 05:33	1
Perfluorooctanoic acid (PFOA)	7.8	U	19	2.7	ng/L		01/17/18 10:50	01/24/18 05:33	1
Perfluorononanoic acid (PFNA)	19	U	23	7.8	ng/L		01/17/18 10:50	01/24/18 05:33	1
Perfluorohexanesulfonic acid (PFHxS)	12	U	29	5.3	ng/L		01/17/18 10:50	01/24/18 05:33	1
Perfluoroheptanoic acid (PFHpA)	3.9	U	9.7	1.8	ng/L		01/17/18 10:50	01/24/18 05:33	1
Perfluorobutanesulfonic acid (PFBS)	35	U	87	16	ng/L		01/17/18 10:50	01/24/18 05:33	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	98		70 - 130	01/17/18 10:50	01/24/18 05:33	1
13C2 PFDA	100		70 - 130	01/17/18 10:50	01/24/18 05:33	1

Client Sample ID: WGNA-010818-RW-4844

Lab Sample ID: 320-34917-12

Date Collected: 01/08/18 13:10

Matrix: Water

Date Received: 01/09/18 10:30

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	7.9	J M	39	6.7	ng/L		01/17/18 10:50	01/24/18 05:38	1
Perfluorooctanoic acid (PFOA)	14	J	20	2.8	ng/L		01/17/18 10:50	01/24/18 05:38	1
Perfluorononanoic acid (PFNA)	20	U	24	7.9	ng/L		01/17/18 10:50	01/24/18 05:38	1
Perfluorohexanesulfonic acid (PFHxS)	12	U	30	5.4	ng/L		01/17/18 10:50	01/24/18 05:38	1
Perfluoroheptanoic acid (PFHpA)	7.1	J	9.9	1.9	ng/L		01/17/18 10:50	01/24/18 05:38	1
Perfluorobutanesulfonic acid (PFBS)	36	U	89	16	ng/L		01/17/18 10:50	01/24/18 05:38	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	97		70 - 130	01/17/18 10:50	01/24/18 05:38	1
13C2 PFDA	98		70 - 130	01/17/18 10:50	01/24/18 05:38	1

Client Sample Results

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-34917-1

Client Sample ID: WGNA-010818-FRB-4844

Lab Sample ID: 320-34917-13

Date Collected: 01/08/18 13:05

Matrix: Water

Date Received: 01/09/18 10:30

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	16	U	40	6.8	ng/L		01/17/18 10:50	01/24/18 05:43	1
Perfluorooctanoic acid (PFOA)	8.0	U	20	2.8	ng/L		01/17/18 10:50	01/24/18 05:43	1
Perfluorononanoic acid (PFNA)	20	U	24	8.0	ng/L		01/17/18 10:50	01/24/18 05:43	1
Perfluorohexanesulfonic acid (PFHxS)	12	U	30	5.5	ng/L		01/17/18 10:50	01/24/18 05:43	1
Perfluoroheptanoic acid (PFHpA)	4.0	U	10	1.9	ng/L		01/17/18 10:50	01/24/18 05:43	1
Perfluorobutanesulfonic acid (PFBS)	36	U	90	16	ng/L		01/17/18 10:50	01/24/18 05:43	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	97		70 - 130	01/17/18 10:50	01/24/18 05:43	1
13C2 PFDA	97		70 - 130	01/17/18 10:50	01/24/18 05:43	1

Client Sample ID: WGNA-010818-RW-0404

Lab Sample ID: 320-34917-14

Date Collected: 01/08/18 09:40

Matrix: Water

Date Received: 01/09/18 10:30

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	26	J M	40	6.8	ng/L		01/17/18 10:50	01/24/18 05:47	1
Perfluorooctanoic acid (PFOA)	21		20	2.8	ng/L		01/17/18 10:50	01/24/18 05:47	1
Perfluorononanoic acid (PFNA)	20	U	24	8.0	ng/L		01/17/18 10:50	01/24/18 05:47	1
Perfluorohexanesulfonic acid (PFHxS)	8.3	J	30	5.5	ng/L		01/17/18 10:50	01/24/18 05:47	1
Perfluoroheptanoic acid (PFHpA)	6.3	J	10	1.9	ng/L		01/17/18 10:50	01/24/18 05:47	1
Perfluorobutanesulfonic acid (PFBS)	36	U	90	16	ng/L		01/17/18 10:50	01/24/18 05:47	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	96		70 - 130	01/17/18 10:50	01/24/18 05:47	1
13C2 PFDA	100		70 - 130	01/17/18 10:50	01/24/18 05:47	1

Client Sample ID: WGNA-010818-FRB-0404

Lab Sample ID: 320-34917-15

Date Collected: 01/08/18 09:35

Matrix: Water

Date Received: 01/09/18 10:30

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	16	U	40	6.7	ng/L		01/17/18 10:50	01/24/18 05:52	1
Perfluorooctanoic acid (PFOA)	7.9	U	20	2.8	ng/L		01/17/18 10:50	01/24/18 05:52	1
Perfluorononanoic acid (PFNA)	20	U	24	7.9	ng/L		01/17/18 10:50	01/24/18 05:52	1
Perfluorohexanesulfonic acid (PFHxS)	12	U	30	5.4	ng/L		01/17/18 10:50	01/24/18 05:52	1
Perfluoroheptanoic acid (PFHpA)	4.0	U	9.9	1.9	ng/L		01/17/18 10:50	01/24/18 05:52	1
Perfluorobutanesulfonic acid (PFBS)	36	U	89	16	ng/L		01/17/18 10:50	01/24/18 05:52	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	103		70 - 130	01/17/18 10:50	01/24/18 05:52	1
13C2 PFDA	103		70 - 130	01/17/18 10:50	01/24/18 05:52	1

Default Detection Limits

Client: Tetra Tech, Inc.

TestAmerica Job ID: 320-34917-1

Project/Site: Warminster: PFAS, NAS JRB Willow Grove

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Prep: 537

Analyte	LOQ	DL	Units	Method
Perfluorobutanesulfonic acid (PFBS)	90	16	ng/L	537
Perfluoroheptanoic acid (PFHpA)	10	1.9	ng/L	537
Perfluorohexanesulfonic acid (PFHxS)	30	5.5	ng/L	537
Perfluorononanoic acid (PFNA)	24	8.0	ng/L	537
Perfluorooctanesulfonic acid (PFOS)	40	6.8	ng/L	537
Perfluorooctanoic acid (PFOA)	20	2.8	ng/L	537

Surrogate Summary

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-34917-1

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Matrix: Water

Prep Type: Total/NA

Lab Sample ID	Client Sample ID	Percent Surrogate Recovery (Acceptance Limits)	
		PFHxA (70-130)	PFDA (70-130)
320-34917-1	WGNA-010818-RW-0344	91	93
320-34917-2	WGNA-010818-FRB-0344	97	98
320-34917-3	WGNA-010818-RW-3957	91	104
320-34917-4	WGNA-010818-FRB-3957	96	98
320-34917-5	WGNA-010818-DUP-16	96	109
320-34917-6	WGNA-010818-RW-3178	90	102
320-34917-7	WGNA-010818-FRB-3178	98	103
320-34917-8	NAWC-010818-RW-141	88	96
320-34917-9	NAWC-010818-FRB-141	95	99
320-34917-10	WGNA-010818-RW-4024	71	93
320-34917-10 LMS	WGNA-010818-RW-4024	88	95
320-34917-10 LMSD	WGNA-010818-RW-4024	90	97
320-34917-11	WGNA-010818-FRB-4024	98	100
320-34917-12	WGNA-010818-RW-4844	97	98
320-34917-13	WGNA-010818-FRB-4844	97	97
320-34917-14	WGNA-010818-RW-0404	96	100
320-34917-15	WGNA-010818-FRB-0404	103	103
LLCS 320-204304/2-A	Lab Control Sample	97	103
MB 320-204304/1-A	Method Blank	86	96

Surrogate Legend

PFHxA = 13C2 PFHxA

PFDA = 13C2 PFDA

QC Sample Results

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-34917-1

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Lab Sample ID: MB 320-204304/1-A
Matrix: Water
Analysis Batch: 204872

Client Sample ID: Method Blank
Prep Type: Total/NA
Prep Batch: 204304

Analyte	MB	MB	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
	Result	Qualifier							
Perfluorooctanesulfonic acid (PFOS)	16	U	40	6.8	ng/L		01/17/18 10:50	01/20/18 19:01	1
Perfluorooctanoic acid (PFOA)	8.0	U	20	2.8	ng/L		01/17/18 10:50	01/20/18 19:01	1
Perfluorononanoic acid (PFNA)	20	U	24	8.0	ng/L		01/17/18 10:50	01/20/18 19:01	1
Perfluorohexanesulfonic acid (PFHxS)	12	U	30	5.5	ng/L		01/17/18 10:50	01/20/18 19:01	1
Perfluoroheptanoic acid (PFHpA)	4.0	U	10	1.9	ng/L		01/17/18 10:50	01/20/18 19:01	1
Perfluorobutanesulfonic acid (PFBS)	36	U	90	16	ng/L		01/17/18 10:50	01/20/18 19:01	1
Surrogate	MB	MB	Limits				Prepared	Analyzed	Dil Fac
	%Recovery	Qualifier							
13C2 PFHxA	86		70 - 130				01/17/18 10:50	01/20/18 19:01	1
13C2 PFDA	96		70 - 130				01/17/18 10:50	01/20/18 19:01	1

Lab Sample ID: LLCS 320-204304/2-A
Matrix: Water
Analysis Batch: 204872

Client Sample ID: Lab Control Sample
Prep Type: Total/NA
Prep Batch: 204304

Analyte	Spike Added	LLCS	LLCS	Unit	D	%Rec	Limits
		Result	Qualifier				
Perfluorooctanesulfonic acid (PFOS)	40.0	39.2	J	ng/L		98	50 - 150
Perfluorooctanoic acid (PFOA)	20.0	20.1		ng/L		100	50 - 150
Perfluorononanoic acid (PFNA)	20.0	19.7	J	ng/L		98	50 - 150
Perfluorohexanesulfonic acid (PFHxS)	30.0	30.9		ng/L		103	50 - 150
Perfluoroheptanoic acid (PFHpA)	10.0	10.4		ng/L		104	50 - 150
Perfluorobutanesulfonic acid (PFBS)	90.0	85.8	J	ng/L		95	50 - 150
Surrogate	LLCS	LLCS	Limits			%Rec	Limits
	%Recovery	Qualifier					
13C2 PFHxA	97		70 - 130				
13C2 PFDA	103		70 - 130				

Lab Sample ID: 320-34917-10 LMS
Matrix: Water
Analysis Batch: 205331

Client Sample ID: WGNA-010818-RW-4024
Prep Type: Total/NA
Prep Batch: 204304

Analyte	Sample	Sample	Spike Added	LMS	LMS	Unit	D	%Rec	Limits
	Result	Qualifier		Result	Qualifier				
Perfluorooctanesulfonic acid (PFOS)	18	J M	40.2	58.5	M	ng/L		102	50 - 150
Perfluorooctanoic acid (PFOA)	12	J	20.1	31.9		ng/L		99	50 - 150
Perfluorononanoic acid (PFNA)	20	U	20.1	22.9	J	ng/L		114	50 - 150
Perfluorohexanesulfonic acid (PFHxS)	12	U	30.1	36.4		ng/L		121	50 - 150
Perfluoroheptanoic acid (PFHpA)	3.6	J	10.0	14.4		ng/L		108	50 - 150
Perfluorobutanesulfonic acid (PFBS)	36	U	90.3	95.9		ng/L		106	50 - 150
Surrogate	LMS	LMS	Limits					%Rec	Limits
	%Recovery	Qualifier							
13C2 PFHxA	88		70 - 130						
13C2 PFDA	95		70 - 130						

QC Sample Results

Client: Tetra Tech, Inc.
 Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-34917-1

Method: 537 - Perfluorinated Alkyl Acids (LC/MS) (Continued)

Lab Sample ID: 320-34917-10 LMSD

Matrix: Water

Analysis Batch: 205331

Client Sample ID: WGNA-010818-RW-4024

Prep Type: Total/NA

Prep Batch: 204304

Analyte	Sample	Sample	Spike	LMSD	LMSD	Unit	D	%Rec	%Rec.	RPD	RPD
	Result	Qualifier	Added	Result	Qualifier				Limits	Limit	
Perfluorooctanesulfonic acid (PFOS)	18	J M	38.8	56.7	M	ng/L		101	50 - 150	3	50
Perfluorooctanoic acid (PFOA)	12	J	19.4	32.3		ng/L		105	50 - 150	1	50
Perfluorononanoic acid (PFNA)	20	U	19.4	21.5	J	ng/L		111	50 - 150	6	50
Perfluorohexanesulfonic acid (PFHxS)	12	U	29.1	33.8		ng/L		116	50 - 150	7	50
Perfluoroheptanoic acid (PFHpA)	3.6	J	9.70	13.8		ng/L		106	50 - 150	4	50
Perfluorobutanesulfonic acid (PFBS)	36	U	87.3	98.5		ng/L		113	50 - 150	3	50
		LMSD	LMSD								
Surrogate		%Recovery	Qualifier	Limits							
13C2 PFHxA		90		70 - 130							
13C2 PFDA		97		70 - 130							

QC Association Summary

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-34917-1

LCMS

Prep Batch: 204304

Lab Sample ID	Client Sample ID	Prep Type	Matrix	Method	Prep Batch
320-34917-1	WGNA-010818-RW-0344	Total/NA	Water	537	
320-34917-2	WGNA-010818-FRB-0344	Total/NA	Water	537	
320-34917-3	WGNA-010818-RW-3957	Total/NA	Water	537	
320-34917-4	WGNA-010818-FRB-3957	Total/NA	Water	537	
320-34917-5	WGNA-010818-DUP-16	Total/NA	Water	537	
320-34917-6	WGNA-010818-RW-3178	Total/NA	Water	537	
320-34917-7	WGNA-010818-FRB-3178	Total/NA	Water	537	
320-34917-8	NAWC-010818-RW-141	Total/NA	Water	537	
320-34917-9	NAWC-010818-FRB-141	Total/NA	Water	537	
320-34917-10	WGNA-010818-RW-4024	Total/NA	Water	537	
320-34917-11	WGNA-010818-FRB-4024	Total/NA	Water	537	
320-34917-12	WGNA-010818-RW-4844	Total/NA	Water	537	
320-34917-13	WGNA-010818-FRB-4844	Total/NA	Water	537	
320-34917-14	WGNA-010818-RW-0404	Total/NA	Water	537	
320-34917-15	WGNA-010818-FRB-0404	Total/NA	Water	537	
MB 320-204304/1-A	Method Blank	Total/NA	Water	537	
LLCS 320-204304/2-A	Lab Control Sample	Total/NA	Water	537	
320-34917-10 LMS	WGNA-010818-RW-4024	Total/NA	Water	537	
320-34917-10 LMSD	WGNA-010818-RW-4024	Total/NA	Water	537	

Analysis Batch: 204872

Lab Sample ID	Client Sample ID	Prep Type	Matrix	Method	Prep Batch
320-34917-1	WGNA-010818-RW-0344	Total/NA	Water	537	204304
320-34917-2	WGNA-010818-FRB-0344	Total/NA	Water	537	204304
320-34917-3	WGNA-010818-RW-3957	Total/NA	Water	537	204304
320-34917-4	WGNA-010818-FRB-3957	Total/NA	Water	537	204304
320-34917-5	WGNA-010818-DUP-16	Total/NA	Water	537	204304
320-34917-6	WGNA-010818-RW-3178	Total/NA	Water	537	204304
320-34917-7	WGNA-010818-FRB-3178	Total/NA	Water	537	204304
320-34917-8	NAWC-010818-RW-141	Total/NA	Water	537	204304
MB 320-204304/1-A	Method Blank	Total/NA	Water	537	204304
LLCS 320-204304/2-A	Lab Control Sample	Total/NA	Water	537	204304

Analysis Batch: 205331

Lab Sample ID	Client Sample ID	Prep Type	Matrix	Method	Prep Batch
320-34917-9	NAWC-010818-FRB-141	Total/NA	Water	537	204304
320-34917-10	WGNA-010818-RW-4024	Total/NA	Water	537	204304
320-34917-11	WGNA-010818-FRB-4024	Total/NA	Water	537	204304
320-34917-12	WGNA-010818-RW-4844	Total/NA	Water	537	204304
320-34917-13	WGNA-010818-FRB-4844	Total/NA	Water	537	204304
320-34917-14	WGNA-010818-RW-0404	Total/NA	Water	537	204304
320-34917-15	WGNA-010818-FRB-0404	Total/NA	Water	537	204304
320-34917-10 LMS	WGNA-010818-RW-4024	Total/NA	Water	537	204304
320-34917-10 LMSD	WGNA-010818-RW-4024	Total/NA	Water	537	204304

Lab Chronicle

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-34917-1

Client Sample ID: WGNA-010818-RW-0344

Date Collected: 01/08/18 08:10

Date Received: 01/09/18 10:30

Lab Sample ID: 320-34917-1

Matrix: Water

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			204304	01/17/18 10:50	SK	TAL SAC
Total/NA	Analysis	537		1	204872	01/20/18 19:11	AAR	TAL SAC

Client Sample ID: WGNA-010818-FRB-0344

Date Collected: 01/08/18 08:05

Date Received: 01/09/18 10:30

Lab Sample ID: 320-34917-2

Matrix: Water

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			204304	01/17/18 10:50	SK	TAL SAC
Total/NA	Analysis	537		1	204872	01/20/18 19:15	AAR	TAL SAC

Client Sample ID: WGNA-010818-RW-3957

Date Collected: 01/08/18 08:40

Date Received: 01/09/18 10:30

Lab Sample ID: 320-34917-3

Matrix: Water

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			204304	01/17/18 10:50	SK	TAL SAC
Total/NA	Analysis	537		1	204872	01/20/18 19:20	AAR	TAL SAC

Client Sample ID: WGNA-010818-FRB-3957

Date Collected: 01/08/18 08:35

Date Received: 01/09/18 10:30

Lab Sample ID: 320-34917-4

Matrix: Water

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			204304	01/17/18 10:50	SK	TAL SAC
Total/NA	Analysis	537		1	204872	01/20/18 19:25	AAR	TAL SAC

Client Sample ID: WGNA-010818-DUP-16

Date Collected: 01/08/18 07:00

Date Received: 01/09/18 10:30

Lab Sample ID: 320-34917-5

Matrix: Water

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			204304	01/17/18 10:50	SK	TAL SAC
Total/NA	Analysis	537		1	204872	01/20/18 19:29	AAR	TAL SAC

Client Sample ID: WGNA-010818-RW-3178

Date Collected: 01/08/18 10:10

Date Received: 01/09/18 10:30

Lab Sample ID: 320-34917-6

Matrix: Water

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			204304	01/17/18 10:50	SK	TAL SAC
Total/NA	Analysis	537		1	204872	01/20/18 19:34	AAR	TAL SAC

TestAmerica Sacramento

Lab Chronicle

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-34917-1

Client Sample ID: WGNA-010818-FRB-3178

Lab Sample ID: 320-34917-7

Date Collected: 01/08/18 10:05

Matrix: Water

Date Received: 01/09/18 10:30

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			204304	01/17/18 10:50	SK	TAL SAC
Total/NA	Analysis	537		1	204872	01/20/18 19:39	AAR	TAL SAC

Client Sample ID: NAWC-010818-RW-141

Lab Sample ID: 320-34917-8

Date Collected: 01/08/18 11:10

Matrix: Water

Date Received: 01/09/18 10:30

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			204304	01/17/18 10:50	SK	TAL SAC
Total/NA	Analysis	537		1	204872	01/20/18 19:43	AAR	TAL SAC

Client Sample ID: NAWC-010818-FRB-141

Lab Sample ID: 320-34917-9

Date Collected: 01/08/18 11:05

Matrix: Water

Date Received: 01/09/18 10:30

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			204304	01/17/18 10:50	SK	TAL SAC
Total/NA	Analysis	537		1	205331	01/24/18 05:15	AAR	TAL SAC

Client Sample ID: WGNA-010818-RW-4024

Lab Sample ID: 320-34917-10

Date Collected: 01/08/18 11:40

Matrix: Water

Date Received: 01/09/18 10:30

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			204304	01/17/18 10:50	SK	TAL SAC
Total/NA	Analysis	537		1	205331	01/24/18 05:19	AAR	TAL SAC

Client Sample ID: WGNA-010818-FRB-4024

Lab Sample ID: 320-34917-11

Date Collected: 01/08/18 11:35

Matrix: Water

Date Received: 01/09/18 10:30

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			204304	01/17/18 10:50	SK	TAL SAC
Total/NA	Analysis	537		1	205331	01/24/18 05:33	AAR	TAL SAC

Client Sample ID: WGNA-010818-RW-4844

Lab Sample ID: 320-34917-12

Date Collected: 01/08/18 13:10

Matrix: Water

Date Received: 01/09/18 10:30

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			204304	01/17/18 10:50	SK	TAL SAC
Total/NA	Analysis	537		1	205331	01/24/18 05:38	AAR	TAL SAC

TestAmerica Sacramento

Lab Chronicle

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-34917-1

Client Sample ID: WGNA-010818-FRB-4844

Lab Sample ID: 320-34917-13

Date Collected: 01/08/18 13:05

Matrix: Water

Date Received: 01/09/18 10:30

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			204304	01/17/18 10:50	SK	TAL SAC
Total/NA	Analysis	537		1	205331	01/24/18 05:43	AAR	TAL SAC

Client Sample ID: WGNA-010818-RW-0404

Lab Sample ID: 320-34917-14

Date Collected: 01/08/18 09:40

Matrix: Water

Date Received: 01/09/18 10:30

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			204304	01/17/18 10:50	SK	TAL SAC
Total/NA	Analysis	537		1	205331	01/24/18 05:47	AAR	TAL SAC

Client Sample ID: WGNA-010818-FRB-0404

Lab Sample ID: 320-34917-15

Date Collected: 01/08/18 09:35

Matrix: Water

Date Received: 01/09/18 10:30

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			204304	01/17/18 10:50	SK	TAL SAC
Total/NA	Analysis	537		1	205331	01/24/18 05:52	AAR	TAL SAC

Laboratory References:

TAL SAC = TestAmerica Sacramento, 880 Riverside Parkway, West Sacramento, CA 95605, TEL (916)373-5600

Accreditation/Certification Summary

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-34917-1

Laboratory: TestAmerica Sacramento

All accreditations/certifications held by this laboratory are listed. Not all accreditations/certifications are applicable to this report.

Authority	Program	EPA Region	Identification Number	Expiration Date
Alaska (UST)	State Program	10	UST-055	01-31-18
Arizona	State Program	9	AZ0708	08-11-18
Arkansas DEQ	State Program	6	88-0691	06-17-18
California	State Program	9	2897	01-31-19
Colorado	State Program	8	CA00044	08-31-18
Connecticut	State Program	1	PH-0691	06-30-19
Florida	NELAP	4	E87570	06-30-18
Georgia	State Program	4	N/A	01-28-19
Hawaii	State Program	9	N/A	01-29-19
Illinois	NELAP	5	200060	03-17-18
Kansas	NELAP	7	E-10375	10-31-18
L-A-B	DoD ELAP		L2468	01-20-21
Louisiana	NELAP	6	30612	06-30-18
Maine	State Program	1	CA0004	04-14-18
Michigan	State Program	5	9947	01-31-18
Nevada	State Program	9	CA00044	07-31-18
New Hampshire	NELAP	1	2997	04-18-18
New Jersey	NELAP	2	CA005	06-30-18
New York	NELAP	2	11666	04-01-18
Oregon	NELAP	10	4040	01-29-20
Pennsylvania	NELAP	3	68-01272	03-31-18
Texas	NELAP	6	T104704399	05-31-18
US Fish & Wildlife	Federal		LE148388-0	07-31-18
USDA	Federal		P330-11-00436	01-17-21
USEPA UCMR	Federal	1	CA00044	11-06-18
Utah	NELAP	8	CA00044	02-28-18
Virginia	NELAP	3	460278	03-14-18
Washington	State Program	10	C581	05-05-18
Wyoming	State Program	8	8TMS-L	01-28-19

Method Summary

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-34917-1

Method	Method Description	Protocol	Laboratory
537	Perfluorinated Alkyl Acids (LC/MS)	EPA	TAL SAC

Protocol References:

EPA = US Environmental Protection Agency

Laboratory References:

TAL SAC = TestAmerica Sacramento, 880 Riverside Parkway, West Sacramento, CA 95605, TEL (916)373-5600

Sample Summary

Client: Tetra Tech, Inc.

TestAmerica Job ID: 320-34917-1

Project/Site: Warminster: PFAS, NAS JRB Willow Grove

Lab Sample ID	Client Sample ID	Matrix	Collected	Received
320-34917-1	WGNA-010818-RW-0344	Water	01/08/18 08:10	01/09/18 10:30
320-34917-2	WGNA-010818-FRB-0344	Water	01/08/18 08:05	01/09/18 10:30
320-34917-3	WGNA-010818-RW-3957	Water	01/08/18 08:40	01/09/18 10:30
320-34917-4	WGNA-010818-FRB-3957	Water	01/08/18 08:35	01/09/18 10:30
320-34917-5	WGNA-010818-DUP-16	Water	01/08/18 07:00	01/09/18 10:30
320-34917-6	WGNA-010818-RW-3178	Water	01/08/18 10:10	01/09/18 10:30
320-34917-7	WGNA-010818-FRB-3178	Water	01/08/18 10:05	01/09/18 10:30
320-34917-8	NAWC-010818-RW-141	Water	01/08/18 11:10	01/09/18 10:30
320-34917-9	NAWC-010818-FRB-141	Water	01/08/18 11:05	01/09/18 10:30
320-34917-10	WGNA-010818-RW-4024	Water	01/08/18 11:40	01/09/18 10:30
320-34917-11	WGNA-010818-FRB-4024	Water	01/08/18 11:35	01/09/18 10:30
320-34917-12	WGNA-010818-RW-4844	Water	01/08/18 13:10	01/09/18 10:30
320-34917-13	WGNA-010818-FRB-4844	Water	01/08/18 13:05	01/09/18 10:30
320-34917-14	WGNA-010818-RW-0404	Water	01/08/18 09:40	01/09/18 10:30
320-34917-15	WGNA-010818-FRB-0404	Water	01/08/18 09:35	01/09/18 10:30

LCMS MANUAL INTEGRATION SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1

SDG No.: _____

Instrument ID: A8_N Analysis Batch Number: 192908

Lab Sample ID: IC 320-192908/4 Client Sample ID: _____

Date Analyzed: 11/03/17 13:37 Lab File ID: 2017.11.03_537XICAL_004.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.16	Assign Peak	phomsophat	11/06/17 07:17

Lab Sample ID: IC 320-192908/5 Client Sample ID: _____

Date Analyzed: 11/03/17 13:42 Lab File ID: 2017.11.03_537XICAL_005.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.16	Assign Peak	phomsophat	11/06/17 07:18

Lab Sample ID: IC 320-192908/7 ICISAV Client Sample ID: _____

Date Analyzed: 11/03/17 13:52 Lab File ID: 2017.11.03_537XICAL_007.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.16	Assign Peak	phomsophat	11/06/17 07:20

LCMS MANUAL INTEGRATION SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1

SDG No.: _____

Instrument ID: A8_N Analysis Batch Number: 204872

Lab Sample ID: 320-34917-3 Client Sample ID: WGNA-010818-RW-3957

Date Analyzed: 01/20/18 19:20 Lab File ID: 2018.01.20_537AA_011.d GC Column: GeminiC18 3x1 ID: 3 (mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorononanoic acid (PFNA)	2.06	Assign Peak	roycea	01/22/18 13:25

LCMS MANUAL INTEGRATION SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1

SDG No.: _____

Instrument ID: A8_N Analysis Batch Number: 205331

Lab Sample ID: CCVL 320-205331/1 Client Sample ID: _____

Date Analyzed: 01/24/18 05:01 Lab File ID: 2018.01.23537A_004.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.06	User Assigned	roycea	01/24/18 09:52

Lab Sample ID: CCV 320-205331/2 CCVIS Client Sample ID: _____

Date Analyzed: 01/24/18 05:05 Lab File ID: 2018.01.23537A_005.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.07	User Assigned	roycea	01/24/18 09:52

Lab Sample ID: 320-34917-10 Client Sample ID: WGNA-010818-RW-4024

Date Analyzed: 01/24/18 05:19 Lab File ID: 2018.01.23537A_008.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.06	Assign Peak	roycea	01/24/18 09:53

Lab Sample ID: 320-34917-10 LMS Client Sample ID: WGNA-010818-RW-4024 LMS

Date Analyzed: 01/24/18 05:24 Lab File ID: 2018.01.23537A_009.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.06	User Assigned	roycea	01/24/18 09:54

LCMS MANUAL INTEGRATION SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1

SDG No.: _____

Instrument ID: A8_N Analysis Batch Number: 205331

Lab Sample ID: 320-34917-10 LMSD Client Sample ID: WGNA-010818-RW-4024 LMSD

Date Analyzed: 01/24/18 05:29 Lab File ID: 2018.01.23537A_010.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.06	User Assigned	roycea	01/24/18 09:55

Lab Sample ID: 320-34917-12 Client Sample ID: WGNA-010818-RW-4844

Date Analyzed: 01/24/18 05:38 Lab File ID: 2018.01.23537A_012.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.06	Assign Peak	roycea	01/24/18 09:56

Lab Sample ID: 320-34917-14 Client Sample ID: WGNA-010818-RW-0404

Date Analyzed: 01/24/18 05:47 Lab File ID: 2018.01.23537A_014.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.06	User Assigned	roycea	01/24/18 09:57

Lab Sample ID: CCV 320-205331/13 CCVIS Client Sample ID: _____

Date Analyzed: 01/24/18 05:57 Lab File ID: 2018.01.23537A_016.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.06	User Assigned	roycea	01/24/18 09:58

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-34917-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
LC537-ICV_00028	01/05/18	08/02/17	MeOH/H2O, Lot 067374	10 mL	LC537-IS_00045	1000 uL	13C2-PFOA	10 ng/mL
.LC537-IS_00045	01/05/18	07/05/17	Methanol, Lot 090285	30000 uL	LCM2PFOA_00007	60 uL	13C2-PFOA	28.68 ng/mL
..LCM2PFOA_00007	02/12/21	Wellington Laboratories, Lot M2PFOA0216			(Purchased Reagent)		13C2-PFOA	0.1 ug/mL
..LCMPFOS_00019	08/03/21	Wellington Laboratories, Lot MPFOS0816			(Purchased Reagent)		13C4 PFOS	0.2868 ug/mL
LC537-ICV_00028	01/05/18	08/02/17	MeOH/H2O, Lot 067374	10 mL	LC537-SU_00046	1000 uL	13C2 PFDA	50 ug/mL
.LC537-SU_00046	01/05/18	07/05/17	Methanol, Lot 104453	30000 uL	LC537ICIM_00019	20 uL	13C2 PFHxA	47.8 ug/mL
..LCMPFDA_00012	09/30/21	Wellington Laboratories, Lot MPFDA0916			(Purchased Reagent)		13C2 PFDA	10 ng/mL
..LCMPFHxA_00013	04/08/21	Wellington Laboratories, Lot MPFHxA0416			(Purchased Reagent)		13C2 PFHxA	10 ng/mL
.LC537ICIM_00019	01/25/18	08/01/17	Methanol, Lot 090285	25 mL	LC537-PFBS2_00008	0.6 mL	Perfluorobutanesulfonic acid (PFBS)	100.119 ng/mL
..LC537-PFBS2_00008	01/25/18	07/25/17	Methanol, Lot 090285	20 mL	LC537-PFHxA2_00011	0.061 mL	Perfluoroheptanoic acid (PFHpA)	9.99613 ng/mL
...LC537-PFHxA2_00011	09/08/22	Santa Cruz Biotechnology, Lot F0917			(Purchased Reagent)		Perfluoroheptanoic acid (PFHpA)	20.0761 ng/mL
..LC537-PFHxA2_00011	01/25/18	07/25/17	Methanol, Lot 09092	31 mL	LC537-PFHxS2_00008	0.122 mL	Perfluorohexanesulfonic acid (PFHxS)	20.1272 ng/mL
...LC537-PFHxS2_00008	06/13/22	Afla Aesar, Lot 10200390			(Purchased Reagent)		Perfluorohexanesulfonic acid (PFHxS)	20.4843 ng/mL
..LC537-PFHxS2_00008	01/25/18	07/25/17	Methanol, Lot 090285	21 mL	LC537-PFNA2_00009	0.126 mL	Perfluorononanoic acid (PFNA)	19.698 ng/mL
...LC537-PFNA2_00009	06/08/22	Santa Cruz Biotechnology, Lot G2516			(Purchased Reagent)		Perfluorononanoic acid (PFNA)	19.698 ng/mL
..LC537-PFOA2_00010	01/25/18	08/01/17	Methanol, Lot 090285	20 mL	LC537-PFOA2_00010	0.122 mL	Perfluorooctanoic acid (PFOA)	20.1272 ng/mL
...LC537-PFOA2_00010	06/09/22	Afla Aesar, Lot 10199078			(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	20.4843 ng/mL
..LC537-PFOS2_00010	01/25/18	08/01/17	Methanol, Lot 090285	20 mL	LC537-PFOS2_00010	0.124 mL	Perfluorooctanesulfonic acid (PFOS)	20.4843 ng/mL
...LC537-PFOS2_00010	06/09/22	Afla Aesar, Lot 10199078			(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	19.698 ng/mL
..LC537-PFOS2_00002	01/25/18	07/25/17	Methanol, Lot 090285	21 mL	LC537-PFOS2_00002	0.0418 g	Perfluorobutanesulfonic acid (PFBS)	2085.82 ug/mL
...LC537-PFOS2_00002	09/08/22	Santa Cruz Biotechnology, Lot F0917			(Purchased Reagent)		Perfluorobutanesulfonic acid (PFBS)	2085.82 ug/mL
..LC537-PFHxA2_00011	01/25/18	07/25/17	Methanol, Lot 09092	31 mL	LC537-PFHxA2_00002	0.0635 g	Perfluoroheptanoic acid (PFHpA)	0.998 g/g
...LC537-PFHxA2_00002	06/13/22	Afla Aesar, Lot 10200390			(Purchased Reagent)		Perfluoroheptanoic acid (PFHpA)	2048.39 ug/mL
..LC537-PFHxS2_00008	01/25/18	07/25/17	Methanol, Lot 090285	21 mL	LC537-PFHxS2_00002	0.0475 g	Perfluorohexanesulfonic acid (PFHxS)	1 g/g
...LC537-PFHxS2_00002	06/08/22	Santa Cruz Biotechnology, Lot G2516			(Purchased Reagent)		Perfluorohexanesulfonic acid (PFHxS)	2056.98 ug/mL
..LC537-PFNA2_00009	01/25/18	07/25/17	Methanol, Lot 090285	21 mL	LC537-PFNA2_00002	0.0421 g	Perfluorohexanesulfonic acid (PFHxS)	0.9094 g/g
...LC537-PFNA2_00002	06/14/22	Aldrich, Lot MKCC0699			(Purchased Reagent)		Perfluorohexanesulfonic acid (PFHxS)	0.9094 g/g
..LC537-PFOA2_00010	01/25/18	08/01/17	Methanol, Lot 090285	20 mL	LC537-PFOA2_00002	0.0424 g	Perfluorononanoic acid (PFNA)	1996.74 ug/mL
...LC537-PFOA2_00002	06/09/22	Afla Aesar, Lot 10199078			(Purchased Reagent)		Perfluorononanoic acid (PFNA)	1996.74 ug/mL
..LC537-PFOA2_00002	01/25/18	08/01/17	Methanol, Lot 090285	20 mL	LC537-PFOA2_00002	0.0424 g	Perfluorononanoic acid (PFNA)	0.996 g/g
...LC537-PFOA2_00002	06/09/22	Afla Aesar, Lot 10199078			(Purchased Reagent)		Perfluorononanoic acid (PFNA)	0.996 g/g
..LC537-PFOA2_00002	01/25/18	08/01/17	Methanol, Lot 090285	20 mL	LC537-PFOA2_00002	0.0424 g	Perfluorooctanoic acid (PFOA)	2098.8 ug/mL
...LC537-PFOA2_00002	06/09/22	Afla Aesar, Lot 10199078			(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	2098.8 ug/mL
..LC537-PFOA2_00002	01/25/18	08/01/17	Methanol, Lot 090285	20 mL	LC537-PFOA2_00002	0.0424 g	Perfluorooctanoic acid (PFOA)	0.99 g/g
...LC537-PFOA2_00002	06/09/22	Afla Aesar, Lot 10199078			(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	0.99 g/g

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-34917-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
..LC537-PFOS2_00010	01/25/18	08/01/17	Methanol, Lot 090285	22 mL	LC537_PFOS2_00002	0.0561 g	Perfluorooctanesulfonic acid (PFOS)	1985.68 ug/mL
...LC537_PFOS2_00002	06/14/22		Sigma, Lot BCBQ0108V		(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	0.7787 g/g
LC537-IS_00056	05/27/18	11/27/17	Methanol, Lot 090285	30000 uL	LCM2PFOA_00007	60 uL	13C2-PFOA	0.1 ug/mL
					LCMPFOS_00021	180 uL	13C4 PFOS	0.2868 ug/mL
..LCM2PFOA_00007	02/12/21	Wellington Laboratories, Lot M2PFOA0216			(Purchased Reagent)		13C2-PFOA	50 ug/mL
..LCMPFOS_00021	12/12/21	Wellington Laboratories, Lot MPFOS1216			(Purchased Reagent)		13C4 PFOS	47.8 ug/mL
LC537-L1_00020	02/04/18	08/14/17	MeOH/H2O, Lot 090285	5 mL	LC537-IS_00048	500 uL	13C2-PFOA	10 ng/mL
							13C4 PFOS	28.68 ng/mL
					LC537-MSP_00029	60 uL	Perfluorobutanesulfonic acid (PFBS)	9.0018 ng/mL
							Perfluoroheptanoic acid (PFHpA)	1.00036 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	3.00103 ng/mL
							Perfluorononanoic acid (PFNA)	2.0006 ng/mL
							Perfluorooctanoic acid (PFOA)	2.00191 ng/mL
							Perfluorooctanesulfonic acid (PFOS)	4.00146 ng/mL
					LC537-SU_00049	500 uL	13C2 PFDA	10 ng/mL
							13C2 PFHxA	10 ng/mL
..LC537-IS_00048	02/04/18	08/04/17	Methanol, Lot 090285	30000 uL	LCM2PFOA_00007	60 uL	13C2-PFOA	0.1 ug/mL
					LCMPFOS_00021	180 uL	13C4 PFOS	0.2868 ug/mL
..LCM2PFOA_00007	02/12/21	Wellington Laboratories, Lot M2PFOA0216			(Purchased Reagent)		13C2-PFOA	50 ug/mL
..LCMPFOS_00021	12/12/21	Wellington Laboratories, Lot MPFOS1216			(Purchased Reagent)		13C4 PFOS	47.8 ug/mL
..LC537-MSP_00029	02/10/18	08/10/17	Methanol, Lot 141039	20000 uL	LC537SPIM_00023	166.7 uL	Perfluorobutanesulfonic acid (PFBS)	750.15 ng/mL
							Perfluoroheptanoic acid (PFHpA)	83.3637 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	250.086 ng/mL
							Perfluorononanoic acid (PFNA)	166.716 ng/mL
							Perfluorooctanoic acid (PFOA)	166.826 ng/mL
							Perfluorooctanesulfonic acid (PFOS)	333.455 ng/mL
..LC537SPIM_00023	02/10/18	08/10/17	Methanol, Lot 104453	10000 uL	LC537-PFBS_00008	450 uL	Perfluorobutanesulfonic acid (PFBS)	90 ug/mL
					LC537-PFHpA_00015	100 uL	Perfluoroheptanoic acid (PFHpA)	10.0016 ug/mL
					LC537-PFHxS_00010	150 uL	Perfluorohexanesulfonic acid (PFHxS)	30.0043 ug/mL
					LC537-PFNA_00013	200 uL	Perfluorononanoic acid (PFNA)	20.002 ug/mL
					LC537-PFOA_00013	200 uL	Perfluorooctanoic acid (PFOA)	20.0151 ug/mL
					LC537-PFOS_00008	400 uL	Perfluorooctanesulfonic acid (PFOS)	40.0066 ug/mL
...LC537-PFBS_00008	02/10/18	08/10/17	Methanol, Lot 090285	49.6 mL	LC537_PFBS_00002	0.0992 g	Perfluorobutanesulfonic acid (PFBS)	2 mg/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-34917-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
....LC537_PFBs_00002	04/01/18		Sigma, Lot MKBP8842V		(Purchased Reagent)		Perfluorobutanesulfonic acid (PFBS)	1 g/g
...LC537-PFHpA_00015	02/10/18	08/10/17	Methanol, Lot 090285	48.7 mL	LC537_PFHpA_00002	0.0492 g	Perfluoroheptanoic acid (PFHpA)	1.00016 mg/mL
....LC537_PFHpA_00002	04/01/18		Aldrich, Lot BCBM2579V		(Purchased Reagent)		Perfluoroheptanoic acid (PFHpA)	0.99 g/g
...LC537-PFHxS_00010	02/10/18	08/10/17	Methanol, Lot 090285	55.92 mL	LC537_PFHxS_00002	0.123 g	Perfluorohexanesulfonic acid (PFHxS)	2.00029 mg/mL
....LC537_PFHxS_00002	04/01/18		Sigma, Lot BCBL3545V		(Purchased Reagent)		Perfluorohexanesulfonic acid (PFHxS)	0.9094 g/g
..LC537-PFNA_00013	02/10/18	08/10/17	Methanol, Lot 090285	62.3 mL	LC537 PFNA_00002	0.0647 g	Perfluorononanoic acid (PFNA)	1000.1 ug/mL
....LC537 PFNA_00002	04/01/18		TCI America, Lot QN44F		(Purchased Reagent)		Perfluorononanoic acid (PFNA)	0.963 g/g
...LC537-PFOA_00013	02/10/18	08/10/17	Methanol, Lot 090285	22.76 mL	LC537 PFOA_00003	0.0228 g	Perfluorooctanoic acid (PFOA)	1.00076 mg/mL
....LC537 PFOA_00003	10/31/23		SIGMA ALDRICH, Lot BCBS1198V		(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	0.999 g/g
...LC537-PFOS_00008	02/10/18	08/10/17	Methanol, Lot 090285	44.43 mL	LC537_PFOS_00003	0.0488 g	Perfluorooctanesulfonic acid (PFOS)	1.00016 mg/mL
....LC537_PFOS_00003	04/17/19		sigma alrich, Lot SZBE107XV		(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	0.9106 g/g
.LC537-SU_00049	02/04/18	08/04/17	Methanol, Lot 104453	30000 uL	LCMPFDA_00012	60 uL	13C2 PFDA	0.1 ug/mL
..LCMPFDA_00012	09/30/21		Wellington Laboratories, Lot MPFDA0916		(Purchased Reagent)		13C2 PFDA	50 ug/mL
..LCMPFHxA_00013	04/08/21		Wellington Laboratories, Lot MPFHxA0416		(Purchased Reagent)		13C2 PFHxA	50 ug/mL
LC537-L2_00020	02/04/18	08/14/17	MeOH/H2O, Lot 090285	5 mL	LC537-HSP_00025	80 uL	Perfluorobutanesulfonic acid (PFBS)	20.0016 ng/mL
							Perfluoroheptanoic acid (PFHpA)	2.22277 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	6.66817 ng/mL
							Perfluorononanoic acid (PFNA)	4.44524 ng/mL
							Perfluorooctanoic acid (PFOA)	4.44816 ng/mL
							Perfluorooctanesulfonic acid (PFOS)	8.89106 ng/mL
LC537-IS_00048	500 uL	13C2-PFOA	10 ng/mL					
LC537-SU_00049	500 uL	13C4 PFOS	28.68 ng/mL					
.LC537-HSP_00025	02/10/18	08/10/17	Methanol, Lot 141039	20000 uL	LC537SPIM_00023	277.8 uL	Perfluorobutanesulfonic acid (PFBS)	1250.1 ng/mL
							Perfluoroheptanoic acid (PFHpA)	138.923 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	416.76 ng/mL
							Perfluorononanoic acid (PFNA)	277.827 ng/mL
							Perfluorooctanoic acid (PFOA)	278.01 ng/mL
							Perfluorooctanesulfonic acid (PFOS)	555.691 ng/mL
..LC537SPIM_00023	02/10/18	08/10/17	Methanol, Lot 104453	10000 uL	LC537-PFBS_00008	450 uL	Perfluorobutanesulfonic acid (PFBS)	90 ug/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-34917-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
					LC537-PFHpA_00015	100 uL	Perfluoroheptanoic acid (PFHpA)	10.0016 ug/mL
					LC537-PFHxS_00010	150 uL	Perfluorohexanesulfonic acid (PFHxS)	30.0043 ug/mL
					LC537-PFNA_00013	200 uL	Perfluorononanoic acid (PFNA)	20.002 ug/mL
					LC537-PFOA_00013	200 uL	Perfluorooctanoic acid (PFOA)	20.0151 ug/mL
					LC537-PFOS_00008	400 uL	Perfluorooctanesulfonic acid (PFOS)	40.0066 ug/mL
...LC537-PFBS_00008	02/10/18	08/10/17	Methanol, Lot 090285	49.6 mL	LC537_PFBS_00002	0.0992 g	Perfluorobutanesulfonic acid (PFBS)	2 mg/mL
....LC537_PFBS_00002	04/01/18	Sigma, Lot MKBP8842V			(Purchased Reagent)		Perfluorobutanesulfonic acid (PFBS)	1 g/g
...LC537-PFHpA_00015	02/10/18	08/10/17	Methanol, Lot 090285	48.7 mL	LC537_PFHpA_00002	0.0492 g	Perfluoroheptanoic acid (PFHpA)	1.00016 mg/mL
....LC537_PFHpA_00002	04/01/18	Aldrich, Lot BCM2579V			(Purchased Reagent)		Perfluoroheptanoic acid (PFHpA)	0.99 g/g
...LC537-PFHxS_00010	02/10/18	08/10/17	Methanol, Lot 090285	55.92 mL	LC537_PFHxS_00002	0.123 g	Perfluorohexanesulfonic acid (PFHxS)	2.00029 mg/mL
....LC537_PFHxS_00002	04/01/18	Sigma, Lot BCBL3545V			(Purchased Reagent)		Perfluorohexanesulfonic acid (PFHxS)	0.9094 g/g
...LC537-PFNA_00013	02/10/18	08/10/17	Methanol, Lot 090285	62.3 mL	LC537_PFNA_00002	0.0647 g	Perfluorononanoic acid (PFNA)	1000.1 ug/mL
....LC537_PFNA_00002	04/01/18	TCI America, Lot QN44F			(Purchased Reagent)		Perfluorononanoic acid (PFNA)	0.963 g/g
...LC537-PFOA_00013	02/10/18	08/10/17	Methanol, Lot 090285	22.76 mL	LC537_PFOA_00003	0.0228 g	Perfluorooctanoic acid (PFOA)	1.00076 mg/mL
....LC537_PFOA_00003	10/31/23	SIGMA ALDRICH, Lot BCBS1198V			(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	0.999 g/g
...LC537-PFOS_00008	02/10/18	08/10/17	Methanol, Lot 090285	44.43 mL	LC537_PFOS_00003	0.0488 g	Perfluorooctanesulfonic acid (PFOS)	1.00016 mg/mL
....LC537_PFOS_00003	04/17/19	sigma alrich, Lot SZBE107XV			(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	0.9106 g/g
.LC537-IS_00048	02/04/18	08/04/17	Methanol, Lot 090285	30000 uL	LCM2PFOA_00007	60 uL	13C2-PFOA	0.1 ug/mL
..LCM2PFOA_00007	02/12/21	Wellington Laboratories, Lot M2PFOA0216			LCMPFOS_00021	180 uL	13C4 PFOS	0.2868 ug/mL
..LCMPFOS_00021	12/12/21	Wellington Laboratories, Lot MPFOS1216			(Purchased Reagent)		13C2-PFOA	50 ug/mL
.LC537-SU_00049	02/04/18	08/04/17	Methanol, Lot 104453	30000 uL	LCMPFDA_00012	60 uL	13C2 PFDA	47.8 ug/mL
..LCMPFDA_00012	09/30/21	Wellington Laboratories, Lot MPFDA0916			LCMPFHxA_00013	60 uL	13C2 PFHxA	0.1 ug/mL
..LCMPFHxA_00013	04/08/21	Wellington Laboratories, Lot MPFHxA0416			(Purchased Reagent)		13C2 PFDA	50 ug/mL
							13C2 PFHxA	50 ug/mL
LC537-L3_00023	02/04/18	08/14/17	MeOH/H2O, Lot 090285	5 mL	LC537-HSP_00025	180 uL	Perfluorobutanesulfonic acid (PFBS)	45.0036 ng/mL
							Perfluoroheptanoic acid (PFHpA)	5.00122 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	15.0034 ng/mL
							Perfluorononanoic acid (PFNA)	10.0018 ng/mL
							Perfluorooctanoic acid (PFOA)	10.0084 ng/mL
							Perfluorooctanesulfonic acid (PFOS)	20.0049 ng/mL
					LC537-IS_00048	500 uL	13C2-PFOA	10 ng/mL
							13C4 PFOS	28.68 ng/mL
					LC537-SU_00049	500 uL	13C2 PFDA	10 ng/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-34917-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration		
					Reagent ID	Volume Added				
.LC537-HSP_00025	02/10/18	08/10/17	Methanol, Lot 141039	20000 uL	LC537SPIM_00023	277.8 uL	13C2 PFHxA	10 ng/mL		
							Perfluorobutanesulfonic acid (PFBS)	1250.1 ng/mL		
							Perfluoroheptanoic acid (PFHpA)	138.923 ng/mL		
							Perfluorohexanesulfonic acid (PFHxS)	416.76 ng/mL		
							Perfluorononanoic acid (PFNA)	277.827 ng/mL		
Perfluorooctanoic acid (PFOA)	278.01 ng/mL									
Perfluorooctanesulfonic acid (PFOS)	555.691 ng/mL									
..LC537SPIM_00023	02/10/18	08/10/17	Methanol, Lot 104453	10000 uL	LC537-PFBS_00008	450 uL	Perfluorobutanesulfonic acid (PFBS)	90 ug/mL		
							LC537-PFHpA_00015	100 uL	Perfluoroheptanoic acid (PFHpA)	10.0016 ug/mL
							LC537-PFHxS_00010	150 uL	Perfluorohexanesulfonic acid (PFHxS)	30.0043 ug/mL
							LC537-PFNA_00013	200 uL	Perfluorononanoic acid (PFNA)	20.002 ug/mL
							LC537-PFOA_00013	200 uL	Perfluorooctanoic acid (PFOA)	20.0151 ug/mL
							LC537-PFOS_00008	400 uL	Perfluorooctanesulfonic acid (PFOS)	40.0066 ug/mL
...LC537-PFBS_00008	02/10/18	08/10/17	Methanol, Lot 090285	49.6 mL	LC537_PFBS_00002	0.0992 g	Perfluorobutanesulfonic acid (PFBS)	2 mg/mL		
....LC537_PFBS_00002	04/01/18		Sigma, Lot MKBP8842V		(Purchased Reagent)		Perfluorobutanesulfonic acid (PFBS)	1 g/g		
...LC537-PFHpA_00015	02/10/18	08/10/17	Methanol, Lot 090285	48.7 mL	LC537_PFHpA_00002	0.0492 g	Perfluoroheptanoic acid (PFHpA)	1.00016 mg/mL		
....LC537_PFHpA_00002	04/01/18		Aldrich, Lot BCBM2579V		(Purchased Reagent)		Perfluoroheptanoic acid (PFHpA)	0.99 g/g		
...LC537-PFHxS_00010	02/10/18	08/10/17	Methanol, Lot 090285	55.92 mL	LC537_PFHxS_00002	0.123 g	Perfluorohexanesulfonic acid (PFHxS)	2.00029 mg/mL		
....LC537_PFHxS_00002	04/01/18		Sigma, Lot BCBL3545V		(Purchased Reagent)		Perfluorohexanesulfonic acid (PFHxS)	0.9094 g/g		
...LC537-PFNA_00013	02/10/18	08/10/17	Methanol, Lot 090285	62.3 mL	LC537 PFNA_00002	0.0647 g	Perfluorononanoic acid (PFNA)	1000.1 ug/mL		
....LC537 PFNA_00002	04/01/18		TCI America, Lot QN44F		(Purchased Reagent)		Perfluorononanoic acid (PFNA)	0.963 g/g		
...LC537-PFOA_00013	02/10/18	08/10/17	Methanol, Lot 090285	22.76 mL	LC537 PFOA_00003	0.0228 g	Perfluorooctanoic acid (PFOA)	1.00076 mg/mL		
....LC537 PFOA_00003	10/31/23		SIGMA ALDRICH, Lot BCBS1198V		(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	0.999 g/g		
...LC537-PFOS_00008	02/10/18	08/10/17	Methanol, Lot 090285	44.43 mL	LC537_PFOS_00003	0.0488 g	Perfluorooctanesulfonic acid (PFOS)	1.00016 mg/mL		
....LC537_PFOS_00003	04/17/19		sigma alrich, Lot SZBE107XV		(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	0.9106 g/g		
.LC537-IS_00048	02/04/18	08/04/17	Methanol, Lot 090285	30000 uL	LCM2PFOA_00007	60 uL	13C2-PFOA	0.1 ug/mL		
..LCM2PFOA_00007	02/12/21		Wellington Laboratories, Lot M2PFOA0216		(Purchased Reagent)		13C4 PFOS	0.2868 ug/mL		
..LCMPFOS_00021	12/12/21		Wellington Laboratories, Lot MPFOS1216		(Purchased Reagent)		13C2-PFOA	50 ug/mL		
.LC537-SU_00049	02/04/18	08/04/17	Methanol, Lot 104453	30000 uL	LCMPFDA_00012	60 uL	13C2 PFDA	0.1 ug/mL		
..LCMPFDA_00012	09/30/21		Wellington Laboratories, Lot MPFDA0916		(Purchased Reagent)		13C2 PFHxA	0.1 ug/mL		
..LCMPFHxA_00013	04/08/21		Wellington Laboratories, Lot MPFHxA0416		(Purchased Reagent)		13C2 PFHxA	50 ug/mL		

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-34917-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration		
					Reagent ID	Volume Added				
LC537-L4_00020	02/04/18	08/14/17	MeOH/H2O, Lot 090285	5 mL	LC537-HSP_00025	360 uL	Perfluorobutanesulfonic acid (PFBS)	90.0072 ng/mL		
							Perfluoroheptanoic acid (PFHpA)	10.0024 ng/mL		
							Perfluorohexanesulfonic acid (PFHxS)	30.0067 ng/mL		
							Perfluorononanoic acid (PFNA)	20.0036 ng/mL		
							Perfluorooctanoic acid (PFOA)	20.0167 ng/mL		
					Perfluorooctanesulfonic acid (PFOS)	40.0098 ng/mL				
					LC537-IS_00048	500 uL	13C2-PFOA	10 ng/mL		
LC537-SU_00049	500 uL	13C2 PFDA	10 ng/mL							
.LC537-HSP_00025	02/10/18	08/10/17	Methanol, Lot 141039	20000 uL	LC537SPIM_00023	277.8 uL	Perfluorobutanesulfonic acid (PFBS)	1250.1 ng/mL		
							Perfluoroheptanoic acid (PFHpA)	138.923 ng/mL		
							Perfluorohexanesulfonic acid (PFHxS)	416.76 ng/mL		
							Perfluorononanoic acid (PFNA)	277.827 ng/mL		
							Perfluorooctanoic acid (PFOA)	278.01 ng/mL		
Perfluorooctanesulfonic acid (PFOS)	555.691 ng/mL									
..LC537SPIM_00023	02/10/18	08/10/17	Methanol, Lot 104453	10000 uL	LC537-PFBS_00008	450 uL	Perfluorobutanesulfonic acid (PFBS)	90 ug/mL		
							LC537-PFHpA_00015	100 uL	Perfluoroheptanoic acid (PFHpA)	10.0016 ug/mL
							LC537-PFHxS_00010	150 uL	Perfluorohexanesulfonic acid (PFHxS)	30.0043 ug/mL
							LC537-PFNA_00013	200 uL	Perfluorononanoic acid (PFNA)	20.002 ug/mL
							LC537-PFOA_00013	200 uL	Perfluorooctanoic acid (PFOA)	20.0151 ug/mL
							LC537-PFOS_00008	400 uL	Perfluorooctanesulfonic acid (PFOS)	40.0066 ug/mL
...LC537-PFBS_00008	02/10/18	08/10/17	Methanol, Lot 090285	49.6 mL	LC537_PFBS_00002	0.0992 g	Perfluorobutanesulfonic acid (PFBS)	2 mg/mL		
....LC537_PFBS_00002	04/01/18		Sigma, Lot MKBP8842V		(Purchased Reagent)		Perfluorobutanesulfonic acid (PFBS)	1 g/g		
...LC537-PFHpA_00015	02/10/18	08/10/17	Methanol, Lot 090285	48.7 mL	LC537_PFHpA_00002	0.0492 g	Perfluoroheptanoic acid (PFHpA)	1.00016 mg/mL		
....LC537_PFHpA_00002	04/01/18		Aldrich, Lot BCBM2579V		(Purchased Reagent)		Perfluoroheptanoic acid (PFHpA)	0.99 g/g		
...LC537-PFHxS_00010	02/10/18	08/10/17	Methanol, Lot 090285	55.92 mL	LC537_PFHxS_00002	0.123 g	Perfluorohexanesulfonic acid (PFHxS)	2.00029 mg/mL		
....LC537_PFHxS_00002	04/01/18		Sigma, Lot BCBL3545V		(Purchased Reagent)		Perfluorohexanesulfonic acid (PFHxS)	0.9094 g/g		
...LC537-PFNA_00013	02/10/18	08/10/17	Methanol, Lot 090285	62.3 mL	LC537 PFNA_00002	0.0647 g	Perfluorononanoic acid (PFNA)	1000.1 ug/mL		
....LC537 PFNA_00002	04/01/18		TCI America, Lot QN44F		(Purchased Reagent)		Perfluorononanoic acid (PFNA)	0.963 g/g		
...LC537-PFOA_00013	02/10/18	08/10/17	Methanol, Lot 090285	22.76 mL	LC537 PFOA_00003	0.0228 g	Perfluorooctanoic acid (PFOA)	1.00076 mg/mL		
....LC537_PFOA_00003	10/31/23		SIGMA ALDRICH, Lot BCBS1198V		(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	0.999 g/g		

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-34917-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
...LC537-PFOS_00008	02/10/18	08/10/17	Methanol, Lot 090285	44.43 mL	LC537_PFOS_00003	0.0488 g	Perfluorooctanesulfonic acid (PFOS)	1.00016 mg/mL
....LC537_PFOS_00003	04/17/19	sigma alrich, Lot SZBE107XV			(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	0.9106 g/g
.LC537-IS_00048	02/04/18	08/04/17	Methanol, Lot 090285	30000 uL	LCM2PFOA 00007	60 uL	13C2-PFOA	0.1 ug/mL
					LCMPFOS 00021	180 uL	13C4 PFOS	0.2868 ug/mL
..LCM2PFOA 00007	02/12/21	Wellington Laboratories, Lot M2PFOA0216			(Purchased Reagent)		13C2-PFOA	50 ug/mL
..LCMPFOS 00021	12/12/21	Wellington Laboratories, Lot MPFOS1216			(Purchased Reagent)		13C4 PFOS	47.8 ug/mL
.LC537-SU_00049	02/04/18	08/04/17	Methanol, Lot 104453	30000 uL	LCMPFDA 00012	60 uL	13C2 PFDA	0.1 ug/mL
					LCMPFHxA 00013	60 uL	13C2 PFHxA	0.1 ug/mL
..LCMPFDA 00012	09/30/21	Wellington Laboratories, Lot MPFDA0916			(Purchased Reagent)		13C2 PFDA	50 ug/mL
..LCMPFHxA 00013	04/08/21	Wellington Laboratories, Lot MPFHxA0416			(Purchased Reagent)		13C2 PFHxA	50 ug/mL
LC537-L5_00024	02/04/18	08/14/17	MeOH/H2O, Lot 090285	5 mL	LC537-HSP_00025	540 uL	Perfluorobutanesulfonic acid (PFBS)	135.011 ng/mL
							Perfluoroheptanoic acid (PFHpA)	15.0037 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	45.0101 ng/mL
							Perfluorononanoic acid (PFNA)	30.0053 ng/mL
							Perfluorooctanoic acid (PFOA)	30.0251 ng/mL
							Perfluorooctanesulfonic acid (PFOS)	60.0146 ng/mL
					LC537-IS_00048	500 uL	13C2-PFOA	10 ng/mL
							13C4 PFOS	28.68 ng/mL
					LC537-SU_00049	500 uL	13C2 PFDA	10 ng/mL
							13C2 PFHxA	10 ng/mL
.LC537-HSP_00025	02/10/18	08/10/17	Methanol, Lot 141039	20000 uL	LC537SPIM_00023	277.8 uL	Perfluorobutanesulfonic acid (PFBS)	1250.1 ng/mL
							Perfluoroheptanoic acid (PFHpA)	138.923 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	416.76 ng/mL
							Perfluorononanoic acid (PFNA)	277.827 ng/mL
							Perfluorooctanoic acid (PFOA)	278.01 ng/mL
							Perfluorooctanesulfonic acid (PFOS)	555.691 ng/mL
..LC537SPIM_00023	02/10/18	08/10/17	Methanol, Lot 104453	10000 uL	LC537-PFBS_00008	450 uL	Perfluorobutanesulfonic acid (PFBS)	90 ug/mL
					LC537-PFHpA_00015	100 uL	Perfluoroheptanoic acid (PFHpA)	10.0016 ug/mL
					LC537-PFHxS_00010	150 uL	Perfluorohexanesulfonic acid (PFHxS)	30.0043 ug/mL
					LC537-PFNA 00013	200 uL	Perfluorononanoic acid (PFNA)	20.002 ug/mL
					LC537-PFOA 00013	200 uL	Perfluorooctanoic acid (PFOA)	20.0151 ug/mL
					LC537-PFOS_00008	400 uL	Perfluorooctanesulfonic acid (PFOS)	40.0066 ug/mL
...LC537-PFBS_00008	02/10/18	08/10/17	Methanol, Lot 090285	49.6 mL	LC537_PFBS_00002	0.0992 g	Perfluorobutanesulfonic acid (PFBS)	2 mg/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-34917-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
....LC537_PFB_S_00002	04/01/18		Sigma, Lot MKBP8842V		(Purchased Reagent)		Perfluorobutanesulfonic acid (PFBS)	1 g/g
...LC537-PFHpA_00015	02/10/18	08/10/17	Methanol, Lot 090285	48.7 mL	LC537_PFHpA_00002	0.0492 g	Perfluoroheptanoic acid (PFHpA)	1.00016 mg/mL
....LC537_PFHpA_00002	04/01/18		Aldrich, Lot BCBM2579V		(Purchased Reagent)		Perfluoroheptanoic acid (PFHpA)	0.99 g/g
...LC537-PFHxS_00010	02/10/18	08/10/17	Methanol, Lot 090285	55.92 mL	LC537_PFHxS_00002	0.123 g	Perfluorohexanesulfonic acid (PFHxS)	2.00029 mg/mL
....LC537_PFHxS_00002	04/01/18		Sigma, Lot BCBL3545V		(Purchased Reagent)		Perfluorohexanesulfonic acid (PFHxS)	0.9094 g/g
..LC537-PFNA_00013	02/10/18	08/10/17	Methanol, Lot 090285	62.3 mL	LC537_PFNA_00002	0.0647 g	Perfluorononanoic acid (PFNA)	1000.1 ug/mL
....LC537_PFNA_00002	04/01/18		TCI America, Lot QN44F		(Purchased Reagent)		Perfluorononanoic acid (PFNA)	0.963 g/g
..LC537-PFOA_00013	02/10/18	08/10/17	Methanol, Lot 090285	22.76 mL	LC537_PFOA_00003	0.0228 g	Perfluorooctanoic acid (PFOA)	1.00076 mg/mL
....LC537_PFOA_00003	10/31/23		SIGMA ALDRICH, Lot BCBS1198V		(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	0.999 g/g
..LC537-PFOS_00008	02/10/18	08/10/17	Methanol, Lot 090285	44.43 mL	LC537_PFOS_00003	0.0488 g	Perfluorooctanesulfonic acid (PFOS)	1.00016 mg/mL
....LC537_PFOS_00003	04/17/19		sigma alrich, Lot SZBE107XV		(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	0.9106 g/g
.LC537-IS_00048	02/04/18	08/04/17	Methanol, Lot 090285	30000 uL	LCM2PFOA_00007	60 uL	13C2-PFOA	0.1 ug/mL
..LCM2PFOA_00007	02/12/21		Wellington Laboratories, Lot M2PFOA0216		(Purchased Reagent)		13C2-PFOA	50 ug/mL
..LCMPFOS_00021	12/12/21		Wellington Laboratories, Lot MPFOS1216		(Purchased Reagent)		13C4 PFOS	47.8 ug/mL
.LC537-SU_00049	02/04/18	08/04/17	Methanol, Lot 104453	30000 uL	LCMPFDA_00012	60 uL	13C2 PFDA	0.1 ug/mL
..LCMPFDA_00012	09/30/21		Wellington Laboratories, Lot MPFDA0916		(Purchased Reagent)		13C2 PFDA	50 ug/mL
..LCMPFHxA_00013	04/08/21		Wellington Laboratories, Lot MPFHxA0416		(Purchased Reagent)		13C2 PFHxA	50 ug/mL
LC537-L6_00020	02/04/18	08/14/17	MeOH/H2O, Lot 090285	5 mL	LC537-HSP_00025	720 uL	Perfluorobutanesulfonic acid (PFBS)	180.014 ng/mL
							Perfluoroheptanoic acid (PFHpA)	20.0049 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	60.0135 ng/mL
							Perfluorononanoic acid (PFNA)	40.0071 ng/mL
							Perfluorooctanoic acid (PFOA)	40.0334 ng/mL
							Perfluorooctanesulfonic acid (PFOS)	80.0195 ng/mL
.LC537-IS_00048	02/10/18	08/10/17	Methanol, Lot 141039	20000 uL	LC537-IS_00048	500 uL	13C2-PFOA	10 ng/mL
							13C4 PFOS	28.68 ng/mL
							13C2 PFDA	10 ng/mL
.LC537-SU_00049	02/10/18	08/10/17	Methanol, Lot 141039	20000 uL	LC537-SU_00049	500 uL	13C2 PFHxA	10 ng/mL
							Perfluorobutanesulfonic acid (PFBS)	1250.1 ng/mL
							Perfluoroheptanoic acid (PFHpA)	138.923 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	416.76 ng/mL
.LC537-HSP_00025	02/10/18	08/10/17	Methanol, Lot 141039	20000 uL	LC537SPIM_00023	277.8 uL	Perfluorononanoic acid (PFNA)	277.827 ng/mL
							Perfluorooctanoic acid (PFOA)	278.01 ng/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-34917-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
							Perfluorooctanesulfonic acid (PFOS)	555.691 ng/mL
..LC537SPIM_00023	02/10/18	08/10/17	Methanol, Lot 104453	10000 uL	LC537-PFBS_00008	450 uL	Perfluorobutanesulfonic acid (PFBS)	90 ug/mL
					LC537-PFHpA_00015	100 uL	Perfluoroheptanoic acid (PFHpA)	10.0016 ug/mL
					LC537-PFHxS_00010	150 uL	Perfluorohexanesulfonic acid (PFHxS)	30.0043 ug/mL
					LC537-PFNA_00013	200 uL	Perfluorononanoic acid (PFNA)	20.002 ug/mL
					LC537-PFOA_00013	200 uL	Perfluorooctanoic acid (PFOA)	20.0151 ug/mL
					LC537-PFOS_00008	400 uL	Perfluorooctanesulfonic acid (PFOS)	40.0066 ug/mL
...LC537-PFBS_00008	02/10/18	08/10/17	Methanol, Lot 090285	49.6 mL	LC537_PFBS_00002	0.0992 g	Perfluorobutanesulfonic acid (PFBS)	2 mg/mL
....LC537_PFBS_00002	04/01/18		Sigma, Lot MKBP8842V		(Purchased Reagent)		Perfluorobutanesulfonic acid (PFBS)	1 g/g
...LC537-PFHpA_00015	02/10/18	08/10/17	Methanol, Lot 090285	48.7 mL	LC537_PFHpA_00002	0.0492 g	Perfluoroheptanoic acid (PFHpA)	1.00016 mg/mL
....LC537_PFHpA_00002	04/01/18		Aldrich, Lot BCBM2579V		(Purchased Reagent)		Perfluoroheptanoic acid (PFHpA)	0.99 g/g
...LC537-PFHxS_00010	02/10/18	08/10/17	Methanol, Lot 090285	55.92 mL	LC537_PFHxS_00002	0.123 g	Perfluorohexanesulfonic acid (PFHxS)	2.00029 mg/mL
....LC537_PFHxS_00002	04/01/18		Sigma, Lot BCBL3545V		(Purchased Reagent)		Perfluorohexanesulfonic acid (PFHxS)	0.9094 g/g
...LC537-PFNA_00013	02/10/18	08/10/17	Methanol, Lot 090285	62.3 mL	LC537 PFNA_00002	0.0647 g	Perfluorononanoic acid (PFNA)	1000.1 ug/mL
....LC537 PFNA_00002	04/01/18		TCI America, Lot QN44F		(Purchased Reagent)		Perfluorononanoic acid (PFNA)	0.963 g/g
...LC537-PFOA_00013	02/10/18	08/10/17	Methanol, Lot 090285	22.76 mL	LC537 PFOA_00003	0.0228 g	Perfluorooctanoic acid (PFOA)	1.00076 mg/mL
....LC537 PFOA_00003	10/31/23		SIGMA ALDRICH, Lot BCBS1198V		(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	0.999 g/g
...LC537-PFOS_00008	02/10/18	08/10/17	Methanol, Lot 090285	44.43 mL	LC537_PFOS_00003	0.0488 g	Perfluorooctanesulfonic acid (PFOS)	1.00016 mg/mL
....LC537_PFOS_00003	04/17/19		sigma alrich, Lot SZBE107XV		(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	0.9106 g/g
.LC537-IS_00048	02/04/18	08/04/17	Methanol, Lot 090285	30000 uL	LCM2PFOA_00007	60 uL	13C2-PFOA	0.1 ug/mL
					LCMPFOS_00021	180 uL	13C4 PFOS	0.2868 ug/mL
..LCM2PFOA_00007	02/12/21		Wellington Laboratories, Lot M2PFOA0216		(Purchased Reagent)		13C2-PFOA	50 ug/mL
..LCMPFOS_00021	12/12/21		Wellington Laboratories, Lot MPFOS1216		(Purchased Reagent)		13C4 PFOS	47.8 ug/mL
.LC537-SU_00049	02/04/18	08/04/17	Methanol, Lot 104453	30000 uL	LCMPFDA_00012	60 uL	13C2 PFDA	0.1 ug/mL
					LCMPFHxA_00013	60 uL	13C2 PFHxA	0.1 ug/mL
..LCMPFDA_00012	09/30/21		Wellington Laboratories, Lot MPFDA0916		(Purchased Reagent)		13C2 PFDA	50 ug/mL
..LCMPFHxA_00013	04/08/21		Wellington Laboratories, Lot MPFHxA0416		(Purchased Reagent)		13C2 PFHxA	50 ug/mL
LC537-LSP_00025	02/10/18	08/10/17	Methanol, Lot 090285	20000 uL	LC537SPIM_00023	50 uL	Perfluorobutane Sulfonate	225 ng/mL
							Perfluorobutanesulfonic acid (PFBS)	225 ng/mL
							Perfluoroheptanoic acid (PFHpA)	25.0041 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	75.0109 ng/mL
							Perfluorononanoic acid (PFNA)	50.0049 ng/mL
							Perfluorooctanoic acid (PFOA)	50.0378 ng/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-34917-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
							Perfluorooctanesulfonic acid (PFOS)	100.016 ng/mL
.LC537SPIM_00023	02/10/18	08/10/17	Methanol, Lot 104453	10000 uL	LC537-PFBS_00008	450 uL	Perfluorobutane Sulfonate	90 ug/mL
							Perfluorobutanesulfonic acid (PFBS)	90 ug/mL
					LC537-PFHpA_00015	100 uL	Perfluoroheptanoic acid (PFHpA)	10.0016 ug/mL
					LC537-PFHxS_00010	150 uL	Perfluorohexanesulfonic acid (PFHxS)	30.0043 ug/mL
					LC537-PFNA_00013	200 uL	Perfluorononanoic acid (PFNA)	20.002 ug/mL
					LC537-PFOA_00013	200 uL	Perfluorooctanoic acid (PFOA)	20.0151 ug/mL
					LC537-PFOS_00008	400 uL	Perfluorooctanesulfonic acid (PFOS)	40.0066 ug/mL
..LC537-PFBS_00008	02/10/18	08/10/17	Methanol, Lot 090285	49.6 mL	LC537_PFBS_00002	0.0992 g	Perfluorobutane Sulfonate	2 mg/mL
							Perfluorobutanesulfonic acid (PFBS)	2 mg/mL
...LC537_PFBS_00002	04/01/18	Sigma, Lot MKBP8842V			(Purchased Reagent)		Perfluorobutane Sulfonate	1 g/g
							Perfluorobutanesulfonic acid (PFBS)	1 g/g
..LC537-PFHpA_00015	02/10/18	08/10/17	Methanol, Lot 090285	48.7 mL	LC537_PFHpA_00002	0.0492 g	Perfluoroheptanoic acid (PFHpA)	1.00016 mg/mL
...LC537_PFHpA_00002	04/01/18	Aldrich, Lot BCM2579V			(Purchased Reagent)		Perfluoroheptanoic acid (PFHpA)	0.99 g/g
..LC537-PFHxS_00010	02/10/18	08/10/17	Methanol, Lot 090285	55.92 mL	LC537_PFHxS_00002	0.123 g	Perfluorohexanesulfonic acid (PFHxS)	2.00029 mg/mL
...LC537_PFHxS_00002	04/01/18	Sigma, Lot BCBL3545V			(Purchased Reagent)		Perfluorohexanesulfonic acid (PFHxS)	0.9094 g/g
..LC537-PFNA_00013	02/10/18	08/10/17	Methanol, Lot 090285	62.3 mL	LC537 PFNA_00002	0.0647 g	Perfluorononanoic acid (PFNA)	1000.1 ug/mL
..LC537 PFNA_00002	04/01/18	TCI America, Lot QN44F			(Purchased Reagent)		Perfluorononanoic acid (PFNA)	0.963 g/g
..LC537-PFOA_00013	02/10/18	08/10/17	Methanol, Lot 090285	22.76 mL	LC537 PFOA_00003	0.0228 g	Perfluorooctanoic acid (PFOA)	1.00076 mg/mL
..LC537 PFOA_00003	10/31/23	SIGMA ALDRICH, Lot BCBS1198V			(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	0.999 g/g
..LC537-PFOS_00008	02/10/18	08/10/17	Methanol, Lot 090285	44.43 mL	LC537_PFOS_00003	0.0488 g	Perfluorooctanesulfonic acid (PFOS)	1.00016 mg/mL
...LC537_PFOS_00003	04/17/19	sigma alrich, Lot SZBE107XV			(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	0.9106 g/g
LC537-SU_00054	05/27/18	11/27/17	Methanol, Lot 104453	30000 uL	LCMPFDA_00012	60 uL	13C2 PFDA	0.1 ug/mL
					LCMPFHxA_00015	60 uL	13C2 PFHxA	0.1 ug/mL
.LCMPFDA_00012	09/30/21	Wellington Laboratories, Lot MPFDA0916			(Purchased Reagent)		13C2 PFDA	50 ug/mL
.LCMPFHxA_00015	11/22/21	Wellington Laboratories, Lot MPFHxA1116			(Purchased Reagent)		13C2 PFHxA	50 ug/mL

Reagent

LC537_PFB_00002


#: 4/1/15 SPV

3050 Spruce Street, Saint Louis, MO 63103, USA
Website: www.sigmaaldrich.com
Email USA: techserv@sial.com
Outside USA: eurtechserv@sial.com

Certificate of Analysis

Product Name:
Nonafluorobutane-1-sulfonic acid - 97%

Product Number: 562629
Batch Number: MKBP8842V
Brand: ALDRICH
CAS Number: 375-73-5
MDL Number: MFCD01320794
Formula: C4HF9O3S
Formula Weight: 300.10 g/mol
Storage Temperature: Store at 2 - 8 °C
Quality Release Date: 11 OCT 2013



PFBS

Test	Specification	Result
Appearance (Color)	Colorless	Colorless
Appearance (Form)	Liquid	Liquid
Infrared Spectrum	Conforms to Structure	Conforms
Fluorine NMR Spectrum	Conforms to Structure	Conforms
Purity (Titration by NaOH)	96.5 - 103.5 %	101.6 %

Jamie Gleason


Jamie Gleason, Manager
Quality Control
Milwaukee, Wisconsin US

Sigma-Aldrich warrants, that at the time of the quality release or subsequent retest date this product conformed to the information contained in this publication. The current Specification sheet may be available at Sigma-Aldrich.com. For further inquiries, please contact Technical Service. Purchaser must determine the suitability of the product for its particular use. See reverse side of invoice or packing slip for additional terms and conditions of sale.

Reagent

LC537_PFB2_00002

F: 6.8.17 SW



CERTIFICATE OF ANALYSIS

The Power to Question

Catalog Number: sc-236187
Lot Number: F0917
Product Name: Nonafluorobutane-1-sulfonic acid
CAS Number: 375-73-5
Molecular Formula: $C_4HF_9O_3S$
Molecular Weight: 300.10

Test	Specification	Result
Appearance	Colorless liquid	Complies
Identification (19F-NMR)	Conforms to structure	Complies
Purity (Sodium Hydroxide Titration)	$\geq 97\%$	101.3%
Infrared Spectrum	Conforms to structure	Complies

Reagent

LC537_PFHpA_00002

R: 4/1/15 4V

Certificate of Analysis

Product Name: PERFLUOROHEPTANOIC ACID
 99 %
Product Number: 342041
Batch Number: BCBM2579V
Brand: Aldrich
CAS Number: 375-85-9
Formula: $CF_3(CF_2)_5CO_2H$
Formula Weight: 364.06
Quality Release Date: 06 DEC 2013
Recommended Retest Date: OCT 2018

PFHpA

TEST	SPECIFICATION	RESULT
APPEARANCE (COLOR)	COLORLESS OR WHITE	WHITE
APPEARANCE (FORM)	LIQUID OR SOLID	SOLID
TITRATION	98.5 - 101.5 %	99.8 %
TITRATION (METHOD)	-	BACK TITRATION
PURITY (GC AREA %)	≥ 98.5 %	99.5 %
INFRARED SPECTRUM	CONFORMS TO STRUCTURE	CONFORMS

Dr. Claudia Geitner
Manager Quality Control
Buchs, Switzerland

Sigma-Aldrich warrants that at the time of the quality release or subsequent retest date this product conformed to the information contained in this publication. The current specification sheet may be available at Sigma-Aldrich.com. For further inquiries, please contact Technical Service. Purchaser must determine the suitability of the product for its particular use. See reverse side of invoice or packing slip for additional terms and conditions of sale.

Reagent

LC537_PFHpA2_00002

Certificate of analysis

r:6.13.17 SW

Product No.: A12092
Product: Perfluoroheptanoic acid, 98+%
Lot No.: 10200390

PFHe A

Appearance: White fused solid
Water Content (Karl-Fischer): 0.30%
Melting Point: 32.0-34.3°C
Assay (Aqueous acid-base titration): 99.7%
Identification (FTIR): Conforms

This document has been electronically generated and does not require a signature.

Order our products online www.alfa.com

ThermoFisher
SCIENTIFIC

Reagent

LC537_PFHxS_00002

r: 4/1/15 stw

Certificate of Analysis

Product Name: TRIDECAFLUOROHEXANE-1-SULFONIC ACID POTASSIUM SALT
 >= 98.0 % T

Product Number: 50929

Batch Number: BCBL3545V

Brand: Aldrich

CAS Number: 3871-99-6

Formula: C₆F₁₃KO₃S

Formula Weight: 438.20

Quality Release Date: 20 JUN 2013

PFH₁₃S-K

TEST	SPECIFICATION	RESULT
APPEARANCE (COLOR)	WHITE TO FAINT BEIGE	WHITE
APPEARANCE (FORM)	POWDER OR CRYSTALS	POWDER
TITRATION (ION EXCHANGE)	≥ 98.0 %	99.5 %
INFRARED SPECTRUM	CONFORMS TO STRUCTURE	CONFORMS

Dr. Claudia Geitner
Manager Quality Control
Buchs, Switzerland

$$MW_{corr} = \frac{(k_{form}) - (k) + (H)}{438.20 (k_{form})} = \frac{(438.20 - 3910 + 101)}{438.20 (k_{form})} = 0.91307 \text{ (anion form)}$$

$$Purity = 90.94 \% \text{ w/m.w correction}$$

stw 4/1/15

Sigma-Aldrich warrants that at the time of the quality release or subsequent retest date this product conformed to the information contained in this publication. The current specification sheet may be available at Sigma-Aldrich.com. For further inquiries, please contact Technical Service. Purchaser must determine the suitability of the product for its particular use. See reverse side of invoice or packing slip for additional terms and conditions of sale.

Reagent

LC537_PFHxS2_00002

n: 6-8-17 SKJ




The Future of Science

CERTIFICATE OF ANALYSIS

Catalog Number: sc-237289
 Lot Number: G2516
 Product Name: Tridecafluorohexane-1-sulfonic acid potassium salt
 CAS Number: 3871-99-6
 Molecular Formula: $C_6F_{13}KO_3S$
 Molecular Weight: 438.20

Test	Specification	Result
Appearance	White to faint beige powder or crystals	White powder
Identification (Infrared Spectrum)	Consistent with structure	Complies
Purity (Titration, Ion Exchange)	≥ 98.0%	100.4%



MW correction = $\frac{400.11}{438.201} = 0.91307$ PFH₁₃S
 CAS# 355-46-4

Purity $\frac{1}{9}$ MW correction = 90.9%

This document was produced electronically and is valid without a signature.

Reagent

LC537_PENA_00002

R: 4/1/15 SKV



Certificate of Analysis

Apr 2, 2015 (JST)

TOKYO CHEMICAL INDUSTRY CO.,LTD.
4-10-1 Nihonbashi-Honcho, Chuo-ku, Tokyo 103-0023 Japan

Chemical Name: Heptadecafluorononanoic Acid		
Product Number: H0843 CAS: 375-95-1	Lot: QN44F	

Tests	Results	Specifications
Purity(GC)	96.3 %	min. 95.0 %
Purity(Neutralization titration)	98.1 %	min. 95.0 %
Melting point	63.3 deg-C	62.0 to 67.0 deg-C

TCI Lot numbers are 4-5 characters in length.
Characters listed after the first 4-5 characters are control numbers for internal purpose only.

Customer service:

TCI AMERICA
Tel: +1-800-423-8616 / +1-503-283-1681
Fax: +1-888-520-1075 / +1-503-283-1987
E-mail: Sales-US@TCIchemicals.com

PFNA

Reagent

LC537_PFN2_00002

P: 6.14.17 SKW

3050 Spruce Street, Saint Louis, MO 63103, USA

Website: www.sigmaaldrich.com


Email USA: techserv@sial.com

Outside USA: eurtechserv@sial.com

Certificate of Analysis

Product Name:
Perfluorononanoic acid - 97%

Product Number: 394459
Batch Number: MKCC0699
Brand: ALDRICH
CAS Number: 375-95-1
MDL Number: MFCD00039605
Formula: C9HF17O2
Formula Weight: 464.08 g/mol
Quality Release Date: 07 DEC 2016



Test	Specification	Result
Appearance (Color)	White to Off-White	White
Appearance (Form)	Powder or Crystals or Crystalline Chunk(s) or Granule or Flakes or Solid	Powder
Infrared Spectrum	Conforms to Structure	Conforms
GC (area %)	≥ 96.5 %	98.2 %

Michael Grady, Manager
Quality Control
Milwaukee, WI US

PFNA

Sigma-Aldrich warrants, that at the time of the quality release or subsequent retest date this product conformed to the information contained in this publication. The current Specification sheet may be available at Sigma-Aldrich.com. For further inquiries, please contact Technical Service. Purchaser must determine the suitability of the product for its particular use. See reverse side of Invoice or packing slip for additional terms and conditions of sale.

Reagent

LC537_PFOA_00003

T: 11/30/16 SKV
PFA

SIGMA-ALDRICH

3050 Spruce Street, Saint Louis, MO 63103 USA
Email USA: techserv@sial.com Outside USA: eurtechserv@sial.com

Certificate of Analysis

Product Name: PENTADECAFLUOROOCCTANOIC ACID
analytical standard
Product Number: 33824
Batch Number: BCBS1198V
Brand: Sigma-Aldrich
CAS Number: 335-67-1
Formula: $\text{CF}_3(\text{CF}_2)_6\text{COOH}$
Formula Weight: 414.07
Expiration Date: OCT 2023
Quality Release Date: 12 MAY 2016

TEST	SPECIFICATION	RESULT
PURITY (HPLC AREA %)	≥ 98.0%	100.0%
IDENTIFICATION (LC-MS)	IDENTITY CONFORMS	CONFORMS



Dr. Claudia Geitner
Manager Quality Control
Buchs, Switzerland

Sigma-Aldrich warrants that at the time of the quality release or subsequent retest date this product conformed to the information contained in this publication. The current specification sheet may be available at Sigma-Aldrich.com. For further inquiries, please contact Technical Service. Purchaser must determine the suitability of the product for its particular use. See reverse side of invoice or packing slip for additional terms and conditions of sale.

Reagent

LC537_PFOA2_00002

Certificate of analysis

P: 6/21/17 SW ✓

Product No.: L08862
Product: Perfluorooctanoic acid, 95%
Lot No.: 10199078

PFOA

Appearance: White powder
Water Content (Karl-Fischer): 1.30%
Melting Point: 47.6-54.0°C
Assay (Aqueous acid-base titration): 98.4%
Assay (GC Silyl Deriv): 97.2%

This document has been electronically generated and does not require a signature.

Order our products online www.alfa.com

ThermoFisher
SCIENTIFIC

Reagent

LC537_PFOs_00003

Reagent

LC537_PFOs2_00002

R: 6.14.17 SKV

Certificate of Analysis

Product Name: HEPTADEC AFLUORO OCTANESULFONIC ACID TETRAETHYLAMMONIUM SALT
98 %

Product Number: 365289

Batch Number: BCBQ0108V

Brand: Aldrich

CAS Number: 56773-42-3

Formula: $CF_3(CF_2)_6CF_2SO_3N(C_2H_5)_4$

Formula Weight: 629.37


Quality Release Date: 11 JUN 2015

TEST	SPECIFICATION	RESULT
APPEARANCE (COLOR)	WHITE TO OFF WHITE	OFF-WHITE
APPEARANCE (FORM)	POWDER OR POWDER WITH CHUNK(S)	POWDER
CARBON CONTENT	29.77 % - 31.29 %	29.97 %
INFRARED SPECTRUM	CONFORMS TO STRUCTURE	CONFORMS

Dr. Claudia Geitner
Manager Quality Control
Buchs, Switzerland

MW correction: $\frac{500.125}{629.37} = 0.7946$

Purity & MW correction = 77.37%



	$C_8 F_{17} SO_3^+ H$	$C_8 H_{20} N$
C = 12.011	96.088	96.088
F = 18.998	322.966	—
S = 32.066	32.066	—
O = 16.999	47.997	20.60
H = 1.008	1.008	14.007
N = 14.007	—	—
	<hr/>	<hr/>
	500.125	130.255

Reagent

LCM2PFOA_00007

P: 5/11/17 SKV




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: M2PFOA
COMPOUND: Perfluoro-n-[1,2-¹³C₂]octanoic acid

LOT NUMBER: M2PFOA0216

STRUCTURE: **CAS #:** Not available

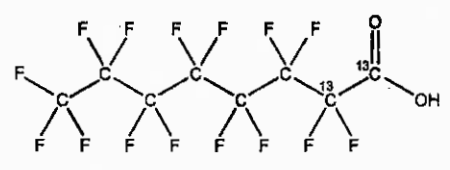

MOLECULAR FORMULA: ¹³C₂¹²C₆HF₁₆O₂
CONCENTRATION: 50 ± 2.5 µg/ml

MOLECULAR WEIGHT: 416.05
SOLVENT(S): Methanol
Water (<1%)

CHEMICAL PURITY: >98%
LAST TESTED: (mm/dd/yyyy) 02/12/2016
EXPIRY DATE: (mm/dd/yyyy) 02/12/2021

ISOTOPIC PURITY: ≥99%¹³C
(1,2-¹³C₂)

RECOMMENDED STORAGE: Store ampoule in a cool, dark place

DOCUMENTATION/ DATA ATTACHED:

- Figure 1: LC/MS Data (TIC and Mass Spectrum)
- Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent conversion of the carboxylic acid to the methyl ester.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: 
B.G. Chittim

Date: 02/24/2016
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:


Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: M2PFOA; LC/MS Data (TIC and Mass Spectrum)



Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm


Mobile phase: Gradient
Start: 50% (80:20 MeOH:ACN) / 50% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 90% organic over 7.5 min and hold for 1.5 min
before returning to initial conditions in 0.5 min.
Time: 10 min

Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (150 - 850 amu)
Source: Electrospray (negative)
Capillary Voltage (kV) = 3.00
Cone Voltage (V) = 15.00
Cone Gas Flow (l/hr) = 100
Desolvation Gas Flow (l/hr) = 750

Figure 2: M2PFOA; LC/MS/MS Data (Selected MRM Transitions)

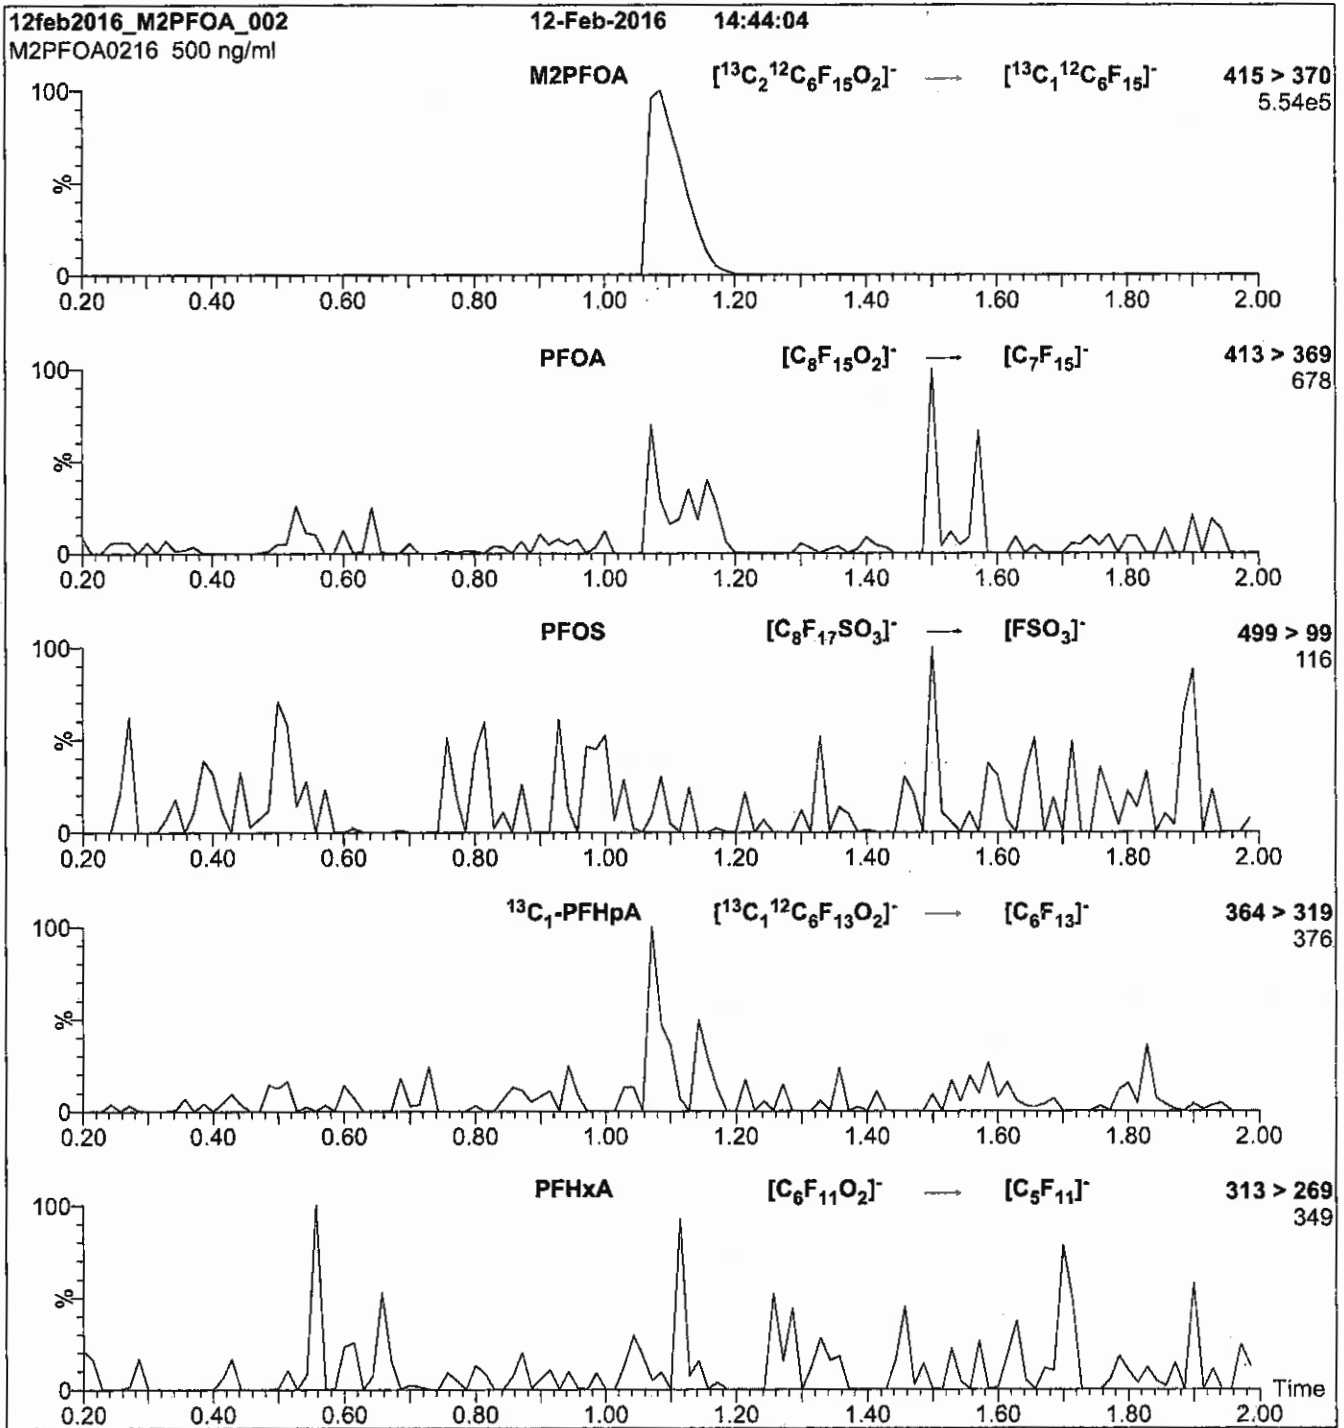

Conditions for Figure 2:

Injection: Direct loop injection
10 μl (500 ng/ml M2PFOA)

Mobile phase: Isocratic 80% MeOH / 20% H_2O

Flow: 300 $\mu\text{l}/\text{min}$

MS Parameters

Collision Gas (mbar) = 3.39e-3
Collision Energy (eV) = 10

Reagent

LCMPFDA_00012

R: SBC 12/21/16



814255

ID: LCMPPFDA_00012

Exp: 09/30/21 Prpd: SBC

13C2-Perfluorodecanoic a




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: MPFDA **LOT NUMBER:** MPFDA0916
COMPOUND: Perfluoro-n-[1,2-¹³C₂]decanoic acid

STRUCTURE: **CAS #:** Not available



MOLECULAR FORMULA: ¹³C₂¹²C₈HF₁₉O₂ **MOLECULAR WEIGHT:** 516.07
CONCENTRATION: 50 ± 2.5 µg/ml **SOLVENT(S):** Methanol
Water (<1%)
CHEMICAL PURITY: >98% **ISOTOPIC PURITY:** ≥99% ¹³C
(1,2-¹³C₂)
LAST TESTED: (mm/dd/yyyy) 09/30/2016
EXPIRY DATE: (mm/dd/yyyy) 09/30/2021
RECOMMENDED STORAGE: Store ampoule in a cool, dark place


DOCUMENTATION/ DATA ATTACHED:

Figure 1: LC/MS Data (TIC and Mass Spectrum)
Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent conversion of the carboxylic acid to the methyl ester.
- Contains < 0.1% of ¹³C₁-PFNA.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: 
B.G. Chríttim **Date:** 10/07/2016
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: MPFDA; LC/MS Data (TIC and Mass Spectrum)



Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions


Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm
Mobile phase: Gradient
Start: 50% (80:20 MeOH:ACN) / 50% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 90% organic over 7 min and hold for 1.5 min
before returning to initial conditions in 0.5 min.
Time: 10 min

Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (225 - 850 amu)
Source: Electrospray (negative)
Capillary Voltage (kV) = 2.00
Cone Voltage (V) = 15.00
Cone Gas Flow (l/hr) = 50
Desolvation Gas Flow (l/hr) = 750

Figure 2: MPFDA; LC/MS/MS Data (Selected MRM Transitions)



Conditions for Figure 2:

Injection: Direct loop injection
10 μ l (500 ng/ml MPFDA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
(both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.31e-3
Collision Energy (eV) = 13

Reagent

LCMPFHxA_00013

R: SBC 12/21/16



814258
ID: LCMPFHxA_00013
Exp: 04/08/21 Ppdt. SBC
13C2-Perfluorohexanoic ac



WELLINGTON LABORATORIES


CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: MPFHxA
COMPOUND: Perfluoro-n-[1,2-¹³C₂]hexanoic acid

LOT NUMBER: MPFHxA0416

STRUCTURE:

CAS #: Not available



MOLECULAR FORMULA: ¹³C₂¹²C₄HF₁₁O₂
CONCENTRATION: 50 ± 2.5 µg/ml

MOLECULAR WEIGHT: 316.04
SOLVENT(S): Methanol
Water (<1%)

CHEMICAL PURITY: >98%
LAST TESTED: (mm/dd/yyyy) 04/08/2016

ISOTOPIC PURITY: ≥99%¹³C
(1,2-¹³C₂)

EXPIRY DATE: (mm/dd/yyyy) 04/08/2021

RECOMMENDED STORAGE: Store ampoule in a cool, dark place

DOCUMENTATION/ DATA ATTACHED:

- Figure 1: LC/MS Data (TIC and Mass Spectrum)
- Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent conversion of the carboxylic acid to the methyl ester.
- Contains < 0.1% of perfluoro-n-hexanoic acid and ~ 0.3% of perfluoro-n-octanoic acid.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By:
B.G. Chittim

Date: 04/29/2016
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: MPFHxA; LC/MS Data (TIC and Mass Spectrum)



Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
 1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
 Start: 50% (80:20 MeOH:ACN) / 50% H₂O
 (both with 10 mM NH₄OAc buffer)
 Ramp to 90% organic over 7.5 min and hold for 1.5 min
 before returning to initial conditions over 0.5 min.
 Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (150 - 850 amu)

Source: Electrospray (negative)
 Capillary Voltage (kV) = 2.00
 Cone Voltage (V) = 15.00
 Cone Gas Flow (l/hr) = 100
 Desolvation Gas Flow (l/hr) = 750

Figure 2: MPFHxA; LC/MS/MS Data (Selected MRM Transitions)



Conditions for Figure 2:

Injection: Direct loop injection
10 μ l (500 ng/ml MPFHxA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
(both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.39e-3
Collision Energy (eV) = 10

Reagent

LCMPFHxA_00015

r: 5/10/17 skd




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: MPFHxA
COMPOUND: Perfluoro-n-[1,2-¹³C₂]hexanoic acid

LOT NUMBER: MPFHxA1116

STRUCTURE: **CAS #:** Not available



MOLECULAR FORMULA: ¹³C₂¹²C₄HF₁₁O₂
CONCENTRATION: 50 ± 2.5 µg/ml

MOLECULAR WEIGHT: 316.04
SOLVENT(S): Methanol
Water (<1%)

CHEMICAL PURITY: >98%

ISOTOPIC PURITY: ≥99% ¹³C
(1,2-¹³C₂)

LAST TESTED: (mm/dd/yyyy) 11/22/2016

EXPIRY DATE: (mm/dd/yyyy) 11/22/2021

RECOMMENDED STORAGE: Store ampoule in a cool, dark place

DOCUMENTATION/ DATA ATTACHED:

- Figure 1: LC/MS Data (TIC and Mass Spectrum)
- Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent conversion of the carboxylic acid to the methyl ester.
- Contains < 0.1% of perfluoro-n-hexanoic acid and ~ 0.3% of perfluoro-n-octanoic acid.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: 
B.G. Chittim

Date: 12/13/2016
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:


Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: MPFHxA; LC/MS Data (TIC and Mass Spectrum)



Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm


Mobile phase: Gradient
Start: 40% (80:20 MeOH:ACN) / 60% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 90% organic over 7 min and hold for 2 min
before returning to initial conditions over 0.5 min.
Time: 10 min

Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (150 - 850 amu)
Source: Electrospray (negative)
Capillary Voltage (kV) = 2.00
Cone Voltage (V) = 15.00
Cone Gas Flow (l/hr) = 100
Desolvation Gas Flow (l/hr) = 750

Figure 2: MPFHxA; LC/MS/MS Data (Selected MRM Transitions)



Conditions for Figure 2:

Injection: Direct loop injection
10 μl (500 ng/ml MPFHxA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H_2O
(both with 10 mM NH_4OAc buffer)

Flow: 300 $\mu\text{l}/\text{min}$

MS Parameters

Collision Gas (mbar) = $3.46\text{e-}3$
Collision Energy (eV) = 10

Reagent

LCMPFOS_00019

R: SBC 12/21/16



814253
ID: LCMPFOS_00019
Exp: 08/03/21 Ppfd: SBC
13C4-Perfluorooctanesulfo




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: MPFOS **LOT NUMBER:** MPFOS0816
COMPOUND: Sodium perfluoro-1-[1,2,3,4-¹³C₄]octanesulfonate

STRUCTURE: **CAS #:** Not available



MOLECULAR FORMULA: ¹³C₄¹²C₄F₁₇SO₃Na **MOLECULAR WEIGHT:** 526.08
CONCENTRATION: 50.0 ± 2.5 µg/ml (Na salt) **SOLVENT(S):** Methanol
47.8 ± 2.4 µg/ml (MPFOS anion)
CHEMICAL PURITY: >98% **ISOTOPIC PURITY:** ≥99% ¹³C
LAST TESTED: (mm/dd/yyyy) 08/03/2016 (1,2,3,4-¹³C₄)
EXPIRY DATE: (mm/dd/yyyy) 08/03/2021
RECOMMENDED STORAGE: Store ampoule in a cool, dark place


DOCUMENTATION/ DATA ATTACHED:

Figure 1: LC/MS Data (TIC and Mass Spectrum)
Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains ~ 0.8% Sodium perfluoro-1-[1,2,3-¹³C₃]heptanesulfonate.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: 
B.G. Chittim **Date:** 08/05/2016
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:


Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: MPFOS; LC/MS Data (TIC and Mass Spectrum)



Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
 1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
 Start: 45% (80:20 MeOH:ACN) / 55% H₂O
 (both with 10 mM NH₄OAc buffer)
 Ramp to 90% organic over 7 min and hold for 1.5 min
 before returning to initial conditions in 0.5 min.
 Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (225 - 850 amu)

Source: Electrospray (negative)
 Capillary Voltage (kV) = 3.00
 Cone Voltage (V) = 60.00
 Cone Gas Flow (l/hr) = 50
 Desolvation Gas Flow (l/hr) = 750

Figure 2: MPFOS; LC/MS/MS Data (Selected MRM Transitions)



Conditions for Figure 2:

Injection: Direct loop injection
10 μl (500 ng/ml MPFOS)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H_2O
(both with 10 mM NH_4OAc buffer)

Flow: 300 $\mu\text{l}/\text{min}$

MS Parameters

Collision Gas (mbar) = 3.46e-3
Collision Energy (eV) = 40

Reagent

LCMPFOS_00021

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:


Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: MPFOS; LC/MS Data (TIC and Mass Spectrum)



Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
 1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
 Start: 50% (80:20 MeOH:ACN) / 50% H₂O
 (both with 10 mM NH₄OAc buffer)
 Ramp to 85% organic over 7.5 min and hold for 1.5 min
 before returning to initial conditions in 0.5 min.
 Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (150 - 850 amu)

Source: Electrospray (negative)
 Capillary Voltage (kV) = 3.00
 Cone Voltage (V) = 60.00
 Cone Gas Flow (l/hr) = 50
 Desolvation Gas Flow (l/hr) = 750

Figure 2: MPFOS; LC/MS/MS Data (Selected MRM Transitions)



Conditions for Figure 2:

Injection: Direct loop injection
10 μl (500 ng/ml MPFOS)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H_2O
(both with 10 mM NH_4OAc buffer)

Flow: 300 $\mu\text{l}/\text{min}$

MS Parameters

Collision Gas (mbar) = 3.35e-3
Collision Energy (eV) = 40

Method 537 DOD

Perfluorinated Alkyl Acids (LC/MS)
by Method 537 DOD

FORM II
LCMS SURROGATE RECOVERY

Lab Name: TestAmerica Sacramento

Job No.: 320-34917-1

SDG No.: _____

Matrix: Water

Level: Low

GC Column (1): GeminiC18 3 ID: 3 (mm)

Client Sample ID	Lab Sample ID	PFHxA #	PFDA #
WGNA-010818-RW-034 4	320-34917-1	91	93
WGNA-010818-FRB-03 44	320-34917-2	97	98
WGNA-010818-RW-395 7	320-34917-3	91	104
WGNA-010818-FRB-39 57	320-34917-4	96	98
WGNA-010818-DUP-16	320-34917-5	96	109
WGNA-010818-RW-317 8	320-34917-6	90	102
WGNA-010818-FRB-31 78	320-34917-7	98	103
NAWC-010818-RW-141	320-34917-8	88	96
NAWC-010818-FRB-14 1	320-34917-9	95	99
WGNA-010818-RW-402 4	320-34917-10	71	93
WGNA-010818-FRB-40 24	320-34917-11	98	100
WGNA-010818-RW-484 4	320-34917-12	97	98
WGNA-010818-FRB-48 44	320-34917-13	97	97
WGNA-010818-RW-040 4	320-34917-14	96	100
WGNA-010818-FRB-04 04	320-34917-15	103	103
	MB 320-204304/1-A	86	96
	LLCS 320-204304/2-A	97	103
WGNA-010818-RW-402 4 LMS	320-34917-10 LMS	88	95
WGNA-010818-RW-402 4 LMSD	320-34917-10 LMSD	90	97

PFHxA = 13C2 PFHxA
PFDA = 13C2 PFDA

QC LIMITS
70-130
70-130

Column to be used to flag recovery values

FORM III
LCMS LOW LEVEL CONTROL SAMPLE RECOVERY

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1

SDG No.: _____

Matrix: Water Level: Low Lab File ID: 2018.01.20_537AA_008.d

Lab ID: LLCS 320-204304/2-A Client ID: _____

COMPOUND	SPIKE ADDED (ng/L)	LLCS CONCENTRATION (ng/L)	LLCS % REC	QC LIMITS REC	#
Perfluorooctanesulfonic acid (PFOS)	40.0	39.2 J	98	50-150	
Perfluorooctanoic acid (PFOA)	20.0	20.1	100	50-150	
Perfluorononanoic acid (PFNA)	20.0	19.7 J	98	50-150	
Perfluorohexanesulfonic acid (PFHxS)	30.0	30.9	103	50-150	
Perfluoroheptanoic acid (PFHpA)	10.0	10.4	104	50-150	
Perfluorobutanesulfonic acid (PFBS)	90.0	85.8 J	95	50-150	

Column to be used to flag recovery and RPD values

FORM III
LCMS LOW LEVEL MATRIX SPIKE RECOVERY

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Matrix: Water Level: Low Lab File ID: 2018.01.23537A_009.d
 Lab ID: 320-34917-10 LMS Client ID: WGNA-010818-RW-4024 LMS

COMPOUND	SPIKE ADDED (ng/L)	SAMPLE CONCENTRATION (ng/L)	LMS CONCENTRATION (ng/L)	LMS % REC	QC LIMITS REC	#
Perfluorooctanesulfonic acid (PFOS)	40.2	18 J	58.5	102	50-150	M
Perfluorooctanoic acid (PFOA)	20.1	12 J	31.9	99	50-150	
Perfluorononanoic acid (PFNA)	20.1	20 U	22.9 J	114	50-150	
Perfluorohexanesulfonic acid (PFHxS)	30.1	12 U	36.4	121	50-150	
Perfluoroheptanoic acid (PFHpA)	10.0	3.6 J	14.4	108	50-150	
Perfluorobutanesulfonic acid (PFBS)	90.3	36 U	95.9	106	50-150	

Column to be used to flag recovery and RPD values

FORM III
LCMS LOW LEVEL MATRIX SPIKE DUPLICATE RECOVERY

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Matrix: Water Level: Low Lab File ID: 2018.01.23537A_010.d
 Lab ID: 320-34917-10 LMSD Client ID: WGNA-010818-RW-4024 LMSD

COMPOUND	SPIKE ADDED (ng/L)	LMSD CONCENTRATION (ng/L)	LMSD % REC	% RPD	QC LIMITS		#
					RPD	REC	
Perfluorooctanesulfonic acid (PFOS)	38.8	56.7	101	3	50	50-150	M
Perfluorooctanoic acid (PFOA)	19.4	32.3	105	1	50	50-150	
Perfluorononanoic acid (PFNA)	19.4	21.5 J	111	6	50	50-150	
Perfluorohexanesulfonic acid (PFHxS)	29.1	33.8	116	7	50	50-150	
Perfluoroheptanoic acid (PFHpA)	9.70	13.8	106	4	50	50-150	
Perfluorobutanesulfonic acid (PFBS)	87.3	98.5	113	3	50	50-150	

Column to be used to flag recovery and RPD values

FORM IV
LCMS METHOD BLANK SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Lab File ID: 2018.01.20_537AA_007.d Lab Sample ID: MB 320-204304/1-A
 Matrix: Water Date Extracted: 01/17/2018 10:50
 Instrument ID: A8_N Date Analyzed: 01/20/2018 19:01
 Level: (Low/Med) Low

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES:

CLIENT SAMPLE ID	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED
	LLCS 320-204304/2-A	2018.01.20_537AA_008.d	01/20/2018 19:06
WGNA-010818-RW-0344	320-34917-1	2018.01.20_537AA_009.d	01/20/2018 19:11
WGNA-010818-FRB-0344	320-34917-2	2018.01.20_537AA_010.d	01/20/2018 19:15
WGNA-010818-RW-3957	320-34917-3	2018.01.20_537AA_011.d	01/20/2018 19:20
WGNA-010818-FRB-3957	320-34917-4	2018.01.20_537AA_012.d	01/20/2018 19:25
WGNA-010818-DUP-16	320-34917-5	2018.01.20_537AA_013.d	01/20/2018 19:29
WGNA-010818-RW-3178	320-34917-6	2018.01.20_537AA_014.d	01/20/2018 19:34
WGNA-010818-FRB-3178	320-34917-7	2018.01.20_537AA_015.d	01/20/2018 19:39
NAWC-010818-RW-141	320-34917-8	2018.01.20_537AA_016.d	01/20/2018 19:43
NAWC-010818-FRB-141	320-34917-9	2018.01.23537A_007.d	01/24/2018 05:15
WGNA-010818-RW-4024	320-34917-10	2018.01.23537A_008.d	01/24/2018 05:19
WGNA-010818-RW-4024 LMS	320-34917-10 LMS	2018.01.23537A_009.d	01/24/2018 05:24
WGNA-010818-RW-4024 LMSD	320-34917-10 LMSD	2018.01.23537A_010.d	01/24/2018 05:29
WGNA-010818-FRB-4024	320-34917-11	2018.01.23537A_011.d	01/24/2018 05:33
WGNA-010818-RW-4844	320-34917-12	2018.01.23537A_012.d	01/24/2018 05:38
WGNA-010818-FRB-4844	320-34917-13	2018.01.23537A_013.d	01/24/2018 05:43
WGNA-010818-RW-0404	320-34917-14	2018.01.23537A_014.d	01/24/2018 05:47
WGNA-010818-FRB-0404	320-34917-15	2018.01.23537A_015.d	01/24/2018 05:52

FORM VIII
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Instrument ID: A8_N Calibration Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3(mm) Calibration End Date: 11/03/2017 14:01
 Calibration ID: 36012

		13PFOA		PFOS			
		AREA #	RT #	AREA #	RT #	AREA #	RT #
INITIAL CALIBRATION MEAN AREA AND MEAN RT		1535518	1.91	3276559	2.15		
UPPER LIMIT		2303277	2.41	4914839	2.65		
LOWER LIMIT		767759	1.41	1638280	1.65		
LAB SAMPLE ID	CLIENT SAMPLE ID						
CCVL 320-192908/11		1586829	1.91	3305852	2.15		
ICV 320-192908/13		1512045	1.90	3433628	2.14		
CCVL 320-204872/1		1654416	1.81	3432875	2.06		
CCV 320-204872/2 CCVIS		1716899	1.81	3708679	2.06		
MB 320-204304/1-A		1804768	1.81	3734647	2.06		
LLCS 320-204304/2-A		1751473	1.81	3675151	2.06		
320-34917-1	WGNA-010818-RW-0344	1728428	1.82	3615761	2.06		
320-34917-2	WGNA-010818-FRB-0344	1775689	1.81	3694502	2.06		
320-34917-3	WGNA-010818-RW-3957	1666710	1.80	3707714	2.05		
320-34917-4	WGNA-010818-FRB-3957	1772939	1.81	3774506	2.06		
320-34917-5	WGNA-010818-DUP-16	1672120	1.80	3625224	2.05		
320-34917-6	WGNA-010818-RW-3178	1689952	1.80	3685668	2.05		
320-34917-7	WGNA-010818-FRB-3178	1703218	1.81	3729940	2.06		
320-34917-8	NAWC-010818-RW-141	1819910	1.80	3905757	2.05		
CCV 320-204872/14 CCVIS		1591448	1.80	3614871	2.05		
CCVL 320-205331/1		1522908	1.81	3142156	2.06		
CCV 320-205331/2 CCVIS		1578125	1.81	3472309	2.06		
320-34917-9	NAWC-010818-FRB-141	1561349	1.81	3372514	2.06		
320-34917-10	WGNA-010818-RW-4024	1713401	1.81	3759831	2.06		
320-34917-10 LMS	WGNA-010818-RW-4024 LMS	1640988	1.81	3643189	2.06		
320-34917-10 LMSD	WGNA-010818-RW-4024 LMSD	1685962	1.80	3866207	2.05		
320-34917-11	WGNA-010818-FRB-4024	1568292	1.81	3544184	2.06		
320-34917-12	WGNA-010818-RW-4844	1654396	1.81	3689900	2.06		
320-34917-13	WGNA-010818-FRB-4844	1557173	1.81	3476391	2.06		
320-34917-14	WGNA-010818-RW-0404	1567961	1.81	3414209	2.06		
320-34917-15	WGNA-010818-FRB-0404	1573488	1.81	3522216	2.06		
CCV 320-205331/13 CCVIS		1485112	1.81	3186147	2.06		

13PFOA = 13C2-PFOA
 PFOS = 13C4 PFOS

Area Limit = 50%-150% of internal standard area
 RT Limit = ± 0.5 minutes of internal standard RT

Column used to flag values outside QC limits

FORM VIII
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Sample No.: CCV 320-204872/2 Date Analyzed: 01/20/2018 18:52
 Instrument ID: A8_N GC Column: GeminiC18 3x100 ID: 3 (mm)
 Lab File ID (Standard): 2018.01.20_537AA_00 Heated Purge: (Y/N) N
 Calibration ID: 36012

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	1716899	1.81	3708679	2.06		
UPPER LIMIT	2403659	2.31	5192151	2.56		
LOWER LIMIT	1201829	1.31	2596075	1.56		
LAB SAMPLE ID	CLIENT SAMPLE ID					
MB 320-204304/1-A		1804768	1.81	3734647	2.06	
LLCS 320-204304/2-A		1751473	1.81	3675151	2.06	
320-34917-1	WGNA-010818-RW-0344	1728428	1.82	3615761	2.06	
320-34917-2	WGNA-010818-FRB-0344	1775689	1.81	3694502	2.06	
320-34917-3	WGNA-010818-RW-3957	1666710	1.80	3707714	2.05	
320-34917-4	WGNA-010818-FRB-3957	1772939	1.81	3774506	2.06	
320-34917-5	WGNA-010818-DUP-16	1672120	1.80	3625224	2.05	
320-34917-6	WGNA-010818-RW-3178	1689952	1.80	3685668	2.05	
320-34917-7	WGNA-010818-FRB-3178	1703218	1.81	3729940	2.06	
320-34917-8	NAWC-010818-RW-141	1819910	1.80	3905757	2.05	

13PFOA = 13C2-PFOA

PFOS = 13C4 PFOS

Area Limit = 70%-140% of internal standard area
 RT Limit = ± 0.5 minutes of internal standard RT

Column used to flag values outside QC limits

FORM VIII
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Sample No.: CCV 320-204872/14 Date Analyzed: 01/20/2018 19:48
 Instrument ID: A8_N GC Column: GeminiC18 3x100 ID: 3 (mm)
 Lab File ID (Standard): 2018.01.20_537AA_01 Heated Purge: (Y/N) N
 Calibration ID: 36012

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	1591448	1.80	3614871	2.05		
UPPER LIMIT	2228027	2.30	5060819	2.55		
LOWER LIMIT	1114014	1.30	2530410	1.55		
LAB SAMPLE ID	CLIENT SAMPLE ID					
MB 320-204304/1-A		1804768	1.81	3734647	2.06	
LLCS 320-204304/2-A		1751473	1.81	3675151	2.06	
320-34917-1	WGNA-010818-RW-0344	1728428	1.82	3615761	2.06	
320-34917-2	WGNA-010818-FRB-0344	1775689	1.81	3694502	2.06	
320-34917-3	WGNA-010818-RW-3957	1666710	1.80	3707714	2.05	
320-34917-4	WGNA-010818-FRB-3957	1772939	1.81	3774506	2.06	
320-34917-5	WGNA-010818-DUP-16	1672120	1.80	3625224	2.05	
320-34917-6	WGNA-010818-RW-3178	1689952	1.80	3685668	2.05	
320-34917-7	WGNA-010818-FRB-3178	1703218	1.81	3729940	2.06	
320-34917-8	NAWC-010818-RW-141	1819910	1.80	3905757	2.05	

13PFOA = 13C2-PFOA
 PFOS = 13C4 PFOS

Area Limit = 70%-140% of internal standard area
 RT Limit = ± 0.5 minutes of internal standard RT

Column used to flag values outside QC limits

FORM VIII
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Sample No.: CCV 320-205331/2 Date Analyzed: 01/24/2018 05:05
 Instrument ID: A8_N GC Column: GeminiC18 3x100 ID: 3 (mm)
 Lab File ID (Standard): 2018.01.23537A_005. Heated Purge: (Y/N) N
 Calibration ID: 36012

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	1578125	1.81	3472309	2.06		
UPPER LIMIT	2209375	2.31	4861233	2.56		
LOWER LIMIT	1104688	1.31	2430616	1.56		
LAB SAMPLE ID	CLIENT SAMPLE ID					
320-34917-9	NAWC-010818-FRB-141	1561349	1.81	3372514	2.06	
320-34917-10	WGNA-010818-RW-4024	1713401	1.81	3759831	2.06	
320-34917-10 LMS	WGNA-010818-RW-4024 LMS	1640988	1.81	3643189	2.06	
320-34917-10 LMSD	WGNA-010818-RW-4024 LMSD	1685962	1.80	3866207	2.05	
320-34917-11	WGNA-010818-FRB-4024	1568292	1.81	3544184	2.06	
320-34917-12	WGNA-010818-RW-4844	1654396	1.81	3689900	2.06	
320-34917-13	WGNA-010818-FRB-4844	1557173	1.81	3476391	2.06	
320-34917-14	WGNA-010818-RW-0404	1567961	1.81	3414209	2.06	
320-34917-15	WGNA-010818-FRB-0404	1573488	1.81	3522216	2.06	

13PFOA = 13C2-PFOA
 PFOS = 13C4 PFOS

Area Limit = 70%-140% of internal standard area
 RT Limit = ± 0.5 minutes of internal standard RT

Column used to flag values outside QC limits

FORM VIII
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Sample No.: CCV 320-205331/13 Date Analyzed: 01/24/2018 05:57
 Instrument ID: A8_N GC Column: GeminiC18 3x100 ID: 3 (mm)
 Lab File ID (Standard): 2018.01.23537A_016. Heated Purge: (Y/N) N
 Calibration ID: 36012

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	1485112	1.81	3186147	2.06		
UPPER LIMIT	2079157	2.31	4460606	2.56		
LOWER LIMIT	1039578	1.31	2230303	1.56		
LAB SAMPLE ID	CLIENT SAMPLE ID					
320-34917-9	NAWC-010818-FRB-141	1561349	1.81	3372514	2.06	
320-34917-10	WGNA-010818-RW-4024	1713401	1.81	3759831	2.06	
320-34917-10 LMS	WGNA-010818-RW-4024 LMS	1640988	1.81	3643189	2.06	
320-34917-10 LMSD	WGNA-010818-RW-4024 LMSD	1685962	1.80	3866207	2.05	
320-34917-11	WGNA-010818-FRB-4024	1568292	1.81	3544184	2.06	
320-34917-12	WGNA-010818-RW-4844	1654396	1.81	3689900	2.06	
320-34917-13	WGNA-010818-FRB-4844	1557173	1.81	3476391	2.06	
320-34917-14	WGNA-010818-RW-0404	1567961	1.81	3414209	2.06	
320-34917-15	WGNA-010818-FRB-0404	1573488	1.81	3522216	2.06	

13PFOA = 13C2-PFOA

PFOS = 13C4 PFOS

Area Limit = 70%-140% of internal standard area

RT Limit = ± 0.5 minutes of internal standard RT

Column used to flag values outside QC limits

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: WGNA-010818-RW-0344 Lab Sample ID: 320-34917-1
 Matrix: Water Lab File ID: 2018.01.20_537AA_009.d
 Analysis Method: 537 Date Collected: 01/08/2018 08:10
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 248.7(mL) Date Analyzed: 01/20/2018 19:11
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 204872 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	32	J	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	24		20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	32		24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	18	J	30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	6.4	J	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	91		70-130
STL00996	13C2 PFDA	93		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\2018.01.20_537AA_009.d
 Lims ID: 320-34917-A-1-A
 Client ID: WGNA-010818-RW-0344
 Sample Type: Client
 Inject. Date: 20-Jan-2018 19:11:11 ALS Bottle#: 6 Worklist Smp#: 6
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-34917-a-1-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 22-Jan-2018 13:30:12 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK027

First Level Reviewer: roycea Date: 22-Jan-2018 11:20:19

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.373	1.444	-0.071	1.000	228847	1.63		268	
298.90 > 99.00	1.373	1.444	-0.071	1.000	169656		1.35(0.00-0.00)	403	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.487	1.573	-0.086	1.000	1726156	9.08		7036	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.631	1.725	-0.094	1.000	952334	4.51		577	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.631	1.725	-0.094	1.000	257095	1.59		42.0	
* 6 13C2-PFOA									
415.00 > 370.00	1.821	1.913	-0.092		1728428	10.0		5372	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.821	1.914	-0.093	1.000	973463	6.08		123	
413.00 > 169.00	1.813	1.914	-0.101	0.996	587978		1.66(0.00-0.00)	1517	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.064	2.048	0.016	1.000	941358	7.95		209	
499.00 > 99.00	2.064	2.048	0.016	1.000	167367		5.62(0.00-0.00)	243	
* 7 13C4 PFOS									
503.00 > 80.00	2.064	2.151	-0.087		3615761	28.7		4171	
9 Perfluorononanoic acid									
463.00 > 419.00	2.071	2.158	-0.087	1.000	902861	7.86		111	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.238	2.312	-0.074	1.000	1236585	9.35		6939	




TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\2018.01.20_537AA_009.d
Injection Date: 20-Jan-2018 19:11:11 Instrument ID: A8_N
Lims ID: 320-34917-A-1-A Lab Sample ID: 320-34917-1
Client ID: WGNA-010818-RW-0344
Operator ID: SACINSTLCMS01 ALS Bottle#: 6 Worklist Smp#: 6
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid




8 Perfluorooctane sulfonic acid

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\2018.01.20_537AA_009.d
 Lims ID: 320-34917-A-1-A
 Client ID: WGNA-010818-RW-0344
 Sample Type: Client
 Inject. Date: 20-Jan-2018 19:11:11 ALS Bottle#: 6 Worklist Smp#: 6
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-34917-a-1-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 22-Jan-2018 13:30:12 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK027

First Level Reviewer: roycea Date: 22-Jan-2018 11:20:19

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	9.08	90.77
\$ 10 13C2 PFDA	10.0	9.35	93.50

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: WGNA-010818-FRB-0344 Lab Sample ID: 320-34917-2
 Matrix: Water Lab File ID: 2018.01.20_537AA_010.d
 Analysis Method: 537 Date Collected: 01/08/2018 08:05
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 253.2 (mL) Date Analyzed: 01/20/2018 19:15
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 204872 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	39	16	6.7
335-67-1	Perfluorooctanoic acid (PFOA)	7.9	U	20	7.9	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	7.9
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	30	12	5.4
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.9	U	9.9	3.9	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	89	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	97		70-130
STL00996	13C2 PFDA	98		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\2018.01.20_537AA_010.d
 Lims ID: 320-34917-A-2-A
 Client ID: WGNA-010818-FRB-0344
 Sample Type: Client
 Inject. Date: 20-Jan-2018 19:15:52 ALS Bottle#: 7 Worklist Smp#: 7
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-34917-a-2-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 22-Jan-2018 13:30:12 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK027


First Level Reviewer: roycea Date: 22-Jan-2018 13:23:06

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
\$ 2 13C2 PFHxA	315.00 > 270.00	1.487	1.573	-0.086	1.000	1900186	9.73	7804	
* 6 13C2-PFOA	415.00 > 370.00	1.806	1.913	-0.107		1775689	10.0	5839	
* 7 13C4 PFOS	503.00 > 80.00	2.056	2.151	-0.095		3694502	28.7	8496	
\$ 10 13C2 PFDA	515.00 > 470.00	2.238	2.312	-0.074	1.000	1336945	9.84	6560	


TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\2018.01.20_537AA_010.d
Injection Date: 20-Jan-2018 19:15:52 Instrument ID: A8_N
Lims ID: 320-34917-A-2-A Lab Sample ID: 320-34917-2
Client ID: WGNA-010818-FRB-0344
Operator ID: SACINSTLCMS01 ALS Bottle#: 7 Worklist Smp#: 7
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL


1 Perfluorobutanesulfonic acid (ND) 1 Perfluorobutanesulfonic acid (ND) \$ 2 13C2 PFHxA




3 Perfluorohexanesulfonic acid (ND) 4 Perfluoroheptanoic acid (ND) * 6 13C2-PFOA




5 Perfluorooctanoic acid (ND) 5 Perfluorooctanoic acid (ND) 8 Perfluorooctane sulfonic acid (ND)



8 Perfluorooctane sulfonic acid (ND) * 7 13C4 PFOS 9 Perfluorononanoic acid (ND)



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\2018.01.20_537AA_010.d
 Lims ID: 320-34917-A-2-A
 Client ID: WGNA-010818-FRB-0344
 Sample Type: Client
 Inject. Date: 20-Jan-2018 19:15:52 ALS Bottle#: 7 Worklist Smp#: 7
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-34917-a-2-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 22-Jan-2018 13:30:12 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK027

First Level Reviewer: roycea Date: 22-Jan-2018 13:23:06

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	9.73	97.26
\$ 10 13C2 PFDA	10.0	9.84	98.39

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: WGNA-010818-RW-3957 Lab Sample ID: 320-34917-3
 Matrix: Water Lab File ID: 2018.01.20_537AA_011.d
 Analysis Method: 537 Date Collected: 01/08/2018 08:40
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 257.4 (mL) Date Analyzed: 01/20/2018 19:20
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 204872 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	18	J	39	16	6.6
335-67-1	Perfluorooctanoic acid (PFOA)	15	J	19	7.8	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U M	23	19	7.8
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	6.5	J	29	12	5.3
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	J	9.7	3.9	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	35	U	87	35	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	91		70-130
STL00996	13C2 PFDA	104		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\2018.01.20_537AA_011.d
 Lims ID: 320-34917-A-3-A
 Client ID: WGNA-010818-RW-3957
 Sample Type: Client
 Inject. Date: 20-Jan-2018 19:20:33 ALS Bottle#: 8 Worklist Smp#: 8
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-34917-a-3-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 22-Jan-2018 13:30:12 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK027

First Level Reviewer: roycea Date: 22-Jan-2018 13:23:36

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.358	1.444	-0.086	1.000	199545	1.38		196	
298.90 > 99.00	1.358	1.444	-0.086	1.000	138671		1.44(0.00-0.00)	329	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.479	1.573	-0.094	1.000	1675943	9.14		7269	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.616	1.725	-0.109	1.000	359824	1.66		179	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.616	1.725	-0.109	1.000	152996	0.9798		22.3	
* 6 13C2-PFOA									
415.00 > 370.00	1.798	1.913	-0.115		1666710	10.0		5710	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.798	1.914	-0.116	1.000	578995	3.75		63.4	
413.00 > 169.00	1.798	1.914	-0.116	1.000	368417		1.57(0.00-0.00)	819	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.048	2.048	0.0	1.000	568168	4.68		111	
499.00 > 99.00	2.048	2.048	0.0	1.000	98293		5.78(0.00-0.00)	109	
* 7 13C4 PFOS									
503.00 > 80.00	2.048	2.151	-0.103		3707714	28.7		3235	
9 Perfluorononanoic acid									
463.00 > 419.00	2.056	2.158	-0.102	1.000	44621	0.4031		4.7	M
\$ 10 13C2 PFDA									
515.00 > 470.00	2.238	2.312	-0.074	1.000	1325043	10.4		6419	

QC Flag Legend

Review Flags

M - Manually Integrated




TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\2018.01.20_537AA_011.d
Injection Date: 20-Jan-2018 19:20:33 Instrument ID: A8_N
Lims ID: 320-34917-A-3-A Lab Sample ID: 320-34917-3
Client ID: WGNA-010818-RW-3957
Operator ID: SACINSTLCMS01 ALS Bottle#: 8 Worklist Smp#: 8
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid




8 Perfluorooctane sulfonic acid

* 7 13C4 PFOS

9 Perfluorononanoic acid (M)



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\2018.01.20_537AA_011.d
 Lims ID: 320-34917-A-3-A
 Client ID: WGNA-010818-RW-3957
 Sample Type: Client
 Inject. Date: 20-Jan-2018 19:20:33 ALS Bottle#: 8 Worklist Smp#: 8
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-34917-a-3-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 22-Jan-2018 13:30:12 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK027

First Level Reviewer: roycea Date: 22-Jan-2018 13:23:36

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	9.14	91.39
\$ 10 13C2 PFDA	10.0	10.4	103.89

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\2018.01.20_537AA_011.d
Injection Date: 20-Jan-2018 19:20:33 Instrument ID: A8_N
Lims ID: 320-34917-A-3-A Lab Sample ID: 320-34917-3
Client ID: WGNA-010818-RW-3957
Operator ID: SACINSTLCMS01 ALS Bottle#: 8 Worklist Smp#: 8
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

9 Perfluorononanoic acid, CAS: 375-95-1

Signal: 1


RT: 1.97
Area: 45654
Amount: 0.412426
Amount Units: ng/ml

Processing Integration Results



RT: 2.06
Area: 44621
Amount: 0.403094
Amount Units: ng/ml

Manual Integration Results



Reviewer: roycea, 22-Jan-2018 13:24:33

Audit Action: Marked Compound Undetected

Audit Reason: Invalid Compound ID

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\2018.01.20_537AA_011.d
Injection Date: 20-Jan-2018 19:20:33 Instrument ID: A8_N
Lims ID: 320-34917-A-3-A Lab Sample ID: 320-34917-3
Client ID: WGNA-010818-RW-3957
Operator ID: SACINSTLCMS01 ALS Bottle#: 8 Worklist Smp#: 8
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

9 Perfluorononanoic acid, CAS: 375-95-1

Signal: 1


RT: 1.97
Area: 45654
Amount: 0.412426
Amount Units: ng/ml

Processing Integration Results



RT: 2.06
Area: 44621
Amount: 0.403094
Amount Units: ng/ml

Manual Integration Results



FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: WGNA-010818-FRB-3957 Lab Sample ID: 320-34917-4
 Matrix: Water Lab File ID: 2018.01.20_537AA_012.d
 Analysis Method: 537 Date Collected: 01/08/2018 08:35
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 256.1(mL) Date Analyzed: 01/20/2018 19:25
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 204872 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	39	16	6.6
335-67-1	Perfluorooctanoic acid (PFOA)	7.8	U	20	7.8	2.7
375-95-1	Perfluorononanoic acid (PFNA)	20	U	23	20	7.8
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	29	12	5.4
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.9	U	9.8	3.9	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	35	U	88	35	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	96		70-130
STL00996	13C2 PFDA	98		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\2018.01.20_537AA_012.d
 Lims ID: 320-34917-A-4-A
 Client ID: WGNA-010818-FRB-3957
 Sample Type: Client
 Inject. Date: 20-Jan-2018 19:25:13 ALS Bottle#: 9 Worklist Smp#: 9
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-34917-a-4-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 22-Jan-2018 13:30:12 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK027


First Level Reviewer: roycea Date: 22-Jan-2018 13:26:23

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
\$ 2 13C2 PFHxA	315.00 > 270.00	1.479	1.573	-0.094	1.000	1875316	9.61	8569	
* 6 13C2-PFOA	415.00 > 370.00	1.806	1.913	-0.107		1772939	10.0	6018	
* 7 13C4 PFOS	503.00 > 80.00	2.056	2.151	-0.095		3774506	28.7	7347	
\$ 10 13C2 PFDA	515.00 > 470.00	2.238	2.312	-0.074	1.000	1333910	9.83	7214	


TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\2018.01.20_537AA_012.d
Injection Date: 20-Jan-2018 19:25:13 Instrument ID: A8_N
Lims ID: 320-34917-A-4-A Lab Sample ID: 320-34917-4
Client ID: WGNA-010818-FRB-3957
Operator ID: SACINSTLCMS01 ALS Bottle#: 9 Worklist Smp#: 9
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL


1 Perfluorobutanesulfonic acid (ND) 1 Perfluorobutanesulfonic acid (ND) \$ 2 13C2 PFHxA




3 Perfluorohexanesulfonic acid (ND) 4 Perfluoroheptanoic acid (ND) * 6 13C2-PFOA




5 Perfluorooctanoic acid (ND) 5 Perfluorooctanoic acid (ND) 8 Perfluorooctane sulfonic acid (ND)



8 Perfluorooctane sulfonic acid (ND) * 7 13C4 PFOS 9 Perfluorononanoic acid (ND)



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\2018.01.20_537AA_012.d
 Lims ID: 320-34917-A-4-A
 Client ID: WGNA-010818-FRB-3957
 Sample Type: Client
 Inject. Date: 20-Jan-2018 19:25:13 ALS Bottle#: 9 Worklist Smp#: 9
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-34917-a-4-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 22-Jan-2018 13:30:12 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK027

First Level Reviewer: roycea Date: 22-Jan-2018 13:26:23

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	9.61	96.13
\$ 10 13C2 PFDA	10.0	9.83	98.32

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: WGNA-010818-DUP-16 Lab Sample ID: 320-34917-5
 Matrix: Water Lab File ID: 2018.01.20_537AA_013.d
 Analysis Method: 537 Date Collected: 01/08/2018 07:00
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 262.5 (mL) Date Analyzed: 01/20/2018 19:29
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 204872 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	25	J	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	21		19	7.6	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	8.0	J	29	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	6.2	J	9.5	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	86	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	96		70-130
STL00996	13C2 PFDA	109		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\2018.01.20_537AA_013.d
 Lims ID: 320-34917-A-5-A
 Client ID: WGNA-010818-DUP-16
 Sample Type: Client
 Inject. Date: 20-Jan-2018 19:29:54 ALS Bottle#: 10 Worklist Smp#: 10
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-34917-a-5-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 22-Jan-2018 13:30:12 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK027

First Level Reviewer: roycea Date: 22-Jan-2018 13:26:54

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.358	1.444	-0.086	1.000	225700	1.60		123	
298.90 > 99.00	1.358	1.444	-0.086	1.000	154094		1.46(0.00-0.00)	306	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.479	1.573	-0.094	1.000	1771611	9.63		7419	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.624	1.725	-0.101	1.000	443228	2.09		167	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.624	1.725	-0.101	1.000	256199	1.64		36.6	
* 6 13C2-PFOA									
415.00 > 370.00	1.798	1.913	-0.115		1672120	10.0		5552	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.798	1.914	-0.116	1.000	841841	5.44		98.8	
413.00 > 169.00	1.798	1.914	-0.116	1.000	527107		1.60(0.00-0.00)	1220	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.056	2.048	0.008	1.000	782108	6.59		139	
499.00 > 99.00	2.056	2.048	0.008	1.000	138692		5.64(0.00-0.00)	153	
* 7 13C4 PFOS									
503.00 > 80.00	2.048	2.151	-0.103		3625224	28.7		2645	
9 Perfluorononanoic acid									
463.00 > 419.00	2.064	2.158	-0.094	1.000	72063	0.6489		8.2	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.246	2.312	-0.066	1.000	1391608	10.9		7293	




TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\2018.01.20_537AA_013.d
Injection Date: 20-Jan-2018 19:29:54 Instrument ID: A8_N
Lims ID: 320-34917-A-5-A Lab Sample ID: 320-34917-5
Client ID: WGNA-010818-DUP-16
Operator ID: SACINSTLCMS01 ALS Bottle#: 10 Worklist Smp#: 10
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid




8 Perfluorooctane sulfonic acid

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\2018.01.20_537AA_013.d
 Lims ID: 320-34917-A-5-A
 Client ID: WGNA-010818-DUP-16
 Sample Type: Client
 Inject. Date: 20-Jan-2018 19:29:54 ALS Bottle#: 10 Worklist Smp#: 10
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-34917-a-5-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 22-Jan-2018 13:30:12 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK027

First Level Reviewer: roycea Date: 22-Jan-2018 13:26:54

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	9.63	96.29
\$ 10 13C2 PFDA	10.0	10.9	108.76

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: WGNA-010818-RW-3178 Lab Sample ID: 320-34917-6
 Matrix: Water Lab File ID: 2018.01.20_537AA_014.d
 Analysis Method: 537 Date Collected: 01/08/2018 10:10
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 239.2 (mL) Date Analyzed: 01/20/2018 19:34
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 204872 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	J	42	17	7.1
335-67-1	Perfluorooctanoic acid (PFOA)	9.8	J	21	8.4	2.9
375-95-1	Perfluorononanoic acid (PFNA)	21	U	25	21	8.4
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	7.0	J	31	13	5.7
375-85-9	Perfluoroheptanoic acid (PFHpA)	2.8	J	10	4.2	2.0
375-73-5	Perfluorobutanesulfonic acid (PFBS)	38	U	94	38	17

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	90		70-130
STL00996	13C2 PFDA	102		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\2018.01.20_537AA_014.d
 Lims ID: 320-34917-A-6-A
 Client ID: WGNA-010818-RW-3178
 Sample Type: Client
 Inject. Date: 20-Jan-2018 19:34:35 ALS Bottle#: 11 Worklist Smp#: 11
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-34917-a-6-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 22-Jan-2018 13:30:12 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK027

First Level Reviewer: roycea Date: 22-Jan-2018 13:27:19

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.366	1.444	-0.078	1.000	167575	1.17		183	
298.90 > 99.00	1.366	1.444	-0.078	1.000	126419		1.33(0.00-0.00)	282	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.479	1.573	-0.094	1.000	1679593	9.03		7551	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.624	1.725	-0.101	1.000	360910	1.68		193	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.624	1.725	-0.101	1.000	105726	0.6677		16.1	
* 6 13C2-PFOA									
415.00 > 370.00	1.798	1.913	-0.115		1689952	10.0		5673	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.806	1.914	-0.108	1.000	367085	2.35		43.3	
413.00 > 169.00	1.798	1.914	-0.116	0.996	217833		1.69(0.00-0.00)	462	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.056	2.048	0.008	1.000	470745	3.90		77.2	
499.00 > 99.00	2.048	2.048	0.0	0.996	83442		5.64(0.00-0.00)	68.0	
* 7 13C4 PFOS									
503.00 > 80.00	2.048	2.151	-0.103		3685668	28.7		3905	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.238	2.312	-0.074	1.000	1321419	10.2		7886	




TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\2018.01.20_537AA_014.d
Injection Date: 20-Jan-2018 19:34:35 Instrument ID: A8_N
Lims ID: 320-34917-A-6-A Lab Sample ID: 320-34917-6
Client ID: WGNA-010818-RW-3178
Operator ID: SACINSTLCMS01 ALS Bottle#: 11 Worklist Smp#: 11
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid




8 Perfluorooctane sulfonic acid

* 7 13C4 PFOS

9 Perfluorononanoic acid (ND)



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\2018.01.20_537AA_014.d
 Lims ID: 320-34917-A-6-A
 Client ID: WGNA-010818-RW-3178
 Sample Type: Client
 Inject. Date: 20-Jan-2018 19:34:35 ALS Bottle#: 11 Worklist Smp#: 11
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-34917-a-6-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 22-Jan-2018 13:30:12 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK027

First Level Reviewer: roycea Date: 22-Jan-2018 13:27:19

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	9.03	90.33
\$ 10 13C2 PFDA	10.0	10.2	102.19

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: WGNA-010818-FRB-3178 Lab Sample ID: 320-34917-7
 Matrix: Water Lab File ID: 2018.01.20_537AA_015.d
 Analysis Method: 537 Date Collected: 01/08/2018 10:05
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 256.7(mL) Date Analyzed: 01/20/2018 19:39
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 204872 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	39	16	6.6
335-67-1	Perfluorooctanoic acid (PFOA)	7.8	U	19	7.8	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.8
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	29	12	5.4
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.9	U	9.7	3.9	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	35	U	88	35	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	98		70-130
STL00996	13C2 PFDA	103		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\2018.01.20_537AA_015.d
 Lims ID: 320-34917-A-7-A
 Client ID: WGNA-010818-FRB-3178
 Sample Type: Client
 Inject. Date: 20-Jan-2018 19:39:17 ALS Bottle#: 12 Worklist Smp#: 12
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-34917-a-7-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 22-Jan-2018 13:30:12 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK027


First Level Reviewer: roycea Date: 22-Jan-2018 13:28:58

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
\$ 2 13C2 PFHxA	315.00 > 270.00	1.479	1.573	-0.094	1.000	1838518	9.81	7307	
* 6 13C2-PFOA	415.00 > 370.00	1.806	1.913	-0.107		1703218	10.0	5405	
* 7 13C4 PFOS	503.00 > 80.00	2.056	2.151	-0.095		3729940	28.7	7922	
\$ 10 13C2 PFDA	515.00 > 470.00	2.238	2.312	-0.074	1.000	1342017	10.3	7850	


TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\2018.01.20_537AA_015.d
Injection Date: 20-Jan-2018 19:39:17 Instrument ID: A8_N
Lims ID: 320-34917-A-7-A Lab Sample ID: 320-34917-7
Client ID: WGNA-010818-FRB-3178
Operator ID: SACINSTLCMS01 ALS Bottle#: 12 Worklist Smp#: 12
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL


1 Perfluorobutanesulfonic acid (ND) 1 Perfluorobutanesulfonic acid (ND) \$ 2 13C2 PFHxA




3 Perfluorohexanesulfonic acid (ND) 4 Perfluoroheptanoic acid (ND) * 6 13C2-PFOA




5 Perfluorooctanoic acid (ND) 5 Perfluorooctanoic acid (ND) 8 Perfluorooctane sulfonic acid (ND)



8 Perfluorooctane sulfonic acid (ND) * 7 13C4 PFOS 9 Perfluorononanoic acid (ND)



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\2018.01.20_537AA_015.d
 Lims ID: 320-34917-A-7-A
 Client ID: WGNA-010818-FRB-3178
 Sample Type: Client
 Inject. Date: 20-Jan-2018 19:39:17 ALS Bottle#: 12 Worklist Smp#: 12
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-34917-a-7-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 22-Jan-2018 13:30:12 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK027

First Level Reviewer: roycea Date: 22-Jan-2018 13:28:58

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	9.81	98.10
\$ 10 13C2 PFDA	10.0	10.3	102.97

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: NAWC-010818-RW-141 Lab Sample ID: 320-34917-8
 Matrix: Water Lab File ID: 2018.01.20_537AA_016.d
 Analysis Method: 537 Date Collected: 01/08/2018 11:10
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 257.5 (mL) Date Analyzed: 01/20/2018 19:43
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 204872 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	24	J	39	16	6.6
335-67-1	Perfluorooctanoic acid (PFOA)	15	J	19	7.8	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.8
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	16	J	29	12	5.3
375-85-9	Perfluoroheptanoic acid (PFHpA)	7.6	J	9.7	3.9	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	35	U	87	35	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	88		70-130
STL00996	13C2 PFDA	96		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\2018.01.20_537AA_016.d
 Lims ID: 320-34917-A-8-A
 Client ID: NAWC-010818-RW-141
 Sample Type: Client
 Inject. Date: 20-Jan-2018 19:43:57 ALS Bottle#: 13 Worklist Smp#: 13
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-34917-a-8-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 22-Jan-2018 13:30:12 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK027

First Level Reviewer: roycea Date: 22-Jan-2018 13:29:37

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.366	1.444	-0.078	1.000	285384	1.88		277	
298.90 > 99.00	1.366	1.444	-0.078	1.000	204957		1.39(0.00-0.00)	449	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.479	1.573	-0.094	1.000	1759186	8.79		8077	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.624	1.725	-0.101	1.000	931647	4.09		559	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.624	1.725	-0.101	1.000	335832	1.97		57.5	
* 6 13C2-PFOA									
415.00 > 370.00	1.798	1.913	-0.115		1819910	10.0		5944	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.798	1.914	-0.116	1.000	670352	3.98		83.3	
413.00 > 169.00	1.798	1.914	-0.116	1.000	396391		1.69(0.00-0.00)	954	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.048	2.048	0.0	1.000	783128	6.12		158	
499.00 > 99.00	2.048	2.048	0.0	1.000	143844		5.44(0.00-0.00)	190	
* 7 13C4 PFOS									
503.00 > 80.00	2.048	2.151	-0.103		3905757	28.7		3822	
9 Perfluorononanoic acid									
463.00 > 419.00	2.056	2.158	-0.102	1.000	54373	0.4498		6.5	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.238	2.312	-0.074	1.000	1338670	9.61		7714	


TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\2018.01.20_537AA_016.d
Injection Date: 20-Jan-2018 19:43:57 Instrument ID: A8_N
Lims ID: 320-34917-A-8-A Lab Sample ID: 320-34917-8
Client ID: NAWC-010818-RW-141
Operator ID: SACINSTLCMS01 ALS Bottle#: 13 Worklist Smp#: 13
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid


\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid


* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid


8 Perfluorooctane sulfonic acid




8 Perfluorooctane sulfonic acid

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\2018.01.20_537AA_016.d
 Lims ID: 320-34917-A-8-A
 Client ID: NAWC-010818-RW-141
 Sample Type: Client
 Inject. Date: 20-Jan-2018 19:43:57 ALS Bottle#: 13 Worklist Smp#: 13
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-34917-a-8-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 22-Jan-2018 13:30:12 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK027

First Level Reviewer: roycea Date: 22-Jan-2018 13:29:37

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	8.79	87.85
\$ 10 13C2 PFDA	10.0	9.61	96.13

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: NAWC-010818-FRB-141 Lab Sample ID: 320-34917-9
 Matrix: Water Lab File ID: 2018.01.23537A_007.d
 Analysis Method: 537 Date Collected: 01/08/2018 11:05
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 266.1(mL) Date Analyzed: 01/24/2018 05:15
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 205331 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	38	15	6.4
335-67-1	Perfluorooctanoic acid (PFOA)	7.5	U	19	7.5	2.6
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.5
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	U	9.4	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	85	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	95		70-130
STL00996	13C2 PFDA	99		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\2018.01.23537A_007.d
 Lims ID: 320-34917-A-9-A
 Client ID: NAWC-010818-FRB-141
 Sample Type: Client
 Inject. Date: 24-Jan-2018 05:15:10 ALS Bottle#: 14 Worklist Smp#: 4
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-34917-a-9-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 24-Jan-2018 09:58:52 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK024


First Level Reviewer: roycea Date: 24-Jan-2018 09:53:27

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
\$ 2 13C2 PFHxA	315.00 > 270.00	1.479	1.487	-0.008	1.000	1625381	9.46	8692	
* 6 13C2-PFOA	415.00 > 370.00	1.806	1.813	-0.007		1561349	10.0	6569	
* 7 13C4 PFOS	503.00 > 80.00	2.064	2.064	0.0		3372514	28.7	6897	
\$ 10 13C2 PFDA	515.00 > 470.00	2.246	2.246	0.0	1.000	1177265	9.85	6822	


TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\2018.01.23537A_007.d
Injection Date: 24-Jan-2018 05:15:10 Instrument ID: A8_N
Lims ID: 320-34917-A-9-A Lab Sample ID: 320-34917-9
Client ID: NAWC-010818-FRB-141
Operator ID: SACINSTLCMS01 ALS Bottle#: 14 Worklist Smp#: 4
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL


1 Perfluorobutanesulfonic acid (ND) 1 Perfluorobutanesulfonic acid (ND) \$ 2 13C2 PFHxA




4 Perfluoroheptanoic acid (ND) 3 Perfluorohexanesulfonic acid (ND) * 6 13C2-PFOA




5 Perfluorooctanoic acid (ND) 5 Perfluorooctanoic acid (ND) 8 Perfluorooctane sulfonic acid (ND)



8 Perfluorooctane sulfonic acid (ND) * 7 13C4 PFOS 9 Perfluorononanoic acid (ND)



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\2018.01.23537A_007.d
 Lims ID: 320-34917-A-9-A
 Client ID: NAWC-010818-FRB-141
 Sample Type: Client
 Inject. Date: 24-Jan-2018 05:15:10 ALS Bottle#: 14 Worklist Smp#: 4
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-34917-a-9-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 24-Jan-2018 09:58:52 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK024

First Level Reviewer: roycea Date: 24-Jan-2018 09:53:27

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	9.46	94.61
\$ 10 13C2 PFDA	10.0	9.85	98.54

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: WGNA-010818-RW-4024 Lab Sample ID: 320-34917-10
 Matrix: Water Lab File ID: 2018.01.23537A_008.d
 Analysis Method: 537 Date Collected: 01/08/2018 11:40
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 251.2 (mL) Date Analyzed: 01/24/2018 05:19
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 205331 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	18	J M	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	12	J	20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.6	J	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	71		70-130
STL00996	13C2 PFDA	93		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\2018.01.23537A_008.d
 Lims ID: 320-34917-A-10-A
 Client ID: WGNA-010818-RW-4024
 Sample Type: Client
 Inject. Date: 24-Jan-2018 05:19:52 ALS Bottle#: 15 Worklist Smp#: 5
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-34917-a-10-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 24-Jan-2018 09:58:52 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK024

First Level Reviewer: roycea Date: 24-Jan-2018 09:54:31

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.366	1.366	0.0	1.000	164377	1.12		72.7	
298.90 > 99.00	1.366	1.366	0.0	1.000	120298		1.37(0.00-0.00)	147	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.487	1.487	0.0	1.000	1332125	7.07		6422	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.631	1.631	0.0	1.000	144068	0.8974		18.3	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.624	1.631	-0.007	1.000	222146	1.01		69.8	
* 6 13C2-PFOA									
415.00 > 370.00	1.813	1.813	0.0		1713401	10.0		6632	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.813	1.813	0.0	1.000	476365	3.00		52.4	
413.00 > 169.00	1.813	1.813	0.0	1.000	268194		1.78(0.00-0.00)	453	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.064	2.056	0.008	1.000	544981	4.43		113	Ma
499.00 > 99.00	2.064	2.056	0.008	1.000	88000		6.19(0.00-0.00)	89.1	M
* 7 13C4 PFOS									
503.00 > 80.00	2.064	2.064	0.0		3759831	28.7		2559	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.246	2.246	0.0	1.000	1220839	9.31		8017	

QC Flag Legend

Review Flags

M - Manually Integrated

a - User Assigned ID

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\2018.01.23537A_008.d

Injection Date: 24-Jan-2018 05:19:52

Instrument ID: A8_N

Lims ID: 320-34917-A-10-A

Lab Sample ID: 320-34917-10

Client ID: WGNA-010818-RW-4024

Operator ID: SACINSTLCMS01

ALS Bottle#: 15

Worklist Smp#: 5

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



4 Perfluoroheptanoic acid

3 Perfluorohexanesulfonic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

* 7 13C4 PFOS

9 Perfluorononanoic acid (ND)



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\2018.01.23537A_008.d
 Lims ID: 320-34917-A-10-A
 Client ID: WGNA-010818-RW-4024
 Sample Type: Client
 Inject. Date: 24-Jan-2018 05:19:52 ALS Bottle#: 15 Worklist Smp#: 5
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-34917-a-10-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 24-Jan-2018 09:58:52 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK024

First Level Reviewer: roycea Date: 24-Jan-2018 09:54:31

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	7.07	70.66
\$ 10 13C2 PFDA	10.0	9.31	93.12

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\2018.01.23537A_008.d
Injection Date: 24-Jan-2018 05:19:52 Instrument ID: A8_N
Lims ID: 320-34917-A-10-A Lab Sample ID: 320-34917-10
Client ID: WGNA-010818-RW-4024
Operator ID: SACINSTLCMS01 ALS Bottle#: 15 Worklist Smp#: 5
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1


Signal: 2

Not Detected
Expected RT: 2.06

Processing Integration Results



Manual Integration Results



RT: 2.06
Area: 88000
Amount: 4.427416
Amount Units: ng/ml

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\2018.01.23537A_008.d
Injection Date: 24-Jan-2018 05:19:52 Instrument ID: A8_N
Lims ID: 320-34917-A-10-A Lab Sample ID: 320-34917-10
Client ID: WGNA-010818-RW-4024
Operator ID: SACINSTLCMS01 ALS Bottle#: 15 Worklist Smp#: 5
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.06

Processing Integration Results



Manual Integration Results

RT: 2.06
Area: 544981
Amount: 4.427416
Amount Units: ng/ml



FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: WGNA-010818-FRB-4024 Lab Sample ID: 320-34917-11
 Matrix: Water Lab File ID: 2018.01.23537A_011.d
 Analysis Method: 537 Date Collected: 01/08/2018 11:35
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 257.4 (mL) Date Analyzed: 01/24/2018 05:33
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 205331 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	39	16	6.6
335-67-1	Perfluorooctanoic acid (PFOA)	7.8	U	19	7.8	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.8
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	29	12	5.3
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.9	U	9.7	3.9	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	35	U	87	35	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	98		70-130
STL00996	13C2 PFDA	100		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\2018.01.23537A_011.d
 Lims ID: 320-34917-A-11-A
 Client ID: WGNA-010818-FRB-4024
 Sample Type: Client
 Inject. Date: 24-Jan-2018 05:33:54 ALS Bottle#: 18 Worklist Smp#: 8
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-34917-a-11-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 24-Jan-2018 09:58:52 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK024


First Level Reviewer: roycea Date: 24-Jan-2018 09:56:07

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
\$ 2 13C2 PFHxA	315.00 > 270.00	1.479	1.487	-0.008	1.000	1697258	9.84	8378	
* 6 13C2-PFOA	415.00 > 370.00	1.806	1.813	-0.007		1568292	10.0	6477	
* 7 13C4 PFOS	503.00 > 80.00	2.056	2.064	-0.008		3544184	28.7	8313	
\$ 10 13C2 PFDA	515.00 > 470.00	2.246	2.246	0.0	1.000	1200858	10.0	8252	


TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\2018.01.23537A_011.d
Injection Date: 24-Jan-2018 05:33:54 Instrument ID: A8_N
Lims ID: 320-34917-A-11-A Lab Sample ID: 320-34917-11
Client ID: WGNA-010818-FRB-4024
Operator ID: SACINSTLCMS01 ALS Bottle#: 18 Worklist Smp#: 8
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL


1 Perfluorobutanesulfonic acid (ND) 1 Perfluorobutanesulfonic acid (ND) \$ 2 13C2 PFHxA




4 Perfluoroheptanoic acid (ND) 3 Perfluorohexanesulfonic acid (ND) * 6 13C2-PFOA




5 Perfluorooctanoic acid (ND) 5 Perfluorooctanoic acid (ND) 8 Perfluorooctane sulfonic acid (ND)



8 Perfluorooctane sulfonic acid (ND) * 7 13C4 PFOS 9 Perfluorononanoic acid (ND)



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\2018.01.23537A_011.d
 Lims ID: 320-34917-A-11-A
 Client ID: WGNA-010818-FRB-4024
 Sample Type: Client
 Inject. Date: 24-Jan-2018 05:33:54 ALS Bottle#: 18 Worklist Smp#: 8
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-34917-a-11-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 24-Jan-2018 09:58:52 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK024

First Level Reviewer: roycea Date: 24-Jan-2018 09:56:07

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	9.84	98.36
\$ 10 13C2 PFDA	10.0	10.0	100.07

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: WGNA-010818-RW-4844 Lab Sample ID: 320-34917-12
 Matrix: Water Lab File ID: 2018.01.23537A_012.d
 Analysis Method: 537 Date Collected: 01/08/2018 13:10
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 253.5 (mL) Date Analyzed: 01/24/2018 05:38
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 205331 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	7.9	J M	39	16	6.7
335-67-1	Perfluorooctanoic acid (PFOA)	14	J	20	7.9	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	7.9
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	30	12	5.4
375-85-9	Perfluoroheptanoic acid (PFHpA)	7.1	J	9.9	3.9	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	89	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	97		70-130
STL00996	13C2 PFDA	98		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\2018.01.23537A_012.d
 Lims ID: 320-34917-A-12-A
 Client ID: WGNA-010818-RW-4844
 Sample Type: Client
 Inject. Date: 24-Jan-2018 05:38:35 ALS Bottle#: 19 Worklist Smp#: 9
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-34917-a-12-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 24-Jan-2018 09:58:52 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK024

First Level Reviewer: roycea Date: 24-Jan-2018 09:56:49

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.366	1.366	0.0	1.000	143898	1.00		77.0	
298.90 > 99.00	1.366	1.366	0.0	1.000	105709		1.36(0.00-0.00)	126	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.487	1.487	0.0	1.000	1763189	9.69		7739	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.624	1.631	-0.007	1.000	278017	1.79		52.1	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.624	1.631	-0.007	1.000	129117	0.5995		62.6	
* 6 13C2-PFOA									
415.00 > 370.00	1.806	1.813	-0.007		1654396	10.0		6350	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.813	1.813	0.0	1.000	545798	3.56		87.2	
413.00 > 169.00	1.806	1.813	-0.007	0.996	320795		1.70(0.00-0.00)	589	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.056	2.056	0.0	1.000	241497	2.00		83.5	Ma
499.00 > 99.00	2.064	2.056	0.008	1.004	42971		5.62(0.00-0.00)	59.4	M
* 7 13C4 PFOS									
503.00 > 80.00	2.056	2.064	-0.008		3689900	28.7		3608	
9 Perfluorononanoic acid									
463.00 > 419.00	2.071	2.079	-0.008	1.000	80785	0.7352		13.4	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.238	2.246	-0.008	1.000	1245590	9.84		8032	

QC Flag Legend

Review Flags

M - Manually Integrated

a - User Assigned ID




TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\2018.01.23537A_012.d
Injection Date: 24-Jan-2018 05:38:35 Instrument ID: A8_N
Lims ID: 320-34917-A-12-A Lab Sample ID: 320-34917-12
Client ID: WGNA-010818-RW-4844
Operator ID: SACINSTLCMS01 ALS Bottle#: 19 Worklist Smp#: 9
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



4 Perfluoroheptanoic acid

3 Perfluorohexanesulfonic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\2018.01.23537A_012.d
 Lims ID: 320-34917-A-12-A
 Client ID: WGNA-010818-RW-4844
 Sample Type: Client
 Inject. Date: 24-Jan-2018 05:38:35 ALS Bottle#: 19 Worklist Smp#: 9
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-34917-a-12-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 24-Jan-2018 09:58:52 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK024

First Level Reviewer: roycea Date: 24-Jan-2018 09:56:49

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	9.69	96.86
\$ 10 13C2 PFDA	10.0	9.84	98.39

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\2018.01.23537A_012.d
Injection Date: 24-Jan-2018 05:38:35 Instrument ID: A8_N
Lims ID: 320-34917-A-12-A Lab Sample ID: 320-34917-12
Client ID: WGNA-010818-RW-4844
Operator ID: SACINSTLCMS01 ALS Bottle#: 19 Worklist Smp#: 9
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected
Expected RT: 2.06

Processing Integration Results



Manual Integration Results

RT: 2.06
Area: 42971
Amount: 1.999100
Amount Units: ng/ml



Reviewer: roycea, 24-Jan-2018 09:56:19
Audit Action: Manually Integrated

Audit Reason: Assign Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\2018.01.23537A_012.d
Injection Date: 24-Jan-2018 05:38:35 Instrument ID: A8_N
Lims ID: 320-34917-A-12-A Lab Sample ID: 320-34917-12
Client ID: WGNA-010818-RW-4844
Operator ID: SACINSTLCMS01 ALS Bottle#: 19 Worklist Smp#: 9
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.06

Processing Integration Results



RT: 2.06
Area: 241497
Amount: 1.999100
Amount Units: ng/ml

Manual Integration Results



Reviewer: roycea, 24-Jan-2018 09:56:23

Audit Action: Manually Integrated

Audit Reason: Assign Peak

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: WGNA-010818-FRB-4844 Lab Sample ID: 320-34917-13
 Matrix: Water Lab File ID: 2018.01.23537A_013.d
 Analysis Method: 537 Date Collected: 01/08/2018 13:05
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 249.5 (mL) Date Analyzed: 01/24/2018 05:43
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 205331 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	8.0	U	20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.0	U	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	97		70-130
STL00996	13C2 PFDA	97		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\2018.01.23537A_013.d
 Lims ID: 320-34917-A-13-A
 Client ID: WGNA-010818-FRB-4844
 Sample Type: Client
 Inject. Date: 24-Jan-2018 05:43:15 ALS Bottle#: 20 Worklist Smp#: 10
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-34917-a-13-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 24-Jan-2018 09:58:52 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK024


First Level Reviewer: roycea Date: 24-Jan-2018 09:57:02

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
\$ 2 13C2 PFHxA	315.00 > 270.00	1.487	1.487	0.0	1.000	1653991	9.65	7784	
* 6 13C2-PFOA	415.00 > 370.00	1.813	1.813	0.0		1557173	10.0	6618	
* 7 13C4 PFOS	503.00 > 80.00	2.064	2.064	0.0		3476391	28.7	6690	
\$ 10 13C2 PFDA	515.00 > 470.00	2.246	2.246	0.0	1.000	1156963	9.71	7270	


TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\2018.01.23537A_013.d
Injection Date: 24-Jan-2018 05:43:15 Instrument ID: A8_N
Lims ID: 320-34917-A-13-A Lab Sample ID: 320-34917-13
Client ID: WGNA-010818-FRB-4844
Operator ID: SACINSTLCMS01 ALS Bottle#: 20 Worklist Smp#: 10
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL


1 Perfluorobutanesulfonic acid (ND) 1 Perfluorobutanesulfonic acid (ND) \$ 2 13C2 PFHxA




4 Perfluoroheptanoic acid (ND) 3 Perfluorohexanesulfonic acid (ND) * 6 13C2-PFOA




5 Perfluorooctanoic acid (ND) 5 Perfluorooctanoic acid (ND) 8 Perfluorooctane sulfonic acid (ND)



8 Perfluorooctane sulfonic acid (ND) * 7 13C4 PFOS 9 Perfluorononanoic acid (ND)



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\2018.01.23537A_013.d
 Lims ID: 320-34917-A-13-A
 Client ID: WGNA-010818-FRB-4844
 Sample Type: Client
 Inject. Date: 24-Jan-2018 05:43:15 ALS Bottle#: 20 Worklist Smp#: 10
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-34917-a-13-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 24-Jan-2018 09:58:52 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK024

First Level Reviewer: roycea Date: 24-Jan-2018 09:57:02

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	9.65	96.54
\$ 10 13C2 PFDA	10.0	9.71	97.10

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: WGNA-010818-RW-0404 Lab Sample ID: 320-34917-14
 Matrix: Water Lab File ID: 2018.01.23537A_014.d
 Analysis Method: 537 Date Collected: 01/08/2018 09:40
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 249.4 (mL) Date Analyzed: 01/24/2018 05:47
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 205331 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	26	J M	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	21		20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	8.3	J	30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	6.3	J	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	96		70-130
STL00996	13C2 PFDA	100		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\2018.01.23537A_014.d
 Lims ID: 320-34917-A-14-A
 Client ID: WGNA-010818-RW-0404
 Sample Type: Client
 Inject. Date: 24-Jan-2018 05:47:56 ALS Bottle#: 21 Worklist Smp#: 11
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-34917-a-14-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 24-Jan-2018 09:58:52 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK024

First Level Reviewer: roycea Date: 24-Jan-2018 09:57:51

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.358	1.366	-0.008	1.000	175064	1.32		109	
298.90 > 99.00	1.358	1.366	-0.008	1.000	127796		1.37(0.00-0.00)	158	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.479	1.487	-0.008	1.000	1660117	9.62		7637	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.624	1.631	-0.007	1.000	231832	1.58		47.8	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.624	1.631	-0.007	1.000	411468	2.06		227	
* 6 13C2-PFOA									
415.00 > 370.00	1.806	1.813	-0.007		1567961	10.0		5944	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.806	1.813	-0.007	1.000	767825	5.29		125	
413.00 > 169.00	1.806	1.813	-0.007	1.000	458176		1.68(0.00-0.00)	850	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.056	2.056	0.0	1.000	711598	6.37		221	a
499.00 > 99.00	2.056	2.056	0.0	1.000	140322		5.07(0.00-0.00)	225	a
* 7 13C4 PFOS									
503.00 > 80.00	2.056	2.064	-0.008		3414209	28.7		3454	
9 Perfluorononanoic acid									
463.00 > 419.00	2.064	2.079	-0.015	1.000	61789	0.5933		10.4	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.238	2.246	-0.008	1.000	1203401	10.0		8190	

QC Flag Legend

Review Flags

a - User Assigned ID


TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\2018.01.23537A_014.d
Injection Date: 24-Jan-2018 05:47:56 Instrument ID: A8_N
Lims ID: 320-34917-A-14-A Lab Sample ID: 320-34917-14
Client ID: WGNA-010818-RW-0404
Operator ID: SACINSTLCMS01 ALS Bottle#: 21 Worklist Smp#: 11
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid


\$ 2 13C2 PFHxA



4 Perfluoroheptanoic acid

3 Perfluorohexanesulfonic acid


* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid


8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\2018.01.23537A_014.d
 Lims ID: 320-34917-A-14-A
 Client ID: WGNA-010818-RW-0404
 Sample Type: Client
 Inject. Date: 24-Jan-2018 05:47:56 ALS Bottle#: 21 Worklist Smp#: 11
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-34917-a-14-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 24-Jan-2018 09:58:52 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK024

First Level Reviewer: roycea Date: 24-Jan-2018 09:57:51

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	9.62	96.23
\$ 10 13C2 PFDA	10.0	10.0	100.30

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\2018.01.23537A_014.d
Injection Date: 24-Jan-2018 05:47:56 Instrument ID: A8_N
Lims ID: 320-34917-A-14-A Lab Sample ID: 320-34917-14
Client ID: WGNA-010818-RW-0404
Operator ID: SACINSTLCMS01 ALS Bottle#: 21 Worklist Smp#: 11
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.06

Processing Integration Results



RT: 2.06
Area: 711598
Amount: 6.366224
Amount Units: ng/ml

Manual Integration Results



FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: WGNA-010818-FRB-0404 Lab Sample ID: 320-34917-15
 Matrix: Water Lab File ID: 2018.01.23537A_015.d
 Analysis Method: 537 Date Collected: 01/08/2018 09:35
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 252.5 (mL) Date Analyzed: 01/24/2018 05:52
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 205331 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	40	16	6.7
335-67-1	Perfluorooctanoic acid (PFOA)	7.9	U	20	7.9	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	7.9
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	30	12	5.4
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.0	U	9.9	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	89	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	103		70-130
STL00996	13C2 PFDA	103		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\2018.01.23537A_015.d
 Lims ID: 320-34917-A-15-A
 Client ID: WGNA-010818-FRB-0404
 Sample Type: Client
 Inject. Date: 24-Jan-2018 05:52:37 ALS Bottle#: 22 Worklist Smp#: 12
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-34917-a-15-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 24-Jan-2018 09:58:52 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK024

First Level Reviewer: roycea Date: 24-Jan-2018 09:58:13

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
\$ 2 13C2 PFHxA	315.00 > 270.00	1.479	1.487	-0.008	1.000	1778722	10.3	9201	
* 6 13C2-PFOA	415.00 > 370.00	1.806	1.813	-0.007		1573488	10.0	5997	
* 7 13C4 PFOS	503.00 > 80.00	2.056	2.064	-0.008		3522216	28.7	7497	
\$ 10 13C2 PFDA	515.00 > 470.00	2.238	2.246	-0.008	1.000	1242097	10.3	8152	

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\2018.01.23537A_015.d

Injection Date: 24-Jan-2018 05:52:37

Instrument ID: A8_N

Lims ID: 320-34917-A-15-A

Lab Sample ID: 320-34917-15

Client ID: WGNA-010818-FRB-0404

Operator ID: SACINSTLCMS01

ALS Bottle#: 22

Worklist Smp#: 12

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid (ND)

1 Perfluorobutanesulfonic acid (ND)




\$ 2 13C2 PFHxA



4 Perfluoroheptanoic acid (ND)

3 Perfluorohexanesulfonic acid (ND)




* 6 13C2-PFOA



5 Perfluorooctanoic acid (ND)




5 Perfluorooctanoic acid (ND)

8 Perfluorooctane sulfonic acid (ND)




8 Perfluorooctane sulfonic acid (ND) * 7 13C4 PFOS

9 Perfluorononanoic acid (ND)



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\2018.01.23537A_015.d
 Lims ID: 320-34917-A-15-A
 Client ID: WGNA-010818-FRB-0404
 Sample Type: Client
 Inject. Date: 24-Jan-2018 05:52:37 ALS Bottle#: 22 Worklist Smp#: 12
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-34917-a-15-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 24-Jan-2018 09:58:52 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK024

First Level Reviewer: roycea Date: 24-Jan-2018 09:58:13

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	10.3	102.74
\$ 10 13C2 PFDA	10.0	10.3	103.16

FORM VI
LCMS BY INTERNAL STANDARD - INITIAL CALIBRATION DATA
CURVE EVALUATION

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1 Analy Batch No.: 192908

SDG No.: _____

Instrument ID: A8_N GC Column: GeminiC18 3 ID: 3(mm) Heated Purge: (Y/N) N

Calibration Start Date: 11/03/2017 13:37 Calibration End Date: 11/03/2017 14:01 Calibration ID: 36012

Calibration Files:

LEVEL:	LAB SAMPLE ID:	LAB FILE ID:
Level 1	IC 320-192908/4	2017.11.03_537XICAL_004.d
Level 2	IC 320-192908/5	2017.11.03_537XICAL_005.d
Level 3	IC 320-192908/6	2017.11.03_537XICAL_006.d
Level 4	IC 320-192908/7	2017.11.03_537XICAL_007.d
Level 5	IC 320-192908/8	2017.11.03_537XICAL_008.d
Level 6	IC 320-192908/9	2017.11.03_537XICAL_009.d

ANALYTE	RRF					CURVE TYPE	COEFFICIENT			#	MIN RRF	%RSD	#	MAX %RSD	R ² OR COD	#	MIN R ² OR COD
	LVL 1 LVL 6	LVL 2	LVL 3	LVL 4	LVL 5		B	M1	M2								
Perfluorobutanesulfonic acid (PFBS)	1.0397 0.8468	1.0767	1.0898	0.9577	0.9303	QuaF		1.1193	-0.001498					0.9990			0.9600
Perfluoroheptanoic acid (PFHpA)	0.9433 0.9848	0.9187	0.9551	0.9185	0.9011	Ave		0.9369			3.2		30.0				
Perfluorohexanesulfonic acid (PFHxS)	1.6459 1.6841	1.6355	1.7405	1.6631	1.6755	Ave		1.6741			2.2		30.0				
Perfluorooctanoic acid (PFOA)	0.9757 0.9799	0.8919	0.9000	0.8953	0.9117	Ave		0.9258			4.4		30.0				
Perfluorooctanesulfonic acid (PFOS)	0.8958 0.9902	0.9213	0.9281	0.9268	0.9715	Ave		0.9389			3.7		30.0				
Perfluorononanoic acid (PFNA)	0.6610 0.7042	0.6285	0.6624	0.6810	0.6478	Ave		0.6642			3.9		30.0				
13C2 PFHxA	1.0891 1.1664	1.0526	1.1042	1.1123	1.0772	Ave		1.1003			3.5		30.0				
13C2 PFDA	0.7748 0.8159	0.7295	0.7569	0.7811	0.7330	Ave		0.7652			4.3		30.0				

Note: The M1 coefficient is the same as Ave RRF for an Ave curve type.

FORM VI
LCMS BY INTERNAL STANDARD - INITIAL CALIBRATION DATA
RESPONSE AND CONCENTRATION

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1 Analy Batch No.: 192908

SDG No.: _____

Instrument ID: A8_N GC Column: GeminiC18 3 ID: 3(mm) Heated Purge: (Y/N) N

Calibration Start Date: 11/03/2017 13:37 Calibration End Date: 11/03/2017 14:01 Calibration ID: 36012

Calibration Files:

LEVEL:	LAB SAMPLE ID:	LAB FILE ID:
Level 1	IC 320-192908/4	2017.11.03_537XICAL_004.d
Level 2	IC 320-192908/5	2017.11.03_537XICAL_005.d
Level 3	IC 320-192908/6	2017.11.03_537XICAL_006.d
Level 4	IC 320-192908/7	2017.11.03_537XICAL_007.d
Level 5	IC 320-192908/8	2017.11.03_537XICAL_008.d
Level 6	IC 320-192908/9	2017.11.03_537XICAL_009.d

ANALYTE	IS REF	CURVE TYPE	RESPONSE					CONCENTRATION (NG/ML)				
			LVL 1 LVL 6	LVL 2	LVL 3	LVL 4	LVL 5	LVL 1 LVL 6	LVL 2	LVL 3	LVL 4	LVL 5
Perfluorobutanesulfonic acid (PFBS)	PFOS	QuaF	1076553 16699152	2591121	5461974	10142530	14011858	9.00 180	20.0	45.0	90.0	135
Perfluoroheptanoic acid (PFHpA)	13PF OA	Ave	143455 2810797	331548	736034	1420703	2102676	1.00 20.0	2.22	5.00	10.0	15.0
Perfluorohexanesulfonic acid (PFHxS)	PFOS	Ave	568156 11071993	1312135	2908204	5871843	8413133	3.00 60.0	6.67	15.0	30.0	45.0
Perfluorooctanoic acid (PFOA)	13PF OA	Ave	296934 5597122	644149	1388033	2771271	4257225	2.00 40.0	4.45	10.0	20.0	30.0
Perfluorooctanesulfonic acid (PFOS)	PFOS	Ave	412315 8679676	985487	2067792	4363079	6504279	4.00 80.0	8.89	20.0	40.0	60.0
Perfluorononanoic acid (PFNA)	13PF OA	Ave	201053 4019666	453612	1020851	2106479	3023088	2.00 40.0	4.45	10.0	20.0	30.0
13C2 PFHxA	13PF OA	Ave	1655691 1664260	1708988	1701491	1719911	1675220	10.0 10.0	10.0	10.0	10.0	10.0
13C2 PFDA	13PF OA	Ave	1177922 1164156	1184358	1166275	1207887	1139992	10.0 10.0	10.0	10.0	10.0	10.0

Curve Type Legend:

Ave = Average ISTD
QuaF = Quadratic ISTD forced zero

FORM VI
 LCMS BY INTERNAL STANDARD - INITIAL CALIBRATION DATA
 READBACK PERCENT ERROR

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1 Analy Batch No.: 192908

SDG No.: _____


Instrument ID: A8_N GC Column: GeminiC18 3 ID: 3 (mm) Heated Purge: (Y/N) N


Calibration Start Date: 11/03/2017 13:37 Calibration End Date: 11/03/2017 14:01 Calibration ID: 36012

Calibration Files:

LEVEL:	LAB SAMPLE ID:	LAB FILE ID:
Level 1	IC 320-192908/4	2017.11.03_537XICAL_004.d
Level 2	IC 320-192908/5	2017.11.03_537XICAL_005.d
Level 3	IC 320-192908/6	2017.11.03_537XICAL_006.d
Level 4	IC 320-192908/7	2017.11.03_537XICAL_007.d
Level 5	IC 320-192908/8	2017.11.03_537XICAL_008.d
Level 6	IC 320-192908/9	2017.11.03_537XICAL_009.d

ANALYTE	PERCENT ERROR						PERCENT ERROR LIMIT					
	LVL 1 #	LVL 2 #	LVL 3 #	LVL 4 #	LVL 5 #	LVL 6 #	LVL 1	LVL 2	LVL 3	LVL 4	LVL 5	LVL 6
Perfluorobutanesulfonic acid (PFBS)	-6.0	-1.2	3.9	-3.1	1.9	-0.5	50	30	30	30	30	30
Perfluoroheptanoic acid (PFHpA)	0.7	-1.9	1.9	-2.0	-3.8	5.1	50	30	30	30	30	30
Perfluorohexanesulfonic acid (PFHxS)	-1.7	-2.3	4.0	-0.7	0.1	0.6	50	30	30	30	30	30
Perfluorooctanoic acid (PFOA)	5.4	-3.7	-2.8	-3.3	-1.5	5.8	50	30	30	30	30	30
Perfluorooctanesulfonic acid (PFOS)	-4.6	-1.9	-1.2	-1.3	3.5	5.5	50	30	30	30	30	30
Perfluorononanoic acid (PFNA)	-0.5	-5.4	-0.3	2.5	-2.5	6.0	50	30	30	30	30	30
13C2 PFHxA	-1.0	-4.3	0.4	1.1	-2.1	6.0	30	30	30	30	30	30
13C2 PFDA	1.3	-4.7	-1.1	2.1	-4.2	6.6	30	30	30	30	30	30





TestAmerica Laboratories
Istd/Surrogate Recovery Report

Worklist Name: 03NOV2017_537A_ICAL

Worklist Num: 49975

Instrument: A8_N

Method: 537_A8_N

Batch Directory: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b

Limit Group: LC 537 ICAL

Analysis Type: SemiVOA

Inj Volume: 2.00

Inj Vol Units: ul

Lims Batch: 192908

CCV IS Mode: Select Ical Level, Cal Level: 3

Non-Cal IS Mode: Last Ccal Sample

\$ 2 13C2 PFHxA

\$ 10 13C2 PFDA

Lab ID	Inj Date	\$ 2	\$ 10	* 6 13C2-PFOA	* 7 13C4 PFOS
	IS Std			2864400 1.87	6253426 2.11
# 1 RB	03-Nov-2017 13:23:59			1485386 51.9	3471256 55.5
# 2 RB	03-Nov-2017 13:28:38			1511056 52.8	3340239 53.4
# 3 RB	03-Nov-2017 13:33:19			1483949 51.8	3285228 52.5
	IS Std				
# 4 IC L1	03-Nov-2017 13:37:59	1.58 98.98	2.31 101.30	1520258> 100.0*	3298877> 100.0*
# 5 IC L2	03-Nov-2017 13:42:39	1.58 95.66	2.31 95.33	1623614> 106.8*	3450592> 104.6*
# 6 IC L3	03-Nov-2017 13:47:20	1.57 100.40	2.31 98.91	1540946> 101.4*	3194016> 96.8*
# 7 IC L4	03-Nov-2017 13:52:00	1.57 101.10	2.31 102.10	1546307> 101.7*	3374600> 102.3*
# 8 IC L5	03-Nov-2017 13:56:41	1.57 97.90	2.31 95.80	1555174> 102.3*	3199479> 97.0*
# 9 IC L6	03-Nov-2017 14:01:24	1.57 106.00	2.31 106.60	1426806> 93.9*	3141787> 95.2*
	IS Std			1540946 1.91	3194016 2.15
#10 RB	03-Nov-2017 14:06:04			1395383 90.6	3212781 100.6
	IS Std			1546307 1.91	3374600 2.16
#11 CCVL	03-Nov-2017 14:10:44	1.58 97.03	2.31 97.49	1586829 102.6	3305852 98.0
	IS Std			1586829 1.91	3305852 2.15
#12 RB	03-Nov-2017 14:15:23			1415042 89.2	3122656 94.5
	IS Std			1546307 1.91	3374600 2.16
#13 ICV	03-Nov-2017 14:20:03	1.57 94.41	2.31 96.59	1512045 97.8	3433628 101.7
	IS Std			1395100 1.91	3254950 2.15
#14 RB	03-Nov-2017 14:24:44			1395100 100.0	3254950 100.0

13C2-PFOA

$$RPD = \frac{1623614 - 1426806}{\left(\frac{1623614 + 1426806}{2}\right)} (100) = 12.9$$

13C4-PFOS

$$RPD = \frac{3450592 - 3141787}{\left(\frac{3450592 + 3141787}{2}\right)} (100) = 9.37$$

JRB
11-6-17

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_004.d
 Lims ID: IC L1
 Client ID:
 Sample Type: IC Calib Level: 1
 Inject. Date: 03-Nov-2017 13:37:59 ALS Bottle#: 1 Worklist Smp#: 4
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: L1_537
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub1

Method: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Nov-2017 15:52:07 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK021

First Level Reviewer: phomsophat Date: 06-Nov-2017 07:18:01

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.449	1.444	0.005	1.000	1076553	8.46		654	
298.90 > 99.00	1.449	1.444	0.005	1.000	763262		1.41(0.00-0.00)	2025	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.578	1.573	0.005	1.000	1655691	9.90		8732	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.730	1.725	0.005	1.000	568156	2.95		1122	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.730	1.725	0.005	1.000	143455	1.01		42.2	
* 6 13C2-PFOA									
415.00 > 370.00	1.920	1.913	0.007		1520258	10.0		6863	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.920	1.914	0.006	1.000	296934	2.11		53.5	
413.00 > 169.00	1.920	1.914	0.006	1.000	149720		1.98(0.00-0.00)	184	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.155	2.147	0.008	1.000	412315	3.82		235	M
499.00 > 99.00	2.155	2.147	0.008	1.000	85347		4.83(0.00-0.00)	209	M
* 7 13C4 PFOS									
503.00 > 80.00	2.155	2.151	0.004		3298877	28.7		5279	
9 Perfluorononanoic acid									
463.00 > 419.00	2.162	2.158	0.004	1.000	201053	1.99		67.8	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.314	2.312	0.002	1.000	1177922	10.1		7012	

QC Flag Legend

Review Flags

M - Manually Integrated

Reagents:

LC537-L1_00020

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537ICAL_004.d

Injection Date: 03-Nov-2017 13:37:59

Instrument ID: A8_N

Lims ID: IC L1

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 1

Worklist Smp#: 4

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA

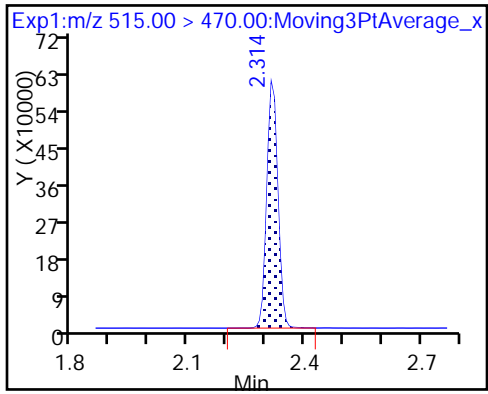

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_004.d
Injection Date: 03-Nov-2017 13:37:59 Instrument ID: A8_N
Lims ID: IC L1
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 1 Worklist Smp#: 4
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.15

Processing Integration Results

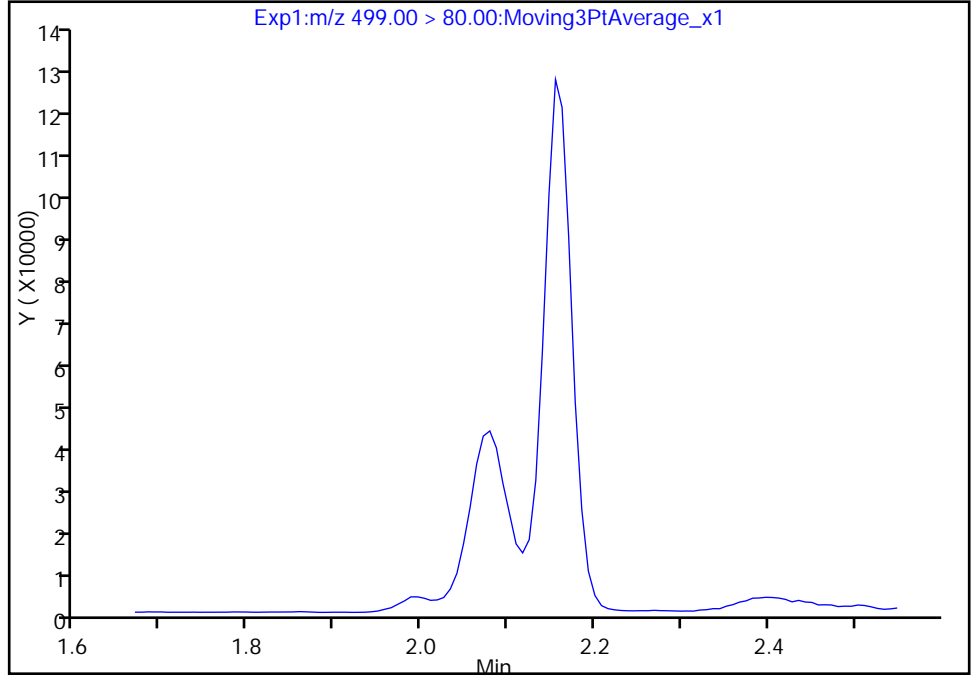

Manual Integration Results

RT: 2.15
Area: 412315
Amount: 3.817687
Amount Units: ng/ml



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\201711106-49975.b\2017.11.03_537XICAL_004.d
Injection Date: 03-Nov-2017 13:37:59 Instrument ID: A8_N
Lims ID: IC L1
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 1 Worklist Smp#: 4
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected
Expected RT: 2.15

Processing Integration Results

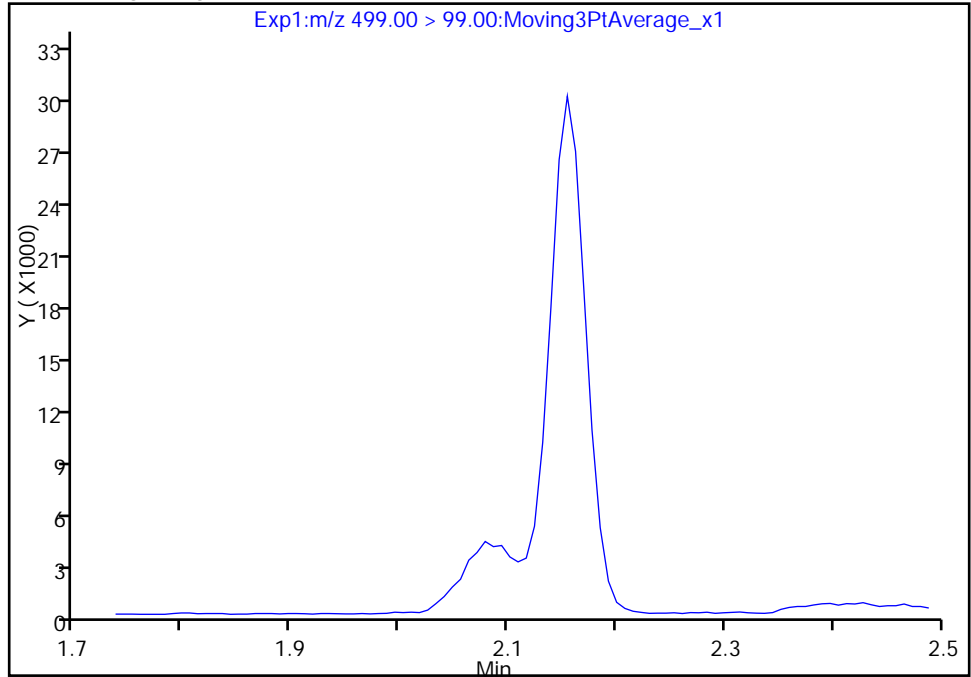

Manual Integration Results

RT: 2.15
Area: 85347
Amount: 3.817687
Amount Units: ng/ml

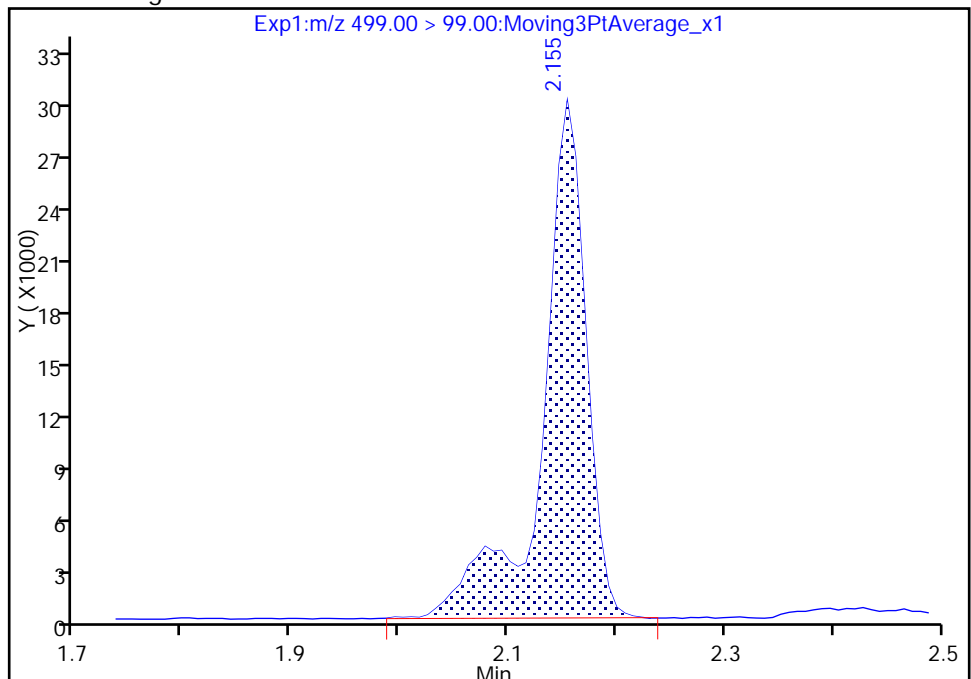

Reviewer: phomsophat, 06-Nov-2017 07:17:37

Audit Action: Manually Integrated

Audit Reason: Assign Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\201711106-49975.b\2017.11.03_537XICAL_004.d
Injection Date: 03-Nov-2017 13:37:59 Instrument ID: A8_N
Lims ID: IC L1
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 1 Worklist Smp#: 4
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.15

Processing Integration Results



Manual Integration Results

RT: 2.15
Area: 412315
Amount: 3.817687
Amount Units: ng/ml



TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_005.d
 Lims ID: IC L2
 Client ID:
 Sample Type: IC Calib Level: 2
 Inject. Date: 03-Nov-2017 13:42:39 ALS Bottle#: 2 Worklist Smp#: 5
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: L2_537
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub1

Method: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Nov-2017 15:52:08 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK021

First Level Reviewer: phomsophat Date: 06-Nov-2017 07:18:56

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.449	1.444	0.005	1.000	2591121	19.8		1479	
298.90 > 99.00	1.442	1.444	-0.002	0.995	1874928		1.38(0.00-0.00)	4315	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.578	1.573	0.005	1.000	1708988	9.57		8562	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.730	1.725	0.005	1.000	331548	2.18		87.8	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.730	1.725	0.005	1.000	1312135	6.51		2317	
* 6 13C2-PFOA									
415.00 > 370.00	1.920	1.913	0.007		1623614	10.0		6970	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.920	1.914	0.006	1.000	644149	4.29		113	
413.00 > 169.00	1.920	1.914	0.006	1.000	329479		1.96(0.00-0.00)	459	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.155	2.147	0.008	1.000	985487	8.72		578	M
499.00 > 99.00	2.155	2.147	0.008	1.000	200739		4.91(0.00-0.00)	449	M
* 7 13C4 PFOS									
503.00 > 80.00	2.155	2.151	0.004		3450592	28.7		5334	
9 Perfluorononanoic acid									
463.00 > 419.00	2.162	2.158	0.004	1.000	453612	4.21		136	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.314	2.312	0.002	1.000	1184358	9.53		7573	

QC Flag Legend

Review Flags

M - Manually Integrated

Reagents:

LC537-L2_00020

Amount Added: 1.00

Units: mL

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_005.d

Injection Date: 03-Nov-2017 13:42:39

Instrument ID: A8_N

Lims ID: IC L2

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 2

Worklist Smp#: 5

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



4 Perfluoroheptanoic acid

3 Perfluorohexanesulfonic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_005.d
Injection Date: 03-Nov-2017 13:42:39 Instrument ID: A8_N
Lims ID: IC L2
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 2 Worklist Smp#: 5
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.15

Processing Integration Results

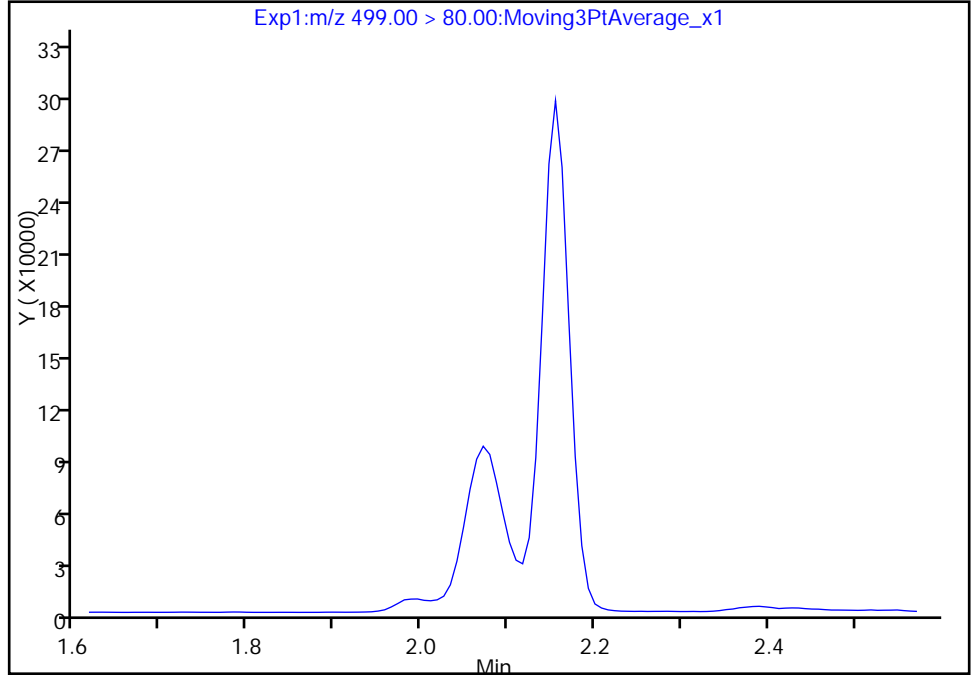

RT: 2.15
Area: 985487
Amount: 8.723576
Amount Units: ng/ml

Manual Integration Results

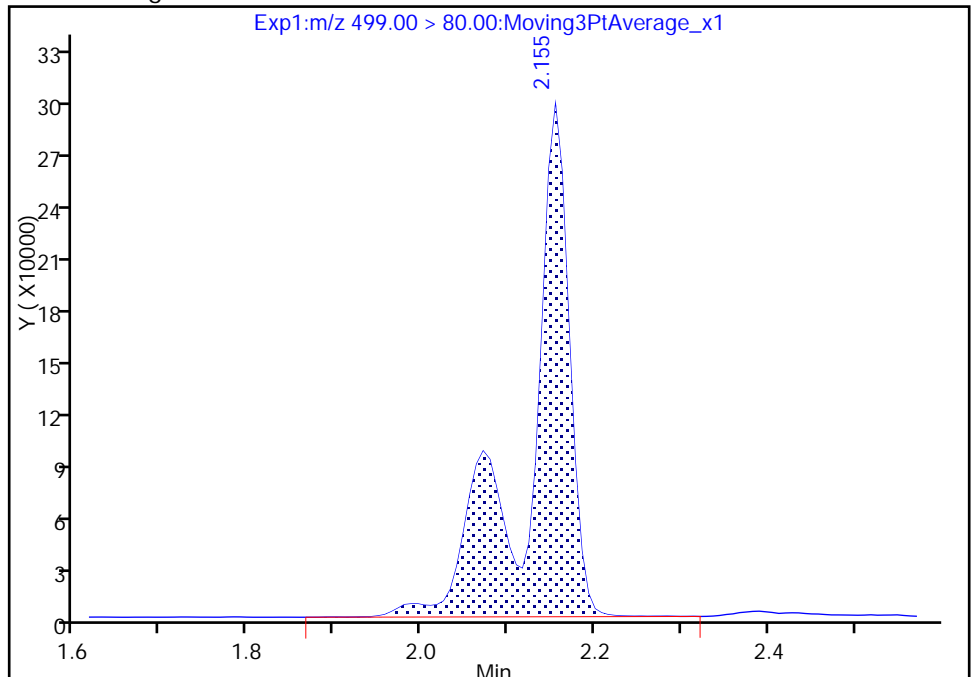

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\201711106-49975.b\2017.11.03_537XICAL_005.d
Injection Date: 03-Nov-2017 13:42:39 Instrument ID: A8_N
Lims ID: IC L2
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 2 Worklist Smp#: 5
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected
Expected RT: 2.15

Processing Integration Results

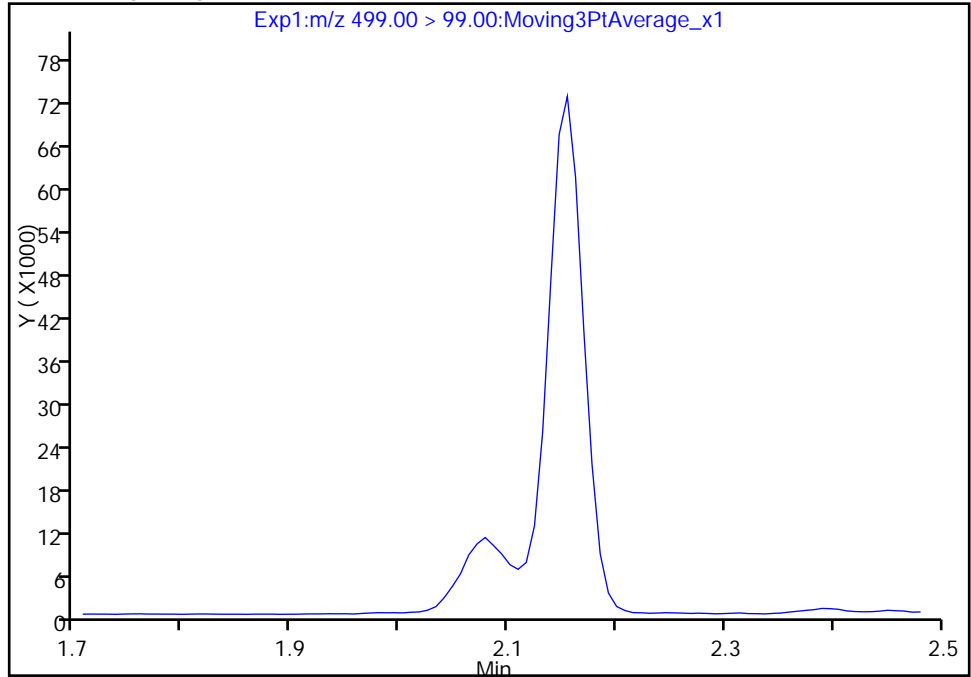

RT: 2.15
Area: 200739
Amount: 8.723576
Amount Units: ng/ml

Manual Integration Results

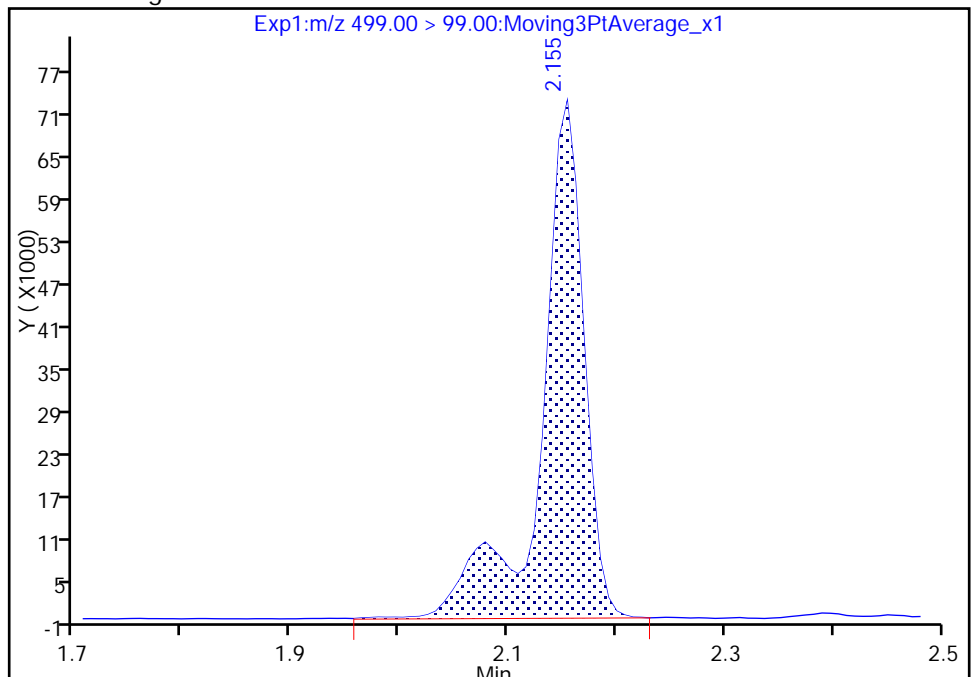

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\201711106-49975.b\2017.11.03_537XICAL_005.d
Injection Date: 03-Nov-2017 13:42:39 Instrument ID: A8_N
Lims ID: IC L2
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 2 Worklist Smp#: 5
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.15

Processing Integration Results

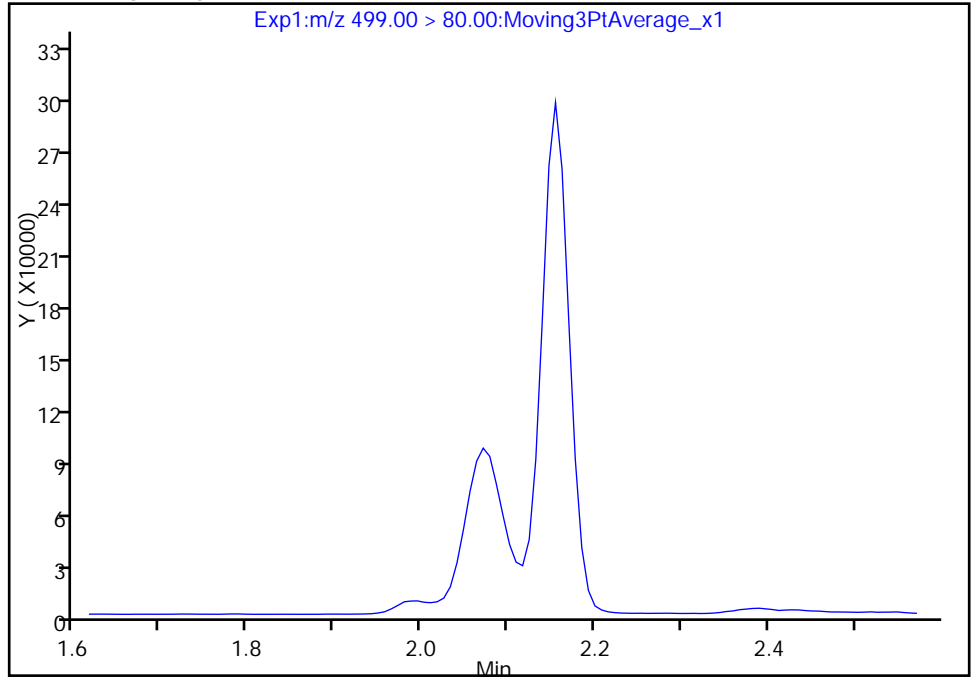

RT: 2.15
Area: 985487
Amount: 8.723576
Amount Units: ng/ml

Manual Integration Results



Reviewer: phomsophat, 06-Nov-2017 07:18:24

Audit Action: Manually Integrated

Audit Reason: Assign Peak

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_006.d
 Lims ID: IC L3
 Client ID:
 Sample Type: IC Calib Level: 3
 Inject. Date: 03-Nov-2017 13:47:20 ALS Bottle#: 3 Worklist Smp#: 6
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: L3_537
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub1

Method: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Nov-2017 15:52:09 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK021

First Level Reviewer: phomsophat Date: 06-Nov-2017 07:20:04

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.442	1.444	-0.002	1.000	5461974	46.7		3220	
298.90 > 99.00	1.442	1.444	-0.002	1.000	3903438		1.40(0.00-0.00)	8589	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.571	1.573	-0.003	1.000	1701491	10.0		9021	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.722	1.725	-0.003	1.000	2908204	15.6		5000	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.722	1.725	-0.003	1.000	736034	5.10		208	
* 6 13C2-PFOA									
415.00 > 370.00	1.912	1.913	-0.001		1540946	10.0		6787	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.912	1.914	-0.002	1.000	1388033	9.73		256	
413.00 > 169.00	1.912	1.914	-0.002	1.000	715399		1.94(0.00-0.00)	904	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.147	2.147	0.0	1.000	2067792	19.8		2001	
499.00 > 99.00	2.147	2.147	0.0	1.000	431075		4.80(0.00-0.00)	922	
* 7 13C4 PFOS									
503.00 > 80.00	2.147	2.151	-0.004		3194016	28.7		4956	
9 Perfluorononanoic acid									
463.00 > 419.00	2.155	2.158	-0.003	1.000	1020851	9.97		302	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.306	2.312	-0.006	1.000	1166275	9.89		6310	

Reagents:

LC537-L3_00023

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537ICAL_006.d

Injection Date: 03-Nov-2017 13:47:20

Instrument ID: A8_N

Lims ID: IC L3

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 3

Worklist Smp#: 6

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid

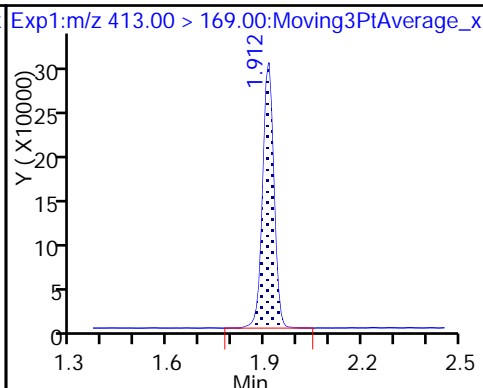


8 Perfluorooctane sulfonic acid

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_007.d
 Lims ID: IC L4
 Client ID:
 Sample Type: ICISAV Calib Level: 4
 Inject. Date: 03-Nov-2017 13:52:00 ALS Bottle#: 4 Worklist Smp#: 7
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: L4_537
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub1

Method: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Nov-2017 15:52:10 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK021

First Level Reviewer: phomsophat Date: 06-Nov-2017 07:20:46

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.442	1.444	-0.002	1.000	10142530	87.2		5274	
298.90 > 99.00	1.442	1.444	-0.002	1.000	7408390		1.37(0.00-0.00)	12862	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.571	1.573	-0.003	1.000	1719911	10.1		8503	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.722	1.725	-0.003	1.000	1420703	9.81		399	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.722	1.725	-0.003	1.000	5871843	29.8		7622	
* 6 13C2-PFOA									
415.00 > 370.00	1.912	1.913	-0.001		1546307	10.0		6563	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.912	1.914	-0.002	1.000	2771271	19.4		505	
413.00 > 169.00	1.912	1.914	-0.002	1.000	1520933		1.82(0.00-0.00)	1919	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.155	2.147	0.008	1.000	4363079	39.5		3896	M
499.00 > 99.00	2.155	2.147	0.008	1.000	902486		4.83(0.00-0.00)	1588	M
* 7 13C4 PFOS									
503.00 > 80.00	2.155	2.151	0.004		3374600	28.7		5331	
9 Perfluorononanoic acid									
463.00 > 419.00	2.162	2.158	0.004	1.000	2106479	20.5		638	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.314	2.312	0.002	1.000	1207887	10.2		7165	

QC Flag Legend

Review Flags

M - Manually Integrated

Reagents:

LC537-L4_00020

Amount Added: 1.00

Units: mL

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537ICAL_007.d

Injection Date: 03-Nov-2017 13:52:00

Instrument ID: A8_N

Lims ID: IC L4

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 4

Worklist Smp#: 7

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



4 Perfluoroheptanoic acid

3 Perfluorohexanesulfonic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA

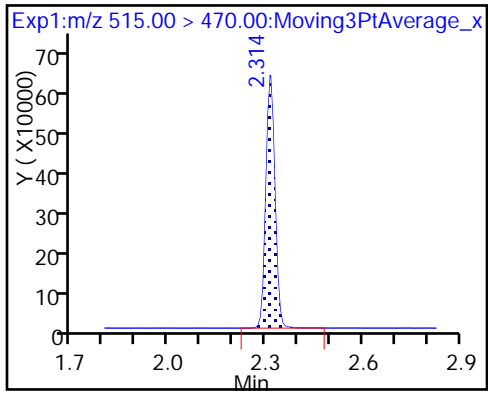

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_007.d
Injection Date: 03-Nov-2017 13:52:00 Instrument ID: A8_N
Lims ID: IC L4
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 4 Worklist Smp#: 7
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.15

Processing Integration Results



Manual Integration Results

RT: 2.15
Area: 4363079
Amount: 39.491903
Amount Units: ng/ml



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\201711106-49975.b\2017.11.03_537XICAL_007.d
Injection Date: 03-Nov-2017 13:52:00 Instrument ID: A8_N
Lims ID: IC L4
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 4 Worklist Smp#: 7
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected
Expected RT: 2.15

Processing Integration Results

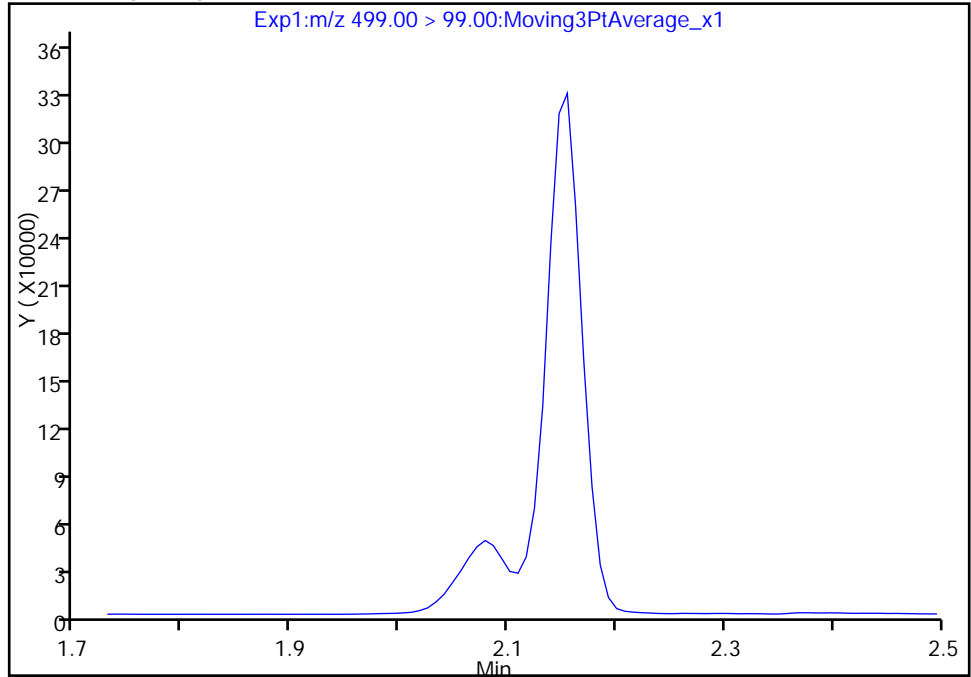

Manual Integration Results

RT: 2.15
Area: 902486
Amount: 39.491903
Amount Units: ng/ml

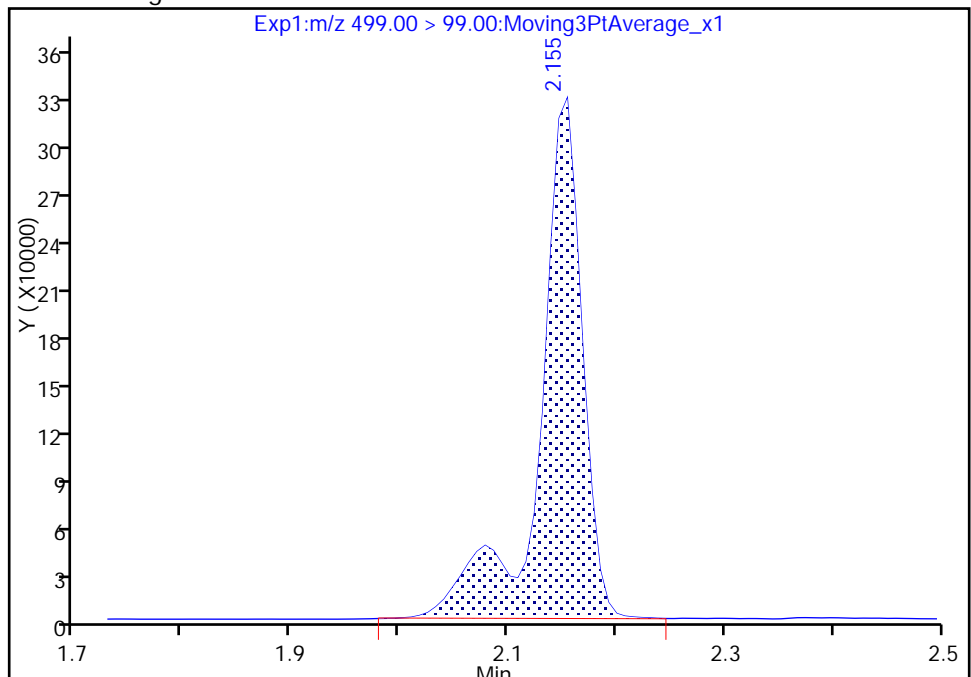

Reviewer: phomsophat, 06-Nov-2017 07:20:20

Audit Action: Manually Integrated

Audit Reason: Assign Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\201711106-49975.b\2017.11.03_537XICAL_007.d
Injection Date: 03-Nov-2017 13:52:00 Instrument ID: A8_N
Lims ID: IC L4
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 4 Worklist Smp#: 7
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.15

Processing Integration Results



RT: 2.15
Area: 4363079
Amount: 39.491903
Amount Units: ng/ml

Manual Integration Results



Reviewer: phomsophat, 06-Nov-2017 07:20:20

Audit Action: Manually Integrated

Audit Reason: Assign Peak

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_008.d
 Lims ID: IC L5
 Client ID:
 Sample Type: IC Calib Level: 5
 Inject. Date: 03-Nov-2017 13:56:41 ALS Bottle#: 5 Worklist Smp#: 8
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: L5_537
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub1

Method: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Nov-2017 15:52:11 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK021

First Level Reviewer: phomsophat Date: 06-Nov-2017 07:21:19

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.442	1.444	-0.002	1.000	14011858	137.5		6452	
298.90 > 99.00	1.442	1.444	-0.002	1.000	10411479		1.35(0.00-0.00)	14800	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.571	1.573	-0.003	1.000	1675220	9.79		9525	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.722	1.725	-0.003	1.000	8413133	45.0		9078	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.722	1.725	-0.003	1.000	2102676	14.4		562	
* 6 13C2-PFOA									
415.00 > 370.00	1.912	1.913	-0.001		1555174	10.0		6769	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.912	1.914	-0.002	1.000	4257225	29.6		800	
413.00 > 169.00	1.912	1.914	-0.002	1.000	2294552		1.86(0.00-0.00)	2838	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.147	2.147	0.0	1.000	6504279	62.1		5682	
499.00 > 99.00	2.147	2.147	0.0	1.000	1339120		4.86(0.00-0.00)	2329	
* 7 13C4 PFOS									
503.00 > 80.00	2.147	2.151	-0.004		3199479	28.7		4946	
9 Perfluorononanoic acid									
463.00 > 419.00	2.155	2.158	-0.003	1.000	3023088	29.3		870	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.314	2.312	0.002	1.000	1139992	9.58		5885	

Reagents:

LC537-L5_00024

Amount Added: 1.00

Units: mL

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_008.d

Injection Date: 03-Nov-2017 13:56:41

Instrument ID: A8_N

Lims ID: IC L5

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 5

Worklist Smp#: 8

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid




8 Perfluorooctane sulfonic acid

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Lims ID: IC L6
 Client ID:
 Sample Type: IC Calib Level: 6
 Inject. Date: 03-Nov-2017 14:01:24 ALS Bottle#: 6 Worklist Smp#: 9
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: L6_537
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub1

Method: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Nov-2017 15:52:12 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK021

First Level Reviewer: phomsophat Date: 06-Nov-2017 07:25:41

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.442	1.444	-0.002	1.000	16699152	179.1		7089	
298.90 > 99.00	1.442	1.444	-0.002	1.000	12929978		1.29(0.00-0.00)	15608	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.571	1.573	-0.003	1.000	1664260	10.6		9116	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.722	1.725	-0.003	1.000	2810797	21.0		763	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.722	1.725	-0.003	1.000	11071993	60.4		10884	
* 6 13C2-PFOA									
415.00 > 370.00	1.904	1.913	-0.009		1426806	10.0		5446	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.912	1.914	-0.002	1.000	5597122	42.4		962	
413.00 > 169.00	1.904	1.914	-0.010	0.996	3028676		1.85(0.00-0.00)	3704	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.147	2.147	0.0	1.000	8679676	84.4		6114	
499.00 > 99.00	2.147	2.147	0.0	1.000	1807143		4.80(0.00-0.00)	2991	
* 7 13C4 PFOS									
503.00 > 80.00	2.147	2.151	-0.004		3141787	28.7		4961	
9 Perfluorononanoic acid									
463.00 > 419.00	2.155	2.158	-0.003	1.000	4019666	42.4		1149	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.306	2.312	-0.006	1.000	1164156	10.7		6124	

Reagents:

LC537-L6_00020

Amount Added: 1.00

Units: mL

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537ICAL_009.d

Injection Date: 03-Nov-2017 14:01:24

Instrument ID: A8_N

Lims ID: IC L6

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 6

Worklist Smp#: 9

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA

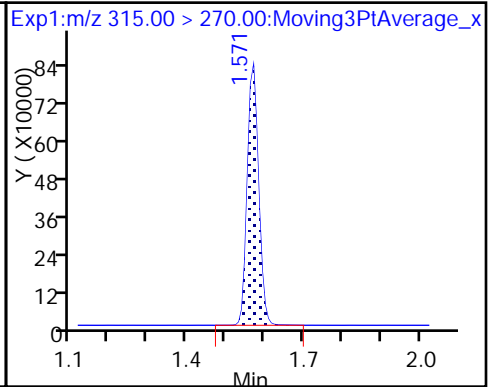

4 Perfluoroheptanoic acid

3 Perfluorohexanesulfonic acid




* 6 13C2-PFOA

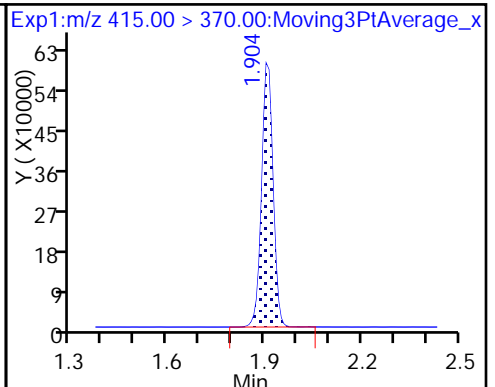

5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid

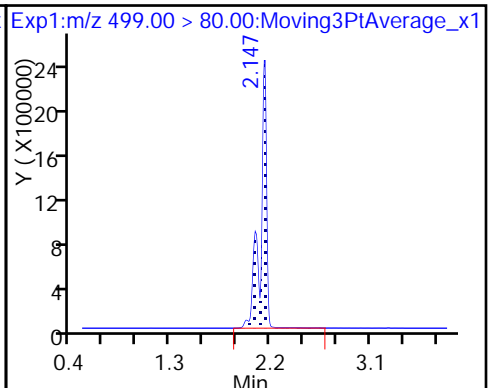


8 Perfluorooctane sulfonic acid

* 7 13C4 PFOS

9 Perfluorononanoic acid

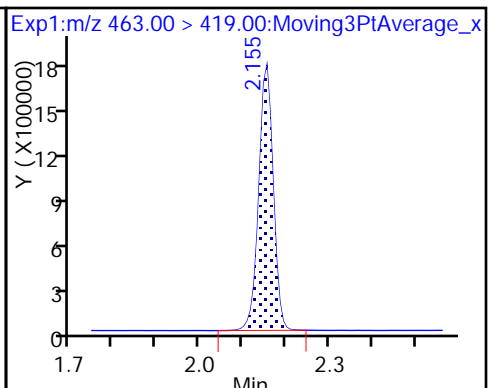

\$ 10 13C2 PFDA



FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Lab Sample ID: CCVL 320-192908/11 Calibration Date: 11/03/2017 14:10
 Instrument ID: A8_N Calib Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 11/03/2017 14:01
 Lab File ID: 2017.11.03_537XICAL_011.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		1.109		20.4	20.0	1.9	50.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9369	0.9382		2.23	2.22	0.1	50.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.674	1.688		6.72	6.67	0.8	50.0
Perfluorooctanoic acid (PFOA)	Ave	0.9258	0.8825		4.24	4.45	-4.7	50.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9389	0.9176		8.69	8.89	-2.3	50.0
Perfluorononanoic acid (PFNA)	Ave	0.6642	0.6625		4.43	4.45	-0.2	50.0
13C2 PFHxA	Ave	1.100	1.068		9.70	10.0	-3.0	30.0
13C2 PFDA	Ave	0.7652	0.7460		9.75	10.0	-2.5	30.0

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_011.d
 Lims ID: CCVL
 Client ID:
 Sample Type: CCVL
 Inject. Date: 03-Nov-2017 14:10:44 ALS Bottle#: 2 Worklist Smp#: 11
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: CCV L2
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub1
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Nov-2017 15:39:07 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK021

First Level Reviewer: phomsophat Date: 06-Nov-2017 07:26:29

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.449	1.444	0.005	1.000	2556738	20.4		1537	
298.90 > 99.00	1.449	1.444	0.005	1.000	1750170		1.46(0.00-0.00)	4023	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.578	1.573	0.005	1.000	1694196	9.70		8915	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.730	1.725	0.005	1.000	1297654	6.72		2410	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.730	1.725	0.005	1.000	330927	2.23		99.4	
* 6 13C2-PFOA									
415.00 > 370.00	1.912	1.913	-0.001		1586829	10.0		6840	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.912	1.914	-0.002	1.000	622915	4.24		116	
413.00 > 169.00	1.912	1.914	-0.002	1.000	335080		1.86(0.00-0.00)	460	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.155	2.147	0.008	1.000	940397	8.69		528	
499.00 > 99.00	2.147	2.147	0.0	0.996	196397		4.79(0.00-0.00)	430	
* 7 13C4 PFOS									
503.00 > 80.00	2.147	2.151	-0.004		3305852	28.7		5135	
9 Perfluorononanoic acid									
463.00 > 419.00	2.162	2.158	0.004	1.000	467323	4.43		143	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.314	2.312	0.002	1.000	1183747	9.75		6763	

Reagents:

LC537-L2_00020

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537ICAL_011.d

Injection Date: 03-Nov-2017 14:10:44

Instrument ID: A8_N

Lims ID: CCVL

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 2

Worklist Smp#: 11

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid

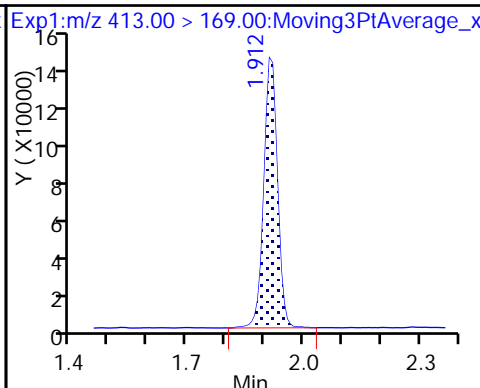


8 Perfluorooctane sulfonic acid

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA

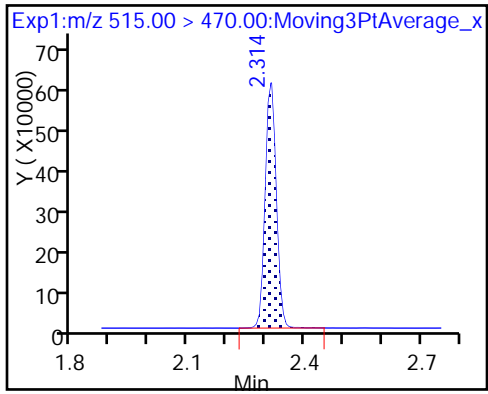

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Lab Sample ID: ICV 320-192908/13 Calibration Date: 11/03/2017 14:20
 Instrument ID: A8_N Calib Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 11/03/2017 14:01
 Lab File ID: 2017.11.03_537XICAL_013.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		0.8310		83.7	100	-16.4	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9369	0.8136		8.68	10.0	-13.2	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.674	1.463		17.5	20.1	-12.6	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9258	0.7995		17.7	20.5	-13.6	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9389	0.8637		18.1	19.7	-8.0	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6642	0.6428		19.5	20.1	-3.2	30.0
13C2 PFHxA	Ave	1.100	1.039		9.44	10.0	-5.6	30.0
13C2 PFDA	Ave	0.7652	0.7391		9.66	10.0	-3.4	30.0

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_013.d
 Lims ID: ICV
 Client ID:
 Sample Type: ICV
 Inject. Date: 03-Nov-2017 14:20:03 ALS Bottle#: 7 Worklist Smp#: 13
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: ICV
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist:

Method: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Nov-2017 15:39:08 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK021

First Level Reviewer: phomsophat Date: 06-Nov-2017 07:27:24

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.442	1.444	-0.002	1.000	9960387	83.7		4998	
298.90 > 99.00	1.442	1.444	-0.002	1.000	7235967		1.38(0.00-0.00)	13514	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.571	1.573	-0.003	1.000	1570629	9.44		8393	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.722	1.725	-0.003	1.000	3517469	17.5		5659	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.722	1.725	-0.003	1.000	1229696	8.68		345	
* 6 13C2-PFOA									
415.00 > 370.00	1.904	1.913	-0.009		1512045	10.0		7643	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.904	1.914	-0.010	1.000	2476221	17.7		475	
413.00 > 169.00	1.904	1.914	-0.010	1.000	1327388		1.87(0.00-0.00)	1724	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.140	2.147	-0.007	1.000	2036944	18.1		2323	
499.00 > 99.00	2.140	2.147	-0.007	1.000	389736		5.23(0.00-0.00)	830	
* 7 13C4 PFOS									
503.00 > 80.00	2.140	2.151	-0.011		3433628	28.7		5334	
9 Perfluorononanoic acid									
463.00 > 419.00	2.147	2.158	-0.011	1.000	1956116	19.5		652	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.306	2.312	-0.006	1.000	1117553	9.66		6230	

Reagents:

LC537-ICV_00028

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_013.d

Injection Date: 03-Nov-2017 14:20:03

Instrument ID: A8_N

Lims ID: ICV

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 7

Worklist Smp#: 13

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid




8 Perfluorooctane sulfonic acid

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Lab Sample ID: CCVL 320-204872/1 Calibration Date: 01/20/2018 18:47
 Instrument ID: A8_N Calib Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 11/03/2017 14:01
 Lab File ID: 2018.01.20_537AA_004.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		1.131		20.8	20.0	3.9	50.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.674	1.714		6.83	6.67	2.4	50.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9369	0.9361		2.22	2.22	-0.0	50.0
Perfluorooctanoic acid (PFOA)	Ave	0.9258	0.9051		4.35	4.45	-2.2	50.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9389	0.9446		8.94	8.89	0.6	50.0
Perfluorononanoic acid (PFNA)	Ave	0.6642	0.6563		4.39	4.45	-1.2	50.0
13C2 PFHxA	Ave	1.100	1.083		9.84	10.0	-1.6	30.0
13C2 PFDA	Ave	0.7652	0.7793		10.2	10.0	1.8	30.0

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\2018.01.20_537AA_004.d
 Lims ID: CCVL
 Client ID:
 Sample Type: CCVL
 Inject. Date: 20-Jan-2018 18:47:50 ALS Bottle#: 2 Worklist Smp#: 1
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: CCV L2
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub1
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 22-Jan-2018 11:19:44 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK027

First Level Reviewer: roycea Date: 22-Jan-2018 11:18:25

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.366	1.366	0.0	1.000	2707711	20.8		5673	
298.90 > 99.00	1.366	1.366	0.0	1.000	1985907		1.36(0.00-0.00)	6392	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.487	1.487	0.0	1.000	1791323	9.84		7614	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.624	1.624	0.0	1.000	1367841	6.83		2145	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.631	1.631	0.0	1.000	344231	2.22		93.6	
* 6 13C2-PFOA									
415.00 > 370.00	1.813	1.813	0.0		1654416	10.0		4879	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.813	1.813	0.0	1.000	666096	4.35		130	
413.00 > 169.00	1.813	1.813	0.0	1.000	368046		1.81(0.00-0.00)	1270	
* 7 13C4 PFOS									
503.00 > 80.00	2.064	2.064	0.0		3432875	28.7		7623	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.071	2.064	0.007	1.000	1005302	8.94		322	
499.00 > 99.00	2.064	2.064	0.0	0.996	223417		4.50(0.00-0.00)	1016	
9 Perfluorononanoic acid									
463.00 > 419.00	2.079	2.079	0.0	1.000	482648	4.39		119	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.253	2.253	0.0	1.000	1289197	10.2		5535	

Reagents:

LC537-L2_00020

Amount Added: 1.00

Units: mL

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\2018.01.20_537AA_004.d

Injection Date: 20-Jan-2018 18:47:50

Instrument ID: A8_N

Lims ID: CCVL

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 2

Worklist Smp#: 1

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




* 7 13C4 PFOS




8 Perfluorooctane sulfonic acid

8 Perfluorooctane sulfonic acid

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Lab Sample ID: CCV 320-204872/2 Calibration Date: 01/20/2018 18:52
 Instrument ID: A8_N Calib Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 11/03/2017 14:01
 Lab File ID: 2018.01.20_537AA_005.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		1.037		44.3	45.0	-1.5	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9369	0.9246		4.94	5.00	-1.3	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.674	1.649		14.8	15.0	-1.5	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9258	0.9210		9.96	10.0	-0.5	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9389	0.9230		19.7	20.0	-1.7	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6642	0.6292		9.48	10.0	-5.3	30.0
13C2 PFHxA	Ave	1.100	1.097		9.97	10.0	-0.3	30.0
13C2 PFDA	Ave	0.7652	0.8118		10.6	10.0	6.1	30.0

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\2018.01.20_537AA_005.d
 Lims ID: CCV L3
 Client ID:
 Sample Type: CCVIS
 Inject. Date: 20-Jan-2018 18:52:29 ALS Bottle#: 3 Worklist Smp#: 2
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: CCV L3
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub1
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 22-Jan-2018 13:23:53 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK027

First Level Reviewer: roycea Date: 22-Jan-2018 13:23:53

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.366	1.444	-0.078	1.000	6034331	44.3		10105	
298.90 > 99.00	1.366	1.444	-0.078	1.000	4453643		1.35(0.00-0.00)	11197	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.487	1.573	-0.086	1.000	1883006	9.97		7819	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.624	1.725	-0.101	1.000	3198759	14.8		4783	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.624	1.725	-0.101	1.000	793913	4.94		220	
* 6 13C2-PFOA									
415.00 > 370.00	1.806	1.913	-0.107		1716899	10.0		5061	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.806	1.914	-0.108	1.000	1582591	9.96		296	
413.00 > 169.00	1.806	1.914	-0.108	1.000	845653		1.87(0.00-0.00)	2845	
* 7 13C4 PFOS									
503.00 > 80.00	2.056	2.151	-0.095		3708679	28.7		7728	
9 Perfluorononanoic acid									
463.00 > 419.00	2.071	2.158	-0.087	1.000	1080476	9.48		245	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.064	2.064	0.0	1.000	2387637	19.7		2548	
499.00 > 99.00	2.056	2.064	-0.008	0.996	495293		4.82(0.00-0.00)	843	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.246	2.312	-0.066	1.000	1393783	10.6		7245	

Reagents:

LC537-L3_00023

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\2018.01.20_537AA_005.d

Injection Date: 20-Jan-2018 18:52:29

Instrument ID: A8_N

Lims ID: CCV L3

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 3

Worklist Smp#: 2

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




* 7 13C4 PFOS




9 Perfluorononanoic acid

8 Perfluorooctane sulfonic acid

8 Perfluorooctane sulfonic acid



\$ 10 13C2 PFDA



FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Lab Sample ID: CCV 320-204872/14 Calibration Date: 01/20/2018 19:48
 Instrument ID: A8_N Calib Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 11/03/2017 14:01
 Lab File ID: 2018.01.20_537AA_017.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		0.8990		132	135	-2.5	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9369	0.9143		14.6	15.0	-2.4	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.674	1.637		44.0	45.0	-2.2	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9258	0.9376		30.4	30.0	1.3	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9389	0.9669		61.8	60.0	3.0	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6642	0.6706		30.3	30.0	1.0	30.0
13C2 PFHxA	Ave	1.100	1.177		10.7	10.0	7.0	30.0
13C2 PFDA	Ave	0.7652	0.8069		10.5	10.0	5.5	30.0

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\2018.01.20_537AA_017.d
 Lims ID: CCV L5
 Client ID:
 Sample Type: CCVIS
 Inject. Date: 20-Jan-2018 19:48:38 ALS Bottle#: 5 Worklist Smp#: 14
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: CCV L5
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub1
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 22-Jan-2018 13:32:01 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK027

First Level Reviewer: roycea Date: 22-Jan-2018 13:32:01

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.366	1.444	-0.078	1.000	15298494	131.6		14722	
298.90 > 99.00	1.366	1.444	-0.078	1.000	11454394		1.34(0.00-0.00)	16937	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.479	1.573	-0.094	1.000	1873556	10.7		8596	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.624	1.725	-0.101	1.000	9286029	44.0		14417	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.624	1.725	-0.101	1.000	2183038	14.6		619	
* 6 13C2-PFOA									
415.00 > 370.00	1.798	1.913	-0.115		1591448	10.0		4940	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.798	1.914	-0.116	1.000	4480068	30.4		721	
413.00 > 169.00	1.798	1.914	-0.116	1.000	2373727		1.89(0.00-0.00)	6209	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.048	2.048	0.0	1.000	7314148	61.8		6036	
499.00 > 99.00	2.048	2.048	0.0	1.000	1509876		4.84(0.00-0.00)	5216	
* 7 13C4 PFOS									
503.00 > 80.00	2.048	2.151	-0.103		3614871	28.7		7343	
9 Perfluorononanoic acid									
463.00 > 419.00	2.056	2.158	-0.102	1.000	3202164	30.3		677	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.238	2.312	-0.074	1.000	1284181	10.5		5297	

Reagents:

LC537-L5_00024

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\2018.01.20_537AA_017.d

Injection Date: 20-Jan-2018 19:48:38

Instrument ID: A8_N

Lims ID: CCV L5

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 5

Worklist Smp#: 14

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid




8 Perfluorooctane sulfonic acid

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Lab Sample ID: CCVL 320-205331/1 Calibration Date: 01/24/2018 05:01
 Instrument ID: A8_N Calib Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 11/03/2017 14:01
 Lab File ID: 2018.01.23537A_004.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		1.196		22.0	20.0	10.0	50.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9369	0.9347		2.22	2.22	-0.2	50.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.674	1.793		7.14	6.67	7.1	50.0
Perfluorooctanoic acid (PFOA)	Ave	0.9258	0.9224		4.43	4.45	-0.4	50.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9389	0.9591		9.08	8.89	2.1	50.0
Perfluorononanoic acid (PFNA)	Ave	0.6642	0.6472		4.33	4.45	-2.6	50.0
13C2 PFHxA	Ave	1.100	1.113		10.1	10.0	1.1	30.0
13C2 PFDA	Ave	0.7652	0.7500		9.80	10.0	-2.0	30.0

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\2018.01.23537A_004.d
 Lims ID: CCVL
 Client ID:
 Sample Type: CCVL
 Inject. Date: 24-Jan-2018 05:01:08 ALS Bottle#: 2 Worklist Smp#: 1
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: CCV L2
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub1
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 24-Jan-2018 09:58:50 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK024

First Level Reviewer: roycea Date: 24-Jan-2018 09:52:38

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.366	1.366	0.0	1.000	2619767	22.0		2903	
298.90 > 99.00	1.366	1.366	0.0	1.000	1983412		1.32(0.00-0.00)	3088	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.479	1.479	0.0	1.000	1694436	10.1		7824	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.624	1.624	0.0	1.000	316392	2.22		129	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.624	1.624	0.0	1.000	1309682	7.14		3837	
* 6 13C2-PFOA									
415.00 > 370.00	1.813	1.806	0.007		1522908	10.0		6079	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.813	1.806	0.007	1.000	624821	4.43		174	
413.00 > 169.00	1.813	1.806	0.007	1.000	336011		1.86(0.00-0.00)	972	
* 7 13C4 PFOS									
503.00 > 80.00	2.064	2.056	0.008		3142156	28.7		5353	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.064	2.056	0.008	1.000	934211	9.08		552	a
499.00 > 99.00	2.064	2.056	0.008	1.000	205948		4.54(0.00-0.00)	659	a
9 Perfluorononanoic acid									
463.00 > 419.00	2.071	2.064	0.007	1.000	438149	4.33		199	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.246	2.238	0.008	1.000	1142197	9.80		7347	

QC Flag Legend

Review Flags

a - User Assigned ID

Reagents:

LC537-L2_00020

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\2018.01.23537A_004.d

Injection Date: 24-Jan-2018 05:01:08

Instrument ID: A8_N

Lims ID: CCVL

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 2

Worklist Smp#: 1

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



4 Perfluoroheptanoic acid

3 Perfluorohexanesulfonic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




* 7 13C4 PFOS




8 Perfluorooctane sulfonic acid (M)

8 Perfluorooctane sulfonic acid

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\2018.01.23537A_004.d
Injection Date: 24-Jan-2018 05:01:08 Instrument ID: A8_N
Lims ID: CCVL
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 2 Worklist Smp#: 1
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.06

Processing Integration Results



Manual Integration Results

RT: 2.06
Area: 934211
Amount: 9.081436
Amount Units: ng/ml



Reviewer: roycea, 24-Jan-2018 09:52:11
Audit Action: Assigned Compound ID

Audit Reason: User Assigned

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Lab Sample ID: CCV 320-205331/2 Calibration Date: 01/24/2018 05:05
 Instrument ID: A8_N Calib Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 11/03/2017 14:01
 Lab File ID: 2018.01.23537A_005.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		0.9384		139	135	3.0	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9369	0.9563		15.3	15.0	2.1	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.674	1.697		45.6	45.0	1.4	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9258	0.9181		29.8	30.0	-0.8	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9389	0.9568		61.2	60.0	1.9	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6642	0.6405		28.9	30.0	-3.6	30.0
13C2 PFHxA	Ave	1.100	1.167		10.6	10.0	6.1	30.0
13C2 PFDA	Ave	0.7652	0.7591		9.92	10.0	-0.8	30.0

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\2018.01.23537A_005.d
 Lims ID: CCV L5
 Client ID:
 Sample Type: CCVIS
 Inject. Date: 24-Jan-2018 05:05:49 ALS Bottle#: 5 Worklist Smp#: 2
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: CCV L5
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub1
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 24-Jan-2018 09:58:52 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK024

First Level Reviewer: roycea Date: 24-Jan-2018 09:53:05

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.366	1.366	0.0	1.000	15338988	139.1		10581	
298.90 > 99.00	1.366	1.366	0.0	1.000	11800446		1.30(0.00-0.00)	11652	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.487	1.487	0.0	1.000	1841720	10.6		8983	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.631	1.631	0.0	1.000	2264313	15.3		884	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.631	1.631	0.0	1.000	9249702	45.6		14210	
* 6 13C2-PFOA									
415.00 > 370.00	1.813	1.813	0.0		1578125	10.0		6522	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.813	1.813	0.0	1.000	4350095	29.8		1209	
413.00 > 169.00	1.813	1.813	0.0	1.000	2365895		1.84(0.00-0.00)	5407	
* 7 13C4 PFOS									
503.00 > 80.00	2.064	2.064	0.0		3472309	28.7		6594	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.071	2.056	0.015	1.000	6951981	61.2		5567	a
499.00 > 99.00	2.064	2.056	0.008	0.996	1462291		4.75(0.00-0.00)	3119	a
9 Perfluorononanoic acid									
463.00 > 419.00	2.079	2.079	0.0	1.000	3032732	28.9		1255	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.246	2.246	0.0	1.000	1197924	9.92		6392	

QC Flag Legend

Review Flags

a - User Assigned ID

Reagents:

LC537-L5_00024

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\2018.01.23537A_005.d

Injection Date: 24-Jan-2018 05:05:49

Instrument ID: A8_N

Lims ID: CCV L5

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 5

Worklist Smp#: 2

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



4 Perfluoroheptanoic acid

3 Perfluorohexanesulfonic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




* 7 13C4 PFOS




8 Perfluorooctane sulfonic acid (M)

8 Perfluorooctane sulfonic acid

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\2018.01.23537A_005.d
Injection Date: 24-Jan-2018 05:05:49 Instrument ID: A8_N
Lims ID: CCV L5
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 5 Worklist Smp#: 2
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1


Signal: 1

Not Detected
Expected RT: 2.06

Processing Integration Results



Manual Integration Results



RT: 2.07
Area: 6951981
Amount: 61.154370
Amount Units: ng/ml

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Lab Sample ID: CCV 320-205331/13 Calibration Date: 01/24/2018 05:57
 Instrument ID: A8_N Calib Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 11/03/2017 14:01
 Lab File ID: 2018.01.23537A_016.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		1.131		48.6	45.0	8.1	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9369	0.9320		4.97	5.00	-0.5	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.674	1.784		16.0	15.0	6.6	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9258	0.9062		9.80	10.0	-2.1	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9389	0.9221		19.6	20.0	-1.8	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6642	0.6398		9.64	10.0	-3.7	30.0
13C2 PFHxA	Ave	1.100	1.131		10.3	10.0	2.8	30.0
13C2 PFDA	Ave	0.7652	0.7849		10.3	10.0	2.6	30.0

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\2018.01.23537A_016.d
 Lims ID: CCV L3
 Client ID:
 Sample Type: CCVIS
 Inject. Date: 24-Jan-2018 05:57:17 ALS Bottle#: 3 Worklist Smp#: 13
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: CCV L3
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub1
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 24-Jan-2018 09:59:00 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK024

First Level Reviewer: roycea Date: 24-Jan-2018 09:58:44

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.366	1.366	0.0	1.000	5653653	48.6		6077	
298.90 > 99.00	1.366	1.366	0.0	1.000	4422651		1.28(0.00-0.00)	5695	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.479	1.479	0.0	1.000	1680000	10.3		8323	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.624	1.624	0.0	1.000	692228	4.97		272	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.624	1.624	0.0	1.000	2974328	16.0		7498	
* 6 13C2-PFOA									
415.00 > 370.00	1.806	1.806	0.0		1485112	10.0		5938	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.806	1.806	0.0	1.000	1346854	9.80		371	
413.00 > 169.00	1.806	1.806	0.0	1.000	735970		1.83(0.00-0.00)	2071	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.056	2.056	0.0	1.000	2049169	19.6		1938	a
499.00 > 99.00	2.056	2.056	0.0	1.000	445422		4.60(0.00-0.00)	1388	a
* 7 13C4 PFOS									
503.00 > 80.00	2.056	2.056	0.0		3186147	28.7		6536	
9 Perfluorononanoic acid									
463.00 > 419.00	2.064	2.064	0.0	1.000	950356	9.64		352	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.238	2.238	0.0	1.000	1165655	10.3		6718	

QC Flag Legend

Review Flags

a - User Assigned ID

Reagents:

LC537-L3_00023

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\2018.01.23537A_016.d

Injection Date: 24-Jan-2018 05:57:17

Instrument ID: A8_N

Lims ID: CCV L3

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 3

Worklist Smp#: 13

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



4 Perfluoroheptanoic acid

3 Perfluorohexanesulfonic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\2018.01.23537A_016.d
Injection Date: 24-Jan-2018 05:57:17 Instrument ID: A8_N
Lims ID: CCV L3
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 3 Worklist Smp#: 13
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.06

Processing Integration Results



RT: 2.06
Area: 2049169
Amount: 19.644874
Amount Units: ng/ml

Manual Integration Results



FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: _____ Lab Sample ID: MB 320-204304/1-A
 Matrix: Water Lab File ID: 2018.01.20_537AA_007.d
 Analysis Method: 537 Date Collected: _____
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 250 (mL) Date Analyzed: 01/20/2018 19:01
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 204872 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	8.0	U	20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.0	U	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	86		70-130
STL00996	13C2 PFDA	96		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\2018.01.20_537AA_007.d
 Lims ID: MB 320-204304/1-A
 Client ID:
 Sample Type: MB
 Inject. Date: 20-Jan-2018 19:01:50 ALS Bottle#: 4 Worklist Smp#: 4
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: mb 320-204304/1-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 22-Jan-2018 11:19:45 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK027

First Level Reviewer: roycea Date: 22-Jan-2018 11:19:07

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
\$ 2 13C2 PFHxA	315.00 > 270.00	1.479	1.573	-0.094	1.000	1702891	8.58	7589	
* 6 13C2-PFOA	415.00 > 370.00	1.806	1.913	-0.107		1804768	10.0	5586	
* 7 13C4 PFOS	503.00 > 80.00	2.056	2.151	-0.095		3734647	28.7	6068	
\$ 10 13C2 PFDA	515.00 > 470.00	2.238	2.312	-0.074	1.000	1319091	9.55	7526	

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\2018.01.20_537AA_007.d

Injection Date: 20-Jan-2018 19:01:50

Instrument ID: A8_N

Lims ID: MB 320-204304/1-A

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 4

Worklist Smp#: 4

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid (ND)

1 Perfluorobutanesulfonic acid (ND)




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid (ND)

4 Perfluoroheptanoic acid (ND)




* 6 13C2-PFOA



5 Perfluorooctanoic acid (ND)

5 Perfluorooctanoic acid (ND)




8 Perfluorooctane sulfonic acid (ND)




8 Perfluorooctane sulfonic acid (ND)

* 7 13C4 PFOS

9 Perfluorononanoic acid (ND)



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\2018.01.20_537AA_007.d
 Lims ID: MB 320-204304/1-A
 Client ID:
 Sample Type: MB
 Inject. Date: 20-Jan-2018 19:01:50 ALS Bottle#: 4 Worklist Smp#: 4
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: mb 320-204304/1-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 22-Jan-2018 11:19:45 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK027

First Level Reviewer: roycea Date: 22-Jan-2018 11:19:07

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	8.58	85.75
\$ 10 13C2 PFDA	10.0	9.55	95.52

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: _____ Lab Sample ID: LLCS 320-204304/2-A
 Matrix: Water Lab File ID: 2018.01.20_537AA_008.d
 Analysis Method: 537 Date Collected: _____
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 250 (mL) Date Analyzed: 01/20/2018 19:06
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 204872 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	39.2	J	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	20.1		20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	19.7	J	24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	30.9		30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	10.4		10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	85.8	J	90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	97		70-130
STL00996	13C2 PFDA	103		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\2018.01.20_537AA_008.d
 Lims ID: LLCS 320-204304/2-A
 Client ID:
 Sample Type: LLCS
 Inject. Date: 20-Jan-2018 19:06:31 ALS Bottle#: 5 Worklist Smp#: 5
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: llcs 320-204304/2-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 22-Jan-2018 11:19:45 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK027

First Level Reviewer: roycea Date: 22-Jan-2018 11:19:38

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.366	1.444	-0.078	1.000	2989837	21.5		4282	
298.90 > 99.00	1.366	1.444	-0.078	1.000	2224205		1.34(0.00-0.00)	5211	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.479	1.573	-0.094	1.000	1861454	9.66		7907	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.624	1.725	-0.101	1.000	1656897	7.72		3407	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.624	1.725	-0.101	1.000	425040	2.59		119	
* 6 13C2-PFOA									
415.00 > 370.00	1.806	1.913	-0.107		1751473	10.0		5455	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.806	1.914	-0.108	1.000	813816	5.02		149	
413.00 > 169.00	1.806	1.914	-0.108	1.000	435562		1.87(0.00-0.00)	1735	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.056	2.064	-0.008	1.000	1178242	9.79		378	
499.00 > 99.00	2.056	2.064	-0.008	1.000	237806		4.95(0.00-0.00)	368	
* 7 13C4 PFOS									
503.00 > 80.00	2.056	2.151	-0.095		3675151	28.7		7038	
9 Perfluorononanoic acid									
463.00 > 419.00	2.064	2.158	-0.094	1.000	571520	4.91		89.0	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.246	2.312	-0.066	1.000	1385037	10.3		7648	

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\2018.01.20_537AA_008.d

Injection Date: 20-Jan-2018 19:06:31

Instrument ID: A8_N

Lims ID: LLCS 320-204304/2-A

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 5

Worklist Smp#: 5

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid




8 Perfluorooctane sulfonic acid

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\2018.01.20_537AA_008.d
 Lims ID: LLCS 320-204304/2-A
 Client ID:
 Sample Type: LLCS
 Inject. Date: 20-Jan-2018 19:06:31 ALS Bottle#: 5 Worklist Smp#: 5
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: llcs 320-204304/2-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 22-Jan-2018 11:19:45 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK027

First Level Reviewer: roycea Date: 22-Jan-2018 11:19:38

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	9.66	96.59
\$ 10 13C2 PFDA	10.0	10.3	103.34

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: WGNA-010818-RW-4024 LMS Lab Sample ID: 320-34917-10 LMS
 Matrix: Water Lab File ID: 2018.01.23537A_009.d
 Analysis Method: 537 Date Collected: 01/08/2018 11:40
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 249.1(mL) Date Analyzed: 01/24/2018 05:24
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 205331 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	58.5	M	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	31.9		20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	22.9	J	24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	36.4		30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	14.4		10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	95.9		90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	88		70-130
STL00996	13C2 PFDA	95		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\2018.01.23537A_009.d
 Lims ID: 320-34917-A-10-D LMS
 Client ID:
 Sample Type: LMS
 Inject. Date: 24-Jan-2018 05:24:32 ALS Bottle#: 16 Worklist Smp#: 6
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-34917-a-10-d lms
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 24-Jan-2018 09:58:52 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK024

First Level Reviewer: roycea Date: 24-Jan-2018 09:55:15

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.366	1.366	0.0	1.000	3286872	23.9		1515	
298.90 > 99.00	1.366	1.366	0.0	1.000	2488688		1.32(0.00-0.00)	2800	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.479	1.487	-0.008	1.000	1581750	8.76		6599	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.624	1.631	-0.007	1.000	552831	3.60		73.8	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.624	1.631	-0.007	1.000	1926066	9.06		638	
* 6 13C2-PFOA									
415.00 > 370.00	1.806	1.813	-0.007		1640988	10.0		6259	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.806	1.813	-0.007	1.000	1208619	7.96		137	
413.00 > 169.00	1.813	1.813	0.0	1.004	686827		1.76(0.00-0.00)	1322	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.064	2.056	0.008	1.000	1738515	14.6		515	a
499.00 > 99.00	2.064	2.056	0.008	1.000	334820		5.19(0.00-0.00)	391	a
* 7 13C4 PFOS									
503.00 > 80.00	2.064	2.064	0.0		3643189	28.7		2285	
9 Perfluorononanoic acid									
463.00 > 419.00	2.071	2.079	-0.008	1.000	620900	5.70		87.1	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.246	2.246	0.0	1.000	1198133	9.54		6871	

QC Flag Legend

Review Flags

a - User Assigned ID

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\2018.01.23537A_009.d

Injection Date: 24-Jan-2018 05:24:32

Instrument ID: A8_N

Lims ID: 320-34917-A-10-D LMS

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 16

Worklist Smp#: 6

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



4 Perfluoroheptanoic acid

3 Perfluorohexanesulfonic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\2018.01.23537A_009.d
 Lims ID: 320-34917-A-10-D LMS
 Client ID:
 Sample Type: LMS
 Inject. Date: 24-Jan-2018 05:24:32 ALS Bottle#: 16 Worklist Smp#: 6
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-34917-a-10-d lms
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 24-Jan-2018 09:58:52 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK024

First Level Reviewer: roycea Date: 24-Jan-2018 09:55:15

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	8.76	87.60
\$ 10 13C2 PFDA	10.0	9.54	95.42

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\2018.01.23537A_009.d
Injection Date: 24-Jan-2018 05:24:32 Instrument ID: A8_N
Lims ID: 320-34917-A-10-D LMS
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 16 Worklist Smp#: 6
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.06

Processing Integration Results



RT: 2.06
Area: 1738515
Amount: 14.575855
Amount Units: ng/ml

Manual Integration Results



Reviewer: roycea, 24-Jan-2018 09:54:36
Audit Action: Assigned Compound ID

Audit Reason: User Assigned

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: WGNA-010818-RW-4024 LMSD Lab Sample ID: 320-34917-10 LMSD
 Matrix: Water Lab File ID: 2018.01.23537A_010.d
 Analysis Method: 537 Date Collected: 01/08/2018 11:40
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 257.7(mL) Date Analyzed: 01/24/2018 05:29
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 205331 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	56.7	M	39	16	6.6
335-67-1	Perfluorooctanoic acid (PFOA)	32.3		19	7.8	2.7
375-95-1	Perfluorononanoic acid (PFNA)	21.5	J	23	19	7.8
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	33.8		29	12	5.3
375-85-9	Perfluoroheptanoic acid (PFHpA)	13.8		9.7	3.9	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	98.5		87	35	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	90		70-130
STL00996	13C2 PFDA	97		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\2018.01.23537A_010.d
 Lims ID: 320-34917-A-10-E LMSD
 Client ID:
 Sample Type: LMSD
 Inject. Date: 24-Jan-2018 05:29:13 ALS Bottle#: 17 Worklist Smp#: 7
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-34917-a-10-e lmsd
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 24-Jan-2018 09:58:52 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK024

First Level Reviewer: roycea Date: 24-Jan-2018 09:55:46

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.358	1.366	-0.008	1.000	3700522	25.4		1549	
298.90 > 99.00	1.358	1.366	-0.008	1.000	2680499		1.38(0.00-0.00)	2957	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.479	1.487	-0.008	1.000	1662776	8.96		7877	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.616	1.631	-0.015	1.000	563376	3.57		70.2	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.616	1.631	-0.015	1.000	1966964	8.72		551	
* 6 13C2-PFOA									
415.00 > 370.00	1.798	1.813	-0.015		1685962	10.0		6609	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.798	1.813	-0.015	1.000	1299119	8.32		153	
413.00 > 169.00	1.798	1.813	-0.015	1.000	747663		1.74(0.00-0.00)	1398	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.056	2.056	0.0	1.000	1848259	14.6		531	a
499.00 > 99.00	2.056	2.056	0.0	1.000	358854		5.15(0.00-0.00)	478	a
* 7 13C4 PFOS									
503.00 > 80.00	2.048	2.064	-0.016		3866207	28.7		2493	
9 Perfluorononanoic acid									
463.00 > 419.00	2.064	2.079	-0.015	1.000	621048	5.55		84.0	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.238	2.246	-0.008	1.000	1257614	9.75		8087	

QC Flag Legend

Review Flags

a - User Assigned ID

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\2018.01.23537A_010.d

Injection Date: 24-Jan-2018 05:29:13

Instrument ID: A8_N

Lims ID: 320-34917-A-10-E LMSD

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 17

Worklist Smp#: 7

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



4 Perfluoroheptanoic acid

3 Perfluorohexanesulfonic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\2018.01.23537A_010.d
 Lims ID: 320-34917-A-10-E LMSD
 Client ID:
 Sample Type: LMSD
 Inject. Date: 24-Jan-2018 05:29:13 ALS Bottle#: 17 Worklist Smp#: 7
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-34917-a-10-e lmsd
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 24-Jan-2018 09:58:52 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK024

First Level Reviewer: roycea Date: 24-Jan-2018 09:55:46

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	8.96	89.64
\$ 10 13C2 PFDA	10.0	9.75	97.48

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b\2018.01.23537A_010.d
Injection Date: 24-Jan-2018 05:29:13 Instrument ID: A8_N
Lims ID: 320-34917-A-10-E LMSD
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 17 Worklist Smp#: 7
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.06

Processing Integration Results



Manual Integration Results

RT: 2.06
Area: 1848259
Amount: 14.602090
Amount Units: ng/ml



Reviewer: roycea, 24-Jan-2018 09:55:20
Audit Action: Assigned Compound ID

Audit Reason: User Assigned

LCMS ANALYSIS RUN LOG

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1

SDG No.: _____

Instrument ID: A8_N Start Date: 11/03/2017 13:37

Analysis Batch Number: 192908 End Date: 11/03/2017 14:24

LAB SAMPLE ID	CLIENT SAMPLE ID	DATE ANALYZED	DILUTION FACTOR	LAB FILE ID	COLUMN ID
IC 320-192908/4		11/03/2017 13:37	1	2017.11.03_537X ICAL 004.d	GeminiC18 3x100 3(mm)
IC 320-192908/5		11/03/2017 13:42	1	2017.11.03_537X ICAL 005.d	GeminiC18 3x100 3(mm)
IC 320-192908/6		11/03/2017 13:47	1	2017.11.03_537X ICAL 006.d	GeminiC18 3x100 3(mm)
IC 320-192908/7 ICISAV		11/03/2017 13:52	1	2017.11.03_537X ICAL 007.d	GeminiC18 3x100 3(mm)
IC 320-192908/8		11/03/2017 13:56	1	2017.11.03_537X ICAL 008.d	GeminiC18 3x100 3(mm)
IC 320-192908/9		11/03/2017 14:01	1	2017.11.03_537X ICAL 009.d	GeminiC18 3x100 3(mm)
ZZZZZ		11/03/2017 14:06	1		GeminiC18 3x100 3(mm)
CCVL 320-192908/11		11/03/2017 14:10	1	2017.11.03_537X ICAL 011.d	GeminiC18 3x100 3(mm)
ZZZZZ		11/03/2017 14:15	1		GeminiC18 3x100 3(mm)
ICV 320-192908/13		11/03/2017 14:20	1	2017.11.03_537X ICAL 013.d	GeminiC18 3x100 3(mm)
ZZZZZ		11/03/2017 14:24	1		GeminiC18 3x100 3(mm)

LCMS ANALYSIS RUN LOG

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1

SDG No.: _____

Instrument ID: A8_N Start Date: 01/20/2018 18:47

Analysis Batch Number: 204872 End Date: 01/20/2018 19:48

LAB SAMPLE ID	CLIENT SAMPLE ID	DATE ANALYZED	DILUTION FACTOR	LAB FILE ID	COLUMN ID
CCVL 320-204872/1		01/20/2018 18:47	1	2018.01.20_537A A 004.d	GeminiC18 3x100 3(mm)
CCV 320-204872/2 CCVIS		01/20/2018 18:52	1	2018.01.20_537A A 005.d	GeminiC18 3x100 3(mm)
MB 320-204304/1-A		01/20/2018 19:01	1	2018.01.20_537A A 007.d	GeminiC18 3x100 3(mm)
LLCS 320-204304/2-A		01/20/2018 19:06	1	2018.01.20_537A A 008.d	GeminiC18 3x100 3(mm)
320-34917-1		01/20/2018 19:11	1	2018.01.20_537A A 009.d	GeminiC18 3x100 3(mm)
320-34917-2		01/20/2018 19:15	1	2018.01.20_537A A 010.d	GeminiC18 3x100 3(mm)
320-34917-3		01/20/2018 19:20	1	2018.01.20_537A A 011.d	GeminiC18 3x100 3(mm)
320-34917-4		01/20/2018 19:25	1	2018.01.20_537A A 012.d	GeminiC18 3x100 3(mm)
320-34917-5		01/20/2018 19:29	1	2018.01.20_537A A 013.d	GeminiC18 3x100 3(mm)
320-34917-6		01/20/2018 19:34	1	2018.01.20_537A A 014.d	GeminiC18 3x100 3(mm)
320-34917-7		01/20/2018 19:39	1	2018.01.20_537A A 015.d	GeminiC18 3x100 3(mm)
320-34917-8		01/20/2018 19:43	1	2018.01.20_537A A 016.d	GeminiC18 3x100 3(mm)
CCV 320-204872/14 CCVIS		01/20/2018 19:48	1	2018.01.20_537A A 017.d	GeminiC18 3x100 3(mm)

LCMS ANALYSIS RUN LOG

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1

SDG No.: _____

Instrument ID: A8_N Start Date: 01/24/2018 05:01

Analysis Batch Number: 205331 End Date: 01/24/2018 05:57

LAB SAMPLE ID	CLIENT SAMPLE ID	DATE ANALYZED	DILUTION FACTOR	LAB FILE ID	COLUMN ID
CCVL 320-205331/1		01/24/2018 05:01	1	2018.01.23537A_004.d	GeminiC18 3x100 3(mm)
CCV 320-205331/2 CCVIS		01/24/2018 05:05	1	2018.01.23537A_005.d	GeminiC18 3x100 3(mm)
320-34917-9		01/24/2018 05:15	1	2018.01.23537A_007.d	GeminiC18 3x100 3(mm)
320-34917-10		01/24/2018 05:19	1	2018.01.23537A_008.d	GeminiC18 3x100 3(mm)
320-34917-10 LMS		01/24/2018 05:24	1	2018.01.23537A_009.d	GeminiC18 3x100 3(mm)
320-34917-10 LMSD		01/24/2018 05:29	1	2018.01.23537A_010.d	GeminiC18 3x100 3(mm)
320-34917-11		01/24/2018 05:33	1	2018.01.23537A_011.d	GeminiC18 3x100 3(mm)
320-34917-12		01/24/2018 05:38	1	2018.01.23537A_012.d	GeminiC18 3x100 3(mm)
320-34917-13		01/24/2018 05:43	1	2018.01.23537A_013.d	GeminiC18 3x100 3(mm)
320-34917-14		01/24/2018 05:47	1	2018.01.23537A_014.d	GeminiC18 3x100 3(mm)
320-34917-15		01/24/2018 05:52	1	2018.01.23537A_015.d	GeminiC18 3x100 3(mm)
CCV 320-205331/13 CCVIS		01/24/2018 05:57	1	2018.01.23537A_016.d	GeminiC18 3x100 3(mm)

LCMS BATCH WORKSHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1

SDG No.: _____

Batch Number: 204304 Batch Start Date: 01/17/18 10:49 Batch Analyst: Kouchari, Shamiran

Batch Method: 537 Batch End Date: 01/18/18 18:46

Lab Sample ID	Client Sample ID	Method Chain	Basis	GrossWeight	TareWeight	InitialAmount	FinalAmount	ReceivedpH	LC537-IS 00056
MB 320-204304/1		537, 537				250 mL	1.00 mL	7 SU	100 uL
LLCS 320-204304/2		537, 537				250 mL	1.00 mL	7 SU	100 uL
320-34917-A-1	WGNA-010818-RW-0344	537, 537	T	276.13 g	27.43 g	248.7 mL	1.00 mL	7 SU	100 uL
320-34917-A-2	WGNA-010818-FRB-0344	537, 537	T	280.44 g	27.20 g	253.2 mL	1.00 mL	7 SU	100 uL
320-34917-A-3	WGNA-010818-RW-3957	537, 537	T	285.26 g	27.84 g	257.4 mL	1.00 mL	7 SU	100 uL
320-34917-A-4	WGNA-010818-FRB-3957	537, 537	T	283.33 g	27.28 g	256.1 mL	1.00 mL	7 SU	100 uL
320-34917-A-5	WGNA-010818-DUP-16	537, 537	T	290.10 g	27.65 g	262.5 mL	1.00 mL	7 SU	100 uL
320-34917-A-6	WGNA-010818-RW-3178	537, 537	T	267.18 g	27.96 g	239.2 mL	1.00 mL	7 SU	100 uL
320-34917-A-7	WGNA-010818-FRB-3178	537, 537	T	284.45 g	27.74 g	256.7 mL	1.00 mL	7 SU	100 uL
320-34917-A-8	NAWC-010818-RW-141	537, 537	T	284.94 g	27.43 g	257.5 mL	1.00 mL	7 SU	100 uL
320-34917-A-9	NAWC-010818-FRB-141	537, 537	T	293.45 g	27.32 g	266.1 mL	1.00 mL	7 SU	100 uL
320-34917-A-10	WGNA-010818-RW-4024	537, 537	T	278.90 g	27.73 g	251.2 mL	1.00 mL	7 SU	100 uL
320-34917-A-10 LMS	WGNA-010818-RW-4024	537, 537	T	276.69 g	27.64 g	249.1 mL	1.00 mL	7 SU	100 uL
320-34917-A-10 LMSD	WGNA-010818-RW-4024	537, 537	T	285.36 g	27.65 g	257.7 mL	1.00 mL	7 SU	100 uL
320-34917-A-11	WGNA-010818-FRB-4024	537, 537	T	284.88 g	27.53 g	257.4 mL	1.00 mL	7 SU	100 uL
320-34917-A-12	WGNA-010818-RW-4844	537, 537	T	281.28 g	27.81 g	253.5 mL	1.00 mL	7 SU	100 uL
320-34917-A-13	WGNA-010818-FRB-4844	537, 537	T	276.54 g	27.04 g	249.5 mL	1.00 mL	7 SU	100 uL
320-34917-A-14	WGNA-010818-RW-0404	537, 537	T	276.80 g	27.41 g	249.4 mL	1.00 mL	7 SU	100 uL
320-34917-A-15	WGNA-010818-FRB-0404	537, 537	T	279.74 g	27.27 g	252.5 mL	1.00 mL	7 SU	100 uL

Lab Sample ID	Client Sample ID	Method Chain	Basis	LC537-LSP 00025	LC537-SU 00054	AnalysisComment			
MB 320-204304/1		537, 537			100 uL	ch nd			

The pound sign (#) in the amount added field denotes that the reagent was used undiluted. All calculations are performed using the stated concentration for this reagent.

LCMS BATCH WORKSHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1

SDG No.: _____

Batch Number: 204304 Batch Start Date: 01/17/18 10:49 Batch Analyst: Kouchari, Shamiran

Batch Method: 537 Batch End Date: 01/18/18 18:46

Lab Sample ID	Client Sample ID	Method Chain	Basis	LC537-LSP 00025	LC537-SU 00054	AnalysisComment			
LLCS 320-204304/2		537, 537		100 uL	100 uL	ch nd			
320-34917-A-1	WGNA-010818-RW-0344	537, 537	T		100 uL	ch nd			
320-34917-A-2	WGNA-010818-FRB-0344	537, 537	T		100 uL	ch nd			
320-34917-A-3	WGNA-010818-RW-3957	537, 537	T		100 uL	ch nd			
320-34917-A-4	WGNA-010818-FRB-3957	537, 537	T		100 uL	ch nd			
320-34917-A-5	WGNA-010818-DUP-16	537, 537	T		100 uL	ch nd			
320-34917-A-6	WGNA-010818-RW-3178	537, 537	T		100 uL	ch nd			
320-34917-A-7	WGNA-010818-FRB-3178	537, 537	T		100 uL	ch nd			
320-34917-A-8	NAWC-010818-RW-141	537, 537	T		100 uL	ch nd			
320-34917-A-9	NAWC-010818-FRB-141	537, 537	T		100 uL	ch nd			
320-34917-A-10	WGNA-010818-RW-4024	537, 537	T		100 uL	ch nd			
320-34917-A-10 LMS	WGNA-010818-RW-4024	537, 537	T	100 uL	100 uL	ch nd			
320-34917-A-10 LMSD	WGNA-010818-RW-4024	537, 537	T	100 uL	100 uL	ch nd			
320-34917-A-11	WGNA-010818-FRB-4024	537, 537	T		100 uL	ch nd			
320-34917-A-12	WGNA-010818-RW-4844	537, 537	T		100 uL	ch nd			
320-34917-A-13	WGNA-010818-FRB-4844	537, 537	T		100 uL	ch nd			
320-34917-A-14	WGNA-010818-RW-0404	537, 537	T		100 uL	ch nd			
320-34917-A-15	WGNA-010818-FRB-0404	537, 537	T		100 uL	ch nd			

The pound sign (#) in the amount added field denotes that the reagent was used undiluted. All calculations are performed using the stated concentration for this reagent.

LCMS BATCH WORKSHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1

SDG No.: _____

Batch Number: 204304 Batch Start Date: 01/17/18 10:49 Batch Analyst: Kouchari, Shamiran

Batch Method: 537 Batch End Date: 01/18/18 18:46

Batch Notes	
Analyst ID - Aliquot Step	KMK
Batch Comment	Label ID's checked: SKD 1-17-18
Analyst ID - Concentration	CCB
Analyst ID - Final Volume Step	KMK
Internal Standard ID#	1099356
Manifold ID	3,1
Methanol ID	1123833
pH Indicator ID	1617
Pipette ID	M16387D
Analyst ID - IS Reagent Drop	JER
Analyst ID - IS Reagent Drop Witness	KMK
Analyst ID - SU Reagent Drop	CCB
Analyst ID - SU Reagent Drop Witness	HJA
Analyst ID - TA Reagent Drop	CCB
Analyst ID - TA Reagent Drop Witness	HJA
SPE Cartridge ID	6357081-11
Trizma ID	SLBR4303V
Reagent Water ID	1-11-18

Basis	Basis Description
T	Total/NA

The pound sign (#) in the amount added field denotes that the reagent was used undiluted. All calculations are performed using the stated concentration for this reagent.

Job No: 34917, 34946 Instrument ID & Date: A8 1/22/18 ICAL Batch: 192908
 Extraction Batch: 204506, 204304, 204304 Worklist #: 53168, 53187, 53264 TALS Batch: 205018, 204917, 204918
Handwritten notes: 204872, 204894, 205331, 204921, 204922

Review Items	-- Level 1 --			Level 2
	Yes	No	N/A	
Initial Calibration				
1. Is ICAL verified and locked in Chrom & TALS?	✓			✓
2. Is ICV properly linked in TALS?	✓			✓
Continuing Calibration				
1. Low-range CCV injected at start of analytical run? CCV injected after every 10 samples and at the end of the analytical run and alternated between Low-range, Mid-range and High-range?	✓			✓
2. If sequence was not after an ICAL was a low and mid range CCV injected at the start of the analytical run?	✓			✓
3. Native compounds and surrogates in control? Low-range within ±50% of true value Mid and High-range within ±30% of true value	✓			✓
4. Internal Standard areas in control? Areas ≥ 50% of average area of the ICAL and 70-140% of the most recent CCV.	✓			✓
Client Samples & QC Sample Results				
1. Were preparation and analysis done within holding times?	✓			✓
2. Are Chromatograms reviewed and spectra verified?	✓			✓
3. Are positive results within calibration range?	✓			✓
4. Dilutions due to target cpds? <u>0</u> Dilutions due to non-targets? <u>0</u>			✓	
5. All target compounds in MB < 1/3 RL? (Requires NCM if "no.")	✓			✓
6. Are target constituents in LCS/LCSD within method control limits?	✓			✓
7. Internal Standard areas in control for all samples and QC reported? ±50% from the average area of the ICAL and 70-140% of the most recent CCV	✓			✓
8. Do results (e.g., dilutions/trip blanks) make sense?	✓			✓
9. Are MS/MSD recoveries and RPDs within method control limits?	✓			✓
10. Are all QC samples properly linked in TALS?	✓			✓
11. All manual integrations appropriate and completely documented?	✓			✓
12. Are nonconformances documented as NCMs?	✓			✓
13. Are all Chrom graphics uploaded?	✓			✓

1st Level Reviewer / Date: aar 1/23/18 1/24/18 2nd Level Reviewer / Date: Neway 1/24/2018
JRB 1-23-18

NCM # and Comments: 106466

A8

Instrument ID & Date: 11-3-17 Worklist#: 49975

ICAL Batch: 192908, 192909 Calibration ID number: 36012, 36013

Review Items	-- Level 1 --			Level 2
	Yes	No	N/A	
Initial Calibration				
1. Mass calibration, as needed, verified by full scan of PFC stock standard. All PFC ions used for quantitation are within 0.3 m/z of true mass?	✓			✓
2. Responses increase with increasing concentration?	✓			✓
3. Fit used (circle): <u>Average</u> Linear (1/x ²)Linear <u>Quadratic</u> (6 points minimum)				
4. Meets fit criteria? Intercept ≤ ½ RL RSD ≤ 30% for Average R ² ≥ 0.990 for Linear R ² ≥ 0.990 for Quadratic NOTE: "Force through Zero" must be used and weighted if needed	✓			✓
5. If quadratic fit used the curve does not "bend over".	✓			✓
6. Feed calibration points into the calculated curve. Are points ≤MRL within ±50% of true value? Are points >MRL within ±30% of true value?	✓			✓
7. Any carryover from the high calibration point must be ≤ 1/3 RL	✓			✓
8. Asymmetry check meets criteria for the first two eluting peaks? (0.8 - 1.5).	✓			✓
9. Is the asymmetry check scanned and linked in TALS to the calibration point?	✓			✓
10. Is ICV (2 nd source) ± 30% of true value?	✓			✓
11. Is ICV (2 nd source) internal standards ±50% of average area of the ICAL?	✓			✓
12. ICAL locked in Chrom and uploaded to TALS?	✓			✓
13. ICAL locked in TALS and scanned?				✓

1st Level Reviewer / Date: JRB 11-6-17

2nd Level Reviewer / Date: Murphy 11/6/2017

NCM # and Comments: _____

TestAmerica Laboratories
Worklist QC Batch Report

Worklist Name: 20JAN2018_537A
Instrument Name: A8_N
Data Directory: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b
QC Batching: Enabled

Worklist Number: 53155
Chrom Method: 537_A8_N
Limit Group Batching: Enabled

QC Batch: 1	LC 537 CS ICAL Raw Batch: 204871	LC 537 ICAL Raw Batch: 204872
# 1 CCVL	# 1 CCVL	# 1 CCVL
# 2 CCV L3	# 2 CCV L3	# 2 CCV L3
# 3 RB	# 3 RB	# 3 RB
# 4 MB 320-204304/1-A		# 4 MB 320-204304/1-A
# 5 LLCS 320-204304/2-A		# 5 LLCS 320-204304/2-A
# 6 320-34917-A-1-A		# 6 320-34917-A-1-A
# 7 320-34917-A-2-A		# 7 320-34917-A-2-A
# 8 320-34917-A-3-A		# 8 320-34917-A-3-A
# 9 320-34917-A-4-A		# 9 320-34917-A-4-A
#10 320-34917-A-5-A		#10 320-34917-A-5-A
#11 320-34917-A-6-A		#11 320-34917-A-6-A
#12 320-34917-A-7-A		#12 320-34917-A-7-A
#13 320-34917-A-8-A		#13 320-34917-A-8-A
#14 CCV L5	#14 CCV L5	#14 CCV L5

QC Batch: 2	LC 537 CS ICAL Raw Batch: 204873	LC 537 ICAL Raw Batch: 204874
#14 CCV L5	#14 CCV L5	#14 CCV L5
#15 RB	#15 RB	#15 RB
#16 320-34917-A-9-A		#16 320-34917-A-9-A
#17 320-34917-A-10-A		#17 320-34917-A-10-A
#18 320-34917-A-10-D LMS		#18 320-34917-A-10-D LMS
#19 320-34917-A-10-E LMSD		#19 320-34917-A-10-E LMSD
#20 320-34917-A-11-A		#20 320-34917-A-11-A
#21 320-34917-A-12-A		#21 320-34917-A-12-A
#22 320-34917-A-13-A		#22 320-34917-A-13-A
#23 320-34917-A-14-A		#23 320-34917-A-14-A
#24 320-34917-A-15-A		#24 320-34917-A-15-A
#25 CCV L3	#25 CCV L3	#25 CCV L3
#26 RB	#26 RB	#26 RB

RA

ICAL: 192908

TestAmerica Laboratories
Worklist QC Batch Report

Worklist Name: 22JAN2018_537A Worklist Number: 53168
 Instrument Name: A8_N Chrom Method: 537_A8_N
 Data Directory: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53168.b
 QC Batching: Enabled Limit Group Batching: Enabled

QC Batch: 1	LC 537 CS ICAL Raw Batch: 204916	LC 537 ICAL Raw Batch: 204917
# 1 CCVL # 2 CCV L5 # 3 RB # 4 320-34917-A-10-A # 5 320-34917-A-10-D LMS # 6 320-34917-A-10-E LMSD # 7 CCV L3	# 1 CCVL # 2 CCV L5 # 3 RB # 7 CCV L3	# 1 CCVL # 2 CCV L5 # 3 RB # 4 320-34917-A-10-A # 5 320-34917-A-10-D LMS # 6 320-34917-A-10-E LMSD # 7 CCV L3

RA

QC Batch: 2	LC 537 ICAL Raw Batch: 204918	LC 537 CS ICAL Raw Batch: 204919
# 7 CCV L3 # 8 RB # 9 MB 320-204506/1-A #10 LCS 320-204506/2-A #11 LCSD 320-204506/3-A #12 320-34946-A-1-A #13 320-34946-A-2-A #14 320-34946-A-3-A #15 320-34946-A-4-A #16 320-34946-A-5-A #17 320-34946-A-6-A #18 320-34946-A-7-A #19 CCV L5	# 7 CCV L3 # 8 RB # 9 MB 320-204506/1-A #10 LCS 320-204506/2-A #11 LCSD 320-204506/3-A #12 320-34946-A-1-A #13 320-34946-A-2-A #14 320-34946-A-3-A #15 320-34946-A-4-A #16 320-34946-A-5-A #17 320-34946-A-6-A #18 320-34946-A-7-A #19 CCV L5	# 7 CCV L3 # 8 RB #19 CCV L5

RA
dueto
ccv

QC Batch: 3	LC 537 CS ICAL Raw Batch: 204920	LC 537 ICAL Raw Batch: 204921
#19 CCV L5 #20 RB #21 320-34946-A-8-A #22 320-34946-A-9-A #23 320-34946-A-10-A #24 320-34946-A-11-A #25 320-34946-A-12-A #26 320-34946-A-13-A #27 320-34946-A-14-A #28 320-34946-A-15-A #29 320-34946-A-16-A #30 320-34946-A-17-A #31 CCV L3	#19 CCV L5 #20 RB #31 CCV L3	#19 CCV L5 #20 RB #21 320-34946-A-8-A #22 320-34946-A-9-A #23 320-34946-A-10-A #24 320-34946-A-11-A #25 320-34946-A-12-A #26 320-34946-A-13-A #27 320-34946-A-14-A #28 320-34946-A-15-A #29 320-34946-A-16-A #30 320-34946-A-17-A #31 CCV L3

QC Batch: 4	LC 537 ICAL Raw Batch: 204922	LC 537 CS ICAL Raw Batch: 204923
#31 CCV L3 #32 RB #33 320-34946-A-18-A #34 320-34946-A-19-A #35 CCV L5 #36 RB	#31 CCV L3 #32 RB #33 320-34946-A-18-A #34 320-34946-A-19-A #35 CCV L5 #36 RB	#31 CCV L3 #32 RB #35 CCV L5 #36 RB

TestAmerica Laboratories
Worklist QC Batch Report

Worklist Name: 22JAN2018_537B Worklist Number: 53187
Instrument Name: A8_N Chrom Method: 537_A8_N
Data Directory: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53187.b
QC Batching: Enabled Limit Group Batching: Enabled

QC Batch: 1	LC 537 ICAL Raw Batch: 205018	LC 537 CS ICAL Raw Batch: 205019
# 1 CCV L3	# 1 CCV L3	# 1 CCV L3
# 2 RB	# 2 RB	# 2 RB
# 3 MB 320-204506/1-A	# 3 MB 320-204506/1-A	
# 4 LCS 320-204506/2-A	# 4 LCS 320-204506/2-A	
# 5 LCSD 320-204506/3-A	# 5 LCSD 320-204506/3-A	
# 6 320-34946-A-1-A	# 6 320-34946-A-1-A	
# 7 320-34946-A-2-A	# 7 320-34946-A-2-A	
# 8 320-34946-A-3-A	# 8 320-34946-A-3-A	
# 9 320-34946-A-4-A	# 9 320-34946-A-4-A	
#10 320-34946-A-5-A	#10 320-34946-A-5-A	
#11 320-34946-A-6-A	#11 320-34946-A-6-A	
#12 320-34946-A-7-A	#12 320-34946-A-7-A	
#13 CCV L5	#13 CCV L5	#13 CCV L5
#14 RB	#14 RB	#14 RB

ICAL: 192908
CCVL: 204917

TestAmerica Laboratories
Worklist QC Batch Report

Worklist Name: 23JAN2018_537A Worklist Number: 53264
 Instrument Name: A8_N Chrom Method: 537_A8_N
 Data Directory: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b
 QC Batching: Enabled Limit Group Batching: Enabled

QC Batch: 1	LC 537 CS ICAL Raw Batch: 205330	LC 537 ICAL Raw Batch: 205331
# 1 CCVL	# 1 CCVL	# 1 CCVL
# 2 CCV L5	# 2 CCV L5	# 2 CCV L5
# 3 RB	# 3 RB	# 3 RB
# 4 320-34917-A-9-A		# 4 320-34917-A-9-A
# 5 320-34917-A-10-A		# 5 320-34917-A-10-A
# 6 320-34917-A-10-D LMS		# 6 320-34917-A-10-D LMS
# 7 320-34917-A-10-E LMSD		# 7 320-34917-A-10-E LMSD
# 8 320-34917-A-11-A		# 8 320-34917-A-11-A
# 9 320-34917-A-12-A		# 9 320-34917-A-12-A
#10 320-34917-A-13-A		#10 320-34917-A-13-A
#11 320-34917-A-14-A		#11 320-34917-A-14-A
#12 320-34917-A-15-A		#12 320-34917-A-15-A
#13 CCV L3	#13 CCV L3	#13 CCV L3

QC Batch: 2	LC 537 ICAL Raw Batch: 205332	LC 537 CS ICAL Raw Batch: 205333
#13 CCV L3	#13 CCV L3	#13 CCV L3
#14 RB	#14 RB	#14 RB
#15 MB 320-204684/1-A	#15 MB 320-204684/1-A	
#16 LCS 320-204684/2-A	#16 LCS 320-204684/2-A	
#17 320-35149-A-1-A	#17 320-35149-A-1-A	
#18 320-35149-A-2-A	#18 320-35149-A-2-A	
#19 320-35149-A-3-A	#19 320-35149-A-3-A	
#20 320-35149-A-4-A	#20 320-35149-A-4-A	
#21 320-35149-A-4-B MS	#21 320-35149-A-4-B MS	
#22 320-35149-A-4-C MSD	#22 320-35149-A-4-C MSD	
#23 QC ICV	#23 QC ICV	#23 QC ICV
#24 CCV L5	#24 CCV L5	#24 CCV L5
#25 RB	#25 RB	#25 RB

ICAL: 192908

TestAmerica Laboratories
Worklist Run Log Report

Worklist Name: 20JAN2018_537A

Worklist Num: 53155

Instrument: A8_N

Method: 537_A8_N

Batch Directory: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53155.b

Analysis Type: SemiVOA

Creator: Royce, Amani A

Inj Volume: 2.00

Inj Vol Units: ul

Lab ID	Worklist ID	Sample Type	Inj Date/Time	File Name	Vial	Dil Factor	Client ID	Fract
CCVL	320-0053155-001	CCVL	20-Jan-2018 18:47:50	2018.01.20_537AA_004.d	2	1.0		sv
CCV L3	320-0053155-002	CCVIS	20-Jan-2018 18:52:29	2018.01.20_537AA_005.d	3	1.0		sv
RB	320-0053155-003	RB	20-Jan-2018 18:57:10	2018.01.20_537AA_006.d	8	1.0		sv
MB 320-204304/1-A	320-0053155-004	MB	20-Jan-2018 19:01:50	2018.01.20_537AA_007.d	4	1.0		sv
LLCS 320-204304/2-A	320-0053155-005	LLCS	20-Jan-2018 19:06:31	2018.01.20_537AA_008.d	5	1.0		sv
320-34917-A-1-A	320-0053155-006	Client	20-Jan-2018 19:11:11	2018.01.20_537AA_009.d	6	1.0	WGNA-010818-RW-0344	sv
320-34917-A-2-A	320-0053155-007	Client	20-Jan-2018 19:15:52	2018.01.20_537AA_010.d	7	1.0	WGNA-010818-FRB-0344	sv
320-34917-A-3-A	320-0053155-008	Client	20-Jan-2018 19:20:33	2018.01.20_537AA_011.d	8	1.0	WGNA-010818-RW-3957	sv
320-34917-A-4-A	320-0053155-009	Client	20-Jan-2018 19:25:13	2018.01.20_537AA_012.d	9	1.0	WGNA-010818-FRB-3957	sv
320-34917-A-5-A	320-0053155-010	Client	20-Jan-2018 19:29:54	2018.01.20_537AA_013.d	10	1.0	WGNA-010818-DUP-16	sv
320-34917-A-6-A	320-0053155-011	Client	20-Jan-2018 19:34:35	2018.01.20_537AA_014.d	11	1.0	WGNA-010818-RW-3178	sv
320-34917-A-7-A	320-0053155-012	Client	20-Jan-2018 19:39:17	2018.01.20_537AA_015.d	12	1.0	WGNA-010818-FRB-3178	sv
320-34917-A-8-A	320-0053155-013	Client	20-Jan-2018 19:43:57	2018.01.20_537AA_016.d	13	1.0	NAWC-010818-RW-141	sv
CCV L5	320-0053155-014	CCVIS	20-Jan-2018 19:48:38	2018.01.20_537AA_017.d	5	1.0		sv
RB	320-0053155-015	RB	20-Jan-2018 19:53:18	2018.01.20_537AA_018.d	8	1.0		sv
320-34917-A-9-A	320-0053155-016	Client	20-Jan-2018 19:57:59	2018.01.20_537AA_019.d	14	1.0	NAWC-010818-FRB-141	sv
320-34917-A-10-A	320-0053155-017	Client	20-Jan-2018 20:02:40	2018.01.20_537AA_020.d	15	1.0	WGNA-010818-RW-4024	sv
320-34917-A-10-D LMS	320-0053155-018	LMS	20-Jan-2018 20:07:19	2018.01.20_537AA_021.d	16	1.0		sv
320-34917-A-10-E LMSD	320-0053155-019	LMSD	20-Jan-2018 20:11:59	2018.01.20_537AA_022.d	17	1.0		sv
320-34917-A-11-A	320-0053155-020	Client	20-Jan-2018 20:16:40	2018.01.20_537AA_023.d	18	1.0	WGNA-010818-FRB-4024	sv
320-34917-A-12-A	320-0053155-021	Client	20-Jan-2018 20:21:21	2018.01.20_537AA_024.d	19	1.0	WGNA-010818-RW-4844	sv
320-34917-A-13-A	320-0053155-022	Client	20-Jan-2018 20:26:02	2018.01.20_537AA_025.d	20	1.0	WGNA-010818-FRB-4844	sv
320-34917-A-14-A	320-0053155-023	Client	20-Jan-2018 20:30:42	2018.01.20_537AA_026.d	21	1.0	WGNA-010818-RW-0404	sv
320-34917-A-15-A	320-0053155-024	Client	20-Jan-2018 20:35:22	2018.01.20_537AA_027.d	22	1.0	WGNA-010818-FRB-0404	sv
CCV L3	320-0053155-025	CCVIS	20-Jan-2018 20:40:03	2018.01.20_537AA_028.d	3	1.0		sv

Lab ID	Worklist ID	Sample Type	Inj Date/Time	File Name	Vial	Dil Factor	Client ID	Fract
RB	320-0053155-026	RB	20-Jan-2018 20:44:44	2018.01.20_537AA_029.d	8	1.0		sv

TestAmerica Laboratories
Worklist Run Log Report

Worklist Name: 22JAN2018_537A

Worklist Num: 53168

Instrument: A8_N

Method: 537_A8_N

Batch Directory: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53168.b

Anaylysis Type: SemiVOA

Creator: Royce, Amani A

Inj Volume: 2.00

Inj Vol Units: ul

Lab ID	Worklist ID	Sample Type	Inj Date/Time	File Name	Vial	Dil Factor	Client ID	Fract
CCVL	320-0053168-001	CCVL	22-Jan-2018 09:58:02	2018.01.22_537A_004.d	2	1.0		sv
CCV L5	320-0053168-002	CCVIS	22-Jan-2018 10:02:45	2018.01.22_537A_005.d	5	1.0		sv
RB	320-0053168-003	RB	22-Jan-2018 10:07:29	2018.01.22_537A_006.d	8	1.0		sv
320-34917-A-10-A	320-0053168-004	Client	22-Jan-2018 10:12:10	2018.01.22_537A_007.d	15	1.0	WGNA-010818-RW-4024	sv
320-34917-A-10-D LMS	320-0053168-005	LMS	22-Jan-2018 10:16:50	2018.01.22_537A_008.d	16	1.0		sv
320-34917-A-10-E LMSD	320-0053168-006	LMSD	22-Jan-2018 10:21:31	2018.01.22_537A_009.d	17	1.0		sv
CCV L3	320-0053168-007	CCVIS	22-Jan-2018 10:26:11	2018.01.22_537A_010.d	3	1.0		sv
RB	320-0053168-008	RB	22-Jan-2018 10:30:51	2018.01.22_537A_011.d	8	1.0		sv
MB 320-204506/1-A	320-0053168-009	MB	22-Jan-2018 10:35:30	2018.01.22_537A_012.d	23	1.0		sv
LCS 320-204506/2-A	320-0053168-010	LCS	22-Jan-2018 10:40:10	2018.01.22_537A_013.d	24	1.0		sv
LCSD 320-204506/3-A	320-0053168-011	LCSD	22-Jan-2018 10:44:52	2018.01.22_537A_014.d	25	1.0		sv
320-34946-A-1-A	320-0053168-012	Client	22-Jan-2018 10:49:32	2018.01.22_537A_015.d	26	1.0	NAWC-010918-RW-206	sv
320-34946-A-2-A	320-0053168-013	Client	22-Jan-2018 10:54:12	2018.01.22_537A_016.d	27	1.0	NAWC-010918-FRB-206	sv
320-34946-A-3-A	320-0053168-014	Client	22-Jan-2018 10:58:52	2018.01.22_537A_017.d	28	1.0	NAWC-010918-RW-029	sv
320-34946-A-4-A	320-0053168-015	Client	22-Jan-2018 11:03:32	2018.01.22_537A_018.d	29	1.0	NAWC-010918-FRB-029	sv
320-34946-A-5-A	320-0053168-016	Client	22-Jan-2018 11:08:13	2018.01.22_537A_019.d	30	1.0	WGNA-010918-RW-0533	sv
320-34946-A-6-A	320-0053168-017	Client	22-Jan-2018 11:12:53	2018.01.22_537A_020.d	31	1.0	WGNA-010918-FRB-0533	sv
320-34946-A-7-A	320-0053168-018	Client	22-Jan-2018 11:17:33	2018.01.22_537A_021.d	32	1.0	WGNA-010918-RW-3193	sv
CCV L5	320-0053168-019	CCVIS	22-Jan-2018 11:22:13	2018.01.22_537A_022.d	5	1.0		sv
RB	320-0053168-020	RB	22-Jan-2018 11:26:53	2018.01.22_537A_023.d	8	1.0		sv
320-34946-A-8-A	320-0053168-021	Client	22-Jan-2018 11:31:33	2018.01.22_537A_024.d	33	1.0	WGNA-010918-FRB-3193	sv
320-34946-A-9-A	320-0053168-022	Client	22-Jan-2018 11:36:13	2018.01.22_537A_025.d	34	1.0	WGNA-010918-DUP-17	sv
320-34946-A-10-A	320-0053168-023	Client	22-Jan-2018 11:40:53	2018.01.22_537A_026.d	35	1.0	NAWC-010918-RW-138	sv
320-34946-A-11-A	320-0053168-024	Client	22-Jan-2018 11:45:34	2018.01.22_537A_027.d	36	1.0	NAWC-010918-FRB-138	sv
320-34946-A-12-A	320-0053168-025	Client	22-Jan-2018 11:50:14	2018.01.22_537A_028.d	37	1.0	NAWC-010918-RW-351	sv

Lab ID	Worklist ID	Sample Type	Inj Date/Time	File Name	Vial	Dil Factor	Client ID	Fract
320-34946-A-13-A	320-0053168-026	Client	22-Jan-2018 11:54:53	2018.01.22_537A_029.d	38	1.0	NAWC-010918-FRB-351	sv
320-34946-A-14-A	320-0053168-027	Client	22-Jan-2018 11:59:34	2018.01.22_537A_030.d	39	1.0	NAWC-010918-RW-352	sv
320-34946-A-15-A	320-0053168-028	Client	22-Jan-2018 12:04:15	2018.01.22_537A_031.d	40	1.0	NAWC-010918-FRB-352	sv
320-34946-A-16-A	320-0053168-029	Client	22-Jan-2018 12:08:55	2018.01.22_537A_032.d	41	1.0	NAWC-010918-RW-353	sv
320-34946-A-17-A	320-0053168-030	Client	22-Jan-2018 12:13:35	2018.01.22_537A_033.d	42	1.0	NAWC-010918-FRB-353	sv
CCV L3	320-0053168-031	CCVIS	22-Jan-2018 12:18:17	2018.01.22_537A_034.d	3	1.0		sv
RB	320-0053168-032	RB	22-Jan-2018 12:22:57	2018.01.22_537A_035.d	8	1.0		sv
320-34946-A-18-A	320-0053168-033	Client	22-Jan-2018 12:27:38	2018.01.22_537A_036.d	43	1.0	NAWC-010918-RW-350	sv
320-34946-A-19-A	320-0053168-034	Client	22-Jan-2018 12:32:17	2018.01.22_537A_037.d	44	1.0	NAWC-010918-FRB-350	sv
CCV L5	320-0053168-035	CCVIS	22-Jan-2018 12:36:59	2018.01.22_537A_038.d	5	1.0		sv
RB	320-0053168-036	RB	22-Jan-2018 12:41:39	2018.01.22_537A_039.d	8	1.0		sv

TestAmerica Laboratories
Worklist Run Log Report

Worklist Name: 22JAN2018_537B

Worklist Num: 53187

Instrument: A8_N

Method: 537_A8_N

Batch Directory: \\ChromNa\Sacramento\ChromData\A8_N\20180122-53187.b

Analysis Type: SemiVOA

Creator: Royce, Amani A

Inj Volume: 2.00

Inj Vol Units: ul

Lab ID	Worklist ID	Sample Type	Inj Date/Time	File Name	Vial	Dil Factor	Client ID	Fract
CCV L3	320-0053187-001	CCVIS	22-Jan-2018 16:15:57	2018.01.22_537AA_010.d	3	1.0		sv
RB	320-0053187-002	RB	22-Jan-2018 16:20:37	2018.01.22_537AA_011.d	8	1.0		sv
MB 320-204506/1-A	320-0053187-003	MB	22-Jan-2018 16:25:18	2018.01.22_537AA_012.d	23	1.0		sv
LCS 320-204506/2-A	320-0053187-004	LCS	22-Jan-2018 16:29:58	2018.01.22_537AA_013.d	24	1.0		sv
LCSD 320-204506/3-A	320-0053187-005	LCSD	22-Jan-2018 16:34:38	2018.01.22_537AA_014.d	25	1.0		sv
320-34946-A-1-A	320-0053187-006	Client	22-Jan-2018 16:39:19	2018.01.22_537AA_015.d	26	1.0	NAWC-010918-RW-206	sv
320-34946-A-2-A	320-0053187-007	Client	22-Jan-2018 16:43:59	2018.01.22_537AA_016.d	27	1.0	NAWC-010918-FRB-206	sv
320-34946-A-3-A	320-0053187-008	Client	22-Jan-2018 16:48:38	2018.01.22_537AA_017.d	28	1.0	NAWC-010918-RW-029	sv
320-34946-A-4-A	320-0053187-009	Client	22-Jan-2018 16:53:19	2018.01.22_537AA_018.d	29	1.0	NAWC-010918-FRB-029	sv
320-34946-A-5-A	320-0053187-010	Client	22-Jan-2018 16:58:00	2018.01.22_537AA_019.d	30	1.0	WGNA-010918-RW-0533	sv
320-34946-A-6-A	320-0053187-011	Client	22-Jan-2018 17:02:40	2018.01.22_537AA_020.d	31	1.0	WGNA-010918-FRB-0533	sv
320-34946-A-7-A	320-0053187-012	Client	22-Jan-2018 17:07:20	2018.01.22_537AA_021.d	32	1.0	WGNA-010918-RW-3193	sv
CCV L5	320-0053187-013	CCVIS	22-Jan-2018 17:12:01	2018.01.22_537AA_022.d	5	1.0		sv
RB	320-0053187-014	RB	22-Jan-2018 17:16:40	2018.01.22_537AA_023.d	8	1.0		sv

TestAmerica Laboratories
Worklist Run Log Report

Worklist Name: 23JAN2018_537A

Worklist Num: 53264

Instrument: A8_N

Method: 537_A8_N

Batch Directory: \\ChromNa\Sacramento\ChromData\A8_N\20180124-53264.b

Analysis Type: SemiVOA

Creator: Royce, Armani A

Inj Volume: 2.00

Inj Vol Units: ul

Lab ID	Worklist ID	Sample Type	Inj Date/Time	File Name	Vial	Dil Factor	Client ID	Fract
CCVL	320-0053264-001	CCVL	24-Jan-2018 05:01:08	2018.01.23537A_004.d	2	1.0		sv
CCV L5	320-0053264-002	CCVIS	24-Jan-2018 05:05:49	2018.01.23537A_005.d	5	1.0		sv
RB	320-0053264-003	RB	24-Jan-2018 05:10:30	2018.01.23537A_006.d	8	1.0		sv
320-34917-A-9-A	320-0053264-004	Client	24-Jan-2018 05:15:10	2018.01.23537A_007.d	14	1.0	NAWC-010818-FRB-141	sv
320-34917-A-10-A	320-0053264-005	Client	24-Jan-2018 05:19:52	2018.01.23537A_008.d	15	1.0	WGNA-010818-RW-4024	sv
320-34917-A-10-D LMS	320-0053264-006	LMS	24-Jan-2018 05:24:32	2018.01.23537A_009.d	16	1.0		sv
320-34917-A-10-E LMSD	320-0053264-007	LMSD	24-Jan-2018 05:29:13	2018.01.23537A_010.d	17	1.0		sv
320-34917-A-11-A	320-0053264-008	Client	24-Jan-2018 05:33:54	2018.01.23537A_011.d	18	1.0	WGNA-010818-FRB-4024	sv
320-34917-A-12-A	320-0053264-009	Client	24-Jan-2018 05:38:35	2018.01.23537A_012.d	19	1.0	WGNA-010818-RW-4844	sv
320-34917-A-13-A	320-0053264-010	Client	24-Jan-2018 05:43:15	2018.01.23537A_013.d	20	1.0	WGNA-010818-FRB-4844	sv
320-34917-A-14-A	320-0053264-011	Client	24-Jan-2018 05:47:56	2018.01.23537A_014.d	21	1.0	WGNA-010818-RW-0404	sv
320-34917-A-15-A	320-0053264-012	Client	24-Jan-2018 05:52:37	2018.01.23537A_015.d	22	1.0	WGNA-010818-FRB-0404	sv
CCV L3	320-0053264-013	CCVIS	24-Jan-2018 05:57:17	2018.01.23537A_016.d	3	1.0		sv
RB	320-0053264-014	RB	24-Jan-2018 06:01:58	2018.01.23537A_017.d	8	1.0		sv
MB 320-204684/1-A	320-0053264-015	MB	24-Jan-2018 06:06:38	2018.01.23537A_018.d	45	1.0		sv
LCS 320-204684/2-A	320-0053264-016	LCS	24-Jan-2018 06:11:17	2018.01.23537A_019.d	46	1.0		sv
320-35149-A-1-A	320-0053264-017	Client	24-Jan-2018 06:15:57	2018.01.23537A_020.d	47	1.0	WS-025	sv
320-35149-A-2-A	320-0053264-018	Client	24-Jan-2018 06:20:38	2018.01.23537A_021.d	48	1.0	DUP-14	sv
320-35149-A-3-A	320-0053264-019	Client	24-Jan-2018 06:25:19	2018.01.23537A_022.d	49	1.0	FIELD BLANK (01/16/2018)	sv
320-35149-A-4-A	320-0053264-020	Client	24-Jan-2018 06:29:59	2018.01.23537A_023.d	50	1.0	WS-092	sv
320-35149-A-4-B MS	320-0053264-021	MS	24-Jan-2018 06:34:39	2018.01.23537A_024.d	51	1.0	WS-092	sv
320-35149-A-4-C MSD	320-0053264-022	MSD	24-Jan-2018 06:39:20	2018.01.23537A_025.d	52	1.0	WS-092	sv
QC ICV	320-0053264-023	QC	24-Jan-2018 06:44:00	2018.01.23537A_026.d	54	1.0		sv
CCV L5	320-0053264-024	CCVIS	24-Jan-2018 06:48:41	2018.01.23537A_027.d	5	1.0		sv
RB	320-0053264-025	RB	24-Jan-2018 06:53:20	2018.01.23537A_028.d	8	1.0		sv

55

Aqueous Extraction Analysis Sheet

A8 1/22/18

(To Accompany Samples to Instruments)

Batch Number: 320-204506











Analyst: Kolstad, Kate M

Batch Open: 1/18/2018 12:21:00PM

Method Code: 320-537_Prep-320

Batch End: 1/19/2018 4:56:00PM

Extraction of Perfluorinated Alkyl Acids

Input Sample Lab ID (Analytical Method)	SDG (Job #)	GrossWt TareWt	InitAmnt FinAmnt	PHs Rcvd	Adj1	Adj2	Due Date	Analytical TAT	Div Rank	Comments	Output Sample Lab ID
1 MB-320-204506/1 N/A	N/A		250.0 mL	7			N/A	N/A	N/A	CI ND RI	
			1.0 mL								
2 LCS-320-204506/2 N/A	N/A		250.0 mL	7			N/A	N/A	N/A	CI ND	
			1.0 mL								
3 LCSD-320-204506/3 N/A	N/A		250.0 mL	7			N/A	N/A	N/A	CI ND	
			1.0 mL								
4 320-34946-A-1 (537_DOD5)	N/A (320-34946-1)	278.90 g	251.3 mL	7			1/14/18	16_Days	4	CI ND	
		27.62 g	1.0 mL								
5 320-34946-A-2 (537_DOD5)	N/A (320-34946-1)	273.25 g	245.8 mL	7			1/14/18	16_Days	4	CI ND	
		27.44 g	1.0 mL								
6 320-34946-A-3 (537_DOD5)	N/A (320-34946-1)	272.94 g	245.5 mL	7			1/14/18	16_Days	4	CI ND	
		27.49 g	1.0 mL								
7 320-34946-A-4 (537_DOD5)	N/A (320-34946-1)	275.56 g	247.8 mL	7			1/14/18	16_Days	4	CI ND	
		27.80 g	1.0 mL								
8 320-34946-A-5 (537_DOD5)	N/A (320-34946-1)	275.23 g	248.2 mL	7			1/14/18	16_Days	4	CI ND	
		27.08 g	1.0 mL								
9 320-34946-A-6 (537_DOD5)	N/A (320-34946-1)	274.51 g	246.8 mL	7			1/14/18	16_Days	4	CI ND	
		27.73 g	1.0 mL								
10 320-34946-A-7 (537_DOD5)	N/A (320-34946-1)	270.99 g	243.5 mL	7			1/14/18	16_Days	4	CI ND	
		27.46 g	1.0 mL								

Page 313 of 329



Aqueous Extraction Analysis Sheet

(To Accompany Samples to Instruments)













Batch Number: 320-204506

Analyst: Kolstad, Kate M

Batch Open: 1/18/2018 12:21:00PM

Method Code: 320-537_Prep-320

Batch End: 1/19/2018 4:56:00PM

11	320-34946-A-8 (537_DOD5)	N/A (320-34946-1)	273.10 g	245.6 mL	7		1/14/18	16_Days	4	CI ND	
			27.47 g	1.0 mL							
12	320-34946-A-9 (537_DOD5)	N/A (320-34946-1)	276.66 g	249.2 mL	7		1/14/18	16_Days	4	CI ND	
			27.47 g	1.0 mL							
13	320-34946-A-10 (537_DOD5)	N/A (320-34946-1)	268.45 g	240.1 mL	7		1/14/18	16_Days	4	CI ND	
			28.37 g	1.0 mL							
14	320-34946-A-11 (537_DOD5)	N/A (320-34946-1)	272.57 g	245.2 mL	7		1/14/18	16_Days	4	CI ND	
			27.35 g	1.0 mL							
15	320-34946-A-12 (537_DOD5)	N/A (320-34946-1)	274.45 g	246.8 mL	7		1/14/18	16_Days	4	CI ND	
			27.67 g	1.0 mL							
16	320-34946-A-13 (537_DOD5)	N/A (320-34946-1)	277.01 g	250 mL	7		1/14/18	16_Days	4	CI ND	
			27.05 g	1.0 mL							
17	320-34946-A-14 (537_DOD5)	N/A (320-34946-1)	275.28 g	247.8 mL	7		1/14/18	16_Days	4	CI ND	
			27.45 g	1.0 mL							
18	320-34946-A-15 (537_DOD5)	N/A (320-34946-1)	272.12 g	244.9 mL	7		1/14/18	16_Days	4	CI ND	
			27.21 g	1.0 mL							
19	320-34946-A-16 (537_DOD5)	N/A (320-34946-1)	271.46 g	244 mL	7		1/14/18	16_Days	4	CI ND	
			27.49 g	1.0 mL							
20	320-34946-A-17 (537_DOD5)	N/A (320-34946-1)	274.27 g	246.6 mL	7		1/14/18	16_Days	4	CI ND	
			27.72 g	1.0 mL							
21	320-34946-A-18 (537_DOD5)	N/A (320-34946-1)	267.71 g	240 mL	7		1/14/18	16_Days	4	CI ND	
			27.75 g	1.0 mL							
22	320-34946-A-19 (537_DOD5)	N/A (320-34946-1)	274.62 g	247.4 mL	7		1/14/18	16_Days	4	CI ND	
			27.21 g	1.0 mL							

Page 314 of 329

Aqueous Extraction Analysis Sheet

(To Accompany Samples to Instruments)

Batch Number: 320-204506

Analyst: Kolstad, Kate M

Batch Open: 1/18/2018 12:21:00PM

Method Code: 320-537_Prep-320

Batch End: 1/19/2018 4:56:00PM

Batch Notes

Manifold ID 3, 4

pH Indicator ID 2517

Trizma ID SLBR4303V

SPE Cartridge ID 6357081-11

Methanol ID 1127832

Reagent Water ID 1-11-18

Internal Standard ID# 1099356

Pipette ID M16387D

Analyst ID - TA Reagent Drop CCB

Analyst ID - TA Reagent Drop KMK

Witness

Analyst ID - SU Reagent Drop CCB

Analyst ID - SU Reagent Drop KMK

Witness

Analyst ID - IS Reagent Drop JER

Analyst ID - IS Reagent Drop KMK

Witness

Analyst ID - Concentration CCB/KMK

Analyst ID - Aliquot Step KMK

Analyst ID - Final Volume Step KMK

Batch Comment Label ID's checked: KMK 1-18-18

Aqueous Extraction Analysis Sheet

(To Accompany Samples to Instruments)

Batch Number: 320-204506

Analyst: Kolstad, Kate M

Batch Open: 1/18/2018 12:21:00PM

Method Code: 320-537__Prep-320

Batch End:

Comments

Aqueous Extraction Analysis Sheet

(To Accompany Samples to Instruments)

Batch Number: 320-204506



Analyst: Kolstad, Kate M

Batch Open: 1/18/2018 12:21:00PM

Method Code: 320-537_Prep-320

Batch End:

Reagent Additions Worksheet

Lab ID	Reagent Code	Amount Added	Final Amount	By	Witness
MB 320-204506/1	LC537-SU_00054	100 uL	1.0 mL	<i>ceB 1-18-18</i> 	<i>KMK 1-18-18</i> 
LCS 320-204506/2	LC537-MSP_00027	100 uL	1.0 mL		
LCS 320-204506/2	LC537-SU_00054	100 uL	1.0 mL		
LCSD 320-204506/3	LC537-MSP_00027	100 uL	1.0 mL		
LCSD 320-204506/3	LC537-SU_00054	100 uL	1.0 mL		
320-34946-A-1	LC537-SU_00054	100 uL	1.0 mL		
320-34946-A-2	LC537-SU_00054	100 uL	1.0 mL		
320-34946-A-3	LC537-SU_00054	100 uL	1.0 mL		
320-34946-A-4	LC537-SU_00054	100 uL	1.0 mL		
320-34946-A-5	LC537-SU_00054	100 uL	1.0 mL		
320-34946-A-6	LC537-SU_00054	100 uL	1.0 mL		
320-34946-A-7	LC537-SU_00054	100 uL	1.0 mL		
320-34946-A-8	LC537-SU_00054	100 uL	1.0 mL		
320-34946-A-9	LC537-SU_00054	100 uL	1.0 mL		
320-34946-A-10	LC537-SU_00054	100 uL	1.0 mL		
320-34946-A-11	LC537-SU_00054	100 uL	1.0 mL		
320-34946-A-12	LC537-SU_00054	100 uL	1.0 mL		
320-34946-A-13	LC537-SU_00054	100 uL	1.0 mL		

Page 317 of 329

Aqueous Extraction Analysis Sheet

(To Accompany Samples to Instruments)

Batch Number: 320-204506

Analyst: Kolstad, Kate M

Batch Open: 1/18/2018 12:21:00PM

Method Code: 320-537_Prep-320

Batch End:

320-34946-A-14	LC537-SU_00054	100 uL	1.0 mL	1-18-18 ↓	KMK 1-18-18 ↓
320-34946-A-15	LC537-SU_00054	100 uL	1.0 mL		
320-34946-A-16	LC537-SU_00054	100 uL	1.0 mL		
320-34946-A-17	LC537-SU_00054	100 uL	1.0 mL		
320-34946-A-18	LC537-SU_00054	100 uL	1.0 mL		
320-34946-A-19	LC537-SU_00054	100 uL	1.0 mL		

Other Reagents:

Reagent

Amount/Units

Lot#:

Page 318 of 329

Preparation Batch Number(s) 204506 Test 537

Earliest Holding Time 1-23-18

Batch Information	1 st Level Reviewer	2 nd Level Reviewer
Date and time accurate and entered into TALS correctly	/	✓
All necessary batch information complete and entered into TALS correctly	/	✓
BD, FV, and AL initials are transcribed into the batch comment	/	✓
Sample List Tab	1 st Level Reviewer	2 nd Level Reviewer
Samples identified to the correct method	/	✓
Holding time violation NCM filed	NA	NA
MS/MSD or MS/DU NCM filed	/	✓
NCM for any anomalies filed	NA	NA
All NCMs include method code, matrix, and prep batch	/	✓
Method/sample/login/QAS checked and correct	/	✓
Batch contains no more than 20 live samples	/	✓
Worksheet Tab	1 st Level Reviewer	2 nd Level Reviewer
All samples properly preserved	/	✓
Weights in anticipated range and not targeted	/	✓
All additional test requirements performed, documented, and uploaded to TALS correctly (e.g. final amount, initial amount, turbidity, and CI Check)	/	✓
The pH is transcribed properly in TALS	/	✓
All additional information is transcribed into TALS and is correct and raw data is attached	/	✓
Comments/Observations are transcribed correctly in TALS	/	✓
Reagents Tab	1 st Level Reviewer	2 nd Level Reviewer
All necessary reagents not expired and checked into TALS	/	✓
All spike amounts correct and added to necessary samples and QC	/	✓
Internal Standard is added to the reagents	/	✓
All units are correctly transcribed into TALS	/	✓

1st Level Reviewer: kmk

Date: 1-19-18

2nd Level Reviewer: VPM

Date: 1/22/18

Comments: _____

54

Aqueous Extraction Analysis Sheet

(To Accompany Samples to Instruments)

AS 1/20/18
AS 1/22/18
AY 1/23/18

Batch Number: 320-204304

Analyst: Kouchari, Shamiran

Batch Open: 1/17/2018 10:49:00AM

Method Code: 320-537_Prep-320

Batch End: 1/18/2018 6:46:00PM

Extraction of Perfluorinated Alkyl Acids

	Input Sample Lab ID (Analytical Method)	SDG (Job #)	GrossWt TareWt	InitAmnt FinAmnt	PHs		Due Date	Analytical TAT	Div Rank	Comments	Output Sample Lab ID	
					Rcvd	Adj1						Adj2
1	MB-320-204304/1 N/A	N/A		250 mL	7			N/A	N/A	N/A	ch nd	
				1.00 mL								
2	LLCS-320-204304/2 N/A	N/A		250 mL	7			N/A	N/A	N/A	ch nd	
				1.00 mL								
3	320-34917-A-1 (537_DOD5)	N/A (320-34917-1)	276.13 g	248.7 mL	7			1/13/18	16_Days	4	ch nd	
			27.43 g	1.00 mL								
	320-34917-A-2 (537_DOD5)	N/A (320-34917-1)	280.44 g	253.2 mL	7			1/13/18	16_Days	4	ch nd	
			27.20 g	1.00 mL								
	320-34917-A-3 (537_DOD5)	N/A (320-34917-1)	285.26 g	257.4 mL	7			1/13/18	16_Days	4	ch nd	
			27.84 g	1.00 mL								
6	320-34917-A-4 (537_DOD5)	N/A (320-34917-1)	283.33 g	256.1 mL	7			1/13/18	16_Days	4	ch nd	
			27.28 g	1.00 mL								
7	320-34917-A-5 (537_DOD5)	N/A (320-34917-1)	290.10 g	262.5 mL	7			1/13/18	16_Days	4	ch nd	
			27.65 g	1.00 mL								
8	320-34917-A-6 (537_DOD5)	N/A (320-34917-1)	267.18 g	239.2 mL	7			1/13/18	16_Days	4	ch nd	
			27.96 g	1.00 mL								
9	320-34917-A-7 (537_DOD5)	N/A (320-34917-1)	284.45 g	256.7 mL	7			1/13/18	16_Days	4	ch nd	
			27.74 g	1.00 mL								
10	320-34917-A-8 (537_DOD5)	N/A (320-34917-1)	284.94 g	257.5 mL	7			1/13/18	16_Days	4	ch nd	
			27.43 g	1.00 mL								

Page 320 of 329

Aqueous Extraction Analysis Sheet

(To Accompany Samples to Instruments)










Batch Number: 320-204304

Analyst: Kouchari, Shamiran

Batch Open: 1/17/2018 10:49:00AM

Method Code: 320-537_Prep-320

Batch End: 1/18/2018 6:46:00PM

11	320-34917-A-9 (537_DOD5)	N/A (320-34917-1)	293.45 g	266.1 mL	7		1/13/18	16_Days	4	ch nd	RI	
			27.32 g	1.00 mL								
12	320-34917-A-10 (537_DOD5)	N/A (320-34917-1)	278.90 g	251.2 mL	7		1/13/18	16_Days	4	ch nd	RI	
			27.73 g	1.00 mL								
13	320-34917-A-10-LMS (537_DOD5)	N/A (320-34917-1)	276.69 g	249.1 mL	7		1/13/18	16_Days	4	ch nd	RI	
			27.64 g	1.00 mL								
14	320-34917-A-10-LMSD (537_DOD5)	N/A (320-34917-1)	285.36 g	257.7 mL	7		1/13/18	16_Days	4	ch nd	RI	
			27.65 g	1.00 mL								
15	320-34917-A-11 (537_DOD5)	N/A (320-34917-1)	284.88 g	257.4 mL	7		1/13/18	16_Days	4	ch nd	RI	
			27.53 g	1.00 mL								
16	320-34917-A-12 (537_DOD5)	N/A (320-34917-1)	281.28 g	253.5 mL	7		1/13/18	16_Days	4	ch nd		
			27.81 g	1.00 mL								
17	320-34917-A-13 (537_DOD5)	N/A (320-34917-1)	276.54 g	249.5 mL	7		1/13/18	16_Days	4	ch nd		
			27.04 g	1.00 mL								
18	320-34917-A-14 (537_DOD5)	N/A (320-34917-1)	276.80 g	249.4 mL	7		1/13/18	16_Days	4	ch nd		
			27.41 g	1.00 mL								
19	320-34917-A-15 (537_DOD5)	N/A (320-34917-1)	279.74 g	252.5 mL	7		1/13/18	16_Days	4	ch nd		
			27.27 g	1.00 mL								

Page 321 of 329

Aqueous Extraction Analysis Sheet

(To Accompany Samples to Instruments)

Batch Number: 320-204304

Analyst: Kouchari, Shamiran

Batch Open: 1/17/2018 10:49:00AM

Method Code: 320-537_Prep-320

Batch End: 1/18/2018 6:46:00PM

Batch Notes

Manifold ID 3,1

pH Indicator ID 1617

Trizma ID SLBR4303V

SPE Cartridge ID 6357081-11

Methanol ID 1123833

Reagent Water ID 1-11-18

Internal Standard ID# 1099356

Pipette ID M16387D

Analyst ID - TA Reagent Drop CCB

Analyst ID - TA Reagent Drop HJA

Witness

Analyst ID - SU Reagent Drop CCB

Analyst ID - SU Reagent Drop HJA

Witness

Analyst ID - IS Reagent Drop JER

Analyst ID - IS Reagent Drop KMK

Witness

Analyst ID - Concentration CCB

Analyst ID - Aliquot Step KMK

Analyst ID - Final Volume Step KMK

Batch Comment Label ID's checked: SKD 1-17-18

Aqueous Extraction Analysis Sheet

(To Accompany Samples to Instruments)

Batch Number: 320-204304

Analyst: Kouchari, Shamiran

Batch Open: 1/17/2018 10:49:00AM

Method Code: 320-537_Prep-320

Batch End: 1/18/2018 6:46:00PM

Comments

Aqueous Extraction Analysis Sheet

(To Accompany Samples to Instruments)

Batch Number: 320-204304

Analyst: Kouchari, Shamiran

Batch Open: 1/17/2018 10:49:00AM

Method Code: 320-537_Prep-320

Batch End:

Reagent Additions Worksheet

Lab ID	Reagent Code	Amount Added	Final Amount	By	Witness
MB 320-204304/1	LC537-SU_00054	100 uL	1.00 mL	CBS 1-17-18	HSD 1-17-18
LLCS 320-204304/2	LC537-LSP_00025	100 uL	1.00 mL		
LLCS 320-204304/2	LC537-SU_00054	100 uL	1.00 mL		
320-34917-A-1	LC537-SU_00054	100 uL	1.00 mL		
320-34917-A-2	LC537-SU_00054	100 uL	1.00 mL		
320-34917-A-3	LC537-SU_00054	100 uL	1.00 mL		
320-34917-A-4	LC537-SU_00054	100 uL	1.00 mL		
320-34917-A-5	LC537-SU_00054	100 uL	1.00 mL		
320-34917-A-6	LC537-SU_00054	100 uL	1.00 mL		
320-34917-A-7	LC537-SU_00054	100 uL	1.00 mL		
320-34917-A-8	LC537-SU_00054	100 uL	1.00 mL		
320-34917-A-9	LC537-SU_00054	100 uL	1.00 mL		
320-34917-A-10	LC537-SU_00054	100 uL	1.00 mL		
320-34917-A-10 LMS	LC537-LSP_00025	100 uL	1.00 mL		
320-34917-A-10 LMS	LC537-SU_00054	100 uL	1.00 mL		
320-34917-A-10 LMSD	LC537-LSP_00025	100 uL	1.00 mL		
320-34917-A-10 LMSD	LC537-SU_00054	100 uL	1.00 mL		
320-34917-A-11	LC537-SU_00054	100 uL	1.00 mL	N	

Page 324 of 329

Aqueous Extraction Analysis Sheet

(To Accompany Samples to Instruments)

Batch Number: 320-204304

Analyst: Kouchari, Shamiran

Batch Open: 1/17/2018 10:49:00AM

Method Code: 320-537_Prep-320

Batch End:

320-34917-A-12	LC537-SU_00054	100 uL	1.00 mL	<i>CES 1-17-18</i> ↓	<i>HSA 1-17-18</i> ↓
320-34917-A-13	LC537-SU_00054	100 uL	1.00 mL		
320-34917-A-14	LC537-SU_00054	100 uL	1.00 mL		
320-34917-A-15	LC537-SU_00054	100 uL	1.00 mL		

Other Reagents:

Reagent	Amount/Units	Lot#:

Page 325 of 329

Preparation Batch Number(s) 204304 Test 537

Earliest Holding Time 1-22-18

Batch Information	1 st Level Reviewer	2 nd Level Reviewer
Date and time accurate and entered into TALS correctly	/	✓
All necessary batch information complete and entered into TALS correctly	/	✓
BD, FV, and AL initials are transcribed into the batch comment	/	✓
Sample List Tab	1 st Level Reviewer	2 nd Level Reviewer
Samples identified to the correct method	/	✓
Holding time violation NCM filed	NA	NA
MS/MSD or MS/DU NCM filed	NA	NA
NCM for any anomalies filed	NA	NA
All NCMs include method code, matrix, and prep batch	NA	NA
Method/sample/login/QAS checked and correct	/	✓
Batch contains no more than 20 live samples	/	✓
Worksheet Tab	1 st Level Reviewer	2 nd Level Reviewer
All samples properly preserved	/	✓
Weights in anticipated range and not targeted	/	✓
All additional test requirements performed, documented, and uploaded to TALS correctly (e.g. final amount, initial amount, turbidity, and CI Check)	/	✓
The pH is transcribed properly in TALS	/	✓
All additional information is transcribed into TALS and is correct and raw data is attached	/	✓
Comments/Observations are transcribed correctly in TALS	/	✓
Reagents Tab	1 st Level Reviewer	2 nd Level Reviewer
All necessary reagents not expired and checked into TALS	/	✓
All spike amounts correct and added to necessary samples and QC	/	✓
Internal Standard is added to the reagents	/	✓
All units are correctly transcribed into TALS	/	✓

1st Level Reviewer: KMK

Date: 1-18-18

2nd Level Reviewer: VPM

Date: 1/22/18

Comments: VPM 1/22/18

Shipping and Receiving Documents

TestAmerica Sacramento
 880 Riverside Parkway
 West Sacramento, CA 95605-1500
 phone 916.373.5600 fax 303.467.7248

Chain of Custody Record

TestAmerica
 THE LEADER IN ENVIRONMENTAL TESTING
TestAmerica Laboratories, Inc.

Regulatory Program: DW NPDES RCRA Other:

Client Contact	Project Manager: Andy Frebowitz	Site Contact: Mary Kay Bond	Date: 1/8/2018	COC No:
TetraTech	Tel/Fax: 610.382.1170	Lab Contact: Dave Alltucker	Carrier: FedEx	1 of 1 COCs
234 Mall Boulevard Suite 260	Analysis Turnaround Time			Sampler: Mary Kay Bond
King of Prussia, PA 19406	<input type="checkbox"/> CALENDAR DAYS <input type="checkbox"/> WORKING DAYS			For Lab Use Only:
610-382-1174	TAT if different from Below 21			Walk-in Client:
610-491-9688	<input type="checkbox"/> 2 weeks			Lab Sampling:
Project Name: WE04	<input type="checkbox"/> 1 week			
Site: WE04	<input type="checkbox"/> 2 days			
P O # 1132358 (through EarthToxics)	<input type="checkbox"/> 1 day			Job / SDG No.:


Sample Identification	Sample Date	Sample Time	Sample Type (C=Comp, G=Grab)	Matrix	# of Cont.	Filtered Sample (Y/N)	Perform MS/MSD (Y/N)	EPA 537 UCMRS	Sample Specific Notes:
WGNA-010818-RW-0344	1/8/2018	08:10	G	DW	2	N	N	Y	
WGNA-010818-FRB-0344	1/8/2018	08:05	G	DW	2	N	N	Y	Field Reagent Blank
WGNA-010818-RW-3957	1/8/2018	08:40	G	DW	2	N	N	Y	
WGNA-010818-FRB-3957	1/8/2018	08:35	G	DW	2	N	N	Y	Field Reagent Blank
WGNA-010818-DUP-16	1/8/2018	07:00	G	DW	2	N	N	Y	Duplicate
WGNA-010818-RW-3178	1/8/2018	10:10	G	DW	2	N	N	Y	
WGNA-010818-FRB-3178	1/8/2018	10:05	G	DW	2	N	N	Y	Field Reagent Blank
NAWC-010818-RW-141	1/8/2018	11:10	G	DW	2	N	N	Y	
NAWC-010818-FRB-141	1/8/2018	11:05	G	DW	2	N	N	Y	Field Reagent Blank
WGNA-010818-RW-4024	1/8/2018	11:40	G	DW	6	N	Y	Y	MS/MSD
WGNA-010818-FRB-4024	1/8/2018	11:35	G	DW	2	N	N	Y	Field Reagent Blank
WGNA-010818-RW-4844	1/8/2018	13:10	G	DW	2	N	N	Y	
WGNA-010818-FRB-4844	1/8/2018	13:05	G	DW	2	N	N	Y	Field Reagent Blank
WGNA-010818-RW-0404	1/8/2018	09:40	G	DW	2	N	N	Y	
WGNA-010818-FRB-0404	1/8/2018	09:35	G	DW	2	N	N	Y	Field Reagent Blank

Preservation Used: 1= Ice, 2= HCl; 3= H2SO4; 4=HNO3; 5=NaOH; 6= Other: Trizma

Possible Hazard Identification: Are any samples from a listed EPA Hazardous Waste? Please List any EPA Waste Codes for the sample in the	Sample Disposal (A fee may be assessed if samples are retained longer than 1 month)
<input checked="" type="checkbox"/> Non-Hazard <input type="checkbox"/> Flammable <input type="checkbox"/> Skin Irritant <input type="checkbox"/> Poison B <input type="checkbox"/> Unknown	<input type="checkbox"/> Return to Client <input checked="" type="checkbox"/> Disposal by Lab <input type="checkbox"/> Archive for _____ Months

Fed Ex Tracking: 77116333 5860

Custody Seals Intact: <input type="checkbox"/> Yes <input type="checkbox"/> No	Custody Seal No.:	Cooler Temp. (°C): Obs'd: 5.2	Corr'd: 5.2	Therm ID No.: AK-2 100
Relinquished by: <i>Christina M. Simon</i>	Company: Tetra Tech	Date/Time: 1/8/2018 18:00	Received by: <i>D. Alltucker</i>	Company: <i>THSae</i>
Relinquished by:	Company:	Date/Time:	Received by:	Company:
Relinquished by:	Company:	Date/Time:	Received in Laboratory by:	Company:



320-34917 Chain of Custody

Page 328 of 329

Login Sample Receipt Checklist

Client: Tetra Tech, Inc.

Job Number: 320-34917-1

Login Number: 34917

List Source: TestAmerica Sacramento

List Number: 1

Creator: Turpen, Troy

Question	Answer	Comment
Radioactivity wasn't checked or is \leq background as measured by a survey meter.	True	
The cooler's custody seal, if present, is intact.	True	
Sample custody seals, if present, are intact.	N/A	
The cooler or samples do not appear to have been compromised or tampered with.	True	
Samples were received on ice.	True	
Cooler Temperature is acceptable.	True	
Cooler Temperature is recorded.	True	
COC is present.	True	
COC is filled out in ink and legible.	True	
COC is filled out with all pertinent information.	True	
Is the Field Sampler's name present on COC?	True	
There are no discrepancies between the containers received and the COC.	True	
Samples are received within Holding Time (excluding tests with immediate HTs)	True	
Sample containers have legible labels.	True	
Containers are not broken or leaking.	True	
Sample collection date/times are provided.	True	
Appropriate sample containers are used.	True	
Sample bottles are completely filled.	True	
Sample Preservation Verified.	N/A	
There is sufficient vol. for all requested analyses, incl. any requested MS/MSDs	True	
Containers requiring zero headspace have no headspace or bubble is $<6\text{mm}$ (1/4").	True	
Multiphasic samples are not present.	True	
Samples do not require splitting or compositing.	True	
Residual Chlorine Checked.	N/A	

"WGNA-010818-RW-0344", "537", "RES", "320-34917-1", "TALSAC", "1763-23-1", "Perfluorooctanesulfonic acid (PFOS)", "32", "ng/L", "J", "6.8", "DL", "", "TRG", "", "", "40", "LOQ", "YES", "-99", "", "248.7", "1.00", "16", ""

"WGNA-010818-RW-0344", "537", "RES", "320-34917-1", "TALSAC", "335-67-1", "Perfluorooctanoic acid (PFOA)", "24", "ng/L", "", "2.8", "DL", "", "TRG", "", "", "20", "LOQ", "YES", "-99", "", "248.7", "1.00", "8.0", ""

"WGNA-010818-RW-0344", "537", "RES", "320-34917-1", "TALSAC", "355-46-4", "Perfluorohexanesulfonic acid (PFHxS)", "18", "ng/L", "J", "5.5", "DL", "", "TRG", "", "", "30", "LOQ", "YES", "-99", "", "248.7", "1.00", "12", ""

"WGNA-010818-RW-0344", "537", "RES", "320-34917-1", "TALSAC", "375-73-5", "Perfluorobutanesulfonic acid (PFBS)", "36", "ng/L", "U", "16", "DL", "", "TRG", "", "", "90", "LOQ", "YES", "-99", "", "248.7", "1.00", "36", ""

"WGNA-010818-RW-0344", "537", "RES", "320-34917-1", "TALSAC", "375-85-9", "Perfluoroheptanoic acid (PFHpA)", "6.4", "ng/L", "J", "1.9", "DL", "", "TRG", "", "", "10", "LOQ", "YES", "-99", "", "248.7", "1.00", "4.0", ""

"WGNA-010818-RW-0344", "537", "RES", "320-34917-1", "TALSAC", "375-95-1", "Perfluorononanoic acid (PFNA)", "32", "ng/L", "", "8.0", "DL", "", "TRG", "", "", "24", "LOQ", "YES", "-99", "", "248.7", "1.00", "20", ""

"WGNA-010818-RW-0344", "537", "RES", "320-34917-1", "TALSAC", "STL00993", "13C2 PFHxA", "36", "ng/L", "", "-99", "DL", "", "SURR", "91", "", "-99", "LOQ", "YES", "40.2", "", "248.7", "1.00", "0", ""

"WGNA-010818-RW-0344", "537", "RES", "320-34917-1", "TALSAC", "STL00996", "13C2 PFDA", "38", "ng/L", "", "-99", "DL", "", "SURR", "93", "", "-99", "LOQ", "YES", "40.2", "", "248.7", "1.00", "0", ""

"WGNA-010818-RW-4024", "537", "RES", "320-34917-10", "TALSAC", "1763-23-1", "Perfluorooctanesulfonic acid (PFOS)", "18", "ng/L", "J M", "6.8", "DL", "", "TRG", "", "", "40", "LOQ", "YES", "-99", "", "251.2", "1.00", "16", ""

"WGNA-010818-RW-4024", "537", "RES", "320-34917-10", "TALSAC", "335-67-1", "Perfluorooctanoic acid (PFOA)", "12", "ng/L", "J", "2.8", "DL", "", "TRG", "", "", "20", "LOQ", "YES", "-99", "", "251.2", "1.00", "8.0", ""

"WGNA-010818-RW-4024", "537", "RES", "320-34917-10", "TALSAC", "355-46-4", "Perfluorohexanesulfonic acid (PFHxS)", "12", "ng/L", "U", "5.5", "DL", "", "TRG", "", "", "30", "LOQ", "YES", "-99", "", "251.2", "1.00", "12", ""

"WGNA-010818-RW-4024", "537", "RES", "320-34917-10", "TALSAC", "375-73-5", "Perfluorobutanesulfonic acid (PFBS)", "36", "ng/L", "U", "16", "DL", "", "TRG", "", "", "90", "LOQ", "YES", "-99", "", "251.2", "1.00", "36", ""

"WGNA-010818-RW-4024", "537", "RES", "320-34917-10", "TALSAC", "375-85-9", "Perfluoroheptanoic acid (PFHpA)", "3.6", "ng/L", "J", "1.9", "DL", "", "TRG", "", "", "10", "LOQ", "YES", "-99", "", "251.2", "1.00", "4.0", ""

"WGNA-010818-RW-4024", "537", "RES", "320-34917-10", "TALSAC", "375-95-1", "Perfluorononanoic acid (PFNA)", "20", "ng/L", "U", "8.0", "DL", "", "TRG", "", "", "24", "LOQ", "YES", "-99", "", "251.2", "1.00", "20", ""

"WGNA-010818-RW-4024", "537", "RES", "320-34917-10", "TALSAC", "STL00993", "13C2 PFHxA", "28", "ng/L", "", "-99", "DL", "", "SURR", "71", "", "-99", "LOQ", "YES", "39.8", "", "251.2", "1.00", "0", ""

"WGNA-010818-RW-4024", "537", "RES", "320-34917-10", "TALSAC", "STL00996", "13C2 PFDA", "37", "ng/L", "", "-99", "DL", "", "SURR", "93", "", "-99", "LOQ", "YES", "39.8", "", "251.2", "1.00", "0", ""

"WGNA-010818-RW-4024MS", "537", "RES", "320-34917-10MS", "TALSAC", "1763-23-1", "Perfluorooctanesulfonic acid (PFOS)", "58.5", "ng/L", "M", "6.8", "DL", "", "SPK", "102", "", "40", "LOQ", "YES", "40.2", "WGNA-010818-RW-4024", "249.1", "1.00", "16", ""

"WGNA-010818-RW-4024MS", "537", "RES", "320-34917-10MS", "TALSAC", "335-67-1", "Perfluorooctanoic acid (PFOA)", "31.9", "ng/L", "", "2.8", "DL", "", "SPK", "99", "", "20", "LOQ", "YES", "20.1", "WGNA-010818-RW-4024", "249.1", "1.00", "8.0", ""

"WGNA-010818-RW-4024MS", "537", "RES", "320-34917-10MS", "TALSAC", "355-46-4", "Perfluorohexanesulfonic acid (PFHxS)", "36.4", "ng/L", "", "5.5", "DL", "", "SPK", "121", "", "30", "LOQ", "YES", "30.1", "WGNA-010818-RW-4024", "249.1", "1.00", "12", ""

"WGNA-010818-RW-4024MS", "537", "RES", "320-34917-10MS", "TALSAC", "375-73-5", "Perfluorobutanesulfonic acid (PFBS)", "95.9", "ng/L", "", "16", "DL", "", "SPK", "106", "", "90", "LOQ", "YES", "90.3", "WGNA-010818-RW-4024", "249.1", "1.00", "36", ""

"WGNA-010818-RW-4024MS", "537", "RES", "320-34917-10MS", "TALSAC", "375-85-9", "Perfluoroheptanoic acid (PFHpA)", "14.4", "ng/L", "", "1.9", "DL", "", "SPK", "108", "", "10", "LOQ", "YES", "10.0", "WGNA-010818-RW-4024", "249.1", "1.00", "4.0", ""

"WGNA-010818-RW-4024MS", "537", "RES", "320-34917-10MS", "TALSAC", "375-95-1", "Perfluorononanoic acid (PFNA)", "22.9", "ng/L", "J", "8.0", "DL", "", "SPK", "114", "", "24", "LOQ", "YES", "20.1", "WGNA-010818-RW-4024", "249.1", "1.00", "20", ""

"WGNA-010818-RW-4024MS", "537", "RES", "320-34917-10MS", "TALSAC", "STL00993", "13C2 PFHxA", "35.2", "ng/L", "", "-99", "DL", "", "SURR", "88", "", "-99", "LOQ", "YES", "40.1", "WGNA-010818-RW-4024", "249.1", "1.00", "0", ""

"WGNA-010818-RW-4024MS", "537", "RES", "320-34917-10MS", "TALSAC", "STL00996", "13C2
PFDA", "38.3", "ng/L", "", "-99", "DL", "", "SURR", "95", "", "-99", "LOQ", "YES", "40.1", "WGNA-010818-RW-
4024", "249.1", "1.00", "0", ""
"WGNA-010818-RW-4024MSD", "537", "RES", "320-34917-10MSD", "TALSAC", "1763-23-
1", "Perfluorooctanesulfonic acid
(PFOS)", "56.7", "ng/L", "M", "6.6", "DL", "", "SPK", "101", "3", "39", "LOQ", "YES", "38.8", "WGNA-010818-RW-
4024", "257.7", "1.00", "16", ""
"WGNA-010818-RW-4024MSD", "537", "RES", "320-34917-10MSD", "TALSAC", "335-67-1", "Perfluorooctanoic acid
(PFOA)", "32.3", "ng/L", "", "2.7", "DL", "", "SPK", "105", "1", "19", "LOQ", "YES", "19.4", "WGNA-010818-RW-
4024", "257.7", "1.00", "7.8", ""
"WGNA-010818-RW-4024MSD", "537", "RES", "320-34917-10MSD", "TALSAC", "355-46-4", "Perfluorohexanesulfonic
acid (PFHxS)", "33.8", "ng/L", "", "5.3", "DL", "", "SPK", "116", "7", "29", "LOQ", "YES", "29.1", "WGNA-010818-RW-
4024", "257.7", "1.00", "12", ""
"WGNA-010818-RW-4024MSD", "537", "RES", "320-34917-10MSD", "TALSAC", "375-73-5", "Perfluorobutanesulfonic
acid (PFBS)", "98.5", "ng/L", "", "16", "DL", "", "SPK", "113", "3", "87", "LOQ", "YES", "87.3", "WGNA-010818-RW-
4024", "257.7", "1.00", "35", ""
"WGNA-010818-RW-4024MSD", "537", "RES", "320-34917-10MSD", "TALSAC", "375-85-9", "Perfluoroheptanoic acid
(PFHpA)", "13.8", "ng/L", "", "1.8", "DL", "", "SPK", "106", "4", "9.7", "LOQ", "YES", "9.70", "WGNA-010818-RW-
4024", "257.7", "1.00", "3.9", ""
"WGNA-010818-RW-4024MSD", "537", "RES", "320-34917-10MSD", "TALSAC", "375-95-1", "Perfluorononanoic acid
(PFNA)", "21.5", "ng/L", "J", "7.8", "DL", "", "SPK", "111", "6", "23", "LOQ", "YES", "19.4", "WGNA-010818-RW-
4024", "257.7", "1.00", "19", ""
"WGNA-010818-RW-4024MSD", "537", "RES", "320-34917-10MSD", "TALSAC", "STL00993", "13C2
PFHxA", "34.8", "ng/L", "", "-99", "DL", "", "SURR", "90", "", "-99", "LOQ", "YES", "38.8", "WGNA-010818-RW-
4024", "257.7", "1.00", "0", ""
"WGNA-010818-RW-4024MSD", "537", "RES", "320-34917-10MSD", "TALSAC", "STL00996", "13C2
PFDA", "37.8", "ng/L", "", "-99", "DL", "", "SURR", "97", "", "-99", "LOQ", "YES", "38.8", "WGNA-010818-RW-
4024", "257.7", "1.00", "0", ""
"WGNA-010818-FRB-4024", "537", "RES", "320-34917-11", "TALSAC", "1763-23-1", "Perfluorooctanesulfonic acid
(PFOS)", "16", "ng/L", "U", "6.6", "DL", "", "TRG", "", "", "39", "LOQ", "YES", "-99", "", "257.4", "1.00", "16", ""
"WGNA-010818-FRB-4024", "537", "RES", "320-34917-11", "TALSAC", "335-67-1", "Perfluorooctanoic acid
(PFOA)", "7.8", "ng/L", "U", "2.7", "DL", "", "TRG", "", "", "19", "LOQ", "YES", "-99", "", "257.4", "1.00", "7.8", ""
"WGNA-010818-FRB-4024", "537", "RES", "320-34917-11", "TALSAC", "355-46-4", "Perfluorohexanesulfonic acid
(PFHxS)", "12", "ng/L", "U", "5.3", "DL", "", "TRG", "", "", "29", "LOQ", "YES", "-99", "", "257.4", "1.00", "12", ""
"WGNA-010818-FRB-4024", "537", "RES", "320-34917-11", "TALSAC", "375-73-5", "Perfluorobutanesulfonic acid
(PFBS)", "35", "ng/L", "U", "16", "DL", "", "TRG", "", "", "87", "LOQ", "YES", "-99", "", "257.4", "1.00", "35", ""
"WGNA-010818-FRB-4024", "537", "RES", "320-34917-11", "TALSAC", "375-85-9", "Perfluoroheptanoic acid
(PFHpA)", "3.9", "ng/L", "U", "1.8", "DL", "", "TRG", "", "", "9.7", "LOQ", "YES", "-99", "", "257.4", "1.00", "3.9", ""
"WGNA-010818-FRB-4024", "537", "RES", "320-34917-11", "TALSAC", "375-95-1", "Perfluorononanoic acid
(PFNA)", "19", "ng/L", "U", "7.8", "DL", "", "TRG", "", "", "23", "LOQ", "YES", "-99", "", "257.4", "1.00", "19", ""
"WGNA-010818-FRB-4024", "537", "RES", "320-34917-11", "TALSAC", "STL00993", "13C2
PFHxA", "38", "ng/L", "", "-99", "DL", "", "SURR", "98", "", "-99", "LOQ", "YES", "38.9", "", "257.4", "1.00", "0", ""
"WGNA-010818-FRB-4024", "537", "RES", "320-34917-11", "TALSAC", "STL00996", "13C2
PFDA", "39", "ng/L", "", "-99", "DL", "", "SURR", "100", "", "-99", "LOQ", "YES", "38.9", "", "257.4", "1.00", "0", ""
"WGNA-010818-RW-4844", "537", "RES", "320-34917-12", "TALSAC", "1763-23-1", "Perfluorooctanesulfonic acid
(PFOS)", "7.9", "ng/L", "J M", "6.7", "DL", "", "TRG", "", "", "39", "LOQ", "YES", "-99", "", "253.5", "1.00", "16", ""
"WGNA-010818-RW-4844", "537", "RES", "320-34917-12", "TALSAC", "335-67-1", "Perfluorooctanoic acid
(PFOA)", "14", "ng/L", "J", "2.8", "DL", "", "TRG", "", "", "20", "LOQ", "YES", "-99", "", "253.5", "1.00", "7.9", ""
"WGNA-010818-RW-4844", "537", "RES", "320-34917-12", "TALSAC", "355-46-4", "Perfluorohexanesulfonic acid
(PFHxS)", "12", "ng/L", "U", "5.4", "DL", "", "TRG", "", "", "30", "LOQ", "YES", "-99", "", "253.5", "1.00", "12", ""
"WGNA-010818-RW-4844", "537", "RES", "320-34917-12", "TALSAC", "375-73-5", "Perfluorobutanesulfonic acid
(PFBS)", "36", "ng/L", "U", "16", "DL", "", "TRG", "", "", "89", "LOQ", "YES", "-99", "", "253.5", "1.00", "36", ""
"WGNA-010818-RW-4844", "537", "RES", "320-34917-12", "TALSAC", "375-85-9", "Perfluoroheptanoic acid
(PFHpA)", "7.1", "ng/L", "J", "1.9", "DL", "", "TRG", "", "", "9.9", "LOQ", "YES", "-99", "", "253.5", "1.00", "3.9", ""

"WGNA-010818-RW-4844", "537", "RES", "320-34917-12", "TALSAC", "375-95-1", "Perfluorononanoic acid (PFNA)", "20", "ng/L", "U", "7.9", "DL", "", "TRG", "", "", "24", "LOQ", "YES", "-99", "", "253.5", "1.00", "20", ""

"WGNA-010818-RW-4844", "537", "RES", "320-34917-12", "TALSAC", "STL00993", "13C2 PFHxA", "38", "ng/L", "", "-99", "DL", "", "SURR", "97", "", "-99", "LOQ", "YES", "39.4", "", "253.5", "1.00", "0", ""

"WGNA-010818-RW-4844", "537", "RES", "320-34917-12", "TALSAC", "STL00996", "13C2 PFDA", "39", "ng/L", "", "-99", "DL", "", "SURR", "98", "", "-99", "LOQ", "YES", "39.4", "", "253.5", "1.00", "0", ""

"WGNA-010818-FRB-4844", "537", "RES", "320-34917-13", "TALSAC", "1763-23-1", "Perfluorooctanesulfonic acid (PFOS)", "16", "ng/L", "U", "6.8", "DL", "", "TRG", "", "", "40", "LOQ", "YES", "-99", "", "249.5", "1.00", "16", ""

"WGNA-010818-FRB-4844", "537", "RES", "320-34917-13", "TALSAC", "335-67-1", "Perfluorooctanoic acid (PFOA)", "8.0", "ng/L", "U", "2.8", "DL", "", "TRG", "", "", "20", "LOQ", "YES", "-99", "", "249.5", "1.00", "8.0", ""

"WGNA-010818-FRB-4844", "537", "RES", "320-34917-13", "TALSAC", "355-46-4", "Perfluorohexanesulfonic acid (PFHxS)", "12", "ng/L", "U", "5.5", "DL", "", "TRG", "", "", "30", "LOQ", "YES", "-99", "", "249.5", "1.00", "12", ""

"WGNA-010818-FRB-4844", "537", "RES", "320-34917-13", "TALSAC", "375-73-5", "Perfluorobutanesulfonic acid (PFBS)", "36", "ng/L", "U", "16", "DL", "", "TRG", "", "", "90", "LOQ", "YES", "-99", "", "249.5", "1.00", "36", ""

"WGNA-010818-FRB-4844", "537", "RES", "320-34917-13", "TALSAC", "375-85-9", "Perfluoroheptanoic acid (PFHpA)", "4.0", "ng/L", "U", "1.9", "DL", "", "TRG", "", "", "10", "LOQ", "YES", "-99", "", "249.5", "1.00", "4.0", ""

"WGNA-010818-FRB-4844", "537", "RES", "320-34917-13", "TALSAC", "375-95-1", "Perfluorononanoic acid (PFNA)", "20", "ng/L", "U", "8.0", "DL", "", "TRG", "", "", "24", "LOQ", "YES", "-99", "", "249.5", "1.00", "20", ""

"WGNA-010818-FRB-4844", "537", "RES", "320-34917-13", "TALSAC", "STL00993", "13C2 PFHxA", "39", "ng/L", "", "-99", "DL", "", "SURR", "97", "", "-99", "LOQ", "YES", "40.1", "", "249.5", "1.00", "0", ""

"WGNA-010818-FRB-4844", "537", "RES", "320-34917-13", "TALSAC", "STL00996", "13C2 PFDA", "39", "ng/L", "", "-99", "DL", "", "SURR", "97", "", "-99", "LOQ", "YES", "40.1", "", "249.5", "1.00", "0", ""

"WGNA-010818-RW-0404", "537", "RES", "320-34917-14", "TALSAC", "1763-23-1", "Perfluorooctanesulfonic acid (PFOS)", "26", "ng/L", "J M", "6.8", "DL", "", "TRG", "", "", "40", "LOQ", "YES", "-99", "", "249.4", "1.00", "16", ""

"WGNA-010818-RW-0404", "537", "RES", "320-34917-14", "TALSAC", "335-67-1", "Perfluorooctanoic acid (PFOA)", "21", "ng/L", "", "2.8", "DL", "", "TRG", "", "", "20", "LOQ", "YES", "-99", "", "249.4", "1.00", "8.0", ""

"WGNA-010818-RW-0404", "537", "RES", "320-34917-14", "TALSAC", "355-46-4", "Perfluorohexanesulfonic acid (PFHxS)", "8.3", "ng/L", "J", "5.5", "DL", "", "TRG", "", "", "30", "LOQ", "YES", "-99", "", "249.4", "1.00", "12", ""

"WGNA-010818-RW-0404", "537", "RES", "320-34917-14", "TALSAC", "375-73-5", "Perfluorobutanesulfonic acid (PFBS)", "36", "ng/L", "U", "16", "DL", "", "TRG", "", "", "90", "LOQ", "YES", "-99", "", "249.4", "1.00", "36", ""

"WGNA-010818-RW-0404", "537", "RES", "320-34917-14", "TALSAC", "375-85-9", "Perfluoroheptanoic acid (PFHpA)", "6.3", "ng/L", "J", "1.9", "DL", "", "TRG", "", "", "10", "LOQ", "YES", "-99", "", "249.4", "1.00", "4.0", ""

"WGNA-010818-RW-0404", "537", "RES", "320-34917-14", "TALSAC", "375-95-1", "Perfluorononanoic acid (PFNA)", "20", "ng/L", "U", "8.0", "DL", "", "TRG", "", "", "24", "LOQ", "YES", "-99", "", "249.4", "1.00", "20", ""

"WGNA-010818-RW-0404", "537", "RES", "320-34917-14", "TALSAC", "STL00993", "13C2 PFHxA", "39", "ng/L", "", "-99", "DL", "", "SURR", "96", "", "-99", "LOQ", "YES", "40.1", "", "249.4", "1.00", "0", ""

"WGNA-010818-RW-0404", "537", "RES", "320-34917-14", "TALSAC", "STL00996", "13C2 PFDA", "40", "ng/L", "", "-99", "DL", "", "SURR", "100", "", "-99", "LOQ", "YES", "40.1", "", "249.4", "1.00", "0", ""

"WGNA-010818-FRB-0404", "537", "RES", "320-34917-15", "TALSAC", "1763-23-1", "Perfluorooctanesulfonic acid (PFOS)", "16", "ng/L", "U", "6.7", "DL", "", "TRG", "", "", "40", "LOQ", "YES", "-99", "", "252.5", "1.00", "16", ""

"WGNA-010818-FRB-0404", "537", "RES", "320-34917-15", "TALSAC", "335-67-1", "Perfluorooctanoic acid (PFOA)", "7.9", "ng/L", "U", "2.8", "DL", "", "TRG", "", "", "20", "LOQ", "YES", "-99", "", "252.5", "1.00", "7.9", ""

"WGNA-010818-FRB-0404", "537", "RES", "320-34917-15", "TALSAC", "355-46-4", "Perfluorohexanesulfonic acid (PFHxS)", "12", "ng/L", "U", "5.4", "DL", "", "TRG", "", "", "30", "LOQ", "YES", "-99", "", "252.5", "1.00", "12", ""

"WGNA-010818-FRB-0404", "537", "RES", "320-34917-15", "TALSAC", "375-73-5", "Perfluorobutanesulfonic acid (PFBS)", "36", "ng/L", "U", "16", "DL", "", "TRG", "", "", "89", "LOQ", "YES", "-99", "", "252.5", "1.00", "36", ""

"WGNA-010818-FRB-0404", "537", "RES", "320-34917-15", "TALSAC", "375-85-9", "Perfluoroheptanoic acid (PFHpA)", "4.0", "ng/L", "U", "1.9", "DL", "", "TRG", "", "", "9.9", "LOQ", "YES", "-99", "", "252.5", "1.00", "4.0", ""

"WGNA-010818-FRB-0404", "537", "RES", "320-34917-15", "TALSAC", "375-95-1", "Perfluorononanoic acid (PFNA)", "20", "ng/L", "U", "7.9", "DL", "", "TRG", "", "", "24", "LOQ", "YES", "-99", "", "252.5", "1.00", "20", ""

"WGNA-010818-FRB-0404", "537", "RES", "320-34917-15", "TALSAC", "STL00993", "13C2 PFHxA", "41", "ng/L", "", "-99", "DL", "", "SURR", "103", "", "-99", "LOQ", "YES", "39.6", "", "252.5", "1.00", "0", ""

"WGNA-010818-FRB-0404", "537", "RES", "320-34917-15", "TALSAC", "STL00996", "13C2 PFDA", "41", "ng/L", "", "-99", "DL", "", "SURR", "103", "", "-99", "LOQ", "YES", "39.6", "", "252.5", "1.00", "0", ""

"WGNA-010818-FRB-0344","537","RES","320-34917-2","TALSAC","1763-23-1","Perfluorooctanesulfonic acid (PFOS)","16","ng/L","U","6.7","DL","","TRG","","","39","LOQ","YES","-99","","253.2","1.00","16",""
"WGNA-010818-FRB-0344","537","RES","320-34917-2","TALSAC","335-67-1","Perfluorooctanoic acid (PFOA)","7.9","ng/L","U","2.8","DL","","TRG","","","20","LOQ","YES","-99","","253.2","1.00","7.9",""
"WGNA-010818-FRB-0344","537","RES","320-34917-2","TALSAC","355-46-4","Perfluorohexanesulfonic acid (PFHxS)","12","ng/L","U","5.4","DL","","TRG","","","30","LOQ","YES","-99","","253.2","1.00","12",""
"WGNA-010818-FRB-0344","537","RES","320-34917-2","TALSAC","375-73-5","Perfluorobutanesulfonic acid (PFBS)","36","ng/L","U","16","DL","","TRG","","","89","LOQ","YES","-99","","253.2","1.00","36",""
"WGNA-010818-FRB-0344","537","RES","320-34917-2","TALSAC","375-85-9","Perfluoroheptanoic acid (PFHpA)","3.9","ng/L","U","1.9","DL","","TRG","","","9.9","LOQ","YES","-99","","253.2","1.00","3.9",""
"WGNA-010818-FRB-0344","537","RES","320-34917-2","TALSAC","375-95-1","Perfluorononanoic acid (PFNA)","20","ng/L","U","7.9","DL","","TRG","","","24","LOQ","YES","-99","","253.2","1.00","20",""
"WGNA-010818-FRB-0344","537","RES","320-34917-2","TALSAC","STL00993","13C2 PFHxA","38","ng/L","","-99","DL","","SURR","97","","-99","LOQ","YES","39.5","","253.2","1.00","0",""
"WGNA-010818-FRB-0344","537","RES","320-34917-2","TALSAC","STL00996","13C2 PFDA","39","ng/L","","-99","DL","","SURR","98","","-99","LOQ","YES","39.5","","253.2","1.00","0",""
"WGNA-010818-RW-3957","537","RES","320-34917-3","TALSAC","1763-23-1","Perfluorooctanesulfonic acid (PFOS)","18","ng/L","J","6.6","DL","","TRG","","","39","LOQ","YES","-99","","257.4","1.00","16",""
"WGNA-010818-RW-3957","537","RES","320-34917-3","TALSAC","335-67-1","Perfluorooctanoic acid (PFOA)","15","ng/L","J","2.7","DL","","TRG","","","19","LOQ","YES","-99","","257.4","1.00","7.8",""
"WGNA-010818-RW-3957","537","RES","320-34917-3","TALSAC","355-46-4","Perfluorohexanesulfonic acid (PFHxS)","6.5","ng/L","J","5.3","DL","","TRG","","","29","LOQ","YES","-99","","257.4","1.00","12",""
"WGNA-010818-RW-3957","537","RES","320-34917-3","TALSAC","375-73-5","Perfluorobutanesulfonic acid (PFBS)","35","ng/L","U","16","DL","","TRG","","","87","LOQ","YES","-99","","257.4","1.00","35",""
"WGNA-010818-RW-3957","537","RES","320-34917-3","TALSAC","375-85-9","Perfluoroheptanoic acid (PFHpA)","3.8","ng/L","J","1.8","DL","","TRG","","","9.7","LOQ","YES","-99","","257.4","1.00","3.9",""
"WGNA-010818-RW-3957","537","RES","320-34917-3","TALSAC","375-95-1","Perfluorononanoic acid (PFNA)","19","ng/L","U M","7.8","DL","","TRG","","","23","LOQ","YES","-99","","257.4","1.00","19",""
"WGNA-010818-RW-3957","537","RES","320-34917-3","TALSAC","STL00993","13C2 PFHxA","36","ng/L","","-99","DL","","SURR","91","","-99","LOQ","YES","38.9","","257.4","1.00","0",""
"WGNA-010818-RW-3957","537","RES","320-34917-3","TALSAC","STL00996","13C2 PFDA","40","ng/L","","-99","DL","","SURR","104","","-99","LOQ","YES","38.9","","257.4","1.00","0",""
"WGNA-010818-FRB-3957","537","RES","320-34917-4","TALSAC","1763-23-1","Perfluorooctanesulfonic acid (PFOS)","16","ng/L","U","6.6","DL","","TRG","","","39","LOQ","YES","-99","","256.1","1.00","16",""
"WGNA-010818-FRB-3957","537","RES","320-34917-4","TALSAC","335-67-1","Perfluorooctanoic acid (PFOA)","7.8","ng/L","U","2.7","DL","","TRG","","","20","LOQ","YES","-99","","256.1","1.00","7.8",""
"WGNA-010818-FRB-3957","537","RES","320-34917-4","TALSAC","355-46-4","Perfluorohexanesulfonic acid (PFHxS)","12","ng/L","U","5.4","DL","","TRG","","","29","LOQ","YES","-99","","256.1","1.00","12",""
"WGNA-010818-FRB-3957","537","RES","320-34917-4","TALSAC","375-73-5","Perfluorobutanesulfonic acid (PFBS)","35","ng/L","U","16","DL","","TRG","","","88","LOQ","YES","-99","","256.1","1.00","35",""
"WGNA-010818-FRB-3957","537","RES","320-34917-4","TALSAC","375-85-9","Perfluoroheptanoic acid (PFHpA)","3.9","ng/L","U","1.9","DL","","TRG","","","9.8","LOQ","YES","-99","","256.1","1.00","3.9",""
"WGNA-010818-FRB-3957","537","RES","320-34917-4","TALSAC","375-95-1","Perfluorononanoic acid (PFNA)","20","ng/L","U","7.8","DL","","TRG","","","23","LOQ","YES","-99","","256.1","1.00","20",""
"WGNA-010818-FRB-3957","537","RES","320-34917-4","TALSAC","STL00993","13C2 PFHxA","38","ng/L","","-99","DL","","SURR","96","","-99","LOQ","YES","39.0","","256.1","1.00","0",""
"WGNA-010818-FRB-3957","537","RES","320-34917-4","TALSAC","STL00996","13C2 PFDA","38","ng/L","","-99","DL","","SURR","98","","-99","LOQ","YES","39.0","","256.1","1.00","0",""
"WGNA-010818-DUP-16","537","RES","320-34917-5","TALSAC","1763-23-1","Perfluorooctanesulfonic acid (PFOS)","25","ng/L","J","6.5","DL","","TRG","","","38","LOQ","YES","-99","","262.5","1.00","15",""
"WGNA-010818-DUP-16","537","RES","320-34917-5","TALSAC","335-67-1","Perfluorooctanoic acid (PFOA)","21","ng/L","","2.7","DL","","TRG","","","19","LOQ","YES","-99","","262.5","1.00","7.6",""
"WGNA-010818-DUP-16","537","RES","320-34917-5","TALSAC","355-46-4","Perfluorohexanesulfonic acid (PFHxS)","8.0","ng/L","J","5.2","DL","","TRG","","","29","LOQ","YES","-99","","262.5","1.00","11",""

"WGNA-010818-DUP-16","537","RES","320-34917-5","TALSAC","375-73-5","Perfluorobutanesulfonic acid (PFBS)","34","ng/L","U","15","DL","","TRG","","","86","LOQ","YES","-99","","262.5","1.00","34",""
"WGNA-010818-DUP-16","537","RES","320-34917-5","TALSAC","375-85-9","Perfluoroheptanoic acid (PFHpA)","6.2","ng/L","J","1.8","DL","","TRG","","","9.5","LOQ","YES","-99","","262.5","1.00","3.8",""
"WGNA-010818-DUP-16","537","RES","320-34917-5","TALSAC","375-95-1","Perfluorononanoic acid (PFNA)","19","ng/L","U","7.6","DL","","TRG","","","23","LOQ","YES","-99","","262.5","1.00","19",""
"WGNA-010818-DUP-16","537","RES","320-34917-5","TALSAC","STL00993","13C2 PFHxA","37","ng/L","","-99","DL","","SURR","96","","-99","LOQ","YES","38.1","","262.5","1.00","0",""
"WGNA-010818-DUP-16","537","RES","320-34917-5","TALSAC","STL00996","13C2 PFDA","41","ng/L","","-99","DL","","SURR","109","","-99","LOQ","YES","38.1","","262.5","1.00","0",""
"WGNA-010818-RW-3178","537","RES","320-34917-6","TALSAC","1763-23-1","Perfluorooctanesulfonic acid (PFOS)","16","ng/L","J","7.1","DL","","TRG","","","42","LOQ","YES","-99","","239.2","1.00","17",""
"WGNA-010818-RW-3178","537","RES","320-34917-6","TALSAC","335-67-1","Perfluorooctanoic acid (PFOA)","9.8","ng/L","J","2.9","DL","","TRG","","","21","LOQ","YES","-99","","239.2","1.00","8.4",""
"WGNA-010818-RW-3178","537","RES","320-34917-6","TALSAC","355-46-4","Perfluorohexanesulfonic acid (PFHxS)","7.0","ng/L","J","5.7","DL","","TRG","","","31","LOQ","YES","-99","","239.2","1.00","13",""
"WGNA-010818-RW-3178","537","RES","320-34917-6","TALSAC","375-73-5","Perfluorobutanesulfonic acid (PFBS)","38","ng/L","U","17","DL","","TRG","","","94","LOQ","YES","-99","","239.2","1.00","38",""
"WGNA-010818-RW-3178","537","RES","320-34917-6","TALSAC","375-85-9","Perfluoroheptanoic acid (PFHpA)","2.8","ng/L","J","2.0","DL","","TRG","","","10","LOQ","YES","-99","","239.2","1.00","4.2",""
"WGNA-010818-RW-3178","537","RES","320-34917-6","TALSAC","375-95-1","Perfluorononanoic acid (PFNA)","21","ng/L","U","8.4","DL","","TRG","","","25","LOQ","YES","-99","","239.2","1.00","21",""
"WGNA-010818-RW-3178","537","RES","320-34917-6","TALSAC","STL00993","13C2 PFHxA","38","ng/L","","-99","DL","","SURR","90","","-99","LOQ","YES","41.8","","239.2","1.00","0",""
"WGNA-010818-RW-3178","537","RES","320-34917-6","TALSAC","STL00996","13C2 PFDA","43","ng/L","","-99","DL","","SURR","102","","-99","LOQ","YES","41.8","","239.2","1.00","0",""
"WGNA-010818-FRB-3178","537","RES","320-34917-7","TALSAC","1763-23-1","Perfluorooctanesulfonic acid (PFOS)","16","ng/L","U","6.6","DL","","TRG","","","39","LOQ","YES","-99","","256.7","1.00","16",""
"WGNA-010818-FRB-3178","537","RES","320-34917-7","TALSAC","335-67-1","Perfluorooctanoic acid (PFOA)","7.8","ng/L","U","2.7","DL","","TRG","","","19","LOQ","YES","-99","","256.7","1.00","7.8",""
"WGNA-010818-FRB-3178","537","RES","320-34917-7","TALSAC","355-46-4","Perfluorohexanesulfonic acid (PFHxS)","12","ng/L","U","5.4","DL","","TRG","","","29","LOQ","YES","-99","","256.7","1.00","12",""
"WGNA-010818-FRB-3178","537","RES","320-34917-7","TALSAC","375-73-5","Perfluorobutanesulfonic acid (PFBS)","35","ng/L","U","16","DL","","TRG","","","88","LOQ","YES","-99","","256.7","1.00","35",""
"WGNA-010818-FRB-3178","537","RES","320-34917-7","TALSAC","375-85-9","Perfluoroheptanoic acid (PFHpA)","3.9","ng/L","U","1.9","DL","","TRG","","","9.7","LOQ","YES","-99","","256.7","1.00","3.9",""
"WGNA-010818-FRB-3178","537","RES","320-34917-7","TALSAC","375-95-1","Perfluorononanoic acid (PFNA)","19","ng/L","U","7.8","DL","","TRG","","","23","LOQ","YES","-99","","256.7","1.00","19",""
"WGNA-010818-FRB-3178","537","RES","320-34917-7","TALSAC","STL00993","13C2 PFHxA","38","ng/L","","-99","DL","","SURR","98","","-99","LOQ","YES","39.0","","256.7","1.00","0",""
"WGNA-010818-FRB-3178","537","RES","320-34917-7","TALSAC","STL00996","13C2 PFDA","40","ng/L","","-99","DL","","SURR","103","","-99","LOQ","YES","39.0","","256.7","1.00","0",""
"NAWC-010818-RW-141","537","RES","320-34917-8","TALSAC","1763-23-1","Perfluorooctanesulfonic acid (PFOS)","24","ng/L","J","6.6","DL","","TRG","","","39","LOQ","YES","-99","","257.5","1.00","16",""
"NAWC-010818-RW-141","537","RES","320-34917-8","TALSAC","335-67-1","Perfluorooctanoic acid (PFOA)","15","ng/L","J","2.7","DL","","TRG","","","19","LOQ","YES","-99","","257.5","1.00","7.8",""
"NAWC-010818-RW-141","537","RES","320-34917-8","TALSAC","355-46-4","Perfluorohexanesulfonic acid (PFHxS)","16","ng/L","J","5.3","DL","","TRG","","","29","LOQ","YES","-99","","257.5","1.00","12",""
"NAWC-010818-RW-141","537","RES","320-34917-8","TALSAC","375-73-5","Perfluorobutanesulfonic acid (PFBS)","35","ng/L","U","16","DL","","TRG","","","87","LOQ","YES","-99","","257.5","1.00","35",""
"NAWC-010818-RW-141","537","RES","320-34917-8","TALSAC","375-85-9","Perfluoroheptanoic acid (PFHpA)","7.6","ng/L","J","1.8","DL","","TRG","","","9.7","LOQ","YES","-99","","257.5","1.00","3.9",""
"NAWC-010818-RW-141","537","RES","320-34917-8","TALSAC","375-95-1","Perfluorononanoic acid (PFNA)","19","ng/L","U","7.8","DL","","TRG","","","23","LOQ","YES","-99","","257.5","1.00","19",""

"NAWC-010818-RW-141","537","RES","320-34917-8","TALSAC","STL00993","13C2
PFHxA","34","ng/L","",-99,"DL","",,"SURR","88","",-99,"LOQ","YES","38.8","",,"257.5","1.00","0",""
"NAWC-010818-RW-141","537","RES","320-34917-8","TALSAC","STL00996","13C2
PFDA","37","ng/L","",-99,"DL","",,"SURR","96","",-99,"LOQ","YES","38.8","",,"257.5","1.00","0",""
"NAWC-010818-FRB-141","537","RES","320-34917-9","TALSAC","1763-23-1","Perfluorooctanesulfonic acid
(PFOS)","15","ng/L","U","6.4","DL","",,"TRG","",,"",,"38","LOQ","YES","-99","",,"266.1","1.00","15",""
"NAWC-010818-FRB-141","537","RES","320-34917-9","TALSAC","335-67-1","Perfluorooctanoic acid
(PFOA)","7.5","ng/L","U","2.6","DL","",,"TRG","",,"",,"19","LOQ","YES","-99","",,"266.1","1.00","7.5",""
"NAWC-010818-FRB-141","537","RES","320-34917-9","TALSAC","355-46-4","Perfluorohexanesulfonic acid
(PFHxS)","11","ng/L","U","5.2","DL","",,"TRG","",,"",,"28","LOQ","YES","-99","",,"266.1","1.00","11",""
"NAWC-010818-FRB-141","537","RES","320-34917-9","TALSAC","375-73-5","Perfluorobutanesulfonic acid
(PFBS)","34","ng/L","U","15","DL","",,"TRG","",,"",,"85","LOQ","YES","-99","",,"266.1","1.00","34",""
"NAWC-010818-FRB-141","537","RES","320-34917-9","TALSAC","375-85-9","Perfluoroheptanoic acid
(PFHpA)","3.8","ng/L","U","1.8","DL","",,"TRG","",,"",,"9.4","LOQ","YES","-99","",,"266.1","1.00","3.8",""
"NAWC-010818-FRB-141","537","RES","320-34917-9","TALSAC","375-95-1","Perfluorononanoic acid
(PFNA)","19","ng/L","U","7.5","DL","",,"TRG","",,"",,"23","LOQ","YES","-99","",,"266.1","1.00","19",""
"NAWC-010818-FRB-141","537","RES","320-34917-9","TALSAC","STL00993","13C2
PFHxA","36","ng/L","",-99,"DL","",,"SURR","95","",-99,"LOQ","YES","37.6","",,"266.1","1.00","0",""
"NAWC-010818-FRB-141","537","RES","320-34917-9","TALSAC","STL00996","13C2
PFDA","37","ng/L","",-99,"DL","",,"SURR","99","",-99,"LOQ","YES","37.6","",,"266.1","1.00","0",""
"LLCS 320-204304/2-A","537","RES","LLCS 320-204304/2-A","TALSAC","1763-23-1","Perfluorooctanesulfonic
acid (PFOS)","39.2","ng/L","J","6.8","DL","",,"SPK","98","",,"40","LOQ","YES","40.0","",,"250","1.00","16",""
"LLCS 320-204304/2-A","537","RES","LLCS 320-204304/2-A","TALSAC","335-67-1","Perfluorooctanoic acid
(PFOA)","20.1","ng/L","",,"2.8","DL","",,"SPK","100","",,"20","LOQ","YES","20.0","",,"250","1.00","8.0",""
"LLCS 320-204304/2-A","537","RES","LLCS 320-204304/2-A","TALSAC","355-46-4","Perfluorohexanesulfonic acid
(PFHxS)","30.9","ng/L","",,"5.5","DL","",,"SPK","103","",,"30","LOQ","YES","30.0","",,"250","1.00","12",""
"LLCS 320-204304/2-A","537","RES","LLCS 320-204304/2-A","TALSAC","375-73-5","Perfluorobutanesulfonic acid
(PFBS)","85.8","ng/L","J","16","DL","",,"SPK","95","",,"90","LOQ","YES","90.0","",,"250","1.00","36",""
"LLCS 320-204304/2-A","537","RES","LLCS 320-204304/2-A","TALSAC","375-85-9","Perfluoroheptanoic acid
(PFHpA)","10.4","ng/L","",,"1.9","DL","",,"SPK","104","",,"10","LOQ","YES","10.0","",,"250","1.00","4.0",""
"LLCS 320-204304/2-A","537","RES","LLCS 320-204304/2-A","TALSAC","375-95-1","Perfluorononanoic acid
(PFNA)","19.7","ng/L","J","8.0","DL","",,"SPK","98","",,"24","LOQ","YES","20.0","",,"250","1.00","20",""
"LLCS 320-204304/2-A","537","RES","LLCS 320-204304/2-A","TALSAC","STL00993","13C2
PFHxA","38.6","ng/L","",-99,"DL","",,"SURR","97","",-99,"LOQ","YES","40.0","",,"250","1.00","0",""
"LLCS 320-204304/2-A","537","RES","LLCS 320-204304/2-A","TALSAC","STL00996","13C2
PFDA","41.3","ng/L","",-99,"DL","",,"SURR","103","",-99,"LOQ","YES","40.0","",,"250","1.00","0",""
"MB 320-204304/1-A","537","RES","MB 320-204304/1-A","TALSAC","1763-23-1","Perfluorooctanesulfonic acid
(PFOS)","16","ng/L","U","6.8","DL","",,"TRG","",,"",,"40","LOQ","YES","-99","",,"250","1.00","16",""
"MB 320-204304/1-A","537","RES","MB 320-204304/1-A","TALSAC","335-67-1","Perfluorooctanoic acid
(PFOA)","8.0","ng/L","U","2.8","DL","",,"TRG","",,"",,"20","LOQ","YES","-99","",,"250","1.00","8.0",""
"MB 320-204304/1-A","537","RES","MB 320-204304/1-A","TALSAC","355-46-4","Perfluorohexanesulfonic acid
(PFHxS)","12","ng/L","U","5.5","DL","",,"TRG","",,"",,"30","LOQ","YES","-99","",,"250","1.00","12",""
"MB 320-204304/1-A","537","RES","MB 320-204304/1-A","TALSAC","375-73-5","Perfluorobutanesulfonic acid
(PFBS)","36","ng/L","U","16","DL","",,"TRG","",,"",,"90","LOQ","YES","-99","",,"250","1.00","36",""
"MB 320-204304/1-A","537","RES","MB 320-204304/1-A","TALSAC","375-85-9","Perfluoroheptanoic acid
(PFHpA)","4.0","ng/L","U","1.9","DL","",,"TRG","",,"",,"10","LOQ","YES","-99","",,"250","1.00","4.0",""
"MB 320-204304/1-A","537","RES","MB 320-204304/1-A","TALSAC","375-95-1","Perfluorononanoic acid
(PFNA)","20","ng/L","U","8.0","DL","",,"TRG","",,"",,"24","LOQ","YES","-99","",,"250","1.00","20",""
"MB 320-204304/1-A","537","RES","MB 320-204304/1-A","TALSAC","STL00993","13C2
PFHxA","34.3","ng/L","",-99,"DL","",,"SURR","86","",-99,"LOQ","YES","40.0","",,"250","1.00","0",""
"MB 320-204304/1-A","537","RES","MB 320-204304/1-A","TALSAC","STL00996","13C2
PFDA","38.2","ng/L","",-99,"DL","",,"SURR","96","",-99,"LOQ","YES","40.0","",,"250","1.00","0",""
"Unknown","Unknown","WGNA-010818-RW-0344","01/08/2018 08:10","AQ","320-34917-
1","NM","",,"3.20","537","METHOD","RES","01/17/2018 10:50","01/20/2018

19:11", "TALSAC", "COA", "WET", "NA", "1", "NA", "NA", "", "100", "320-204304", "320-204304", "NA", "320-204872", "320-34917-1", "01/09/2018 10:30", "01/09/2018 14:45", ""
"Unknown", "Unknown", "WGNA-010818-RW-4024", "01/08/2018 11:40", "AQ", "320-34917-10", "NM", "", "3.20", "537", "METHOD", "RES", "01/17/2018 10:50", "01/24/2018 05:19", "TALSAC", "COA", "WET", "NA", "1", "NA", "NA", "", "100", "320-204304", "320-204304", "NA", "320-205331", "320-34917-1", "01/09/2018 10:30", "01/09/2018 14:45", ""
"Unknown", "Unknown", "WGNA-010818-RW-4024MS", "01/08/2018 11:40", "AQ", "320-34917-10MS", "MS", "", "3.20", "537", "METHOD", "RES", "01/17/2018 10:50", "01/24/2018 05:24", "TALSAC", "COA", "WET", "NA", "1", "NA", "NA", "", "100", "320-204304", "320-204304", "NA", "320-205331", "320-34917-1", "01/09/2018 10:30", "01/09/2018 14:45", ""
"Unknown", "Unknown", "WGNA-010818-RW-4024MSD", "01/08/2018 11:40", "AQ", "320-34917-10MSD", "MSD", "", "3.20", "537", "METHOD", "RES", "01/17/2018 10:50", "01/24/2018 05:29", "TALSAC", "COA", "WET", "NA", "1", "NA", "NA", "", "100", "320-204304", "320-204304", "NA", "320-205331", "320-34917-1", "01/09/2018 10:30", "01/09/2018 14:45", ""
"Unknown", "Unknown", "WGNA-010818-FRB-4024", "01/08/2018 11:35", "AQ", "320-34917-11", "FB", "", "3.20", "537", "METHOD", "RES", "01/17/2018 10:50", "01/24/2018 05:33", "TALSAC", "COA", "WET", "NA", "1", "NA", "NA", "", "100", "320-204304", "320-204304", "NA", "320-205331", "320-34917-1", "01/09/2018 10:30", "01/09/2018 14:45", ""
"Unknown", "Unknown", "WGNA-010818-RW-4844", "01/08/2018 13:10", "AQ", "320-34917-12", "NM", "", "3.20", "537", "METHOD", "RES", "01/17/2018 10:50", "01/24/2018 05:38", "TALSAC", "COA", "WET", "NA", "1", "NA", "NA", "", "100", "320-204304", "320-204304", "NA", "320-205331", "320-34917-1", "01/09/2018 10:30", "01/09/2018 14:45", ""
"Unknown", "Unknown", "WGNA-010818-FRB-4844", "01/08/2018 13:05", "AQ", "320-34917-13", "FB", "", "3.20", "537", "METHOD", "RES", "01/17/2018 10:50", "01/24/2018 05:43", "TALSAC", "COA", "WET", "NA", "1", "NA", "NA", "", "100", "320-204304", "320-204304", "NA", "320-205331", "320-34917-1", "01/09/2018 10:30", "01/09/2018 14:45", ""
"Unknown", "Unknown", "WGNA-010818-RW-0404", "01/08/2018 09:40", "AQ", "320-34917-14", "NM", "", "3.20", "537", "METHOD", "RES", "01/17/2018 10:50", "01/24/2018 05:47", "TALSAC", "COA", "WET", "NA", "1", "NA", "NA", "", "100", "320-204304", "320-204304", "NA", "320-205331", "320-34917-1", "01/09/2018 10:30", "01/09/2018 14:45", ""
"Unknown", "Unknown", "WGNA-010818-FRB-0404", "01/08/2018 09:35", "AQ", "320-34917-15", "FB", "", "3.20", "537", "METHOD", "RES", "01/17/2018 10:50", "01/24/2018 05:52", "TALSAC", "COA", "WET", "NA", "1", "NA", "NA", "", "100", "320-204304", "320-204304", "NA", "320-205331", "320-34917-1", "01/09/2018 10:30", "01/09/2018 14:45", ""
"Unknown", "Unknown", "WGNA-010818-FRB-0344", "01/08/2018 08:05", "AQ", "320-34917-2", "FB", "", "3.20", "537", "METHOD", "RES", "01/17/2018 10:50", "01/20/2018 19:15", "TALSAC", "COA", "WET", "NA", "1", "NA", "NA", "", "100", "320-204304", "320-204304", "NA", "320-204872", "320-34917-1", "01/09/2018 10:30", "01/09/2018 14:45", ""
"Unknown", "Unknown", "WGNA-010818-RW-3957", "01/08/2018 08:40", "AQ", "320-34917-3", "NM", "", "3.20", "537", "METHOD", "RES", "01/17/2018 10:50", "01/20/2018 19:20", "TALSAC", "COA", "WET", "NA", "1", "NA", "NA", "", "100", "320-204304", "320-204304", "NA", "320-204872", "320-34917-1", "01/09/2018 10:30", "01/09/2018 14:45", ""
"Unknown", "Unknown", "WGNA-010818-FRB-3957", "01/08/2018 08:35", "AQ", "320-34917-4", "FB", "", "3.20", "537", "METHOD", "RES", "01/17/2018 10:50", "01/20/2018 19:25", "TALSAC", "COA", "WET", "NA", "1", "NA", "NA", "", "100", "320-204304", "320-204304", "NA", "320-204872", "320-34917-1", "01/09/2018 10:30", "01/09/2018 14:45", ""
"Unknown", "Unknown", "WGNA-010818-DUP-16", "01/08/2018 07:00", "AQ", "320-34917-5", "FD", "", "3.20", "537", "METHOD", "RES", "01/17/2018 10:50", "01/20/2018 19:29", "TALSAC", "COA", "WET", "NA", "1", "NA", "NA", "", "100", "320-204304", "320-204304", "NA", "320-204872", "320-34917-1", "01/09/2018 10:30", "01/09/2018 14:45", ""
"Unknown", "Unknown", "WGNA-010818-RW-3178", "01/08/2018 10:10", "AQ", "320-34917-6", "NM", "", "3.20", "537", "METHOD", "RES", "01/17/2018 10:50", "01/20/2018 19:34", "TALSAC", "COA", "WET", "NA", "1", "NA", "NA", "", "100", "320-204304", "320-204304", "NA", "320-204872", "320-34917-1", "01/09/2018 10:30", "01/09/2018 14:45", ""

"Unknown","Unknown","WGNA-010818-FRB-3178","01/08/2018 10:05","AQ","320-34917-7","FB","","3.20","537","METHOD","RES","01/17/2018 10:50","01/20/2018 19:39","TALSAC","COA","WET","NA","1","NA","NA","","100","320-204304","320-204304","NA","320-204872","320-34917-1","01/09/2018 10:30","01/09/2018 14:45",""

"Unknown","Unknown","NAWC-010818-RW-141","01/08/2018 11:10","AQ","320-34917-8","NM","","3.20","537","METHOD","RES","01/17/2018 10:50","01/20/2018 19:43","TALSAC","COA","WET","NA","1","NA","NA","","100","320-204304","320-204304","NA","320-204872","320-34917-1","01/09/2018 10:30","01/09/2018 14:45",""

"Unknown","Unknown","NAWC-010818-FRB-141","01/08/2018 11:05","AQ","320-34917-9","FB","","3.20","537","METHOD","RES","01/17/2018 10:50","01/24/2018 05:15","TALSAC","COA","WET","NA","1","NA","NA","","100","320-204304","320-204304","NA","320-205331","320-34917-1","01/09/2018 10:30","01/09/2018 14:45",""

"Unknown","Unknown","LLCS 320-204304/2-A","","AQ","LLCS 320-204304/2-A","LCS","","-99","537","METHOD","RES","01/17/2018 10:50","01/20/2018 19:06","TALSAC","COA","WET","NA","1","NA","NA","","100","320-204304","320-204304","NA","320-204872","320-34917-1","01/17/2018 10:50","01/09/2018 14:45",""

"Unknown","Unknown","MB 320-204304/1-A","","AQ","MB 320-204304/1-A","MB","","-99","537","METHOD","RES","01/17/2018 10:50","01/20/2018 19:01","TALSAC","COA","WET","NA","1","NA","NA","","100","320-204304","320-204304","NA","320-204872","320-34917-1","01/17/2018 10:50","01/09/2018 14:45",""

TO: A. FREBOWITZ
SDG: 320-34917-1

PAGE 2

Notes

Samples with detections and their associated FRBs are summarized below. No detected results were present in the FRBs.

<u>Sample</u>	<u>Associated FRB</u>
WGNA-010818-RW-0344	WGNA-010818-FRB-0344
WGNA-010818-RW-3957	WGNA-010818-FRB-3957
WGNA-010818-DUP-16	WGNA-010818-FRB-0404
WGNA-010818-RW-3178	WGNA-010818-FRB-3178
NAWC-010818-RW-141	NAWC-010818-FRB-141
WGNA-010818-RW-4024	WGNA-010818-FRB-4024
WGNA-010818-RW-4844	WGNA-010818-FRB-4844
WGNA-010818-RW-0404	WGNA-010818-FRB-0404

Non-detected results were reported to the Limit of Detection (LOD).

The buffering agent Trizma was added to all drinking water samples.

Executive Summary

Laboratory Performance: No issues.

Other Factors Affecting Data Quality: Results below the RL were estimated.

The data for these analyses were reviewed with reference to the Environmental Protection Agency document EPA/600/R-08/092, Method 537, "Determination of Selected Perfluorinated Alkyl Acids in Drinking Water by Solid Phase Extraction and Liquid Chromatography/Tandem Mass Spectrometry (LC/MS/MS)", (September 2009) and the US EPA National Functional Guidelines for Organic Data Review (January 2017) as applicable. The text of this report has been formulated to address only those areas affecting data quality.



Tetra Tech, Inc.
Terri L. Solomon
Chemist/Data Validator



Tetra Tech, Inc.
Joseph A. Samchuck
Data Validation Manager

Attachments:

Appendix A – Qualified Analytical Results
Appendix B – Results as Reported by the Laboratory
Appendix C – Support Documentation

Data Qualifier Definitions

The following definitions provide brief explanations of the validation qualifiers assigned to results in the data review process.

U	The analyte was analyzed for, but was not detected at a level greater than or equal to the level of the adjusted method detection limit for sample and method.
J	The analyte was positively identified and the associated numerical value is the approximate concentration of the analyte in the sample (due either to the quality of the data generated because certain quality control criteria were not met, or the concentration of the analyte was below the reporting limit).
J+	The result is an estimated quantity, but the result may be biased high.
J-	The result is an estimated quantity, but the result may be biased low.
UJ	The analyte was analyzed for, but was not detected. The reported detection limit is approximate and may be inaccurate or imprecise.
R	The sample result (detected) is unusable due to the quality of the data generated because certain criteria were not met. The analyte may or may not be present in the sample.
UR	The sample result (nondetected) is unusable due to the quality of the data generated because certain criteria were not met. The analyte may or may not be present in the sample.

Appendix A

Qualified Analytical Results

Qualifier Codes:

- A = Lab Blank Contamination
- B = Field Blank Contamination
- C = Calibration Noncompliance (i.e., % RSDs, %Ds, ICVs, CCVs, RRFs, etc.)
- C01 = GC/MS Tuning Noncompliance
- D = MS/MSD Recovery Noncompliance
- E = LCS/LCSD Recovery Noncompliance
- F = Lab Duplicate Imprecision
- G = Field Duplicate Imprecision
- H = Holding Time Exceedance
- I = ICP Serial Dilution Noncompliance
- J = ICP PDS Recovery Noncompliance; MSA's $r < 0.995$
- K = ICP Interference - includes ICS % R Noncompliance
- L = Instrument Calibration Range Exceedance
- M = Sample Preservation Noncompliance
- N = Internal Standard Noncompliance
- N01 = Internal Standard Recovery Noncompliance Dioxins
- N02 = Recovery Standard Noncompliance Dioxins
- N03 = Clean-up Standard Noncompliance Dioxins
- O = Poor Instrument Performance (i.e., base-time drifting)
- P = Uncertainty near detection limit ($< 2 \times$ IDL for inorganics and $<$ CRQL for organics)
- Q = Other problems (can encompass a number of issues; i.e.chromatography,interferences, etc.)
- R = Surrogates Recovery Noncompliance
- S = Pesticide/PCB Resolution
- T = % Breakdown Noncompliance for DDT and Endrin
- U = RPD between columns/detectors $>40\%$ for positive results determined via GC/HPLC
- V = Non-linear calibrations; correlation coefficient $r < 0.995$
- W = EMPC result
- X = Signal to noise response drop
- Y = Percent solids $<30\%$
- Z = Uncertainty at 2 standard deviations is greater than sample activity
- Z1 = Tentatively Identified Compound considered presumptively present
- Z2 = Tentatively Identified Compound column bleed
- Z3 = Tentatively Identified Compound aldol condensate
- Z4 = Sample activity is less than the at uncertainty at 3 standard deviations and greater than the MDC
- Z5 = Sample activity is less than the at uncertainty at 3 standard deviations and less than the MDC

PROJ_NO: 08005-WE04 SDG: 320-34917-1 FRACTION: PFAS MEDIA: WATER	NSAMPLE	NAWC-010818-FRB-141			NAWC-010818-RW-141			WGNA-010818-DUP-16			WGNA-010818-FRB-0344		
	LAB_ID	320-34917-9			320-34917-8			320-34917-5			320-34917-2		
	SAMP_DATE	1/8/2018			1/8/2018			1/8/2018			1/8/2018		
	QC_TYPE	FB			NM			FD			FB		
	UNITS	NG/L			NG/L			NG/L			NG/L		
	PCT_SOLIDS	0.0			0.0			0.0			0.0		
	DUP_OF							WGNA-010818-RW-0404					
PARAMETER	RESULT	VQL	QLCD	RESULT	VQL	QLCD	RESULT	VQL	QLCD	RESULT	VQL	QLCD	
PENTADECAFLUOROOCTANOIC ACID	7.5	U		15	J	P	21			7.9	U		
PERFLUOROBUTANESULFONIC ACID	34	U		35	U		34	U		36	U		
PERFLUOROHEPTANOIC ACID	3.8	U		7.6	J	P	6.2	J	P	3.9	U		
PERFLUOROHXANESULFONIC ACID	11	U		16	J	P	8	J	P	12	U		
PERFLUORONONANOIC ACID	19	U		19	U		19	U		20	U		
PERFLUOROOCTANE SULFONIC ACID	15	U		24	J	P	25	J	P	16	U		

PROJ_NO: 08005-WE04 SDG: 320-34917-1 FRACTION: PFAS MEDIA: WATER	NSAMPLE	WGNA-010818-FRB-0404			WGNA-010818-FRB-3178			WGNA-010818-FRB-3957			WGNA-010818-FRB-4024		
	LAB_ID	320-34917-15			320-34917-7			320-34917-4			320-34917-11		
	SAMP_DATE	1/8/2018			1/8/2018			1/8/2018			1/8/2018		
	QC_TYPE	FB			FB			FB			FB		
	UNITS	NG/L			NG/L			NG/L			NG/L		
	PCT_SOLIDS	0.0			0.0			0.0			0.0		
	DUP_OF												
PARAMETER	RESULT	VQL	QLCD	RESULT	VQL	QLCD	RESULT	VQL	QLCD	RESULT	VQL	QLCD	
PENTADECAFLUOROOCTANOIC ACID	7.9	U		7.8	U		7.8	U		7.8	U		
PERFLUOROBUTANESULFONIC ACID	36	U		35	U		35	U		35	U		
PERFLUOROHEPTANOIC ACID	4	U		3.9	U		3.9	U		3.9	U		
PERFLUOROHXANESULFONIC ACID	12	U		12	U		12	U		12	U		
PERFLUORONONANOIC ACID	20	U		19	U		20	U		19	U		
PERFLUOROOCTANE SULFONIC ACID	16	U		16	U		16	U		16	U		

PROJ_NO: 08005-WE04 SDG: 320-34917-1 FRACTION: PFAS MEDIA: WATER	NSAMPLE	WGNA-010818-FRB-4844			WGNA-010818-RW-0344			WGNA-010818-RW-0404			WGNA-010818-RW-3178		
	LAB_ID	320-34917-13			320-34917-1			320-34917-14			320-34917-6		
	SAMP_DATE	1/8/2018			1/8/2018			1/8/2018			1/8/2018		
	QC_TYPE	FB			NM			NM			NM		
	UNITS	NG/L			NG/L			NG/L			NG/L		
	PCT_SOLIDS	0.0			0.0			0.0			0.0		
	DUP_OF												
PARAMETER	RESULT	VQL	QLCD	RESULT	VQL	QLCD	RESULT	VQL	QLCD	RESULT	VQL	QLCD	
PENTADECAFLUOROOCTANOIC ACID	8	U		24			21			9.8	J	P	
PERFLUOROBUTANESULFONIC ACID	36	U		36	U		36	U		38	U		
PERFLUOROHEPTANOIC ACID	4	U		6.4	J	P	6.3	J	P	2.8	J	P	
PERFLUOROHXANESULFONIC ACID	12	U		18	J	P	8.3	J	P	7	J	P	
PERFLUORONONANOIC ACID	20	U		32			20	U		21	U		
PERFLUOROOCTANE SULFONIC ACID	16	U		32	J	P	26	J	P	16	J	P	

PROJ_NO: 08005-WE04 SDG: 320-34917-1 FRACTION: PFAS MEDIA: WATER	NSAMPLE	WGNA-010818-RW-3957			WGNA-010818-RW-4024			WGNA-010818-RW-4844		
	LAB_ID	320-34917-3			320-34917-10			320-34917-12		
	SAMP_DATE	1/8/2018			1/8/2018			1/8/2018		
	QC_TYPE	NM			NM			NM		
	UNITS	NG/L			NG/L			NG/L		
	PCT_SOLIDS	0.0			0.0			0.0		
	DUP_OF									
PARAMETER	RESULT	VQL	QLCD	RESULT	VQL	QLCD	RESULT	VQL	QLCD	
PENTADECAFLUOROOCTANOIC ACID	15	J	P	12	J	P	14	J	P	
PERFLUOROBUTANESULFONIC ACID	35	U		36	U		36	U		
PERFLUOROHEPTANOIC ACID	3.8	J	P	3.6	J	P	7.1	J	P	
PERFLUOROHXANESULFONIC ACID	6.5	J	P	12	U		12	U		
PERFLUORONONANOIC ACID	19	U		20	U		20	U		
PERFLUOROOCTANE SULFONIC ACID	18	J	P	18	J	P	7.9	J	P	

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: WGNA-010818-RW-0344 Lab Sample ID: 320-34917-1
 Matrix: Water Lab File ID: 2018.01.20_537AA_009.d
 Analysis Method: 537 Date Collected: 01/08/2018 08:10
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 248.7(mL) Date Analyzed: 01/20/2018 19:11
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 204872 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	32	J	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	24		20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	32		24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	18	J	30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	6.4	J	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	91		70-130
STL00996	13C2 PFDA	93		70-130

Steve L. Selman
02/02/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: WGNA-010818-FRB-0344 Lab Sample ID: 320-34917-2
 Matrix: Water Lab File ID: 2018.01.20_537AA_010.d
 Analysis Method: 537 Date Collected: 01/08/2018 08:05
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 253.2 (mL) Date Analyzed: 01/20/2018 19:15
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 204872 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	39	16	6.7
335-67-1	Perfluorooctanoic acid (PFOA)	7.9	U	20	7.9	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	7.9
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	30	12	5.4
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.9	U	9.9	3.9	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	89	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	97		70-130
STL00996	13C2 PFDA	98		70-130

Wesley L. Selman
02/02/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: WGNA-010818-RW-3957 Lab Sample ID: 320-34917-3
 Matrix: Water Lab File ID: 2018.01.20_537AA_011.d
 Analysis Method: 537 Date Collected: 01/08/2018 08:40
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 257.4 (mL) Date Analyzed: 01/20/2018 19:20
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 204872 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	18	J	39	16	6.6
335-67-1	Perfluorooctanoic acid (PFOA)	15	J	19	7.8	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U M	23	19	7.8
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	6.5	J	29	12	5.3
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	J	9.7	3.9	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	35	U	87	35	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	91		70-130
STL00996	13C2 PFDA	104		70-130

Wesley L. Selman
02/02/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: WGNA-010818-FRB-3957 Lab Sample ID: 320-34917-4
 Matrix: Water Lab File ID: 2018.01.20_537AA_012.d
 Analysis Method: 537 Date Collected: 01/08/2018 08:35
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 256.1(mL) Date Analyzed: 01/20/2018 19:25
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 204872 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	39	16	6.6
335-67-1	Perfluorooctanoic acid (PFOA)	7.8	U	20	7.8	2.7
375-95-1	Perfluorononanoic acid (PFNA)	20	U	23	20	7.8
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	29	12	5.4
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.9	U	9.8	3.9	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	35	U	88	35	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	96		70-130
STL00996	13C2 PFDA	98		70-130

W. J. Selman

02/02/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: WGNA-010818-DUP-16 Lab Sample ID: 320-34917-5
 Matrix: Water Lab File ID: 2018.01.20_537AA_013.d
 Analysis Method: 537 Date Collected: 01/08/2018 07:00
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 262.5 (mL) Date Analyzed: 01/20/2018 19:29
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 204872 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	25	J	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	21		19	7.6	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	8.0	J	29	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	6.2	J	9.5	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	86	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	96		70-130
STL00996	13C2 PFDA	109		70-130

Wesley L. Salmeron
02/02/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: WGNA-010818-RW-3178 Lab Sample ID: 320-34917-6
 Matrix: Water Lab File ID: 2018.01.20_537AA_014.d
 Analysis Method: 537 Date Collected: 01/08/2018 10:10
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 239.2 (mL) Date Analyzed: 01/20/2018 19:34
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 204872 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	J	42	17	7.1
335-67-1	Perfluorooctanoic acid (PFOA)	9.8	J	21	8.4	2.9
375-95-1	Perfluorononanoic acid (PFNA)	21	U	25	21	8.4
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	7.0	J	31	13	5.7
375-85-9	Perfluoroheptanoic acid (PFHpA)	2.8	J	10	4.2	2.0
375-73-5	Perfluorobutanesulfonic acid (PFBS)	38	U	94	38	17

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	90		70-130
STL00996	13C2 PFDA	102		70-130

Steve L. Selman
02/02/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: WGNA-010818-FRB-3178 Lab Sample ID: 320-34917-7
 Matrix: Water Lab File ID: 2018.01.20_537AA_015.d
 Analysis Method: 537 Date Collected: 01/08/2018 10:05
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 256.7(mL) Date Analyzed: 01/20/2018 19:39
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 204872 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	39	16	6.6
335-67-1	Perfluorooctanoic acid (PFOA)	7.8	U	19	7.8	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.8
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	29	12	5.4
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.9	U	9.7	3.9	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	35	U	88	35	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	98		70-130
STL00996	13C2 PFDA	103		70-130

Steve L. Selman
02/02/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: NAWC-010818-RW-141 Lab Sample ID: 320-34917-8
 Matrix: Water Lab File ID: 2018.01.20_537AA_016.d
 Analysis Method: 537 Date Collected: 01/08/2018 11:10
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 257.5 (mL) Date Analyzed: 01/20/2018 19:43
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 204872 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	24	J	39	16	6.6
335-67-1	Perfluorooctanoic acid (PFOA)	15	J	19	7.8	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.8
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	16	J	29	12	5.3
375-85-9	Perfluoroheptanoic acid (PFHpA)	7.6	J	9.7	3.9	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	35	U	87	35	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	88		70-130
STL00996	13C2 PFDA	96		70-130

Wesley L. Selman
02/02/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: NAWC-010818-FRB-141 Lab Sample ID: 320-34917-9
 Matrix: Water Lab File ID: 2018.01.23537A_007.d
 Analysis Method: 537 Date Collected: 01/08/2018 11:05
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 266.1(mL) Date Analyzed: 01/24/2018 05:15
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 205331 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	38	15	6.4
335-67-1	Perfluorooctanoic acid (PFOA)	7.5	U	19	7.5	2.6
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.5
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	U	9.4	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	85	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	95		70-130
STL00996	13C2 PFDA	99		70-130

Steve L. Salzman
02/02/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: WGNA-010818-RW-4024 Lab Sample ID: 320-34917-10
 Matrix: Water Lab File ID: 2018.01.23537A_008.d
 Analysis Method: 537 Date Collected: 01/08/2018 11:40
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 251.2 (mL) Date Analyzed: 01/24/2018 05:19
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 205331 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	18	J-M	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	12	J	20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.6	J	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	71		70-130
STL00996	13C2 PFDA	93		70-130

Mari L. Selman

02/02/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: WGNA-010818-FRB-4024 Lab Sample ID: 320-34917-11
 Matrix: Water Lab File ID: 2018.01.23537A_011.d
 Analysis Method: 537 Date Collected: 01/08/2018 11:35
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 257.4 (mL) Date Analyzed: 01/24/2018 05:33
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 205331 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	39	16	6.6
335-67-1	Perfluorooctanoic acid (PFOA)	7.8	U	19	7.8	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.8
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	29	12	5.3
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.9	U	9.7	3.9	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	35	U	87	35	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	98		70-130
STL00996	13C2 PFDA	100		70-130

Steve L. Selman
02/02/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: WGNA-010818-RW-4844 Lab Sample ID: 320-34917-12
 Matrix: Water Lab File ID: 2018.01.23537A_012.d
 Analysis Method: 537 Date Collected: 01/08/2018 13:10
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 253.5 (mL) Date Analyzed: 01/24/2018 05:38
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 205331 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	7.9	J M	39	16	6.7
335-67-1	Perfluorooctanoic acid (PFOA)	14	J	20	7.9	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	7.9
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	30	12	5.4
375-85-9	Perfluoroheptanoic acid (PFHpA)	7.1	J	9.9	3.9	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	89	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	97		70-130
STL00996	13C2 PFDA	98		70-130

Mari L. Salmeron
02/02/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: WGNA-010818-FRB-4844 Lab Sample ID: 320-34917-13
 Matrix: Water Lab File ID: 2018.01.23537A_013.d
 Analysis Method: 537 Date Collected: 01/08/2018 13:05
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 249.5 (mL) Date Analyzed: 01/24/2018 05:43
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 205331 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	8.0	U	20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.0	U	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	97		70-130
STL00996	13C2 PFDA	97		70-130

Mari L. Selman
02/02/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: WGNA-010818-RW-0404 Lab Sample ID: 320-34917-14
 Matrix: Water Lab File ID: 2018.01.23537A_014.d
 Analysis Method: 537 Date Collected: 01/08/2018 09:40
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 249.4 (mL) Date Analyzed: 01/24/2018 05:47
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 205331 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	26	J M	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	21		20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	8.3	J	30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	6.3	J	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	96		70-130
STL00996	13C2 PFDA	100		70-130

Maria L. Selman
02/02/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: WGNA-010818-FRB-0404 Lab Sample ID: 320-34917-15
 Matrix: Water Lab File ID: 2018.01.23537A_015.d
 Analysis Method: 537 Date Collected: 01/08/2018 09:35
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 252.5 (mL) Date Analyzed: 01/24/2018 05:52
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 205331 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	40	16	6.7
335-67-1	Perfluorooctanoic acid (PFOA)	7.9	U	20	7.9	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	7.9
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	30	12	5.4
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.0	U	9.9	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	89	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	103		70-130
STL00996	13C2 PFDA	103		70-130

Maria L. Selman
02/02/2018

Appendix B

Results as Reported by the Laboratory

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: WGNA-010818-RW-0344 Lab Sample ID: 320-34917-1
 Matrix: Water Lab File ID: 2018.01.20_537AA_009.d
 Analysis Method: 537 Date Collected: 01/08/2018 08:10
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 248.7(mL) Date Analyzed: 01/20/2018 19:11
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 204872 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	32	J	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	24		20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	32		24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	18	J	30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	6.4	J	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	91		70-130
STL00996	13C2 PFDA	93		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: WGNA-010818-FRB-0344 Lab Sample ID: 320-34917-2
 Matrix: Water Lab File ID: 2018.01.20_537AA_010.d
 Analysis Method: 537 Date Collected: 01/08/2018 08:05
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 253.2 (mL) Date Analyzed: 01/20/2018 19:15
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 204872 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	39	16	6.7
335-67-1	Perfluorooctanoic acid (PFOA)	7.9	U	20	7.9	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	7.9
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	30	12	5.4
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.9	U	9.9	3.9	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	89	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	97		70-130
STL00996	13C2 PFDA	98		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: WGNA-010818-RW-3957 Lab Sample ID: 320-34917-3
 Matrix: Water Lab File ID: 2018.01.20_537AA_011.d
 Analysis Method: 537 Date Collected: 01/08/2018 08:40
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 257.4 (mL) Date Analyzed: 01/20/2018 19:20
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 204872 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	18	J	39	16	6.6
335-67-1	Perfluorooctanoic acid (PFOA)	15	J	19	7.8	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U M	23	19	7.8
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	6.5	J	29	12	5.3
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	J	9.7	3.9	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	35	U	87	35	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	91		70-130
STL00996	13C2 PFDA	104		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: WGNA-010818-FRB-3957 Lab Sample ID: 320-34917-4
 Matrix: Water Lab File ID: 2018.01.20_537AA_012.d
 Analysis Method: 537 Date Collected: 01/08/2018 08:35
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 256.1(mL) Date Analyzed: 01/20/2018 19:25
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 204872 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	39	16	6.6
335-67-1	Perfluorooctanoic acid (PFOA)	7.8	U	20	7.8	2.7
375-95-1	Perfluorononanoic acid (PFNA)	20	U	23	20	7.8
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	29	12	5.4
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.9	U	9.8	3.9	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	35	U	88	35	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	96		70-130
STL00996	13C2 PFDA	98		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: WGNA-010818-DUP-16 Lab Sample ID: 320-34917-5
 Matrix: Water Lab File ID: 2018.01.20_537AA_013.d
 Analysis Method: 537 Date Collected: 01/08/2018 07:00
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 262.5 (mL) Date Analyzed: 01/20/2018 19:29
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 204872 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	25	J	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	21		19	7.6	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	8.0	J	29	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	6.2	J	9.5	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	86	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	96		70-130
STL00996	13C2 PFDA	109		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: WGNA-010818-RW-3178 Lab Sample ID: 320-34917-6
 Matrix: Water Lab File ID: 2018.01.20_537AA_014.d
 Analysis Method: 537 Date Collected: 01/08/2018 10:10
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 239.2 (mL) Date Analyzed: 01/20/2018 19:34
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 204872 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	J	42	17	7.1
335-67-1	Perfluorooctanoic acid (PFOA)	9.8	J	21	8.4	2.9
375-95-1	Perfluorononanoic acid (PFNA)	21	U	25	21	8.4
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	7.0	J	31	13	5.7
375-85-9	Perfluoroheptanoic acid (PFHpA)	2.8	J	10	4.2	2.0
375-73-5	Perfluorobutanesulfonic acid (PFBS)	38	U	94	38	17

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	90		70-130
STL00996	13C2 PFDA	102		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: WGNA-010818-FRB-3178 Lab Sample ID: 320-34917-7
 Matrix: Water Lab File ID: 2018.01.20_537AA_015.d
 Analysis Method: 537 Date Collected: 01/08/2018 10:05
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 256.7(mL) Date Analyzed: 01/20/2018 19:39
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 204872 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	39	16	6.6
335-67-1	Perfluorooctanoic acid (PFOA)	7.8	U	19	7.8	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.8
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	29	12	5.4
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.9	U	9.7	3.9	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	35	U	88	35	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	98		70-130
STL00996	13C2 PFDA	103		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: NAWC-010818-RW-141 Lab Sample ID: 320-34917-8
 Matrix: Water Lab File ID: 2018.01.20_537AA_016.d
 Analysis Method: 537 Date Collected: 01/08/2018 11:10
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 257.5 (mL) Date Analyzed: 01/20/2018 19:43
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 204872 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	24	J	39	16	6.6
335-67-1	Perfluorooctanoic acid (PFOA)	15	J	19	7.8	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.8
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	16	J	29	12	5.3
375-85-9	Perfluoroheptanoic acid (PFHpA)	7.6	J	9.7	3.9	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	35	U	87	35	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	88		70-130
STL00996	13C2 PFDA	96		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: NAWC-010818-FRB-141 Lab Sample ID: 320-34917-9
 Matrix: Water Lab File ID: 2018.01.23537A_007.d
 Analysis Method: 537 Date Collected: 01/08/2018 11:05
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 266.1(mL) Date Analyzed: 01/24/2018 05:15
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 205331 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	38	15	6.4
335-67-1	Perfluorooctanoic acid (PFOA)	7.5	U	19	7.5	2.6
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.5
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	U	9.4	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	85	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	95		70-130
STL00996	13C2 PFDA	99		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: WGNA-010818-RW-4024 Lab Sample ID: 320-34917-10
 Matrix: Water Lab File ID: 2018.01.23537A_008.d
 Analysis Method: 537 Date Collected: 01/08/2018 11:40
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 251.2 (mL) Date Analyzed: 01/24/2018 05:19
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 205331 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	18	J M	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	12	J	20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.6	J	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	71		70-130
STL00996	13C2 PFDA	93		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: WGNA-010818-FRB-4024 Lab Sample ID: 320-34917-11
 Matrix: Water Lab File ID: 2018.01.23537A_011.d
 Analysis Method: 537 Date Collected: 01/08/2018 11:35
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 257.4 (mL) Date Analyzed: 01/24/2018 05:33
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 205331 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	39	16	6.6
335-67-1	Perfluorooctanoic acid (PFOA)	7.8	U	19	7.8	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.8
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	29	12	5.3
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.9	U	9.7	3.9	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	35	U	87	35	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	98		70-130
STL00996	13C2 PFDA	100		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: WGNA-010818-RW-4844 Lab Sample ID: 320-34917-12
 Matrix: Water Lab File ID: 2018.01.23537A_012.d
 Analysis Method: 537 Date Collected: 01/08/2018 13:10
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 253.5 (mL) Date Analyzed: 01/24/2018 05:38
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 205331 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	7.9	J M	39	16	6.7
335-67-1	Perfluorooctanoic acid (PFOA)	14	J	20	7.9	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	7.9
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	30	12	5.4
375-85-9	Perfluoroheptanoic acid (PFHpA)	7.1	J	9.9	3.9	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	89	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	97		70-130
STL00996	13C2 PFDA	98		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: WGNA-010818-FRB-4844 Lab Sample ID: 320-34917-13
 Matrix: Water Lab File ID: 2018.01.23537A_013.d
 Analysis Method: 537 Date Collected: 01/08/2018 13:05
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 249.5 (mL) Date Analyzed: 01/24/2018 05:43
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 205331 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	8.0	U	20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.0	U	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	97		70-130
STL00996	13C2 PFDA	97		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: WGNA-010818-RW-0404 Lab Sample ID: 320-34917-14
 Matrix: Water Lab File ID: 2018.01.23537A_014.d
 Analysis Method: 537 Date Collected: 01/08/2018 09:40
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 249.4 (mL) Date Analyzed: 01/24/2018 05:47
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 205331 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	26	J M	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	21		20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	8.3	J	30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	6.3	J	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	96		70-130
STL00996	13C2 PFDA	100		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: WGNA-010818-FRB-0404 Lab Sample ID: 320-34917-15
 Matrix: Water Lab File ID: 2018.01.23537A_015.d
 Analysis Method: 537 Date Collected: 01/08/2018 09:35
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 252.5 (mL) Date Analyzed: 01/24/2018 05:52
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 205331 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	40	16	6.7
335-67-1	Perfluorooctanoic acid (PFOA)	7.9	U	20	7.9	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	7.9
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	30	12	5.4
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.0	U	9.9	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	89	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	103		70-130
STL00996	13C2 PFDA	103		70-130

Appendix C

Support Documentation

ANALYTE	ORIGINAL RW-0404	DUPLICATE DUP-16	RL	RPD	RPD > 50%	ORIGINAL SAMPLE CONC >5xRL	DUPLICATE SAMPLE CONC >5xRL	DIFFERENCE >2XRL
Perfluorooctanoic acid (PFOA)	21	21	20	0	FALSE	FALSE	FALSE	FALSE
Perfluoroheptanoic acid (PFHpA)	6.3	6.2	10	1.6	FALSE	FALSE	FALSE	FALSE
Perfluorohexanesulfonic acid (PFHxS)	8.3	8	30	3.68	FALSE	FALSE	FALSE	FALSE
Perfluorooctanesulfonic acid (PFOS)	26	25	40	3.92	FALSE	FALSE	FALSE	FALSE

TestAmerica Sacramento
 880 Riverside Parkway
 West Sacramento, CA 95605-1500
 phone 916.373.5600 fax 303.467.7248

Chain of Custody Record

TestAmerica
 THE LEADER IN ENVIRONMENTAL TESTING
TestAmerica Laboratories, Inc.

Regulatory Program: DW NPDES RCRA Other:

Client Contact	Project Manager: Andy Frebowitz	Site Contact: Mary Kay Bond	Date: 1/8/2018	COC No:
TetraTech	Tel/Fax: 610.382.1170	Lab Contact: Dave Alltucker	Carrier: FedEx	1 of 1 COCs
234 Mall Boulevard Suite 260	Analysis Turnaround Time			Sampler: Mary Kay Bond
King of Prussia, PA 19406	<input type="checkbox"/> CALENDAR DAYS <input type="checkbox"/> WORKING DAYS			For Lab Use Only:
610-382-1174	TAT if different from Below 21			Walk-in Client:
610-491-9688	<input type="checkbox"/> 2 weeks			Lab Sampling:
Project Name: WE04	<input type="checkbox"/> 1 week			
Site: WE04	<input type="checkbox"/> 2 days			
P O # 1132358 (through EarthToxics)	<input type="checkbox"/> 1 day			Job / SDG No.:

Sample Identification	Sample Date	Sample Time	Sample Type (C=Comp, G=Grab)	Matrix	# of Cont.	Filtered Sample (Y/N)	Perform MS/MSD (Y/N)	EPA 537 UCMRS	Sample Specific Notes:
WGNA-010818-RW-0344	1/8/2018	08:10	G	DW	2	N	Y		
WGNA-010818-FRB-0344	1/8/2018	08:05	G	DW	2	N	Y		Field Reagent Blank
WGNA-010818-RW-3957	1/8/2018	08:40	G	DW	2	N	Y		
WGNA-010818-FRB-3957	1/8/2018	08:35	G	DW	2	N	Y		Field Reagent Blank
WGNA-010818-DUP-16	1/8/2018	07:00	G	DW	2	N	Y		Duplicate
WGNA-010818-RW-3178	1/8/2018	10:10	G	DW	2	N	Y		
WGNA-010818-FRB-3178	1/8/2018	10:05	G	DW	2	N	Y		Field Reagent Blank
NAWC-010818-RW-141	1/8/2018	11:10	G	DW	2	N	Y		
NAWC-010818-FRB-141	1/8/2018	11:05	G	DW	2	N	Y		Field Reagent Blank
WGNA-010818-RW-4024	1/8/2018	11:40	G	DW	6	N	Y		MS/MSD
WGNA-010818-FRB-4024	1/8/2018	11:35	G	DW	2	N	Y		Field Reagent Blank
WGNA-010818-RW-4844	1/8/2018	13:10	G	DW	2	N	Y		
WGNA-010818-FRB-4844	1/8/2018	13:05	G	DW	2	N	Y		Field Reagent Blank
WGNA-010818-RW-0404	1/8/2018	09:40	G	DW	2	N	Y		
WGNA-010818-FRB-0404	1/8/2018	09:35	G	DW	2	N	Y		Field Reagent Blank

Preservation Used: 1= Ice, 2= HCl; 3= H2SO4; 4=HNO3; 5=NaOH; 6= Other: Trizma

Possible Hazard Identification:
 Are any samples from a listed EPA Hazardous Waste? Please List any EPA Waste Codes for the sample in the


Non-Hazard Flammable Skin Irritant Poison B Unknown

Sample Disposal (A fee may be assessed if samples are retained longer than 1 month)
 Return to Client Disposal by Lab Archive for _____ Months

Fed Ex Tracking: 77116333 5860

Custody Seals Intact: Yes No Custody Seal No.: _____ Cooler Temp. (°C): Obs'd: 5.2 Corr'd: 5.2 Therm ID No.: AK-2 100

Relinquished by: <i>Christina M. Simon</i>	Company: Tetra Tech	Date/Time: 1/8/2018 18:00	Received by: <i>D. H.</i>	Company: <i>TH Sae</i>	Date/Time: 1/9/18 10:30
Relinquished by:	Company:	Date/Time:	Received by:	Company:	Date/Time:
Relinquished by:	Company:	Date/Time:	Received in Laboratory by:	Company:	Date/Time:



320-34917 Chain of Custody

Page 328 of 329

Case Narrative

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-34917-1

Job ID: 320-34917-1

Laboratory: TestAmerica Sacramento

Narrative

**Job Narrative
320-34917-1**

Receipt

The samples were received on 1/9/2018 10:30 AM; the samples arrived in good condition, properly preserved and, where required, on ice. The temperature of the cooler at receipt was 3.2° C.

LCMS

Method(s) 537: The first level standard from the initial calibration curve is used to evaluate the tune criteria. The instrument mass windows are set at +/- 0.5amu; therefore, detection of the analyte serves as verification that the assigned mass is within +/- 0.5amu of the true value, which meets the DoD/DOE QSM tune criterion.

No additional analytical or quality issues were noted, other than those described above or in the Definitions/Glossary page.

Organic Prep

No analytical or quality issues were noted, other than those described in the Definitions/Glossary page.

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13
- 14
- 15

Sample Summary

Client: Tetra Tech, Inc.

TestAmerica Job ID: 320-34917-1

Project/Site: Warminster: PFAS, NAS JRB Willow Grove

Lab Sample ID	Client Sample ID	Matrix	Collected	Received
320-34917-1	WGNA-010818-RW-0344	Water	01/08/18 08:10	01/09/18 10:30
320-34917-2	WGNA-010818-FRB-0344	Water	01/08/18 08:05	01/09/18 10:30
320-34917-3	WGNA-010818-RW-3957	Water	01/08/18 08:40	01/09/18 10:30
320-34917-4	WGNA-010818-FRB-3957	Water	01/08/18 08:35	01/09/18 10:30
320-34917-5	WGNA-010818-DUP-16	Water	01/08/18 07:00	01/09/18 10:30
320-34917-6	WGNA-010818-RW-3178	Water	01/08/18 10:10	01/09/18 10:30
320-34917-7	WGNA-010818-FRB-3178	Water	01/08/18 10:05	01/09/18 10:30
320-34917-8	NAWC-010818-RW-141	Water	01/08/18 11:10	01/09/18 10:30
320-34917-9	NAWC-010818-FRB-141	Water	01/08/18 11:05	01/09/18 10:30
320-34917-10	WGNA-010818-RW-4024	Water	01/08/18 11:40	01/09/18 10:30
320-34917-11	WGNA-010818-FRB-4024	Water	01/08/18 11:35	01/09/18 10:30
320-34917-12	WGNA-010818-RW-4844	Water	01/08/18 13:10	01/09/18 10:30
320-34917-13	WGNA-010818-FRB-4844	Water	01/08/18 13:05	01/09/18 10:30
320-34917-14	WGNA-010818-RW-0404	Water	01/08/18 09:40	01/09/18 10:30
320-34917-15	WGNA-010818-FRB-0404	Water	01/08/18 09:35	01/09/18 10:30

Definitions/Glossary

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-34917-1

Qualifiers

LCMS

Qualifier	Qualifier Description
U	Undetected at the Limit of Detection.
J	Estimated: The analyte was positively identified; the quantitation is an estimation
M	Manual integrated compound.

Glossary

Abbreviation	These commonly used abbreviations may or may not be present in this report.
α	Listed under the "D" column to designate that the result is reported on a dry weight basis
%R	Percent Recovery
CFL	Contains Free Liquid
CNF	Contains No Free Liquid
DER	Duplicate Error Ratio (normalized absolute difference)
Dil Fac	Dilution Factor
DL	Detection Limit (DoD/DOE)
DL, RA, RE, IN	Indicates a Dilution, Re-analysis, Re-extraction, or additional Initial metals/anion analysis of the sample
DLC	Decision Level Concentration (Radiochemistry)
EDL	Estimated Detection Limit (Dioxin)
LOD	Limit of Detection (DoD/DOE)
LOQ	Limit of Quantitation (DoD/DOE)
MDA	Minimum Detectable Activity (Radiochemistry)
MDC	Minimum Detectable Concentration (Radiochemistry)
MDL	Method Detection Limit
ML	Minimum Level (Dioxin)
NC	Not Calculated
ND	Not Detected at the reporting limit (or MDL or EDL if shown)
PQL	Practical Quantitation Limit
QC	Quality Control
RER	Relative Error Ratio (Radiochemistry)
RL	Reporting Limit or Requested Limit (Radiochemistry)
RPD	Relative Percent Difference, a measure of the relative difference between two points
TEF	Toxicity Equivalent Factor (Dioxin)
TEQ	Toxicity Equivalent Quotient (Dioxin)

Method Summary

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-34917-1

Method	Method Description	Protocol	Laboratory
537	Perfluorinated Alkyl Acids (LC/MS)	EPA	TAL SAC

Protocol References:

EPA = US Environmental Protection Agency

Laboratory References:

TAL SAC = TestAmerica Sacramento, 880 Riverside Parkway, West Sacramento, CA 95605, TEL (916)373-5600

FORM II
LCMS SURROGATE RECOVERY

Lab Name: TestAmerica Sacramento

Job No.: 320-34917-1

SDG No.: _____

Matrix: Water

Level: Low

GC Column (1): GeminiC18 3 ID: 3 (mm)

Client Sample ID	Lab Sample ID	PFHxA #	PFDA #
WGNA-010818-RW-034 4	320-34917-1	91	93
WGNA-010818-FRB-03 44	320-34917-2	97	98
WGNA-010818-RW-395 7	320-34917-3	91	104
WGNA-010818-FRB-39 57	320-34917-4	96	98
WGNA-010818-DUP-16	320-34917-5	96	109
WGNA-010818-RW-317 8	320-34917-6	90	102
WGNA-010818-FRB-31 78	320-34917-7	98	103
NAWC-010818-RW-141	320-34917-8	88	96
NAWC-010818-FRB-14 1	320-34917-9	95	99
WGNA-010818-RW-402 4	320-34917-10	71	93
WGNA-010818-FRB-40 24	320-34917-11	98	100
WGNA-010818-RW-484 4	320-34917-12	97	98
WGNA-010818-FRB-48 44	320-34917-13	97	97
WGNA-010818-RW-040 4	320-34917-14	96	100
WGNA-010818-FRB-04 04	320-34917-15	103	103
	MB 320-204304/1-A	86	96
	LLCS 320-204304/2-A	97	103
WGNA-010818-RW-402 4 LMS	320-34917-10 LMS	88	95
WGNA-010818-RW-402 4 LMSD	320-34917-10 LMSD	90	97

PFHxA = 13C2 PFHxA
PFDA = 13C2 PFDA

QC LIMITS
70-130
70-130

Column to be used to flag recovery values

FORM III
LCMS LOW LEVEL CONTROL SAMPLE RECOVERY

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1

SDG No.: _____

Matrix: Water Level: Low Lab File ID: 2018.01.20_537AA_008.d

Lab ID: LLCS 320-204304/2-A Client ID: _____

COMPOUND	SPIKE ADDED (ng/L)	LLCS CONCENTRATION (ng/L)	LLCS % REC	QC LIMITS REC	#
Perfluorooctanesulfonic acid (PFOS)	40.0	39.2 J	98	50-150	
Perfluorooctanoic acid (PFOA)	20.0	20.1	100	50-150	
Perfluorononanoic acid (PFNA)	20.0	19.7 J	98	50-150	
Perfluorohexanesulfonic acid (PFHxS)	30.0	30.9	103	50-150	
Perfluoroheptanoic acid (PFHpA)	10.0	10.4	104	50-150	
Perfluorobutanesulfonic acid (PFBS)	90.0	85.8 J	95	50-150	

Column to be used to flag recovery and RPD values

FORM III
LCMS LOW LEVEL MATRIX SPIKE RECOVERY

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Matrix: Water Level: Low Lab File ID: 2018.01.23537A_009.d
 Lab ID: 320-34917-10 LMS Client ID: WGNA-010818-RW-4024 LMS

COMPOUND	SPIKE ADDED (ng/L)	SAMPLE CONCENTRATION (ng/L)	LMS CONCENTRATION (ng/L)	LMS % REC	QC LIMITS REC	#
Perfluorooctanesulfonic acid (PFOS)	40.2	18 J	58.5	102	50-150	M
Perfluorooctanoic acid (PFOA)	20.1	12 J	31.9	99	50-150	
Perfluorononanoic acid (PFNA)	20.1	20 U	22.9 J	114	50-150	
Perfluorohexanesulfonic acid (PFHxS)	30.1	12 U	36.4	121	50-150	
Perfluoroheptanoic acid (PFHpA)	10.0	3.6 J	14.4	108	50-150	
Perfluorobutanesulfonic acid (PFBS)	90.3	36 U	95.9	106	50-150	

Column to be used to flag recovery and RPD values

FORM III
LCMS LOW LEVEL MATRIX SPIKE DUPLICATE RECOVERY

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Matrix: Water Level: Low Lab File ID: 2018.01.23537A_010.d
 Lab ID: 320-34917-10 LMSD Client ID: WGNA-010818-RW-4024 LMSD

COMPOUND	SPIKE ADDED (ng/L)	LMSD CONCENTRATION (ng/L)	LMSD % REC	% RPD	QC LIMITS		#
					RPD	REC	
Perfluorooctanesulfonic acid (PFOS)	38.8	56.7	101	3	50	50-150	M
Perfluorooctanoic acid (PFOA)	19.4	32.3	105	1	50	50-150	
Perfluorononanoic acid (PFNA)	19.4	21.5 J	111	6	50	50-150	
Perfluorohexanesulfonic acid (PFHxS)	29.1	33.8	116	7	50	50-150	
Perfluoroheptanoic acid (PFHpA)	9.70	13.8	106	4	50	50-150	
Perfluorobutanesulfonic acid (PFBS)	87.3	98.5	113	3	50	50-150	

Column to be used to flag recovery and RPD values

FORM IV
LCMS METHOD BLANK SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Lab File ID: 2018.01.20_537AA_007.d Lab Sample ID: MB 320-204304/1-A
 Matrix: Water Date Extracted: 01/17/2018 10:50
 Instrument ID: A8_N Date Analyzed: 01/20/2018 19:01
 Level: (Low/Med) Low

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES:

CLIENT SAMPLE ID	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED
	LLCS 320-204304/2-A	2018.01.20_537AA_008.d	01/20/2018 19:06
WGNA-010818-RW-0344	320-34917-1	2018.01.20_537AA_009.d	01/20/2018 19:11
WGNA-010818-FRB-0344	320-34917-2	2018.01.20_537AA_010.d	01/20/2018 19:15
WGNA-010818-RW-3957	320-34917-3	2018.01.20_537AA_011.d	01/20/2018 19:20
WGNA-010818-FRB-3957	320-34917-4	2018.01.20_537AA_012.d	01/20/2018 19:25
WGNA-010818-DUP-16	320-34917-5	2018.01.20_537AA_013.d	01/20/2018 19:29
WGNA-010818-RW-3178	320-34917-6	2018.01.20_537AA_014.d	01/20/2018 19:34
WGNA-010818-FRB-3178	320-34917-7	2018.01.20_537AA_015.d	01/20/2018 19:39
NAWC-010818-RW-141	320-34917-8	2018.01.20_537AA_016.d	01/20/2018 19:43
NAWC-010818-FRB-141	320-34917-9	2018.01.23537A_007.d	01/24/2018 05:15
WGNA-010818-RW-4024	320-34917-10	2018.01.23537A_008.d	01/24/2018 05:19
WGNA-010818-RW-4024 LMS	320-34917-10 LMS	2018.01.23537A_009.d	01/24/2018 05:24
WGNA-010818-RW-4024 LMSD	320-34917-10 LMSD	2018.01.23537A_010.d	01/24/2018 05:29
WGNA-010818-FRB-4024	320-34917-11	2018.01.23537A_011.d	01/24/2018 05:33
WGNA-010818-RW-4844	320-34917-12	2018.01.23537A_012.d	01/24/2018 05:38
WGNA-010818-FRB-4844	320-34917-13	2018.01.23537A_013.d	01/24/2018 05:43
WGNA-010818-RW-0404	320-34917-14	2018.01.23537A_014.d	01/24/2018 05:47
WGNA-010818-FRB-0404	320-34917-15	2018.01.23537A_015.d	01/24/2018 05:52

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Client Sample ID: _____ Lab Sample ID: MB 320-204304/1-A
 Matrix: Water Lab File ID: 2018.01.20_537AA_007.d
 Analysis Method: 537 Date Collected: _____
 Extraction Method: 537 Date Extracted: 01/17/2018 10:50
 Sample wt/vol: 250 (mL) Date Analyzed: 01/20/2018 19:01
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 204872 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	8.0	U	20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.0	U	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	86		70-130
STL00996	13C2 PFDA	96		70-130

FORM VIII
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Instrument ID: A8_N Calibration Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3(mm) Calibration End Date: 11/03/2017 14:01
 Calibration ID: 36012

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
INITIAL CALIBRATION MEAN AREA AND MEAN RT	1535518	1.91	3276559	2.15		
UPPER LIMIT	2303277	2.41	4914839	2.65		
LOWER LIMIT	767759	1.41	1638280	1.65		
LAB SAMPLE ID	CLIENT SAMPLE ID					
CCVL 320-192908/11		1586829	1.91	3305852	2.15	
ICV 320-192908/13		1512045	1.90	3433628	2.14	
CCVL 320-204872/1		1654416	1.81	3432875	2.06	
CCV 320-204872/2 CCVIS		1716899	1.81	3708679	2.06	
MB 320-204304/1-A		1804768	1.81	3734647	2.06	
LLCS 320-204304/2-A		1751473	1.81	3675151	2.06	
320-34917-1	WGNA-010818-RW-0344	1728428	1.82	3615761	2.06	
320-34917-2	WGNA-010818-FRB-0344	1775689	1.81	3694502	2.06	
320-34917-3	WGNA-010818-RW-3957	1666710	1.80	3707714	2.05	
320-34917-4	WGNA-010818-FRB-3957	1772939	1.81	3774506	2.06	
320-34917-5	WGNA-010818-DUP-16	1672120	1.80	3625224	2.05	
320-34917-6	WGNA-010818-RW-3178	1689952	1.80	3685668	2.05	
320-34917-7	WGNA-010818-FRB-3178	1703218	1.81	3729940	2.06	
320-34917-8	NAWC-010818-RW-141	1819910	1.80	3905757	2.05	
CCV 320-204872/14 CCVIS		1591448	1.80	3614871	2.05	
CCVL 320-205331/1		1522908	1.81	3142156	2.06	
CCV 320-205331/2 CCVIS		1578125	1.81	3472309	2.06	
320-34917-9	NAWC-010818-FRB-141	1561349	1.81	3372514	2.06	
320-34917-10	WGNA-010818-RW-4024	1713401	1.81	3759831	2.06	
320-34917-10 LMS	WGNA-010818-RW-4024 LMS	1640988	1.81	3643189	2.06	
320-34917-10 LMSD	WGNA-010818-RW-4024 LMSD	1685962	1.80	3866207	2.05	
320-34917-11	WGNA-010818-FRB-4024	1568292	1.81	3544184	2.06	
320-34917-12	WGNA-010818-RW-4844	1654396	1.81	3689900	2.06	
320-34917-13	WGNA-010818-FRB-4844	1557173	1.81	3476391	2.06	
320-34917-14	WGNA-010818-RW-0404	1567961	1.81	3414209	2.06	
320-34917-15	WGNA-010818-FRB-0404	1573488	1.81	3522216	2.06	
CCV 320-205331/13 CCVIS		1485112	1.81	3186147	2.06	

13PFOA = 13C2-PFOA
 PFOS = 13C4 PFOS

Area Limit = 50%-150% of internal standard area
 RT Limit = ± 0.5 minutes of internal standard RT

Column used to flag values outside QC limits

FORM VIII
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Sample No.: CCV 320-204872/2 Date Analyzed: 01/20/2018 18:52
 Instrument ID: A8_N GC Column: GeminiC18 3x100 ID: 3 (mm)
 Lab File ID (Standard): 2018.01.20_537AA_00 Heated Purge: (Y/N) N
 Calibration ID: 36012

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	1716899	1.81	3708679	2.06		
UPPER LIMIT	2403659	2.31	5192151	2.56		
LOWER LIMIT	1201829	1.31	2596075	1.56		
LAB SAMPLE ID	CLIENT SAMPLE ID					
MB 320-204304/1-A		1804768	1.81	3734647	2.06	
LLCS 320-204304/2-A		1751473	1.81	3675151	2.06	
320-34917-1	WGNA-010818-RW-0344	1728428	1.82	3615761	2.06	
320-34917-2	WGNA-010818-FRB-0344	1775689	1.81	3694502	2.06	
320-34917-3	WGNA-010818-RW-3957	1666710	1.80	3707714	2.05	
320-34917-4	WGNA-010818-FRB-3957	1772939	1.81	3774506	2.06	
320-34917-5	WGNA-010818-DUP-16	1672120	1.80	3625224	2.05	
320-34917-6	WGNA-010818-RW-3178	1689952	1.80	3685668	2.05	
320-34917-7	WGNA-010818-FRB-3178	1703218	1.81	3729940	2.06	
320-34917-8	NAWC-010818-RW-141	1819910	1.80	3905757	2.05	

13PFOA = 13C2-PFOA
 PFOS = 13C4 PFOS

Area Limit = 70%-140% of internal standard area
 RT Limit = ± 0.5 minutes of internal standard RT

Column used to flag values outside QC limits

FORM VIII
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Sample No.: CCV 320-204872/14 Date Analyzed: 01/20/2018 19:48
 Instrument ID: A8_N GC Column: GeminiC18 3x100 ID: 3 (mm)
 Lab File ID (Standard): 2018.01.20_537AA_01 Heated Purge: (Y/N) N
 Calibration ID: 36012

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	1591448	1.80	3614871	2.05		
UPPER LIMIT	2228027	2.30	5060819	2.55		
LOWER LIMIT	1114014	1.30	2530410	1.55		
LAB SAMPLE ID	CLIENT SAMPLE ID					
MB 320-204304/1-A		1804768	1.81	3734647	2.06	
LLCS 320-204304/2-A		1751473	1.81	3675151	2.06	
320-34917-1	WGNA-010818-RW-0344	1728428	1.82	3615761	2.06	
320-34917-2	WGNA-010818-FRB-0344	1775689	1.81	3694502	2.06	
320-34917-3	WGNA-010818-RW-3957	1666710	1.80	3707714	2.05	
320-34917-4	WGNA-010818-FRB-3957	1772939	1.81	3774506	2.06	
320-34917-5	WGNA-010818-DUP-16	1672120	1.80	3625224	2.05	
320-34917-6	WGNA-010818-RW-3178	1689952	1.80	3685668	2.05	
320-34917-7	WGNA-010818-FRB-3178	1703218	1.81	3729940	2.06	
320-34917-8	NAWC-010818-RW-141	1819910	1.80	3905757	2.05	

13PFOA = 13C2-PFOA
 PFOS = 13C4 PFOS

Area Limit = 70%-140% of internal standard area
 RT Limit = ± 0.5 minutes of internal standard RT

Column used to flag values outside QC limits

FORM VIII
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Sample No.: CCV 320-205331/2 Date Analyzed: 01/24/2018 05:05
 Instrument ID: A8_N GC Column: GeminiC18 3x100 ID: 3 (mm)
 Lab File ID (Standard): 2018.01.23537A_005. Heated Purge: (Y/N) N
 Calibration ID: 36012

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	1578125	1.81	3472309	2.06		
UPPER LIMIT	2209375	2.31	4861233	2.56		
LOWER LIMIT	1104688	1.31	2430616	1.56		
LAB SAMPLE ID	CLIENT SAMPLE ID					
320-34917-9	NAWC-010818-FRB-141	1561349	1.81	3372514	2.06	
320-34917-10	WGNA-010818-RW-4024	1713401	1.81	3759831	2.06	
320-34917-10 LMS	WGNA-010818-RW-4024 LMS	1640988	1.81	3643189	2.06	
320-34917-10 LMSD	WGNA-010818-RW-4024 LMSD	1685962	1.80	3866207	2.05	
320-34917-11	WGNA-010818-FRB-4024	1568292	1.81	3544184	2.06	
320-34917-12	WGNA-010818-RW-4844	1654396	1.81	3689900	2.06	
320-34917-13	WGNA-010818-FRB-4844	1557173	1.81	3476391	2.06	
320-34917-14	WGNA-010818-RW-0404	1567961	1.81	3414209	2.06	
320-34917-15	WGNA-010818-FRB-0404	1573488	1.81	3522216	2.06	

13PFOA = 13C2-PFOA
 PFOS = 13C4 PFOS

Area Limit = 70%-140% of internal standard area
 RT Limit = ± 0.5 minutes of internal standard RT

Column used to flag values outside QC limits

FORM VIII
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Sample No.: CCV 320-205331/13 Date Analyzed: 01/24/2018 05:57
 Instrument ID: A8_N GC Column: GeminiC18 3x100 ID: 3 (mm)
 Lab File ID (Standard): 2018.01.23537A_016. Heated Purge: (Y/N) N
 Calibration ID: 36012

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	1485112	1.81	3186147	2.06		
UPPER LIMIT	2079157	2.31	4460606	2.56		
LOWER LIMIT	1039578	1.31	2230303	1.56		
LAB SAMPLE ID	CLIENT SAMPLE ID					
320-34917-9	NAWC-010818-FRB-141	1561349	1.81	3372514	2.06	
320-34917-10	WGNA-010818-RW-4024	1713401	1.81	3759831	2.06	
320-34917-10 LMS	WGNA-010818-RW-4024 LMS	1640988	1.81	3643189	2.06	
320-34917-10 LMSD	WGNA-010818-RW-4024 LMSD	1685962	1.80	3866207	2.05	
320-34917-11	WGNA-010818-FRB-4024	1568292	1.81	3544184	2.06	
320-34917-12	WGNA-010818-RW-4844	1654396	1.81	3689900	2.06	
320-34917-13	WGNA-010818-FRB-4844	1557173	1.81	3476391	2.06	
320-34917-14	WGNA-010818-RW-0404	1567961	1.81	3414209	2.06	
320-34917-15	WGNA-010818-FRB-0404	1573488	1.81	3522216	2.06	

13PFOA = 13C2-PFOA

PFOS = 13C4 PFOS

Area Limit = 70%-140% of internal standard area

RT Limit = ± 0.5 minutes of internal standard RT

Column used to flag values outside QC limits

FORM VI
LCMS BY INTERNAL STANDARD - INITIAL CALIBRATION DATA
CURVE EVALUATION

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1 Analy Batch No.: 192908

SDG No.: _____

Instrument ID: A8_N GC Column: GeminiC18 3 ID: 3(mm) Heated Purge: (Y/N) N

Calibration Start Date: 11/03/2017 13:37 Calibration End Date: 11/03/2017 14:01 Calibration ID: 36012

Calibration Files:

LEVEL:	LAB SAMPLE ID:	LAB FILE ID:
Level 1	IC 320-192908/4	2017.11.03_537XICAL_004.d
Level 2	IC 320-192908/5	2017.11.03_537XICAL_005.d
Level 3	IC 320-192908/6	2017.11.03_537XICAL_006.d
Level 4	IC 320-192908/7	2017.11.03_537XICAL_007.d
Level 5	IC 320-192908/8	2017.11.03_537XICAL_008.d
Level 6	IC 320-192908/9	2017.11.03_537XICAL_009.d

ANALYTE	RRF					CURVE TYPE	COEFFICIENT			#	MIN RRF	%RSD	#	MAX %RSD	R ² OR COD	#	MIN R ² OR COD
	LVL 1 LVL 6	LVL 2	LVL 3	LVL 4	LVL 5		B	M1	M2								
Perfluorobutanesulfonic acid (PFBS)	1.0397 0.8468	1.0767	1.0898	0.9577	0.9303	QuaF		1.1193	-0.001498					0.9990			0.9600
Perfluoroheptanoic acid (PFHpA)	0.9433 0.9848	0.9187	0.9551	0.9185	0.9011	Ave		0.9369			3.2		30.0				
Perfluorohexanesulfonic acid (PFHxS)	1.6459 1.6841	1.6355	1.7405	1.6631	1.6755	Ave		1.6741			2.2		30.0				
Perfluorooctanoic acid (PFOA)	0.9757 0.9799	0.8919	0.9000	0.8953	0.9117	Ave		0.9258			4.4		30.0				
Perfluorooctanesulfonic acid (PFOS)	0.8958 0.9902	0.9213	0.9281	0.9268	0.9715	Ave		0.9389			3.7		30.0				
Perfluorononanoic acid (PFNA)	0.6610 0.7042	0.6285	0.6624	0.6810	0.6478	Ave		0.6642			3.9		30.0				
13C2 PFHxA	1.0891 1.1664	1.0526	1.1042	1.1123	1.0772	Ave		1.1003			3.5		30.0				
13C2 PFDA	0.7748 0.8159	0.7295	0.7569	0.7811	0.7330	Ave		0.7652			4.3		30.0				

Note: The M1 coefficient is the same as Ave RRF for an Ave curve type.

FORM VI
LCMS BY INTERNAL STANDARD - INITIAL CALIBRATION DATA
RESPONSE AND CONCENTRATION

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1 Analy Batch No.: 192908

SDG No.: _____

Instrument ID: A8_N GC Column: GeminiC18 3 ID: 3(mm) Heated Purge: (Y/N) N

Calibration Start Date: 11/03/2017 13:37 Calibration End Date: 11/03/2017 14:01 Calibration ID: 36012

Calibration Files:

LEVEL:	LAB SAMPLE ID:	LAB FILE ID:
Level 1	IC 320-192908/4	2017.11.03_537XICAL_004.d
Level 2	IC 320-192908/5	2017.11.03_537XICAL_005.d
Level 3	IC 320-192908/6	2017.11.03_537XICAL_006.d
Level 4	IC 320-192908/7	2017.11.03_537XICAL_007.d
Level 5	IC 320-192908/8	2017.11.03_537XICAL_008.d
Level 6	IC 320-192908/9	2017.11.03_537XICAL_009.d

ANALYTE	IS REF	CURVE TYPE	RESPONSE					CONCENTRATION (NG/ML)				
			LVL 1 LVL 6	LVL 2	LVL 3	LVL 4	LVL 5	LVL 1 LVL 6	LVL 2	LVL 3	LVL 4	LVL 5
Perfluorobutanesulfonic acid (PFBS)	PFOS	QuaF	1076553 16699152	2591121	5461974	10142530	14011858	9.00 180	20.0	45.0	90.0	135
Perfluoroheptanoic acid (PFHpA)	13PF OA	Ave	143455 2810797	331548	736034	1420703	2102676	1.00 20.0	2.22	5.00	10.0	15.0
Perfluorohexanesulfonic acid (PFHxS)	PFOS	Ave	568156 11071993	1312135	2908204	5871843	8413133	3.00 60.0	6.67	15.0	30.0	45.0
Perfluorooctanoic acid (PFOA)	13PF OA	Ave	296934 5597122	644149	1388033	2771271	4257225	2.00 40.0	4.45	10.0	20.0	30.0
Perfluorooctanesulfonic acid (PFOS)	PFOS	Ave	412315 8679676	985487	2067792	4363079	6504279	4.00 80.0	8.89	20.0	40.0	60.0
Perfluorononanoic acid (PFNA)	13PF OA	Ave	201053 4019666	453612	1020851	2106479	3023088	2.00 40.0	4.45	10.0	20.0	30.0
13C2 PFHxA	13PF OA	Ave	1655691 1664260	1708988	1701491	1719911	1675220	10.0 10.0	10.0	10.0	10.0	10.0
13C2 PFDA	13PF OA	Ave	1177922 1164156	1184358	1166275	1207887	1139992	10.0 10.0	10.0	10.0	10.0	10.0

Curve Type Legend:

Ave = Average ISTD
QuaF = Quadratic ISTD forced zero

FORM VI
 LCMS BY INTERNAL STANDARD - INITIAL CALIBRATION DATA
 READBACK PERCENT ERROR

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1 Analy Batch No.: 192908

SDG No.: _____


Instrument ID: A8_N GC Column: GeminiC18 3 ID: 3 (mm) Heated Purge: (Y/N) N


Calibration Start Date: 11/03/2017 13:37 Calibration End Date: 11/03/2017 14:01 Calibration ID: 36012

Calibration Files:

LEVEL:	LAB SAMPLE ID:	LAB FILE ID:
Level 1	IC 320-192908/4	2017.11.03_537XICAL_004.d
Level 2	IC 320-192908/5	2017.11.03_537XICAL_005.d
Level 3	IC 320-192908/6	2017.11.03_537XICAL_006.d
Level 4	IC 320-192908/7	2017.11.03_537XICAL_007.d
Level 5	IC 320-192908/8	2017.11.03_537XICAL_008.d
Level 6	IC 320-192908/9	2017.11.03_537XICAL_009.d

ANALYTE	PERCENT ERROR						PERCENT ERROR LIMIT					
	LVL 1 #	LVL 2 #	LVL 3 #	LVL 4 #	LVL 5 #	LVL 6 #	LVL 1	LVL 2	LVL 3	LVL 4	LVL 5	LVL 6
Perfluorobutanesulfonic acid (PFBS)	-6.0	-1.2	3.9	-3.1	1.9	-0.5	50	30	30	30	30	30
Perfluoroheptanoic acid (PFHpA)	0.7	-1.9	1.9	-2.0	-3.8	5.1	50	30	30	30	30	30
Perfluorohexanesulfonic acid (PFHxS)	-1.7	-2.3	4.0	-0.7	0.1	0.6	50	30	30	30	30	30
Perfluorooctanoic acid (PFOA)	5.4	-3.7	-2.8	-3.3	-1.5	5.8	50	30	30	30	30	30
Perfluorooctanesulfonic acid (PFOS)	-4.6	-1.9	-1.2	-1.3	3.5	5.5	50	30	30	30	30	30
Perfluorononanoic acid (PFNA)	-0.5	-5.4	-0.3	2.5	-2.5	6.0	50	30	30	30	30	30
13C2 PFHxA	-1.0	-4.3	0.4	1.1	-2.1	6.0	30	30	30	30	30	30
13C2 PFDA	1.3	-4.7	-1.1	2.1	-4.2	6.6	30	30	30	30	30	30





FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Lab Sample ID: CCVL 320-192908/11 Calibration Date: 11/03/2017 14:10
 Instrument ID: A8_N Calib Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 11/03/2017 14:01
 Lab File ID: 2017.11.03_537XICAL_011.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		1.109		20.4	20.0	1.9	50.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9369	0.9382		2.23	2.22	0.1	50.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.674	1.688		6.72	6.67	0.8	50.0
Perfluorooctanoic acid (PFOA)	Ave	0.9258	0.8825		4.24	4.45	-4.7	50.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9389	0.9176		8.69	8.89	-2.3	50.0
Perfluorononanoic acid (PFNA)	Ave	0.6642	0.6625		4.43	4.45	-0.2	50.0
13C2 PFHxA	Ave	1.100	1.068		9.70	10.0	-3.0	30.0
13C2 PFDA	Ave	0.7652	0.7460		9.75	10.0	-2.5	30.0

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Lab Sample ID: ICV 320-192908/13 Calibration Date: 11/03/2017 14:20
 Instrument ID: A8_N Calib Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 11/03/2017 14:01
 Lab File ID: 2017.11.03_537XICAL_013.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		0.8310		83.7	100	-16.4	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9369	0.8136		8.68	10.0	-13.2	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.674	1.463		17.5	20.1	-12.6	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9258	0.7995		17.7	20.5	-13.6	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9389	0.8637		18.1	19.7	-8.0	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6642	0.6428		19.5	20.1	-3.2	30.0
13C2 PFHxA	Ave	1.100	1.039		9.44	10.0	-5.6	30.0
13C2 PFDA	Ave	0.7652	0.7391		9.66	10.0	-3.4	30.0

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Lab Sample ID: CCVL 320-204872/1 Calibration Date: 01/20/2018 18:47
 Instrument ID: A8_N Calib Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 11/03/2017 14:01
 Lab File ID: 2018.01.20_537AA_004.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		1.131		20.8	20.0	3.9	50.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.674	1.714		6.83	6.67	2.4	50.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9369	0.9361		2.22	2.22	-0.0	50.0
Perfluorooctanoic acid (PFOA)	Ave	0.9258	0.9051		4.35	4.45	-2.2	50.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9389	0.9446		8.94	8.89	0.6	50.0
Perfluorononanoic acid (PFNA)	Ave	0.6642	0.6563		4.39	4.45	-1.2	50.0
13C2 PFHxA	Ave	1.100	1.083		9.84	10.0	-1.6	30.0
13C2 PFDA	Ave	0.7652	0.7793		10.2	10.0	1.8	30.0

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Lab Sample ID: CCV 320-204872/2 Calibration Date: 01/20/2018 18:52
 Instrument ID: A8_N Calib Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 11/03/2017 14:01
 Lab File ID: 2018.01.20_537AA_005.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		1.037		44.3	45.0	-1.5	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9369	0.9246		4.94	5.00	-1.3	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.674	1.649		14.8	15.0	-1.5	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9258	0.9210		9.96	10.0	-0.5	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9389	0.9230		19.7	20.0	-1.7	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6642	0.6292		9.48	10.0	-5.3	30.0
13C2 PFHxA	Ave	1.100	1.097		9.97	10.0	-0.3	30.0
13C2 PFDA	Ave	0.7652	0.8118		10.6	10.0	6.1	30.0

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Lab Sample ID: CCV 320-204872/14 Calibration Date: 01/20/2018 19:48
 Instrument ID: A8_N Calib Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 11/03/2017 14:01
 Lab File ID: 2018.01.20_537AA_017.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		0.8990		132	135	-2.5	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9369	0.9143		14.6	15.0	-2.4	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.674	1.637		44.0	45.0	-2.2	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9258	0.9376		30.4	30.0	1.3	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9389	0.9669		61.8	60.0	3.0	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6642	0.6706		30.3	30.0	1.0	30.0
13C2 PFHxA	Ave	1.100	1.177		10.7	10.0	7.0	30.0
13C2 PFDA	Ave	0.7652	0.8069		10.5	10.0	5.5	30.0

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Lab Sample ID: CCVL 320-205331/1 Calibration Date: 01/24/2018 05:01
 Instrument ID: A8_N Calib Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 11/03/2017 14:01
 Lab File ID: 2018.01.23537A_004.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		1.196		22.0	20.0	10.0	50.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9369	0.9347		2.22	2.22	-0.2	50.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.674	1.793		7.14	6.67	7.1	50.0
Perfluorooctanoic acid (PFOA)	Ave	0.9258	0.9224		4.43	4.45	-0.4	50.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9389	0.9591		9.08	8.89	2.1	50.0
Perfluorononanoic acid (PFNA)	Ave	0.6642	0.6472		4.33	4.45	-2.6	50.0
13C2 PFHxA	Ave	1.100	1.113		10.1	10.0	1.1	30.0
13C2 PFDA	Ave	0.7652	0.7500		9.80	10.0	-2.0	30.0

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Lab Sample ID: CCV 320-205331/2 Calibration Date: 01/24/2018 05:05
 Instrument ID: A8_N Calib Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 11/03/2017 14:01
 Lab File ID: 2018.01.23537A_005.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		0.9384		139	135	3.0	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9369	0.9563		15.3	15.0	2.1	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.674	1.697		45.6	45.0	1.4	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9258	0.9181		29.8	30.0	-0.8	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9389	0.9568		61.2	60.0	1.9	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6642	0.6405		28.9	30.0	-3.6	30.0
13C2 PFHxA	Ave	1.100	1.167		10.6	10.0	6.1	30.0
13C2 PFDA	Ave	0.7652	0.7591		9.92	10.0	-0.8	30.0

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1
 SDG No.: _____
 Lab Sample ID: CCV 320-205331/13 Calibration Date: 01/24/2018 05:57
 Instrument ID: A8_N Calib Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 11/03/2017 14:01
 Lab File ID: 2018.01.23537A_016.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		1.131		48.6	45.0	8.1	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9369	0.9320		4.97	5.00	-0.5	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.674	1.784		16.0	15.0	6.6	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9258	0.9062		9.80	10.0	-2.1	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9389	0.9221		19.6	20.0	-1.8	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6642	0.6398		9.64	10.0	-3.7	30.0
13C2 PFHxA	Ave	1.100	1.131		10.3	10.0	2.8	30.0
13C2 PFDA	Ave	0.7652	0.7849		10.3	10.0	2.6	30.0

LCMS ANALYSIS RUN LOG

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1

SDG No.: _____

Instrument ID: A8_N Start Date: 11/03/2017 13:37

Analysis Batch Number: 192908 End Date: 11/03/2017 14:24

LAB SAMPLE ID	CLIENT SAMPLE ID	DATE ANALYZED	DILUTION FACTOR	LAB FILE ID	COLUMN ID
IC 320-192908/4		11/03/2017 13:37	1	2017.11.03_537X ICAL 004.d	GeminiC18 3x100 3(mm)
IC 320-192908/5		11/03/2017 13:42	1	2017.11.03_537X ICAL 005.d	GeminiC18 3x100 3(mm)
IC 320-192908/6		11/03/2017 13:47	1	2017.11.03_537X ICAL 006.d	GeminiC18 3x100 3(mm)
IC 320-192908/7 ICISAV		11/03/2017 13:52	1	2017.11.03_537X ICAL 007.d	GeminiC18 3x100 3(mm)
IC 320-192908/8		11/03/2017 13:56	1	2017.11.03_537X ICAL 008.d	GeminiC18 3x100 3(mm)
IC 320-192908/9		11/03/2017 14:01	1	2017.11.03_537X ICAL 009.d	GeminiC18 3x100 3(mm)
ZZZZZ		11/03/2017 14:06	1		GeminiC18 3x100 3(mm)
CCVL 320-192908/11		11/03/2017 14:10	1	2017.11.03_537X ICAL 011.d	GeminiC18 3x100 3(mm)
ZZZZZ		11/03/2017 14:15	1		GeminiC18 3x100 3(mm)
ICV 320-192908/13		11/03/2017 14:20	1	2017.11.03_537X ICAL 013.d	GeminiC18 3x100 3(mm)
ZZZZZ		11/03/2017 14:24	1		GeminiC18 3x100 3(mm)

LCMS ANALYSIS RUN LOG

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1

SDG No.: _____

Instrument ID: A8_N Start Date: 01/20/2018 18:47

Analysis Batch Number: 204872 End Date: 01/20/2018 19:48

LAB SAMPLE ID	CLIENT SAMPLE ID	DATE ANALYZED	DILUTION FACTOR	LAB FILE ID	COLUMN ID
CCVL 320-204872/1		01/20/2018 18:47	1	2018.01.20_537A A 004.d	GeminiC18 3x100 3(mm)
CCV 320-204872/2 CCVIS		01/20/2018 18:52	1	2018.01.20_537A A 005.d	GeminiC18 3x100 3(mm)
MB 320-204304/1-A		01/20/2018 19:01	1	2018.01.20_537A A 007.d	GeminiC18 3x100 3(mm)
LLCS 320-204304/2-A		01/20/2018 19:06	1	2018.01.20_537A A 008.d	GeminiC18 3x100 3(mm)
320-34917-1		01/20/2018 19:11	1	2018.01.20_537A A 009.d	GeminiC18 3x100 3(mm)
320-34917-2		01/20/2018 19:15	1	2018.01.20_537A A 010.d	GeminiC18 3x100 3(mm)
320-34917-3		01/20/2018 19:20	1	2018.01.20_537A A 011.d	GeminiC18 3x100 3(mm)
320-34917-4		01/20/2018 19:25	1	2018.01.20_537A A 012.d	GeminiC18 3x100 3(mm)
320-34917-5		01/20/2018 19:29	1	2018.01.20_537A A 013.d	GeminiC18 3x100 3(mm)
320-34917-6		01/20/2018 19:34	1	2018.01.20_537A A 014.d	GeminiC18 3x100 3(mm)
320-34917-7		01/20/2018 19:39	1	2018.01.20_537A A 015.d	GeminiC18 3x100 3(mm)
320-34917-8		01/20/2018 19:43	1	2018.01.20_537A A 016.d	GeminiC18 3x100 3(mm)
CCV 320-204872/14 CCVIS		01/20/2018 19:48	1	2018.01.20_537A A 017.d	GeminiC18 3x100 3(mm)

LCMS ANALYSIS RUN LOG

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1

SDG No.: _____

Instrument ID: A8_N Start Date: 01/24/2018 05:01

Analysis Batch Number: 205331 End Date: 01/24/2018 05:57

LAB SAMPLE ID	CLIENT SAMPLE ID	DATE ANALYZED	DILUTION FACTOR	LAB FILE ID	COLUMN ID
CCVL 320-205331/1		01/24/2018 05:01	1	2018.01.23537A_004.d	GeminiC18 3x100 3(mm)
CCV 320-205331/2 CCVIS		01/24/2018 05:05	1	2018.01.23537A_005.d	GeminiC18 3x100 3(mm)
320-34917-9		01/24/2018 05:15	1	2018.01.23537A_007.d	GeminiC18 3x100 3(mm)
320-34917-10		01/24/2018 05:19	1	2018.01.23537A_008.d	GeminiC18 3x100 3(mm)
320-34917-10 LMS		01/24/2018 05:24	1	2018.01.23537A_009.d	GeminiC18 3x100 3(mm)
320-34917-10 LMSD		01/24/2018 05:29	1	2018.01.23537A_010.d	GeminiC18 3x100 3(mm)
320-34917-11		01/24/2018 05:33	1	2018.01.23537A_011.d	GeminiC18 3x100 3(mm)
320-34917-12		01/24/2018 05:38	1	2018.01.23537A_012.d	GeminiC18 3x100 3(mm)
320-34917-13		01/24/2018 05:43	1	2018.01.23537A_013.d	GeminiC18 3x100 3(mm)
320-34917-14		01/24/2018 05:47	1	2018.01.23537A_014.d	GeminiC18 3x100 3(mm)
320-34917-15		01/24/2018 05:52	1	2018.01.23537A_015.d	GeminiC18 3x100 3(mm)
CCV 320-205331/13 CCVIS		01/24/2018 05:57	1	2018.01.23537A_016.d	GeminiC18 3x100 3(mm)

LCMS BATCH WORKSHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1

SDG No.: _____

Batch Number: 204304 Batch Start Date: 01/17/18 10:49 Batch Analyst: Kouchari, Shamiran

Batch Method: 537 Batch End Date: 01/18/18 18:46

Lab Sample ID	Client Sample ID	Method Chain	Basis	GrossWeight	TareWeight	InitialAmount	FinalAmount	ReceivedpH	LC537-IS 00056
MB 320-204304/1		537, 537				250 mL	1.00 mL	7 SU	100 uL
LLCS 320-204304/2		537, 537				250 mL	1.00 mL	7 SU	100 uL
320-34917-A-1	WGNA-010818-RW-0344	537, 537	T	276.13 g	27.43 g	248.7 mL	1.00 mL	7 SU	100 uL
320-34917-A-2	WGNA-010818-FRB-0344	537, 537	T	280.44 g	27.20 g	253.2 mL	1.00 mL	7 SU	100 uL
320-34917-A-3	WGNA-010818-RW-3957	537, 537	T	285.26 g	27.84 g	257.4 mL	1.00 mL	7 SU	100 uL
320-34917-A-4	WGNA-010818-FRB-3957	537, 537	T	283.33 g	27.28 g	256.1 mL	1.00 mL	7 SU	100 uL
320-34917-A-5	WGNA-010818-DUP-16	537, 537	T	290.10 g	27.65 g	262.5 mL	1.00 mL	7 SU	100 uL
320-34917-A-6	WGNA-010818-RW-3178	537, 537	T	267.18 g	27.96 g	239.2 mL	1.00 mL	7 SU	100 uL
320-34917-A-7	WGNA-010818-FRB-3178	537, 537	T	284.45 g	27.74 g	256.7 mL	1.00 mL	7 SU	100 uL
320-34917-A-8	NAWC-010818-RW-141	537, 537	T	284.94 g	27.43 g	257.5 mL	1.00 mL	7 SU	100 uL
320-34917-A-9	NAWC-010818-FRB-141	537, 537	T	293.45 g	27.32 g	266.1 mL	1.00 mL	7 SU	100 uL
320-34917-A-10	WGNA-010818-RW-4024	537, 537	T	278.90 g	27.73 g	251.2 mL	1.00 mL	7 SU	100 uL
320-34917-A-10 LMS	WGNA-010818-RW-4024	537, 537	T	276.69 g	27.64 g	249.1 mL	1.00 mL	7 SU	100 uL
320-34917-A-10 LMSD	WGNA-010818-RW-4024	537, 537	T	285.36 g	27.65 g	257.7 mL	1.00 mL	7 SU	100 uL
320-34917-A-11	WGNA-010818-FRB-4024	537, 537	T	284.88 g	27.53 g	257.4 mL	1.00 mL	7 SU	100 uL
320-34917-A-12	WGNA-010818-RW-4844	537, 537	T	281.28 g	27.81 g	253.5 mL	1.00 mL	7 SU	100 uL
320-34917-A-13	WGNA-010818-FRB-4844	537, 537	T	276.54 g	27.04 g	249.5 mL	1.00 mL	7 SU	100 uL
320-34917-A-14	WGNA-010818-RW-0404	537, 537	T	276.80 g	27.41 g	249.4 mL	1.00 mL	7 SU	100 uL
320-34917-A-15	WGNA-010818-FRB-0404	537, 537	T	279.74 g	27.27 g	252.5 mL	1.00 mL	7 SU	100 uL

Lab Sample ID	Client Sample ID	Method Chain	Basis	LC537-LSP 00025	LC537-SU 00054	AnalysisComment			
MB 320-204304/1		537, 537			100 uL	ch nd			

The pound sign (#) in the amount added field denotes that the reagent was used undiluted. All calculations are performed using the stated concentration for this reagent.

LCMS BATCH WORKSHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1

SDG No.: _____

Batch Number: 204304 Batch Start Date: 01/17/18 10:49 Batch Analyst: Kouchari, Shamiran

Batch Method: 537 Batch End Date: 01/18/18 18:46

Lab Sample ID	Client Sample ID	Method Chain	Basis	LC537-LSP 00025	LC537-SU 00054	AnalysisComment			
LLCS 320-204304/2		537, 537		100 uL	100 uL	ch nd			
320-34917-A-1	WGNA-010818-RW-0344	537, 537	T		100 uL	ch nd			
320-34917-A-2	WGNA-010818-FRB-0344	537, 537	T		100 uL	ch nd			
320-34917-A-3	WGNA-010818-RW-3957	537, 537	T		100 uL	ch nd			
320-34917-A-4	WGNA-010818-FRB-3957	537, 537	T		100 uL	ch nd			
320-34917-A-5	WGNA-010818-DUP-16	537, 537	T		100 uL	ch nd			
320-34917-A-6	WGNA-010818-RW-3178	537, 537	T		100 uL	ch nd			
320-34917-A-7	WGNA-010818-FRB-3178	537, 537	T		100 uL	ch nd			
320-34917-A-8	NAWC-010818-RW-141	537, 537	T		100 uL	ch nd			
320-34917-A-9	NAWC-010818-FRB-141	537, 537	T		100 uL	ch nd			
320-34917-A-10	WGNA-010818-RW-4024	537, 537	T		100 uL	ch nd			
320-34917-A-10 LMS	WGNA-010818-RW-4024	537, 537	T	100 uL	100 uL	ch nd			
320-34917-A-10 LMSD	WGNA-010818-RW-4024	537, 537	T	100 uL	100 uL	ch nd			
320-34917-A-11	WGNA-010818-FRB-4024	537, 537	T		100 uL	ch nd			
320-34917-A-12	WGNA-010818-RW-4844	537, 537	T		100 uL	ch nd			
320-34917-A-13	WGNA-010818-FRB-4844	537, 537	T		100 uL	ch nd			
320-34917-A-14	WGNA-010818-RW-0404	537, 537	T		100 uL	ch nd			
320-34917-A-15	WGNA-010818-FRB-0404	537, 537	T		100 uL	ch nd			

The pound sign (#) in the amount added field denotes that the reagent was used undiluted. All calculations are performed using the stated concentration for this reagent.

LCMS BATCH WORKSHEET

Lab Name: TestAmerica Sacramento Job No.: 320-34917-1

SDG No.: _____

Batch Number: 204304 Batch Start Date: 01/17/18 10:49 Batch Analyst: Kouchari, Shamiran

Batch Method: 537 Batch End Date: 01/18/18 18:46

Batch Notes	
Analyst ID - Aliquot Step	KMK
Batch Comment	Label ID's checked: SKD 1-17-18
Analyst ID - Concentration	CCB
Analyst ID - Final Volume Step	KMK
Internal Standard ID#	1099356
Manifold ID	3,1
Methanol ID	1123833
pH Indicator ID	1617
Pipette ID	M16387D
Analyst ID - IS Reagent Drop	JER
Analyst ID - IS Reagent Drop Witness	KMK
Analyst ID - SU Reagent Drop	CCB
Analyst ID - SU Reagent Drop Witness	HJA
Analyst ID - TA Reagent Drop	CCB
Analyst ID - TA Reagent Drop Witness	HJA
SPE Cartridge ID	6357081-11
Trizma ID	SLBR4303V
Reagent Water ID	1-11-18

Basis	Basis Description
T	Total/NA

The pound sign (#) in the amount added field denotes that the reagent was used undiluted. All calculations are performed using the stated concentration for this reagent.

55

Aqueous Extraction Analysis Sheet

A8 1/22/18

(To Accompany Samples to Instruments)

Batch Number: 320-204506











Analyst: Kolstad, Kate M

Batch Open: 1/18/2018 12:21:00PM

Method Code: 320-537_Prep-320

Batch End: 1/19/2018 4:56:00PM

Extraction of Perfluorinated Alkyl Acids

Input Sample Lab ID (Analytical Method)	SDG (Job #)	GrossWt TareWt	InitAmnt FinAmnt	Rcvd	PHs Adj1	Adj2	Due Date	Analytical TAT	Div Rank	Comments	Output Sample Lab ID
1 MB-320-204506/1 N/A	N/A		250.0 mL	7			N/A	N/A	N/A	CI ND	
			1.0 mL								
2 LCS-320-204506/2 N/A	N/A		250.0 mL	7			N/A	N/A	N/A	CI ND	
			1.0 mL								
3 LCSD-320-204506/3 N/A	N/A		250.0 mL	7			N/A	N/A	N/A	CI ND	
			1.0 mL								
4 320-34946-A-1 (537_DOD5)	N/A (320-34946-1)	278.90 g	251.3 mL	7			1/14/18	16_Days	4	CI ND	
		27.62 g	1.0 mL								
5 320-34946-A-2 (537_DOD5)	N/A (320-34946-1)	273.25 g	245.8 mL	7			1/14/18	16_Days	4	CI ND	
		27.44 g	1.0 mL								
6 320-34946-A-3 (537_DOD5)	N/A (320-34946-1)	272.94 g	245.5 mL	7			1/14/18	16_Days	4	CI ND	
		27.49 g	1.0 mL								
7 320-34946-A-4 (537_DOD5)	N/A (320-34946-1)	275.56 g	247.8 mL	7			1/14/18	16_Days	4	CI ND	
		27.80 g	1.0 mL								
8 320-34946-A-5 (537_DOD5)	N/A (320-34946-1)	275.23 g	248.2 mL	7			1/14/18	16_Days	4	CI ND	
		27.08 g	1.0 mL								
9 320-34946-A-6 (537_DOD5)	N/A (320-34946-1)	274.51 g	246.8 mL	7			1/14/18	16_Days	4	CI ND	
		27.73 g	1.0 mL								
10 320-34946-A-7 (537_DOD5)	N/A (320-34946-1)	270.99 g	243.5 mL	7			1/14/18	16_Days	4	CI ND	
		27.46 g	1.0 mL								

R1

Page 313 of 329



Aqueous Extraction Analysis Sheet

(To Accompany Samples to Instruments)













Batch Number: 320-204506

Analyst: Kolstad, Kate M

Batch Open: 1/18/2018 12:21:00PM

Method Code: 320-537_Prep-320

Batch End: 1/19/2018 4:56:00PM

11	320-34946-A-8 (537_DOD5)	N/A (320-34946-1)	273.10 g 27.47 g	245.6 mL 1.0 mL	7		1/14/18	16_Days	4	CI ND	
12	320-34946-A-9 (537_DOD5)	N/A (320-34946-1)	276.66 g 27.47 g	249.2 mL 1.0 mL	7		1/14/18	16_Days	4	CI ND	
13	320-34946-A-10 (537_DOD5)	N/A (320-34946-1)	268.45 g 28.37 g	240.1 mL 1.0 mL	7		1/14/18	16_Days	4	CI ND	
14	320-34946-A-11 (537_DOD5)	N/A (320-34946-1)	272.57 g 27.35 g	245.2 mL 1.0 mL	7		1/14/18	16_Days	4	CI ND	
15	320-34946-A-12 (537_DOD5)	N/A (320-34946-1)	274.45 g 27.67 g	246.8 mL 1.0 mL	7		1/14/18	16_Days	4	CI ND	
16	320-34946-A-13 (537_DOD5)	N/A (320-34946-1)	277.01 g 27.05 g	250 mL 1.0 mL	7		1/14/18	16_Days	4	CI ND	
17	320-34946-A-14 (537_DOD5)	N/A (320-34946-1)	275.28 g 27.45 g	247.8 mL 1.0 mL	7		1/14/18	16_Days	4	CI ND	
18	320-34946-A-15 (537_DOD5)	N/A (320-34946-1)	272.12 g 27.21 g	244.9 mL 1.0 mL	7		1/14/18	16_Days	4	CI ND	
19	320-34946-A-16 (537_DOD5)	N/A (320-34946-1)	271.46 g 27.49 g	244 mL 1.0 mL	7		1/14/18	16_Days	4	CI ND	
20	320-34946-A-17 (537_DOD5)	N/A (320-34946-1)	274.27 g 27.72 g	246.6 mL 1.0 mL	7		1/14/18	16_Days	4	CI ND	
21	320-34946-A-18 (537_DOD5)	N/A (320-34946-1)	267.71 g 27.75 g	240 mL 1.0 mL	7		1/14/18	16_Days	4	CI ND	
22	320-34946-A-19 (537_DOD5)	N/A (320-34946-1)	274.62 g 27.21 g	247.4 mL 1.0 mL	7		1/14/18	16_Days	4	CI ND	

Page 314 of 329

Aqueous Extraction Analysis Sheet

(To Accompany Samples to Instruments)

Batch Number: 320-204506

Analyst: Kolstad, Kate M

Batch Open: 1/18/2018 12:21:00PM

Method Code: 320-537_Prep-320

Batch End: 1/19/2018 4:56:00PM

Batch Notes

Manifold ID 3, 4

pH Indicator ID 2517

Trizma ID SLBR4303V

SPE Cartridge ID 6357081-11

Methanol ID 1127832

Reagent Water ID 1-11-18

Internal Standard ID# 1099356

Pipette ID M16387D

Analyst ID - TA Reagent Drop CCB

Analyst ID - TA Reagent Drop KMK
Witness

Analyst ID - SU Reagent Drop CCB

Analyst ID - SU Reagent Drop KMK
Witness

Analyst ID - IS Reagent Drop JER

Analyst ID - IS Reagent Drop KMK
Witness

Analyst ID - Concentration CCB/KMK

Analyst ID - Aliquot Step KMK

Analyst ID - Final Volume Step KMK

Batch Comment Label ID's checked: KMK 1-18-18

Page 315 of 329

54

Aqueous Extraction Analysis Sheet

(To Accompany Samples to Instruments)

Analyst: Kouchari, Shamiran

AS 1/20/18
AS 1/22/18
AS 1/23/18

Batch Number: 320-204304

Method Code: 320-537_Prep-320

Batch Open: 1/17/2018 10:49:00AM

Batch End: 1/18/2018 6:46:00PM

Extraction of Perfluorinated Alkyl Acids

Input Sample Lab ID (Analytical Method)	SDG (Job #)	GrossWt TareWt	InitAmnt FinAmnt	Rcvd	PHs Adj1	Adj2	Due Date	Analytical TAT	Div Rank	Comments	Output Sample Lab ID
1 MB-320-204304/1 N/A	N/A		250 mL	7			N/A	N/A	N/A	ch nd	
			1.00 mL								
2 LLCS-320-204304/2 N/A	N/A		250 mL	7			N/A	N/A	N/A	ch nd	
			1.00 mL								
3 320-34917-A-1 (537_DOD5)	N/A (320-34917-1)	276.13 g	248.7 mL	7			1/13/18	16_Days	4	ch nd	
		27.43 g	1.00 mL								
320-34917-A-2 (537_DOD5)	N/A (320-34917-1)	280.44 g	253.2 mL	7			1/13/18	16_Days	4	ch nd	
		27.20 g	1.00 mL								
320-34917-A-3 (537_DOD5)	N/A (320-34917-1)	285.26 g	257.4 mL	7			1/13/18	16_Days	4	ch nd	
		27.84 g	1.00 mL								
6 320-34917-A-4 (537_DOD5)	N/A (320-34917-1)	283.33 g	256.1 mL	7			1/13/18	16_Days	4	ch nd	
		27.28 g	1.00 mL								
7 320-34917-A-5 (537_DOD5)	N/A (320-34917-1)	290.10 g	262.5 mL	7			1/13/18	16_Days	4	ch nd	
		27.65 g	1.00 mL								
8 320-34917-A-6 (537_DOD5)	N/A (320-34917-1)	267.18 g	239.2 mL	7			1/13/18	16_Days	4	ch nd	
		27.96 g	1.00 mL								
9 320-34917-A-7 (537_DOD5)	N/A (320-34917-1)	284.45 g	256.7 mL	7			1/13/18	16_Days	4	ch nd	
		27.74 g	1.00 mL								
10 320-34917-A-8 (537_DOD5)	N/A (320-34917-1)	284.94 g	257.5 mL	7			1/13/18	16_Days	4	ch nd	
		27.43 g	1.00 mL								

Aqueous Extraction Analysis Sheet

(To Accompany Samples to Instruments)










Batch Number: 320-204304

Analyst: Kouchari, Shamiran

Batch Open: 1/17/2018 10:49:00AM

Method Code: 320-537_Prep-320

Batch End: 1/18/2018 6:46:00PM

11	320-34917-A-9 (537_DOD5)	N/A (320-34917-1)	293.45 g	266.1 mL	7			1/13/18	16_Days	4	ch nd	R1	
			27.32 g	1.00 mL									
12	320-34917-A-10 (537_DOD5)	N/A (320-34917-1)	278.90 g	251.2 mL	7			1/13/18	16_Days	4	ch nd	R1	
			27.73 g	1.00 mL									
13	320-34917-A-10-LMS (537_DOD5)	N/A (320-34917-1)	276.69 g	249.1 mL	7			1/13/18	16_Days	4	ch nd	R1	
			27.64 g	1.00 mL									
14	320-34917-A-10-LMSD (537_DOD5)	N/A (320-34917-1)	285.36 g	257.7 mL	7			1/13/18	16_Days	4	ch nd	R1	
			27.65 g	1.00 mL									
15	320-34917-A-11 (537_DOD5)	N/A (320-34917-1)	284.88 g	257.4 mL	7			1/13/18	16_Days	4	ch nd	R1	
			27.53 g	1.00 mL									
16	320-34917-A-12 (537_DOD5)	N/A (320-34917-1)	281.28 g	253.5 mL	7			1/13/18	16_Days	4	ch nd		
			27.81 g	1.00 mL									
17	320-34917-A-13 (537_DOD5)	N/A (320-34917-1)	276.54 g	249.5 mL	7			1/13/18	16_Days	4	ch nd		
			27.04 g	1.00 mL									
18	320-34917-A-14 (537_DOD5)	N/A (320-34917-1)	276.80 g	249.4 mL	7			1/13/18	16_Days	4	ch nd		
			27.41 g	1.00 mL									
19	320-34917-A-15 (537_DOD5)	N/A (320-34917-1)	279.74 g	252.5 mL	7			1/13/18	16_Days	4	ch nd		
			27.27 g	1.00 mL									

Page 321 of 329

Aqueous Extraction Analysis Sheet

(To Accompany Samples to Instruments)

Batch Number: 320-204304

Analyst: Kouchari, Shamiran

Batch Open: 1/17/2018 10:49:00AM

Method Code: 320-537_Prep-320

Batch End: 1/18/2018 6:46:00PM

Batch Notes

Manifold ID 3,1

pH Indicator ID 1617

Trizma ID SLBR4303V

SPE Cartridge ID 6357081-11

Methanol ID 1123833

Reagent Water ID 1-11-18

Internal Standard ID# 1099356

Pipette ID M16387D

Analyst ID - TA Reagent Drop CCB

Analyst ID - TA Reagent Drop HJA

Witness

Analyst ID - SU Reagent Drop CCB

Analyst ID - SU Reagent Drop HJA

Witness

Analyst ID - IS Reagent Drop JER

Analyst ID - IS Reagent Drop KMK

Witness

Analyst ID - Concentration CCB

Analyst ID - Aliquot Step KMK

Analyst ID - Final Volume Step KMK

Batch Comment Label ID's checked: SKD 1-17-18

Page 322 of 329

PFAS Calibration Calculations:

Initial Calibration 11/3/2017
 Instrument A8_N

PFOS

Analyte Concentration	Analyte Response	Internal Standard Response	Internal Standard Amount	RRF	Reported RRF
4	412315	3298877	28.7	0.89678	0.8958
8.89	985487	3450592	28.7	0.92201	0.9213
20	2067792	3194016	28.7	0.92901	0.9281
40	4363079	3374600	28.7	0.92767	0.9268
60	6504279	3199479	28.7	0.97241	0.9715
80	8679676	3141787	28.7	0.99110	0.9902
Average				0.93983	0.9389
Standard Deviation				0.0350	
RSD				0.0372	
%RSD				3.72448	3.7

Continuing Calibration 01/20/2018 @ 18:47
 Instrument A8_N

PFOS

Analyte Concentration	Analyte Response	Internal Standard Response	Internal Standard Amount	RRF	%D	Reported RRF	Reported %D
8.89	1005302	3432875	28.7	0.9454	0.693017	0.9446	0.6

Willow Grove
SDG 320-34917-1

Sample Identification

WGNA-010818-RW-0344

Compound

PFOS

Compound Area

941358

Internal Standard Amount (ng)

28.7

Dilution Factor

1

Internal Standard Area

3615761

Average RRF

0.9389

Sample Volume(L)

0.2487

Volume Extract (ml)

1


Injection Volume (µl)

1

Concentration


31.9994 ug/L

C:\AI\Projects\112008005\WE04\F.S.DR.03\NAWC_201901.mxd MKB 1/24/2019

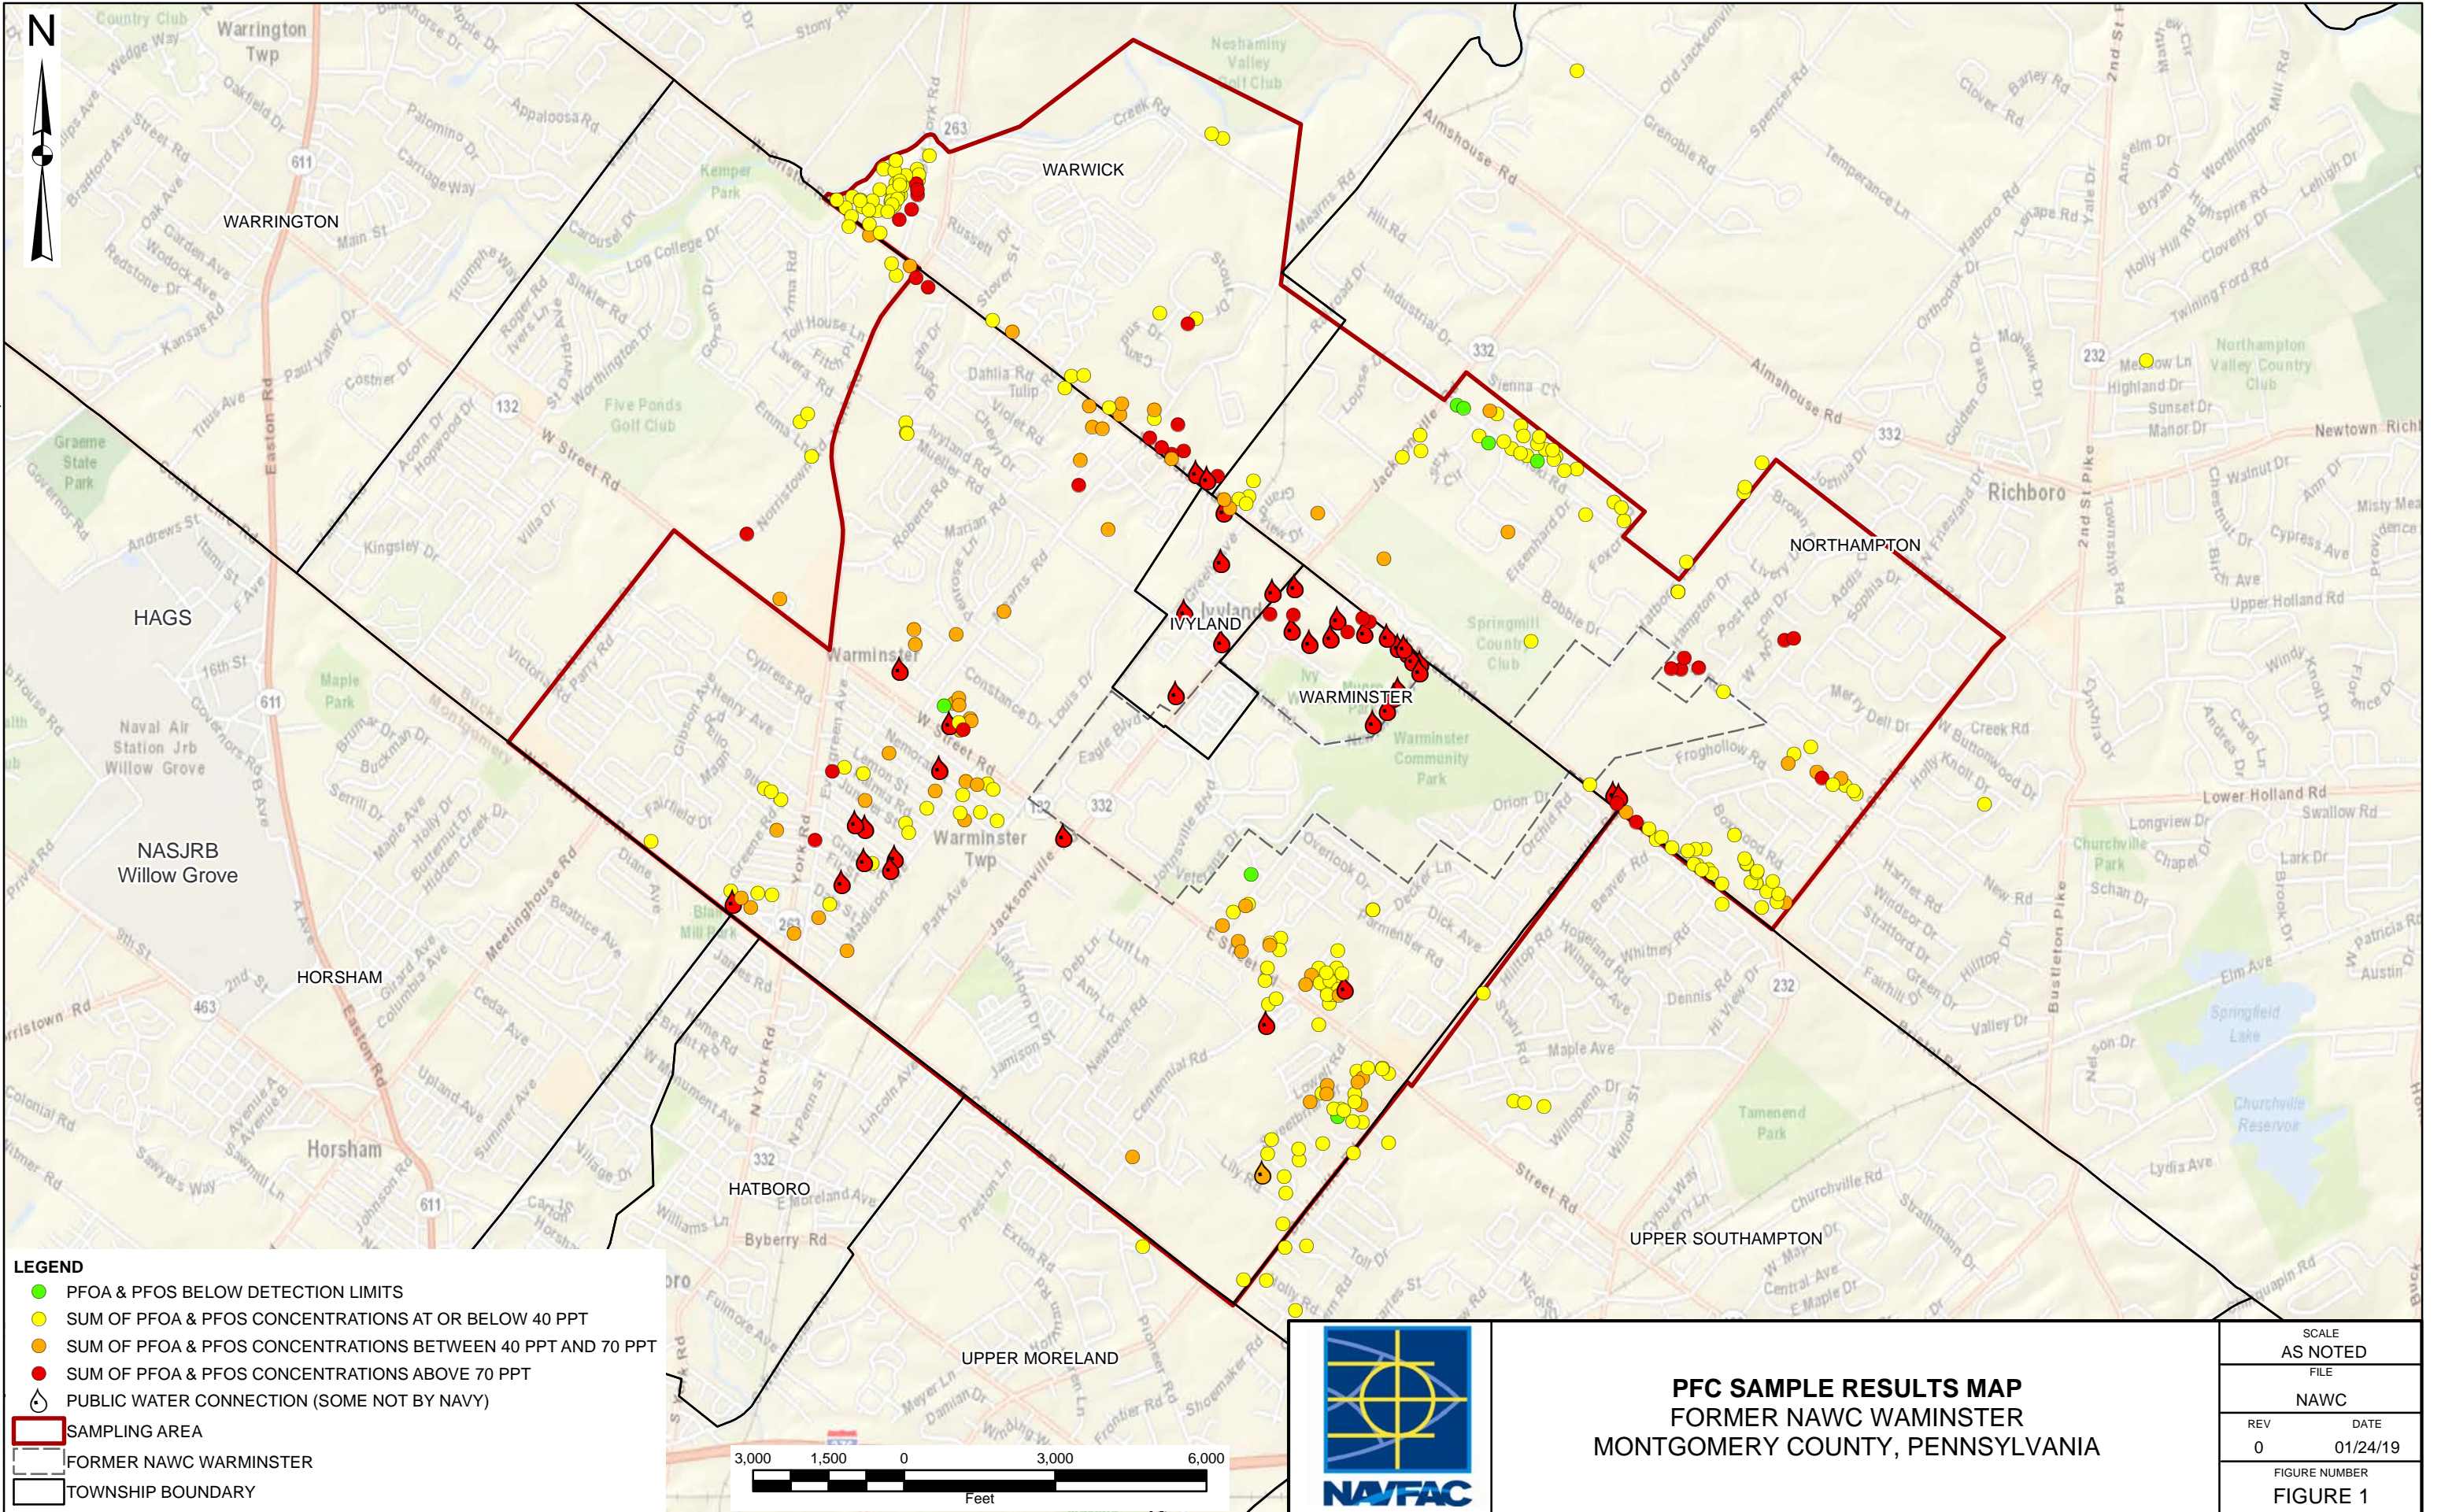

LEGEND

- PFOA & PFOS BELOW DETECTION LIMITS
- SUM OF PFOA & PFOS CONCENTRATIONS AT OR BELOW 40 PPT
- SUM OF PFOA & PFOS CONCENTRATIONS BETWEEN 40 PPT AND 70 PPT
- SUM OF PFOA & PFOS CONCENTRATIONS ABOVE 70 PPT
- 💧 PUBLIC WATER CONNECTION (SOME NOT BY NAVY)
- SAMPLING AREA
- FORMER NAWC WARRINSTER
- TOWNSHIP BOUNDARY



PFC SAMPLE RESULTS MAP
 FORMER NAWC WARRINSTER
 MONTGOMERY COUNTY, PENNSYLVANIA

SCALE AS NOTED	
FILE	
NAWC	
REV 0	DATE 01/24/19
FIGURE NUMBER	
FIGURE 1	