



**Off-Base Drinking Water Sample Results,
Combined Level 2 and Level 4 Laboratory Report,
Electronic Data Deliverable, Data Validation Report,
and the Sample Location Figure, SDG 320-35046-1**

*Naval Air Warfare Center Warminster
Warminster, Pennsylvania*

August 2019

N62269_001133
WARMINSTER_NAWC
SSIC 5000-33c

**LABORATORY DATA PACKAGE, 320-35046-1, NAS WILLOW GROVE NAWC
WARMINSTER PA**
02/02/2018
TESTAMERICA LABORATORIES, INC

Approved for public release: distribution unlimited.

ANALYTICAL REPORT

Job Number: 320-35046-1

Job Description: Warminster: PFAS, NAS JRB Willow Grove

For:
Tetra Tech, Inc.
234 Mall Boulevard
Suite 260
King of Prussia, PA 19406
Attention: Andy Frebowitz



Approved for release.
David R. Alltucker
Project Manager I
2/2/2018 12:32 PM

David R Alltucker, Project Manager I
880 Riverside Parkway, West Sacramento, CA, 95605
(916)374-4383
david.alltucker@testamericainc.com
02/02/2018

Table of Contents

Cover Title Page	1
Data Summaries	4
Definitions	4
Case Narrative	5
Detection Summary	6
Client Sample Results	9
Default Detection Limits	16
Surrogate Summary	17
QC Sample Results	18
QC Association	20
Chronicle	22
Certification Summary	26
Method Summary	27
Sample Summary	28
Manual Integration Summary	29
Reagent Traceability	36
COAs	46
Organic Sample Data	100
LCMS	100
Method 537 DOD	100
Method 537 DOD QC Summary	101
Method 537 DOD Sample Data	114
Standards Data	241
Method 537 DOD ICAL Data	241
Method 537 DOD CCAL Data	280
Raw QC Data	339

Table of Contents

Method 537 DOD Blank Data	339
Method 537 DOD LCS/LCSD Data	344
Method 537 DOD MS/MSD Data	352
Method 537 DOD Run Logs	368
Method 537 DOD Prep Data	373
Shipping and Receiving Documents	389
Client Chain of Custody	390
Sample Receipt Checklist	391

Definitions/Glossary

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-35046-1

Qualifiers

LCMS

Qualifier	Qualifier Description
U	Undetected at the Limit of Detection.
J	Estimated: The analyte was positively identified; the quantitation is an estimation
M	Manual integrated compound.

Glossary

Abbreviation	These commonly used abbreviations may or may not be present in this report.
α	Listed under the "D" column to designate that the result is reported on a dry weight basis
%R	Percent Recovery
CFL	Contains Free Liquid
CNF	Contains No Free Liquid
DER	Duplicate Error Ratio (normalized absolute difference)
Dil Fac	Dilution Factor
DL	Detection Limit (DoD/DOE)
DL, RA, RE, IN	Indicates a Dilution, Re-analysis, Re-extraction, or additional Initial metals/anion analysis of the sample
DLC	Decision Level Concentration (Radiochemistry)
EDL	Estimated Detection Limit (Dioxin)
LOD	Limit of Detection (DoD/DOE)
LOQ	Limit of Quantitation (DoD/DOE)
MDA	Minimum Detectable Activity (Radiochemistry)
MDC	Minimum Detectable Concentration (Radiochemistry)
MDL	Method Detection Limit
ML	Minimum Level (Dioxin)
NC	Not Calculated
ND	Not Detected at the reporting limit (or MDL or EDL if shown)
PQL	Practical Quantitation Limit
QC	Quality Control
RER	Relative Error Ratio (Radiochemistry)
RL	Reporting Limit or Requested Limit (Radiochemistry)
RPD	Relative Percent Difference, a measure of the relative difference between two points
TEF	Toxicity Equivalent Factor (Dioxin)
TEQ	Toxicity Equivalent Quotient (Dioxin)

Job Narrative
320-35046-1

Receipt

The samples were received on 1/12/2018 1:20 PM; the samples arrived in good condition, properly preserved and, where required, on ice. The temperatures of the 2 coolers at receipt time were 3.7° C and 5.1° C.

LCMS

Method(s) 537: The first level standard from the initial calibration curve is used to evaluate the tune criteria. The instrument mass windows are set at +/- 0.5amu; therefore, detection of the analyte serves as verification that the assigned mass is within +/- 0.5amu of the true value, which meets the DoD/DOE QSM tune criterion.

No additional analytical or quality issues were noted, other than those described above or in the Definitions/Glossary page.

Organic Prep

No analytical or quality issues were noted, other than those described in the Definitions/Glossary page.

Detection Summary

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-35046-1

Client Sample ID: WGNA-011118-RW-3103

Lab Sample ID: 320-35046-1

Analyte	Result	Qualifier	LOQ	DL	Unit	Dil Fac	D	Method	Prep Type
Perfluorooctanesulfonic acid (PFOS)	10	J M	35	5.9	ng/L	1		537	Total/NA
Perfluorooctanoic acid (PFOA)	12	J	17	2.4	ng/L	1		537	Total/NA
Perfluorohexanesulfonic acid (PFHxS)	5.2	J	26	4.8	ng/L	1		537	Total/NA
Perfluoroheptanoic acid (PFHpA)	3.4	J	8.7	1.7	ng/L	1		537	Total/NA

Client Sample ID: WGNA-011118-FRB-3103

Lab Sample ID: 320-35046-2

No Detections.

Client Sample ID: WGNA-011118-RW-0683

Lab Sample ID: 320-35046-3

Analyte	Result	Qualifier	LOQ	DL	Unit	Dil Fac	D	Method	Prep Type
Perfluorooctanesulfonic acid (PFOS)	29	J M	38	6.5	ng/L	1		537	Total/NA
Perfluorooctanoic acid (PFOA)	18	J	19	2.7	ng/L	1		537	Total/NA
Perfluorohexanesulfonic acid (PFHxS)	5.8	J	29	5.3	ng/L	1		537	Total/NA
Perfluoroheptanoic acid (PFHpA)	5.2	J	9.6	1.8	ng/L	1		537	Total/NA

Client Sample ID: WGNA-011118-FRB-0683

Lab Sample ID: 320-35046-4

No Detections.

Client Sample ID: NAWC-011118-RW-139

Lab Sample ID: 320-35046-5

Analyte	Result	Qualifier	LOQ	DL	Unit	Dil Fac	D	Method	Prep Type
Perfluorooctanesulfonic acid (PFOS)	12	J M	37	6.3	ng/L	1		537	Total/NA
Perfluorooctanoic acid (PFOA)	16	J	19	2.6	ng/L	1		537	Total/NA
Perfluoroheptanoic acid (PFHpA)	5.4	J	9.3	1.8	ng/L	1		537	Total/NA

Client Sample ID: NAWC-011118-FRB-139

Lab Sample ID: 320-35046-6

No Detections.

Client Sample ID: WGNA-011118-DUP-18

Lab Sample ID: 320-35046-7

Analyte	Result	Qualifier	LOQ	DL	Unit	Dil Fac	D	Method	Prep Type
Perfluorooctanesulfonic acid (PFOS)	12	J M	37	6.3	ng/L	1		537	Total/NA
Perfluorooctanoic acid (PFOA)	15	J	19	2.6	ng/L	1		537	Total/NA
Perfluoroheptanoic acid (PFHpA)	5.2	J	9.3	1.8	ng/L	1		537	Total/NA

Client Sample ID: NAWC-011118-RW-098

Lab Sample ID: 320-35046-8

Analyte	Result	Qualifier	LOQ	DL	Unit	Dil Fac	D	Method	Prep Type
Perfluorooctanesulfonic acid (PFOS)	16	J M	42	7.1	ng/L	1		537	Total/NA
Perfluorooctanoic acid (PFOA)	14	J	21	2.9	ng/L	1		537	Total/NA
Perfluoroheptanoic acid (PFHpA)	3.9	J M	10	2.0	ng/L	1		537	Total/NA

Client Sample ID: NAWC-011118-FRB-098

Lab Sample ID: 320-35046-9

No Detections.

Client Sample ID: NAWC-011118-RW-180

Lab Sample ID: 320-35046-10

This Detection Summary does not include radiochemical test results.

TestAmerica Sacramento

Detection Summary

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-35046-1

Client Sample ID: NAWC-011118-RW-180 (Continued)

Lab Sample ID: 320-35046-10

Analyte	Result	Qualifier	LOQ	DL	Unit	Dil Fac	D	Method	Prep Type
Perfluorooctanesulfonic acid (PFOS)	28	J M	38	6.4	ng/L	1		537	Total/NA
Perfluorooctanoic acid (PFOA)	23		19	2.6	ng/L	1		537	Total/NA
Perfluorohexanesulfonic acid (PFHxS)	11	J	28	5.2	ng/L	1		537	Total/NA
Perfluoroheptanoic acid (PFHpA)	9.1	J	9.4	1.8	ng/L	1		537	Total/NA

Client Sample ID: NAWC-011118-FRB-180

Lab Sample ID: 320-35046-11

No Detections.

Client Sample ID: NAWC-011118-RW-179

Lab Sample ID: 320-35046-12

Analyte	Result	Qualifier	LOQ	DL	Unit	Dil Fac	D	Method	Prep Type
Perfluorooctanesulfonic acid (PFOS)	18	J M	38	6.5	ng/L	1		537	Total/NA
Perfluorooctanoic acid (PFOA)	18	J	19	2.7	ng/L	1		537	Total/NA
Perfluorohexanesulfonic acid (PFHxS)	6.2	J	29	5.3	ng/L	1		537	Total/NA
Perfluoroheptanoic acid (PFHpA)	4.7	J	9.5	1.8	ng/L	1		537	Total/NA

Client Sample ID: NAWC-011118-FRB-179

Lab Sample ID: 320-35046-13

No Detections.

Client Sample ID: NAWC-011118-RW-303

Lab Sample ID: 320-35046-14

Analyte	Result	Qualifier	LOQ	DL	Unit	Dil Fac	D	Method	Prep Type
Perfluorooctanesulfonic acid (PFOS)	21	J M	38	6.5	ng/L	1		537	Total/NA
Perfluorooctanoic acid (PFOA)	20		19	2.7	ng/L	1		537	Total/NA
Perfluorohexanesulfonic acid (PFHxS)	7.3	J	29	5.3	ng/L	1		537	Total/NA
Perfluoroheptanoic acid (PFHpA)	6.0	J	9.6	1.8	ng/L	1		537	Total/NA

Client Sample ID: NAWC-011118-FRB-303

Lab Sample ID: 320-35046-15

No Detections.

Client Sample ID: WGNA-011118-RW-3409

Lab Sample ID: 320-35046-16

Analyte	Result	Qualifier	LOQ	DL	Unit	Dil Fac	D	Method	Prep Type
Perfluorooctanesulfonic acid (PFOS)	20	J M	35	5.9	ng/L	1		537	Total/NA
Perfluorooctanoic acid (PFOA)	14	J	17	2.4	ng/L	1		537	Total/NA
Perfluorohexanesulfonic acid (PFHxS)	7.9	J	26	4.8	ng/L	1		537	Total/NA
Perfluoroheptanoic acid (PFHpA)	5.1	J	8.7	1.6	ng/L	1		537	Total/NA

Client Sample ID: WGNA-011118-FRB-3409

Lab Sample ID: 320-35046-17

No Detections.

Client Sample ID: WGNA-011118-RW-3220

Lab Sample ID: 320-35046-18

Analyte	Result	Qualifier	LOQ	DL	Unit	Dil Fac	D	Method	Prep Type
Perfluorooctanesulfonic acid (PFOS)	38	M	37	6.4	ng/L	1		537	Total/NA
Perfluorooctanoic acid (PFOA)	13	J	19	2.6	ng/L	1		537	Total/NA
Perfluorohexanesulfonic acid (PFHxS)	17	J	28	5.1	ng/L	1		537	Total/NA

This Detection Summary does not include radiochemical test results.

TestAmerica Sacramento

Detection Summary

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-35046-1

Client Sample ID: WGNA-011118-RW-3220 (Continued)

Lab Sample ID: 320-35046-18

Analyte	Result	Qualifier	LOQ	DL	Unit	Dil Fac	D	Method	Prep Type
Perfluoroheptanoic acid (PFHpA)	8.0	J	9.3	1.8	ng/L	1		537	Total/NA
Perfluorobutanesulfonic acid (PFBS)	110		84	15	ng/L	1		537	Total/NA

Client Sample ID: WGNA-011118-FRB-3220

Lab Sample ID: 320-35046-19

No Detections.

This Detection Summary does not include radiochemical test results.

TestAmerica Sacramento

Client Sample Results

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-35046-1

Client Sample ID: WGNA-011118-RW-3103

Lab Sample ID: 320-35046-1

Date Collected: 01/11/18 08:10

Matrix: Water

Date Received: 01/12/18 13:20

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	10	J M	35	5.9	ng/L		01/24/18 20:52	01/31/18 12:12	1
Perfluorooctanoic acid (PFOA)	12	J	17	2.4	ng/L		01/24/18 20:52	01/31/18 12:12	1
Perfluorononanoic acid (PFNA)	17	U	21	7.0	ng/L		01/24/18 20:52	01/31/18 12:12	1
Perfluorohexanesulfonic acid (PFHxS)	5.2	J	26	4.8	ng/L		01/24/18 20:52	01/31/18 12:12	1
Perfluoroheptanoic acid (PFHpA)	3.4	J	8.7	1.7	ng/L		01/24/18 20:52	01/31/18 12:12	1
Perfluorobutanesulfonic acid (PFBS)	31	U	79	14	ng/L		01/24/18 20:52	01/31/18 12:12	1
Surrogate	%Recovery	Qualifier	Limits				Prepared	Analyzed	Dil Fac
13C2 PFHxA	92		70 - 130				01/24/18 20:52	01/31/18 12:12	1
13C2 PFDA	97		70 - 130				01/24/18 20:52	01/31/18 12:12	1

Client Sample ID: WGNA-011118-FRB-3103

Lab Sample ID: 320-35046-2

Date Collected: 01/11/18 08:05

Matrix: Water

Date Received: 01/12/18 13:20

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	15	U	38	6.4	ng/L		01/24/18 20:52	01/31/18 12:16	1
Perfluorooctanoic acid (PFOA)	7.5	U	19	2.6	ng/L		01/24/18 20:52	01/31/18 12:16	1
Perfluorononanoic acid (PFNA)	19	U	23	7.5	ng/L		01/24/18 20:52	01/31/18 12:16	1
Perfluorohexanesulfonic acid (PFHxS)	11	U	28	5.2	ng/L		01/24/18 20:52	01/31/18 12:16	1
Perfluoroheptanoic acid (PFHpA)	3.8	U	9.4	1.8	ng/L		01/24/18 20:52	01/31/18 12:16	1
Perfluorobutanesulfonic acid (PFBS)	34	U	85	15	ng/L		01/24/18 20:52	01/31/18 12:16	1
Surrogate	%Recovery	Qualifier	Limits				Prepared	Analyzed	Dil Fac
13C2 PFHxA	99		70 - 130				01/24/18 20:52	01/31/18 12:16	1
13C2 PFDA	104		70 - 130				01/24/18 20:52	01/31/18 12:16	1

Client Sample ID: WGNA-011118-RW-0683

Lab Sample ID: 320-35046-3

Date Collected: 01/11/18 08:40

Matrix: Water

Date Received: 01/12/18 13:20

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	29	J M	38	6.5	ng/L		01/24/18 20:52	01/31/18 12:21	1
Perfluorooctanoic acid (PFOA)	18	J	19	2.7	ng/L		01/24/18 20:52	01/31/18 12:21	1
Perfluorononanoic acid (PFNA)	19	U	23	7.7	ng/L		01/24/18 20:52	01/31/18 12:21	1
Perfluorohexanesulfonic acid (PFHxS)	5.8	J	29	5.3	ng/L		01/24/18 20:52	01/31/18 12:21	1
Perfluoroheptanoic acid (PFHpA)	5.2	J	9.6	1.8	ng/L		01/24/18 20:52	01/31/18 12:21	1
Perfluorobutanesulfonic acid (PFBS)	34	U	86	15	ng/L		01/24/18 20:52	01/31/18 12:21	1
Surrogate	%Recovery	Qualifier	Limits				Prepared	Analyzed	Dil Fac
13C2 PFHxA	87		70 - 130				01/24/18 20:52	01/31/18 12:21	1
13C2 PFDA	96		70 - 130				01/24/18 20:52	01/31/18 12:21	1

Client Sample Results

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-35046-1

Client Sample ID: WGNA-011118-FRB-0683

Lab Sample ID: 320-35046-4

Date Collected: 01/11/18 08:35

Matrix: Water

Date Received: 01/12/18 13:20

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	15	U	38	6.5	ng/L		01/24/18 20:52	01/31/18 12:26	1
Perfluorooctanoic acid (PFOA)	7.6	U	19	2.7	ng/L		01/24/18 20:52	01/31/18 12:26	1
Perfluorononanoic acid (PFNA)	19	U	23	7.6	ng/L		01/24/18 20:52	01/31/18 12:26	1
Perfluorohexanesulfonic acid (PFHxS)	11	U	29	5.2	ng/L		01/24/18 20:52	01/31/18 12:26	1
Perfluoroheptanoic acid (PFHpA)	3.8	U	9.5	1.8	ng/L		01/24/18 20:52	01/31/18 12:26	1
Perfluorobutanesulfonic acid (PFBS)	34	U	86	15	ng/L		01/24/18 20:52	01/31/18 12:26	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	96		70 - 130	01/24/18 20:52	01/31/18 12:26	1
13C2 PFDA	99		70 - 130	01/24/18 20:52	01/31/18 12:26	1

Client Sample ID: NAWC-011118-RW-139

Lab Sample ID: 320-35046-5

Date Collected: 01/11/18 10:40

Matrix: Water

Date Received: 01/12/18 13:20

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	12	J M	37	6.3	ng/L		01/24/18 20:52	01/31/18 12:30	1
Perfluorooctanoic acid (PFOA)	16	J	19	2.6	ng/L		01/24/18 20:52	01/31/18 12:30	1
Perfluorononanoic acid (PFNA)	19	U	22	7.4	ng/L		01/24/18 20:52	01/31/18 12:30	1
Perfluorohexanesulfonic acid (PFHxS)	11	U	28	5.1	ng/L		01/24/18 20:52	01/31/18 12:30	1
Perfluoroheptanoic acid (PFHpA)	5.4	J	9.3	1.8	ng/L		01/24/18 20:52	01/31/18 12:30	1
Perfluorobutanesulfonic acid (PFBS)	33	U	84	15	ng/L		01/24/18 20:52	01/31/18 12:30	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	92		70 - 130	01/24/18 20:52	01/31/18 12:30	1
13C2 PFDA	97		70 - 130	01/24/18 20:52	01/31/18 12:30	1

Client Sample ID: NAWC-011118-FRB-139

Lab Sample ID: 320-35046-6

Date Collected: 01/11/18 10:35

Matrix: Water

Date Received: 01/12/18 13:20

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	15	U	37	6.2	ng/L		01/24/18 20:52	01/31/18 12:35	1
Perfluorooctanoic acid (PFOA)	7.3	U	18	2.6	ng/L		01/24/18 20:52	01/31/18 12:35	1
Perfluorononanoic acid (PFNA)	18	U	22	7.3	ng/L		01/24/18 20:52	01/31/18 12:35	1
Perfluorohexanesulfonic acid (PFHxS)	11	U	27	5.0	ng/L		01/24/18 20:52	01/31/18 12:35	1
Perfluoroheptanoic acid (PFHpA)	3.7	U	9.2	1.7	ng/L		01/24/18 20:52	01/31/18 12:35	1
Perfluorobutanesulfonic acid (PFBS)	33	U	82	15	ng/L		01/24/18 20:52	01/31/18 12:35	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	90		70 - 130	01/24/18 20:52	01/31/18 12:35	1
13C2 PFDA	96		70 - 130	01/24/18 20:52	01/31/18 12:35	1

Client Sample Results

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-35046-1

Client Sample ID: WGNA-011118-DUP-18

Lab Sample ID: 320-35046-7

Date Collected: 01/11/18 07:00

Matrix: Water

Date Received: 01/12/18 13:20

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	12	J M	37	6.3	ng/L		01/24/18 20:52	01/31/18 12:40	1
Perfluorooctanoic acid (PFOA)	15	J	19	2.6	ng/L		01/24/18 20:52	01/31/18 12:40	1
Perfluorononanoic acid (PFNA)	19	U	22	7.4	ng/L		01/24/18 20:52	01/31/18 12:40	1
Perfluorohexanesulfonic acid (PFHxS)	11	U	28	5.1	ng/L		01/24/18 20:52	01/31/18 12:40	1
Perfluoroheptanoic acid (PFHpA)	5.2	J	9.3	1.8	ng/L		01/24/18 20:52	01/31/18 12:40	1
Perfluorobutanesulfonic acid (PFBS)	33	U	83	15	ng/L		01/24/18 20:52	01/31/18 12:40	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	92		70 - 130	01/24/18 20:52	01/31/18 12:40	1
13C2 PFDA	101		70 - 130	01/24/18 20:52	01/31/18 12:40	1

Client Sample ID: NAWC-011118-RW-098

Lab Sample ID: 320-35046-8

Date Collected: 01/11/18 11:10

Matrix: Water

Date Received: 01/12/18 13:20

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	16	J M	42	7.1	ng/L		01/24/18 20:52	01/31/18 12:44	1
Perfluorooctanoic acid (PFOA)	14	J	21	2.9	ng/L		01/24/18 20:52	01/31/18 12:44	1
Perfluorononanoic acid (PFNA)	21	U M	25	8.3	ng/L		01/24/18 20:52	01/31/18 12:44	1
Perfluorohexanesulfonic acid (PFHxS)	12	U	31	5.7	ng/L		01/24/18 20:52	01/31/18 12:44	1
Perfluoroheptanoic acid (PFHpA)	3.9	J M	10	2.0	ng/L		01/24/18 20:52	01/31/18 12:44	1
Perfluorobutanesulfonic acid (PFBS)	37	U	93	17	ng/L		01/24/18 20:52	01/31/18 12:44	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	91		70 - 130	01/24/18 20:52	01/31/18 12:44	1
13C2 PFDA	102		70 - 130	01/24/18 20:52	01/31/18 12:44	1

Client Sample ID: NAWC-011118-FRB-098

Lab Sample ID: 320-35046-9

Date Collected: 01/11/18 11:05

Matrix: Water

Date Received: 01/12/18 13:20

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	15	U	37	6.3	ng/L		01/24/18 20:52	01/31/18 12:58	1
Perfluorooctanoic acid (PFOA)	7.4	U	19	2.6	ng/L		01/24/18 20:52	01/31/18 12:58	1
Perfluorononanoic acid (PFNA)	19	U	22	7.4	ng/L		01/24/18 20:52	01/31/18 12:58	1
Perfluorohexanesulfonic acid (PFHxS)	11	U	28	5.1	ng/L		01/24/18 20:52	01/31/18 12:58	1
Perfluoroheptanoic acid (PFHpA)	3.7	U	9.3	1.8	ng/L		01/24/18 20:52	01/31/18 12:58	1
Perfluorobutanesulfonic acid (PFBS)	33	U	83	15	ng/L		01/24/18 20:52	01/31/18 12:58	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	93		70 - 130	01/24/18 20:52	01/31/18 12:58	1
13C2 PFDA	94		70 - 130	01/24/18 20:52	01/31/18 12:58	1

Client Sample Results

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-35046-1

Client Sample ID: NAWC-011118-RW-180

Lab Sample ID: 320-35046-10

Date Collected: 01/11/18 12:10

Matrix: Water

Date Received: 01/12/18 13:20

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	28	J M	38	6.4	ng/L		01/24/18 20:52	01/31/18 13:03	1
Perfluorooctanoic acid (PFOA)	23		19	2.6	ng/L		01/24/18 20:52	01/31/18 13:03	1
Perfluorononanoic acid (PFNA)	19	U	23	7.5	ng/L		01/24/18 20:52	01/31/18 13:03	1
Perfluorohexanesulfonic acid (PFHxS)	11	J	28	5.2	ng/L		01/24/18 20:52	01/31/18 13:03	1
Perfluoroheptanoic acid (PFHpA)	9.1	J	9.4	1.8	ng/L		01/24/18 20:52	01/31/18 13:03	1
Perfluorobutanesulfonic acid (PFBS)	34	U	85	15	ng/L		01/24/18 20:52	01/31/18 13:03	1
Surrogate	%Recovery	Qualifier	Limits				Prepared	Analyzed	Dil Fac
13C2 PFHxA	92		70 - 130				01/24/18 20:52	01/31/18 13:03	1
13C2 PFDA	100		70 - 130				01/24/18 20:52	01/31/18 13:03	1

Client Sample ID: NAWC-011118-FRB-180

Lab Sample ID: 320-35046-11

Date Collected: 01/11/18 12:05

Matrix: Water

Date Received: 01/12/18 13:20

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	15	U	38	6.4	ng/L		01/24/18 20:52	01/31/18 13:08	1
Perfluorooctanoic acid (PFOA)	7.6	U	19	2.6	ng/L		01/24/18 20:52	01/31/18 13:08	1
Perfluorononanoic acid (PFNA)	19	U	23	7.6	ng/L		01/24/18 20:52	01/31/18 13:08	1
Perfluorohexanesulfonic acid (PFHxS)	11	U	28	5.2	ng/L		01/24/18 20:52	01/31/18 13:08	1
Perfluoroheptanoic acid (PFHpA)	3.8	U	9.5	1.8	ng/L		01/24/18 20:52	01/31/18 13:08	1
Perfluorobutanesulfonic acid (PFBS)	34	U	85	15	ng/L		01/24/18 20:52	01/31/18 13:08	1
Surrogate	%Recovery	Qualifier	Limits				Prepared	Analyzed	Dil Fac
13C2 PFHxA	99		70 - 130				01/24/18 20:52	01/31/18 13:08	1
13C2 PFDA	100		70 - 130				01/24/18 20:52	01/31/18 13:08	1

Client Sample ID: NAWC-011118-RW-179

Lab Sample ID: 320-35046-12

Date Collected: 01/11/18 12:40

Matrix: Water

Date Received: 01/12/18 13:20

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	18	J M	38	6.5	ng/L		01/24/18 20:52	01/31/18 13:12	1
Perfluorooctanoic acid (PFOA)	18	J	19	2.7	ng/L		01/24/18 20:52	01/31/18 13:12	1
Perfluorononanoic acid (PFNA)	19	U	23	7.6	ng/L		01/24/18 20:52	01/31/18 13:12	1
Perfluorohexanesulfonic acid (PFHxS)	6.2	J	29	5.3	ng/L		01/24/18 20:52	01/31/18 13:12	1
Perfluoroheptanoic acid (PFHpA)	4.7	J	9.5	1.8	ng/L		01/24/18 20:52	01/31/18 13:12	1
Perfluorobutanesulfonic acid (PFBS)	34	U	86	15	ng/L		01/24/18 20:52	01/31/18 13:12	1
Surrogate	%Recovery	Qualifier	Limits				Prepared	Analyzed	Dil Fac
13C2 PFHxA	93		70 - 130				01/24/18 20:52	01/31/18 13:12	1
13C2 PFDA	101		70 - 130				01/24/18 20:52	01/31/18 13:12	1

Client Sample Results

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-35046-1

Client Sample ID: NAWC-011118-FRB-179

Lab Sample ID: 320-35046-13

Date Collected: 01/11/18 12:35

Matrix: Water

Date Received: 01/12/18 13:20

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	15	U	38	6.5	ng/L		01/24/18 20:52	01/31/18 13:26	1
Perfluorooctanoic acid (PFOA)	7.6	U	19	2.7	ng/L		01/24/18 20:52	01/31/18 13:26	1
Perfluorononanoic acid (PFNA)	19	U	23	7.6	ng/L		01/24/18 20:52	01/31/18 13:26	1
Perfluorohexanesulfonic acid (PFHxS)	11	U	29	5.3	ng/L		01/24/18 20:52	01/31/18 13:26	1
Perfluoroheptanoic acid (PFHpA)	3.8	U	9.6	1.8	ng/L		01/24/18 20:52	01/31/18 13:26	1
Perfluorobutanesulfonic acid (PFBS)	34	U	86	15	ng/L		01/24/18 20:52	01/31/18 13:26	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	95		70 - 130	01/24/18 20:52	01/31/18 13:26	1
13C2 PFDA	95		70 - 130	01/24/18 20:52	01/31/18 13:26	1

Client Sample ID: NAWC-011118-RW-303

Lab Sample ID: 320-35046-14

Date Collected: 01/11/18 13:10

Matrix: Water

Date Received: 01/12/18 13:20

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	21	J M	38	6.5	ng/L		01/24/18 20:52	01/31/18 13:31	1
Perfluorooctanoic acid (PFOA)	20		19	2.7	ng/L		01/24/18 20:52	01/31/18 13:31	1
Perfluorononanoic acid (PFNA)	19	U	23	7.7	ng/L		01/24/18 20:52	01/31/18 13:31	1
Perfluorohexanesulfonic acid (PFHxS)	7.3	J	29	5.3	ng/L		01/24/18 20:52	01/31/18 13:31	1
Perfluoroheptanoic acid (PFHpA)	6.0	J	9.6	1.8	ng/L		01/24/18 20:52	01/31/18 13:31	1
Perfluorobutanesulfonic acid (PFBS)	35	U	86	15	ng/L		01/24/18 20:52	01/31/18 13:31	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	91		70 - 130	01/24/18 20:52	01/31/18 13:31	1
13C2 PFDA	103		70 - 130	01/24/18 20:52	01/31/18 13:31	1

Client Sample ID: NAWC-011118-FRB-303

Lab Sample ID: 320-35046-15

Date Collected: 01/11/18 13:05

Matrix: Water

Date Received: 01/12/18 13:20

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	15	U	38	6.5	ng/L		01/24/18 20:52	01/31/18 13:36	1
Perfluorooctanoic acid (PFOA)	7.6	U	19	2.7	ng/L		01/24/18 20:52	01/31/18 13:36	1
Perfluorononanoic acid (PFNA)	19	U	23	7.6	ng/L		01/24/18 20:52	01/31/18 13:36	1
Perfluorohexanesulfonic acid (PFHxS)	11	U	29	5.2	ng/L		01/24/18 20:52	01/31/18 13:36	1
Perfluoroheptanoic acid (PFHpA)	3.8	U	9.5	1.8	ng/L		01/24/18 20:52	01/31/18 13:36	1
Perfluorobutanesulfonic acid (PFBS)	34	U	86	15	ng/L		01/24/18 20:52	01/31/18 13:36	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	92		70 - 130	01/24/18 20:52	01/31/18 13:36	1
13C2 PFDA	102		70 - 130	01/24/18 20:52	01/31/18 13:36	1

Client Sample Results

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-35046-1

Client Sample ID: WGNA-011118-RW-3409

Lab Sample ID: 320-35046-16

Date Collected: 01/11/18 15:10

Matrix: Water

Date Received: 01/12/18 13:20

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	20	J M	35	5.9	ng/L	-	01/24/18 20:52	01/31/18 13:40	1
Perfluorooctanoic acid (PFOA)	14	J	17	2.4	ng/L	-	01/24/18 20:52	01/31/18 13:40	1
Perfluorononanoic acid (PFNA)	17	U	21	6.9	ng/L	-	01/24/18 20:52	01/31/18 13:40	1
Perfluorohexanesulfonic acid (PFHxS)	7.9	J	26	4.8	ng/L	-	01/24/18 20:52	01/31/18 13:40	1
Perfluoroheptanoic acid (PFHpA)	5.1	J	8.7	1.6	ng/L	-	01/24/18 20:52	01/31/18 13:40	1
Perfluorobutanesulfonic acid (PFBS)	31	U	78	14	ng/L	-	01/24/18 20:52	01/31/18 13:40	1
Surrogate	%Recovery	Qualifier	Limits				Prepared	Analyzed	Dil Fac
13C2 PFHxA	91		70 - 130				01/24/18 20:52	01/31/18 13:40	1
13C2 PFDA	100		70 - 130				01/24/18 20:52	01/31/18 13:40	1

Client Sample ID: WGNA-011118-FRB-3409

Lab Sample ID: 320-35046-17

Date Collected: 01/11/18 15:05

Matrix: Water

Date Received: 01/12/18 13:20

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	15	U	38	6.5	ng/L	-	01/24/18 20:52	01/31/18 13:54	1
Perfluorooctanoic acid (PFOA)	7.6	U	19	2.7	ng/L	-	01/24/18 20:52	01/31/18 13:54	1
Perfluorononanoic acid (PFNA)	19	U	23	7.6	ng/L	-	01/24/18 20:52	01/31/18 13:54	1
Perfluorohexanesulfonic acid (PFHxS)	11	U	29	5.3	ng/L	-	01/24/18 20:52	01/31/18 13:54	1
Perfluoroheptanoic acid (PFHpA)	3.8	U	9.6	1.8	ng/L	-	01/24/18 20:52	01/31/18 13:54	1
Perfluorobutanesulfonic acid (PFBS)	34	U	86	15	ng/L	-	01/24/18 20:52	01/31/18 13:54	1
Surrogate	%Recovery	Qualifier	Limits				Prepared	Analyzed	Dil Fac
13C2 PFHxA	99		70 - 130				01/24/18 20:52	01/31/18 13:54	1
13C2 PFDA	101		70 - 130				01/24/18 20:52	01/31/18 13:54	1

Client Sample ID: WGNA-011118-RW-3220

Lab Sample ID: 320-35046-18

Date Collected: 01/11/18 16:10

Matrix: Water

Date Received: 01/12/18 13:20

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	38	M	37	6.4	ng/L	-	01/24/18 20:52	01/31/18 13:59	1
Perfluorooctanoic acid (PFOA)	13	J	19	2.6	ng/L	-	01/24/18 20:52	01/31/18 13:59	1
Perfluorononanoic acid (PFNA)	19	U	22	7.5	ng/L	-	01/24/18 20:52	01/31/18 13:59	1
Perfluorohexanesulfonic acid (PFHxS)	17	J	28	5.1	ng/L	-	01/24/18 20:52	01/31/18 13:59	1
Perfluoroheptanoic acid (PFHpA)	8.0	J	9.3	1.8	ng/L	-	01/24/18 20:52	01/31/18 13:59	1
Perfluorobutanesulfonic acid (PFBS)	110		84	15	ng/L	-	01/24/18 20:52	01/31/18 13:59	1
Surrogate	%Recovery	Qualifier	Limits				Prepared	Analyzed	Dil Fac
13C2 PFHxA	85		70 - 130				01/24/18 20:52	01/31/18 13:59	1
13C2 PFDA	97		70 - 130				01/24/18 20:52	01/31/18 13:59	1

Client Sample Results

Client: Tetra Tech, Inc.
 Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-35046-1

Client Sample ID: WGNA-011118-FRB-3220

Lab Sample ID: 320-35046-19

Date Collected: 01/11/18 16:05

Matrix: Water

Date Received: 01/12/18 13:20

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	15	U	37	6.3	ng/L		01/24/18 20:52	01/31/18 14:04	1
Perfluorooctanoic acid (PFOA)	7.4	U	18	2.6	ng/L		01/24/18 20:52	01/31/18 14:04	1
Perfluorononanoic acid (PFNA)	18	U	22	7.4	ng/L		01/24/18 20:52	01/31/18 14:04	1
Perfluorohexanesulfonic acid (PFHxS)	11	U	28	5.1	ng/L		01/24/18 20:52	01/31/18 14:04	1
Perfluoroheptanoic acid (PFHpA)	3.7	U	9.2	1.7	ng/L		01/24/18 20:52	01/31/18 14:04	1
Perfluorobutanesulfonic acid (PFBS)	33	U	83	15	ng/L		01/24/18 20:52	01/31/18 14:04	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
¹³ C2 PFHxA	95		70 - 130	01/24/18 20:52	01/31/18 14:04	1
¹³ C2 PFDA	101		70 - 130	01/24/18 20:52	01/31/18 14:04	1

Default Detection Limits

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-35046-1

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Prep: 537

Analyte	LOQ	DL	Units	Method
Perfluorobutanesulfonic acid (PFBS)	90	16	ng/L	537
Perfluoroheptanoic acid (PFHpA)	10	1.9	ng/L	537
Perfluorohexanesulfonic acid (PFHxS)	30	5.5	ng/L	537
Perfluorononanoic acid (PFNA)	24	8.0	ng/L	537
Perfluorooctanesulfonic acid (PFOS)	40	6.8	ng/L	537
Perfluorooctanoic acid (PFOA)	20	2.8	ng/L	537

Surrogate Summary

Client: Tetra Tech, Inc.
 Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-35046-1

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Matrix: Water

Prep Type: Total/NA

Lab Sample ID	Client Sample ID	Percent Surrogate Recovery (Acceptance Limits)	
		PFHxA (70-130)	PFDA (70-130)
320-35046-1	WGNA-011118-RW-3103	92	97
320-35046-2	WGNA-011118-FRB-3103	99	104
320-35046-3	WGNA-011118-RW-0683	87	96
320-35046-4	WGNA-011118-FRB-0683	96	99
320-35046-5	NAWC-011118-RW-139	92	97
320-35046-6	NAWC-011118-FRB-139	90	96
320-35046-7	WGNA-011118-DUP-18	92	101
320-35046-8	NAWC-011118-RW-098	91	102
320-35046-9	NAWC-011118-FRB-098	93	94
320-35046-10	NAWC-011118-RW-180	92	100
320-35046-11	NAWC-011118-FRB-180	99	100
320-35046-12	NAWC-011118-RW-179	93	101
320-35046-12 LMS	NAWC-011118-RW-179	94	108
320-35046-12 LMSD	NAWC-011118-RW-179	88	97
320-35046-13	NAWC-011118-FRB-179	95	95
320-35046-14	NAWC-011118-RW-303	91	103
320-35046-15	NAWC-011118-FRB-303	92	102
320-35046-16	WGNA-011118-RW-3409	91	100
320-35046-17	WGNA-011118-FRB-3409	99	101
320-35046-18	WGNA-011118-RW-3220	85	97
320-35046-19	WGNA-011118-FRB-3220	95	101
LLCS 320-205489/2-A	Lab Control Sample	103	104
MB 320-205489/1-A	Method Blank	95	101

Surrogate Legend

PFHxA = 13C2 PFHxA

PFDA = 13C2 PFDA

QC Sample Results

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-35046-1

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Lab Sample ID: MB 320-205489/1-A
Matrix: Water
Analysis Batch: 206408

Client Sample ID: Method Blank
Prep Type: Total/NA
Prep Batch: 205489

Analyte	MB	MB	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
	Result	Qualifier							
Perfluorooctanesulfonic acid (PFOS)	16	U	40	6.8	ng/L		01/24/18 20:52	01/31/18 12:02	1
Perfluorooctanoic acid (PFOA)	8.0	U	20	2.8	ng/L		01/24/18 20:52	01/31/18 12:02	1
Perfluorononanoic acid (PFNA)	20	U	24	8.0	ng/L		01/24/18 20:52	01/31/18 12:02	1
Perfluorohexanesulfonic acid (PFHxS)	12	U	30	5.5	ng/L		01/24/18 20:52	01/31/18 12:02	1
Perfluoroheptanoic acid (PFHpA)	4.0	U	10	1.9	ng/L		01/24/18 20:52	01/31/18 12:02	1
Perfluorobutanesulfonic acid (PFBS)	36	U	90	16	ng/L		01/24/18 20:52	01/31/18 12:02	1

Surrogate	MB	MB	Limits	Prepared	Analyzed	Dil Fac
	%Recovery	Qualifier				
13C2 PFHxA	95		70 - 130	01/24/18 20:52	01/31/18 12:02	1
13C2 PFDA	101		70 - 130	01/24/18 20:52	01/31/18 12:02	1

Lab Sample ID: LLCS 320-205489/2-A
Matrix: Water
Analysis Batch: 206408

Client Sample ID: Lab Control Sample
Prep Type: Total/NA
Prep Batch: 205489

Analyte	Spike Added	LLCS	LLCS	Unit	D	%Rec	Limits
		Result	Qualifier				
Perfluorooctanesulfonic acid (PFOS)	40.0	38.5	J M	ng/L		96	50 - 150
Perfluorooctanoic acid (PFOA)	20.0	20.1		ng/L		100	50 - 150
Perfluorononanoic acid (PFNA)	20.0	19.9	J	ng/L		99	50 - 150
Perfluorohexanesulfonic acid (PFHxS)	30.0	29.0	J	ng/L		97	50 - 150
Perfluoroheptanoic acid (PFHpA)	10.0	11.1		ng/L		111	50 - 150
Perfluorobutanesulfonic acid (PFBS)	90.0	91.7		ng/L		102	50 - 150

Surrogate	LLCS	LLCS	Limits
	%Recovery	Qualifier	
13C2 PFHxA	103		70 - 130
13C2 PFDA	104		70 - 130

Lab Sample ID: 320-35046-12 LMS
Matrix: Water
Analysis Batch: 206410

Client Sample ID: NAWC-011118-RW-179
Prep Type: Total/NA
Prep Batch: 205489

Analyte	Sample	Sample	Spike Added	LMS	LMS	Unit	D	%Rec	Limits
	Result	Qualifier		Result	Qualifier				
Perfluorooctanesulfonic acid (PFOS)	18	J M	39.2	54.3	M	ng/L		94	50 - 150
Perfluorooctanoic acid (PFOA)	18	J	19.6	37.3		ng/L		96	50 - 150
Perfluorononanoic acid (PFNA)	19	U	19.6	21.2	J	ng/L		109	50 - 150
Perfluorohexanesulfonic acid (PFHxS)	6.2	J	29.4	34.9		ng/L		98	50 - 150
Perfluoroheptanoic acid (PFHpA)	4.7	J	9.79	14.9		ng/L		104	50 - 150
Perfluorobutanesulfonic acid (PFBS)	34	U	88.1	90.6		ng/L		103	50 - 150

Surrogate	LMS	LMS	Limits
	%Recovery	Qualifier	
13C2 PFHxA	94		70 - 130
13C2 PFDA	108		70 - 130

TestAmerica Sacramento

QC Sample Results

Client: Tetra Tech, Inc.
 Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-35046-1

Method: 537 - Perfluorinated Alkyl Acids (LC/MS) (Continued)

Lab Sample ID: 320-35046-12 LMSD

Matrix: Water

Analysis Batch: 206410

Client Sample ID: NAWC-011118-RW-179

Prep Type: Total/NA

Prep Batch: 205489

Analyte	Sample	Sample	Spike	LMSD	LMSD	Unit	D	%Rec	%Rec.	RPD	RPD
	Result	Qualifier	Added	Result	Qualifier				Limits	Limits	Limit
Perfluorooctanesulfonic acid (PFOS)	18	J M	37.9	51.8	M	ng/L		90	50 - 150	5	50
Perfluorooctanoic acid (PFOA)	18	J	19.0	35.1		ng/L		88	50 - 150	6	50
Perfluorononanoic acid (PFNA)	19	U	18.9	19.6	J	ng/L		104	50 - 150	8	50
Perfluorohexanesulfonic acid (PFHxS)	6.2	J	28.4	33.0		ng/L		94	50 - 150	6	50
Perfluoroheptanoic acid (PFHpA)	4.7	J	9.47	13.0		ng/L		88	50 - 150	13	50
Perfluorobutanesulfonic acid (PFBS)	34	U	85.3	84.3	J	ng/L		99	50 - 150	7	50
		LMSD	LMSD								
Surrogate		%Recovery	Qualifier	Limits							
13C2 PFHxA		88		70 - 130							
13C2 PFDA		97		70 - 130							

QC Association Summary

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-35046-1

LCMS

Prep Batch: 205489

Lab Sample ID	Client Sample ID	Prep Type	Matrix	Method	Prep Batch
320-35046-1	WGNA-011118-RW-3103	Total/NA	Water	537	
320-35046-2	WGNA-011118-FRB-3103	Total/NA	Water	537	
320-35046-3	WGNA-011118-RW-0683	Total/NA	Water	537	
320-35046-4	WGNA-011118-FRB-0683	Total/NA	Water	537	
320-35046-5	NAWC-011118-RW-139	Total/NA	Water	537	
320-35046-6	NAWC-011118-FRB-139	Total/NA	Water	537	
320-35046-7	WGNA-011118-DUP-18	Total/NA	Water	537	
320-35046-8	NAWC-011118-RW-098	Total/NA	Water	537	
320-35046-9	NAWC-011118-FRB-098	Total/NA	Water	537	
320-35046-10	NAWC-011118-RW-180	Total/NA	Water	537	
320-35046-11	NAWC-011118-FRB-180	Total/NA	Water	537	
320-35046-12	NAWC-011118-RW-179	Total/NA	Water	537	
320-35046-13	NAWC-011118-FRB-179	Total/NA	Water	537	
320-35046-14	NAWC-011118-RW-303	Total/NA	Water	537	
320-35046-15	NAWC-011118-FRB-303	Total/NA	Water	537	
320-35046-16	WGNA-011118-RW-3409	Total/NA	Water	537	
320-35046-17	WGNA-011118-FRB-3409	Total/NA	Water	537	
320-35046-18	WGNA-011118-RW-3220	Total/NA	Water	537	
320-35046-19	WGNA-011118-FRB-3220	Total/NA	Water	537	
MB 320-205489/1-A	Method Blank	Total/NA	Water	537	
LLCS 320-205489/2-A	Lab Control Sample	Total/NA	Water	537	
320-35046-12 LMS	NAWC-011118-RW-179	Total/NA	Water	537	
320-35046-12 LMSD	NAWC-011118-RW-179	Total/NA	Water	537	

Analysis Batch: 206408

Lab Sample ID	Client Sample ID	Prep Type	Matrix	Method	Prep Batch
320-35046-1	WGNA-011118-RW-3103	Total/NA	Water	537	205489
320-35046-2	WGNA-011118-FRB-3103	Total/NA	Water	537	205489
320-35046-3	WGNA-011118-RW-0683	Total/NA	Water	537	205489
320-35046-4	WGNA-011118-FRB-0683	Total/NA	Water	537	205489
320-35046-5	NAWC-011118-RW-139	Total/NA	Water	537	205489
320-35046-6	NAWC-011118-FRB-139	Total/NA	Water	537	205489
320-35046-7	WGNA-011118-DUP-18	Total/NA	Water	537	205489
320-35046-8	NAWC-011118-RW-098	Total/NA	Water	537	205489
MB 320-205489/1-A	Method Blank	Total/NA	Water	537	205489
LLCS 320-205489/2-A	Lab Control Sample	Total/NA	Water	537	205489

Analysis Batch: 206410

Lab Sample ID	Client Sample ID	Prep Type	Matrix	Method	Prep Batch
320-35046-9	NAWC-011118-FRB-098	Total/NA	Water	537	205489
320-35046-10	NAWC-011118-RW-180	Total/NA	Water	537	205489
320-35046-11	NAWC-011118-FRB-180	Total/NA	Water	537	205489
320-35046-12	NAWC-011118-RW-179	Total/NA	Water	537	205489
320-35046-13	NAWC-011118-FRB-179	Total/NA	Water	537	205489
320-35046-14	NAWC-011118-RW-303	Total/NA	Water	537	205489
320-35046-15	NAWC-011118-FRB-303	Total/NA	Water	537	205489
320-35046-16	WGNA-011118-RW-3409	Total/NA	Water	537	205489
320-35046-12 LMS	NAWC-011118-RW-179	Total/NA	Water	537	205489
320-35046-12 LMSD	NAWC-011118-RW-179	Total/NA	Water	537	205489

QC Association Summary

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-35046-1

LCMS (Continued)

Analysis Batch: 206412

Lab Sample ID	Client Sample ID	Prep Type	Matrix	Method	Prep Batch
320-35046-17	WGNA-011118-FRB-3409	Total/NA	Water	537	205489
320-35046-18	WGNA-011118-RW-3220	Total/NA	Water	537	205489
320-35046-19	WGNA-011118-FRB-3220	Total/NA	Water	537	205489

Lab Chronicle

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-35046-1

Client Sample ID: WGNA-011118-RW-3103

Date Collected: 01/11/18 08:10

Date Received: 01/12/18 13:20

Lab Sample ID: 320-35046-1

Matrix: Water

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			205489	01/24/18 20:52	TWL	TAL SAC
Total/NA	Analysis	537		1	206408	01/31/18 12:12	JRB	TAL SAC

Client Sample ID: WGNA-011118-FRB-3103

Date Collected: 01/11/18 08:05

Date Received: 01/12/18 13:20

Lab Sample ID: 320-35046-2

Matrix: Water

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			205489	01/24/18 20:52	TWL	TAL SAC
Total/NA	Analysis	537		1	206408	01/31/18 12:16	JRB	TAL SAC

Client Sample ID: WGNA-011118-RW-0683

Date Collected: 01/11/18 08:40

Date Received: 01/12/18 13:20

Lab Sample ID: 320-35046-3

Matrix: Water

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			205489	01/24/18 20:52	TWL	TAL SAC
Total/NA	Analysis	537		1	206408	01/31/18 12:21	JRB	TAL SAC

Client Sample ID: WGNA-011118-FRB-0683

Date Collected: 01/11/18 08:35

Date Received: 01/12/18 13:20

Lab Sample ID: 320-35046-4

Matrix: Water

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			205489	01/24/18 20:52	TWL	TAL SAC
Total/NA	Analysis	537		1	206408	01/31/18 12:26	JRB	TAL SAC

Client Sample ID: NAWC-011118-RW-139

Date Collected: 01/11/18 10:40

Date Received: 01/12/18 13:20

Lab Sample ID: 320-35046-5

Matrix: Water

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			205489	01/24/18 20:52	TWL	TAL SAC
Total/NA	Analysis	537		1	206408	01/31/18 12:30	JRB	TAL SAC

Client Sample ID: NAWC-011118-FRB-139

Date Collected: 01/11/18 10:35

Date Received: 01/12/18 13:20

Lab Sample ID: 320-35046-6

Matrix: Water

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			205489	01/24/18 20:52	TWL	TAL SAC
Total/NA	Analysis	537		1	206408	01/31/18 12:35	JRB	TAL SAC

TestAmerica Sacramento

Lab Chronicle

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-35046-1

Client Sample ID: WGNA-011118-DUP-18

Date Collected: 01/11/18 07:00

Date Received: 01/12/18 13:20

Lab Sample ID: 320-35046-7

Matrix: Water

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			205489	01/24/18 20:52	TWL	TAL SAC
Total/NA	Analysis	537		1	206408	01/31/18 12:40	JRB	TAL SAC

Client Sample ID: NAWC-011118-RW-098

Date Collected: 01/11/18 11:10

Date Received: 01/12/18 13:20

Lab Sample ID: 320-35046-8

Matrix: Water

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			205489	01/24/18 20:52	TWL	TAL SAC
Total/NA	Analysis	537		1	206408	01/31/18 12:44	JRB	TAL SAC

Client Sample ID: NAWC-011118-FRB-098

Date Collected: 01/11/18 11:05

Date Received: 01/12/18 13:20

Lab Sample ID: 320-35046-9

Matrix: Water

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			205489	01/24/18 20:52	TWL	TAL SAC
Total/NA	Analysis	537		1	206410	01/31/18 12:58	JRB	TAL SAC

Client Sample ID: NAWC-011118-RW-180

Date Collected: 01/11/18 12:10

Date Received: 01/12/18 13:20

Lab Sample ID: 320-35046-10

Matrix: Water

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			205489	01/24/18 20:52	TWL	TAL SAC
Total/NA	Analysis	537		1	206410	01/31/18 13:03	JRB	TAL SAC

Client Sample ID: NAWC-011118-FRB-180

Date Collected: 01/11/18 12:05

Date Received: 01/12/18 13:20

Lab Sample ID: 320-35046-11

Matrix: Water

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			205489	01/24/18 20:52	TWL	TAL SAC
Total/NA	Analysis	537		1	206410	01/31/18 13:08	JRB	TAL SAC

Client Sample ID: NAWC-011118-RW-179

Date Collected: 01/11/18 12:40

Date Received: 01/12/18 13:20

Lab Sample ID: 320-35046-12

Matrix: Water

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			205489	01/24/18 20:52	TWL	TAL SAC
Total/NA	Analysis	537		1	206410	01/31/18 13:12	JRB	TAL SAC

TestAmerica Sacramento

Lab Chronicle

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-35046-1

Client Sample ID: NAWC-011118-FRB-179

Lab Sample ID: 320-35046-13

Date Collected: 01/11/18 12:35

Matrix: Water

Date Received: 01/12/18 13:20

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			205489	01/24/18 20:52	TWL	TAL SAC
Total/NA	Analysis	537		1	206410	01/31/18 13:26	JRB	TAL SAC

Client Sample ID: NAWC-011118-RW-303

Lab Sample ID: 320-35046-14

Date Collected: 01/11/18 13:10

Matrix: Water

Date Received: 01/12/18 13:20

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			205489	01/24/18 20:52	TWL	TAL SAC
Total/NA	Analysis	537		1	206410	01/31/18 13:31	JRB	TAL SAC

Client Sample ID: NAWC-011118-FRB-303

Lab Sample ID: 320-35046-15

Date Collected: 01/11/18 13:05

Matrix: Water

Date Received: 01/12/18 13:20

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			205489	01/24/18 20:52	TWL	TAL SAC
Total/NA	Analysis	537		1	206410	01/31/18 13:36	JRB	TAL SAC

Client Sample ID: WGNA-011118-RW-3409

Lab Sample ID: 320-35046-16

Date Collected: 01/11/18 15:10

Matrix: Water

Date Received: 01/12/18 13:20

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			205489	01/24/18 20:52	TWL	TAL SAC
Total/NA	Analysis	537		1	206410	01/31/18 13:40	JRB	TAL SAC

Client Sample ID: WGNA-011118-FRB-3409

Lab Sample ID: 320-35046-17

Date Collected: 01/11/18 15:05

Matrix: Water

Date Received: 01/12/18 13:20

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			205489	01/24/18 20:52	TWL	TAL SAC
Total/NA	Analysis	537		1	206412	01/31/18 13:54	JRB	TAL SAC

Client Sample ID: WGNA-011118-RW-3220

Lab Sample ID: 320-35046-18

Date Collected: 01/11/18 16:10

Matrix: Water

Date Received: 01/12/18 13:20

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			205489	01/24/18 20:52	TWL	TAL SAC
Total/NA	Analysis	537		1	206412	01/31/18 13:59	JRB	TAL SAC

TestAmerica Sacramento

Lab Chronicle

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-35046-1

Client Sample ID: WGNA-011118-FRB-3220

Lab Sample ID: 320-35046-19

Date Collected: 01/11/18 16:05

Matrix: Water

Date Received: 01/12/18 13:20

<u>Prep Type</u>	<u>Batch Type</u>	<u>Batch Method</u>	<u>Run</u>	<u>Dilution Factor</u>	<u>Batch Number</u>	<u>Prepared or Analyzed</u>	<u>Analyst</u>	<u>Lab</u>
Total/NA	Prep	537			205489	01/24/18 20:52	TWL	TAL SAC
Total/NA	Analysis	537		1	206412	01/31/18 14:04	JRB	TAL SAC

Laboratory References:

TAL SAC = TestAmerica Sacramento, 880 Riverside Parkway, West Sacramento, CA 95605, TEL (916)373-5600

Accreditation/Certification Summary

Client: Tetra Tech, Inc.
 Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-35046-1

Laboratory: TestAmerica Sacramento

All accreditations/certifications held by this laboratory are listed. Not all accreditations/certifications are applicable to this report.

Authority	Program	EPA Region	Identification Number	Expiration Date
Alaska (UST)	State Program	10	UST-055	01-31-18 *
Arizona	State Program	9	AZ0708	08-11-18
Arkansas DEQ	State Program	6	88-0691	06-17-18
California	State Program	9	2897	01-31-19
Colorado	State Program	8	CA00044	08-31-18
Connecticut	State Program	1	PH-0691	06-30-19
Florida	NELAP	4	E87570	06-30-18
Georgia	State Program	4	N/A	01-28-19
Hawaii	State Program	9	N/A	01-29-19
Illinois	NELAP	5	200060	03-17-18
Kansas	NELAP	7	E-10375	10-31-18
L-A-B	DoD ELAP		L2468	01-20-21
Louisiana	NELAP	6	30612	06-30-18
Maine	State Program	1	CA0004	04-14-18
Michigan	State Program	5	9947	01-31-18 *
Nevada	State Program	9	CA00044	07-31-18
New Hampshire	NELAP	1	2997	04-18-18
New Jersey	NELAP	2	CA005	06-30-18
New York	NELAP	2	11666	04-01-18
Oregon	NELAP	10	4040	01-29-20
Pennsylvania	NELAP	3	68-01272	03-31-18
Texas	NELAP	6	T104704399	05-31-18
US Fish & Wildlife	Federal		LE148388-0	07-31-18
USDA	Federal		P330-11-00436	01-17-21
USEPA UCMR	Federal	1	CA00044	11-06-18
Utah	NELAP	8	CA00044	02-28-18
Virginia	NELAP	3	460278	03-14-18
Washington	State Program	10	C581	05-05-18
West Virginia (DW)	State Program	3	9930C	12-31-18
Wyoming	State Program	8	8TMS-L	01-28-19

* Accreditation/Certification renewal pending - accreditation/certification considered valid.

Method Summary

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-35046-1

Method	Method Description	Protocol	Laboratory
537	Perfluorinated Alkyl Acids (LC/MS)	EPA	TAL SAC

Protocol References:

EPA = US Environmental Protection Agency

Laboratory References:

TAL SAC = TestAmerica Sacramento, 880 Riverside Parkway, West Sacramento, CA 95605, TEL (916)373-5600

Sample Summary

Client: Tetra Tech, Inc.

TestAmerica Job ID: 320-35046-1

Project/Site: Warminster: PFAS, NAS JRB Willow Grove

Lab Sample ID	Client Sample ID	Matrix	Collected	Received
320-35046-1	WGNA-011118-RW-3103	Water	01/11/18 08:10	01/12/18 13:20
320-35046-2	WGNA-011118-FRB-3103	Water	01/11/18 08:05	01/12/18 13:20
320-35046-3	WGNA-011118-RW-0683	Water	01/11/18 08:40	01/12/18 13:20
320-35046-4	WGNA-011118-FRB-0683	Water	01/11/18 08:35	01/12/18 13:20
320-35046-5	NAWC-011118-RW-139	Water	01/11/18 10:40	01/12/18 13:20
320-35046-6	NAWC-011118-FRB-139	Water	01/11/18 10:35	01/12/18 13:20
320-35046-7	WGNA-011118-DUP-18	Water	01/11/18 07:00	01/12/18 13:20
320-35046-8	NAWC-011118-RW-098	Water	01/11/18 11:10	01/12/18 13:20
320-35046-9	NAWC-011118-FRB-098	Water	01/11/18 11:05	01/12/18 13:20
320-35046-10	NAWC-011118-RW-180	Water	01/11/18 12:10	01/12/18 13:20
320-35046-11	NAWC-011118-FRB-180	Water	01/11/18 12:05	01/12/18 13:20
320-35046-12	NAWC-011118-RW-179	Water	01/11/18 12:40	01/12/18 13:20
320-35046-13	NAWC-011118-FRB-179	Water	01/11/18 12:35	01/12/18 13:20
320-35046-14	NAWC-011118-RW-303	Water	01/11/18 13:10	01/12/18 13:20
320-35046-15	NAWC-011118-FRB-303	Water	01/11/18 13:05	01/12/18 13:20
320-35046-16	WGNA-011118-RW-3409	Water	01/11/18 15:10	01/12/18 13:20
320-35046-17	WGNA-011118-FRB-3409	Water	01/11/18 15:05	01/12/18 13:20
320-35046-18	WGNA-011118-RW-3220	Water	01/11/18 16:10	01/12/18 13:20
320-35046-19	WGNA-011118-FRB-3220	Water	01/11/18 16:05	01/12/18 13:20

LCMS MANUAL INTEGRATION SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1

SDG No.: _____

Instrument ID: A8_N Analysis Batch Number: 192908

Lab Sample ID: IC 320-192908/4 Client Sample ID: _____

Date Analyzed: 11/03/17 13:37 Lab File ID: 2017.11.03_537XICAL_004.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.16	Assign Peak	phomsophat	11/06/17 07:17

Lab Sample ID: IC 320-192908/5 Client Sample ID: _____

Date Analyzed: 11/03/17 13:42 Lab File ID: 2017.11.03_537XICAL_005.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.16	Assign Peak	phomsophat	11/06/17 07:18

Lab Sample ID: IC 320-192908/7 ICISAV Client Sample ID: _____

Date Analyzed: 11/03/17 13:52 Lab File ID: 2017.11.03_537XICAL_007.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.16	Assign Peak	phomsophat	11/06/17 07:20

LCMS MANUAL INTEGRATION SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1

SDG No.: _____

Instrument ID: A8_N Analysis Batch Number: 206407

Lab Sample ID: CCVL 320-206407/1 Client Sample ID: _____

Date Analyzed: 01/31/18 10:52 Lab File ID: 2018.01.31_537A_004.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.09	Assign Peak	barnettj	01/31/18 15:58

LCMS MANUAL INTEGRATION SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1

SDG No.: _____

Instrument ID: A8_N Analysis Batch Number: 206408

Lab Sample ID: CCV 320-206408/14 CCVIS Client Sample ID: _____

Date Analyzed: 01/31/18 11:53 Lab File ID: 2018.01.31_537A_017.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.07	Assign Peak	barnettj	01/31/18 16:00

Lab Sample ID: LLCS 320-205489/2-A Client Sample ID: _____

Date Analyzed: 01/31/18 12:07 Lab File ID: 2018.01.31_537A_020.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.08	Assign Peak	barnettj	01/31/18 16:11

Lab Sample ID: 320-35046-1 Client Sample ID: WGNA-011118-RW-3103

Date Analyzed: 01/31/18 12:12 Lab File ID: 2018.01.31_537A_021.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.07	Assign Peak	barnettj	01/31/18 16:12

Lab Sample ID: 320-35046-3 Client Sample ID: WGNA-011118-RW-0683

Date Analyzed: 01/31/18 12:21 Lab File ID: 2018.01.31_537A_023.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.07	Assign Peak	barnettj	01/31/18 16:13

LCMS MANUAL INTEGRATION SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1

SDG No.: _____

Instrument ID: A8_N Analysis Batch Number: 206408

Lab Sample ID: 320-35046-5 Client Sample ID: NAWC-011118-RW-139

Date Analyzed: 01/31/18 12:30 Lab File ID: 2018.01.31_537A_025.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.08	Assign Peak	barnettj	01/31/18 16:14

Lab Sample ID: 320-35046-7 Client Sample ID: WGNA-011118-DUP-18

Date Analyzed: 01/31/18 12:40 Lab File ID: 2018.01.31_537A_027.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.07	Assign Peak	barnettj	01/31/18 16:15

Lab Sample ID: 320-35046-8 Client Sample ID: NAWC-011118-RW-098

Date Analyzed: 01/31/18 12:44 Lab File ID: 2018.01.31_537A_028.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluoroheptanoic acid (PFHpA)	1.63	Missed Peak	barnettj	01/31/18 16:16
Perfluorooctanesulfonic acid (PFOS)	2.07	Assign Peak	barnettj	01/31/18 16:17
Perfluorononanoic acid (PFNA)	2.08	Missed Peak	barnettj	01/31/18 16:17

Lab Sample ID: CCV 320-206408/26 CCVIS Client Sample ID: _____

Date Analyzed: 01/31/18 12:49 Lab File ID: 2018.01.31_537A_029.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.07	Assign Peak	barnettj	01/31/18 16:01

LCMS MANUAL INTEGRATION SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1

SDG No.: _____

Instrument ID: A8_N Analysis Batch Number: 206410

Lab Sample ID: CCV 320-206410/26 CCVIS Client Sample ID: _____

Date Analyzed: 01/31/18 12:49 Lab File ID: 2018.01.31_537A_029.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.07	Assign Peak	barnettj	01/31/18 16:01

Lab Sample ID: 320-35046-10 Client Sample ID: NAWC-011118-RW-180

Date Analyzed: 01/31/18 13:03 Lab File ID: 2018.01.31_537A_032.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.07	Assign Peak	barnettj	01/31/18 16:19

Lab Sample ID: 320-35046-12 Client Sample ID: NAWC-011118-RW-179

Date Analyzed: 01/31/18 13:12 Lab File ID: 2018.01.31_537A_034.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.07	Assign Peak	barnettj	01/31/18 16:21

Lab Sample ID: 320-35046-12 LMS Client Sample ID: NAWC-011118-RW-179 LMS

Date Analyzed: 01/31/18 13:17 Lab File ID: 2018.01.31_537A_035.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.06	Assign Peak	barnettj	01/31/18 16:22

LCMS MANUAL INTEGRATION SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1

SDG No.: _____

Instrument ID: A8_N Analysis Batch Number: 206410

Lab Sample ID: 320-35046-12 LMSD Client Sample ID: NAWC-011118-RW-179 LMSD

Date Analyzed: 01/31/18 13:22 Lab File ID: 2018.01.31_537A_036.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.07	Assign Peak	barnettj	01/31/18 16:23

Lab Sample ID: 320-35046-14 Client Sample ID: NAWC-011118-RW-303

Date Analyzed: 01/31/18 13:31 Lab File ID: 2018.01.31_537A_038.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.07	Assign Peak	barnettj	01/31/18 16:24

Lab Sample ID: 320-35046-16 Client Sample ID: WGNA-011118-RW-3409

Date Analyzed: 01/31/18 13:40 Lab File ID: 2018.01.31_537A_040.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.07	Assign Peak	barnettj	01/31/18 16:25

Lab Sample ID: CCV 320-206410/38 CCVIS Client Sample ID: _____

Date Analyzed: 01/31/18 13:45 Lab File ID: 2018.01.31_537A_041.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.07	Assign Peak	barnettj	01/31/18 16:02

LCMS MANUAL INTEGRATION SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1

SDG No.: _____

Instrument ID: A8_N Analysis Batch Number: 206412

Lab Sample ID: CCV 320-206412/38 CCVIS Client Sample ID: _____

Date Analyzed: 01/31/18 13:45 Lab File ID: 2018.01.31_537A_041.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.07	Assign Peak	barnettj	01/31/18 16:02

Lab Sample ID: 320-35046-18 Client Sample ID: WGNA-011118-RW-3220

Date Analyzed: 01/31/18 13:59 Lab File ID: 2018.01.31_537A_044.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.07	Assign Peak	barnettj	01/31/18 16:26

Lab Sample ID: CCV 320-206412/43 CCVIS Client Sample ID: _____

Date Analyzed: 01/31/18 14:08 Lab File ID: 2018.01.31_537A_046.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.07	Assign Peak	barnettj	01/31/18 16:03

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-35046-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
LC537-ICV_00028	01/05/18	08/02/17	MeOH/H2O, Lot 067374	10 mL	LC537-IS_00045	1000 uL	13C2-PFOA	10 ng/mL
.LC537-IS_00045	01/05/18	07/05/17	Methanol, Lot 090285	30000 uL	LCM2PFOA_00007	60 uL	13C2-PFOA	28.68 ng/mL
..LCM2PFOA_00007	02/12/21	Wellington Laboratories, Lot M2PFOA0216			(Purchased Reagent)		13C2-PFOA	0.1 ug/mL
..LCMPFOS_00019	08/03/21	Wellington Laboratories, Lot MPFOS0816			(Purchased Reagent)		13C4 PFOS	0.2868 ug/mL
LC537-ICV_00028	01/05/18	08/02/17	MeOH/H2O, Lot 067374	10 mL	LC537-SU_00046	1000 uL	13C2 PFDA	50 ug/mL
.LC537-SU_00046	01/05/18	07/05/17	Methanol, Lot 104453	30000 uL	LC537ICIM_00019	20 uL	13C2 PFHxA	47.8 ug/mL
..LCMPFDA_00012	09/30/21	Wellington Laboratories, Lot MPFDA0916			(Purchased Reagent)		13C2 PFDA	10 ng/mL
..LCMPFHxA_00013	04/08/21	Wellington Laboratories, Lot MPFHxA0416			(Purchased Reagent)		13C2 PFHxA	10 ng/mL
.LC537ICIM_00019	01/25/18	08/01/17	Methanol, Lot 090285	25 mL	LC537-PFBS2_00008	0.6 mL	Perfluorobutanesulfonic acid (PFBS)	100.119 ng/mL
..LC537-PFBS2_00008	01/25/18	07/25/17	Methanol, Lot 090285	20 mL	LC537-PFHxA2_00011	0.061 mL	Perfluoroheptanoic acid (PFHpA)	9.99613 ng/mL
...LC537-PFHxA2_00011	09/08/22	Santa Cruz Biotechnology, Lot F0917			(Purchased Reagent)		13C2 PFDA	20.0761 ng/mL
..LC537-PFHxA2_00011	01/25/18	07/25/17	Methanol, Lot 09092	31 mL	LC537-PFHxS2_00008	0.122 mL	Perfluorohexanesulfonic acid (PFHxS)	20.1272 ng/mL
...LC537-PFHxS2_00008	06/13/22	Afla Aesar, Lot 10200390			(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	20.4843 ng/mL
..LC537-PFHxS2_00008	01/25/18	07/25/17	Methanol, Lot 090285	21 mL	LC537-PFNA2_00009	0.126 mL	Perfluorononanoic acid (PFNA)	19.698 ng/mL
...LC537-PFNA2_00009	06/08/22	Santa Cruz Biotechnology, Lot G2516			(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	20.4843 ng/mL
..LC537-PFNA2_00009	01/25/18	07/25/17	Methanol, Lot 090285	21 mL	LC537-PFOA2_00010	0.122 mL	Perfluorooctanoic acid (PFOA)	19.698 ng/mL
...LC537-PFOA2_00010	06/14/22	Aldrich, Lot MKCC0699			(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	20.1272 ng/mL
..LC537-PFOA2_00010	01/25/18	08/01/17	Methanol, Lot 090285	20 mL	LC537-PFOS2_00010	0.124 mL	Perfluorooctanesulfonic acid (PFOS)	20.4843 ng/mL
...LC537-PFOS2_00010	06/09/22	Afla Aesar, Lot 10199078			(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	19.698 ng/mL
..LC537-PFOA2_00002	06/09/22	Afla Aesar, Lot 10199078			(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	19.698 ng/mL
...LC537-PFOA2_00002	06/09/22	Afla Aesar, Lot 10199078			(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	19.698 ng/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-35046-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
..LC537-PFOS2_00010	01/25/18	08/01/17	Methanol, Lot 090285	22 mL	LC537_PFOS2_00002	0.0561 g	Perfluorooctanesulfonic acid (PFOS)	1985.68 ug/mL
...LC537_PFOS2_00002	06/14/22		Sigma, Lot BCBQ0108V		(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	0.7787 g/g
LC537-IS_00055	05/27/18	11/27/17	Methanol, Lot 090285	30000 uL	LCM2PFOA_00007	60 uL	13C2-PFOA	0.1 ug/mL
					LCMPFOS_00021	180 uL	13C4 PFOS	0.2868 ug/mL
..LCM2PFOA_00007	02/12/21	Wellington Laboratories, Lot M2PFOA0216			(Purchased Reagent)		13C2-PFOA	50 ug/mL
..LCMPFOS_00021	12/12/21	Wellington Laboratories, Lot MPFOS1216			(Purchased Reagent)		13C4 PFOS	47.8 ug/mL
LC537-L1_00020	02/04/18	08/14/17	MeOH/H2O, Lot 090285	5 mL	LC537-IS_00048	500 uL	13C2-PFOA	10 ng/mL
							13C4 PFOS	28.68 ng/mL
					LC537-MSP_00029	60 uL	Perfluorobutanesulfonic acid (PFBS)	9.0018 ng/mL
							Perfluoroheptanoic acid (PFHpA)	1.00036 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	3.00103 ng/mL
							Perfluorononanoic acid (PFNA)	2.0006 ng/mL
							Perfluorooctanoic acid (PFOA)	2.00191 ng/mL
							Perfluorooctanesulfonic acid (PFOS)	4.00146 ng/mL
					LC537-SU_00049	500 uL	13C2 PFDA	10 ng/mL
							13C2 PFHxA	10 ng/mL
..LC537-IS_00048	02/04/18	08/04/17	Methanol, Lot 090285	30000 uL	LCM2PFOA_00007	60 uL	13C2-PFOA	0.1 ug/mL
					LCMPFOS_00021	180 uL	13C4 PFOS	0.2868 ug/mL
..LCM2PFOA_00007	02/12/21	Wellington Laboratories, Lot M2PFOA0216			(Purchased Reagent)		13C2-PFOA	50 ug/mL
..LCMPFOS_00021	12/12/21	Wellington Laboratories, Lot MPFOS1216			(Purchased Reagent)		13C4 PFOS	47.8 ug/mL
..LC537-MSP_00029	02/10/18	08/10/17	Methanol, Lot 141039	20000 uL	LC537SPIM_00023	166.7 uL	Perfluorobutanesulfonic acid (PFBS)	750.15 ng/mL
							Perfluoroheptanoic acid (PFHpA)	83.3637 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	250.086 ng/mL
							Perfluorononanoic acid (PFNA)	166.716 ng/mL
							Perfluorooctanoic acid (PFOA)	166.826 ng/mL
							Perfluorooctanesulfonic acid (PFOS)	333.455 ng/mL
..LC537SPIM_00023	02/10/18	08/10/17	Methanol, Lot 104453	10000 uL	LC537-PFBS_00008	450 uL	Perfluorobutanesulfonic acid (PFBS)	90 ug/mL
					LC537-PFHpA_00015	100 uL	Perfluoroheptanoic acid (PFHpA)	10.0016 ug/mL
					LC537-PFHxS_00010	150 uL	Perfluorohexanesulfonic acid (PFHxS)	30.0043 ug/mL
					LC537-PFNA_00013	200 uL	Perfluorononanoic acid (PFNA)	20.002 ug/mL
					LC537-PFOA_00013	200 uL	Perfluorooctanoic acid (PFOA)	20.0151 ug/mL
					LC537-PFOS_00008	400 uL	Perfluorooctanesulfonic acid (PFOS)	40.0066 ug/mL
...LC537-PFBS_00008	02/10/18	08/10/17	Methanol, Lot 090285	49.6 mL	LC537_PFBS_00002	0.0992 g	Perfluorobutanesulfonic acid (PFBS)	2 mg/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-35046-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
....LC537_PFBs_00002	04/01/18		Sigma, Lot MKBP8842V		(Purchased Reagent)		Perfluorobutanesulfonic acid (PFBS)	1 g/g
...LC537-PFHpA_00015	02/10/18	08/10/17	Methanol, Lot 090285	48.7 mL	LC537_PFHpA_00002	0.0492 g	Perfluoroheptanoic acid (PFHpA)	1.00016 mg/mL
....LC537_PFHpA_00002	04/01/18		Aldrich, Lot BCBM2579V		(Purchased Reagent)		Perfluoroheptanoic acid (PFHpA)	0.99 g/g
...LC537-PFHxS_00010	02/10/18	08/10/17	Methanol, Lot 090285	55.92 mL	LC537_PFHxS_00002	0.123 g	Perfluorohexanesulfonic acid (PFHxS)	2.00029 mg/mL
....LC537_PFHxS_00002	04/01/18		Sigma, Lot BCBL3545V		(Purchased Reagent)		Perfluorohexanesulfonic acid (PFHxS)	0.9094 g/g
..LC537-PFNA_00013	02/10/18	08/10/17	Methanol, Lot 090285	62.3 mL	LC537 PFNA_00002	0.0647 g	Perfluorononanoic acid (PFNA)	1000.1 ug/mL
....LC537 PFNA_00002	04/01/18		TCI America, Lot QN44F		(Purchased Reagent)		Perfluorononanoic acid (PFNA)	0.963 g/g
...LC537-PFOA_00013	02/10/18	08/10/17	Methanol, Lot 090285	22.76 mL	LC537 PFOA_00003	0.0228 g	Perfluorooctanoic acid (PFOA)	1.00076 mg/mL
....LC537 PFOA_00003	10/31/23		SIGMA ALDRICH, Lot BCBS1198V		(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	0.999 g/g
...LC537-PFOS_00008	02/10/18	08/10/17	Methanol, Lot 090285	44.43 mL	LC537_PFOS_00003	0.0488 g	Perfluorooctanesulfonic acid (PFOS)	1.00016 mg/mL
....LC537_PFOS_00003	04/17/19		sigma alrich, Lot SZBE107XV		(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	0.9106 g/g
.LC537-SU_00049	02/04/18	08/04/17	Methanol, Lot 104453	30000 uL	LCMPFDA_00012	60 uL	13C2 PFDA	0.1 ug/mL
..LCMPFDA_00012	09/30/21		Wellington Laboratories, Lot MPFDA0916		LCMPFHxA_00013	60 uL	13C2 PFHxA	0.1 ug/mL
..LCMPFHxA_00013	04/08/21		Wellington Laboratories, Lot MPFHxA0416		(Purchased Reagent)		13C2 PFDA	50 ug/mL
LC537-L2_00020	02/04/18	08/14/17	MeOH/H2O, Lot 090285	5 mL	LC537-HSP_00025	80 uL	Perfluorobutanesulfonic acid (PFBS)	20.0016 ng/mL
							Perfluoroheptanoic acid (PFHpA)	2.22277 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	6.66817 ng/mL
							Perfluorononanoic acid (PFNA)	4.44524 ng/mL
							Perfluorooctanoic acid (PFOA)	4.44816 ng/mL
					Perfluorooctanesulfonic acid (PFOS)	8.89106 ng/mL		
					LC537-IS_00048	500 uL	13C2-PFOA	10 ng/mL
LC537-SU_00049	500 uL	13C4 PFOS	28.68 ng/mL					
.LC537-HSP_00025	02/10/18	08/10/17	Methanol, Lot 141039	20000 uL	LC537SPIM_00023	277.8 uL	Perfluorobutanesulfonic acid (PFBS)	1250.1 ng/mL
							Perfluoroheptanoic acid (PFHpA)	138.923 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	416.76 ng/mL
							Perfluorononanoic acid (PFNA)	277.827 ng/mL
							Perfluorooctanoic acid (PFOA)	278.01 ng/mL
							Perfluorooctanesulfonic acid (PFOS)	555.691 ng/mL
..LC537SPIM_00023	02/10/18	08/10/17	Methanol, Lot 104453	10000 uL	LC537-PFBS_00008	450 uL	Perfluorobutanesulfonic acid (PFBS)	90 ug/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-35046-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
					LC537-PFHpA_00015	100 uL	Perfluoroheptanoic acid (PFHpA)	10.0016 ug/mL
					LC537-PFHxS_00010	150 uL	Perfluorohexanesulfonic acid (PFHxS)	30.0043 ug/mL
					LC537-PFNA_00013	200 uL	Perfluorononanoic acid (PFNA)	20.002 ug/mL
					LC537-PFOA_00013	200 uL	Perfluorooctanoic acid (PFOA)	20.0151 ug/mL
					LC537-PFOS_00008	400 uL	Perfluorooctanesulfonic acid (PFOS)	40.0066 ug/mL
...LC537-PFBS_00008	02/10/18	08/10/17	Methanol, Lot 090285	49.6 mL	LC537_PFBS_00002	0.0992 g	Perfluorobutanesulfonic acid (PFBS)	2 mg/mL
....LC537_PFBS_00002	04/01/18	Sigma, Lot MKBP8842V			(Purchased Reagent)		Perfluorobutanesulfonic acid (PFBS)	1 g/g
...LC537-PFHpA_00015	02/10/18	08/10/17	Methanol, Lot 090285	48.7 mL	LC537_PFHpA_00002	0.0492 g	Perfluoroheptanoic acid (PFHpA)	1.00016 mg/mL
....LC537_PFHpA_00002	04/01/18	Aldrich, Lot BCBM2579V			(Purchased Reagent)		Perfluoroheptanoic acid (PFHpA)	0.99 g/g
...LC537-PFHxS_00010	02/10/18	08/10/17	Methanol, Lot 090285	55.92 mL	LC537_PFHxS_00002	0.123 g	Perfluorohexanesulfonic acid (PFHxS)	2.00029 mg/mL
....LC537_PFHxS_00002	04/01/18	Sigma, Lot BCBL3545V			(Purchased Reagent)		Perfluorohexanesulfonic acid (PFHxS)	0.9094 g/g
...LC537-PFNA_00013	02/10/18	08/10/17	Methanol, Lot 090285	62.3 mL	LC537_PFNA_00002	0.0647 g	Perfluorononanoic acid (PFNA)	1000.1 ug/mL
....LC537_PFNA_00002	04/01/18	TCI America, Lot QN44F			(Purchased Reagent)		Perfluorononanoic acid (PFNA)	0.963 g/g
...LC537-PFOA_00013	02/10/18	08/10/17	Methanol, Lot 090285	22.76 mL	LC537_PFOA_00003	0.0228 g	Perfluorooctanoic acid (PFOA)	1.00076 mg/mL
....LC537_PFOA_00003	10/31/23	SIGMA ALDRICH, Lot BCBS1198V			(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	0.999 g/g
...LC537-PFOS_00008	02/10/18	08/10/17	Methanol, Lot 090285	44.43 mL	LC537_PFOS_00003	0.0488 g	Perfluorooctanesulfonic acid (PFOS)	1.00016 mg/mL
....LC537_PFOS_00003	04/17/19	sigma alrich, Lot SZBE107XV			(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	0.9106 g/g
.LC537-IS_00048	02/04/18	08/04/17	Methanol, Lot 090285	30000 uL	LCM2PFOA_00007	60 uL	13C2-PFOA	0.1 ug/mL
..LCM2PFOA_00007	02/12/21	Wellington Laboratories, Lot M2PFOA0216			LCMPFOS_00021	180 uL	13C4 PFOS	0.2868 ug/mL
..LCMPFOS_00021	12/12/21	Wellington Laboratories, Lot MPFOS1216			(Purchased Reagent)		13C2-PFOA	50 ug/mL
.LC537-SU_00049	02/04/18	08/04/17	Methanol, Lot 104453	30000 uL	LCMPFDA_00012	60 uL	13C2 PFDA	47.8 ug/mL
..LCMPFDA_00012	09/30/21	Wellington Laboratories, Lot MPFDA0916			LCMPFHxA_00013	60 uL	13C2 PFHxA	0.1 ug/mL
..LCMPFHxA_00013	04/08/21	Wellington Laboratories, Lot MPFHxA0416			(Purchased Reagent)		13C2 PFDA	50 ug/mL
..LCMPFHxA_00013	04/08/21	Wellington Laboratories, Lot MPFHxA0416			(Purchased Reagent)		13C2 PFHxA	50 ug/mL
LC537-L3_00023	02/04/18	08/14/17	MeOH/H2O, Lot 090285	5 mL	LC537-HSP_00025	180 uL	Perfluorobutanesulfonic acid (PFBS)	45.0036 ng/mL
							Perfluoroheptanoic acid (PFHpA)	5.00122 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	15.0034 ng/mL
							Perfluorononanoic acid (PFNA)	10.0018 ng/mL
							Perfluorooctanoic acid (PFOA)	10.0084 ng/mL
							Perfluorooctanesulfonic acid (PFOS)	20.0049 ng/mL
					LC537-IS_00048	500 uL	13C2-PFOA	10 ng/mL
							13C4 PFOS	28.68 ng/mL
					LC537-SU_00049	500 uL	13C2 PFDA	10 ng/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-35046-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration							
					Reagent ID	Volume Added									
.LC537-HSP_00025	02/10/18	08/10/17	Methanol, Lot 141039	20000 uL	LC537SPIM_00023	277.8 uL	13C2 PFHxA	10 ng/mL							
							Perfluorobutanesulfonic acid (PFBS)	1250.1 ng/mL							
							Perfluoroheptanoic acid (PFHpA)	138.923 ng/mL							
							Perfluorohexanesulfonic acid (PFHxS)	416.76 ng/mL							
							Perfluorononanoic acid (PFNA)	277.827 ng/mL							
..LC537SPIM_00023	02/10/18	08/10/17	Methanol, Lot 104453	10000 uL	LC537-PFBS_00008	450 uL	Perfluorobutanesulfonic acid (PFBS)	90 ug/mL							
							LC537-PFHpA_00015	100 uL	Perfluoroheptanoic acid (PFHpA)	10.0016 ug/mL					
							LC537-PFHxS_00010	150 uL	Perfluorohexanesulfonic acid (PFHxS)	30.0043 ug/mL					
							LC537-PFNA_00013	200 uL	Perfluorononanoic acid (PFNA)	20.002 ug/mL					
							LC537-PFOA_00013	200 uL	Perfluorooctanoic acid (PFOA)	20.0151 ug/mL					
...LC537-PFOS_00008	02/10/18	08/10/17	Methanol, Lot 090285	49.6 mL	LC537-PFOS_00008	400 uL	Perfluorooctanesulfonic acid (PFOS)	555.691 ng/mL							
							LC537-PFBS_00002	0.0992 g	Perfluorobutanesulfonic acid (PFBS)	2 mg/mL					
						LC537-PFBS_00002	04/01/18	Sigma, Lot MKBP8842V		(Purchased Reagent)	Perfluorobutanesulfonic acid (PFBS)	1 g/g		
							...LC537-PFHpA_00015	02/10/18	08/10/17	Methanol, Lot 090285	48.7 mL	LC537-PFHpA_00002	0.0492 g	Perfluoroheptanoic acid (PFHpA)	1.00016 mg/mL
						LC537-PFHpA_00002	04/01/18	Aldrich, Lot BCBM2579V		(Purchased Reagent)	Perfluoroheptanoic acid (PFHpA)	0.99 g/g		
...LC537-PFHxS_00010	02/10/18	08/10/17	Methanol, Lot 090285	55.92 mL	LC537-PFHxS_00002	0.123 g	Perfluorohexanesulfonic acid (PFHxS)	2.00029 mg/mL							
						LC537-PFHxS_00002	04/01/18	Sigma, Lot BCBL3545V		(Purchased Reagent)	Perfluorohexanesulfonic acid (PFHxS)	0.9094 g/g		
							...LC537-PFNA_00013	02/10/18	08/10/17	Methanol, Lot 090285	62.3 mL	LC537-PFNA_00002	0.0647 g	Perfluorononanoic acid (PFNA)	1000.1 ug/mL
						LC537-PFNA_00002	04/01/18	TCI America, Lot QN44F		(Purchased Reagent)	Perfluorononanoic acid (PFNA)	0.963 g/g		
							...LC537-PFOA_00013	02/10/18	08/10/17	Methanol, Lot 090285	22.76 mL	LC537-PFOA_00003	0.0228 g	Perfluorooctanoic acid (PFOA)	1.00076 mg/mL
...LC537-PFOS_00008	02/10/18	08/10/17	Methanol, Lot 090285	44.43 mL	LC537-PFOS_00003	0.0488 g	Perfluorooctanesulfonic acid (PFOS)	1.00016 mg/mL							
						LC537-PFOS_00003	04/17/19	sigma alrich, Lot SZBE107XV		(Purchased Reagent)	Perfluorooctanesulfonic acid (PFOS)	0.9106 g/g		
							.LC537-IS_00048	02/04/18	08/04/17	Methanol, Lot 090285	30000 uL	LCM2PFOA_00007	60 uL	13C2-PFOA	0.1 ug/mL
							..LCM2PFOA_00007	02/12/21	Wellington Laboratories, Lot M2PFOA0216		(Purchased Reagent)	LCMPFOS_00021	180 uL	13C4 PFOS	0.2868 ug/mL
							..LCMPFOS_00021	12/12/21	Wellington Laboratories, Lot MPFOS1216		(Purchased Reagent)	13C4 PFOS		47.8 ug/mL	
.LC537-SU_00049	02/04/18	08/04/17	Methanol, Lot 104453	30000 uL	LCMPFDA_00012	60 uL	13C2 PFDA	0.1 ug/mL							
							LCMPFHxA_00013	60 uL	13C2 PFHxA	0.1 ug/mL					
							..LCMPFDA_00012	09/30/21	Wellington Laboratories, Lot MPFDA0916		(Purchased Reagent)	13C2 PFDA	50 ug/mL		
							..LCMPFHxA_00013	04/08/21	Wellington Laboratories, Lot MPFHxA0416		(Purchased Reagent)	13C2 PFHxA	50 ug/mL		

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-35046-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration		
					Reagent ID	Volume Added				
LC537-L4_00020	02/04/18	08/14/17	MeOH/H2O, Lot 090285	5 mL	LC537-HSP_00025	360 uL	Perfluorobutanesulfonic acid (PFBS)	90.0072 ng/mL		
							Perfluoroheptanoic acid (PFHpA)	10.0024 ng/mL		
							Perfluorohexanesulfonic acid (PFHxS)	30.0067 ng/mL		
							Perfluorononanoic acid (PFNA)	20.0036 ng/mL		
							Perfluorooctanoic acid (PFOA)	20.0167 ng/mL		
					Perfluorooctanesulfonic acid (PFOS)	40.0098 ng/mL				
					LC537-IS_00048	500 uL	13C2-PFOA	10 ng/mL		
LC537-SU_00049	500 uL	13C2 PFDA	10 ng/mL							
.LC537-HSP_00025	02/10/18	08/10/17	Methanol, Lot 141039	20000 uL	LC537SPIM_00023	277.8 uL	Perfluorobutanesulfonic acid (PFBS)	1250.1 ng/mL		
							Perfluoroheptanoic acid (PFHpA)	138.923 ng/mL		
							Perfluorohexanesulfonic acid (PFHxS)	416.76 ng/mL		
							Perfluorononanoic acid (PFNA)	277.827 ng/mL		
							Perfluorooctanoic acid (PFOA)	278.01 ng/mL		
Perfluorooctanesulfonic acid (PFOS)	555.691 ng/mL									
..LC537SPIM_00023	02/10/18	08/10/17	Methanol, Lot 104453	10000 uL	LC537-PFBS_00008	450 uL	Perfluorobutanesulfonic acid (PFBS)	90 ug/mL		
							LC537-PFHpA_00015	100 uL	Perfluoroheptanoic acid (PFHpA)	10.0016 ug/mL
							LC537-PFHxS_00010	150 uL	Perfluorohexanesulfonic acid (PFHxS)	30.0043 ug/mL
							LC537-PFNA_00013	200 uL	Perfluorononanoic acid (PFNA)	20.002 ug/mL
							LC537-PFOA_00013	200 uL	Perfluorooctanoic acid (PFOA)	20.0151 ug/mL
							LC537-PFOS_00008	400 uL	Perfluorooctanesulfonic acid (PFOS)	40.0066 ug/mL
...LC537-PFBS_00008	02/10/18	08/10/17	Methanol, Lot 090285	49.6 mL	LC537_PFBS_00002	0.0992 g	Perfluorobutanesulfonic acid (PFBS)	2 mg/mL		
....LC537_PFBS_00002	04/01/18		Sigma, Lot MKBP8842V		(Purchased Reagent)		Perfluorobutanesulfonic acid (PFBS)	1 g/g		
...LC537-PFHpA_00015	02/10/18	08/10/17	Methanol, Lot 090285	48.7 mL	LC537_PFHpA_00002	0.0492 g	Perfluoroheptanoic acid (PFHpA)	1.00016 mg/mL		
....LC537_PFHpA_00002	04/01/18		Aldrich, Lot BCBM2579V		(Purchased Reagent)		Perfluoroheptanoic acid (PFHpA)	0.99 g/g		
...LC537-PFHxS_00010	02/10/18	08/10/17	Methanol, Lot 090285	55.92 mL	LC537_PFHxS_00002	0.123 g	Perfluorohexanesulfonic acid (PFHxS)	2.00029 mg/mL		
....LC537_PFHxS_00002	04/01/18		Sigma, Lot BCBL3545V		(Purchased Reagent)		Perfluorohexanesulfonic acid (PFHxS)	0.9094 g/g		
...LC537-PFNA_00013	02/10/18	08/10/17	Methanol, Lot 090285	62.3 mL	LC537 PFNA_00002	0.0647 g	Perfluorononanoic acid (PFNA)	1000.1 ug/mL		
....LC537 PFNA_00002	04/01/18		TCI America, Lot QN44F		(Purchased Reagent)		Perfluorononanoic acid (PFNA)	0.963 g/g		
...LC537-PFOA_00013	02/10/18	08/10/17	Methanol, Lot 090285	22.76 mL	LC537 PFOA_00003	0.0228 g	Perfluorooctanoic acid (PFOA)	1.00076 mg/mL		
....LC537_PFOA_00003	10/31/23		SIGMA ALDRICH, Lot BCBS1198V		(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	0.999 g/g		

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-35046-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
...LC537-PFOS_00008	02/10/18	08/10/17	Methanol, Lot 090285	44.43 mL	LC537_PFOS_00003	0.0488 g	Perfluorooctanesulfonic acid (PFOS)	1.00016 mg/mL
....LC537_PFOS_00003	04/17/19	sigma alrich, Lot SZBE107XV			(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	0.9106 g/g
.LC537-IS_00048	02/04/18	08/04/17	Methanol, Lot 090285	30000 uL	LCM2PFOA 00007	60 uL	13C2-PFOA	0.1 ug/mL
					LCMPFOS 00021	180 uL	13C4 PFOS	0.2868 ug/mL
..LCM2PFOA 00007	02/12/21	Wellington Laboratories, Lot M2PFOA0216			(Purchased Reagent)		13C2-PFOA	50 ug/mL
..LCMPFOS 00021	12/12/21	Wellington Laboratories, Lot MPFOS1216			(Purchased Reagent)		13C4 PFOS	47.8 ug/mL
.LC537-SU_00049	02/04/18	08/04/17	Methanol, Lot 104453	30000 uL	LCMPFDA 00012	60 uL	13C2 PFDA	0.1 ug/mL
					LCMPFHxA 00013	60 uL	13C2 PFHxA	0.1 ug/mL
..LCMPFDA 00012	09/30/21	Wellington Laboratories, Lot MPFDA0916			(Purchased Reagent)		13C2 PFDA	50 ug/mL
..LCMPFHxA 00013	04/08/21	Wellington Laboratories, Lot MPFHxA0416			(Purchased Reagent)		13C2 PFHxA	50 ug/mL
LC537-L5_00024	02/04/18	08/14/17	MeOH/H2O, Lot 090285	5 mL	LC537-HSP_00025	540 uL	Perfluorobutanesulfonic acid (PFBS)	135.011 ng/mL
							Perfluoroheptanoic acid (PFHpA)	15.0037 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	45.0101 ng/mL
							Perfluorononanoic acid (PFNA)	30.0053 ng/mL
							Perfluorooctanoic acid (PFOA)	30.0251 ng/mL
							Perfluorooctanesulfonic acid (PFOS)	60.0146 ng/mL
					LC537-IS_00048	500 uL	13C2-PFOA	10 ng/mL
		13C4 PFOS	28.68 ng/mL					
		LC537-SU_00049	500 uL	13C2 PFDA	10 ng/mL			
				13C2 PFHxA	10 ng/mL			
.LC537-HSP_00025	02/10/18	08/10/17	Methanol, Lot 141039	20000 uL	LC537SPIM_00023	277.8 uL	Perfluorobutanesulfonic acid (PFBS)	1250.1 ng/mL
							Perfluoroheptanoic acid (PFHpA)	138.923 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	416.76 ng/mL
							Perfluorononanoic acid (PFNA)	277.827 ng/mL
							Perfluorooctanoic acid (PFOA)	278.01 ng/mL
							Perfluorooctanesulfonic acid (PFOS)	555.691 ng/mL
..LC537SPIM_00023	02/10/18	08/10/17	Methanol, Lot 104453	10000 uL	LC537-PFBS_00008	450 uL	Perfluorobutanesulfonic acid (PFBS)	90 ug/mL
					LC537-PFHpA_00015	100 uL	Perfluoroheptanoic acid (PFHpA)	10.0016 ug/mL
					LC537-PFHxS_00010	150 uL	Perfluorohexanesulfonic acid (PFHxS)	30.0043 ug/mL
					LC537-PFNA 00013	200 uL	Perfluorononanoic acid (PFNA)	20.002 ug/mL
					LC537-PFOA 00013	200 uL	Perfluorooctanoic acid (PFOA)	20.0151 ug/mL
					LC537-PFOS_00008	400 uL	Perfluorooctanesulfonic acid (PFOS)	40.0066 ug/mL
...LC537-PFBS_00008	02/10/18	08/10/17	Methanol, Lot 090285	49.6 mL	LC537_PFBS_00002	0.0992 g	Perfluorobutanesulfonic acid (PFBS)	2 mg/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-35046-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
....LC537_PFB_S_00002	04/01/18		Sigma, Lot MKBP8842V		(Purchased Reagent)		Perfluorobutanesulfonic acid (PFBS)	1 g/g
...LC537-PFHpA_00015	02/10/18	08/10/17	Methanol, Lot 090285	48.7 mL	LC537_PFHpA_00002	0.0492 g	Perfluoroheptanoic acid (PFHpA)	1.00016 mg/mL
....LC537_PFHpA_00002	04/01/18		Aldrich, Lot BCBM2579V		(Purchased Reagent)		Perfluoroheptanoic acid (PFHpA)	0.99 g/g
...LC537-PFHxS_00010	02/10/18	08/10/17	Methanol, Lot 090285	55.92 mL	LC537_PFHxS_00002	0.123 g	Perfluorohexanesulfonic acid (PFHxS)	2.00029 mg/mL
....LC537_PFHxS_00002	04/01/18		Sigma, Lot BCBL3545V		(Purchased Reagent)		Perfluorohexanesulfonic acid (PFHxS)	0.9094 g/g
..LC537-PFNA_00013	02/10/18	08/10/17	Methanol, Lot 090285	62.3 mL	LC537 PFNA_00002	0.0647 g	Perfluorononanoic acid (PFNA)	1000.1 ug/mL
....LC537 PFNA_00002	04/01/18		TCI America, Lot QN44F		(Purchased Reagent)		Perfluorononanoic acid (PFNA)	0.963 g/g
..LC537-PFOA_00013	02/10/18	08/10/17	Methanol, Lot 090285	22.76 mL	LC537 PFOA_00003	0.0228 g	Perfluorooctanoic acid (PFOA)	1.00076 mg/mL
....LC537 PFOA_00003	10/31/23		SIGMA ALDRICH, Lot BCBS1198V		(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	0.999 g/g
..LC537-PFOS_00008	02/10/18	08/10/17	Methanol, Lot 090285	44.43 mL	LC537_PFOS_00003	0.0488 g	Perfluorooctanesulfonic acid (PFOS)	1.00016 mg/mL
....LC537_PFOS_00003	04/17/19		sigma alrich, Lot SZBE107XV		(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	0.9106 g/g
.LC537-IS_00048	02/04/18	08/04/17	Methanol, Lot 090285	30000 uL	LCM2PFOA_00007	60 uL	13C2-PFOA	0.1 ug/mL
..LCM2PFOA_00007	02/12/21		Wellington Laboratories, Lot M2PFOA0216		(Purchased Reagent)		13C2-PFOA	50 ug/mL
..LCMPFOS_00021	12/12/21		Wellington Laboratories, Lot MPFOS1216		(Purchased Reagent)		13C4 PFOS	47.8 ug/mL
.LC537-SU_00049	02/04/18	08/04/17	Methanol, Lot 104453	30000 uL	LCMPFDA_00012	60 uL	13C2 PFDA	0.1 ug/mL
..LCMPFDA_00012	09/30/21		Wellington Laboratories, Lot MPFDA0916		(Purchased Reagent)		13C2 PFDA	50 ug/mL
..LCMPFHxA_00013	04/08/21		Wellington Laboratories, Lot MPFHxA0416		(Purchased Reagent)		13C2 PFHxA	50 ug/mL
LC537-L6_00020	02/04/18	08/14/17	MeOH/H2O, Lot 090285	5 mL	LC537-HSP_00025	720 uL	Perfluorobutanesulfonic acid (PFBS)	180.014 ng/mL
							Perfluoroheptanoic acid (PFHpA)	20.0049 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	60.0135 ng/mL
							Perfluorononanoic acid (PFNA)	40.0071 ng/mL
							Perfluorooctanoic acid (PFOA)	40.0334 ng/mL
							Perfluorooctanesulfonic acid (PFOS)	80.0195 ng/mL
.LC537-IS_00048	02/10/18	08/10/17	Methanol, Lot 141039	20000 uL	LC537-IS_00048	500 uL	13C2-PFOA	10 ng/mL
							13C4 PFOS	28.68 ng/mL
							13C2 PFDA	10 ng/mL
.LC537-SU_00049	02/10/18	08/10/17	Methanol, Lot 141039	20000 uL	LC537-SU_00049	500 uL	13C2 PFHxA	10 ng/mL
							Perfluorobutanesulfonic acid (PFBS)	1250.1 ng/mL
							Perfluoroheptanoic acid (PFHpA)	138.923 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	416.76 ng/mL
.LC537-HSP_00025	02/10/18	08/10/17	Methanol, Lot 141039	20000 uL	LC537SPIM_00023	277.8 uL	Perfluorononanoic acid (PFNA)	277.827 ng/mL
							Perfluorooctanoic acid (PFOA)	278.01 ng/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-35046-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
							Perfluorooctanesulfonic acid (PFOS)	555.691 ng/mL
..LC537SPIM_00023	02/10/18	08/10/17	Methanol, Lot 104453	10000 uL	LC537-PFBS_00008	450 uL	Perfluorobutanesulfonic acid (PFBS)	90 ug/mL
					LC537-PFHpA_00015	100 uL	Perfluoroheptanoic acid (PFHpA)	10.0016 ug/mL
					LC537-PFHxS_00010	150 uL	Perfluorohexanesulfonic acid (PFHxS)	30.0043 ug/mL
					LC537-PFNA_00013	200 uL	Perfluorononanoic acid (PFNA)	20.002 ug/mL
					LC537-PFOA_00013	200 uL	Perfluorooctanoic acid (PFOA)	20.0151 ug/mL
					LC537-PFOS_00008	400 uL	Perfluorooctanesulfonic acid (PFOS)	40.0066 ug/mL
...LC537-PFBS_00008	02/10/18	08/10/17	Methanol, Lot 090285	49.6 mL	LC537_PFBS_00002	0.0992 g	Perfluorobutanesulfonic acid (PFBS)	2 mg/mL
....LC537_PFBS_00002	04/01/18		Sigma, Lot MKBP8842V		(Purchased Reagent)		Perfluorobutanesulfonic acid (PFBS)	1 g/g
...LC537-PFHpA_00015	02/10/18	08/10/17	Methanol, Lot 090285	48.7 mL	LC537_PFHpA_00002	0.0492 g	Perfluoroheptanoic acid (PFHpA)	1.00016 mg/mL
....LC537_PFHpA_00002	04/01/18		Aldrich, Lot BCBM2579V		(Purchased Reagent)		Perfluoroheptanoic acid (PFHpA)	0.99 g/g
...LC537-PFHxS_00010	02/10/18	08/10/17	Methanol, Lot 090285	55.92 mL	LC537_PFHxS_00002	0.123 g	Perfluorohexanesulfonic acid (PFHxS)	2.00029 mg/mL
....LC537_PFHxS_00002	04/01/18		Sigma, Lot BCBL3545V		(Purchased Reagent)		Perfluorohexanesulfonic acid (PFHxS)	0.9094 g/g
...LC537-PFNA_00013	02/10/18	08/10/17	Methanol, Lot 090285	62.3 mL	LC537 PFNA_00002	0.0647 g	Perfluorononanoic acid (PFNA)	1000.1 ug/mL
....LC537 PFNA_00002	04/01/18		TCI America, Lot QN44F		(Purchased Reagent)		Perfluorononanoic acid (PFNA)	0.963 g/g
...LC537-PFOA_00013	02/10/18	08/10/17	Methanol, Lot 090285	22.76 mL	LC537 PFOA_00003	0.0228 g	Perfluorooctanoic acid (PFOA)	1.00076 mg/mL
....LC537 PFOA_00003	10/31/23		SIGMA ALDRICH, Lot BCBS1198V		(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	0.999 g/g
...LC537-PFOS_00008	02/10/18	08/10/17	Methanol, Lot 090285	44.43 mL	LC537_PFOS_00003	0.0488 g	Perfluorooctanesulfonic acid (PFOS)	1.00016 mg/mL
....LC537_PFOS_00003	04/17/19		sigma alrich, Lot SZBE107XV		(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	0.9106 g/g
.LC537-IS_00048	02/04/18	08/04/17	Methanol, Lot 090285	30000 uL	LCM2PFOA_00007	60 uL	13C2-PFOA	0.1 ug/mL
					LCMPFOS_00021	180 uL	13C4 PFOS	0.2868 ug/mL
..LCM2PFOA_00007	02/12/21		Wellington Laboratories, Lot M2PFOA0216		(Purchased Reagent)		13C2-PFOA	50 ug/mL
..LCMPFOS_00021	12/12/21		Wellington Laboratories, Lot MPFOS1216		(Purchased Reagent)		13C4 PFOS	47.8 ug/mL
.LC537-SU_00049	02/04/18	08/04/17	Methanol, Lot 104453	30000 uL	LCMPFDA_00012	60 uL	13C2 PFDA	0.1 ug/mL
					LCMPFHxA_00013	60 uL	13C2 PFHxA	0.1 ug/mL
..LCMPFDA_00012	09/30/21		Wellington Laboratories, Lot MPFDA0916		(Purchased Reagent)		13C2 PFDA	50 ug/mL
..LCMPFHxA_00013	04/08/21		Wellington Laboratories, Lot MPFHxA0416		(Purchased Reagent)		13C2 PFHxA	50 ug/mL
LC537-LSP_00028	02/10/18	08/10/17	Methanol, Lot 090285	20000 uL	LC537SPIM_00023	50 uL	Perfluorobutane Sulfonate	225 ng/mL
							Perfluorobutanesulfonic acid (PFBS)	225 ng/mL
							Perfluoroheptanoic acid (PFHpA)	25.0041 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	75.0109 ng/mL
							Perfluorononanoic acid (PFNA)	50.0049 ng/mL
							Perfluorooctanoic acid (PFOA)	50.0378 ng/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-35046-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
							Perfluorooctanesulfonic acid (PFOS)	100.016 ng/mL
.LC537SPIM_00023	02/10/18	08/10/17	Methanol, Lot 104453	10000 uL	LC537-PFBS_00008	450 uL	Perfluorobutane Sulfonate	90 ug/mL
							Perfluorobutanesulfonic acid (PFBS)	90 ug/mL
					LC537-PFHpA_00015	100 uL	Perfluoroheptanoic acid (PFHpA)	10.0016 ug/mL
					LC537-PFHxS_00010	150 uL	Perfluorohexanesulfonic acid (PFHxS)	30.0043 ug/mL
					LC537-PFNA_00013	200 uL	Perfluorononanoic acid (PFNA)	20.002 ug/mL
					LC537-PFOA_00013	200 uL	Perfluorooctanoic acid (PFOA)	20.0151 ug/mL
					LC537-PFOS_00008	400 uL	Perfluorooctanesulfonic acid (PFOS)	40.0066 ug/mL
..LC537-PFBS_00008	02/10/18	08/10/17	Methanol, Lot 090285	49.6 mL	LC537_PFBS_00002	0.0992 g	Perfluorobutane Sulfonate	2 mg/mL
							Perfluorobutanesulfonic acid (PFBS)	2 mg/mL
...LC537_PFBS_00002	04/01/18	Sigma, Lot MKBP8842V			(Purchased Reagent)		Perfluorobutane Sulfonate	1 g/g
							Perfluorobutanesulfonic acid (PFBS)	1 g/g
..LC537-PFHpA_00015	02/10/18	08/10/17	Methanol, Lot 090285	48.7 mL	LC537_PFHpA_00002	0.0492 g	Perfluoroheptanoic acid (PFHpA)	1.00016 mg/mL
...LC537_PFHpA_00002	04/01/18	Aldrich, Lot BCM2579V			(Purchased Reagent)		Perfluoroheptanoic acid (PFHpA)	0.99 g/g
..LC537-PFHxS_00010	02/10/18	08/10/17	Methanol, Lot 090285	55.92 mL	LC537_PFHxS_00002	0.123 g	Perfluorohexanesulfonic acid (PFHxS)	2.00029 mg/mL
...LC537_PFHxS_00002	04/01/18	Sigma, Lot BCBL3545V			(Purchased Reagent)		Perfluorohexanesulfonic acid (PFHxS)	0.9094 g/g
..LC537-PFNA_00013	02/10/18	08/10/17	Methanol, Lot 090285	62.3 mL	LC537 PFNA_00002	0.0647 g	Perfluorononanoic acid (PFNA)	1000.1 ug/mL
..LC537 PFNA_00002	04/01/18	TCI America, Lot QN44F			(Purchased Reagent)		Perfluorononanoic acid (PFNA)	0.963 g/g
..LC537-PFOA_00013	02/10/18	08/10/17	Methanol, Lot 090285	22.76 mL	LC537 PFOA_00003	0.0228 g	Perfluorooctanoic acid (PFOA)	1.00076 mg/mL
..LC537 PFOA_00003	10/31/23	SIGMA ALDRICH, Lot BCBS1198V			(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	0.999 g/g
..LC537-PFOS_00008	02/10/18	08/10/17	Methanol, Lot 090285	44.43 mL	LC537_PFOS_00003	0.0488 g	Perfluorooctanesulfonic acid (PFOS)	1.00016 mg/mL
...LC537_PFOS_00003	04/17/19	sigma alrich, Lot SZBE107XV			(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	0.9106 g/g
LC537-SU_00053	05/27/18	11/27/17	Methanol, Lot 104453	30000 uL	LCMPFDA_00012	60 uL	13C2 PFDA	0.1 ug/mL
					LCMPFHxA_00015	60 uL	13C2 PFHxA	0.1 ug/mL
.LCMPFDA_00012	09/30/21	Wellington Laboratories, Lot MPFDA0916			(Purchased Reagent)		13C2 PFDA	50 ug/mL
.LCMPFHxA_00015	11/22/21	Wellington Laboratories, Lot MPFHxA1116			(Purchased Reagent)		13C2 PFHxA	50 ug/mL

Reagent

LC537_PFB_00002

4/1/15 SPV

3050 Spruce Street, Saint Louis, MO 63103, USA

Website: www.sigmaaldrich.com


Email USA: techserv@sial.com

Outside USA: eurtechserv@sial.com

Certificate of Analysis

Product Name:
Nonafluorobutane-1-sulfonic acid - 97%

Product Number: 562629
Batch Number: MKBP8842V
Brand: ALDRICH
CAS Number: 375-73-5
MDL Number: MFCD01320794
Formula: C4HF9O3S
Formula Weight: 300.10 g/mol
Storage Temperature: Store at 2 - 8 °C
Quality Release Date: 11 OCT 2013



PFBS

Test	Specification	Result
Appearance (Color)	Colorless	Colorless
Appearance (Form)	Liquid	Liquid
Infrared Spectrum	Conforms to Structure	Conforms
Fluorine NMR Spectrum	Conforms to Structure	Conforms
Purity (Titration by NaOH)	96.5 - 103.5 %	101.6 %

Jamie Gleason, Manager
Quality Control
Milwaukee, Wisconsin US

Sigma-Aldrich warrants, that at the time of the quality release or subsequent retest date this product conformed to the information contained in this publication. The current Specification sheet may be available at Sigma-Aldrich.com. For further inquiries, please contact Technical Service. Purchaser must determine the suitability of the product for its particular use. See reverse side of invoice or packing slip for additional terms and conditions of sale.

Reagent

LC537_PFB2_00002

F: 6.8.17 SW



CERTIFICATE OF ANALYSIS

The Power to Question

Catalog Number: sc-236187
Lot Number: F0917
Product Name: Nonafluorobutane-1-sulfonic acid
CAS Number: 375-73-5
Molecular Formula: $C_4HF_9O_3S$
Molecular Weight: 300.10

Test	Specification	Result
Appearance	Colorless liquid	Complies
Identification (19F-NMR)	Conforms to structure	Complies
Purity (Sodium Hydroxide Titration)	$\geq 97\%$	101.3%
Infrared Spectrum	Conforms to structure	Complies

Reagent

LC537_PFHpA_00002

R: 4/1/15 4V

Certificate of Analysis

Product Name: PERFLUOROHEPTANOIC ACID
 99 %
 Product Number: 342041
 Batch Number: BCBM2579V
 Brand: Aldrich
 CAS Number: 375-85-9
 Formula: $CF_3(CF_2)_5CO_2H$
 Formula Weight: 364.06
 Quality Release Date: 06 DEC 2013
 Recommended Retest Date: OCT 2018

PFHpA

TEST	SPECIFICATION	RESULT
APPEARANCE (COLOR)	COLORLESS OR WHITE	WHITE
APPEARANCE (FORM)	LIQUID OR SOLID	SOLID
TITRATION	98.5 - 101.5 %	99.8 %
TITRATION (METHOD)	-	BACK TITRATION
PURITY (GC AREA %)	≥ 98.5 %	99.5 %
INFRARED SPECTRUM	CONFORMS TO STRUCTURE	CONFORMS

Dr. Claudia Geitner
Manager Quality Control
Buchs, Switzerland

Sigma-Aldrich warrants that at the time of the quality release or subsequent retest date this product conformed to the information contained in this publication. The current specification sheet may be available at Sigma-Aldrich.com. For further inquiries, please contact Technical Service. Purchaser must determine the suitability of the product for its particular use. See reverse side of invoice or packing slip for additional terms and conditions of sale.

Reagent

LC537_PFHpA2_00002

Certificate of analysis

r:6.13.17 SW

Product No.: A12092
Product: Perfluoroheptanoic acid, 98+%
Lot No.: 10200390

PFHe A

Appearance: White fused solid
Water Content (Karl-Fischer): 0.30%
Melting Point: 32.0-34.3°C
Assay (Aqueous acid-base titration): 99.7%
Identification (FTIR): Conforms

This document has been electronically generated and does not require a signature.

Order our products online www.alfa.com

ThermoFisher
SCIENTIFIC

Reagent

LC537_PFHxS_00002

r: 4/1/15 stw

Certificate of Analysis

Product Name: TRIDECAFLUOROHEXANE-1-SULFONIC ACID POTASSIUM SALT
 >= 98.0 % T

Product Number: 50929

Batch Number: BCBL3545V

Brand: Aldrich

CAS Number: 3871-99-6

Formula: C₆F₁₃KO₃S

Formula Weight: 438.20

Quality Release Date: 20 JUN 2013

PFH₁₃S-K

TEST	SPECIFICATION	RESULT
APPEARANCE (COLOR)	WHITE TO FAINT BEIGE	WHITE
APPEARANCE (FORM)	POWDER OR CRYSTALS	POWDER
TITRATION (ION EXCHANGE)	≥ 98.0 %	99.5 %
INFRARED SPECTRUM	CONFORMS TO STRUCTURE	CONFORMS

Dr. Claudia Geitner
Manager Quality Control
Buchs, Switzerland

$$MW_{corr} = \frac{(k_{form}) - (k) + (H)}{438.20 (k_{form})} = \frac{(438.20 - 3910 + 101)}{438.20 (k_{form})} = 0.91307 \text{ (anion form)}$$

$$Purity = 90.94 \% \text{ w/m.w correction}$$

stw 4/1/15

Sigma-Aldrich warrants that at the time of the quality release or subsequent retest date this product conformed to the information contained in this publication. The current specification sheet may be available at Sigma-Aldrich.com. For further inquiries, please contact Technical Service. Purchaser must determine the suitability of the product for its particular use. See reverse side of invoice or packing slip for additional terms and conditions of sale.

Reagent

LC537_PFHxS2_00002

n: 6-8-17 SKJ



The Future of Science

CERTIFICATE OF ANALYSIS

Catalog Number: sc-237289
 Lot Number: G2516
 Product Name: Tridecafluorohexane-1-sulfonic acid potassium salt
 CAS Number: 3871-99-6
 Molecular Formula: $C_6F_{13}KO_3S$
 Molecular Weight: 438.20

Test	Specification	Result
Appearance	White to faint beige powder or crystals	White powder
Identification (Infrared Spectrum)	Consistent with structure	Complies
Purity (Titration, Ion Exchange)	≥ 98.0%	100.4%

PFH₁₃S-K
 $C_6F_{13}SO_3K$ 438.201
 $C_6F_{13}SO_3H$ 400.111

MW correction = $\frac{400.11}{438.201} = 0.91307$ PFH₁₃S
 CAS# 355-46-4

Purity $\frac{1}{9}$ MW correction = 90.9%

This document was produced electronically and is valid without a signature.

Reagent

LC537_PENA_00002

R: 4/1/15 SKV



Certificate of Analysis

Apr 2, 2015 (JST)

TOKYO CHEMICAL INDUSTRY CO.,LTD.
4-10-1 Nihonbashi-Honcho, Chuo-ku, Tokyo 103-0023 Japan

Chemical Name: Heptadecafluorononanoic Acid		
Product Number: H0843 CAS: 375-95-1	Lot: QN44F	

Tests	Results	Specifications
Purity(GC)	96.3 %	min. 95.0 %
Purity(Neutralization titration)	98.1 %	min. 95.0 %
Melting point	63.3 deg-C	62.0 to 67.0 deg-C

TCI Lot numbers are 4-5 characters in length.
Characters listed after the first 4-5 characters are control numbers for internal purpose only.

Customer service:

TCI AMERICA
Tel: +1-800-423-8616 / +1-503-283-1681
Fax: +1-888-520-1075 / +1-503-283-1987
E-mail: Sales-US@TCIchemicals.com

PFNA

Reagent

LC537_PFN2_00002

P: 6.14.17 SKW

3050 Spruce Street, Saint Louis, MO 63103, USA

Website: www.sigmaaldrich.com


Email USA: techserv@sial.com

Outside USA: eurtechserv@sial.com

Certificate of Analysis

Product Name:
Perfluorononanoic acid - 97%

Product Number: 394459
Batch Number: MKCC0699
Brand: ALDRICH
CAS Number: 375-95-1
MDL Number: MFCD00039605
Formula: C9HF17O2
Formula Weight: 464.08 g/mol
Quality Release Date: 07 DEC 2016



Test	Specification	Result
Appearance (Color)	White to Off-White	White
Appearance (Form)	Powder or Crystals or Crystalline Chunk(s) or Granule or Flakes or Solid	Powder
Infrared Spectrum	Conforms to Structure	Conforms
GC (area %)	≥ 96.5 %	98.2 %

Michael Grady, Manager
Quality Control
Milwaukee, WI US

PFNA

Sigma-Aldrich warrants, that at the time of the quality release or subsequent retest date this product conformed to the information contained in this publication. The current Specification sheet may be available at Sigma-Aldrich.com. For further inquiries, please contact Technical Service. Purchaser must determine the suitability of the product for its particular use. See reverse side of Invoice or packing slip for additional terms and conditions of sale.

Reagent

LC537_PFOA_00003

P: 11/30/16 SKV
PFA

SIGMA-ALDRICH

3050 Spruce Street, Saint Louis, MO 63103 USA
Email USA: techserv@sial.com Outside USA: eurtechserv@sial.com

Certificate of Analysis

Product Name: PENTADECAFLUOROOCCTANOIC ACID
analytical standard
Product Number: 33824
Batch Number: BCBS1198V
Brand: Sigma-Aldrich
CAS Number: 335-67-1
Formula: $\text{CF}_3(\text{CF}_2)_6\text{COOH}$
Formula Weight: 414.07
Expiration Date: OCT 2023
Quality Release Date: 12 MAY 2016

TEST	SPECIFICATION	RESULT
PURITY (HPLC AREA %)	≥ 98.0%	100.0%
IDENTIFICATION (LC-MS)	IDENTITY CONFORMS	CONFORMS



Dr. Claudia Geitner
Manager Quality Control
Buchs, Switzerland

Sigma-Aldrich warrants that at the time of the quality release or subsequent retest date this product conformed to the information contained in this publication. The current specification sheet may be available at Sigma-Aldrich.com. For further inquiries, please contact Technical Service. Purchaser must determine the suitability of the product for its particular use. See reverse side of invoice or packing slip for additional terms and conditions of sale.

Reagent

LC537_PFOA2_00002

Certificate of analysis

P: 6/21/17 SW

Product No.: L08862
Product: Perfluorooctanoic acid, 95%
Lot No.: 10199078

PFOA

Appearance: White powder
Water Content (Karl-Fischer): 1.30%
Melting Point: 47.6-54.0°C
Assay (Aqueous acid-base titration): 98.4%
Assay (GC Silyl Deriv): 97.2%

This document has been electronically generated and does not require a signature.

Order our products online www.alfa.com

ThermoFisher
SCIENTIFIC

Reagent

LC537_PFOs_00003

n: 11/30/16 SV
PFOS

SIGMA-ALDRICH

CERTIFICATE OF ANALYSIS

Sigma-Aldrich Laborchemikalien GmbH D-30918 Seelze
Telefon: +49 5137 8238-150

Seelze, 22.04.2014/524107/14/08646

Order-No.:

Customer-No.:

Order-Code:

Quantity:

Production Date: 17.Apr.2014

Expiry Date: 17.Apr.2019

Article/Product: 33829

Batch : SZBE107XV

Heptadecafluorooctanesulfonic acid potassium salt OEKANAL®

Reference Material (RM)

1. General Information

Formula: C₈F₁₇KO₃S

CAS-No.: [2795-39-3]

Usage : PFOS

Molar mass: 538.22 g/Mole

Recomm. storage temp.: roomtemp.

The estimated uncertainty of a single measurement of the assay can be expected to be 0.5 % relative (confidence level = 95%, n= 6) whereby the assay measurements are calculated by 100% minus found impurities.

2. Batch Analysis

Identity

Assay (LC-MS)

Date of Analysis

complying

98 %

22.Apr.2014

3. Advice and Remarks

- The expiry date is based on the current knowledge and holds only for proper storage conditions in the originally closed flasks/ packages.
- Whenever the container is opened for removal of aliquot portions of the substance, the person handling the substance must assure, that the integrity of the substance is maintained and proper records of all its handlings are kept. Special care has to be taken to avoid any contamination or adulteration of the substance.
- We herewith confirm that the delivery is effected according to the technical delivery conditions agreed.
- Particular properties of the products or the suitability for a particular area of application are not assured.
- We guarantee a proper quality within our General Conditions of Sales.

Sigma-Aldrich Laborchemikalien GmbH
Quality Management SA-LC

Reagent

LC537_PFOs2_00002

R: 6.14.17 SKV

Certificate of Analysis

Product Name: HEPTADECAFLUOROOCCTANESULFONIC ACID TETRAETHYLAMMONIUM SALT
 98 %
Product Number: 365289
Batch Number: BCBQ0108V
Brand: Aldrich
CAS Number: 56773-42-3
Formula: $CF_3(CF_2)_6CF_2SO_3N(C_2H_5)_4$
Formula Weight: 629.37
Quality Release Date: 11 JUN 2015


TEST	SPECIFICATION	RESULT
APPEARANCE (COLOR)	WHITE TO OFF WHITE	OFF-WHITE
APPEARANCE (FORM)	POWDER OR POWDER WITH CHUNK(S)	POWDER
CARBON CONTENT	29.77 % - 31.29 %	29.97 %
INFRARED SPECTRUM	CONFORMS TO STRUCTURE	CONFORMS

Claudia Geitner

Dr. Claudia Geitner
 Manager Quality Control
 Buchs, Switzerland

MW correction: $\frac{500.125}{629.37} = 0.7946$

Purity & MW correction = 77.37%



	$C_{17}F_{17}SO_3 + H$	$C_8H_{20}N$
C = 12.011	96.088	96.088
F = 18.998	322.966	—
S = 32.066	32.066	—
O = 16.999	47.997	20.60
H = 1.008	1.008	14.007
N = 14.007	—	—
	<hr/>	<hr/>
	500.125	130.255

Reagent

LCM2PFOA_00007




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: M2PFOA
COMPOUND: Perfluoro-n-[1,2-¹³C₂]octanoic acid

LOT NUMBER: M2PFOA0216

STRUCTURE: **CAS #:** Not available



MOLECULAR FORMULA: ¹³C₂¹²C₆HF₁₆O₂
CONCENTRATION: 50 ± 2.5 µg/ml

MOLECULAR WEIGHT: 416.05
SOLVENT(S): Methanol
Water (<1%)

CHEMICAL PURITY: >98%
LAST TESTED: (mm/dd/yyyy) 02/12/2016
EXPIRY DATE: (mm/dd/yyyy) 02/12/2021

ISOTOPIC PURITY: ≥99% ¹³C
(1,2-¹³C₂)

RECOMMENDED STORAGE: Store ampoule in a cool, dark place

DOCUMENTATION/ DATA ATTACHED:

- Figure 1: LC/MS Data (TIC and Mass Spectrum)
- Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent conversion of the carboxylic acid to the methyl ester.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By:
B.G. Chittim

Date: 02/24/2016
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:


Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: M2PFOA; LC/MS Data (TIC and Mass Spectrum)



Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm


Mobile phase: Gradient
Start: 50% (80:20 MeOH:ACN) / 50% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 90% organic over 7.5 min and hold for 1.5 min
before returning to initial conditions in 0.5 min.
Time: 10 min

Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (150 - 850 amu)
Source: Electrospray (negative)
Capillary Voltage (kV) = 3.00
Cone Voltage (V) = 15.00
Cone Gas Flow (l/hr) = 100
Desolvation Gas Flow (l/hr) = 750

Figure 2: M2PFOA; LC/MS/MS Data (Selected MRM Transitions)



Conditions for Figure 2:

Injection: Direct loop injection
 10 μl (500 ng/ml M2PFOA)

Mobile phase: Isocratic 80% MeOH / 20% H₂O

Flow: 300 $\mu\text{l}/\text{min}$

MS Parameters

Collision Gas (mbar) = 3.39e-3
 Collision Energy (eV) = 10

Reagent

LCMPFDA_00012

R: SBC 12/21/16



814255

ID: LCMPPFDA_00012

Exp: 09/30/21 Prpd: SBC

13C2-Perfluorodecanoic acid




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: MPFDA **LOT NUMBER:** MPFDA0916
COMPOUND: Perfluoro-n-[1,2-¹³C₂]decanoic acid

STRUCTURE: **CAS #:** Not available



MOLECULAR FORMULA: ¹³C₂¹²C₈HF₁₉O₂
CONCENTRATION: 50 ± 2.5 µg/ml

MOLECULAR WEIGHT: 516.07
SOLVENT(S): Methanol
Water (<1%)

CHEMICAL PURITY: >98%

ISOTOPIC PURITY: ≥99% ¹³C
(1,2-¹³C₂)

LAST TESTED: (mm/dd/yyyy) 09/30/2016

EXPIRY DATE: (mm/dd/yyyy) 09/30/2021

RECOMMENDED STORAGE: Store ampoule in a cool, dark place

DOCUMENTATION/ DATA ATTACHED:

Figure 1: LC/MS Data (TIC and Mass Spectrum)

Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent conversion of the carboxylic acid to the methyl ester.
- Contains < 0.1% of ¹³C₁-PFNA.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By:
B.G. Chríttim

Date: 10/07/2016
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: MPFDA; LC/MS Data (TIC and Mass Spectrum)



Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions


Column: Acquity UPLC BEH Shield RP₁₈
1.7 μm, 2.1 x 100 mm
Mobile phase: Gradient
Start: 50% (80:20 MeOH:ACN) / 50% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 90% organic over 7 min and hold for 1.5 min
before returning to initial conditions in 0.5 min.
Time: 10 min

Flow: 300 μl/min

MS Parameters

Experiment: Full Scan (225 - 850 amu)
Source: Electrospray (negative)
Capillary Voltage (kV) = 2.00
Cone Voltage (V) = 15.00
Cone Gas Flow (l/hr) = 50
Desolvation Gas Flow (l/hr) = 750

Figure 2: MPFDA; LC/MS/MS Data (Selected MRM Transitions)

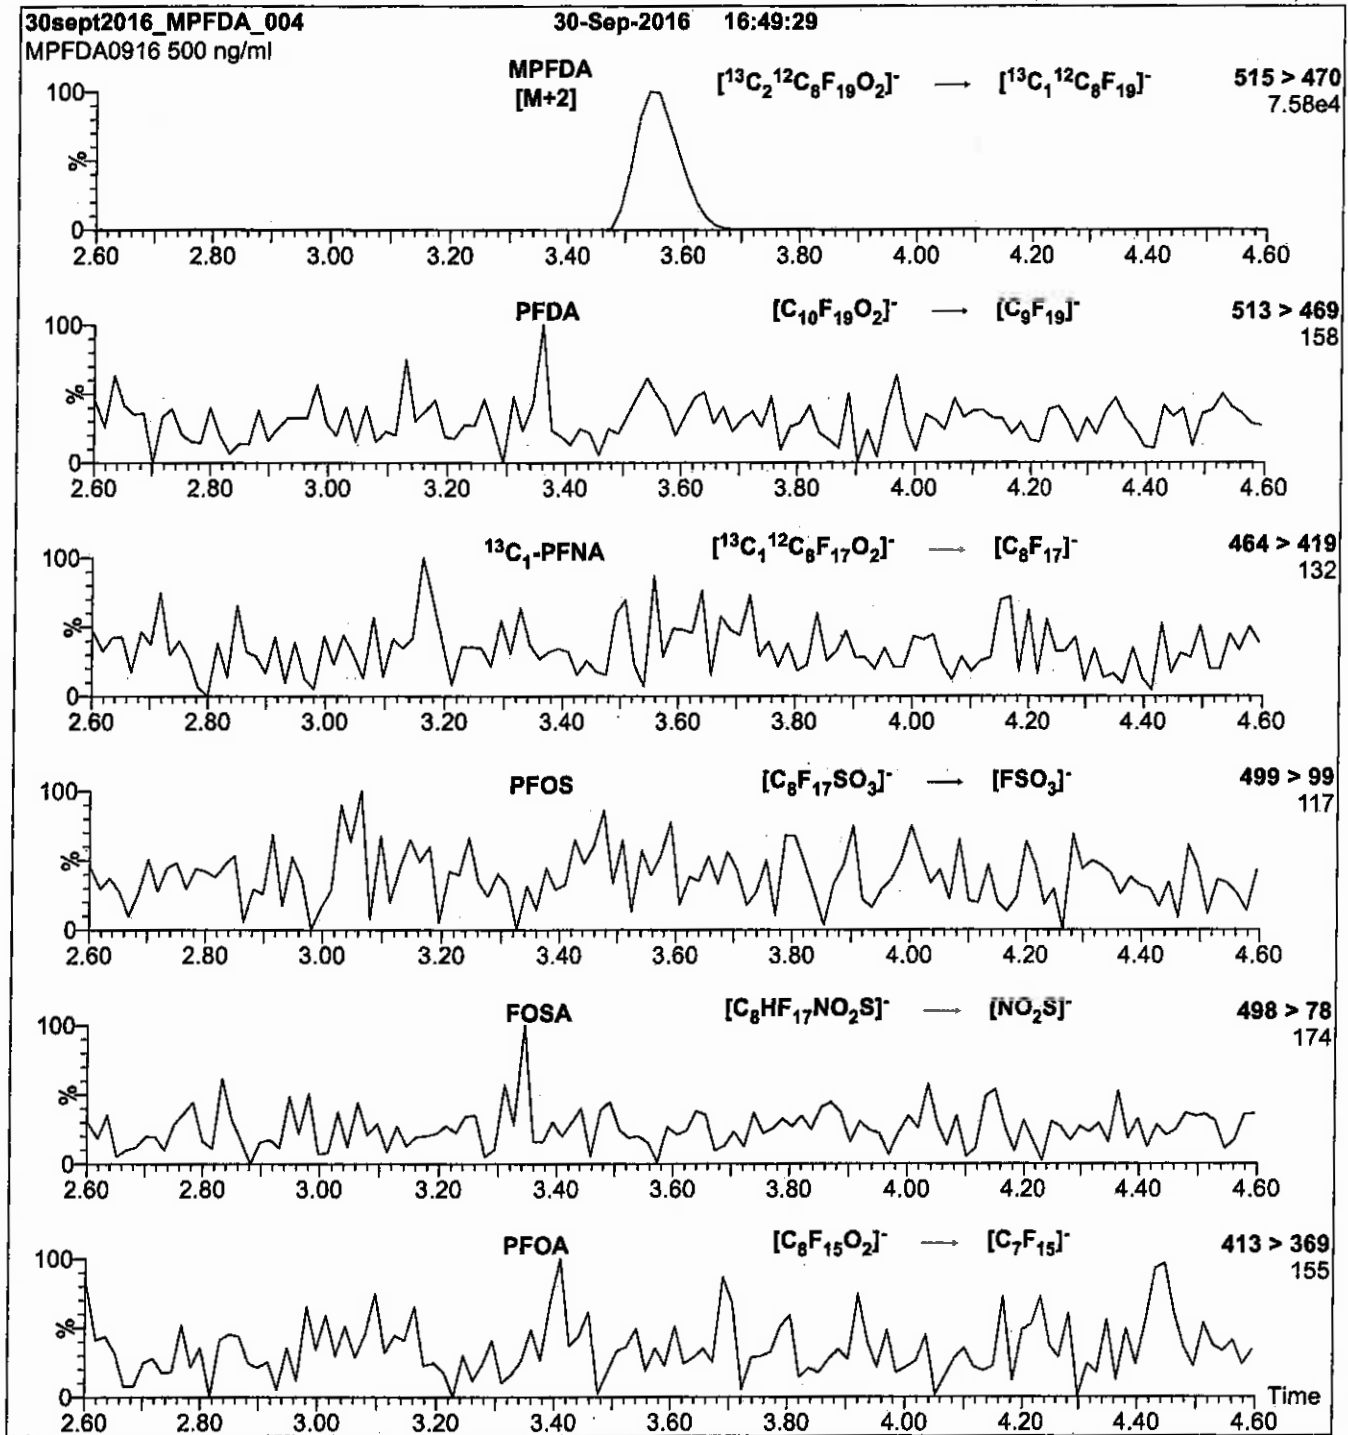

Conditions for Figure 2:

Injection: Direct loop injection
10 μ l (500 ng/ml MPFDA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
(both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.31e-3
Collision Energy (eV) = 13

Reagent

LCMPFHxA_00013

R: SBC 12/21/16



814258
ID: LCMPFHxA_00013
Exp: 04/08/21 Ppdt. SBC
13C2-Perfluorohexanoic ac



WELLINGTON LABORATORIES


CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: MPFHxA
COMPOUND: Perfluoro-n-[1,2-¹³C₂]hexanoic acid

LOT NUMBER: MPFHxA0416

STRUCTURE:

CAS #: Not available

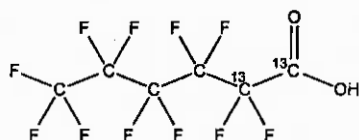

MOLECULAR FORMULA: ¹³C₂¹²C₄HF₁₁O₂
CONCENTRATION: 50 ± 2.5 µg/ml

MOLECULAR WEIGHT: 316.04
SOLVENT(S): Methanol
Water (<1%)

CHEMICAL PURITY: >98%

ISOTOPIC PURITY: ≥99%¹³C
(1,2-¹³C₂)

LAST TESTED: (mm/dd/yyyy) 04/08/2016

EXPIRY DATE: (mm/dd/yyyy) 04/08/2021

RECOMMENDED STORAGE: Store ampoule in a cool, dark place

DOCUMENTATION/ DATA ATTACHED:

- Figure 1: LC/MS Data (TIC and Mass Spectrum)
- Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent conversion of the carboxylic acid to the methyl ester.
- Contains < 0.1% of perfluoro-n-hexanoic acid and ~ 0.3% of perfluoro-n-octanoic acid.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By:
B.G. Chittim

Date: 04/29/2016
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: MPFHxA; LC/MS Data (TIC and Mass Spectrum)



Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
 1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
 Start: 50% (80:20 MeOH:ACN) / 50% H₂O
 (both with 10 mM NH₄OAc buffer)
 Ramp to 90% organic over 7.5 min and hold for 1.5 min
 before returning to initial conditions over 0.5 min.
 Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (150 - 850 amu)

Source: Electrospray (negative)
 Capillary Voltage (kV) = 2.00
 Cone Voltage (V) = 15.00
 Cone Gas Flow (l/hr) = 100
 Desolvation Gas Flow (l/hr) = 750

Figure 2: MPFHxA; LC/MS/MS Data (Selected MRM Transitions)



Conditions for Figure 2:

Injection: Direct loop injection
10 μ l (500 ng/ml MPFHxA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
(both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.39e-3
Collision Energy (eV) = 10

Reagent

LCMPFHxA_00015

r: 5/10/17 skd



WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: MPFHxA
COMPOUND: Perfluoro-n-[1,2-¹³C₂]hexanoic acid

LOT NUMBER: MPFHxA1116

STRUCTURE:

CAS #: Not available



MOLECULAR FORMULA: ¹³C₂¹²C₄HF₁₁O₂
CONCENTRATION: 50 ± 2.5 µg/ml

MOLECULAR WEIGHT: 316.04
SOLVENT(S): Methanol
Water (<1%)

CHEMICAL PURITY: >98%
LAST TESTED: (mm/dd/yyyy) 11/22/2016

ISOTOPIC PURITY: ≥99% ¹³C
(1,2-¹³C₂)

EXPIRY DATE: (mm/dd/yyyy) 11/22/2021
RECOMMENDED STORAGE: Store ampoule in a cool, dark place


DOCUMENTATION/ DATA ATTACHED:

- Figure 1: LC/MS Data (TIC and Mass Spectrum)
- Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent conversion of the carboxylic acid to the methyl ester.
- Contains < 0.1% of perfluoro-n-hexanoic acid and ~ 0.3% of perfluoro-n-octanoic acid.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: 
B.G. Chittim

Date: 12/13/2016
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:


Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: MPFHxA; LC/MS Data (TIC and Mass Spectrum)

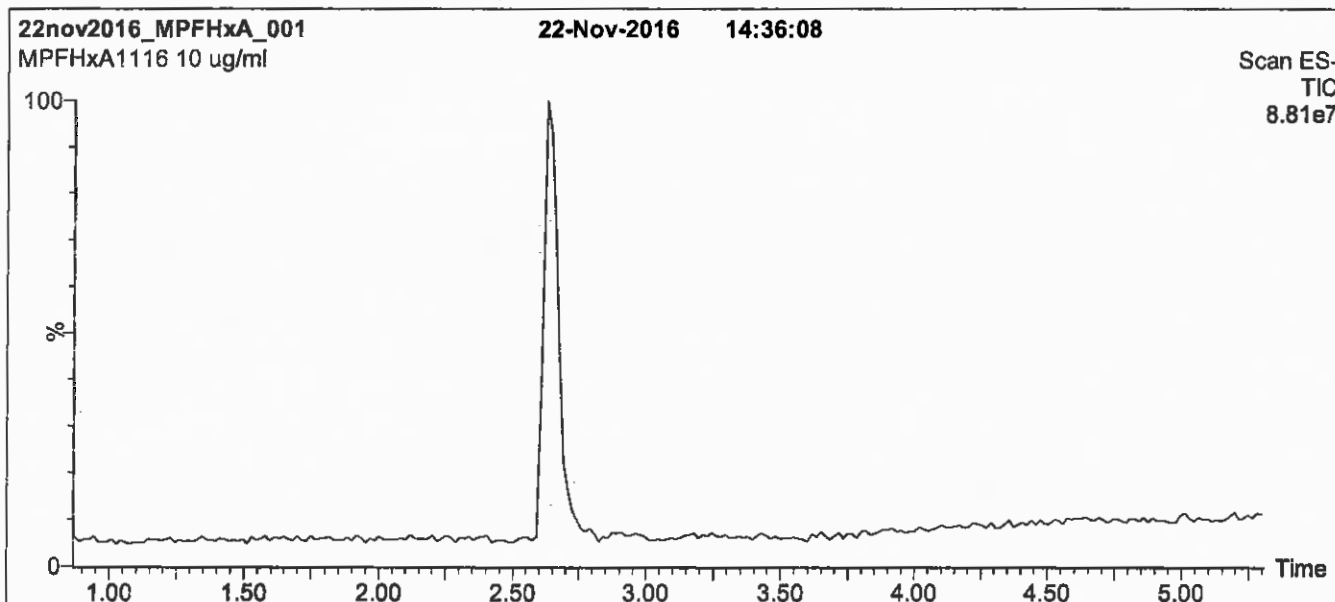

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm


Mobile phase: Gradient
Start: 40% (80:20 MeOH:ACN) / 60% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 90% organic over 7 min and hold for 2 min
before returning to initial conditions over 0.5 min.
Time: 10 min

Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (150 - 850 amu)
Source: Electrospray (negative)
Capillary Voltage (kV) = 2.00
Cone Voltage (V) = 15.00
Cone Gas Flow (l/hr) = 100
Desolvation Gas Flow (l/hr) = 750

Figure 2: MPFHxA; LC/MS/MS Data (Selected MRM Transitions)

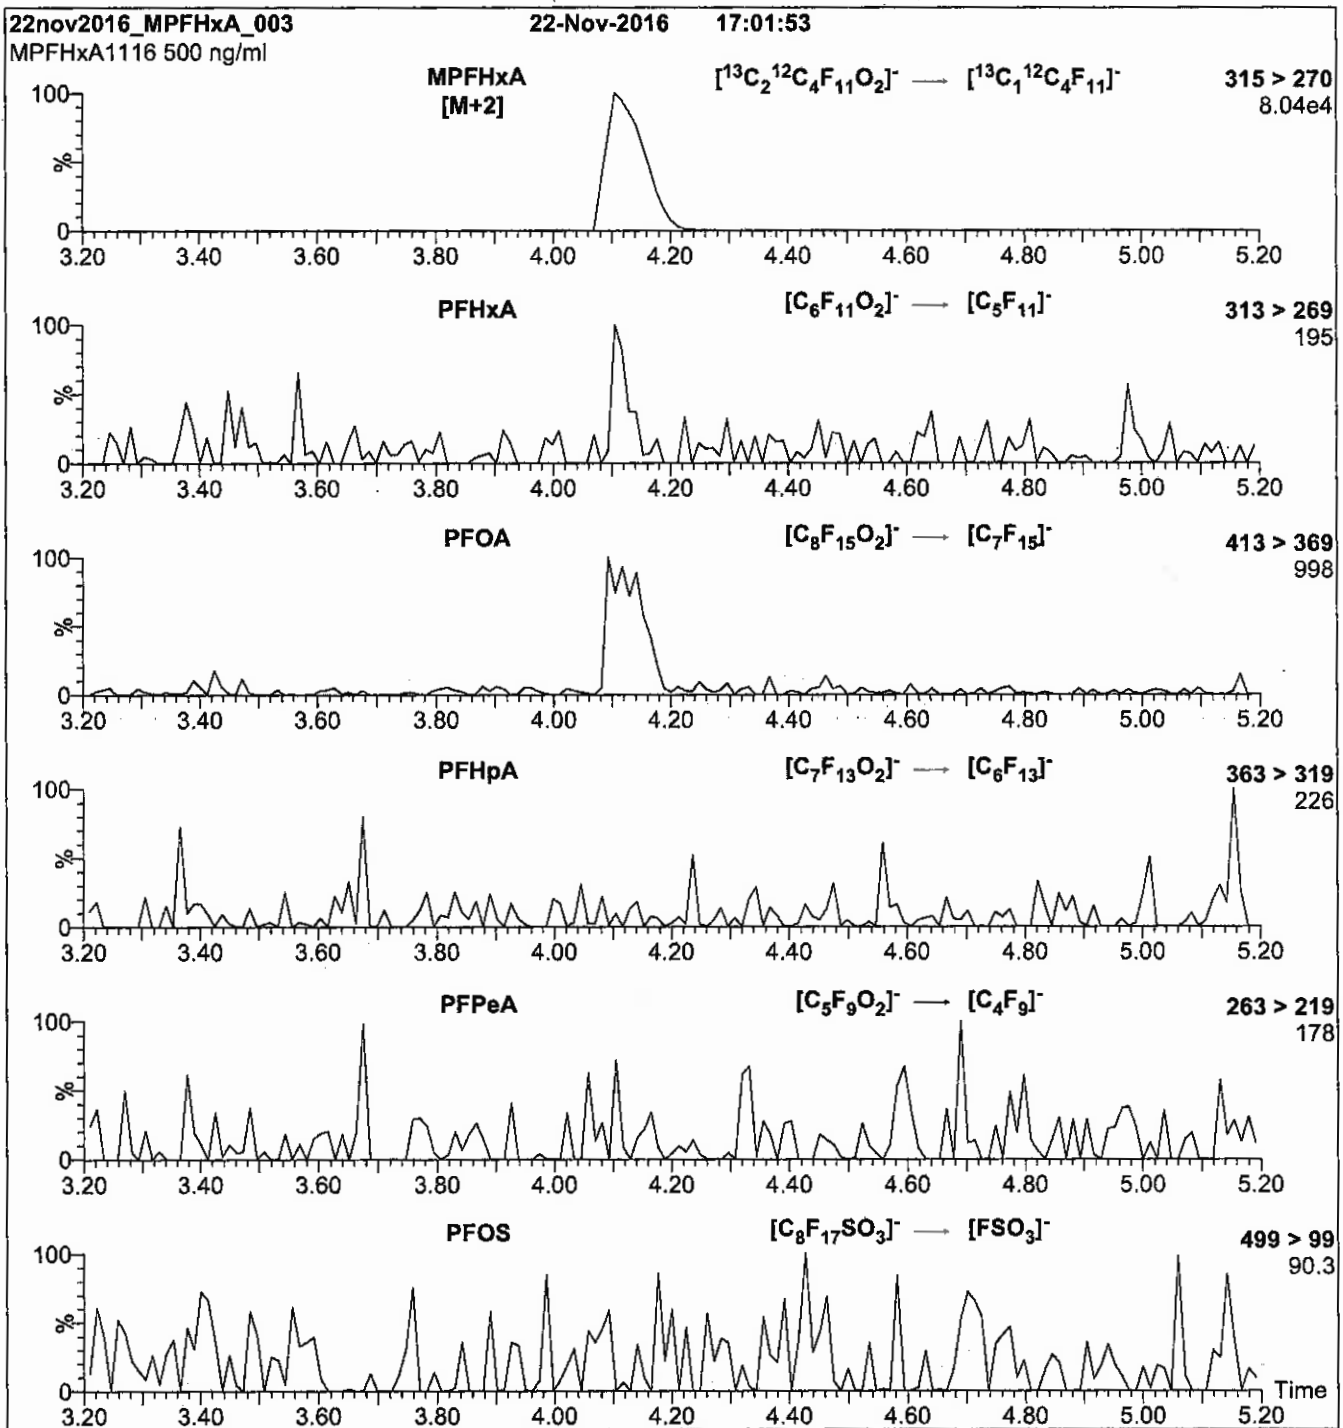

Conditions for Figure 2:

Injection: Direct loop injection
10 μ l (500 ng/ml MPFHxA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
(both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.46e-3
Collision Energy (eV) = 10

Reagent

LCMPFOS_00019

R: SBC 12/21/16



814253
ID: LCMPFOS_00019
Exp: 08/03/21 Ppfd: SBC
13C4-Perfluorooctanesulfo




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: MPFOS **LOT NUMBER:** MPFOS0816
COMPOUND: Sodium perfluoro-1-[1,2,3,4-¹³C₄]octanesulfonate

STRUCTURE: **CAS #:** Not available



MOLECULAR FORMULA: ¹³C₄¹²C₄F₁₇SO₃Na **MOLECULAR WEIGHT:** 526.08
CONCENTRATION: 50.0 ± 2.5 µg/ml (Na salt) **SOLVENT(S):** Methanol
47.8 ± 2.4 µg/ml (MPFOS anion)
CHEMICAL PURITY: >98% **ISOTOPIC PURITY:** ≥99% ¹³C
LAST TESTED: (mm/dd/yyyy) 08/03/2016 (1,2,3,4-¹³C₄)
EXPIRY DATE: (mm/dd/yyyy) 08/03/2021
RECOMMENDED STORAGE: Store ampoule in a cool, dark place


DOCUMENTATION/ DATA ATTACHED:

Figure 1: LC/MS Data (TIC and Mass Spectrum)
Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains ~ 0.8% Sodium perfluoro-1-[1,2,3-¹³C₃]heptanesulfonate.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: 
B.G. Chittim **Date:** 08/05/2016
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:


Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: MPFOS; LC/MS Data (TIC and Mass Spectrum)

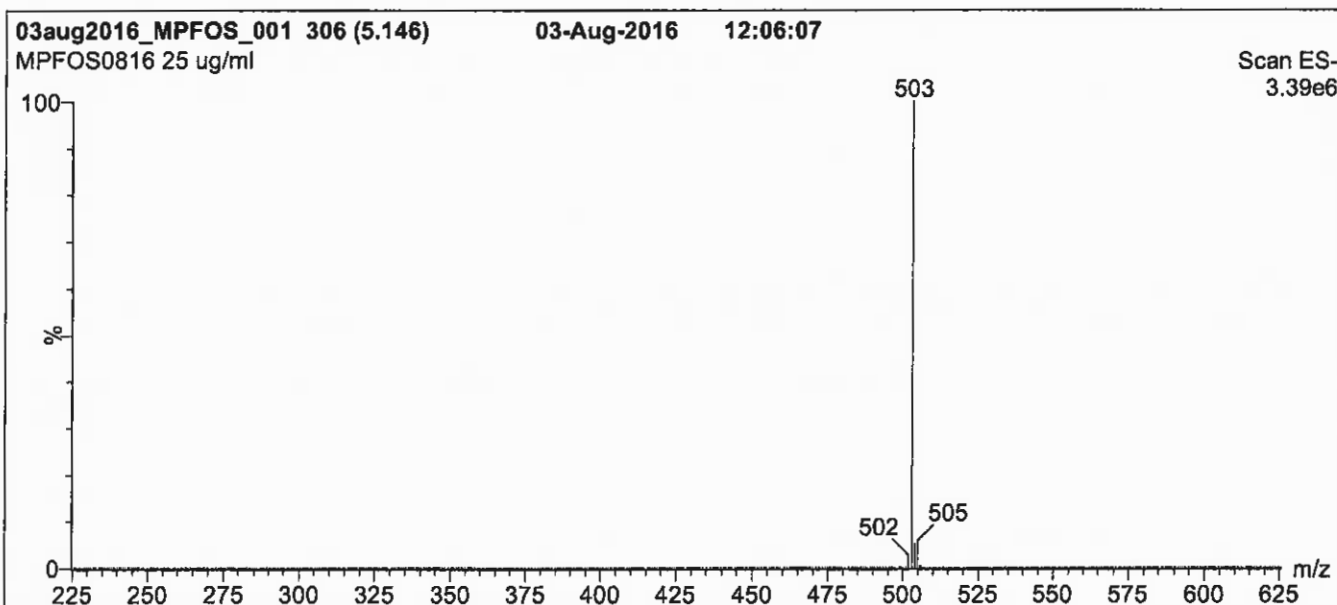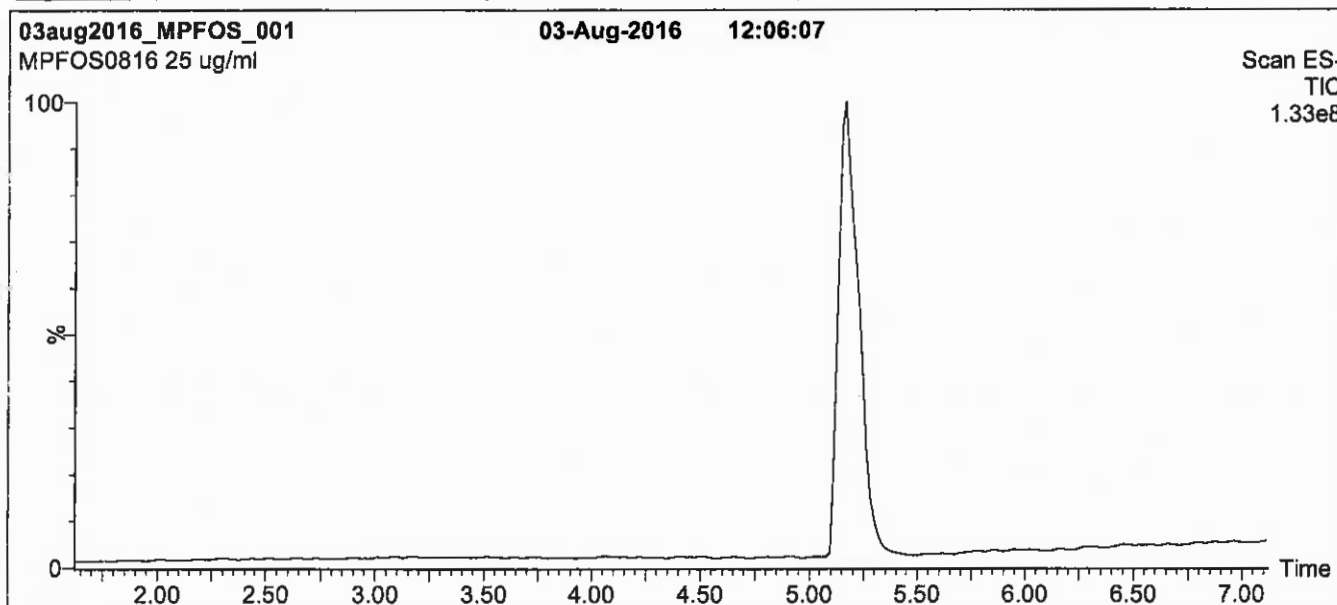

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
Start: 45% (80:20 MeOH:ACN) / 55% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 90% organic over 7 min and hold for 1.5 min
before returning to initial conditions in 0.5 min.
Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (225 - 850 amu)

Source: Electrospray (negative)
Capillary Voltage (kV) = 3.00
Cone Voltage (V) = 60.00
Cone Gas Flow (l/hr) = 50
Desolvation Gas Flow (l/hr) = 750

Figure 2: MPFOS; LC/MS/MS Data (Selected MRM Transitions)



Conditions for Figure 2:

Injection: Direct loop injection
10 μl (500 ng/ml MPFOS)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H_2O
(both with 10 mM NH_4OAc buffer)

Flow: 300 $\mu\text{l}/\text{min}$

MS Parameters

Collision Gas (mbar) = 3.46e-3
Collision Energy (eV) = 40

Reagent

LCMPFOS_00021

r: 5/6/17 SKV




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: MPFOS **LOT NUMBER:** MPFOS1216
COMPOUND: Sodium perfluoro-1-[1,2,3,4-¹³C₄]octanesulfonate

STRUCTURE: **CAS #:** Not available



MOLECULAR FORMULA:	¹³ C ₄ ¹² C ₄ F ₁₇ SO ₃ Na	MOLECULAR WEIGHT:	526.08
CONCENTRATION:	50.0 ± 2.5 µg/ml (Na salt) 47.8 ± 2.4 µg/ml (MPFOS anion)	SOLVENT(S):	Methanol
CHEMICAL PURITY:	>98%	ISOTOPIC PURITY:	≥99% ¹³ C (1,2,3,4- ¹³ C ₄)
LAST TESTED: (mm/dd/yyyy)	12/12/2016		
EXPIRY DATE: (mm/dd/yyyy)	12/12/2021		
RECOMMENDED STORAGE:	Store ampoule in a cool, dark place		


DOCUMENTATION/ DATA ATTACHED:

- Figure 1: LC/MS Data (TIC and Mass Spectrum)
- Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains ~ 0.8% Sodium perfluoro-1-[1,2,3-¹³C₃]heptanesulfonate.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: 
B.G. Chittim Date: 12/14/2016
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: MPFOS; LC/MS Data (TIC and Mass Spectrum)

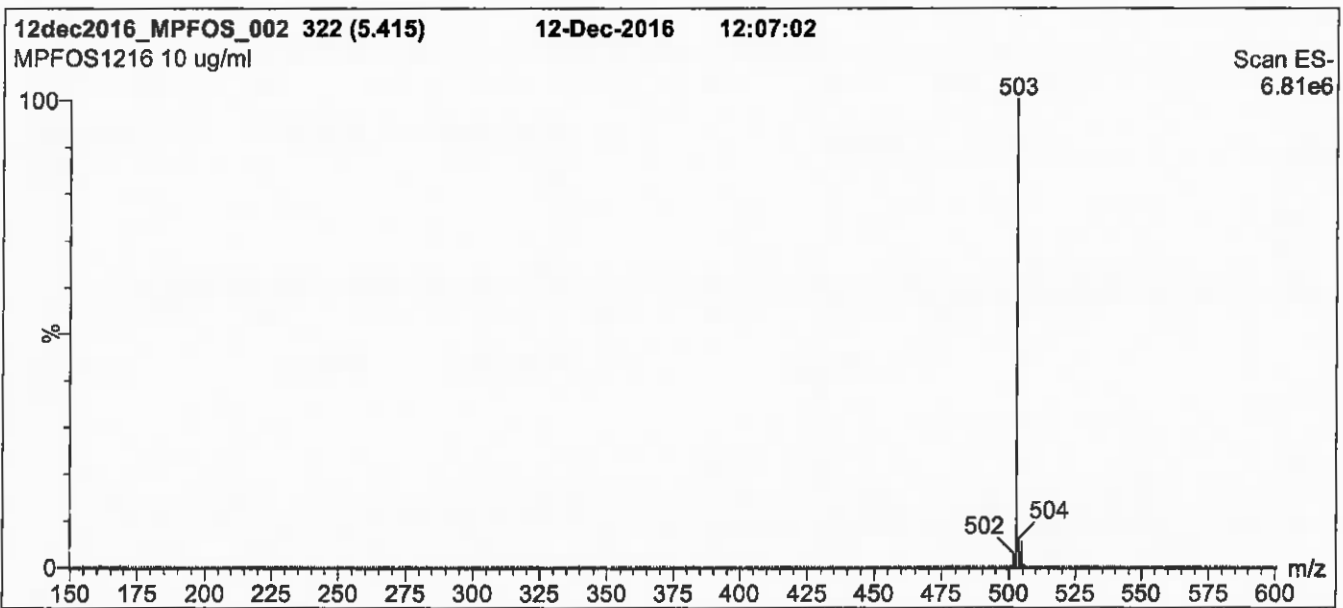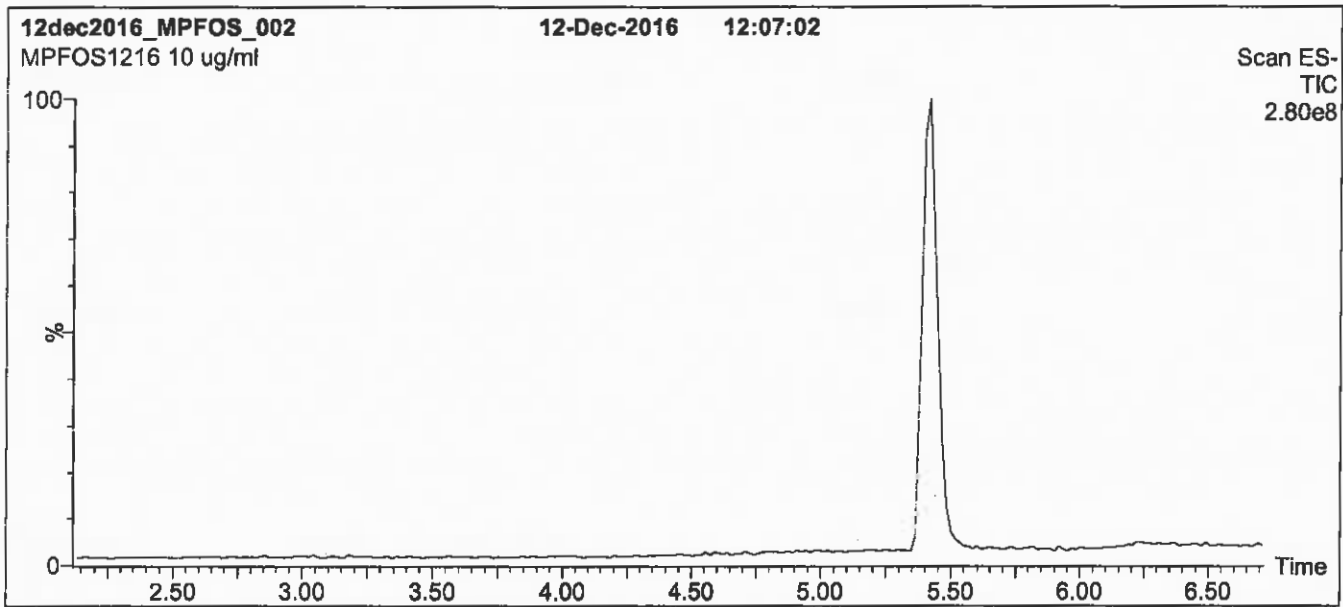

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
 1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
 Start: 50% (80:20 MeOH:ACN) / 50% H₂O
 (both with 10 mM NH₄OAc buffer)
 Ramp to 85% organic over 7.5 min and hold for 1.5 min
 before returning to initial conditions in 0.5 min.
 Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (150 - 850 amu)

Source: Electrospray (negative)
 Capillary Voltage (kV) = 3.00
 Cone Voltage (V) = 60.00
 Cone Gas Flow (l/hr) = 50
 Desolvation Gas Flow (l/hr) = 750

Figure 2: MPFOS; LC/MS/MS Data (Selected MRM Transitions)

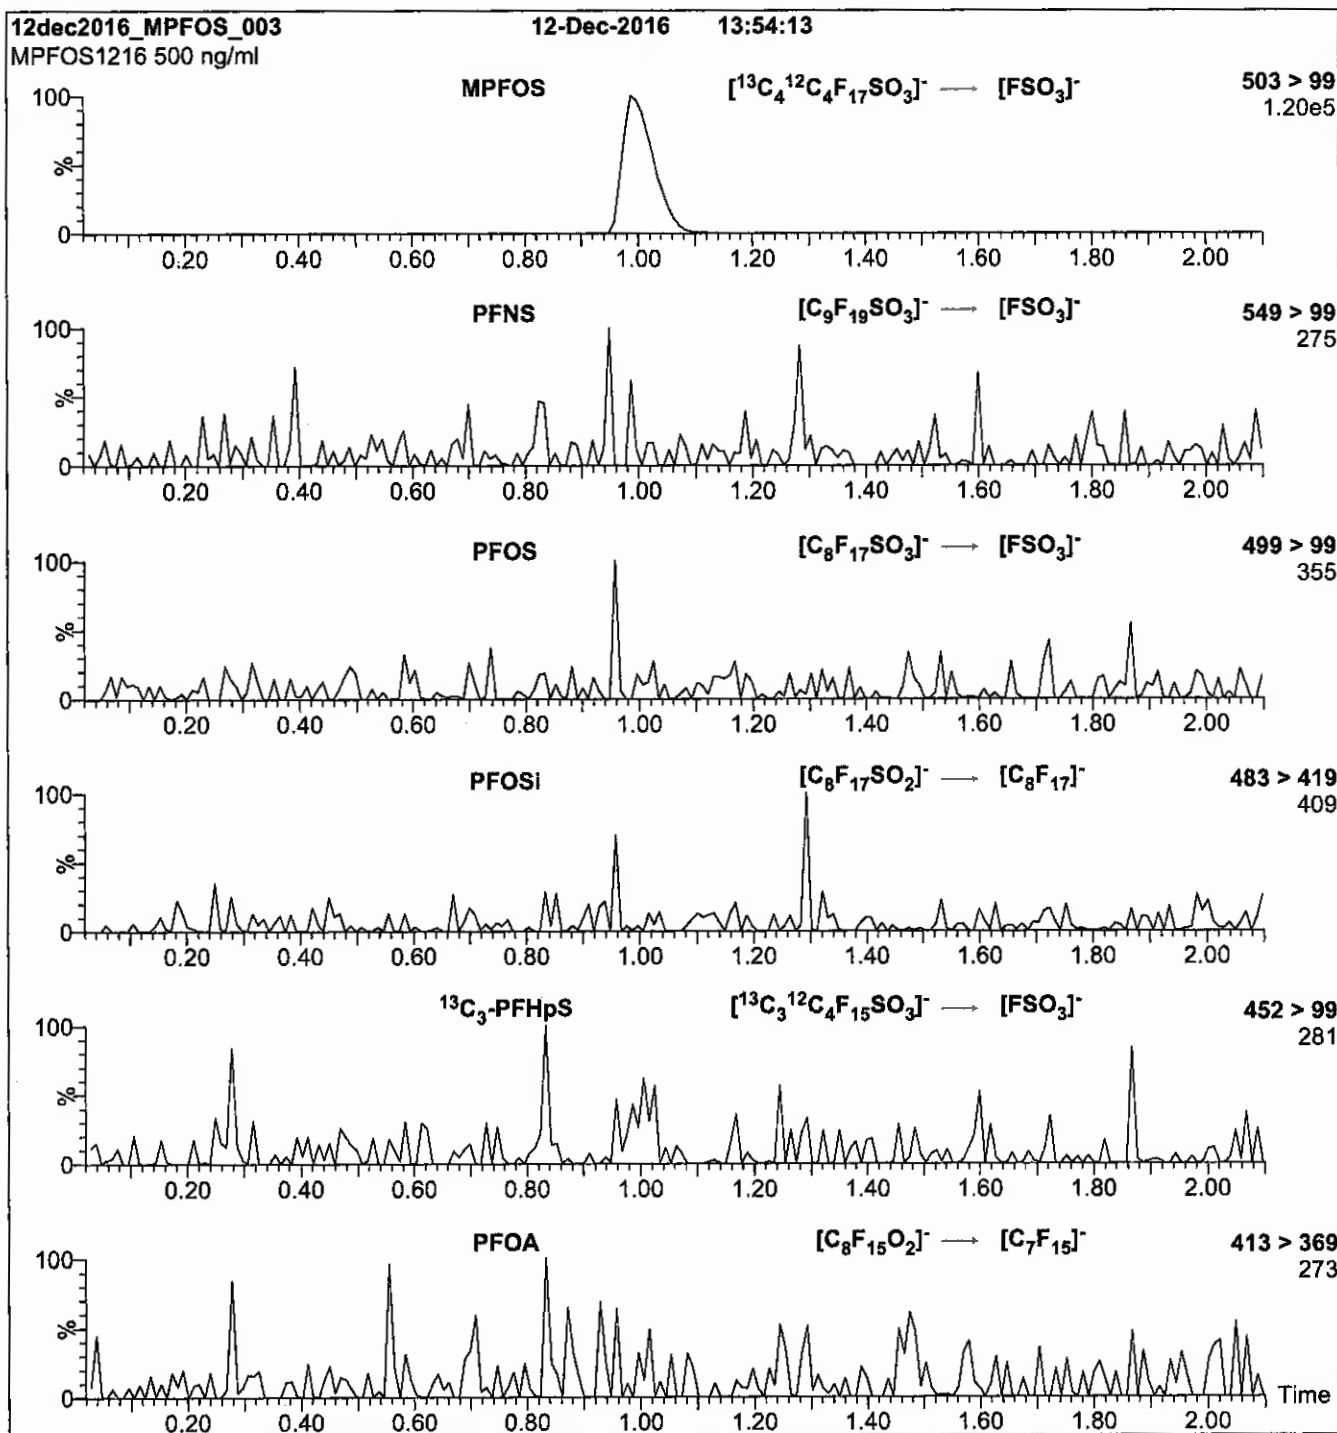

Conditions for Figure 2:

Injection: Direct loop injection
10 μl (500 ng/ml MPFOS)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H_2O
(both with 10 mM NH_4OAc buffer)

Flow: 300 $\mu\text{l}/\text{min}$

MS Parameters

Collision Gas (mbar) = 3.35e-3
Collision Energy (eV) = 40

Method 537 DOD

Perfluorinated Alkyl Acids (LC/MS)
by Method 537 DOD

FORM II
LCMS SURROGATE RECOVERY

Lab Name: TestAmerica Sacramento

Job No.: 320-35046-1

SDG No.: _____

Matrix: Water

Level: Low

GC Column (1): GeminiC18 3 ID: 3 (mm)

Client Sample ID	Lab Sample ID	PFHxA #	PFDA #
WGNA-011118-RW-310 3	320-35046-1	92	97
WGNA-011118-FRB-31 03	320-35046-2	99	104
WGNA-011118-RW-068 3	320-35046-3	87	96
WGNA-011118-FRB-06 83	320-35046-4	96	99
NAWC-011118-RW-139	320-35046-5	92	97
NAWC-011118-FRB-13 9	320-35046-6	90	96
WGNA-011118-DUP-18	320-35046-7	92	101
NAWC-011118-RW-098	320-35046-8	91	102
NAWC-011118-FRB-09 8	320-35046-9	93	94
NAWC-011118-RW-180	320-35046-10	92	100
NAWC-011118-FRB-18 0	320-35046-11	99	100
NAWC-011118-RW-179	320-35046-12	93	101
NAWC-011118-FRB-17 9	320-35046-13	95	95
NAWC-011118-RW-303	320-35046-14	91	103
NAWC-011118-FRB-30 3	320-35046-15	92	102
WGNA-011118-RW-340 9	320-35046-16	91	100
WGNA-011118-FRB-34 09	320-35046-17	99	101
WGNA-011118-RW-322 0	320-35046-18	85	97
WGNA-011118-FRB-32 20	320-35046-19	95	101
	MB 320-205489/1-A	95	101
	LLCS 320-205489/2-A	103	104
NAWC-011118-RW-179 LMS	320-35046-12 LMS	94	108
NAWC-011118-RW-179 LMSD	320-35046-12 LMSD	88	97

PFHxA = 13C2 PFHxA
PFDA = 13C2 PFDA

QC LIMITS
70-130
70-130

Column to be used to flag recovery values

FORM III
LCMS LOW LEVEL CONTROL SAMPLE RECOVERY

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1

SDG No.: _____

Matrix: Water Level: Low Lab File ID: 2018.01.31_537A_020.d

Lab ID: LLCS 320-205489/2-A Client ID: _____

COMPOUND	SPIKE ADDED (ng/L)	LLCS CONCENTRATION (ng/L)	LLCS % REC	QC LIMITS REC	#
Perfluorooctanesulfonic acid (PFOS)	40.0	38.5 J	96	50-150	M
Perfluorooctanoic acid (PFOA)	20.0	20.1	100	50-150	
Perfluorononanoic acid (PFNA)	20.0	19.9 J	99	50-150	
Perfluorohexanesulfonic acid (PFHxS)	30.0	29.0 J	97	50-150	
Perfluoroheptanoic acid (PFHpA)	10.0	11.1	111	50-150	
Perfluorobutanesulfonic acid (PFBS)	90.0	91.7	102	50-150	

Column to be used to flag recovery and RPD values

FORM III
LCMS LOW LEVEL MATRIX SPIKE RECOVERY

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Matrix: Water Level: Low Lab File ID: 2018.01.31_537A_035.d
 Lab ID: 320-35046-12 LMS Client ID: NAWC-011118-RW-179 LMS

COMPOUND	SPIKE ADDED (ng/L)	SAMPLE CONCENTRATION (ng/L)	LMS CONCENTRATION (ng/L)	LMS % REC	QC LIMITS REC	#
Perfluorooctanesulfonic acid (PFOS)	39.2	18 J	54.3	94	50-150	M
Perfluorooctanoic acid (PFOA)	19.6	18 J	37.3	96	50-150	
Perfluorononanoic acid (PFNA)	19.6	19 U	21.2 J	109	50-150	
Perfluorohexanesulfonic acid (PFHxS)	29.4	6.2 J	34.9	98	50-150	
Perfluoroheptanoic acid (PFHpA)	9.79	4.7 J	14.9	104	50-150	
Perfluorobutanesulfonic acid (PFBS)	88.1	34 U	90.6	103	50-150	

Column to be used to flag recovery and RPD values

FORM III
LCMS LOW LEVEL MATRIX SPIKE DUPLICATE RECOVERY

Lab Name: TestAmerica Sacramento

Job No.: 320-35046-1

SDG No.: _____

Matrix: Water Level: Low

Lab File ID: 2018.01.31_537A_036.d

Lab ID: 320-35046-12 LMSD

Client ID: NAWC-011118-RW-179 LMSD

COMPOUND	SPIKE ADDED (ng/L)	LMSD CONCENTRATION (ng/L)	LMSD % REC	% RPD	QC LIMITS		#
					RPD	REC	
Perfluorooctanesulfonic acid (PFOS)	37.9	51.8	90	5	50	50-150	M
Perfluorooctanoic acid (PFOA)	19.0	35.1	88	6	50	50-150	
Perfluorononanoic acid (PFNA)	18.9	19.6 J	104	8	50	50-150	
Perfluorohexanesulfonic acid (PFHxS)	28.4	33.0	94	6	50	50-150	
Perfluoroheptanoic acid (PFHpA)	9.47	13.0	88	13	50	50-150	
Perfluorobutanesulfonic acid (PFBS)	85.3	84.3 J	99	7	50	50-150	

Column to be used to flag recovery and RPD values

FORM IV
LCMS METHOD BLANK SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Lab File ID: 2018.01.31_537A_019.d Lab Sample ID: MB 320-205489/1-A
 Matrix: Water Date Extracted: 01/24/2018 20:52
 Instrument ID: A8_N Date Analyzed: 01/31/2018 12:02
 Level: (Low/Med) Low

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES:

CLIENT SAMPLE ID	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED
	LLCS 320-205489/2-A	2018.01.31_537A_020.d	01/31/2018 12:07
WGNA-011118-RW-3103	320-35046-1	2018.01.31_537A_021.d	01/31/2018 12:12
WGNA-011118-FRB-3103	320-35046-2	2018.01.31_537A_022.d	01/31/2018 12:16
WGNA-011118-RW-0683	320-35046-3	2018.01.31_537A_023.d	01/31/2018 12:21
WGNA-011118-FRB-0683	320-35046-4	2018.01.31_537A_024.d	01/31/2018 12:26
NAWC-011118-RW-139	320-35046-5	2018.01.31_537A_025.d	01/31/2018 12:30
NAWC-011118-FRB-139	320-35046-6	2018.01.31_537A_026.d	01/31/2018 12:35
WGNA-011118-DUP-18	320-35046-7	2018.01.31_537A_027.d	01/31/2018 12:40
NAWC-011118-RW-098	320-35046-8	2018.01.31_537A_028.d	01/31/2018 12:44
NAWC-011118-FRB-098	320-35046-9	2018.01.31_537A_031.d	01/31/2018 12:58
NAWC-011118-RW-180	320-35046-10	2018.01.31_537A_032.d	01/31/2018 13:03
NAWC-011118-FRB-180	320-35046-11	2018.01.31_537A_033.d	01/31/2018 13:08
NAWC-011118-RW-179	320-35046-12	2018.01.31_537A_034.d	01/31/2018 13:12
NAWC-011118-RW-179 LMS	320-35046-12 LMS	2018.01.31_537A_035.d	01/31/2018 13:17
NAWC-011118-RW-179 LMSD	320-35046-12 LMSD	2018.01.31_537A_036.d	01/31/2018 13:22
NAWC-011118-FRB-179	320-35046-13	2018.01.31_537A_037.d	01/31/2018 13:26
NAWC-011118-RW-303	320-35046-14	2018.01.31_537A_038.d	01/31/2018 13:31
NAWC-011118-FRB-303	320-35046-15	2018.01.31_537A_039.d	01/31/2018 13:36
WGNA-011118-RW-3409	320-35046-16	2018.01.31_537A_040.d	01/31/2018 13:40
WGNA-011118-FRB-3409	320-35046-17	2018.01.31_537A_043.d	01/31/2018 13:54
WGNA-011118-RW-3220	320-35046-18	2018.01.31_537A_044.d	01/31/2018 13:59
WGNA-011118-FRB-3220	320-35046-19	2018.01.31_537A_045.d	01/31/2018 14:04

FORM VIII
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Instrument ID: A8_N Calibration Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3(mm) Calibration End Date: 11/03/2017 14:01
 Calibration ID: 36012

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
INITIAL CALIBRATION MEAN AREA AND MEAN RT	1535518	1.91	3276559	2.15		
UPPER LIMIT	2303277	2.41	4914839	2.65		
LOWER LIMIT	767759	1.41	1638280	1.65		
LAB SAMPLE ID	CLIENT SAMPLE ID					
CCVL 320-192908/11	1586829	1.91	3305852	2.15		
ICV 320-192908/13	1512045	1.90	3433628	2.14		
CCVL 320-206407/1	1570514	1.84	3320314	2.09		
CCV 320-206408/14 CCVIS	1524185	1.82	3201796	2.07		
MB 320-205489/1-A	1514419	1.83	3315723	2.08		
LLCS 320-205489/2-A	1437381	1.83	3330580	2.08		
320-35046-1	WGNA-011118-RW-3103	1511383	1.81	3351158	2.07	
320-35046-2	WGNA-011118-FRB-3103	1469356	1.82	3274315	2.08	
320-35046-3	WGNA-011118-RW-0683	1551777	1.81	3339406	2.07	
320-35046-4	WGNA-011118-FRB-0683	1427812	1.82	3143756	2.08	
320-35046-5	NAWC-011118-RW-139	1551998	1.82	3530101	2.07	
320-35046-6	NAWC-011118-FRB-139	1503114	1.82	3436163	2.07	
320-35046-7	WGNA-011118-DUP-18	1522059	1.82	3381704	2.07	
320-35046-8	NAWC-011118-RW-098	1495096	1.82	3259129	2.07	
CCV 320-206408/26 CCVIS	1463849	1.81	3172960	2.07		
CCV 320-206410/26 CCVIS	1463849	1.81	3172960	2.07		
320-35046-9	NAWC-011118-FRB-098	1546187	1.82	3372040	2.07	
320-35046-10	NAWC-011118-RW-180	1537799	1.81	3430335	2.07	
320-35046-11	NAWC-011118-FRB-180	1532214	1.82	3442464	2.07	
320-35046-12	NAWC-011118-RW-179	1472481	1.82	3387330	2.07	
320-35046-12 LMS	NAWC-011118-RW-179 LMS	1527332	1.81	3460115	2.06	
320-35046-12 LMSD	NAWC-011118-RW-179 LMSD	1566820	1.81	3420572	2.07	
320-35046-13	NAWC-011118-FRB-179	1558738	1.82	3496002	2.07	
320-35046-14	NAWC-011118-RW-303	1470595	1.81	3380751	2.06	
320-35046-15	NAWC-011118-FRB-303	1560240	1.81	3459417	2.07	
320-35046-16	WGNA-011118-RW-3409	1548213	1.81	3403494	2.07	
CCV 320-206410/38 CCVIS	1511534	1.81	3175124	2.07		

13PFOA = 13C2-PFOA

PFOS = 13C4 PFOS

Area Limit = 50%-150% of internal standard area
 RT Limit = ± 0.5 minutes of internal standard RT

Column used to flag values outside QC limits

FORM VIII
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Instrument ID: A8_N Calibration Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3(mm) Calibration End Date: 11/03/2017 14:01
 Calibration ID: 36012

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
INITIAL CALIBRATION MEAN AREA AND MEAN RT	1535518	1.91	3276559	2.15		
UPPER LIMIT	2303277	2.41	4914839	2.65		
LOWER LIMIT	767759	1.41	1638280	1.65		
LAB SAMPLE ID	CLIENT SAMPLE ID					
CCV 320-206412/38 CCVIS		1511534	1.81	3175124	2.07	
320-35046-17	WGNA-011118-FRB-3409	1481492	1.82	3346629	2.07	
320-35046-18	WGNA-011118-RW-3220	1573796	1.81	3375758	2.06	
320-35046-19	WGNA-011118-FRB-3220	1520384	1.81	3387119	2.06	
CCV 320-206412/43 CCVIS		1503053	1.82	3253442	2.07	

13PFOA = 13C2-PFOA
 PFOS = 13C4 PFOS

Area Limit = 50%-150% of internal standard area
 RT Limit = ± 0.5 minutes of internal standard RT

Column used to flag values outside QC limits

FORM VIII
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Sample No.: CCV 320-206408/14 Date Analyzed: 01/31/2018 11:53
 Instrument ID: A8_N GC Column: GeminiC18 3x100 ID: 3 (mm)
 Lab File ID (Standard): 2018.01.31_537A_017 Heated Purge: (Y/N) N
 Calibration ID: 36012

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	1524185	1.82	3201796	2.07		
UPPER LIMIT	2133859	2.32	4482514	2.57		
LOWER LIMIT	1066930	1.32	2241257	1.57		
LAB SAMPLE ID	CLIENT SAMPLE ID					
MB 320-205489/1-A		1514419	1.83	3315723	2.08	
LLCS 320-205489/2-A		1437381	1.83	3330580	2.08	
320-35046-1	WGNA-011118-RW-3103	1511383	1.81	3351158	2.07	
320-35046-2	WGNA-011118-FRB-3103	1469356	1.82	3274315	2.08	
320-35046-3	WGNA-011118-RW-0683	1551777	1.81	3339406	2.07	
320-35046-4	WGNA-011118-FRB-0683	1427812	1.82	3143756	2.08	
320-35046-5	NAWC-011118-RW-139	1551998	1.82	3530101	2.07	
320-35046-6	NAWC-011118-FRB-139	1503114	1.82	3436163	2.07	
320-35046-7	WGNA-011118-DUP-18	1522059	1.82	3381704	2.07	
320-35046-8	NAWC-011118-RW-098	1495096	1.82	3259129	2.07	

13PFOA = 13C2-PFOA
 PFOS = 13C4 PFOS

Area Limit = 70%-140% of internal standard area
 RT Limit = ± 0.5 minutes of internal standard RT

Column used to flag values outside QC limits

FORM VIII
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Sample No.: CCV 320-206408/26 Date Analyzed: 01/31/2018 12:49
 Instrument ID: A8_N GC Column: GeminiC18 3x100 ID: 3 (mm)
 Lab File ID (Standard): 2018.01.31_537A_029 Heated Purge: (Y/N) N
 Calibration ID: 36012

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	1463849	1.81	3172960	2.07		
UPPER LIMIT	2049389	2.31	4442144	2.57		
LOWER LIMIT	1024694	1.31	2221072	1.57		
LAB SAMPLE ID	CLIENT SAMPLE ID					
MB 320-205489/1-A		1514419	1.83	3315723	2.08	
LLCS 320-205489/2-A		1437381	1.83	3330580	2.08	
320-35046-1	WGNA-011118-RW-3103	1511383	1.81	3351158	2.07	
320-35046-2	WGNA-011118-FRB-3103	1469356	1.82	3274315	2.08	
320-35046-3	WGNA-011118-RW-0683	1551777	1.81	3339406	2.07	
320-35046-4	WGNA-011118-FRB-0683	1427812	1.82	3143756	2.08	
320-35046-5	NAWC-011118-RW-139	1551998	1.82	3530101	2.07	
320-35046-6	NAWC-011118-FRB-139	1503114	1.82	3436163	2.07	
320-35046-7	WGNA-011118-DUP-18	1522059	1.82	3381704	2.07	
320-35046-8	NAWC-011118-RW-098	1495096	1.82	3259129	2.07	

13PFOA = 13C2-PFOA

PFOS = 13C4 PFOS

Area Limit = 70%-140% of internal standard area

RT Limit = ± 0.5 minutes of internal standard RT

Column used to flag values outside QC limits

FORM VIII
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Sample No.: CCV 320-206410/26 Date Analyzed: 01/31/2018 12:49
 Instrument ID: A8_N GC Column: GeminiC18 3x100 ID: 3 (mm)
 Lab File ID (Standard): 2018.01.31_537A_029 Heated Purge: (Y/N) N
 Calibration ID: 36012

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	1463849	1.81	3172960	2.07		
UPPER LIMIT	2049389	2.31	4442144	2.57		
LOWER LIMIT	1024694	1.31	2221072	1.57		
LAB SAMPLE ID	CLIENT SAMPLE ID					
320-35046-9	NAWC-011118-FRB-098	1546187	1.82	3372040	2.07	
320-35046-10	NAWC-011118-RW-180	1537799	1.81	3430335	2.07	
320-35046-11	NAWC-011118-FRB-180	1532214	1.82	3442464	2.07	
320-35046-12	NAWC-011118-RW-179	1472481	1.82	3387330	2.07	
320-35046-12 LMS	NAWC-011118-RW-179 LMS	1527332	1.81	3460115	2.06	
320-35046-12 LMSD	NAWC-011118-RW-179 LMSD	1566820	1.81	3420572	2.07	
320-35046-13	NAWC-011118-FRB-179	1558738	1.82	3496002	2.07	
320-35046-14	NAWC-011118-RW-303	1470595	1.81	3380751	2.06	
320-35046-15	NAWC-011118-FRB-303	1560240	1.81	3459417	2.07	
320-35046-16	WGNA-011118-RW-3409	1548213	1.81	3403494	2.07	

13PFOA = 13C2-PFOA
 PFOS = 13C4 PFOS

Area Limit = 70%-140% of internal standard area
 RT Limit = ± 0.5 minutes of internal standard RT

Column used to flag values outside QC limits

FORM VIII
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Sample No.: CCV 320-206410/38 Date Analyzed: 01/31/2018 13:45
 Instrument ID: A8_N GC Column: GeminiC18 3x100 ID: 3 (mm)
 Lab File ID (Standard): 2018.01.31_537A_041 Heated Purge: (Y/N) N
 Calibration ID: 36012

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	1511534	1.81	3175124	2.07		
UPPER LIMIT	2116148	2.31	4445174	2.57		
LOWER LIMIT	1058074	1.31	2222587	1.57		
LAB SAMPLE ID	CLIENT SAMPLE ID					
320-35046-9	NAWC-011118-FRB-098	1546187	1.82	3372040	2.07	
320-35046-10	NAWC-011118-RW-180	1537799	1.81	3430335	2.07	
320-35046-11	NAWC-011118-FRB-180	1532214	1.82	3442464	2.07	
320-35046-12	NAWC-011118-RW-179	1472481	1.82	3387330	2.07	
320-35046-12 LMS	NAWC-011118-RW-179 LMS	1527332	1.81	3460115	2.06	
320-35046-12 LMSD	NAWC-011118-RW-179 LMSD	1566820	1.81	3420572	2.07	
320-35046-13	NAWC-011118-FRB-179	1558738	1.82	3496002	2.07	
320-35046-14	NAWC-011118-RW-303	1470595	1.81	3380751	2.06	
320-35046-15	NAWC-011118-FRB-303	1560240	1.81	3459417	2.07	
320-35046-16	WGNA-011118-RW-3409	1548213	1.81	3403494	2.07	

13PFOA = 13C2-PFOA
 PFOS = 13C4 PFOS

Area Limit = 70%-140% of internal standard area
 RT Limit = ± 0.5 minutes of internal standard RT

Column used to flag values outside QC limits

FORM VIII
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Sample No.: CCV 320-206412/38 Date Analyzed: 01/31/2018 13:45
 Instrument ID: A8_N GC Column: GeminiC18 3x100 ID: 3 (mm)
 Lab File ID (Standard): 2018.01.31_537A_041 Heated Purge: (Y/N) N
 Calibration ID: 36012

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	1511534	1.81	3175124	2.07		
UPPER LIMIT	2116148	2.31	4445174	2.57		
LOWER LIMIT	1058074	1.31	2222587	1.57		
LAB SAMPLE ID	CLIENT SAMPLE ID					
320-35046-17	WGNA-011118-FRB-3409	1481492	1.82	3346629	2.07	
320-35046-18	WGNA-011118-RW-3220	1573796	1.81	3375758	2.06	
320-35046-19	WGNA-011118-FRB-3220	1520384	1.81	3387119	2.06	

13PFOA = 13C2-PFOA
 PFOS = 13C4 PFOS

Area Limit = 70%-140% of internal standard area
 RT Limit = ± 0.5 minutes of internal standard RT

Column used to flag values outside QC limits

FORM VIII
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Sample No.: CCV 320-206412/43 Date Analyzed: 01/31/2018 14:08
 Instrument ID: A8_N GC Column: GeminiC18 3x100 ID: 3 (mm)
 Lab File ID (Standard): 2018.01.31_537A_046 Heated Purge: (Y/N) N
 Calibration ID: 36012

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	1503053	1.82	3253442	2.07		
UPPER LIMIT	2104274	2.32	4554819	2.57		
LOWER LIMIT	1052137	1.32	2277409	1.57		
LAB SAMPLE ID	CLIENT SAMPLE ID					
320-35046-17	WGNA-011118-FRB-3409	1481492	1.82	3346629	2.07	
320-35046-18	WGNA-011118-RW-3220	1573796	1.81	3375758	2.06	
320-35046-19	WGNA-011118-FRB-3220	1520384	1.81	3387119	2.06	

13PFOA = 13C2-PFOA
 PFOS = 13C4 PFOS

Area Limit = 70%-140% of internal standard area
 RT Limit = ± 0.5 minutes of internal standard RT

Column used to flag values outside QC limits

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: WGNA-011118-RW-3103 Lab Sample ID: 320-35046-1
 Matrix: Water Lab File ID: 2018.01.31_537A_021.d
 Analysis Method: 537 Date Collected: 01/11/2018 08:10
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 285.9(mL) Date Analyzed: 01/31/2018 12:12
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	10	J M	35	14	5.9
335-67-1	Perfluorooctanoic acid (PFOA)	12	J	17	7.0	2.4
375-95-1	Perfluorononanoic acid (PFNA)	17	U	21	17	7.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	5.2	J	26	10	4.8
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.4	J	8.7	3.5	1.7
375-73-5	Perfluorobutanesulfonic acid (PFBS)	31	U	79	31	14

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	92		70-130
STL00996	13C2 PFDA	97		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_021.d
 Lims ID: 320-35046-A-1-A
 Client ID: WGNA-011118-RW-3103
 Sample Type: Client
 Inject. Date: 31-Jan-2018 12:12:02 ALS Bottle#: 19 Worklist Smp#: 18
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35046-a-1-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:27:52 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK006

First Level Reviewer: barnettj Date: 31-Jan-2018 16:12:47

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.366	1.373	-0.007	1.000	156086	1.20		196	
298.90 > 99.00	1.366	1.373	-0.007	1.000	119554		1.31(0.00-0.00)	154	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.487	1.495	-0.008	1.000	1535821	9.24		7568	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.631	1.631	0.0	1.000	289560	1.48		173	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.631	1.631	0.0	1.000	139048	0.9820		31.7	
* 6 13C2-PFOA									
415.00 > 370.00	1.813	1.821	-0.008		1511383	10.0		5989	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.813	1.821	-0.008	1.000	484660	3.46		59.9	
413.00 > 169.00	1.813	1.821	-0.008	1.000	300107		1.61(0.00-0.00)	610	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.071	2.071	0.0	1.000	327364	2.98		150	Ma
499.00 > 99.00	2.071	2.071	0.0	1.000	52444		6.24(0.00-0.00)	63.4	M
* 7 13C4 PFOS									
503.00 > 80.00	2.071	2.071	0.0		3351158	28.7		5725	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.246	2.253	-0.007	1.000	1117035	9.66		6893	

QC Flag Legend

Review Flags

M - Manually Integrated

a - User Assigned ID

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_021.d

Injection Date: 31-Jan-2018 12:12:02

Instrument ID: A8_N

Lims ID: 320-35046-A-1-A

Lab Sample ID: 320-35046-1

Client ID: WGNA-011118-RW-3103

Operator ID: SACINSTLCMS01

ALS Bottle#: 19

Worklist Smp#: 18

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

* 7 13C4 PFOS

9 Perfluorononanoic acid (ND)



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_021.d
 Lims ID: 320-35046-A-1-A
 Client ID: WGNA-011118-RW-3103
 Sample Type: Client
 Inject. Date: 31-Jan-2018 12:12:02 ALS Bottle#: 19 Worklist Smp#: 18
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35046-a-1-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:27:52 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK006

First Level Reviewer: barnettj Date: 31-Jan-2018 16:12:47

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	9.24	92.35
\$ 10 13C2 PFDA	10.0	9.66	96.59

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_021.d
Injection Date: 31-Jan-2018 12:12:02 Instrument ID: A8_N
Lims ID: 320-35046-A-1-A Lab Sample ID: 320-35046-1
Client ID: WGNA-011118-RW-3103
Operator ID: SACINSTLCMS01 ALS Bottle#: 19 Worklist Smp#: 18
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected
Expected RT: 2.07

Processing Integration Results



Manual Integration Results

RT: 2.07
Area: 52444
Amount: 2.983825
Amount Units: ng/ml



Reviewer: barnettj, 31-Jan-2018 16:12:30
Audit Action: Manually Integrated

Audit Reason: Assign Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_021.d
Injection Date: 31-Jan-2018 12:12:02 Instrument ID: A8_N
Lims ID: 320-35046-A-1-A Lab Sample ID: 320-35046-1
Client ID: WGNA-011118-RW-3103
Operator ID: SACINSTLCMS01 ALS Bottle#: 19 Worklist Smp#: 18
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.07

Processing Integration Results



Manual Integration Results

RT: 2.07
Area: 327364
Amount: 2.983825
Amount Units: ng/ml



FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: WGNA-011118-FRB-3103 Lab Sample ID: 320-35046-2
 Matrix: Water Lab File ID: 2018.01.31_537A_022.d
 Analysis Method: 537 Date Collected: 01/11/2018 08:05
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 266(mL) Date Analyzed: 01/31/2018 12:16
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	38	15	6.4
335-67-1	Perfluorooctanoic acid (PFOA)	7.5	U	19	7.5	2.6
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.5
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	U	9.4	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	85	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	99		70-130
STL00996	13C2 PFDA	104		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_022.d
 Lims ID: 320-35046-A-2-A
 Client ID: WGNA-011118-FRB-3103
 Sample Type: Client
 Inject. Date: 31-Jan-2018 12:16:42 ALS Bottle#: 20 Worklist Smp#: 19
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35046-a-2-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:27:52 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK006

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
\$ 2 13C2 PFHxA	315.00 > 270.00	1.487	1.495	-0.008	1.000	1603292	9.92	7988	
* 6 13C2-PFOA	415.00 > 370.00	1.821	1.821	0.0		1469356	10.0	5329	
* 7 13C4 PFOS	503.00 > 80.00	2.079	2.071	0.008		3274315	28.7	7094	
\$ 10 13C2 PFDA	515.00 > 470.00	2.253	2.253	0.0	1.000	1173941	10.4	7857	

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_022.d

Injection Date: 31-Jan-2018 12:16:42

Instrument ID: A8_N

Lims ID: 320-35046-A-2-A

Lab Sample ID: 320-35046-2

Client ID: WGNA-011118-FRB-3103

Operator ID: SACINSTLCMS01

ALS Bottle#: 20

Worklist Smp#: 19




Injection Vol: 2.0 ul

Dil. Factor: 1.0000

Method: 537_A8_N

Limit Group: LC 537 ICAL




1 Perfluorobutanesulfonic acid (ND) 1 Perfluorobutanesulfonic acid (ND) \$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid (ND)

4 Perfluoroheptanoic acid (ND)




* 6 13C2-PFOA



5 Perfluorooctanoic acid (ND)




5 Perfluorooctanoic acid (ND)

8 Perfluorooctane sulfonic acid (ND)




8 Perfluorooctane sulfonic acid (ND) * 7 13C4 PFOS

9 Perfluorononanoic acid (ND)



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_022.d
 Lims ID: 320-35046-A-2-A
 Client ID: WGNA-011118-FRB-3103
 Sample Type: Client
 Inject. Date: 31-Jan-2018 12:16:42 ALS Bottle#: 20 Worklist Smp#: 19
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35046-a-2-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:27:52 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK006

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	9.92	99.17
\$ 10 13C2 PFDA	10.0	10.4	104.41

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: WGNA-011118-RW-0683 Lab Sample ID: 320-35046-3
 Matrix: Water Lab File ID: 2018.01.31_537A_023.d
 Analysis Method: 537 Date Collected: 01/11/2018 08:40
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 261(mL) Date Analyzed: 01/31/2018 12:21
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	29	J M	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	18	J	19	7.7	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.7
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	5.8	J	29	11	5.3
375-85-9	Perfluoroheptanoic acid (PFHpA)	5.2	J	9.6	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	86	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	87		70-130
STL00996	13C2 PFDA	96		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_023.d
 Lims ID: 320-35046-A-3-A
 Client ID: WGNA-011118-RW-0683
 Sample Type: Client
 Inject. Date: 31-Jan-2018 12:21:23 ALS Bottle#: 21 Worklist Smp#: 20
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35046-a-3-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:27:52 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK006

First Level Reviewer: barnettj Date: 31-Jan-2018 16:13:45

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.366	1.373	-0.007	1.000	273648	2.11		221	
298.90 > 99.00	1.366	1.373	-0.007	1.000	192417		1.42(0.00-0.00)	275	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.487	1.495	-0.008	1.000	1490758	8.73		7608	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.631	1.631	0.0	1.000	294024	1.51		108	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.631	1.631	0.0	1.000	196717	1.35		33.9	
* 6 13C2-PFOA									
415.00 > 370.00	1.813	1.821	-0.008		1551777	10.0		6100	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.821	1.821	0.0	1.000	673724	4.69		75.6	
413.00 > 169.00	1.821	1.821	0.0	1.000	395561		1.70(0.00-0.00)	768	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.071	2.071	0.0	1.000	824524	7.54		278	Ma
499.00 > 99.00	2.071	2.071	0.0	1.000	144751		5.70(0.00-0.00)	164	M
* 7 13C4 PFOS									
503.00 > 80.00	2.071	2.071	0.0		3339406	28.7		3197	
9 Perfluorononanoic acid									
463.00 > 419.00	2.086	2.079	0.007	1.000	54689	0.5306		8.9	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.253	2.253	0.0	1.000	1144648	9.64		7214	

QC Flag Legend

Review Flags

M - Manually Integrated

a - User Assigned ID

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_023.d

Injection Date: 31-Jan-2018 12:21:23

Instrument ID: A8_N

Lims ID: 320-35046-A-3-A

Lab Sample ID: 320-35046-3

Client ID: WGNA-011118-RW-0683

Operator ID: SACINSTLCMS01

ALS Bottle#: 21

Worklist Smp#: 20

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_023.d
 Lims ID: 320-35046-A-3-A
 Client ID: WGNA-011118-RW-0683
 Sample Type: Client
 Inject. Date: 31-Jan-2018 12:21:23 ALS Bottle#: 21 Worklist Smp#: 20
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35046-a-3-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:27:52 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK006

First Level Reviewer: barnettj Date: 31-Jan-2018 16:13:45

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	8.73	87.31
\$ 10 13C2 PFDA	10.0	9.64	96.40

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_023.d
Injection Date: 31-Jan-2018 12:21:23 Instrument ID: A8_N
Lims ID: 320-35046-A-3-A Lab Sample ID: 320-35046-3
Client ID: WGNA-011118-RW-0683
Operator ID: SACINSTLCMS01 ALS Bottle#: 21 Worklist Smp#: 20
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected
Expected RT: 2.07

Processing Integration Results



Manual Integration Results

RT: 2.07
Area: 144751
Amount: 7.541737
Amount Units: ng/ml



Reviewer: barnettj, 31-Jan-2018 16:13:28
Audit Action: Manually Integrated

Audit Reason: Assign Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_023.d
Injection Date: 31-Jan-2018 12:21:23 Instrument ID: A8_N
Lims ID: 320-35046-A-3-A Lab Sample ID: 320-35046-3
Client ID: WGNA-011118-RW-0683
Operator ID: SACINSTLCMS01 ALS Bottle#: 21 Worklist Smp#: 20
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.07

Processing Integration Results



Manual Integration Results

RT: 2.07
Area: 824524
Amount: 7.541737
Amount Units: ng/ml



Reviewer: barnettj, 31-Jan-2018 16:13:28

Audit Action: Manually Integrated

Audit Reason: Assign Peak

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: WGNA-011118-FRB-0683 Lab Sample ID: 320-35046-4
 Matrix: Water Lab File ID: 2018.01.31_537A_024.d
 Analysis Method: 537 Date Collected: 01/11/2018 08:35
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 262.8(mL) Date Analyzed: 01/31/2018 12:26
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	7.6	U	19	7.6	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	29	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	U	9.5	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	86	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	96		70-130
STL00996	13C2 PFDA	99		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_024.d
 Lims ID: 320-35046-A-4-A
 Client ID: WGNA-011118-FRB-0683
 Sample Type: Client
 Inject. Date: 31-Jan-2018 12:26:04 ALS Bottle#: 22 Worklist Smp#: 21
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35046-a-4-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:27:52 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK006

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
\$ 2 13C2 PFHxA	315.00 > 270.00	1.487	1.495	-0.008	1.000	1515280	9.65	7811	
* 6 13C2-PFOA	415.00 > 370.00	1.821	1.821	0.0		1427812	10.0	5728	
* 7 13C4 PFOS	503.00 > 80.00	2.079	2.071	0.008		3143756	28.7	5724	
\$ 10 13C2 PFDA	515.00 > 470.00	2.261	2.253	0.008	1.000	1083510	9.92	6972	

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_024.d

Injection Date: 31-Jan-2018 12:26:04

Instrument ID: A8_N

Lims ID: 320-35046-A-4-A

Lab Sample ID: 320-35046-4

Client ID: WGNA-011118-FRB-0683

Operator ID: SACINSTLCMS01

ALS Bottle#: 22

Worklist Smp#: 21

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid (ND)

1 Perfluorobutanesulfonic acid (ND)




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid (ND)

4 Perfluoroheptanoic acid (ND)




* 6 13C2-PFOA



5 Perfluorooctanoic acid (ND)

5 Perfluorooctanoic acid (ND)




8 Perfluorooctane sulfonic acid (ND)




8 Perfluorooctane sulfonic acid (ND)

* 7 13C4 PFOS

9 Perfluorononanoic acid (ND)



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_024.d
 Lims ID: 320-35046-A-4-A
 Client ID: WGNA-011118-FRB-0683
 Sample Type: Client
 Inject. Date: 31-Jan-2018 12:26:04 ALS Bottle#: 22 Worklist Smp#: 21
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35046-a-4-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:27:52 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK006

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	9.65	96.45
\$ 10 13C2 PFDA	10.0	9.92	99.17

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: NAWC-011118-RW-139 Lab Sample ID: 320-35046-5
 Matrix: Water Lab File ID: 2018.01.31_537A_025.d
 Analysis Method: 537 Date Collected: 01/11/2018 10:40
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 268.8(mL) Date Analyzed: 01/31/2018 12:30
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	12	J M	37	15	6.3
335-67-1	Perfluorooctanoic acid (PFOA)	16	J	19	7.4	2.6
375-95-1	Perfluorononanoic acid (PFNA)	19	U	22	19	7.4
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.1
375-85-9	Perfluoroheptanoic acid (PFHpA)	5.4	J	9.3	3.7	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	33	U	84	33	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	92		70-130
STL00996	13C2 PFDA	97		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_025.d
 Lims ID: 320-35046-A-5-A
 Client ID: NAWC-011118-RW-139
 Sample Type: Client
 Inject. Date: 31-Jan-2018 12:30:44 ALS Bottle#: 23 Worklist Smp#: 22
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35046-a-5-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:27:52 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK006

First Level Reviewer: barnettj Date: 31-Jan-2018 16:14:42

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.373	1.373	0.0	1.000	165394	1.20		207	
298.90 > 99.00	1.373	1.373	0.0	1.000	122386		1.35(0.00-0.00)	154	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.487	1.495	-0.008	1.000	1567392	9.18		7402	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.631	1.631	0.0	1.000	174930	0.8489		101	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.631	1.631	0.0	1.000	210418	1.45		46.0	
* 6 13C2-PFOA									
415.00 > 370.00	1.821	1.821	0.0		1551998	10.0		6491	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.821	1.821	0.0	1.000	607578	4.23		78.3	
413.00 > 169.00	1.821	1.821	0.0	1.000	345502		1.76(0.00-0.00)	729	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.079	2.071	0.008	1.000	364916	3.16		174	Ma
499.00 > 99.00	2.071	2.071	0.0	0.996	66104		5.52(0.00-0.00)	85.1	M
* 7 13C4 PFOS									
503.00 > 80.00	2.071	2.071	0.0		3530101	28.7		5339	
9 Perfluorononanoic acid									
463.00 > 419.00	2.086	2.079	0.007	1.000	60450	0.5865		9.9	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.253	2.253	0.0	1.000	1149995	9.68		7883	

QC Flag Legend

Review Flags

M - Manually Integrated

a - User Assigned ID

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_025.d

Injection Date: 31-Jan-2018 12:30:44

Instrument ID: A8_N

Lims ID: 320-35046-A-5-A

Lab Sample ID: 320-35046-5

Client ID: NAWC-011118-RW-139

Operator ID: SACINSTLCMS01

ALS Bottle#: 23

Worklist Smp#: 22

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_025.d
 Lims ID: 320-35046-A-5-A
 Client ID: NAWC-011118-RW-139
 Sample Type: Client
 Inject. Date: 31-Jan-2018 12:30:44 ALS Bottle#: 23 Worklist Smp#: 22
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35046-a-5-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:27:52 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK006

First Level Reviewer: barnettj Date: 31-Jan-2018 16:14:42

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	9.18	91.79
\$ 10 13C2 PFDA	10.0	9.68	96.83

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_025.d
Injection Date: 31-Jan-2018 12:30:44 Instrument ID: A8_N
Lims ID: 320-35046-A-5-A Lab Sample ID: 320-35046-5
Client ID: NAWC-011118-RW-139
Operator ID: SACINSTLCMS01 ALS Bottle#: 23 Worklist Smp#: 22
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1


Signal: 2

Not Detected
Expected RT: 2.07

Processing Integration Results



Manual Integration Results



RT: 2.07
Area: 66104
Amount: 3.157498
Amount Units: ng/ml

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_025.d
Injection Date: 31-Jan-2018 12:30:44 Instrument ID: A8_N
Lims ID: 320-35046-A-5-A Lab Sample ID: 320-35046-5
Client ID: NAWC-011118-RW-139
Operator ID: SACINSTLCMS01 ALS Bottle#: 23 Worklist Smp#: 22
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.07

Processing Integration Results



Manual Integration Results

RT: 2.08
Area: 364916
Amount: 3.157498
Amount Units: ng/ml



FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: NAWC-011118-FRB-139 Lab Sample ID: 320-35046-6
 Matrix: Water Lab File ID: 2018.01.31_537A_026.d
 Analysis Method: 537 Date Collected: 01/11/2018 10:35
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 273.2 (mL) Date Analyzed: 01/31/2018 12:35
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	37	15	6.2
335-67-1	Perfluorooctanoic acid (PFOA)	7.3	U	18	7.3	2.6
375-95-1	Perfluorononanoic acid (PFNA)	18	U	22	18	7.3
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	27	11	5.0
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.7	U	9.2	3.7	1.7
375-73-5	Perfluorobutanesulfonic acid (PFBS)	33	U	82	33	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	90		70-130
STL00996	13C2 PFDA	96		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_026.d
 Lims ID: 320-35046-A-6-A
 Client ID: NAWC-011118-FRB-139
 Sample Type: Client
 Inject. Date: 31-Jan-2018 12:35:24 ALS Bottle#: 24 Worklist Smp#: 23
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35046-a-6-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:27:52 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK006

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
\$ 2 13C2 PFHxA	315.00 > 270.00	1.487	1.495	-0.008	1.000	1490137	9.01	8361	
* 6 13C2-PFOA	415.00 > 370.00	1.821	1.821	0.0		1503114	10.0	6397	
* 7 13C4 PFOS	503.00 > 80.00	2.071	2.071	0.0		3436163	28.7	6667	
\$ 10 13C2 PFDA	515.00 > 470.00	2.253	2.253	0.0	1.000	1109023	9.64	6654	

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_026.d

Injection Date: 31-Jan-2018 12:35:24

Instrument ID: A8_N

Lims ID: 320-35046-A-6-A

Lab Sample ID: 320-35046-6

Client ID: NAWC-011118-FRB-139

Operator ID: SACINSTLCMS01

ALS Bottle#: 24

Worklist Smp#: 23




Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL




1 Perfluorobutanesulfonic acid (ND) 1 Perfluorobutanesulfonic acid (ND) \$ 2 13C2 PFHxA






3 Perfluorohexanesulfonic acid (ND) 4 Perfluoroheptanoic acid (ND) * 6 13C2-PFOA




5 Perfluorooctanoic acid (ND) 5 Perfluorooctanoic acid (ND) 8 Perfluorooctane sulfonic acid (ND)



8 Perfluorooctane sulfonic acid (ND) * 7 13C4 PFOS 9 Perfluorononanoic acid (ND)



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_026.d
 Lims ID: 320-35046-A-6-A
 Client ID: NAWC-011118-FRB-139
 Sample Type: Client
 Inject. Date: 31-Jan-2018 12:35:24 ALS Bottle#: 24 Worklist Smp#: 23
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35046-a-6-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:27:52 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK006

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	9.01	90.10
\$ 10 13C2 PFDA	10.0	9.64	96.42

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: WGNA-011118-DUP-18 Lab Sample ID: 320-35046-7
 Matrix: Water Lab File ID: 2018.01.31_537A_027.d
 Analysis Method: 537 Date Collected: 01/11/2018 07:00
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 270.1(mL) Date Analyzed: 01/31/2018 12:40
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	12	J M	37	15	6.3
335-67-1	Perfluorooctanoic acid (PFOA)	15	J	19	7.4	2.6
375-95-1	Perfluorononanoic acid (PFNA)	19	U	22	19	7.4
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.1
375-85-9	Perfluoroheptanoic acid (PFHpA)	5.2	J	9.3	3.7	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	33	U	83	33	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	92		70-130
STL00996	13C2 PFDA	101		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_027.d
 Lims ID: 320-35046-A-7-A
 Client ID: WGNA-011118-DUP-18
 Sample Type: Client
 Inject. Date: 31-Jan-2018 12:40:06 ALS Bottle#: 25 Worklist Smp#: 24
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35046-a-7-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:27:52 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK006

First Level Reviewer: barnettj Date: 31-Jan-2018 16:16:05

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.373	1.373	0.0	1.000	172129	1.31		222	
298.90 > 99.00	1.373	1.373	0.0	1.000	127695		1.35(0.00-0.00)	211	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.487	1.495	-0.008	1.000	1544647	9.22		7607	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.631	1.631	0.0	1.000	166529	0.8436		93.8	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.631	1.631	0.0	1.000	201629	1.41		42.9	
* 6 13C2-PFOA									
415.00 > 370.00	1.821	1.821	0.0		1522059	10.0		6421	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.821	1.821	0.0	1.000	569448	4.04		70.9	
413.00 > 169.00	1.821	1.821	0.0	1.000	348179		1.64(0.00-0.00)	872	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.071	2.071	0.0	1.000	370103	3.34		178	Ma
499.00 > 99.00	2.071	2.071	0.0	1.000	65079		5.69(0.00-0.00)	91.5	M
* 7 13C4 PFOS									
503.00 > 80.00	2.071	2.071	0.0		3381704	28.7		4941	
9 Perfluorononanoic acid									
463.00 > 419.00	2.079	2.079	0.0	1.000	59113	0.5848		10.8	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.253	2.253	0.0	1.000	1174889	10.1		7744	

QC Flag Legend

Review Flags

M - Manually Integrated

a - User Assigned ID

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_027.d

Injection Date: 31-Jan-2018 12:40:06

Instrument ID: A8_N

Lims ID: 320-35046-A-7-A

Lab Sample ID: 320-35046-7

Client ID: WGNA-011118-DUP-18

Operator ID: SACINSTLCMS01

ALS Bottle#: 25

Worklist Smp#: 24

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_027.d
 Lims ID: 320-35046-A-7-A
 Client ID: WGNA-011118-DUP-18
 Sample Type: Client
 Inject. Date: 31-Jan-2018 12:40:06 ALS Bottle#: 25 Worklist Smp#: 24
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35046-a-7-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:27:52 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK006

First Level Reviewer: barnettj Date: 31-Jan-2018 16:16:05

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	9.22	92.23
\$ 10 13C2 PFDA	10.0	10.1	100.88

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_027.d
Injection Date: 31-Jan-2018 12:40:06 Instrument ID: A8_N
Lims ID: 320-35046-A-7-A Lab Sample ID: 320-35046-7
Client ID: WGNA-011118-DUP-18
Operator ID: SACINSTLCMS01 ALS Bottle#: 25 Worklist Smp#: 24
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected
Expected RT: 2.07

Processing Integration Results



Manual Integration Results

RT: 2.07
Area: 65079
Amount: 3.342907
Amount Units: ng/ml



Reviewer: barnettj, 31-Jan-2018 16:15:20
Audit Action: Manually Integrated

Audit Reason: Assign Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_027.d
Injection Date: 31-Jan-2018 12:40:06 Instrument ID: A8_N
Lims ID: 320-35046-A-7-A Lab Sample ID: 320-35046-7
Client ID: WGNA-011118-DUP-18
Operator ID: SACINSTLCMS01 ALS Bottle#: 25 Worklist Smp#: 24
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.07

Processing Integration Results



RT: 2.07
Area: 370103
Amount: 3.342907
Amount Units: ng/ml

Manual Integration Results



FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: NAWC-011118-RW-098 Lab Sample ID: 320-35046-8
 Matrix: Water Lab File ID: 2018.01.31_537A_028.d
 Analysis Method: 537 Date Collected: 01/11/2018 11:10
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 240.8(mL) Date Analyzed: 01/31/2018 12:44
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	J M	42	17	7.1
335-67-1	Perfluorooctanoic acid (PFOA)	14	J	21	8.3	2.9
375-95-1	Perfluorononanoic acid (PFNA)	21	U M	25	21	8.3
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	31	12	5.7
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.9	J M	10	4.2	2.0
375-73-5	Perfluorobutanesulfonic acid (PFBS)	37	U	93	37	17

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	91		70-130
STL00996	13C2 PFDA	102		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_028.d
 Lims ID: 320-35046-A-8-A
 Client ID: NAWC-011118-RW-098
 Sample Type: Client
 Inject. Date: 31-Jan-2018 12:44:47 ALS Bottle#: 26 Worklist Smp#: 25
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35046-a-8-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:27:52 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK006

First Level Reviewer: barnettj Date: 31-Jan-2018 16:17:50

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.373	1.373	0.0	1.000	219464	1.73		251	
298.90 > 99.00	1.373	1.373	0.0	1.000	153654		1.43(0.00-0.00)	234	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.495	1.495	0.0	1.000	1503594	9.14		8530	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.631	1.631	0.0	1.000	227587	1.20		129	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.631	1.631	0.0	1.000	132246	0.9441		26.6	M
* 6 13C2-PFOA									
415.00 > 370.00	1.821	1.821	0.0		1495096	10.0		5897	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.821	1.821	0.0	1.000	459802	3.32		54.7	
413.00 > 169.00	1.821	1.821	0.0	1.000	283953		1.62(0.00-0.00)	646	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.071	2.071	0.0	1.000	398454	3.73		154	Ma
499.00 > 99.00	2.071	2.071	0.0	1.000	66116		6.03(0.00-0.00)	68.9	M
* 7 13C4 PFOS									
503.00 > 80.00	2.071	2.071	0.0		3259129	28.7		3917	
9 Perfluorononanoic acid									
463.00 > 419.00	2.079	2.079	0.0	1.000	40917	0.4121		7.1	M
\$ 10 13C2 PFDA									
515.00 > 470.00	2.253	2.253	0.0	1.000	1169902	10.2		8121	

QC Flag Legend

Review Flags

M - Manually Integrated

a - User Assigned ID

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_028.d

Injection Date: 31-Jan-2018 12:44:47

Instrument ID: A8_N

Lims ID: 320-35046-A-8-A

Lab Sample ID: 320-35046-8

Client ID: NAWC-011118-RW-098

Operator ID: SACINSTLCMS01

ALS Bottle#: 26

Worklist Smp#: 25

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid (M)




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

* 7 13C4 PFOS

9 Perfluorononanoic acid (M)



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_028.d
 Lims ID: 320-35046-A-8-A
 Client ID: NAWC-011118-RW-098
 Sample Type: Client
 Inject. Date: 31-Jan-2018 12:44:47 ALS Bottle#: 26 Worklist Smp#: 25
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35046-a-8-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:27:52 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK006

First Level Reviewer: barnettj Date: 31-Jan-2018 16:17:50

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	9.14	91.40
\$ 10 13C2 PFDA	10.0	10.2	102.26

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_028.d
Injection Date: 31-Jan-2018 12:44:47 Instrument ID: A8_N
Lims ID: 320-35046-A-8-A Lab Sample ID: 320-35046-8
Client ID: NAWC-011118-RW-098
Operator ID: SACINSTLCMS01 ALS Bottle#: 26 Worklist Smp#: 25
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected
Expected RT: 2.07

Processing Integration Results



Manual Integration Results

RT: 2.07
Area: 66116
Amount: 3.734341
Amount Units: ng/ml



Reviewer: barnettj, 31-Jan-2018 16:17:22
Audit Action: Manually Integrated

Audit Reason: Assign Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_028.d
Injection Date: 31-Jan-2018 12:44:47 Instrument ID: A8_N
Lims ID: 320-35046-A-8-A Lab Sample ID: 320-35046-8
Client ID: NAWC-011118-RW-098
Operator ID: SACINSTLCMS01 ALS Bottle#: 26 Worklist Smp#: 25
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.07

Processing Integration Results



RT: 2.07
Area: 398454
Amount: 3.734341
Amount Units: ng/ml

Manual Integration Results



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_028.d
Injection Date: 31-Jan-2018 12:44:47 Instrument ID: A8_N
Lims ID: 320-35046-A-8-A Lab Sample ID: 320-35046-8
Client ID: NAWC-011118-RW-098
Operator ID: SACINSTLCMS01 ALS Bottle#: 26 Worklist Smp#: 25
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

9 Perfluorononanoic acid, CAS: 375-95-1

Signal: 1


Not Detected
Expected RT: 2.08

Processing Integration Results



Manual Integration Results

RT: 2.08
Area: 40917
Amount: 0.412061
Amount Units: ng/ml



Reviewer: barnettj, 31-Jan-2018 16:17:41
Audit Action: Manually Integrated

Audit Reason: Missed Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_028.d
Injection Date: 31-Jan-2018 12:44:47 Instrument ID: A8_N
Lims ID: 320-35046-A-8-A Lab Sample ID: 320-35046-8
Client ID: NAWC-011118-RW-098
Operator ID: SACINSTLCMS01 ALS Bottle#: 26 Worklist Smp#: 25
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

4 Perfluoroheptanoic acid, CAS: 375-85-9


Signal: 1

Not Detected
Expected RT: 1.63

Processing Integration Results



Manual Integration Results



RT: 1.63
Area: 132246
Amount: 0.944090
Amount Units: ng/ml

Reviewer: barnettj, 31-Jan-2018 16:16:45
Audit Action: Manually Integrated

Audit Reason: Missed Peak

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: NAWC-011118-FRB-098 Lab Sample ID: 320-35046-9
 Matrix: Water Lab File ID: 2018.01.31_537A_031.d
 Analysis Method: 537 Date Collected: 01/11/2018 11:05
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 269.9(mL) Date Analyzed: 01/31/2018 12:58
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206410 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	37	15	6.3
335-67-1	Perfluorooctanoic acid (PFOA)	7.4	U	19	7.4	2.6
375-95-1	Perfluorononanoic acid (PFNA)	19	U	22	19	7.4
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.1
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.7	U	9.3	3.7	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	33	U	83	33	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	93		70-130
STL00996	13C2 PFDA	94		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_031.d
 Lims ID: 320-35046-A-9-A
 Client ID: NAWC-011118-FRB-098
 Sample Type: Client
 Inject. Date: 31-Jan-2018 12:58:44 ALS Bottle#: 27 Worklist Smp#: 28
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35046-a-9-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:28:14 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK006

First Level Reviewer: barnettj Date: 31-Jan-2018 16:19:11

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
\$ 2 13C2 PFHxA	315.00 > 270.00	1.487	1.487	0.0	1.000	1574689	9.26	9454	
* 6 13C2-PFOA	415.00 > 370.00	1.821	1.813	0.008		1546187	10.0	6480	
5 Perfluorooctanoic acid	413.00 > 369.00	1.821	1.813	0.008	1.000	59669	0.4169	7.6	
	413.00 > 169.00	1.821	1.813	0.008	1.000	34466	1.73(0.00-0.00)	73.4	
* 7 13C4 PFOS	503.00 > 80.00	2.071	2.071	0.0		3372040	28.7	7145	
\$ 10 13C2 PFDA	515.00 > 470.00	2.253	2.246	0.007	1.000	1117632	9.45	7180	

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_031.d

Injection Date: 31-Jan-2018 12:58:44

Instrument ID: A8_N

Lims ID: 320-35046-A-9-A

Lab Sample ID: 320-35046-9

Client ID: NAWC-011118-FRB-098

Operator ID: SACINSTLCMS01

ALS Bottle#: 27

Worklist Smp#: 28

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid (ND)

1 Perfluorobutanesulfonic acid (ND)




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid (ND)

4 Perfluoroheptanoic acid (ND)




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (ND)




8 Perfluorooctane sulfonic acid (ND)

* 7 13C4 PFOS

9 Perfluorononanoic acid (ND)



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_031.d
 Lims ID: 320-35046-A-9-A
 Client ID: NAWC-011118-FRB-098
 Sample Type: Client
 Inject. Date: 31-Jan-2018 12:58:44 ALS Bottle#: 27 Worklist Smp#: 28
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35046-a-9-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:28:14 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK006

First Level Reviewer: barnettj Date: 31-Jan-2018 16:19:11

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	9.26	92.56
\$ 10 13C2 PFDA	10.0	9.45	94.46

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: NAWC-011118-RW-180 Lab Sample ID: 320-35046-10
 Matrix: Water Lab File ID: 2018.01.31_537A_032.d
 Analysis Method: 537 Date Collected: 01/11/2018 12:10
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 265.4 (mL) Date Analyzed: 01/31/2018 13:03
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206410 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	28	J M	38	15	6.4
335-67-1	Perfluorooctanoic acid (PFOA)	23		19	7.5	2.6
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.5
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	J	28	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	9.1	J	9.4	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	85	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	92		70-130
STL00996	13C2 PFDA	100		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_032.d
 Lims ID: 320-35046-A-10-A
 Client ID: NAWC-011118-RW-180
 Sample Type: Client
 Inject. Date: 31-Jan-2018 13:03:24 ALS Bottle#: 28 Worklist Smp#: 29
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35046-a-10-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:28:14 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK006

First Level Reviewer: barnettj Date: 31-Jan-2018 16:20:18

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.366	1.366	0.0	1.000	422986	3.17		329	
298.90 > 99.00	1.366	1.366	0.0	1.000	299555		1.41(0.00-0.00)	436	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.487	1.487	0.0	1.000	1552021	9.17		7907	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.631	1.631	0.0	1.000	561738	2.81		236	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.631	1.631	0.0	1.000	347680	2.41		67.1	
* 6 13C2-PFOA									
415.00 > 370.00	1.813	1.813	0.0		1537799	10.0		6553	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.813	1.813	0.0	1.000	862613	6.06		103	
413.00 > 169.00	1.813	1.813	0.0	1.000	511813		1.69(0.00-0.00)	1097	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.071	2.071	0.0	1.000	848615	7.56		336	Ma
499.00 > 99.00	2.071	2.071	0.0	1.000	161798		5.24(0.00-0.00)	186	M
* 7 13C4 PFOS									
503.00 > 80.00	2.071	2.071	0.0		3430335	28.7		3837	
9 Perfluorononanoic acid									
463.00 > 419.00	2.079	2.079	0.0	1.000	86218	0.8442		14.8	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.246	2.246	0.0	1.000	1179840	10.0		7422	

QC Flag Legend

Review Flags

M - Manually Integrated

a - User Assigned ID

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_032.d

Injection Date: 31-Jan-2018 13:03:24

Instrument ID: A8_N

Lims ID: 320-35046-A-10-A

Lab Sample ID: 320-35046-10

Client ID: NAWC-011118-RW-180

Operator ID: SACINSTLCMS01

ALS Bottle#: 28

Worklist Smp#: 29

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_032.d
 Lims ID: 320-35046-A-10-A
 Client ID: NAWC-011118-RW-180
 Sample Type: Client
 Inject. Date: 31-Jan-2018 13:03:24 ALS Bottle#: 28 Worklist Smp#: 29
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35046-a-10-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:28:14 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK006

First Level Reviewer: barnettj Date: 31-Jan-2018 16:20:18

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	9.17	91.73
\$ 10 13C2 PFDA	10.0	10.0	100.26

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_032.d
Injection Date: 31-Jan-2018 13:03:24 Instrument ID: A8_N
Lims ID: 320-35046-A-10-A Lab Sample ID: 320-35046-10
Client ID: NAWC-011118-RW-180
Operator ID: SACINSTLCMS01 ALS Bottle#: 28 Worklist Smp#: 29
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1


Signal: 2

Not Detected
Expected RT: 2.07

Processing Integration Results



Manual Integration Results



RT: 2.07
Area: 161798
Amount: 7.556339
Amount Units: ng/ml

Reviewer: barnettj, 31-Jan-2018 16:19:59
Audit Action: Manually Integrated

Audit Reason: Assign Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_032.d
Injection Date: 31-Jan-2018 13:03:24 Instrument ID: A8_N
Lims ID: 320-35046-A-10-A Lab Sample ID: 320-35046-10
Client ID: NAWC-011118-RW-180
Operator ID: SACINSTLCMS01 ALS Bottle#: 28 Worklist Smp#: 29
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.07

Processing Integration Results



RT: 2.07
Area: 848615
Amount: 7.556339
Amount Units: ng/ml

Manual Integration Results



Reviewer: barnettj, 31-Jan-2018 16:19:59

Audit Action: Manually Integrated

Audit Reason: Assign Peak

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: NAWC-011118-FRB-180 Lab Sample ID: 320-35046-11
 Matrix: Water Lab File ID: 2018.01.31_537A_033.d
 Analysis Method: 537 Date Collected: 01/11/2018 12:05
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 264.2 (mL) Date Analyzed: 01/31/2018 13:08
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206410 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	38	15	6.4
335-67-1	Perfluorooctanoic acid (PFOA)	7.6	U	19	7.6	2.6
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	U	9.5	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	85	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	99		70-130
STL00996	13C2 PFDA	100		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_033.d
 Lims ID: 320-35046-A-11-A
 Client ID: NAWC-011118-FRB-180
 Sample Type: Client
 Inject. Date: 31-Jan-2018 13:08:04 ALS Bottle#: 29 Worklist Smp#: 30
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35046-a-11-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:28:14 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK006

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
\$ 2 13C2 PFHxA	315.00 > 270.00	1.495	1.487	0.008	1.000	1676199	9.94	8930	
* 6 13C2-PFOA	415.00 > 370.00	1.821	1.813	0.008		1532214	10.0	6171	
* 7 13C4 PFOS	503.00 > 80.00	2.071	2.071	0.0		3442464	28.7	6320	
\$ 10 13C2 PFDA	515.00 > 470.00	2.253	2.246	0.007	1.000	1177649	10.0	8057	

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_033.d

Injection Date: 31-Jan-2018 13:08:04

Instrument ID: A8_N

Lims ID: 320-35046-A-11-A

Lab Sample ID: 320-35046-11

Client ID: NAWC-011118-FRB-180

Operator ID: SACINSTLCMS01

ALS Bottle#: 29

Worklist Smp#: 30




Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL




1 Perfluorobutanesulfonic acid (ND) 1 Perfluorobutanesulfonic acid (ND) \$ 2 13C2 PFHxA






3 Perfluorohexanesulfonic acid (ND) 4 Perfluoroheptanoic acid (ND) * 6 13C2-PFOA




5 Perfluorooctanoic acid (ND) 5 Perfluorooctanoic acid (ND) 8 Perfluorooctane sulfonic acid (ND)



8 Perfluorooctane sulfonic acid (ND) * 7 13C4 PFOS 9 Perfluorononanoic acid (ND)



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_033.d
 Lims ID: 320-35046-A-11-A
 Client ID: NAWC-011118-FRB-180
 Sample Type: Client
 Inject. Date: 31-Jan-2018 13:08:04 ALS Bottle#: 29 Worklist Smp#: 30
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35046-a-11-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:28:14 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK006

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	9.94	99.43
\$ 10 13C2 PFDA	10.0	10.0	100.44

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: NAWC-011118-RW-179 Lab Sample ID: 320-35046-12
 Matrix: Water Lab File ID: 2018.01.31_537A_034.d
 Analysis Method: 537 Date Collected: 01/11/2018 12:40
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 261.9(mL) Date Analyzed: 01/31/2018 13:12
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206410 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	18	J M	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	18	J	19	7.6	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	6.2	J	29	11	5.3
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.7	J	9.5	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	86	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	93		70-130
STL00996	13C2 PFDA	101		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_034.d
 Lims ID: 320-35046-A-12-A
 Client ID: NAWC-011118-RW-179
 Sample Type: Client
 Inject. Date: 31-Jan-2018 13:12:44 ALS Bottle#: 30 Worklist Smp#: 31
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35046-a-12-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:28:14 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK006

First Level Reviewer: barnettj Date: 31-Jan-2018 16:21:20

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.373	1.366	0.007	1.000	190045	1.44		217	
298.90 > 99.00	1.373	1.366	0.007	1.000	140984		1.35(0.00-0.00)	202	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.495	1.487	0.008	1.000	1509762	9.32		8075	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.639	1.631	0.008	1.000	319987	1.62		165	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.631	1.631	0.0	1.000	171221	1.24		34.0	
* 6 13C2-PFOA									
415.00 > 370.00	1.821	1.813	0.008		1472481	10.0		6379	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.821	1.813	0.008	1.000	656413	4.82		80.2	
413.00 > 169.00	1.821	1.813	0.008	1.000	381700		1.72(0.00-0.00)	855	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.071	2.071	0.0	1.000	509817	4.60		192	Ma
499.00 > 99.00	2.071	2.071	0.0	1.000	89760		5.68(0.00-0.00)	86.9	M
* 7 13C4 PFOS									
503.00 > 80.00	2.071	2.071	0.0		3387330	28.7		4171	
9 Perfluorononanoic acid									
463.00 > 419.00	2.079	2.079	0.0	1.000	63350	0.6478		10.0	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.253	2.246	0.007	1.000	1133882	10.1		7866	

QC Flag Legend

Review Flags

M - Manually Integrated

a - User Assigned ID

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_034.d

Injection Date: 31-Jan-2018 13:12:44

Instrument ID: A8_N

Lims ID: 320-35046-A-12-A

Lab Sample ID: 320-35046-12

Client ID: NAWC-011118-RW-179

Operator ID: SACINSTLCMS01

ALS Bottle#: 30

Worklist Smp#: 31

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_034.d
 Lims ID: 320-35046-A-12-A
 Client ID: NAWC-011118-RW-179
 Sample Type: Client
 Inject. Date: 31-Jan-2018 13:12:44 ALS Bottle#: 30 Worklist Smp#: 31
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35046-a-12-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:28:14 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK006

First Level Reviewer: barnettj Date: 31-Jan-2018 16:21:20

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	9.32	93.19
\$ 10 13C2 PFDA	10.0	10.1	100.63

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_034.d
Injection Date: 31-Jan-2018 13:12:44 Instrument ID: A8_N
Lims ID: 320-35046-A-12-A Lab Sample ID: 320-35046-12
Client ID: NAWC-011118-RW-179
Operator ID: SACINSTLCMS01 ALS Bottle#: 30 Worklist Smp#: 31
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected
Expected RT: 2.07

Processing Integration Results



Manual Integration Results

RT: 2.07
Area: 89760
Amount: 4.597207
Amount Units: ng/ml



Reviewer: barnettj, 31-Jan-2018 16:21:00
Audit Action: Manually Integrated

Audit Reason: Assign Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_034.d
Injection Date: 31-Jan-2018 13:12:44 Instrument ID: A8_N
Lims ID: 320-35046-A-12-A Lab Sample ID: 320-35046-12
Client ID: NAWC-011118-RW-179
Operator ID: SACINSTLCMS01 ALS Bottle#: 30 Worklist Smp#: 31
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.07

Processing Integration Results



Manual Integration Results

RT: 2.07
Area: 509817
Amount: 4.597207
Amount Units: ng/ml



Reviewer: barnettj, 31-Jan-2018 16:21:00

Audit Action: Manually Integrated

Audit Reason: Assign Peak

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: NAWC-011118-FRB-179 Lab Sample ID: 320-35046-13
 Matrix: Water Lab File ID: 2018.01.31_537A_037.d
 Analysis Method: 537 Date Collected: 01/11/2018 12:35
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 261.5 (mL) Date Analyzed: 01/31/2018 13:26
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206410 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	7.6	U	19	7.6	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	29	11	5.3
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	U	9.6	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	86	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	95		70-130
STL00996	13C2 PFDA	95		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_037.d
 Lims ID: 320-35046-A-13-A
 Client ID: NAWC-011118-FRB-179
 Sample Type: Client
 Inject. Date: 31-Jan-2018 13:26:44 ALS Bottle#: 33 Worklist Smp#: 34
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35046-a-13-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:28:14 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK006

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
\$ 2 13C2 PFHxA	315.00 > 270.00	1.495	1.487	0.008	1.000	1629293	9.50	8876	
* 6 13C2-PFOA	415.00 > 370.00	1.821	1.813	0.008		1558738	10.0	7025	
* 7 13C4 PFOS	503.00 > 80.00	2.071	2.071	0.0		3496002	28.7	7118	
\$ 10 13C2 PFDA	515.00 > 470.00	2.253	2.246	0.007	1.000	1136294	9.53	8102	

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_037.d

Injection Date: 31-Jan-2018 13:26:44

Instrument ID: A8_N

Lims ID: 320-35046-A-13-A

Lab Sample ID: 320-35046-13

Client ID: NAWC-011118-FRB-179

Operator ID: SACINSTLCMS01

ALS Bottle#: 33

Worklist Smp#: 34




Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL




1 Perfluorobutanesulfonic acid (ND) 1 Perfluorobutanesulfonic acid (ND) \$ 2 13C2 PFHxA






3 Perfluorohexanesulfonic acid (ND) 4 Perfluoroheptanoic acid (ND) * 6 13C2-PFOA




5 Perfluorooctanoic acid (ND) 5 Perfluorooctanoic acid (ND) 8 Perfluorooctane sulfonic acid (ND)



8 Perfluorooctane sulfonic acid (ND) * 7 13C4 PFOS 9 Perfluorononanoic acid (ND)



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_037.d
 Lims ID: 320-35046-A-13-A
 Client ID: NAWC-011118-FRB-179
 Sample Type: Client
 Inject. Date: 31-Jan-2018 13:26:44 ALS Bottle#: 33 Worklist Smp#: 34
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35046-a-13-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:28:14 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK006

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	9.50	95.00
\$ 10 13C2 PFDA	10.0	9.53	95.27

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: NAWC-011118-RW-303 Lab Sample ID: 320-35046-14
 Matrix: Water Lab File ID: 2018.01.31_537A_038.d
 Analysis Method: 537 Date Collected: 01/11/2018 13:10
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 260.8(mL) Date Analyzed: 01/31/2018 13:31
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206410 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	21	J M	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	20		19	7.7	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.7
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	7.3	J	29	12	5.3
375-85-9	Perfluoroheptanoic acid (PFHpA)	6.0	J	9.6	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	35	U	86	35	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	91		70-130
STL00996	13C2 PFDA	103		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_038.d
 Lims ID: 320-35046-A-14-A
 Client ID: NAWC-011118-RW-303
 Sample Type: Client
 Inject. Date: 31-Jan-2018 13:31:25 ALS Bottle#: 34 Worklist Smp#: 35
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35046-a-14-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:28:14 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK006

First Level Reviewer: barnettj Date: 31-Jan-2018 16:24:26

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.366	1.366	0.0	1.000	195710	1.49		213	
298.90 > 99.00	1.366	1.366	0.0	1.000	135585		1.44(0.00-0.00)	202	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.487	1.487	0.0	1.000	1480110	9.15		7609	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.631	1.631	0.0	1.000	375199	1.90		230	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.631	1.631	0.0	1.000	215712	1.57		46.1	
* 6 13C2-PFOA									
415.00 > 370.00	1.813	1.813	0.0		1470595	10.0		5932	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.813	1.813	0.0	1.000	715415	5.25		85.5	
413.00 > 169.00	1.813	1.813	0.0	1.000	421496		1.70(0.00-0.00)	1247	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.071	2.071	0.0	1.000	607133	5.49		266	Ma
499.00 > 99.00	2.071	2.071	0.0	1.000	106082		5.72(0.00-0.00)	141	M
* 7 13C4 PFOS									
503.00 > 80.00	2.064	2.071	-0.007		3380751	28.7		4427	
9 Perfluorononanoic acid									
463.00 > 419.00	2.079	2.079	0.0	1.000	52629	0.5388		8.9	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.246	2.246	0.0	1.000	1158359	10.3		7777	

QC Flag Legend

Review Flags

M - Manually Integrated

a - User Assigned ID

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_038.d

Injection Date: 31-Jan-2018 13:31:25

Instrument ID: A8_N

Lims ID: 320-35046-A-14-A

Lab Sample ID: 320-35046-14

Client ID: NAWC-011118-RW-303

Operator ID: SACINSTLCMS01

ALS Bottle#: 34

Worklist Smp#: 35

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_038.d
 Lims ID: 320-35046-A-14-A
 Client ID: NAWC-011118-RW-303
 Sample Type: Client
 Inject. Date: 31-Jan-2018 13:31:25 ALS Bottle#: 34 Worklist Smp#: 35
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35046-a-14-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:28:14 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK006

First Level Reviewer: barnettj Date: 31-Jan-2018 16:24:26

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	9.15	91.47
\$ 10 13C2 PFDA	10.0	10.3	102.94

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_038.d
Injection Date: 31-Jan-2018 13:31:25 Instrument ID: A8_N
Lims ID: 320-35046-A-14-A Lab Sample ID: 320-35046-14
Client ID: NAWC-011118-RW-303
Operator ID: SACINSTLCMS01 ALS Bottle#: 34 Worklist Smp#: 35
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected
Expected RT: 2.07

Processing Integration Results



Manual Integration Results

RT: 2.07
Area: 106082
Amount: 5.485395
Amount Units: ng/ml



Reviewer: barnettj, 31-Jan-2018 16:24:07
Audit Action: Manually Integrated

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_038.d
Injection Date: 31-Jan-2018 13:31:25 Instrument ID: A8_N
Lims ID: 320-35046-A-14-A Lab Sample ID: 320-35046-14
Client ID: NAWC-011118-RW-303
Operator ID: SACINSTLCMS01 ALS Bottle#: 34 Worklist Smp#: 35
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.07

Processing Integration Results



Manual Integration Results

RT: 2.07
Area: 607133
Amount: 5.485395
Amount Units: ng/ml



FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: NAWC-011118-FRB-303 Lab Sample ID: 320-35046-15
 Matrix: Water Lab File ID: 2018.01.31_537A_039.d
 Analysis Method: 537 Date Collected: 01/11/2018 13:05
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 262 (mL) Date Analyzed: 01/31/2018 13:36
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206410 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	7.6	U	19	7.6	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	29	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	U	9.5	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	86	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	92		70-130
STL00996	13C2 PFDA	102		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_039.d
 Lims ID: 320-35046-A-15-A
 Client ID: NAWC-011118-FRB-303
 Sample Type: Client
 Inject. Date: 31-Jan-2018 13:36:05 ALS Bottle#: 35 Worklist Smp#: 36
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35046-a-15-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:28:14 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK006

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
\$ 2 13C2 PFHxA	315.00 > 270.00	1.487	1.487	0.0	1.000	1580670	9.21	9253	
* 6 13C2-PFOA	415.00 > 370.00	1.813	1.813	0.0		1560240	10.0	6778	
* 7 13C4 PFOS	503.00 > 80.00	2.071	2.071	0.0		3459417	28.7	6464	
\$ 10 13C2 PFDA	515.00 > 470.00	2.253	2.246	0.007	1.000	1219654	10.2	9148	

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_039.d

Injection Date: 31-Jan-2018 13:36:05

Instrument ID: A8_N

Lims ID: 320-35046-A-15-A

Lab Sample ID: 320-35046-15

Client ID: NAWC-011118-FRB-303

Operator ID: SACINSTLCMS01

ALS Bottle#: 35

Worklist Smp#: 36




Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL




1 Perfluorobutanesulfonic acid (ND) 1 Perfluorobutanesulfonic acid (ND) \$ 2 13C2 PFHxA






3 Perfluorohexanesulfonic acid (ND) 4 Perfluoroheptanoic acid (ND) * 6 13C2-PFOA




5 Perfluorooctanoic acid (ND) 5 Perfluorooctanoic acid (ND) 8 Perfluorooctane sulfonic acid (ND)



8 Perfluorooctane sulfonic acid (ND) * 7 13C4 PFOS 9 Perfluorononanoic acid (ND)



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_039.d
 Lims ID: 320-35046-A-15-A
 Client ID: NAWC-011118-FRB-303
 Sample Type: Client
 Inject. Date: 31-Jan-2018 13:36:05 ALS Bottle#: 35 Worklist Smp#: 36
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35046-a-15-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:28:14 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK006

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	9.21	92.08
\$ 10 13C2 PFDA	10.0	10.2	102.16

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: WGNA-011118-RW-3409 Lab Sample ID: 320-35046-16
 Matrix: Water Lab File ID: 2018.01.31_537A_040.d
 Analysis Method: 537 Date Collected: 01/11/2018 15:10
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 288 (mL) Date Analyzed: 01/31/2018 13:40
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206410 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	20	J M	35	14	5.9
335-67-1	Perfluorooctanoic acid (PFOA)	14	J	17	6.9	2.4
375-95-1	Perfluorononanoic acid (PFNA)	17	U	21	17	6.9
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	7.9	J	26	10	4.8
375-85-9	Perfluoroheptanoic acid (PFHpA)	5.1	J	8.7	3.5	1.6
375-73-5	Perfluorobutanesulfonic acid (PFBS)	31	U	78	31	14

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	91		70-130
STL00996	13C2 PFDA	100		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_040.d
 Lims ID: 320-35046-A-16-A
 Client ID: WGNA-011118-RW-3409
 Sample Type: Client
 Inject. Date: 31-Jan-2018 13:40:45 ALS Bottle#: 36 Worklist Smp#: 37
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35046-a-16-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:28:14 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK006

First Level Reviewer: barnettj Date: 31-Jan-2018 16:25:22

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.366	1.366	0.0	1.000	325035	2.46		221	
298.90 > 99.00	1.366	1.366	0.0	1.000	236801		1.37(0.00-0.00)	330	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.487	1.487	0.0	1.000	1556865	9.14		7586	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.631	1.631	0.0	1.000	451144	2.27		180	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.631	1.631	0.0	1.000	214009	1.48		34.7	
* 6 13C2-PFOA									
415.00 > 370.00	1.813	1.813	0.0		1548213	10.0		6706	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.813	1.813	0.0	1.000	595609	4.16		62.3	
413.00 > 169.00	1.813	1.813	0.0	1.000	370786		1.61(0.00-0.00)	897	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.071	2.071	0.0	1.000	645923	5.80		184	Ma
499.00 > 99.00	2.071	2.071	0.0	1.000	118540		5.45(0.00-0.00)	155	M
* 7 13C4 PFOS									
503.00 > 80.00	2.071	2.071	0.0		3403494	28.7		2820	
9 Perfluorononanoic acid									
463.00 > 419.00	2.079	2.079	0.0	1.000	51876	0.5045		7.1	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.246	2.246	0.0	1.000	1189332	10.0		8635	

QC Flag Legend

Review Flags

M - Manually Integrated

a - User Assigned ID

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_040.d

Injection Date: 31-Jan-2018 13:40:45

Instrument ID: A8_N

Lims ID: 320-35046-A-16-A

Lab Sample ID: 320-35046-16

Client ID: WGNA-011118-RW-3409

Operator ID: SACINSTLCMS01

ALS Bottle#: 36

Worklist Smp#: 37

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_040.d
 Lims ID: 320-35046-A-16-A
 Client ID: WGNA-011118-RW-3409
 Sample Type: Client
 Inject. Date: 31-Jan-2018 13:40:45 ALS Bottle#: 36 Worklist Smp#: 37
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35046-a-16-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:28:14 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK006

First Level Reviewer: barnettj Date: 31-Jan-2018 16:25:22

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	9.14	91.39
\$ 10 13C2 PFDA	10.0	10.0	100.39

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_040.d
Injection Date: 31-Jan-2018 13:40:45 Instrument ID: A8_N
Lims ID: 320-35046-A-16-A Lab Sample ID: 320-35046-16
Client ID: WGNA-011118-RW-3409
Operator ID: SACINSTLCMS01 ALS Bottle#: 36 Worklist Smp#: 37
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1


Signal: 2

Not Detected
Expected RT: 2.07

Processing Integration Results



Manual Integration Results



RT: 2.07
Area: 118540
Amount: 5.796863
Amount Units: ng/ml

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_040.d
Injection Date: 31-Jan-2018 13:40:45 Instrument ID: A8_N
Lims ID: 320-35046-A-16-A Lab Sample ID: 320-35046-16
Client ID: WGNA-011118-RW-3409
Operator ID: SACINSTLCMS01 ALS Bottle#: 36 Worklist Smp#: 37
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.07

Processing Integration Results



Manual Integration Results

RT: 2.07
Area: 645923
Amount: 5.796863
Amount Units: ng/ml



FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: WGNA-011118-FRB-3409 Lab Sample ID: 320-35046-17
 Matrix: Water Lab File ID: 2018.01.31_537A_043.d
 Analysis Method: 537 Date Collected: 01/11/2018 15:05
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 261.5 (mL) Date Analyzed: 01/31/2018 13:54
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206412 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	7.6	U	19	7.6	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	29	11	5.3
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	U	9.6	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	86	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	99		70-130
STL00996	13C2 PFDA	101		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_043.d
 Lims ID: 320-35046-A-17-A
 Client ID: WGNA-011118-FRB-3409
 Sample Type: Client
 Inject. Date: 31-Jan-2018 13:54:46 ALS Bottle#: 37 Worklist Smp#: 40
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35046-a-17-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:28:41 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK006

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
\$ 2 13C2 PFHxA	315.00 > 270.00	1.495	1.487	0.008	1.000	1606909	9.86	8893	
* 6 13C2-PFOA	415.00 > 370.00	1.821	1.813	0.008		1481492	10.0	6721	
* 7 13C4 PFOS	503.00 > 80.00	2.071	2.071	0.0		3346629	28.7	8140	
\$ 10 13C2 PFDA	515.00 > 470.00	2.253	2.246	0.007	1.000	1145385	10.1	8102	

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_043.d

Injection Date: 31-Jan-2018 13:54:46

Instrument ID: A8_N

Lims ID: 320-35046-A-17-A

Lab Sample ID: 320-35046-17

Client ID: WGNA-011118-FRB-3409

Operator ID: SACINSTLCMS01

ALS Bottle#: 37

Worklist Smp#: 40




Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL




1 Perfluorobutanesulfonic acid (ND) 1 Perfluorobutanesulfonic acid (ND) \$ 2 13C2 PFHxA






3 Perfluorohexanesulfonic acid (ND) 4 Perfluoroheptanoic acid (ND) * 6 13C2-PFOA




5 Perfluorooctanoic acid (ND) 5 Perfluorooctanoic acid (ND) 8 Perfluorooctane sulfonic acid (ND)



8 Perfluorooctane sulfonic acid (ND) * 7 13C4 PFOS 9 Perfluorononanoic acid (ND)



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_043.d
 Lims ID: 320-35046-A-17-A
 Client ID: WGNA-011118-FRB-3409
 Sample Type: Client
 Inject. Date: 31-Jan-2018 13:54:46 ALS Bottle#: 37 Worklist Smp#: 40
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35046-a-17-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:28:41 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK006

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	9.86	98.58
\$ 10 13C2 PFDA	10.0	10.1	101.04

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: WGNA-011118-RW-3220 Lab Sample ID: 320-35046-18
 Matrix: Water Lab File ID: 2018.01.31_537A_044.d
 Analysis Method: 537 Date Collected: 01/11/2018 16:10
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 267.7(mL) Date Analyzed: 01/31/2018 13:59
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206412 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	38	M	37	15	6.4
335-67-1	Perfluorooctanoic acid (PFOA)	13	J	19	7.5	2.6
375-95-1	Perfluorononanoic acid (PFNA)	19	U	22	19	7.5
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	17	J	28	11	5.1
375-85-9	Perfluoroheptanoic acid (PFHpA)	8.0	J	9.3	3.7	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	110		84	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	85		70-130
STL00996	13C2 PFDA	97		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_044.d
 Lims ID: 320-35046-A-18-A
 Client ID: WGNA-011118-RW-3220
 Sample Type: Client
 Inject. Date: 31-Jan-2018 13:59:26 ALS Bottle#: 38 Worklist Smp#: 41
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35046-a-18-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:28:41 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK006

First Level Reviewer: barnettj Date: 31-Jan-2018 16:26:19

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.366	1.366	0.0	1.000	3677694	29.0		3342	
298.90 > 99.00	1.366	1.366	0.0	1.000	2726266		1.35(0.00-0.00)	4502	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.487	1.487	0.0	1.000	1475957	8.52		7944	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.631	1.631	0.0	1.000	922942	4.68		536	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.631	1.631	0.0	1.000	313826	2.13		61.7	
* 6 13C2-PFOA									
415.00 > 370.00	1.813	1.813	0.0		1573796	10.0		7221	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.821	1.821	0.0	1.000	494018	3.39		60.1	
413.00 > 169.00	1.813	1.821	-0.008	0.996	276735		1.79(0.00-0.00)	758	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.071	2.071	0.0	1.000	1120089	10.1		477	Ma
499.00 > 99.00	2.064	2.071	-0.007	0.996	237070		4.72(0.00-0.00)	347	M
* 7 13C4 PFOS									
503.00 > 80.00	2.064	2.071	-0.007		3375758	28.7		3698	
9 Perfluorononanoic acid									
463.00 > 419.00	2.079	2.079	0.0	1.000	65916	0.6306		12.4	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.246	2.246	0.0	1.000	1166315	9.68		9342	

QC Flag Legend

Review Flags

M - Manually Integrated

a - User Assigned ID

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_044.d

Injection Date: 31-Jan-2018 13:59:26

Instrument ID: A8_N

Lims ID: 320-35046-A-18-A

Lab Sample ID: 320-35046-18

Client ID: WGNA-011118-RW-3220

Operator ID: SACINSTLCMS01

ALS Bottle#: 38

Worklist Smp#: 41

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_044.d
 Lims ID: 320-35046-A-18-A
 Client ID: WGNA-011118-RW-3220
 Sample Type: Client
 Inject. Date: 31-Jan-2018 13:59:26 ALS Bottle#: 38 Worklist Smp#: 41
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35046-a-18-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:28:41 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK006

First Level Reviewer: barnettj Date: 31-Jan-2018 16:26:19

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	8.52	85.24
\$ 10 13C2 PFDA	10.0	9.68	96.85

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_044.d
Injection Date: 31-Jan-2018 13:59:26 Instrument ID: A8_N
Lims ID: 320-35046-A-18-A Lab Sample ID: 320-35046-18
Client ID: WGNA-011118-RW-3220
Operator ID: SACINSTLCMS01 ALS Bottle#: 38 Worklist Smp#: 41
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected
Expected RT: 2.07

Processing Integration Results



Manual Integration Results

RT: 2.06
Area: 237070
Amount: 10.134878
Amount Units: ng/ml



Reviewer: barnettj, 31-Jan-2018 16:26:02
Audit Action: Manually Integrated

Audit Reason: Assign Peak
Page 234 of 391

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_044.d
Injection Date: 31-Jan-2018 13:59:26 Instrument ID: A8_N
Lims ID: 320-35046-A-18-A Lab Sample ID: 320-35046-18
Client ID: WGNA-011118-RW-3220
Operator ID: SACINSTLCMS01 ALS Bottle#: 38 Worklist Smp#: 41
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.07

Processing Integration Results



RT: 2.07
Area: 1120089
Amount: 10.134878
Amount Units: ng/ml

Manual Integration Results



FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: WGNA-011118-FRB-3220 Lab Sample ID: 320-35046-19
 Matrix: Water Lab File ID: 2018.01.31_537A_045.d
 Analysis Method: 537 Date Collected: 01/11/2018 16:05
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 271.7(mL) Date Analyzed: 01/31/2018 14:04
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206412 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	37	15	6.3
335-67-1	Perfluorooctanoic acid (PFOA)	7.4	U	18	7.4	2.6
375-95-1	Perfluorononanoic acid (PFNA)	18	U	22	18	7.4
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.1
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.7	U	9.2	3.7	1.7
375-73-5	Perfluorobutanesulfonic acid (PFBS)	33	U	83	33	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	95		70-130
STL00996	13C2 PFDA	101		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_045.d
 Lims ID: 320-35046-A-19-A
 Client ID: WGNA-011118-FRB-3220
 Sample Type: Client
 Inject. Date: 31-Jan-2018 14:04:06 ALS Bottle#: 39 Worklist Smp#: 42
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35046-a-19-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:28:41 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK006

First Level Reviewer: barnettj Date: 31-Jan-2018 16:28:41

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
\$ 2 13C2 PFHxA	315.00 > 270.00	1.487	1.487	0.0	1.000	1586546	9.48	9208	
* 6 13C2-PFOA	415.00 > 370.00	1.813	1.813	0.0		1520384	10.0	6595	
* 7 13C4 PFOS	503.00 > 80.00	2.064	2.071	-0.007		3387119	28.7	6507	
\$ 10 13C2 PFDA	515.00 > 470.00	2.246	2.246	0.0	1.000	1171645	10.1	8853	

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_045.d

Injection Date: 31-Jan-2018 14:04:06

Instrument ID: A8_N

Lims ID: 320-35046-A-19-A

Lab Sample ID: 320-35046-19

Client ID: WGNA-011118-FRB-3220

Operator ID: SACINSTLCMS01

ALS Bottle#: 39

Worklist Smp#: 42




Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL




1 Perfluorobutanesulfonic acid (ND) 1 Perfluorobutanesulfonic acid (ND) \$ 2 13C2 PFHxA






3 Perfluorohexanesulfonic acid (ND) 4 Perfluoroheptanoic acid (ND) * 6 13C2-PFOA




5 Perfluorooctanoic acid (ND) 5 Perfluorooctanoic acid (ND) 8 Perfluorooctane sulfonic acid (ND)



8 Perfluorooctane sulfonic acid (ND) * 7 13C4 PFOS 9 Perfluorononanoic acid (ND)



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_045.d
 Lims ID: 320-35046-A-19-A
 Client ID: WGNA-011118-FRB-3220
 Sample Type: Client
 Inject. Date: 31-Jan-2018 14:04:06 ALS Bottle#: 39 Worklist Smp#: 42
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35046-a-19-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:28:41 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK006

First Level Reviewer: barnettj Date: 31-Jan-2018 16:28:41

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	9.48	94.84
\$ 10 13C2 PFDA	10.0	10.1	100.71

FORM VI
LCMS BY INTERNAL STANDARD - INITIAL CALIBRATION DATA
CURVE EVALUATION

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1 Analy Batch No.: 192908

SDG No.: _____

Instrument ID: A8_N GC Column: GeminiC18 3 ID: 3(mm) Heated Purge: (Y/N) N

Calibration Start Date: 11/03/2017 13:37 Calibration End Date: 11/03/2017 14:01 Calibration ID: 36012

Calibration Files:

LEVEL:	LAB SAMPLE ID:	LAB FILE ID:
Level 1	IC 320-192908/4	2017.11.03_537XICAL_004.d
Level 2	IC 320-192908/5	2017.11.03_537XICAL_005.d
Level 3	IC 320-192908/6	2017.11.03_537XICAL_006.d
Level 4	IC 320-192908/7	2017.11.03_537XICAL_007.d
Level 5	IC 320-192908/8	2017.11.03_537XICAL_008.d
Level 6	IC 320-192908/9	2017.11.03_537XICAL_009.d

ANALYTE	RRF					CURVE TYPE	COEFFICIENT			#	MIN RRF	%RSD	#	MAX %RSD	R ² OR COD	#	MIN R ² OR COD
	LVL 1 LVL 6	LVL 2	LVL 3	LVL 4	LVL 5		B	M1	M2								
Perfluorobutanesulfonic acid (PFBS)	1.0397 0.8468	1.0767	1.0898	0.9577	0.9303	QuaF		1.1193	-0.001498					0.9990			0.9600
Perfluoroheptanoic acid (PFHpA)	0.9433 0.9848	0.9187	0.9551	0.9185	0.9011	Ave		0.9369			3.2		30.0				
Perfluorohexanesulfonic acid (PFHxS)	1.6459 1.6841	1.6355	1.7405	1.6631	1.6755	Ave		1.6741			2.2		30.0				
Perfluorooctanoic acid (PFOA)	0.9757 0.9799	0.8919	0.9000	0.8953	0.9117	Ave		0.9258			4.4		30.0				
Perfluorooctanesulfonic acid (PFOS)	0.8958 0.9902	0.9213	0.9281	0.9268	0.9715	Ave		0.9389			3.7		30.0				
Perfluorononanoic acid (PFNA)	0.6610 0.7042	0.6285	0.6624	0.6810	0.6478	Ave		0.6642			3.9		30.0				
13C2 PFHxA	1.0891 1.1664	1.0526	1.1042	1.1123	1.0772	Ave		1.1003			3.5		30.0				
13C2 PFDA	0.7748 0.8159	0.7295	0.7569	0.7811	0.7330	Ave		0.7652			4.3		30.0				

Note: The M1 coefficient is the same as Ave RRF for an Ave curve type.

FORM VI
 LCMS BY INTERNAL STANDARD - INITIAL CALIBRATION DATA
 RESPONSE AND CONCENTRATION

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1 Analy Batch No.: 192908

SDG No.: _____

Instrument ID: A8_N GC Column: GeminiC18 3 ID: 3(mm) Heated Purge: (Y/N) N

Calibration Start Date: 11/03/2017 13:37 Calibration End Date: 11/03/2017 14:01 Calibration ID: 36012

Calibration Files:

LEVEL:	LAB SAMPLE ID:	LAB FILE ID:
Level 1	IC 320-192908/4	2017.11.03_537XICAL_004.d
Level 2	IC 320-192908/5	2017.11.03_537XICAL_005.d
Level 3	IC 320-192908/6	2017.11.03_537XICAL_006.d
Level 4	IC 320-192908/7	2017.11.03_537XICAL_007.d
Level 5	IC 320-192908/8	2017.11.03_537XICAL_008.d
Level 6	IC 320-192908/9	2017.11.03_537XICAL_009.d

ANALYTE	IS REF	CURVE TYPE	RESPONSE					CONCENTRATION (NG/ML)				
			LVL 1 LVL 6	LVL 2	LVL 3	LVL 4	LVL 5	LVL 1 LVL 6	LVL 2	LVL 3	LVL 4	LVL 5
Perfluorobutanesulfonic acid (PFBS)	PFOS	QuaF	1076553 16699152	2591121	5461974	10142530	14011858	9.00 180	20.0	45.0	90.0	135
Perfluoroheptanoic acid (PFHpA)	13PF OA	Ave	143455 2810797	331548	736034	1420703	2102676	1.00 20.0	2.22	5.00	10.0	15.0
Perfluorohexanesulfonic acid (PFHxS)	PFOS	Ave	568156 11071993	1312135	2908204	5871843	8413133	3.00 60.0	6.67	15.0	30.0	45.0
Perfluorooctanoic acid (PFOA)	13PF OA	Ave	296934 5597122	644149	1388033	2771271	4257225	2.00 40.0	4.45	10.0	20.0	30.0
Perfluorooctanesulfonic acid (PFOS)	PFOS	Ave	412315 8679676	985487	2067792	4363079	6504279	4.00 80.0	8.89	20.0	40.0	60.0
Perfluorononanoic acid (PFNA)	13PF OA	Ave	201053 4019666	453612	1020851	2106479	3023088	2.00 40.0	4.45	10.0	20.0	30.0
13C2 PFHxA	13PF OA	Ave	1655691 1664260	1708988	1701491	1719911	1675220	10.0 10.0	10.0	10.0	10.0	10.0
13C2 PFDA	13PF OA	Ave	1177922 1164156	1184358	1166275	1207887	1139992	10.0 10.0	10.0	10.0	10.0	10.0

Curve Type Legend:

Ave = Average ISTD
QuaF = Quadratic ISTD forced zero

FORM VI
 LCMS BY INTERNAL STANDARD - INITIAL CALIBRATION DATA
 READBACK PERCENT ERROR

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1 Analy Batch No.: 192908

SDG No.: _____


Instrument ID: A8_N GC Column: GeminiC18 3 ID: 3 (mm) Heated Purge: (Y/N) N


Calibration Start Date: 11/03/2017 13:37 Calibration End Date: 11/03/2017 14:01 Calibration ID: 36012

Calibration Files:

LEVEL:	LAB SAMPLE ID:	LAB FILE ID:
Level 1	IC 320-192908/4	2017.11.03_537XICAL_004.d
Level 2	IC 320-192908/5	2017.11.03_537XICAL_005.d
Level 3	IC 320-192908/6	2017.11.03_537XICAL_006.d
Level 4	IC 320-192908/7	2017.11.03_537XICAL_007.d
Level 5	IC 320-192908/8	2017.11.03_537XICAL_008.d
Level 6	IC 320-192908/9	2017.11.03_537XICAL_009.d

ANALYTE	PERCENT ERROR						PERCENT ERROR LIMIT					
	LVL 1 #	LVL 2 #	LVL 3 #	LVL 4 #	LVL 5 #	LVL 6 #	LVL 1	LVL 2	LVL 3	LVL 4	LVL 5	LVL 6
Perfluorobutanesulfonic acid (PFBS)	-6.0	-1.2	3.9	-3.1	1.9	-0.5	50	30	30	30	30	30
Perfluoroheptanoic acid (PFHpA)	0.7	-1.9	1.9	-2.0	-3.8	5.1	50	30	30	30	30	30
Perfluorohexanesulfonic acid (PFHxS)	-1.7	-2.3	4.0	-0.7	0.1	0.6	50	30	30	30	30	30
Perfluorooctanoic acid (PFOA)	5.4	-3.7	-2.8	-3.3	-1.5	5.8	50	30	30	30	30	30
Perfluorooctanesulfonic acid (PFOS)	-4.6	-1.9	-1.2	-1.3	3.5	5.5	50	30	30	30	30	30
Perfluorononanoic acid (PFNA)	-0.5	-5.4	-0.3	2.5	-2.5	6.0	50	30	30	30	30	30
13C2 PFHxA	-1.0	-4.3	0.4	1.1	-2.1	6.0	30	30	30	30	30	30
13C2 PFDA	1.3	-4.7	-1.1	2.1	-4.2	6.6	30	30	30	30	30	30





TestAmerica Laboratories
Istd/Surrogate Recovery Report

Worklist Name: 03NOV2017_537A_ICAL

Worklist Num: 49975

Instrument: A8_N

Method: 537_A8_N

Batch Directory: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b

Limit Group: LC 537 ICAL

Analysis Type: SemiVOA

Inj Volume: 2.00

Inj Vol Units: ul

Lims Batch: 192908

CCV IS Mode: Select Ical Level, Cal Level: 3

Non-Cal IS Mode: Last Ccal Sample

\$ 2 13C2 PFHxA

\$ 10 13C2 PFDA

Lab ID	Inj Date	\$ 2	\$ 10	* 6 13C2-PFOA	* 7 13C4 PFOS
	IS Std			2864400 1.87	6253426 2.11
# 1 RB	03-Nov-2017 13:23:59			1485386 51.9	3471256 55.5
# 2 RB	03-Nov-2017 13:28:38			1511056 52.8	3340239 53.4
# 3 RB	03-Nov-2017 13:33:19			1483949 51.8	3285228 52.5
	IS Std				
# 4 IC L1	03-Nov-2017 13:37:59	1.58 98.98	2.31 101.30	1520258> 100.0*	3298877> 100.0*
# 5 IC L2	03-Nov-2017 13:42:39	1.58 95.66	2.31 95.33	1623614> 106.8*	3450592> 104.6*
# 6 IC L3	03-Nov-2017 13:47:20	1.57 100.40	2.31 98.91	1540946> 101.4*	3194016> 96.8*
# 7 IC L4	03-Nov-2017 13:52:00	1.57 101.10	2.31 102.10	1546307> 101.7*	3374600> 102.3*
# 8 IC L5	03-Nov-2017 13:56:41	1.57 97.90	2.31 95.80	1555174> 102.3*	3199479> 97.0*
# 9 IC L6	03-Nov-2017 14:01:24	1.57 106.00	2.31 106.60	1426806> 93.9*	3141787> 95.2*
	IS Std			1540946 1.91	3194016 2.15
#10 RB	03-Nov-2017 14:06:04			1395383 90.6	3212781 100.6
	IS Std			1546307 1.91	3374600 2.16
#11 CCVL	03-Nov-2017 14:10:44	1.58 97.03	2.31 97.49	1586829 102.6	3305852 98.0
	IS Std			1586829 1.91	3305852 2.15
#12 RB	03-Nov-2017 14:15:23			1415042 89.2	3122656 94.5
	IS Std			1546307 1.91	3374600 2.16
#13 ICV	03-Nov-2017 14:20:03	1.57 94.41	2.31 96.59	1512045 97.8	3433628 101.7
	IS Std			1395100 1.91	3254950 2.15
#14 RB	03-Nov-2017 14:24:44			1395100 100.0	3254950 100.0

13C2-PFOA

$$RPD = \frac{1623614 - 1426806}{\left(\frac{1623614 + 1426806}{2}\right)} (100) = 12.9$$

13C4-PFOS

$$RPD = \frac{3450592 - 3141787}{\left(\frac{3450592 + 3141787}{2}\right)} (100) = 9.37$$

JRB
11-6-17

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_004.d
 Lims ID: IC L1
 Client ID:
 Sample Type: IC Calib Level: 1
 Inject. Date: 03-Nov-2017 13:37:59 ALS Bottle#: 1 Worklist Smp#: 4
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: L1_537
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub1

Method: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Nov-2017 15:52:07 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK021

First Level Reviewer: phomsophat Date: 06-Nov-2017 07:18:01

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.449	1.444	0.005	1.000	1076553	8.46		654	
298.90 > 99.00	1.449	1.444	0.005	1.000	763262		1.41(0.00-0.00)	2025	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.578	1.573	0.005	1.000	1655691	9.90		8732	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.730	1.725	0.005	1.000	568156	2.95		1122	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.730	1.725	0.005	1.000	143455	1.01		42.2	
* 6 13C2-PFOA									
415.00 > 370.00	1.920	1.913	0.007		1520258	10.0		6863	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.920	1.914	0.006	1.000	296934	2.11		53.5	
413.00 > 169.00	1.920	1.914	0.006	1.000	149720		1.98(0.00-0.00)	184	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.155	2.147	0.008	1.000	412315	3.82		235	M
499.00 > 99.00	2.155	2.147	0.008	1.000	85347		4.83(0.00-0.00)	209	M
* 7 13C4 PFOS									
503.00 > 80.00	2.155	2.151	0.004		3298877	28.7		5279	
9 Perfluorononanoic acid									
463.00 > 419.00	2.162	2.158	0.004	1.000	201053	1.99		67.8	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.314	2.312	0.002	1.000	1177922	10.1		7012	

QC Flag Legend

Review Flags

M - Manually Integrated

Reagents:

LC537-L1_00020

Amount Added: 1.00

Units: mL

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537ICAL_004.d

Injection Date: 03-Nov-2017 13:37:59

Instrument ID: A8_N

Lims ID: IC L1

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 1

Worklist Smp#: 4

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_004.d
Injection Date: 03-Nov-2017 13:37:59 Instrument ID: A8_N
Lims ID: IC L1
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 1 Worklist Smp#: 4
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.15

Processing Integration Results



Manual Integration Results

RT: 2.15
Area: 412315
Amount: 3.817687
Amount Units: ng/ml



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\201711106-49975.b\2017.11.03_537XICAL_004.d
Injection Date: 03-Nov-2017 13:37:59 Instrument ID: A8_N
Lims ID: IC L1
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 1 Worklist Smp#: 4
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected
Expected RT: 2.15

Processing Integration Results



Manual Integration Results

RT: 2.15
Area: 85347
Amount: 3.817687
Amount Units: ng/ml



Reviewer: phomsophat, 06-Nov-2017 07:17:37

Audit Action: Manually Integrated

Audit Reason: Assign Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\201711106-49975.b\2017.11.03_537XICAL_004.d
Injection Date: 03-Nov-2017 13:37:59 Instrument ID: A8_N
Lims ID: IC L1
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 1 Worklist Smp#: 4
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.15

Processing Integration Results



Manual Integration Results

RT: 2.15
Area: 412315
Amount: 3.817687
Amount Units: ng/ml



Reviewer: phomsophat, 06-Nov-2017 07:17:37

Audit Action: Manually Integrated

Audit Reason: Assign Peak

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_005.d
 Lims ID: IC L2
 Client ID:
 Sample Type: IC Calib Level: 2
 Inject. Date: 03-Nov-2017 13:42:39 ALS Bottle#: 2 Worklist Smp#: 5
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: L2_537
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub1

Method: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Nov-2017 15:52:08 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK021

First Level Reviewer: phomsophat Date: 06-Nov-2017 07:18:56

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.449	1.444	0.005	1.000	2591121	19.8		1479	
298.90 > 99.00	1.442	1.444	-0.002	0.995	1874928		1.38(0.00-0.00)	4315	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.578	1.573	0.005	1.000	1708988	9.57		8562	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.730	1.725	0.005	1.000	331548	2.18		87.8	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.730	1.725	0.005	1.000	1312135	6.51		2317	
* 6 13C2-PFOA									
415.00 > 370.00	1.920	1.913	0.007		1623614	10.0		6970	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.920	1.914	0.006	1.000	644149	4.29		113	
413.00 > 169.00	1.920	1.914	0.006	1.000	329479		1.96(0.00-0.00)	459	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.155	2.147	0.008	1.000	985487	8.72		578	M
499.00 > 99.00	2.155	2.147	0.008	1.000	200739		4.91(0.00-0.00)	449	M
* 7 13C4 PFOS									
503.00 > 80.00	2.155	2.151	0.004		3450592	28.7		5334	
9 Perfluorononanoic acid									
463.00 > 419.00	2.162	2.158	0.004	1.000	453612	4.21		136	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.314	2.312	0.002	1.000	1184358	9.53		7573	

QC Flag Legend

Review Flags

M - Manually Integrated

Reagents:

LC537-L2_00020

Amount Added: 1.00

Units: mL

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_005.d

Injection Date: 03-Nov-2017 13:42:39

Instrument ID: A8_N

Lims ID: IC L2

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 2

Worklist Smp#: 5

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



4 Perfluoroheptanoic acid

3 Perfluorohexanesulfonic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_005.d
Injection Date: 03-Nov-2017 13:42:39 Instrument ID: A8_N
Lims ID: IC L2
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 2 Worklist Smp#: 5
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.15

Processing Integration Results



Manual Integration Results

RT: 2.15
Area: 985487
Amount: 8.723576
Amount Units: ng/ml



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\201711106-49975.b\2017.11.03_537XICAL_005.d
Injection Date: 03-Nov-2017 13:42:39 Instrument ID: A8_N
Lims ID: IC L2
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 2 Worklist Smp#: 5
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected
Expected RT: 2.15

Processing Integration Results



RT: 2.15
Area: 200739
Amount: 8.723576
Amount Units: ng/ml

Manual Integration Results



Reviewer: phomsophat, 06-Nov-2017 07:18:24

Audit Action: Manually Integrated

Audit Reason: Assign Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\201711106-49975.b\2017.11.03_537XICAL_005.d
Injection Date: 03-Nov-2017 13:42:39 Instrument ID: A8_N
Lims ID: IC L2
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 2 Worklist Smp#: 5
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.15

Processing Integration Results



RT: 2.15
Area: 985487
Amount: 8.723576
Amount Units: ng/ml

Manual Integration Results



Reviewer: phomsophat, 06-Nov-2017 07:18:24

Audit Action: Manually Integrated

Audit Reason: Assign Peak

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_006.d
 Lims ID: IC L3
 Client ID:
 Sample Type: IC Calib Level: 3
 Inject. Date: 03-Nov-2017 13:47:20 ALS Bottle#: 3 Worklist Smp#: 6
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: L3_537
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub1

Method: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Nov-2017 15:52:09 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK021

First Level Reviewer: phomsophat Date: 06-Nov-2017 07:20:04

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.442	1.444	-0.002	1.000	5461974	46.7		3220	
298.90 > 99.00	1.442	1.444	-0.002	1.000	3903438		1.40(0.00-0.00)	8589	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.571	1.573	-0.003	1.000	1701491	10.0		9021	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.722	1.725	-0.003	1.000	2908204	15.6		5000	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.722	1.725	-0.003	1.000	736034	5.10		208	
* 6 13C2-PFOA									
415.00 > 370.00	1.912	1.913	-0.001		1540946	10.0		6787	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.912	1.914	-0.002	1.000	1388033	9.73		256	
413.00 > 169.00	1.912	1.914	-0.002	1.000	715399		1.94(0.00-0.00)	904	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.147	2.147	0.0	1.000	2067792	19.8		2001	
499.00 > 99.00	2.147	2.147	0.0	1.000	431075		4.80(0.00-0.00)	922	
* 7 13C4 PFOS									
503.00 > 80.00	2.147	2.151	-0.004		3194016	28.7		4956	
9 Perfluorononanoic acid									
463.00 > 419.00	2.155	2.158	-0.003	1.000	1020851	9.97		302	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.306	2.312	-0.006	1.000	1166275	9.89		6310	

Reagents:

LC537-L3_00023

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537ICAL_006.d

Injection Date: 03-Nov-2017 13:47:20

Instrument ID: A8_N

Lims ID: IC L3

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 3

Worklist Smp#: 6

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid




8 Perfluorooctane sulfonic acid

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_007.d
 Lims ID: IC L4
 Client ID:
 Sample Type: ICISAV Calib Level: 4
 Inject. Date: 03-Nov-2017 13:52:00 ALS Bottle#: 4 Worklist Smp#: 7
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: L4_537
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub1

Method: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Nov-2017 15:52:10 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK021

First Level Reviewer: phomsophat Date: 06-Nov-2017 07:20:46

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.442	1.444	-0.002	1.000	10142530	87.2		5274	
298.90 > 99.00	1.442	1.444	-0.002	1.000	7408390		1.37(0.00-0.00)	12862	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.571	1.573	-0.003	1.000	1719911	10.1		8503	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.722	1.725	-0.003	1.000	1420703	9.81		399	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.722	1.725	-0.003	1.000	5871843	29.8		7622	
* 6 13C2-PFOA									
415.00 > 370.00	1.912	1.913	-0.001		1546307	10.0		6563	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.912	1.914	-0.002	1.000	2771271	19.4		505	
413.00 > 169.00	1.912	1.914	-0.002	1.000	1520933		1.82(0.00-0.00)	1919	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.155	2.147	0.008	1.000	4363079	39.5		3896	M
499.00 > 99.00	2.155	2.147	0.008	1.000	902486		4.83(0.00-0.00)	1588	M
* 7 13C4 PFOS									
503.00 > 80.00	2.155	2.151	0.004		3374600	28.7		5331	
9 Perfluorononanoic acid									
463.00 > 419.00	2.162	2.158	0.004	1.000	2106479	20.5		638	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.314	2.312	0.002	1.000	1207887	10.2		7165	

QC Flag Legend

Review Flags

M - Manually Integrated

Reagents:

LC537-L4_00020

Amount Added: 1.00

Units: mL

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537ICAL_007.d

Injection Date: 03-Nov-2017 13:52:00

Instrument ID: A8_N

Lims ID: IC L4

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 4

Worklist Smp#: 7

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



4 Perfluoroheptanoic acid

3 Perfluorohexanesulfonic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_007.d
Injection Date: 03-Nov-2017 13:52:00 Instrument ID: A8_N
Lims ID: IC L4
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 4 Worklist Smp#: 7
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.15

Processing Integration Results



Manual Integration Results

RT: 2.15
Area: 4363079
Amount: 39.491903
Amount Units: ng/ml



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\201711106-49975.b\2017.11.03_537XICAL_007.d
Injection Date: 03-Nov-2017 13:52:00 Instrument ID: A8_N
Lims ID: IC L4
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 4 Worklist Smp#: 7
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected
Expected RT: 2.15

Processing Integration Results



Manual Integration Results

RT: 2.15
Area: 902486
Amount: 39.491903
Amount Units: ng/ml



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\201711106-49975.b\2017.11.03_537XICAL_007.d
Injection Date: 03-Nov-2017 13:52:00 Instrument ID: A8_N
Lims ID: IC L4
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 4 Worklist Smp#: 7
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.15

Processing Integration Results



RT: 2.15
Area: 4363079
Amount: 39.491903
Amount Units: ng/ml

Manual Integration Results



Reviewer: phomsophat, 06-Nov-2017 07:20:20

Audit Action: Manually Integrated

Audit Reason: Assign Peak

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_008.d
 Lims ID: IC L5
 Client ID:
 Sample Type: IC Calib Level: 5
 Inject. Date: 03-Nov-2017 13:56:41 ALS Bottle#: 5 Worklist Smp#: 8
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: L5_537
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub1

Method: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Nov-2017 15:52:11 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK021

First Level Reviewer: phomsophat Date: 06-Nov-2017 07:21:19

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.442	1.444	-0.002	1.000	14011858	137.5		6452	
298.90 > 99.00	1.442	1.444	-0.002	1.000	10411479		1.35(0.00-0.00)	14800	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.571	1.573	-0.003	1.000	1675220	9.79		9525	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.722	1.725	-0.003	1.000	8413133	45.0		9078	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.722	1.725	-0.003	1.000	2102676	14.4		562	
* 6 13C2-PFOA									
415.00 > 370.00	1.912	1.913	-0.001		1555174	10.0		6769	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.912	1.914	-0.002	1.000	4257225	29.6		800	
413.00 > 169.00	1.912	1.914	-0.002	1.000	2294552		1.86(0.00-0.00)	2838	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.147	2.147	0.0	1.000	6504279	62.1		5682	
499.00 > 99.00	2.147	2.147	0.0	1.000	1339120		4.86(0.00-0.00)	2329	
* 7 13C4 PFOS									
503.00 > 80.00	2.147	2.151	-0.004		3199479	28.7		4946	
9 Perfluorononanoic acid									
463.00 > 419.00	2.155	2.158	-0.003	1.000	3023088	29.3		870	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.314	2.312	0.002	1.000	1139992	9.58		5885	

Reagents:

LC537-L5_00024

Amount Added: 1.00

Units: mL

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537ICAL_008.d

Injection Date: 03-Nov-2017 13:56:41

Instrument ID: A8_N

Lims ID: IC L5

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 5

Worklist Smp#: 8

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid




8 Perfluorooctane sulfonic acid

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Lims ID: IC L6
 Client ID:
 Sample Type: IC Calib Level: 6
 Inject. Date: 03-Nov-2017 14:01:24 ALS Bottle#: 6 Worklist Smp#: 9
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: L6_537
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub1

Method: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Nov-2017 15:52:12 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK021

First Level Reviewer: phomsophat Date: 06-Nov-2017 07:25:41

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.442	1.444	-0.002	1.000	16699152	179.1		7089	
298.90 > 99.00	1.442	1.444	-0.002	1.000	12929978		1.29(0.00-0.00)	15608	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.571	1.573	-0.003	1.000	1664260	10.6		9116	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.722	1.725	-0.003	1.000	2810797	21.0		763	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.722	1.725	-0.003	1.000	11071993	60.4		10884	
* 6 13C2-PFOA									
415.00 > 370.00	1.904	1.913	-0.009		1426806	10.0		5446	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.912	1.914	-0.002	1.000	5597122	42.4		962	
413.00 > 169.00	1.904	1.914	-0.010	0.996	3028676		1.85(0.00-0.00)	3704	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.147	2.147	0.0	1.000	8679676	84.4		6114	
499.00 > 99.00	2.147	2.147	0.0	1.000	1807143		4.80(0.00-0.00)	2991	
* 7 13C4 PFOS									
503.00 > 80.00	2.147	2.151	-0.004		3141787	28.7		4961	
9 Perfluorononanoic acid									
463.00 > 419.00	2.155	2.158	-0.003	1.000	4019666	42.4		1149	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.306	2.312	-0.006	1.000	1164156	10.7		6124	

Reagents:

LC537-L6_00020

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537ICAL_009.d

Injection Date: 03-Nov-2017 14:01:24

Instrument ID: A8_N

Lims ID: IC L6

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 6

Worklist Smp#: 9

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



4 Perfluoroheptanoic acid

3 Perfluorohexanesulfonic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid




8 Perfluorooctane sulfonic acid

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Lab Sample ID: CCVL 320-192908/11 Calibration Date: 11/03/2017 14:10
 Instrument ID: A8_N Calib Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 11/03/2017 14:01
 Lab File ID: 2017.11.03_537XICAL_011.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		1.109		20.4	20.0	1.9	50.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9369	0.9382		2.23	2.22	0.1	50.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.674	1.688		6.72	6.67	0.8	50.0
Perfluorooctanoic acid (PFOA)	Ave	0.9258	0.8825		4.24	4.45	-4.7	50.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9389	0.9176		8.69	8.89	-2.3	50.0
Perfluorononanoic acid (PFNA)	Ave	0.6642	0.6625		4.43	4.45	-0.2	50.0
13C2 PFHxA	Ave	1.100	1.068		9.70	10.0	-3.0	30.0
13C2 PFDA	Ave	0.7652	0.7460		9.75	10.0	-2.5	30.0

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_011.d
 Lims ID: CCVL
 Client ID:
 Sample Type: CCVL
 Inject. Date: 03-Nov-2017 14:10:44 ALS Bottle#: 2 Worklist Smp#: 11
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: CCV L2
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub1
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Nov-2017 15:39:07 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK021

First Level Reviewer: phomsophat Date: 06-Nov-2017 07:26:29

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.449	1.444	0.005	1.000	2556738	20.4		1537	
298.90 > 99.00	1.449	1.444	0.005	1.000	1750170		1.46(0.00-0.00)	4023	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.578	1.573	0.005	1.000	1694196	9.70		8915	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.730	1.725	0.005	1.000	1297654	6.72		2410	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.730	1.725	0.005	1.000	330927	2.23		99.4	
* 6 13C2-PFOA									
415.00 > 370.00	1.912	1.913	-0.001		1586829	10.0		6840	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.912	1.914	-0.002	1.000	622915	4.24		116	
413.00 > 169.00	1.912	1.914	-0.002	1.000	335080		1.86(0.00-0.00)	460	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.155	2.147	0.008	1.000	940397	8.69		528	
499.00 > 99.00	2.147	2.147	0.0	0.996	196397		4.79(0.00-0.00)	430	
* 7 13C4 PFOS									
503.00 > 80.00	2.147	2.151	-0.004		3305852	28.7		5135	
9 Perfluorononanoic acid									
463.00 > 419.00	2.162	2.158	0.004	1.000	467323	4.43		143	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.314	2.312	0.002	1.000	1183747	9.75		6763	

Reagents:

LC537-L2_00020

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_011.d

Injection Date: 03-Nov-2017 14:10:44

Instrument ID: A8_N

Lims ID: CCVL

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 2

Worklist Smp#: 11

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid




8 Perfluorooctane sulfonic acid

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Lab Sample ID: ICV 320-192908/13 Calibration Date: 11/03/2017 14:20
 Instrument ID: A8_N Calib Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 11/03/2017 14:01
 Lab File ID: 2017.11.03_537XICAL_013.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		0.8310		83.7	100	-16.4	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9369	0.8136		8.68	10.0	-13.2	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.674	1.463		17.5	20.1	-12.6	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9258	0.7995		17.7	20.5	-13.6	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9389	0.8637		18.1	19.7	-8.0	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6642	0.6428		19.5	20.1	-3.2	30.0
13C2 PFHxA	Ave	1.100	1.039		9.44	10.0	-5.6	30.0
13C2 PFDA	Ave	0.7652	0.7391		9.66	10.0	-3.4	30.0

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_013.d
 Lims ID: ICV
 Client ID:
 Sample Type: ICV
 Inject. Date: 03-Nov-2017 14:20:03 ALS Bottle#: 7 Worklist Smp#: 13
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: ICV
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist:

Method: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Nov-2017 15:39:08 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK021

First Level Reviewer: phomsophat Date: 06-Nov-2017 07:27:24

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.442	1.444	-0.002	1.000	9960387	83.7		4998	
298.90 > 99.00	1.442	1.444	-0.002	1.000	7235967		1.38(0.00-0.00)	13514	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.571	1.573	-0.003	1.000	1570629	9.44		8393	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.722	1.725	-0.003	1.000	3517469	17.5		5659	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.722	1.725	-0.003	1.000	1229696	8.68		345	
* 6 13C2-PFOA									
415.00 > 370.00	1.904	1.913	-0.009		1512045	10.0		7643	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.904	1.914	-0.010	1.000	2476221	17.7		475	
413.00 > 169.00	1.904	1.914	-0.010	1.000	1327388		1.87(0.00-0.00)	1724	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.140	2.147	-0.007	1.000	2036944	18.1		2323	
499.00 > 99.00	2.140	2.147	-0.007	1.000	389736		5.23(0.00-0.00)	830	
* 7 13C4 PFOS									
503.00 > 80.00	2.140	2.151	-0.011		3433628	28.7		5334	
9 Perfluorononanoic acid									
463.00 > 419.00	2.147	2.158	-0.011	1.000	1956116	19.5		652	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.306	2.312	-0.006	1.000	1117553	9.66		6230	

Reagents:

LC537-ICV_00028

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_013.d

Injection Date: 03-Nov-2017 14:20:03

Instrument ID: A8_N

Lims ID: ICV

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 7

Worklist Smp#: 13

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid




8 Perfluorooctane sulfonic acid

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Lab Sample ID: CCVL 320-206407/1 Calibration Date: 01/31/2018 10:52
 Instrument ID: A8_N Calib Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 11/03/2017 14:01
 Lab File ID: 2018.01.31_537A_004.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		1.094		20.1	20.0	0.4	50.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9369	0.9074		2.15	2.22	-3.2	50.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.674	1.681		6.69	6.67	0.4	50.0
Perfluorooctanoic acid (PFOA)	Ave	0.9258	0.8944		4.30	4.45	-3.4	50.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9389	0.9026		8.55	8.89	-3.9	50.0
Perfluorononanoic acid (PFNA)	Ave	0.6642	0.6340		4.24	4.45	-4.5	50.0
13C2 PFHxA	Ave	1.100	1.073		9.75	10.0	-2.5	30.0
13C2 PFDA	Ave	0.7652	0.7889		10.3	10.0	3.1	30.0

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_004.d
 Lims ID: CCVL
 Client ID:
 Sample Type: CCVL
 Inject. Date: 31-Jan-2018 10:52:35 ALS Bottle#: 2 Worklist Smp#: 1
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: CCV L2
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub1
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:27:16 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK006

First Level Reviewer: barnettj Date: 31-Jan-2018 15:58:25

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.373	1.373	0.0	1.000	2533247	20.1		4166	
298.90 > 99.00	1.373	1.373	0.0	1.000	1898440		1.33(0.00-0.00)	3404	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.495	1.495	0.0	1.000	1684478	9.75		8385	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.639	1.639	0.0	1.000	1297419	6.69		1386	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.639	1.639	0.0	1.000	316748	2.15		106	
* 6 13C2-PFOA									
415.00 > 370.00	1.836	1.821	0.015		1570514	10.0		6035	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.836	1.821	0.015	1.000	624791	4.30		108	
413.00 > 169.00	1.836	1.821	0.015	1.000	353036		1.77(0.00-0.00)	1010	
* 7 13C4 PFOS									
503.00 > 80.00	2.094	2.071	0.023		3320314	28.7		7469	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.094	2.071	0.023	1.000	929101	8.55		792	Ma
499.00 > 99.00	2.094	2.071	0.023	1.000	198284		4.69(0.00-0.00)	406	M
9 Perfluorononanoic acid									
463.00 > 419.00	2.102	2.079	0.023	1.000	442628	4.24		165	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.261	2.253	0.008	1.000	1238939	10.3		7270	

QC Flag Legend

Review Flags

M - Manually Integrated

a - User Assigned ID

Reagents:

LC537-L2_00020

Amount Added: 1.00

Units: mL

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_004.d

Injection Date: 31-Jan-2018 10:52:35

Instrument ID: A8_N

Lims ID: CCVL

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 2

Worklist Smp#: 1

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




* 7 13C4 PFOS




8 Perfluorooctane sulfonic acid (M)

8 Perfluorooctane sulfonic acid (M)

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_004.d
Injection Date: 31-Jan-2018 10:52:35 Instrument ID: A8_N
Lims ID: CCVL
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 2 Worklist Smp#: 1
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected
Expected RT: 2.07

Processing Integration Results



RT: 2.09
Area: 198284
Amount: 8.547145
Amount Units: ng/ml

Manual Integration Results



Reviewer: barnettj, 31-Jan-2018 15:58:08
Audit Action: Manually Integrated

Audit Reason: Assign Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_004.d
Injection Date: 31-Jan-2018 10:52:35 Instrument ID: A8_N
Lims ID: CCVL
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 2 Worklist Smp#: 1
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.07

Processing Integration Results



RT: 2.09
Area: 929101
Amount: 8.547145
Amount Units: ng/ml

Manual Integration Results



Reviewer: barnettj, 31-Jan-2018 15:58:08

Audit Action: Manually Integrated

Audit Reason: Assign Peak

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Lab Sample ID: CCV 320-206408/14 Calibration Date: 01/31/2018 11:53
 Instrument ID: A8_N Calib Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 11/03/2017 14:01
 Lab File ID: 2018.01.31_537A_017.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		1.062		45.5	45.0	1.0	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9369	0.9327		4.98	5.00	-0.5	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.674	1.745		15.6	15.0	4.3	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9258	0.8632		9.33	10.0	-6.8	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9389	0.9124		19.4	20.0	-2.8	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6642	0.6303		9.49	10.0	-5.1	30.0
13C2 PFHxA	Ave	1.100	1.097		9.97	10.0	-0.3	30.0
13C2 PFDA	Ave	0.7652	0.7539		9.85	10.0	-1.5	30.0

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_017.d
 Lims ID: CCV L3
 Client ID:
 Sample Type: CCVIS
 Inject. Date: 31-Jan-2018 11:53:20 ALS Bottle#: 3 Worklist Smp#: 14
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: CCV L3
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub1
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:27:39 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK006

First Level Reviewer: barnettj Date: 31-Jan-2018 16:00:51

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.373	1.373	0.0	1.000	5335628	45.5		7435	
298.90 > 99.00	1.373	1.373	0.0	1.000	4135322		1.29(0.00-0.00)	6300	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.495	1.495	0.0	1.000	1672582	9.97		8363	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.631	1.631	0.0	1.000	2923255	15.6		2915	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.631	1.631	0.0	1.000	710957	4.98		230	
* 6 13C2-PFOA									
415.00 > 370.00	1.821	1.821	0.0		1524185	10.0		5523	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.821	1.821	0.0	1.000	1316739	9.33		222	
413.00 > 169.00	1.821	1.821	0.0	1.000	733480		1.80(0.00-0.00)	2072	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.071	2.071	0.0	1.000	2037649	19.4		1505	Ma
499.00 > 99.00	2.079	2.071	0.008	1.004	427598		4.77(0.00-0.00)	692	M
* 7 13C4 PFOS									
503.00 > 80.00	2.071	2.071	0.0		3201796	28.7		6593	
9 Perfluorononanoic acid									
463.00 > 419.00	2.079	2.079	0.0	1.000	960875	9.49		300	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.253	2.253	0.0	1.000	1149033	9.85		6659	

QC Flag Legend

Review Flags

M - Manually Integrated

a - User Assigned ID

Reagents:

LC537-L3_00023

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_017.d

Injection Date: 31-Jan-2018 11:53:20

Instrument ID: A8_N

Lims ID: CCV L3

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 3

Worklist Smp#: 14

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_017.d
Injection Date: 31-Jan-2018 11:53:20 Instrument ID: A8_N
Lims ID: CCV L3
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 3 Worklist Smp#: 14
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected
Expected RT: 2.07

Processing Integration Results



Manual Integration Results

RT: 2.08
Area: 427598
Amount: 19.438959
Amount Units: ng/ml



Reviewer: barnettj, 31-Jan-2018 16:00:38
Audit Action: Manually Integrated

Audit Reason: Assign Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_017.d
Injection Date: 31-Jan-2018 11:53:20 Instrument ID: A8_N
Lims ID: CCV L3
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 3 Worklist Smp#: 14
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.07

Processing Integration Results



RT: 2.07
Area: 2037649
Amount: 19.438959
Amount Units: ng/ml

Manual Integration Results



FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Lab Sample ID: CCV 320-206408/26 Calibration Date: 01/31/2018 12:49
 Instrument ID: A8_N Calib Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 11/03/2017 14:01
 Lab File ID: 2018.01.31_537A_029.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		0.9466		141	135	4.2	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9369	0.9398		15.1	15.0	0.3	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.674	1.737		46.7	45.0	3.7	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9258	0.9631		31.2	30.0	4.0	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9389	0.9508		60.8	60.0	1.3	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6642	0.6784		30.6	30.0	2.1	30.0
13C2 PFHxA	Ave	1.100	1.151		10.5	10.0	4.6	30.0
13C2 PFDA	Ave	0.7652	0.8128		10.6	10.0	6.2	30.0

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Lab Sample ID: CCV 320-206410/26 Calibration Date: 01/31/2018 12:49
 Instrument ID: A8_N Calib Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 11/03/2017 14:01
 Lab File ID: 2018.01.31_537A_029.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		0.9466		141	135	4.2	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9369	0.9398		15.1	15.0	0.3	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.674	1.737		46.7	45.0	3.7	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9258	0.9631		31.2	30.0	4.0	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9389	0.9508		60.8	60.0	1.3	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6642	0.6784		30.6	30.0	2.1	30.0
13C2 PFHxA	Ave	1.100	1.151		10.5	10.0	4.6	30.0
13C2 PFDA	Ave	0.7652	0.8128		10.6	10.0	6.2	30.0

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_029.d
 Lims ID: CCV L5
 Client ID:
 Sample Type: CCVIS
 Inject. Date: 31-Jan-2018 12:49:26 ALS Bottle#: 5 Worklist Smp#: 26
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: CCV L5
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub1
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:28:14 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK006

First Level Reviewer: barnettj Date: 31-Jan-2018 16:01:34

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.366	1.366	0.0	1.000	14139035	140.7		12910	
298.90 > 99.00	1.366	1.366	0.0	1.000	11074671		1.28(0.00-0.00)	11878	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.487	1.487	0.0	1.000	1684592	10.5		8999	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.631	1.631	0.0	1.000	8648322	46.7		6946	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.631	1.631	0.0	1.000	2064113	15.1		659	
* 6 13C2-PFOA									
415.00 > 370.00	1.813	1.813	0.0		1463849	10.0		5640	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.813	1.813	0.0	1.000	4233099	31.2		620	
413.00 > 169.00	1.813	1.813	0.0	1.000	2291391		1.85(0.00-0.00)	5544	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.071	2.071	0.0	1.000	6312713	60.8		3342	Ma
499.00 > 99.00	2.071	2.071	0.0	1.000	1295026		4.87(0.00-0.00)	1919	M
* 7 13C4 PFOS									
503.00 > 80.00	2.071	2.071	0.0		3172960	28.7		5867	
9 Perfluorononanoic acid									
463.00 > 419.00	2.079	2.079	0.0	1.000	2979773	30.6		817	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.246	2.246	0.0	1.000	1189772	10.6		7830	

QC Flag Legend

Review Flags

M - Manually Integrated

a - User Assigned ID

Reagents:

LC537-L5_00024

Amount Added: 1.00

Units: mL

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_029.d
 Lims ID: CCV L5
 Client ID:
 Sample Type: CCVIS
 Inject. Date: 31-Jan-2018 12:49:26 ALS Bottle#: 5 Worklist Smp#: 26
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: CCV L5
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub1
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:28:14 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK006

First Level Reviewer: barnettj Date: 31-Jan-2018 16:01:34

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.366	1.366	0.0	1.000	14139035	140.7		12910	
298.90 > 99.00	1.366	1.366	0.0	1.000	11074671		1.28(0.00-0.00)	11878	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.487	1.487	0.0	1.000	1684592	10.5		8999	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.631	1.631	0.0	1.000	8648322	46.7		6946	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.631	1.631	0.0	1.000	2064113	15.1		659	
* 6 13C2-PFOA									
415.00 > 370.00	1.813	1.813	0.0		1463849	10.0		5640	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.813	1.813	0.0	1.000	4233099	31.2		620	
413.00 > 169.00	1.813	1.813	0.0	1.000	2291391		1.85(0.00-0.00)	5544	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.071	2.071	0.0	1.000	6312713	60.8		3342	Ma
499.00 > 99.00	2.071	2.071	0.0	1.000	1295026		4.87(0.00-0.00)	1919	M
* 7 13C4 PFOS									
503.00 > 80.00	2.071	2.071	0.0		3172960	28.7		5867	
9 Perfluorononanoic acid									
463.00 > 419.00	2.079	2.079	0.0	1.000	2979773	30.6		817	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.246	2.246	0.0	1.000	1189772	10.6		7830	

QC Flag Legend

Review Flags

M - Manually Integrated

a - User Assigned ID

Reagents:

LC537-L5_00024

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_029.d

Injection Date: 31-Jan-2018 12:49:26

Instrument ID: A8_N

Lims ID: CCV L5

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 5

Worklist Smp#: 26

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_029.d

Injection Date: 31-Jan-2018 12:49:26

Instrument ID: A8_N

Lims ID: CCV L5

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 5

Worklist Smp#: 26

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_029.d
Injection Date: 31-Jan-2018 12:49:26 Instrument ID: A8_N
Lims ID: CCV L5
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 5 Worklist Smp#: 26
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected
Expected RT: 2.07

Processing Integration Results



Manual Integration Results

RT: 2.07
Area: 1295026
Amount: 60.769930
Amount Units: ng/ml



Reviewer: barnettj, 31-Jan-2018 16:01:22
Audit Action: Manually Integrated

Audit Reason: Assign Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_029.d
Injection Date: 31-Jan-2018 12:49:26 Instrument ID: A8_N
Lims ID: CCV L5
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 5 Worklist Smp#: 26
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.07

Processing Integration Results



RT: 2.07
Area: 6312713
Amount: 60.769930
Amount Units: ng/ml

Manual Integration Results



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_029.d
Injection Date: 31-Jan-2018 12:49:26 Instrument ID: A8_N
Lims ID: CCV L5
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 5 Worklist Smp#: 26
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected
Expected RT: 2.07

Processing Integration Results



Manual Integration Results

RT: 2.07
Area: 1295026
Amount: 60.769930
Amount Units: ng/ml



Reviewer: barnettj, 31-Jan-2018 16:01:22
Audit Action: Manually Integrated

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_029.d
Injection Date: 31-Jan-2018 12:49:26 Instrument ID: A8_N
Lims ID: CCV L5
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 5 Worklist Smp#: 26
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.07

Processing Integration Results



RT: 2.07
Area: 6312713
Amount: 60.769930
Amount Units: ng/ml

Manual Integration Results



Reviewer: barnettj, 31-Jan-2018 16:01:22

Audit Action: Manually Integrated

Audit Reason: Assign Peak

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Lab Sample ID: CCV 320-206410/38 Calibration Date: 01/31/2018 13:45
 Instrument ID: A8_N Calib Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 11/03/2017 14:01
 Lab File ID: 2018.01.31_537A_041.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		1.069		45.8	45.0	1.8	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9369	0.8966		4.79	5.00	-4.3	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.674	1.768		15.8	15.0	5.6	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9258	0.8792		9.51	10.0	-5.0	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9389	0.9125		19.4	20.0	-2.8	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6642	0.6157		9.27	10.0	-7.3	30.0
13C2 PFHxA	Ave	1.100	1.101		10.0	10.0	0.1	30.0
13C2 PFDA	Ave	0.7652	0.7772		10.2	10.0	1.6	30.0

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Lab Sample ID: CCV 320-206412/38 Calibration Date: 01/31/2018 13:45
 Instrument ID: A8_N Calib Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 11/03/2017 14:01
 Lab File ID: 2018.01.31_537A_041.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		1.069		45.8	45.0	1.8	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9369	0.8966		4.79	5.00	-4.3	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.674	1.768		15.8	15.0	5.6	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9258	0.8792		9.51	10.0	-5.0	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9389	0.9125		19.4	20.0	-2.8	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6642	0.6157		9.27	10.0	-7.3	30.0
13C2 PFHxA	Ave	1.100	1.101		10.0	10.0	0.1	30.0
13C2 PFDA	Ave	0.7652	0.7772		10.2	10.0	1.6	30.0

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_041.d
 Lims ID: CCV L3
 Client ID:
 Sample Type: CCVIS
 Inject. Date: 31-Jan-2018 13:45:26 ALS Bottle#: 3 Worklist Smp#: 38
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: CCV L3
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub1
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:28:31 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK006

First Level Reviewer: barnettj Date: 31-Jan-2018 16:02:55

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.366	1.366	0.0	1.000	5327875	45.8		7036	
298.90 > 99.00	1.366	1.366	0.0	1.000	3968349		1.34(0.00-0.00)	7024	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.487	1.487	0.0	1.000	1664809	10.0		8583	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.631	1.631	0.0	1.000	2936892	15.8		4273	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.631	1.631	0.0	1.000	677790	4.79		219	
* 6 13C2-PFOA									
415.00 > 370.00	1.813	1.813	0.0		1511534	10.0		6154	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.821	1.821	0.0	1.000	1330114	9.51		194	
413.00 > 169.00	1.813	1.821	-0.008	0.996	731272		1.82(0.00-0.00)	2415	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.071	2.071	0.0	1.000	2020970	19.4		1495	Ma
499.00 > 99.00	2.071	2.071	0.0	1.000	433172		4.67(0.00-0.00)	908	M
* 7 13C4 PFOS									
503.00 > 80.00	2.071	2.071	0.0		3175124	28.7		6203	
9 Perfluorononanoic acid									
463.00 > 419.00	2.079	2.079	0.0	1.000	930756	9.27		237	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.246	2.246	0.0	1.000	1174794	10.2		7430	

QC Flag Legend

Review Flags

M - Manually Integrated

a - User Assigned ID

Reagents:

LC537-L3_00023

Amount Added: 1.00

Units: mL

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_041.d
 Lims ID: CCV L3
 Client ID:
 Sample Type: CCVIS
 Inject. Date: 31-Jan-2018 13:45:26 ALS Bottle#: 3 Worklist Smp#: 38
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: CCV L3
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub1
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:28:31 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK006

First Level Reviewer: barnettj Date: 31-Jan-2018 16:02:55

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.366	1.366	0.0	1.000	5327875	45.8		7036	
298.90 > 99.00	1.366	1.366	0.0	1.000	3968349		1.34(0.00-0.00)	7024	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.487	1.487	0.0	1.000	1664809	10.0		8583	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.631	1.631	0.0	1.000	2936892	15.8		4273	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.631	1.631	0.0	1.000	677790	4.79		219	
* 6 13C2-PFOA									
415.00 > 370.00	1.813	1.813	0.0		1511534	10.0		6154	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.821	1.821	0.0	1.000	1330114	9.51		194	
413.00 > 169.00	1.813	1.821	-0.008	0.996	731272		1.82(0.00-0.00)	2415	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.071	2.071	0.0	1.000	2020970	19.4		1495	Ma
499.00 > 99.00	2.071	2.071	0.0	1.000	433172		4.67(0.00-0.00)	908	M
* 7 13C4 PFOS									
503.00 > 80.00	2.071	2.071	0.0		3175124	28.7		6203	
9 Perfluorononanoic acid									
463.00 > 419.00	2.079	2.079	0.0	1.000	930756	9.27		237	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.246	2.246	0.0	1.000	1174794	10.2		7430	

QC Flag Legend

Review Flags

M - Manually Integrated

a - User Assigned ID

Reagents:

LC537-L3_00023

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_041.d

Injection Date: 31-Jan-2018 13:45:26

Instrument ID: A8_N

Lims ID: CCV L3

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 3

Worklist Smp#: 38

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_041.d

Injection Date: 31-Jan-2018 13:45:26

Instrument ID: A8_N

Lims ID: CCV L3

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 3

Worklist Smp#: 38

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_041.d
Injection Date: 31-Jan-2018 13:45:26 Instrument ID: A8_N
Lims ID: CCV L3
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 3 Worklist Smp#: 38
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected
Expected RT: 2.07

Processing Integration Results



Manual Integration Results

RT: 2.07
Area: 433172
Amount: 19.441800
Amount Units: ng/ml



Reviewer: barnettj, 31-Jan-2018 16:02:20
Audit Action: Manually Integrated

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_041.d
Injection Date: 31-Jan-2018 13:45:26 Instrument ID: A8_N
Lims ID: CCV L3
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 3 Worklist Smp#: 38
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.07

Processing Integration Results



RT: 2.07
Area: 2020970
Amount: 19.441800
Amount Units: ng/ml

Manual Integration Results



Reviewer: barnettj, 31-Jan-2018 16:02:20

Audit Action: Manually Integrated

Audit Reason: Assign Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_041.d
Injection Date: 31-Jan-2018 13:45:26 Instrument ID: A8_N
Lims ID: CCV L3
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 3 Worklist Smp#: 38
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected
Expected RT: 2.07

Processing Integration Results



Manual Integration Results

RT: 2.07
Area: 433172
Amount: 19.441800
Amount Units: ng/ml



Reviewer: barnettj, 31-Jan-2018 16:02:20
Audit Action: Manually Integrated

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_041.d
Injection Date: 31-Jan-2018 13:45:26 Instrument ID: A8_N
Lims ID: CCV L3
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 3 Worklist Smp#: 38
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.07

Processing Integration Results



RT: 2.07
Area: 2020970
Amount: 19.441800
Amount Units: ng/ml

Manual Integration Results



Reviewer: barnettj, 31-Jan-2018 16:02:20

Audit Action: Manually Integrated

Audit Reason: Assign Peak

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Lab Sample ID: CCV 320-206412/43 Calibration Date: 01/31/2018 14:08
 Instrument ID: A8_N Calib Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 11/03/2017 14:01
 Lab File ID: 2018.01.31_537A_046.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		0.9232		136	135	0.9	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9369	0.9580		15.3	15.0	2.2	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.674	1.716		46.1	45.0	2.5	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9258	0.9180		29.8	30.0	-0.8	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9389	0.9527		60.9	60.0	1.5	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6642	0.6593		29.8	30.0	-0.7	30.0
13C2 PFHxA	Ave	1.100	1.095		9.96	10.0	-0.4	30.0
13C2 PFDA	Ave	0.7652	0.7685		10.0	10.0	0.4	30.0

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_046.d
 Lims ID: CCV L5
 Client ID:
 Sample Type: CCVIS
 Inject. Date: 31-Jan-2018 14:08:46 ALS Bottle#: 5 Worklist Smp#: 43
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: CCV L5
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub1
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:49:01 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK006

First Level Reviewer: barnettj Date: 31-Jan-2018 16:04:03

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.373	1.373	0.0	1.000	14139176	136.2		13428	
298.90 > 99.00	1.373	1.373	0.0	1.000	11215984		1.26(0.00-0.00)	13947	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.495	1.495	0.0	1.000	1646415	9.96		8682	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.639	1.639	0.0	1.000	8759665	46.1		9099	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.639	1.639	0.0	1.000	2160371	15.3		701	
* 6 13C2-PFOA									
415.00 > 370.00	1.821	1.821	0.0		1503053	10.0		6960	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.821	1.821	0.0	1.000	4142773	29.8		645	
413.00 > 169.00	1.821	1.821	0.0	1.000	2284492		1.81(0.00-0.00)	6814	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.071	2.071	0.0	1.000	6486160	60.9		3091	Ma
499.00 > 99.00	2.071	2.071	0.0	1.000	1378323		4.71(0.00-0.00)	2413	M
* 7 13C4 PFOS									
503.00 > 80.00	2.071	2.071	0.0		3253442	28.7		6642	
9 Perfluorononanoic acid									
463.00 > 419.00	2.079	2.079	0.0	1.000	2973302	29.8		791	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.253	2.253	0.0	1.000	1155111	10.0		6649	

QC Flag Legend

Review Flags

M - Manually Integrated

a - User Assigned ID

Reagents:

LC537-L5_00024

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_046.d

Injection Date: 31-Jan-2018 14:08:46

Instrument ID: A8_N

Lims ID: CCV L5

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 5

Worklist Smp#: 43

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_046.d
Injection Date: 31-Jan-2018 14:08:46 Instrument ID: A8_N
Lims ID: CCV L5
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 5 Worklist Smp#: 43
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected
Expected RT: 2.07

Processing Integration Results



RT: 2.07
Area: 1378323
Amount: 60.895033
Amount Units: ng/ml

Manual Integration Results



Reviewer: barnettj, 31-Jan-2018 16:03:40
Audit Action: Manually Integrated

Audit Reason: Assign Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_046.d
Injection Date: 31-Jan-2018 14:08:46 Instrument ID: A8_N
Lims ID: CCV L5
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 5 Worklist Smp#: 43
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.07

Processing Integration Results



RT: 2.07
Area: 6486160
Amount: 60.895033
Amount Units: ng/ml

Manual Integration Results



FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: _____ Lab Sample ID: MB 320-205489/1-A
 Matrix: Water Lab File ID: 2018.01.31_537A_019.d
 Analysis Method: 537 Date Collected: _____
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 250 (mL) Date Analyzed: 01/31/2018 12:02
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	8.0	U	20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.0	U	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	95		70-130
STL00996	13C2 PFDA	101		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_019.d
 Lims ID: MB 320-205489/1-A
 Client ID:
 Sample Type: MB
 Inject. Date: 31-Jan-2018 12:02:42 ALS Bottle#: 17 Worklist Smp#: 16
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: mb 320-205489/1-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:27:52 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK006

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
\$ 2 13C2 PFHxA	315.00 > 270.00	1.495	1.495	0.0	1.000	1583576	9.50	8193	
* 6 13C2-PFOA	415.00 > 370.00	1.828	1.821	0.007		1514419	10.0	6091	
* 7 13C4 PFOS	503.00 > 80.00	2.079	2.071	0.008		3315723	28.7	7540	
\$ 10 13C2 PFDA	515.00 > 470.00	2.253	2.253	0.0	1.000	1168748	10.1	8708	

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_019.d

Injection Date: 31-Jan-2018 12:02:42

Instrument ID: A8_N

Lims ID: MB 320-205489/1-A

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 17

Worklist Smp#: 16

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid (ND)

1 Perfluorobutanesulfonic acid (ND)




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid (ND)

4 Perfluoroheptanoic acid (ND)




* 6 13C2-PFOA



5 Perfluorooctanoic acid (ND)

5 Perfluorooctanoic acid (ND)




8 Perfluorooctane sulfonic acid (ND)




8 Perfluorooctane sulfonic acid (ND)

* 7 13C4 PFOS

9 Perfluorononanoic acid (ND)



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_019.d
 Lims ID: MB 320-205489/1-A
 Client ID:
 Sample Type: MB
 Inject. Date: 31-Jan-2018 12:02:42 ALS Bottle#: 17 Worklist Smp#: 16
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: mb 320-205489/1-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:27:52 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK006

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	9.50	95.04
\$ 10 13C2 PFDA	10.0	10.1	100.86

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: _____ Lab Sample ID: LLCS 320-205489/2-A
 Matrix: Water Lab File ID: 2018.01.31_537A_020.d
 Analysis Method: 537 Date Collected: _____
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 250 (mL) Date Analyzed: 01/31/2018 12:07
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	38.5	J M	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	20.1		20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	19.9	J	24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	29.0	J	30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	11.1		10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	91.7		90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	103		70-130
STL00996	13C2 PFDA	104		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_020.d
 Lims ID: LLCS 320-205489/2-A
 Client ID:
 Sample Type: LLCS
 Inject. Date: 31-Jan-2018 12:07:21 ALS Bottle#: 18 Worklist Smp#: 17
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: llcs 320-205489/2-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:27:52 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK006

First Level Reviewer: barnettj Date: 31-Jan-2018 16:12:01

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.373	1.373	0.0	1.000	2889207	22.9		4664	
298.90 > 99.00	1.373	1.373	0.0	1.000	2089780		1.38(0.00-0.00)	2950	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.495	1.495	0.0	1.000	1635156	10.3		7919	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.639	1.631	0.008	1.000	1410385	7.25		1528	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.639	1.631	0.008	1.000	374876	2.78		119	
* 6 13C2-PFOA									
415.00 > 370.00	1.828	1.821	0.007		1437381	10.0		6390	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.828	1.821	0.007	1.000	668462	5.02		109	
413.00 > 169.00	1.828	1.821	0.007	1.000	374271		1.79(0.00-0.00)	1040	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.079	2.071	0.008	1.000	1049554	9.63		828	Ma
499.00 > 99.00	2.079	2.071	0.008	1.000	212470		4.94(0.00-0.00)	383	M
* 7 13C4 PFOS									
503.00 > 80.00	2.079	2.071	0.008		3330580	28.7		7472	
9 Perfluorononanoic acid									
463.00 > 419.00	2.086	2.079	0.007	1.000	474294	4.97		129	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.253	2.253	0.0	1.000	1144069	10.4		7470	

QC Flag Legend

Review Flags

M - Manually Integrated

a - User Assigned ID

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_020.d

Injection Date: 31-Jan-2018 12:07:21 Instrument ID: A8_N

Lims ID: LLCS 320-205489/2-A

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 18

Worklist Smp#: 17

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_020.d
 Lims ID: LLCS 320-205489/2-A
 Client ID:
 Sample Type: LLCS
 Inject. Date: 31-Jan-2018 12:07:21 ALS Bottle#: 18 Worklist Smp#: 17
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: llcs 320-205489/2-a
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:27:52 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK006

First Level Reviewer: barnettj Date: 31-Jan-2018 16:12:01

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	10.3	103.39
\$ 10 13C2 PFDA	10.0	10.4	104.02

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_020.d
Injection Date: 31-Jan-2018 12:07:21 Instrument ID: A8_N
Lims ID: LLCS 320-205489/2-A
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 18 Worklist Smp#: 17
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected
Expected RT: 2.07

Processing Integration Results



Manual Integration Results

RT: 2.08
Area: 212470
Amount: 9.625476
Amount Units: ng/ml



Reviewer: barnettj, 31-Jan-2018 16:11:42
Audit Action: Manually Integrated

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_020.d
Injection Date: 31-Jan-2018 12:07:21 Instrument ID: A8_N
Lims ID: LLCS 320-205489/2-A
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 18 Worklist Smp#: 17
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.07

Processing Integration Results



Manual Integration Results

RT: 2.08
Area: 1049554
Amount: 9.625476
Amount Units: ng/ml



FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: NAWC-011118-RW-179 LMS Lab Sample ID: 320-35046-12 LMS
 Matrix: Water Lab File ID: 2018.01.31_537A_035.d
 Analysis Method: 537 Date Collected: 01/11/2018 12:40
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 255.4 (mL) Date Analyzed: 01/31/2018 13:17
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206410 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	54.3	M	39	16	6.7
335-67-1	Perfluorooctanoic acid (PFOA)	37.3		20	7.8	2.7
375-95-1	Perfluorononanoic acid (PFNA)	21.2	J	23	20	7.8
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	34.9		29	12	5.4
375-85-9	Perfluoroheptanoic acid (PFHpA)	14.9		9.8	3.9	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	90.6		88	35	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	94		70-130
STL00996	13C2 PFDA	108		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_035.d
 Lims ID: 320-35046-A-12-D LMS
 Client ID:
 Sample Type: LMS
 Inject. Date: 31-Jan-2018 13:17:24 ALS Bottle#: 31 Worklist Smp#: 32
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35046-a-12-d lms
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:28:14 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK006

First Level Reviewer: barnettj Date: 31-Jan-2018 16:22:24

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.366	1.366	0.0	1.000	3027188	23.1		3334	
298.90 > 99.00	1.366	1.366	0.0	1.000	2165508		1.40(0.00-0.00)	2843	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.487	1.487	0.0	1.000	1577074	9.38		7820	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.631	1.631	0.0	1.000	1800325	8.91		934	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.631	1.631	0.0	1.000	544321	3.80		115	
* 6 13C2-PFOA									
415.00 > 370.00	1.813	1.813	0.0		1527332	10.0		6260	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.813	1.813	0.0	1.000	1346246	9.52		174	
413.00 > 169.00	1.813	1.813	0.0	1.000	790948		1.70(0.00-0.00)	1704	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.064	2.071	-0.007	1.000	1572176	13.9		697	Ma
499.00 > 99.00	2.064	2.071	-0.007	1.000	310260		5.07(0.00-0.00)	403	M
* 7 13C4 PFOS									
503.00 > 80.00	2.064	2.071	-0.007		3460115	28.7		3903	
9 Perfluorononanoic acid									
463.00 > 419.00	2.079	2.079	0.0	1.000	550366	5.43		86.6	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.246	2.246	0.0	1.000	1258236	10.8		7499	

QC Flag Legend

Review Flags

M - Manually Integrated

a - User Assigned ID

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_035.d

Injection Date: 31-Jan-2018 13:17:24

Instrument ID: A8_N

Lims ID: 320-35046-A-12-D LMS

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 31

Worklist Smp#: 32

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_035.d
 Lims ID: 320-35046-A-12-D LMS
 Client ID:
 Sample Type: LMS
 Inject. Date: 31-Jan-2018 13:17:24 ALS Bottle#: 31 Worklist Smp#: 32
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35046-a-12-d lms
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:28:14 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK006

First Level Reviewer: barnettj Date: 31-Jan-2018 16:22:24

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	9.38	93.85
\$ 10 13C2 PFDA	10.0	10.8	107.66

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_035.d
Injection Date: 31-Jan-2018 13:17:24 Instrument ID: A8_N
Lims ID: 320-35046-A-12-D LMS
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 31 Worklist Smp#: 32
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected
Expected RT: 2.07

Processing Integration Results



RT: 2.06
Area: 310260
Amount: 13.878672
Amount Units: ng/ml

Manual Integration Results



Reviewer: barnettj, 31-Jan-2018 16:22:02
Audit Action: Manually Integrated

Audit Reason: Assign Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_035.d
Injection Date: 31-Jan-2018 13:17:24 Instrument ID: A8_N
Lims ID: 320-35046-A-12-D LMS
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 31 Worklist Smp#: 32
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.07

Processing Integration Results



RT: 2.06
Area: 1572176
Amount: 13.878672
Amount Units: ng/ml

Manual Integration Results



FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: NAWC-011118-RW-179 LMSD Lab Sample ID: 320-35046-12 LMSD
 Matrix: Water Lab File ID: 2018.01.31_537A_036.d
 Analysis Method: 537 Date Collected: 01/11/2018 12:40
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 263.9(mL) Date Analyzed: 01/31/2018 13:22
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206410 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	51.8	M	38	15	6.4
335-67-1	Perfluorooctanoic acid (PFOA)	35.1		19	7.6	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19.6	J	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	33.0		28	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	13.0		9.5	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	84.3	J	85	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	88		70-130
STL00996	13C2 PFDA	97		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_036.d
 Lims ID: 320-35046-A-12-E LMSD
 Client ID:
 Sample Type: LMSD
 Inject. Date: 31-Jan-2018 13:22:04 ALS Bottle#: 32 Worklist Smp#: 33
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35046-a-12-e lmsd
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:28:14 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK006

First Level Reviewer: barnettj Date: 31-Jan-2018 16:23:24

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.373	1.366	0.007	1.000	2882147	22.3		3092	
298.90 > 99.00	1.373	1.366	0.007	1.000	2149923		1.34(0.00-0.00)	2754	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.487	1.487	0.0	1.000	1511707	8.77		7055	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.631	1.631	0.0	1.000	1737709	8.70		887	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.631	1.631	0.0	1.000	505125	3.44		97.7	
* 6 13C2-PFOA									
415.00 > 370.00	1.813	1.813	0.0		1566820	10.0		6132	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.821	1.813	0.008	1.000	1344211	9.27		169	
413.00 > 169.00	1.821	1.813	0.008	1.000	780390		1.72(0.00-0.00)	1931	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.071	2.071	0.0	1.000	1530817	13.7		696	Ma
499.00 > 99.00	2.071	2.071	0.0	1.000	300614		5.09(0.00-0.00)	367	M
* 7 13C4 PFOS									
503.00 > 80.00	2.071	2.071	0.0		3420572	28.7		4015	
9 Perfluorononanoic acid									
463.00 > 419.00	2.079	2.079	0.0	1.000	539298	5.18		80.2	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.253	2.246	0.007	1.000	1159916	9.67		7836	

QC Flag Legend

Review Flags

M - Manually Integrated

a - User Assigned ID

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_036.d

Injection Date: 31-Jan-2018 13:22:04

Instrument ID: A8_N

Lims ID: 320-35046-A-12-E LMSD

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 32

Worklist Smp#: 33

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_036.d
 Lims ID: 320-35046-A-12-E LMSD
 Client ID:
 Sample Type: LMSD
 Inject. Date: 31-Jan-2018 13:22:04 ALS Bottle#: 32 Worklist Smp#: 33
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35046-a-12-e lmsd
 Misc. Info.: Plate: 1 Rack: 2
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 31-Jan-2018 16:28:14 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK006

First Level Reviewer: barnettj Date: 31-Jan-2018 16:23:24

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	8.77	87.69
\$ 10 13C2 PFDA	10.0	9.67	96.75

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_036.d
Injection Date: 31-Jan-2018 13:22:04 Instrument ID: A8_N
Lims ID: 320-35046-A-12-E LMSD
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 32 Worklist Smp#: 33
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected
Expected RT: 2.07

Processing Integration Results



Manual Integration Results

RT: 2.07
Area: 300614
Amount: 13.669789
Amount Units: ng/ml



Reviewer: barnettj, 31-Jan-2018 16:23:08
Audit Action: Manually Integrated

Audit Reason: Assign Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b\2018.01.31_537A_036.d
Injection Date: 31-Jan-2018 13:22:04 Instrument ID: A8_N
Lims ID: 320-35046-A-12-E LMSD
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 32 Worklist Smp#: 33
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.07

Processing Integration Results



Manual Integration Results

RT: 2.07
Area: 1530817
Amount: 13.669789
Amount Units: ng/ml



LCMS ANALYSIS RUN LOG

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1

SDG No.: _____

Instrument ID: A8_N Start Date: 11/03/2017 13:37

Analysis Batch Number: 192908 End Date: 11/03/2017 14:24

LAB SAMPLE ID	CLIENT SAMPLE ID	DATE ANALYZED	DILUTION FACTOR	LAB FILE ID	COLUMN ID
IC 320-192908/4		11/03/2017 13:37	1	2017.11.03_537X ICAL 004.d	GeminiC18 3x100 3(mm)
IC 320-192908/5		11/03/2017 13:42	1	2017.11.03_537X ICAL 005.d	GeminiC18 3x100 3(mm)
IC 320-192908/6		11/03/2017 13:47	1	2017.11.03_537X ICAL 006.d	GeminiC18 3x100 3(mm)
IC 320-192908/7 ICISAV		11/03/2017 13:52	1	2017.11.03_537X ICAL 007.d	GeminiC18 3x100 3(mm)
IC 320-192908/8		11/03/2017 13:56	1	2017.11.03_537X ICAL 008.d	GeminiC18 3x100 3(mm)
IC 320-192908/9		11/03/2017 14:01	1	2017.11.03_537X ICAL 009.d	GeminiC18 3x100 3(mm)
ZZZZZ		11/03/2017 14:06	1		GeminiC18 3x100 3(mm)
CCVL 320-192908/11		11/03/2017 14:10	1	2017.11.03_537X ICAL 011.d	GeminiC18 3x100 3(mm)
ZZZZZ		11/03/2017 14:15	1		GeminiC18 3x100 3(mm)
ICV 320-192908/13		11/03/2017 14:20	1	2017.11.03_537X ICAL 013.d	GeminiC18 3x100 3(mm)
ZZZZZ		11/03/2017 14:24	1		GeminiC18 3x100 3(mm)

LCMS ANALYSIS RUN LOG

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1

SDG No.: _____

Instrument ID: A8_N Start Date: 01/31/2018 10:52

Analysis Batch Number: 206407 End Date: 01/31/2018 11:53

LAB SAMPLE ID	CLIENT SAMPLE ID	DATE ANALYZED	DILUTION FACTOR	LAB FILE ID	COLUMN ID
CCVL 320-206407/1		01/31/2018 10:52	1	2018.01.31_537A 004.d	GeminiC18 3x100 3(mm)
CCV 320-206407/2 CCVIS		01/31/2018 10:57	1		GeminiC18 3x100 3(mm)
ZZZZZ		01/31/2018 11:06	1		GeminiC18 3x100 3(mm)
ZZZZZ		01/31/2018 11:11	1		GeminiC18 3x100 3(mm)
ZZZZZ		01/31/2018 11:15	1		GeminiC18 3x100 3(mm)
ZZZZZ		01/31/2018 11:20	1		GeminiC18 3x100 3(mm)
ZZZZZ		01/31/2018 11:25	1		GeminiC18 3x100 3(mm)
ZZZZZ		01/31/2018 11:29	1		GeminiC18 3x100 3(mm)
ZZZZZ		01/31/2018 11:34	1		GeminiC18 3x100 3(mm)
ZZZZZ		01/31/2018 11:39	1		GeminiC18 3x100 3(mm)
ZZZZZ		01/31/2018 11:43	1		GeminiC18 3x100 3(mm)
ZZZZZ		01/31/2018 11:48	1		GeminiC18 3x100 3(mm)
CCV 320-206407/14 CCVIS		01/31/2018 11:53	1		GeminiC18 3x100 3(mm)

LCMS ANALYSIS RUN LOG

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1

SDG No.: _____

Instrument ID: A8_N Start Date: 01/31/2018 11:53

Analysis Batch Number: 206408 End Date: 01/31/2018 12:49

LAB SAMPLE ID	CLIENT SAMPLE ID	DATE ANALYZED	DILUTION FACTOR	LAB FILE ID	COLUMN ID
CCV 320-206408/14 CCVIS		01/31/2018 11:53	1	2018.01.31_537A 017.d	GeminiC18 3x100 3(mm)
MB 320-205489/1-A		01/31/2018 12:02	1	2018.01.31_537A 019.d	GeminiC18 3x100 3(mm)
LLCS 320-205489/2-A		01/31/2018 12:07	1	2018.01.31_537A 020.d	GeminiC18 3x100 3(mm)
320-35046-1		01/31/2018 12:12	1	2018.01.31_537A 021.d	GeminiC18 3x100 3(mm)
320-35046-2		01/31/2018 12:16	1	2018.01.31_537A 022.d	GeminiC18 3x100 3(mm)
320-35046-3		01/31/2018 12:21	1	2018.01.31_537A 023.d	GeminiC18 3x100 3(mm)
320-35046-4		01/31/2018 12:26	1	2018.01.31_537A 024.d	GeminiC18 3x100 3(mm)
320-35046-5		01/31/2018 12:30	1	2018.01.31_537A 025.d	GeminiC18 3x100 3(mm)
320-35046-6		01/31/2018 12:35	1	2018.01.31_537A 026.d	GeminiC18 3x100 3(mm)
320-35046-7		01/31/2018 12:40	1	2018.01.31_537A 027.d	GeminiC18 3x100 3(mm)
320-35046-8		01/31/2018 12:44	1	2018.01.31_537A 028.d	GeminiC18 3x100 3(mm)
CCV 320-206408/26 CCVIS		01/31/2018 12:49	1	2018.01.31_537A 029.d	GeminiC18 3x100 3(mm)

LCMS ANALYSIS RUN LOG

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1

SDG No.: _____

Instrument ID: A8_N Start Date: 01/31/2018 12:49

Analysis Batch Number: 206410 End Date: 01/31/2018 13:45

LAB SAMPLE ID	CLIENT SAMPLE ID	DATE ANALYZED	DILUTION FACTOR	LAB FILE ID	COLUMN ID
CCV 320-206410/26 CCVIS		01/31/2018 12:49	1	2018.01.31_537A 029.d	GeminiC18 3x100 3(mm)
320-35046-9		01/31/2018 12:58	1	2018.01.31_537A 031.d	GeminiC18 3x100 3(mm)
320-35046-10		01/31/2018 13:03	1	2018.01.31_537A 032.d	GeminiC18 3x100 3(mm)
320-35046-11		01/31/2018 13:08	1	2018.01.31_537A 033.d	GeminiC18 3x100 3(mm)
320-35046-12		01/31/2018 13:12	1	2018.01.31_537A 034.d	GeminiC18 3x100 3(mm)
320-35046-12 LMS		01/31/2018 13:17	1	2018.01.31_537A 035.d	GeminiC18 3x100 3(mm)
320-35046-12 LMSD		01/31/2018 13:22	1	2018.01.31_537A 036.d	GeminiC18 3x100 3(mm)
320-35046-13		01/31/2018 13:26	1	2018.01.31_537A 037.d	GeminiC18 3x100 3(mm)
320-35046-14		01/31/2018 13:31	1	2018.01.31_537A 038.d	GeminiC18 3x100 3(mm)
320-35046-15		01/31/2018 13:36	1	2018.01.31_537A 039.d	GeminiC18 3x100 3(mm)
320-35046-16		01/31/2018 13:40	1	2018.01.31_537A 040.d	GeminiC18 3x100 3(mm)
CCV 320-206410/38 CCVIS		01/31/2018 13:45	1	2018.01.31_537A 041.d	GeminiC18 3x100 3(mm)

LCMS ANALYSIS RUN LOG

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1

SDG No.: _____

Instrument ID: A8_N Start Date: 01/31/2018 13:45

Analysis Batch Number: 206412 End Date: 01/31/2018 14:08

LAB SAMPLE ID	CLIENT SAMPLE ID	DATE ANALYZED	DILUTION FACTOR	LAB FILE ID	COLUMN ID
CCV 320-206412/38 CCVIS		01/31/2018 13:45	1	2018.01.31_537A 041.d	GeminiC18 3x100 3(mm)
320-35046-17		01/31/2018 13:54	1	2018.01.31_537A 043.d	GeminiC18 3x100 3(mm)
320-35046-18		01/31/2018 13:59	1	2018.01.31_537A 044.d	GeminiC18 3x100 3(mm)
320-35046-19		01/31/2018 14:04	1	2018.01.31_537A 045.d	GeminiC18 3x100 3(mm)
CCV 320-206412/43 CCVIS		01/31/2018 14:08	1	2018.01.31_537A 046.d	GeminiC18 3x100 3(mm)

LCMS BATCH WORKSHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1

SDG No.: _____

Batch Number: 205489 Batch Start Date: 01/25/18 14:25 Batch Analyst: Long, Tyrel W

Batch Method: 537 Batch End Date: 01/25/18 22:10

Lab Sample ID	Client Sample ID	Method Chain	Basis	GrossWeight	TareWeight	InitialAmount	FinalAmount	ReceivedpH	LC537-IS 00055
MB 320-205489/1		537, 537				250 mL	1.00 mL	7 SU	100 uL
LLCS 320-205489/2		537, 537				250 mL	1.00 mL	7 SU	100 uL
320-35046-A-1	WGNA-011118-RW-3 103	537, 537	T	314.59 g	28.73 g	285.9 mL	1.00 mL	7 SU	100 uL
320-35046-A-2	WGNA-011118-FRB- 3103	537, 537	T	292.93 g	26.95 g	266 mL	1.00 mL	7 SU	100 uL
320-35046-A-3	WGNA-011118-RW-0 683	537, 537	T	289.57 g	28.60 g	261 mL	1.00 mL	7 SU	100 uL
320-35046-A-4	WGNA-011118-FRB- 0683	537, 537	T	289.77 g	26.99 g	262.8 mL	1.00 mL	7 SU	100 uL
320-35046-A-5	NAWC-011118-RW-1 39	537, 537	T	297.46 g	28.67 g	268.8 mL	1.00 mL	7 SU	100 uL
320-35046-A-6	NAWC-011118-FRB- 139	537, 537	T	300.19 g	27.02 g	273.2 mL	1.00 mL	7 SU	100 uL
320-35046-A-7	WGNA-011118-DUP- 18	537, 537	T	298.89 g	28.75 g	270.1 mL	1.00 mL	7 SU	100 uL
320-35046-A-8	NAWC-011118-RW-0 98	537, 537	T	269.36 g	28.60 g	240.8 mL	1.00 mL	7 SU	100 uL
320-35046-A-9	NAWC-011118-FRB- 098	537, 537	T	296.99 g	27.08 g	269.9 mL	1.00 mL	7 SU	100 uL
320-35046-A-10	NAWC-011118-RW-1 80	537, 537	T	293.90 g	28.52 g	265.4 mL	1.00 mL	7 SU	100 uL
320-35046-A-11	NAWC-011118-FRB- 180	537, 537	T	291.23 g	27.05 g	264.2 mL	1.00 mL	7 SU	100 uL
320-35046-A-12	NAWC-011118-RW-1 79	537, 537	T	290.54 g	28.61 g	261.9 mL	1.00 mL	7 SU	100 uL
320-35046-A-12	NAWC-011118-RW-1 LMS 79	537, 537	T	283.43 g	27.99 g	255.4 mL	1.00 mL	7 SU	100 uL
320-35046-A-12	NAWC-011118-RW-1 LMSD 79	537, 537	T	292.51 g	28.63 g	263.9 mL	1.00 mL	7 SU	100 uL
320-35046-A-13	NAWC-011118-FRB- 179	537, 537	T	288.76 g	27.27 g	261.5 mL	1.00 mL	7 SU	100 uL
320-35046-A-14	NAWC-011118-RW-3 03	537, 537	T	289.16 g	28.40 g	260.8 mL	1.00 mL	7 SU	100 uL
320-35046-A-15	NAWC-011118-FRB- 303	537, 537	T	289.19 g	27.24 g	262 mL	1.00 mL	7 SU	100 uL
320-35046-A-16	WGNA-011118-RW-3 409	537, 537	T	315.88 g	27.90 g	288 mL	1.00 mL	7 SU	100 uL
320-35046-A-17	WGNA-011118-FRB- 3409	537, 537	T	288.88 g	27.37 g	261.5 mL	1.00 mL	7 SU	100 uL
320-35046-A-18	WGNA-011118-RW-3 220	537, 537	T	296.30 g	28.63 g	267.7 mL	1.00 mL	7 SU	100 uL

The pound sign (#) in the amount added field denotes that the reagent was used undiluted. All calculations are performed using the stated concentration for this reagent.

LCMS BATCH WORKSHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1

SDG No.: _____

Batch Number: 205489 Batch Start Date: 01/25/18 14:25 Batch Analyst: Long, Tyrel W

Batch Method: 537 Batch End Date: 01/25/18 22:10

Lab Sample ID	Client Sample ID	Method Chain	Basis	GrossWeight	TareWeight	InitialAmount	FinalAmount	ReceivedpH	LC537-IS 00055
320-35046-A-19	WGNA-011118-FRB-3220	537, 537	T	298.97 g	27.24 g	271.7 mL	1.00 mL	7 SU	100 uL

Lab Sample ID	Client Sample ID	Method Chain	Basis	LC537-LSP 00028	LC537-SU 00053	AnalysisComment			
MB 320-205489/1		537, 537			100 uL	Chlorine ND			
LLCS 320-205489/2		537, 537		100 uL	100 uL	Chlorine ND			
320-35046-A-1	WGNA-011118-RW-3103	537, 537	T		100 uL	Chlorine ND			
320-35046-A-2	WGNA-011118-FRB-3103	537, 537	T		100 uL	Chlorine ND			
320-35046-A-3	WGNA-011118-RW-0683	537, 537	T		100 uL	Chlorine ND			
320-35046-A-4	WGNA-011118-FRB-0683	537, 537	T		100 uL	Chlorine ND			
320-35046-A-5	NAWC-011118-RW-139	537, 537	T		100 uL	Chlorine ND			
320-35046-A-6	NAWC-011118-FRB-139	537, 537	T		100 uL	Chlorine ND			
320-35046-A-7	WGNA-011118-DUP-18	537, 537	T		100 uL	Chlorine ND			
320-35046-A-8	NAWC-011118-RW-098	537, 537	T		100 uL	Chlorine ND			
320-35046-A-9	NAWC-011118-FRB-098	537, 537	T		100 uL	Chlorine ND			
320-35046-A-10	NAWC-011118-RW-180	537, 537	T		100 uL	Chlorine ND			
320-35046-A-11	NAWC-011118-FRB-180	537, 537	T		100 uL	Chlorine ND			
320-35046-A-12	NAWC-011118-RW-179	537, 537	T		100 uL	Chlorine ND			
320-35046-A-12 LMS	NAWC-011118-RW-179	537, 537	T	100 uL	100 uL	Chlorine ND			
320-35046-A-12 LMSD	NAWC-011118-RW-179	537, 537	T	100 uL	100 uL	Chlorine ND			
320-35046-A-13	NAWC-011118-FRB-179	537, 537	T		100 uL	Chlorine ND			
320-35046-A-14	NAWC-011118-RW-303	537, 537	T		100 uL	Chlorine ND			
320-35046-A-15	NAWC-011118-FRB-303	537, 537	T		100 uL	Chlorine ND			

The pound sign (#) in the amount added field denotes that the reagent was used undiluted. All calculations are performed using the stated concentration for this reagent.

LCMS BATCH WORKSHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1

SDG No.: _____

Batch Number: 205489 Batch Start Date: 01/25/18 14:25 Batch Analyst: Long, Tyrel W

Batch Method: 537 Batch End Date: 01/25/18 22:10

Lab Sample ID	Client Sample ID	Method Chain	Basis	LC537-LSP 00028	LC537-SU 00053	AnalysisComment			
320-35046-A-16	WGNA-011118-RW-3409	537, 537	T		100 uL	Chlorine ND			
320-35046-A-17	WGNA-011118-FRB-3409	537, 537	T		100 uL	Chlorine ND			
320-35046-A-18	WGNA-011118-RW-3220	537, 537	T		100 uL	Chlorine ND			
320-35046-A-19	WGNA-011118-FRB-3220	537, 537	T		100 uL	Chlorine ND			

Batch Notes	
Analyst ID - Aliquot Step	TWL
Batch Comment	Label ID's checked: TWL 1/25/18
Analyst ID - Concentration	TWL
Analyst ID - Final Volume Step	TWL
Internal Standard ID#	1099355
Manifold ID	1
Methanol ID	1127847
pH Indicator ID	2517
Pipette ID	M16387D
Analyst ID - IS Reagent Drop	JER
Analyst ID - IS Reagent Drop Witness	TWL
Analyst ID - SU Reagent Drop	JER
Analyst ID - SU Reagent Drop Witness	TWL
Analyst ID - TA Reagent Drop	JER
Analyst ID - TA Reagent Drop Witness	TWL
SPE Cartridge ID	6369499-03
Trizma ID	SLBR4303V
Reagent Water ID	1-19-18

Basis	Basis Description
T	Total/NA

The pound sign (#) in the amount added field denotes that the reagent was used undiluted. All calculations are performed using the stated concentration for this reagent.

Job No: 35046 Instrument ID & Date: A8 1-31-18 ICAL Batch: 192908
 Extraction Batch: 205489 Worklist #: 53554 TALS Batch: 206408, 206410, 206412

Review Items	-- Level 1 --			Level 2
	Yes	No	N/A	
Initial Calibration				
1. Is ICAL verified and locked in Chrom & TALS?	✓			✓
2. Is ICV properly linked in TALS?	✓			✓
Continuing Calibration				
1. Low-range CCV injected at start of analytical run? CCV injected after every 10 samples and at the end of the analytical run and alternated between Low-range, Mid-range and High-range?	✓			✓
2. If sequence was not after an ICAL was a low and mid range CCV injected at the start of the analytical run?	✓			✓
3. Native compounds and surrogates in control? Low-range within ±50% of true value Mid and High-range within ±30% of true value	✓			✓
4. Internal Standard areas in control? Areas ≥ 50% of average area of the ICAL and 70-140% of the most recent CCV.	✓			✓
Client Samples & QC Sample Results				
1. Were preparation and analysis done within holding times?	✓			✓
2. Are Chromatograms reviewed and spectra verified?	✓			✓
3. Are positive results within calibration range?	✓			✓
4. Dilutions due to target cpds? <input checked="" type="radio"/> Dilutions due to non-targets? <input type="radio"/>			✓	
5. All target compounds in MB < 1/3 RL ? (Requires NCM if "no.")	✓			✓
6. Are target constituents in LCS/LCSD within method control limits?	✓			✓
7. Internal Standard areas in control for all samples and QC reported? ±50% from the average area of the ICAL and 70-140% of the most recent CCV	✓			✓
8. Do results (e.g., dilutions/trip blanks) make sense?	✓			✓
9. Are MS/MSD recoveries and RPDs within method control limits?	✓			✓
10. Are all QC samples properly linked in TALS?	✓			✓
11. All manual integrations appropriate and completely documented?	✓			✓
12. Are nonconformances documented as NCMs?			✓	✓
13. Are all Chrom graphics uploaded?	✓			✓

1st Level Reviewer / Date: JRB 2-1-18 2nd Level Reviewer / Date: MK Walf 2/2/18

NCM # and Comments: _____

A8

Instrument ID & Date: 11-3-17 Worklist#: 49975

ICAL Batch: 192908, 192909 Calibration ID number: 36012, 36013

Review Items	-- Level 1 --			Level 2
	Yes	No	N/A	
Initial Calibration				
1. Mass calibration, as needed, verified by full scan of PFC stock standard. All PFC ions used for quantitation are within 0.3 m/z of true mass?	✓			✓
2. Responses increase with increasing concentration?	✓			✓
3. Fit used (circle): <u>Average</u> Linear (1/x ²)Linear <u>Quadratic</u> (6 points minimum)				
4. Meets fit criteria? Intercept ≤ 1/2 RL RSD ≤ 30% for Average R ² ≥ 0.990 for Linear R ² ≥ 0.990 for Quadratic NOTE: "Force through Zero" must be used and weighted if needed	✓			✓
5. If quadratic fit used the curve does not "bend over".	✓			✓
6. Feed calibration points into the calculated curve. Are points ≤MRL within ±50% of true value? Are points >MRL within ±30% of true value?	✓			✓
7. Any carryover from the high calibration point must be < 1/3 RL	✓			✓
8. Asymmetry check meets criteria for the first two eluting peaks? (0.8 - 1.5).	✓			✓
9. Is the asymmetry check scanned and linked in TALS to the calibration point?	✓			✓
10. Is ICV (2 nd source) ± 30% of true value?	✓			✓
11. Is ICV (2 nd source) internal standards ±50% of average area of the ICAL?	✓			✓
12. ICAL locked in Chrom and uploaded to TALS?	✓			✓
13. ICAL locked in TALS and scanned?				✓

1st Level Reviewer / Date: JRB 11-6-17

2nd Level Reviewer / Date: MW 11/6/2017

NCM # and Comments: _____

TestAmerica Laboratories
Worklist QC Batch Report

Worklist Name: 31JAN2018_537A

Worklist Number: 53554

Instrument Name: A8_N

Chrom Method: 537_A8_N

Data Directory: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b

QC Batching: Enabled

Limit Group Batching: Enabled

QC Batch: 1	LC 537 CS ICAL Raw Batch: 206406	LC 537 ICAL Raw Batch: 206407
# 1 CCVL	# 1 CCVL	# 1 CCVL
# 2 CCV L5		# 2 CCV L5
# 3 RB		# 3 RB
# 4 MB 320-205771/1-A		# 4 MB 320-205771/1-A
# 5 LCS 320-205771/2-A		# 5 LCS 320-205771/2-A
# 6 320-35362-A-1-A		# 6 320-35362-A-1-A
# 7 320-35362-A-2-A		# 7 320-35362-A-2-A
# 8 320-35362-A-2-B MS		# 8 320-35362-A-2-B MS
# 9 320-35362-A-2-C MSD		# 9 320-35362-A-2-C MSD
#10 320-35362-A-3-A		#10 320-35362-A-3-A
#11 320-35362-A-4-A		#11 320-35362-A-4-A
#12 320-35362-A-5-A		#12 320-35362-A-5-A
#13 320-35362-A-6-A		#13 320-35362-A-6-A
#14 CCV L3		#14 CCV L3

QC Batch: 2	LC 537 ICAL Raw Batch: 206408
#14 CCV L3	#14 CCV L3
#15 RB	#15 RB
#16 MB 320-205489/1-A	#16 MB 320-205489/1-A
#17 LLCS 320-205489/2-A	#17 LLCS 320-205489/2-A
#18 320-35046-A-1-A	#18 320-35046-A-1-A
#19 320-35046-A-2-A	#19 320-35046-A-2-A
#20 320-35046-A-3-A	#20 320-35046-A-3-A
#21 320-35046-A-4-A	#21 320-35046-A-4-A
#22 320-35046-A-5-A	#22 320-35046-A-5-A
#23 320-35046-A-6-A	#23 320-35046-A-6-A
#24 320-35046-A-7-A	#24 320-35046-A-7-A
#25 320-35046-A-8-A	#25 320-35046-A-8-A
#26 CCV L5	#26 CCV L5

QC Batch: 3	LC 537 ICAL Raw Batch: 206410
#26 CCV L5	#26 CCV L5
#27 RB	#27 RB
#28 320-35046-A-9-A	#28 320-35046-A-9-A
#29 320-35046-A-10-A	#29 320-35046-A-10-A
#30 320-35046-A-11-A	#30 320-35046-A-11-A
#31 320-35046-A-12-A	#31 320-35046-A-12-A
#32 320-35046-A-12-D LMS	#32 320-35046-A-12-D LMS
#33 320-35046-A-12-E LMSD	#33 320-35046-A-12-E LMSD
#34 320-35046-A-13-A	#34 320-35046-A-13-A
#35 320-35046-A-14-A	#35 320-35046-A-14-A
#36 320-35046-A-15-A	#36 320-35046-A-15-A
#37 320-35046-A-16-A	#37 320-35046-A-16-A
#38 CCV L3	#38 CCV L3

QC Batch: 4	LC 537 ICAL Raw Batch: 206412
#38 CCV L3	#38 CCV L3

QC Batch: 4	LC 537 ICAL Raw Batch: 206412
#39 RB	#39 RB
#40 320-35046-A-17-A	#40 320-35046-A-17-A
#41 320-35046-A-18-A	#41 320-35046-A-18-A
#42 320-35046-A-19-A	#42 320-35046-A-19-A
#43 CCV L5	#43 CCV L5
#44 RB	#44 RB

TestAmerica Laboratories
Worklist Run Log Report

Worklist Name: 31JAN2018_537A

Worklist Num: 53554

Instrument: A8_N

Method: 537_A8_N

Batch Directory: \\ChromNa\Sacramento\ChromData\A8_N\20180131-53554.b

Analysis Type: SemiVOA

Creator: Royce, Amani A

Inj Volume: 2.00

Inj Vol Units: ul

Lab ID	Worklist ID	Sample Type	Inj Date/Time	File Name	Vial	Dil Factor	Client ID	Fract
CCVL	320-0053554-001	CCVL	31-Jan-2018 10:52:35	2018.01.31_537A_004.d	2	1.0		sv
CCV L5	320-0053554-002	CCVIS	31-Jan-2018 10:57:15	2018.01.31_537A_005.d	5	1.0		sv
RB	320-0053554-003	RB	31-Jan-2018 11:01:55	2018.01.31_537A_006.d	8	1.0		sv
MB 320-205771/1-A	320-0053554-004	MB	31-Jan-2018 11:06:34	2018.01.31_537A_007.d	7	1.0		sv
LCS 320-205771/2-A	320-0053554-005	LCS	31-Jan-2018 11:11:14	2018.01.31_537A_008.d	8	1.0		sv
320-35362-A-1-A	320-0053554-006	Client	31-Jan-2018 11:15:55	2018.01.31_537A_009.d	9	1.0	WS-018	sv
320-35362-A-2-A	320-0053554-007	Client	31-Jan-2018 11:20:35	2018.01.31_537A_010.d	10	1.0	WS-095	sv
320-35362-A-2-B MS	320-0053554-008	MS	31-Jan-2018 11:25:15	2018.01.31_537A_011.d	11	1.0	WS-095	sv
320-35362-A-2-C MSD	320-0053554-009	MSD	31-Jan-2018 11:29:55	2018.01.31_537A_012.d	12	1.0	WS-095	sv
320-35362-A-3-A	320-0053554-010	Client	31-Jan-2018 11:34:36	2018.01.31_537A_013.d	13	1.0	DUP-017	sv
320-35362-A-4-A	320-0053554-011	Client	31-Jan-2018 11:39:17	2018.01.31_537A_014.d	14	1.0	FIELD BLANK 01-23-18	sv
320-35362-A-5-A	320-0053554-012	Client	31-Jan-2018 11:43:57	2018.01.31_537A_015.d	15	1.0	WS-096	sv
320-35362-A-6-A	320-0053554-013	Client	31-Jan-2018 11:48:38	2018.01.31_537A_016.d	16	1.0	WS-097	sv
CCV L3	320-0053554-014	CCVIS	31-Jan-2018 11:53:20	2018.01.31_537A_017.d	3	1.0		sv
RB	320-0053554-015	RB	31-Jan-2018 11:58:01	2018.01.31_537A_018.d	8	1.0		sv
MB 320-205489/1-A	320-0053554-016	MB	31-Jan-2018 12:02:42	2018.01.31_537A_019.d	17	1.0		sv
LLCS 320-205489/2-A	320-0053554-017	LLCS	31-Jan-2018 12:07:21	2018.01.31_537A_020.d	18	1.0		sv
320-35046-A-1-A	320-0053554-018	Client	31-Jan-2018 12:12:02	2018.01.31_537A_021.d	19	1.0	WGNA-011118-RW-3103	sv
320-35046-A-2-A	320-0053554-019	Client	31-Jan-2018 12:16:42	2018.01.31_537A_022.d	20	1.0	WGNA-011118-FRB-3103	sv
320-35046-A-3-A	320-0053554-020	Client	31-Jan-2018 12:21:23	2018.01.31_537A_023.d	21	1.0	WGNA-011118-RW-0683	sv
320-35046-A-4-A	320-0053554-021	Client	31-Jan-2018 12:26:04	2018.01.31_537A_024.d	22	1.0	WGNA-011118-FRB-0683	sv
320-35046-A-5-A	320-0053554-022	Client	31-Jan-2018 12:30:44	2018.01.31_537A_025.d	23	1.0	NAWC-011118-RW-139	sv
320-35046-A-6-A	320-0053554-023	Client	31-Jan-2018 12:35:24	2018.01.31_537A_026.d	24	1.0	NAWC-011118-FRB-139	sv
320-35046-A-7-A	320-0053554-024	Client	31-Jan-2018 12:40:06	2018.01.31_537A_027.d	25	1.0	WGNA-011118-DUP-18	sv
320-35046-A-8-A	320-0053554-025	Client	31-Jan-2018 12:44:47	2018.01.31_537A_028.d	26	1.0	NAWC-011118-RW-098	sv

Lab ID	Worklist ID	Sample Type	Inj Date/Time	File Name	Vial	Dil Factor	Client ID	Fract
CCV L5	320-0053554-026	CCVIS	31-Jan-2018 12:49:26	2018.01.31_537A_029.d	5	1.0		sv
RB	320-0053554-027	RB	31-Jan-2018 12:54:06	2018.01.31_537A_030.d	8	1.0		sv
320-35046-A-9-A	320-0053554-028	Client	31-Jan-2018 12:58:44	2018.01.31_537A_031.d	27	1.0	NAWC-011118-FRB-098	sv
320-35046-A-10-A	320-0053554-029	Client	31-Jan-2018 13:03:24	2018.01.31_537A_032.d	28	1.0	NAWC-011118-RW-180	sv
320-35046-A-11-A	320-0053554-030	Client	31-Jan-2018 13:08:04	2018.01.31_537A_033.d	29	1.0	NAWC-011118-FRB-180	sv
320-35046-A-12-A	320-0053554-031	Client	31-Jan-2018 13:12:44	2018.01.31_537A_034.d	30	1.0	NAWC-011118-RW-179	sv
320-35046-A-12-D LMS	320-0053554-032	LMS	31-Jan-2018 13:17:24	2018.01.31_537A_035.d	31	1.0		sv
320-35046-A-12-E LMSD	320-0053554-033	LMSD	31-Jan-2018 13:22:04	2018.01.31_537A_036.d	32	1.0		sv
320-35046-A-13-A	320-0053554-034	Client	31-Jan-2018 13:26:44	2018.01.31_537A_037.d	33	1.0	NAWC-011118-FRB-179	sv
320-35046-A-14-A	320-0053554-035	Client	31-Jan-2018 13:31:25	2018.01.31_537A_038.d	34	1.0	NAWC-011118-RW-303	sv
320-35046-A-15-A	320-0053554-036	Client	31-Jan-2018 13:36:05	2018.01.31_537A_039.d	35	1.0	NAWC-011118-FRB-303	sv
320-35046-A-16-A	320-0053554-037	Client	31-Jan-2018 13:40:45	2018.01.31_537A_040.d	36	1.0	WGNA-011118-RW-3409	sv
CCV L3	320-0053554-038	CCVIS	31-Jan-2018 13:45:26	2018.01.31_537A_041.d	3	1.0		sv
RB	320-0053554-039	RB	31-Jan-2018 13:50:07	2018.01.31_537A_042.d	8	1.0		sv
320-35046-A-17-A	320-0053554-040	Client	31-Jan-2018 13:54:46	2018.01.31_537A_043.d	37	1.0	WGNA-011118-FRB-3409	sv
320-35046-A-18-A	320-0053554-041	Client	31-Jan-2018 13:59:26	2018.01.31_537A_044.d	38	1.0	WGNA-011118-RW-3220	sv
320-35046-A-19-A	320-0053554-042	Client	31-Jan-2018 14:04:06	2018.01.31_537A_045.d	39	1.0	WGNA-011118-FRB-3220	sv
CCV L5	320-0053554-043	CCVIS	31-Jan-2018 14:08:46	2018.01.31_537A_046.d	5	1.0		sv
RB	320-0053554-044	RB	31-Jan-2018 14:13:26	2018.01.31_537A_047.d	8	1.0		sv

Aqueous Extraction Analysis Sheet

(To Accompany Samples to Instruments)

Analyst: Long, Tyrel W

63

A8 1/31/18











Batch Number: 320-205489

Method Code: 320-537_Prep-320

Batch Open: 1/25/2018 2:25:00PM

Batch End: 1/25/2018 10:10:00PM

Extraction of Perfluorinated Alkyl Acids

Input Sample Lab ID (Analytical Method)	SDG (Job #)	GrossWt TareWt	InitAmnt FinAmnt	Rcvd	PHs Adj1 Adj2	Due Date	Analytical TAT	Div Rank	Comments	Output Sample Lab ID
1 MB-320-205489/1 N/A	N/A		250 mL	7		N/A	N/A	N/A	Chlorine ND	
			1.00 mL							
2 LLCS-320-205489/2 N/A	N/A		250 mL	7		N/A	N/A	N/A	Chlorine ND	
			1.00 mL							
3 320-35046-A-1 (537_DOD5)	N/A (320-35046-1)	314.59 g	285.9 mL	7		1/16/18	16_Days	4	Chlorine ND	
		28.73 g	1.00 mL							
320-35046-A-2 (537_DOD5)	N/A (320-35046-1)	292.93 g	266 mL	7		1/16/18	16_Days	4	Chlorine ND	
		26.95 g	1.00 mL							
320-35046-A-3 (537_DOD5)	N/A (320-35046-1)	289.57 g	261 mL	7		1/16/18	16_Days	4	Chlorine ND	
		28.60 g	1.00 mL							
6 320-35046-A-4 (537_DOD5)	N/A (320-35046-1)	289.77 g	262.8 mL	7		1/16/18	16_Days	4	Chlorine ND	
		26.99 g	1.00 mL							
7 320-35046-A-5 (537_DOD5)	N/A (320-35046-1)	297.46 g	268.8 mL	7		1/16/18	16_Days	4	Chlorine ND	
		28.67 g	1.00 mL							
8 320-35046-A-6 (537_DOD5)	N/A (320-35046-1)	300.19 g	273.2 mL	7		1/16/18	16_Days	4	Chlorine ND	
		27.02 g	1.00 mL							
9 320-35046-A-7 (537_DOD5)	N/A (320-35046-1)	298.89 g	270.1 mL	7		1/16/18	16_Days	4	Chlorine ND	
		28.75 g	1.00 mL							
10 320-35046-A-8 (537_DOD5)	N/A (320-35046-1)	269.36 g	240.8 mL	7		1/16/18	16_Days	4	Chlorine ND	
		28.60 g	1.00 mL							

Page 382 of 391

Aqueous Extraction Analysis Sheet

(To Accompany Samples to Instruments)













Batch Number: 320-205489

Analyst: Long, Tyrel W

Batch Open: 1/25/2018 2:25:00PM

Method Code: 320-537_Prep-320

Batch End: 1/25/2018 10:10:00PM

11	320-35046-A-9 (537_DOD5)	N/A (320-35046-1)	296.99 g	269.9 mL	7			1/16/18	16_Days	4	Chlorine ND	
			27.08 g	1.00 mL								
12	320-35046-A-10 (537_DOD5)	N/A (320-35046-1)	293.90 g	265.4 mL	7			1/16/18	16_Days	4	Chlorine ND	
			28.52 g	1.00 mL								
13	320-35046-A-11 (537_DOD5)	N/A (320-35046-1)	291.23 g	264.2 mL	7			1/16/18	16_Days	4	Chlorine ND	
			27.05 g	1.00 mL								
14	320-35046-A-12 (537_DOD5)	N/A (320-35046-1)	290.54 g	261.9 mL	7			1/16/18	16_Days	4	Chlorine ND	
			28.61 g	1.00 mL								
15	320-35046-A-12-LMS (537_DOD5)	N/A (320-35046-1)	283.43 g	255.4 mL	7			1/16/18	16_Days	4	Chlorine ND	
			27.99 g	1.00 mL								
16	320-35046-A-12-LMSD (537_DOD5)	N/A (320-35046-1)	292.51 g	263.9 mL	7			1/16/18	16_Days	4	Chlorine ND	
			28.63 g	1.00 mL								
17	320-35046-A-13 (537_DOD5)	N/A (320-35046-1)	288.76 g	261.5 mL	7			1/16/18	16_Days	4	Chlorine ND	
			27.27 g	1.00 mL								
18	320-35046-A-14 (537_DOD5)	N/A (320-35046-1)	289.16 g	260.8 mL	7			1/16/18	16_Days	4	Chlorine ND	
			28.40 g	1.00 mL								
19	320-35046-A-15 (537_DOD5)	N/A (320-35046-1)	289.19 g	262 mL	7			1/16/18	16_Days	4	Chlorine ND	
			27.24 g	1.00 mL								
20	320-35046-A-16 (537_DOD5)	N/A (320-35046-1)	315.88 g	288 mL	7			1/16/18	16_Days	4	Chlorine ND	
			27.90 g	1.00 mL								
21	320-35046-A-17 (537_DOD5)	N/A (320-35046-1)	288.88 g	261.5 mL	7			1/16/18	16_Days	4	Chlorine ND	
			27.37 g	1.00 mL								
22	320-35046-A-18 (537_DOD5)	N/A (320-35046-1)	296.30 g	267.7 mL	7			1/16/18	16_Days	4	Chlorine ND	
			28.63 g	1.00 mL								

Aqueous Extraction Analysis Sheet

(To Accompany Samples to Instruments)

Batch Number: 320-205489


Analyst: Long, Tyrel W

Batch Open: 1/25/2018 2:25:00PM

Method Code: 320-537_Prep-320

Batch End: 1/25/2018 10:10:00PM

23

320-35046-A-19 (537_DOD5)	N/A (320-35046-1)	298.97 g	271.7 mL	7			1/16/18	16_Days	4	Chlorine ND	 <small>3 2 0 - 3 5 0 4 6 - A - 1 9 - A</small>
		27.24 g	1.00 mL								

Batch Notes

Manifold ID 1

pH Indicator ID 2517

Trizma ID SLBR4303V

SPE Cartridge ID 6369499-03

Methanol ID 1127847

Reagent Water ID 1-19-18

Internal Standard ID# 1099355

Pipette ID M16387D

Analyst ID - TA Reagent Drop JER

Analyst ID - TA Reagent Drop TWL

Witness

Analyst ID - SU Reagent Drop JER

Analyst ID - SU Reagent Drop TWL

Witness

Analyst ID - IS Reagent Drop JER

Analyst ID - IS Reagent Drop TWL

Witness

Analyst ID - Concentration TWL

Analyst ID - Aliquot Step TWL

Analyst ID - Final Volume Step TWL

Batch Comment Label ID's checked: TWL 1/25/18

Page 384 of 391

Aqueous Extraction Analysis Sheet

(To Accompany Samples to Instruments)

Batch Number: 320-205489

Analyst: Long, Tyrel W

Batch Open: 1/25/2018 2:25:00PM

Method Code: 320-537_Prep-320

Batch End: 1/25/2018 10:10:00PM

Comments

Aqueous Extraction Analysis Sheet

(To Accompany Samples to Instruments)

Batch Number: 320-205489



Analyst: Long, Tyrel W

Batch Open: 1/25/2018 2:25:00PM

Method Code: 320-537_Prep-320

Batch End:

Reagent Additions Worksheet

Lab ID	Reagent Code	Amount Added	Final Amount	By	Witness
MB 320-205489/1	LC537-SU_00053	100 uL	1.00 mL	 1/25/18	TWL 1/25/18 
LLCS 320-205489/2	LC537-LSP_00028	100 uL	1.00 mL		
LLCS 320-205489/2	LC537-SU_00053	100 uL	1.00 mL		
320-35046-A-1	LC537-SU_00053	100 uL	1.00 mL		
320-35046-A-2	LC537-SU_00053	100 uL	1.00 mL		
320-35046-A-3	LC537-SU_00053	100 uL	1.00 mL		
320-35046-A-4	LC537-SU_00053	100 uL	1.00 mL		
320-35046-A-5	LC537-SU_00053	100 uL	1.00 mL		
320-35046-A-6	LC537-SU_00053	100 uL	1.00 mL		
320-35046-A-7	LC537-SU_00053	100 uL	1.00 mL		
320-35046-A-8	LC537-SU_00053	100 uL	1.00 mL		
320-35046-A-9	LC537-SU_00053	100 uL	1.00 mL		
320-35046-A-10	LC537-SU_00053	100 uL	1.00 mL		
320-35046-A-11	LC537-SU_00053	100 uL	1.00 mL		
320-35046-A-12	LC537-SU_00053	100 uL	1.00 mL		
320-35046-A-12 LMS	LC537-LSP_00028	100 uL	1.00 mL		
320-35046-A-12 LMS	LC537-SU_00053	100 uL	1.00 mL		
320-35046-A-12 LMSD	LC537-LSP_00028	100 uL	1.00 mL		

Page 386 of 391

Aqueous Extraction Analysis Sheet

(To Accompany Samples to Instruments)

Batch Number: 320-205489

Analyst: Long, Tyrel W

Batch Open: 1/25/2018 2:25:00PM

Method Code: 320-537_Prep-320

Batch End:

320-35046-A-12 LMSD	LC537-SU_00053	100 uL	1.00 mL	<i>[Signature]</i> 1/25/18	<i>TWZ</i> 1/25/18
320-35046-A-13	LC537-SU_00053	100 uL	1.00 mL		
320-35046-A-14	LC537-SU_00053	100 uL	1.00 mL		
320-35046-A-15	LC537-SU_00053	100 uL	1.00 mL		
320-35046-A-16	LC537-SU_00053	100 uL	1.00 mL		
320-35046-A-17	LC537-SU_00053	100 uL	1.00 mL		
320-35046-A-18	LC537-SU_00053	100 uL	1.00 mL		
320-35046-A-19	LC537-SU_00053	100 uL	1.00 mL		

Other Reagents:

Reagent

Amount/Units

Lot#:

Page 387 of 391

Preparation Batch Number(s) 205489

Test 537- Prep

Earliest Holding Time 1/25/18

Batch Information	1 st Level Reviewer	2 nd Level Reviewer
Date and time accurate and entered into TALS correctly	✓	✓
All necessary batch information complete and entered into TALS correctly	✓	✓
BD, FV, and AL initials are transcribed into the batch comment	✓	✓
Sample List Tab	1 st Level Reviewer	2 nd Level Reviewer
Samples identified to the correct method	✓	✓
Holding time violation NCM filed	NA	NA
MS/MSD or MS/DU NCM filed	NA	NA
NCM for any anomalies filed	NA	NA
All NCMs include method code, matrix, and prep batch	NA	NA
Method/sample/login/QAS checked and correct	✓	✓
Batch contains no more than 20 live samples	✓	✓
Worksheet Tab	1 st Level Reviewer	2 nd Level Reviewer
All samples properly preserved	✓	✓
Weights in anticipated range and not targeted	✓	✓
All additional test requirements performed, documented, and uploaded to TALS correctly (e.g. final amount, initial amount, turbidity, and CI Check)	✓	✓
The pH is transcribed properly in TALS	✓	✓
All additional information is transcribed into TALS and is correct and raw data is attached	✓	✓
Comments/Observations are transcribed correctly in TALS	✓	✓
Reagents Tab	1 st Level Reviewer	2 nd Level Reviewer
All necessary reagents not expired and checked into TALS	✓	✓
All spike amounts correct and added to necessary samples and QC	✓	✓
Internal Standard is added to the reagents	✓	✓
All units are correctly transcribed into TALS	✓	✓

1st Level Reviewer: 

Date: 1/30/18

2nd Level Reviewer: VPM

Date: 1/30/18 - 1/31/18

Comments: _____

VPM 1/31/18

Shipping and Receiving Documents

TestAmerica Sacramento
 880 Riverside Parkway
 West Sacramento, CA 95605-1500
 phone 916.373.5600 fax 303.467.7248

Chain of Custody Record

TestAmerica
 THE LEADER IN ENVIRONMENTAL TESTING
TestAmerica Laboratories, Inc.

Regulatory Program: DW NPDES RCRA Other:

Client Contact		Project Manager: Andy Frebowitz		Site Contact: Mary Kay Bond		Date: 1/11/2018		COC No.:	
TetraTech 234 Mall Boulevard Suite 260 King of Prussia, PA 19406 610-382-1174 610-491-9688 Project Name: WE04 Site: WE04 P O # 1132358 (through EarthToxics)		Tel/Fax: 610.382.1170		Lab Contact: Dave Alltucker		Carrier: FedEx		1 of 1 COCs	
		Analysis Turnaround Time		Filtered Sample (Y/N) Perform MS/MSD (Y/N) EPA 537 UCMR3				For Lab Use Only: Walk-in Client: Lab Sampling: Job / SDG No.:	
		<input type="checkbox"/> CALENDAR DAYS <input type="checkbox"/> WORKING DAYS							
		TAT if different from Below 21							
		<input type="checkbox"/> 2 weeks <input type="checkbox"/> 1 week <input type="checkbox"/> 2 days <input type="checkbox"/> 1 day							
Sample Identification	Sample Date	Sample Time	Sample Type (C=Comp, G=Grab)	Matrix	# of Cont.				Sample Specific Notes:
WGNA-011118-RW-3103	1/11/2018	08:10	G	DW	2	N	N	X	
WGNA-011118-FRB-3103	1/11/2018	08:05	G	DW	2	N	N	X	Field Reagent Blank
WGNA-011118-RW-0683	1/11/2018	08:40	G	DW	2	N	N	X	
WGNA-011118-FRB-0683	1/11/2018	08:35	G	DW	2	N	N	X	Field Reagent Blank
NAWC-011118-RW-139	1/11/2018	10:40	G	DW	2	N	N	X	
NAWC-011118-FRB-139	1/11/2018	10:35	G	DW	2	N	N	X	Field Reagent Blank
WGNA-011118-DUP-18	1/11/2018	07:00	G	DW	2	N	N	X	DUPLICATE
NAWC-011118-RW-098	1/11/2018	11:10	G	DW	2	N	N	X	
NAWC-011118-FRB-098	1/11/2018	11:05	G	DW	2	N	N	X	Field Reagent Blank
NAWC-011118-RW-180	1/11/2018	12:10	G	DW	2	N	N	X	
NAWC-011118-FRB-180	1/11/2018	12:05	G	DW	2	N	N	X	Field Reagent Blank
NAWC-011118-RW-179	1/11/2018	12:40	G	DW	6	N	Y	X	MS/MSD
NAWC-011118-FRB-179	1/11/2018	12:35	G	DW	2	N	N	X	Field Reagent Blank
NAWC-011118-RW-303	1/11/2018	13:10	G	DW	2	N	N	X	
NAWC-011118-FRB-303	1/11/2018	13:05	G	DW	2	N	N	X	Field Reagent Blank
WGNA-011118-RW-3409	1/11/2018	15:10	G	DW	2	N	N	X	
WGNA-011118-FRB-3409	1/11/2018	15:05	G	DW	2	N	N	X	Field Reagent Blank
WGNA-011118-RW-3220	1/11/2018	16:10	G	DW	2	N	N	X	
WGNA-011118-FRB-3220	1/11/2018	16:05	G	DW	2	N	N	X	Field Reagent Blank
Preservation Used: 1= Ice, 2= HCl; 3= H2SO4; 4=HNO3; 5=NaOH; 6= Other: Trizma						6			
Possible Hazard Identification: Are any samples from a listed EPA Hazardous Waste? Please List any EPA Waste Codes for the sample in the						Sample Disposal (A fee may be assessed if samples are retained longer than 1 month)			
<input checked="" type="checkbox"/> Non-Hazard <input type="checkbox"/> Flammable <input type="checkbox"/> Skin Irritant <input type="checkbox"/> Poison B <input type="checkbox"/> Unknown						<input type="checkbox"/> Return to Client <input checked="" type="checkbox"/> Disposal by Lab <input type="checkbox"/> Archive for _____ Months			
Fed Ex Tracking: 7711 9926 0435						3-7 5.1			
Custody Seals Intact: <input type="checkbox"/> Yes <input type="checkbox"/> No		Custody Seal No.:		Cooler Temp. (°C): Obs'd: _____		Corr'd: _____		Therm ID No.: AK2	
Relinquished by: <i>Mary Kay Bond</i>		Company: Tetra Tech		Date/Time: 1/11/2018 18:00		Received by: <i>[Signature]</i>		Company: <i>TH-Sac</i> Date/Time: <i>1/12/18 1320</i>	
Relinquished by:		Company:		Date/Time:		Received by:		Company:	
Relinquished by:		Company:		Date/Time:		Received in Laboratory by:			



320-35046 Chain of Custody

3/2017

Login Sample Receipt Checklist

Client: Tetra Tech, Inc.

Job Number: 320-35046-1

Login Number: 35046

List Source: TestAmerica Sacramento

List Number: 1

Creator: Turpen, Troy

Question	Answer	Comment
Radioactivity wasn't checked or is \leq background as measured by a survey meter.	True	
The cooler's custody seal, if present, is intact.	True	
Sample custody seals, if present, are intact.	N/A	
The cooler or samples do not appear to have been compromised or tampered with.	True	
Samples were received on ice.	True	
Cooler Temperature is acceptable.	True	
Cooler Temperature is recorded.	True	
COC is present.	True	
COC is filled out in ink and legible.	True	
COC is filled out with all pertinent information.	True	
Is the Field Sampler's name present on COC?	True	
There are no discrepancies between the containers received and the COC.	True	
Samples are received within Holding Time (excluding tests with immediate HTs)	True	
Sample containers have legible labels.	True	
Containers are not broken or leaking.	True	
Sample collection date/times are provided.	True	
Appropriate sample containers are used.	True	
Sample bottles are completely filled.	True	
Sample Preservation Verified.	N/A	
There is sufficient vol. for all requested analyses, incl. any requested MS/MSDs	True	
Containers requiring zero headspace have no headspace or bubble is $<6\text{mm}$ (1/4").	True	
Multiphasic samples are not present.	True	
Samples do not require splitting or compositing.	True	
Residual Chlorine Checked.	N/A	

"WGNA-011118-RW-3103", "537", "RES", "320-35046-1", "TALSAC", "1763-23-1", "Perfluorooctanesulfonic acid (PFOS)", "10", "ng/L", "J M", "5.9", "DL", "", "TRG", "", "", "35", "LOQ", "YES", "-99", "", "285.9", "1.00", "14", ""

"WGNA-011118-RW-3103", "537", "RES", "320-35046-1", "TALSAC", "335-67-1", "Perfluorooctanoic acid (PFOA)", "12", "ng/L", "J", "2.4", "DL", "", "TRG", "", "", "17", "LOQ", "YES", "-99", "", "285.9", "1.00", "7.0", ""

"WGNA-011118-RW-3103", "537", "RES", "320-35046-1", "TALSAC", "355-46-4", "Perfluorohexanesulfonic acid (PFHxS)", "5.2", "ng/L", "J", "4.8", "DL", "", "TRG", "", "", "26", "LOQ", "YES", "-99", "", "285.9", "1.00", "10", ""

"WGNA-011118-RW-3103", "537", "RES", "320-35046-1", "TALSAC", "375-73-5", "Perfluorobutanesulfonic acid (PFBS)", "31", "ng/L", "U", "14", "DL", "", "TRG", "", "", "79", "LOQ", "YES", "-99", "", "285.9", "1.00", "31", ""

"WGNA-011118-RW-3103", "537", "RES", "320-35046-1", "TALSAC", "375-85-9", "Perfluoroheptanoic acid (PFHpA)", "3.4", "ng/L", "J", "1.7", "DL", "", "TRG", "", "", "8.7", "LOQ", "YES", "-99", "", "285.9", "1.00", "3.5", ""

"WGNA-011118-RW-3103", "537", "RES", "320-35046-1", "TALSAC", "375-95-1", "Perfluorononanoic acid (PFNA)", "17", "ng/L", "U", "7.0", "DL", "", "TRG", "", "", "21", "LOQ", "YES", "-99", "", "285.9", "1.00", "17", ""

"WGNA-011118-RW-3103", "537", "RES", "320-35046-1", "TALSAC", "STL00993", "13C2
PFHxA", "32", "ng/L", "", "-99", "DL", "", "SURR", "92", "", "-99", "LOQ", "YES", "35.0", "", "285.9", "1.00", "0", ""

"WGNA-011118-RW-3103", "537", "RES", "320-35046-1", "TALSAC", "STL00996", "13C2
PFDA", "34", "ng/L", "", "-99", "DL", "", "SURR", "97", "", "-99", "LOQ", "YES", "35.0", "", "285.9", "1.00", "0", ""

"NAWC-011118-RW-180", "537", "RES", "320-35046-10", "TALSAC", "1763-23-1", "Perfluorooctanesulfonic acid (PFOS)", "28", "ng/L", "J M", "6.4", "DL", "", "TRG", "", "", "38", "LOQ", "YES", "-99", "", "265.4", "1.00", "15", ""

"NAWC-011118-RW-180", "537", "RES", "320-35046-10", "TALSAC", "335-67-1", "Perfluorooctanoic acid (PFOA)", "23", "ng/L", "", "2.6", "DL", "", "TRG", "", "", "19", "LOQ", "YES", "-99", "", "265.4", "1.00", "7.5", ""

"NAWC-011118-RW-180", "537", "RES", "320-35046-10", "TALSAC", "355-46-4", "Perfluorohexanesulfonic acid (PFHxS)", "11", "ng/L", "J", "5.2", "DL", "", "TRG", "", "", "28", "LOQ", "YES", "-99", "", "265.4", "1.00", "11", ""

"NAWC-011118-RW-180", "537", "RES", "320-35046-10", "TALSAC", "375-73-5", "Perfluorobutanesulfonic acid (PFBS)", "34", "ng/L", "U", "15", "DL", "", "TRG", "", "", "85", "LOQ", "YES", "-99", "", "265.4", "1.00", "34", ""

"NAWC-011118-RW-180", "537", "RES", "320-35046-10", "TALSAC", "375-85-9", "Perfluoroheptanoic acid (PFHpA)", "9.1", "ng/L", "J", "1.8", "DL", "", "TRG", "", "", "9.4", "LOQ", "YES", "-99", "", "265.4", "1.00", "3.8", ""

"NAWC-011118-RW-180", "537", "RES", "320-35046-10", "TALSAC", "375-95-1", "Perfluorononanoic acid (PFNA)", "19", "ng/L", "U", "7.5", "DL", "", "TRG", "", "", "23", "LOQ", "YES", "-99", "", "265.4", "1.00", "19", ""

"NAWC-011118-RW-180", "537", "RES", "320-35046-10", "TALSAC", "STL00993", "13C2
PFHxA", "35", "ng/L", "", "-99", "DL", "", "SURR", "92", "", "-99", "LOQ", "YES", "37.7", "", "265.4", "1.00", "0", ""

"NAWC-011118-RW-180", "537", "RES", "320-35046-10", "TALSAC", "STL00996", "13C2
PFDA", "38", "ng/L", "", "-99", "DL", "", "SURR", "100", "", "-99", "LOQ", "YES", "37.7", "", "265.4", "1.00", "0", ""

"NAWC-011118-FRB-180", "537", "RES", "320-35046-11", "TALSAC", "1763-23-1", "Perfluorooctanesulfonic acid (PFOS)", "15", "ng/L", "U", "6.4", "DL", "", "TRG", "", "", "38", "LOQ", "YES", "-99", "", "264.2", "1.00", "15", ""

"NAWC-011118-FRB-180", "537", "RES", "320-35046-11", "TALSAC", "335-67-1", "Perfluorooctanoic acid (PFOA)", "7.6", "ng/L", "U", "2.6", "DL", "", "TRG", "", "", "19", "LOQ", "YES", "-99", "", "264.2", "1.00", "7.6", ""

"NAWC-011118-FRB-180", "537", "RES", "320-35046-11", "TALSAC", "355-46-4", "Perfluorohexanesulfonic acid (PFHxS)", "11", "ng/L", "U", "5.2", "DL", "", "TRG", "", "", "28", "LOQ", "YES", "-99", "", "264.2", "1.00", "11", ""

"NAWC-011118-FRB-180", "537", "RES", "320-35046-11", "TALSAC", "375-73-5", "Perfluorobutanesulfonic acid (PFBS)", "34", "ng/L", "U", "15", "DL", "", "TRG", "", "", "85", "LOQ", "YES", "-99", "", "264.2", "1.00", "34", ""

"NAWC-011118-FRB-180", "537", "RES", "320-35046-11", "TALSAC", "375-85-9", "Perfluoroheptanoic acid (PFHpA)", "3.8", "ng/L", "U", "1.8", "DL", "", "TRG", "", "", "9.5", "LOQ", "YES", "-99", "", "264.2", "1.00", "3.8", ""

"NAWC-011118-FRB-180", "537", "RES", "320-35046-11", "TALSAC", "375-95-1", "Perfluorononanoic acid (PFNA)", "19", "ng/L", "U", "7.6", "DL", "", "TRG", "", "", "23", "LOQ", "YES", "-99", "", "264.2", "1.00", "19", ""

"NAWC-011118-FRB-180", "537", "RES", "320-35046-11", "TALSAC", "STL00993", "13C2
PFHxA", "38", "ng/L", "", "-99", "DL", "", "SURR", "99", "", "-99", "LOQ", "YES", "37.9", "", "264.2", "1.00", "0", ""

"NAWC-011118-FRB-180", "537", "RES", "320-35046-11", "TALSAC", "STL00996", "13C2
PFDA", "38", "ng/L", "", "-99", "DL", "", "SURR", "100", "", "-99", "LOQ", "YES", "37.9", "", "264.2", "1.00", "0", ""

"NAWC-011118-RW-179", "537", "RES", "320-35046-12", "TALSAC", "1763-23-1", "Perfluorooctanesulfonic acid (PFOS)", "18", "ng/L", "J M", "6.5", "DL", "", "TRG", "", "", "38", "LOQ", "YES", "-99", "", "261.9", "1.00", "15", ""

"NAWC-011118-RW-179", "537", "RES", "320-35046-12", "TALSAC", "335-67-1", "Perfluorooctanoic acid (PFOA)", "18", "ng/L", "J", "2.7", "DL", "", "TRG", "", "", "19", "LOQ", "YES", "-99", "", "261.9", "1.00", "7.6", ""

"NAWC-011118-RW-179", "537", "RES", "320-35046-12", "TALSAC", "355-46-4", "Perfluorohexanesulfonic acid

(PFHxS)", "6.2", "ng/L", "J", "5.3", "DL", "", "TRG", "", "", "29", "LOQ", "YES", "-99", "", "261.9", "1.00", "11", "", "NAWC-011118-RW-179", "537", "RES", "320-35046-12", "TALSAC", "375-73-5", "Perfluorobutanesulfonic acid (PFBS)", "34", "ng/L", "U", "15", "DL", "", "TRG", "", "", "86", "LOQ", "YES", "-99", "", "261.9", "1.00", "34", "", "NAWC-011118-RW-179", "537", "RES", "320-35046-12", "TALSAC", "375-85-9", "Perfluoroheptanoic acid (PFHpA)", "4.7", "ng/L", "J", "1.8", "DL", "", "TRG", "", "", "9.5", "LOQ", "YES", "-99", "", "261.9", "1.00", "3.8", "", "NAWC-011118-RW-179", "537", "RES", "320-35046-12", "TALSAC", "375-95-1", "Perfluorononanoic acid (PFNA)", "19", "ng/L", "U", "7.6", "DL", "", "TRG", "", "", "23", "LOQ", "YES", "-99", "", "261.9", "1.00", "19", "", "NAWC-011118-RW-179", "537", "RES", "320-35046-12", "TALSAC", "STL00993", "13C2 PFHxA", "36", "ng/L", "", "-99", "DL", "", "SURR", "93", "", "-99", "LOQ", "YES", "38.2", "", "261.9", "1.00", "0", "", "NAWC-011118-RW-179", "537", "RES", "320-35046-12", "TALSAC", "STL00996", "13C2 PFDA", "38", "ng/L", "", "-99", "DL", "", "SURR", "101", "", "-99", "LOQ", "YES", "38.2", "", "261.9", "1.00", "0", "", "NAWC-011118-RW-179MS", "537", "RES", "320-35046-12MS", "TALSAC", "1763-23-1", "Perfluorooctanesulfonic acid (PFOS)", "54.3", "ng/L", "M", "6.7", "DL", "", "SPK", "94", "", "39", "LOQ", "YES", "39.2", "NAWC-011118-RW-179", "255.4", "1.00", "16", "" "NAWC-011118-RW-179MS", "537", "RES", "320-35046-12MS", "TALSAC", "335-67-1", "Perfluorooctanoic acid (PFOA)", "37.3", "ng/L", "", "2.7", "DL", "", "SPK", "96", "", "20", "LOQ", "YES", "19.6", "NAWC-011118-RW-179", "255.4", "1.00", "7.8", "" "NAWC-011118-RW-179MS", "537", "RES", "320-35046-12MS", "TALSAC", "355-46-4", "Perfluorohexanesulfonic acid (PFHxS)", "34.9", "ng/L", "", "5.4", "DL", "", "SPK", "98", "", "29", "LOQ", "YES", "29.4", "NAWC-011118-RW-179", "255.4", "1.00", "12", "" "NAWC-011118-RW-179MS", "537", "RES", "320-35046-12MS", "TALSAC", "375-73-5", "Perfluorobutanesulfonic acid (PFBS)", "90.6", "ng/L", "", "16", "DL", "", "SPK", "103", "", "88", "LOQ", "YES", "88.1", "NAWC-011118-RW-179", "255.4", "1.00", "35", "" "NAWC-011118-RW-179MS", "537", "RES", "320-35046-12MS", "TALSAC", "375-85-9", "Perfluoroheptanoic acid (PFHpA)", "14.9", "ng/L", "", "1.9", "DL", "", "SPK", "104", "", "9.8", "LOQ", "YES", "9.79", "NAWC-011118-RW-179", "255.4", "1.00", "3.9", "" "NAWC-011118-RW-179MS", "537", "RES", "320-35046-12MS", "TALSAC", "375-95-1", "Perfluorononanoic acid (PFNA)", "21.2", "ng/L", "J", "7.8", "DL", "", "SPK", "109", "", "23", "LOQ", "YES", "19.6", "NAWC-011118-RW-179", "255.4", "1.00", "20", "" "NAWC-011118-RW-179MS", "537", "RES", "320-35046-12MS", "TALSAC", "STL00993", "13C2 PFHxA", "36.7", "ng/L", "", "-99", "DL", "", "SURR", "94", "", "-99", "LOQ", "YES", "39.2", "NAWC-011118-RW-179", "255.4", "1.00", "0", "" "NAWC-011118-RW-179MS", "537", "RES", "320-35046-12MS", "TALSAC", "STL00996", "13C2 PFDA", "42.2", "ng/L", "", "-99", "DL", "", "SURR", "108", "", "-99", "LOQ", "YES", "39.2", "NAWC-011118-RW-179", "255.4", "1.00", "0", "" "NAWC-011118-RW-179MSD", "537", "RES", "320-35046-12MSD", "TALSAC", "1763-23-1", "Perfluorooctanesulfonic acid (PFOS)", "51.8", "ng/L", "M", "6.4", "DL", "", "SPK", "90", "5", "38", "LOQ", "YES", "37.9", "NAWC-011118-RW-179", "263.9", "1.00", "15", "" "NAWC-011118-RW-179MSD", "537", "RES", "320-35046-12MSD", "TALSAC", "335-67-1", "Perfluorooctanoic acid (PFOA)", "35.1", "ng/L", "", "2.7", "DL", "", "SPK", "88", "6", "19", "LOQ", "YES", "19.0", "NAWC-011118-RW-179", "263.9", "1.00", "7.6", "" "NAWC-011118-RW-179MSD", "537", "RES", "320-35046-12MSD", "TALSAC", "355-46-4", "Perfluorohexanesulfonic acid (PFHxS)", "33.0", "ng/L", "", "5.2", "DL", "", "SPK", "94", "6", "28", "LOQ", "YES", "28.4", "NAWC-011118-RW-179", "263.9", "1.00", "11", "" "NAWC-011118-RW-179MSD", "537", "RES", "320-35046-12MSD", "TALSAC", "375-73-5", "Perfluorobutanesulfonic acid (PFBS)", "84.3", "ng/L", "J", "15", "DL", "", "SPK", "99", "7", "85", "LOQ", "YES", "85.3", "NAWC-011118-RW-179", "263.9", "1.00", "34", "" "NAWC-011118-RW-179MSD", "537", "RES", "320-35046-12MSD", "TALSAC", "375-85-9", "Perfluoroheptanoic acid (PFHpA)", "13.0", "ng/L", "", "1.8", "DL", "", "SPK", "88", "13", "9.5", "LOQ", "YES", "9.47", "NAWC-011118-RW-179", "263.9", "1.00", "3.8", "" "NAWC-011118-RW-179MSD", "537", "RES", "320-35046-12MSD", "TALSAC", "375-95-1", "Perfluorononanoic acid (PFNA)", "19.6", "ng/L", "J", "7.6", "DL", "", "SPK", "104", "8", "23", "LOQ", "YES", "18.9", "NAWC-011118-RW-179", "263.9", "1.00", "19", "" "NAWC-011118-RW-179MSD", "537", "RES", "320-35046-12MSD", "TALSAC", "STL00993", "13C2

PFHxA", "33.2", "ng/L", "", "-99", "DL", "", "SURR", "88", "", "-99", "LOQ", "YES", "37.9", "NAWC-011118-RW-179", "263.9", "1.00", "0", ""

"NAWC-011118-RW-179MSD", "537", "RES", "320-35046-12MSD", "TALSAC", "STL00996", "13C2
PFDA", "36.7", "ng/L", "", "-99", "DL", "", "SURR", "97", "", "-99", "LOQ", "YES", "37.9", "NAWC-011118-RW-179", "263.9", "1.00", "0", ""

"NAWC-011118-FRB-179", "537", "RES", "320-35046-13", "TALSAC", "1763-23-1", "Perfluorooctanesulfonic acid (PFOS)", "15", "ng/L", "U", "6.5", "DL", "", "TRG", "", "", "38", "LOQ", "YES", "-99", "", "261.5", "1.00", "15", ""

"NAWC-011118-FRB-179", "537", "RES", "320-35046-13", "TALSAC", "335-67-1", "Perfluorooctanoic acid (PFOA)", "7.6", "ng/L", "U", "2.7", "DL", "", "TRG", "", "", "19", "LOQ", "YES", "-99", "", "261.5", "1.00", "7.6", ""

"NAWC-011118-FRB-179", "537", "RES", "320-35046-13", "TALSAC", "355-46-4", "Perfluorohexanesulfonic acid (PFHxS)", "11", "ng/L", "U", "5.3", "DL", "", "TRG", "", "", "29", "LOQ", "YES", "-99", "", "261.5", "1.00", "11", ""

"NAWC-011118-FRB-179", "537", "RES", "320-35046-13", "TALSAC", "375-73-5", "Perfluorobutanesulfonic acid (PFBS)", "34", "ng/L", "U", "15", "DL", "", "TRG", "", "", "86", "LOQ", "YES", "-99", "", "261.5", "1.00", "34", ""

"NAWC-011118-FRB-179", "537", "RES", "320-35046-13", "TALSAC", "375-85-9", "Perfluoroheptanoic acid (PFHpA)", "3.8", "ng/L", "U", "1.8", "DL", "", "TRG", "", "", "9.6", "LOQ", "YES", "-99", "", "261.5", "1.00", "3.8", ""

"NAWC-011118-FRB-179", "537", "RES", "320-35046-13", "TALSAC", "375-95-1", "Perfluorononanoic acid (PFNA)", "19", "ng/L", "U", "7.6", "DL", "", "TRG", "", "", "23", "LOQ", "YES", "-99", "", "261.5", "1.00", "19", ""

"NAWC-011118-FRB-179", "537", "RES", "320-35046-13", "TALSAC", "STL00993", "13C2
PFHxA", "36", "ng/L", "", "-99", "DL", "", "SURR", "95", "", "-99", "LOQ", "YES", "38.2", "", "261.5", "1.00", "0", ""

"NAWC-011118-FRB-179", "537", "RES", "320-35046-13", "TALSAC", "STL00996", "13C2
PFDA", "36", "ng/L", "", "-99", "DL", "", "SURR", "95", "", "-99", "LOQ", "YES", "38.2", "", "261.5", "1.00", "0", ""

"NAWC-011118-RW-303", "537", "RES", "320-35046-14", "TALSAC", "1763-23-1", "Perfluorooctanesulfonic acid (PFOS)", "21", "ng/L", "J M", "6.5", "DL", "", "TRG", "", "", "38", "LOQ", "YES", "-99", "", "260.8", "1.00", "15", ""

"NAWC-011118-RW-303", "537", "RES", "320-35046-14", "TALSAC", "335-67-1", "Perfluorooctanoic acid (PFOA)", "20", "ng/L", "", "2.7", "DL", "", "TRG", "", "", "19", "LOQ", "YES", "-99", "", "260.8", "1.00", "7.7", ""

"NAWC-011118-RW-303", "537", "RES", "320-35046-14", "TALSAC", "355-46-4", "Perfluorohexanesulfonic acid (PFHxS)", "7.3", "ng/L", "J", "5.3", "DL", "", "TRG", "", "", "29", "LOQ", "YES", "-99", "", "260.8", "1.00", "12", ""

"NAWC-011118-RW-303", "537", "RES", "320-35046-14", "TALSAC", "375-73-5", "Perfluorobutanesulfonic acid (PFBS)", "35", "ng/L", "U", "15", "DL", "", "TRG", "", "", "86", "LOQ", "YES", "-99", "", "260.8", "1.00", "35", ""

"NAWC-011118-RW-303", "537", "RES", "320-35046-14", "TALSAC", "375-85-9", "Perfluoroheptanoic acid (PFHpA)", "6.0", "ng/L", "J", "1.8", "DL", "", "TRG", "", "", "9.6", "LOQ", "YES", "-99", "", "260.8", "1.00", "3.8", ""

"NAWC-011118-RW-303", "537", "RES", "320-35046-14", "TALSAC", "375-95-1", "Perfluorononanoic acid (PFNA)", "19", "ng/L", "U", "7.7", "DL", "", "TRG", "", "", "23", "LOQ", "YES", "-99", "", "260.8", "1.00", "19", ""

"NAWC-011118-RW-303", "537", "RES", "320-35046-14", "TALSAC", "STL00993", "13C2
PFHxA", "35", "ng/L", "", "-99", "DL", "", "SURR", "91", "", "-99", "LOQ", "YES", "38.3", "", "260.8", "1.00", "0", ""

"NAWC-011118-RW-303", "537", "RES", "320-35046-14", "TALSAC", "STL00996", "13C2
PFDA", "39", "ng/L", "", "-99", "DL", "", "SURR", "103", "", "-99", "LOQ", "YES", "38.3", "", "260.8", "1.00", "0", ""

"NAWC-011118-FRB-303", "537", "RES", "320-35046-15", "TALSAC", "1763-23-1", "Perfluorooctanesulfonic acid (PFOS)", "15", "ng/L", "U", "6.5", "DL", "", "TRG", "", "", "38", "LOQ", "YES", "-99", "", "262", "1.00", "15", ""

"NAWC-011118-FRB-303", "537", "RES", "320-35046-15", "TALSAC", "335-67-1", "Perfluorooctanoic acid (PFOA)", "7.6", "ng/L", "U", "2.7", "DL", "", "TRG", "", "", "19", "LOQ", "YES", "-99", "", "262", "1.00", "7.6", ""

"NAWC-011118-FRB-303", "537", "RES", "320-35046-15", "TALSAC", "355-46-4", "Perfluorohexanesulfonic acid (PFHxS)", "11", "ng/L", "U", "5.2", "DL", "", "TRG", "", "", "29", "LOQ", "YES", "-99", "", "262", "1.00", "11", ""

"NAWC-011118-FRB-303", "537", "RES", "320-35046-15", "TALSAC", "375-73-5", "Perfluorobutanesulfonic acid (PFBS)", "34", "ng/L", "U", "15", "DL", "", "TRG", "", "", "86", "LOQ", "YES", "-99", "", "262", "1.00", "34", ""

"NAWC-011118-FRB-303", "537", "RES", "320-35046-15", "TALSAC", "375-85-9", "Perfluoroheptanoic acid (PFHpA)", "3.8", "ng/L", "U", "1.8", "DL", "", "TRG", "", "", "9.5", "LOQ", "YES", "-99", "", "262", "1.00", "3.8", ""

"NAWC-011118-FRB-303", "537", "RES", "320-35046-15", "TALSAC", "375-95-1", "Perfluorononanoic acid (PFNA)", "19", "ng/L", "U", "7.6", "DL", "", "TRG", "", "", "23", "LOQ", "YES", "-99", "", "262", "1.00", "19", ""

"NAWC-011118-FRB-303", "537", "RES", "320-35046-15", "TALSAC", "STL00993", "13C2
PFHxA", "35", "ng/L", "", "-99", "DL", "", "SURR", "92", "", "-99", "LOQ", "YES", "38.2", "", "262", "1.00", "0", ""

"NAWC-011118-FRB-303", "537", "RES", "320-35046-15", "TALSAC", "STL00996", "13C2
PFDA", "39", "ng/L", "", "-99", "DL", "", "SURR", "102", "", "-99", "LOQ", "YES", "38.2", "", "262", "1.00", "0", ""

"WGNA-011118-RW-3409", "537", "RES", "320-35046-16", "TALSAC", "1763-23-1", "Perfluorooctanesulfonic acid

(PFOS),"20","ng/L","J M","5.9","DL","","TRG","","","35","LOQ","YES",-99","","288","1.00","14","","
"WGNA-011118-RW-3409","537","RES","320-35046-16","TALSAC","335-67-1","Perfluorooctanoic acid
(PFOA),"14","ng/L","J","2.4","DL","","TRG","","","17","LOQ","YES",-99","","288","1.00","6.9","","
"WGNA-011118-RW-3409","537","RES","320-35046-16","TALSAC","355-46-4","Perfluorohexanesulfonic acid
(PFHxS),"7.9","ng/L","J","4.8","DL","","TRG","","","26","LOQ","YES",-99","","288","1.00","10","","
"WGNA-011118-RW-3409","537","RES","320-35046-16","TALSAC","375-73-5","Perfluorobutanesulfonic acid
(PFBS),"31","ng/L","U","14","DL","","TRG","","","78","LOQ","YES",-99","","288","1.00","31","","
"WGNA-011118-RW-3409","537","RES","320-35046-16","TALSAC","375-85-9","Perfluoroheptanoic acid
(PFHpA),"5.1","ng/L","J","1.6","DL","","TRG","","","8.7","LOQ","YES",-99","","288","1.00","3.5","","
"WGNA-011118-RW-3409","537","RES","320-35046-16","TALSAC","375-95-1","Perfluorononanoic acid
(PFNA),"17","ng/L","U","6.9","DL","","TRG","","","21","LOQ","YES",-99","","288","1.00","17","","
"WGNA-011118-RW-3409","537","RES","320-35046-16","TALSAC","STL00993","13C2
PFHxA","32","ng/L","","-99","DL","","SURR","91","","-99","LOQ","YES","34.7","","288","1.00","0","","
"WGNA-011118-RW-3409","537","RES","320-35046-16","TALSAC","STL00996","13C2
PFDA","35","ng/L","","-99","DL","","SURR","100","","-99","LOQ","YES","34.7","","288","1.00","0","","
"WGNA-011118-FRB-3409","537","RES","320-35046-17","TALSAC","1763-23-1","Perfluorooctanesulfonic acid
(PFOS),"15","ng/L","U","6.5","DL","","TRG","","","38","LOQ","YES",-99","","261.5","1.00","15","","
"WGNA-011118-FRB-3409","537","RES","320-35046-17","TALSAC","335-67-1","Perfluorooctanoic acid
(PFOA),"7.6","ng/L","U","2.7","DL","","TRG","","","19","LOQ","YES",-99","","261.5","1.00","7.6","","
"WGNA-011118-FRB-3409","537","RES","320-35046-17","TALSAC","355-46-4","Perfluorohexanesulfonic acid
(PFHxS),"11","ng/L","U","5.3","DL","","TRG","","","29","LOQ","YES",-99","","261.5","1.00","11","","
"WGNA-011118-FRB-3409","537","RES","320-35046-17","TALSAC","375-73-5","Perfluorobutanesulfonic acid
(PFBS),"34","ng/L","U","15","DL","","TRG","","","86","LOQ","YES",-99","","261.5","1.00","34","","
"WGNA-011118-FRB-3409","537","RES","320-35046-17","TALSAC","375-85-9","Perfluoroheptanoic acid
(PFHpA),"3.8","ng/L","U","1.8","DL","","TRG","","","9.6","LOQ","YES",-99","","261.5","1.00","3.8","","
"WGNA-011118-FRB-3409","537","RES","320-35046-17","TALSAC","375-95-1","Perfluorononanoic acid
(PFNA),"19","ng/L","U","7.6","DL","","TRG","","","23","LOQ","YES",-99","","261.5","1.00","19","","
"WGNA-011118-FRB-3409","537","RES","320-35046-17","TALSAC","STL00993","13C2
PFHxA","38","ng/L","","-99","DL","","SURR","99","","-99","LOQ","YES","38.2","","261.5","1.00","0","","
"WGNA-011118-FRB-3409","537","RES","320-35046-17","TALSAC","STL00996","13C2
PFDA","39","ng/L","","-99","DL","","SURR","101","","-99","LOQ","YES","38.2","","261.5","1.00","0","","
"WGNA-011118-RW-3220","537","RES","320-35046-18","TALSAC","1763-23-1","Perfluorooctanesulfonic acid
(PFOS),"38","ng/L","M","6.4","DL","","TRG","","","37","LOQ","YES",-99","","267.7","1.00","15","","
"WGNA-011118-RW-3220","537","RES","320-35046-18","TALSAC","335-67-1","Perfluorooctanoic acid
(PFOA),"13","ng/L","J","2.6","DL","","TRG","","","19","LOQ","YES",-99","","267.7","1.00","7.5","","
"WGNA-011118-RW-3220","537","RES","320-35046-18","TALSAC","355-46-4","Perfluorohexanesulfonic acid
(PFHxS),"17","ng/L","J","5.1","DL","","TRG","","","28","LOQ","YES",-99","","267.7","1.00","11","","
"WGNA-011118-RW-3220","537","RES","320-35046-18","TALSAC","375-73-5","Perfluorobutanesulfonic acid
(PFBS),"110","ng/L","","15","DL","","TRG","","","84","LOQ","YES",-99","","267.7","1.00","34","","
"WGNA-011118-RW-3220","537","RES","320-35046-18","TALSAC","375-85-9","Perfluoroheptanoic acid
(PFHpA),"8.0","ng/L","J","1.8","DL","","TRG","","","9.3","LOQ","YES",-99","","267.7","1.00","3.7","","
"WGNA-011118-RW-3220","537","RES","320-35046-18","TALSAC","375-95-1","Perfluorononanoic acid
(PFNA),"19","ng/L","U","7.5","DL","","TRG","","","22","LOQ","YES",-99","","267.7","1.00","19","","
"WGNA-011118-RW-3220","537","RES","320-35046-18","TALSAC","STL00993","13C2
PFHxA","32","ng/L","","-99","DL","","SURR","85","","-99","LOQ","YES","37.4","","267.7","1.00","0","","
"WGNA-011118-RW-3220","537","RES","320-35046-18","TALSAC","STL00996","13C2
PFDA","36","ng/L","","-99","DL","","SURR","97","","-99","LOQ","YES","37.4","","267.7","1.00","0","","
"WGNA-011118-FRB-3220","537","RES","320-35046-19","TALSAC","1763-23-1","Perfluorooctanesulfonic acid
(PFOS),"15","ng/L","U","6.3","DL","","TRG","","","37","LOQ","YES",-99","","271.7","1.00","15","","
"WGNA-011118-FRB-3220","537","RES","320-35046-19","TALSAC","335-67-1","Perfluorooctanoic acid
(PFOA),"7.4","ng/L","U","2.6","DL","","TRG","","","18","LOQ","YES",-99","","271.7","1.00","7.4","","
"WGNA-011118-FRB-3220","537","RES","320-35046-19","TALSAC","355-46-4","Perfluorohexanesulfonic acid
(PFHxS),"11","ng/L","U","5.1","DL","","TRG","","","28","LOQ","YES",-99","","271.7","1.00","11","","
"WGNA-011118-FRB-3220","537","RES","320-35046-19","TALSAC","375-73-5","Perfluorobutanesulfonic acid

(PFBS)", "33", "ng/L", "U", "15", "DL", "", "TRG", "", "", "83", "LOQ", "YES", "-99", "", "271.7", "1.00", "33", ""
"WGNA-011118-FRB-3220", "537", "RES", "320-35046-19", "TALSAC", "375-85-9", "Perfluoroheptanoic acid
(PFHpA)", "3.7", "ng/L", "U", "1.7", "DL", "", "TRG", "", "", "9.2", "LOQ", "YES", "-99", "", "271.7", "1.00", "3.7", ""
"WGNA-011118-FRB-3220", "537", "RES", "320-35046-19", "TALSAC", "375-95-1", "Perfluorononanoic acid
(PFNA)", "18", "ng/L", "U", "7.4", "DL", "", "TRG", "", "", "22", "LOQ", "YES", "-99", "", "271.7", "1.00", "18", ""
"WGNA-011118-FRB-3220", "537", "RES", "320-35046-19", "TALSAC", "STL00993", "13C2
PFHxA", "35", "ng/L", "", "-99", "DL", "", "SURR", "95", "", "-99", "LOQ", "YES", "36.8", "", "271.7", "1.00", "0", ""
"WGNA-011118-FRB-3220", "537", "RES", "320-35046-19", "TALSAC", "STL00996", "13C2
PFDA", "37", "ng/L", "", "-99", "DL", "", "SURR", "101", "", "-99", "LOQ", "YES", "36.8", "", "271.7", "1.00", "0", ""
"WGNA-011118-FRB-3103", "537", "RES", "320-35046-2", "TALSAC", "1763-23-1", "Perfluorooctanesulfonic acid
(PFOS)", "15", "ng/L", "U", "6.4", "DL", "", "TRG", "", "", "38", "LOQ", "YES", "-99", "", "266", "1.00", "15", ""
"WGNA-011118-FRB-3103", "537", "RES", "320-35046-2", "TALSAC", "335-67-1", "Perfluorooctanoic acid
(PFOA)", "7.5", "ng/L", "U", "2.6", "DL", "", "TRG", "", "", "19", "LOQ", "YES", "-99", "", "266", "1.00", "7.5", ""
"WGNA-011118-FRB-3103", "537", "RES", "320-35046-2", "TALSAC", "355-46-4", "Perfluorohexanesulfonic acid
(PFHxS)", "11", "ng/L", "U", "5.2", "DL", "", "TRG", "", "", "28", "LOQ", "YES", "-99", "", "266", "1.00", "11", ""
"WGNA-011118-FRB-3103", "537", "RES", "320-35046-2", "TALSAC", "375-73-5", "Perfluorobutanesulfonic acid
(PFBS)", "34", "ng/L", "U", "15", "DL", "", "TRG", "", "", "85", "LOQ", "YES", "-99", "", "266", "1.00", "34", ""
"WGNA-011118-FRB-3103", "537", "RES", "320-35046-2", "TALSAC", "375-85-9", "Perfluoroheptanoic acid
(PFHpA)", "3.8", "ng/L", "U", "1.8", "DL", "", "TRG", "", "", "9.4", "LOQ", "YES", "-99", "", "266", "1.00", "3.8", ""
"WGNA-011118-FRB-3103", "537", "RES", "320-35046-2", "TALSAC", "375-95-1", "Perfluorononanoic acid
(PFNA)", "19", "ng/L", "U", "7.5", "DL", "", "TRG", "", "", "23", "LOQ", "YES", "-99", "", "266", "1.00", "19", ""
"WGNA-011118-FRB-3103", "537", "RES", "320-35046-2", "TALSAC", "STL00993", "13C2
PFHxA", "37", "ng/L", "", "-99", "DL", "", "SURR", "99", "", "-99", "LOQ", "YES", "37.6", "", "266", "1.00", "0", ""
"WGNA-011118-FRB-3103", "537", "RES", "320-35046-2", "TALSAC", "STL00996", "13C2
PFDA", "39", "ng/L", "", "-99", "DL", "", "SURR", "104", "", "-99", "LOQ", "YES", "37.6", "", "266", "1.00", "0", ""
"WGNA-011118-RW-0683", "537", "RES", "320-35046-3", "TALSAC", "1763-23-1", "Perfluorooctanesulfonic acid
(PFOS)", "29", "ng/L", "J M", "6.5", "DL", "", "TRG", "", "", "38", "LOQ", "YES", "-99", "", "261", "1.00", "15", ""
"WGNA-011118-RW-0683", "537", "RES", "320-35046-3", "TALSAC", "335-67-1", "Perfluorooctanoic acid
(PFOA)", "18", "ng/L", "J", "2.7", "DL", "", "TRG", "", "", "19", "LOQ", "YES", "-99", "", "261", "1.00", "7.7", ""
"WGNA-011118-RW-0683", "537", "RES", "320-35046-3", "TALSAC", "355-46-4", "Perfluorohexanesulfonic acid
(PFHxS)", "5.8", "ng/L", "J", "5.3", "DL", "", "TRG", "", "", "29", "LOQ", "YES", "-99", "", "261", "1.00", "11", ""
"WGNA-011118-RW-0683", "537", "RES", "320-35046-3", "TALSAC", "375-73-5", "Perfluorobutanesulfonic acid
(PFBS)", "34", "ng/L", "U", "15", "DL", "", "TRG", "", "", "86", "LOQ", "YES", "-99", "", "261", "1.00", "34", ""
"WGNA-011118-RW-0683", "537", "RES", "320-35046-3", "TALSAC", "375-85-9", "Perfluoroheptanoic acid
(PFHpA)", "5.2", "ng/L", "J", "1.8", "DL", "", "TRG", "", "", "9.6", "LOQ", "YES", "-99", "", "261", "1.00", "3.8", ""
"WGNA-011118-RW-0683", "537", "RES", "320-35046-3", "TALSAC", "375-95-1", "Perfluorononanoic acid
(PFNA)", "19", "ng/L", "U", "7.7", "DL", "", "TRG", "", "", "23", "LOQ", "YES", "-99", "", "261", "1.00", "19", ""
"WGNA-011118-RW-0683", "537", "RES", "320-35046-3", "TALSAC", "STL00993", "13C2
PFHxA", "33", "ng/L", "", "-99", "DL", "", "SURR", "87", "", "-99", "LOQ", "YES", "38.3", "", "261", "1.00", "0", ""
"WGNA-011118-RW-0683", "537", "RES", "320-35046-3", "TALSAC", "STL00996", "13C2
PFDA", "37", "ng/L", "", "-99", "DL", "", "SURR", "96", "", "-99", "LOQ", "YES", "38.3", "", "261", "1.00", "0", ""
"WGNA-011118-FRB-0683", "537", "RES", "320-35046-4", "TALSAC", "1763-23-1", "Perfluorooctanesulfonic acid
(PFOS)", "15", "ng/L", "U", "6.5", "DL", "", "TRG", "", "", "38", "LOQ", "YES", "-99", "", "262.8", "1.00", "15", ""
"WGNA-011118-FRB-0683", "537", "RES", "320-35046-4", "TALSAC", "335-67-1", "Perfluorooctanoic acid
(PFOA)", "7.6", "ng/L", "U", "2.7", "DL", "", "TRG", "", "", "19", "LOQ", "YES", "-99", "", "262.8", "1.00", "7.6", ""
"WGNA-011118-FRB-0683", "537", "RES", "320-35046-4", "TALSAC", "355-46-4", "Perfluorohexanesulfonic acid
(PFHxS)", "11", "ng/L", "U", "5.2", "DL", "", "TRG", "", "", "29", "LOQ", "YES", "-99", "", "262.8", "1.00", "11", ""
"WGNA-011118-FRB-0683", "537", "RES", "320-35046-4", "TALSAC", "375-73-5", "Perfluorobutanesulfonic acid
(PFBS)", "34", "ng/L", "U", "15", "DL", "", "TRG", "", "", "86", "LOQ", "YES", "-99", "", "262.8", "1.00", "34", ""
"WGNA-011118-FRB-0683", "537", "RES", "320-35046-4", "TALSAC", "375-85-9", "Perfluoroheptanoic acid
(PFHpA)", "3.8", "ng/L", "U", "1.8", "DL", "", "TRG", "", "", "9.5", "LOQ", "YES", "-99", "", "262.8", "1.00", "3.8", ""
"WGNA-011118-FRB-0683", "537", "RES", "320-35046-4", "TALSAC", "375-95-1", "Perfluorononanoic acid
(PFNA)", "19", "ng/L", "U", "7.6", "DL", "", "TRG", "", "", "23", "LOQ", "YES", "-99", "", "262.8", "1.00", "19", ""
"WGNA-011118-FRB-0683", "537", "RES", "320-35046-4", "TALSAC", "STL00993", "13C2

PFHxA","37","ng/L","",-99","DL","","SURR","96","",-99","LOQ","YES","38.1","","262.8","1.00","0",""
"WGNA-011118-FRB-0683","537","RES","320-35046-4","TALSAC","STL00996","13C2
PFDA","38","ng/L","",-99","DL","","SURR","99","",-99","LOQ","YES","38.1","","262.8","1.00","0",""
"NAWC-011118-RW-139","537","RES","320-35046-5","TALSAC","1763-23-1","Perfluorooctanesulfonic acid
(PFOS)","12","ng/L","J M","6.3","DL","","TRG","","","37","LOQ","YES","-99","","268.8","1.00","15",""
"NAWC-011118-RW-139","537","RES","320-35046-5","TALSAC","335-67-1","Perfluorooctanoic acid
(PFOA)","16","ng/L","J","2.6","DL","","TRG","","","19","LOQ","YES","-99","","268.8","1.00","7.4",""
"NAWC-011118-RW-139","537","RES","320-35046-5","TALSAC","355-46-4","Perfluorohexanesulfonic acid
(PFHxS)","11","ng/L","U","5.1","DL","","TRG","","","28","LOQ","YES","-99","","268.8","1.00","11",""
"NAWC-011118-RW-139","537","RES","320-35046-5","TALSAC","375-73-5","Perfluorobutanesulfonic acid
(PFBS)","33","ng/L","U","15","DL","","TRG","","","84","LOQ","YES","-99","","268.8","1.00","33",""
"NAWC-011118-RW-139","537","RES","320-35046-5","TALSAC","375-85-9","Perfluoroheptanoic acid
(PFHpA)","5.4","ng/L","J","1.8","DL","","TRG","","","9.3","LOQ","YES","-99","","268.8","1.00","3.7",""
"NAWC-011118-RW-139","537","RES","320-35046-5","TALSAC","375-95-1","Perfluorononanoic acid
(PFNA)","19","ng/L","U","7.4","DL","","TRG","","","22","LOQ","YES","-99","","268.8","1.00","19",""
"NAWC-011118-RW-139","537","RES","320-35046-5","TALSAC","STL00993","13C2
PFHxA","34","ng/L","",-99","DL","","SURR","92","",-99","LOQ","YES","37.2","","268.8","1.00","0",""
"NAWC-011118-RW-139","537","RES","320-35046-5","TALSAC","STL00996","13C2
PFDA","36","ng/L","",-99","DL","","SURR","97","",-99","LOQ","YES","37.2","","268.8","1.00","0",""
"NAWC-011118-FRB-139","537","RES","320-35046-6","TALSAC","1763-23-1","Perfluorooctanesulfonic acid
(PFOS)","15","ng/L","U","6.2","DL","","TRG","","","37","LOQ","YES","-99","","273.2","1.00","15",""
"NAWC-011118-FRB-139","537","RES","320-35046-6","TALSAC","335-67-1","Perfluorooctanoic acid
(PFOA)","7.3","ng/L","U","2.6","DL","","TRG","","","18","LOQ","YES","-99","","273.2","1.00","7.3",""
"NAWC-011118-FRB-139","537","RES","320-35046-6","TALSAC","355-46-4","Perfluorohexanesulfonic acid
(PFHxS)","11","ng/L","U","5.0","DL","","TRG","","","27","LOQ","YES","-99","","273.2","1.00","11",""
"NAWC-011118-FRB-139","537","RES","320-35046-6","TALSAC","375-73-5","Perfluorobutanesulfonic acid
(PFBS)","33","ng/L","U","15","DL","","TRG","","","82","LOQ","YES","-99","","273.2","1.00","33",""
"NAWC-011118-FRB-139","537","RES","320-35046-6","TALSAC","375-85-9","Perfluoroheptanoic acid
(PFHpA)","3.7","ng/L","U","1.7","DL","","TRG","","","9.2","LOQ","YES","-99","","273.2","1.00","3.7",""
"NAWC-011118-FRB-139","537","RES","320-35046-6","TALSAC","375-95-1","Perfluorononanoic acid
(PFNA)","18","ng/L","U","7.3","DL","","TRG","","","22","LOQ","YES","-99","","273.2","1.00","18",""
"NAWC-011118-FRB-139","537","RES","320-35046-6","TALSAC","STL00993","13C2
PFHxA","33","ng/L","",-99","DL","","SURR","90","",-99","LOQ","YES","36.6","","273.2","1.00","0",""
"NAWC-011118-FRB-139","537","RES","320-35046-6","TALSAC","STL00996","13C2
PFDA","35","ng/L","",-99","DL","","SURR","96","",-99","LOQ","YES","36.6","","273.2","1.00","0",""
"WGNA-011118-DUP-18","537","RES","320-35046-7","TALSAC","1763-23-1","Perfluorooctanesulfonic acid
(PFOS)","12","ng/L","J M","6.3","DL","","TRG","","","37","LOQ","YES","-99","","270.1","1.00","15",""
"WGNA-011118-DUP-18","537","RES","320-35046-7","TALSAC","335-67-1","Perfluorooctanoic acid
(PFOA)","15","ng/L","J","2.6","DL","","TRG","","","19","LOQ","YES","-99","","270.1","1.00","7.4",""
"WGNA-011118-DUP-18","537","RES","320-35046-7","TALSAC","355-46-4","Perfluorohexanesulfonic acid
(PFHxS)","11","ng/L","U","5.1","DL","","TRG","","","28","LOQ","YES","-99","","270.1","1.00","11",""
"WGNA-011118-DUP-18","537","RES","320-35046-7","TALSAC","375-73-5","Perfluorobutanesulfonic acid
(PFBS)","33","ng/L","U","15","DL","","TRG","","","83","LOQ","YES","-99","","270.1","1.00","33",""
"WGNA-011118-DUP-18","537","RES","320-35046-7","TALSAC","375-85-9","Perfluoroheptanoic acid
(PFHpA)","5.2","ng/L","J","1.8","DL","","TRG","","","9.3","LOQ","YES","-99","","270.1","1.00","3.7",""
"WGNA-011118-DUP-18","537","RES","320-35046-7","TALSAC","375-95-1","Perfluorononanoic acid
(PFNA)","19","ng/L","U","7.4","DL","","TRG","","","22","LOQ","YES","-99","","270.1","1.00","19",""
"WGNA-011118-DUP-18","537","RES","320-35046-7","TALSAC","STL00993","13C2
PFHxA","34","ng/L","",-99","DL","","SURR","92","",-99","LOQ","YES","37.0","","270.1","1.00","0",""
"WGNA-011118-DUP-18","537","RES","320-35046-7","TALSAC","STL00996","13C2
PFDA","37","ng/L","",-99","DL","","SURR","101","",-99","LOQ","YES","37.0","","270.1","1.00","0",""
"NAWC-011118-RW-098","537","RES","320-35046-8","TALSAC","1763-23-1","Perfluorooctanesulfonic acid
(PFOS)","16","ng/L","J M","7.1","DL","","TRG","","","42","LOQ","YES","-99","","240.8","1.00","17",""
"NAWC-011118-RW-098","537","RES","320-35046-8","TALSAC","335-67-1","Perfluorooctanoic acid

(PFOA),"14","ng/L","J","2.9","DL","","TRG","","","21","LOQ","YES",-99","","240.8","1.00","8.3","","
"NAWC-011118-RW-098","537","RES","320-35046-8","TALSAC","355-46-4","Perfluorohexanesulfonic acid
(PFHxS),"12","ng/L","U","5.7","DL","","TRG","","","31","LOQ","YES",-99","","240.8","1.00","12","","
"NAWC-011118-RW-098","537","RES","320-35046-8","TALSAC","375-73-5","Perfluorobutanesulfonic acid
(PFBS),"37","ng/L","U","17","DL","","TRG","","","93","LOQ","YES",-99","","240.8","1.00","37","","
"NAWC-011118-RW-098","537","RES","320-35046-8","TALSAC","375-85-9","Perfluoroheptanoic acid
(PFHpA),"3.9","ng/L","J M","2.0","DL","","TRG","","","10","LOQ","YES",-99","","240.8","1.00","4.2","","
"NAWC-011118-RW-098","537","RES","320-35046-8","TALSAC","375-95-1","Perfluorononanoic acid
(PFNA),"21","ng/L","U M","8.3","DL","","TRG","","","25","LOQ","YES",-99","","240.8","1.00","21","","
"NAWC-011118-RW-098","537","RES","320-35046-8","TALSAC","STL00993","13C2
PFHxA","38","ng/L","","-99","DL","","SURR","91","","-99","LOQ","YES","41.5","","240.8","1.00","0","","
"NAWC-011118-RW-098","537","RES","320-35046-8","TALSAC","STL00996","13C2
PFDA","42","ng/L","","-99","DL","","SURR","102","","-99","LOQ","YES","41.5","","240.8","1.00","0","","
"NAWC-011118-FRB-098","537","RES","320-35046-9","TALSAC","1763-23-1","Perfluorooctanesulfonic acid
(PFOS),"15","ng/L","U","6.3","DL","","TRG","","","37","LOQ","YES",-99","","269.9","1.00","15","","
"NAWC-011118-FRB-098","537","RES","320-35046-9","TALSAC","335-67-1","Perfluorooctanoic acid
(PFOA),"7.4","ng/L","U","2.6","DL","","TRG","","","19","LOQ","YES",-99","","269.9","1.00","7.4","","
"NAWC-011118-FRB-098","537","RES","320-35046-9","TALSAC","355-46-4","Perfluorohexanesulfonic acid
(PFHxS),"11","ng/L","U","5.1","DL","","TRG","","","28","LOQ","YES",-99","","269.9","1.00","11","","
"NAWC-011118-FRB-098","537","RES","320-35046-9","TALSAC","375-73-5","Perfluorobutanesulfonic acid
(PFBS),"33","ng/L","U","15","DL","","TRG","","","83","LOQ","YES",-99","","269.9","1.00","33","","
"NAWC-011118-FRB-098","537","RES","320-35046-9","TALSAC","375-85-9","Perfluoroheptanoic acid
(PFHpA),"3.7","ng/L","U","1.8","DL","","TRG","","","9.3","LOQ","YES",-99","","269.9","1.00","3.7","","
"NAWC-011118-FRB-098","537","RES","320-35046-9","TALSAC","375-95-1","Perfluorononanoic acid
(PFNA),"19","ng/L","U","7.4","DL","","TRG","","","22","LOQ","YES",-99","","269.9","1.00","19","","
"NAWC-011118-FRB-098","537","RES","320-35046-9","TALSAC","STL00993","13C2
PFHxA","34","ng/L","","-99","DL","","SURR","93","","-99","LOQ","YES","37.1","","269.9","1.00","0","","
"NAWC-011118-FRB-098","537","RES","320-35046-9","TALSAC","STL00996","13C2
PFDA","35","ng/L","","-99","DL","","SURR","94","","-99","LOQ","YES","37.1","","269.9","1.00","0","","
"LLCS 320-205489/2-A","537","RES","LLCS 320-205489/2-A","TALSAC","1763-23-1","Perfluorooctanesulfonic
acid (PFOS),"38.5","ng/L","J M","6.8","DL","","SPK","96","","40","LOQ","YES","40.0","","250","1.00","16","","
"LLCS 320-205489/2-A","537","RES","LLCS 320-205489/2-A","TALSAC","335-67-1","Perfluorooctanoic acid
(PFOA),"20.1","ng/L","","2.8","DL","","SPK","100","","20","LOQ","YES","20.0","","250","1.00","8.0","","
"LLCS 320-205489/2-A","537","RES","LLCS 320-205489/2-A","TALSAC","355-46-4","Perfluorohexanesulfonic acid
(PFHxS),"29.0","ng/L","J","5.5","DL","","SPK","97","","30","LOQ","YES","30.0","","250","1.00","12","","
"LLCS 320-205489/2-A","537","RES","LLCS 320-205489/2-A","TALSAC","375-73-5","Perfluorobutanesulfonic acid
(PFBS),"91.7","ng/L","","16","DL","","SPK","102","","90","LOQ","YES","90.0","","250","1.00","36","","
"LLCS 320-205489/2-A","537","RES","LLCS 320-205489/2-A","TALSAC","375-85-9","Perfluoroheptanoic acid
(PFHpA),"11.1","ng/L","","1.9","DL","","SPK","111","","10","LOQ","YES","10.0","","250","1.00","4.0","","
"LLCS 320-205489/2-A","537","RES","LLCS 320-205489/2-A","TALSAC","375-95-1","Perfluorononanoic acid
(PFNA),"19.9","ng/L","J","8.0","DL","","SPK","99","","24","LOQ","YES","20.0","","250","1.00","20","","
"LLCS 320-205489/2-A","537","RES","LLCS 320-205489/2-A","TALSAC","STL00993","13C2
PFHxA","41.4","ng/L","","-99","DL","","SURR","103","","-99","LOQ","YES","40.0","","250","1.00","0","","
"LLCS 320-205489/2-A","537","RES","LLCS 320-205489/2-A","TALSAC","STL00996","13C2
PFDA","41.6","ng/L","","-99","DL","","SURR","104","","-99","LOQ","YES","40.0","","250","1.00","0","","
"MB 320-205489/1-A","537","RES","MB 320-205489/1-A","TALSAC","1763-23-1","Perfluorooctanesulfonic acid
(PFOS),"16","ng/L","U","6.8","DL","","TRG","","","40","LOQ","YES",-99","","250","1.00","16","","
"MB 320-205489/1-A","537","RES","MB 320-205489/1-A","TALSAC","335-67-1","Perfluorooctanoic acid
(PFOA),"8.0","ng/L","U","2.8","DL","","TRG","","","20","LOQ","YES",-99","","250","1.00","8.0","","
"MB 320-205489/1-A","537","RES","MB 320-205489/1-A","TALSAC","355-46-4","Perfluorohexanesulfonic acid
(PFHxS),"12","ng/L","U","5.5","DL","","TRG","","","30","LOQ","YES",-99","","250","1.00","12","","
"MB 320-205489/1-A","537","RES","MB 320-205489/1-A","TALSAC","375-73-5","Perfluorobutanesulfonic acid
(PFBS),"36","ng/L","U","16","DL","","TRG","","","90","LOQ","YES",-99","","250","1.00","36","","
"MB 320-205489/1-A","537","RES","MB 320-205489/1-A","TALSAC","375-85-9","Perfluoroheptanoic acid

(PFHpA),"4.0","ng/L","U","1.9","DL","","TRG","","","10","LOQ","YES",-99","","250","1.00","4.0","","
"MB 320-205489/1-A","537","RES","MB 320-205489/1-A","TALSAC","375-95-1","Perfluorononanoic acid
(PFNA),"20","ng/L","U","8.0","DL","","TRG","","","24","LOQ","YES",-99","","250","1.00","20","","
"MB 320-205489/1-A","537","RES","MB 320-205489/1-A","TALSAC","STL00993","13C2
PFHxA","38.0","ng/L","","-99","DL","","SURR","95","","-99","LOQ","YES","40.0","","250","1.00","0","","
"MB 320-205489/1-A","537","RES","MB 320-205489/1-A","TALSAC","STL00996","13C2
PFDA","40.3","ng/L","","-99","DL","","SURR","101","","-99","LOQ","YES","40.0","","250","1.00","0","","
"Unknown","Unknown","WGNA-011118-RW-3103","01/11/2018 08:10","AQ","320-35046-
1","NM","","5.1","537","METHOD","RES","01/24/2018 20:52","01/31/2018
12:12","TALSAC","COA","WET","NA","1","NA","NA","","100","320-205489","320-205489","NA","320-
206408","320-35046-1","01/12/2018 13:20","01/15/2018 16:05","","
"Unknown","Unknown","NAWC-011118-RW-180","01/11/2018 12:10","AQ","320-35046-
10","NM","","5.1","537","METHOD","RES","01/24/2018 20:52","01/31/2018
13:03","TALSAC","COA","WET","NA","1","NA","NA","","100","320-205489","320-205489","NA","320-
206410","320-35046-1","01/12/2018 13:20","01/15/2018 16:05","","
"Unknown","Unknown","NAWC-011118-FRB-180","01/11/2018 12:05","AQ","320-35046-
11","FB","","5.1","537","METHOD","RES","01/24/2018 20:52","01/31/2018
13:08","TALSAC","COA","WET","NA","1","NA","NA","","100","320-205489","320-205489","NA","320-
206410","320-35046-1","01/12/2018 13:20","01/15/2018 16:05","","
"Unknown","Unknown","NAWC-011118-RW-179","01/11/2018 12:40","AQ","320-35046-
12","NM","","5.1","537","METHOD","RES","01/24/2018 20:52","01/31/2018
13:12","TALSAC","COA","WET","NA","1","NA","NA","","100","320-205489","320-205489","NA","320-
206410","320-35046-1","01/12/2018 13:20","01/15/2018 16:05","","
"Unknown","Unknown","NAWC-011118-RW-179MS","01/11/2018 12:40","AQ","320-35046-
12MS","MS","","5.1","537","METHOD","RES","01/24/2018 20:52","01/31/2018
13:17","TALSAC","COA","WET","NA","1","NA","NA","","100","320-205489","320-205489","NA","320-
206410","320-35046-1","01/12/2018 13:20","01/15/2018 16:05","","
"Unknown","Unknown","NAWC-011118-RW-179MSD","01/11/2018 12:40","AQ","320-35046-
12MSD","MSD","","5.1","537","METHOD","RES","01/24/2018 20:52","01/31/2018
13:22","TALSAC","COA","WET","NA","1","NA","NA","","100","320-205489","320-205489","NA","320-
206410","320-35046-1","01/12/2018 13:20","01/15/2018 16:05","","
"Unknown","Unknown","NAWC-011118-FRB-179","01/11/2018 12:35","AQ","320-35046-
13","FB","","5.1","537","METHOD","RES","01/24/2018 20:52","01/31/2018
13:26","TALSAC","COA","WET","NA","1","NA","NA","","100","320-205489","320-205489","NA","320-
206410","320-35046-1","01/12/2018 13:20","01/15/2018 16:05","","
"Unknown","Unknown","NAWC-011118-RW-303","01/11/2018 13:10","AQ","320-35046-
14","NM","","5.1","537","METHOD","RES","01/24/2018 20:52","01/31/2018
13:31","TALSAC","COA","WET","NA","1","NA","NA","","100","320-205489","320-205489","NA","320-
206410","320-35046-1","01/12/2018 13:20","01/15/2018 16:05","","
"Unknown","Unknown","NAWC-011118-FRB-303","01/11/2018 13:05","AQ","320-35046-
15","FB","","5.1","537","METHOD","RES","01/24/2018 20:52","01/31/2018
13:36","TALSAC","COA","WET","NA","1","NA","NA","","100","320-205489","320-205489","NA","320-
206410","320-35046-1","01/12/2018 13:20","01/15/2018 16:05","","
"Unknown","Unknown","WGNA-011118-RW-3409","01/11/2018 15:10","AQ","320-35046-
16","NM","","5.1","537","METHOD","RES","01/24/2018 20:52","01/31/2018
13:40","TALSAC","COA","WET","NA","1","NA","NA","","100","320-205489","320-205489","NA","320-
206410","320-35046-1","01/12/2018 13:20","01/15/2018 16:05","","
"Unknown","Unknown","WGNA-011118-FRB-3409","01/11/2018 15:05","AQ","320-35046-
17","FB","","5.1","537","METHOD","RES","01/24/2018 20:52","01/31/2018
13:54","TALSAC","COA","WET","NA","1","NA","NA","","100","320-205489","320-205489","NA","320-
206412","320-35046-1","01/12/2018 13:20","01/15/2018 16:05","","
"Unknown","Unknown","WGNA-011118-RW-3220","01/11/2018 16:10","AQ","320-35046-
18","NM","","5.1","537","METHOD","RES","01/24/2018 20:52","01/31/2018
13:59","TALSAC","COA","WET","NA","1","NA","NA","","100","320-205489","320-205489","NA","320-

206412","320-35046-1","01/12/2018 13:20","01/15/2018 16:05", ""
"Unknown","Unknown","WGNA-011118-FRB-3220","01/11/2018 16:05","AQ","320-35046-19","FB", "", "5.1", "537", "METHOD", "RES", "01/24/2018 20:52", "01/31/2018 14:04", "TALSAC", "COA", "WET", "NA", "1", "NA", "NA", "", "100", "320-205489", "320-205489", "NA", "320-206412", "320-35046-1", "01/12/2018 13:20", "01/15/2018 16:05", ""
"Unknown","Unknown","WGNA-011118-FRB-3103","01/11/2018 08:05","AQ","320-35046-2","FB", "", "5.1", "537", "METHOD", "RES", "01/24/2018 20:52", "01/31/2018 12:16", "TALSAC", "COA", "WET", "NA", "1", "NA", "NA", "", "100", "320-205489", "320-205489", "NA", "320-206408", "320-35046-1", "01/12/2018 13:20", "01/15/2018 16:05", ""
"Unknown","Unknown","WGNA-011118-RW-0683","01/11/2018 08:40","AQ","320-35046-3","NM", "", "5.1", "537", "METHOD", "RES", "01/24/2018 20:52", "01/31/2018 12:21", "TALSAC", "COA", "WET", "NA", "1", "NA", "NA", "", "100", "320-205489", "320-205489", "NA", "320-206408", "320-35046-1", "01/12/2018 13:20", "01/15/2018 16:05", ""
"Unknown","Unknown","WGNA-011118-FRB-0683","01/11/2018 08:35","AQ","320-35046-4","FB", "", "5.1", "537", "METHOD", "RES", "01/24/2018 20:52", "01/31/2018 12:26", "TALSAC", "COA", "WET", "NA", "1", "NA", "NA", "", "100", "320-205489", "320-205489", "NA", "320-206408", "320-35046-1", "01/12/2018 13:20", "01/15/2018 16:05", ""
"Unknown","Unknown","NAWC-011118-RW-139","01/11/2018 10:40","AQ","320-35046-5","NM", "", "5.1", "537", "METHOD", "RES", "01/24/2018 20:52", "01/31/2018 12:30", "TALSAC", "COA", "WET", "NA", "1", "NA", "NA", "", "100", "320-205489", "320-205489", "NA", "320-206408", "320-35046-1", "01/12/2018 13:20", "01/15/2018 16:05", ""
"Unknown","Unknown","NAWC-011118-FRB-139","01/11/2018 10:35","AQ","320-35046-6","FB", "", "5.1", "537", "METHOD", "RES", "01/24/2018 20:52", "01/31/2018 12:35", "TALSAC", "COA", "WET", "NA", "1", "NA", "NA", "", "100", "320-205489", "320-205489", "NA", "320-206408", "320-35046-1", "01/12/2018 13:20", "01/15/2018 16:05", ""
"Unknown","Unknown","WGNA-011118-DUP-18","01/11/2018 07:00","AQ","320-35046-7","FD", "", "5.1", "537", "METHOD", "RES", "01/24/2018 20:52", "01/31/2018 12:40", "TALSAC", "COA", "WET", "NA", "1", "NA", "NA", "", "100", "320-205489", "320-205489", "NA", "320-206408", "320-35046-1", "01/12/2018 13:20", "01/15/2018 16:05", ""
"Unknown","Unknown","NAWC-011118-RW-098","01/11/2018 11:10","AQ","320-35046-8","NM", "", "5.1", "537", "METHOD", "RES", "01/24/2018 20:52", "01/31/2018 12:44", "TALSAC", "COA", "WET", "NA", "1", "NA", "NA", "", "100", "320-205489", "320-205489", "NA", "320-206408", "320-35046-1", "01/12/2018 13:20", "01/15/2018 16:05", ""
"Unknown","Unknown","NAWC-011118-FRB-098","01/11/2018 11:05","AQ","320-35046-9","FB", "", "5.1", "537", "METHOD", "RES", "01/24/2018 20:52", "01/31/2018 12:58", "TALSAC", "COA", "WET", "NA", "1", "NA", "NA", "", "100", "320-205489", "320-205489", "NA", "320-206410", "320-35046-1", "01/12/2018 13:20", "01/15/2018 16:05", ""
"Unknown","Unknown","LLCS 320-205489/2-A", "", "AQ", "LLCS 320-205489/2-A", "LCS", "", "-99", "537", "METHOD", "RES", "01/24/2018 20:52", "01/31/2018 12:07", "TALSAC", "COA", "WET", "NA", "1", "NA", "NA", "", "100", "320-205489", "320-205489", "NA", "320-206408", "320-35046-1", "01/24/2018 20:52", "01/15/2018 16:05", ""
"Unknown","Unknown","MB 320-205489/1-A", "", "AQ", "MB 320-205489/1-A", "MB", "", "-99", "537", "METHOD", "RES", "01/24/2018 20:52", "01/31/2018 12:02", "TALSAC", "COA", "WET", "NA", "1", "NA", "NA", "", "100", "320-205489", "320-205489", "NA", "320-206408", "320-35046-1", "01/24/2018 20:52", "01/15/2018 16:05", ""



TO: A. FREBOWITZ **DATE:** FEBRUARY 5, 2018
FROM: TERRI L. SOLOMON **COPIES:** DV FILE
SUBJECT: ORGANIC DATA VALIDATION –POLYFLUOROALKYL SUBSTANCES (PFAS)
 NAS JRB WILLOW GROVE
 SAMPLE DELIVERY GROUP (SDG) 320-35046-1

SAMPLES: 9/Field Reagent Blank (FRB)
 WGNA-011118-FRB-3103 WGNA-011118-FRB-0683
 NAWC-011118-FRB-139 WGNA-011118-FRB-098
 NAWC-011118-FRB-180 NAWC-011118-FRB-179
 NAWC-011118-FRB-303 WGNA-011118-FRB-3409
 WGNA-011118-FRB-3220

10/Drinking Water
 WGNA-011118-RW-3103 WGNA-011118-RW-0683
 NAWC-011118-RW-139 WGNA-011118-DUP-18
 WGNA-011118-RW-098 NAWC-011118-RW-180
 NAWC-011118-RW-179 NAWC-011118-RW-303
 WGNA-011118-RW-3409 WGNA-011118-RW-3220

Overview

The sample set for NAS JRB Willow Grove, SDG 320-35046-1, consisted of ten (10) drinking water samples and nine (9) FRB samples. All samples were analyzed for select perfluorinated alkyl acids including pentadecafluorooctanoic acid (PFOA), perfluorobutane sulfonic acid (PFBS), perfluoroheptanoic acid (PFHpA), perfluorohexanesulfonic acid (PFHxS), perfluorononanoic acid (PFNA) and perfluorooctane sulfonic acid (PFOS). One (1) field duplicate sample pair (NAWC-011118-RW-139 / WGNA-011118-DUP-18) was included in this SDG.

The samples were collected by Tetra Tech on January 11, 2018 and analyzed by Test America-Sacramento. All sample analyses were conducted in accordance with EPA Method 537 version 1.1 analytical and reporting protocols.

The data contained in this SDG was validated with regard to the following parameters: data completeness, holding times, initial/continuing calibrations, laboratory method/FRBs, surrogate spike recoveries, laboratory control sample results, matrix spike / matrix spike duplicate results, field duplicate results, internal standard areas and recoveries, chromatographic resolution, analyte identification, analyte quantitation, and detection limits. Areas of concern are listed below.

Major

None.

Minor

Detected results reported below the limit of quantitation (LOQ) but above the detection limit (DL) were qualified as estimated, (J).

TO: A. FREBOWITZ
SDG: 320-35046-1

PAGE 2

Notes

Samples with detections and their associated FRBs are summarized below. No detected results were present in the FRBs.

<u>Sample</u>	<u>Associated FRB</u>
WGNA-011118-RW-3103	WGNA-011118-FRB-3103
WGNA-011118-RW-0683	WGNA-011118-FRB-3103
NAWC-011118-RW-139	NAWC-011118-FRB-3103
WGNA-011118-DUP-18	NAWC-011118-RW-139
WGNA-011118-RW-098	WGNA-011118-FRB-098
NAWC-011118-RW-180	NAWC-011118-FRB-180
NAWC-011118-RW-179	NAWC-011118-FRB-179
NAWC-011118-RW-303	NAWC-011118-FRB-303
WGNA-011118-RW-3409	WGNA-011118-FRB-3409
WGNA-011118-RW-3220	WGNA-011118-FRB-3220

Non-detected results were reported to the Limit of Detection (LOD).


The buffering agent Trizma was added to all drinking water samples.

Executive Summary


Laboratory Performance: No issues.

Other Factors Affecting Data Quality: Results below the RL were estimated.

The data for these analyses were reviewed with reference to the Environmental Protection Agency document EPA/600/R-08/092, Method 537, "Determination of Selected Perfluorinated Alkyl Acids in Drinking Water by Solid Phase Extraction and Liquid Chromatography/Tandem Mass Spectrometry (LC/MS/MS)", (September 2009) and the US EPA National Functional Guidelines for Organic Data Review (January 2017) as applicable. The text of this report has been formulated to address only those areas affecting data quality.



Tetra Tech, Inc.
Terri L. Solomon
Chemist/Data Validator



Tetra Tech, Inc.
Joseph A. Samchuck
Data Validation Manager

for

Attachments:

- Appendix A – Qualified Analytical Results
- Appendix B – Results as Reported by the Laboratory
- Appendix C – Support Documentation

Data Qualifier Definitions

The following definitions provide brief explanations of the validation qualifiers assigned to results in the data review process.

U	The analyte was analyzed for, but was not detected at a level greater than or equal to the level of the adjusted method detection limit for sample and method.
J	The analyte was positively identified and the associated numerical value is the approximate concentration of the analyte in the sample (due either to the quality of the data generated because certain quality control criteria were not met, or the concentration of the analyte was below the reporting limit).
J+	The result is an estimated quantity, but the result may be biased high.
J-	The result is an estimated quantity, but the result may be biased low.
UJ	The analyte was analyzed for, but was not detected. The reported detection limit is approximate and may be inaccurate or imprecise.
R	The sample result (detected) is unusable due to the quality of the data generated because certain criteria were not met. The analyte may or may not be present in the sample.
UR	The sample result (nondetected) is unusable due to the quality of the data generated because certain criteria were not met. The analyte may or may not be present in the sample.

Appendix A

Qualified Analytical Results

Qualifier Codes:

- A = Lab Blank Contamination
- B = Field Blank Contamination
- C = Calibration Noncompliance (i.e., % RSDs, %Ds, ICVs, CCVs, RRFs, etc.)
- C01 = GC/MS Tuning Noncompliance
- D = MS/MSD Recovery Noncompliance
- E = LCS/LCSD Recovery Noncompliance
- F = Lab Duplicate Imprecision
- G = Field Duplicate Imprecision
- H = Holding Time Exceedance
- I = ICP Serial Dilution Noncompliance
- J = ICP PDS Recovery Noncompliance; MSA's $r < 0.995$
- K = ICP Interference - includes ICS % R Noncompliance
- L = Instrument Calibration Range Exceedance
- M = Sample Preservation Noncompliance
- N = Internal Standard Noncompliance
- N01 = Internal Standard Recovery Noncompliance Dioxins
- N02 = Recovery Standard Noncompliance Dioxins
- N03 = Clean-up Standard Noncompliance Dioxins
- O = Poor Instrument Performance (i.e., base-time drifting)
- P = Uncertainty near detection limit ($< 2 \times$ IDL for inorganics and $<$ CRQL for organics)
- Q = Other problems (can encompass a number of issues; i.e.chromatography,interferences, etc.)
- R = Surrogates Recovery Noncompliance
- S = Pesticide/PCB Resolution
- T = % Breakdown Noncompliance for DDT and Endrin
- U = RPD between columns/detectors $>40\%$ for positive results determined via GC/HPLC
- V = Non-linear calibrations; correlation coefficient $r < 0.995$
- W = EMPC result
- X = Signal to noise response drop
- Y = Percent solids $<30\%$
- Z = Uncertainty at 2 standard deviations is greater than sample activity
- Z1 = Tentatively Identified Compound considered presumptively present
- Z2 = Tentatively Identified Compound column bleed
- Z3 = Tentatively Identified Compound aldol condensate
- Z4 = Sample activity is less than the at uncertainty at 3 standard deviations and greater than the MDC
- Z5 = Sample activity is less than the at uncertainty at 3 standard deviations and less than the MDC

PROJ_NO: 08005-WE04 SDG: 320-35046-1 FRACTION: PFAS MEDIA: WATER	NSAMPLE	NAWC-011118-FRB-098			NAWC-011118-FRB-139			NAWC-011118-FRB-179			NAWC-011118-FRB-180		
	LAB_ID	320-35046-9			320-35046-6			320-35046-13			320-35046-11		
	SAMP_DATE	1/11/2018			1/11/2018			1/11/2018			1/11/2018		
	QC_TYPE	FB			FB			FB			FB		
	UNITS	NG/L			NG/L			NG/L			NG/L		
	PCT_SOLIDS	0.0			0.0			0.0			0.0		
	DUP_OF												
PARAMETER	RESULT	VQL	QLCD	RESULT	VQL	QLCD	RESULT	VQL	QLCD	RESULT	VQL	QLCD	
PENTADECAFLUOROOCTANOIC ACID	7.4	U		7.3	U		7.6	U		7.6	U		
PERFLUOROBUTANESULFONIC ACID	33	U		33	U		34	U		34	U		
PERFLUOROHEPTANOIC ACID	3.7	U		3.7	U		3.8	U		3.8	U		
PERFLUOROHXANESULFONIC ACID	11	U		11	U		11	U		11	U		
PERFLUORONONANOIC ACID	19	U		18	U		19	U		19	U		
PERFLUOROOCTANE SULFONIC ACID	15	U		15	U		15	U		15	U		

PROJ_NO: 08005-WE04 SDG: 320-35046-1 FRACTION: PFAS MEDIA: WATER	NSAMPLE	NAWC-011118-FRB-303			NAWC-011118-RW-098			NAWC-011118-RW-139			NAWC-011118-RW-179		
	LAB_ID	320-35046-15			320-35046-8			320-35046-5			320-35046-12		
	SAMP_DATE	1/11/2018			1/11/2018			1/11/2018			1/11/2018		
	QC_TYPE	FB			NM			NM			NM		
	UNITS	NG/L			NG/L			NG/L			NG/L		
	PCT_SOLIDS	0.0			0.0			0.0			0.0		
	DUP_OF												
PARAMETER	RESULT	VQL	QLCD	RESULT	VQL	QLCD	RESULT	VQL	QLCD	RESULT	VQL	QLCD	
PENTADECAFLUOROOCTANOIC ACID	7.6	U		14	J	P	16	J	P	18	J	P	
PERFLUOROBUTANESULFONIC ACID	34	U		37	U		33	U		34	U		
PERFLUOROHEPTANOIC ACID	3.8	U		3.9	J	P	5.4	J	P	4.7	J	P	
PERFLUOROHXANESULFONIC ACID	11	U		12	U		11	U		6.2	J	P	
PERFLUORONONANOIC ACID	19	U		21	U		19	U		19	U		
PERFLUOROOCTANE SULFONIC ACID	15	U		16	J	P	12	J	P	18	J	P	

PROJ_NO: 08005-WE04 SDG: 320-35046-1 FRACTION: PFAS MEDIA: WATER	NSAMPLE	NAWC-011118-RW-180			NAWC-011118-RW-303			WGNA-011118-DUP-18			WGNA-011118-FRB-0683		
	LAB_ID	320-35046-10			320-35046-14			320-35046-7			320-35046-4		
	SAMP_DATE	1/11/2018			1/11/2018			1/11/2018			1/11/2018		
	QC_TYPE	NM			NM			FD			FB		
	UNITS	NG/L			NG/L			NG/L			NG/L		
	PCT_SOLIDS	0.0			0.0			0.0			0.0		
	DUP_OF							NAWC-011118-RW-139					
PARAMETER	RESULT	VQL	QLCD	RESULT	VQL	QLCD	RESULT	VQL	QLCD	RESULT	VQL	QLCD	
PENTADECAFLUOROOCTANOIC ACID	23			20			15	J	P	7.6	U		
PERFLUOROBUTANESULFONIC ACID	34	U		35	U		33	U		34	U		
PERFLUOROHEPTANOIC ACID	9.1	J	P	6	J	P	5.2	J	P	3.8	U		
PERFLUOROHXANESULFONIC ACID	11	J	P	7.3	J	P	11	U		11	U		
PERFLUORONONANOIC ACID	19	U		19	U		19	U		19	U		
PERFLUOROOCTANE SULFONIC ACID	28	J	P	21	J	P	12	J	P	15	U		

PROJ_NO: 08005-WE04 SDG: 320-35046-1 FRACTION: PFAS MEDIA: WATER	NSAMPLE	WGNA-011118-FRB-3103			WGNA-011118-FRB-3220			WGNA-011118-FRB-3409			WGNA-011118-RW-0683		
	LAB_ID	320-35046-2			320-35046-19			320-35046-17			320-35046-3		
	SAMP_DATE	1/11/2018			1/11/2018			1/11/2018			1/11/2018		
	QC_TYPE	FB			FB			FB			NM		
	UNITS	NG/L			NG/L			NG/L			NG/L		
	PCT_SOLIDS	0.0			0.0			0.0			0.0		
	DUP_OF												
PARAMETER	RESULT	VQL	QLCD	RESULT	VQL	QLCD	RESULT	VQL	QLCD	RESULT	VQL	QLCD	
PENTADECAFLUOROOCTANOIC ACID	7.5	U		7.4	U		7.6	U		18	J	P	
PERFLUOROBUTANESULFONIC ACID	34	U		33	U		34	U		34	U		
PERFLUOROHEPTANOIC ACID	3.8	U		3.7	U		3.8	U		5.2	J	P	
PERFLUOROHXANESULFONIC ACID	11	U		11	U		11	U		5.8	J	P	
PERFLUORONONANOIC ACID	19	U		18	U		19	U		19	U		
PERFLUOROOCTANE SULFONIC ACID	15	U		15	U		15	U		29	J	P	

PROJ_NO: 08005-WE04 SDG: 320-35046-1 FRACTION: PFAS MEDIA: WATER	NSAMPLE	WGNA-011118-RW-3103			WGNA-011118-RW-3220			WGNA-011118-RW-3409		
	LAB_ID	320-35046-1			320-35046-18			320-35046-16		
	SAMP_DATE	1/11/2018			1/11/2018			1/11/2018		
	QC_TYPE	NM			NM			NM		
	UNITS	NG/L			NG/L			NG/L		
	PCT_SOLIDS	0.0			0.0			0.0		
	DUP_OF									
PARAMETER	RESULT	VQL	QLCD	RESULT	VQL	QLCD	RESULT	VQL	QLCD	
PENTADECAFLUOROOCTANOIC ACID	12	J	P	13	J	P	14	J	P	
PERFLUOROBUTANESULFONIC ACID	31	U		110			31	U		
PERFLUOROHEPTANOIC ACID	3.4	J	P	8	J	P	5.1	J	P	
PERFLUOROHXANESULFONIC ACID	5.2	J	P	17	J	P	7.9	J	P	
PERFLUORONONANOIC ACID	17	U		19	U		17	U		
PERFLUOROOCTANE SULFONIC ACID	10	J	P	38			20	J	P	

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: WGNA-011118-RW-3103 Lab Sample ID: 320-35046-1
 Matrix: Water Lab File ID: 2018.01.31_537A_021.d
 Analysis Method: 537 Date Collected: 01/11/2018 08:10
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 285.9(mL) Date Analyzed: 01/31/2018 12:12
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	10	J M	35	14	5.9
335-67-1	Perfluorooctanoic acid (PFOA)	12	J	17	7.0	2.4
375-95-1	Perfluorononanoic acid (PFNA)	17	U	21	17	7.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	5.2	J	26	10	4.8
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.4	J	8.7	3.5	1.7
375-73-5	Perfluorobutanesulfonic acid (PFBS)	31	U	79	31	14

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	92		70-130
STL00996	13C2 PFDA	97		70-130

Wesley L. Selman
02/05/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: WGNA-011118-FRB-3103 Lab Sample ID: 320-35046-2
 Matrix: Water Lab File ID: 2018.01.31_537A_022.d
 Analysis Method: 537 Date Collected: 01/11/2018 08:05
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 266(mL) Date Analyzed: 01/31/2018 12:16
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	38	15	6.4
335-67-1	Perfluorooctanoic acid (PFOA)	7.5	U	19	7.5	2.6
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.5
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	U	9.4	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	85	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	99		70-130
STL00996	13C2 PFDA	104		70-130

Steve L. Salomon
02/05/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: WGNA-011118-RW-0683 Lab Sample ID: 320-35046-3
 Matrix: Water Lab File ID: 2018.01.31_537A_023.d
 Analysis Method: 537 Date Collected: 01/11/2018 08:40
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 261(mL) Date Analyzed: 01/31/2018 12:21
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	29	J M	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	18	J	19	7.7	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.7
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	5.8	J	29	11	5.3
375-85-9	Perfluoroheptanoic acid (PFHpA)	5.2	J	9.6	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	86	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	87		70-130
STL00996	13C2 PFDA	96		70-130

M. J. Salem
02/05/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: WGNA-011118-FRB-0683 Lab Sample ID: 320-35046-4
 Matrix: Water Lab File ID: 2018.01.31_537A_024.d
 Analysis Method: 537 Date Collected: 01/11/2018 08:35
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 262.8 (mL) Date Analyzed: 01/31/2018 12:26
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	7.6	U	19	7.6	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	29	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	U	9.5	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	86	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	96		70-130
STL00996	13C2 PFDA	99		70-130

Wesley J. Salmeron
02/05/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: NAWC-011118-RW-139 Lab Sample ID: 320-35046-5
 Matrix: Water Lab File ID: 2018.01.31_537A_025.d
 Analysis Method: 537 Date Collected: 01/11/2018 10:40
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 268.8 (mL) Date Analyzed: 01/31/2018 12:30
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	12	J M	37	15	6.3
335-67-1	Perfluorooctanoic acid (PFOA)	16	J	19	7.4	2.6
375-95-1	Perfluorononanoic acid (PFNA)	19	U	22	19	7.4
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.1
375-85-9	Perfluoroheptanoic acid (PFHpA)	5.4	J	9.3	3.7	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	33	U	84	33	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	92		70-130
STL00996	13C2 PFDA	97		70-130

Wesley L. Selman
02/05/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: NAWC-011118-FRB-139 Lab Sample ID: 320-35046-6
 Matrix: Water Lab File ID: 2018.01.31_537A_026.d
 Analysis Method: 537 Date Collected: 01/11/2018 10:35
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 273.2 (mL) Date Analyzed: 01/31/2018 12:35
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	37	15	6.2
335-67-1	Perfluorooctanoic acid (PFOA)	7.3	U	18	7.3	2.6
375-95-1	Perfluorononanoic acid (PFNA)	18	U	22	18	7.3
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	27	11	5.0
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.7	U	9.2	3.7	1.7
375-73-5	Perfluorobutanesulfonic acid (PFBS)	33	U	82	33	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	90		70-130
STL00996	13C2 PFDA	96		70-130

Amir L. Salameh
02/05/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: WGNA-011118-DUP-18 Lab Sample ID: 320-35046-7
 Matrix: Water Lab File ID: 2018.01.31_537A_027.d
 Analysis Method: 537 Date Collected: 01/11/2018 07:00
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 270.1(mL) Date Analyzed: 01/31/2018 12:40
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	12	J M	37	15	6.3
335-67-1	Perfluorooctanoic acid (PFOA)	15	J	19	7.4	2.6
375-95-1	Perfluorononanoic acid (PFNA)	19	U	22	19	7.4
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.1
375-85-9	Perfluoroheptanoic acid (PFHpA)	5.2	J	9.3	3.7	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	33	U	83	33	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	92		70-130
STL00996	13C2 PFDA	101		70-130

Wesley L. Selmer
02/05/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: NAWC-011118-RW-098 Lab Sample ID: 320-35046-8
 Matrix: Water Lab File ID: 2018.01.31_537A_028.d
 Analysis Method: 537 Date Collected: 01/11/2018 11:10
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 240.8(mL) Date Analyzed: 01/31/2018 12:44
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	J M	42	17	7.1
335-67-1	Perfluorooctanoic acid (PFOA)	14	J	21	8.3	2.9
375-95-1	Perfluorononanoic acid (PFNA)	21	U M	25	21	8.3
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	31	12	5.7
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.9	J M	10	4.2	2.0
375-73-5	Perfluorobutanesulfonic acid (PFBS)	37	U	93	37	17

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	91		70-130
STL00996	13C2 PFDA	102		70-130

Maria L. Selman
02/05/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: NAWC-011118-FRB-098 Lab Sample ID: 320-35046-9
 Matrix: Water Lab File ID: 2018.01.31_537A_031.d
 Analysis Method: 537 Date Collected: 01/11/2018 11:05
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 269.9(mL) Date Analyzed: 01/31/2018 12:58
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206410 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	37	15	6.3
335-67-1	Perfluorooctanoic acid (PFOA)	7.4	U	19	7.4	2.6
375-95-1	Perfluorononanoic acid (PFNA)	19	U	22	19	7.4
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.1
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.7	U	9.3	3.7	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	33	U	83	33	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	93		70-130
STL00996	13C2 PFDA	94		70-130

Ali L. Selman
02/05/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: NAWC-011118-RW-180 Lab Sample ID: 320-35046-10
 Matrix: Water Lab File ID: 2018.01.31_537A_032.d
 Analysis Method: 537 Date Collected: 01/11/2018 12:10
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 265.4 (mL) Date Analyzed: 01/31/2018 13:03
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206410 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	28	J M	38	15	6.4
335-67-1	Perfluorooctanoic acid (PFOA)	23		19	7.5	2.6
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.5
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	J	28	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	9.1	J	9.4	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	85	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	92		70-130
STL00996	13C2 PFDA	100		70-130

Wesley L. Selman
02/05/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: NAWC-011118-FRB-180 Lab Sample ID: 320-35046-11
 Matrix: Water Lab File ID: 2018.01.31_537A_033.d
 Analysis Method: 537 Date Collected: 01/11/2018 12:05
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 264.2 (mL) Date Analyzed: 01/31/2018 13:08
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206410 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	38	15	6.4
335-67-1	Perfluorooctanoic acid (PFOA)	7.6	U	19	7.6	2.6
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	U	9.5	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	85	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	99		70-130
STL00996	13C2 PFDA	100		70-130

Wesley L. Selman
02/05/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: NAWC-011118-RW-179 Lab Sample ID: 320-35046-12
 Matrix: Water Lab File ID: 2018.01.31_537A_034.d
 Analysis Method: 537 Date Collected: 01/11/2018 12:40
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 261.9(mL) Date Analyzed: 01/31/2018 13:12
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206410 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	18	J M	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	18	J	19	7.6	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	6.2	J	29	11	5.3
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.7	J	9.5	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	86	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	93		70-130
STL00996	13C2 PFDA	101		70-130

Steve L. Selman
02/05/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: NAWC-011118-FRB-179 Lab Sample ID: 320-35046-13
 Matrix: Water Lab File ID: 2018.01.31_537A_037.d
 Analysis Method: 537 Date Collected: 01/11/2018 12:35
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 261.5 (mL) Date Analyzed: 01/31/2018 13:26
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206410 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	7.6	U	19	7.6	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	29	11	5.3
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	U	9.6	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	86	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	95		70-130
STL00996	13C2 PFDA	95		70-130

Steve L. Selman
02/05/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: NAWC-011118-RW-303 Lab Sample ID: 320-35046-14
 Matrix: Water Lab File ID: 2018.01.31_537A_038.d
 Analysis Method: 537 Date Collected: 01/11/2018 13:10
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 260.8(mL) Date Analyzed: 01/31/2018 13:31
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206410 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	21	J M	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	20		19	7.7	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.7
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	7.3	J	29	12	5.3
375-85-9	Perfluoroheptanoic acid (PFHpA)	6.0	J	9.6	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	35	U	86	35	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	91		70-130
STL00996	13C2 PFDA	103		70-130

Wami L. Selman
02/05/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: NAWC-011118-FRB-303 Lab Sample ID: 320-35046-15
 Matrix: Water Lab File ID: 2018.01.31_537A_039.d
 Analysis Method: 537 Date Collected: 01/11/2018 13:05
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 262 (mL) Date Analyzed: 01/31/2018 13:36
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206410 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	7.6	U	19	7.6	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	29	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	U	9.5	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	86	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	92		70-130
STL00996	13C2 PFDA	102		70-130

Wesley L. Salzman
02/05/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: WGNA-011118-RW-3409 Lab Sample ID: 320-35046-16
 Matrix: Water Lab File ID: 2018.01.31_537A_040.d
 Analysis Method: 537 Date Collected: 01/11/2018 15:10
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 288 (mL) Date Analyzed: 01/31/2018 13:40
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206410 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	20	J M	35	14	5.9
335-67-1	Perfluorooctanoic acid (PFOA)	14	J	17	6.9	2.4
375-95-1	Perfluorononanoic acid (PFNA)	17	U	21	17	6.9
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	7.9	J	26	10	4.8
375-85-9	Perfluoroheptanoic acid (PFHpA)	5.1	J	8.7	3.5	1.6
375-73-5	Perfluorobutanesulfonic acid (PFBS)	31	U	78	31	14

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	91		70-130
STL00996	13C2 PFDA	100		70-130

Maria L. Salmeron
02/05/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: WGNA-011118-FRB-3409 Lab Sample ID: 320-35046-17
 Matrix: Water Lab File ID: 2018.01.31_537A_043.d
 Analysis Method: 537 Date Collected: 01/11/2018 15:05
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 261.5 (mL) Date Analyzed: 01/31/2018 13:54
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206412 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	7.6	U	19	7.6	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	29	11	5.3
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	U	9.6	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	86	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	99		70-130
STL00996	13C2 PFDA	101		70-130

Maria L. Salmeron
02/05/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: WGNA-011118-RW-3220 Lab Sample ID: 320-35046-18
 Matrix: Water Lab File ID: 2018.01.31_537A_044.d
 Analysis Method: 537 Date Collected: 01/11/2018 16:10
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 267.7(mL) Date Analyzed: 01/31/2018 13:59
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206412 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	38	M	37	15	6.4
335-67-1	Perfluorooctanoic acid (PFOA)	13	J	19	7.5	2.6
375-95-1	Perfluorononanoic acid (PFNA)	19	U	22	19	7.5
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	17	J	28	11	5.1
375-85-9	Perfluoroheptanoic acid (PFHpA)	8.0	J	9.3	3.7	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	110		84	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	85		70-130
STL00996	13C2 PFDA	97		70-130

Maria L. Salomon
02/05/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: WGNA-011118-FRB-3220 Lab Sample ID: 320-35046-19
 Matrix: Water Lab File ID: 2018.01.31_537A_045.d
 Analysis Method: 537 Date Collected: 01/11/2018 16:05
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 271.7(mL) Date Analyzed: 01/31/2018 14:04
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206412 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	37	15	6.3
335-67-1	Perfluorooctanoic acid (PFOA)	7.4	U	18	7.4	2.6
375-95-1	Perfluorononanoic acid (PFNA)	18	U	22	18	7.4
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.1
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.7	U	9.2	3.7	1.7
375-73-5	Perfluorobutanesulfonic acid (PFBS)	33	U	83	33	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	95		70-130
STL00996	13C2 PFDA	101		70-130

Mari L. Selman
02/05/2018

Appendix B

Results as Reported by the Laboratory

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: WGNA-011118-RW-3103 Lab Sample ID: 320-35046-1
 Matrix: Water Lab File ID: 2018.01.31_537A_021.d
 Analysis Method: 537 Date Collected: 01/11/2018 08:10
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 285.9(mL) Date Analyzed: 01/31/2018 12:12
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	10	J M	35	14	5.9
335-67-1	Perfluorooctanoic acid (PFOA)	12	J	17	7.0	2.4
375-95-1	Perfluorononanoic acid (PFNA)	17	U	21	17	7.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	5.2	J	26	10	4.8
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.4	J	8.7	3.5	1.7
375-73-5	Perfluorobutanesulfonic acid (PFBS)	31	U	79	31	14

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	92		70-130
STL00996	13C2 PFDA	97		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: WGNA-011118-FRB-3103 Lab Sample ID: 320-35046-2
 Matrix: Water Lab File ID: 2018.01.31_537A_022.d
 Analysis Method: 537 Date Collected: 01/11/2018 08:05
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 266(mL) Date Analyzed: 01/31/2018 12:16
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	38	15	6.4
335-67-1	Perfluorooctanoic acid (PFOA)	7.5	U	19	7.5	2.6
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.5
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	U	9.4	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	85	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	99		70-130
STL00996	13C2 PFDA	104		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: WGNA-011118-RW-0683 Lab Sample ID: 320-35046-3
 Matrix: Water Lab File ID: 2018.01.31_537A_023.d
 Analysis Method: 537 Date Collected: 01/11/2018 08:40
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 261(mL) Date Analyzed: 01/31/2018 12:21
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	29	J M	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	18	J	19	7.7	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.7
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	5.8	J	29	11	5.3
375-85-9	Perfluoroheptanoic acid (PFHpA)	5.2	J	9.6	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	86	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	87		70-130
STL00996	13C2 PFDA	96		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: WGNA-011118-FRB-0683 Lab Sample ID: 320-35046-4
 Matrix: Water Lab File ID: 2018.01.31_537A_024.d
 Analysis Method: 537 Date Collected: 01/11/2018 08:35
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 262.8(mL) Date Analyzed: 01/31/2018 12:26
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	7.6	U	19	7.6	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	29	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	U	9.5	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	86	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	96		70-130
STL00996	13C2 PFDA	99		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: NAWC-011118-RW-139 Lab Sample ID: 320-35046-5
 Matrix: Water Lab File ID: 2018.01.31_537A_025.d
 Analysis Method: 537 Date Collected: 01/11/2018 10:40
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 268.8(mL) Date Analyzed: 01/31/2018 12:30
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	12	J M	37	15	6.3
335-67-1	Perfluorooctanoic acid (PFOA)	16	J	19	7.4	2.6
375-95-1	Perfluorononanoic acid (PFNA)	19	U	22	19	7.4
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.1
375-85-9	Perfluoroheptanoic acid (PFHpA)	5.4	J	9.3	3.7	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	33	U	84	33	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	92		70-130
STL00996	13C2 PFDA	97		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: NAWC-011118-FRB-139 Lab Sample ID: 320-35046-6
 Matrix: Water Lab File ID: 2018.01.31_537A_026.d
 Analysis Method: 537 Date Collected: 01/11/2018 10:35
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 273.2 (mL) Date Analyzed: 01/31/2018 12:35
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	37	15	6.2
335-67-1	Perfluorooctanoic acid (PFOA)	7.3	U	18	7.3	2.6
375-95-1	Perfluorononanoic acid (PFNA)	18	U	22	18	7.3
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	27	11	5.0
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.7	U	9.2	3.7	1.7
375-73-5	Perfluorobutanesulfonic acid (PFBS)	33	U	82	33	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	90		70-130
STL00996	13C2 PFDA	96		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: WGNA-011118-DUP-18 Lab Sample ID: 320-35046-7
 Matrix: Water Lab File ID: 2018.01.31_537A_027.d
 Analysis Method: 537 Date Collected: 01/11/2018 07:00
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 270.1(mL) Date Analyzed: 01/31/2018 12:40
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	12	J M	37	15	6.3
335-67-1	Perfluorooctanoic acid (PFOA)	15	J	19	7.4	2.6
375-95-1	Perfluorononanoic acid (PFNA)	19	U	22	19	7.4
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.1
375-85-9	Perfluoroheptanoic acid (PFHpA)	5.2	J	9.3	3.7	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	33	U	83	33	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	92		70-130
STL00996	13C2 PFDA	101		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: NAWC-011118-RW-098 Lab Sample ID: 320-35046-8
 Matrix: Water Lab File ID: 2018.01.31_537A_028.d
 Analysis Method: 537 Date Collected: 01/11/2018 11:10
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 240.8(mL) Date Analyzed: 01/31/2018 12:44
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	J M	42	17	7.1
335-67-1	Perfluorooctanoic acid (PFOA)	14	J	21	8.3	2.9
375-95-1	Perfluorononanoic acid (PFNA)	21	U M	25	21	8.3
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	31	12	5.7
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.9	J M	10	4.2	2.0
375-73-5	Perfluorobutanesulfonic acid (PFBS)	37	U	93	37	17

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	91		70-130
STL00996	13C2 PFDA	102		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: NAWC-011118-FRB-098 Lab Sample ID: 320-35046-9
 Matrix: Water Lab File ID: 2018.01.31_537A_031.d
 Analysis Method: 537 Date Collected: 01/11/2018 11:05
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 269.9(mL) Date Analyzed: 01/31/2018 12:58
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206410 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	37	15	6.3
335-67-1	Perfluorooctanoic acid (PFOA)	7.4	U	19	7.4	2.6
375-95-1	Perfluorononanoic acid (PFNA)	19	U	22	19	7.4
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.1
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.7	U	9.3	3.7	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	33	U	83	33	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	93		70-130
STL00996	13C2 PFDA	94		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: NAWC-011118-RW-180 Lab Sample ID: 320-35046-10
 Matrix: Water Lab File ID: 2018.01.31_537A_032.d
 Analysis Method: 537 Date Collected: 01/11/2018 12:10
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 265.4 (mL) Date Analyzed: 01/31/2018 13:03
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206410 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	28	J M	38	15	6.4
335-67-1	Perfluorooctanoic acid (PFOA)	23		19	7.5	2.6
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.5
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	J	28	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	9.1	J	9.4	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	85	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	92		70-130
STL00996	13C2 PFDA	100		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: NAWC-011118-FRB-180 Lab Sample ID: 320-35046-11
 Matrix: Water Lab File ID: 2018.01.31_537A_033.d
 Analysis Method: 537 Date Collected: 01/11/2018 12:05
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 264.2 (mL) Date Analyzed: 01/31/2018 13:08
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206410 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	38	15	6.4
335-67-1	Perfluorooctanoic acid (PFOA)	7.6	U	19	7.6	2.6
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	U	9.5	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	85	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	99		70-130
STL00996	13C2 PFDA	100		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: NAWC-011118-RW-179 Lab Sample ID: 320-35046-12
 Matrix: Water Lab File ID: 2018.01.31_537A_034.d
 Analysis Method: 537 Date Collected: 01/11/2018 12:40
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 261.9(mL) Date Analyzed: 01/31/2018 13:12
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206410 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	18	J M	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	18	J	19	7.6	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	6.2	J	29	11	5.3
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.7	J	9.5	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	86	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	93		70-130
STL00996	13C2 PFDA	101		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: NAWC-011118-FRB-179 Lab Sample ID: 320-35046-13
 Matrix: Water Lab File ID: 2018.01.31_537A_037.d
 Analysis Method: 537 Date Collected: 01/11/2018 12:35
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 261.5 (mL) Date Analyzed: 01/31/2018 13:26
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206410 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	7.6	U	19	7.6	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	29	11	5.3
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	U	9.6	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	86	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	95		70-130
STL00996	13C2 PFDA	95		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: NAWC-011118-RW-303 Lab Sample ID: 320-35046-14
 Matrix: Water Lab File ID: 2018.01.31_537A_038.d
 Analysis Method: 537 Date Collected: 01/11/2018 13:10
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 260.8(mL) Date Analyzed: 01/31/2018 13:31
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206410 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	21	J M	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	20		19	7.7	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.7
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	7.3	J	29	12	5.3
375-85-9	Perfluoroheptanoic acid (PFHpA)	6.0	J	9.6	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	35	U	86	35	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	91		70-130
STL00996	13C2 PFDA	103		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: NAWC-011118-FRB-303 Lab Sample ID: 320-35046-15
 Matrix: Water Lab File ID: 2018.01.31_537A_039.d
 Analysis Method: 537 Date Collected: 01/11/2018 13:05
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 262 (mL) Date Analyzed: 01/31/2018 13:36
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206410 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	7.6	U	19	7.6	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	29	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	U	9.5	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	86	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	92		70-130
STL00996	13C2 PFDA	102		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: WGNA-011118-RW-3409 Lab Sample ID: 320-35046-16
 Matrix: Water Lab File ID: 2018.01.31_537A_040.d
 Analysis Method: 537 Date Collected: 01/11/2018 15:10
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 288 (mL) Date Analyzed: 01/31/2018 13:40
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206410 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	20	J M	35	14	5.9
335-67-1	Perfluorooctanoic acid (PFOA)	14	J	17	6.9	2.4
375-95-1	Perfluorononanoic acid (PFNA)	17	U	21	17	6.9
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	7.9	J	26	10	4.8
375-85-9	Perfluoroheptanoic acid (PFHpA)	5.1	J	8.7	3.5	1.6
375-73-5	Perfluorobutanesulfonic acid (PFBS)	31	U	78	31	14

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	91		70-130
STL00996	13C2 PFDA	100		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: WGNA-011118-FRB-3409 Lab Sample ID: 320-35046-17
 Matrix: Water Lab File ID: 2018.01.31_537A_043.d
 Analysis Method: 537 Date Collected: 01/11/2018 15:05
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 261.5 (mL) Date Analyzed: 01/31/2018 13:54
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206412 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	7.6	U	19	7.6	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	29	11	5.3
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	U	9.6	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	86	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	99		70-130
STL00996	13C2 PFDA	101		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: WGNA-011118-RW-3220 Lab Sample ID: 320-35046-18
 Matrix: Water Lab File ID: 2018.01.31_537A_044.d
 Analysis Method: 537 Date Collected: 01/11/2018 16:10
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 267.7(mL) Date Analyzed: 01/31/2018 13:59
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206412 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	38	M	37	15	6.4
335-67-1	Perfluorooctanoic acid (PFOA)	13	J	19	7.5	2.6
375-95-1	Perfluorononanoic acid (PFNA)	19	U	22	19	7.5
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	17	J	28	11	5.1
375-85-9	Perfluoroheptanoic acid (PFHpA)	8.0	J	9.3	3.7	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	110		84	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	85		70-130
STL00996	13C2 PFDA	97		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: WGNA-011118-FRB-3220 Lab Sample ID: 320-35046-19
 Matrix: Water Lab File ID: 2018.01.31_537A_045.d
 Analysis Method: 537 Date Collected: 01/11/2018 16:05
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 271.7(mL) Date Analyzed: 01/31/2018 14:04
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206412 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	37	15	6.3
335-67-1	Perfluorooctanoic acid (PFOA)	7.4	U	18	7.4	2.6
375-95-1	Perfluorononanoic acid (PFNA)	18	U	22	18	7.4
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.1
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.7	U	9.2	3.7	1.7
375-73-5	Perfluorobutanesulfonic acid (PFBS)	33	U	83	33	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	95		70-130
STL00996	13C2 PFDA	101		70-130

Appendix C

Support Documentation

ANALYTE	ORIGINAL	DUPLICATE	RL	RPD	RPD > 50%	ORIGINAL SAMPLE	DUPLICATE SAMPLE	DIFFERENCE >2XRL
	011118-RW-139	011118-DUP-18				CONC >5xRL	CONC >5xRL	
Perfluorooctanoic acid (PFOA)	16	15	19	6.45	FALSE	FALSE	FALSE	FALSE
Perfluoroheptanoic acid (PFHpA)	5.4	5.2	9.3	3.77	FALSE	FALSE	FALSE	FALSE
Perfluorooctanesulfonic acid (PFOS)	12	12	37	0	FALSE	FALSE	FALSE	FALSE

TestAmerica Sacramento
 880 Riverside Parkway
 West Sacramento, CA 95605-1500
 phone 916.373.5600 fax 303.467.7248

Chain of Custody Record

TestAmerica
 THE LEADER IN ENVIRONMENTAL TESTING
TestAmerica Laboratories, Inc.

Regulatory Program: DW NPDES RCRA Other:

Client Contact		Project Manager: Andy Frebowitz		Site Contact: Mary Kay Bond		Date: 1/11/2018		COC No.:			
TetraTech 234 Mall Boulevard Suite 260 King of Prussia, PA 19406 610-382-1174 610-491-9688 Project Name: WE04 Site: WE04 P O # 1132358 (through EarthToxics)		Tel/Fax: 610.382.1170		Lab Contact: Dave Alltucker		Carrier: FedEx		1 of 1 COCs			
		Analysis Turnaround Time		Filtered Sample (Y/N) Perform MS/MSD (Y/N) EPA 537 UCMR3				Sampler: Mary Kay Bond For Lab Use Only: Walk-in Client: <input type="checkbox"/> Lab Sampling: <input type="checkbox"/> Job / SDG No.:			
		<input type="checkbox"/> CALENDAR DAYS <input type="checkbox"/> WORKING DAYS TAT if different from Below 21 <input type="checkbox"/> 2 weeks <input type="checkbox"/> 1 week <input type="checkbox"/> 2 days <input type="checkbox"/> 1 day									
Sample Identification		Sample Date	Sample Time	Sample Type (C=Comp, G=Grab)	Matrix	# of Cont.			Sample Specific Notes:		
WGNA-011118-RW-3103		1/11/2018	06:10	G	DW	2	N	N	X		
WGNA-011118-FRB-3103		1/11/2018	08:05	G	DW	2	N	N	X		
WGNA-011118-RW-0683		1/11/2018	08:40	G	DW	2	N	N	X		
WGNA-011118-FRB-0683		1/11/2018	08:35	G	DW	2	N	N	X		
NAWC-011118-RW-139		1/11/2018	10:40	G	DW	2	N	N	X		
NAWC-011118-FRB-139		1/11/2018	10:35	G	DW	2	N	N	X		
WGNA-011118-DUP-18		1/11/2018	07:00	G	DW	2	N	N	X		
NAWC-011118-RW-098		1/11/2018	11:10	G	DW	2	N	N	X		
NAWC-011118-FRB-098		1/11/2018	11:05	G	DW	2	N	N	X		
NAWC-011118-RW-180		1/11/2018	12:10	G	DW	2	N	N	X		
NAWC-011118-FRB-180		1/11/2018	12:05	G	DW	2	N	N	X		
NAWC-011118-RW-179		1/11/2018	12:40	G	DW	6	N	Y	X		
NAWC-011118-FRB-179		1/11/2018	12:35	G	DW	2	N	N	X		
NAWC-011118-RW-303		1/11/2018	13:10	G	DW	2	N	N	X		
NAWC-011118-FRB-303		1/11/2018	13:05	G	DW	2	N	N	X		
WGNA-011118-RW-3409		1/11/2018	15:10	G	DW	2	N	N	X		
WGNA-011118-FRB-3409		1/11/2018	15:05	G	DW	2	N	N	X		
WGNA-011118-RW-3220		1/11/2018	16:10	G	DW	2	N	N	X		
WGNA-011118-FRB-3220		1/11/2018	16:05	G	DW	2	N	N	X		
Preservation Used: 1= Ice, 2= HCl; 3= H2SO4; 4=HNO3; 5=NaOH; 6= Other: Trizma							6				
Possible Hazard Identification: Are any samples from a listed EPA Hazardous Waste? Please List any EPA Waste Codes for the sample in the							Sample Disposal (A fee may be assessed if samples are retained longer than 1 month)				
<input checked="" type="checkbox"/> Non-Hazard <input type="checkbox"/> Flammable <input type="checkbox"/> Skin Irritant <input type="checkbox"/> Poison B <input type="checkbox"/> Unknown							<input type="checkbox"/> Return to Client <input checked="" type="checkbox"/> Disposal by Lab <input type="checkbox"/> Archive for _____ Months				
Fed Ex Tracking: 7711 9926 0435							3-7 5.1				
Custody Seals Intact: <input type="checkbox"/> Yes <input type="checkbox"/> No		Custody Seal No.:		Cooler Temp. (°C): Obs'd:		Therm ID No.:		AK2			
Relinquished by: <i>Mary Kay Bond</i>		Company: Tetra Tech		Date/Time: 1/11/2018 18:00		Received by: <i>[Signature]</i>		Company: <i>TH-Sac</i> Date/Time: <i>1/11/2018 13:20</i>			
Relinquished by:		Company:		Date/Time:		Received by:		Company:			
Relinquished by:		Company:		Date/Time:		Received in Laboratory by:					

Page 390 of 391



320-35046 Chain of Custody

3/2017

Job Narrative
320-35046-1

Receipt

The samples were received on 1/12/2018 1:20 PM; the samples arrived in good condition, properly preserved and, where required, on ice. The temperatures of the 2 coolers at receipt time were 3.7° C and 5.1° C.

LCMS

Method(s) 537: The first level standard from the initial calibration curve is used to evaluate the tune criteria. The instrument mass windows are set at +/- 0.5amu; therefore, detection of the analyte serves as verification that the assigned mass is within +/- 0.5amu of the true value, which meets the DoD/DOE QSM tune criterion.

No additional analytical or quality issues were noted, other than those described above or in the Definitions/Glossary page.

Organic Prep

No analytical or quality issues were noted, other than those described in the Definitions/Glossary page.

Definitions/Glossary

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-35046-1

Qualifiers

LCMS

Qualifier	Qualifier Description
U	Undetected at the Limit of Detection.
J	Estimated: The analyte was positively identified; the quantitation is an estimation
M	Manual integrated compound.

Glossary

Abbreviation	These commonly used abbreviations may or may not be present in this report.
α	Listed under the "D" column to designate that the result is reported on a dry weight basis
%R	Percent Recovery
CFL	Contains Free Liquid
CNF	Contains No Free Liquid
DER	Duplicate Error Ratio (normalized absolute difference)
Dil Fac	Dilution Factor
DL	Detection Limit (DoD/DOE)
DL, RA, RE, IN	Indicates a Dilution, Re-analysis, Re-extraction, or additional Initial metals/anion analysis of the sample
DLC	Decision Level Concentration (Radiochemistry)
EDL	Estimated Detection Limit (Dioxin)
LOD	Limit of Detection (DoD/DOE)
LOQ	Limit of Quantitation (DoD/DOE)
MDA	Minimum Detectable Activity (Radiochemistry)
MDC	Minimum Detectable Concentration (Radiochemistry)
MDL	Method Detection Limit
ML	Minimum Level (Dioxin)
NC	Not Calculated
ND	Not Detected at the reporting limit (or MDL or EDL if shown)
PQL	Practical Quantitation Limit
QC	Quality Control
RER	Relative Error Ratio (Radiochemistry)
RL	Reporting Limit or Requested Limit (Radiochemistry)
RPD	Relative Percent Difference, a measure of the relative difference between two points
TEF	Toxicity Equivalent Factor (Dioxin)
TEQ	Toxicity Equivalent Quotient (Dioxin)

Sample Summary

Client: Tetra Tech, Inc.

TestAmerica Job ID: 320-35046-1

Project/Site: Warminster: PFAS, NAS JRB Willow Grove

Lab Sample ID	Client Sample ID	Matrix	Collected	Received
320-35046-1	WGNA-011118-RW-3103	Water	01/11/18 08:10	01/12/18 13:20
320-35046-2	WGNA-011118-FRB-3103	Water	01/11/18 08:05	01/12/18 13:20
320-35046-3	WGNA-011118-RW-0683	Water	01/11/18 08:40	01/12/18 13:20
320-35046-4	WGNA-011118-FRB-0683	Water	01/11/18 08:35	01/12/18 13:20
320-35046-5	NAWC-011118-RW-139	Water	01/11/18 10:40	01/12/18 13:20
320-35046-6	NAWC-011118-FRB-139	Water	01/11/18 10:35	01/12/18 13:20
320-35046-7	WGNA-011118-DUP-18	Water	01/11/18 07:00	01/12/18 13:20
320-35046-8	NAWC-011118-RW-098	Water	01/11/18 11:10	01/12/18 13:20
320-35046-9	NAWC-011118-FRB-098	Water	01/11/18 11:05	01/12/18 13:20
320-35046-10	NAWC-011118-RW-180	Water	01/11/18 12:10	01/12/18 13:20
320-35046-11	NAWC-011118-FRB-180	Water	01/11/18 12:05	01/12/18 13:20
320-35046-12	NAWC-011118-RW-179	Water	01/11/18 12:40	01/12/18 13:20
320-35046-13	NAWC-011118-FRB-179	Water	01/11/18 12:35	01/12/18 13:20
320-35046-14	NAWC-011118-RW-303	Water	01/11/18 13:10	01/12/18 13:20
320-35046-15	NAWC-011118-FRB-303	Water	01/11/18 13:05	01/12/18 13:20
320-35046-16	WGNA-011118-RW-3409	Water	01/11/18 15:10	01/12/18 13:20
320-35046-17	WGNA-011118-FRB-3409	Water	01/11/18 15:05	01/12/18 13:20
320-35046-18	WGNA-011118-RW-3220	Water	01/11/18 16:10	01/12/18 13:20
320-35046-19	WGNA-011118-FRB-3220	Water	01/11/18 16:05	01/12/18 13:20

Method Summary

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-35046-1

Method	Method Description	Protocol	Laboratory
537	Perfluorinated Alkyl Acids (LC/MS)	EPA	TAL SAC

Protocol References:

EPA = US Environmental Protection Agency

Laboratory References:

TAL SAC = TestAmerica Sacramento, 880 Riverside Parkway, West Sacramento, CA 95605, TEL (916)373-5600

FORM II
LCMS SURROGATE RECOVERY

Lab Name: TestAmerica Sacramento

Job No.: 320-35046-1

SDG No.: _____

Matrix: Water

Level: Low

GC Column (1): GeminiC18 3 ID: 3 (mm)

Client Sample ID	Lab Sample ID	PFHxA #	PFDA #
WGNA-011118-RW-310 3	320-35046-1	92	97
WGNA-011118-FRB-31 03	320-35046-2	99	104
WGNA-011118-RW-068 3	320-35046-3	87	96
WGNA-011118-FRB-06 83	320-35046-4	96	99
NAWC-011118-RW-139	320-35046-5	92	97
NAWC-011118-FRB-13 9	320-35046-6	90	96
WGNA-011118-DUP-18	320-35046-7	92	101
NAWC-011118-RW-098	320-35046-8	91	102
NAWC-011118-FRB-09 8	320-35046-9	93	94
NAWC-011118-RW-180	320-35046-10	92	100
NAWC-011118-FRB-18 0	320-35046-11	99	100
NAWC-011118-RW-179	320-35046-12	93	101
NAWC-011118-FRB-17 9	320-35046-13	95	95
NAWC-011118-RW-303	320-35046-14	91	103
NAWC-011118-FRB-30 3	320-35046-15	92	102
WGNA-011118-RW-340 9	320-35046-16	91	100
WGNA-011118-FRB-34 09	320-35046-17	99	101
WGNA-011118-RW-322 0	320-35046-18	85	97
WGNA-011118-FRB-32 20	320-35046-19	95	101
	MB 320-205489/1-A	95	101
	LLCS 320-205489/2-A	103	104
NAWC-011118-RW-179 LMS	320-35046-12 LMS	94	108
NAWC-011118-RW-179 LMSD	320-35046-12 LMSD	88	97

PFHxA = 13C2 PFHxA
PFDA = 13C2 PFDA

QC LIMITS
70-130
70-130

Column to be used to flag recovery values

FORM III
LCMS LOW LEVEL CONTROL SAMPLE RECOVERY

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1

SDG No.: _____

Matrix: Water Level: Low Lab File ID: 2018.01.31_537A_020.d

Lab ID: LLCS 320-205489/2-A Client ID: _____

COMPOUND	SPIKE ADDED (ng/L)	LLCS CONCENTRATION (ng/L)	LLCS % REC	QC LIMITS REC	#
Perfluorooctanesulfonic acid (PFOS)	40.0	38.5 J	96	50-150	M
Perfluorooctanoic acid (PFOA)	20.0	20.1	100	50-150	
Perfluorononanoic acid (PFNA)	20.0	19.9 J	99	50-150	
Perfluorohexanesulfonic acid (PFHxS)	30.0	29.0 J	97	50-150	
Perfluoroheptanoic acid (PFHpA)	10.0	11.1	111	50-150	
Perfluorobutanesulfonic acid (PFBS)	90.0	91.7	102	50-150	

Column to be used to flag recovery and RPD values

FORM III
LCMS LOW LEVEL MATRIX SPIKE RECOVERY

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Matrix: Water Level: Low Lab File ID: 2018.01.31_537A_035.d
 Lab ID: 320-35046-12 LMS Client ID: NAWC-011118-RW-179 LMS

COMPOUND	SPIKE ADDED (ng/L)	SAMPLE CONCENTRATION (ng/L)	LMS CONCENTRATION (ng/L)	LMS % REC	QC LIMITS REC	#
Perfluorooctanesulfonic acid (PFOS)	39.2	18 J	54.3	94	50-150	M
Perfluorooctanoic acid (PFOA)	19.6	18 J	37.3	96	50-150	
Perfluorononanoic acid (PFNA)	19.6	19 U	21.2 J	109	50-150	
Perfluorohexanesulfonic acid (PFHxS)	29.4	6.2 J	34.9	98	50-150	
Perfluoroheptanoic acid (PFHpA)	9.79	4.7 J	14.9	104	50-150	
Perfluorobutanesulfonic acid (PFBS)	88.1	34 U	90.6	103	50-150	

Column to be used to flag recovery and RPD values

FORM III
LCMS LOW LEVEL MATRIX SPIKE DUPLICATE RECOVERY

Lab Name: TestAmerica Sacramento

Job No.: 320-35046-1

SDG No.: _____

Matrix: Water Level: Low

Lab File ID: 2018.01.31_537A_036.d

Lab ID: 320-35046-12 LMSD

Client ID: NAWC-011118-RW-179 LMSD

COMPOUND	SPIKE ADDED (ng/L)	LMSD CONCENTRATION (ng/L)	LMSD % REC	% RPD	QC LIMITS		#
					RPD	REC	
Perfluorooctanesulfonic acid (PFOS)	37.9	51.8	90	5	50	50-150	M
Perfluorooctanoic acid (PFOA)	19.0	35.1	88	6	50	50-150	
Perfluorononanoic acid (PFNA)	18.9	19.6 J	104	8	50	50-150	
Perfluorohexanesulfonic acid (PFHxS)	28.4	33.0	94	6	50	50-150	
Perfluoroheptanoic acid (PFHpA)	9.47	13.0	88	13	50	50-150	
Perfluorobutanesulfonic acid (PFBS)	85.3	84.3 J	99	7	50	50-150	

Column to be used to flag recovery and RPD values

FORM IV
LCMS METHOD BLANK SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-35046-1

SDG No.: _____

Lab File ID: 2018.01.31_537A_019.d

Lab Sample ID: MB 320-205489/1-A

Matrix: Water

Date Extracted: 01/24/2018 20:52

Instrument ID: A8_N

Date Analyzed: 01/31/2018 12:02

Level: (Low/Med) Low

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES:

CLIENT SAMPLE ID	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED
	LLCS 320-205489/2-A	2018.01.31_537A_020.d	01/31/2018 12:07
WGNA-011118-RW-3103	320-35046-1	2018.01.31_537A_021.d	01/31/2018 12:12
WGNA-011118-FRB-3103	320-35046-2	2018.01.31_537A_022.d	01/31/2018 12:16
WGNA-011118-RW-0683	320-35046-3	2018.01.31_537A_023.d	01/31/2018 12:21
WGNA-011118-FRB-0683	320-35046-4	2018.01.31_537A_024.d	01/31/2018 12:26
NAWC-011118-RW-139	320-35046-5	2018.01.31_537A_025.d	01/31/2018 12:30
NAWC-011118-FRB-139	320-35046-6	2018.01.31_537A_026.d	01/31/2018 12:35
WGNA-011118-DUP-18	320-35046-7	2018.01.31_537A_027.d	01/31/2018 12:40
NAWC-011118-RW-098	320-35046-8	2018.01.31_537A_028.d	01/31/2018 12:44
NAWC-011118-FRB-098	320-35046-9	2018.01.31_537A_031.d	01/31/2018 12:58
NAWC-011118-RW-180	320-35046-10	2018.01.31_537A_032.d	01/31/2018 13:03
NAWC-011118-FRB-180	320-35046-11	2018.01.31_537A_033.d	01/31/2018 13:08
NAWC-011118-RW-179	320-35046-12	2018.01.31_537A_034.d	01/31/2018 13:12
NAWC-011118-RW-179 LMS	320-35046-12 LMS	2018.01.31_537A_035.d	01/31/2018 13:17
NAWC-011118-RW-179 LMSD	320-35046-12 LMSD	2018.01.31_537A_036.d	01/31/2018 13:22
NAWC-011118-FRB-179	320-35046-13	2018.01.31_537A_037.d	01/31/2018 13:26
NAWC-011118-RW-303	320-35046-14	2018.01.31_537A_038.d	01/31/2018 13:31
NAWC-011118-FRB-303	320-35046-15	2018.01.31_537A_039.d	01/31/2018 13:36
WGNA-011118-RW-3409	320-35046-16	2018.01.31_537A_040.d	01/31/2018 13:40
WGNA-011118-FRB-3409	320-35046-17	2018.01.31_537A_043.d	01/31/2018 13:54
WGNA-011118-RW-3220	320-35046-18	2018.01.31_537A_044.d	01/31/2018 13:59
WGNA-011118-FRB-3220	320-35046-19	2018.01.31_537A_045.d	01/31/2018 14:04

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Client Sample ID: _____ Lab Sample ID: MB 320-205489/1-A
 Matrix: Water Lab File ID: 2018.01.31_537A_019.d
 Analysis Method: 537 Date Collected: _____
 Extraction Method: 537 Date Extracted: 01/24/2018 20:52
 Sample wt/vol: 250 (mL) Date Analyzed: 01/31/2018 12:02
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 206408 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	8.0	U	20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.0	U	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	95		70-130
STL00996	13C2 PFDA	101		70-130

FORM VIII
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Instrument ID: A8_N Calibration Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3(mm) Calibration End Date: 11/03/2017 14:01
 Calibration ID: 36012

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
INITIAL CALIBRATION MEAN AREA AND MEAN RT	1535518	1.91	3276559	2.15		
UPPER LIMIT	2303277	2.41	4914839	2.65		
LOWER LIMIT	767759	1.41	1638280	1.65		
LAB SAMPLE ID	CLIENT SAMPLE ID					
CCVL 320-192908/11	1586829	1.91	3305852	2.15		
ICV 320-192908/13	1512045	1.90	3433628	2.14		
CCVL 320-206407/1	1570514	1.84	3320314	2.09		
CCV 320-206408/14 CCVIS	1524185	1.82	3201796	2.07		
MB 320-205489/1-A	1514419	1.83	3315723	2.08		
LLCS 320-205489/2-A	1437381	1.83	3330580	2.08		
320-35046-1	WGNA-011118-RW-3103	1511383	1.81	3351158	2.07	
320-35046-2	WGNA-011118-FRB-3103	1469356	1.82	3274315	2.08	
320-35046-3	WGNA-011118-RW-0683	1551777	1.81	3339406	2.07	
320-35046-4	WGNA-011118-FRB-0683	1427812	1.82	3143756	2.08	
320-35046-5	NAWC-011118-RW-139	1551998	1.82	3530101	2.07	
320-35046-6	NAWC-011118-FRB-139	1503114	1.82	3436163	2.07	
320-35046-7	WGNA-011118-DUP-18	1522059	1.82	3381704	2.07	
320-35046-8	NAWC-011118-RW-098	1495096	1.82	3259129	2.07	
CCV 320-206408/26 CCVIS	1463849	1.81	3172960	2.07		
CCV 320-206410/26 CCVIS	1463849	1.81	3172960	2.07		
320-35046-9	NAWC-011118-FRB-098	1546187	1.82	3372040	2.07	
320-35046-10	NAWC-011118-RW-180	1537799	1.81	3430335	2.07	
320-35046-11	NAWC-011118-FRB-180	1532214	1.82	3442464	2.07	
320-35046-12	NAWC-011118-RW-179	1472481	1.82	3387330	2.07	
320-35046-12 LMS	NAWC-011118-RW-179 LMS	1527332	1.81	3460115	2.06	
320-35046-12 LMSD	NAWC-011118-RW-179 LMSD	1566820	1.81	3420572	2.07	
320-35046-13	NAWC-011118-FRB-179	1558738	1.82	3496002	2.07	
320-35046-14	NAWC-011118-RW-303	1470595	1.81	3380751	2.06	
320-35046-15	NAWC-011118-FRB-303	1560240	1.81	3459417	2.07	
320-35046-16	WGNA-011118-RW-3409	1548213	1.81	3403494	2.07	
CCV 320-206410/38 CCVIS	1511534	1.81	3175124	2.07		

13PFOA = 13C2-PFOA

PFOS = 13C4 PFOS

Area Limit = 50%-150% of internal standard area
 RT Limit = ± 0.5 minutes of internal standard RT

Column used to flag values outside QC limits

FORM VIII
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Instrument ID: A8_N Calibration Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3(mm) Calibration End Date: 11/03/2017 14:01
 Calibration ID: 36012

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
INITIAL CALIBRATION MEAN AREA AND MEAN RT	1535518	1.91	3276559	2.15		
UPPER LIMIT	2303277	2.41	4914839	2.65		
LOWER LIMIT	767759	1.41	1638280	1.65		
LAB SAMPLE ID	CLIENT SAMPLE ID					
CCV 320-206412/38 CCVIS		1511534	1.81	3175124	2.07	
320-35046-17	WGNA-011118-FRB-3409	1481492	1.82	3346629	2.07	
320-35046-18	WGNA-011118-RW-3220	1573796	1.81	3375758	2.06	
320-35046-19	WGNA-011118-FRB-3220	1520384	1.81	3387119	2.06	
CCV 320-206412/43 CCVIS		1503053	1.82	3253442	2.07	

13PFOA = 13C2-PFOA
 PFOS = 13C4 PFOS

Area Limit = 50%-150% of internal standard area
 RT Limit = ± 0.5 minutes of internal standard RT

Column used to flag values outside QC limits

FORM VIII
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Sample No.: CCV 320-206408/14 Date Analyzed: 01/31/2018 11:53
 Instrument ID: A8_N GC Column: GeminiC18 3x100 ID: 3 (mm)
 Lab File ID (Standard): 2018.01.31_537A_017 Heated Purge: (Y/N) N
 Calibration ID: 36012

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	1524185	1.82	3201796	2.07		
UPPER LIMIT	2133859	2.32	4482514	2.57		
LOWER LIMIT	1066930	1.32	2241257	1.57		
LAB SAMPLE ID	CLIENT SAMPLE ID					
MB 320-205489/1-A		1514419	1.83	3315723	2.08	
LLCS 320-205489/2-A		1437381	1.83	3330580	2.08	
320-35046-1	WGNA-011118-RW-3103	1511383	1.81	3351158	2.07	
320-35046-2	WGNA-011118-FRB-3103	1469356	1.82	3274315	2.08	
320-35046-3	WGNA-011118-RW-0683	1551777	1.81	3339406	2.07	
320-35046-4	WGNA-011118-FRB-0683	1427812	1.82	3143756	2.08	
320-35046-5	NAWC-011118-RW-139	1551998	1.82	3530101	2.07	
320-35046-6	NAWC-011118-FRB-139	1503114	1.82	3436163	2.07	
320-35046-7	WGNA-011118-DUP-18	1522059	1.82	3381704	2.07	
320-35046-8	NAWC-011118-RW-098	1495096	1.82	3259129	2.07	

13PFOA = 13C2-PFOA
 PFOS = 13C4 PFOS

Area Limit = 70%-140% of internal standard area
 RT Limit = ± 0.5 minutes of internal standard RT

Column used to flag values outside QC limits

FORM VIII
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Sample No.: CCV 320-206408/26 Date Analyzed: 01/31/2018 12:49
 Instrument ID: A8_N GC Column: GeminiC18 3x100 ID: 3 (mm)
 Lab File ID (Standard): 2018.01.31_537A_029 Heated Purge: (Y/N) N
 Calibration ID: 36012

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	1463849	1.81	3172960	2.07		
UPPER LIMIT	2049389	2.31	4442144	2.57		
LOWER LIMIT	1024694	1.31	2221072	1.57		
LAB SAMPLE ID	CLIENT SAMPLE ID					
MB 320-205489/1-A		1514419	1.83	3315723	2.08	
LLCS 320-205489/2-A		1437381	1.83	3330580	2.08	
320-35046-1	WGNA-011118-RW-3103	1511383	1.81	3351158	2.07	
320-35046-2	WGNA-011118-FRB-3103	1469356	1.82	3274315	2.08	
320-35046-3	WGNA-011118-RW-0683	1551777	1.81	3339406	2.07	
320-35046-4	WGNA-011118-FRB-0683	1427812	1.82	3143756	2.08	
320-35046-5	NAWC-011118-RW-139	1551998	1.82	3530101	2.07	
320-35046-6	NAWC-011118-FRB-139	1503114	1.82	3436163	2.07	
320-35046-7	WGNA-011118-DUP-18	1522059	1.82	3381704	2.07	
320-35046-8	NAWC-011118-RW-098	1495096	1.82	3259129	2.07	

13PFOA = 13C2-PFOA
 PFOS = 13C4 PFOS

Area Limit = 70%-140% of internal standard area
 RT Limit = ± 0.5 minutes of internal standard RT

Column used to flag values outside QC limits

FORM VIII
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Sample No.: CCV 320-206410/26 Date Analyzed: 01/31/2018 12:49
 Instrument ID: A8_N GC Column: GeminiC18 3x100 ID: 3 (mm)
 Lab File ID (Standard): 2018.01.31_537A_029 Heated Purge: (Y/N) N
 Calibration ID: 36012

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	1463849	1.81	3172960	2.07		
UPPER LIMIT	2049389	2.31	4442144	2.57		
LOWER LIMIT	1024694	1.31	2221072	1.57		
LAB SAMPLE ID	CLIENT SAMPLE ID					
320-35046-9	NAWC-011118-FRB-098	1546187	1.82	3372040	2.07	
320-35046-10	NAWC-011118-RW-180	1537799	1.81	3430335	2.07	
320-35046-11	NAWC-011118-FRB-180	1532214	1.82	3442464	2.07	
320-35046-12	NAWC-011118-RW-179	1472481	1.82	3387330	2.07	
320-35046-12 LMS	NAWC-011118-RW-179 LMS	1527332	1.81	3460115	2.06	
320-35046-12 LMSD	NAWC-011118-RW-179 LMSD	1566820	1.81	3420572	2.07	
320-35046-13	NAWC-011118-FRB-179	1558738	1.82	3496002	2.07	
320-35046-14	NAWC-011118-RW-303	1470595	1.81	3380751	2.06	
320-35046-15	NAWC-011118-FRB-303	1560240	1.81	3459417	2.07	
320-35046-16	WGNA-011118-RW-3409	1548213	1.81	3403494	2.07	

13PFOA = 13C2-PFOA
 PFOS = 13C4 PFOS

Area Limit = 70%-140% of internal standard area
 RT Limit = ± 0.5 minutes of internal standard RT

Column used to flag values outside QC limits

FORM VIII
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Sample No.: CCV 320-206410/38 Date Analyzed: 01/31/2018 13:45
 Instrument ID: A8_N GC Column: GeminiC18 3x100 ID: 3 (mm)
 Lab File ID (Standard): 2018.01.31_537A_041 Heated Purge: (Y/N) N
 Calibration ID: 36012

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	1511534	1.81	3175124	2.07		
UPPER LIMIT	2116148	2.31	4445174	2.57		
LOWER LIMIT	1058074	1.31	2222587	1.57		
LAB SAMPLE ID	CLIENT SAMPLE ID					
320-35046-9	NAWC-011118-FRB-098	1546187	1.82	3372040	2.07	
320-35046-10	NAWC-011118-RW-180	1537799	1.81	3430335	2.07	
320-35046-11	NAWC-011118-FRB-180	1532214	1.82	3442464	2.07	
320-35046-12	NAWC-011118-RW-179	1472481	1.82	3387330	2.07	
320-35046-12 LMS	NAWC-011118-RW-179 LMS	1527332	1.81	3460115	2.06	
320-35046-12 LMSD	NAWC-011118-RW-179 LMSD	1566820	1.81	3420572	2.07	
320-35046-13	NAWC-011118-FRB-179	1558738	1.82	3496002	2.07	
320-35046-14	NAWC-011118-RW-303	1470595	1.81	3380751	2.06	
320-35046-15	NAWC-011118-FRB-303	1560240	1.81	3459417	2.07	
320-35046-16	WGNA-011118-RW-3409	1548213	1.81	3403494	2.07	

13PFOA = 13C2-PFOA
 PFOS = 13C4 PFOS

Area Limit = 70%-140% of internal standard area
 RT Limit = ± 0.5 minutes of internal standard RT

Column used to flag values outside QC limits

FORM VIII
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Sample No.: CCV 320-206412/38 Date Analyzed: 01/31/2018 13:45
 Instrument ID: A8_N GC Column: GeminiC18 3x100 ID: 3 (mm)
 Lab File ID (Standard): 2018.01.31_537A_041 Heated Purge: (Y/N) N
 Calibration ID: 36012

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	1511534	1.81	3175124	2.07		
UPPER LIMIT	2116148	2.31	4445174	2.57		
LOWER LIMIT	1058074	1.31	2222587	1.57		
LAB SAMPLE ID	CLIENT SAMPLE ID					
320-35046-17	WGNA-011118-FRB-3409		1481492	1.82	3346629	2.07
320-35046-18	WGNA-011118-RW-3220		1573796	1.81	3375758	2.06
320-35046-19	WGNA-011118-FRB-3220		1520384	1.81	3387119	2.06

13PFOA = 13C2-PFOA
 PFOS = 13C4 PFOS

Area Limit = 70%-140% of internal standard area
 RT Limit = ± 0.5 minutes of internal standard RT

Column used to flag values outside QC limits

FORM VIII
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Sample No.: CCV 320-206412/43 Date Analyzed: 01/31/2018 14:08
 Instrument ID: A8_N GC Column: GeminiC18 3x100 ID: 3 (mm)
 Lab File ID (Standard): 2018.01.31_537A_046 Heated Purge: (Y/N) N
 Calibration ID: 36012

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	1503053	1.82	3253442	2.07		
UPPER LIMIT	2104274	2.32	4554819	2.57		
LOWER LIMIT	1052137	1.32	2277409	1.57		
LAB SAMPLE ID	CLIENT SAMPLE ID					
320-35046-17	WGNA-011118-FRB-3409	1481492	1.82	3346629	2.07	
320-35046-18	WGNA-011118-RW-3220	1573796	1.81	3375758	2.06	
320-35046-19	WGNA-011118-FRB-3220	1520384	1.81	3387119	2.06	

13PFOA = 13C2-PFOA
 PFOS = 13C4 PFOS

Area Limit = 70%-140% of internal standard area
 RT Limit = ± 0.5 minutes of internal standard RT

Column used to flag values outside QC limits

FORM VI
LCMS BY INTERNAL STANDARD - INITIAL CALIBRATION DATA
CURVE EVALUATION

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1 Analy Batch No.: 192908

SDG No.: _____

Instrument ID: A8_N GC Column: GeminiC18 3 ID: 3(mm) Heated Purge: (Y/N) N

Calibration Start Date: 11/03/2017 13:37 Calibration End Date: 11/03/2017 14:01 Calibration ID: 36012

Calibration Files:

LEVEL:	LAB SAMPLE ID:	LAB FILE ID:
Level 1	IC 320-192908/4	2017.11.03_537XICAL_004.d
Level 2	IC 320-192908/5	2017.11.03_537XICAL_005.d
Level 3	IC 320-192908/6	2017.11.03_537XICAL_006.d
Level 4	IC 320-192908/7	2017.11.03_537XICAL_007.d
Level 5	IC 320-192908/8	2017.11.03_537XICAL_008.d
Level 6	IC 320-192908/9	2017.11.03_537XICAL_009.d

ANALYTE	RRF					CURVE TYPE	COEFFICIENT			#	MIN RRF	%RSD	#	MAX %RSD	R ² OR COD	#	MIN R ² OR COD
	LVL 1 LVL 6	LVL 2	LVL 3	LVL 4	LVL 5		B	M1	M2								
Perfluorobutanesulfonic acid (PFBS)	1.0397 0.8468	1.0767	1.0898	0.9577	0.9303	QuaF		1.1193	-0.001498					0.9990			0.9600
Perfluoroheptanoic acid (PFHpA)	0.9433 0.9848	0.9187	0.9551	0.9185	0.9011	Ave		0.9369			3.2		30.0				
Perfluorohexanesulfonic acid (PFHxS)	1.6459 1.6841	1.6355	1.7405	1.6631	1.6755	Ave		1.6741			2.2		30.0				
Perfluorooctanoic acid (PFOA)	0.9757 0.9799	0.8919	0.9000	0.8953	0.9117	Ave		0.9258			4.4		30.0				
Perfluorooctanesulfonic acid (PFOS)	0.8958 0.9902	0.9213	0.9281	0.9268	0.9715	Ave		0.9389			3.7		30.0				
Perfluorononanoic acid (PFNA)	0.6610 0.7042	0.6285	0.6624	0.6810	0.6478	Ave		0.6642			3.9		30.0				
13C2 PFHxA	1.0891 1.1664	1.0526	1.1042	1.1123	1.0772	Ave		1.1003			3.5		30.0				
13C2 PFDA	0.7748 0.8159	0.7295	0.7569	0.7811	0.7330	Ave		0.7652			4.3		30.0				

Note: The M1 coefficient is the same as Ave RRF for an Ave curve type.

FORM VI
LCMS BY INTERNAL STANDARD - INITIAL CALIBRATION DATA
RESPONSE AND CONCENTRATION

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1 Analy Batch No.: 192908

SDG No.: _____

Instrument ID: A8_N GC Column: GeminiC18 3 ID: 3(mm) Heated Purge: (Y/N) N

Calibration Start Date: 11/03/2017 13:37 Calibration End Date: 11/03/2017 14:01 Calibration ID: 36012

Calibration Files:

LEVEL:	LAB SAMPLE ID:	LAB FILE ID:
Level 1	IC 320-192908/4	2017.11.03_537XICAL_004.d
Level 2	IC 320-192908/5	2017.11.03_537XICAL_005.d
Level 3	IC 320-192908/6	2017.11.03_537XICAL_006.d
Level 4	IC 320-192908/7	2017.11.03_537XICAL_007.d
Level 5	IC 320-192908/8	2017.11.03_537XICAL_008.d
Level 6	IC 320-192908/9	2017.11.03_537XICAL_009.d

ANALYTE	IS REF	CURVE TYPE	RESPONSE					CONCENTRATION (NG/ML)				
			LVL 1 LVL 6	LVL 2	LVL 3	LVL 4	LVL 5	LVL 1 LVL 6	LVL 2	LVL 3	LVL 4	LVL 5
Perfluorobutanesulfonic acid (PFBS)	PFOS	QuaF	1076553 16699152	2591121	5461974	10142530	14011858	9.00 180	20.0	45.0	90.0	135
Perfluoroheptanoic acid (PFHpA)	13PF OA	Ave	143455 2810797	331548	736034	1420703	2102676	1.00 20.0	2.22	5.00	10.0	15.0
Perfluorohexanesulfonic acid (PFHxS)	PFOS	Ave	568156 11071993	1312135	2908204	5871843	8413133	3.00 60.0	6.67	15.0	30.0	45.0
Perfluorooctanoic acid (PFOA)	13PF OA	Ave	296934 5597122	644149	1388033	2771271	4257225	2.00 40.0	4.45	10.0	20.0	30.0
Perfluorooctanesulfonic acid (PFOS)	PFOS	Ave	412315 8679676	985487	2067792	4363079	6504279	4.00 80.0	8.89	20.0	40.0	60.0
Perfluorononanoic acid (PFNA)	13PF OA	Ave	201053 4019666	453612	1020851	2106479	3023088	2.00 40.0	4.45	10.0	20.0	30.0
13C2 PFHxA	13PF OA	Ave	1655691 1664260	1708988	1701491	1719911	1675220	10.0 10.0	10.0	10.0	10.0	10.0
13C2 PFDA	13PF OA	Ave	1177922 1164156	1184358	1166275	1207887	1139992	10.0 10.0	10.0	10.0	10.0	10.0

Curve Type Legend:

Ave = Average ISTD
QuaF = Quadratic ISTD forced zero

FORM VI
 LCMS BY INTERNAL STANDARD - INITIAL CALIBRATION DATA
 READBACK PERCENT ERROR

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1 Analy Batch No.: 192908

SDG No.: _____


Instrument ID: A8_N GC Column: GeminiC18 3 ID: 3 (mm) Heated Purge: (Y/N) N


Calibration Start Date: 11/03/2017 13:37 Calibration End Date: 11/03/2017 14:01 Calibration ID: 36012

Calibration Files:

LEVEL:	LAB SAMPLE ID:	LAB FILE ID:
Level 1	IC 320-192908/4	2017.11.03_537XICAL_004.d
Level 2	IC 320-192908/5	2017.11.03_537XICAL_005.d
Level 3	IC 320-192908/6	2017.11.03_537XICAL_006.d
Level 4	IC 320-192908/7	2017.11.03_537XICAL_007.d
Level 5	IC 320-192908/8	2017.11.03_537XICAL_008.d
Level 6	IC 320-192908/9	2017.11.03_537XICAL_009.d

ANALYTE	PERCENT ERROR						PERCENT ERROR LIMIT					
	LVL 1 #	LVL 2 #	LVL 3 #	LVL 4 #	LVL 5 #	LVL 6 #	LVL 1	LVL 2	LVL 3	LVL 4	LVL 5	LVL 6
Perfluorobutanesulfonic acid (PFBS)	-6.0	-1.2	3.9	-3.1	1.9	-0.5	50	30	30	30	30	30
Perfluoroheptanoic acid (PFHpA)	0.7	-1.9	1.9	-2.0	-3.8	5.1	50	30	30	30	30	30
Perfluorohexanesulfonic acid (PFHxS)	-1.7	-2.3	4.0	-0.7	0.1	0.6	50	30	30	30	30	30
Perfluorooctanoic acid (PFOA)	5.4	-3.7	-2.8	-3.3	-1.5	5.8	50	30	30	30	30	30
Perfluorooctanesulfonic acid (PFOS)	-4.6	-1.9	-1.2	-1.3	3.5	5.5	50	30	30	30	30	30
Perfluorononanoic acid (PFNA)	-0.5	-5.4	-0.3	2.5	-2.5	6.0	50	30	30	30	30	30
13C2 PFHxA	-1.0	-4.3	0.4	1.1	-2.1	6.0	30	30	30	30	30	30
13C2 PFDA	1.3	-4.7	-1.1	2.1	-4.2	6.6	30	30	30	30	30	30





FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Lab Sample ID: CCVL 320-192908/11 Calibration Date: 11/03/2017 14:10
 Instrument ID: A8_N Calib Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 11/03/2017 14:01
 Lab File ID: 2017.11.03_537XICAL_011.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		1.109		20.4	20.0	1.9	50.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9369	0.9382		2.23	2.22	0.1	50.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.674	1.688		6.72	6.67	0.8	50.0
Perfluorooctanoic acid (PFOA)	Ave	0.9258	0.8825		4.24	4.45	-4.7	50.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9389	0.9176		8.69	8.89	-2.3	50.0
Perfluorononanoic acid (PFNA)	Ave	0.6642	0.6625		4.43	4.45	-0.2	50.0
13C2 PFHxA	Ave	1.100	1.068		9.70	10.0	-3.0	30.0
13C2 PFDA	Ave	0.7652	0.7460		9.75	10.0	-2.5	30.0

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Lab Sample ID: ICV 320-192908/13 Calibration Date: 11/03/2017 14:20
 Instrument ID: A8_N Calib Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 11/03/2017 14:01
 Lab File ID: 2017.11.03_537XICAL_013.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		0.8310		83.7	100	-16.4	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9369	0.8136		8.68	10.0	-13.2	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.674	1.463		17.5	20.1	-12.6	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9258	0.7995		17.7	20.5	-13.6	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9389	0.8637		18.1	19.7	-8.0	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6642	0.6428		19.5	20.1	-3.2	30.0
13C2 PFHxA	Ave	1.100	1.039		9.44	10.0	-5.6	30.0
13C2 PFDA	Ave	0.7652	0.7391		9.66	10.0	-3.4	30.0

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Lab Sample ID: CCVL 320-206407/1 Calibration Date: 01/31/2018 10:52
 Instrument ID: A8_N Calib Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 11/03/2017 14:01
 Lab File ID: 2018.01.31_537A_004.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		1.094		20.1	20.0	0.4	50.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9369	0.9074		2.15	2.22	-3.2	50.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.674	1.681		6.69	6.67	0.4	50.0
Perfluorooctanoic acid (PFOA)	Ave	0.9258	0.8944		4.30	4.45	-3.4	50.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9389	0.9026		8.55	8.89	-3.9	50.0
Perfluorononanoic acid (PFNA)	Ave	0.6642	0.6340		4.24	4.45	-4.5	50.0
13C2 PFHxA	Ave	1.100	1.073		9.75	10.0	-2.5	30.0
13C2 PFDA	Ave	0.7652	0.7889		10.3	10.0	3.1	30.0

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Lab Sample ID: CCV 320-206408/14 Calibration Date: 01/31/2018 11:53
 Instrument ID: A8_N Calib Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 11/03/2017 14:01
 Lab File ID: 2018.01.31_537A_017.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		1.062		45.5	45.0	1.0	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9369	0.9327		4.98	5.00	-0.5	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.674	1.745		15.6	15.0	4.3	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9258	0.8632		9.33	10.0	-6.8	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9389	0.9124		19.4	20.0	-2.8	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6642	0.6303		9.49	10.0	-5.1	30.0
13C2 PFHxA	Ave	1.100	1.097		9.97	10.0	-0.3	30.0
13C2 PFDA	Ave	0.7652	0.7539		9.85	10.0	-1.5	30.0

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Lab Sample ID: CCV 320-206408/26 Calibration Date: 01/31/2018 12:49
 Instrument ID: A8_N Calib Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 11/03/2017 14:01
 Lab File ID: 2018.01.31_537A_029.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		0.9466		141	135	4.2	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9369	0.9398		15.1	15.0	0.3	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.674	1.737		46.7	45.0	3.7	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9258	0.9631		31.2	30.0	4.0	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9389	0.9508		60.8	60.0	1.3	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6642	0.6784		30.6	30.0	2.1	30.0
13C2 PFHxA	Ave	1.100	1.151		10.5	10.0	4.6	30.0
13C2 PFDA	Ave	0.7652	0.8128		10.6	10.0	6.2	30.0

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Lab Sample ID: CCV 320-206410/26 Calibration Date: 01/31/2018 12:49
 Instrument ID: A8_N Calib Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 11/03/2017 14:01
 Lab File ID: 2018.01.31_537A_029.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		0.9466		141	135	4.2	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9369	0.9398		15.1	15.0	0.3	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.674	1.737		46.7	45.0	3.7	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9258	0.9631		31.2	30.0	4.0	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9389	0.9508		60.8	60.0	1.3	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6642	0.6784		30.6	30.0	2.1	30.0
13C2 PFHxA	Ave	1.100	1.151		10.5	10.0	4.6	30.0
13C2 PFDA	Ave	0.7652	0.8128		10.6	10.0	6.2	30.0

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Lab Sample ID: CCV 320-206410/38 Calibration Date: 01/31/2018 13:45
 Instrument ID: A8_N Calib Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 11/03/2017 14:01
 Lab File ID: 2018.01.31_537A_041.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		1.069		45.8	45.0	1.8	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9369	0.8966		4.79	5.00	-4.3	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.674	1.768		15.8	15.0	5.6	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9258	0.8792		9.51	10.0	-5.0	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9389	0.9125		19.4	20.0	-2.8	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6642	0.6157		9.27	10.0	-7.3	30.0
13C2 PFHxA	Ave	1.100	1.101		10.0	10.0	0.1	30.0
13C2 PFDA	Ave	0.7652	0.7772		10.2	10.0	1.6	30.0

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Lab Sample ID: CCV 320-206412/38 Calibration Date: 01/31/2018 13:45
 Instrument ID: A8_N Calib Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 11/03/2017 14:01
 Lab File ID: 2018.01.31_537A_041.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		1.069		45.8	45.0	1.8	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9369	0.8966		4.79	5.00	-4.3	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.674	1.768		15.8	15.0	5.6	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9258	0.8792		9.51	10.0	-5.0	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9389	0.9125		19.4	20.0	-2.8	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6642	0.6157		9.27	10.0	-7.3	30.0
13C2 PFHxA	Ave	1.100	1.101		10.0	10.0	0.1	30.0
13C2 PFDA	Ave	0.7652	0.7772		10.2	10.0	1.6	30.0

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1
 SDG No.: _____
 Lab Sample ID: CCV 320-206412/43 Calibration Date: 01/31/2018 14:08
 Instrument ID: A8_N Calib Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 11/03/2017 14:01
 Lab File ID: 2018.01.31_537A_046.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		0.9232		136	135	0.9	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9369	0.9580		15.3	15.0	2.2	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.674	1.716		46.1	45.0	2.5	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9258	0.9180		29.8	30.0	-0.8	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9389	0.9527		60.9	60.0	1.5	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6642	0.6593		29.8	30.0	-0.7	30.0
13C2 PFHxA	Ave	1.100	1.095		9.96	10.0	-0.4	30.0
13C2 PFDA	Ave	0.7652	0.7685		10.0	10.0	0.4	30.0

LCMS ANALYSIS RUN LOG

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1

SDG No.: _____

Instrument ID: A8_N Start Date: 11/03/2017 13:37

Analysis Batch Number: 192908 End Date: 11/03/2017 14:24

LAB SAMPLE ID	CLIENT SAMPLE ID	DATE ANALYZED	DILUTION FACTOR	LAB FILE ID	COLUMN ID
IC 320-192908/4		11/03/2017 13:37	1	2017.11.03_537X ICAL 004.d	GeminiC18 3x100 3(mm)
IC 320-192908/5		11/03/2017 13:42	1	2017.11.03_537X ICAL 005.d	GeminiC18 3x100 3(mm)
IC 320-192908/6		11/03/2017 13:47	1	2017.11.03_537X ICAL 006.d	GeminiC18 3x100 3(mm)
IC 320-192908/7 ICISAV		11/03/2017 13:52	1	2017.11.03_537X ICAL 007.d	GeminiC18 3x100 3(mm)
IC 320-192908/8		11/03/2017 13:56	1	2017.11.03_537X ICAL 008.d	GeminiC18 3x100 3(mm)
IC 320-192908/9		11/03/2017 14:01	1	2017.11.03_537X ICAL 009.d	GeminiC18 3x100 3(mm)
ZZZZZ		11/03/2017 14:06	1		GeminiC18 3x100 3(mm)
CCVL 320-192908/11		11/03/2017 14:10	1	2017.11.03_537X ICAL 011.d	GeminiC18 3x100 3(mm)
ZZZZZ		11/03/2017 14:15	1		GeminiC18 3x100 3(mm)
ICV 320-192908/13		11/03/2017 14:20	1	2017.11.03_537X ICAL 013.d	GeminiC18 3x100 3(mm)
ZZZZZ		11/03/2017 14:24	1		GeminiC18 3x100 3(mm)

LCMS ANALYSIS RUN LOG

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1

SDG No.: _____

Instrument ID: A8_N Start Date: 01/31/2018 10:52

Analysis Batch Number: 206407 End Date: 01/31/2018 11:53

LAB SAMPLE ID	CLIENT SAMPLE ID	DATE ANALYZED	DILUTION FACTOR	LAB FILE ID	COLUMN ID
CCVL 320-206407/1		01/31/2018 10:52	1	2018.01.31_537A 004.d	GeminiC18 3x100 3(mm)
CCV 320-206407/2 CCVIS		01/31/2018 10:57	1		GeminiC18 3x100 3(mm)
ZZZZZ		01/31/2018 11:06	1		GeminiC18 3x100 3(mm)
ZZZZZ		01/31/2018 11:11	1		GeminiC18 3x100 3(mm)
ZZZZZ		01/31/2018 11:15	1		GeminiC18 3x100 3(mm)
ZZZZZ		01/31/2018 11:20	1		GeminiC18 3x100 3(mm)
ZZZZZ		01/31/2018 11:25	1		GeminiC18 3x100 3(mm)
ZZZZZ		01/31/2018 11:29	1		GeminiC18 3x100 3(mm)
ZZZZZ		01/31/2018 11:34	1		GeminiC18 3x100 3(mm)
ZZZZZ		01/31/2018 11:39	1		GeminiC18 3x100 3(mm)
ZZZZZ		01/31/2018 11:43	1		GeminiC18 3x100 3(mm)
ZZZZZ		01/31/2018 11:48	1		GeminiC18 3x100 3(mm)
CCV 320-206407/14 CCVIS		01/31/2018 11:53	1		GeminiC18 3x100 3(mm)

LCMS ANALYSIS RUN LOG

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1

SDG No.: _____

Instrument ID: A8_N Start Date: 01/31/2018 11:53

Analysis Batch Number: 206408 End Date: 01/31/2018 12:49

LAB SAMPLE ID	CLIENT SAMPLE ID	DATE ANALYZED	DILUTION FACTOR	LAB FILE ID	COLUMN ID
CCV 320-206408/14 CCVIS		01/31/2018 11:53	1	2018.01.31_537A 017.d	GeminiC18 3x100 3(mm)
MB 320-205489/1-A		01/31/2018 12:02	1	2018.01.31_537A 019.d	GeminiC18 3x100 3(mm)
LLCS 320-205489/2-A		01/31/2018 12:07	1	2018.01.31_537A 020.d	GeminiC18 3x100 3(mm)
320-35046-1		01/31/2018 12:12	1	2018.01.31_537A 021.d	GeminiC18 3x100 3(mm)
320-35046-2		01/31/2018 12:16	1	2018.01.31_537A 022.d	GeminiC18 3x100 3(mm)
320-35046-3		01/31/2018 12:21	1	2018.01.31_537A 023.d	GeminiC18 3x100 3(mm)
320-35046-4		01/31/2018 12:26	1	2018.01.31_537A 024.d	GeminiC18 3x100 3(mm)
320-35046-5		01/31/2018 12:30	1	2018.01.31_537A 025.d	GeminiC18 3x100 3(mm)
320-35046-6		01/31/2018 12:35	1	2018.01.31_537A 026.d	GeminiC18 3x100 3(mm)
320-35046-7		01/31/2018 12:40	1	2018.01.31_537A 027.d	GeminiC18 3x100 3(mm)
320-35046-8		01/31/2018 12:44	1	2018.01.31_537A 028.d	GeminiC18 3x100 3(mm)
CCV 320-206408/26 CCVIS		01/31/2018 12:49	1	2018.01.31_537A 029.d	GeminiC18 3x100 3(mm)

LCMS ANALYSIS RUN LOG

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1

SDG No.: _____

Instrument ID: A8_N Start Date: 01/31/2018 12:49

Analysis Batch Number: 206410 End Date: 01/31/2018 13:45

LAB SAMPLE ID	CLIENT SAMPLE ID	DATE ANALYZED	DILUTION FACTOR	LAB FILE ID	COLUMN ID
CCV 320-206410/26 CCVIS		01/31/2018 12:49	1	2018.01.31_537A 029.d	GeminiC18 3x100 3(mm)
320-35046-9		01/31/2018 12:58	1	2018.01.31_537A 031.d	GeminiC18 3x100 3(mm)
320-35046-10		01/31/2018 13:03	1	2018.01.31_537A 032.d	GeminiC18 3x100 3(mm)
320-35046-11		01/31/2018 13:08	1	2018.01.31_537A 033.d	GeminiC18 3x100 3(mm)
320-35046-12		01/31/2018 13:12	1	2018.01.31_537A 034.d	GeminiC18 3x100 3(mm)
320-35046-12 LMS		01/31/2018 13:17	1	2018.01.31_537A 035.d	GeminiC18 3x100 3(mm)
320-35046-12 LMSD		01/31/2018 13:22	1	2018.01.31_537A 036.d	GeminiC18 3x100 3(mm)
320-35046-13		01/31/2018 13:26	1	2018.01.31_537A 037.d	GeminiC18 3x100 3(mm)
320-35046-14		01/31/2018 13:31	1	2018.01.31_537A 038.d	GeminiC18 3x100 3(mm)
320-35046-15		01/31/2018 13:36	1	2018.01.31_537A 039.d	GeminiC18 3x100 3(mm)
320-35046-16		01/31/2018 13:40	1	2018.01.31_537A 040.d	GeminiC18 3x100 3(mm)
CCV 320-206410/38 CCVIS		01/31/2018 13:45	1	2018.01.31_537A 041.d	GeminiC18 3x100 3(mm)

LCMS ANALYSIS RUN LOG

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1

SDG No.: _____

Instrument ID: A8_N Start Date: 01/31/2018 13:45

Analysis Batch Number: 206412 End Date: 01/31/2018 14:08

LAB SAMPLE ID	CLIENT SAMPLE ID	DATE ANALYZED	DILUTION FACTOR	LAB FILE ID	COLUMN ID
CCV 320-206412/38 CCVIS		01/31/2018 13:45	1	2018.01.31_537A 041.d	GeminiC18 3x100 3(mm)
320-35046-17		01/31/2018 13:54	1	2018.01.31_537A 043.d	GeminiC18 3x100 3(mm)
320-35046-18		01/31/2018 13:59	1	2018.01.31_537A 044.d	GeminiC18 3x100 3(mm)
320-35046-19		01/31/2018 14:04	1	2018.01.31_537A 045.d	GeminiC18 3x100 3(mm)
CCV 320-206412/43 CCVIS		01/31/2018 14:08	1	2018.01.31_537A 046.d	GeminiC18 3x100 3(mm)

LCMS BATCH WORKSHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1

SDG No.: _____

Batch Number: 205489 Batch Start Date: 01/25/18 14:25 Batch Analyst: Long, Tyrel W

Batch Method: 537 Batch End Date: 01/25/18 22:10

Lab Sample ID	Client Sample ID	Method Chain	Basis	GrossWeight	TareWeight	InitialAmount	FinalAmount	ReceivedpH	LC537-IS 00055
MB 320-205489/1		537, 537				250 mL	1.00 mL	7 SU	100 uL
LLCS 320-205489/2		537, 537				250 mL	1.00 mL	7 SU	100 uL
320-35046-A-1	WGNA-011118-RW-3 103	537, 537	T	314.59 g	28.73 g	285.9 mL	1.00 mL	7 SU	100 uL
320-35046-A-2	WGNA-011118-FRB- 3103	537, 537	T	292.93 g	26.95 g	266 mL	1.00 mL	7 SU	100 uL
320-35046-A-3	WGNA-011118-RW-0 683	537, 537	T	289.57 g	28.60 g	261 mL	1.00 mL	7 SU	100 uL
320-35046-A-4	WGNA-011118-FRB- 0683	537, 537	T	289.77 g	26.99 g	262.8 mL	1.00 mL	7 SU	100 uL
320-35046-A-5	NAWC-011118-RW-1 39	537, 537	T	297.46 g	28.67 g	268.8 mL	1.00 mL	7 SU	100 uL
320-35046-A-6	NAWC-011118-FRB- 139	537, 537	T	300.19 g	27.02 g	273.2 mL	1.00 mL	7 SU	100 uL
320-35046-A-7	WGNA-011118-DUP- 18	537, 537	T	298.89 g	28.75 g	270.1 mL	1.00 mL	7 SU	100 uL
320-35046-A-8	NAWC-011118-RW-0 98	537, 537	T	269.36 g	28.60 g	240.8 mL	1.00 mL	7 SU	100 uL
320-35046-A-9	NAWC-011118-FRB- 098	537, 537	T	296.99 g	27.08 g	269.9 mL	1.00 mL	7 SU	100 uL
320-35046-A-10	NAWC-011118-RW-1 80	537, 537	T	293.90 g	28.52 g	265.4 mL	1.00 mL	7 SU	100 uL
320-35046-A-11	NAWC-011118-FRB- 180	537, 537	T	291.23 g	27.05 g	264.2 mL	1.00 mL	7 SU	100 uL
320-35046-A-12	NAWC-011118-RW-1 79	537, 537	T	290.54 g	28.61 g	261.9 mL	1.00 mL	7 SU	100 uL
320-35046-A-12	NAWC-011118-RW-1 79	537, 537	T	283.43 g	27.99 g	255.4 mL	1.00 mL	7 SU	100 uL
LMS 320-35046-A-12	NAWC-011118-RW-1 79	537, 537	T	292.51 g	28.63 g	263.9 mL	1.00 mL	7 SU	100 uL
LMSD 320-35046-A-13	NAWC-011118-FRB- 179	537, 537	T	288.76 g	27.27 g	261.5 mL	1.00 mL	7 SU	100 uL
320-35046-A-14	NAWC-011118-RW-3 03	537, 537	T	289.16 g	28.40 g	260.8 mL	1.00 mL	7 SU	100 uL
320-35046-A-15	NAWC-011118-FRB- 303	537, 537	T	289.19 g	27.24 g	262 mL	1.00 mL	7 SU	100 uL
320-35046-A-16	WGNA-011118-RW-3 409	537, 537	T	315.88 g	27.90 g	288 mL	1.00 mL	7 SU	100 uL
320-35046-A-17	WGNA-011118-FRB- 3409	537, 537	T	288.88 g	27.37 g	261.5 mL	1.00 mL	7 SU	100 uL
320-35046-A-18	WGNA-011118-RW-3 220	537, 537	T	296.30 g	28.63 g	267.7 mL	1.00 mL	7 SU	100 uL

The pound sign (#) in the amount added field denotes that the reagent was used undiluted. All calculations are performed using the stated concentration for this reagent.

LCMS BATCH WORKSHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1

SDG No.: _____

Batch Number: 205489 Batch Start Date: 01/25/18 14:25 Batch Analyst: Long, Tyrel W

Batch Method: 537 Batch End Date: 01/25/18 22:10

Lab Sample ID	Client Sample ID	Method Chain	Basis	GrossWeight	TareWeight	InitialAmount	FinalAmount	ReceivedpH	LC537-IS 00055
320-35046-A-19	WGNA-011118-FRB-3220	537, 537	T	298.97 g	27.24 g	271.7 mL	1.00 mL	7 SU	100 uL

Lab Sample ID	Client Sample ID	Method Chain	Basis	LC537-LSP 00028	LC537-SU 00053	AnalysisComment			
MB 320-205489/1		537, 537			100 uL	Chlorine ND			
LLCS 320-205489/2		537, 537		100 uL	100 uL	Chlorine ND			
320-35046-A-1	WGNA-011118-RW-3103	537, 537	T		100 uL	Chlorine ND			
320-35046-A-2	WGNA-011118-FRB-3103	537, 537	T		100 uL	Chlorine ND			
320-35046-A-3	WGNA-011118-RW-0683	537, 537	T		100 uL	Chlorine ND			
320-35046-A-4	WGNA-011118-FRB-0683	537, 537	T		100 uL	Chlorine ND			
320-35046-A-5	NAWC-011118-RW-139	537, 537	T		100 uL	Chlorine ND			
320-35046-A-6	NAWC-011118-FRB-139	537, 537	T		100 uL	Chlorine ND			
320-35046-A-7	WGNA-011118-DUP-18	537, 537	T		100 uL	Chlorine ND			
320-35046-A-8	NAWC-011118-RW-098	537, 537	T		100 uL	Chlorine ND			
320-35046-A-9	NAWC-011118-FRB-098	537, 537	T		100 uL	Chlorine ND			
320-35046-A-10	NAWC-011118-RW-180	537, 537	T		100 uL	Chlorine ND			
320-35046-A-11	NAWC-011118-FRB-180	537, 537	T		100 uL	Chlorine ND			
320-35046-A-12	NAWC-011118-RW-179	537, 537	T		100 uL	Chlorine ND			
320-35046-A-12 LMS	NAWC-011118-RW-179	537, 537	T	100 uL	100 uL	Chlorine ND			
320-35046-A-12 LMSD	NAWC-011118-RW-179	537, 537	T	100 uL	100 uL	Chlorine ND			
320-35046-A-13	NAWC-011118-FRB-179	537, 537	T		100 uL	Chlorine ND			
320-35046-A-14	NAWC-011118-RW-303	537, 537	T		100 uL	Chlorine ND			
320-35046-A-15	NAWC-011118-FRB-303	537, 537	T		100 uL	Chlorine ND			

The pound sign (#) in the amount added field denotes that the reagent was used undiluted. All calculations are performed using the stated concentration for this reagent.

LCMS BATCH WORKSHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35046-1

SDG No.: _____

Batch Number: 205489 Batch Start Date: 01/25/18 14:25 Batch Analyst: Long, Tyrel W

Batch Method: 537 Batch End Date: 01/25/18 22:10

Lab Sample ID	Client Sample ID	Method Chain	Basis	LC537-LSP 00028	LC537-SU 00053	AnalysisComment			
320-35046-A-16	WGNA-011118-RW-3409	537, 537	T		100 uL	Chlorine ND			
320-35046-A-17	WGNA-011118-FRB-3409	537, 537	T		100 uL	Chlorine ND			
320-35046-A-18	WGNA-011118-RW-3220	537, 537	T		100 uL	Chlorine ND			
320-35046-A-19	WGNA-011118-FRB-3220	537, 537	T		100 uL	Chlorine ND			

Batch Notes	
Analyst ID - Aliquot Step	TWL
Batch Comment	Label ID's checked: TWL 1/25/18
Analyst ID - Concentration	TWL
Analyst ID - Final Volume Step	TWL
Internal Standard ID#	1099355
Manifold ID	1
Methanol ID	1127847
pH Indicator ID	2517
Pipette ID	M16387D
Analyst ID - IS Reagent Drop	JER
Analyst ID - IS Reagent Drop Witness	TWL
Analyst ID - SU Reagent Drop	JER
Analyst ID - SU Reagent Drop Witness	TWL
Analyst ID - TA Reagent Drop	JER
Analyst ID - TA Reagent Drop Witness	TWL
SPE Cartridge ID	6369499-03
Trizma ID	SLBR4303V
Reagent Water ID	1-19-18

Basis	Basis Description
T	Total/NA

The pound sign (#) in the amount added field denotes that the reagent was used undiluted. All calculations are performed using the stated concentration for this reagent.

Aqueous Extraction Analysis Sheet

(To Accompany Samples to Instruments)

Batch Number: 320-205489

Analyst: Long, Tyrel W

Batch Open: 1/25/2018 2:25:00PM











Method Code: 320-537_Prep-320

Batch End: 1/25/2018 10:10:00PM

63

AS 1/31/18

Extraction of Perfluorinated Alkyl Acids

Input Sample Lab ID (Analytical Method)	SDG (Job #)	GrossWt TareWt	InitAmnt FinAmnt	Rcvd	PHs Adj1 Adj2	Due Date	Analytical TAT	Div Rank	Comments	Output Sample Lab ID
1 MB-320-205489/1 N/A	N/A		250 mL	7		N/A	N/A	N/A	Chlorine ND	
			1.00 mL							
2 LLCS-320-205489/2 N/A	N/A		250 mL	7		N/A	N/A	N/A	Chlorine ND	
			1.00 mL							
3 320-35046-A-1 (537_DOD5)	N/A (320-35046-1)	314.59 g	285.9 mL	7		1/16/18	16_Days	4	Chlorine ND	
		28.73 g	1.00 mL							
320-35046-A-2 (537_DOD5)	N/A (320-35046-1)	292.93 g	266 mL	7		1/16/18	16_Days	4	Chlorine ND	
		26.95 g	1.00 mL							
320-35046-A-3 (537_DOD5)	N/A (320-35046-1)	289.57 g	261 mL	7		1/16/18	16_Days	4	Chlorine ND	
		28.60 g	1.00 mL							
6 320-35046-A-4 (537_DOD5)	N/A (320-35046-1)	289.77 g	262.8 mL	7		1/16/18	16_Days	4	Chlorine ND	
		26.99 g	1.00 mL							
7 320-35046-A-5 (537_DOD5)	N/A (320-35046-1)	297.46 g	268.8 mL	7		1/16/18	16_Days	4	Chlorine ND	
		28.67 g	1.00 mL							
8 320-35046-A-6 (537_DOD5)	N/A (320-35046-1)	300.19 g	273.2 mL	7		1/16/18	16_Days	4	Chlorine ND	
		27.02 g	1.00 mL							
9 320-35046-A-7 (537_DOD5)	N/A (320-35046-1)	298.89 g	270.1 mL	7		1/16/18	16_Days	4	Chlorine ND	
		28.75 g	1.00 mL							
10 320-35046-A-8 (537_DOD5)	N/A (320-35046-1)	269.36 g	240.8 mL	7		1/16/18	16_Days	4	Chlorine ND	
		28.60 g	1.00 mL							

Page 382 of 391

Aqueous Extraction Analysis Sheet

(To Accompany Samples to Instruments)













Batch Number: 320-205489

Analyst: Long, Tyrel W

Batch Open: 1/25/2018 2:25:00PM

Method Code: 320-537_Prep-320

Batch End: 1/25/2018 10:10:00PM

11	320-35046-A-9 (537_DOD5)	N/A (320-35046-1)	296.99 g	269.9 mL	7		1/16/18	16_Days	4	Chlorine ND	
			27.08 g	1.00 mL							
12	320-35046-A-10 (537_DOD5)	N/A (320-35046-1)	293.90 g	265.4 mL	7		1/16/18	16_Days	4	Chlorine ND	
			28.52 g	1.00 mL							
13	320-35046-A-11 (537_DOD5)	N/A (320-35046-1)	291.23 g	264.2 mL	7		1/16/18	16_Days	4	Chlorine ND	
			27.05 g	1.00 mL							
14	320-35046-A-12 (537_DOD5)	N/A (320-35046-1)	290.54 g	261.9 mL	7		1/16/18	16_Days	4	Chlorine ND	
			28.61 g	1.00 mL							
15	320-35046-A-12-LMS (537_DOD5)	N/A (320-35046-1)	283.43 g	255.4 mL	7		1/16/18	16_Days	4	Chlorine ND	
			27.99 g	1.00 mL							
16	320-35046-A-12-LMSD (537_DOD5)	N/A (320-35046-1)	292.51 g	263.9 mL	7		1/16/18	16_Days	4	Chlorine ND	
			28.63 g	1.00 mL							
17	320-35046-A-13 (537_DOD5)	N/A (320-35046-1)	288.76 g	261.5 mL	7		1/16/18	16_Days	4	Chlorine ND	
			27.27 g	1.00 mL							
18	320-35046-A-14 (537_DOD5)	N/A (320-35046-1)	289.16 g	260.8 mL	7		1/16/18	16_Days	4	Chlorine ND	
			28.40 g	1.00 mL							
19	320-35046-A-15 (537_DOD5)	N/A (320-35046-1)	289.19 g	262 mL	7		1/16/18	16_Days	4	Chlorine ND	
			27.24 g	1.00 mL							
20	320-35046-A-16 (537_DOD5)	N/A (320-35046-1)	315.88 g	288 mL	7		1/16/18	16_Days	4	Chlorine ND	
			27.90 g	1.00 mL							
21	320-35046-A-17 (537_DOD5)	N/A (320-35046-1)	288.88 g	261.5 mL	7		1/16/18	16_Days	4	Chlorine ND	
			27.37 g	1.00 mL							
22	320-35046-A-18 (537_DOD5)	N/A (320-35046-1)	296.30 g	267.7 mL	7		1/16/18	16_Days	4	Chlorine ND	
			28.63 g	1.00 mL							

Page 383 of 391

Aqueous Extraction Analysis Sheet

(To Accompany Samples to Instruments)

Batch Number: 320-205489


Analyst: Long, Tyrel W

Batch Open: 1/25/2018 2:25:00PM

Method Code: 320-537_Prep-320

Batch End: 1/25/2018 10:10:00PM

23

320-35046-A-19 (537_DOD5)	N/A (320-35046-1)	298.97 g	271.7 mL	7			1/16/18	16_Days	4	Chlorine ND	
		27.24 g	1.00 mL								

Batch Notes

Manifold ID 1

pH Indicator ID 2517

Trizma ID **SLBR4303V**

SPE Cartridge ID 6369499-03

Methanol ID 1127847

Reagent Water ID 1-19-18

Internal Standard ID# 1099355

Pipette ID M16387D

Analyst ID - TA Reagent Drop JER

Analyst ID - TA Reagent Drop TWL

Witness

Analyst ID - SU Reagent Drop JER

Analyst ID - SU Reagent Drop TWL

Witness

Analyst ID - IS Reagent Drop JER

Analyst ID - IS Reagent Drop TWL

Witness

Analyst ID - Concentration TWL

Analyst ID - Aliquot Step TWL

Analyst ID - Final Volume Step TWL

Batch Comment Label ID's checked: TWL 1/25/18

Page 384 of 391

PFAS Calibration Calculations:

Initial Calibration 11/3/2017
 Instrument A8_N

PFOS

Analyte Concentration	Analyte Response	Internal Standard Response	Internal Standard Amount	RRF	Reported RRF
4	412315	3298877	28.7	0.89678	0.8958
8.89	985487	3450592	28.7	0.92201	0.9213
20	2067792	3194016	28.7	0.92901	0.9281
40	4363079	3374600	28.7	0.92767	0.9268
60	6504279	3199479	28.7	0.97241	0.9715
80	8679676	3141787	28.7	0.99110	0.9902
Average				0.93983	0.9389
Standard Deviation				0.0350	
RSD				0.0372	
%RSD				3.72448	3.7

Continuing Calibration 01/31/2018 @ 11:53
 Instrument A8_N

PFOS

Analyte Concentration	Analyte Response	Internal Standard Response	Internal Standard Amount	RRF	%D	Reported RRF	Reported %D
20	2037649	3201796	28.7	0.9132	-2.732382	0.9124	-2.8

Willow Grove
SDG 320-35046-1

Sample Identification

WGNA-011118-RW-3103

Compound

PFOS

Compound Area

327364

Internal Standard Amount (ng)

28.7

Dilution Factor

1

Internal Standard Area

3351158

Average RRF

0.9389

Sample Volume(L)

0.2859

Volume Extract (ml)

1


Injection Volume (µl)

1

Concentration

10.4444 ug/L

C:\AI\Projects\112008005\WE04\F.S.DR.03\NAWC_201901.mxd MKB 1/24/2019

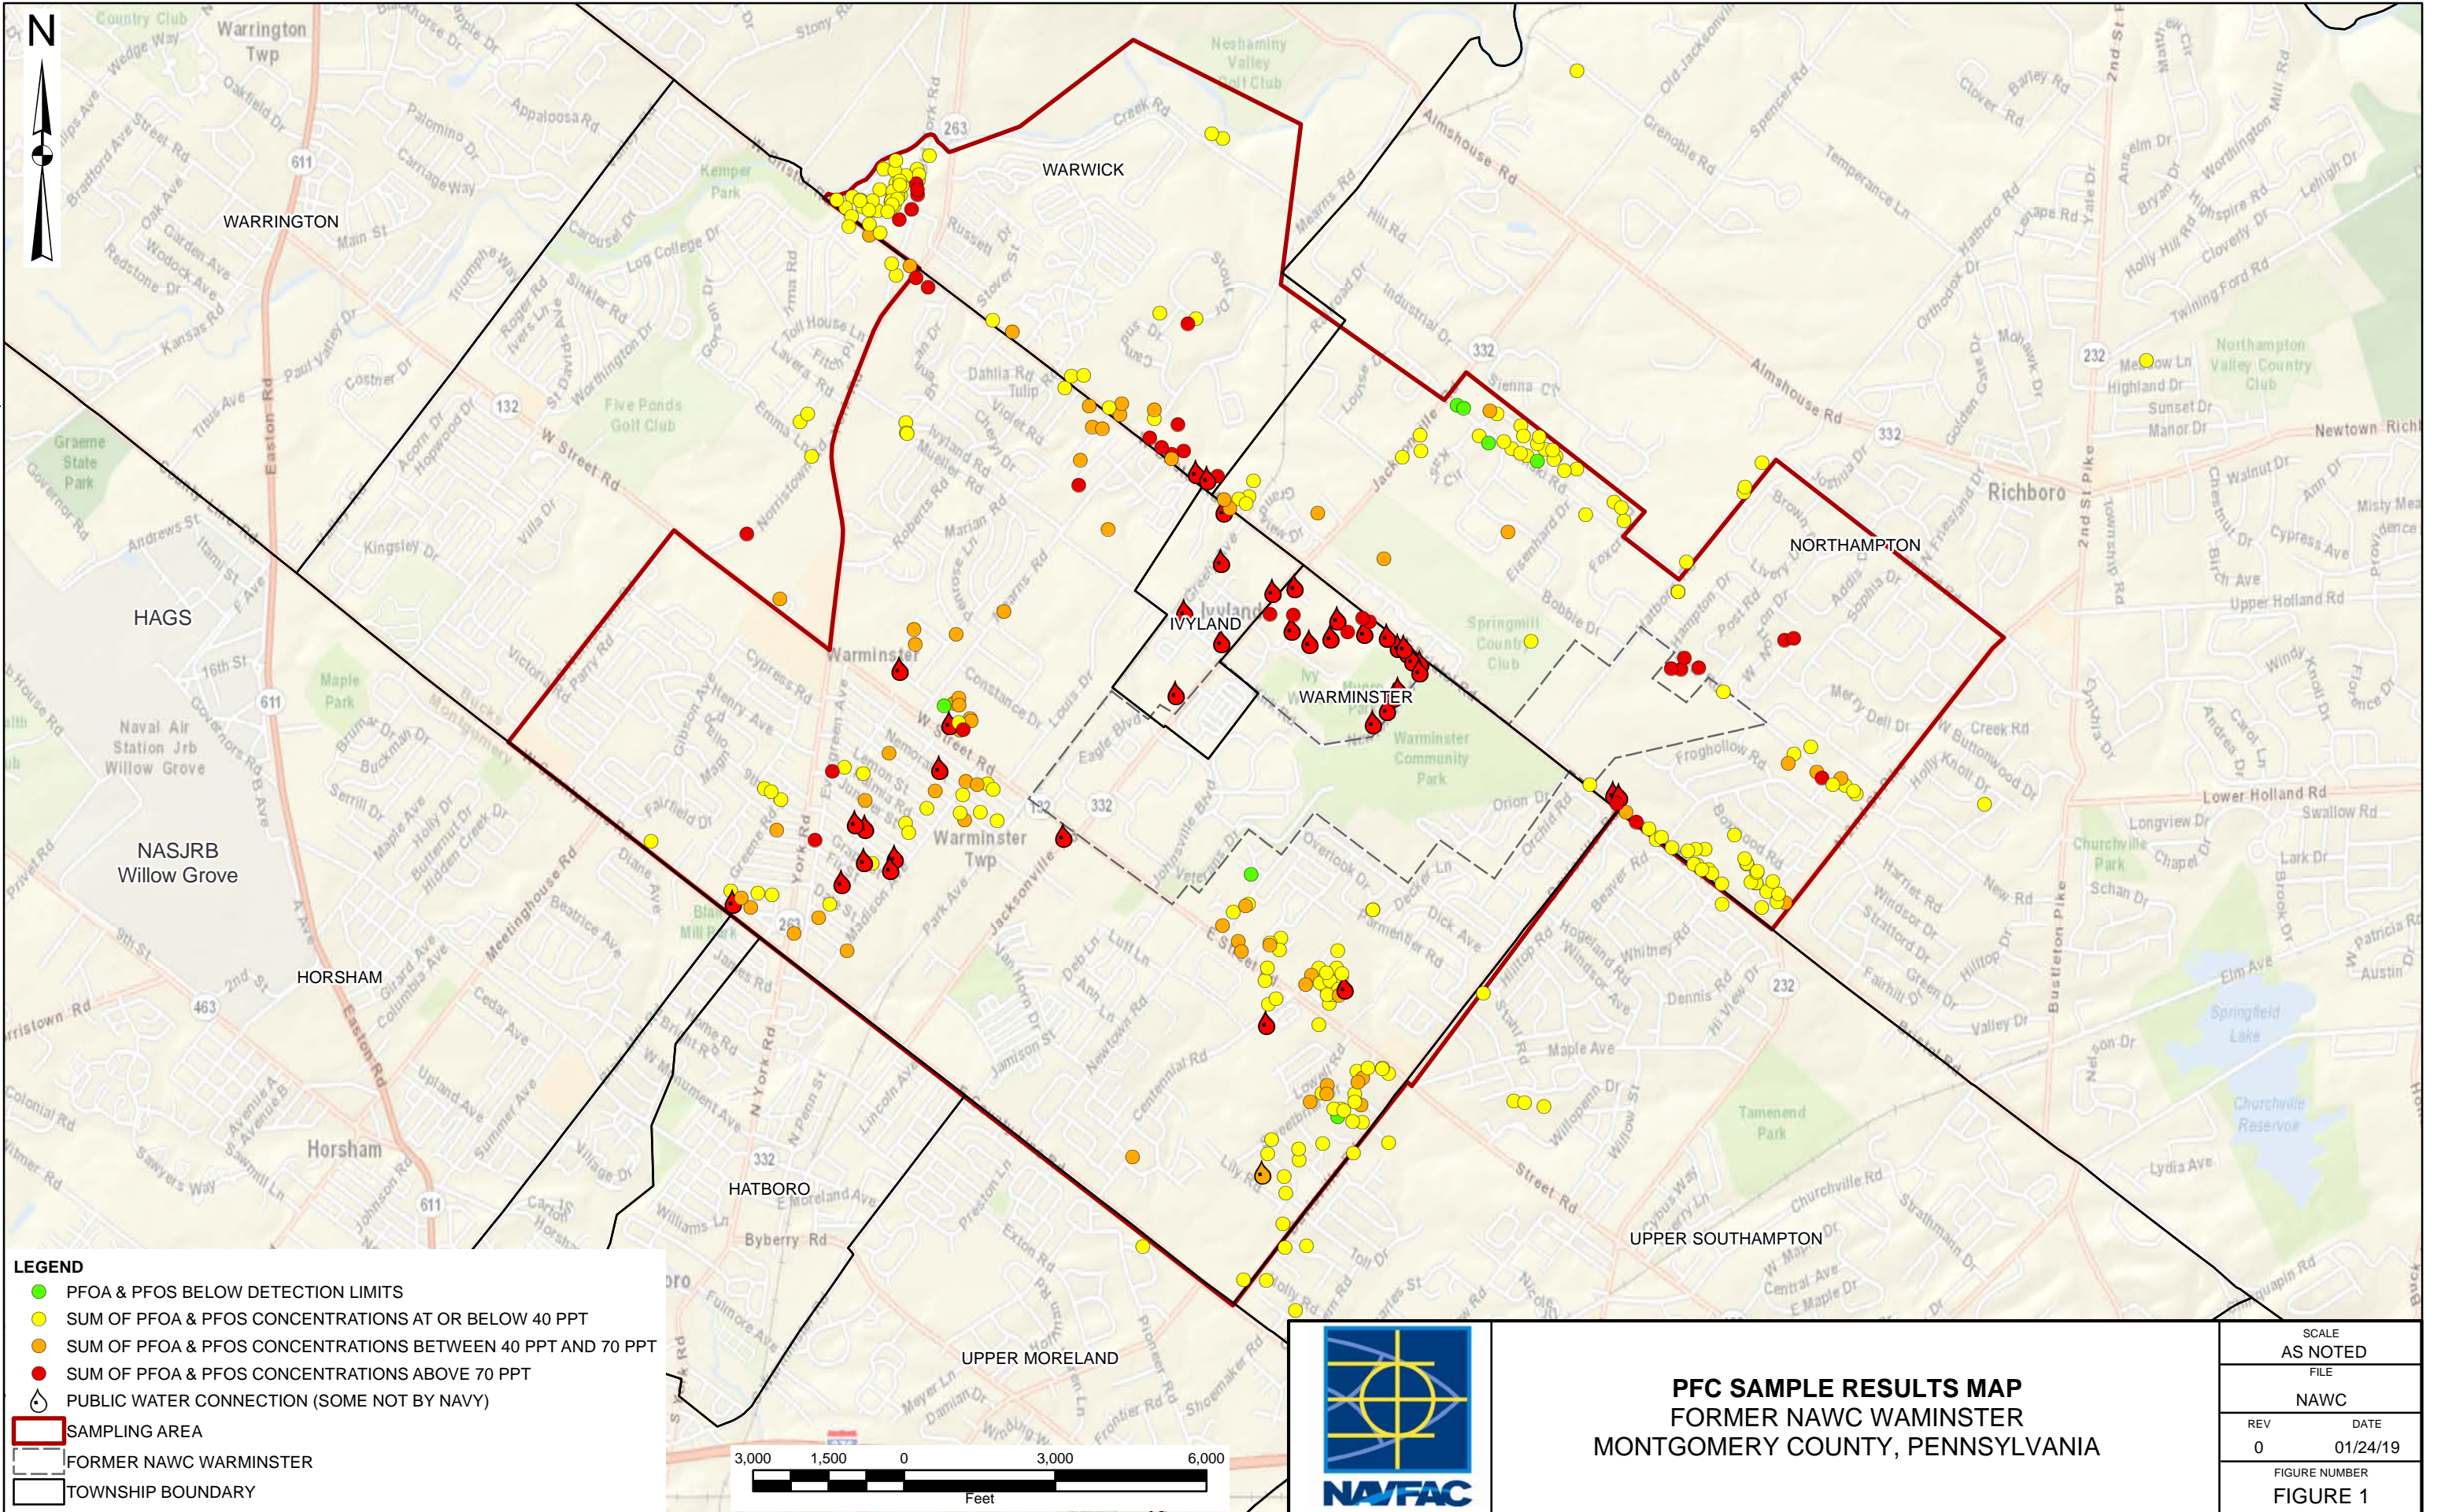

LEGEND

- PFOA & PFOS BELOW DETECTION LIMITS
- SUM OF PFOA & PFOS CONCENTRATIONS AT OR BELOW 40 PPT
- SUM OF PFOA & PFOS CONCENTRATIONS BETWEEN 40 PPT AND 70 PPT
- SUM OF PFOA & PFOS CONCENTRATIONS ABOVE 70 PPT
- 👉 PUBLIC WATER CONNECTION (SOME NOT BY NAVY)
- SAMPLING AREA
- FORMER NAWC WARRINSTER
- TOWNSHIP BOUNDARY



PFC SAMPLE RESULTS MAP
 FORMER NAWC WARRINSTER
 MONTGOMERY COUNTY, PENNSYLVANIA

SCALE AS NOTED	
FILE	
NAWC	
REV 0	DATE 01/24/19
FIGURE NUMBER	
FIGURE 1	