



**Off-Base Drinking Water Sample Results,
Combined Level 2 and Level 4 Laboratory Report,
Electronic Data Deliverable, Data Validation Report,
and the Sample Location Figure, SDG 320-35207-1**

*Naval Air Warfare Center Warminster
Warminster, Pennsylvania*

August 2019

N62269_001167
WARMINSTER_NAWC
SSIC 5000-33c

**LABORATORY DATA PACKAGE, 320-35207-1, NAS WILLOW GROVE NAWC
WARMINSTER PA**
02/07/2018
TESTAMERICA LABORATORIES INC

Approved for public release: distribution unlimited.

ANALYTICAL REPORT

Job Number: 320-35207-1

Job Description: Warminster: PFAS, NAS JRB Willow Grove

For:
Tetra Tech, Inc.
234 Mall Boulevard
Suite 260
King of Prussia, PA 19406
Attention: Andy Frebowitz



Approved for release.
David R. Alltucker
Project Manager I
2/7/2018 2:39 PM

David R Alltucker, Project Manager I
880 Riverside Parkway, West Sacramento, CA, 95605
(916)374-4383
david.alltucker@testamericainc.com
02/07/2018

Table of Contents

Cover Title Page	1
Data Summaries	4
Definitions	4
Case Narrative	5
Detection Summary	6
Client Sample Results	8
Default Detection Limits	12
Surrogate Summary	13
QC Sample Results	14
QC Association	15
Chronicle	16
Certification Summary	19
Method Summary	20
Sample Summary	21
Manual Integration Summary	22
Reagent Traceability	28
COAs	42
Organic Sample Data	96
LCMS	96
Method 537 DOD	96
Method 537 DOD QC Summary	97
Method 537 DOD Sample Data	106
Standards Data	184
Method 537 DOD ICAL Data	184
Method 537 DOD CCAL Data	223
Raw QC Data	263

Table of Contents

Method 537 DOD Blank Data	263
Method 537 DOD LCS/LCSD Data	268
Method 537 DOD Run Logs	282
Method 537 DOD Prep Data	286
Shipping and Receiving Documents	299
Client Chain of Custody	300
Sample Receipt Checklist	301

Definitions/Glossary

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-35207-1

Qualifiers

LCMS

Qualifier	Qualifier Description
U	Undetected at the Limit of Detection.
J	Estimated: The analyte was positively identified; the quantitation is an estimation
M	Manual integrated compound.

Glossary

Abbreviation	These commonly used abbreviations may or may not be present in this report.
α	Listed under the "D" column to designate that the result is reported on a dry weight basis
%R	Percent Recovery
CFL	Contains Free Liquid
CNF	Contains No Free Liquid
DER	Duplicate Error Ratio (normalized absolute difference)
Dil Fac	Dilution Factor
DL	Detection Limit (DoD/DOE)
DL, RA, RE, IN	Indicates a Dilution, Re-analysis, Re-extraction, or additional Initial metals/anion analysis of the sample
DLC	Decision Level Concentration (Radiochemistry)
EDL	Estimated Detection Limit (Dioxin)
LOD	Limit of Detection (DoD/DOE)
LOQ	Limit of Quantitation (DoD/DOE)
MDA	Minimum Detectable Activity (Radiochemistry)
MDC	Minimum Detectable Concentration (Radiochemistry)
MDL	Method Detection Limit
ML	Minimum Level (Dioxin)
NC	Not Calculated
ND	Not Detected at the reporting limit (or MDL or EDL if shown)
PQL	Practical Quantitation Limit
QC	Quality Control
RER	Relative Error Ratio (Radiochemistry)
RL	Reporting Limit or Requested Limit (Radiochemistry)
RPD	Relative Percent Difference, a measure of the relative difference between two points
TEF	Toxicity Equivalent Factor (Dioxin)
TEQ	Toxicity Equivalent Quotient (Dioxin)

Job Narrative
320-35207-1

Receipt

The samples were received on 1/19/2018 9:30 AM; the samples arrived in good condition, properly preserved and, where required, on ice. The temperature of the cooler at receipt was 4.7° C.

LCMS

No analytical or quality issues were noted, other than those described in the Definitions/Glossary page.

Organic Prep

Method(s) 537: Insufficient sample volume was available to perform a matrix spike/matrix spike duplicate (MS/MSD) associated with preparation batch 320-206379

Method(s) 537: The following sample, WGNA-011818-RW-3325 (320-35207-1) in preparation batch 320-206379 had a received pH of 9.

No additional analytical or quality issues were noted, other than those described above or in the Definitions/Glossary page.

Detection Summary

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-35207-1

Client Sample ID: WGNA-011818-RW-3325

Lab Sample ID: 320-35207-1

Analyte	Result	Qualifier	LOQ	DL	Unit	Dil Fac	D	Method	Prep Type
Perfluorooctanesulfonic acid (PFOS)	14	J M	40	6.9	ng/L	1		537	Total/NA
Perfluorooctanoic acid (PFOA)	14	J	20	2.8	ng/L	1		537	Total/NA
Perfluorohexanesulfonic acid (PFHxS)	13	J	30	5.6	ng/L	1		537	Total/NA
Perfluoroheptanoic acid (PFHpA)	4.2	J	10	1.9	ng/L	1		537	Total/NA

Client Sample ID: WGNA-011818-FRB-3325

Lab Sample ID: 320-35207-2

No Detections.

Client Sample ID: NAWC-011818-RW-316

Lab Sample ID: 320-35207-3

Analyte	Result	Qualifier	LOQ	DL	Unit	Dil Fac	D	Method	Prep Type
Perfluorooctanesulfonic acid (PFOS)	45	M	40	6.9	ng/L	1		537	Total/NA
Perfluorooctanoic acid (PFOA)	24	M	20	2.8	ng/L	1		537	Total/NA
Perfluorohexanesulfonic acid (PFHxS)	32		30	5.6	ng/L	1		537	Total/NA
Perfluoroheptanoic acid (PFHpA)	9.0	J	10	1.9	ng/L	1		537	Total/NA

Client Sample ID: NAWC-011818-FRB-316

Lab Sample ID: 320-35207-4

No Detections.

Client Sample ID: NAWC-011818-RW-260

Lab Sample ID: 320-35207-5

Analyte	Result	Qualifier	LOQ	DL	Unit	Dil Fac	D	Method	Prep Type
Perfluorooctanesulfonic acid (PFOS)	23	J M	41	7.0	ng/L	1		537	Total/NA
Perfluorooctanoic acid (PFOA)	24		20	2.9	ng/L	1		537	Total/NA
Perfluorohexanesulfonic acid (PFHxS)	8.6	J	31	5.6	ng/L	1		537	Total/NA
Perfluoroheptanoic acid (PFHpA)	7.0	J	10	1.9	ng/L	1		537	Total/NA
Perfluorobutanesulfonic acid (PFBS)	16	J	92	16	ng/L	1		537	Total/NA

Client Sample ID: NAWC-011818-FRB-260

Lab Sample ID: 320-35207-6

No Detections.

Client Sample ID: NAWC-011818-RW-281

Lab Sample ID: 320-35207-7

Analyte	Result	Qualifier	LOQ	DL	Unit	Dil Fac	D	Method	Prep Type
Perfluorooctanesulfonic acid (PFOS)	13	J M	40	6.9	ng/L	1		537	Total/NA
Perfluorooctanoic acid (PFOA)	15	J	20	2.8	ng/L	1		537	Total/NA
Perfluorohexanesulfonic acid (PFHxS)	6.4	J	30	5.6	ng/L	1		537	Total/NA
Perfluoroheptanoic acid (PFHpA)	4.4	J	10	1.9	ng/L	1		537	Total/NA

Client Sample ID: NAWC-011818-FRB-281

Lab Sample ID: 320-35207-8

No Detections.

Client Sample ID: NAWC-011818-RW-032

Lab Sample ID: 320-35207-9

Analyte	Result	Qualifier	LOQ	DL	Unit	Dil Fac	D	Method	Prep Type
Perfluorooctanesulfonic acid (PFOS)	20	J M	40	6.9	ng/L	1		537	Total/NA
Perfluorooctanoic acid (PFOA)	16	J	20	2.8	ng/L	1		537	Total/NA

This Detection Summary does not include radiochemical test results.

TestAmerica Sacramento

Detection Summary

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-35207-1

Client Sample ID: NAWC-011818-RW-032 (Continued)

Lab Sample ID: 320-35207-9

Analyte	Result	Qualifier	LOQ	DL	Unit	Dil Fac	D	Method	Prep Type
Perfluorohexanesulfonic acid (PFHxS)	14	J	30	5.6	ng/L	1		537	Total/NA
Perfluoroheptanoic acid (PFHpA)	5.4	J	10	1.9	ng/L	1		537	Total/NA

Client Sample ID: NAWC-011818-FRB-032

Lab Sample ID: 320-35207-10

No Detections.

Client Sample ID: NAWC-011818-RW-038

Lab Sample ID: 320-35207-11

Analyte	Result	Qualifier	LOQ	DL	Unit	Dil Fac	D	Method	Prep Type
Perfluorooctanesulfonic acid (PFOS)	25	J M	40	6.8	ng/L	1		537	Total/NA
Perfluorooctanoic acid (PFOA)	21		20	2.8	ng/L	1		537	Total/NA
Perfluorohexanesulfonic acid (PFHxS)	6.2	J	30	5.5	ng/L	1		537	Total/NA
Perfluoroheptanoic acid (PFHpA)	5.6	J	10	1.9	ng/L	1		537	Total/NA

Client Sample ID: NAWC-011818-FRB-038

Lab Sample ID: 320-35207-12

No Detections.

This Detection Summary does not include radiochemical test results.

TestAmerica Sacramento

Client Sample Results

Client: Tetra Tech, Inc.
 Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-35207-1

Client Sample ID: WGNA-011818-RW-3325

Lab Sample ID: 320-35207-1

Date Collected: 01/18/18 09:10

Matrix: Water

Date Received: 01/19/18 09:30

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	14	J M	40	6.9	ng/L		01/31/18 12:34	02/06/18 18:47	1
Perfluorooctanoic acid (PFOA)	14	J	20	2.8	ng/L		01/31/18 12:34	02/06/18 18:47	1
Perfluorononanoic acid (PFNA)	20	U M	24	8.1	ng/L		01/31/18 12:34	02/06/18 18:47	1
Perfluorohexanesulfonic acid (PFHxS)	13	J	30	5.6	ng/L		01/31/18 12:34	02/06/18 18:47	1
Perfluoroheptanoic acid (PFHpA)	4.2	J	10	1.9	ng/L		01/31/18 12:34	02/06/18 18:47	1
Perfluorobutanesulfonic acid (PFBS)	36	U	91	16	ng/L		01/31/18 12:34	02/06/18 18:47	1
Surrogate	%Recovery	Qualifier	Limits				Prepared	Analyzed	Dil Fac
13C2 PFHxA	96		70 - 130				01/31/18 12:34	02/06/18 18:47	1
13C2 PFDA	109		70 - 130				01/31/18 12:34	02/06/18 18:47	1

Client Sample ID: WGNA-011818-FRB-3325

Lab Sample ID: 320-35207-2

Date Collected: 01/18/18 09:05

Matrix: Water

Date Received: 01/19/18 09:30

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	16	U	40	6.8	ng/L		01/31/18 12:34	02/06/18 18:51	1
Perfluorooctanoic acid (PFOA)	7.9	U	20	2.8	ng/L		01/31/18 12:34	02/06/18 18:51	1
Perfluorononanoic acid (PFNA)	20	U	24	7.9	ng/L		01/31/18 12:34	02/06/18 18:51	1
Perfluorohexanesulfonic acid (PFHxS)	12	U	30	5.5	ng/L		01/31/18 12:34	02/06/18 18:51	1
Perfluoroheptanoic acid (PFHpA)	4.0	U	9.9	1.9	ng/L		01/31/18 12:34	02/06/18 18:51	1
Perfluorobutanesulfonic acid (PFBS)	36	U	89	16	ng/L		01/31/18 12:34	02/06/18 18:51	1
Surrogate	%Recovery	Qualifier	Limits				Prepared	Analyzed	Dil Fac
13C2 PFHxA	114		70 - 130				01/31/18 12:34	02/06/18 18:51	1
13C2 PFDA	104		70 - 130				01/31/18 12:34	02/06/18 18:51	1

Client Sample ID: NAWC-011818-RW-316

Lab Sample ID: 320-35207-3

Date Collected: 01/18/18 10:10

Matrix: Water

Date Received: 01/19/18 09:30

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	45	M	40	6.9	ng/L		01/31/18 12:34	02/06/18 18:56	1
Perfluorooctanoic acid (PFOA)	24	M	20	2.8	ng/L		01/31/18 12:34	02/06/18 18:56	1
Perfluorononanoic acid (PFNA)	20	U	24	8.1	ng/L		01/31/18 12:34	02/06/18 18:56	1
Perfluorohexanesulfonic acid (PFHxS)	32		30	5.6	ng/L		01/31/18 12:34	02/06/18 18:56	1
Perfluoroheptanoic acid (PFHpA)	9.0	J	10	1.9	ng/L		01/31/18 12:34	02/06/18 18:56	1
Perfluorobutanesulfonic acid (PFBS)	36	U	91	16	ng/L		01/31/18 12:34	02/06/18 18:56	1
Surrogate	%Recovery	Qualifier	Limits				Prepared	Analyzed	Dil Fac
13C2 PFHxA	103		70 - 130				01/31/18 12:34	02/06/18 18:56	1
13C2 PFDA	102		70 - 130				01/31/18 12:34	02/06/18 18:56	1

Client Sample Results

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-35207-1

Client Sample ID: NAWC-011818-FRB-316

Lab Sample ID: 320-35207-4

Date Collected: 01/18/18 10:05

Matrix: Water

Date Received: 01/19/18 09:30

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	16	U	40	6.7	ng/L		01/31/18 12:34	02/06/18 19:01	1
Perfluorooctanoic acid (PFOA)	7.9	U	20	2.8	ng/L		01/31/18 12:34	02/06/18 19:01	1
Perfluorononanoic acid (PFNA)	20	U	24	7.9	ng/L		01/31/18 12:34	02/06/18 19:01	1
Perfluorohexanesulfonic acid (PFHxS)	12	U	30	5.4	ng/L		01/31/18 12:34	02/06/18 19:01	1
Perfluoroheptanoic acid (PFHpA)	4.0	U	9.9	1.9	ng/L		01/31/18 12:34	02/06/18 19:01	1
Perfluorobutanesulfonic acid (PFBS)	36	U	89	16	ng/L		01/31/18 12:34	02/06/18 19:01	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	109		70 - 130	01/31/18 12:34	02/06/18 19:01	1
13C2 PFDA	100		70 - 130	01/31/18 12:34	02/06/18 19:01	1

Client Sample ID: NAWC-011818-RW-260

Lab Sample ID: 320-35207-5

Date Collected: 01/18/18 12:10

Matrix: Water

Date Received: 01/19/18 09:30

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	23	J M	41	7.0	ng/L		01/31/18 12:34	02/06/18 19:05	1
Perfluorooctanoic acid (PFOA)	24		20	2.9	ng/L		01/31/18 12:34	02/06/18 19:05	1
Perfluorononanoic acid (PFNA)	20	U M	25	8.2	ng/L		01/31/18 12:34	02/06/18 19:05	1
Perfluorohexanesulfonic acid (PFHxS)	8.6	J	31	5.6	ng/L		01/31/18 12:34	02/06/18 19:05	1
Perfluoroheptanoic acid (PFHpA)	7.0	J	10	1.9	ng/L		01/31/18 12:34	02/06/18 19:05	1
Perfluorobutanesulfonic acid (PFBS)	16	J	92	16	ng/L		01/31/18 12:34	02/06/18 19:05	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	104		70 - 130	01/31/18 12:34	02/06/18 19:05	1
13C2 PFDA	105		70 - 130	01/31/18 12:34	02/06/18 19:05	1

Client Sample ID: NAWC-011818-FRB-260

Lab Sample ID: 320-35207-6

Date Collected: 01/18/18 12:05

Matrix: Water

Date Received: 01/19/18 09:30

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	16	U	40	6.8	ng/L		01/31/18 12:34	02/06/18 19:19	1
Perfluorooctanoic acid (PFOA)	8.0	U	20	2.8	ng/L		01/31/18 12:34	02/06/18 19:19	1
Perfluorononanoic acid (PFNA)	20	U	24	8.0	ng/L		01/31/18 12:34	02/06/18 19:19	1
Perfluorohexanesulfonic acid (PFHxS)	12	U	30	5.5	ng/L		01/31/18 12:34	02/06/18 19:19	1
Perfluoroheptanoic acid (PFHpA)	4.0	U	10	1.9	ng/L		01/31/18 12:34	02/06/18 19:19	1
Perfluorobutanesulfonic acid (PFBS)	36	U	90	16	ng/L		01/31/18 12:34	02/06/18 19:19	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	104		70 - 130	01/31/18 12:34	02/06/18 19:19	1
13C2 PFDA	102		70 - 130	01/31/18 12:34	02/06/18 19:19	1

Client Sample Results

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-35207-1

Client Sample ID: NAWC-011818-RW-281

Lab Sample ID: 320-35207-7

Date Collected: 01/18/18 13:10

Matrix: Water

Date Received: 01/19/18 09:30

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	13	J M	40	6.9	ng/L		01/31/18 12:34	02/06/18 19:24	1
Perfluorooctanoic acid (PFOA)	15	J	20	2.8	ng/L		01/31/18 12:34	02/06/18 19:24	1
Perfluorononanoic acid (PFNA)	20	U	24	8.1	ng/L		01/31/18 12:34	02/06/18 19:24	1
Perfluorohexanesulfonic acid (PFHxS)	6.4	J	30	5.6	ng/L		01/31/18 12:34	02/06/18 19:24	1
Perfluoroheptanoic acid (PFHpA)	4.4	J	10	1.9	ng/L		01/31/18 12:34	02/06/18 19:24	1
Perfluorobutanesulfonic acid (PFBS)	36	U	91	16	ng/L		01/31/18 12:34	02/06/18 19:24	1
Surrogate	%Recovery	Qualifier	Limits				Prepared	Analyzed	Dil Fac
13C2 PFHxA	99		70 - 130				01/31/18 12:34	02/06/18 19:24	1
13C2 PFDA	103		70 - 130				01/31/18 12:34	02/06/18 19:24	1

Client Sample ID: NAWC-011818-FRB-281

Lab Sample ID: 320-35207-8

Date Collected: 01/18/18 13:05

Matrix: Water

Date Received: 01/19/18 09:30

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	16	U	40	6.8	ng/L		01/31/18 12:34	02/06/18 19:29	1
Perfluorooctanoic acid (PFOA)	8.0	U	20	2.8	ng/L		01/31/18 12:34	02/06/18 19:29	1
Perfluorononanoic acid (PFNA)	20	U	24	8.0	ng/L		01/31/18 12:34	02/06/18 19:29	1
Perfluorohexanesulfonic acid (PFHxS)	12	U	30	5.5	ng/L		01/31/18 12:34	02/06/18 19:29	1
Perfluoroheptanoic acid (PFHpA)	4.0	U	10	1.9	ng/L		01/31/18 12:34	02/06/18 19:29	1
Perfluorobutanesulfonic acid (PFBS)	36	U	90	16	ng/L		01/31/18 12:34	02/06/18 19:29	1
Surrogate	%Recovery	Qualifier	Limits				Prepared	Analyzed	Dil Fac
13C2 PFHxA	103		70 - 130				01/31/18 12:34	02/06/18 19:29	1
13C2 PFDA	102		70 - 130				01/31/18 12:34	02/06/18 19:29	1

Client Sample ID: NAWC-011818-RW-032

Lab Sample ID: 320-35207-9

Date Collected: 01/18/18 13:40

Matrix: Water

Date Received: 01/19/18 09:30

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	20	J M	40	6.9	ng/L		01/31/18 12:34	02/06/18 19:33	1
Perfluorooctanoic acid (PFOA)	16	J	20	2.8	ng/L		01/31/18 12:34	02/06/18 19:33	1
Perfluorononanoic acid (PFNA)	20	U	24	8.1	ng/L		01/31/18 12:34	02/06/18 19:33	1
Perfluorohexanesulfonic acid (PFHxS)	14	J	30	5.6	ng/L		01/31/18 12:34	02/06/18 19:33	1
Perfluoroheptanoic acid (PFHpA)	5.4	J	10	1.9	ng/L		01/31/18 12:34	02/06/18 19:33	1
Perfluorobutanesulfonic acid (PFBS)	36	U	91	16	ng/L		01/31/18 12:34	02/06/18 19:33	1
Surrogate	%Recovery	Qualifier	Limits				Prepared	Analyzed	Dil Fac
13C2 PFHxA	88		70 - 130				01/31/18 12:34	02/06/18 19:33	1
13C2 PFDA	104		70 - 130				01/31/18 12:34	02/06/18 19:33	1

Client Sample Results

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-35207-1

Client Sample ID: NAWC-011818-FRB-032

Lab Sample ID: 320-35207-10

Date Collected: 01/18/18 13:35

Matrix: Water

Date Received: 01/19/18 09:30

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	16	U	41	7.0	ng/L		01/31/18 12:34	02/06/18 19:38	1
Perfluorooctanoic acid (PFOA)	8.2	U	20	2.9	ng/L		01/31/18 12:34	02/06/18 19:38	1
Perfluorononanoic acid (PFNA)	20	U	25	8.2	ng/L		01/31/18 12:34	02/06/18 19:38	1
Perfluorohexanesulfonic acid (PFHxS)	12	U	31	5.6	ng/L		01/31/18 12:34	02/06/18 19:38	1
Perfluoroheptanoic acid (PFHpA)	4.1	U	10	1.9	ng/L		01/31/18 12:34	02/06/18 19:38	1
Perfluorobutanesulfonic acid (PFBS)	37	U	92	16	ng/L		01/31/18 12:34	02/06/18 19:38	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	104		70 - 130	01/31/18 12:34	02/06/18 19:38	1
13C2 PFDA	105		70 - 130	01/31/18 12:34	02/06/18 19:38	1

Client Sample ID: NAWC-011818-RW-038

Lab Sample ID: 320-35207-11

Date Collected: 01/18/18 14:10

Matrix: Water

Date Received: 01/19/18 09:30

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	25	J M	40	6.8	ng/L		01/31/18 12:34	02/06/18 19:43	1
Perfluorooctanoic acid (PFOA)	21		20	2.8	ng/L		01/31/18 12:34	02/06/18 19:43	1
Perfluorononanoic acid (PFNA)	20	U	24	8.0	ng/L		01/31/18 12:34	02/06/18 19:43	1
Perfluorohexanesulfonic acid (PFHxS)	6.2	J	30	5.5	ng/L		01/31/18 12:34	02/06/18 19:43	1
Perfluoroheptanoic acid (PFHpA)	5.6	J	10	1.9	ng/L		01/31/18 12:34	02/06/18 19:43	1
Perfluorobutanesulfonic acid (PFBS)	36	U	90	16	ng/L		01/31/18 12:34	02/06/18 19:43	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	90		70 - 130	01/31/18 12:34	02/06/18 19:43	1
13C2 PFDA	97		70 - 130	01/31/18 12:34	02/06/18 19:43	1

Client Sample ID: NAWC-011818-FRB-038

Lab Sample ID: 320-35207-12

Date Collected: 01/18/18 14:05

Matrix: Water

Date Received: 01/19/18 09:30

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	16	U	40	6.8	ng/L		01/31/18 12:34	02/06/18 19:47	1
Perfluorooctanoic acid (PFOA)	8.0	U	20	2.8	ng/L		01/31/18 12:34	02/06/18 19:47	1
Perfluorononanoic acid (PFNA)	20	U	24	8.0	ng/L		01/31/18 12:34	02/06/18 19:47	1
Perfluorohexanesulfonic acid (PFHxS)	12	U	30	5.5	ng/L		01/31/18 12:34	02/06/18 19:47	1
Perfluoroheptanoic acid (PFHpA)	4.0	U	10	1.9	ng/L		01/31/18 12:34	02/06/18 19:47	1
Perfluorobutanesulfonic acid (PFBS)	36	U	90	16	ng/L		01/31/18 12:34	02/06/18 19:47	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	107		70 - 130	01/31/18 12:34	02/06/18 19:47	1
13C2 PFDA	102		70 - 130	01/31/18 12:34	02/06/18 19:47	1

Default Detection Limits

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-35207-1

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Prep: 537

Analyte	LOQ	DL	Units	Method
Perfluorobutanesulfonic acid (PFBS)	90	16	ng/L	537
Perfluoroheptanoic acid (PFHpA)	10	1.9	ng/L	537
Perfluorohexanesulfonic acid (PFHxS)	30	5.5	ng/L	537
Perfluorononanoic acid (PFNA)	24	8.0	ng/L	537
Perfluorooctanesulfonic acid (PFOS)	40	6.8	ng/L	537
Perfluorooctanoic acid (PFOA)	20	2.8	ng/L	537

Surrogate Summary

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-35207-1

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Matrix: Water

Prep Type: Total/NA

Lab Sample ID	Client Sample ID	Percent Surrogate Recovery (Acceptance Limits)	
		PFHxA (70-130)	PFDA (70-130)
320-35207-1	WGNA-011818-RW-3325	96	109
320-35207-2	WGNA-011818-FRB-3325	114	104
320-35207-3	NAWC-011818-RW-316	103	102
320-35207-4	NAWC-011818-FRB-316	109	100
320-35207-5	NAWC-011818-RW-260	104	105
320-35207-6	NAWC-011818-FRB-260	104	102
320-35207-7	NAWC-011818-RW-281	99	103
320-35207-8	NAWC-011818-FRB-281	103	102
320-35207-9	NAWC-011818-RW-032	88	104
320-35207-10	NAWC-011818-FRB-032	104	105
320-35207-11	NAWC-011818-RW-038	90	97
320-35207-12	NAWC-011818-FRB-038	107	102
LLCS 320-206379/2-A	Lab Control Sample	106	104
LLCSD 320-206379/3-A	Lab Control Sample Dup	109	104
MB 320-206379/1-A	Method Blank	114	110

Surrogate Legend

PFHxA = 13C2 PFHxA

PFDA = 13C2 PFDA

QC Sample Results

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-35207-1

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Lab Sample ID: MB 320-206379/1-A
Matrix: Water
Analysis Batch: 207292

Client Sample ID: Method Blank
Prep Type: Total/NA
Prep Batch: 206379

Analyte	MB MB		LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
	Result	Qualifier							
Perfluorooctanesulfonic acid (PFOS)	16	U	40	6.8	ng/L		01/31/18 12:34	02/06/18 18:33	1
Perfluorooctanoic acid (PFOA)	8.0	U	20	2.8	ng/L		01/31/18 12:34	02/06/18 18:33	1
Perfluorononanoic acid (PFNA)	20	U	24	8.0	ng/L		01/31/18 12:34	02/06/18 18:33	1
Perfluorohexanesulfonic acid (PFHxS)	12	U	30	5.5	ng/L		01/31/18 12:34	02/06/18 18:33	1
Perfluoroheptanoic acid (PFHpA)	4.0	U	10	1.9	ng/L		01/31/18 12:34	02/06/18 18:33	1
Perfluorobutanesulfonic acid (PFBS)	36	U	90	16	ng/L		01/31/18 12:34	02/06/18 18:33	1

Surrogate	MB MB		Limits	Prepared	Analyzed	Dil Fac
	%Recovery	Qualifier				
13C2 PFHxA	114		70 - 130	01/31/18 12:34	02/06/18 18:33	1
13C2 PFDA	110		70 - 130	01/31/18 12:34	02/06/18 18:33	1

Lab Sample ID: LLCS 320-206379/2-A
Matrix: Water
Analysis Batch: 207292

Client Sample ID: Lab Control Sample
Prep Type: Total/NA
Prep Batch: 206379

Analyte	Spike Added	LLCS LLCS		Unit	D	%Rec	%Rec. Limits
		Result	Qualifier				
Perfluorooctanesulfonic acid (PFOS)	40.0	40.2	M	ng/L		100	50 - 150
Perfluorooctanoic acid (PFOA)	20.0	22.1		ng/L		111	50 - 150
Perfluorononanoic acid (PFNA)	20.0	21.9	J	ng/L		110	50 - 150
Perfluorohexanesulfonic acid (PFHxS)	30.0	33.0		ng/L		110	50 - 150
Perfluoroheptanoic acid (PFHpA)	10.0	11.6		ng/L		116	50 - 150
Perfluorobutanesulfonic acid (PFBS)	90.0	94.5		ng/L		105	50 - 150

Surrogate	LLCS LLCS		Limits
	%Recovery	Qualifier	
13C2 PFHxA	106		70 - 130
13C2 PFDA	104		70 - 130

Lab Sample ID: LLCSD 320-206379/3-A
Matrix: Water
Analysis Batch: 207292

Client Sample ID: Lab Control Sample Dup
Prep Type: Total/NA
Prep Batch: 206379

Analyte	Spike Added	LLCSD LLCSD		Unit	D	%Rec	%Rec. Limits	RPD	
		Result	Qualifier					RPD	Limit
Perfluorooctanesulfonic acid (PFOS)	40.0	37.6	J M	ng/L		94	50 - 150	7	50
Perfluorooctanoic acid (PFOA)	20.0	22.5		ng/L		112	50 - 150	1	50
Perfluorononanoic acid (PFNA)	20.0	22.2	J	ng/L		111	50 - 150	1	50
Perfluorohexanesulfonic acid (PFHxS)	30.0	31.4		ng/L		105	50 - 150	5	50
Perfluoroheptanoic acid (PFHpA)	10.0	11.4		ng/L		114	50 - 150	1	50
Perfluorobutanesulfonic acid (PFBS)	90.0	94.8		ng/L		105	50 - 150	0.3	50

Surrogate	LLCSD LLCSD		Limits
	%Recovery	Qualifier	
13C2 PFHxA	109		70 - 130
13C2 PFDA	104		70 - 130

QC Association Summary

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-35207-1

LCMS

Prep Batch: 206379

Lab Sample ID	Client Sample ID	Prep Type	Matrix	Method	Prep Batch
320-35207-1	WGNA-011818-RW-3325	Total/NA	Water	537	
320-35207-2	WGNA-011818-FRB-3325	Total/NA	Water	537	
320-35207-3	NAWC-011818-RW-316	Total/NA	Water	537	
320-35207-4	NAWC-011818-FRB-316	Total/NA	Water	537	
320-35207-5	NAWC-011818-RW-260	Total/NA	Water	537	
320-35207-6	NAWC-011818-FRB-260	Total/NA	Water	537	
320-35207-7	NAWC-011818-RW-281	Total/NA	Water	537	
320-35207-8	NAWC-011818-FRB-281	Total/NA	Water	537	
320-35207-9	NAWC-011818-RW-032	Total/NA	Water	537	
320-35207-10	NAWC-011818-FRB-032	Total/NA	Water	537	
320-35207-11	NAWC-011818-RW-038	Total/NA	Water	537	
320-35207-12	NAWC-011818-FRB-038	Total/NA	Water	537	
MB 320-206379/1-A	Method Blank	Total/NA	Water	537	
LLCS 320-206379/2-A	Lab Control Sample	Total/NA	Water	537	
LLCSD 320-206379/3-A	Lab Control Sample Dup	Total/NA	Water	537	

Analysis Batch: 207292

Lab Sample ID	Client Sample ID	Prep Type	Matrix	Method	Prep Batch
320-35207-1	WGNA-011818-RW-3325	Total/NA	Water	537	206379
320-35207-2	WGNA-011818-FRB-3325	Total/NA	Water	537	206379
320-35207-3	NAWC-011818-RW-316	Total/NA	Water	537	206379
320-35207-4	NAWC-011818-FRB-316	Total/NA	Water	537	206379
320-35207-5	NAWC-011818-RW-260	Total/NA	Water	537	206379
MB 320-206379/1-A	Method Blank	Total/NA	Water	537	206379
LLCS 320-206379/2-A	Lab Control Sample	Total/NA	Water	537	206379
LLCSD 320-206379/3-A	Lab Control Sample Dup	Total/NA	Water	537	206379

Analysis Batch: 207294

Lab Sample ID	Client Sample ID	Prep Type	Matrix	Method	Prep Batch
320-35207-6	NAWC-011818-FRB-260	Total/NA	Water	537	206379
320-35207-7	NAWC-011818-RW-281	Total/NA	Water	537	206379
320-35207-8	NAWC-011818-FRB-281	Total/NA	Water	537	206379
320-35207-9	NAWC-011818-RW-032	Total/NA	Water	537	206379
320-35207-10	NAWC-011818-FRB-032	Total/NA	Water	537	206379
320-35207-11	NAWC-011818-RW-038	Total/NA	Water	537	206379
320-35207-12	NAWC-011818-FRB-038	Total/NA	Water	537	206379

Lab Chronicle

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-35207-1

Client Sample ID: WGNA-011818-RW-3325

Date Collected: 01/18/18 09:10

Date Received: 01/19/18 09:30

Lab Sample ID: 320-35207-1

Matrix: Water

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			206379	01/31/18 12:34	KMK	TAL SAC
Total/NA	Analysis	537		1	207292	02/06/18 18:47	SHK	TAL SAC

Client Sample ID: WGNA-011818-FRB-3325

Date Collected: 01/18/18 09:05

Date Received: 01/19/18 09:30

Lab Sample ID: 320-35207-2

Matrix: Water

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			206379	01/31/18 12:34	KMK	TAL SAC
Total/NA	Analysis	537		1	207292	02/06/18 18:51	SHK	TAL SAC

Client Sample ID: NAWC-011818-RW-316

Date Collected: 01/18/18 10:10

Date Received: 01/19/18 09:30

Lab Sample ID: 320-35207-3

Matrix: Water

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			206379	01/31/18 12:34	KMK	TAL SAC
Total/NA	Analysis	537		1	207292	02/06/18 18:56	SHK	TAL SAC

Client Sample ID: NAWC-011818-FRB-316

Date Collected: 01/18/18 10:05

Date Received: 01/19/18 09:30

Lab Sample ID: 320-35207-4

Matrix: Water

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			206379	01/31/18 12:34	KMK	TAL SAC
Total/NA	Analysis	537		1	207292	02/06/18 19:01	SHK	TAL SAC

Client Sample ID: NAWC-011818-RW-260

Date Collected: 01/18/18 12:10

Date Received: 01/19/18 09:30

Lab Sample ID: 320-35207-5

Matrix: Water

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			206379	01/31/18 12:34	KMK	TAL SAC
Total/NA	Analysis	537		1	207292	02/06/18 19:05	SHK	TAL SAC

Client Sample ID: NAWC-011818-FRB-260

Date Collected: 01/18/18 12:05

Date Received: 01/19/18 09:30

Lab Sample ID: 320-35207-6

Matrix: Water

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			206379	01/31/18 12:34	KMK	TAL SAC
Total/NA	Analysis	537		1	207294	02/06/18 19:19	SHK	TAL SAC

TestAmerica Sacramento

Lab Chronicle

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-35207-1

Client Sample ID: NAWC-011818-RW-281

Lab Sample ID: 320-35207-7

Date Collected: 01/18/18 13:10

Matrix: Water

Date Received: 01/19/18 09:30

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			206379	01/31/18 12:34	KMK	TAL SAC
Total/NA	Analysis	537		1	207294	02/06/18 19:24	SHK	TAL SAC

Client Sample ID: NAWC-011818-FRB-281

Lab Sample ID: 320-35207-8

Date Collected: 01/18/18 13:05

Matrix: Water

Date Received: 01/19/18 09:30

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			206379	01/31/18 12:34	KMK	TAL SAC
Total/NA	Analysis	537		1	207294	02/06/18 19:29	SHK	TAL SAC

Client Sample ID: NAWC-011818-RW-032

Lab Sample ID: 320-35207-9

Date Collected: 01/18/18 13:40

Matrix: Water

Date Received: 01/19/18 09:30

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			206379	01/31/18 12:34	KMK	TAL SAC
Total/NA	Analysis	537		1	207294	02/06/18 19:33	SHK	TAL SAC

Client Sample ID: NAWC-011818-FRB-032

Lab Sample ID: 320-35207-10

Date Collected: 01/18/18 13:35

Matrix: Water

Date Received: 01/19/18 09:30

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			206379	01/31/18 12:34	KMK	TAL SAC
Total/NA	Analysis	537		1	207294	02/06/18 19:38	SHK	TAL SAC

Client Sample ID: NAWC-011818-RW-038

Lab Sample ID: 320-35207-11

Date Collected: 01/18/18 14:10

Matrix: Water

Date Received: 01/19/18 09:30

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			206379	01/31/18 12:34	KMK	TAL SAC
Total/NA	Analysis	537		1	207294	02/06/18 19:43	SHK	TAL SAC

Client Sample ID: NAWC-011818-FRB-038

Lab Sample ID: 320-35207-12

Date Collected: 01/18/18 14:05

Matrix: Water

Date Received: 01/19/18 09:30

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			206379	01/31/18 12:34	KMK	TAL SAC
Total/NA	Analysis	537		1	207294	02/06/18 19:47	SHK	TAL SAC

TestAmerica Sacramento

Lab Chronicle

Client: Tetra Tech, Inc.

TestAmerica Job ID: 320-35207-1

Project/Site: Warminster: PFAS, NAS JRB Willow Grove

Laboratory References:

TAL SAC = TestAmerica Sacramento, 880 Riverside Parkway, West Sacramento, CA 95605, TEL (916)373-5600

Accreditation/Certification Summary

Client: Tetra Tech, Inc.
 Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-35207-1

Laboratory: TestAmerica Sacramento

All accreditations/certifications held by this laboratory are listed. Not all accreditations/certifications are applicable to this report.

Authority	Program	EPA Region	Identification Number	Expiration Date
Alaska (UST)	State Program	10	17-020	01-20-21
Arizona	State Program	9	AZ0708	08-11-18
Arkansas DEQ	State Program	6	88-0691	06-17-18
California	State Program	9	2897	01-31-19
Colorado	State Program	8	CA00044	08-31-18
Connecticut	State Program	1	PH-0691	06-30-19
Florida	NELAP	4	E87570	06-30-18
Georgia	State Program	4	N/A	01-28-19
Hawaii	State Program	9	N/A	01-29-19
Illinois	NELAP	5	200060	03-17-18
Kansas	NELAP	7	E-10375	10-31-18
L-A-B	DoD ELAP		L2468	01-20-21
Louisiana	NELAP	6	30612	06-30-18
Maine	State Program	1	CA0004	04-14-18
Michigan	State Program	5	9947	01-31-18 *
Nevada	State Program	9	CA00044	07-31-18
New Hampshire	NELAP	1	2997	04-18-18
New Jersey	NELAP	2	CA005	06-30-18
New York	NELAP	2	11666	04-01-18
Oregon	NELAP	10	4040	01-29-20
Pennsylvania	NELAP	3	68-01272	03-31-18
Texas	NELAP	6	T104704399	05-31-18
US Fish & Wildlife	Federal		LE148388-0	07-31-18
USDA	Federal		P330-11-00436	01-17-21
USEPA UCMR	Federal	1	CA00044	11-06-18
Utah	NELAP	8	CA00044	02-28-18
Virginia	NELAP	3	460278	03-14-18
Washington	State Program	10	C581	05-05-18
West Virginia (DW)	State Program	3	9930C	12-31-18
Wyoming	State Program	8	8TMS-L	01-28-19

* Accreditation/Certification renewal pending - accreditation/certification considered valid.

Method Summary

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-35207-1

Method	Method Description	Protocol	Laboratory
537	Perfluorinated Alkyl Acids (LC/MS)	EPA	TAL SAC

Protocol References:

EPA = US Environmental Protection Agency

Laboratory References:

TAL SAC = TestAmerica Sacramento, 880 Riverside Parkway, West Sacramento, CA 95605, TEL (916)373-5600

Sample Summary

Client: Tetra Tech, Inc.

TestAmerica Job ID: 320-35207-1

Project/Site: Warminster: PFAS, NAS JRB Willow Grove

Lab Sample ID	Client Sample ID	Matrix	Collected	Received
320-35207-1	WGNA-011818-RW-3325	Water	01/18/18 09:10	01/19/18 09:30
320-35207-2	WGNA-011818-FRB-3325	Water	01/18/18 09:05	01/19/18 09:30
320-35207-3	NAWC-011818-RW-316	Water	01/18/18 10:10	01/19/18 09:30
320-35207-4	NAWC-011818-FRB-316	Water	01/18/18 10:05	01/19/18 09:30
320-35207-5	NAWC-011818-RW-260	Water	01/18/18 12:10	01/19/18 09:30
320-35207-6	NAWC-011818-FRB-260	Water	01/18/18 12:05	01/19/18 09:30
320-35207-7	NAWC-011818-RW-281	Water	01/18/18 13:10	01/19/18 09:30
320-35207-8	NAWC-011818-FRB-281	Water	01/18/18 13:05	01/19/18 09:30
320-35207-9	NAWC-011818-RW-032	Water	01/18/18 13:40	01/19/18 09:30
320-35207-10	NAWC-011818-FRB-032	Water	01/18/18 13:35	01/19/18 09:30
320-35207-11	NAWC-011818-RW-038	Water	01/18/18 14:10	01/19/18 09:30
320-35207-12	NAWC-011818-FRB-038	Water	01/18/18 14:05	01/19/18 09:30

LCMS MANUAL INTEGRATION SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1

SDG No.: _____

Instrument ID: A8_N Analysis Batch Number: 192908

Lab Sample ID: IC 320-192908/4 Client Sample ID: _____

Date Analyzed: 11/03/17 13:37 Lab File ID: 2017.11.03_537XICAL_004.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.16	Assign Peak	phomsopha t	11/06/17 07:17

Lab Sample ID: IC 320-192908/5 Client Sample ID: _____

Date Analyzed: 11/03/17 13:42 Lab File ID: 2017.11.03_537XICAL_005.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.16	Assign Peak	phomsopha t	11/06/17 07:18

Lab Sample ID: IC 320-192908/7 ICISAV Client Sample ID: _____

Date Analyzed: 11/03/17 13:52 Lab File ID: 2017.11.03_537XICAL_007.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.16	Assign Peak	phomsopha t	11/06/17 07:20

LCMS MANUAL INTEGRATION SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1

SDG No.: _____

Instrument ID: A8_N Analysis Batch Number: 207097

Lab Sample ID: CCVL 320-207097/1 Client Sample ID: _____

Date Analyzed: 02/06/18 08:30 Lab File ID: 2018.02.06_537A_003.d GC Column: GeminiC18 3x1 ID: 3 (mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.06	User Assigned	roycea	02/06/18 09:48

LCMS MANUAL INTEGRATION SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1

SDG No.: _____

Instrument ID: A8_N Analysis Batch Number: 207292

Lab Sample ID: CCV 320-207292/1 CCVIS Client Sample ID: _____

Date Analyzed: 02/06/18 18:23 Lab File ID: 2018.02.06_537XX_042.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.05	User Assigned	krenns	02/07/18 11:36

Lab Sample ID: LLCS 320-206379/2-A Client Sample ID: _____

Date Analyzed: 02/06/18 18:37 Lab File ID: 2018.02.06_537XX_045.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.05	User Assigned	krenns	02/07/18 11:43

Lab Sample ID: LLCSD 320-206379/3-A Client Sample ID: _____

Date Analyzed: 02/06/18 18:42 Lab File ID: 2018.02.06_537XX_046.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.05	User Assigned	krenns	02/07/18 11:44

Lab Sample ID: 320-35207-1 Client Sample ID: WGNA-011818-RW-3325

Date Analyzed: 02/06/18 18:47 Lab File ID: 2018.02.06_537XX_047.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.05	User Assigned	krenns	02/07/18 11:44
Perfluorononanoic acid (PFNA)	2.06	Split Peak	krenns	02/07/18 13:41

LCMS MANUAL INTEGRATION SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1

SDG No.: _____

Instrument ID: A8_N Analysis Batch Number: 207292

Lab Sample ID: 320-35207-3 Client Sample ID: NAWC-011818-RW-316

Date Analyzed: 02/06/18 18:56 Lab File ID: 2018.02.06_537XX_049.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanoic acid (PFOA)	1.80	Incomplete Integration	krenns	02/07/18 11:46
Perfluorooctanesulfonic acid (PFOS)	2.04	Split Peak	krenns	02/07/18 13:42

Lab Sample ID: 320-35207-5 Client Sample ID: NAWC-011818-RW-260

Date Analyzed: 02/06/18 19:05 Lab File ID: 2018.02.06_537XX_051.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.05	Split Peak	krenns	02/07/18 13:42
Perfluorononanoic acid (PFNA)	2.06	Split Peak	krenns	02/07/18 13:43

Lab Sample ID: CCV 320-207292/11 CCVIS Client Sample ID: _____

Date Analyzed: 02/06/18 19:10 Lab File ID: 2018.02.06_537XX_052.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.04	User Assigned	krenns	02/07/18 11:47

LCMS MANUAL INTEGRATION SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1

SDG No.: _____

Instrument ID: A8_N Analysis Batch Number: 207294

Lab Sample ID: CCV 320-207294/11 CCVIS Client Sample ID: _____

Date Analyzed: 02/06/18 19:10 Lab File ID: 2018.02.06_537XX_052.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.04	User Assigned	krenns	02/07/18 11:47

Lab Sample ID: 320-35207-7 Client Sample ID: NAWC-011818-RW-281

Date Analyzed: 02/06/18 19:24 Lab File ID: 2018.02.06_537XX_055.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.05	User Assigned	krenns	02/07/18 11:48

Lab Sample ID: 320-35207-9 Client Sample ID: NAWC-011818-RW-032

Date Analyzed: 02/06/18 19:33 Lab File ID: 2018.02.06_537XX_057.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.05	User Assigned	krenns	02/07/18 11:49

Lab Sample ID: 320-35207-11 Client Sample ID: NAWC-011818-RW-038

Date Analyzed: 02/06/18 19:43 Lab File ID: 2018.02.06_537XX_059.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.04	Split Peak	krenns	02/07/18 13:44

LCMS MANUAL INTEGRATION SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1

SDG No.: _____

Instrument ID: A8_N Analysis Batch Number: 207294

Lab Sample ID: CCV 320-207294/20 CCVIS Client Sample ID: _____

Date Analyzed: 02/06/18 19:52 Lab File ID: 2018.02.06_537XX_061.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.04	User Assigned	krenns	02/07/18 11:50

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-35207-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
LC537-ICV_00028	01/05/18	08/02/17	MeOH/H2O, Lot 067374	10 mL	LC537-IS_00045	1000 uL	13C2-PFOA	10 ng/mL
.LC537-IS_00045	01/05/18	07/05/17	Methanol, Lot 090285	30000 uL	LCM2PFOA_00007	60 uL	13C2-PFOA	28.68 ng/mL
..LCM2PFOA_00007	02/12/21	Wellington Laboratories, Lot M2PFOA0216			(Purchased Reagent)		13C4 PFOS	0.1 ug/mL
..LCMPFOS_00019	08/03/21	Wellington Laboratories, Lot MPFOS0816			(Purchased Reagent)		13C4 PFOS	0.2868 ug/mL
LC537-ICV_00028	01/05/18	08/02/17	MeOH/H2O, Lot 067374	10 mL	LC537-SU_00046	1000 uL	13C2 PFDA	50 ug/mL
.LC537-SU_00046	01/05/18	07/05/17	Methanol, Lot 104453	30000 uL	LC537ICIM_00019	20 uL	13C2 PFHxA	47.8 ug/mL
..LCMPFDA_00012	09/30/21	Wellington Laboratories, Lot MPFDA0916			(Purchased Reagent)		13C2 PFDA	10 ng/mL
..LCMPFHxA_00013	04/08/21	Wellington Laboratories, Lot MPFHxA0416			(Purchased Reagent)		13C2 PFHxA	100.119 ng/mL
.LC537ICIM_00019	01/25/18	08/01/17	Methanol, Lot 090285	25 mL	LC537-PFBS2_00008	0.6 mL	Perfluorobutanesulfonic acid (PFBS)	9.99613 ng/mL
..LC537-PFBS2_00008	01/25/18	07/25/17	Methanol, Lot 090285	20 mL	LC537-PFHxA2_00011	0.061 mL	Perfluoroheptanoic acid (PFHpA)	20.0761 ng/mL
...LC537-PFHxA2_00011	09/08/22	Santa Cruz Biotechnology, Lot F0917			(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	20.1272 ng/mL
..LC537-PFHxA2_00011	01/25/18	07/25/17	Methanol, Lot 09092	31 mL	LC537-PFHxS2_00008	0.122 mL	Perfluorohexanesulfonic acid (PFHxS)	20.4843 ng/mL
...LC537-PFHxS2_00008	06/13/22	Afla Aesar, Lot 10200390			(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	19.698 ng/mL
..LC537-PFHxS2_00008	01/25/18	07/25/17	Methanol, Lot 090285	21 mL	LC537-PFNA2_00009	0.126 mL	Perfluorononanoic acid (PFNA)	20.2421 ug/mL
...LC537-PFNA2_00009	06/08/22	Santa Cruz Biotechnology, Lot G2516			(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	9.849 ug/mL
..LC537-PFNA2_00009	01/25/18	07/25/17	Methanol, Lot 090285	21 mL	LC537-PFOA2_00010	0.122 mL	Perfluorooctanoic acid (PFOA)	10.0636 ug/mL
...LC537-PFOA2_00010	06/14/22	Aldrich, Lot MKCC0699			(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	10.2421 ug/mL
..LC537-PFOA2_00010	01/25/18	08/01/17	Methanol, Lot 090285	20 mL	LC537-PFOS2_00010	0.124 mL	Perfluorooctanoic acid (PFOA)	9.849 ug/mL
...LC537-PFOS2_00010	06/09/22	Afla Aesar, Lot 10199078			(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	2085.82 ug/mL
..LC537-PFOA2_00002	06/09/22	Afla Aesar, Lot 10199078			(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	0.998 g/g
..LC537-PFOA2_00002	01/25/18	07/25/17	Methanol, Lot 09092	31 mL	LC537-PFHxA2_00002	0.0635 g	Perfluoroheptanoic acid (PFHpA)	1 g/g
...LC537-PFHxA2_00002	06/13/22	Afla Aesar, Lot 10200390			(Purchased Reagent)		Perfluoroheptanoic acid (PFHpA)	1 g/g
..LC537-PFHxA2_00002	01/25/18	07/25/17	Methanol, Lot 090285	21 mL	LC537-PFHxS2_00002	0.0475 g	Perfluorohexanesulfonic acid (PFHxS)	2056.98 ug/mL
...LC537-PFHxS2_00002	06/08/22	Santa Cruz Biotechnology, Lot G2516			(Purchased Reagent)		Perfluorohexanesulfonic acid (PFHxS)	0.9094 g/g
..LC537-PFNA2_00009	01/25/18	07/25/17	Methanol, Lot 090285	21 mL	LC537-PFNA2_00002	0.0421 g	Perfluorononanoic acid (PFNA)	1996.74 ug/mL
...LC537-PFNA2_00002	06/14/22	Aldrich, Lot MKCC0699			(Purchased Reagent)		Perfluorononanoic acid (PFNA)	0.996 g/g
..LC537-PFOA2_00010	01/25/18	08/01/17	Methanol, Lot 090285	20 mL	LC537-PFOA2_00002	0.0424 g	Perfluorooctanoic acid (PFOA)	2098.8 ug/mL
...LC537-PFOA2_00002	06/09/22	Afla Aesar, Lot 10199078			(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	0.99 g/g

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-35207-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
..LC537-PFOS2_00010	01/25/18	08/01/17	Methanol, Lot 090285	22 mL	LC537_PFOS2_00002	0.0561 g	Perfluorooctanesulfonic acid (PFOS)	1985.68 ug/mL
...LC537_PFOS2_00002	06/14/22		Sigma, Lot BCBQ0108V		(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	0.7787 g/g
LC537-IS_00057	07/30/18	01/30/18	Methanol, Lot 090285	30000 uL	LCM2PFOA_00007	60 uL	13C2-PFOA	0.1 ug/mL
					LCMPFOS_00021	180 uL	13C4 PFOS	0.2868 ug/mL
..LCM2PFOA_00007	02/12/21		Wellington Laboratories, Lot M2PFOA0216		(Purchased Reagent)		13C2-PFOA	50 ug/mL
..LCMPFOS_00021	12/12/21		Wellington Laboratories, Lot MPFOS1216		(Purchased Reagent)		13C4 PFOS	47.8 ug/mL
LC537-L1_00020	02/04/18	08/14/17	MeOH/H2O, Lot 090285	5 mL	LC537-IS_00048	500 uL	13C2-PFOA	10 ng/mL
							13C4 PFOS	28.68 ng/mL
					LC537-MSP_00029	60 uL	Perfluorobutanesulfonic acid (PFBS)	9.0018 ng/mL
							Perfluoroheptanoic acid (PFHpA)	1.00036 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	3.00103 ng/mL
							Perfluorononanoic acid (PFNA)	2.0006 ng/mL
							Perfluorooctanoic acid (PFOA)	2.00191 ng/mL
							Perfluorooctanesulfonic acid (PFOS)	4.00146 ng/mL
					LC537-SU_00049	500 uL	13C2 PFDA	10 ng/mL
							13C2 PFHxA	10 ng/mL
..LC537-IS_00048	02/04/18	08/04/17	Methanol, Lot 090285	30000 uL	LCM2PFOA_00007	60 uL	13C2-PFOA	0.1 ug/mL
					LCMPFOS_00021	180 uL	13C4 PFOS	0.2868 ug/mL
..LCM2PFOA_00007	02/12/21		Wellington Laboratories, Lot M2PFOA0216		(Purchased Reagent)		13C2-PFOA	50 ug/mL
..LCMPFOS_00021	12/12/21		Wellington Laboratories, Lot MPFOS1216		(Purchased Reagent)		13C4 PFOS	47.8 ug/mL
..LC537-MSP_00029	02/10/18	08/10/17	Methanol, Lot 141039	20000 uL	LC537SPIM_00023	166.7 uL	Perfluorobutanesulfonic acid (PFBS)	750.15 ng/mL
							Perfluoroheptanoic acid (PFHpA)	83.3637 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	250.086 ng/mL
							Perfluorononanoic acid (PFNA)	166.716 ng/mL
							Perfluorooctanoic acid (PFOA)	166.826 ng/mL
							Perfluorooctanesulfonic acid (PFOS)	333.455 ng/mL
..LC537SPIM_00023	02/10/18	08/10/17	Methanol, Lot 104453	10000 uL	LC537-PFBS_00008	450 uL	Perfluorobutanesulfonic acid (PFBS)	90 ug/mL
					LC537-PFHpA_00015	100 uL	Perfluoroheptanoic acid (PFHpA)	10.0016 ug/mL
					LC537-PFHxS_00010	150 uL	Perfluorohexanesulfonic acid (PFHxS)	30.0043 ug/mL
					LC537-PFNA_00013	200 uL	Perfluorononanoic acid (PFNA)	20.002 ug/mL
					LC537-PFOA_00013	200 uL	Perfluorooctanoic acid (PFOA)	20.0151 ug/mL
					LC537-PFOS_00008	400 uL	Perfluorooctanesulfonic acid (PFOS)	40.0066 ug/mL
...LC537-PFBS_00008	02/10/18	08/10/17	Methanol, Lot 090285	49.6 mL	LC537_PFBS_00002	0.0992 g	Perfluorobutanesulfonic acid (PFBS)	2 mg/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-35207-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
....LC537_PFBs_00002	04/01/18		Sigma, Lot MKBP8842V			(Purchased Reagent)	Perfluorobutanesulfonic acid (PFBS)	1 g/g
...LC537-PFHpA_00015	02/10/18	08/10/17	Methanol, Lot 090285	48.7 mL	LC537_PFHpA_00002	0.0492 g	Perfluoroheptanoic acid (PFHpA)	1.00016 mg/mL
....LC537_PFHpA_00002	04/01/18		Aldrich, Lot BCBM2579V			(Purchased Reagent)	Perfluoroheptanoic acid (PFHpA)	0.99 g/g
...LC537-PFHxS_00010	02/10/18	08/10/17	Methanol, Lot 090285	55.92 mL	LC537_PFHxS_00002	0.123 g	Perfluorohexanesulfonic acid (PFHxS)	2.00029 mg/mL
....LC537_PFHxS_00002	04/01/18		Sigma, Lot BCBL3545V			(Purchased Reagent)	Perfluorohexanesulfonic acid (PFHxS)	0.9094 g/g
..LC537-PFNA_00013	02/10/18	08/10/17	Methanol, Lot 090285	62.3 mL	LC537 PFNA_00002	0.0647 g	Perfluorononanoic acid (PFNA)	1000.1 ug/mL
....LC537 PFNA_00002	04/01/18		TCI America, Lot QN44F			(Purchased Reagent)	Perfluorononanoic acid (PFNA)	0.963 g/g
...LC537-PFOA_00013	02/10/18	08/10/17	Methanol, Lot 090285	22.76 mL	LC537 PFOA_00003	0.0228 g	Perfluorooctanoic acid (PFOA)	1.00076 mg/mL
....LC537 PFOA_00003	10/31/23		SIGMA ALDRICH, Lot BCBS1198V			(Purchased Reagent)	Perfluorooctanoic acid (PFOA)	0.999 g/g
...LC537-PFOS_00008	02/10/18	08/10/17	Methanol, Lot 090285	44.43 mL	LC537_PFOS_00003	0.0488 g	Perfluorooctanesulfonic acid (PFOS)	1.00016 mg/mL
....LC537_PFOS_00003	04/17/19		sigma alrich, Lot SZBE107XV			(Purchased Reagent)	Perfluorooctanesulfonic acid (PFOS)	0.9106 g/g
.LC537-SU_00049	02/04/18	08/04/17	Methanol, Lot 104453	30000 uL	LCMPFDA_00012	60 uL	13C2 PFDA	0.1 ug/mL
..LCMPFDA_00012	09/30/21		Wellington Laboratories, Lot MPFDA0916		LCMPFHxA_00013	60 uL	13C2 PFHxA	0.1 ug/mL
..LCMPFHxA_00013	04/08/21		Wellington Laboratories, Lot MPFHxA0416			(Purchased Reagent)	13C2 PFDA	50 ug/mL
						(Purchased Reagent)	13C2 PFHxA	50 ug/mL
LC537-L2_00020	02/04/18	08/14/17	MeOH/H2O, Lot 090285	5 mL	LC537-HSP_00025	80 uL	Perfluorobutanesulfonic acid (PFBS)	20.0016 ng/mL
							Perfluoroheptanoic acid (PFHpA)	2.22277 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	6.66817 ng/mL
							Perfluorononanoic acid (PFNA)	4.44524 ng/mL
							Perfluorooctanoic acid (PFOA)	4.44816 ng/mL
							Perfluorooctanesulfonic acid (PFOS)	8.89106 ng/mL
					LC537-IS_00048	500 uL	13C2-PFOA	10 ng/mL
							13C4 PFOS	28.68 ng/mL
					LC537-SU_00049	500 uL	13C2 PFDA	10 ng/mL
							13C2 PFHxA	10 ng/mL
.LC537-HSP_00025	02/10/18	08/10/17	Methanol, Lot 141039	20000 uL	LC537SPIM_00023	277.8 uL	Perfluorobutanesulfonic acid (PFBS)	1250.1 ng/mL
							Perfluoroheptanoic acid (PFHpA)	138.923 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	416.76 ng/mL
							Perfluorononanoic acid (PFNA)	277.827 ng/mL
							Perfluorooctanoic acid (PFOA)	278.01 ng/mL
							Perfluorooctanesulfonic acid (PFOS)	555.691 ng/mL
..LC537SPIM_00023	02/10/18	08/10/17	Methanol, Lot 104453	10000 uL	LC537-PFBS_00008	450 uL	Perfluorobutanesulfonic acid (PFBS)	90 ug/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-35207-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
					LC537-PFHpA_00015	100 uL	Perfluoroheptanoic acid (PFHpA)	10.0016 ug/mL
					LC537-PFHxS_00010	150 uL	Perfluorohexanesulfonic acid (PFHxS)	30.0043 ug/mL
					LC537-PFNA_00013	200 uL	Perfluorononanoic acid (PFNA)	20.002 ug/mL
					LC537-PFOA_00013	200 uL	Perfluorooctanoic acid (PFOA)	20.0151 ug/mL
					LC537-PFOS_00008	400 uL	Perfluorooctanesulfonic acid (PFOS)	40.0066 ug/mL
...LC537-PFBS_00008	02/10/18	08/10/17	Methanol, Lot 090285	49.6 mL	LC537_PFBS_00002	0.0992 g	Perfluorobutanesulfonic acid (PFBS)	2 mg/mL
....LC537_PFBS_00002	04/01/18	Sigma, Lot MKBP8842V			(Purchased Reagent)		Perfluorobutanesulfonic acid (PFBS)	1 g/g
...LC537-PFHpA_00015	02/10/18	08/10/17	Methanol, Lot 090285	48.7 mL	LC537_PFHpA_00002	0.0492 g	Perfluoroheptanoic acid (PFHpA)	1.00016 mg/mL
....LC537_PFHpA_00002	04/01/18	Aldrich, Lot BCM2579V			(Purchased Reagent)		Perfluoroheptanoic acid (PFHpA)	0.99 g/g
...LC537-PFHxS_00010	02/10/18	08/10/17	Methanol, Lot 090285	55.92 mL	LC537_PFHxS_00002	0.123 g	Perfluorohexanesulfonic acid (PFHxS)	2.00029 mg/mL
....LC537_PFHxS_00002	04/01/18	Sigma, Lot BCBL3545V			(Purchased Reagent)		Perfluorohexanesulfonic acid (PFHxS)	0.9094 g/g
...LC537-PFNA_00013	02/10/18	08/10/17	Methanol, Lot 090285	62.3 mL	LC537_PFNA_00002	0.0647 g	Perfluorononanoic acid (PFNA)	1000.1 ug/mL
....LC537_PFNA_00002	04/01/18	TCI America, Lot QN44F			(Purchased Reagent)		Perfluorononanoic acid (PFNA)	0.963 g/g
...LC537-PFOA_00013	02/10/18	08/10/17	Methanol, Lot 090285	22.76 mL	LC537_PFOA_00003	0.0228 g	Perfluorooctanoic acid (PFOA)	1.00076 mg/mL
....LC537_PFOA_00003	10/31/23	SIGMA ALDRICH, Lot BCBS1198V			(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	0.999 g/g
...LC537-PFOS_00008	02/10/18	08/10/17	Methanol, Lot 090285	44.43 mL	LC537_PFOS_00003	0.0488 g	Perfluorooctanesulfonic acid (PFOS)	1.00016 mg/mL
....LC537_PFOS_00003	04/17/19	sigma alrich, Lot SZBE107XV			(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	0.9106 g/g
.LC537-IS_00048	02/04/18	08/04/17	Methanol, Lot 090285	30000 uL	LCM2PFOA_00007	60 uL	13C2-PFOA	0.1 ug/mL
..LCM2PFOA_00007	02/12/21	Wellington Laboratories, Lot M2PFOA0216			LCMPFOS_00021	180 uL	13C4 PFOS	0.2868 ug/mL
..LCMPFOS_00021	12/12/21	Wellington Laboratories, Lot MPFOS1216			(Purchased Reagent)		13C2-PFOA	50 ug/mL
.LC537-SU_00049	02/04/18	08/04/17	Methanol, Lot 104453	30000 uL	LCMPFDA_00012	60 uL	13C4 PFOS	47.8 ug/mL
..LCMPFDA_00012	09/30/21	Wellington Laboratories, Lot MPFDA0916			LCMPFHxA_00013	60 uL	13C2 PFDA	0.1 ug/mL
..LCMPFHxA_00013	04/08/21	Wellington Laboratories, Lot MPFHxA0416			(Purchased Reagent)		13C2 PFDA	50 ug/mL
..LCMPFHxA_00013	04/08/21	Wellington Laboratories, Lot MPFHxA0416			(Purchased Reagent)		13C2 PFHxA	50 ug/mL
LC537-L2_00021	04/01/18	02/05/18	MeOH/H2O, Lot 090285	20 mL	LC537-IS_00059	2 mL	13C2-PFOA	10 ng/mL
.LC537-IS_00059	07/30/18	01/30/18	Methanol, Lot 090285	30000 uL	LCM2PFOA_00007	60 uL	13C4 PFOS	28.68 ng/mL
..LCM2PFOA_00007	02/12/21	Wellington Laboratories, Lot M2PFOA0216			LCMPFOS_00021	180 uL	13C2-PFOA	0.1 ug/mL
..LCMPFOS_00021	12/12/21	Wellington Laboratories, Lot MPFOS1216			(Purchased Reagent)		13C4 PFOS	0.2868 ug/mL
LC537-L2_00021	04/01/18	02/05/18	MeOH/H2O, Lot 090285	20 mL	LC537-HSP_00027	320 uL	Perfluorobutanesulfonic acid (PFBS)	20.0016 ng/mL
							Perfluoroheptanoic acid (PFHpA)	2.22264 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	6.66884 ng/mL
							Perfluorononanoic acid (PFNA)	4.44587 ng/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-35207-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
							Perfluorooctanoic acid (PFOA)	4.469 ng/mL
							Perfluorooctanesulfonic acid (PFOS)	8.92684 ng/mL
					LC537-SU_00059	2 mL	13C2 PFDA	10 ng/mL
							13C2 PFHxA	10 ng/mL
.LC537-HSP_00027	04/01/18	01/30/18	Methanol, Lot 141039	40000 uL	LC537SPIM_00026	555.6 uL	Perfluorobutanesulfonic acid (PFBS)	1250.1 ng/mL
							Perfluoroheptanoic acid (PFHpA)	138.915 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	416.802 ng/mL
							Perfluorononanoic acid (PFNA)	277.867 ng/mL
							Perfluorooctanoic acid (PFOA)	279.313 ng/mL
							Perfluorooctanesulfonic acid (PFOS)	557.928 ng/mL
..LC537SPIM_00026	04/01/18	01/30/18	Methanol, Lot 104453	20000 uL	LC537-PFBS_00009	900 uL	Perfluorobutanesulfonic acid (PFBS)	90 ug/mL
					LC537-PFHpA_00016	100 uL	Perfluoroheptanoic acid (PFHpA)	10.0011 ug/mL
					LC537-PFHxS_00011	300 uL	Perfluorohexanesulfonic acid (PFHxS)	30.0074 ug/mL
					LC537-PFNA_00014	400 uL	Perfluorononanoic acid (PFNA)	20.0048 ug/mL
					LC537-PFOA_00015	400 uL	Perfluorooctanoic acid (PFOA)	20.1089 ug/mL
					LC537-PFOS_00009	800 uL	Perfluorooctanesulfonic acid (PFOS)	40.1676 ug/mL
...LC537-PFBS_00009	04/01/18	01/30/18	Methanol, Lot 090285	48.7 mL	LC537_PFBS_00002	0.0974 g	Perfluorobutanesulfonic acid (PFBS)	2 mg/mL
....LC537_PFBS_00002	04/01/18		Sigma, Lot MKBP8842V		(Purchased Reagent)		Perfluorobutanesulfonic acid (PFBS)	1 g/g
...LC537-PFHpA_00016	04/01/18	01/30/18	Methanol, Lot 090285	59.74 mL	LC537_PFHpA_00002	0.1207 g	Perfluoroheptanoic acid (PFHpA)	2.00022 mg/mL
....LC537_PFHpA_00002	04/01/18		Aldrich, Lot BCBM2579V		(Purchased Reagent)		Perfluoroheptanoic acid (PFHpA)	0.99 g/g
...LC537-PFHxS_00011	04/01/18	01/30/18	Methanol, Lot 090285	38.64 mL	LC537_PFHxS_00002	0.085 g	Perfluorohexanesulfonic acid (PFHxS)	2.00049 mg/mL
....LC537_PFHxS_00002	04/01/18		Sigma, Lot BCBL3545V		(Purchased Reagent)		Perfluorohexanesulfonic acid (PFHxS)	0.9094 g/g
...LC537-PFNA_00014	04/01/18	01/30/18	Methanol, Lot 090285	62.58 mL	LC537 PFNA_00002	0.065 g	Perfluorononanoic acid (PFNA)	1000.24 ug/mL
....LC537 PFNA_00002	04/01/18		TCI America, Lot QN44F		(Purchased Reagent)		Perfluorononanoic acid (PFNA)	0.963 g/g
...LC537-PFOA_00015	07/30/18	01/30/18	Methanol, Lot 090285	31 mL	LC537 PFOA_00003	0.0312 g	Perfluorooctanoic acid (PFOA)	1.00545 mg/mL
....LC537 PFOA_00003	10/31/23		SIGMA ALDRICH, Lot BCBS1198V		(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	0.999 g/g
...LC537-PFOS_00009	07/30/18	01/30/18	Methanol, Lot 090285	36 mL	LC537_PFOS_00003	0.0397 g	Perfluorooctanesulfonic acid (PFOS)	1.00419 mg/mL
....LC537_PFOS_00003	04/17/19		sigma alrich, Lot SZBE107XV		(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	0.9106 g/g
.LC537-SU_00059	07/30/18	01/30/18	Methanol, Lot 104453	30000 uL	LCMPFDA_00012	60 uL	13C2 PFDA	0.1 ug/mL
					LCMPFHxA_00015	60 uL	13C2 PFHxA	0.1 ug/mL
..LCMPFDA_00012	09/30/21		Wellington Laboratories, Lot MPFDA0916		(Purchased Reagent)		13C2 PFDA	50 ug/mL
..LCMPFHxA_00015	11/22/21		Wellington Laboratories, Lot MPFHxA1116		(Purchased Reagent)		13C2 PFHxA	50 ug/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-35207-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration		
					Reagent ID	Volume Added				
LC537-L3_00023	02/04/18	08/14/17	MeOH/H2O, Lot 090285	5 mL	LC537-HSP_00025	180 uL	Perfluorobutanesulfonic acid (PFBS)	45.0036 ng/mL		
							Perfluoroheptanoic acid (PFHpA)	5.00122 ng/mL		
							Perfluorohexanesulfonic acid (PFHxS)	15.0034 ng/mL		
							Perfluorononanoic acid (PFNA)	10.0018 ng/mL		
							Perfluorooctanoic acid (PFOA)	10.0084 ng/mL		
					Perfluorooctanesulfonic acid (PFOS)	20.0049 ng/mL				
					LC537-IS_00048	500 uL	13C2-PFOA	10 ng/mL		
LC537-SU_00049	500 uL	13C2 PFDA	10 ng/mL							
.LC537-HSP_00025	02/10/18	08/10/17	Methanol, Lot 141039	20000 uL	LC537SPIM_00023	277.8 uL	Perfluorobutanesulfonic acid (PFBS)	1250.1 ng/mL		
							Perfluoroheptanoic acid (PFHpA)	138.923 ng/mL		
							Perfluorohexanesulfonic acid (PFHxS)	416.76 ng/mL		
							Perfluorononanoic acid (PFNA)	277.827 ng/mL		
							Perfluorooctanoic acid (PFOA)	278.01 ng/mL		
Perfluorooctanesulfonic acid (PFOS)	555.691 ng/mL									
..LC537SPIM_00023	02/10/18	08/10/17	Methanol, Lot 104453	10000 uL	LC537-PFBS_00008	450 uL	Perfluorobutanesulfonic acid (PFBS)	90 ug/mL		
							LC537-PFHpA_00015	100 uL	Perfluoroheptanoic acid (PFHpA)	10.0016 ug/mL
							LC537-PFHxS_00010	150 uL	Perfluorohexanesulfonic acid (PFHxS)	30.0043 ug/mL
							LC537-PFNA_00013	200 uL	Perfluorononanoic acid (PFNA)	20.002 ug/mL
							LC537-PFOA_00013	200 uL	Perfluorooctanoic acid (PFOA)	20.0151 ug/mL
							LC537-PFOS_00008	400 uL	Perfluorooctanesulfonic acid (PFOS)	40.0066 ug/mL
...LC537-PFBS_00008	02/10/18	08/10/17	Methanol, Lot 090285	49.6 mL	LC537_PFBS_00002	0.0992 g	Perfluorobutanesulfonic acid (PFBS)	2 mg/mL		
....LC537_PFBS_00002	04/01/18	Sigma, Lot MKBP8842V			(Purchased Reagent)		Perfluorobutanesulfonic acid (PFBS)	1 g/g		
...LC537-PFHpA_00015	02/10/18	08/10/17	Methanol, Lot 090285	48.7 mL	LC537_PFHpA_00002	0.0492 g	Perfluoroheptanoic acid (PFHpA)	1.00016 mg/mL		
....LC537_PFHpA_00002	04/01/18	Aldrich, Lot BCBM2579V			(Purchased Reagent)		Perfluoroheptanoic acid (PFHpA)	0.99 g/g		
...LC537-PFHxS_00010	02/10/18	08/10/17	Methanol, Lot 090285	55.92 mL	LC537_PFHxS_00002	0.123 g	Perfluorohexanesulfonic acid (PFHxS)	2.00029 mg/mL		
....LC537_PFHxS_00002	04/01/18	Sigma, Lot BCBL3545V			(Purchased Reagent)		Perfluorohexanesulfonic acid (PFHxS)	0.9094 g/g		
...LC537-PFNA_00013	02/10/18	08/10/17	Methanol, Lot 090285	62.3 mL	LC537 PFNA_00002	0.0647 g	Perfluorononanoic acid (PFNA)	1000.1 ug/mL		
....LC537 PFNA_00002	04/01/18	TCI America, Lot QN44F			(Purchased Reagent)		Perfluorononanoic acid (PFNA)	0.963 g/g		
...LC537-PFOA_00013	02/10/18	08/10/17	Methanol, Lot 090285	22.76 mL	LC537 PFOA_00003	0.0228 g	Perfluorooctanoic acid (PFOA)	1.00076 mg/mL		
....LC537_PFOA_00003	10/31/23	SIGMA ALDRICH, Lot BCBS1198V			(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	0.999 g/g		

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-35207-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
...LC537-PFOS_00008	02/10/18	08/10/17	Methanol, Lot 090285	44.43 mL	LC537_PFOS_00003	0.0488 g	Perfluorooctanesulfonic acid (PFOS)	1.00016 mg/mL
....LC537_PFOS_00003	04/17/19	sigma alrich, Lot SZBE107XV			(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	0.9106 g/g
.LC537-IS_00048	02/04/18	08/04/17	Methanol, Lot 090285	30000 uL	LCM2PFOA 00007	60 uL	13C2-PFOA	0.1 ug/mL
					LCMPFOS 00021	180 uL	13C4 PFOS	0.2868 ug/mL
..LCM2PFOA 00007	02/12/21	Wellington Laboratories, Lot M2PFOA0216			(Purchased Reagent)		13C2-PFOA	50 ug/mL
..LCMPFOS 00021	12/12/21	Wellington Laboratories, Lot MPFOS1216			(Purchased Reagent)		13C4 PFOS	47.8 ug/mL
.LC537-SU_00049	02/04/18	08/04/17	Methanol, Lot 104453	30000 uL	LCMPFDA 00012	60 uL	13C2 PFDA	0.1 ug/mL
					LCMPFHxA 00013	60 uL	13C2 PFHxA	0.1 ug/mL
..LCMPFDA 00012	09/30/21	Wellington Laboratories, Lot MPFDA0916			(Purchased Reagent)		13C2 PFDA	50 ug/mL
..LCMPFHxA 00013	04/08/21	Wellington Laboratories, Lot MPFHxA0416			(Purchased Reagent)		13C2 PFHxA	50 ug/mL
LC537-L3_00024	04/01/18	02/05/18	MeOH/H2O, Lot 090285	20 mL	LC537-IS_00059	2 mL	13C2-PFOA	10 ng/mL
.LC537-IS_00059	07/30/18	01/30/18	Methanol, Lot 090285	30000 uL	LCM2PFOA 00007	60 uL	13C4 PFOS	28.68 ng/mL
					LCMPFOS 00021	180 uL	13C2-PFOA	0.1 ug/mL
..LCM2PFOA 00007	02/12/21	Wellington Laboratories, Lot M2PFOA0216			(Purchased Reagent)		13C4 PFOS	0.2868 ug/mL
..LCMPFOS 00021	12/12/21	Wellington Laboratories, Lot MPFOS1216			(Purchased Reagent)		13C2-PFOA	50 ug/mL
LC537-L3_00024	04/01/18	02/05/18	MeOH/H2O, Lot 090285	20 mL	LC537-HSP_00027	720 uL	Perfluorobutanesulfonic acid (PFBS)	45.0036 ng/mL
							Perfluoroheptanoic acid (PFHpA)	5.00094 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	15.0049 ng/mL
							Perfluorononanoic acid (PFNA)	10.0032 ng/mL
							Perfluorooctanoic acid (PFOA)	10.0553 ng/mL
							Perfluorooctanesulfonic acid (PFOS)	20.0854 ng/mL
					LC537-SU_00059	2 mL	13C2 PFDA	10 ng/mL
							13C2 PFHxA	10 ng/mL
.LC537-HSP_00027	04/01/18	01/30/18	Methanol, Lot 141039	40000 uL	LC537SPIM_00026	555.6 uL	Perfluorobutanesulfonic acid (PFBS)	1250.1 ng/mL
							Perfluoroheptanoic acid (PFHpA)	138.915 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	416.802 ng/mL
							Perfluorononanoic acid (PFNA)	277.867 ng/mL
							Perfluorooctanoic acid (PFOA)	279.313 ng/mL
							Perfluorooctanesulfonic acid (PFOS)	557.928 ng/mL
..LC537SPIM_00026	04/01/18	01/30/18	Methanol, Lot 104453	20000 uL	LC537-PFBS_00009	900 uL	Perfluorobutanesulfonic acid (PFBS)	90 ug/mL
					LC537-PFHpA_00016	100 uL	Perfluoroheptanoic acid (PFHpA)	10.0011 ug/mL
					LC537-PFHxS_00011	300 uL	Perfluorohexanesulfonic acid (PFHxS)	30.0074 ug/mL
					LC537-PFNA 00014	400 uL	Perfluorononanoic acid (PFNA)	20.0048 ug/mL
					LC537-PFOA_00015	400 uL	Perfluorooctanoic acid (PFOA)	20.1089 ug/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-35207-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
					LC537-PFOS_00009	800 uL	Perfluorooctanesulfonic acid (PFOS)	40.1676 ug/mL
...LC537-PFBS_00009	04/01/18	01/30/18	Methanol, Lot 090285	48.7 mL	LC537_PFBS_00002	0.0974 g	Perfluorobutanesulfonic acid (PFBS)	2 mg/mL
....LC537_PFBS_00002	04/01/18		Sigma, Lot MKBP8842V		(Purchased Reagent)		Perfluorobutanesulfonic acid (PFBS)	1 g/g
...LC537-PFHpA_00016	04/01/18	01/30/18	Methanol, Lot 090285	59.74 mL	LC537_PFHpA_00002	0.1207 g	Perfluoroheptanoic acid (PFHpA)	2.00022 mg/mL
....LC537_PFHpA_00002	04/01/18		Aldrich, Lot BCM2579V		(Purchased Reagent)		Perfluoroheptanoic acid (PFHpA)	0.99 g/g
...LC537-PFHxS_00011	04/01/18	01/30/18	Methanol, Lot 090285	38.64 mL	LC537_PFHxS_00002	0.085 g	Perfluorohexanesulfonic acid (PFHxS)	2.00049 mg/mL
....LC537_PFHxS_00002	04/01/18		Sigma, Lot BCBL3545V		(Purchased Reagent)		Perfluorohexanesulfonic acid (PFHxS)	0.9094 g/g
...LC537-PFNA_00014	04/01/18	01/30/18	Methanol, Lot 090285	62.58 mL	LC537 PFNA_00002	0.065 g	Perfluorononanoic acid (PFNA)	1000.24 ug/mL
....LC537 PFNA_00002	04/01/18		TCI America, Lot QN44F		(Purchased Reagent)		Perfluorononanoic acid (PFNA)	0.963 g/g
...LC537-PFOA_00015	07/30/18	01/30/18	Methanol, Lot 090285	31 mL	LC537 PFOA_00003	0.0312 g	Perfluorooctanoic acid (PFOA)	1.00545 mg/mL
....LC537 PFOA_00003	10/31/23		SIGMA ALDRICH, Lot BCBS1198V		(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	0.999 g/g
...LC537-PFOS_00009	07/30/18	01/30/18	Methanol, Lot 090285	36 mL	LC537_PFOS_00003	0.0397 g	Perfluorooctanesulfonic acid (PFOS)	1.00419 mg/mL
....LC537_PFOS_00003	04/17/19		sigma alrich, Lot SZBE107XV		(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	0.9106 g/g
.LC537-SU_00059	07/30/18	01/30/18	Methanol, Lot 104453	30000 uL	LCMPFDA_00012	60 uL	13C2 PFDA	0.1 ug/mL
					LCMPFHxA_00015	60 uL	13C2 PFHxA	0.1 ug/mL
..LCMPFDA_00012	09/30/21		Wellington Laboratories, Lot MPFDA0916		(Purchased Reagent)		13C2 PFDA	50 ug/mL
..LCMPFHxA_00015	11/22/21		Wellington Laboratories, Lot MPFHxA1116		(Purchased Reagent)		13C2 PFHxA	50 ug/mL
LC537-L4_00020	02/04/18	08/14/17	MeOH/H2O, Lot 090285	5 mL	LC537-HSP_00025	360 uL	Perfluorobutanesulfonic acid (PFBS)	90.0072 ng/mL
							Perfluoroheptanoic acid (PFHpA)	10.0024 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	30.0067 ng/mL
							Perfluorononanoic acid (PFNA)	20.0036 ng/mL
							Perfluorooctanoic acid (PFOA)	20.0167 ng/mL
							Perfluorooctanesulfonic acid (PFOS)	40.0098 ng/mL
LC537-IS_00048	500 uL	13C2-PFOA	10 ng/mL					
		13C4 PFOS	28.68 ng/mL					
LC537-SU_00049	500 uL	13C2 PFDA	10 ng/mL					
		13C2 PFHxA	10 ng/mL					
.LC537-HSP_00025	02/10/18	08/10/17	Methanol, Lot 141039	20000 uL	LC537SPIM_00023	277.8 uL	Perfluorobutanesulfonic acid (PFBS)	1250.1 ng/mL
							Perfluoroheptanoic acid (PFHpA)	138.923 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	416.76 ng/mL
							Perfluorononanoic acid (PFNA)	277.827 ng/mL
							Perfluorooctanoic acid (PFOA)	278.01 ng/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-35207-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
							Perfluorooctanesulfonic acid (PFOS)	555.691 ng/mL
..LC537SPIM_00023	02/10/18	08/10/17	Methanol, Lot 104453	10000 uL	LC537-PFBS_00008	450 uL	Perfluorobutanesulfonic acid (PFBS)	90 ug/mL
					LC537-PFHpA_00015	100 uL	Perfluoroheptanoic acid (PFHpA)	10.0016 ug/mL
					LC537-PFHxS_00010	150 uL	Perfluorohexanesulfonic acid (PFHxS)	30.0043 ug/mL
					LC537-PFNA_00013	200 uL	Perfluorononanoic acid (PFNA)	20.002 ug/mL
					LC537-PFOA_00013	200 uL	Perfluorooctanoic acid (PFOA)	20.0151 ug/mL
					LC537-PFOS_00008	400 uL	Perfluorooctanesulfonic acid (PFOS)	40.0066 ug/mL
...LC537-PFBS_00008	02/10/18	08/10/17	Methanol, Lot 090285	49.6 mL	LC537_PFBS_00002	0.0992 g	Perfluorobutanesulfonic acid (PFBS)	2 mg/mL
....LC537_PFBS_00002	04/01/18		Sigma, Lot MKBP8842V		(Purchased Reagent)		Perfluorobutanesulfonic acid (PFBS)	1 g/g
...LC537-PFHpA_00015	02/10/18	08/10/17	Methanol, Lot 090285	48.7 mL	LC537_PFHpA_00002	0.0492 g	Perfluoroheptanoic acid (PFHpA)	1.00016 mg/mL
....LC537_PFHpA_00002	04/01/18		Aldrich, Lot BCBM2579V		(Purchased Reagent)		Perfluoroheptanoic acid (PFHpA)	0.99 g/g
...LC537-PFHxS_00010	02/10/18	08/10/17	Methanol, Lot 090285	55.92 mL	LC537_PFHxS_00002	0.123 g	Perfluorohexanesulfonic acid (PFHxS)	2.00029 mg/mL
....LC537_PFHxS_00002	04/01/18		Sigma, Lot BCBL3545V		(Purchased Reagent)		Perfluorohexanesulfonic acid (PFHxS)	0.9094 g/g
...LC537-PFNA_00013	02/10/18	08/10/17	Methanol, Lot 090285	62.3 mL	LC537 PFNA_00002	0.0647 g	Perfluorononanoic acid (PFNA)	1000.1 ug/mL
....LC537 PFNA_00002	04/01/18		TCI America, Lot QN44F		(Purchased Reagent)		Perfluorononanoic acid (PFNA)	0.963 g/g
...LC537-PFOA_00013	02/10/18	08/10/17	Methanol, Lot 090285	22.76 mL	LC537 PFOA_00003	0.0228 g	Perfluorooctanoic acid (PFOA)	1.00076 mg/mL
....LC537 PFOA_00003	10/31/23		SIGMA ALDRICH, Lot BCBS1198V		(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	0.999 g/g
...LC537-PFOS_00008	02/10/18	08/10/17	Methanol, Lot 090285	44.43 mL	LC537_PFOS_00003	0.0488 g	Perfluorooctanesulfonic acid (PFOS)	1.00016 mg/mL
....LC537_PFOS_00003	04/17/19		sigma alrich, Lot SZBE107XV		(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	0.9106 g/g
.LC537-IS_00048	02/04/18	08/04/17	Methanol, Lot 090285	30000 uL	LCM2PFOA_00007	60 uL	13C2-PFOA	0.1 ug/mL
					LCMPFOS_00021	180 uL	13C4 PFOS	0.2868 ug/mL
..LCM2PFOA_00007	02/12/21		Wellington Laboratories, Lot M2PFOA0216		(Purchased Reagent)		13C2-PFOA	50 ug/mL
..LCMPFOS_00021	12/12/21		Wellington Laboratories, Lot MPFOS1216		(Purchased Reagent)		13C4 PFOS	47.8 ug/mL
.LC537-SU_00049	02/04/18	08/04/17	Methanol, Lot 104453	30000 uL	LCMPFDA_00012	60 uL	13C2 PFDA	0.1 ug/mL
					LCMPFHxA_00013	60 uL	13C2 PFHxA	0.1 ug/mL
..LCMPFDA_00012	09/30/21		Wellington Laboratories, Lot MPFDA0916		(Purchased Reagent)		13C2 PFDA	50 ug/mL
..LCMPFHxA_00013	04/08/21		Wellington Laboratories, Lot MPFHxA0416		(Purchased Reagent)		13C2 PFHxA	50 ug/mL
LC537-L5_00024	02/04/18	08/14/17	MeOH/H2O, Lot 090285	5 mL	LC537-HSP_00025	540 uL	Perfluorobutanesulfonic acid (PFBS)	135.011 ng/mL
							Perfluoroheptanoic acid (PFHpA)	15.0037 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	45.0101 ng/mL
							Perfluorononanoic acid (PFNA)	30.0053 ng/mL
							Perfluorooctanoic acid (PFOA)	30.0251 ng/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-35207-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
							Perfluorooctanesulfonic acid (PFOS)	60.0146 ng/mL
					LC537-IS_00048	500 uL	13C2-PFOA	10 ng/mL
							13C4 PFOS	28.68 ng/mL
					LC537-SU_00049	500 uL	13C2 PFDA	10 ng/mL
							13C2 PFHxA	10 ng/mL
.LC537-HSP_00025	02/10/18	08/10/17	Methanol, Lot 141039	20000 uL	LC537SPIM_00023	277.8 uL	Perfluorobutanesulfonic acid (PFBS)	1250.1 ng/mL
							Perfluoroheptanoic acid (PFHpA)	138.923 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	416.76 ng/mL
							Perfluorononanoic acid (PFNA)	277.827 ng/mL
							Perfluorooctanoic acid (PFOA)	278.01 ng/mL
							Perfluorooctanesulfonic acid (PFOS)	555.691 ng/mL
..LC537SPIM_00023	02/10/18	08/10/17	Methanol, Lot 104453	10000 uL	LC537-PFBS_00008	450 uL	Perfluorobutanesulfonic acid (PFBS)	90 ug/mL
					LC537-PFHpA_00015	100 uL	Perfluoroheptanoic acid (PFHpA)	10.0016 ug/mL
					LC537-PFHxS_00010	150 uL	Perfluorohexanesulfonic acid (PFHxS)	30.0043 ug/mL
					LC537-PFNA_00013	200 uL	Perfluorononanoic acid (PFNA)	20.002 ug/mL
					LC537-PFOA_00013	200 uL	Perfluorooctanoic acid (PFOA)	20.0151 ug/mL
					LC537-PFOS_00008	400 uL	Perfluorooctanesulfonic acid (PFOS)	40.0066 ug/mL
...LC537-PFBS_00008	02/10/18	08/10/17	Methanol, Lot 090285	49.6 mL	LC537_PFBS_00002	0.0992 g	Perfluorobutanesulfonic acid (PFBS)	2 mg/mL
....LC537_PFBS_00002	04/01/18		Sigma, Lot MKBP8842V		(Purchased Reagent)		Perfluorobutanesulfonic acid (PFBS)	1 g/g
..LC537-PFHpA_00015	02/10/18	08/10/17	Methanol, Lot 090285	48.7 mL	LC537_PFHpA_00002	0.0492 g	Perfluoroheptanoic acid (PFHpA)	1.00016 mg/mL
....LC537_PFHpA_00002	04/01/18		Aldrich, Lot BCM2579V		(Purchased Reagent)		Perfluoroheptanoic acid (PFHpA)	0.99 g/g
..LC537-PFHxS_00010	02/10/18	08/10/17	Methanol, Lot 090285	55.92 mL	LC537_PFHxS_00002	0.123 g	Perfluorohexanesulfonic acid (PFHxS)	2.00029 mg/mL
....LC537_PFHxS_00002	04/01/18		Sigma, Lot BCBL3545V		(Purchased Reagent)		Perfluorohexanesulfonic acid (PFHxS)	0.9094 g/g
...LC537-PFNA_00013	02/10/18	08/10/17	Methanol, Lot 090285	62.3 mL	LC537_PFNA_00002	0.0647 g	Perfluorononanoic acid (PFNA)	1000.1 ug/mL
....LC537 PFNA_00002	04/01/18		TCI America, Lot QN44F		(Purchased Reagent)		Perfluorononanoic acid (PFNA)	0.963 g/g
...LC537-PFOA_00013	02/10/18	08/10/17	Methanol, Lot 090285	22.76 mL	LC537_PFOA_00003	0.0228 g	Perfluorooctanoic acid (PFOA)	1.00076 mg/mL
....LC537 PFOA_00003	10/31/23		SIGMA ALDRICH, Lot BCBS1198V		(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	0.999 g/g
...LC537-PFOS_00008	02/10/18	08/10/17	Methanol, Lot 090285	44.43 mL	LC537_PFOS_00003	0.0488 g	Perfluorooctanesulfonic acid (PFOS)	1.00016 mg/mL
....LC537_PFOS_00003	04/17/19		sigma alrich, Lot SZBE107XV		(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	0.9106 g/g
.LC537-IS_00048	02/04/18	08/04/17	Methanol, Lot 090285	30000 uL	LCM2PFOA_00007	60 uL	13C2-PFOA	0.1 ug/mL
					LCMPFOS_00021	180 uL	13C4 PFOS	0.2868 ug/mL
..LCM2PFOA_00007	02/12/21		Wellington Laboratories, Lot M2PFOA0216		(Purchased Reagent)		13C2-PFOA	50 ug/mL
..LCMPFOS_00021	12/12/21		Wellington Laboratories, Lot MPFOS1216		(Purchased Reagent)		13C4 PFOS	47.8 ug/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-35207-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
.LC537-SU_00049	02/04/18	08/04/17	Methanol, Lot 104453	30000 uL	LCMPFDA_00012	60 uL	13C2 PFDA	0.1 ug/mL
					LCMPFHxA_00013	60 uL	13C2 PFHxA	0.1 ug/mL
..LCMPFDA_00012	09/30/21	Wellington Laboratories, Lot MPFDA0916			(Purchased Reagent)		13C2 PFDA	50 ug/mL
..LCMPFHxA_00013	04/08/21	Wellington Laboratories, Lot MPFHxA0416			(Purchased Reagent)		13C2 PFHxA	50 ug/mL
LC537-L5_00025	04/01/18	02/05/18	MeOH/H2O, Lot 090285	20 mL	LC537-IS_00059	2 mL	13C2-PFOA	10 ng/mL
							13C4 PFOS	28.68 ng/mL
.LC537-IS_00059	07/30/18	01/30/18	Methanol, Lot 090285	30000 uL	LCM2PFOA_00007	60 uL	13C2-PFOA	0.1 ug/mL
					LCMPFOS_00021	180 uL	13C4 PFOS	0.2868 ug/mL
..LCM2PFOA_00007	02/12/21	Wellington Laboratories, Lot M2PFOA0216			(Purchased Reagent)		13C2-PFOA	50 ug/mL
..LCMPFOS_00021	12/12/21	Wellington Laboratories, Lot MPFOS1216			(Purchased Reagent)		13C4 PFOS	47.8 ug/mL
LC537-L5_00025	04/01/18	02/05/18	MeOH/H2O, Lot 090285	20 mL	LC537-HSP_00027	2160 uL	Perfluorobutanesulfonic acid (PFBS)	135.011 ng/mL
							Perfluoroheptanoic acid (PFHpA)	15.0028 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	45.0147 ng/mL
							Perfluorononanoic acid (PFNA)	30.0096 ng/mL
							Perfluorooctanoic acid (PFOA)	30.1658 ng/mL
							Perfluorooctanesulfonic acid (PFOS)	60.2562 ng/mL
					LC537-SU_00059	2 mL	13C2 PFDA	10 ng/mL
							13C2 PFHxA	10 ng/mL
.LC537-HSP_00027	04/01/18	01/30/18	Methanol, Lot 141039	40000 uL	LC537SPIM_00026	555.6 uL	Perfluorobutanesulfonic acid (PFBS)	1250.1 ng/mL
							Perfluoroheptanoic acid (PFHpA)	138.915 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	416.802 ng/mL
							Perfluorononanoic acid (PFNA)	277.867 ng/mL
							Perfluorooctanoic acid (PFOA)	279.313 ng/mL
							Perfluorooctanesulfonic acid (PFOS)	557.928 ng/mL
..LC537SPIM_00026	04/01/18	01/30/18	Methanol, Lot 104453	20000 uL	LC537-PFBS_00009	900 uL	Perfluorobutanesulfonic acid (PFBS)	90 ug/mL
					LC537-PFHpA_00016	100 uL	Perfluoroheptanoic acid (PFHpA)	10.0011 ug/mL
					LC537-PFHxS_00011	300 uL	Perfluorohexanesulfonic acid (PFHxS)	30.0074 ug/mL
					LC537-PFNA_00014	400 uL	Perfluorononanoic acid (PFNA)	20.0048 ug/mL
					LC537-PFOA_00015	400 uL	Perfluorooctanoic acid (PFOA)	20.1089 ug/mL
					LC537-PFOS_00009	800 uL	Perfluorooctanesulfonic acid (PFOS)	40.1676 ug/mL
...LC537-PFBS_00009	04/01/18	01/30/18	Methanol, Lot 090285	48.7 mL	LC537_PFBS_00002	0.0974 g	Perfluorobutanesulfonic acid (PFBS)	2 mg/mL
....LC537_PFBS_00002	04/01/18	Sigma, Lot MKBP8842V			(Purchased Reagent)		Perfluorobutanesulfonic acid (PFBS)	1 g/g
..LC537-PFHpA_00016	04/01/18	01/30/18	Methanol, Lot 090285	59.74 mL	LC537_PFHpA_00002	0.1207 g	Perfluoroheptanoic acid (PFHpA)	2.00022 mg/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-35207-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
....LC537_PFHpA_00002	04/01/18		Aldrich, Lot BCM2579V		(Purchased Reagent)		Perfluoroheptanoic acid (PFHpA)	0.99 g/g
...LC537-PFHxS_00011	04/01/18	01/30/18	Methanol, Lot 090285	38.64 mL	LC537_PFHxS_00002	0.085 g	Perfluorohexanesulfonic acid (PFHxS)	2.00049 mg/mL
....LC537_PFHxS_00002	04/01/18		Sigma, Lot BCBL3545V		(Purchased Reagent)		Perfluorohexanesulfonic acid (PFHxS)	0.9094 g/g
...LC537-PFNA_00014	04/01/18	01/30/18	Methanol, Lot 090285	62.58 mL	LC537_PFNA_00002	0.065 g	Perfluorononanoic acid (PFNA)	1000.24 ug/mL
....LC537_PFNA_00002	04/01/18		TCI America, Lot QN44F		(Purchased Reagent)		Perfluorononanoic acid (PFNA)	0.963 g/g
...LC537-PFOA_00015	07/30/18	01/30/18	Methanol, Lot 090285	31 mL	LC537_PFOA_00003	0.0312 g	Perfluorooctanoic acid (PFOA)	1.00545 mg/mL
....LC537_PFOA_00003	10/31/23		SIGMA ALDRICH, Lot BCBS1198V		(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	0.999 g/g
...LC537-PFOS_00009	07/30/18	01/30/18	Methanol, Lot 090285	36 mL	LC537_PFOS_00003	0.0397 g	Perfluorooctanesulfonic acid (PFOS)	1.00419 mg/mL
....LC537_PFOS_00003	04/17/19		sigma alrich, Lot SZBE107XV		(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	0.9106 g/g
.LC537-SU_00059	07/30/18	01/30/18	Methanol, Lot 104453	30000 uL	LCMPFDA_00012	60 uL	13C2 PFDA	0.1 ug/mL
..LCMPFDA_00012	09/30/21		Wellington Laboratories, Lot MPFDA0916		LCMPFHxA_00015	60 uL	13C2 PFHxA	0.1 ug/mL
..LCMPFHxA_00015	11/22/21		Wellington Laboratories, Lot MPFHxA1116		(Purchased Reagent)		13C2 PFDA	50 ug/mL
					(Purchased Reagent)		13C2 PFHxA	50 ug/mL
LC537-L6_00020	02/04/18	08/14/17	MeOH/H2O, Lot 090285	5 mL	LC537-HSP_00025	720 uL	Perfluorobutanesulfonic acid (PFBS)	180.014 ng/mL
							Perfluoroheptanoic acid (PFHpA)	20.0049 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	60.0135 ng/mL
							Perfluorononanoic acid (PFNA)	40.0071 ng/mL
							Perfluorooctanoic acid (PFOA)	40.0334 ng/mL
							Perfluorooctanesulfonic acid (PFOS)	80.0195 ng/mL
					LC537-IS_00048	500 uL	13C2-PFOA	10 ng/mL
							13C4 PFOS	28.68 ng/mL
					LC537-SU_00049	500 uL	13C2 PFDA	10 ng/mL
							13C2 PFHxA	10 ng/mL
.LC537-HSP_00025	02/10/18	08/10/17	Methanol, Lot 141039	20000 uL	LC537SPIM_00023	277.8 uL	Perfluorobutanesulfonic acid (PFBS)	1250.1 ng/mL
							Perfluoroheptanoic acid (PFHpA)	138.923 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	416.76 ng/mL
							Perfluorononanoic acid (PFNA)	277.827 ng/mL
							Perfluorooctanoic acid (PFOA)	278.01 ng/mL
							Perfluorooctanesulfonic acid (PFOS)	555.691 ng/mL
..LC537SPIM_00023	02/10/18	08/10/17	Methanol, Lot 104453	10000 uL	LC537-PFBS_00008	450 uL	Perfluorobutanesulfonic acid (PFBS)	90 ug/mL
					LC537-PFHpA_00015	100 uL	Perfluoroheptanoic acid (PFHpA)	10.0016 ug/mL
					LC537-PFHxS_00010	150 uL	Perfluorohexanesulfonic acid (PFHxS)	30.0043 ug/mL
					LC537-PFNA_00013	200 uL	Perfluorononanoic acid (PFNA)	20.002 ug/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-35207-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
					LC537-PFOA_00013	200 uL	Perfluorooctanoic acid (PFOA)	20.0151 ug/mL
					LC537-PFOS_00008	400 uL	Perfluorooctanesulfonic acid (PFOS)	40.0066 ug/mL
...LC537-PFBS_00008	02/10/18	08/10/17	Methanol, Lot 090285	49.6 mL	LC537_PFBFS_00002	0.0992 g	Perfluorobutanesulfonic acid (PFBS)	2 mg/mL
....LC537_PFBFS_00002	04/01/18		Sigma, Lot MKBP8842V		(Purchased Reagent)		Perfluorobutanesulfonic acid (PFBS)	1 g/g
...LC537-PFHpA_00015	02/10/18	08/10/17	Methanol, Lot 090285	48.7 mL	LC537_PFHpA_00002	0.0492 g	Perfluoroheptanoic acid (PFHpA)	1.00016 mg/mL
....LC537_PFHpA_00002	04/01/18		Aldrich, Lot BCBM2579V		(Purchased Reagent)		Perfluoroheptanoic acid (PFHpA)	0.99 g/g
...LC537-PFHxS_00010	02/10/18	08/10/17	Methanol, Lot 090285	55.92 mL	LC537_PFHxS_00002	0.123 g	Perfluorohexanesulfonic acid (PFHxS)	2.00029 mg/mL
....LC537_PFHxS_00002	04/01/18		Sigma, Lot BCBL3545V		(Purchased Reagent)		Perfluorohexanesulfonic acid (PFHxS)	0.9094 g/g
...LC537-PFNA_00013	02/10/18	08/10/17	Methanol, Lot 090285	62.3 mL	LC537 PFNA_00002	0.0647 g	Perfluorononanoic acid (PFNA)	1000.1 ug/mL
....LC537 PFNA_00002	04/01/18		TCI America, Lot QN44F		(Purchased Reagent)		Perfluorononanoic acid (PFNA)	0.963 g/g
...LC537-PFOA_00013	02/10/18	08/10/17	Methanol, Lot 090285	22.76 mL	LC537 PFOA_00003	0.0228 g	Perfluorooctanoic acid (PFOA)	1.00076 mg/mL
....LC537 PFOA_00003	10/31/23		SIGMA ALDRICH, Lot BCBS1198V		(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	0.999 g/g
...LC537-PFOS_00008	02/10/18	08/10/17	Methanol, Lot 090285	44.43 mL	LC537_PFOS_00003	0.0488 g	Perfluorooctanesulfonic acid (PFOS)	1.00016 mg/mL
....LC537_PFOS_00003	04/17/19		sigma alrich, Lot SZBE107XV		(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	0.9106 g/g
.LC537-IS_00048	02/04/18	08/04/17	Methanol, Lot 090285	30000 uL	LCM2PFOA_00007	60 uL	13C2-PFOA	0.1 ug/mL
..LCM2PFOA_00007	02/12/21		Wellington Laboratories, Lot M2PFOA0216		(Purchased Reagent)		13C2-PFOA	50 ug/mL
..LCMPFOS_00021	12/12/21		Wellington Laboratories, Lot MPFOS1216		(Purchased Reagent)		13C4 PFOS	47.8 ug/mL
.LC537-SU_00049	02/04/18	08/04/17	Methanol, Lot 104453	30000 uL	LCMPFDA_00012	60 uL	13C2 PFDA	0.1 ug/mL
..LCMPFDA_00012	09/30/21		Wellington Laboratories, Lot MPFDA0916		(Purchased Reagent)		13C2 PFDA	50 ug/mL
..LCMPFHxA_00013	04/08/21		Wellington Laboratories, Lot MPFHxA0416		(Purchased Reagent)		13C2 PFHxA	50 ug/mL
LC537-LSP_00026	02/10/18	08/10/17	Methanol, Lot 090285	20000 uL	LC537SPIM_00023	50 uL	Perfluorobutane Sulfonate	225 ng/mL
							Perfluorobutanesulfonic acid (PFBS)	225 ng/mL
							Perfluoroheptanoic acid (PFHpA)	25.0041 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	75.0109 ng/mL
							Perfluorononanoic acid (PFNA)	50.0049 ng/mL
							Perfluorooctanoic acid (PFOA)	50.0378 ng/mL
							Perfluorooctanesulfonic acid (PFOS)	100.016 ng/mL
.LC537SPIM_00023	02/10/18	08/10/17	Methanol, Lot 104453	10000 uL	LC537-PFBS_00008	450 uL	Perfluorobutane Sulfonate	90 ug/mL
							Perfluorobutanesulfonic acid (PFBS)	90 ug/mL
					LC537-PFHpA_00015	100 uL	Perfluoroheptanoic acid (PFHpA)	10.0016 ug/mL
					LC537-PFHxS_00010	150 uL	Perfluorohexanesulfonic acid (PFHxS)	30.0043 ug/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-35207-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
					LC537-PFNA_00013	200 uL	Perfluorononanoic acid (PFNA)	20.002 ug/mL
					LC537-PFOA_00013	200 uL	Perfluorooctanoic acid (PFOA)	20.0151 ug/mL
					LC537-PFOS_00008	400 uL	Perfluorooctanesulfonic acid (PFOS)	40.0066 ug/mL
..LC537-PFBS_00008	02/10/18	08/10/17	Methanol, Lot 090285	49.6 mL	LC537_PFBS_00002	0.0992 g	Perfluorobutane Sulfonate	2 mg/mL
							Perfluorobutanesulfonic acid (PFBS)	2 mg/mL
...LC537_PFBS_00002	04/01/18	Sigma, Lot MKBP8842V			(Purchased Reagent)		Perfluorobutane Sulfonate	1 g/g
							Perfluorobutanesulfonic acid (PFBS)	1 g/g
..LC537-PFHpA_00015	02/10/18	08/10/17	Methanol, Lot 090285	48.7 mL	LC537_PFHpA_00002	0.0492 g	Perfluoroheptanoic acid (PFHpA)	1.00016 mg/mL
...LC537_PFHpA_00002	04/01/18	Aldrich, Lot BCBM2579V			(Purchased Reagent)		Perfluoroheptanoic acid (PFHpA)	0.99 g/g
..LC537-PFHxS_00010	02/10/18	08/10/17	Methanol, Lot 090285	55.92 mL	LC537_PFHxS_00002	0.123 g	Perfluorohexanesulfonic acid (PFHxS)	2.00029 mg/mL
...LC537_PFHxS_00002	04/01/18	Sigma, Lot BCBL3545V			(Purchased Reagent)		Perfluorohexanesulfonic acid (PFHxS)	0.9094 g/g
..LC537-PFNA_00013	02/10/18	08/10/17	Methanol, Lot 090285	62.3 mL	LC537_PFNA_00002	0.0647 g	Perfluorononanoic acid (PFNA)	1000.1 ug/mL
...LC537_PFNA_00002	04/01/18	TCI America, Lot QN44F			(Purchased Reagent)		Perfluorononanoic acid (PFNA)	0.963 g/g
..LC537-PFOA_00013	02/10/18	08/10/17	Methanol, Lot 090285	22.76 mL	LC537_PFOA_00003	0.0228 g	Perfluorooctanoic acid (PFOA)	1.00076 mg/mL
...LC537_PFOA_00003	10/31/23	SIGMA ALDRICH, Lot BCBS1198V			(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	0.999 g/g
..LC537-PFOS_00008	02/10/18	08/10/17	Methanol, Lot 090285	44.43 mL	LC537_PFOS_00003	0.0488 g	Perfluorooctanesulfonic acid (PFOS)	1.00016 mg/mL
...LC537_PFOS_00003	04/17/19	sigma alrich, Lot SZBE107XV			(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	0.9106 g/g
LC537-SU_00053	05/27/18	11/27/17	Methanol, Lot 104453	30000 uL	LCMPFDA_00012	60 uL	13C2 PFDA	0.1 ug/mL
					LCMPFHxA_00015	60 uL	13C2 PFHxA	0.1 ug/mL
.LCMPFDA_00012	09/30/21	Wellington Laboratories, Lot MPFDA0916			(Purchased Reagent)		13C2 PFDA	50 ug/mL
.LCMPFHxA_00015	11/22/21	Wellington Laboratories, Lot MPFHxA1116			(Purchased Reagent)		13C2 PFHxA	50 ug/mL

Reagent

LC537_PFB_00002

7: 4/1/15 SPV

3050 Spruce Street, Saint Louis, MO 63103, USA

Website: www.sigmaaldrich.com

Email USA: techserv@sial.com


Outside USA: eurtechserv@sial.com

Certificate of Analysis

Product Name:

Nonafluorobutane-1-sulfonic acid - 97%

Product Number: 562629
Batch Number: MKBP8842V
Brand: ALDRICH
CAS Number: 375-73-5
MDL Number: MFCD01320794
Formula: C4HF9O3S
Formula Weight: 300.10 g/mol
Storage Temperature: Store at 2 - 8 °C
Quality Release Date: 11 OCT 2013



PFBS

Test	Specification	Result
Appearance (Color)	Colorless	Colorless
Appearance (Form)	Liquid	Liquid
Infrared Spectrum	Conforms to Structure	Conforms
Fluorine NMR Spectrum	Conforms to Structure	Conforms
Purity (Titration by NaOH)	96.5 - 103.5 %	101.6 %


Jamie Gleason, Manager
 Quality Control
 Milwaukee, Wisconsin US

Sigma-Aldrich warrants, that at the time of the quality release or subsequent retest date this product conformed to the information contained in this publication. The current Specification sheet may be available at Sigma-Aldrich.com. For further inquiries, please contact Technical Service. Purchaser must determine the suitability of the product for its particular use. See reverse side of invoice or packing slip for additional terms and conditions of sale.

Reagent

LC537_PFB2_00002

F: 6.8.17 SW



CERTIFICATE OF ANALYSIS

The Power to Question

Catalog Number: sc-236187
Lot Number: F0917
Product Name: Nonafluorobutane-1-sulfonic acid
CAS Number: 375-73-5
Molecular Formula: $C_4HF_9O_3S$
Molecular Weight: 300.10

Test	Specification	Result
Appearance	Colorless liquid	Complies
Identification (19F-NMR)	Conforms to structure	Complies
Purity (Sodium Hydroxide Titration)	$\geq 97\%$	101.3%
Infrared Spectrum	Conforms to structure	Complies

Reagent

LC537_PFHpA_00002

R: 4/1/15 4V

Certificate of Analysis

Product Name: PERFLUOROHEPTANOIC ACID
 99 %
Product Number: 342041
Batch Number: BCBM2579V
Brand: Aldrich
CAS Number: 375-85-9
Formula: $CF_3(CF_2)_5CO_2H$
Formula Weight: 364.06
Quality Release Date: 06 DEC 2013
Recommended Retest Date: OCT 2018

PFHpA

TEST	SPECIFICATION	RESULT
APPEARANCE (COLOR)	COLORLESS OR WHITE	WHITE
APPEARANCE (FORM)	LIQUID OR SOLID	SOLID
TITRATION	98.5 - 101.5 %	99.8 %
TITRATION (METHOD)	-	BACK TITRATION
PURITY (GC AREA %)	≥ 98.5 %	99.5 %
INFRARED SPECTRUM	CONFORMS TO STRUCTURE	CONFORMS

Dr. Claudia Geitner
 Manager Quality Control
 Buchs, Switzerland

Sigma-Aldrich warrants that at the time of the quality release or subsequent retest date this product conformed to the information contained in this publication. The current specification sheet may be available at Sigma-Aldrich.com. For further inquiries, please contact Technical Service. Purchaser must determine the suitability of the product for its particular use. See reverse side of invoice or packing slip for additional terms and conditions of sale.

Reagent

LC537_PFHpA2_00002

Certificate of analysis

r:6.13.17 SW

Product No.: A12092
Product: Perfluoroheptanoic acid, 98+%
Lot No.: 10200390

PFHe A

Appearance: White fused solid
Water Content (Karl-Fischer): 0.30%
Melting Point: 32.0-34.3°C
Assay (Aqueous acid-base titration): 99.7%
Identification (FTIR): Conforms

This document has been electronically generated and does not require a signature.

Order our products online www.alfa.com

ThermoFisher
SCIENTIFIC

Reagent

LC537_PFHxS_00002

r: 4/1/15 stw

Certificate of Analysis

Product Name: TRIDECAFLUOROHEXANE-1-SULFONIC ACID POTASSIUM SALT
 >= 98.0 % T

Product Number: 50929

Batch Number: BCBL3545V

Brand: Aldrich

CAS Number: 3871-99-6

Formula: C₆F₁₃KO₃S

Formula Weight: 438.20

Quality Release Date: 20 JUN 2013

PFH₁₃S-K

TEST	SPECIFICATION	RESULT
APPEARANCE (COLOR)	WHITE TO FAINT BEIGE	WHITE
APPEARANCE (FORM)	POWDER OR CRYSTALS	POWDER
TITRATION (ION EXCHANGE)	≥ 98.0 %	99.5 %
INFRARED SPECTRUM	CONFORMS TO STRUCTURE	CONFORMS

Dr. Claudia Geitner
Manager Quality Control
Buchs, Switzerland

$$MW_{corr} = \frac{(k_{form}) - (k) + (H)}{438.20 (k_{form})} = \frac{(438.20 - 391.0 + 1.01)}{438.20 (k_{form})} = 0.91307 \text{ (anion form)}$$

$$Purity = 90.94 \% \text{ w/m.w correction}$$

stw 4/1/15

Sigma-Aldrich warrants that at the time of the quality release or subsequent retest date this product conformed to the information contained in this publication. The current specification sheet may be available at Sigma-Aldrich.com. For further inquiries, please contact Technical Service. Purchaser must determine the suitability of the product for its particular use. See reverse side of invoice or packing slip for additional terms and conditions of sale.

Reagent

LC537_PFHxS2_00002

n: 6-8-17 SKJ




The Future of Science

CERTIFICATE OF ANALYSIS

Catalog Number: sc-237289
 Lot Number: G2516
 Product Name: Tridecafluorohexane-1-sulfonic acid potassium salt
 CAS Number: 3871-99-6
 Molecular Formula: $C_6F_{13}KO_3S$
 Molecular Weight: 438.20

Test	Specification	Result
Appearance	White to faint beige powder or crystals	White powder
Identification (Infrared Spectrum)	Consistent with structure	Complies
Purity (Titration, Ion Exchange)	≥ 98.0%	100.4%

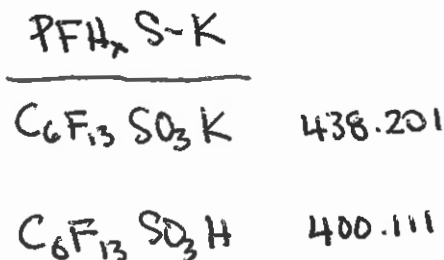

MW correction = $\frac{400.11}{438.201} = 0.91307$ PFH₁₃S
 CAS# 355-46-4

Purity $\frac{1}{9}$ MW correction = 90.9%

This document was produced electronically and is valid without a signature.

Reagent

LC537_PENA_00002

R: 4/1/15 SKV



Certificate of Analysis

Apr 2, 2015 (JST)

TOKYO CHEMICAL INDUSTRY CO.,LTD.
4-10-1 Nihonbashi-Honcho, Chuo-ku, Tokyo 103-0023 Japan

Chemical Name: Heptadecafluorononanoic Acid		
Product Number: H0843 CAS: 375-95-1	Lot: QN44F	

Tests	Results	Specifications
Purity(GC)	96.3 %	min. 95.0 %
Purity(Neutralization titration)	98.1 %	min. 95.0 %
Melting point	63.3 deg-C	62.0 to 67.0 deg-C

TCI Lot numbers are 4-5 characters in length.
Characters listed after the first 4-5 characters are control numbers for internal purpose only.

Customer service:
TCI AMERICA
Tel: +1-800-423-8616 / +1-503-283-1681
Fax: +1-888-520-1075 / +1-503-283-1987
E-mail: Sales-US@TCIchemicals.com

PFNA

Reagent

LC537_PFN2_00002

P: 6.14.17 SKW

3050 Spruce Street, Saint Louis, MO 63103, USA

Website: www.sigmaaldrich.com


Email USA: techserv@sial.com

Outside USA: eurtechserv@sial.com

Certificate of Analysis

Product Name:
Perfluorononanoic acid - 97%

Product Number: 394459
Batch Number: MKCC0699
Brand: ALDRICH
CAS Number: 375-95-1
MDL Number: MFCD00039605
Formula: C₉H_F17O₂
Formula Weight: 464.08 g/mol
Quality Release Date: 07 DEC 2016



Test	Specification	Result
Appearance (Color)	White to Off-White	White
Appearance (Form)	Powder or Crystals or Crystalline Chunk(s) or Granule or Flakes or Solid	Powder
Infrared Spectrum	Conforms to Structure	Conforms
GC (area %)	≥ 96.5 %	98.2 %

Michael Grady, Manager
Quality Control
Milwaukee, WI US

PFNA

Sigma-Aldrich warrants, that at the time of the quality release or subsequent retest date this product conformed to the information contained in this publication. The current Specification sheet may be available at Sigma-Aldrich.com. For further inquiries, please contact Technical Service. Purchaser must determine the suitability of the product for its particular use. See reverse side of Invoice or packing slip for additional terms and conditions of sale.

Reagent

LC537_PFOA_00003

T: 11/30/16 SKV
PFA

SIGMA-ALDRICH

3050 Spruce Street, Saint Louis, MO 63103 USA
Email USA: techserv@sial.com Outside USA: eurtechserv@sial.com

Certificate of Analysis

Product Name: PENTADECAFLUOROOCCTANOIC ACID
analytical standard
Product Number: 33824
Batch Number: BCBS1198V
Brand: Sigma-Aldrich
CAS Number: 335-67-1
Formula: $\text{CF}_3(\text{CF}_2)_6\text{COOH}$
Formula Weight: 414.07
Expiration Date: OCT 2023
Quality Release Date: 12 MAY 2016

TEST	SPECIFICATION	RESULT
PURITY (HPLC AREA %)	≥ 98.0%	100.0%
IDENTIFICATION (LC-MS)	IDENTITY CONFORMS	CONFORMS



Dr. Claudia Geitner
Manager Quality Control
Buchs, Switzerland

Sigma-Aldrich warrants that at the time of the quality release or subsequent retest date this product conformed to the information contained in this publication. The current specification sheet may be available at Sigma-Aldrich.com. For further inquiries, please contact Technical Service. Purchaser must determine the suitability of the product for its particular use. See reverse side of invoice or packing slip for additional terms and conditions of sale.

Reagent

LC537_PFOA2_00002

Certificate of analysis

P: 6/21/17 SW ✓

Product No.: L08862
Product: Perfluorooctanoic acid, 95%
Lot No.: 10199078

PFOA

Appearance: White powder
Water Content (Karl-Fischer): 1.30%
Melting Point: 47.6-54.0°C
Assay (Aqueous acid-base titration): 98.4%
Assay (GC Silyl Deriv): 97.2%

This document has been electronically generated and does not require a signature.

Order our products online www.alfa.com

ThermoFisher
SCIENTIFIC

Reagent

LC537_PFOs_00003

Reagent

LC537_PFOs2_00002

R: 6.14.17 SKV

Certificate of Analysis

Product Name: HEPTADECAFLUOROCTANESULFONIC ACID TETRAETHYLAMMONIUM SALT
 98 %
Product Number: 365289
Batch Number: BCBQ0108V
Brand: Aldrich
CAS Number: 56773-42-3
Formula: $CF_3(CF_2)_6CF_2SO_3N(C_2H_5)_4$
Formula Weight: 629.37
Quality Release Date: 11 JUN 2015


TEST	SPECIFICATION	RESULT
APPEARANCE (COLOR)	WHITE TO OFF WHITE	OFF-WHITE
APPEARANCE (FORM)	POWDER OR POWDER WITH CHUNK(S)	POWDER
CARBON CONTENT	29.77 % - 31.29 %	29.97 %
INFRARED SPECTRUM	CONFORMS TO STRUCTURE	CONFORMS

Claudia Geitner

Dr. Claudia Geitner
 Manager Quality Control
 Buchs, Switzerland

MW correction: $\frac{500.125}{629.37} = 0.7946$

Purity & MW correction = 77.87%



	$C_8F_{17}SO_3^+H$	$C_8H_{20}N$
C = 12.011	96.088	96.088
F = 18.998	322.966	—
S = 32.066	32.066	—
O = 16.000	47.947	20.60
H = 1.008	1.008	14.007
N = 14.007	—	14.007
	<hr/>	<hr/>
	500.125	130.255

Reagent

LCM2PFOA_00007

P: 5/11/17 SKV




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: M2PFOA
COMPOUND: Perfluoro-n-[1,2-¹³C₂]octanoic acid

LOT NUMBER: M2PFOA0216

STRUCTURE:
CAS #: Not available



MOLECULAR FORMULA: ¹³C₂¹²C₆HF₁₆O₂
CONCENTRATION: 50 ± 2.5 µg/ml

MOLECULAR WEIGHT: 416.05
SOLVENT(S): Methanol
Water (<1%)

CHEMICAL PURITY: >98%
LAST TESTED: (mm/dd/yyyy) 02/12/2016
EXPIRY DATE: (mm/dd/yyyy) 02/12/2021

ISOTOPIC PURITY: ≥99% ¹³C
(1,2-¹³C₂)

RECOMMENDED STORAGE: Store ampoule in a cool, dark place

DOCUMENTATION/ DATA ATTACHED:

- Figure 1: LC/MS Data (TIC and Mass Spectrum)
- Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent conversion of the carboxylic acid to the methyl ester.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By:
B.G. Chittim

Date: 02/24/2016
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:


Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: M2PFOA; LC/MS Data (TIC and Mass Spectrum)



Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm


Mobile phase: Gradient
Start: 50% (80:20 MeOH:ACN) / 50% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 90% organic over 7.5 min and hold for 1.5 min
before returning to initial conditions in 0.5 min.
Time: 10 min

Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (150 - 850 amu)
Source: Electrospray (negative)
Capillary Voltage (kV) = 3.00
Cone Voltage (V) = 15.00
Cone Gas Flow (l/hr) = 100
Desolvation Gas Flow (l/hr) = 750

Figure 2: M2PFOA; LC/MS/MS Data (Selected MRM Transitions)



Conditions for Figure 2:

Injection: Direct loop injection
10 μl (500 ng/ml M2PFOA)

Mobile phase: Isocratic 80% MeOH / 20% H₂O

Flow: 300 $\mu\text{l}/\text{min}$

MS Parameters

Collision Gas (mbar) = 3.39e-3
Collision Energy (eV) = 10

Reagent

LCMPFDA_00012

R: SBC 12/21/16



814255

ID: LCMPPFDA_00012

Exp: 09/30/21 Prpd: SBC

13C2-Perfluorodecanoic acid



WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE:

MPFDA

LOT NUMBER:

MPFDA0916

COMPOUND:

Perfluoro-n-[1,2-¹³C₂]decanoic acid

STRUCTURE:

CAS #:

Not available



MOLECULAR FORMULA:

¹³C₂¹²C₈HF₁₉O₂

MOLECULAR WEIGHT:

516.07

CONCENTRATION:

50 ± 2.5 µg/ml

SOLVENT(S):

Methanol
Water (<1%)

CHEMICAL PURITY:

>98%

ISOTOPIC PURITY:

≥99% ¹³C
(1,2-¹³C₂)

LAST TESTED: (mm/dd/yyyy)

09/30/2016

EXPIRY DATE: (mm/dd/yyyy)

09/30/2021

RECOMMENDED STORAGE:

Store ampoule in a cool, dark place

DOCUMENTATION/ DATA ATTACHED:

Figure 1: LC/MS Data (TIC and Mass Spectrum)

Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent conversion of the carboxylic acid to the methyl ester.
- Contains < 0.1% of ¹³C₁-PFNA.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By:

B.G. Chríttim

Date: 10/07/2016

(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: MPFDA; LC/MS Data (TIC and Mass Spectrum)



Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions


Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm
Mobile phase: Gradient
Start: 50% (80:20 MeOH:ACN) / 50% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 90% organic over 7 min and hold for 1.5 min
before returning to initial conditions in 0.5 min.
Time: 10 min

Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (225 - 850 amu)
Source: Electrospray (negative)
Capillary Voltage (kV) = 2.00
Cone Voltage (V) = 15.00
Cone Gas Flow (l/hr) = 50
Desolvation Gas Flow (l/hr) = 750

Figure 2: MPFDA; LC/MS/MS Data (Selected MRM Transitions)



Conditions for Figure 2:

Injection: Direct loop injection
10 μ l (500 ng/ml MPFDA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
(both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.31e-3
Collision Energy (eV) = 13

Reagent

LCMPFHxA_00013

R: SBC 12/21/16



814258
ID: LCMPFHxA_00013
Exp: 04/08/21 Prgd: SBC
13C2-Perfluorohexanoic ac



WELLINGTON LABORATORIES


CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: MPFHxA
COMPOUND: Perfluoro-n-[1,2-¹³C₂]hexanoic acid

LOT NUMBER: MPFHxA0416

STRUCTURE:

CAS #: Not available



MOLECULAR FORMULA: ¹³C₂¹²C₄HF₁₁O₂
CONCENTRATION: 50 ± 2.5 µg/ml

MOLECULAR WEIGHT: 316.04
SOLVENT(S): Methanol
Water (<1%)

CHEMICAL PURITY: >98%
LAST TESTED: (mm/dd/yyyy) 04/08/2016

ISOTOPIC PURITY: ≥99%¹³C
(1,2-¹³C₂)

EXPIRY DATE: (mm/dd/yyyy) 04/08/2021

RECOMMENDED STORAGE: Store ampoule in a cool, dark place

DOCUMENTATION/ DATA ATTACHED:

- Figure 1: LC/MS Data (TIC and Mass Spectrum)
- Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent conversion of the carboxylic acid to the methyl ester.
- Contains < 0.1% of perfluoro-n-hexanoic acid and ~ 0.3% of perfluoro-n-octanoic acid.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By:
B.G. Chittim

Date: 04/29/2016
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: MPFHxA; LC/MS Data (TIC and Mass Spectrum)

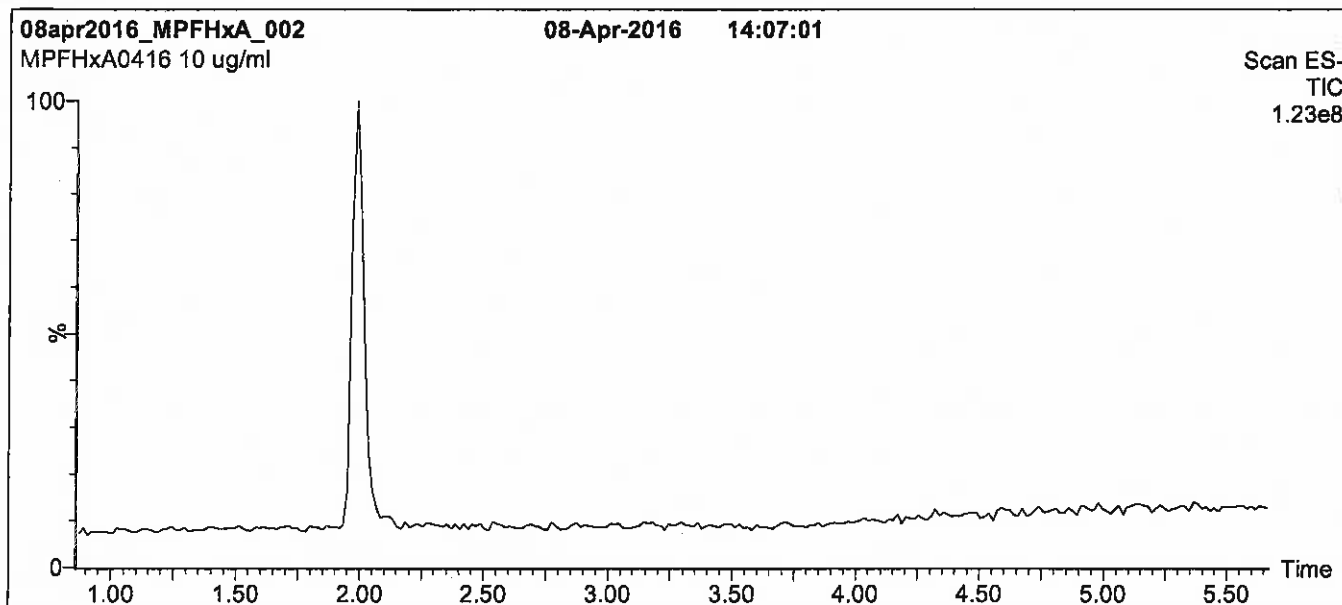

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
 1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
 Start: 50% (80:20 MeOH:ACN) / 50% H₂O
 (both with 10 mM NH₄OAc buffer)
 Ramp to 90% organic over 7.5 min and hold for 1.5 min
 before returning to initial conditions over 0.5 min.
 Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (150 - 850 amu)

Source: Electrospray (negative)
 Capillary Voltage (kV) = 2.00
 Cone Voltage (V) = 15.00
 Cone Gas Flow (l/hr) = 100
 Desolvation Gas Flow (l/hr) = 750

Figure 2: MPFHxA; LC/MS/MS Data (Selected MRM Transitions)

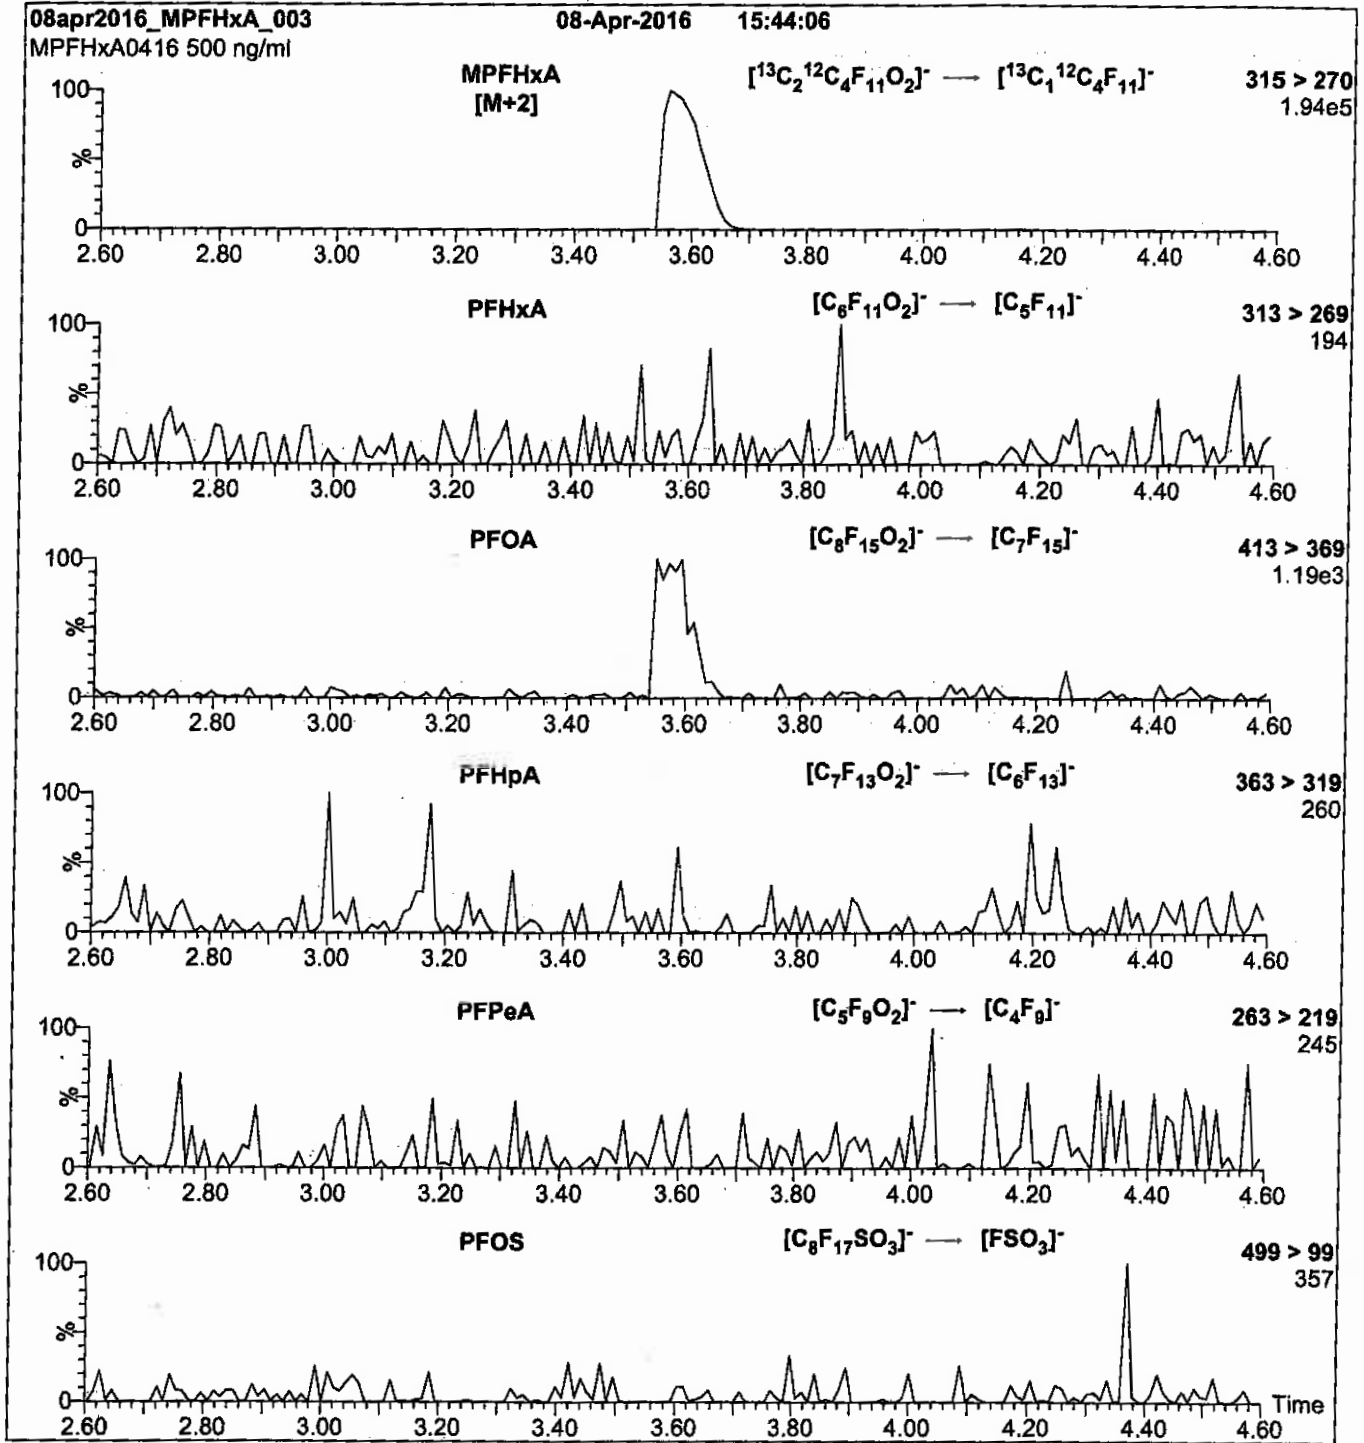

Conditions for Figure 2:

Injection: Direct loop injection
10 μ l (500 ng/ml MPFHxA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
(both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.39e-3
Collision Energy (eV) = 10

Reagent

LCMPFHxA_00015

r: 5/10/17 skd




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: MPFHxA
COMPOUND: Perfluoro-n-[1,2-¹³C₂]hexanoic acid

LOT NUMBER: MPFHxA1116

STRUCTURE: **CAS #:** Not available

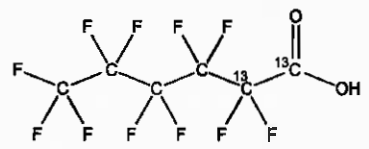

MOLECULAR FORMULA: ¹³C₂¹²C₄HF₁₁O₂
CONCENTRATION: 50 ± 2.5 µg/ml

MOLECULAR WEIGHT: 316.04
SOLVENT(S): Methanol
Water (<1%)

CHEMICAL PURITY: >98%
LAST TESTED: (mm/dd/yyyy) 11/22/2016
EXPIRY DATE: (mm/dd/yyyy) 11/22/2021

ISOTOPIC PURITY: ≥99% ¹³C
(1,2-¹³C₂)

RECOMMENDED STORAGE: Store ampoule in a cool, dark place

DOCUMENTATION/ DATA ATTACHED:

- Figure 1: LC/MS Data (TIC and Mass Spectrum)
- Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent conversion of the carboxylic acid to the methyl ester.
- Contains < 0.1% of perfluoro-n-hexanoic acid and ~ 0.3% of perfluoro-n-octanoic acid.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: 
B.G. Chittim

Date: 12/13/2016
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:


Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: MPFHxA; LC/MS Data (TIC and Mass Spectrum)

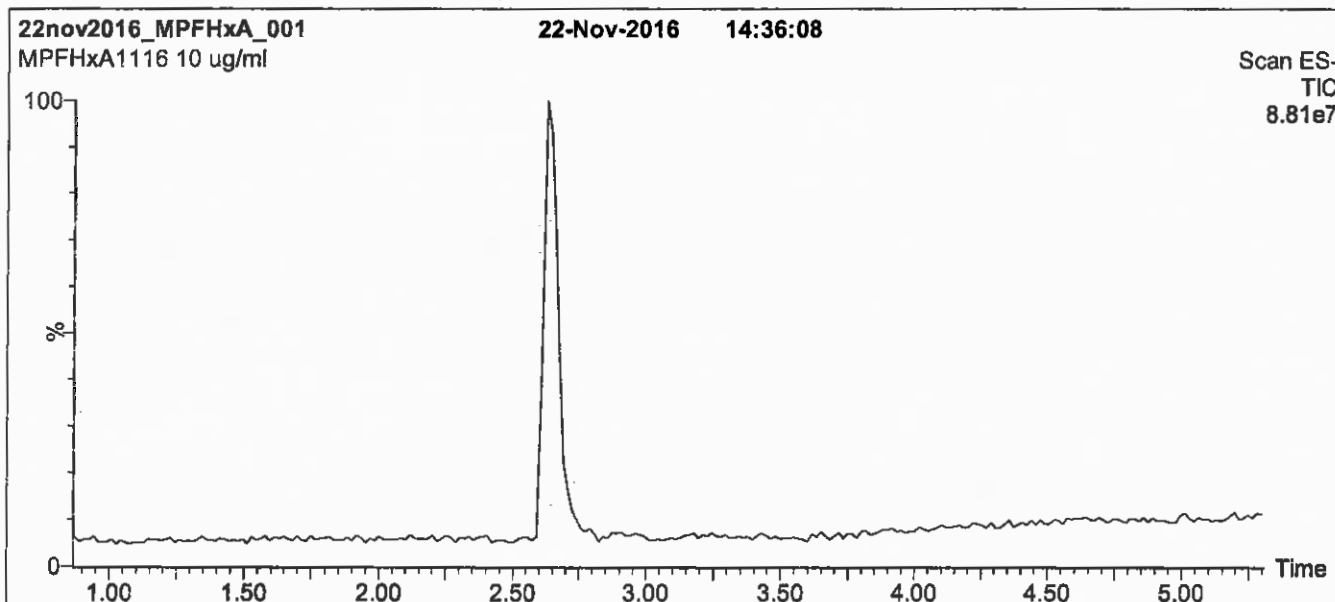

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions


Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm
Mobile phase: Gradient
Start: 40% (80:20 MeOH:ACN) / 60% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 90% organic over 7 min and hold for 2 min
before returning to initial conditions over 0.5 min.
Time: 10 min

Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (150 - 850 amu)
Source: Electrospray (negative)
Capillary Voltage (kV) = 2.00
Cone Voltage (V) = 15.00
Cone Gas Flow (l/hr) = 100
Desolvation Gas Flow (l/hr) = 750

Figure 2: MPFHxA; LC/MS/MS Data (Selected MRM Transitions)

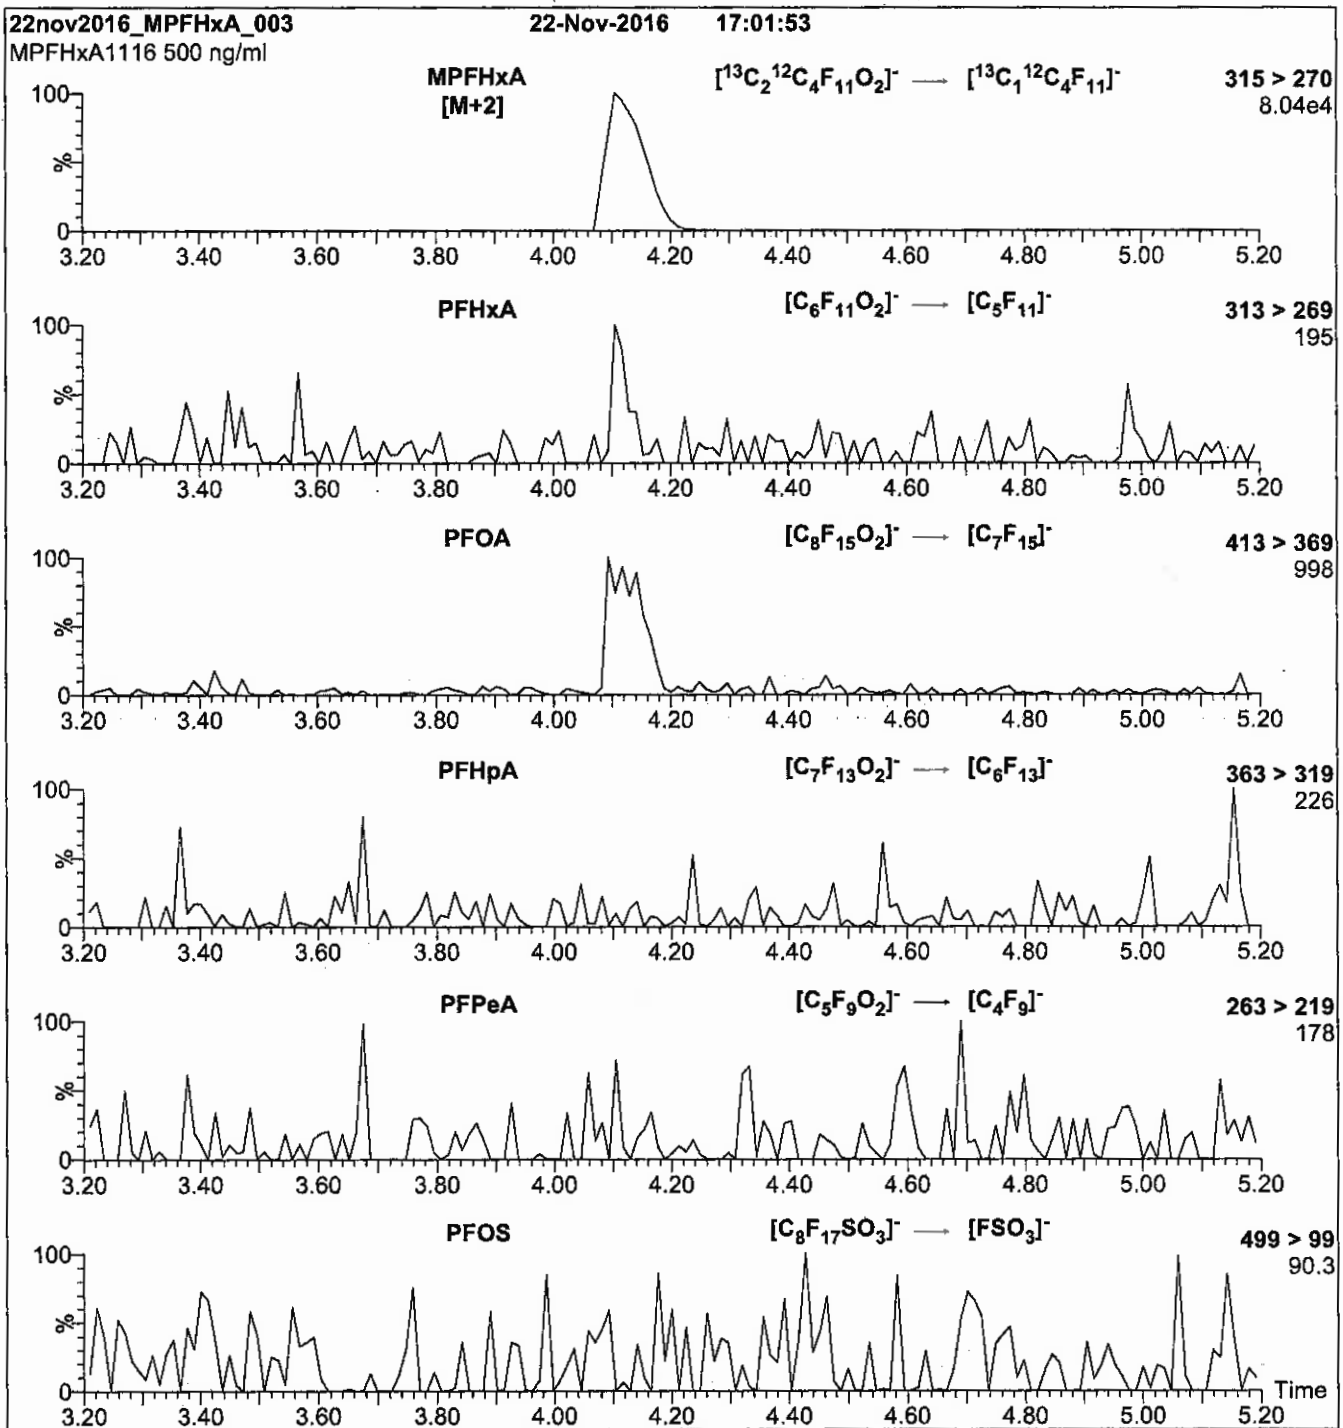

Conditions for Figure 2:

Injection: Direct loop injection
10 μl (500 ng/ml MPFHxA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H_2O
(both with 10 mM NH_4OAc buffer)

Flow: 300 $\mu\text{l}/\text{min}$

MS Parameters

Collision Gas (mbar) = $3.46\text{e-}3$
Collision Energy (eV) = 10

Reagent

LCMPFOS_00019

R: SBC 12/21/16



814253
ID: LCMPFOS_00019
Exp: 08/03/21 Ppfd: SBC
13C4-Perfluorooctanesulfo




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: MPFOS **LOT NUMBER:** MPFOS0816
COMPOUND: Sodium perfluoro-1-[1,2,3,4-¹³C₄]octanesulfonate

STRUCTURE: **CAS #:** Not available

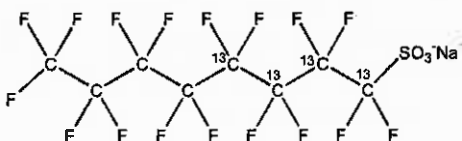

MOLECULAR FORMULA: ¹³C₄¹²C₄F₁₇SO₃Na **MOLECULAR WEIGHT:** 526.08
CONCENTRATION: 50.0 ± 2.5 µg/ml (Na salt) **SOLVENT(S):** Methanol
47.8 ± 2.4 µg/ml (MPFOS anion)
CHEMICAL PURITY: >98% **ISOTOPIC PURITY:** ≥99% ¹³C
LAST TESTED: (mm/dd/yyyy) 08/03/2016 (1,2,3,4-¹³C₄)
EXPIRY DATE: (mm/dd/yyyy) 08/03/2021
RECOMMENDED STORAGE: Store ampoule in a cool, dark place


DOCUMENTATION/ DATA ATTACHED:

Figure 1: LC/MS Data (TIC and Mass Spectrum)
Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains ~ 0.8% Sodium perfluoro-1-[1,2,3-¹³C₃]heptanesulfonate.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: 
B.G. Chittim **Date:** 08/05/2016
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:


Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: MPFOS; LC/MS Data (TIC and Mass Spectrum)

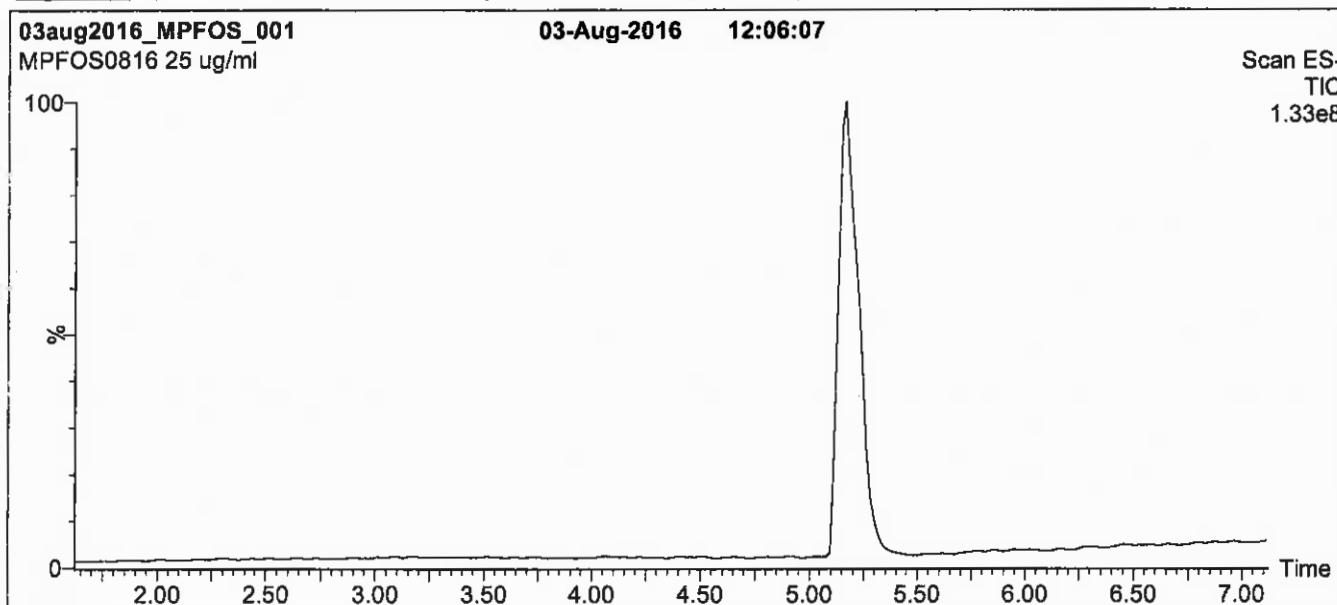

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
Start: 45% (80:20 MeOH:ACN) / 55% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 90% organic over 7 min and hold for 1.5 min
before returning to initial conditions in 0.5 min.
Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (225 - 850 amu)

Source: Electrospray (negative)
Capillary Voltage (kV) = 3.00
Cone Voltage (V) = 60.00
Cone Gas Flow (l/hr) = 50
Desolvation Gas Flow (l/hr) = 750

Figure 2: MPFOS; LC/MS/MS Data (Selected MRM Transitions)



Conditions for Figure 2:

Injection: Direct loop injection
10 μl (500 ng/ml MPFOS)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H_2O
(both with 10 mM NH_4OAc buffer)

Flow: 300 $\mu\text{l}/\text{min}$

MS Parameters

Collision Gas (mbar) = 3.46e-3

Collision Energy (eV) = 40

Reagent

LCMPFOS_00021

r: 5/6/17 SKV




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: MPFOS **LOT NUMBER:** MPFOS1216
COMPOUND: Sodium perfluoro-1-[1,2,3,4-¹³C₄]octanesulfonate

STRUCTURE: **CAS #:** Not available



MOLECULAR FORMULA:	¹³ C ₄ ¹² C ₄ F ₁₇ SO ₃ Na	MOLECULAR WEIGHT:	526.08
CONCENTRATION:	50.0 ± 2.5 µg/ml (Na salt) 47.8 ± 2.4 µg/ml (MPFOS anion)	SOLVENT(S):	Methanol
CHEMICAL PURITY:	>98%	ISOTOPIC PURITY:	≥99% ¹³ C (1,2,3,4- ¹³ C ₄)
LAST TESTED: (mm/dd/yyyy)	12/12/2016		
EXPIRY DATE: (mm/dd/yyyy)	12/12/2021		
RECOMMENDED STORAGE:	Store ampoule in a cool, dark place		


DOCUMENTATION/ DATA ATTACHED:

- Figure 1: LC/MS Data (TIC and Mass Spectrum)
- Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains ~ 0.8% Sodium perfluoro-1-[1,2,3-¹³C₃]heptanesulfonate.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: 
B.G. Chittim **Date:** 12/14/2016
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
 519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:


Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: MPFOS; LC/MS Data (TIC and Mass Spectrum)

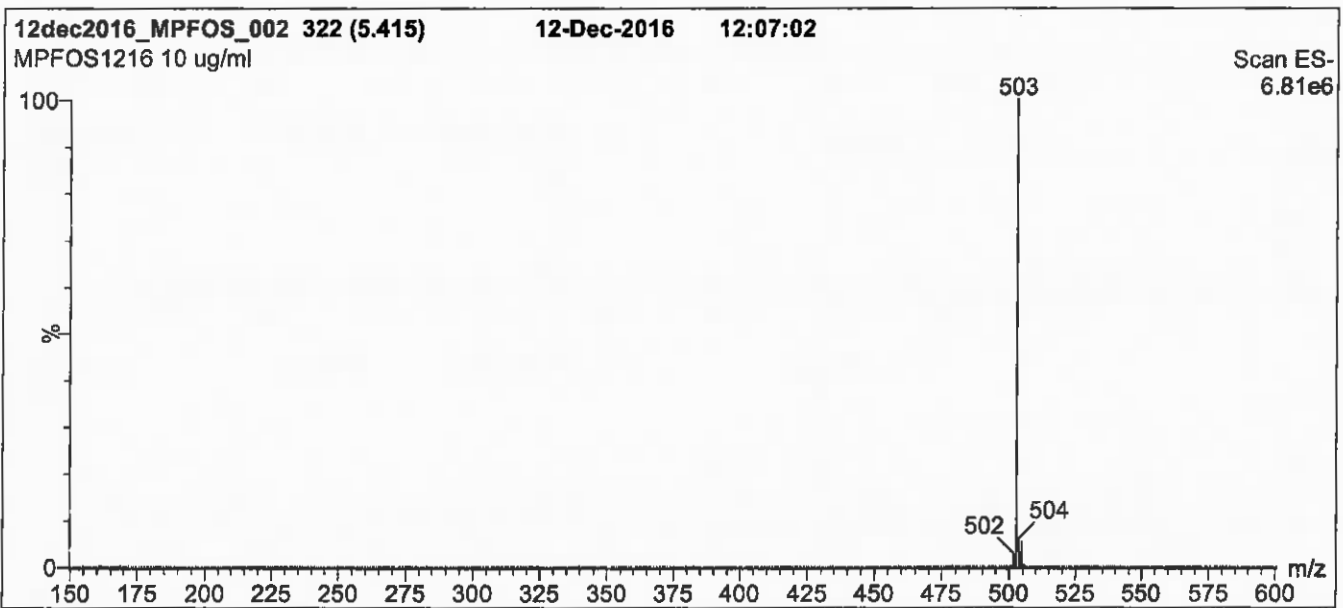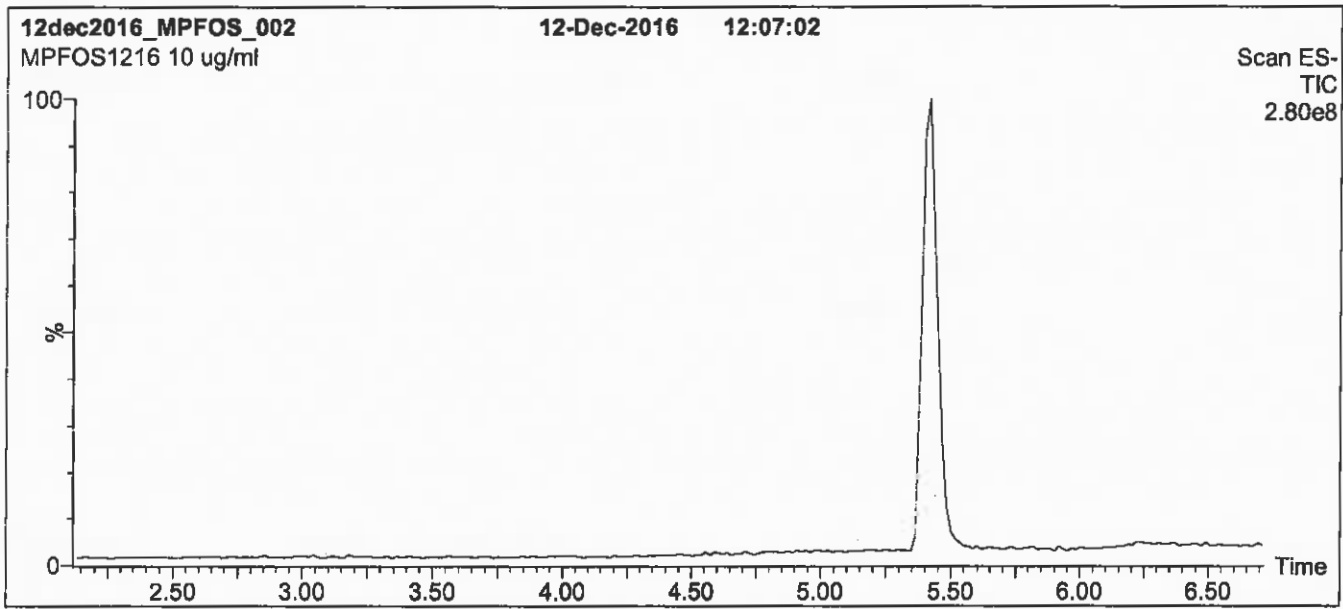

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
 1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
 Start: 50% (80:20 MeOH:ACN) / 50% H₂O
 (both with 10 mM NH₄OAc buffer)
 Ramp to 85% organic over 7.5 min and hold for 1.5 min
 before returning to initial conditions in 0.5 min.
 Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (150 - 850 amu)

Source: Electrospray (negative)
 Capillary Voltage (kV) = 3.00
 Cone Voltage (V) = 60.00
 Cone Gas Flow (l/hr) = 50
 Desolvation Gas Flow (l/hr) = 750

Figure 2: MPFOS; LC/MS/MS Data (Selected MRM Transitions)

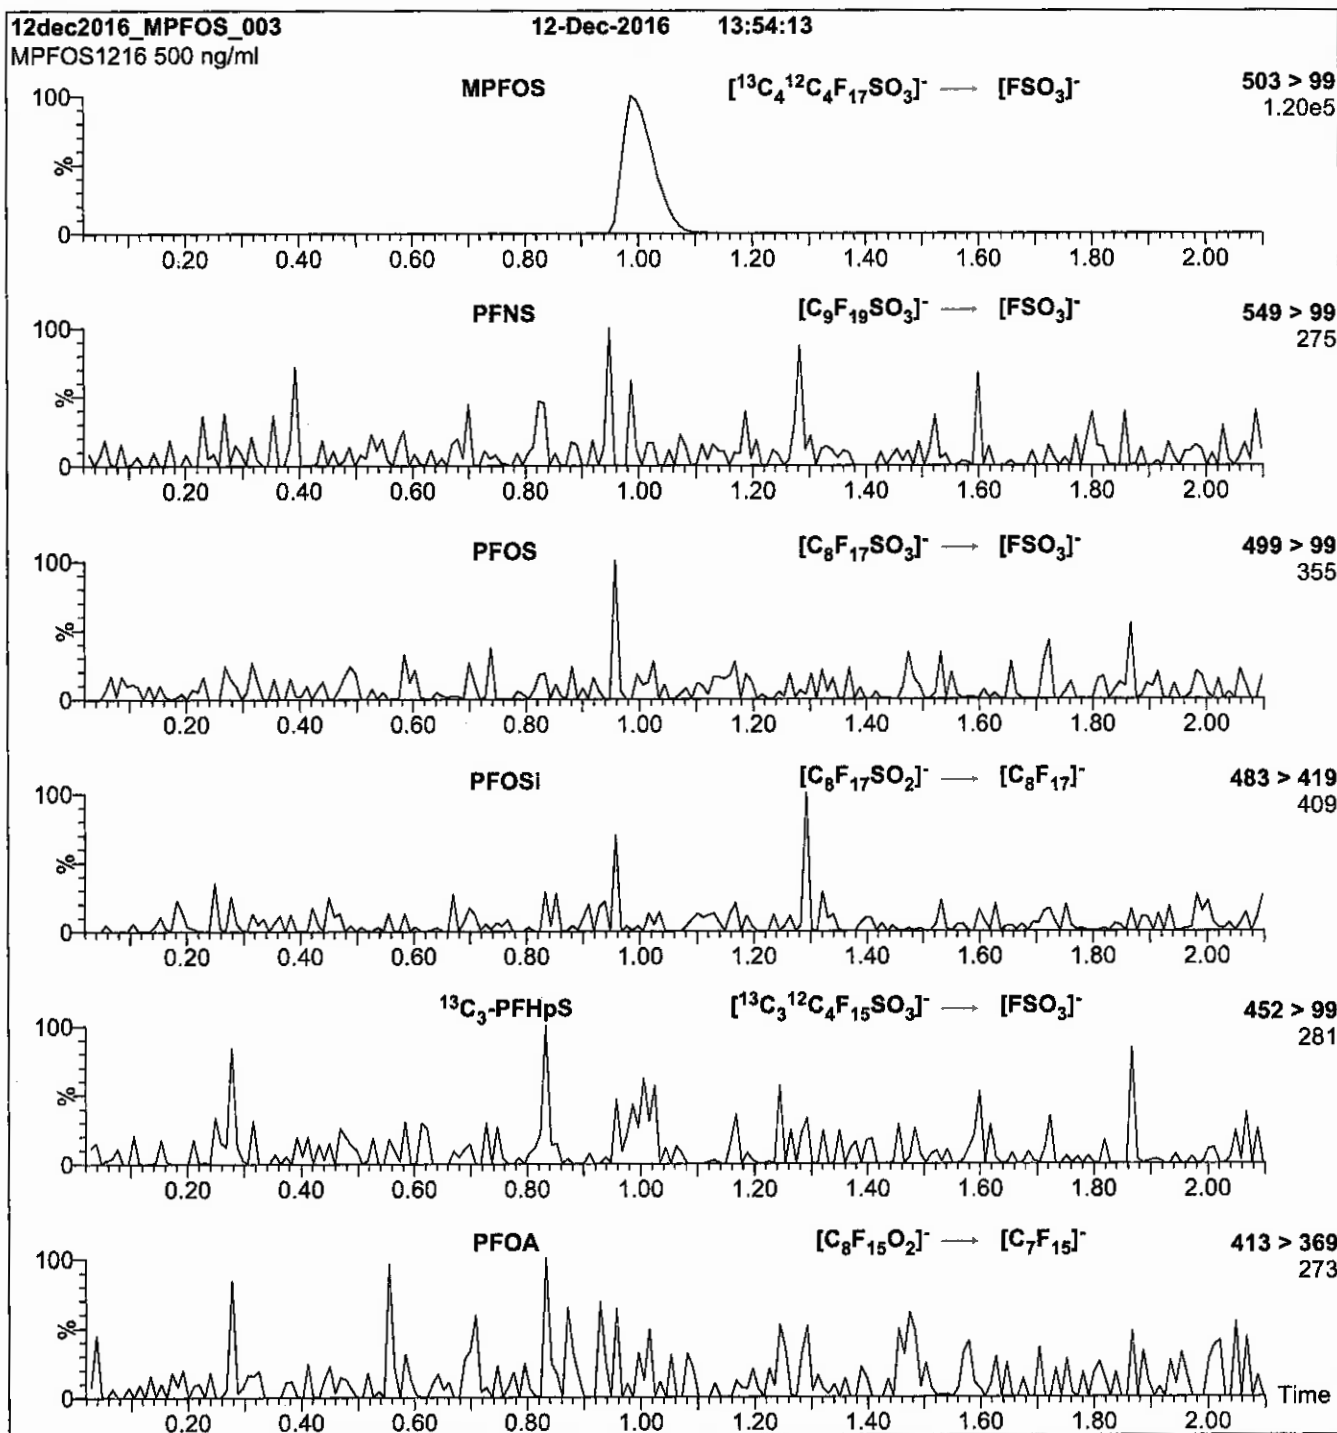

Conditions for Figure 2:

Injection: Direct loop injection
10 μl (500 ng/ml MPFOS)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H_2O
(both with 10 mM NH_4OAc buffer)

Flow: 300 $\mu\text{l}/\text{min}$

MS Parameters

Collision Gas (mbar) = 3.35e-3
Collision Energy (eV) = 40

Method 537 DOD

Perfluorinated Alkyl Acids (LC/MS)
by Method 537 DOD

FORM II
LCMS SURROGATE RECOVERY

Lab Name: TestAmerica Sacramento

Job No.: 320-35207-1

SDG No.: _____

Matrix: Water

Level: Low

GC Column (1): GeminiC18 3 ID: 3 (mm)

Client Sample ID	Lab Sample ID	PFHxA #	PFDA #
WGNA-011818-RW-332 5	320-35207-1	96	109
WGNA-011818-FRB-33 25	320-35207-2	114	104
NAWC-011818-RW-316	320-35207-3	103	102
NAWC-011818-FRB-31 6	320-35207-4	109	100
NAWC-011818-RW-260	320-35207-5	104	105
NAWC-011818-FRB-26 0	320-35207-6	104	102
NAWC-011818-RW-281	320-35207-7	99	103
NAWC-011818-FRB-28 1	320-35207-8	103	102
NAWC-011818-RW-032	320-35207-9	88	104
NAWC-011818-FRB-03 2	320-35207-10	104	105
NAWC-011818-RW-038	320-35207-11	90	97
NAWC-011818-FRB-03 8	320-35207-12	107	102
	MB 320-206379/1-A	114	110
	LLCS 320-206379/2-A	106	104
	LLCSD 320-206379/3-A	109	104

PFHxA = 13C2 PFHxA
PFDA = 13C2 PFDA

QC LIMITS
70-130
70-130

Column to be used to flag recovery values

FORM III
LCMS LOW LEVEL CONTROL SAMPLE RECOVERY

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Matrix: Water Level: Low Lab File ID: 2018.02.06_537XX_045.d
 Lab ID: LLCS 320-206379/2-A Client ID: _____

COMPOUND	SPIKE ADDED (ng/L)	LLCS CONCENTRATION (ng/L)	LLCS % REC	QC LIMITS REC	#
Perfluorooctanesulfonic acid (PFOS)	40.0	40.2	100	50-150	M
Perfluorooctanoic acid (PFOA)	20.0	22.1	111	50-150	
Perfluorononanoic acid (PFNA)	20.0	21.9 J	110	50-150	
Perfluorohexanesulfonic acid (PFHxS)	30.0	33.0	110	50-150	
Perfluoroheptanoic acid (PFHpA)	10.0	11.6	116	50-150	
Perfluorobutanesulfonic acid (PFBS)	90.0	94.5	105	50-150	

Column to be used to flag recovery and RPD values

FORM III
LCMS LOW LEVEL CONTROL STANDARD DUPLICATE RECOVERY

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1

SDG No.: _____

Matrix: Water Level: Low Lab File ID: 2018.02.06_537XX_046.d

Lab ID: LLCSD 320-206379/3-A Client ID: _____

COMPOUND	SPIKE ADDED (ng/L)	LLCSD CONCENTRATION (ng/L)	LLCSD % REC	% RPD	QC LIMITS		#
					RPD	REC	
Perfluorooctanesulfonic acid (PFOS)	40.0	37.6 J	94	7	50	50-150	M
Perfluorooctanoic acid (PFOA)	20.0	22.5	112	1	50	50-150	
Perfluorononanoic acid (PFNA)	20.0	22.2 J	111	1	50	50-150	
Perfluorohexanesulfonic acid (PFHxS)	30.0	31.4	105	5	50	50-150	
Perfluoroheptanoic acid (PFHpA)	10.0	11.4	114	1	50	50-150	
Perfluorobutanesulfonic acid (PFBS)	90.0	94.8	105	0.3	50	50-150	

Column to be used to flag recovery and RPD values

FORM IV
LCMS METHOD BLANK SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Lab File ID: 2018.02.06_537XX_044.d Lab Sample ID: MB 320-206379/1-A
 Matrix: Water Date Extracted: 01/31/2018 12:34
 Instrument ID: A8_N Date Analyzed: 02/06/2018 18:33
 Level: (Low/Med) Low

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES:

CLIENT SAMPLE ID	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED
	LLCS 320-206379/2-A	2018.02.06_537XX_045.d	02/06/2018 18:37
	LLCSD 320-206379/3-A	2018.02.06_537XX_046.d	02/06/2018 18:42
WGNA-011818-RW-3325	320-35207-1	2018.02.06_537XX_047.d	02/06/2018 18:47
WGNA-011818-FRB-3325	320-35207-2	2018.02.06_537XX_048.d	02/06/2018 18:51
NAWC-011818-RW-316	320-35207-3	2018.02.06_537XX_049.d	02/06/2018 18:56
NAWC-011818-FRB-316	320-35207-4	2018.02.06_537XX_050.d	02/06/2018 19:01
NAWC-011818-RW-260	320-35207-5	2018.02.06_537XX_051.d	02/06/2018 19:05
NAWC-011818-FRB-260	320-35207-6	2018.02.06_537XX_054.d	02/06/2018 19:19
NAWC-011818-RW-281	320-35207-7	2018.02.06_537XX_055.d	02/06/2018 19:24
NAWC-011818-FRB-281	320-35207-8	2018.02.06_537XX_056.d	02/06/2018 19:29
NAWC-011818-RW-032	320-35207-9	2018.02.06_537XX_057.d	02/06/2018 19:33
NAWC-011818-FRB-032	320-35207-10	2018.02.06_537XX_058.d	02/06/2018 19:38
NAWC-011818-RW-038	320-35207-11	2018.02.06_537XX_059.d	02/06/2018 19:43
NAWC-011818-FRB-038	320-35207-12	2018.02.06_537XX_060.d	02/06/2018 19:47

FORM VIII
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Instrument ID: A8_N Calibration Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3(mm) Calibration End Date: 11/03/2017 14:01
 Calibration ID: 36012

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
INITIAL CALIBRATION MEAN AREA AND MEAN RT	1535518	1.91	3276559	2.15		
UPPER LIMIT	2303277	2.41	4914839	2.65		
LOWER LIMIT	767759	1.41	1638280	1.65		
LAB SAMPLE ID	CLIENT SAMPLE ID					
CCVL 320-192908/11		1586829	1.91	3305852	2.15	
ICV 320-192908/13		1512045	1.90	3433628	2.14	
CCVL 320-207097/1		1375995	1.81	3051061	2.05	
CCV 320-207292/1 CCVIS		1328760	1.81	3042209	2.05	
MB 320-206379/1-A		1243942	1.80	2945240	2.05	
LLCS 320-206379/2-A		1313107	1.81	3024316	2.05	
LLCSD 320-206379/3-A		1273817	1.80	3050466	2.05	
320-35207-1	WGNA-011818-RW-3325	1281071	1.80	2980694	2.05	
320-35207-2	WGNA-011818-FRB-3325	1232911	1.80	3018263	2.04	
320-35207-3	NAWC-011818-RW-316	1338968	1.80	2966673	2.04	
320-35207-4	NAWC-011818-FRB-316	1244262	1.80	3004650	2.05	
320-35207-5	NAWC-011818-RW-260	1302427	1.81	3143419	2.05	
CCV 320-207292/11 CCVIS		1315133	1.80	3035313	2.04	
CCV 320-207294/11 CCVIS		1315133	1.80	3035313	2.04	
320-35207-6	NAWC-011818-FRB-260	1299420	1.80	3069150	2.05	
320-35207-7	NAWC-011818-RW-281	1354367	1.81	3207550	2.05	
320-35207-8	NAWC-011818-FRB-281	1354309	1.81	3260304	2.05	
320-35207-9	NAWC-011818-RW-032	1279796	1.81	3134922	2.05	
320-35207-10	NAWC-011818-FRB-032	1269005	1.80	3041394	2.04	
320-35207-11	NAWC-011818-RW-038	1373697	1.79	3369231	2.04	
320-35207-12	NAWC-011818-FRB-038	1356647	1.80	3181172	2.04	
CCV 320-207294/20 CCVIS		1309862	1.79	3183039	2.04	

13PFOA = 13C2-PFOA
 PFOS = 13C4 PFOS

Area Limit = 50%-150% of internal standard area
 RT Limit = ± 0.5 minutes of internal standard RT

Column used to flag values outside QC limits

FORM VIII
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Sample No.: CCV 320-207292/1 Date Analyzed: 02/06/2018 18:23
 Instrument ID: A8_N GC Column: GeminiC18 3x100 ID: 3 (mm)
 Lab File ID (Standard): 2018.02.06_537XX_04 Heated Purge: (Y/N) N
 Calibration ID: 36012

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	1328760	1.81	3042209	2.05		
UPPER LIMIT	1860264	2.31	4259093	2.55		
LOWER LIMIT	930132	1.31	2129546	1.55		
LAB SAMPLE ID	CLIENT SAMPLE ID					
MB 320-206379/1-A		1243942	1.80	2945240	2.05	
LLCS 320-206379/2-A		1313107	1.81	3024316	2.05	
LLCSD 320-206379/3-A		1273817	1.80	3050466	2.05	
320-35207-1	WGNA-011818-RW-3325	1281071	1.80	2980694	2.05	
320-35207-2	WGNA-011818-FRB-3325	1232911	1.80	3018263	2.04	
320-35207-3	NAWC-011818-RW-316	1338968	1.80	2966673	2.04	
320-35207-4	NAWC-011818-FRB-316	1244262	1.80	3004650	2.05	
320-35207-5	NAWC-011818-RW-260	1302427	1.81	3143419	2.05	

13PFOA = 13C2-PFOA

PFOS = 13C4 PFOS

Area Limit = 70%-140% of internal standard area

RT Limit = ± 0.5 minutes of internal standard RT

Column used to flag values outside QC limits

FORM VIII
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Sample No.: CCV 320-207292/11 Date Analyzed: 02/06/2018 19:10
 Instrument ID: A8_N GC Column: GeminiC18 3x100 ID: 3 (mm)
 Lab File ID (Standard): 2018.02.06_537XX_05 Heated Purge: (Y/N) N
 Calibration ID: 36012

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	1315133	1.80	3035313	2.04		
UPPER LIMIT	1841186	2.30	4249438	2.54		
LOWER LIMIT	920593	1.30	2124719	1.54		
LAB SAMPLE ID	CLIENT SAMPLE ID					
MB 320-206379/1-A		1243942	1.80	2945240	2.05	
LLCS 320-206379/2-A		1313107	1.81	3024316	2.05	
LLCSD 320-206379/3-A		1273817	1.80	3050466	2.05	
320-35207-1	WGNA-011818-RW-3325	1281071	1.80	2980694	2.05	
320-35207-2	WGNA-011818-FRB-3325	1232911	1.80	3018263	2.04	
320-35207-3	NAWC-011818-RW-316	1338968	1.80	2966673	2.04	
320-35207-4	NAWC-011818-FRB-316	1244262	1.80	3004650	2.05	
320-35207-5	NAWC-011818-RW-260	1302427	1.81	3143419	2.05	

13PFOA = 13C2-PFOA

PFOS = 13C4 PFOS

Area Limit = 70%-140% of internal standard area
 RT Limit = ± 0.5 minutes of internal standard RT

Column used to flag values outside QC limits

FORM VIII
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Sample No.: CCV 320-207294/11 Date Analyzed: 02/06/2018 19:10
 Instrument ID: A8_N GC Column: GeminiC18 3x100 ID: 3 (mm)
 Lab File ID (Standard): 2018.02.06_537XX_05 Heated Purge: (Y/N) N
 Calibration ID: 36012

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	1315133	1.80	3035313	2.04		
UPPER LIMIT	1841186	2.30	4249438	2.54		
LOWER LIMIT	920593	1.30	2124719	1.54		
LAB SAMPLE ID	CLIENT SAMPLE ID					
320-35207-6	NAWC-011818-FRB-260	1299420	1.80	3069150	2.05	
320-35207-7	NAWC-011818-RW-281	1354367	1.81	3207550	2.05	
320-35207-8	NAWC-011818-FRB-281	1354309	1.81	3260304	2.05	
320-35207-9	NAWC-011818-RW-032	1279796	1.81	3134922	2.05	
320-35207-10	NAWC-011818-FRB-032	1269005	1.80	3041394	2.04	
320-35207-11	NAWC-011818-RW-038	1373697	1.79	3369231	2.04	
320-35207-12	NAWC-011818-FRB-038	1356647	1.80	3181172	2.04	

13PFOA = 13C2-PFOA
 PFOS = 13C4 PFOS

Area Limit = 70%-140% of internal standard area
 RT Limit = ± 0.5 minutes of internal standard RT

Column used to flag values outside QC limits

FORM VIII
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Sample No.: CCV 320-207294/20 Date Analyzed: 02/06/2018 19:52
 Instrument ID: A8_N GC Column: GeminiC18 3x100 ID: 3 (mm)
 Lab File ID (Standard): 2018.02.06_537XX_06 Heated Purge: (Y/N) N
 Calibration ID: 36012

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	1309862	1.79	3183039	2.04		
UPPER LIMIT	1833807	2.29	4456255	2.54		
LOWER LIMIT	916903	1.29	2228127	1.54		
LAB SAMPLE ID	CLIENT SAMPLE ID					
320-35207-6	NAWC-011818-FRB-260	1299420	1.80	3069150	2.05	
320-35207-7	NAWC-011818-RW-281	1354367	1.81	3207550	2.05	
320-35207-8	NAWC-011818-FRB-281	1354309	1.81	3260304	2.05	
320-35207-9	NAWC-011818-RW-032	1279796	1.81	3134922	2.05	
320-35207-10	NAWC-011818-FRB-032	1269005	1.80	3041394	2.04	
320-35207-11	NAWC-011818-RW-038	1373697	1.79	3369231	2.04	
320-35207-12	NAWC-011818-FRB-038	1356647	1.80	3181172	2.04	

13PFOA = 13C2-PFOA

PFOS = 13C4 PFOS

Area Limit = 70%-140% of internal standard area
 RT Limit = ± 0.5 minutes of internal standard RT

Column used to flag values outside QC limits

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Client Sample ID: WGNA-011818-RW-3325 Lab Sample ID: 320-35207-1
 Matrix: Water Lab File ID: 2018.02.06_537XX_047.d
 Analysis Method: 537 Date Collected: 01/18/2018 09:10
 Extraction Method: 537 Date Extracted: 01/31/2018 12:34
 Sample wt/vol: 247.6(mL) Date Analyzed: 02/06/2018 18:47
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 207292 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	14	J M	40	16	6.9
335-67-1	Perfluorooctanoic acid (PFOA)	14	J	20	8.1	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U M	24	20	8.1
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	13	J	30	12	5.6
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.2	J	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	91	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	96		70-130
STL00996	13C2 PFDA	109		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_047.d
 Lims ID: 320-35207-A-1-A
 Client ID: WGNA-011818-RW-3325
 Sample Type: Client
 Inject. Date: 06-Feb-2018 18:47:09 ALS Bottle#: 34 Worklist Smp#: 6
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35207-a-1-a
 Misc. Info.: Plate: 1 Rack: 3
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Feb-2018 13:42:00 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: CTXT1

First Level Reviewer: krenns Date: 07-Feb-2018 13:42:00

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.373	1.366	0.007	1.000	127590	1.10		165	
298.90 > 99.00	1.366	1.366	0.0	0.994	91931		1.39(0.00-0.00)	269	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.487	1.479	0.008	1.000	1352259	9.59		7413	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.624	1.616	0.008	1.000	575672	3.31		348	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.624	1.616	0.008	1.000	123418	1.03		18.6	
* 6 13C2-PFOA									
415.00 > 370.00	1.798	1.791	0.007		1281071	10.0		5655	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.798	1.798	0.0	1.000	419465	3.54		49.9	
413.00 > 169.00	1.798	1.798	0.0	1.000	245962		1.71(0.00-0.00)	683	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.048	2.041	0.007	1.000	336610	3.45		90.2	a
499.00 > 99.00	2.048	2.041	0.007	1.000	55508		6.06(0.00-0.00)	72.6	a
* 7 13C4 PFOS									
503.00 > 80.00	2.048	2.041	0.007		2980694	28.7		2904	
9 Perfluorononanoic acid									
463.00 > 419.00	2.056	2.048	0.008	1.000	55851	0.6564		7.7	M
\$ 10 13C2 PFDA									
515.00 > 470.00	2.238	2.231	0.007	1.000	1070310	10.9		7601	

QC Flag Legend

Review Flags

M - Manually Integrated

a - User Assigned ID




TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_047.d
Injection Date: 06-Feb-2018 18:47:09 Instrument ID: A8_N
Lims ID: 320-35207-A-1-A Lab Sample ID: 320-35207-1
Client ID: WGNA-011818-RW-3325
Operator ID: SACINSTLCMS01 ALS Bottle#: 34 Worklist Smp#: 6
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid

* 7 13C4 PFOS

9 Perfluorononanoic acid (M)



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_047.d
 Lims ID: 320-35207-A-1-A
 Client ID: WGNA-011818-RW-3325
 Sample Type: Client
 Inject. Date: 06-Feb-2018 18:47:09 ALS Bottle#: 34 Worklist Smp#: 6
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35207-a-1-a
 Misc. Info.: Plate: 1 Rack: 3
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Feb-2018 13:42:00 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: CTXT1

First Level Reviewer: krenns Date: 07-Feb-2018 13:42:00

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	9.59	95.94
\$ 10 13C2 PFDA	10.0	10.9	109.18

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_047.d
Injection Date: 06-Feb-2018 18:47:09 Instrument ID: A8_N
Lims ID: 320-35207-A-1-A Lab Sample ID: 320-35207-1
Client ID: WGNA-011818-RW-3325
Operator ID: SACINSTLCMS01 ALS Bottle#: 34 Worklist Smp#: 6
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.04

Processing Integration Results



Manual Integration Results

RT: 2.05
Area: 336610
Amount: 3.449427
Amount Units: ng/ml



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_047.d
Injection Date: 06-Feb-2018 18:47:09 Instrument ID: A8_N
Lims ID: 320-35207-A-1-A Lab Sample ID: 320-35207-1
Client ID: WGNA-011818-RW-3325
Operator ID: SACINSTLCMS01 ALS Bottle#: 34 Worklist Smp#: 6
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

9 Perfluorononanoic acid, CAS: 375-95-1


Signal: 1

Not Detected
Expected RT: 2.05

Processing Integration Results



Manual Integration Results



RT: 2.06
Area: 55851
Amount: 0.656424
Amount Units: ng/ml

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Client Sample ID: WGNA-011818-FRB-3325 Lab Sample ID: 320-35207-2
 Matrix: Water Lab File ID: 2018.02.06_537XX_048.d
 Analysis Method: 537 Date Collected: 01/18/2018 09:05
 Extraction Method: 537 Date Extracted: 01/31/2018 12:34
 Sample wt/vol: 251.8(mL) Date Analyzed: 02/06/2018 18:51
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 207292 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	7.9	U	20	7.9	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	7.9
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.0	U	9.9	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	89	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	114		70-130
STL00996	13C2 PFDA	104		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_048.d
 Lims ID: 320-35207-A-2-A
 Client ID: WGNA-011818-FRB-3325
 Sample Type: Client
 Inject. Date: 06-Feb-2018 18:51:50 ALS Bottle#: 35 Worklist Smp#: 7
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35207-a-2-a
 Misc. Info.: Plate: 1 Rack: 3
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Feb-2018 11:48:41 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d


Column 1 : Det: EXP1
 Process Host: CTXT1

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
\$ 2 13C2 PFHxA	315.00 > 270.00	1.487	1.487	0.0	1.000	1548701	11.4	8437	
* 6 13C2-PFOA	415.00 > 370.00	1.798	1.806	-0.008		1232911	10.0	5279	
* 7 13C4 PFOS	503.00 > 80.00	2.041	2.048	-0.007		3018263	28.7	6612	
\$ 10 13C2 PFDA	515.00 > 470.00	2.231	2.238	-0.007	1.000	982280	10.4	6584	


TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_048.d
Injection Date: 06-Feb-2018 18:51:50 Instrument ID: A8_N
Lims ID: 320-35207-A-2-A Lab Sample ID: 320-35207-2
Client ID: WGNA-011818-FRB-3325
Operator ID: SACINSTLCMS01 ALS Bottle#: 35 Worklist Smp#: 7
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL


1 Perfluorobutanesulfonic acid (ND) 1 Perfluorobutanesulfonic acid (ND) \$ 2 13C2 PFHxA




3 Perfluorohexanesulfonic acid (ND) 4 Perfluoroheptanoic acid (ND) * 6 13C2-PFOA




5 Perfluorooctanoic acid (ND) 5 Perfluorooctanoic acid (ND) 8 Perfluorooctane sulfonic acid (ND)



8 Perfluorooctane sulfonic acid (ND) * 7 13C4 PFOS 9 Perfluorononanoic acid (ND)



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_048.d
 Lims ID: 320-35207-A-2-A
 Client ID: WGNA-011818-FRB-3325
 Sample Type: Client
 Inject. Date: 06-Feb-2018 18:51:50 ALS Bottle#: 35 Worklist Smp#: 7
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35207-a-2-a
 Misc. Info.: Plate: 1 Rack: 3
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Feb-2018 11:48:41 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: CTXT1

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	11.4	114.16
\$ 10 13C2 PFDA	10.0	10.4	104.12

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Client Sample ID: NAWC-011818-RW-316 Lab Sample ID: 320-35207-3
 Matrix: Water Lab File ID: 2018.02.06_537XX_049.d
 Analysis Method: 537 Date Collected: 01/18/2018 10:10
 Extraction Method: 537 Date Extracted: 01/31/2018 12:34
 Sample wt/vol: 247.1(mL) Date Analyzed: 02/06/2018 18:56
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 207292 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	45	M	40	16	6.9
335-67-1	Perfluorooctanoic acid (PFOA)	24	M	20	8.1	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	8.1
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	32		30	12	5.6
375-85-9	Perfluoroheptanoic acid (PFHpA)	9.0	J	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	91	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	103		70-130
STL00996	13C2 PFDA	102		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_049.d
 Lims ID: 320-35207-A-3-A
 Client ID: NAWC-011818-RW-316
 Sample Type: Client
 Inject. Date: 06-Feb-2018 18:56:33 ALS Bottle#: 36 Worklist Smp#: 8
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35207-a-3-a
 Misc. Info.: Plate: 1 Rack: 3
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Feb-2018 13:42:33 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: CTXT1

First Level Reviewer: krenns Date: 07-Feb-2018 11:46:30

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.366	1.366	0.0	1.000	153837	1.33		270	
298.90 > 99.00	1.366	1.366	0.0	1.000	126008		1.22(0.00-0.00)	456	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.487	1.479	0.008	1.000	1523422	10.3		9697	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.624	1.616	0.008	1.000	1369116	7.91		1519	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.624	1.616	0.008	1.000	277540	2.21		68.6	
* 6 13C2-PFOA									
415.00 > 370.00	1.798	1.791	0.007		1338968	10.0		5877	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.798	1.798	0.0	1.000	749033	6.04		111	Ma
413.00 > 169.00	1.798	1.798	0.0	1.000	431817		1.73(0.00-0.00)	1398	M
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.041	2.041	0.0	1.000	1087234	11.2		492	Ma
499.00 > 99.00	2.041	2.041	0.0	1.000	233805		4.65(0.00-0.00)	430	M
* 7 13C4 PFOS									
503.00 > 80.00	2.041	2.041	0.0		2966673	28.7		5318	
9 Perfluorononanoic acid									
463.00 > 419.00	2.048	2.048	0.0	1.000	58611	0.6591		9.5	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.238	2.231	0.007	1.000	1046310	10.2		7251	

QC Flag Legend

Review Flags

M - Manually Integrated

a - User Assigned ID




TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_049.d
Injection Date: 06-Feb-2018 18:56:33 Instrument ID: A8_N
Lims ID: 320-35207-A-3-A Lab Sample ID: 320-35207-3
Client ID: NAWC-011818-RW-316
Operator ID: SACINSTLCMS01 ALS Bottle#: 36 Worklist Smp#: 8
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid (M)

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_049.d
 Lims ID: 320-35207-A-3-A
 Client ID: NAWC-011818-RW-316
 Sample Type: Client
 Inject. Date: 06-Feb-2018 18:56:33 ALS Bottle#: 36 Worklist Smp#: 8
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35207-a-3-a
 Misc. Info.: Plate: 1 Rack: 3
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Feb-2018 13:42:33 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: CTXT1

First Level Reviewer: krenns Date: 07-Feb-2018 11:46:30

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	10.3	103.41
\$ 10 13C2 PFDA	10.0	10.2	102.12

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_049.d
Injection Date: 06-Feb-2018 18:56:33 Instrument ID: A8_N
Lims ID: 320-35207-A-3-A Lab Sample ID: 320-35207-3
Client ID: NAWC-011818-RW-316
Operator ID: SACINSTLCMS01 ALS Bottle#: 36 Worklist Smp#: 8
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.04

Processing Integration Results



RT: 2.04
Area: 1087234
Amount: 11.194137
Amount Units: ng/ml

Manual Integration Results



Reviewer: krenns, 07-Feb-2018 13:42:23
Audit Action: Split an Integrated Peak

Audit Reason: Split Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_049.d
Injection Date: 06-Feb-2018 18:56:33 Instrument ID: A8_N
Lims ID: 320-35207-A-3-A Lab Sample ID: 320-35207-3
Client ID: NAWC-011818-RW-316
Operator ID: SACINSTLCMS01 ALS Bottle#: 36 Worklist Smp#: 8
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected
Expected RT: 2.04

Processing Integration Results



Manual Integration Results

RT: 2.04
Area: 233805
Amount: 11.194137
Amount Units: ng/ml



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_049.d
Injection Date: 06-Feb-2018 18:56:33 Instrument ID: A8_N
Lims ID: 320-35207-A-3-A Lab Sample ID: 320-35207-3
Client ID: NAWC-011818-RW-316
Operator ID: SACINSTLCMS01 ALS Bottle#: 36 Worklist Smp#: 8
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

5 Perfluorooctanoic acid, CAS: 335-67-1

Signal: 1


RT: 1.80
Area: 358970
Amount: 2.895947
Amount Units: ng/ml

Processing Integration Results



RT: 1.80
Area: 749033
Amount: 6.042733
Amount Units: ng/ml

Manual Integration Results



Reviewer: krenns, 07-Feb-2018 11:46:12

Audit Action: Manually Integrated/Assigned Compound ID Audit Reason: Incomplete Integration

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Client Sample ID: NAWC-011818-FRB-316 Lab Sample ID: 320-35207-4
 Matrix: Water Lab File ID: 2018.02.06_537XX_050.d
 Analysis Method: 537 Date Collected: 01/18/2018 10:05
 Extraction Method: 537 Date Extracted: 01/31/2018 12:34
 Sample wt/vol: 252.5 (mL) Date Analyzed: 02/06/2018 19:01
 Con. Extract Vol.: 1.0 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 207292 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	40	16	6.7
335-67-1	Perfluorooctanoic acid (PFOA)	7.9	U	20	7.9	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	7.9
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	30	12	5.4
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.0	U	9.9	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	89	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	109		70-130
STL00996	13C2 PFDA	100		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_050.d
 Lims ID: 320-35207-A-4-A
 Client ID: NAWC-011818-FRB-316
 Sample Type: Client
 Inject. Date: 06-Feb-2018 19:01:13 ALS Bottle#: 37 Worklist Smp#: 9
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35207-a-4-a
 Misc. Info.: Plate: 1 Rack: 3
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Feb-2018 11:48:41 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d


Column 1 : Det: EXP1
 Process Host: CTXT1

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
\$ 2 13C2 PFHxA	315.00 > 270.00	1.487	1.487	0.0	1.000	1498814	10.9	8343	
* 6 13C2-PFOA	415.00 > 370.00	1.798	1.806	-0.008		1244262	10.0	5765	
* 7 13C4 PFOS	503.00 > 80.00	2.048	2.048	0.0		3004650	28.7	5949	
\$ 10 13C2 PFDA	515.00 > 470.00	2.238	2.238	0.0	1.000	955357	10.0	6373	


TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_050.d
Injection Date: 06-Feb-2018 19:01:13 Instrument ID: A8_N
Lims ID: 320-35207-A-4-A Lab Sample ID: 320-35207-4
Client ID: NAWC-011818-FRB-316
Operator ID: SACINSTLCMS01 ALS Bottle#: 37 Worklist Smp#: 9
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL


1 Perfluorobutanesulfonic acid (ND) 1 Perfluorobutanesulfonic acid (ND) \$ 2 13C2 PFHxA




3 Perfluorohexanesulfonic acid (ND) 4 Perfluoroheptanoic acid (ND) * 6 13C2-PFOA




5 Perfluorooctanoic acid (ND) 5 Perfluorooctanoic acid (ND) 8 Perfluorooctane sulfonic acid (ND)



8 Perfluorooctane sulfonic acid (ND) * 7 13C4 PFOS 9 Perfluorononanoic acid (ND)



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_050.d
 Lims ID: 320-35207-A-4-A
 Client ID: NAWC-011818-FRB-316
 Sample Type: Client
 Inject. Date: 06-Feb-2018 19:01:13 ALS Bottle#: 37 Worklist Smp#: 9
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35207-a-4-a
 Misc. Info.: Plate: 1 Rack: 3
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Feb-2018 11:48:41 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: CTXT1

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	10.9	109.48
\$ 10 13C2 PFDA	10.0	10.0	100.34

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Client Sample ID: NAWC-011818-RW-260 Lab Sample ID: 320-35207-5
 Matrix: Water Lab File ID: 2018.02.06_537XX_051.d
 Analysis Method: 537 Date Collected: 01/18/2018 12:10
 Extraction Method: 537 Date Extracted: 01/31/2018 12:34
 Sample wt/vol: 244.2 (mL) Date Analyzed: 02/06/2018 19:05
 Con. Extract Vol.: 1.0 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 207292 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	23	J M	41	16	7.0
335-67-1	Perfluorooctanoic acid (PFOA)	24		20	8.2	2.9
375-95-1	Perfluorononanoic acid (PFNA)	20	U M	25	20	8.2
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	8.6	J	31	12	5.6
375-85-9	Perfluoroheptanoic acid (PFHpA)	7.0	J	10	4.1	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	16	J	92	37	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	104		70-130
STL00996	13C2 PFDA	105		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_051.d
 Lims ID: 320-35207-A-5-A
 Client ID: NAWC-011818-RW-260
 Sample Type: Client
 Inject. Date: 06-Feb-2018 19:05:53 ALS Bottle#: 38 Worklist Smp#: 10
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35207-a-5-a
 Misc. Info.: Plate: 1 Rack: 3
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Feb-2018 13:43:40 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: CTXT1

First Level Reviewer: krenns Date: 07-Feb-2018 13:43:40

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.373	1.366	0.007	1.000	482389	3.95		764	
298.90 > 99.00	1.373	1.366	0.007	1.000	356441		1.35(0.00-0.00)	942	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.487	1.479	0.008	1.000	1486079	10.4		8367	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.624	1.616	0.008	1.000	387110	2.11		328	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.624	1.616	0.008	1.000	208323	1.71		41.3	
* 6 13C2-PFOA									
415.00 > 370.00	1.806	1.791	0.015		1302427	10.0		6051	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.806	1.798	0.008	1.000	697644	5.79		95.7	
413.00 > 169.00	1.806	1.798	0.008	1.000	427954		1.63(0.00-0.00)	1158	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.048	2.041	0.007	1.000	581106	5.65		209	Ma
499.00 > 99.00	2.048	2.041	0.007	1.000	102017		5.70(0.00-0.00)	159	M
* 7 13C4 PFOS									
503.00 > 80.00	2.048	2.041	0.007		3143419	28.7		4616	
9 Perfluorononanoic acid									
463.00 > 419.00	2.056	2.048	0.008	1.000	53524	0.6188		7.3	M
\$ 10 13C2 PFDA									
515.00 > 470.00	2.238	2.231	0.007	1.000	1049547	10.5		7966	

QC Flag Legend

Review Flags

M - Manually Integrated

a - User Assigned ID

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_051.d

Injection Date: 06-Feb-2018 19:05:53

Instrument ID: A8_N

Lims ID: 320-35207-A-5-A

Lab Sample ID: 320-35207-5

Client ID: NAWC-011818-RW-260

Operator ID: SACINSTLCMS01

ALS Bottle#: 38

Worklist Smp#: 10

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

* 7 13C4 PFOS

9 Perfluorononanoic acid (M)



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_051.d
 Lims ID: 320-35207-A-5-A
 Client ID: NAWC-011818-RW-260
 Sample Type: Client
 Inject. Date: 06-Feb-2018 19:05:53 ALS Bottle#: 38 Worklist Smp#: 10
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35207-a-5-a
 Misc. Info.: Plate: 1 Rack: 3
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Feb-2018 13:43:40 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: CTXT1

First Level Reviewer: krenns Date: 07-Feb-2018 13:43:40

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	10.4	103.70
\$ 10 13C2 PFDA	10.0	10.5	105.31

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_051.d
Injection Date: 06-Feb-2018 19:05:53 Instrument ID: A8_N
Lims ID: 320-35207-A-5-A Lab Sample ID: 320-35207-5
Client ID: NAWC-011818-RW-260
Operator ID: SACINSTLCMS01 ALS Bottle#: 38 Worklist Smp#: 10
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.04

Processing Integration Results



RT: 2.05
Area: 581106
Amount: 5.646644
Amount Units: ng/ml

Manual Integration Results



Reviewer: krenns, 07-Feb-2018 13:42:59
Audit Action: Split an Integrated Peak

Audit Reason: Split Peak

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_051.d


Injection Date:	06-Feb-2018 19:05:53	Instrument ID:	A8_N		
Lims ID:	320-35207-A-5-A	Lab Sample ID:	320-35207-5		
Client ID:	NAWC-011818-RW-260				
Operator ID:	SACINSTLCMS01	ALS Bottle#:	38	Worklist Smp#:	10
Injection Vol:	2.0 ul	Dil. Factor:	1.0000		
Method:	537_A8_N	Limit Group:	LC 537 ICAL		
Column:		Detector:	EXP1		

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected
Expected RT: 2.04

Processing Integration Results



Manual Integration Results

RT: 2.05
Area: 102017
Amount: 5.646644
Amount Units: ng/ml



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_051.d
Injection Date: 06-Feb-2018 19:05:53 Instrument ID: A8_N
Lims ID: 320-35207-A-5-A Lab Sample ID: 320-35207-5
Client ID: NAWC-011818-RW-260
Operator ID: SACINSTLCMS01 ALS Bottle#: 38 Worklist Smp#: 10
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

9 Perfluorononanoic acid, CAS: 375-95-1

Signal: 1


Not Detected
Expected RT: 2.05

Processing Integration Results



RT: 2.06
Area: 53524
Amount: 0.618760
Amount Units: ng/ml

Manual Integration Results



Reviewer: krenns, 07-Feb-2018 13:43:14
Audit Action: Manually Integrated

Audit Reason: Split Peak

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Client Sample ID: NAWC-011818-FRB-260 Lab Sample ID: 320-35207-6
 Matrix: Water Lab File ID: 2018.02.06_537XX_054.d
 Analysis Method: 537 Date Collected: 01/18/2018 12:05
 Extraction Method: 537 Date Extracted: 01/31/2018 12:34
 Sample wt/vol: 250.8(mL) Date Analyzed: 02/06/2018 19:19
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 207294 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	8.0	U	20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.0	U	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	104		70-130
STL00996	13C2 PFDA	102		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_054.d
 Lims ID: 320-35207-A-6-A
 Client ID: NAWC-011818-FRB-260
 Sample Type: Client
 Inject. Date: 06-Feb-2018 19:19:53 ALS Bottle#: 39 Worklist Smp#: 13
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35207-a-6-a
 Misc. Info.: Plate: 1 Rack: 3
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Feb-2018 11:50:42 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d


Column 1 : Det: EXP1
 Process Host: CTXT1

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
\$ 2 13C2 PFHxA	315.00 > 270.00	1.487	1.479	0.008	1.000	1493114	10.4	8674	
* 6 13C2-PFOA	415.00 > 370.00	1.798	1.791	0.007		1299420	10.0	5251	
* 7 13C4 PFOS	503.00 > 80.00	2.048	2.041	0.007		3069150	28.7	7302	
\$ 10 13C2 PFDA	515.00 > 470.00	2.238	2.231	0.007	1.000	1017486	10.2	8117	


TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_054.d
Injection Date: 06-Feb-2018 19:19:53 Instrument ID: A8_N
Lims ID: 320-35207-A-6-A Lab Sample ID: 320-35207-6
Client ID: NAWC-011818-FRB-260
Operator ID: SACINSTLCMS01 ALS Bottle#: 39 Worklist Smp#: 13
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL


1 Perfluorobutanesulfonic acid (ND) 1 Perfluorobutanesulfonic acid (ND) \$ 2 13C2 PFHxA




3 Perfluorohexanesulfonic acid (ND) 4 Perfluoroheptanoic acid (ND) * 6 13C2-PFOA




5 Perfluorooctanoic acid (ND) 5 Perfluorooctanoic acid (ND) 8 Perfluorooctane sulfonic acid (ND)



8 Perfluorooctane sulfonic acid (ND) * 7 13C4 PFOS 9 Perfluorononanoic acid (ND)



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_054.d
 Lims ID: 320-35207-A-6-A
 Client ID: NAWC-011818-FRB-260
 Sample Type: Client
 Inject. Date: 06-Feb-2018 19:19:53 ALS Bottle#: 39 Worklist Smp#: 13
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35207-a-6-a
 Misc. Info.: Plate: 1 Rack: 3
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Feb-2018 11:50:42 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: CTXT1

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	10.4	104.43
\$ 10 13C2 PFDA	10.0	10.2	102.33

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Client Sample ID: NAWC-011818-RW-281 Lab Sample ID: 320-35207-7
 Matrix: Water Lab File ID: 2018.02.06_537XX_055.d
 Analysis Method: 537 Date Collected: 01/18/2018 13:10
 Extraction Method: 537 Date Extracted: 01/31/2018 12:34
 Sample wt/vol: 247.5 (mL) Date Analyzed: 02/06/2018 19:24
 Con. Extract Vol.: 1.0 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 207294 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	13	J M	40	16	6.9
335-67-1	Perfluorooctanoic acid (PFOA)	15	J	20	8.1	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	8.1
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	6.4	J	30	12	5.6
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.4	J	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	91	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	99		70-130
STL00996	13C2 PFDA	103		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_055.d
 Lims ID: 320-35207-A-7-A
 Client ID: NAWC-011818-RW-281
 Sample Type: Client
 Inject. Date: 06-Feb-2018 19:24:34 ALS Bottle#: 40 Worklist Smp#: 14
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35207-a-7-a
 Misc. Info.: Plate: 1 Rack: 3
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Feb-2018 11:50:42 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: CTXT1

First Level Reviewer: krenns Date: 07-Feb-2018 11:48:31

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.373	1.366	0.007	1.000	132668	1.06		242	
298.90 > 99.00	1.373	1.366	0.007	1.000	93920		1.41(0.00-0.00)	216	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.487	1.479	0.008	1.000	1470060	9.86		8022	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.631	1.616	0.015	1.000	294889	1.57		298	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.631	1.616	0.015	1.000	139228	1.10		30.7	
* 6 13C2-PFOA									
415.00 > 370.00	1.806	1.791	0.015		1354367	10.0		5682	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.806	1.798	0.008	1.000	463652	3.70		68.2	
413.00 > 169.00	1.806	1.798	0.008	1.000	280697		1.65(0.00-0.00)	818	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.048	2.041	0.007	1.000	342340	3.26		114	a
499.00 > 99.00	2.048	2.041	0.007	1.000	55879		6.13(0.00-0.00)	95.1	a
* 7 13C4 PFOS									
503.00 > 80.00	2.048	2.041	0.007		3207550	28.7		4338	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.238	2.231	0.007	1.000	1066122	10.3		7086	

QC Flag Legend

Review Flags

a - User Assigned ID




TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_055.d
Injection Date: 06-Feb-2018 19:24:34 Instrument ID: A8_N
Lims ID: 320-35207-A-7-A Lab Sample ID: 320-35207-7
Client ID: NAWC-011818-RW-281
Operator ID: SACINSTLCMS01 ALS Bottle#: 40 Worklist Smp#: 14
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid

* 7 13C4 PFOS

9 Perfluorononanoic acid (ND)



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_055.d
 Lims ID: 320-35207-A-7-A
 Client ID: NAWC-011818-RW-281
 Sample Type: Client
 Inject. Date: 06-Feb-2018 19:24:34 ALS Bottle#: 40 Worklist Smp#: 14
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35207-a-7-a
 Misc. Info.: Plate: 1 Rack: 3
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Feb-2018 11:50:42 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: CTXT1

First Level Reviewer: krenns Date: 07-Feb-2018 11:48:31

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	9.86	98.65
\$ 10 13C2 PFDA	10.0	10.3	102.87

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_055.d
Injection Date: 06-Feb-2018 19:24:34 Instrument ID: A8_N
Lims ID: 320-35207-A-7-A Lab Sample ID: 320-35207-7
Client ID: NAWC-011818-RW-281
Operator ID: SACINSTLCMS01 ALS Bottle#: 40 Worklist Smp#: 14
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1


Signal: 1

Not Detected
Expected RT: 2.04

Processing Integration Results



Manual Integration Results



RT: 2.05
Area: 342340
Amount: 3.260029
Amount Units: ng/ml

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Client Sample ID: NAWC-011818-FRB-281 Lab Sample ID: 320-35207-8
 Matrix: Water Lab File ID: 2018.02.06_537XX_056.d
 Analysis Method: 537 Date Collected: 01/18/2018 13:05
 Extraction Method: 537 Date Extracted: 01/31/2018 12:34
 Sample wt/vol: 249.6(mL) Date Analyzed: 02/06/2018 19:29
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 207294 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	8.0	U	20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.0	U	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	103		70-130
STL00996	13C2 PFDA	102		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_056.d
 Lims ID: 320-35207-A-8-A
 Client ID: NAWC-011818-FRB-281
 Sample Type: Client
 Inject. Date: 06-Feb-2018 19:29:15 ALS Bottle#: 41 Worklist Smp#: 15
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35207-a-8-a
 Misc. Info.: Plate: 1 Rack: 3
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Feb-2018 11:50:42 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d


Column 1 : Det: EXP1
 Process Host: CTXT1

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
\$ 2 13C2 PFHxA	315.00 > 270.00	1.487	1.479	0.008	1.000	1539315	10.3	8577	
* 6 13C2-PFOA	415.00 > 370.00	1.806	1.791	0.015		1354309	10.0	6044	
* 7 13C4 PFOS	503.00 > 80.00	2.048	2.041	0.007		3260304	28.7	8096	
\$ 10 13C2 PFDA	515.00 > 470.00	2.238	2.231	0.007	1.000	1053106	10.2	7228	


TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_056.d
Injection Date: 06-Feb-2018 19:29:15 Instrument ID: A8_N
Lims ID: 320-35207-A-8-A Lab Sample ID: 320-35207-8
Client ID: NAWC-011818-FRB-281
Operator ID: SACINSTLCMS01 ALS Bottle#: 41 Worklist Smp#: 15
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL


1 Perfluorobutanesulfonic acid (ND) 1 Perfluorobutanesulfonic acid (ND) \$ 2 13C2 PFHxA




3 Perfluorohexanesulfonic acid (ND) 4 Perfluoroheptanoic acid (ND) * 6 13C2-PFOA




5 Perfluorooctanoic acid (ND) 5 Perfluorooctanoic acid (ND) 8 Perfluorooctane sulfonic acid (ND)



8 Perfluorooctane sulfonic acid (ND) * 7 13C4 PFOS 9 Perfluorononanoic acid (ND)



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_056.d
 Lims ID: 320-35207-A-8-A
 Client ID: NAWC-011818-FRB-281
 Sample Type: Client
 Inject. Date: 06-Feb-2018 19:29:15 ALS Bottle#: 41 Worklist Smp#: 15
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35207-a-8-a
 Misc. Info.: Plate: 1 Rack: 3
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Feb-2018 11:50:42 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: CTXT1

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	10.3	103.30
\$ 10 13C2 PFDA	10.0	10.2	101.62

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Client Sample ID: NAWC-011818-RW-032 Lab Sample ID: 320-35207-9
 Matrix: Water Lab File ID: 2018.02.06_537XX_057.d
 Analysis Method: 537 Date Collected: 01/18/2018 13:40
 Extraction Method: 537 Date Extracted: 01/31/2018 12:34
 Sample wt/vol: 247.2 (mL) Date Analyzed: 02/06/2018 19:33
 Con. Extract Vol.: 1.0 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 207294 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	20	J M	40	16	6.9
335-67-1	Perfluorooctanoic acid (PFOA)	16	J	20	8.1	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	8.1
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	14	J	30	12	5.6
375-85-9	Perfluoroheptanoic acid (PFHpA)	5.4	J	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	91	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	88		70-130
STL00996	13C2 PFDA	104		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_057.d
 Lims ID: 320-35207-A-9-A
 Client ID: NAWC-011818-RW-032
 Sample Type: Client
 Inject. Date: 06-Feb-2018 19:33:55 ALS Bottle#: 42 Worklist Smp#: 16
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35207-a-9-a
 Misc. Info.: Plate: 1 Rack: 3
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Feb-2018 11:50:42 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: CTXT1

First Level Reviewer: krenns Date: 07-Feb-2018 11:49:58

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.373	1.366	0.007	1.000	147089	1.20		227	
298.90 > 99.00	1.366	1.366	0.0	0.994	114277		1.29(0.00-0.00)	269	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.487	1.479	0.008	1.000	1234153	8.76		6809	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.624	1.616	0.008	1.000	639242	3.49		648	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.624	1.616	0.008	1.000	159840	1.33		36.1	
* 6 13C2-PFOA									
415.00 > 370.00	1.806	1.791	0.015		1279796	10.0		6290	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.806	1.798	0.008	1.000	456468	3.85		63.6	
413.00 > 169.00	1.798	1.798	0.0	0.996	267891		1.70(0.00-0.00)	738	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.048	2.041	0.007	1.000	505102	4.92		216	a
499.00 > 99.00	2.048	2.041	0.007	1.000	98991		5.10(0.00-0.00)	169	a
* 7 13C4 PFOS									
503.00 > 80.00	2.048	2.041	0.007		3134922	28.7		5020	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.238	2.231	0.007	1.000	1016770	10.4		6622	

QC Flag Legend

Review Flags

a - User Assigned ID




TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_057.d
Injection Date: 06-Feb-2018 19:33:55 Instrument ID: A8_N
Lims ID: 320-35207-A-9-A Lab Sample ID: 320-35207-9
Client ID: NAWC-011818-RW-032
Operator ID: SACINSTLCMS01 ALS Bottle#: 42 Worklist Smp#: 16
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid

* 7 13C4 PFOS

9 Perfluorononanoic acid (ND)



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_057.d
 Lims ID: 320-35207-A-9-A
 Client ID: NAWC-011818-RW-032
 Sample Type: Client
 Inject. Date: 06-Feb-2018 19:33:55 ALS Bottle#: 42 Worklist Smp#: 16
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35207-a-9-a
 Misc. Info.: Plate: 1 Rack: 3
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Feb-2018 11:50:42 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: CTXT1

First Level Reviewer: krenns Date: 07-Feb-2018 11:49:58

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	8.76	87.64
\$ 10 13C2 PFDA	10.0	10.4	103.83

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_057.d
Injection Date: 06-Feb-2018 19:33:55 Instrument ID: A8_N
Lims ID: 320-35207-A-9-A Lab Sample ID: 320-35207-9
Client ID: NAWC-011818-RW-032
Operator ID: SACINSTLCMS01 ALS Bottle#: 42 Worklist Smp#: 16
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.04

Processing Integration Results



RT: 2.05
Area: 505102
Amount: 4.921411
Amount Units: ng/ml

Manual Integration Results



Reviewer: krenns, 07-Feb-2018 11:49:51
Audit Action: Assigned Compound ID

Audit Reason: User Assigned

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Client Sample ID: NAWC-011818-FRB-032 Lab Sample ID: 320-35207-10
 Matrix: Water Lab File ID: 2018.02.06_537XX_058.d
 Analysis Method: 537 Date Collected: 01/18/2018 13:35
 Extraction Method: 537 Date Extracted: 01/31/2018 12:34
 Sample wt/vol: 244.2 (mL) Date Analyzed: 02/06/2018 19:38
 Con. Extract Vol.: 1.0 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 207294 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	41	16	7.0
335-67-1	Perfluorooctanoic acid (PFOA)	8.2	U	20	8.2	2.9
375-95-1	Perfluorononanoic acid (PFNA)	20	U	25	20	8.2
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	31	12	5.6
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.1	U	10	4.1	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	37	U	92	37	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	104		70-130
STL00996	13C2 PFDA	105		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_058.d
 Lims ID: 320-35207-A-10-A
 Client ID: NAWC-011818-FRB-032
 Sample Type: Client
 Inject. Date: 06-Feb-2018 19:38:37 ALS Bottle#: 43 Worklist Smp#: 17
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35207-a-10-a
 Misc. Info.: Plate: 1 Rack: 3
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Feb-2018 11:50:42 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d


Column 1 : Det: EXP1
 Process Host: CTXT1

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
\$ 2 13C2 PFHxA	315.00 > 270.00	1.479	1.479	0.0	1.000	1448921	10.4	8362	
* 6 13C2-PFOA	415.00 > 370.00	1.798	1.791	0.007		1269005	10.0	5577	
* 7 13C4 PFOS	503.00 > 80.00	2.041	2.041	0.0		3041394	28.7	7562	
\$ 10 13C2 PFDA	515.00 > 470.00	2.238	2.231	0.007	1.000	1022296	10.5	8293	


TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_058.d
Injection Date: 06-Feb-2018 19:38:37 Instrument ID: A8_N
Lims ID: 320-35207-A-10-A Lab Sample ID: 320-35207-10
Client ID: NAWC-011818-FRB-032
Operator ID: SACINSTLCMS01 ALS Bottle#: 43 Worklist Smp#: 17
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL


1 Perfluorobutanesulfonic acid (ND) 1 Perfluorobutanesulfonic acid (ND) \$ 2 13C2 PFHxA




3 Perfluorohexanesulfonic acid (ND) 4 Perfluoroheptanoic acid (ND) * 6 13C2-PFOA




5 Perfluorooctanoic acid (ND) 5 Perfluorooctanoic acid (ND) 8 Perfluorooctane sulfonic acid (ND)



8 Perfluorooctane sulfonic acid (ND) * 7 13C4 PFOS 9 Perfluorononanoic acid (ND)



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_058.d
 Lims ID: 320-35207-A-10-A
 Client ID: NAWC-011818-FRB-032
 Sample Type: Client
 Inject. Date: 06-Feb-2018 19:38:37 ALS Bottle#: 43 Worklist Smp#: 17
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35207-a-10-a
 Misc. Info.: Plate: 1 Rack: 3
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Feb-2018 11:50:42 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: CTXT1

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	10.4	103.77
\$ 10 13C2 PFDA	10.0	10.5	105.28

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Client Sample ID: NAWC-011818-RW-038 Lab Sample ID: 320-35207-11
 Matrix: Water Lab File ID: 2018.02.06_537XX_059.d
 Analysis Method: 537 Date Collected: 01/18/2018 14:10
 Extraction Method: 537 Date Extracted: 01/31/2018 12:34
 Sample wt/vol: 249.6(mL) Date Analyzed: 02/06/2018 19:43
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 207294 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	25	J M	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	21		20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	6.2	J	30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	5.6	J	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	90		70-130
STL00996	13C2 PFDA	97		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_059.d
 Lims ID: 320-35207-A-11-A
 Client ID: NAWC-011818-RW-038
 Sample Type: Client
 Inject. Date: 06-Feb-2018 19:43:18 ALS Bottle#: 44 Worklist Smp#: 18
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35207-a-11-a
 Misc. Info.: Plate: 1 Rack: 3
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Feb-2018 13:44:24 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: CTXT1

First Level Reviewer: krenns Date: 07-Feb-2018 11:50:18

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.366	1.366	0.0	1.000	325257	2.48		103	
298.90 > 99.00	1.366	1.366	0.0	1.000	213687		1.52(0.00-0.00)	369	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.479	1.479	0.0	1.000	1365904	9.04		6279	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.616	1.616	0.0	1.000	302979	1.54		47.9	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.616	1.616	0.0	1.000	180257	1.40		15.0	
* 6 13C2-PFOA									
415.00 > 370.00	1.791	1.791	0.0		1373697	10.0		5786	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.798	1.798	0.0	1.000	679602	5.34		50.8	
413.00 > 169.00	1.791	1.798	-0.007	0.996	420736		1.62(0.00-0.00)	969	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.041	2.041	0.0	1.000	684252	6.20		90.9	Ma
499.00 > 99.00	2.041	2.041	0.0	1.000	115574		5.92(0.00-0.00)	118	M
* 7 13C4 PFOS									
503.00 > 80.00	2.041	2.041	0.0		3369231	28.7		1299	
9 Perfluorononanoic acid									
463.00 > 419.00	2.048	2.048	0.0	1.000	72315	0.7926		6.7	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.231	2.231	0.0	1.000	1023599	9.74		8219	

QC Flag Legend

Review Flags

M - Manually Integrated

a - User Assigned ID




TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_059.d
Injection Date: 06-Feb-2018 19:43:18 Instrument ID: A8_N
Lims ID: 320-35207-A-11-A Lab Sample ID: 320-35207-11
Client ID: NAWC-011818-RW-038
Operator ID: SACINSTLCMS01 ALS Bottle#: 44 Worklist Smp#: 18
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_059.d
 Lims ID: 320-35207-A-11-A
 Client ID: NAWC-011818-RW-038
 Sample Type: Client
 Inject. Date: 06-Feb-2018 19:43:18 ALS Bottle#: 44 Worklist Smp#: 18
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35207-a-11-a
 Misc. Info.: Plate: 1 Rack: 3
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Feb-2018 13:44:24 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: CTXT1

First Level Reviewer: krenns Date: 07-Feb-2018 11:50:18

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	9.04	90.37
\$ 10 13C2 PFDA	10.0	9.74	97.38

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_059.d
Injection Date: 06-Feb-2018 19:43:18 Instrument ID: A8_N
Lims ID: 320-35207-A-11-A Lab Sample ID: 320-35207-11
Client ID: NAWC-011818-RW-038
Operator ID: SACINSTLCMS01 ALS Bottle#: 44 Worklist Smp#: 18
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.04

Processing Integration Results



RT: 2.04
Area: 684252
Amount: 6.203297
Amount Units: ng/ml

Manual Integration Results



Reviewer: krenns, 07-Feb-2018 13:44:06
Audit Action: Split an Integrated Peak

Audit Reason: Split Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_059.d
Injection Date: 06-Feb-2018 19:43:18 Instrument ID: A8_N
Lims ID: 320-35207-A-11-A Lab Sample ID: 320-35207-11
Client ID: NAWC-011818-RW-038
Operator ID: SACINSTLCMS01 ALS Bottle#: 44 Worklist Smp#: 18
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected
Expected RT: 2.04

Processing Integration Results



Manual Integration Results

RT: 2.04
Area: 115574
Amount: 6.203297
Amount Units: ng/ml



FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Client Sample ID: NAWC-011818-FRB-038 Lab Sample ID: 320-35207-12
 Matrix: Water Lab File ID: 2018.02.06_537XX_060.d
 Analysis Method: 537 Date Collected: 01/18/2018 14:05
 Extraction Method: 537 Date Extracted: 01/31/2018 12:34
 Sample wt/vol: 249.7(mL) Date Analyzed: 02/06/2018 19:47
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 207294 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	8.0	U	20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.0	U	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	107		70-130
STL00996	13C2 PFDA	102		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_060.d
 Lims ID: 320-35207-A-12-A
 Client ID: NAWC-011818-FRB-038
 Sample Type: Client
 Inject. Date: 06-Feb-2018 19:47:58 ALS Bottle#: 45 Worklist Smp#: 19
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35207-a-12-a
 Misc. Info.: Plate: 1 Rack: 3
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Feb-2018 11:50:42 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d


Column 1 : Det: EXP1
 Process Host: CTXT1

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
\$ 2 13C2 PFHxA	315.00 > 270.00	1.487	1.479	0.008	1.000	1603238	10.7	8979	
* 6 13C2-PFOA	415.00 > 370.00	1.798	1.791	0.007		1356647	10.0	6039	
* 7 13C4 PFOS	503.00 > 80.00	2.041	2.041	0.0		3181172	28.7	6067	
\$ 10 13C2 PFDA	515.00 > 470.00	2.238	2.231	0.007	1.000	1064026	10.2	7237	


TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_060.d
Injection Date: 06-Feb-2018 19:47:58 Instrument ID: A8_N
Lims ID: 320-35207-A-12-A Lab Sample ID: 320-35207-12
Client ID: NAWC-011818-FRB-038
Operator ID: SACINSTLCMS01 ALS Bottle#: 45 Worklist Smp#: 19
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL


1 Perfluorobutanesulfonic acid (ND) 1 Perfluorobutanesulfonic acid (ND) \$ 2 13C2 PFHxA




3 Perfluorohexanesulfonic acid (ND) 4 Perfluoroheptanoic acid (ND) * 6 13C2-PFOA




5 Perfluorooctanoic acid (ND) 5 Perfluorooctanoic acid (ND) 8 Perfluorooctane sulfonic acid (ND)



8 Perfluorooctane sulfonic acid (ND) * 7 13C4 PFOS 9 Perfluorononanoic acid (ND)



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_060.d
 Lims ID: 320-35207-A-12-A
 Client ID: NAWC-011818-FRB-038
 Sample Type: Client
 Inject. Date: 06-Feb-2018 19:47:58 ALS Bottle#: 45 Worklist Smp#: 19
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-35207-a-12-a
 Misc. Info.: Plate: 1 Rack: 3
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Feb-2018 11:50:42 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: CTXT1

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	10.7	107.40
\$ 10 13C2 PFDA	10.0	10.2	102.50

FORM VI
LCMS BY INTERNAL STANDARD - INITIAL CALIBRATION DATA
CURVE EVALUATION

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1 Analy Batch No.: 192908

SDG No.: _____

Instrument ID: A8_N GC Column: GeminiC18 3 ID: 3(mm) Heated Purge: (Y/N) N

Calibration Start Date: 11/03/2017 13:37 Calibration End Date: 11/03/2017 14:01 Calibration ID: 36012

Calibration Files:

LEVEL:	LAB SAMPLE ID:	LAB FILE ID:
Level 1	IC 320-192908/4	2017.11.03_537XICAL_004.d
Level 2	IC 320-192908/5	2017.11.03_537XICAL_005.d
Level 3	IC 320-192908/6	2017.11.03_537XICAL_006.d
Level 4	IC 320-192908/7	2017.11.03_537XICAL_007.d
Level 5	IC 320-192908/8	2017.11.03_537XICAL_008.d
Level 6	IC 320-192908/9	2017.11.03_537XICAL_009.d

ANALYTE	RRF					CURVE TYPE	COEFFICIENT			#	MIN RRF	%RSD	#	MAX %RSD	R ² OR COD	#	MIN R ² OR COD
	LVL 1 LVL 6	LVL 2	LVL 3	LVL 4	LVL 5		B	M1	M2								
Perfluorobutanesulfonic acid (PFBS)	1.0397 0.8468	1.0767	1.0898	0.9577	0.9303	QuaF		1.1193	-0.001498					0.9990			0.9600
Perfluoroheptanoic acid (PFHpA)	0.9433 0.9848	0.9187	0.9551	0.9185	0.9011	Ave		0.9369			3.2		30.0				
Perfluorohexanesulfonic acid (PFHxS)	1.6459 1.6841	1.6355	1.7405	1.6631	1.6755	Ave		1.6741			2.2		30.0				
Perfluorooctanoic acid (PFOA)	0.9757 0.9799	0.8919	0.9000	0.8953	0.9117	Ave		0.9258			4.4		30.0				
Perfluorooctanesulfonic acid (PFOS)	0.8958 0.9902	0.9213	0.9281	0.9268	0.9715	Ave		0.9389			3.7		30.0				
Perfluorononanoic acid (PFNA)	0.6610 0.7042	0.6285	0.6624	0.6810	0.6478	Ave		0.6642			3.9		30.0				
13C2 PFHxA	1.0891 1.1664	1.0526	1.1042	1.1123	1.0772	Ave		1.1003			3.5		30.0				
13C2 PFDA	0.7748 0.8159	0.7295	0.7569	0.7811	0.7330	Ave		0.7652			4.3		30.0				

Note: The M1 coefficient is the same as Ave RRF for an Ave curve type.

FORM VI
LCMS BY INTERNAL STANDARD - INITIAL CALIBRATION DATA
RESPONSE AND CONCENTRATION

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1 Analy Batch No.: 192908

SDG No.: _____

Instrument ID: A8_N GC Column: GeminiC18 3 ID: 3(mm) Heated Purge: (Y/N) N

Calibration Start Date: 11/03/2017 13:37 Calibration End Date: 11/03/2017 14:01 Calibration ID: 36012

Calibration Files:

LEVEL:	LAB SAMPLE ID:	LAB FILE ID:
Level 1	IC 320-192908/4	2017.11.03_537XICAL_004.d
Level 2	IC 320-192908/5	2017.11.03_537XICAL_005.d
Level 3	IC 320-192908/6	2017.11.03_537XICAL_006.d
Level 4	IC 320-192908/7	2017.11.03_537XICAL_007.d
Level 5	IC 320-192908/8	2017.11.03_537XICAL_008.d
Level 6	IC 320-192908/9	2017.11.03_537XICAL_009.d

ANALYTE	IS REF	CURVE TYPE	RESPONSE					CONCENTRATION (NG/ML)				
			LVL 1 LVL 6	LVL 2	LVL 3	LVL 4	LVL 5	LVL 1 LVL 6	LVL 2	LVL 3	LVL 4	LVL 5
Perfluorobutanesulfonic acid (PFBS)	PFOS	QuaF	1076553 16699152	2591121	5461974	10142530	14011858	9.00 180	20.0	45.0	90.0	135
Perfluoroheptanoic acid (PFHpA)	13PF OA	Ave	143455 2810797	331548	736034	1420703	2102676	1.00 20.0	2.22	5.00	10.0	15.0
Perfluorohexanesulfonic acid (PFHxS)	PFOS	Ave	568156 11071993	1312135	2908204	5871843	8413133	3.00 60.0	6.67	15.0	30.0	45.0
Perfluorooctanoic acid (PFOA)	13PF OA	Ave	296934 5597122	644149	1388033	2771271	4257225	2.00 40.0	4.45	10.0	20.0	30.0
Perfluorooctanesulfonic acid (PFOS)	PFOS	Ave	412315 8679676	985487	2067792	4363079	6504279	4.00 80.0	8.89	20.0	40.0	60.0
Perfluorononanoic acid (PFNA)	13PF OA	Ave	201053 4019666	453612	1020851	2106479	3023088	2.00 40.0	4.45	10.0	20.0	30.0
13C2 PFHxA	13PF OA	Ave	1655691 1664260	1708988	1701491	1719911	1675220	10.0 10.0	10.0	10.0	10.0	10.0
13C2 PFDA	13PF OA	Ave	1177922 1164156	1184358	1166275	1207887	1139992	10.0 10.0	10.0	10.0	10.0	10.0

Curve Type Legend:

Ave = Average ISTD
QuaF = Quadratic ISTD forced zero

FORM VI
 LCMS BY INTERNAL STANDARD - INITIAL CALIBRATION DATA
 READBACK PERCENT ERROR

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1 Analy Batch No.: 192908

SDG No.: _____


Instrument ID: A8_N GC Column: GeminiC18 3 ID: 3 (mm) Heated Purge: (Y/N) N


Calibration Start Date: 11/03/2017 13:37 Calibration End Date: 11/03/2017 14:01 Calibration ID: 36012

Calibration Files:

LEVEL:	LAB SAMPLE ID:	LAB FILE ID:
Level 1	IC 320-192908/4	2017.11.03_537XICAL_004.d
Level 2	IC 320-192908/5	2017.11.03_537XICAL_005.d
Level 3	IC 320-192908/6	2017.11.03_537XICAL_006.d
Level 4	IC 320-192908/7	2017.11.03_537XICAL_007.d
Level 5	IC 320-192908/8	2017.11.03_537XICAL_008.d
Level 6	IC 320-192908/9	2017.11.03_537XICAL_009.d

ANALYTE	PERCENT ERROR						PERCENT ERROR LIMIT					
	LVL 1 #	LVL 2 #	LVL 3 #	LVL 4 #	LVL 5 #	LVL 6 #	LVL 1	LVL 2	LVL 3	LVL 4	LVL 5	LVL 6
Perfluorobutanesulfonic acid (PFBS)	-6.0	-1.2	3.9	-3.1	1.9	-0.5	50	30	30	30	30	30
Perfluoroheptanoic acid (PFHpA)	0.7	-1.9	1.9	-2.0	-3.8	5.1	50	30	30	30	30	30
Perfluorohexanesulfonic acid (PFHxS)	-1.7	-2.3	4.0	-0.7	0.1	0.6	50	30	30	30	30	30
Perfluorooctanoic acid (PFOA)	5.4	-3.7	-2.8	-3.3	-1.5	5.8	50	30	30	30	30	30
Perfluorooctanesulfonic acid (PFOS)	-4.6	-1.9	-1.2	-1.3	3.5	5.5	50	30	30	30	30	30
Perfluorononanoic acid (PFNA)	-0.5	-5.4	-0.3	2.5	-2.5	6.0	50	30	30	30	30	30
13C2 PFHxA	-1.0	-4.3	0.4	1.1	-2.1	6.0	30	30	30	30	30	30
13C2 PFDA	1.3	-4.7	-1.1	2.1	-4.2	6.6	30	30	30	30	30	30



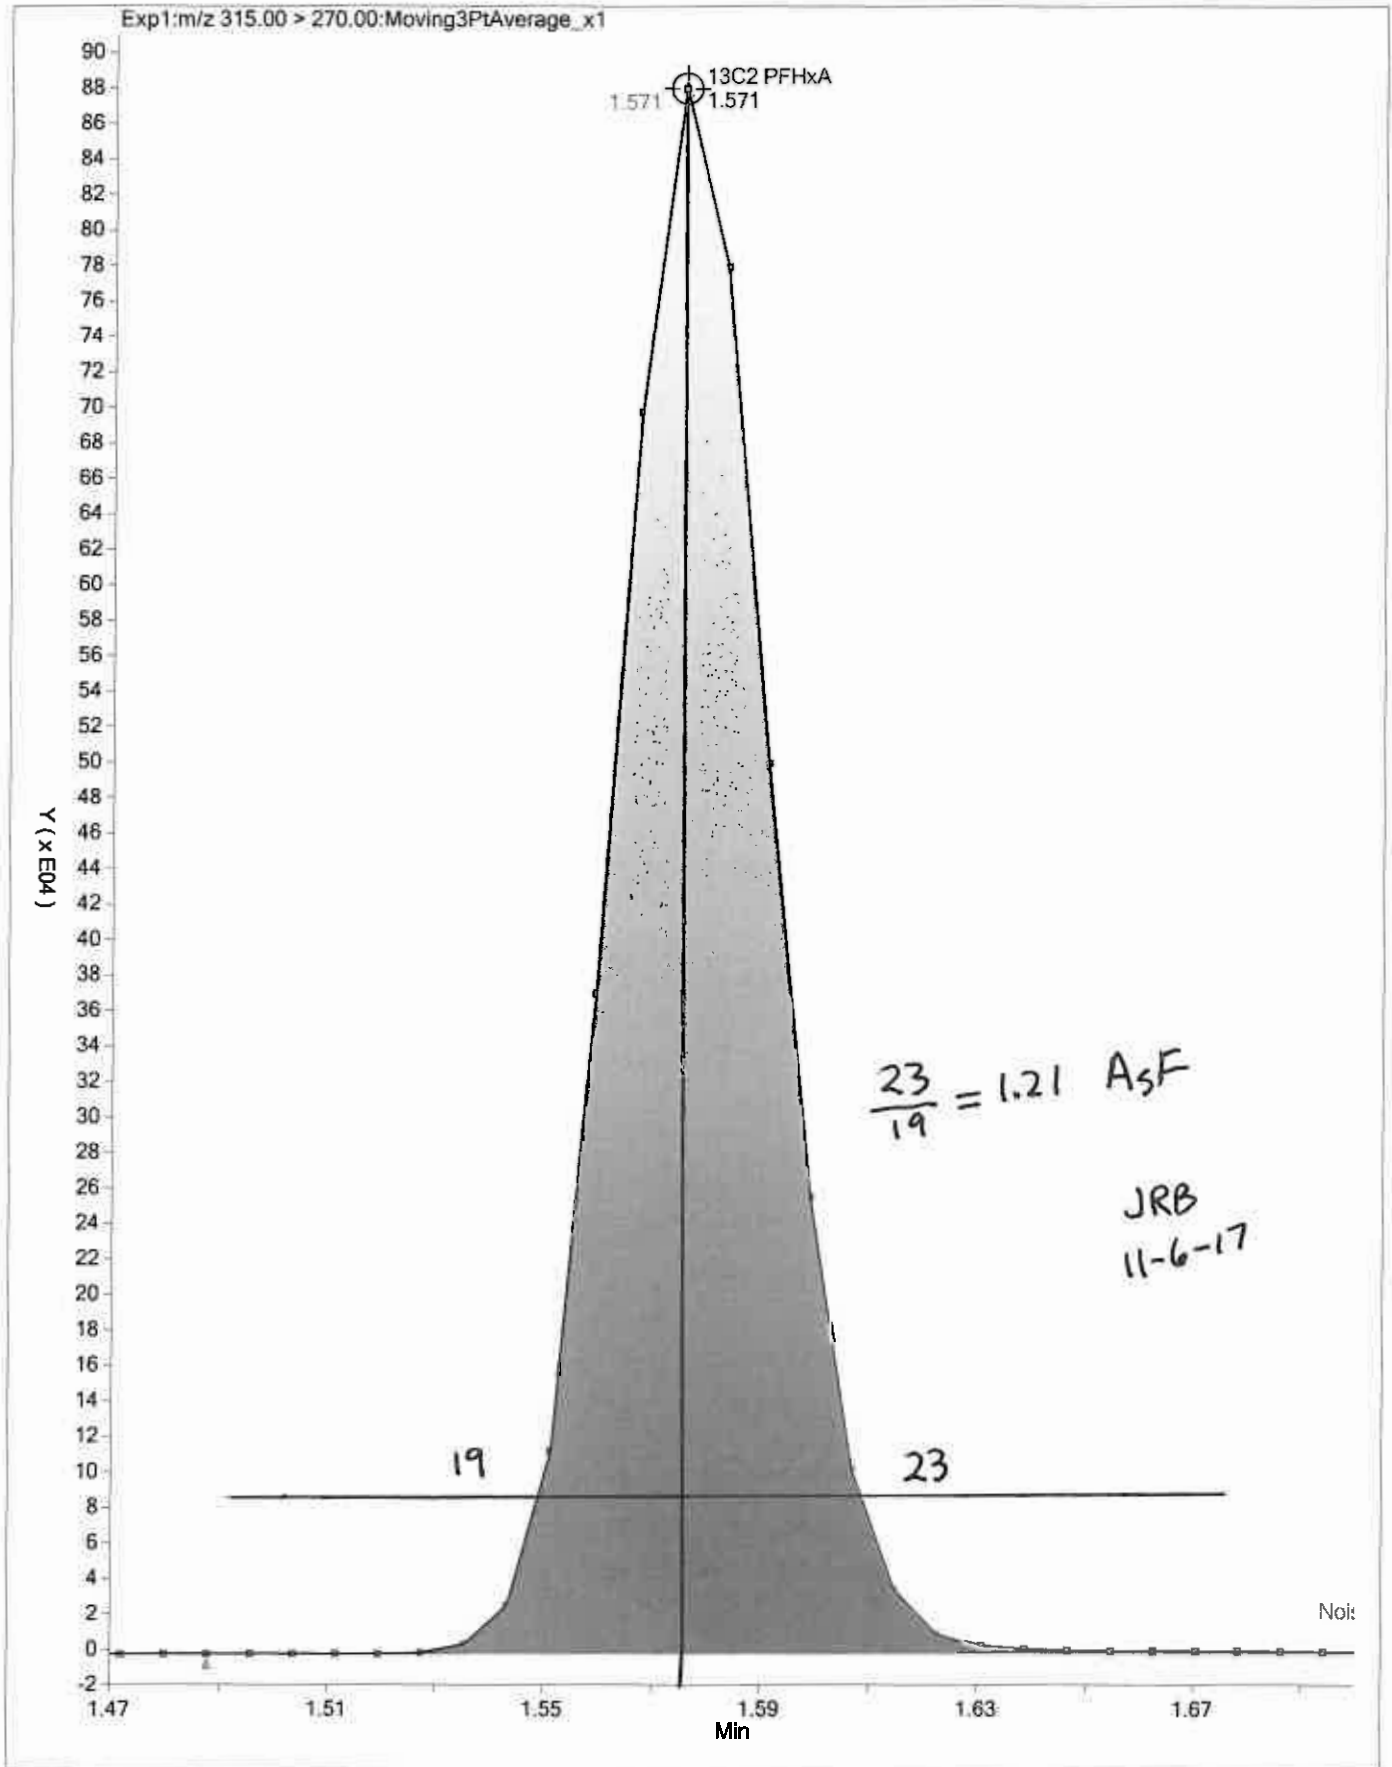

TestAmerica Laboratories
Istd/Surrogate Recovery Report

Worklist Name: 03NOV2017_537A_ICAL

Worklist Num: 49975

Instrument: A8_N

Method: 537_A8_N

Batch Directory: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b

Limit Group: LC 537 ICAL

Analysis Type: SemiVOA

Inj Volume: 2.00

Inj Vol Units: ul

Lims Batch: 192908

CCV IS Mode: Select Ical Level, Cal Level: 3

Non-Cal IS Mode: Last Ccal Sample

\$ 2 13C2 PFHxA

\$ 10 13C2 PFDA

Lab ID	Inj Date	\$ 2	\$ 10	* 6 13C2-PFOA	* 7 13C4 PFOS
	IS Std			2864400 1.87	6253426 2.11
# 1 RB	03-Nov-2017 13:23:59			1485386 51.9	3471256 55.5
# 2 RB	03-Nov-2017 13:28:38			1511056 52.8	3340239 53.4
# 3 RB	03-Nov-2017 13:33:19			1483949 51.8	3285228 52.5
	IS Std				
# 4 IC L1	03-Nov-2017 13:37:59	1.58 98.98	2.31 101.30	1520258> 100.0*	3298877> 100.0*
# 5 IC L2	03-Nov-2017 13:42:39	1.58 95.66	2.31 95.33	1623614> 106.8*	3450592> 104.6*
# 6 IC L3	03-Nov-2017 13:47:20	1.57 100.40	2.31 98.91	1540946> 101.4*	3194016> 96.8*
# 7 IC L4	03-Nov-2017 13:52:00	1.57 101.10	2.31 102.10	1546307> 101.7*	3374600> 102.3*
# 8 IC L5	03-Nov-2017 13:56:41	1.57 97.90	2.31 95.80	1555174> 102.3*	3199479> 97.0*
# 9 IC L6	03-Nov-2017 14:01:24	1.57 106.00	2.31 106.60	1426806> 93.9*	3141787> 95.2*
	IS Std			1540946 1.91	3194016 2.15
#10 RB	03-Nov-2017 14:06:04			1395383 90.6	3212781 100.6
	IS Std			1546307 1.91	3374600 2.16
#11 CCVL	03-Nov-2017 14:10:44	1.58 97.03	2.31 97.49	1586829 102.6	3305852 98.0
	IS Std			1586829 1.91	3305852 2.15
#12 RB	03-Nov-2017 14:15:23			1415042 89.2	3122656 94.5
	IS Std			1546307 1.91	3374600 2.16
#13 ICV	03-Nov-2017 14:20:03	1.57 94.41	2.31 96.59	1512045 97.8	3433628 101.7
	IS Std			1395100 1.91	3254950 2.15
#14 RB	03-Nov-2017 14:24:44			1395100 100.0	3254950 100.0

13C2-PFOA

$$RPD = \frac{1623614 - 1426806}{\left(\frac{1623614 + 1426806}{2}\right)} (100) = 12.9$$

13C4-PFOS

$$RPD = \frac{3450592 - 3141787}{\left(\frac{3450592 + 3141787}{2}\right)} (100) = 9.37$$

JRB
11-6-17

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_004.d
 Lims ID: IC L1
 Client ID:
 Sample Type: IC Calib Level: 1
 Inject. Date: 03-Nov-2017 13:37:59 ALS Bottle#: 1 Worklist Smp#: 4
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: L1_537
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub1

Method: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Nov-2017 15:52:07 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last Ical File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK021

First Level Reviewer: phomsophat Date: 06-Nov-2017 07:18:01

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.449	1.444	0.005	1.000	1076553	8.46		654	
298.90 > 99.00	1.449	1.444	0.005	1.000	763262		1.41(0.00-0.00)	2025	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.578	1.573	0.005	1.000	1655691	9.90		8732	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.730	1.725	0.005	1.000	568156	2.95		1122	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.730	1.725	0.005	1.000	143455	1.01		42.2	
* 6 13C2-PFOA									
415.00 > 370.00	1.920	1.913	0.007		1520258	10.0		6863	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.920	1.914	0.006	1.000	296934	2.11		53.5	
413.00 > 169.00	1.920	1.914	0.006	1.000	149720		1.98(0.00-0.00)	184	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.155	2.147	0.008	1.000	412315	3.82		235	M
499.00 > 99.00	2.155	2.147	0.008	1.000	85347		4.83(0.00-0.00)	209	M
* 7 13C4 PFOS									
503.00 > 80.00	2.155	2.151	0.004		3298877	28.7		5279	
9 Perfluorononanoic acid									
463.00 > 419.00	2.162	2.158	0.004	1.000	201053	1.99		67.8	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.314	2.312	0.002	1.000	1177922	10.1		7012	

QC Flag Legend

Review Flags

M - Manually Integrated

Reagents:

LC537-L1_00020

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537ICAL_004.d

Injection Date: 03-Nov-2017 13:37:59

Instrument ID: A8_N

Lims ID: IC L1

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 1

Worklist Smp#: 4

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)

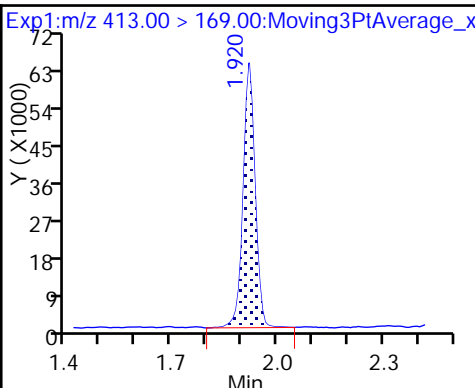


8 Perfluorooctane sulfonic acid (M)

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_004.d
Injection Date: 03-Nov-2017 13:37:59 Instrument ID: A8_N
Lims ID: IC L1
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 1 Worklist Smp#: 4
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.15

Processing Integration Results



Manual Integration Results

RT: 2.15
Area: 412315
Amount: 3.817687
Amount Units: ng/ml



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\201711106-49975.b\2017.11.03_537XICAL_004.d
Injection Date: 03-Nov-2017 13:37:59 Instrument ID: A8_N
Lims ID: IC L1
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 1 Worklist Smp#: 4
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected
Expected RT: 2.15

Processing Integration Results

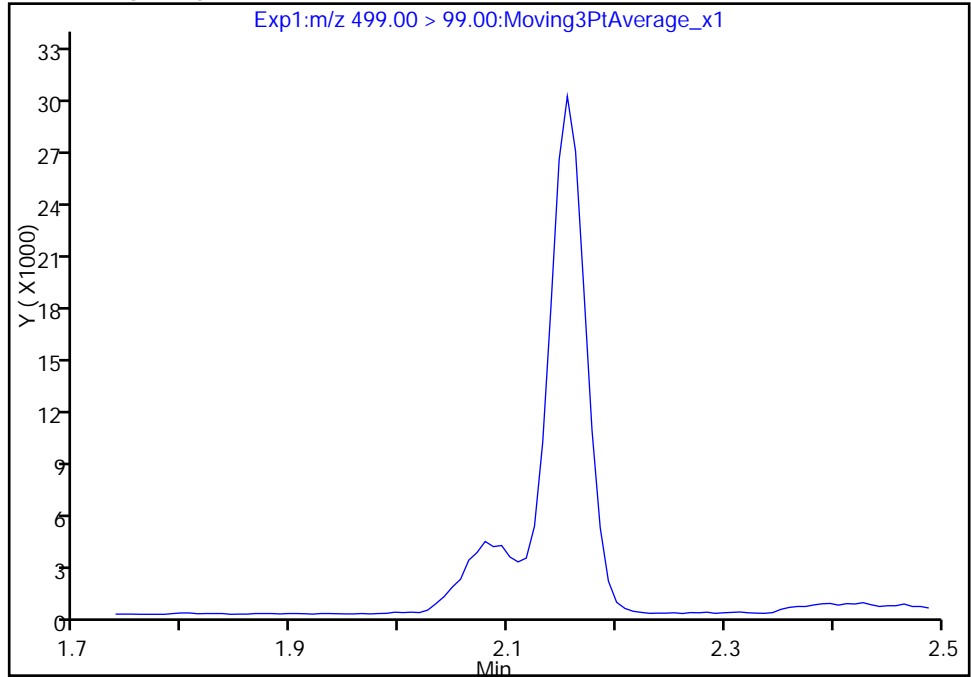

Manual Integration Results

RT: 2.15
Area: 85347
Amount: 3.817687
Amount Units: ng/ml



Reviewer: phomsophat, 06-Nov-2017 07:17:37

Audit Action: Manually Integrated

Audit Reason: Assign Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\201711106-49975.b\2017.11.03_537XICAL_004.d
Injection Date: 03-Nov-2017 13:37:59 Instrument ID: A8_N
Lims ID: IC L1
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 1 Worklist Smp#: 4
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.15

Processing Integration Results

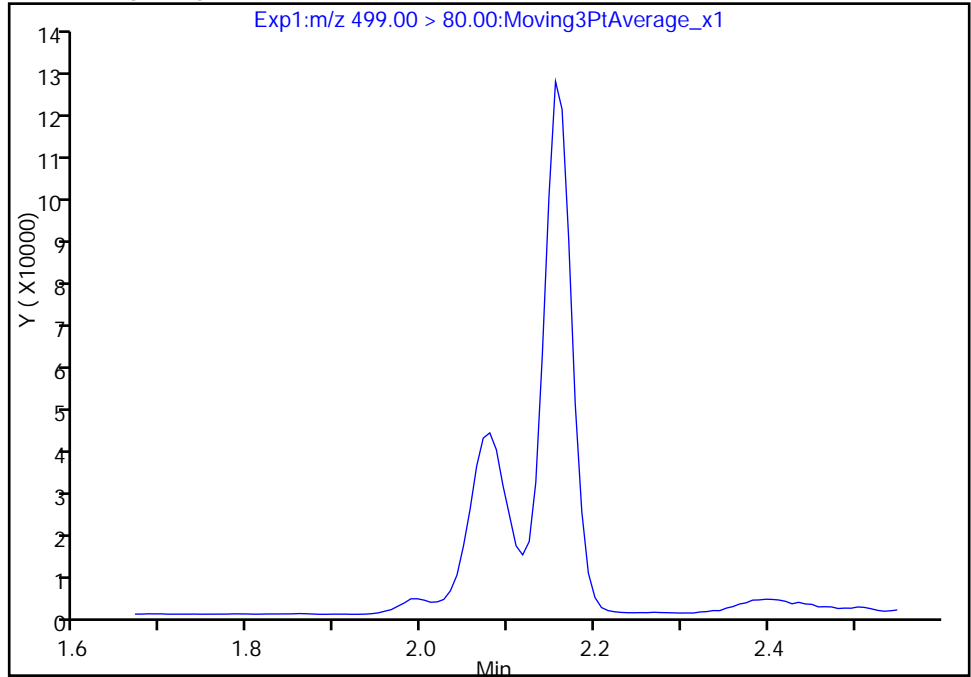

Manual Integration Results

RT: 2.15
Area: 412315
Amount: 3.817687
Amount Units: ng/ml

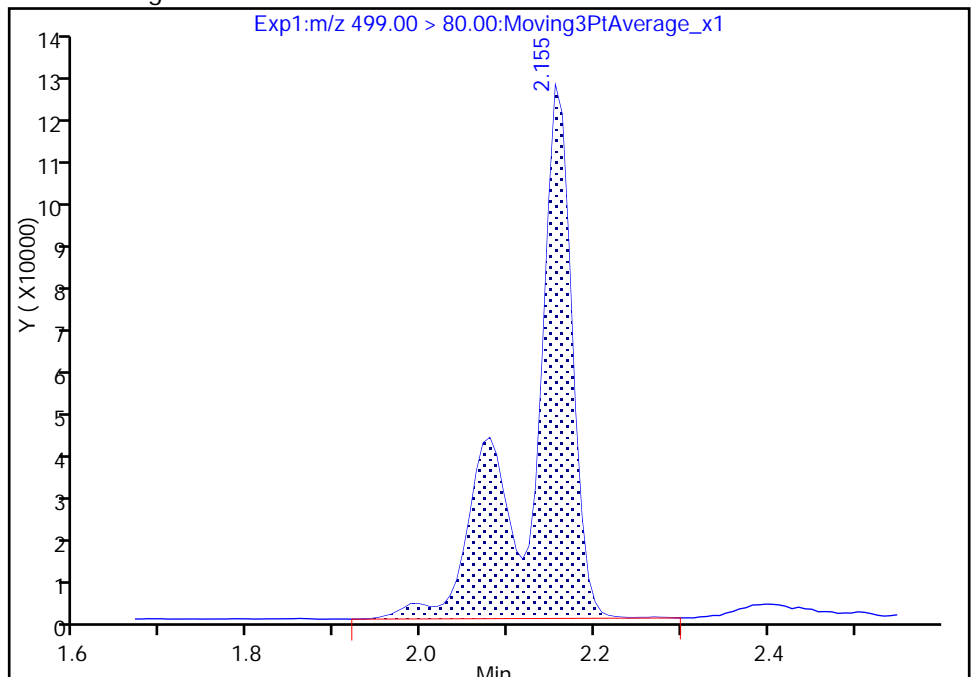

Reviewer: phomsophat, 06-Nov-2017 07:17:37

Audit Action: Manually Integrated

Audit Reason: Assign Peak

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_005.d
 Lims ID: IC L2
 Client ID:
 Sample Type: IC Calib Level: 2
 Inject. Date: 03-Nov-2017 13:42:39 ALS Bottle#: 2 Worklist Smp#: 5
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: L2_537
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub1

Method: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Nov-2017 15:52:08 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK021

First Level Reviewer: phomsophat Date: 06-Nov-2017 07:18:56

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.449	1.444	0.005	1.000	2591121	19.8		1479	
298.90 > 99.00	1.442	1.444	-0.002	0.995	1874928		1.38(0.00-0.00)	4315	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.578	1.573	0.005	1.000	1708988	9.57		8562	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.730	1.725	0.005	1.000	331548	2.18		87.8	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.730	1.725	0.005	1.000	1312135	6.51		2317	
* 6 13C2-PFOA									
415.00 > 370.00	1.920	1.913	0.007		1623614	10.0		6970	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.920	1.914	0.006	1.000	644149	4.29		113	
413.00 > 169.00	1.920	1.914	0.006	1.000	329479		1.96(0.00-0.00)	459	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.155	2.147	0.008	1.000	985487	8.72		578	M
499.00 > 99.00	2.155	2.147	0.008	1.000	200739		4.91(0.00-0.00)	449	M
* 7 13C4 PFOS									
503.00 > 80.00	2.155	2.151	0.004		3450592	28.7		5334	
9 Perfluorononanoic acid									
463.00 > 419.00	2.162	2.158	0.004	1.000	453612	4.21		136	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.314	2.312	0.002	1.000	1184358	9.53		7573	

QC Flag Legend

Review Flags

M - Manually Integrated

Reagents:

LC537-L2_00020

Amount Added: 1.00

Units: mL

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537ICAL_005.d

Injection Date: 03-Nov-2017 13:42:39

Instrument ID: A8_N

Lims ID: IC L2

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 2

Worklist Smp#: 5

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



4 Perfluoroheptanoic acid

3 Perfluorohexanesulfonic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid (M)

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA

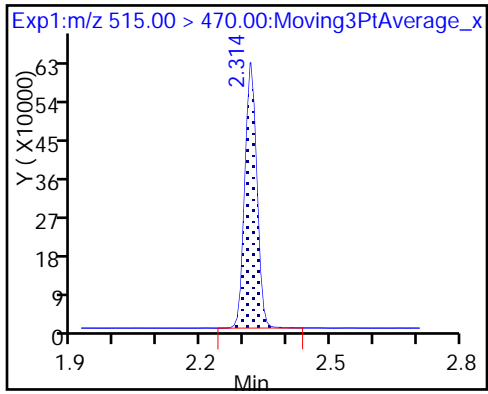

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_005.d
Injection Date: 03-Nov-2017 13:42:39 Instrument ID: A8_N
Lims ID: IC L2
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 2 Worklist Smp#: 5
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.15

Processing Integration Results

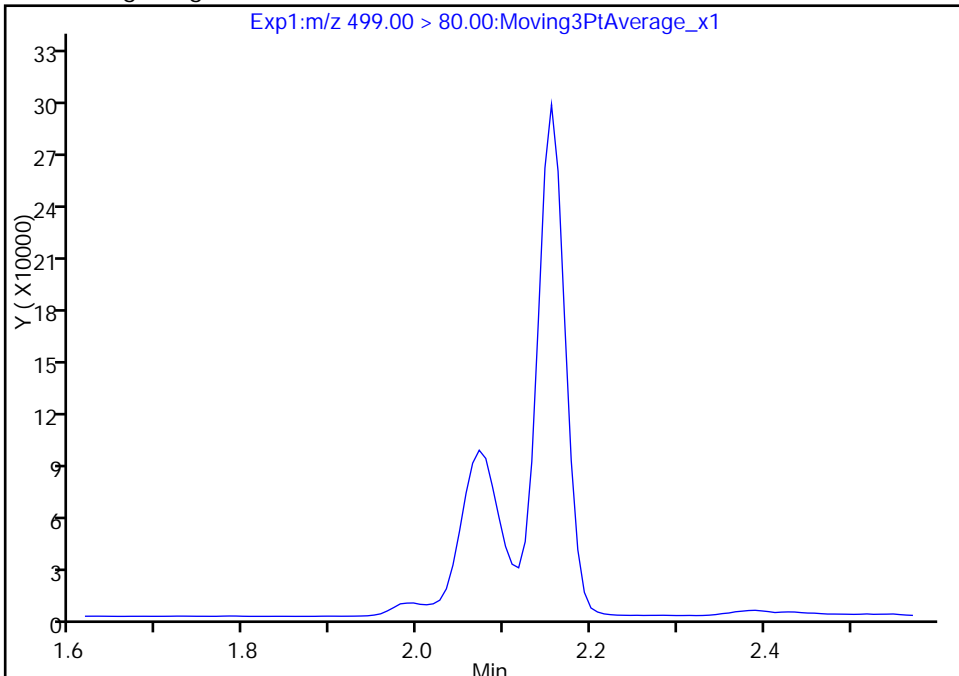

Manual Integration Results

RT: 2.15
Area: 985487
Amount: 8.723576
Amount Units: ng/ml

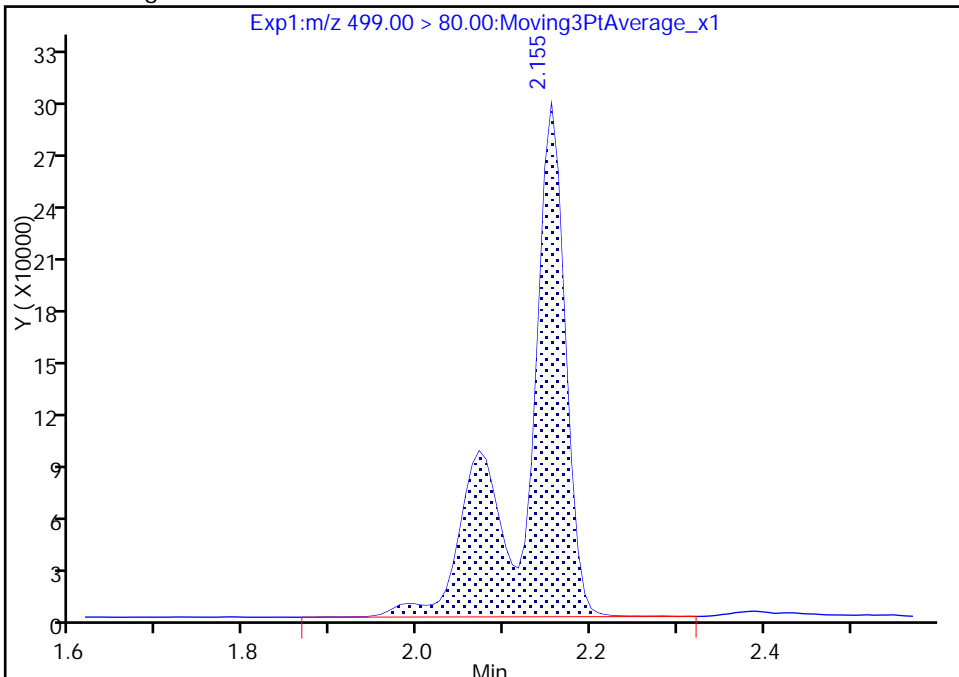

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\201711106-49975.b\2017.11.03_537XICAL_005.d
Injection Date: 03-Nov-2017 13:42:39 Instrument ID: A8_N
Lims ID: IC L2
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 2 Worklist Smp#: 5
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected
Expected RT: 2.15

Processing Integration Results



RT: 2.15
Area: 200739
Amount: 8.723576
Amount Units: ng/ml

Manual Integration Results



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\201711106-49975.b\2017.11.03_537XICAL_005.d
Injection Date: 03-Nov-2017 13:42:39 Instrument ID: A8_N
Lims ID: IC L2
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 2 Worklist Smp#: 5
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.15

Processing Integration Results



Manual Integration Results

RT: 2.15
Area: 985487
Amount: 8.723576
Amount Units: ng/ml



TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_006.d
 Lims ID: IC L3
 Client ID:
 Sample Type: IC Calib Level: 3
 Inject. Date: 03-Nov-2017 13:47:20 ALS Bottle#: 3 Worklist Smp#: 6
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: L3_537
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub1

Method: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Nov-2017 15:52:09 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK021

First Level Reviewer: phomsophat Date: 06-Nov-2017 07:20:04

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.442	1.444	-0.002	1.000	5461974	46.7		3220	
298.90 > 99.00	1.442	1.444	-0.002	1.000	3903438		1.40(0.00-0.00)	8589	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.571	1.573	-0.003	1.000	1701491	10.0		9021	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.722	1.725	-0.003	1.000	2908204	15.6		5000	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.722	1.725	-0.003	1.000	736034	5.10		208	
* 6 13C2-PFOA									
415.00 > 370.00	1.912	1.913	-0.001		1540946	10.0		6787	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.912	1.914	-0.002	1.000	1388033	9.73		256	
413.00 > 169.00	1.912	1.914	-0.002	1.000	715399		1.94(0.00-0.00)	904	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.147	2.147	0.0	1.000	2067792	19.8		2001	
499.00 > 99.00	2.147	2.147	0.0	1.000	431075		4.80(0.00-0.00)	922	
* 7 13C4 PFOS									
503.00 > 80.00	2.147	2.151	-0.004		3194016	28.7		4956	
9 Perfluorononanoic acid									
463.00 > 419.00	2.155	2.158	-0.003	1.000	1020851	9.97		302	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.306	2.312	-0.006	1.000	1166275	9.89		6310	

Reagents:

LC537-L3_00023

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537ICAL_006.d

Injection Date: 03-Nov-2017 13:47:20

Instrument ID: A8_N

Lims ID: IC L3

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 3

Worklist Smp#: 6

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid




8 Perfluorooctane sulfonic acid

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_007.d
 Lims ID: IC L4
 Client ID:
 Sample Type: ICISAV Calib Level: 4
 Inject. Date: 03-Nov-2017 13:52:00 ALS Bottle#: 4 Worklist Smp#: 7
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: L4_537
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub1

Method: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Nov-2017 15:52:10 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK021

First Level Reviewer: phomsophat Date: 06-Nov-2017 07:20:46

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.442	1.444	-0.002	1.000	10142530	87.2		5274	
298.90 > 99.00	1.442	1.444	-0.002	1.000	7408390		1.37(0.00-0.00)	12862	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.571	1.573	-0.003	1.000	1719911	10.1		8503	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.722	1.725	-0.003	1.000	1420703	9.81		399	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.722	1.725	-0.003	1.000	5871843	29.8		7622	
* 6 13C2-PFOA									
415.00 > 370.00	1.912	1.913	-0.001		1546307	10.0		6563	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.912	1.914	-0.002	1.000	2771271	19.4		505	
413.00 > 169.00	1.912	1.914	-0.002	1.000	1520933		1.82(0.00-0.00)	1919	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.155	2.147	0.008	1.000	4363079	39.5		3896	M
499.00 > 99.00	2.155	2.147	0.008	1.000	902486		4.83(0.00-0.00)	1588	M
* 7 13C4 PFOS									
503.00 > 80.00	2.155	2.151	0.004		3374600	28.7		5331	
9 Perfluorononanoic acid									
463.00 > 419.00	2.162	2.158	0.004	1.000	2106479	20.5		638	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.314	2.312	0.002	1.000	1207887	10.2		7165	

QC Flag Legend

Review Flags

M - Manually Integrated

Reagents:

LC537-L4_00020

Amount Added: 1.00

Units: mL

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_007.d

Injection Date: 03-Nov-2017 13:52:00

Instrument ID: A8_N

Lims ID: IC L4

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 4

Worklist Smp#: 7

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



4 Perfluoroheptanoic acid

3 Perfluorohexanesulfonic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)

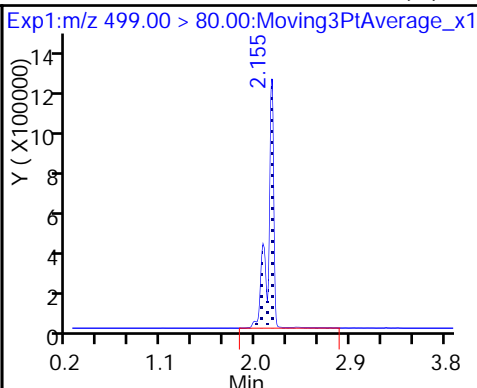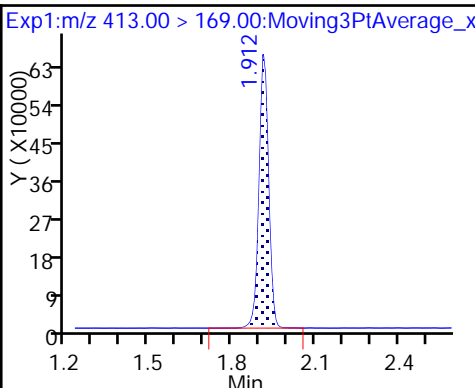


8 Perfluorooctane sulfonic acid (M)

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA

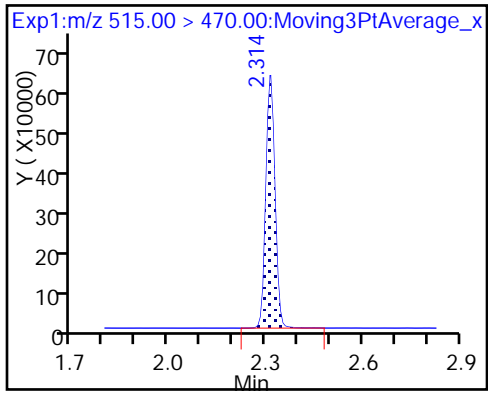

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_007.d
Injection Date: 03-Nov-2017 13:52:00 Instrument ID: A8_N
Lims ID: IC L4
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 4 Worklist Smp#: 7
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.15

Processing Integration Results



Manual Integration Results

RT: 2.15
Area: 4363079
Amount: 39.491903
Amount Units: ng/ml



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_007.d
Injection Date: 03-Nov-2017 13:52:00 Instrument ID: A8_N
Lims ID: IC L4
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 4 Worklist Smp#: 7
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 2


Not Detected
Expected RT: 2.15

Processing Integration Results



Manual Integration Results

RT: 2.15
Area: 902486
Amount: 39.491903
Amount Units: ng/ml



Reviewer: phomsophat, 06-Nov-2017 07:20:20

Audit Action: Manually Integrated

Audit Reason: Assign Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\201711106-49975.b\2017.11.03_537XICAL_007.d
Injection Date: 03-Nov-2017 13:52:00 Instrument ID: A8_N
Lims ID: IC L4
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 4 Worklist Smp#: 7
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.15

Processing Integration Results



RT: 2.15
Area: 4363079
Amount: 39.491903
Amount Units: ng/ml

Manual Integration Results



TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_008.d
 Lims ID: IC L5
 Client ID:
 Sample Type: IC Calib Level: 5
 Inject. Date: 03-Nov-2017 13:56:41 ALS Bottle#: 5 Worklist Smp#: 8
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: L5_537
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub1

Method: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Nov-2017 15:52:11 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK021

First Level Reviewer: phomsophat Date: 06-Nov-2017 07:21:19

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.442	1.444	-0.002	1.000	14011858	137.5		6452	
298.90 > 99.00	1.442	1.444	-0.002	1.000	10411479		1.35(0.00-0.00)	14800	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.571	1.573	-0.003	1.000	1675220	9.79		9525	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.722	1.725	-0.003	1.000	8413133	45.0		9078	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.722	1.725	-0.003	1.000	2102676	14.4		562	
* 6 13C2-PFOA									
415.00 > 370.00	1.912	1.913	-0.001		1555174	10.0		6769	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.912	1.914	-0.002	1.000	4257225	29.6		800	
413.00 > 169.00	1.912	1.914	-0.002	1.000	2294552		1.86(0.00-0.00)	2838	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.147	2.147	0.0	1.000	6504279	62.1		5682	
499.00 > 99.00	2.147	2.147	0.0	1.000	1339120		4.86(0.00-0.00)	2329	
* 7 13C4 PFOS									
503.00 > 80.00	2.147	2.151	-0.004		3199479	28.7		4946	
9 Perfluorononanoic acid									
463.00 > 419.00	2.155	2.158	-0.003	1.000	3023088	29.3		870	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.314	2.312	0.002	1.000	1139992	9.58		5885	

Reagents:

LC537-L5_00024

Amount Added: 1.00

Units: mL

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537ICAL_008.d

Injection Date: 03-Nov-2017 13:56:41

Instrument ID: A8_N

Lims ID: IC L5

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 5

Worklist Smp#: 8

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid




8 Perfluorooctane sulfonic acid

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Lims ID: IC L6
 Client ID:
 Sample Type: IC Calib Level: 6
 Inject. Date: 03-Nov-2017 14:01:24 ALS Bottle#: 6 Worklist Smp#: 9
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: L6_537
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub1

Method: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Nov-2017 15:52:12 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK021

First Level Reviewer: phomsophat Date: 06-Nov-2017 07:25:41

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.442	1.444	-0.002	1.000	16699152	179.1		7089	
298.90 > 99.00	1.442	1.444	-0.002	1.000	12929978		1.29(0.00-0.00)	15608	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.571	1.573	-0.003	1.000	1664260	10.6		9116	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.722	1.725	-0.003	1.000	2810797	21.0		763	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.722	1.725	-0.003	1.000	11071993	60.4		10884	
* 6 13C2-PFOA									
415.00 > 370.00	1.904	1.913	-0.009		1426806	10.0		5446	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.912	1.914	-0.002	1.000	5597122	42.4		962	
413.00 > 169.00	1.904	1.914	-0.010	0.996	3028676		1.85(0.00-0.00)	3704	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.147	2.147	0.0	1.000	8679676	84.4		6114	
499.00 > 99.00	2.147	2.147	0.0	1.000	1807143		4.80(0.00-0.00)	2991	
* 7 13C4 PFOS									
503.00 > 80.00	2.147	2.151	-0.004		3141787	28.7		4961	
9 Perfluorononanoic acid									
463.00 > 419.00	2.155	2.158	-0.003	1.000	4019666	42.4		1149	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.306	2.312	-0.006	1.000	1164156	10.7		6124	

Reagents:

LC537-L6_00020

Amount Added: 1.00

Units: mL

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537ICAL_009.d

Injection Date: 03-Nov-2017 14:01:24

Instrument ID: A8_N

Lims ID: IC L6

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 6

Worklist Smp#: 9

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



4 Perfluoroheptanoic acid

3 Perfluorohexanesulfonic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid




8 Perfluorooctane sulfonic acid

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Lab Sample ID: CCVL 320-192908/11 Calibration Date: 11/03/2017 14:10
 Instrument ID: A8_N Calib Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 11/03/2017 14:01
 Lab File ID: 2017.11.03_537XICAL_011.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		1.109		20.4	20.0	1.9	50.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9369	0.9382		2.23	2.22	0.1	50.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.674	1.688		6.72	6.67	0.8	50.0
Perfluorooctanoic acid (PFOA)	Ave	0.9258	0.8825		4.24	4.45	-4.7	50.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9389	0.9176		8.69	8.89	-2.3	50.0
Perfluorononanoic acid (PFNA)	Ave	0.6642	0.6625		4.43	4.45	-0.2	50.0
13C2 PFHxA	Ave	1.100	1.068		9.70	10.0	-3.0	30.0
13C2 PFDA	Ave	0.7652	0.7460		9.75	10.0	-2.5	30.0

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_011.d
 Lims ID: CCVL
 Client ID:
 Sample Type: CCVL
 Inject. Date: 03-Nov-2017 14:10:44 ALS Bottle#: 2 Worklist Smp#: 11
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: CCV L2
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub1
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Nov-2017 15:39:07 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK021

First Level Reviewer: phomsophat Date: 06-Nov-2017 07:26:29

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.449	1.444	0.005	1.000	2556738	20.4		1537	
298.90 > 99.00	1.449	1.444	0.005	1.000	1750170		1.46(0.00-0.00)	4023	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.578	1.573	0.005	1.000	1694196	9.70		8915	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.730	1.725	0.005	1.000	1297654	6.72		2410	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.730	1.725	0.005	1.000	330927	2.23		99.4	
* 6 13C2-PFOA									
415.00 > 370.00	1.912	1.913	-0.001		1586829	10.0		6840	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.912	1.914	-0.002	1.000	622915	4.24		116	
413.00 > 169.00	1.912	1.914	-0.002	1.000	335080		1.86(0.00-0.00)	460	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.155	2.147	0.008	1.000	940397	8.69		528	
499.00 > 99.00	2.147	2.147	0.0	0.996	196397		4.79(0.00-0.00)	430	
* 7 13C4 PFOS									
503.00 > 80.00	2.147	2.151	-0.004		3305852	28.7		5135	
9 Perfluorononanoic acid									
463.00 > 419.00	2.162	2.158	0.004	1.000	467323	4.43		143	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.314	2.312	0.002	1.000	1183747	9.75		6763	

Reagents:

LC537-L2_00020

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_011.d

Injection Date: 03-Nov-2017 14:10:44

Instrument ID: A8_N

Lims ID: CCVL

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 2

Worklist Smp#: 11

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid




8 Perfluorooctane sulfonic acid

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Lab Sample ID: ICV 320-192908/13 Calibration Date: 11/03/2017 14:20
 Instrument ID: A8_N Calib Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 11/03/2017 14:01
 Lab File ID: 2017.11.03_537XICAL_013.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		0.8310		83.7	100	-16.4	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9369	0.8136		8.68	10.0	-13.2	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.674	1.463		17.5	20.1	-12.6	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9258	0.7995		17.7	20.5	-13.6	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9389	0.8637		18.1	19.7	-8.0	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6642	0.6428		19.5	20.1	-3.2	30.0
13C2 PFHxA	Ave	1.100	1.039		9.44	10.0	-5.6	30.0
13C2 PFDA	Ave	0.7652	0.7391		9.66	10.0	-3.4	30.0

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_013.d
 Lims ID: ICV
 Client ID:
 Sample Type: ICV
 Inject. Date: 03-Nov-2017 14:20:03 ALS Bottle#: 7 Worklist Smp#: 13
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: ICV
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist:

Method: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Nov-2017 15:39:08 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK021

First Level Reviewer: phomsophat Date: 06-Nov-2017 07:27:24

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.442	1.444	-0.002	1.000	9960387	83.7		4998	
298.90 > 99.00	1.442	1.444	-0.002	1.000	7235967		1.38(0.00-0.00)	13514	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.571	1.573	-0.003	1.000	1570629	9.44		8393	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.722	1.725	-0.003	1.000	3517469	17.5		5659	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.722	1.725	-0.003	1.000	1229696	8.68		345	
* 6 13C2-PFOA									
415.00 > 370.00	1.904	1.913	-0.009		1512045	10.0		7643	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.904	1.914	-0.010	1.000	2476221	17.7		475	
413.00 > 169.00	1.904	1.914	-0.010	1.000	1327388		1.87(0.00-0.00)	1724	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.140	2.147	-0.007	1.000	2036944	18.1		2323	
499.00 > 99.00	2.140	2.147	-0.007	1.000	389736		5.23(0.00-0.00)	830	
* 7 13C4 PFOS									
503.00 > 80.00	2.140	2.151	-0.011		3433628	28.7		5334	
9 Perfluorononanoic acid									
463.00 > 419.00	2.147	2.158	-0.011	1.000	1956116	19.5		652	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.306	2.312	-0.006	1.000	1117553	9.66		6230	

Reagents:

LC537-ICV_00028

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_013.d

Injection Date: 03-Nov-2017 14:20:03

Instrument ID: A8_N

Lims ID: ICV

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 7

Worklist Smp#: 13

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid




8 Perfluorooctane sulfonic acid

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA

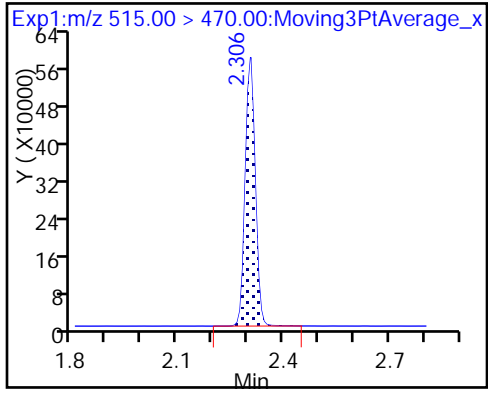

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Lab Sample ID: CCVL 320-207097/1 Calibration Date: 02/06/2018 08:30
 Instrument ID: A8_N Calib Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 11/03/2017 14:01
 Lab File ID: 2018.02.06_537A_003.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		1.081		19.8	20.0	-0.8	50.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.674	1.648		6.56	6.67	-1.6	50.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9369	1.009		2.39	2.22	7.7	50.0
Perfluorooctanoic acid (PFOA)	Ave	0.9258	0.9155		4.42	4.47	-1.1	50.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9389	0.9828		9.34	8.93	4.7	50.0
Perfluorononanoic acid (PFNA)	Ave	0.6642	0.6745		4.52	4.45	1.6	50.0
13C2 PFHxA	Ave	1.100	1.102		10.0	10.0	0.1	30.0
13C2 PFDA	Ave	0.7652	0.7044		9.21	10.0	-7.9	30.0

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180206-53732.b\2018.02.06_537A_003.d
 Lims ID: CCVL
 Client ID:
 Sample Type: CCVL
 Inject. Date: 06-Feb-2018 08:30:44 ALS Bottle#: 2 Worklist Smp#: 1
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: CCVL
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub1
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180206-53732.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 06-Feb-2018 09:58:48 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK002

First Level Reviewer: roycea Date: 06-Feb-2018 09:48:53

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.373	1.366	0.007	1.000	2299622	19.8		6878	
298.90 > 99.00	1.373	1.366	0.007	1.000	1753894		1.31(0.00-0.00)	5999	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.487	1.479	0.008	1.000	1515674	10.0		9438	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.624	1.616	0.008	1.000	1168960	6.56		3098	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.631	1.616	0.015	1.000	308590	2.39		101	
* 6 13C2-PFOA									
415.00 > 370.00	1.806	1.798	0.008		1375995	10.0		5862	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.806	1.798	0.008	1.000	562983	4.42		86.1	
413.00 > 169.00	1.806	1.798	0.008	1.000	310883		1.81(0.00-0.00)	1116	
* 7 13C4 PFOS									
503.00 > 80.00	2.048	2.041	0.007		3051061	28.7		6310	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.056	2.041	0.015	1.000	933344	9.34		1314	a
499.00 > 99.00	2.048	2.041	0.007	0.996	203117		4.60(0.00-0.00)	879	a
9 Perfluorononanoic acid									
463.00 > 419.00	2.064	2.048	0.016	1.000	412629	4.52		115	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.238	2.231	0.007	1.000	969216	9.21		5297	

QC Flag Legend

Review Flags

a - User Assigned ID

Reagents:

LC537-L2_00021

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180206-53732.b\2018.02.06_537A_003.d

Injection Date: 06-Feb-2018 08:30:44

Instrument ID: A8_N

Lims ID: CCVL

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 2

Worklist Smp#: 1

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




* 7 13C4 PFOS




8 Perfluorooctane sulfonic acid (M)

8 Perfluorooctane sulfonic acid

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180206-53732.b\2018.02.06_537A_003.d
Injection Date: 06-Feb-2018 08:30:44 Instrument ID: A8_N
Lims ID: CCVL
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 2 Worklist Smp#: 1
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.04

Processing Integration Results



RT: 2.06
Area: 933344
Amount: 9.343899
Amount Units: ng/ml

Manual Integration Results



FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Lab Sample ID: CCV 320-207292/1 Calibration Date: 02/06/2018 18:23
 Instrument ID: A8_N Calib Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 11/03/2017 14:01
 Lab File ID: 2018.02.06_537XX_042.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		1.104		47.4	45.0	5.3	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.674	1.740		15.6	15.0	3.9	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9369	1.029		5.49	5.00	9.9	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9258	0.9634		10.5	10.1	4.1	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9389	0.9893		21.2	20.1	5.4	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6642	0.6984		10.5	10.0	5.2	30.0
13C2 PFHxA	Ave	1.100	1.120		10.2	10.0	1.8	30.0
13C2 PFDA	Ave	0.7652	0.7367		9.63	10.0	-3.7	30.0

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_042.d
 Lims ID: CCV L3
 Client ID:
 Sample Type: CCVIS
 Inject. Date: 06-Feb-2018 18:23:47 ALS Bottle#: 3 Worklist Smp#: 1
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: CCV L3
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub1
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Feb-2018 11:48:41 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: CTXT1

First Level Reviewer: krenns Date: 07-Feb-2018 11:36:17

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.373	1.373	0.0	1.000	5268896	47.4		11636	
298.90 > 99.00	1.373	1.373	0.0	1.000	3951510		1.33(0.00-0.00)	10562	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.487	1.487	0.0	1.000	1488409	10.2		8752	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.624	1.624	0.0	1.000	2769433	15.6		7058	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.631	1.631	0.0	1.000	684086	5.49		209	
* 6 13C2-PFOA									
415.00 > 370.00	1.806	1.806	0.0		1328760	10.0		6304	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.806	1.806	0.0	1.000	1287144	10.5		220	
413.00 > 169.00	1.806	1.806	0.0	1.000	735373		1.75(0.00-0.00)	2969	
* 7 13C4 PFOS									
503.00 > 80.00	2.048	2.048	0.0		3042209	28.7		6544	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.048	2.041	0.007	1.000	2107702	21.2		2456	a
499.00 > 99.00	2.048	2.041	0.007	1.000	437975		4.81(0.00-0.00)	1202	a
9 Perfluorononanoic acid									
463.00 > 419.00	2.056	2.056	0.0	1.000	928344	10.5		238	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.238	2.238	0.0	1.000	978930	9.63		6823	

QC Flag Legend

Review Flags

a - User Assigned ID

Reagents:

LC537-L3_00024

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_042.d

Injection Date: 06-Feb-2018 18:23:47

Instrument ID: A8_N

Lims ID: CCV L3

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 3

Worklist Smp#: 1

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




* 7 13C4 PFOS




8 Perfluorooctane sulfonic acid (M)

8 Perfluorooctane sulfonic acid

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_042.d
Injection Date: 06-Feb-2018 18:23:47 Instrument ID: A8_N
Lims ID: CCV L3
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 3 Worklist Smp#: 1
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1


Signal: 1

Not Detected
Expected RT: 2.04

Processing Integration Results



Manual Integration Results



RT: 2.05
Area: 2107702
Amount: 21.162036
Amount Units: ng/ml

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Lab Sample ID: CCV 320-207292/11 Calibration Date: 02/06/2018 19:10
 Instrument ID: A8_N Calib Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 11/03/2017 14:01
 Lab File ID: 2018.02.06_537XX_052.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		0.9406		139	135	3.3	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.674	1.695		45.6	45.0	1.2	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9369	1.045		16.7	15.0	11.6	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9258	1.007		32.8	30.2	8.8	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9389	1.007		64.6	60.3	7.2	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6642	0.7206		32.6	30.0	8.5	30.0
13C2 PFHxA	Ave	1.100	1.089		9.90	10.0	-1.0	30.0
13C2 PFDA	Ave	0.7652	0.7564		9.89	10.0	-1.1	30.0

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Lab Sample ID: CCV 320-207294/11 Calibration Date: 02/06/2018 19:10
 Instrument ID: A8_N Calib Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 11/03/2017 14:01
 Lab File ID: 2018.02.06_537XX_052.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		0.9406		139	135	3.3	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.674	1.695		45.6	45.0	1.2	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9369	1.045		16.7	15.0	11.6	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9258	1.007		32.8	30.2	8.8	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9389	1.007		64.6	60.3	7.2	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6642	0.7206		32.6	30.0	8.5	30.0
13C2 PFHxA	Ave	1.100	1.089		9.90	10.0	-1.0	30.0
13C2 PFDA	Ave	0.7652	0.7564		9.89	10.0	-1.1	30.0

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_052.d
 Lims ID: CCV L5
 Client ID:
 Sample Type: CCVIS
 Inject. Date: 06-Feb-2018 19:10:34 ALS Bottle#: 5 Worklist Smp#: 11
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: CCV L5
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub1
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Feb-2018 11:48:57 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: CTXT1

First Level Reviewer: krenns Date: 07-Feb-2018 11:47:49

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.366	1.366	0.0	1.000	13439508	139.5		17972	
298.90 > 99.00	1.366	1.366	0.0	1.000	10512203		1.28(0.00-0.00)	17010	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.479	1.479	0.0	1.000	1432339	9.90		8664	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.616	1.616	0.0	1.000	8074057	45.6		14179	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.624	1.624	0.0	1.000	2062715	16.7		658	
* 6 13C2-PFOA									
415.00 > 370.00	1.798	1.798	0.0		1315133	10.0		5911	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.798	1.798	0.0	1.000	3996192	32.8		713	
413.00 > 169.00	1.798	1.798	0.0	1.000	2065381		1.93(0.00-0.00)	6906	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.041	2.041	0.0	1.000	6419126	64.6		6760	a
499.00 > 99.00	2.041	2.041	0.0	1.000	1332806		4.82(0.00-0.00)	4398	a
* 7 13C4 PFOS									
503.00 > 80.00	2.041	2.041	0.0		3035313	28.7		6395	
9 Perfluorononanoic acid									
463.00 > 419.00	2.048	2.048	0.0	1.000	2843835	32.6		658	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.231	2.231	0.0	1.000	994795	9.89		6308	

QC Flag Legend

Review Flags

a - User Assigned ID

Reagents:

LC537-L5_00025

Amount Added: 1.00

Units: mL

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_052.d
 Lims ID: CCV L5
 Client ID:
 Sample Type: CCVIS
 Inject. Date: 06-Feb-2018 19:10:34 ALS Bottle#: 5 Worklist Smp#: 11
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: CCV L5
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub1
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Feb-2018 11:48:57 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: CTXT1

First Level Reviewer: krenns Date: 07-Feb-2018 11:47:49

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.366	1.366	0.0	1.000	13439508	139.5		17972	
298.90 > 99.00	1.366	1.366	0.0	1.000	10512203		1.28(0.00-0.00)	17010	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.479	1.479	0.0	1.000	1432339	9.90		8664	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.616	1.616	0.0	1.000	8074057	45.6		14179	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.624	1.624	0.0	1.000	2062715	16.7		658	
* 6 13C2-PFOA									
415.00 > 370.00	1.798	1.798	0.0		1315133	10.0		5911	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.798	1.798	0.0	1.000	3996192	32.8		713	
413.00 > 169.00	1.798	1.798	0.0	1.000	2065381		1.93(0.00-0.00)	6906	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.041	2.041	0.0	1.000	6419126	64.6		6760	a
499.00 > 99.00	2.041	2.041	0.0	1.000	1332806		4.82(0.00-0.00)	4398	a
* 7 13C4 PFOS									
503.00 > 80.00	2.041	2.041	0.0		3035313	28.7		6395	
9 Perfluorononanoic acid									
463.00 > 419.00	2.048	2.048	0.0	1.000	2843835	32.6		658	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.231	2.231	0.0	1.000	994795	9.89		6308	

QC Flag Legend

Review Flags

a - User Assigned ID

Reagents:

LC537-L5_00025

Amount Added: 1.00

Units: mL

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_052.d

Injection Date: 06-Feb-2018 19:10:34

Instrument ID: A8_N

Lims ID: CCV L5

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 5

Worklist Smp#: 11

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_052.d

Injection Date: 06-Feb-2018 19:10:34

Instrument ID: A8_N

Lims ID: CCV L5

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 5

Worklist Smp#: 11

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_052.d
Injection Date: 06-Feb-2018 19:10:34 Instrument ID: A8_N
Lims ID: CCV L5
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 5 Worklist Smp#: 11
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.04

Processing Integration Results



Manual Integration Results

RT: 2.04
Area: 6419126
Amount: 64.596606
Amount Units: ng/ml



Reviewer: krenns, 07-Feb-2018 11:47:43
Audit Action: Assigned Compound ID

Audit Reason: User Assigned

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_052.d
Injection Date: 06-Feb-2018 19:10:34 Instrument ID: A8_N
Lims ID: CCV L5
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 5 Worklist Smp#: 11
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1


Signal: 1

Not Detected
Expected RT: 2.04

Processing Integration Results



Manual Integration Results



RT: 2.04
Area: 6419126
Amount: 64.596606
Amount Units: ng/ml

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Lab Sample ID: CCV 320-207294/20 Calibration Date: 02/06/2018 19:52
 Instrument ID: A8_N Calib Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 11/03/2017 14:01
 Lab File ID: 2018.02.06_537XX_061.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		1.043		44.6	45.0	-0.9	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9369	1.064		5.68	5.00	13.6	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.674	1.627		14.6	15.0	-2.8	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9258	0.9471		10.3	10.1	2.3	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9389	0.9332		20.0	20.1	-0.6	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6642	0.7112		10.7	10.0	7.1	30.0
13C2 PFHxA	Ave	1.100	1.131		10.3	10.0	2.8	30.0
13C2 PFDA	Ave	0.7652	0.7430		9.71	10.0	-2.9	30.0

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_061.d
 Lims ID: CCV L3
 Client ID:
 Sample Type: CCVIS
 Inject. Date: 06-Feb-2018 19:52:37 ALS Bottle#: 3 Worklist Smp#: 20
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: CCV L3
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub1
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Feb-2018 11:51:07 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: CTXT1

First Level Reviewer: krenns Date: 07-Feb-2018 11:50:42

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.366	1.366	0.0	1.000	5209417	44.6		13321	
298.90 > 99.00	1.366	1.366	0.0	1.000	3868965		1.35(0.00-0.00)	11450	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.479	1.479	0.0	1.000	1481715	10.3		7691	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.616	1.616	0.0	1.000	2709873	14.6		6286	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.616	1.616	0.0	1.000	696975	5.68		213	
* 6 13C2-PFOA									
415.00 > 370.00	1.791	1.791	0.0		1309862	10.0		5187	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.798	1.798	0.0	1.000	1247471	10.3		205	
413.00 > 169.00	1.791	1.798	-0.007	0.996	705102		1.77(0.00-0.00)	2897	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.041	2.041	0.0	1.000	2080197	20.0		2376	a
499.00 > 99.00	2.041	2.041	0.0	1.000	433628		4.80(0.00-0.00)	1093	a
* 7 13C4 PFOS									
503.00 > 80.00	2.041	2.041	0.0		3183039	28.7		6129	
9 Perfluorononanoic acid									
463.00 > 419.00	2.048	2.048	0.0	1.000	931823	10.7		220	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.231	2.231	0.0	1.000	973275	9.71		5874	

QC Flag Legend

Review Flags

a - User Assigned ID

Reagents:

LC537-L3_00024

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_061.d

Injection Date: 06-Feb-2018 19:52:37

Instrument ID: A8_N

Lims ID: CCV L3

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 3

Worklist Smp#: 20

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_061.d
Injection Date: 06-Feb-2018 19:52:37 Instrument ID: A8_N
Lims ID: CCV L3
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 3 Worklist Smp#: 20
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1


Signal: 1

Not Detected
Expected RT: 2.04

Processing Integration Results



Manual Integration Results



RT: 2.04
Area: 2080197
Amount: 19.961804
Amount Units: ng/ml

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Client Sample ID: _____ Lab Sample ID: MB 320-206379/1-A
 Matrix: Water Lab File ID: 2018.02.06_537XX_044.d
 Analysis Method: 537 Date Collected: _____
 Extraction Method: 537 Date Extracted: 01/31/2018 12:34
 Sample wt/vol: 250.0 (mL) Date Analyzed: 02/06/2018 18:33
 Con. Extract Vol.: 1.0 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 207292 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	8.0	U	20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.0	U	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	114		70-130
STL00996	13C2 PFDA	110		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_044.d
 Lims ID: MB 320-206379/1-A
 Client ID:
 Sample Type: MB
 Inject. Date: 06-Feb-2018 18:33:08 ALS Bottle#: 31 Worklist Smp#: 3
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: mb 320-206379/1-a
 Misc. Info.: Plate: 1 Rack: 3
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Feb-2018 11:48:41 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: CTXT1

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
\$ 2 13C2 PFHxA	315.00 > 270.00	1.487	1.487	0.0	1.000	1561972	11.4	9949	
* 6 13C2-PFOA	415.00 > 370.00	1.798	1.806	-0.008		1243942	10.0	5485	
* 7 13C4 PFOS	503.00 > 80.00	2.048	2.048	0.0		2945240	28.7	6227	
\$ 10 13C2 PFDA	515.00 > 470.00	2.231	2.238	-0.007	1.000	1049082	11.0	6794	

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_044.d

Injection Date: 06-Feb-2018 18:33:08

Instrument ID: A8_N

Lims ID: MB 320-206379/1-A

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 31

Worklist Smp#: 3

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid (ND)

1 Perfluorobutanesulfonic acid (ND)




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid (ND)

4 Perfluoroheptanoic acid (ND)




* 6 13C2-PFOA



5 Perfluorooctanoic acid (ND)

5 Perfluorooctanoic acid (ND)




8 Perfluorooctane sulfonic acid (ND)




8 Perfluorooctane sulfonic acid (ND)

* 7 13C4 PFOS

9 Perfluorononanoic acid (ND)



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_044.d
 Lims ID: MB 320-206379/1-A
 Client ID:
 Sample Type: MB
 Inject. Date: 06-Feb-2018 18:33:08 ALS Bottle#: 31 Worklist Smp#: 3
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: mb 320-206379/1-a
 Misc. Info.: Plate: 1 Rack: 3
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Feb-2018 11:48:41 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d

Column 1 : Det: EXP1
 Process Host: CTXT1

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	11.4	114.12
\$ 10 13C2 PFDA	10.0	11.0	110.21

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Client Sample ID: _____ Lab Sample ID: LLCS 320-206379/2-A
 Matrix: Water Lab File ID: 2018.02.06_537XX_045.d
 Analysis Method: 537 Date Collected: _____
 Extraction Method: 537 Date Extracted: 01/31/2018 12:34
 Sample wt/vol: 250.0 (mL) Date Analyzed: 02/06/2018 18:37
 Con. Extract Vol.: 1.0 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 207292 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	40.2	M	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	22.1		20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	21.9	J	24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	33.0		30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	11.6		10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	94.5		90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	106		70-130
STL00996	13C2 PFDA	104		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_045.d
 Lims ID: LLCS 320-206379/2-A
 Client ID:
 Sample Type: LLCS
 Inject. Date: 06-Feb-2018 18:37:48 ALS Bottle#: 32 Worklist Smp#: 4
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: llcs 320-206379/2-a
 Misc. Info.: Plate: 1 Rack: 3
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Feb-2018 11:48:41 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: CTXT1

First Level Reviewer: krenns Date: 07-Feb-2018 11:44:16

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.373	1.373	0.0	1.000	2700321	23.6		6758	
298.90 > 99.00	1.373	1.373	0.0	1.000	2043129		1.32(0.00-0.00)	6509	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.487	1.487	0.0	1.000	1536656	10.6		8428	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.631	1.624	0.007	1.000	1454557	8.24		3515	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.631	1.631	0.0	1.000	355892	2.89		116	
* 6 13C2-PFOA									
415.00 > 370.00	1.806	1.806	0.0		1313107	10.0		5572	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.806	1.806	0.0	1.000	672833	5.53		126	
413.00 > 169.00	1.806	1.806	0.0	1.000	381354		1.76(0.00-0.00)	1652	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.048	2.041	0.007	1.000	994761	10.0		646	a
499.00 > 99.00	2.048	2.041	0.007	1.000	222500		4.47(0.00-0.00)	519	a
* 7 13C4 PFOS									
503.00 > 80.00	2.048	2.048	0.0		3024316	28.7		6529	
9 Perfluorononanoic acid									
463.00 > 419.00	2.056	2.056	0.0	1.000	477674	5.48		93.9	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.238	2.238	0.0	1.000	1041774	10.4		6694	

QC Flag Legend

Review Flags

a - User Assigned ID

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_045.d

Injection Date: 06-Feb-2018 18:37:48

Instrument ID: A8_N

Lims ID: LLCS 320-206379/2-A

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 32

Worklist Smp#: 4

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_045.d
 Lims ID: LLCS 320-206379/2-A
 Client ID:
 Sample Type: LLCS
 Inject. Date: 06-Feb-2018 18:37:48 ALS Bottle#: 32 Worklist Smp#: 4
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: llcs 320-206379/2-a
 Misc. Info.: Plate: 1 Rack: 3
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Feb-2018 11:48:41 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: CTXT1

First Level Reviewer: krenns Date: 07-Feb-2018 11:44:16

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	10.6	106.36
\$ 10 13C2 PFDA	10.0	10.4	103.68

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_045.d
Injection Date: 06-Feb-2018 18:37:48 Instrument ID: A8_N
Lims ID: LLCS 320-206379/2-A
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 32 Worklist Smp#: 4
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.04

Processing Integration Results



Manual Integration Results

RT: 2.05
Area: 994761
Amount: 10.046826
Amount Units: ng/ml



FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Client Sample ID: _____ Lab Sample ID: LLCSD 320-206379/3-A
 Matrix: Water Lab File ID: 2018.02.06_537XX_046.d
 Analysis Method: 537 Date Collected: _____
 Extraction Method: 537 Date Extracted: 01/31/2018 12:34
 Sample wt/vol: 250.0 (mL) Date Analyzed: 02/06/2018 18:42
 Con. Extract Vol.: 1.0 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 207292 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	37.6	J M	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	22.5		20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	22.2	J	24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	31.4		30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	11.4		10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	94.8		90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	109		70-130
STL00996	13C2 PFDA	104		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_046.d
 Lims ID: LLCSD 320-206379/3-A
 Client ID:
 Sample Type: LLCSD
 Inject. Date: 06-Feb-2018 18:42:29 ALS Bottle#: 33 Worklist Smp#: 5
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: llcsd 320-206379/3-a
 Misc. Info.: Plate: 1 Rack: 3
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Feb-2018 11:48:41 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: CTXT1

First Level Reviewer: krenns Date: 07-Feb-2018 11:44:27

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.366	1.373	-0.007	1.000	2732537	23.7		7391	
298.90 > 99.00	1.366	1.373	-0.007	1.000	2058077		1.33(0.00-0.00)	6186	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.487	1.487	0.0	1.000	1527109	10.9		9085	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.624	1.624	0.0	1.000	1399337	7.86		3568	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.624	1.631	-0.007	1.000	341180	2.86		109	
* 6 13C2-PFOA									
415.00 > 370.00	1.798	1.806	-0.008		1273817	10.0		5748	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.798	1.806	-0.008	1.000	662141	5.61		111	
413.00 > 169.00	1.798	1.806	-0.008	1.000	371615		1.78(0.00-0.00)	1563	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.048	2.041	0.007	1.000	939175	9.40		583	a
499.00 > 99.00	2.041	2.041	0.0	0.996	204056		4.60(0.00-0.00)	479	a
* 7 13C4 PFOS									
503.00 > 80.00	2.048	2.048	0.0		3050466	28.7		6798	
9 Perfluorononanoic acid									
463.00 > 419.00	2.056	2.056	0.0	1.000	469288	5.55		102	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.238	2.238	0.0	1.000	1009896	10.4		6696	

QC Flag Legend

Review Flags

a - User Assigned ID

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_046.d

Injection Date: 06-Feb-2018 18:42:29

Instrument ID: A8_N

Lims ID: LLCSD 320-206379/3-A

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 33

Worklist Smp#: 5

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)




8 Perfluorooctane sulfonic acid

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_046.d
 Lims ID: LLCSD 320-206379/3-A
 Client ID:
 Sample Type: LLCSD
 Inject. Date: 06-Feb-2018 18:42:29 ALS Bottle#: 33 Worklist Smp#: 5
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: llcsd 320-206379/3-a
 Misc. Info.: Plate: 1 Rack: 3
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 07-Feb-2018 11:48:41 Calib Date: 03-Nov-2017 14:01:24
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20171106-49975.b\2017.11.03_537XICAL_009.d
 Column 1 : Det: EXP1
 Process Host: CTXT1

First Level Reviewer: krenns Date: 07-Feb-2018 11:44:27

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	10.9	108.96
\$ 10 13C2 PFDA	10.0	10.4	103.61

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b\2018.02.06_537XX_046.d
Injection Date: 06-Feb-2018 18:42:29 Instrument ID: A8_N
Lims ID: LLCSD 320-206379/3-A
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 33 Worklist Smp#: 5
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.04

Processing Integration Results



RT: 2.05
Area: 939175
Amount: 9.404108
Amount Units: ng/ml

Manual Integration Results



Reviewer: krenns, 07-Feb-2018 11:44:23
Audit Action: Assigned Compound ID

Audit Reason: User Assigned

LCMS ANALYSIS RUN LOG

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1

SDG No.: _____

Instrument ID: A8_N Start Date: 11/03/2017 13:37

Analysis Batch Number: 192908 End Date: 11/03/2017 14:24

LAB SAMPLE ID	CLIENT SAMPLE ID	DATE ANALYZED	DILUTION FACTOR	LAB FILE ID	COLUMN ID
IC 320-192908/4		11/03/2017 13:37	1	2017.11.03_537X ICAL 004.d	GeminiC18 3x100 3(mm)
IC 320-192908/5		11/03/2017 13:42	1	2017.11.03_537X ICAL 005.d	GeminiC18 3x100 3(mm)
IC 320-192908/6		11/03/2017 13:47	1	2017.11.03_537X ICAL 006.d	GeminiC18 3x100 3(mm)
IC 320-192908/7 ICISAV		11/03/2017 13:52	1	2017.11.03_537X ICAL 007.d	GeminiC18 3x100 3(mm)
IC 320-192908/8		11/03/2017 13:56	1	2017.11.03_537X ICAL 008.d	GeminiC18 3x100 3(mm)
IC 320-192908/9		11/03/2017 14:01	1	2017.11.03_537X ICAL 009.d	GeminiC18 3x100 3(mm)
ZZZZZ		11/03/2017 14:06	1		GeminiC18 3x100 3(mm)
CCVL 320-192908/11		11/03/2017 14:10	1	2017.11.03_537X ICAL 011.d	GeminiC18 3x100 3(mm)
ZZZZZ		11/03/2017 14:15	1		GeminiC18 3x100 3(mm)
ICV 320-192908/13		11/03/2017 14:20	1	2017.11.03_537X ICAL 013.d	GeminiC18 3x100 3(mm)
ZZZZZ		11/03/2017 14:24	1		GeminiC18 3x100 3(mm)

LCMS ANALYSIS RUN LOG

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1

SDG No.: _____

Instrument ID: A8_N Start Date: 02/06/2018 08:30

Analysis Batch Number: 207097 End Date: 02/06/2018 09:31

LAB SAMPLE ID	CLIENT SAMPLE ID	DATE ANALYZED	DILUTION FACTOR	LAB FILE ID	COLUMN ID
CCVL 320-207097/1		02/06/2018 08:30	1	2018.02.06_537A 003.d	GeminiC18 3x100 3(mm)
CCV 320-207097/2 CCVIS		02/06/2018 08:35	1		GeminiC18 3x100 3(mm)
ZZZZZ		02/06/2018 08:44	1		GeminiC18 3x100 3(mm)
ZZZZZ		02/06/2018 08:49	1		GeminiC18 3x100 3(mm)
ZZZZZ		02/06/2018 08:54	1		GeminiC18 3x100 3(mm)
ZZZZZ		02/06/2018 08:58	1		GeminiC18 3x100 3(mm)
ZZZZZ		02/06/2018 09:03	1		GeminiC18 3x100 3(mm)
ZZZZZ		02/06/2018 09:08	1		GeminiC18 3x100 3(mm)
ZZZZZ		02/06/2018 09:12	1		GeminiC18 3x100 3(mm)
ZZZZZ		02/06/2018 09:17	1		GeminiC18 3x100 3(mm)
ZZZZZ		02/06/2018 09:22	1		GeminiC18 3x100 3(mm)
ZZZZZ		02/06/2018 09:26	1		GeminiC18 3x100 3(mm)
CCV 320-207097/14 CCVIS		02/06/2018 09:31	1		GeminiC18 3x100 3(mm)

LCMS ANALYSIS RUN LOG

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1

SDG No.: _____

Instrument ID: A8_N Start Date: 02/06/2018 18:23

Analysis Batch Number: 207292 End Date: 02/06/2018 19:10

LAB SAMPLE ID	CLIENT SAMPLE ID	DATE ANALYZED	DILUTION FACTOR	LAB FILE ID	COLUMN ID
CCV 320-207292/1 CCVIS		02/06/2018 18:23	1	2018.02.06_537X X 042.d	GeminiC18 3x100 3(mm)
MB 320-206379/1-A		02/06/2018 18:33	1	2018.02.06_537X X 044.d	GeminiC18 3x100 3(mm)
LLCS 320-206379/2-A		02/06/2018 18:37	1	2018.02.06_537X X 045.d	GeminiC18 3x100 3(mm)
LLCSD 320-206379/3-A		02/06/2018 18:42	1	2018.02.06_537X X 046.d	GeminiC18 3x100 3(mm)
320-35207-1		02/06/2018 18:47	1	2018.02.06_537X X 047.d	GeminiC18 3x100 3(mm)
320-35207-2		02/06/2018 18:51	1	2018.02.06_537X X 048.d	GeminiC18 3x100 3(mm)
320-35207-3		02/06/2018 18:56	1	2018.02.06_537X X 049.d	GeminiC18 3x100 3(mm)
320-35207-4		02/06/2018 19:01	1	2018.02.06_537X X 050.d	GeminiC18 3x100 3(mm)
320-35207-5		02/06/2018 19:05	1	2018.02.06_537X X 051.d	GeminiC18 3x100 3(mm)
CCV 320-207292/11 CCVIS		02/06/2018 19:10	1	2018.02.06_537X X 052.d	GeminiC18 3x100 3(mm)

LCMS ANALYSIS RUN LOG

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1

SDG No.: _____

Instrument ID: A8_N Start Date: 02/06/2018 19:10

Analysis Batch Number: 207294 End Date: 02/06/2018 19:52

LAB SAMPLE ID	CLIENT SAMPLE ID	DATE ANALYZED	DILUTION FACTOR	LAB FILE ID	COLUMN ID
CCV 320-207294/11 CCVIS		02/06/2018 19:10	1	2018.02.06_537X X 052.d	GeminiC18 3x100 3(mm)
320-35207-6		02/06/2018 19:19	1	2018.02.06_537X X 054.d	GeminiC18 3x100 3(mm)
320-35207-7		02/06/2018 19:24	1	2018.02.06_537X X 055.d	GeminiC18 3x100 3(mm)
320-35207-8		02/06/2018 19:29	1	2018.02.06_537X X 056.d	GeminiC18 3x100 3(mm)
320-35207-9		02/06/2018 19:33	1	2018.02.06_537X X 057.d	GeminiC18 3x100 3(mm)
320-35207-10		02/06/2018 19:38	1	2018.02.06_537X X 058.d	GeminiC18 3x100 3(mm)
320-35207-11		02/06/2018 19:43	1	2018.02.06_537X X 059.d	GeminiC18 3x100 3(mm)
320-35207-12		02/06/2018 19:47	1	2018.02.06_537X X 060.d	GeminiC18 3x100 3(mm)
CCV 320-207294/20 CCVIS		02/06/2018 19:52	1	2018.02.06_537X X 061.d	GeminiC18 3x100 3(mm)

LCMS BATCH WORKSHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1

SDG No.: _____

Batch Number: 206379 Batch Start Date: 01/31/18 12:29 Batch Analyst: Kolstad, Kate M

Batch Method: 537 Batch End Date: 02/02/18 17:10

Lab Sample ID	Client Sample ID	Method Chain	Basis	GrossWeight	TareWeight	InitialAmount	FinalAmount	ReceivedpH	LC537-IS 00057
MB 320-206379/1		537, 537				250.0 mL	1.0 mL	7 SU	100 uL
LLCS 320-206379/2		537, 537				250.0 mL	1.0 mL	7 SU	100 uL
LLCSD 320-206379/3		537, 537				250.0 mL	1.0 mL	7 SU	100 uL
320-35207-A-1	WGNA-011818-RW-3 325	537, 537	T	276.06 g	28.47 g	247.6 mL	1.0 mL	9 SU	100 uL
320-35207-A-2	WGNA-011818-FRB- 3325	537, 537	T	278.93 g	27.10 g	251.8 mL	1.0 mL	7 SU	100 uL
320-35207-A-3	NAWC-011818-RW-3 16	537, 537	T	275.06 g	28.01 g	247.1 mL	1.0 mL	7 SU	100 uL
320-35207-A-4	NAWC-011818-FRB- 316	537, 537	T	279.13 g	26.64 g	252.5 mL	1.0 mL	7 SU	100 uL
320-35207-A-5	NAWC-011818-RW-2 60	537, 537	T	272.51 g	28.36 g	244.2 mL	1.0 mL	7 SU	100 uL
320-35207-A-6	NAWC-011818-FRB- 260	537, 537	T	277.53 g	26.70 g	250.8 mL	1.0 mL	7 SU	100 uL
320-35207-A-7	NAWC-011818-RW-2 81	537, 537	T	274.54 g	27.09 g	247.5 mL	1.0 mL	7 SU	100 uL
320-35207-A-8	NAWC-011818-FRB- 281	537, 537	T	276.86 g	27.25 g	249.6 mL	1.0 mL	7 SU	100 uL
320-35207-A-9	NAWC-011818-RW-0 32	537, 537	T	275.67 g	28.44 g	247.2 mL	1.0 mL	7 SU	100 uL
320-35207-A-10	NAWC-011818-FRB- 032	537, 537	T	271.39 g	27.23 g	244.2 mL	1.0 mL	7 SU	100 uL
320-35207-A-11	NAWC-011818-RW-0 38	537, 537	T	278.52 g	28.97 g	249.6 mL	1.0 mL	7 SU	100 uL
320-35207-A-12	NAWC-011818-FRB- 038	537, 537	T	276.83 g	27.18 g	249.7 mL	1.0 mL	7 SU	100 uL

Lab Sample ID	Client Sample ID	Method Chain	Basis	LC537-LSP 00026	LC537-SU 00053	AnalysisComment			
MB 320-206379/1		537, 537			100 uL	C1 ND			
LLCS 320-206379/2		537, 537		100 uL	100 uL	C1 ND			
LLCSD 320-206379/3		537, 537		100 uL	100 uL	C1 ND			
320-35207-A-1	WGNA-011818-RW-3 325	537, 537	T		100 uL	C1 ND			
320-35207-A-2	WGNA-011818-FRB- 3325	537, 537	T		100 uL	C1 ND			

The pound sign (#) in the amount added field denotes that the reagent was used undiluted. All calculations are performed using the stated concentration for this reagent.

LCMS BATCH WORKSHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1

SDG No.: _____

Batch Number: 206379 Batch Start Date: 01/31/18 12:29 Batch Analyst: Kolstad, Kate M

Batch Method: 537 Batch End Date: 02/02/18 17:10

Lab Sample ID	Client Sample ID	Method Chain	Basis	LC537-LSP 00026	LC537-SU 00053	AnalysisComment			
320-35207-A-3	NAWC-011818-RW-316	537, 537	T		100 uL	C1 ND			
320-35207-A-4	NAWC-011818-FRB-316	537, 537	T		100 uL	C1 ND			
320-35207-A-5	NAWC-011818-RW-260	537, 537	T		100 uL	C1 ND			
320-35207-A-6	NAWC-011818-FRB-260	537, 537	T		100 uL	C1 ND			
320-35207-A-7	NAWC-011818-RW-281	537, 537	T		100 uL	C1 ND			
320-35207-A-8	NAWC-011818-FRB-281	537, 537	T		100 uL	C1 ND			
320-35207-A-9	NAWC-011818-RW-032	537, 537	T		100 uL	C1 ND			
320-35207-A-10	NAWC-011818-FRB-032	537, 537	T		100 uL	C1 ND			
320-35207-A-11	NAWC-011818-RW-038	537, 537	T		100 uL	C1 ND			
320-35207-A-12	NAWC-011818-FRB-038	537, 537	T		100 uL	C1 ND			

The pound sign (#) in the amount added field denotes that the reagent was used undiluted. All calculations are performed using the stated concentration for this reagent.

LCMS BATCH WORKSHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1

SDG No.: _____

Batch Number: 206379 Batch Start Date: 01/31/18 12:29 Batch Analyst: Kolstad, Kate M

Batch Method: 537 Batch End Date: 02/02/18 17:10

Batch Notes	
Analyst ID - Aliquot Step	VPM
Batch Comment	Client labels match: KMK 1-30-18
Analyst ID - Concentration	CCB
Analyst ID - Final Volume Step	CCB
Internal Standard ID#	1145836
Manifold ID	3, 10
Methanol ID	1137492
pH Indicator ID	2517
Pipette ID	H14930F
Analyst ID - IS Reagent Drop	CCB
Analyst ID - IS Reagent Drop Witness	TWL
Analyst ID - SU Reagent Drop	CCB
Analyst ID - SU Reagent Drop Witness	KMK
Analyst ID - TA Reagent Drop	CCB
Analyst ID - TA Reagent Drop Witness	KMK
SPE Cartridge ID	6369499-04
Trizma ID	SLBR4303V
Reagent Water ID	1-30-18

Basis	Basis Description
T	Total/NA

The pound sign (#) in the amount added field denotes that the reagent was used undiluted. All calculations are performed using the stated concentration for this reagent.

Job No: 320-35207 Instrument ID & Date: A8, 2/6/18 ICAL Batch: 152908
 Extraction Batch: 200379 Worklist #: 53775 TALS Batch: 207252, 207294

Review Items	--- Level 1 ---			Level 2
	Yes	No	N/A	
Initial Calibration				
1. Is ICAL verified and locked in Chrom & TALS?	✓			✓
2. Is ICV properly linked in TALS?	✓			✓
Continuing Calibration				
1. Low-range CCV injected at start of analytical run? CCV injected after every 10 samples and at the end of the analytical run and alternated between Low-range, Mid-range and High-range?	✓			✓
2. If sequence was not after an ICAL was a low and mid range CCV injected at the start of the analytical run?	✓			✓
3. Native compounds and surrogates in control? Low-range within ±50% of true value Mid and High-range within ±30% of true value	✓			✓
4. Internal Standard areas in control? Areas ≥ 50% of average area of the ICAL and 70-140% of the most recent CCV.	✓			✓
Client Samples & QC Sample Results				
1. Were preparation and analysis done within holding times?	✓			✓
2. Are Chromatograms reviewed and spectra verified?	✓			✓
3. Are positive results within calibration range? <i>J values</i>	✓			✓
4. Dilutions due to target cpds? _____ Dilutions due to non-targets? _____		✓		✓
5. All target compounds in MB < 1/3 RL ? (Requires NCM if "no.")	✓			✓
6. Are target constituents in LCS/LCSD within method control limits?	✓			✓
7. Internal Standard areas in control for all samples and QC reported? ±50% from the average area of the ICAL and 70-140% of the most recent CCV	✓			✓
8. Do results (e.g., dilutions/trip blanks) make sense?	✓			✓
9. Are MS/MSD recoveries and RPDs within method control limits?			✓	
10. Are all QC samples properly linked in TALS?	✓			✓
11. All manual integrations appropriate and completely documented?	✓			✓
12. Are nonconformances documented as NCMs?			✓	✓
13. Are all Chrom graphics uploaded?	✓			✓

1st Level Reviewer / Date: Sub 2/7/18
JRB 2-7-18

2nd Level Reviewer / Date: Amey 2/2/18

NCM # and Comments: _____

TestAmerica Laboratories
Worklist QC Batch Report

Worklist Name: 06FEB2018_537F Worklist Number: 53779
 Instrument Name: A8_N Chrom Method: 537_A8_N
 Data Directory: \\ChromNa\Sacramento\ChromData\A8_N\20180207-53779.b
 QC Batching: Enabled Limit Group Batching: Enabled

QC Batch: 1	LC 537 CS ICAL Raw Batch: 207291	LC 537 ICAL Raw Batch: 207292
# 1 CCV L3 # 2 RB # 3 MB 320-206379/1-A # 4 LLCS 320-206379/2-A # 5 LLCSD 320-206379/3-A # 6 320-35207-A-1-A # 7 320-35207-A-2-A # 8 320-35207-A-3-A # 9 320-35207-A-4-A #10 320-35207-A-5-A #11 CCV L5	# 1 CCV L3 # 2 RB #11 CCV L5	# 1 CCV L3 # 2 RB # 3 MB 320-206379/1-A # 4 LLCS 320-206379/2-A # 5 LLCSD 320-206379/3-A # 6 320-35207-A-1-A # 7 320-35207-A-2-A # 8 320-35207-A-3-A # 9 320-35207-A-4-A #10 320-35207-A-5-A #11 CCV L5

QC Batch: 2	LC 537 CS ICAL Raw Batch: 207293	LC 537 ICAL Raw Batch: 207294
#11 CCV L5 #12 RB #13 320-35207-A-6-A #14 320-35207-A-7-A #15 320-35207-A-8-A #16 320-35207-A-9-A #17 320-35207-A-10-A #18 320-35207-A-11-A #19 320-35207-A-12-A #20 CCV L3 #21 RB	#11 CCV L5 #12 RB #20 CCV L3 #21 RB	#11 CCV L5 #12 RB #13 320-35207-A-6-A #14 320-35207-A-7-A #15 320-35207-A-8-A #16 320-35207-A-9-A #17 320-35207-A-10-A #18 320-35207-A-11-A #19 320-35207-A-12-A #20 CCV L3

ICAL - 192908
CCVL - 207097

A8

Instrument ID & Date: 11-3-17 Worklist#: 49975

ICAL Batch: 192908, 192909 Calibration ID number: 36012, 36013

Review Items	-- Level 1 --			Level 2
	Yes	No	N/A	
Initial Calibration				
1. Mass calibration, as needed, verified by full scan of PFC stock standard. All PFC ions used for quantitation are within 0.3 m/z of true mass?	✓			✓
2. Responses increase with increasing concentration?	✓			✓
3. Fit used (circle): <u>Average</u> Linear (1/x ²)Linear <u>Quadratic</u> (6 points minimum)				
4. Meets fit criteria? Intercept ≤ 1/2 RL RSD ≤ 30% for Average R ² ≥ 0.990 for Linear R ² ≥ 0.990 for Quadratic NOTE: "Force through Zero" must be used and weighted if needed	✓			✓
5. If quadratic fit used the curve does not "bend over".	✓			✓
6. Feed calibration points into the calculated curve. Are points ≤MRL within ±50% of true value? Are points >MRL within ±30% of true value?	✓			✓
7. Any carryover from the high calibration point must be < 1/3 RL	✓			✓
8. Asymmetry check meets criteria for the first two eluting peaks? (0.8 - 1.5).	✓			✓
9. Is the asymmetry check scanned and linked in TALS to the calibration point?	✓			✓
10. Is ICV (2 nd source) ± 30% of true value?	✓			✓
11. Is ICV (2 nd source) internal standards ±50% of average area of the ICAL?	✓			✓
12. ICAL locked in Chrom and uploaded to TALS?	✓			✓
13. ICAL locked in TALS and scanned?				✓

1st Level Reviewer / Date: JRB 11-6-17

2nd Level Reviewer / Date: MWJ 11/6/2017

NCM # and Comments: _____

Aqueous Extraction Analysis Sheet

69 AB 2/5/18

(To Accompany Samples to Instruments)

Batch Number: 320-206379

Analyst: Kolstad, Kate M

Batch Open: 1/31/2018 12:29:00PM

Method Code: 320-537_Prep-320

Batch End: 2/2/2018 5:10:00PM

Extraction of Perfluorinated Alkyl Acids

Due: 2/19

Input Sample Lab ID (Analytical Method)	SDG (Job #)	GrossWt TareWt	InitAmnt FinAmnt	Rcvd	PHs Adj1	Adj2	Due Date	Analytical TAT	Div Rank	Comments	Output Sample Lab ID
1 MB-320-206379/1 N/A	N/A		250.0 mL	7			N/A	N/A	N/A	CI ND	
			1.0 mL								
2 LLCS-320-206379/2 N/A	N/A		250.0 mL	7			N/A	N/A	N/A	CI ND	
			1.0 mL								
3 LLCSD-320-206379/3 N/A	N/A		250.0 mL	7			N/A	N/A	N/A	CI ND	
			1.0 mL								
4 320-35207-A-1 (537_DOD5)	N/A (320-35207-1)	276.06 g	247.6 mL	9			1/23/18	16_Days	4	CI ND	
		28.47 g	1.0 mL								
5 320-35207-A-2 (537_DOD5)	N/A (320-35207-1)	278.93 g	251.8 mL	7			1/23/18	16_Days	4	CI ND	
		27.10 g	1.0 mL								
6 320-35207-A-3 (537_DOD5)	N/A (320-35207-1)	275.06 g	247.1 mL	7			1/23/18	16_Days	4	CI ND	
		28.01 g	1.0 mL								
7 320-35207-A-4 (537_DOD5)	N/A (320-35207-1)	279.13 g	252.5 mL	7			1/23/18	16_Days	4	CI ND	
		26.64 g	1.0 mL								
8 320-35207-A-5 (537_DOD5)	N/A (320-35207-1)	272.51 g	244.2 mL	7			1/23/18	16_Days	4	CI ND	
		28.36 g	1.0 mL								
9 320-35207-A-6 (537_DOD5)	N/A (320-35207-1)	277.53 g	250.8 mL	7			1/23/18	16_Days	4	CI ND	
		26.70 g	1.0 mL								
10 320-35207-A-7 (537_DOD5)	N/A (320-35207-1)	274.54 g	247.5 mL	7			1/23/18	16_Days	4	CI ND	
		27.09 g	1.0 mL								

Page 292 of 301

Aqueous Extraction Analysis Sheet

(To Accompany Samples to Instruments)






Batch Number: 320-206379

Analyst: Kolstad, Kate M

Batch Open: 1/31/2018 12:29:00PM

Method Code: 320-537_Prep-320

Batch End: 2/2/2018 5:10:00PM

11	320-35207-A-8 (537_DOD5)	N/A (320-35207-1)	276.86 g	249.6 mL	7		1/23/18	16_Days	4	CI ND	
			27.25 g	1.0 mL							
12	320-35207-A-9 (537_DOD5)	N/A (320-35207-1)	275.67 g	247.2 mL	7		1/23/18	16_Days	4	CI ND	
			28.44 g	1.0 mL							
13	320-35207-A-10 (537_DOD5)	N/A (320-35207-1)	271.39 g	244.2 mL	7		1/23/18	16_Days	4	CI ND	
			27.23 g	1.0 mL							
14	320-35207-A-11 (537_DOD5)	N/A (320-35207-1)	278.52 g	249.6 mL	7		1/23/18	16_Days	4	CI ND	
			28.97 g	1.0 mL							
15	320-35207-A-12 (537_DOD5)	N/A (320-35207-1)	276.83 g	249.7 mL	7		1/23/18	16_Days	4	CI ND	
			27.18 g	1.0 mL							

Page 293 of 301

Aqueous Extraction Analysis Sheet

(To Accompany Samples to Instruments)

Batch Number: 320-206379

Analyst: Kolstad, Kate M

Batch Open: 1/31/2018 12:29:00PM

Method Code: 320-537_Prep-320

Batch End: 2/2/2018 5:10:00PM

Batch Notes

Manifold ID 3, 10

pH Indicator ID 2517

Trizma ID SLBR4303V

SPE Cartridge ID 6369499-04

Methanol ID 1137492

Reagent Water ID 1-30-18

Internal Standard ID# 1145836

Pipette ID H14930F

Analyst ID - TA Reagent Drop CCB

Analyst ID - TA Reagent Drop KMK
Witness

Analyst ID - SU Reagent Drop CCB

Analyst ID - SU Reagent Drop KMK
Witness

Analyst ID - IS Reagent Drop CCB

Analyst ID - IS Reagent Drop TWL
Witness

Analyst ID - Concentration CCB

Analyst ID - Aliquot Step VPM

Analyst ID - Final Volume Step CCB

Batch Comment Client labels match: KMK 1-30-18

Page 294 of 301

Aqueous Extraction Analysis Sheet

(To Accompany Samples to Instruments)

Batch Number: 320-206379

Analyst: Kolstad, Kate M

Batch Open: 1/31/2018 12:29:00PM

Method Code: 320-537_Prep-320

Batch End: 2/2/2018 5:10:00PM

Comments

Aqueous Extraction Analysis Sheet

(To Accompany Samples to Instruments)

Batch Number: 320-206379

Analyst: Kolstad, Kate M

Batch Open: 1/31/2018 12:29:00PM

Method Code: 320-537_Prep-320

Batch End:

Reagent Additions Worksheet

Lab ID	Reagent Code	Amount Added	Final Amount	By	Witness
MB 320-206379/1	LC537-SU_00053	100 uL	1.0 mL	<i>KMK 1-31-18</i>	<i>KMK 1-31-18</i>
LLCS 320-206379/2	LC537-LSP_00026	100 uL	1.0 mL		
LLCS 320-206379/2	LC537-SU_00053	100 uL	1.0 mL		
LLCSD 320-206379/3	LC537-LSP_00026	100 uL	1.0 mL		
LLCSD 320-206379/3	LC537-SU_00053	100 uL	1.0 mL		
320-35207-A-1	LC537-SU_00053	100 uL	1.0 mL		
320-35207-A-2	LC537-SU_00053	100 uL	1.0 mL		
320-35207-A-3	LC537-SU_00053	100 uL	1.0 mL		
320-35207-A-4	LC537-SU_00053	100 uL	1.0 mL		
320-35207-A-5	LC537-SU_00053	100 uL	1.0 mL		
320-35207-A-6	LC537-SU_00053	100 uL	1.0 mL		
320-35207-A-7	LC537-SU_00053	100 uL	1.0 mL		
320-35207-A-8	LC537-SU_00053	100 uL	1.0 mL		
320-35207-A-9	LC537-SU_00053	100 uL	1.0 mL		
320-35207-A-10	LC537-SU_00053	100 uL	1.0 mL		
320-35207-A-11	LC537-SU_00053	100 uL	1.0 mL		
320-35207-A-12	LC537-SU_00053	100 uL	1.0 mL		

Page 296 of 301

Aqueous Extraction Analysis Sheet

(To Accompany Samples to Instruments)

Batch Number: 320-206379

Analyst: Kolstad, Kate M

Batch Open: 1/31/2018 12:29:00PM

Method Code: 320-537_Prep-320

Batch End:

Other Reagents:		
Reagent	Amount/Units	Lot#:

Page 297 of 301

Preparation Batch Number(s) 206379 Test 537-Prep
 Earliest Holding Time 2-1-18

Batch Information	1 st Level Reviewer	2 nd Level Reviewer
Date and time accurate and entered into TALS correctly	✓	✓
All necessary batch information complete and entered into TALS correctly	✓	✓
BD, FV, and AL initials are transcribed into the batch comment	✓	✓
Sample List Tab	1 st Level Reviewer	2 nd Level Reviewer
Samples identified to the correct method	✓	✓
Holding time violation NCM filed	NT	NA
MS/MSD or MS/DU NCM filed	✓	✓
NCM for any anomalies filed	✓	✓
All NCMs include method code, matrix, and prep batch	✓	✓
Method/sample/login/QAS checked and correct	✓	✓
Batch contains no more than 20 live samples	✓	✓
Worksheet Tab	1 st Level Reviewer	2 nd Level Reviewer
All samples properly preserved	✓	✓
Weights in anticipated range and not targeted	✓	✓
All additional test requirements performed, documented, and uploaded to TALS correctly (e.g. final amount, initial amount, turbidity, and CI Check)	✓	✓
The pH is transcribed properly in TALS	✓	✓
All additional information is transcribed into TALS and is correct and raw data is attached	✓	✓
Comments/Observations are transcribed correctly in TALS	✓	✓
Reagents Tab	1 st Level Reviewer	2 nd Level Reviewer
All necessary reagents not expired and checked into TALS	✓	✓
All spike amounts correct and added to necessary samples and QC	✓	✓
Internal Standard is added to the reagents	✓	✓
All units are correctly transcribed into TALS	✓	✓

1st Level Reviewer: [Signature]
 2nd Level Reviewer: [Signature]
 Comments: _____

Date: 2/2/18
 Date: 2/2/18

Shipping and Receiving Documents

Login Sample Receipt Checklist

Client: Tetra Tech, Inc.

Job Number: 320-35207-1

Login Number: 35207
List Number: 1
Creator: Nelson, Kym D

List Source: TestAmerica Sacramento

Question	Answer	Comment
Radioactivity wasn't checked or is \leq background as measured by a survey meter.	True	
The cooler's custody seal, if present, is intact.	True	
Sample custody seals, if present, are intact.	N/A	
The cooler or samples do not appear to have been compromised or tampered with.	True	
Samples were received on ice.	True	
Cooler Temperature is acceptable.	True	
Cooler Temperature is recorded.	True	
COC is present.	True	
COC is filled out in ink and legible.	True	
COC is filled out with all pertinent information.	True	
Is the Field Sampler's name present on COC?	True	
There are no discrepancies between the containers received and the COC.	True	
Samples are received within Holding Time (excluding tests with immediate HTs)	True	
Sample containers have legible labels.	True	
Containers are not broken or leaking.	True	
Sample collection date/times are provided.	True	
Appropriate sample containers are used.	True	
Sample bottles are completely filled.	True	
Sample Preservation Verified.	N/A	
There is sufficient vol. for all requested analyses, incl. any requested MS/MSDs	True	
Containers requiring zero headspace have no headspace or bubble is $<6\text{mm}$ (1/4").	True	
Multiphasic samples are not present.	True	
Samples do not require splitting or compositing.	True	
Residual Chlorine Checked.	N/A	

"WGNA-011818-RW-3325", "537", "RES", "320-35207-1", "TALSAC", "1763-23-1", "Perfluorooctanesulfonic acid (PFOS)", "14", "ng/L", "J M", "6.9", "DL", "", "TRG", "", "", "40", "LOQ", "YES", "-99", "", "247.6", "1.0", "16", ""

"WGNA-011818-RW-3325", "537", "RES", "320-35207-1", "TALSAC", "335-67-1", "Perfluorooctanoic acid (PFOA)", "14", "ng/L", "J", "2.8", "DL", "", "TRG", "", "", "20", "LOQ", "YES", "-99", "", "247.6", "1.0", "8.1", ""

"WGNA-011818-RW-3325", "537", "RES", "320-35207-1", "TALSAC", "355-46-4", "Perfluorohexanesulfonic acid (PFHxS)", "13", "ng/L", "J", "5.6", "DL", "", "TRG", "", "", "30", "LOQ", "YES", "-99", "", "247.6", "1.0", "12", ""

"WGNA-011818-RW-3325", "537", "RES", "320-35207-1", "TALSAC", "375-73-5", "Perfluorobutanesulfonic acid (PFBS)", "36", "ng/L", "U", "16", "DL", "", "TRG", "", "", "91", "LOQ", "YES", "-99", "", "247.6", "1.0", "36", ""

"WGNA-011818-RW-3325", "537", "RES", "320-35207-1", "TALSAC", "375-85-9", "Perfluoroheptanoic acid (PFHpA)", "4.2", "ng/L", "J", "1.9", "DL", "", "TRG", "", "", "10", "LOQ", "YES", "-99", "", "247.6", "1.0", "4.0", ""

"WGNA-011818-RW-3325", "537", "RES", "320-35207-1", "TALSAC", "375-95-1", "Perfluorononanoic acid (PFNA)", "20", "ng/L", "U M", "8.1", "DL", "", "TRG", "", "", "24", "LOQ", "YES", "-99", "", "247.6", "1.0", "20", ""

"WGNA-011818-RW-3325", "537", "RES", "320-35207-1", "TALSAC", "STL00993", "13C2
PFHxA", "39", "ng/L", "", "-99", "DL", "", "SURR", "96", "", "-99", "LOQ", "YES", "40.4", "", "247.6", "1.0", "0", ""

"WGNA-011818-RW-3325", "537", "RES", "320-35207-1", "TALSAC", "STL00996", "13C2
PFDA", "44", "ng/L", "", "-99", "DL", "", "SURR", "109", "", "-99", "LOQ", "YES", "40.4", "", "247.6", "1.0", "0", ""

"NAWC-011818-FRB-032", "537", "RES", "320-35207-10", "TALSAC", "1763-23-1", "Perfluorooctanesulfonic acid (PFOS)", "16", "ng/L", "U", "7.0", "DL", "", "TRG", "", "", "41", "LOQ", "YES", "-99", "", "244.2", "1.0", "16", ""

"NAWC-011818-FRB-032", "537", "RES", "320-35207-10", "TALSAC", "335-67-1", "Perfluorooctanoic acid (PFOA)", "8.2", "ng/L", "U", "2.9", "DL", "", "TRG", "", "", "20", "LOQ", "YES", "-99", "", "244.2", "1.0", "8.2", ""

"NAWC-011818-FRB-032", "537", "RES", "320-35207-10", "TALSAC", "355-46-4", "Perfluorohexanesulfonic acid (PFHxS)", "12", "ng/L", "U", "5.6", "DL", "", "TRG", "", "", "31", "LOQ", "YES", "-99", "", "244.2", "1.0", "12", ""

"NAWC-011818-FRB-032", "537", "RES", "320-35207-10", "TALSAC", "375-73-5", "Perfluorobutanesulfonic acid (PFBS)", "37", "ng/L", "U", "16", "DL", "", "TRG", "", "", "92", "LOQ", "YES", "-99", "", "244.2", "1.0", "37", ""

"NAWC-011818-FRB-032", "537", "RES", "320-35207-10", "TALSAC", "375-85-9", "Perfluoroheptanoic acid (PFHpA)", "4.1", "ng/L", "U", "1.9", "DL", "", "TRG", "", "", "10", "LOQ", "YES", "-99", "", "244.2", "1.0", "4.1", ""

"NAWC-011818-FRB-032", "537", "RES", "320-35207-10", "TALSAC", "375-95-1", "Perfluorononanoic acid (PFNA)", "20", "ng/L", "U", "8.2", "DL", "", "TRG", "", "", "25", "LOQ", "YES", "-99", "", "244.2", "1.0", "20", ""

"NAWC-011818-FRB-032", "537", "RES", "320-35207-10", "TALSAC", "STL00993", "13C2
PFHxA", "42", "ng/L", "", "-99", "DL", "", "SURR", "104", "", "-99", "LOQ", "YES", "41.0", "", "244.2", "1.0", "0", ""

"NAWC-011818-FRB-032", "537", "RES", "320-35207-10", "TALSAC", "STL00996", "13C2
PFDA", "43", "ng/L", "", "-99", "DL", "", "SURR", "105", "", "-99", "LOQ", "YES", "41.0", "", "244.2", "1.0", "0", ""

"NAWC-011818-RW-038", "537", "RES", "320-35207-11", "TALSAC", "1763-23-1", "Perfluorooctanesulfonic acid (PFOS)", "25", "ng/L", "J M", "6.8", "DL", "", "TRG", "", "", "40", "LOQ", "YES", "-99", "", "249.6", "1.0", "16", ""

"NAWC-011818-RW-038", "537", "RES", "320-35207-11", "TALSAC", "335-67-1", "Perfluorooctanoic acid (PFOA)", "21", "ng/L", "", "2.8", "DL", "", "TRG", "", "", "20", "LOQ", "YES", "-99", "", "249.6", "1.0", "8.0", ""

"NAWC-011818-RW-038", "537", "RES", "320-35207-11", "TALSAC", "355-46-4", "Perfluorohexanesulfonic acid (PFHxS)", "6.2", "ng/L", "J", "5.5", "DL", "", "TRG", "", "", "30", "LOQ", "YES", "-99", "", "249.6", "1.0", "12", ""

"NAWC-011818-RW-038", "537", "RES", "320-35207-11", "TALSAC", "375-73-5", "Perfluorobutanesulfonic acid (PFBS)", "36", "ng/L", "U", "16", "DL", "", "TRG", "", "", "90", "LOQ", "YES", "-99", "", "249.6", "1.0", "36", ""

"NAWC-011818-RW-038", "537", "RES", "320-35207-11", "TALSAC", "375-85-9", "Perfluoroheptanoic acid (PFHpA)", "5.6", "ng/L", "J", "1.9", "DL", "", "TRG", "", "", "10", "LOQ", "YES", "-99", "", "249.6", "1.0", "4.0", ""

"NAWC-011818-RW-038", "537", "RES", "320-35207-11", "TALSAC", "375-95-1", "Perfluorononanoic acid (PFNA)", "20", "ng/L", "U", "8.0", "DL", "", "TRG", "", "", "24", "LOQ", "YES", "-99", "", "249.6", "1.0", "20", ""

"NAWC-011818-RW-038", "537", "RES", "320-35207-11", "TALSAC", "STL00993", "13C2
PFHxA", "36", "ng/L", "", "-99", "DL", "", "SURR", "90", "", "-99", "LOQ", "YES", "40.1", "", "249.6", "1.0", "0", ""

"NAWC-011818-RW-038", "537", "RES", "320-35207-11", "TALSAC", "STL00996", "13C2
PFDA", "39", "ng/L", "", "-99", "DL", "", "SURR", "97", "", "-99", "LOQ", "YES", "40.1", "", "249.6", "1.0", "0", ""

"NAWC-011818-FRB-038", "537", "RES", "320-35207-12", "TALSAC", "1763-23-1", "Perfluorooctanesulfonic acid (PFOS)", "16", "ng/L", "U", "6.8", "DL", "", "TRG", "", "", "40", "LOQ", "YES", "-99", "", "249.7", "1.0", "16", ""

"NAWC-011818-FRB-038", "537", "RES", "320-35207-12", "TALSAC", "335-67-1", "Perfluorooctanoic acid (PFOA)", "8.0", "ng/L", "U", "2.8", "DL", "", "TRG", "", "", "20", "LOQ", "YES", "-99", "", "249.7", "1.0", "8.0", ""

"NAWC-011818-FRB-038", "537", "RES", "320-35207-12", "TALSAC", "355-46-4", "Perfluorohexanesulfonic acid

(PFHxS),"12","ng/L","U","5.5","DL","","TRG","","","30","LOQ","YES",-99","","249.7","1.0","12","","
"NAWC-011818-FRB-038","537","RES","320-35207-12","TALSAC","375-73-5","Perfluorobutanesulfonic acid
(PFBS),"36","ng/L","U","16","DL","","TRG","","","90","LOQ","YES",-99","","249.7","1.0","36","","
"NAWC-011818-FRB-038","537","RES","320-35207-12","TALSAC","375-85-9","Perfluoroheptanoic acid
(PFHpA),"4.0","ng/L","U","1.9","DL","","TRG","","","10","LOQ","YES",-99","","249.7","1.0","4.0","","
"NAWC-011818-FRB-038","537","RES","320-35207-12","TALSAC","375-95-1","Perfluorononanoic acid
(PFNA),"20","ng/L","U","8.0","DL","","TRG","","","24","LOQ","YES",-99","","249.7","1.0","20","","
"NAWC-011818-FRB-038","537","RES","320-35207-12","TALSAC","STL00993","13C2
PFHxA","43","ng/L","","-99","DL","","SURR","107","","-99","LOQ","YES","40.0","","249.7","1.0","0","","
"NAWC-011818-FRB-038","537","RES","320-35207-12","TALSAC","STL00996","13C2
PFDA","41","ng/L","","-99","DL","","SURR","102","","-99","LOQ","YES","40.0","","249.7","1.0","0","","
"WGNA-011818-FRB-3325","537","RES","320-35207-2","TALSAC","1763-23-1","Perfluorooctanesulfonic acid
(PFOS),"16","ng/L","U","6.8","DL","","TRG","","","40","LOQ","YES",-99","","251.8","1.0","16","","
"WGNA-011818-FRB-3325","537","RES","320-35207-2","TALSAC","335-67-1","Perfluorooctanoic acid
(PFOA),"7.9","ng/L","U","2.8","DL","","TRG","","","20","LOQ","YES",-99","","251.8","1.0","7.9","","
"WGNA-011818-FRB-3325","537","RES","320-35207-2","TALSAC","355-46-4","Perfluorohexanesulfonic acid
(PFHxS),"12","ng/L","U","5.5","DL","","TRG","","","30","LOQ","YES",-99","","251.8","1.0","12","","
"WGNA-011818-FRB-3325","537","RES","320-35207-2","TALSAC","375-73-5","Perfluorobutanesulfonic acid
(PFBS),"36","ng/L","U","16","DL","","TRG","","","89","LOQ","YES",-99","","251.8","1.0","36","","
"WGNA-011818-FRB-3325","537","RES","320-35207-2","TALSAC","375-85-9","Perfluoroheptanoic acid
(PFHpA),"4.0","ng/L","U","1.9","DL","","TRG","","","9.9","LOQ","YES",-99","","251.8","1.0","4.0","","
"WGNA-011818-FRB-3325","537","RES","320-35207-2","TALSAC","375-95-1","Perfluorononanoic acid
(PFNA),"20","ng/L","U","7.9","DL","","TRG","","","24","LOQ","YES",-99","","251.8","1.0","20","","
"WGNA-011818-FRB-3325","537","RES","320-35207-2","TALSAC","STL00993","13C2
PFHxA","45","ng/L","","-99","DL","","SURR","114","","-99","LOQ","YES","39.7","","251.8","1.0","0","","
"WGNA-011818-FRB-3325","537","RES","320-35207-2","TALSAC","STL00996","13C2
PFDA","41","ng/L","","-99","DL","","SURR","104","","-99","LOQ","YES","39.7","","251.8","1.0","0","","
"NAWC-011818-RW-316","537","RES","320-35207-3","TALSAC","1763-23-1","Perfluorooctanesulfonic acid
(PFOS),"45","ng/L","M","6.9","DL","","TRG","","","40","LOQ","YES",-99","","247.1","1.0","16","","
"NAWC-011818-RW-316","537","RES","320-35207-3","TALSAC","335-67-1","Perfluorooctanoic acid
(PFOA),"24","ng/L","M","2.8","DL","","TRG","","","20","LOQ","YES",-99","","247.1","1.0","8.1","","
"NAWC-011818-RW-316","537","RES","320-35207-3","TALSAC","355-46-4","Perfluorohexanesulfonic acid
(PFHxS),"32","ng/L","","5.6","DL","","TRG","","","30","LOQ","YES",-99","","247.1","1.0","12","","
"NAWC-011818-RW-316","537","RES","320-35207-3","TALSAC","375-73-5","Perfluorobutanesulfonic acid
(PFBS),"36","ng/L","U","16","DL","","TRG","","","91","LOQ","YES",-99","","247.1","1.0","36","","
"NAWC-011818-RW-316","537","RES","320-35207-3","TALSAC","375-85-9","Perfluoroheptanoic acid
(PFHpA),"9.0","ng/L","J","1.9","DL","","TRG","","","10","LOQ","YES",-99","","247.1","1.0","4.0","","
"NAWC-011818-RW-316","537","RES","320-35207-3","TALSAC","375-95-1","Perfluorononanoic acid
(PFNA),"20","ng/L","U","8.1","DL","","TRG","","","24","LOQ","YES",-99","","247.1","1.0","20","","
"NAWC-011818-RW-316","537","RES","320-35207-3","TALSAC","STL00993","13C2
PFHxA","42","ng/L","","-99","DL","","SURR","103","","-99","LOQ","YES","40.5","","247.1","1.0","0","","
"NAWC-011818-RW-316","537","RES","320-35207-3","TALSAC","STL00996","13C2
PFDA","41","ng/L","","-99","DL","","SURR","102","","-99","LOQ","YES","40.5","","247.1","1.0","0","","
"NAWC-011818-FRB-316","537","RES","320-35207-4","TALSAC","1763-23-1","Perfluorooctanesulfonic acid
(PFOS),"16","ng/L","U","6.7","DL","","TRG","","","40","LOQ","YES",-99","","252.5","1.0","16","","
"NAWC-011818-FRB-316","537","RES","320-35207-4","TALSAC","335-67-1","Perfluorooctanoic acid
(PFOA),"7.9","ng/L","U","2.8","DL","","TRG","","","20","LOQ","YES",-99","","252.5","1.0","7.9","","
"NAWC-011818-FRB-316","537","RES","320-35207-4","TALSAC","355-46-4","Perfluorohexanesulfonic acid
(PFHxS),"12","ng/L","U","5.4","DL","","TRG","","","30","LOQ","YES",-99","","252.5","1.0","12","","
"NAWC-011818-FRB-316","537","RES","320-35207-4","TALSAC","375-73-5","Perfluorobutanesulfonic acid
(PFBS),"36","ng/L","U","16","DL","","TRG","","","89","LOQ","YES",-99","","252.5","1.0","36","","
"NAWC-011818-FRB-316","537","RES","320-35207-4","TALSAC","375-85-9","Perfluoroheptanoic acid
(PFHpA),"4.0","ng/L","U","1.9","DL","","TRG","","","9.9","LOQ","YES",-99","","252.5","1.0","4.0","","
"NAWC-011818-FRB-316","537","RES","320-35207-4","TALSAC","375-95-1","Perfluorononanoic acid

(PFNA),"20","ng/L","U","7.9","DL","","TRG","","","24","LOQ","YES","-99","","252.5","1.0","20","","NAWC-011818-FRB-316","537","RES","320-35207-4","TALSAC","STL00993","13C2
PFHxA","43","ng/L","","-99","DL","","SURR","109","","-99","LOQ","YES","39.6","","252.5","1.0","0","","NAWC-011818-FRB-316","537","RES","320-35207-4","TALSAC","STL00996","13C2
PFDA","40","ng/L","","-99","DL","","SURR","100","","-99","LOQ","YES","39.6","","252.5","1.0","0","","NAWC-011818-RW-260","537","RES","320-35207-5","TALSAC","1763-23-1","Perfluorooctanesulfonic acid (PFOS)","23","ng/L","J M","7.0","DL","","TRG","","","41","LOQ","YES","-99","","244.2","1.0","16","","NAWC-011818-RW-260","537","RES","320-35207-5","TALSAC","335-67-1","Perfluorooctanoic acid (PFOA)","24","ng/L","","2.9","DL","","TRG","","","20","LOQ","YES","-99","","244.2","1.0","8.2","","NAWC-011818-RW-260","537","RES","320-35207-5","TALSAC","355-46-4","Perfluorohexanesulfonic acid (PFHxS)","8.6","ng/L","J","5.6","DL","","TRG","","","31","LOQ","YES","-99","","244.2","1.0","12","","NAWC-011818-RW-260","537","RES","320-35207-5","TALSAC","375-73-5","Perfluorobutanesulfonic acid (PFBS)","16","ng/L","J","16","DL","","TRG","","","92","LOQ","YES","-99","","244.2","1.0","37","","NAWC-011818-RW-260","537","RES","320-35207-5","TALSAC","375-85-9","Perfluoroheptanoic acid (PFHpA)","7.0","ng/L","J","1.9","DL","","TRG","","","10","LOQ","YES","-99","","244.2","1.0","4.1","","NAWC-011818-RW-260","537","RES","320-35207-5","TALSAC","375-95-1","Perfluorononanoic acid (PFNA)","20","ng/L","U M","8.2","DL","","TRG","","","25","LOQ","YES","-99","","244.2","1.0","20","","NAWC-011818-RW-260","537","RES","320-35207-5","TALSAC","STL00993","13C2
PFHxA","42","ng/L","","-99","DL","","SURR","104","","-99","LOQ","YES","41.0","","244.2","1.0","0","","NAWC-011818-RW-260","537","RES","320-35207-5","TALSAC","STL00996","13C2
PFDA","43","ng/L","","-99","DL","","SURR","105","","-99","LOQ","YES","41.0","","244.2","1.0","0","","NAWC-011818-FRB-260","537","RES","320-35207-6","TALSAC","1763-23-1","Perfluorooctanesulfonic acid (PFOS)","16","ng/L","U","6.8","DL","","TRG","","","40","LOQ","YES","-99","","250.8","1.0","16","","NAWC-011818-FRB-260","537","RES","320-35207-6","TALSAC","335-67-1","Perfluorooctanoic acid (PFOA)","8.0","ng/L","U","2.8","DL","","TRG","","","20","LOQ","YES","-99","","250.8","1.0","8.0","","NAWC-011818-FRB-260","537","RES","320-35207-6","TALSAC","355-46-4","Perfluorohexanesulfonic acid (PFHxS)","12","ng/L","U","5.5","DL","","TRG","","","30","LOQ","YES","-99","","250.8","1.0","12","","NAWC-011818-FRB-260","537","RES","320-35207-6","TALSAC","375-73-5","Perfluorobutanesulfonic acid (PFBS)","36","ng/L","U","16","DL","","TRG","","","90","LOQ","YES","-99","","250.8","1.0","36","","NAWC-011818-FRB-260","537","RES","320-35207-6","TALSAC","375-85-9","Perfluoroheptanoic acid (PFHpA)","4.0","ng/L","U","1.9","DL","","TRG","","","10","LOQ","YES","-99","","250.8","1.0","4.0","","NAWC-011818-FRB-260","537","RES","320-35207-6","TALSAC","375-95-1","Perfluorononanoic acid (PFNA)","20","ng/L","U","8.0","DL","","TRG","","","24","LOQ","YES","-99","","250.8","1.0","20","","NAWC-011818-FRB-260","537","RES","320-35207-6","TALSAC","STL00993","13C2
PFHxA","42","ng/L","","-99","DL","","SURR","104","","-99","LOQ","YES","39.9","","250.8","1.0","0","","NAWC-011818-FRB-260","537","RES","320-35207-6","TALSAC","STL00996","13C2
PFDA","41","ng/L","","-99","DL","","SURR","102","","-99","LOQ","YES","39.9","","250.8","1.0","0","","NAWC-011818-RW-281","537","RES","320-35207-7","TALSAC","1763-23-1","Perfluorooctanesulfonic acid (PFOS)","13","ng/L","J M","6.9","DL","","TRG","","","40","LOQ","YES","-99","","247.5","1.0","16","","NAWC-011818-RW-281","537","RES","320-35207-7","TALSAC","335-67-1","Perfluorooctanoic acid (PFOA)","15","ng/L","J","2.8","DL","","TRG","","","20","LOQ","YES","-99","","247.5","1.0","8.1","","NAWC-011818-RW-281","537","RES","320-35207-7","TALSAC","355-46-4","Perfluorohexanesulfonic acid (PFHxS)","6.4","ng/L","J","5.6","DL","","TRG","","","30","LOQ","YES","-99","","247.5","1.0","12","","NAWC-011818-RW-281","537","RES","320-35207-7","TALSAC","375-73-5","Perfluorobutanesulfonic acid (PFBS)","36","ng/L","U","16","DL","","TRG","","","91","LOQ","YES","-99","","247.5","1.0","36","","NAWC-011818-RW-281","537","RES","320-35207-7","TALSAC","375-85-9","Perfluoroheptanoic acid (PFHpA)","4.4","ng/L","J","1.9","DL","","TRG","","","10","LOQ","YES","-99","","247.5","1.0","4.0","","NAWC-011818-RW-281","537","RES","320-35207-7","TALSAC","375-95-1","Perfluorononanoic acid (PFNA)","20","ng/L","U","8.1","DL","","TRG","","","24","LOQ","YES","-99","","247.5","1.0","20","","NAWC-011818-RW-281","537","RES","320-35207-7","TALSAC","STL00993","13C2
PFHxA","40","ng/L","","-99","DL","","SURR","99","","-99","LOQ","YES","40.4","","247.5","1.0","0","","NAWC-011818-RW-281","537","RES","320-35207-7","TALSAC","STL00996","13C2
PFDA","42","ng/L","","-99","DL","","SURR","103","","-99","LOQ","YES","40.4","","247.5","1.0","0","","NAWC-011818-FRB-281","537","RES","320-35207-8","TALSAC","1763-23-1","Perfluorooctanesulfonic acid

(PFOS),"16","ng/L","U","6.8","DL","","TRG","","","40","LOQ","YES","-99","","249.6","1.0","16",""
"NAWC-011818-FRB-281","537","RES","320-35207-8","TALSAC","335-67-1","Perfluorooctanoic acid
(PFOA),"8.0","ng/L","U","2.8","DL","","TRG","","","20","LOQ","YES","-99","","249.6","1.0","8.0",""
"NAWC-011818-FRB-281","537","RES","320-35207-8","TALSAC","355-46-4","Perfluorohexanesulfonic acid
(PFHxS),"12","ng/L","U","5.5","DL","","TRG","","","30","LOQ","YES","-99","","249.6","1.0","12",""
"NAWC-011818-FRB-281","537","RES","320-35207-8","TALSAC","375-73-5","Perfluorobutanesulfonic acid
(PFBS),"36","ng/L","U","16","DL","","TRG","","","90","LOQ","YES","-99","","249.6","1.0","36",""
"NAWC-011818-FRB-281","537","RES","320-35207-8","TALSAC","375-85-9","Perfluoroheptanoic acid
(PFHpA),"4.0","ng/L","U","1.9","DL","","TRG","","","10","LOQ","YES","-99","","249.6","1.0","4.0",""
"NAWC-011818-FRB-281","537","RES","320-35207-8","TALSAC","375-95-1","Perfluorononanoic acid
(PFNA),"20","ng/L","U","8.0","DL","","TRG","","","24","LOQ","YES","-99","","249.6","1.0","20",""
"NAWC-011818-FRB-281","537","RES","320-35207-8","TALSAC","STL00993","13C2
PFHxA","41","ng/L","","-99","DL","","SURR","103","","-99","LOQ","YES","40.1","","249.6","1.0","0",""
"NAWC-011818-FRB-281","537","RES","320-35207-8","TALSAC","STL00996","13C2
PFDA","41","ng/L","","-99","DL","","SURR","102","","-99","LOQ","YES","40.1","","249.6","1.0","0",""
"NAWC-011818-RW-032","537","RES","320-35207-9","TALSAC","1763-23-1","Perfluorooctanesulfonic acid
(PFOS),"20","ng/L","J M","6.9","DL","","TRG","","","40","LOQ","YES","-99","","247.2","1.0","16",""
"NAWC-011818-RW-032","537","RES","320-35207-9","TALSAC","335-67-1","Perfluorooctanoic acid
(PFOA),"16","ng/L","J","2.8","DL","","TRG","","","20","LOQ","YES","-99","","247.2","1.0","8.1",""
"NAWC-011818-RW-032","537","RES","320-35207-9","TALSAC","355-46-4","Perfluorohexanesulfonic acid
(PFHxS),"14","ng/L","J","5.6","DL","","TRG","","","30","LOQ","YES","-99","","247.2","1.0","12",""
"NAWC-011818-RW-032","537","RES","320-35207-9","TALSAC","375-73-5","Perfluorobutanesulfonic acid
(PFBS),"36","ng/L","U","16","DL","","TRG","","","91","LOQ","YES","-99","","247.2","1.0","36",""
"NAWC-011818-RW-032","537","RES","320-35207-9","TALSAC","375-85-9","Perfluoroheptanoic acid
(PFHpA),"5.4","ng/L","J","1.9","DL","","TRG","","","10","LOQ","YES","-99","","247.2","1.0","4.0",""
"NAWC-011818-RW-032","537","RES","320-35207-9","TALSAC","375-95-1","Perfluorononanoic acid
(PFNA),"20","ng/L","U","8.1","DL","","TRG","","","24","LOQ","YES","-99","","247.2","1.0","20",""
"NAWC-011818-RW-032","537","RES","320-35207-9","TALSAC","STL00993","13C2
PFHxA","35","ng/L","","-99","DL","","SURR","88","","-99","LOQ","YES","40.5","","247.2","1.0","0",""
"NAWC-011818-RW-032","537","RES","320-35207-9","TALSAC","STL00996","13C2
PFDA","42","ng/L","","-99","DL","","SURR","104","","-99","LOQ","YES","40.5","","247.2","1.0","0",""
"LLCS 320-206379/2-A","537","RES","LLCS 320-206379/2-A","TALSAC","1763-23-1","Perfluorooctanesulfonic
acid (PFOS),"40.2","ng/L","M","6.8","DL","","SPK","100","","40","LOQ","YES","40.0","","250.0","1.0","16",""
"LLCS 320-206379/2-A","537","RES","LLCS 320-206379/2-A","TALSAC","335-67-1","Perfluorooctanoic acid
(PFOA),"22.1","ng/L","","2.8","DL","","SPK","111","","20","LOQ","YES","20.0","","250.0","1.0","8.0",""
"LLCS 320-206379/2-A","537","RES","LLCS 320-206379/2-A","TALSAC","355-46-4","Perfluorohexanesulfonic acid
(PFHxS),"33.0","ng/L","","5.5","DL","","SPK","110","","30","LOQ","YES","30.0","","250.0","1.0","12",""
"LLCS 320-206379/2-A","537","RES","LLCS 320-206379/2-A","TALSAC","375-73-5","Perfluorobutanesulfonic acid
(PFBS),"94.5","ng/L","","16","DL","","SPK","105","","90","LOQ","YES","90.0","","250.0","1.0","36",""
"LLCS 320-206379/2-A","537","RES","LLCS 320-206379/2-A","TALSAC","375-85-9","Perfluoroheptanoic acid
(PFHpA),"11.6","ng/L","","1.9","DL","","SPK","116","","10","LOQ","YES","10.0","","250.0","1.0","4.0",""
"LLCS 320-206379/2-A","537","RES","LLCS 320-206379/2-A","TALSAC","375-95-1","Perfluorononanoic acid
(PFNA),"21.9","ng/L","J","8.0","DL","","SPK","110","","24","LOQ","YES","20.0","","250.0","1.0","20",""
"LLCS 320-206379/2-A","537","RES","LLCS 320-206379/2-A","TALSAC","STL00993","13C2
PFHxA","42.5","ng/L","","-99","DL","","SURR","106","","-99","LOQ","YES","40.0","","250.0","1.0","0",""
"LLCS 320-206379/2-A","537","RES","LLCS 320-206379/2-A","TALSAC","STL00996","13C2
PFDA","41.5","ng/L","","-99","DL","","SURR","104","","-99","LOQ","YES","40.0","","250.0","1.0","0",""
"LLCSD 320-206379/3-A","537","RES","LLCSD 320-206379/3-A","TALSAC","1763-23-1","Perfluorooctanesulfonic
acid (PFOS),"37.6","ng/L","J M","6.8","DL","","SPK","94","7","40","LOQ","YES","40.0","LLCS 320-206379/2-
A","250.0","1.0","16",""
"LLCSD 320-206379/3-A","537","RES","LLCSD 320-206379/3-A","TALSAC","335-67-1","Perfluorooctanoic acid
(PFOA),"22.5","ng/L","","2.8","DL","","SPK","112","1","20","LOQ","YES","20.0","LLCS 320-206379/2-
A","250.0","1.0","8.0",""
"LLCSD 320-206379/3-A","537","RES","LLCSD 320-206379/3-A","TALSAC","355-46-4","Perfluorohexanesulfonic

acid (PFHxS)", "31.4", "ng/L", "", "5.5", "DL", "", "SPK", "105", "5", "30", "LOQ", "YES", "30.0", "LLCS 320-206379/2-A", "250.0", "1.0", "12", ""

"LLCSD 320-206379/3-A", "537", "RES", "LLCSD 320-206379/3-A", "TALSAC", "375-73-5", "Perfluorobutanesulfonic acid (PFBS)", "94.8", "ng/L", "", "16", "DL", "", "SPK", "105", "0.3", "90", "LOQ", "YES", "90.0", "LLCS 320-206379/2-A", "250.0", "1.0", "36", ""

"LLCSD 320-206379/3-A", "537", "RES", "LLCSD 320-206379/3-A", "TALSAC", "375-85-9", "Perfluoroheptanoic acid (PFHpA)", "11.4", "ng/L", "", "1.9", "DL", "", "SPK", "114", "1", "10", "LOQ", "YES", "10.0", "LLCS 320-206379/2-A", "250.0", "1.0", "4.0", ""

"LLCSD 320-206379/3-A", "537", "RES", "LLCSD 320-206379/3-A", "TALSAC", "375-95-1", "Perfluorononanoic acid (PFNA)", "22.2", "ng/L", "J", "8.0", "DL", "", "SPK", "111", "1", "24", "LOQ", "YES", "20.0", "LLCS 320-206379/2-A", "250.0", "1.0", "20", ""

"LLCSD 320-206379/3-A", "537", "RES", "LLCSD 320-206379/3-A", "TALSAC", "STL00993", "13C2 PFHxA", "43.6", "ng/L", "", "-99", "DL", "", "SURR", "109", "2", "-99", "LOQ", "YES", "40.0", "LLCS 320-206379/2-A", "250.0", "1.0", "0", ""

"LLCSD 320-206379/3-A", "537", "RES", "LLCSD 320-206379/3-A", "TALSAC", "STL00996", "13C2 PFDA", "41.4", "ng/L", "", "-99", "DL", "", "SURR", "104", "0.07", "-99", "LOQ", "YES", "40.0", "LLCS 320-206379/2-A", "250.0", "1.0", "0", ""

"MB 320-206379/1-A", "537", "RES", "MB 320-206379/1-A", "TALSAC", "1763-23-1", "Perfluorooctanesulfonic acid (PFOS)", "16", "ng/L", "U", "6.8", "DL", "", "TRG", "", "", "40", "LOQ", "YES", "-99", "", "250.0", "1.0", "16", ""

"MB 320-206379/1-A", "537", "RES", "MB 320-206379/1-A", "TALSAC", "335-67-1", "Perfluorooctanoic acid (PFOA)", "8.0", "ng/L", "U", "2.8", "DL", "", "TRG", "", "", "20", "LOQ", "YES", "-99", "", "250.0", "1.0", "8.0", ""

"MB 320-206379/1-A", "537", "RES", "MB 320-206379/1-A", "TALSAC", "355-46-4", "Perfluorohexanesulfonic acid (PFHxS)", "12", "ng/L", "U", "5.5", "DL", "", "TRG", "", "", "30", "LOQ", "YES", "-99", "", "250.0", "1.0", "12", ""

"MB 320-206379/1-A", "537", "RES", "MB 320-206379/1-A", "TALSAC", "375-73-5", "Perfluorobutanesulfonic acid (PFBS)", "36", "ng/L", "U", "16", "DL", "", "TRG", "", "", "90", "LOQ", "YES", "-99", "", "250.0", "1.0", "36", ""

"MB 320-206379/1-A", "537", "RES", "MB 320-206379/1-A", "TALSAC", "375-85-9", "Perfluoroheptanoic acid (PFHpA)", "4.0", "ng/L", "U", "1.9", "DL", "", "TRG", "", "", "10", "LOQ", "YES", "-99", "", "250.0", "1.0", "4.0", ""

"MB 320-206379/1-A", "537", "RES", "MB 320-206379/1-A", "TALSAC", "375-95-1", "Perfluorononanoic acid (PFNA)", "20", "ng/L", "U", "8.0", "DL", "", "TRG", "", "", "24", "LOQ", "YES", "-99", "", "250.0", "1.0", "20", ""

"MB 320-206379/1-A", "537", "RES", "MB 320-206379/1-A", "TALSAC", "STL00993", "13C2 PFHxA", "45.6", "ng/L", "", "-99", "DL", "", "SURR", "114", "", "-99", "LOQ", "YES", "40.0", "", "250.0", "1.0", "0", ""

"MB 320-206379/1-A", "537", "RES", "MB 320-206379/1-A", "TALSAC", "STL00996", "13C2 PFDA", "44.1", "ng/L", "", "-99", "DL", "", "SURR", "110", "", "-99", "LOQ", "YES", "40.0", "", "250.0", "1.0", "0", ""

"Unknown", "Unknown", "WGNA-011818-RW-3325", "01/18/2018 09:10", "AQ", "320-35207-1", "NM", "", "4.70", "537", "METHOD", "RES", "01/31/2018 12:34", "02/06/2018 18:47", "TALSAC", "COA", "WET", "NA", "1", "NA", "NA", "", "100", "320-206379", "320-206379", "NA", "320-207292", "320-35207-1", "01/19/2018 09:30", "01/22/2018 08:20", ""

"Unknown", "Unknown", "NAWC-011818-FRB-032", "01/18/2018 13:35", "AQ", "320-35207-10", "FB", "", "4.70", "537", "METHOD", "RES", "01/31/2018 12:34", "02/06/2018 19:38", "TALSAC", "COA", "WET", "NA", "1", "NA", "NA", "", "100", "320-206379", "320-206379", "NA", "320-207294", "320-35207-1", "01/19/2018 09:30", "01/22/2018 08:20", ""

"Unknown", "Unknown", "NAWC-011818-RW-038", "01/18/2018 14:10", "AQ", "320-35207-11", "NM", "", "4.70", "537", "METHOD", "RES", "01/31/2018 12:34", "02/06/2018 19:43", "TALSAC", "COA", "WET", "NA", "1", "NA", "NA", "", "100", "320-206379", "320-206379", "NA", "320-207294", "320-35207-1", "01/19/2018 09:30", "01/22/2018 08:20", ""

"Unknown", "Unknown", "NAWC-011818-FRB-038", "01/18/2018 14:05", "AQ", "320-35207-12", "FB", "", "4.70", "537", "METHOD", "RES", "01/31/2018 12:34", "02/06/2018 19:47", "TALSAC", "COA", "WET", "NA", "1", "NA", "NA", "", "100", "320-206379", "320-206379", "NA", "320-207294", "320-35207-1", "01/19/2018 09:30", "01/22/2018 08:20", ""

"Unknown", "Unknown", "WGNA-011818-FRB-3325", "01/18/2018 09:05", "AQ", "320-35207-2", "FB", "", "4.70", "537", "METHOD", "RES", "01/31/2018 12:34", "02/06/2018 18:51", "TALSAC", "COA", "WET", "NA", "1", "NA", "NA", "", "100", "320-206379", "320-206379", "NA", "320-207292", "320-35207-1", "01/19/2018 09:30", "01/22/2018 08:20", ""

"Unknown", "Unknown", "NAWC-011818-RW-316", "01/18/2018 10:10", "AQ", "320-35207-

3","NM","","4.70","537","METHOD","RES","01/31/2018 12:34","02/06/2018
18:56","TALSAC","COA","WET","NA","1","NA","NA","","100","320-206379","320-206379","NA","320-
207292","320-35207-1","01/19/2018 09:30","01/22/2018 08:20",""
"Unknown","Unknown","NAWC-011818-FRB-316","01/18/2018 10:05","AQ","320-35207-
4","FB","","4.70","537","METHOD","RES","01/31/2018 12:34","02/06/2018
19:01","TALSAC","COA","WET","NA","1","NA","NA","","100","320-206379","320-206379","NA","320-
207292","320-35207-1","01/19/2018 09:30","01/22/2018 08:20",""
"Unknown","Unknown","NAWC-011818-RW-260","01/18/2018 12:10","AQ","320-35207-
5","NM","","4.70","537","METHOD","RES","01/31/2018 12:34","02/06/2018
19:05","TALSAC","COA","WET","NA","1","NA","NA","","100","320-206379","320-206379","NA","320-
207292","320-35207-1","01/19/2018 09:30","01/22/2018 08:20",""
"Unknown","Unknown","NAWC-011818-FRB-260","01/18/2018 12:05","AQ","320-35207-
6","FB","","4.70","537","METHOD","RES","01/31/2018 12:34","02/06/2018
19:19","TALSAC","COA","WET","NA","1","NA","NA","","100","320-206379","320-206379","NA","320-
207294","320-35207-1","01/19/2018 09:30","01/22/2018 08:20",""
"Unknown","Unknown","NAWC-011818-RW-281","01/18/2018 13:10","AQ","320-35207-
7","NM","","4.70","537","METHOD","RES","01/31/2018 12:34","02/06/2018
19:24","TALSAC","COA","WET","NA","1","NA","NA","","100","320-206379","320-206379","NA","320-
207294","320-35207-1","01/19/2018 09:30","01/22/2018 08:20",""
"Unknown","Unknown","NAWC-011818-FRB-281","01/18/2018 13:05","AQ","320-35207-
8","FB","","4.70","537","METHOD","RES","01/31/2018 12:34","02/06/2018
19:29","TALSAC","COA","WET","NA","1","NA","NA","","100","320-206379","320-206379","NA","320-
207294","320-35207-1","01/19/2018 09:30","01/22/2018 08:20",""
"Unknown","Unknown","NAWC-011818-RW-032","01/18/2018 13:40","AQ","320-35207-
9","NM","","4.70","537","METHOD","RES","01/31/2018 12:34","02/06/2018
19:33","TALSAC","COA","WET","NA","1","NA","NA","","100","320-206379","320-206379","NA","320-
207294","320-35207-1","01/19/2018 09:30","01/22/2018 08:20",""
"Unknown","Unknown","LLCS 320-206379/2-A","","AQ","LLCS 320-206379/2-
A","LCS","","-99","537","METHOD","RES","01/31/2018 12:34","02/06/2018
18:37","TALSAC","COA","WET","NA","1","NA","NA","","100","320-206379","320-206379","NA","320-
207292","320-35207-1","01/31/2018 12:34","01/22/2018 08:20",""
"Unknown","Unknown","LLCSD 320-206379/3-A","","AQ","LLCSD 320-206379/3-
A","LCS","","-99","537","METHOD","RES","01/31/2018 12:34","02/06/2018
18:42","TALSAC","COA","WET","NA","1","NA","NA","","100","320-206379","320-206379","NA","320-
207292","320-35207-1","01/31/2018 12:34","01/22/2018 08:20",""
"Unknown","Unknown","MB 320-206379/1-A","","AQ","MB 320-206379/1-
A","MB","","-99","537","METHOD","RES","01/31/2018 12:34","02/06/2018
18:33","TALSAC","COA","WET","NA","1","NA","NA","","100","320-206379","320-206379","NA","320-
207292","320-35207-1","01/31/2018 12:34","01/22/2018 08:20",""



TO: A. FREBOWITZ **DATE:** FEBRUARY 14, 2018
FROM: TERRI L. SOLOMON **COPIES:** DV FILE
SUBJECT: ORGANIC DATA VALIDATION –POLYFLUOROALKYL SUBSTANCES (PFAS)
NAS JRB WILLOW GROVE
SAMPLE DELIVERY GROUP (SDG) 320-35207-1

SAMPLES: 6/Field Reagent Blank (FRB)
NAWC-011818-FRB-032 NAWC-011818-FRB-038
NAWC-011818-FRB-260 NAWC-011818-FRB-281
NAWC-011818-FRB-316 WGNA-011818-FRB-3325

6/Drinking Water
NAWC-011818-RW-032 NAWC-011818-RW-038
NAWC-011818-RW-260 NAWC-011818-RW-281
NAWC-011818-RW-316 WGNA-011818-RW-3325

Overview

The sample set for NAS JRB Willow Grove, SDG 320-35207-1, consisted of six (6) drinking water samples and six (6) FRB samples. All samples were analyzed for select perfluorinated alkyl acids including pentadecafluorooctanoic acid (PFOA), perfluorobutane sulfonic acid (PFBS), perfluoroheptanoic acid (PFHpA), perfluorohexanesulfonic acid (PFHxS), perfluorononanoic acid (PFNA) and perfluorooctane sulfonic acid (PFOS). No field duplicate sample pairs were included in this SDG.

The samples were collected by Tetra Tech on January 18, 2018 and analyzed by Test America-Sacramento. All sample analyses were conducted in accordance with EPA Method 537 version 1.1 analytical and reporting protocols.

The data contained in this SDG was validated with regard to the following parameters: data completeness, holding times, initial/continuing calibrations, laboratory method/FRBs, surrogate spike recoveries, laboratory control sample / laboratory control sample duplicate results, internal standard areas and recoveries, chromatographic resolution, analyte identification, analyte quantitation, and detection limits. Areas of concern are listed below.

Major

None.

Minor

Detected results reported below the limit of quantitation (LOQ) but above the detection limit (DL) were qualified as estimated, (J).

Notes

It was noted that sample WGNA-011818-RW-3325 had a pH of 9. No validation actions were required.

TO: A. FREBOWITZ
SDG: 320-35207-1

PAGE 2

Samples with detections and their associated FRBs are summarized below. No detected results were present in the FRBs.

<u>Sample</u>	<u>Associated FRB</u>
NAWC-011818-RW-032	NAWC-011818-RW-032
NAWC-011818-RW-038	NAWC-011818-RW-038
NAWC-011818-RW-260	NAWC-011818-RW-260
NAWC-011818-RW-281	NAWC-011818-RW-281
NAWC-011818-RW-316	NAWC-011818-RW-316
WGNA-011818-RW-3325	WGNA-011818-FRB-3325

Non-detected results were reported to the Limit of Detection (LOD).

The buffering agent Trizma was added to all drinking water samples.

Executive Summary


Laboratory Performance: No issues.

Other Factors Affecting Data Quality: Results below the RL were estimated.

The data for these analyses were reviewed with reference to the Environmental Protection Agency document EPA/600/R-08/092, Method 537, "Determination of Selected Perfluorinated Alkyl Acids in Drinking Water by Solid Phase Extraction and Liquid Chromatography/Tandem Mass Spectrometry (LC/MS/MS)", (September 2009) and the US EPA National Functional Guidelines for Organic Data Review (January 2017) as applicable. The text of this report has been formulated to address only those areas affecting data quality.



Tetra Tech, Inc.
Terri L. Solomon
Chemist/Data Validator



Tetra Tech, Inc.
Joseph A. Samchuck
Data Validation Manager

Attachments:

- Appendix A – Qualified Analytical Results
- Appendix B – Results as Reported by the Laboratory
- Appendix C – Support Documentation

Data Qualifier Definitions

The following definitions provide brief explanations of the validation qualifiers assigned to results in the data review process.

U	The analyte was analyzed for, but was not detected at a level greater than or equal to the level of the adjusted method detection limit for sample and method.
J	The analyte was positively identified and the associated numerical value is the approximate concentration of the analyte in the sample (due either to the quality of the data generated because certain quality control criteria were not met, or the concentration of the analyte was below the reporting limit).
J+	The result is an estimated quantity, but the result may be biased high.
J-	The result is an estimated quantity, but the result may be biased low.
UJ	The analyte was analyzed for, but was not detected. The reported detection limit is approximate and may be inaccurate or imprecise.
R	The sample result (detected) is unusable due to the quality of the data generated because certain criteria were not met. The analyte may or may not be present in the sample.
UR	The sample result (nondetected) is unusable due to the quality of the data generated because certain criteria were not met. The analyte may or may not be present in the sample.

Appendix A

Qualified Analytical Results

Qualifier Codes:

- A = Lab Blank Contamination
- B = Field Blank Contamination
- C = Calibration Noncompliance (i.e., % RSDs, %Ds, ICVs, CCVs, RRFs, etc.)
- C01 = GC/MS Tuning Noncompliance
- D = MS/MSD Recovery Noncompliance
- E = LCS/LCSD Recovery Noncompliance
- F = Lab Duplicate Imprecision
- G = Field Duplicate Imprecision
- H = Holding Time Exceedance
- I = ICP Serial Dilution Noncompliance
- J = ICP PDS Recovery Noncompliance; MSA's $r < 0.995$
- K = ICP Interference - includes ICS % R Noncompliance
- L = Instrument Calibration Range Exceedance
- M = Sample Preservation Noncompliance
- N = Internal Standard Noncompliance
- N01 = Internal Standard Recovery Noncompliance Dioxins
- N02 = Recovery Standard Noncompliance Dioxins
- N03 = Clean-up Standard Noncompliance Dioxins
- O = Poor Instrument Performance (i.e., base-time drifting)
- P = Uncertainty near detection limit ($< 2 \times$ IDL for inorganics and $<$ CRQL for organics)
- Q = Other problems (can encompass a number of issues; i.e.chromatography,interferences, etc.)
- R = Surrogates Recovery Noncompliance
- S = Pesticide/PCB Resolution
- T = % Breakdown Noncompliance for DDT and Endrin
- U = RPD between columns/detectors $>40\%$ for positive results determined via GC/HPLC
- V = Non-linear calibrations; correlation coefficient $r < 0.995$
- W = EMPC result
- X = Signal to noise response drop
- Y = Percent solids $<30\%$
- Z = Uncertainty at 2 standard deviations is greater than sample activity
- Z1 = Tentatively Identified Compound considered presumptively present
- Z2 = Tentatively Identified Compound column bleed
- Z3 = Tentatively Identified Compound aldol condensate
- Z4 = Sample activity is less than the at uncertainty at 3 standard deviations and greater than the MDC
- Z5 = Sample activity is less than the at uncertainty at 3 standard deviations and less than the MDC

PROJ_NO: 08005-WE04 SDG: 320-35207-1 FRACTION: PFAS MEDIA: WATER	NSAMPLE	NAWC-011818-FRB-032			NAWC-011818-FRB-038			NAWC-011818-FRB-260			NAWC-011818-FRB-281		
	LAB_ID	320-35207-10			320-35207-12			320-35207-6			320-35207-8		
	SAMP_DATE	1/18/2018			1/18/2018			1/18/2018			1/18/2018		
	QC_TYPE	FB			FB			FB			FB		
	UNITS	NG/L			NG/L			NG/L			NG/L		
	PCT_SOLIDS	0.0			0.0			0.0			0.0		
	DUP_OF												
PARAMETER	RESULT	VQL	QLCD	RESULT	VQL	QLCD	RESULT	VQL	QLCD	RESULT	VQL	QLCD	
PENTADECAFLUOROOCTANOIC ACID	8.2	U		8	U		8	U		8	U		
PERFLUOROBUTANESULFONIC ACID	37	U		36	U		36	U		36	U		
PERFLUOROHEPTANOIC ACID	4.1	U		4	U		4	U		4	U		
PERFLUOROHXANESULFONIC ACID	12	U		12	U		12	U		12	U		
PERFLUORONONANOIC ACID	20	U		20	U		20	U		20	U		
PERFLUOROOCTANE SULFONIC ACID	16	U		16	U		16	U		16	U		

PROJ_NO: 08005-WE04 SDG: 320-35207-1 FRACTION: PFAS MEDIA: WATER	NSAMPLE	NAWC-011818-FRB-316			NAWC-011818-RW-032			NAWC-011818-RW-038			NAWC-011818-RW-260		
	LAB_ID	320-35207-4			320-35207-9			320-35207-11			320-35207-5		
	SAMP_DATE	1/18/2018			1/18/2018			1/18/2018			1/18/2018		
	QC_TYPE	FB			NM			NM			NM		
	UNITS	NG/L			NG/L			NG/L			NG/L		
	PCT_SOLIDS	0.0			0.0			0.0			0.0		
	DUP_OF												
PARAMETER	RESULT	VQL	QLCD	RESULT	VQL	QLCD	RESULT	VQL	QLCD	RESULT	VQL	QLCD	
PENTADECAFLUOROOCTANOIC ACID	7.9	U		16	J	P	21			24			
PERFLUOROBUTANESULFONIC ACID	36	U		36	U		36	U		16	J	P	
PERFLUOROHEPTANOIC ACID	4	U		5.4	J	P	5.6	J	P	7	J	P	
PERFLUOROHXANESULFONIC ACID	12	U		14	J	P	6.2	J	P	8.6	J	P	
PERFLUORONONANOIC ACID	20	U		20	U		20	U		20	U		
PERFLUOROOCTANE SULFONIC ACID	16	U		20	J	P	25	J	P	23	J	P	

PROJ_NO: 08005-WE04 SDG: 320-35207-1 FRACTION: PFAS MEDIA: WATER	NSAMPLE	NAWC-011818-RW-281			NAWC-011818-RW-316			WGNA-011818-FRB-3325			WGNA-011818-RW-3325		
	LAB_ID	320-35207-7			320-35207-3			320-35207-2			320-35207-1		
	SAMP_DATE	1/18/2018			1/18/2018			1/18/2018			1/18/2018		
	QC_TYPE	NM			NM			FB			NM		
	UNITS	NG/L			NG/L			NG/L			NG/L		
	PCT_SOLIDS	0.0			0.0			0.0			0.0		
	DUP_OF												
PARAMETER	RESULT	VQL	QLCD	RESULT	VQL	QLCD	RESULT	VQL	QLCD	RESULT	VQL	QLCD	
PENTADECAFLUOROOCTANOIC ACID	15	J	P	24			7.9	U		14	J	P	
PERFLUOROBUTANESULFONIC ACID	36	U		36	U		36	U		36	U		
PERFLUOROHEPTANOIC ACID	4.4	J	P	9	J	P	4	U		4.2	J	P	
PERFLUOROHXANESULFONIC ACID	6.4	J	P	32			12	U		13	J	P	
PERFLUORONONANOIC ACID	20	U		20	U		20	U		20	U		
PERFLUOROOCTANE SULFONIC ACID	13	J	P	45			16	U		14	J	P	

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Client Sample ID: WGNA-011818-RW-3325 Lab Sample ID: 320-35207-1
 Matrix: Water Lab File ID: 2018.02.06_537XX_047.d
 Analysis Method: 537 Date Collected: 01/18/2018 09:10
 Extraction Method: 537 Date Extracted: 01/31/2018 12:34
 Sample wt/vol: 247.6(mL) Date Analyzed: 02/06/2018 18:47
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 207292 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	14	J M	40	16	6.9
335-67-1	Perfluorooctanoic acid (PFOA)	14	J	20	8.1	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U M	24	20	8.1
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	13	J	30	12	5.6
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.2	J	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	91	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	96		70-130
STL00996	13C2 PFDA	109		70-130

Steve L. Salzman
02/14/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Client Sample ID: WGNA-011818-FRB-3325 Lab Sample ID: 320-35207-2
 Matrix: Water Lab File ID: 2018.02.06_537XX_048.d
 Analysis Method: 537 Date Collected: 01/18/2018 09:05
 Extraction Method: 537 Date Extracted: 01/31/2018 12:34
 Sample wt/vol: 251.8(mL) Date Analyzed: 02/06/2018 18:51
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 207292 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	7.9	U	20	7.9	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	7.9
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.0	U	9.9	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	89	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	114		70-130
STL00996	13C2 PFDA	104		70-130

Mari L. Salaman

02/14/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Client Sample ID: NAWC-011818-RW-316 Lab Sample ID: 320-35207-3
 Matrix: Water Lab File ID: 2018.02.06_537XX_049.d
 Analysis Method: 537 Date Collected: 01/18/2018 10:10
 Extraction Method: 537 Date Extracted: 01/31/2018 12:34
 Sample wt/vol: 247.1(mL) Date Analyzed: 02/06/2018 18:56
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 207292 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	45	M	40	16	6.9
335-67-1	Perfluorooctanoic acid (PFOA)	24	M	20	8.1	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	8.1
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	32		30	12	5.6
375-85-9	Perfluoroheptanoic acid (PFHpA)	9.0	J	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	91	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	103		70-130
STL00996	13C2 PFDA	102		70-130

Ami L. Selman
02/14/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Client Sample ID: NAWC-011818-FRB-316 Lab Sample ID: 320-35207-4
 Matrix: Water Lab File ID: 2018.02.06_537XX_050.d
 Analysis Method: 537 Date Collected: 01/18/2018 10:05
 Extraction Method: 537 Date Extracted: 01/31/2018 12:34
 Sample wt/vol: 252.5 (mL) Date Analyzed: 02/06/2018 19:01
 Con. Extract Vol.: 1.0 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 207292 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	40	16	6.7
335-67-1	Perfluorooctanoic acid (PFOA)	7.9	U	20	7.9	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	7.9
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	30	12	5.4
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.0	U	9.9	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	89	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	109		70-130
STL00996	13C2 PFDA	100		70-130

Atqui L. Selman
02/14/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Client Sample ID: NAWC-011818-RW-260 Lab Sample ID: 320-35207-5
 Matrix: Water Lab File ID: 2018.02.06_537XX_051.d
 Analysis Method: 537 Date Collected: 01/18/2018 12:10
 Extraction Method: 537 Date Extracted: 01/31/2018 12:34
 Sample wt/vol: 244.2 (mL) Date Analyzed: 02/06/2018 19:05
 Con. Extract Vol.: 1.0 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 207292 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	23	J M	41	16	7.0
335-67-1	Perfluorooctanoic acid (PFOA)	24		20	8.2	2.9
375-95-1	Perfluorononanoic acid (PFNA)	20	U M	25	20	8.2
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	8.6	J	31	12	5.6
375-85-9	Perfluoroheptanoic acid (PFHpA)	7.0	J	10	4.1	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	16	J	92	37	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	104		70-130
STL00996	13C2 PFDA	105		70-130

Wesley L. Selman

02/14/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Client Sample ID: NAWC-011818-FRB-260 Lab Sample ID: 320-35207-6
 Matrix: Water Lab File ID: 2018.02.06_537XX_054.d
 Analysis Method: 537 Date Collected: 01/18/2018 12:05
 Extraction Method: 537 Date Extracted: 01/31/2018 12:34
 Sample wt/vol: 250.8(mL) Date Analyzed: 02/06/2018 19:19
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 207294 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	8.0	U	20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.0	U	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	104		70-130
STL00996	13C2 PFDA	102		70-130

Steve L. Selman
02/14/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Client Sample ID: NAWC-011818-RW-281 Lab Sample ID: 320-35207-7
 Matrix: Water Lab File ID: 2018.02.06_537XX_055.d
 Analysis Method: 537 Date Collected: 01/18/2018 13:10
 Extraction Method: 537 Date Extracted: 01/31/2018 12:34
 Sample wt/vol: 247.5 (mL) Date Analyzed: 02/06/2018 19:24
 Con. Extract Vol.: 1.0 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 207294 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	13	J M	40	16	6.9
335-67-1	Perfluorooctanoic acid (PFOA)	15	J	20	8.1	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	8.1
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	6.4	J	30	12	5.6
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.4	J	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	91	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	99		70-130
STL00996	13C2 PFDA	103		70-130

Ali L. Salaman
02/14/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Client Sample ID: NAWC-011818-FRB-281 Lab Sample ID: 320-35207-8
 Matrix: Water Lab File ID: 2018.02.06_537XX_056.d
 Analysis Method: 537 Date Collected: 01/18/2018 13:05
 Extraction Method: 537 Date Extracted: 01/31/2018 12:34
 Sample wt/vol: 249.6(mL) Date Analyzed: 02/06/2018 19:29
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 207294 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	8.0	U	20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.0	U	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	103		70-130
STL00996	13C2 PFDA	102		70-130

Ami L. Salmen

02/14/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Client Sample ID: NAWC-011818-RW-032 Lab Sample ID: 320-35207-9
 Matrix: Water Lab File ID: 2018.02.06_537XX_057.d
 Analysis Method: 537 Date Collected: 01/18/2018 13:40
 Extraction Method: 537 Date Extracted: 01/31/2018 12:34
 Sample wt/vol: 247.2 (mL) Date Analyzed: 02/06/2018 19:33
 Con. Extract Vol.: 1.0 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 207294 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	20	J M	40	16	6.9
335-67-1	Perfluorooctanoic acid (PFOA)	16	J	20	8.1	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	8.1
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	14	J	30	12	5.6
375-85-9	Perfluoroheptanoic acid (PFHpA)	5.4	J	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	91	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	88		70-130
STL00996	13C2 PFDA	104		70-130

Teri L. Selman
02/14/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Client Sample ID: NAWC-011818-FRB-032 Lab Sample ID: 320-35207-10
 Matrix: Water Lab File ID: 2018.02.06_537XX_058.d
 Analysis Method: 537 Date Collected: 01/18/2018 13:35
 Extraction Method: 537 Date Extracted: 01/31/2018 12:34
 Sample wt/vol: 244.2 (mL) Date Analyzed: 02/06/2018 19:38
 Con. Extract Vol.: 1.0 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 207294 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	41	16	7.0
335-67-1	Perfluorooctanoic acid (PFOA)	8.2	U	20	8.2	2.9
375-95-1	Perfluorononanoic acid (PFNA)	20	U	25	20	8.2
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	31	12	5.6
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.1	U	10	4.1	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	37	U	92	37	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	104		70-130
STL00996	13C2 PFDA	105		70-130

Wesley L. Selman

02/14/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Client Sample ID: NAWC-011818-RW-038 Lab Sample ID: 320-35207-11
 Matrix: Water Lab File ID: 2018.02.06_537XX_059.d
 Analysis Method: 537 Date Collected: 01/18/2018 14:10
 Extraction Method: 537 Date Extracted: 01/31/2018 12:34
 Sample wt/vol: 249.6(mL) Date Analyzed: 02/06/2018 19:43
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 207294 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	25	J M	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	21		20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	6.2	J	30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	5.6	J	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	90		70-130
STL00996	13C2 PFDA	97		70-130

Wesley L. Selmer

02/14/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Client Sample ID: NAWC-011818-FRB-038 Lab Sample ID: 320-35207-12
 Matrix: Water Lab File ID: 2018.02.06_537XX_060.d
 Analysis Method: 537 Date Collected: 01/18/2018 14:05
 Extraction Method: 537 Date Extracted: 01/31/2018 12:34
 Sample wt/vol: 249.7(mL) Date Analyzed: 02/06/2018 19:47
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 207294 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	8.0	U	20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.0	U	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	107		70-130
STL00996	13C2 PFDA	102		70-130

Wesley L. Selman

02/14/2018

Appendix B

Results as Reported by the Laboratory

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Client Sample ID: WGNA-011818-RW-3325 Lab Sample ID: 320-35207-1
 Matrix: Water Lab File ID: 2018.02.06_537XX_047.d
 Analysis Method: 537 Date Collected: 01/18/2018 09:10
 Extraction Method: 537 Date Extracted: 01/31/2018 12:34
 Sample wt/vol: 247.6(mL) Date Analyzed: 02/06/2018 18:47
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 207292 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	14	J M	40	16	6.9
335-67-1	Perfluorooctanoic acid (PFOA)	14	J	20	8.1	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U M	24	20	8.1
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	13	J	30	12	5.6
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.2	J	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	91	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	96		70-130
STL00996	13C2 PFDA	109		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Client Sample ID: WGNA-011818-FRB-3325 Lab Sample ID: 320-35207-2
 Matrix: Water Lab File ID: 2018.02.06_537XX_048.d
 Analysis Method: 537 Date Collected: 01/18/2018 09:05
 Extraction Method: 537 Date Extracted: 01/31/2018 12:34
 Sample wt/vol: 251.8(mL) Date Analyzed: 02/06/2018 18:51
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 207292 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	7.9	U	20	7.9	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	7.9
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.0	U	9.9	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	89	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	114		70-130
STL00996	13C2 PFDA	104		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Client Sample ID: NAWC-011818-RW-316 Lab Sample ID: 320-35207-3
 Matrix: Water Lab File ID: 2018.02.06_537XX_049.d
 Analysis Method: 537 Date Collected: 01/18/2018 10:10
 Extraction Method: 537 Date Extracted: 01/31/2018 12:34
 Sample wt/vol: 247.1(mL) Date Analyzed: 02/06/2018 18:56
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 207292 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	45	M	40	16	6.9
335-67-1	Perfluorooctanoic acid (PFOA)	24	M	20	8.1	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	8.1
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	32		30	12	5.6
375-85-9	Perfluoroheptanoic acid (PFHpA)	9.0	J	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	91	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	103		70-130
STL00996	13C2 PFDA	102		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Client Sample ID: NAWC-011818-FRB-316 Lab Sample ID: 320-35207-4
 Matrix: Water Lab File ID: 2018.02.06_537XX_050.d
 Analysis Method: 537 Date Collected: 01/18/2018 10:05
 Extraction Method: 537 Date Extracted: 01/31/2018 12:34
 Sample wt/vol: 252.5 (mL) Date Analyzed: 02/06/2018 19:01
 Con. Extract Vol.: 1.0 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 207292 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	40	16	6.7
335-67-1	Perfluorooctanoic acid (PFOA)	7.9	U	20	7.9	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	7.9
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	30	12	5.4
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.0	U	9.9	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	89	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	109		70-130
STL00996	13C2 PFDA	100		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Client Sample ID: NAWC-011818-RW-260 Lab Sample ID: 320-35207-5
 Matrix: Water Lab File ID: 2018.02.06_537XX_051.d
 Analysis Method: 537 Date Collected: 01/18/2018 12:10
 Extraction Method: 537 Date Extracted: 01/31/2018 12:34
 Sample wt/vol: 244.2 (mL) Date Analyzed: 02/06/2018 19:05
 Con. Extract Vol.: 1.0 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 207292 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	23	J M	41	16	7.0
335-67-1	Perfluorooctanoic acid (PFOA)	24		20	8.2	2.9
375-95-1	Perfluorononanoic acid (PFNA)	20	U M	25	20	8.2
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	8.6	J	31	12	5.6
375-85-9	Perfluoroheptanoic acid (PFHpA)	7.0	J	10	4.1	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	16	J	92	37	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	104		70-130
STL00996	13C2 PFDA	105		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Client Sample ID: NAWC-011818-FRB-260 Lab Sample ID: 320-35207-6
 Matrix: Water Lab File ID: 2018.02.06_537XX_054.d
 Analysis Method: 537 Date Collected: 01/18/2018 12:05
 Extraction Method: 537 Date Extracted: 01/31/2018 12:34
 Sample wt/vol: 250.8(mL) Date Analyzed: 02/06/2018 19:19
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 207294 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	8.0	U	20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.0	U	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	104		70-130
STL00996	13C2 PFDA	102		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Client Sample ID: NAWC-011818-RW-281 Lab Sample ID: 320-35207-7
 Matrix: Water Lab File ID: 2018.02.06_537XX_055.d
 Analysis Method: 537 Date Collected: 01/18/2018 13:10
 Extraction Method: 537 Date Extracted: 01/31/2018 12:34
 Sample wt/vol: 247.5 (mL) Date Analyzed: 02/06/2018 19:24
 Con. Extract Vol.: 1.0 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 207294 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	13	J M	40	16	6.9
335-67-1	Perfluorooctanoic acid (PFOA)	15	J	20	8.1	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	8.1
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	6.4	J	30	12	5.6
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.4	J	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	91	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	99		70-130
STL00996	13C2 PFDA	103		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Client Sample ID: NAWC-011818-FRB-281 Lab Sample ID: 320-35207-8
 Matrix: Water Lab File ID: 2018.02.06_537XX_056.d
 Analysis Method: 537 Date Collected: 01/18/2018 13:05
 Extraction Method: 537 Date Extracted: 01/31/2018 12:34
 Sample wt/vol: 249.6(mL) Date Analyzed: 02/06/2018 19:29
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 207294 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	8.0	U	20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.0	U	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	103		70-130
STL00996	13C2 PFDA	102		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Client Sample ID: NAWC-011818-RW-032 Lab Sample ID: 320-35207-9
 Matrix: Water Lab File ID: 2018.02.06_537XX_057.d
 Analysis Method: 537 Date Collected: 01/18/2018 13:40
 Extraction Method: 537 Date Extracted: 01/31/2018 12:34
 Sample wt/vol: 247.2 (mL) Date Analyzed: 02/06/2018 19:33
 Con. Extract Vol.: 1.0 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 207294 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	20	J M	40	16	6.9
335-67-1	Perfluorooctanoic acid (PFOA)	16	J	20	8.1	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	8.1
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	14	J	30	12	5.6
375-85-9	Perfluoroheptanoic acid (PFHpA)	5.4	J	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	91	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	88		70-130
STL00996	13C2 PFDA	104		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Client Sample ID: NAWC-011818-FRB-032 Lab Sample ID: 320-35207-10
 Matrix: Water Lab File ID: 2018.02.06_537XX_058.d
 Analysis Method: 537 Date Collected: 01/18/2018 13:35
 Extraction Method: 537 Date Extracted: 01/31/2018 12:34
 Sample wt/vol: 244.2 (mL) Date Analyzed: 02/06/2018 19:38
 Con. Extract Vol.: 1.0 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 207294 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	41	16	7.0
335-67-1	Perfluorooctanoic acid (PFOA)	8.2	U	20	8.2	2.9
375-95-1	Perfluorononanoic acid (PFNA)	20	U	25	20	8.2
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	31	12	5.6
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.1	U	10	4.1	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	37	U	92	37	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	104		70-130
STL00996	13C2 PFDA	105		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Client Sample ID: NAWC-011818-RW-038 Lab Sample ID: 320-35207-11
 Matrix: Water Lab File ID: 2018.02.06_537XX_059.d
 Analysis Method: 537 Date Collected: 01/18/2018 14:10
 Extraction Method: 537 Date Extracted: 01/31/2018 12:34
 Sample wt/vol: 249.6(mL) Date Analyzed: 02/06/2018 19:43
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 207294 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	25	J M	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	21		20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	6.2	J	30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	5.6	J	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	90		70-130
STL00996	13C2 PFDA	97		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Client Sample ID: NAWC-011818-FRB-038 Lab Sample ID: 320-35207-12
 Matrix: Water Lab File ID: 2018.02.06_537XX_060.d
 Analysis Method: 537 Date Collected: 01/18/2018 14:05
 Extraction Method: 537 Date Extracted: 01/31/2018 12:34
 Sample wt/vol: 249.7(mL) Date Analyzed: 02/06/2018 19:47
 Con. Extract Vol.: 1.0(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 207294 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	8.0	U	20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.0	U	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	107		70-130
STL00996	13C2 PFDA	102		70-130

Appendix C

Support Documentation

TestAmerica Sacramento
 880 Riverside Parkway
 West Sacramento, CA 95605-1500
 phone 916.373.5600 fax 303.467.7248

Chain of Custody Record

TestAmerica

THE LEADER IN ENVIRONMENTAL TESTING

TestAmerica Laboratories, Inc.

Regulatory Program: DW NPDES RCRA Other:

Client Contact		Project Manager: Andy Frebowitz		Site Contact: Mary Kay Bond		Date: 1/18/2018		COC No:	
TetraTech		Tel/Fax: 610.382.1170		Lab Contact: Dave Alltucker		Carrier: FedEx		1 of 1 COCs	
234 Mall Boulevard Suite 260		Analysis Turnaround Time		Filtered Sample (Y/N) Perform MS / MSD (Y/N) EPA 537 UCMR3				Sampler: Mary Kay Bond For Lab Use Only: Walk-in Client: <input type="checkbox"/> Lab Sampling: <input type="checkbox"/> Job / SDG No.: <input type="text"/> Sample Specific Notes:	
King of Prussia, PA 19406		<input type="checkbox"/> CALENDAR DAYS <input type="checkbox"/> WORKING DAYS TAT if different from Below 21							
610-382-1174		<input type="checkbox"/> 2 weeks							
610-491-9688		<input type="checkbox"/> 1 week							
Project Name: WE04		<input type="checkbox"/> 2 days							
Site: WE04		<input type="checkbox"/> 1 day							
P O # 1132358 (through EarthToxics)									
Sample Identification		Sample Date	Sample Time	Sample Type (C=Comp, G=Grab)	Matrix	# of Cont.	Filtered Sample (Y/N)	Perform MS / MSD (Y/N)	EPA 537 UCMR3
WGNA-011818-RW-3325		1/18/2018	09:10	G	DW	2	N	N	Y
WGNA-011818-FRB-3325		1/18/2018	09:05	G	DW	2	N	N	Y
NAWC-011818-RW-316		1/18/2018	10:10	G	DW	2	N	N	Y
NAWC-011818-FRB-316		1/18/2018	10:05	G	DW	2	N	N	Y
NAWC-011818-RW-260		1/18/2018	12:10	G	DW	2	N	N	Y
NAWC-011818-FRB-260		1/18/2018	12:05	G	DW	2	N	N	Y
NAWC-011818-RW-281		1/18/2018	13:10	G	DW	2	N	N	Y
NAWC-011818-FRB-281		1/18/2018	13:05	G	DW	2	N	N	Y
NAWC-011818-RW-032		1/18/2018	13:40	G	DW	2	N	N	Y
NAWC-011818-FRB-032		1/18/2018	13:35	G	DW	2	N	N	Y
NAWC-011818-RW-038		1/18/2018	14:10	G	DW	2	N	N	Y
NAWC-011818-FRB-038		1/18/2018	14:05	G	DW	2	N	N	Y
Preservation Used: 1= Ice, 2= HCl; 3= H2SO4; 4=HNO3; 5=NaOH; 6= Other: Trizma							6		
Possible Hazard Identification: Are any samples from a listed EPA Hazardous Waste? Please List any EPA Waste Codes for the sample in the							Sample Disposal (A fee may be assessed if samples are retained longer than 1 month)		
<input checked="" type="checkbox"/> Non-Hazard <input type="checkbox"/> Flammable <input type="checkbox"/> Skin Irritant <input type="checkbox"/> Poison B <input type="checkbox"/> Unknown							<input type="checkbox"/> Return to Client <input checked="" type="checkbox"/> Disposal by Lab <input type="checkbox"/> Archive for _____ Months		
Fed Ex Tracking: 7712 5015 1760									
Custody Seals Intact: <input type="checkbox"/> Yes <input type="checkbox"/> No		Custody Seal No.:		Cooler Temp. (°C): Obs'd: 4.7		Corr'd:		Therm ID No. AK3	
Relinquished by: <i>Mary Kay Bond</i>		Company: Tetra Tech		Date/Time: 1/18/2018 16:00		Received by: <i>M. S. H.</i>		Company: TA-Sac	
Relinquished by:		Company:		Date/Time:		Received by:		Date/Time: 1-19-18 9:30	
Relinquished by:		Company:		Date/Time:		Received in Laboratory by:		Date/Time:	

Page 300 of 301



320-35207 Chain of Custody

Job Narrative
320-35207-1

Receipt

The samples were received on 1/19/2018 9:30 AM; the samples arrived in good condition, properly preserved and, where required, on ice. The temperature of the cooler at receipt was 4.7° C.

LCMS

No analytical or quality issues were noted, other than those described in the Definitions/Glossary page.

Organic Prep

Method(s) 537: Insufficient sample volume was available to perform a matrix spike/matrix spike duplicate (MS/MSD) associated with preparation batch 320-206379

Method(s) 537: The following sample, WGNA-011818-RW-3325 (320-35207-1) in preparation batch 320-206379 had a received pH of 9.

No additional analytical or quality issues were noted, other than those described above or in the Definitions/Glossary page.

Sample Summary

Client: Tetra Tech, Inc.

TestAmerica Job ID: 320-35207-1

Project/Site: Warminster: PFAS, NAS JRB Willow Grove

Lab Sample ID	Client Sample ID	Matrix	Collected	Received
320-35207-1	WGNA-011818-RW-3325	Water	01/18/18 09:10	01/19/18 09:30
320-35207-2	WGNA-011818-FRB-3325	Water	01/18/18 09:05	01/19/18 09:30
320-35207-3	NAWC-011818-RW-316	Water	01/18/18 10:10	01/19/18 09:30
320-35207-4	NAWC-011818-FRB-316	Water	01/18/18 10:05	01/19/18 09:30
320-35207-5	NAWC-011818-RW-260	Water	01/18/18 12:10	01/19/18 09:30
320-35207-6	NAWC-011818-FRB-260	Water	01/18/18 12:05	01/19/18 09:30
320-35207-7	NAWC-011818-RW-281	Water	01/18/18 13:10	01/19/18 09:30
320-35207-8	NAWC-011818-FRB-281	Water	01/18/18 13:05	01/19/18 09:30
320-35207-9	NAWC-011818-RW-032	Water	01/18/18 13:40	01/19/18 09:30
320-35207-10	NAWC-011818-FRB-032	Water	01/18/18 13:35	01/19/18 09:30
320-35207-11	NAWC-011818-RW-038	Water	01/18/18 14:10	01/19/18 09:30
320-35207-12	NAWC-011818-FRB-038	Water	01/18/18 14:05	01/19/18 09:30

Method Summary

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-35207-1

Method	Method Description	Protocol	Laboratory
537	Perfluorinated Alkyl Acids (LC/MS)	EPA	TAL SAC

Protocol References:

EPA = US Environmental Protection Agency

Laboratory References:

TAL SAC = TestAmerica Sacramento, 880 Riverside Parkway, West Sacramento, CA 95605, TEL (916)373-5600

FORM II
LCMS SURROGATE RECOVERY

Lab Name: TestAmerica Sacramento

Job No.: 320-35207-1

SDG No.: _____

Matrix: Water

Level: Low

GC Column (1): GeminiC18 3 ID: 3 (mm)

Client Sample ID	Lab Sample ID	PFHxA #	PFDA #
WGNA-011818-RW-332 5	320-35207-1	96	109
WGNA-011818-FRB-33 25	320-35207-2	114	104
NAWC-011818-RW-316	320-35207-3	103	102
NAWC-011818-FRB-31 6	320-35207-4	109	100
NAWC-011818-RW-260	320-35207-5	104	105
NAWC-011818-FRB-26 0	320-35207-6	104	102
NAWC-011818-RW-281	320-35207-7	99	103
NAWC-011818-FRB-28 1	320-35207-8	103	102
NAWC-011818-RW-032	320-35207-9	88	104
NAWC-011818-FRB-03 2	320-35207-10	104	105
NAWC-011818-RW-038	320-35207-11	90	97
NAWC-011818-FRB-03 8	320-35207-12	107	102
	MB 320-206379/1-A	114	110
	LLCS 320-206379/2-A	106	104
	LLCSD 320-206379/3-A	109	104

PFHxA = 13C2 PFHxA
PFDA = 13C2 PFDA

QC LIMITS
70-130
70-130

Column to be used to flag recovery values

FORM III
LCMS LOW LEVEL CONTROL SAMPLE RECOVERY

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Matrix: Water Level: Low Lab File ID: 2018.02.06_537XX_045.d
 Lab ID: LLCS 320-206379/2-A Client ID: _____

COMPOUND	SPIKE ADDED (ng/L)	LLCS CONCENTRATION (ng/L)	LLCS % REC	QC LIMITS REC	#
Perfluorooctanesulfonic acid (PFOS)	40.0	40.2	100	50-150	M
Perfluorooctanoic acid (PFOA)	20.0	22.1	111	50-150	
Perfluorononanoic acid (PFNA)	20.0	21.9 J	110	50-150	
Perfluorohexanesulfonic acid (PFHxS)	30.0	33.0	110	50-150	
Perfluoroheptanoic acid (PFHpA)	10.0	11.6	116	50-150	
Perfluorobutanesulfonic acid (PFBS)	90.0	94.5	105	50-150	

Column to be used to flag recovery and RPD values

FORM III
LCMS LOW LEVEL CONTROL STANDARD DUPLICATE RECOVERY

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1

SDG No.: _____

Matrix: Water Level: Low Lab File ID: 2018.02.06_537XX_046.d

Lab ID: LLCSD 320-206379/3-A Client ID: _____

COMPOUND	SPIKE ADDED (ng/L)	LLCSD CONCENTRATION (ng/L)	LLCSD % REC	% RPD	QC LIMITS		#
					RPD	REC	
Perfluorooctanesulfonic acid (PFOS)	40.0	37.6 J	94	7	50	50-150	M
Perfluorooctanoic acid (PFOA)	20.0	22.5	112	1	50	50-150	
Perfluorononanoic acid (PFNA)	20.0	22.2 J	111	1	50	50-150	
Perfluorohexanesulfonic acid (PFHxS)	30.0	31.4	105	5	50	50-150	
Perfluoroheptanoic acid (PFHpA)	10.0	11.4	114	1	50	50-150	
Perfluorobutanesulfonic acid (PFBS)	90.0	94.8	105	0.3	50	50-150	

Column to be used to flag recovery and RPD values

FORM IV
LCMS METHOD BLANK SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Lab File ID: 2018.02.06_537XX_044.d Lab Sample ID: MB 320-206379/1-A
 Matrix: Water Date Extracted: 01/31/2018 12:34
 Instrument ID: A8_N Date Analyzed: 02/06/2018 18:33
 Level: (Low/Med) Low

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES:

CLIENT SAMPLE ID	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED
	LLCS 320-206379/2-A	2018.02.06_537XX_045.d	02/06/2018 18:37
	LLCSD 320-206379/3-A	2018.02.06_537XX_046.d	02/06/2018 18:42
WGNA-011818-RW-3325	320-35207-1	2018.02.06_537XX_047.d	02/06/2018 18:47
WGNA-011818-FRB-3325	320-35207-2	2018.02.06_537XX_048.d	02/06/2018 18:51
NAWC-011818-RW-316	320-35207-3	2018.02.06_537XX_049.d	02/06/2018 18:56
NAWC-011818-FRB-316	320-35207-4	2018.02.06_537XX_050.d	02/06/2018 19:01
NAWC-011818-RW-260	320-35207-5	2018.02.06_537XX_051.d	02/06/2018 19:05
NAWC-011818-FRB-260	320-35207-6	2018.02.06_537XX_054.d	02/06/2018 19:19
NAWC-011818-RW-281	320-35207-7	2018.02.06_537XX_055.d	02/06/2018 19:24
NAWC-011818-FRB-281	320-35207-8	2018.02.06_537XX_056.d	02/06/2018 19:29
NAWC-011818-RW-032	320-35207-9	2018.02.06_537XX_057.d	02/06/2018 19:33
NAWC-011818-FRB-032	320-35207-10	2018.02.06_537XX_058.d	02/06/2018 19:38
NAWC-011818-RW-038	320-35207-11	2018.02.06_537XX_059.d	02/06/2018 19:43
NAWC-011818-FRB-038	320-35207-12	2018.02.06_537XX_060.d	02/06/2018 19:47

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Client Sample ID: _____ Lab Sample ID: MB 320-206379/1-A
 Matrix: Water Lab File ID: 2018.02.06_537XX_044.d
 Analysis Method: 537 Date Collected: _____
 Extraction Method: 537 Date Extracted: 01/31/2018 12:34
 Sample wt/vol: 250.0 (mL) Date Analyzed: 02/06/2018 18:33
 Con. Extract Vol.: 1.0 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 207292 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	8.0	U	20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.0	U	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	114		70-130
STL00996	13C2 PFDA	110		70-130

FORM VIII
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Instrument ID: A8_N Calibration Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3(mm) Calibration End Date: 11/03/2017 14:01
 Calibration ID: 36012

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
INITIAL CALIBRATION MEAN AREA AND MEAN RT	1535518	1.91	3276559	2.15		
UPPER LIMIT	2303277	2.41	4914839	2.65		
LOWER LIMIT	767759	1.41	1638280	1.65		
LAB SAMPLE ID	CLIENT SAMPLE ID					
CCVL 320-192908/11		1586829	1.91	3305852	2.15	
ICV 320-192908/13		1512045	1.90	3433628	2.14	
CCVL 320-207097/1		1375995	1.81	3051061	2.05	
CCV 320-207292/1 CCVIS		1328760	1.81	3042209	2.05	
MB 320-206379/1-A		1243942	1.80	2945240	2.05	
LLCS 320-206379/2-A		1313107	1.81	3024316	2.05	
LLCSD 320-206379/3-A		1273817	1.80	3050466	2.05	
320-35207-1	WGNA-011818-RW-3325	1281071	1.80	2980694	2.05	
320-35207-2	WGNA-011818-FRB-3325	1232911	1.80	3018263	2.04	
320-35207-3	NAWC-011818-RW-316	1338968	1.80	2966673	2.04	
320-35207-4	NAWC-011818-FRB-316	1244262	1.80	3004650	2.05	
320-35207-5	NAWC-011818-RW-260	1302427	1.81	3143419	2.05	
CCV 320-207292/11 CCVIS		1315133	1.80	3035313	2.04	
CCV 320-207294/11 CCVIS		1315133	1.80	3035313	2.04	
320-35207-6	NAWC-011818-FRB-260	1299420	1.80	3069150	2.05	
320-35207-7	NAWC-011818-RW-281	1354367	1.81	3207550	2.05	
320-35207-8	NAWC-011818-FRB-281	1354309	1.81	3260304	2.05	
320-35207-9	NAWC-011818-RW-032	1279796	1.81	3134922	2.05	
320-35207-10	NAWC-011818-FRB-032	1269005	1.80	3041394	2.04	
320-35207-11	NAWC-011818-RW-038	1373697	1.79	3369231	2.04	
320-35207-12	NAWC-011818-FRB-038	1356647	1.80	3181172	2.04	
CCV 320-207294/20 CCVIS		1309862	1.79	3183039	2.04	

13PFOA = 13C2-PFOA
 PFOS = 13C4 PFOS

Area Limit = 50%-150% of internal standard area
 RT Limit = ± 0.5 minutes of internal standard RT

Column used to flag values outside QC limits

FORM VIII
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Sample No.: CCV 320-207292/1 Date Analyzed: 02/06/2018 18:23
 Instrument ID: A8_N GC Column: GeminiC18 3x100 ID: 3 (mm)
 Lab File ID (Standard): 2018.02.06_537XX_04 Heated Purge: (Y/N) N
 Calibration ID: 36012

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	1328760	1.81	3042209	2.05		
UPPER LIMIT	1860264	2.31	4259093	2.55		
LOWER LIMIT	930132	1.31	2129546	1.55		
LAB SAMPLE ID	CLIENT SAMPLE ID					
MB 320-206379/1-A		1243942	1.80	2945240	2.05	
LLCS 320-206379/2-A		1313107	1.81	3024316	2.05	
LLCSD 320-206379/3-A		1273817	1.80	3050466	2.05	
320-35207-1	WGNA-011818-RW-3325	1281071	1.80	2980694	2.05	
320-35207-2	WGNA-011818-FRB-3325	1232911	1.80	3018263	2.04	
320-35207-3	NAWC-011818-RW-316	1338968	1.80	2966673	2.04	
320-35207-4	NAWC-011818-FRB-316	1244262	1.80	3004650	2.05	
320-35207-5	NAWC-011818-RW-260	1302427	1.81	3143419	2.05	

13PFOA = 13C2-PFOA

PFOS = 13C4 PFOS

Area Limit = 70%-140% of internal standard area
 RT Limit = ± 0.5 minutes of internal standard RT

Column used to flag values outside QC limits

FORM VIII
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Sample No.: CCV 320-207292/11 Date Analyzed: 02/06/2018 19:10
 Instrument ID: A8_N GC Column: GeminiC18 3x100 ID: 3 (mm)
 Lab File ID (Standard): 2018.02.06_537XX_05 Heated Purge: (Y/N) N
 Calibration ID: 36012

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	1315133	1.80	3035313	2.04		
UPPER LIMIT	1841186	2.30	4249438	2.54		
LOWER LIMIT	920593	1.30	2124719	1.54		
LAB SAMPLE ID	CLIENT SAMPLE ID					
MB 320-206379/1-A		1243942	1.80	2945240	2.05	
LLCS 320-206379/2-A		1313107	1.81	3024316	2.05	
LLCSD 320-206379/3-A		1273817	1.80	3050466	2.05	
320-35207-1	WGNA-011818-RW-3325	1281071	1.80	2980694	2.05	
320-35207-2	WGNA-011818-FRB-3325	1232911	1.80	3018263	2.04	
320-35207-3	NAWC-011818-RW-316	1338968	1.80	2966673	2.04	
320-35207-4	NAWC-011818-FRB-316	1244262	1.80	3004650	2.05	
320-35207-5	NAWC-011818-RW-260	1302427	1.81	3143419	2.05	

13PFOA = 13C2-PFOA
 PFOS = 13C4 PFOS

Area Limit = 70%-140% of internal standard area
 RT Limit = ± 0.5 minutes of internal standard RT

Column used to flag values outside QC limits

FORM VIII
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Sample No.: CCV 320-207294/11 Date Analyzed: 02/06/2018 19:10
 Instrument ID: A8_N GC Column: GeminiC18 3x100 ID: 3 (mm)
 Lab File ID (Standard): 2018.02.06_537XX_05 Heated Purge: (Y/N) N
 Calibration ID: 36012

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	1315133	1.80	3035313	2.04		
UPPER LIMIT	1841186	2.30	4249438	2.54		
LOWER LIMIT	920593	1.30	2124719	1.54		
LAB SAMPLE ID	CLIENT SAMPLE ID					
320-35207-6	NAWC-011818-FRB-260	1299420	1.80	3069150	2.05	
320-35207-7	NAWC-011818-RW-281	1354367	1.81	3207550	2.05	
320-35207-8	NAWC-011818-FRB-281	1354309	1.81	3260304	2.05	
320-35207-9	NAWC-011818-RW-032	1279796	1.81	3134922	2.05	
320-35207-10	NAWC-011818-FRB-032	1269005	1.80	3041394	2.04	
320-35207-11	NAWC-011818-RW-038	1373697	1.79	3369231	2.04	
320-35207-12	NAWC-011818-FRB-038	1356647	1.80	3181172	2.04	

13PFOA = 13C2-PFOA
 PFOS = 13C4 PFOS

Area Limit = 70%-140% of internal standard area
 RT Limit = ± 0.5 minutes of internal standard RT

Column used to flag values outside QC limits

FORM VIII
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Sample No.: CCV 320-207294/20 Date Analyzed: 02/06/2018 19:52
 Instrument ID: A8_N GC Column: GeminiC18 3x100 ID: 3 (mm)
 Lab File ID (Standard): 2018.02.06_537XX_06 Heated Purge: (Y/N) N
 Calibration ID: 36012

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	1309862	1.79	3183039	2.04		
UPPER LIMIT	1833807	2.29	4456255	2.54		
LOWER LIMIT	916903	1.29	2228127	1.54		
LAB SAMPLE ID	CLIENT SAMPLE ID					
320-35207-6	NAWC-011818-FRB-260	1299420	1.80	3069150	2.05	
320-35207-7	NAWC-011818-RW-281	1354367	1.81	3207550	2.05	
320-35207-8	NAWC-011818-FRB-281	1354309	1.81	3260304	2.05	
320-35207-9	NAWC-011818-RW-032	1279796	1.81	3134922	2.05	
320-35207-10	NAWC-011818-FRB-032	1269005	1.80	3041394	2.04	
320-35207-11	NAWC-011818-RW-038	1373697	1.79	3369231	2.04	
320-35207-12	NAWC-011818-FRB-038	1356647	1.80	3181172	2.04	

13PFOA = 13C2-PFOA
 PFOS = 13C4 PFOS

Area Limit = 70%-140% of internal standard area
 RT Limit = ± 0.5 minutes of internal standard RT

Column used to flag values outside QC limits

FORM VI
LCMS BY INTERNAL STANDARD - INITIAL CALIBRATION DATA
CURVE EVALUATION

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1 Analy Batch No.: 192908

SDG No.: _____

Instrument ID: A8_N GC Column: GeminiC18 3 ID: 3(mm) Heated Purge: (Y/N) N

Calibration Start Date: 11/03/2017 13:37 Calibration End Date: 11/03/2017 14:01 Calibration ID: 36012

Calibration Files:

LEVEL:	LAB SAMPLE ID:	LAB FILE ID:
Level 1	IC 320-192908/4	2017.11.03_537XICAL_004.d
Level 2	IC 320-192908/5	2017.11.03_537XICAL_005.d
Level 3	IC 320-192908/6	2017.11.03_537XICAL_006.d
Level 4	IC 320-192908/7	2017.11.03_537XICAL_007.d
Level 5	IC 320-192908/8	2017.11.03_537XICAL_008.d
Level 6	IC 320-192908/9	2017.11.03_537XICAL_009.d

ANALYTE	RRF					CURVE TYPE	COEFFICIENT			#	MIN RRF	%RSD	#	MAX %RSD	R ² OR COD	#	MIN R ² OR COD
	LVL 1 LVL 6	LVL 2	LVL 3	LVL 4	LVL 5		B	M1	M2								
Perfluorobutanesulfonic acid (PFBS)	1.0397 0.8468	1.0767	1.0898	0.9577	0.9303	QuaF		1.1193	-0.001498					0.9990			0.9600
Perfluoroheptanoic acid (PFHpA)	0.9433 0.9848	0.9187	0.9551	0.9185	0.9011	Ave		0.9369			3.2		30.0				
Perfluorohexanesulfonic acid (PFHxS)	1.6459 1.6841	1.6355	1.7405	1.6631	1.6755	Ave		1.6741			2.2		30.0				
Perfluorooctanoic acid (PFOA)	0.9757 0.9799	0.8919	0.9000	0.8953	0.9117	Ave		0.9258			4.4		30.0				
Perfluorooctanesulfonic acid (PFOS)	0.8958 0.9902	0.9213	0.9281	0.9268	0.9715	Ave		0.9389			3.7		30.0				
Perfluorononanoic acid (PFNA)	0.6610 0.7042	0.6285	0.6624	0.6810	0.6478	Ave		0.6642			3.9		30.0				
13C2 PFHxA	1.0891 1.1664	1.0526	1.1042	1.1123	1.0772	Ave		1.1003			3.5		30.0				
13C2 PFDA	0.7748 0.8159	0.7295	0.7569	0.7811	0.7330	Ave		0.7652			4.3		30.0				

Note: The M1 coefficient is the same as Ave RRF for an Ave curve type.

FORM VI
LCMS BY INTERNAL STANDARD - INITIAL CALIBRATION DATA
RESPONSE AND CONCENTRATION

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1 Analy Batch No.: 192908

SDG No.: _____

Instrument ID: A8_N GC Column: GeminiC18 3 ID: 3(mm) Heated Purge: (Y/N) N

Calibration Start Date: 11/03/2017 13:37 Calibration End Date: 11/03/2017 14:01 Calibration ID: 36012

Calibration Files:

LEVEL:	LAB SAMPLE ID:	LAB FILE ID:
Level 1	IC 320-192908/4	2017.11.03_537XICAL_004.d
Level 2	IC 320-192908/5	2017.11.03_537XICAL_005.d
Level 3	IC 320-192908/6	2017.11.03_537XICAL_006.d
Level 4	IC 320-192908/7	2017.11.03_537XICAL_007.d
Level 5	IC 320-192908/8	2017.11.03_537XICAL_008.d
Level 6	IC 320-192908/9	2017.11.03_537XICAL_009.d

ANALYTE	IS REF	CURVE TYPE	RESPONSE					CONCENTRATION (NG/ML)				
			LVL 1 LVL 6	LVL 2	LVL 3	LVL 4	LVL 5	LVL 1 LVL 6	LVL 2	LVL 3	LVL 4	LVL 5
Perfluorobutanesulfonic acid (PFBS)	PFOS	QuaF	1076553 16699152	2591121	5461974	10142530	14011858	9.00 180	20.0	45.0	90.0	135
Perfluoroheptanoic acid (PFHpA)	13PF OA	Ave	143455 2810797	331548	736034	1420703	2102676	1.00 20.0	2.22	5.00	10.0	15.0
Perfluorohexanesulfonic acid (PFHxS)	PFOS	Ave	568156 11071993	1312135	2908204	5871843	8413133	3.00 60.0	6.67	15.0	30.0	45.0
Perfluorooctanoic acid (PFOA)	13PF OA	Ave	296934 5597122	644149	1388033	2771271	4257225	2.00 40.0	4.45	10.0	20.0	30.0
Perfluorooctanesulfonic acid (PFOS)	PFOS	Ave	412315 8679676	985487	2067792	4363079	6504279	4.00 80.0	8.89	20.0	40.0	60.0
Perfluorononanoic acid (PFNA)	13PF OA	Ave	201053 4019666	453612	1020851	2106479	3023088	2.00 40.0	4.45	10.0	20.0	30.0
13C2 PFHxA	13PF OA	Ave	1655691 1664260	1708988	1701491	1719911	1675220	10.0 10.0	10.0	10.0	10.0	10.0
13C2 PFDA	13PF OA	Ave	1177922 1164156	1184358	1166275	1207887	1139992	10.0 10.0	10.0	10.0	10.0	10.0

Curve Type Legend:

Ave = Average ISTD
QuaF = Quadratic ISTD forced zero

FORM VI
 LCMS BY INTERNAL STANDARD - INITIAL CALIBRATION DATA
 READBACK PERCENT ERROR

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1 Analy Batch No.: 192908

SDG No.: _____


Instrument ID: A8_N GC Column: GeminiC18 3 ID: 3 (mm) Heated Purge: (Y/N) N


Calibration Start Date: 11/03/2017 13:37 Calibration End Date: 11/03/2017 14:01 Calibration ID: 36012

Calibration Files:

LEVEL:	LAB SAMPLE ID:	LAB FILE ID:
Level 1	IC 320-192908/4	2017.11.03_537XICAL_004.d
Level 2	IC 320-192908/5	2017.11.03_537XICAL_005.d
Level 3	IC 320-192908/6	2017.11.03_537XICAL_006.d
Level 4	IC 320-192908/7	2017.11.03_537XICAL_007.d
Level 5	IC 320-192908/8	2017.11.03_537XICAL_008.d
Level 6	IC 320-192908/9	2017.11.03_537XICAL_009.d

ANALYTE	PERCENT ERROR						PERCENT ERROR LIMIT					
	LVL 1 #	LVL 2 #	LVL 3 #	LVL 4 #	LVL 5 #	LVL 6 #	LVL 1	LVL 2	LVL 3	LVL 4	LVL 5	LVL 6
Perfluorobutanesulfonic acid (PFBS)	-6.0	-1.2	3.9	-3.1	1.9	-0.5	50	30	30	30	30	30
Perfluoroheptanoic acid (PFHpA)	0.7	-1.9	1.9	-2.0	-3.8	5.1	50	30	30	30	30	30
Perfluorohexanesulfonic acid (PFHxS)	-1.7	-2.3	4.0	-0.7	0.1	0.6	50	30	30	30	30	30
Perfluorooctanoic acid (PFOA)	5.4	-3.7	-2.8	-3.3	-1.5	5.8	50	30	30	30	30	30
Perfluorooctanesulfonic acid (PFOS)	-4.6	-1.9	-1.2	-1.3	3.5	5.5	50	30	30	30	30	30
Perfluorononanoic acid (PFNA)	-0.5	-5.4	-0.3	2.5	-2.5	6.0	50	30	30	30	30	30
13C2 PFHxA	-1.0	-4.3	0.4	1.1	-2.1	6.0	30	30	30	30	30	30
13C2 PFDA	1.3	-4.7	-1.1	2.1	-4.2	6.6	30	30	30	30	30	30





FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Lab Sample ID: CCVL 320-192908/11 Calibration Date: 11/03/2017 14:10
 Instrument ID: A8_N Calib Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 11/03/2017 14:01
 Lab File ID: 2017.11.03_537XICAL_011.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		1.109		20.4	20.0	1.9	50.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9369	0.9382		2.23	2.22	0.1	50.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.674	1.688		6.72	6.67	0.8	50.0
Perfluorooctanoic acid (PFOA)	Ave	0.9258	0.8825		4.24	4.45	-4.7	50.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9389	0.9176		8.69	8.89	-2.3	50.0
Perfluorononanoic acid (PFNA)	Ave	0.6642	0.6625		4.43	4.45	-0.2	50.0
13C2 PFHxA	Ave	1.100	1.068		9.70	10.0	-3.0	30.0
13C2 PFDA	Ave	0.7652	0.7460		9.75	10.0	-2.5	30.0

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Lab Sample ID: ICV 320-192908/13 Calibration Date: 11/03/2017 14:20
 Instrument ID: A8_N Calib Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 11/03/2017 14:01
 Lab File ID: 2017.11.03_537XICAL_013.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		0.8310		83.7	100	-16.4	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9369	0.8136		8.68	10.0	-13.2	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.674	1.463		17.5	20.1	-12.6	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9258	0.7995		17.7	20.5	-13.6	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9389	0.8637		18.1	19.7	-8.0	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6642	0.6428		19.5	20.1	-3.2	30.0
13C2 PFHxA	Ave	1.100	1.039		9.44	10.0	-5.6	30.0
13C2 PFDA	Ave	0.7652	0.7391		9.66	10.0	-3.4	30.0

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Lab Sample ID: CCVL 320-207097/1 Calibration Date: 02/06/2018 08:30
 Instrument ID: A8_N Calib Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 11/03/2017 14:01
 Lab File ID: 2018.02.06_537A_003.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		1.081		19.8	20.0	-0.8	50.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.674	1.648		6.56	6.67	-1.6	50.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9369	1.009		2.39	2.22	7.7	50.0
Perfluorooctanoic acid (PFOA)	Ave	0.9258	0.9155		4.42	4.47	-1.1	50.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9389	0.9828		9.34	8.93	4.7	50.0
Perfluorononanoic acid (PFNA)	Ave	0.6642	0.6745		4.52	4.45	1.6	50.0
13C2 PFHxA	Ave	1.100	1.102		10.0	10.0	0.1	30.0
13C2 PFDA	Ave	0.7652	0.7044		9.21	10.0	-7.9	30.0

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Lab Sample ID: CCV 320-207292/1 Calibration Date: 02/06/2018 18:23
 Instrument ID: A8_N Calib Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 11/03/2017 14:01
 Lab File ID: 2018.02.06_537XX_042.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		1.104		47.4	45.0	5.3	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.674	1.740		15.6	15.0	3.9	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9369	1.029		5.49	5.00	9.9	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9258	0.9634		10.5	10.1	4.1	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9389	0.9893		21.2	20.1	5.4	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6642	0.6984		10.5	10.0	5.2	30.0
13C2 PFHxA	Ave	1.100	1.120		10.2	10.0	1.8	30.0
13C2 PFDA	Ave	0.7652	0.7367		9.63	10.0	-3.7	30.0

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Lab Sample ID: CCV 320-207292/11 Calibration Date: 02/06/2018 19:10
 Instrument ID: A8_N Calib Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 11/03/2017 14:01
 Lab File ID: 2018.02.06_537XX_052.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		0.9406		139	135	3.3	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.674	1.695		45.6	45.0	1.2	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9369	1.045		16.7	15.0	11.6	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9258	1.007		32.8	30.2	8.8	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9389	1.007		64.6	60.3	7.2	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6642	0.7206		32.6	30.0	8.5	30.0
13C2 PFHxA	Ave	1.100	1.089		9.90	10.0	-1.0	30.0
13C2 PFDA	Ave	0.7652	0.7564		9.89	10.0	-1.1	30.0

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Lab Sample ID: CCV 320-207294/11 Calibration Date: 02/06/2018 19:10
 Instrument ID: A8_N Calib Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 11/03/2017 14:01
 Lab File ID: 2018.02.06_537XX_052.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		0.9406		139	135	3.3	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.674	1.695		45.6	45.0	1.2	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9369	1.045		16.7	15.0	11.6	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9258	1.007		32.8	30.2	8.8	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9389	1.007		64.6	60.3	7.2	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6642	0.7206		32.6	30.0	8.5	30.0
13C2 PFHxA	Ave	1.100	1.089		9.90	10.0	-1.0	30.0
13C2 PFDA	Ave	0.7652	0.7564		9.89	10.0	-1.1	30.0

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1
 SDG No.: _____
 Lab Sample ID: CCV 320-207294/20 Calibration Date: 02/06/2018 19:52
 Instrument ID: A8_N Calib Start Date: 11/03/2017 13:37
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 11/03/2017 14:01
 Lab File ID: 2018.02.06_537XX_061.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	QuaF		1.043		44.6	45.0	-0.9	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	0.9369	1.064		5.68	5.00	13.6	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.674	1.627		14.6	15.0	-2.8	30.0
Perfluorooctanoic acid (PFOA)	Ave	0.9258	0.9471		10.3	10.1	2.3	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	0.9389	0.9332		20.0	20.1	-0.6	30.0
Perfluorononanoic acid (PFNA)	Ave	0.6642	0.7112		10.7	10.0	7.1	30.0
13C2 PFHxA	Ave	1.100	1.131		10.3	10.0	2.8	30.0
13C2 PFDA	Ave	0.7652	0.7430		9.71	10.0	-2.9	30.0

LCMS ANALYSIS RUN LOG

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1

SDG No.: _____

Instrument ID: A8_N Start Date: 11/03/2017 13:37

Analysis Batch Number: 192908 End Date: 11/03/2017 14:24

LAB SAMPLE ID	CLIENT SAMPLE ID	DATE ANALYZED	DILUTION FACTOR	LAB FILE ID	COLUMN ID
IC 320-192908/4		11/03/2017 13:37	1	2017.11.03_537X ICAL 004.d	GeminiC18 3x100 3(mm)
IC 320-192908/5		11/03/2017 13:42	1	2017.11.03_537X ICAL 005.d	GeminiC18 3x100 3(mm)
IC 320-192908/6		11/03/2017 13:47	1	2017.11.03_537X ICAL 006.d	GeminiC18 3x100 3(mm)
IC 320-192908/7 ICISAV		11/03/2017 13:52	1	2017.11.03_537X ICAL 007.d	GeminiC18 3x100 3(mm)
IC 320-192908/8		11/03/2017 13:56	1	2017.11.03_537X ICAL 008.d	GeminiC18 3x100 3(mm)
IC 320-192908/9		11/03/2017 14:01	1	2017.11.03_537X ICAL 009.d	GeminiC18 3x100 3(mm)
ZZZZZ		11/03/2017 14:06	1		GeminiC18 3x100 3(mm)
CCVL 320-192908/11		11/03/2017 14:10	1	2017.11.03_537X ICAL 011.d	GeminiC18 3x100 3(mm)
ZZZZZ		11/03/2017 14:15	1		GeminiC18 3x100 3(mm)
ICV 320-192908/13		11/03/2017 14:20	1	2017.11.03_537X ICAL 013.d	GeminiC18 3x100 3(mm)
ZZZZZ		11/03/2017 14:24	1		GeminiC18 3x100 3(mm)

LCMS ANALYSIS RUN LOG

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1

SDG No.: _____

Instrument ID: A8_N Start Date: 02/06/2018 08:30

Analysis Batch Number: 207097 End Date: 02/06/2018 09:31

LAB SAMPLE ID	CLIENT SAMPLE ID	DATE ANALYZED	DILUTION FACTOR	LAB FILE ID	COLUMN ID
CCVL 320-207097/1		02/06/2018 08:30	1	2018.02.06_537A 003.d	GeminiC18 3x100 3(mm)
CCV 320-207097/2 CCVIS		02/06/2018 08:35	1		GeminiC18 3x100 3(mm)
ZZZZZ		02/06/2018 08:44	1		GeminiC18 3x100 3(mm)
ZZZZZ		02/06/2018 08:49	1		GeminiC18 3x100 3(mm)
ZZZZZ		02/06/2018 08:54	1		GeminiC18 3x100 3(mm)
ZZZZZ		02/06/2018 08:58	1		GeminiC18 3x100 3(mm)
ZZZZZ		02/06/2018 09:03	1		GeminiC18 3x100 3(mm)
ZZZZZ		02/06/2018 09:08	1		GeminiC18 3x100 3(mm)
ZZZZZ		02/06/2018 09:12	1		GeminiC18 3x100 3(mm)
ZZZZZ		02/06/2018 09:17	1		GeminiC18 3x100 3(mm)
ZZZZZ		02/06/2018 09:22	1		GeminiC18 3x100 3(mm)
ZZZZZ		02/06/2018 09:26	1		GeminiC18 3x100 3(mm)
CCV 320-207097/14 CCVIS		02/06/2018 09:31	1		GeminiC18 3x100 3(mm)

LCMS ANALYSIS RUN LOG

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1

SDG No.: _____

Instrument ID: A8_N Start Date: 02/06/2018 18:23

Analysis Batch Number: 207292 End Date: 02/06/2018 19:10

LAB SAMPLE ID	CLIENT SAMPLE ID	DATE ANALYZED	DILUTION FACTOR	LAB FILE ID	COLUMN ID
CCV 320-207292/1 CCVIS		02/06/2018 18:23	1	2018.02.06_537X X 042.d	GeminiC18 3x100 3(mm)
MB 320-206379/1-A		02/06/2018 18:33	1	2018.02.06_537X X 044.d	GeminiC18 3x100 3(mm)
LLCS 320-206379/2-A		02/06/2018 18:37	1	2018.02.06_537X X 045.d	GeminiC18 3x100 3(mm)
LLCSD 320-206379/3-A		02/06/2018 18:42	1	2018.02.06_537X X 046.d	GeminiC18 3x100 3(mm)
320-35207-1		02/06/2018 18:47	1	2018.02.06_537X X 047.d	GeminiC18 3x100 3(mm)
320-35207-2		02/06/2018 18:51	1	2018.02.06_537X X 048.d	GeminiC18 3x100 3(mm)
320-35207-3		02/06/2018 18:56	1	2018.02.06_537X X 049.d	GeminiC18 3x100 3(mm)
320-35207-4		02/06/2018 19:01	1	2018.02.06_537X X 050.d	GeminiC18 3x100 3(mm)
320-35207-5		02/06/2018 19:05	1	2018.02.06_537X X 051.d	GeminiC18 3x100 3(mm)
CCV 320-207292/11 CCVIS		02/06/2018 19:10	1	2018.02.06_537X X 052.d	GeminiC18 3x100 3(mm)

LCMS ANALYSIS RUN LOG

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1

SDG No.: _____

Instrument ID: A8_N Start Date: 02/06/2018 19:10

Analysis Batch Number: 207294 End Date: 02/06/2018 19:52

LAB SAMPLE ID	CLIENT SAMPLE ID	DATE ANALYZED	DILUTION FACTOR	LAB FILE ID	COLUMN ID
CCV 320-207294/11 CCVIS		02/06/2018 19:10	1	2018.02.06_537X X 052.d	GeminiC18 3x100 3(mm)
320-35207-6		02/06/2018 19:19	1	2018.02.06_537X X 054.d	GeminiC18 3x100 3(mm)
320-35207-7		02/06/2018 19:24	1	2018.02.06_537X X 055.d	GeminiC18 3x100 3(mm)
320-35207-8		02/06/2018 19:29	1	2018.02.06_537X X 056.d	GeminiC18 3x100 3(mm)
320-35207-9		02/06/2018 19:33	1	2018.02.06_537X X 057.d	GeminiC18 3x100 3(mm)
320-35207-10		02/06/2018 19:38	1	2018.02.06_537X X 058.d	GeminiC18 3x100 3(mm)
320-35207-11		02/06/2018 19:43	1	2018.02.06_537X X 059.d	GeminiC18 3x100 3(mm)
320-35207-12		02/06/2018 19:47	1	2018.02.06_537X X 060.d	GeminiC18 3x100 3(mm)
CCV 320-207294/20 CCVIS		02/06/2018 19:52	1	2018.02.06_537X X 061.d	GeminiC18 3x100 3(mm)

LCMS BATCH WORKSHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1

SDG No.: _____

Batch Number: 206379 Batch Start Date: 01/31/18 12:29 Batch Analyst: Kolstad, Kate M

Batch Method: 537 Batch End Date: 02/02/18 17:10

Lab Sample ID	Client Sample ID	Method Chain	Basis	GrossWeight	TareWeight	InitialAmount	FinalAmount	ReceivedpH	LC537-IS 00057
MB 320-206379/1		537, 537				250.0 mL	1.0 mL	7 SU	100 uL
LLCS 320-206379/2		537, 537				250.0 mL	1.0 mL	7 SU	100 uL
LLCSD 320-206379/3		537, 537				250.0 mL	1.0 mL	7 SU	100 uL
320-35207-A-1	WGNA-011818-RW-3 325	537, 537	T	276.06 g	28.47 g	247.6 mL	1.0 mL	9 SU	100 uL
320-35207-A-2	WGNA-011818-FRB- 3325	537, 537	T	278.93 g	27.10 g	251.8 mL	1.0 mL	7 SU	100 uL
320-35207-A-3	NAWC-011818-RW-3 16	537, 537	T	275.06 g	28.01 g	247.1 mL	1.0 mL	7 SU	100 uL
320-35207-A-4	NAWC-011818-FRB- 316	537, 537	T	279.13 g	26.64 g	252.5 mL	1.0 mL	7 SU	100 uL
320-35207-A-5	NAWC-011818-RW-2 60	537, 537	T	272.51 g	28.36 g	244.2 mL	1.0 mL	7 SU	100 uL
320-35207-A-6	NAWC-011818-FRB- 260	537, 537	T	277.53 g	26.70 g	250.8 mL	1.0 mL	7 SU	100 uL
320-35207-A-7	NAWC-011818-RW-2 81	537, 537	T	274.54 g	27.09 g	247.5 mL	1.0 mL	7 SU	100 uL
320-35207-A-8	NAWC-011818-FRB- 281	537, 537	T	276.86 g	27.25 g	249.6 mL	1.0 mL	7 SU	100 uL
320-35207-A-9	NAWC-011818-RW-0 32	537, 537	T	275.67 g	28.44 g	247.2 mL	1.0 mL	7 SU	100 uL
320-35207-A-10	NAWC-011818-FRB- 032	537, 537	T	271.39 g	27.23 g	244.2 mL	1.0 mL	7 SU	100 uL
320-35207-A-11	NAWC-011818-RW-0 38	537, 537	T	278.52 g	28.97 g	249.6 mL	1.0 mL	7 SU	100 uL
320-35207-A-12	NAWC-011818-FRB- 038	537, 537	T	276.83 g	27.18 g	249.7 mL	1.0 mL	7 SU	100 uL

Lab Sample ID	Client Sample ID	Method Chain	Basis	LC537-LSP 00026	LC537-SU 00053	AnalysisComment			
MB 320-206379/1		537, 537			100 uL	C1 ND			
LLCS 320-206379/2		537, 537		100 uL	100 uL	C1 ND			
LLCSD 320-206379/3		537, 537		100 uL	100 uL	C1 ND			
320-35207-A-1	WGNA-011818-RW-3 325	537, 537	T		100 uL	C1 ND			
320-35207-A-2	WGNA-011818-FRB- 3325	537, 537	T		100 uL	C1 ND			

The pound sign (#) in the amount added field denotes that the reagent was used undiluted. All calculations are performed using the stated concentration for this reagent.

LCMS BATCH WORKSHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1

SDG No.: _____

Batch Number: 206379 Batch Start Date: 01/31/18 12:29 Batch Analyst: Kolstad, Kate M

Batch Method: 537 Batch End Date: 02/02/18 17:10

Lab Sample ID	Client Sample ID	Method Chain	Basis	LC537-LSP 00026	LC537-SU 00053	AnalysisComment			
320-35207-A-3	NAWC-011818-RW-316	537, 537	T		100 uL	C1 ND			
320-35207-A-4	NAWC-011818-FRB-316	537, 537	T		100 uL	C1 ND			
320-35207-A-5	NAWC-011818-RW-260	537, 537	T		100 uL	C1 ND			
320-35207-A-6	NAWC-011818-FRB-260	537, 537	T		100 uL	C1 ND			
320-35207-A-7	NAWC-011818-RW-281	537, 537	T		100 uL	C1 ND			
320-35207-A-8	NAWC-011818-FRB-281	537, 537	T		100 uL	C1 ND			
320-35207-A-9	NAWC-011818-RW-032	537, 537	T		100 uL	C1 ND			
320-35207-A-10	NAWC-011818-FRB-032	537, 537	T		100 uL	C1 ND			
320-35207-A-11	NAWC-011818-RW-038	537, 537	T		100 uL	C1 ND			
320-35207-A-12	NAWC-011818-FRB-038	537, 537	T		100 uL	C1 ND			

The pound sign (#) in the amount added field denotes that the reagent was used undiluted. All calculations are performed using the stated concentration for this reagent.

LCMS BATCH WORKSHEET

Lab Name: TestAmerica Sacramento Job No.: 320-35207-1

SDG No.: _____

Batch Number: 206379 Batch Start Date: 01/31/18 12:29 Batch Analyst: Kolstad, Kate M

Batch Method: 537 Batch End Date: 02/02/18 17:10

Batch Notes	
Analyst ID - Aliquot Step	VPM
Batch Comment	Client labels match: KMK 1-30-18
Analyst ID - Concentration	CCB
Analyst ID - Final Volume Step	CCB
Internal Standard ID#	1145836
Manifold ID	3, 10
Methanol ID	1137492
pH Indicator ID	2517
Pipette ID	H14930F
Analyst ID - IS Reagent Drop	CCB
Analyst ID - IS Reagent Drop Witness	TWL
Analyst ID - SU Reagent Drop	CCB
Analyst ID - SU Reagent Drop Witness	KMK
Analyst ID - TA Reagent Drop	CCB
Analyst ID - TA Reagent Drop Witness	KMK
SPE Cartridge ID	6369499-04
Trizma ID	SLBR4303V
Reagent Water ID	1-30-18

Basis	Basis Description
T	Total/NA

The pound sign (#) in the amount added field denotes that the reagent was used undiluted. All calculations are performed using the stated concentration for this reagent.

Aqueous Extraction Analysis Sheet

(To Accompany Samples to Instruments)

Batch Number: 320-206379

Analyst: Kolstad, Kate M

Batch Open: 1/31/2018 12:29:00PM

Method Code: 320-537_Prep-320

Batch End: 2/2/2018 5:10:00PM

69

KB 2/5/18

Extraction of Perfluorinated Alkyl Acids

Due: 2/19

Input Sample Lab ID (Analytical Method)	SDG (Job #)	GrossWt TareWt	InitAmnt FinAmnt	Rcvd	PHs Adj1 Adj2	Due Date	Analytical TAT	Div Rank	Comments	Output Sample Lab ID
1 MB-320-206379/1 N/A	N/A		250.0 mL	7		N/A	N/A	N/A	CI ND	
			1.0 mL							
2 LLCS-320-206379/2 N/A	N/A		250.0 mL	7		N/A	N/A	N/A	CI ND	
			1.0 mL							
3 LLCSD-320-206379/3 N/A	N/A		250.0 mL	7		N/A	N/A	N/A	CI ND	
			1.0 mL							
4 320-35207-A-1 (537_DOD5)	N/A (320-35207-1)	276.06 g	247.6 mL	9		1/23/18	16_Days	4	CI ND	
		28.47 g	1.0 mL							
5 320-35207-A-2 (537_DOD5)	N/A (320-35207-1)	278.93 g	251.8 mL	7		1/23/18	16_Days	4	CI ND	
		27.10 g	1.0 mL							
6 320-35207-A-3 (537_DOD5)	N/A (320-35207-1)	275.06 g	247.1 mL	7		1/23/18	16_Days	4	CI ND	
		28.01 g	1.0 mL							
7 320-35207-A-4 (537_DOD5)	N/A (320-35207-1)	279.13 g	252.5 mL	7		1/23/18	16_Days	4	CI ND	
		26.64 g	1.0 mL							
8 320-35207-A-5 (537_DOD5)	N/A (320-35207-1)	272.51 g	244.2 mL	7		1/23/18	16_Days	4	CI ND	
		28.36 g	1.0 mL							
9 320-35207-A-6 (537_DOD5)	N/A (320-35207-1)	277.53 g	250.8 mL	7		1/23/18	16_Days	4	CI ND	
		26.70 g	1.0 mL							
10 320-35207-A-7 (537_DOD5)	N/A (320-35207-1)	274.54 g	247.5 mL	7		1/23/18	16_Days	4	CI ND	
		27.09 g	1.0 mL							

Page 292 of 301

Aqueous Extraction Analysis Sheet

(To Accompany Samples to Instruments)






Batch Number: 320-206379

Analyst: Kolstad, Kate M

Batch Open: 1/31/2018 12:29:00PM

Method Code: 320-537_Prep-320

Batch End: 2/2/2018 5:10:00PM

11	320-35207-A-8 (537_DOD5)	N/A (320-35207-1)	276.86 g	249.6 mL	7			1/23/18	16_Days	4	CI ND	
			27.25 g	1.0 mL								
12	320-35207-A-9 (537_DOD5)	N/A (320-35207-1)	275.67 g	247.2 mL	7			1/23/18	16_Days	4	CI ND	
			28.44 g	1.0 mL								
13	320-35207-A-10 (537_DOD5)	N/A (320-35207-1)	271.39 g	244.2 mL	7			1/23/18	16_Days	4	CI ND	
			27.23 g	1.0 mL								
14	320-35207-A-11 (537_DOD5)	N/A (320-35207-1)	278.52 g	249.6 mL	7			1/23/18	16_Days	4	CI ND	
			28.97 g	1.0 mL								
15	320-35207-A-12 (537_DOD5)	N/A (320-35207-1)	276.83 g	249.7 mL	7			1/23/18	16_Days	4	CI ND	
			27.18 g	1.0 mL								

Page 293 of 301

Aqueous Extraction Analysis Sheet

(To Accompany Samples to Instruments)

Batch Number: 320-206379

Analyst: Kolstad, Kate M

Batch Open: 1/31/2018 12:29:00PM

Method Code: 320-537_Prep-320

Batch End: 2/2/2018 5:10:00PM

Batch Notes

Manifold ID 3, 10

pH Indicator ID 2517

Trizma ID SLBR4303V

SPE Cartridge ID 6369499-04

Methanol ID 1137492

Reagent Water ID 1-30-18

Internal Standard ID# 1145836

Pipette ID H14930F

Analyst ID - TA Reagent Drop CCB

Analyst ID - TA Reagent Drop KMK

Witness

Analyst ID - SU Reagent Drop CCB

Analyst ID - SU Reagent Drop KMK

Witness

Analyst ID - IS Reagent Drop CCB

Analyst ID - IS Reagent Drop TWL

Witness

Analyst ID - Concentration CCB

Analyst ID - Aliquot Step VPM

Analyst ID - Final Volume Step CCB

Batch Comment Client labels match: KMK 1-30-18

Page 294 of 301

PFAS Calibration Calculations:

Initial Calibration 11/3/2017
 Instrument A8_N

PFOA

Analyte Concentration	Analyte Response	Internal Standard Response	Internal Standard Amount	RRF	Reported RRF
2	296934	1520258	10	0.97659	0.9757
4.45	644149	1623614	10	0.89155	0.8919
10	1388033	1540946	10	0.90077	0.9
20	2771271	1546307	10	0.89609	0.8953
30	4257225	1555174	10	0.91249	0.9117
40	5597122	1426806	10	0.98071	0.9799
Average				0.92637	0.9258
Standard Deviation				0.0411	
RSD				0.0444	
%RSD				4.43838	4.4

Continuing Calibration 02/06/2018 @ 18:23

PFOA

Analyte Concentration	Analyte Response	Internal Standard Response	Internal Standard Amount	RRF	%D	Reported RRF	Reported %D
10	1287144	1328760	10	0.9687	4.0613523	0.9634	4.1

Willow Grove
SDG 320-35207-1

Sample Identification

WGNA-011818-RW-3325

Compound

PFOA

Compound Area

419465

Internal Standard Amount (ng)

10

Dilution Factor

1

Internal Standard Area

1281071

Average RRF

0.9258

Sample Volume(L)

0.2476

Volume Extract (ml)

1


Injection Volume (µl)

1

Concentration

14.2842 ng/L

C:\AI\Projects\112008005\WE04\F.S.DR.03\NAWC_201901.mxd MKB 1/24/2019

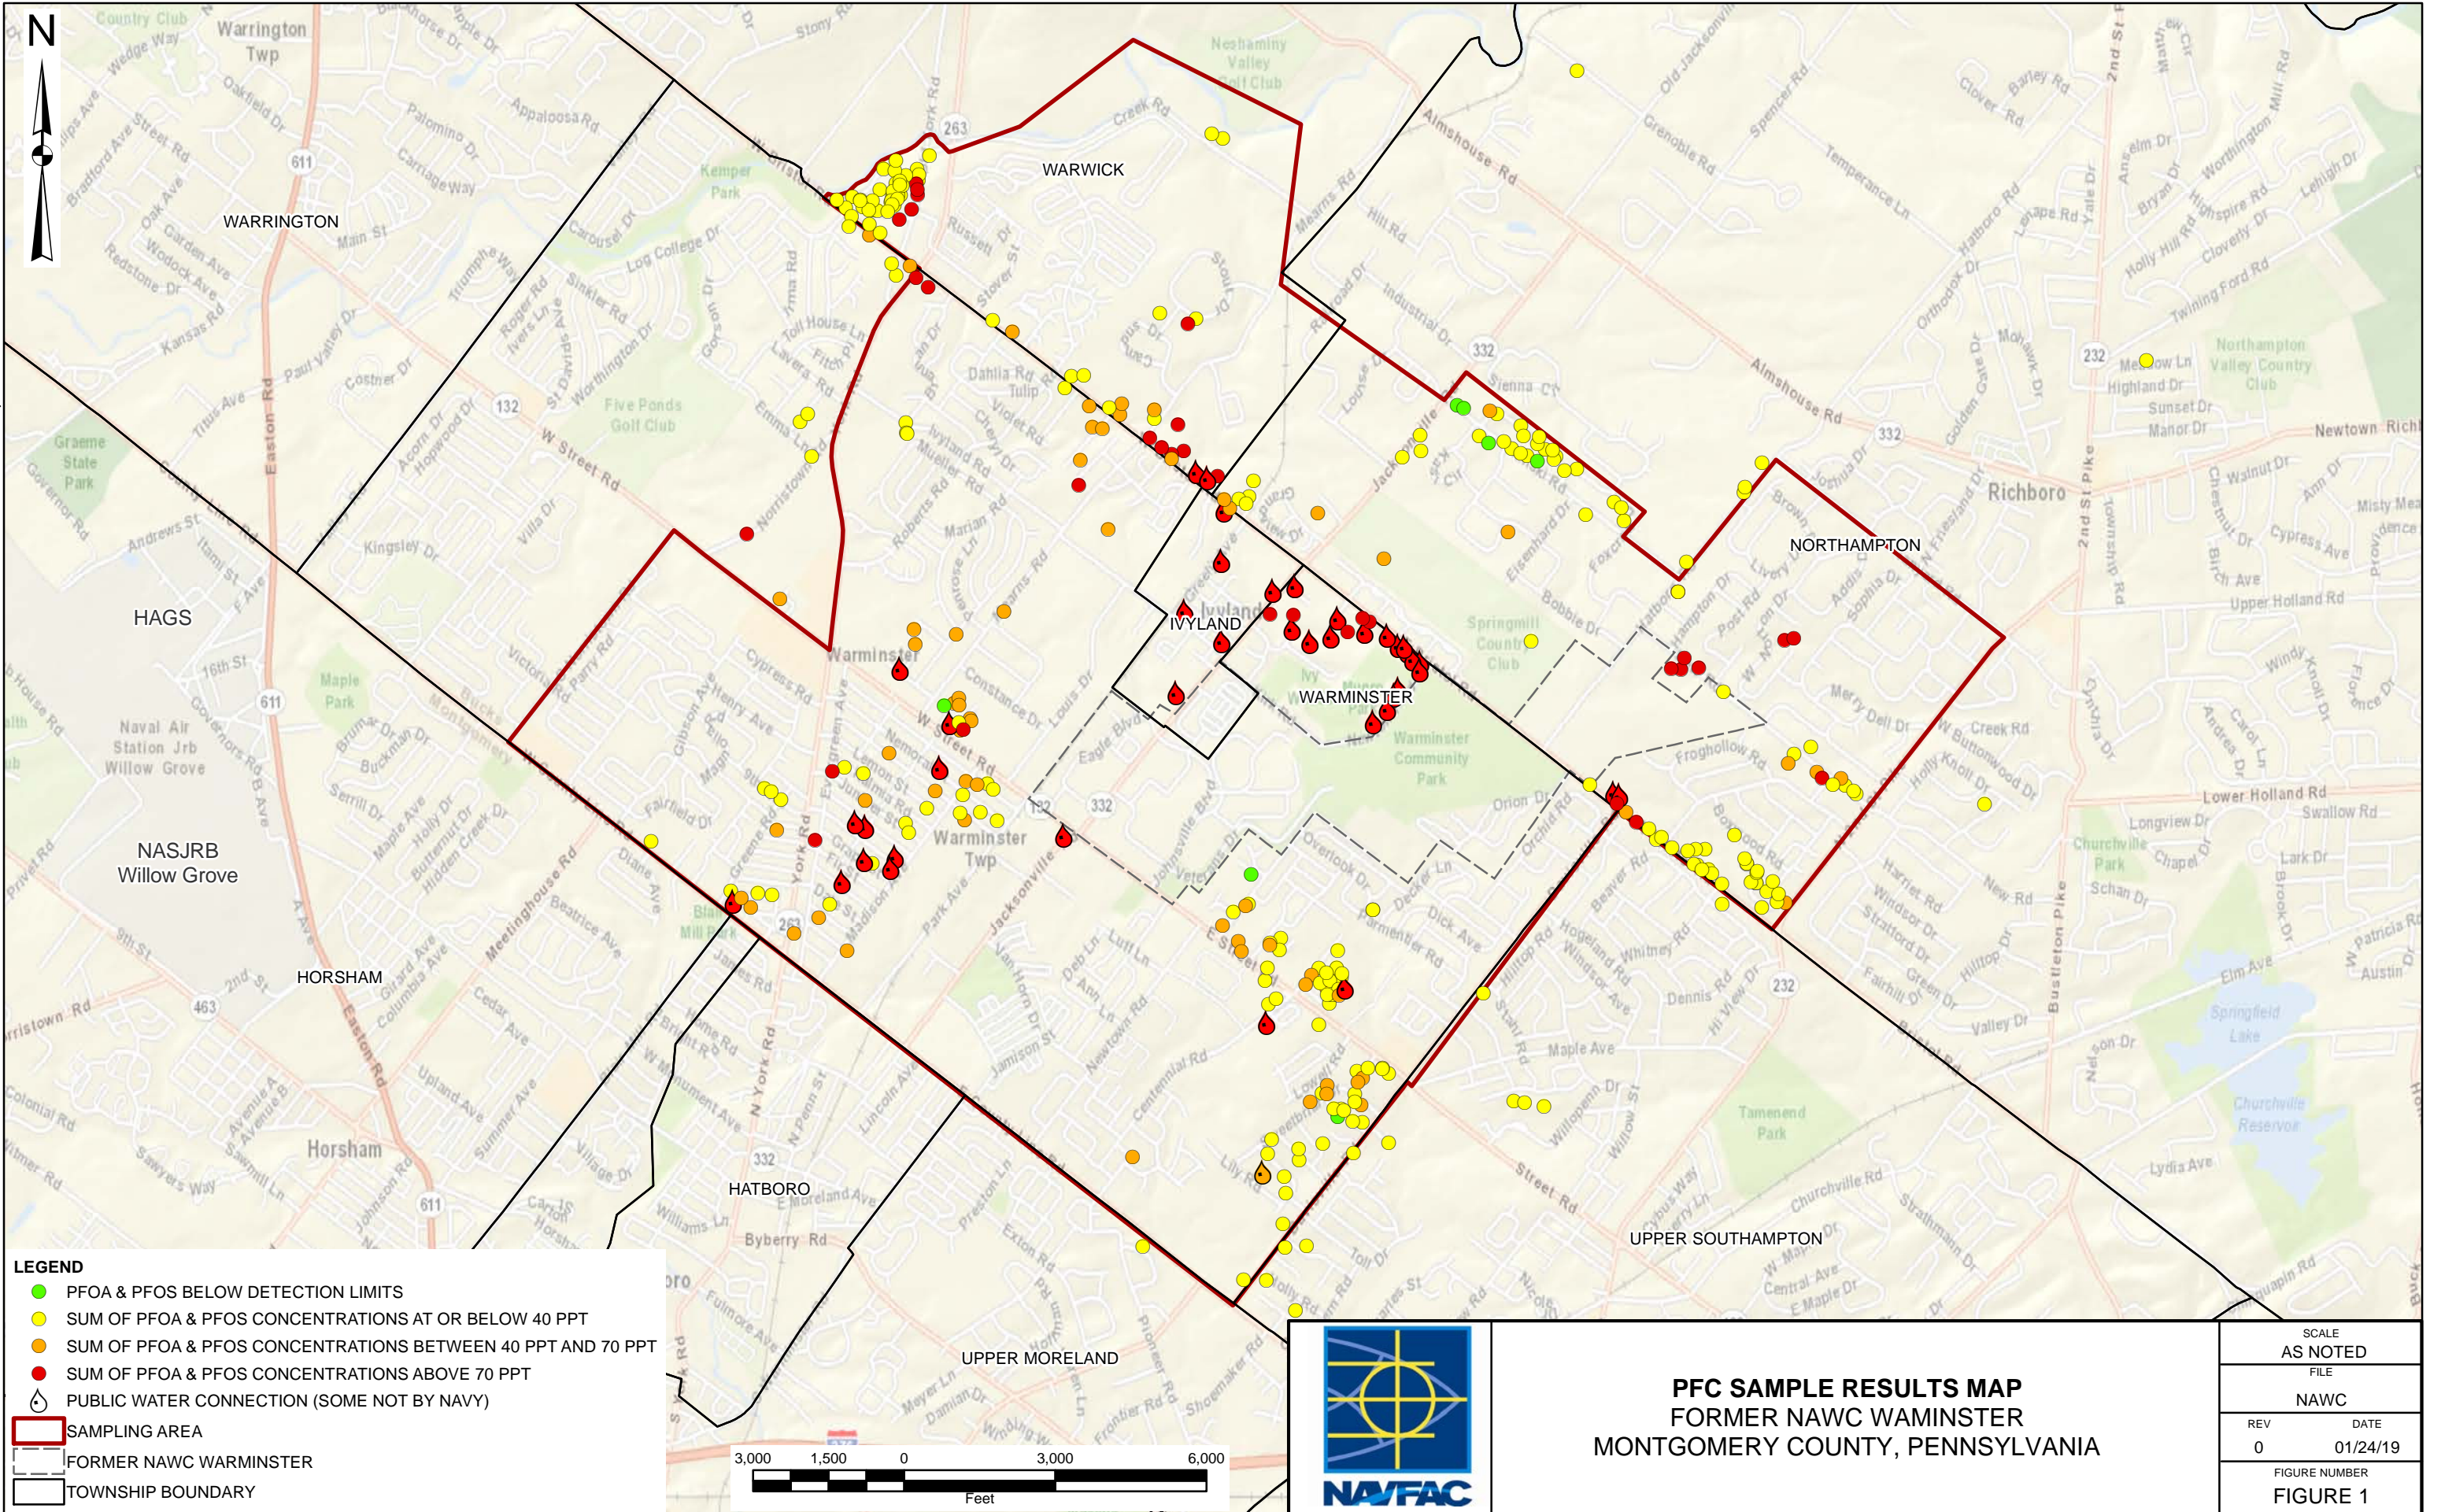

LEGEND

- PFOA & PFOS BELOW DETECTION LIMITS
- SUM OF PFOA & PFOS CONCENTRATIONS AT OR BELOW 40 PPT
- SUM OF PFOA & PFOS CONCENTRATIONS BETWEEN 40 PPT AND 70 PPT
- SUM OF PFOA & PFOS CONCENTRATIONS ABOVE 70 PPT
- 👉 PUBLIC WATER CONNECTION (SOME NOT BY NAVY)
- SAMPLING AREA
- FORMER NAWC WARRINSTER
- TOWNSHIP BOUNDARY



PFC SAMPLE RESULTS MAP
 FORMER NAWC WARRINSTER
 MONTGOMERY COUNTY, PENNSYLVANIA

SCALE AS NOTED	
FILE	
NAWC	
REV 0	DATE 01/24/19
FIGURE NUMBER	
FIGURE 1	