



**Off-Base Drinking Water Sample Results,
Combined Level 2 and Level 4 Laboratory Report,
Electronic Data Deliverable, Data Validation Report,
and the Sample Location Figure, SDG 320-38382-1**

*Naval Air Warfare Center Warminster
Warminster, Pennsylvania*

August 2019

N62269_001170
WARMINSTER_NAWC
SSIC 5000-33c

LABORATORY DATA PACKAGE, 320-38382-1, NAS WILLOW GROVE NAWC
WARMINSTER PA
05/04/2018
TESTAMERICA LABORATORIES INC

Approved for public release: distribution unlimited.

ANALYTICAL REPORT

Job Number: 320-38382-1

Job Description: Warminster: PFAS, NAS JRB Willow Grove

For:
Tetra Tech, Inc.
234 Mall Boulevard
Suite 260
King of Prussia, PA 19406
Attention: Andy Frebowitz



Approved for release.
David R. Alltucker
Project Manager I
5/4/2018 12:49 PM

David R Alltucker, Project Manager I
880 Riverside Parkway, West Sacramento, CA, 95605
(916)374-4383
david.alltucker@testamericainc.com
05/04/2018

Table of Contents

Cover Title Page	1
Data Summaries	4
Definitions	4
Case Narrative	5
Detection Summary	6
Client Sample Results	7
Default Detection Limits	10
Surrogate Summary	11
QC Sample Results	12
QC Association	14
Chronicle	15
Certification Summary	17
Method Summary	18
Sample Summary	19
Manual Integration Summary	20
Reagent Traceability	26
COAs	34
Organic Sample Data	110
LCMS	110
Method 537 DOD	110
Method 537 DOD QC Summary	111
Method 537 DOD Sample Data	121
Standards Data	176
Method 537 DOD ICAL Data	176
Method 537 DOD CCAL Data	220
Raw QC Data	262

Table of Contents

Method 537 DOD Blank Data	262
Method 537 DOD LCS/LCSD Data	267
Method 537 DOD MS/MSD Data	274
Method 537 DOD Run Logs	288
Method 537 DOD Prep Data	292
Shipping and Receiving Documents	295
Client Chain of Custody	296
Sample Receipt Checklist	297

Definitions/Glossary

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-38382-1

Qualifiers

LCMS

Qualifier	Qualifier Description
U	Undetected at the Limit of Detection.
J	Estimated: The analyte was positively identified; the quantitation is an estimation
M	Manual integrated compound.
Q	One or more quality control criteria failed.
J1	Estimated: The quantitation is an estimation due to discrepancies in meeting certain analyte-specific quality control criteria.

Glossary

Abbreviation	These commonly used abbreviations may or may not be present in this report.
α	Listed under the "D" column to designate that the result is reported on a dry weight basis
%R	Percent Recovery
CFL	Contains Free Liquid
CNF	Contains No Free Liquid
DER	Duplicate Error Ratio (normalized absolute difference)
Dil Fac	Dilution Factor
DL	Detection Limit (DoD/DOE)
DL, RA, RE, IN	Indicates a Dilution, Re-analysis, Re-extraction, or additional Initial metals/anion analysis of the sample
DLC	Decision Level Concentration (Radiochemistry)
EDL	Estimated Detection Limit (Dioxin)
LOD	Limit of Detection (DoD/DOE)
LOQ	Limit of Quantitation (DoD/DOE)
MDA	Minimum Detectable Activity (Radiochemistry)
MDC	Minimum Detectable Concentration (Radiochemistry)
MDL	Method Detection Limit
ML	Minimum Level (Dioxin)
NC	Not Calculated
ND	Not Detected at the reporting limit (or MDL or EDL if shown)
PQL	Practical Quantitation Limit
QC	Quality Control
RER	Relative Error Ratio (Radiochemistry)
RL	Reporting Limit or Requested Limit (Radiochemistry)
RPD	Relative Percent Difference, a measure of the relative difference between two points
TEF	Toxicity Equivalent Factor (Dioxin)
TEQ	Toxicity Equivalent Quotient (Dioxin)

Job Narrative
320-38382-1

Receipt

The samples were received on 4/20/2018 9:20 AM; the samples arrived in good condition, properly preserved and, where required, on ice. The temperature of the cooler at receipt was 0.0° C.

LCMS

Method(s) 537: The first level standard from the initial calibration curve is used to evaluate the tune criteria. The instrument mass windows are set at +/- 0.5amu; therefore, detection of the analyte serves as verification that the assigned mass is within +/- 0.5amu of the true value, which meets the DoD/DOE QSM tune criterion.

Method(s) 537: The matrix spike duplicate (MS/MSD) recoveries and MS/MSD precision for preparation batch 320-219896 and analytical batch 320-220845 were outside control limits. Sample matrix interference and/or non-homogeneity are suspected because the associated laboratory control sample (LCS) was within acceptance limits.

Method(s) 537: Surrogate recovery for the following sample was outside control limits: NAWC-041918-RW-154 (320-38382-1[MSD]). Re-analysis was performed with concurring results. The original analysis has been reported.

No additional analytical or quality issues were noted, other than those described above or in the Definitions/Glossary page.

Organic Prep

No analytical or quality issues were noted, other than those described in the Definitions/Glossary page.

Detection Summary

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-38382-1

Client Sample ID: NAWC-041918-RW-154

Lab Sample ID: 320-38382-1

Analyte	Result	Qualifier	LOQ	DL	Unit	Dil Fac	D	Method	Prep Type
Perfluorooctanesulfonic acid (PFOS)	17	J M	40	6.7	ng/L	1		537	Total/NA
Perfluorooctanoic acid (PFOA)	24		20	2.8	ng/L	1		537	Total/NA
Perfluoroheptanoic acid (PFHpA)	8.1	J	9.9	1.9	ng/L	1		537	Total/NA

Client Sample ID: NAWC-041918-FRB-154

Lab Sample ID: 320-38382-2

No Detections.

Client Sample ID: NAWC-041918-RW-146

Lab Sample ID: 320-38382-3

Analyte	Result	Qualifier	LOQ	DL	Unit	Dil Fac	D	Method	Prep Type
Perfluorooctanesulfonic acid (PFOS)	14	J M	49	8.3	ng/L	1		537	Total/NA
Perfluorooctanoic acid (PFOA)	27		24	3.4	ng/L	1		537	Total/NA
Perfluoroheptanoic acid (PFHpA)	7.0	J	12	2.3	ng/L	1		537	Total/NA

Client Sample ID: NAWC-041918-FRB-146

Lab Sample ID: 320-38382-4

No Detections.

Client Sample ID: NAWC-041918-RW-258

Lab Sample ID: 320-38382-5

Analyte	Result	Qualifier	LOQ	DL	Unit	Dil Fac	D	Method	Prep Type
Perfluorooctanesulfonic acid (PFOS)	16	J M	38	6.5	ng/L	1		537	Total/NA
Perfluorooctanoic acid (PFOA)	20		19	2.7	ng/L	1		537	Total/NA
Perfluorononanoic acid (PFNA)	10	J	23	7.7	ng/L	1		537	Total/NA
Perfluoroheptanoic acid (PFHpA)	8.3	J	9.6	1.8	ng/L	1		537	Total/NA

Client Sample ID: NAWC-041918-FRB-258

Lab Sample ID: 320-38382-6

No Detections.

Client Sample ID: WGNA-041918-RW-3571

Lab Sample ID: 320-38382-7

Analyte	Result	Qualifier	LOQ	DL	Unit	Dil Fac	D	Method	Prep Type
Perfluorooctanesulfonic acid (PFOS)	8.0	J M	36	6.1	ng/L	1		537	Total/NA
Perfluorooctanoic acid (PFOA)	10	J	18	2.5	ng/L	1		537	Total/NA
Perfluoroheptanoic acid (PFHpA)	12		9.0	1.7	ng/L	1		537	Total/NA

Client Sample ID: WGNA-041918-FRB-3571

Lab Sample ID: 320-38382-8

No Detections.

This Detection Summary does not include radiochemical test results.

TestAmerica Sacramento

Client Sample Results

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-38382-1

Client Sample ID: NAWC-041918-RW-154

Lab Sample ID: 320-38382-1

Date Collected: 04/19/18 09:10

Matrix: Water

Date Received: 04/20/18 09:20

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	17	J M	40	6.7	ng/L		04/26/18 09:35	05/01/18 12:34	1
Perfluorooctanoic acid (PFOA)	24		20	2.8	ng/L		04/26/18 09:35	05/01/18 12:34	1
Perfluorononanoic acid (PFNA)	20	U M	24	7.9	ng/L		04/26/18 09:35	05/01/18 12:34	1
Perfluorohexanesulfonic acid (PFHxS)	12	U M	30	5.5	ng/L		04/26/18 09:35	05/01/18 12:34	1
Perfluoroheptanoic acid (PFHpA)	8.1	J	9.9	1.9	ng/L		04/26/18 09:35	05/01/18 12:34	1
Perfluorobutanesulfonic acid (PFBS)	36	U	89	16	ng/L		04/26/18 09:35	05/01/18 12:34	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	100		70 - 130	04/26/18 09:35	05/01/18 12:34	1
13C2 PFDA	89		70 - 130	04/26/18 09:35	05/01/18 12:34	1

Client Sample ID: NAWC-041918-FRB-154

Lab Sample ID: 320-38382-2

Date Collected: 04/19/18 09:05

Matrix: Water

Date Received: 04/20/18 09:20

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	15	U	37	6.4	ng/L		04/26/18 09:35	05/01/18 12:48	1
Perfluorooctanoic acid (PFOA)	7.5	U	19	2.6	ng/L		04/26/18 09:35	05/01/18 12:48	1
Perfluorononanoic acid (PFNA)	19	U	22	7.5	ng/L		04/26/18 09:35	05/01/18 12:48	1
Perfluorohexanesulfonic acid (PFHxS)	11	U	28	5.2	ng/L		04/26/18 09:35	05/01/18 12:48	1
Perfluoroheptanoic acid (PFHpA)	3.7	U	9.4	1.8	ng/L		04/26/18 09:35	05/01/18 12:48	1
Perfluorobutanesulfonic acid (PFBS)	34	U	84	15	ng/L		04/26/18 09:35	05/01/18 12:48	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	106		70 - 130	04/26/18 09:35	05/01/18 12:48	1
13C2 PFDA	85		70 - 130	04/26/18 09:35	05/01/18 12:48	1

Client Sample ID: NAWC-041918-RW-146

Lab Sample ID: 320-38382-3

Date Collected: 04/19/18 10:10

Matrix: Water

Date Received: 04/20/18 09:20

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	14	J M	49	8.3	ng/L		04/26/18 09:35	05/01/18 12:52	1
Perfluorooctanoic acid (PFOA)	27		24	3.4	ng/L		04/26/18 09:35	05/01/18 12:52	1
Perfluorononanoic acid (PFNA)	24	U	29	9.8	ng/L		04/26/18 09:35	05/01/18 12:52	1
Perfluorohexanesulfonic acid (PFHxS)	15	U	37	6.7	ng/L		04/26/18 09:35	05/01/18 12:52	1
Perfluoroheptanoic acid (PFHpA)	7.0	J	12	2.3	ng/L		04/26/18 09:35	05/01/18 12:52	1
Perfluorobutanesulfonic acid (PFBS)	44	U	110	20	ng/L		04/26/18 09:35	05/01/18 12:52	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	100		70 - 130	04/26/18 09:35	05/01/18 12:52	1
13C2 PFDA	83		70 - 130	04/26/18 09:35	05/01/18 12:52	1

Client Sample Results

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-38382-1

Client Sample ID: NAWC-041918-FRB-146

Lab Sample ID: 320-38382-4

Date Collected: 04/19/18 10:05

Matrix: Water

Date Received: 04/20/18 09:20

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	15	U	38	6.4	ng/L		04/26/18 09:35	05/01/18 12:57	1
Perfluorooctanoic acid (PFOA)	7.6	U	19	2.7	ng/L		04/26/18 09:35	05/01/18 12:57	1
Perfluorononanoic acid (PFNA)	19	U	23	7.6	ng/L		04/26/18 09:35	05/01/18 12:57	1
Perfluorohexanesulfonic acid (PFHxS)	11	U	28	5.2	ng/L		04/26/18 09:35	05/01/18 12:57	1
Perfluoroheptanoic acid (PFHpA)	3.8	U	9.5	1.8	ng/L		04/26/18 09:35	05/01/18 12:57	1
Perfluorobutanesulfonic acid (PFBS)	34	U	85	15	ng/L		04/26/18 09:35	05/01/18 12:57	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	106		70 - 130	04/26/18 09:35	05/01/18 12:57	1
13C2 PFDA	88		70 - 130	04/26/18 09:35	05/01/18 12:57	1

Client Sample ID: NAWC-041918-RW-258

Lab Sample ID: 320-38382-5

Date Collected: 04/19/18 10:40

Matrix: Water

Date Received: 04/20/18 09:20

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	16	J M	38	6.5	ng/L		04/26/18 09:35	05/01/18 13:02	1
Perfluorooctanoic acid (PFOA)	20		19	2.7	ng/L		04/26/18 09:35	05/01/18 13:02	1
Perfluorononanoic acid (PFNA)	10	J	23	7.7	ng/L		04/26/18 09:35	05/01/18 13:02	1
Perfluorohexanesulfonic acid (PFHxS)	11	U M	29	5.3	ng/L		04/26/18 09:35	05/01/18 13:02	1
Perfluoroheptanoic acid (PFHpA)	8.3	J	9.6	1.8	ng/L		04/26/18 09:35	05/01/18 13:02	1
Perfluorobutanesulfonic acid (PFBS)	34	U	86	15	ng/L		04/26/18 09:35	05/01/18 13:02	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	98		70 - 130	04/26/18 09:35	05/01/18 13:02	1
13C2 PFDA	80		70 - 130	04/26/18 09:35	05/01/18 13:02	1

Client Sample ID: NAWC-041918-FRB-258

Lab Sample ID: 320-38382-6

Date Collected: 04/19/18 10:35

Matrix: Water

Date Received: 04/20/18 09:20

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	15	U	37	6.4	ng/L		04/26/18 09:35	05/01/18 13:06	1
Perfluorooctanoic acid (PFOA)	7.5	U	19	2.6	ng/L		04/26/18 09:35	05/01/18 13:06	1
Perfluorononanoic acid (PFNA)	19	U	22	7.5	ng/L		04/26/18 09:35	05/01/18 13:06	1
Perfluorohexanesulfonic acid (PFHxS)	11	U	28	5.1	ng/L		04/26/18 09:35	05/01/18 13:06	1
Perfluoroheptanoic acid (PFHpA)	3.7	U	9.3	1.8	ng/L		04/26/18 09:35	05/01/18 13:06	1
Perfluorobutanesulfonic acid (PFBS)	34	U	84	15	ng/L		04/26/18 09:35	05/01/18 13:06	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	106		70 - 130	04/26/18 09:35	05/01/18 13:06	1
13C2 PFDA	85		70 - 130	04/26/18 09:35	05/01/18 13:06	1

Client Sample Results

Client: Tetra Tech, Inc.
 Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-38382-1

Client Sample ID: WGNA-041918-RW-3571

Lab Sample ID: 320-38382-7

Date Collected: 04/19/18 11:10

Matrix: Water

Date Received: 04/20/18 09:20

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	8.0	J M	36	6.1	ng/L		04/26/18 09:35	05/01/18 13:20	1
Perfluorooctanoic acid (PFOA)	10	J	18	2.5	ng/L		04/26/18 09:35	05/01/18 13:20	1
Perfluorononanoic acid (PFNA)	18	U M	22	7.2	ng/L		04/26/18 09:35	05/01/18 13:20	1
Perfluorohexanesulfonic acid (PFHxS)	11	U M	27	5.0	ng/L		04/26/18 09:35	05/01/18 13:20	1
Perfluoroheptanoic acid (PFHpA)	12		9.0	1.7	ng/L		04/26/18 09:35	05/01/18 13:20	1
Perfluorobutanesulfonic acid (PFBS)	32	U M	81	15	ng/L		04/26/18 09:35	05/01/18 13:20	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	99		70 - 130	04/26/18 09:35	05/01/18 13:20	1
13C2 PFDA	79		70 - 130	04/26/18 09:35	05/01/18 13:20	1

Client Sample ID: WGNA-041918-FRB-3571

Lab Sample ID: 320-38382-8

Date Collected: 04/19/18 11:05

Matrix: Water

Date Received: 04/20/18 09:20

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
Perfluorooctanesulfonic acid (PFOS)	17	U	43	7.2	ng/L		04/26/18 09:35	05/01/18 13:25	1
Perfluorooctanoic acid (PFOA)	8.5	U	21	3.0	ng/L		04/26/18 09:35	05/01/18 13:25	1
Perfluorononanoic acid (PFNA)	21	U	26	8.5	ng/L		04/26/18 09:35	05/01/18 13:25	1
Perfluorohexanesulfonic acid (PFHxS)	13	U	32	5.9	ng/L		04/26/18 09:35	05/01/18 13:25	1
Perfluoroheptanoic acid (PFHpA)	4.3	U	11	2.0	ng/L		04/26/18 09:35	05/01/18 13:25	1
Perfluorobutanesulfonic acid (PFBS)	38	U	96	17	ng/L		04/26/18 09:35	05/01/18 13:25	1

Surrogate	%Recovery	Qualifier	Limits	Prepared	Analyzed	Dil Fac
13C2 PFHxA	103		70 - 130	04/26/18 09:35	05/01/18 13:25	1
13C2 PFDA	87		70 - 130	04/26/18 09:35	05/01/18 13:25	1

Default Detection Limits

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-38382-1

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Prep: 537

Analyte	LOQ	DL	Units	Method
Perfluorobutanesulfonic acid (PFBS)	90	16	ng/L	537
Perfluoroheptanoic acid (PFHpA)	10	1.9	ng/L	537
Perfluorohexanesulfonic acid (PFHxS)	30	5.5	ng/L	537
Perfluorononanoic acid (PFNA)	24	8.0	ng/L	537
Perfluorooctanesulfonic acid (PFOS)	40	6.8	ng/L	537
Perfluorooctanoic acid (PFOA)	20	2.8	ng/L	537

Surrogate Summary

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-38382-1

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Matrix: Water

Prep Type: Total/NA

Lab Sample ID	Client Sample ID	Percent Surrogate Recovery (Acceptance Limits)	
		PFHxA (70-130)	PFDA (70-130)
320-38382-1	NAWC-041918-RW-154	100	89
320-38382-1 MS	NAWC-041918-RW-154	96	84
320-38382-1 MSD	NAWC-041918-RW-154	66 Q	74
320-38382-2	NAWC-041918-FRB-154	106	85
320-38382-3	NAWC-041918-RW-146	100	83
320-38382-4	NAWC-041918-FRB-146	106	88
320-38382-5	NAWC-041918-RW-258	98	80
320-38382-6	NAWC-041918-FRB-258	106	85
320-38382-7	WGNA-041918-RW-3571	99	79
320-38382-8	WGNA-041918-FRB-3571	103	87
LCS 320-219896/2-A	Lab Control Sample	108	91
MB 320-219896/1-A	Method Blank	107	90

Surrogate Legend

PFHxA = 13C2 PFHxA

PFDA = 13C2 PFDA

QC Sample Results

Client: Tetra Tech, Inc.
 Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-38382-1

Method: 537 - Perfluorinated Alkyl Acids (LC/MS)

Lab Sample ID: MB 320-219896/1-A
Matrix: Water
Analysis Batch: 220845

Client Sample ID: Method Blank
Prep Type: Total/NA
Prep Batch: 219896

Analyte	MB	MB	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
	Result	Qualifier							
Perfluorooctanesulfonic acid (PFOS)	16	U	40	6.8	ng/L		04/26/18 09:35	05/01/18 12:24	1
Perfluorooctanoic acid (PFOA)	8.0	U	20	2.8	ng/L		04/26/18 09:35	05/01/18 12:24	1
Perfluorononanoic acid (PFNA)	20	U	24	8.0	ng/L		04/26/18 09:35	05/01/18 12:24	1
Perfluorohexanesulfonic acid (PFHxS)	12	U	30	5.5	ng/L		04/26/18 09:35	05/01/18 12:24	1
Perfluoroheptanoic acid (PFHpA)	4.0	U	10	1.9	ng/L		04/26/18 09:35	05/01/18 12:24	1
Perfluorobutanesulfonic acid (PFBS)	36	U	90	16	ng/L		04/26/18 09:35	05/01/18 12:24	1

Surrogate	MB	MB	Limits	Prepared	Analyzed	Dil Fac
	%Recovery	Qualifier				
13C2 PFHxA	107		70 - 130	04/26/18 09:35	05/01/18 12:24	1
13C2 PFDA	90		70 - 130	04/26/18 09:35	05/01/18 12:24	1

Lab Sample ID: LCS 320-219896/2-A
Matrix: Water
Analysis Batch: 220845

Client Sample ID: Lab Control Sample
Prep Type: Total/NA
Prep Batch: 219896

Analyte	Spike Added	LCS Result	LCS Qualifier	Unit	D	%Rec	Limits
Perfluorooctanoic acid (PFOA)	110	110		ng/L		100	70 - 130
Perfluorononanoic acid (PFNA)	110	102		ng/L		93	70 - 130
Perfluorohexanesulfonic acid (PFHxS)	168	179		ng/L		106	70 - 130
Perfluoroheptanoic acid (PFHpA)	54.0	58.2		ng/L		108	70 - 130
Perfluorobutanesulfonic acid (PFBS)	500	519		ng/L		104	70 - 130

Surrogate	LCS	LCS	Limits
	%Recovery	Qualifier	
13C2 PFHxA	108		70 - 130
13C2 PFDA	91		70 - 130

Lab Sample ID: 320-38382-1 MS
Matrix: Water
Analysis Batch: 220845

Client Sample ID: NAWC-041918-RW-154
Prep Type: Total/NA
Prep Batch: 219896

Analyte	Sample	Sample	Spike Added	MS Result	MS Qualifier	Unit	D	%Rec	Limits
	Result	Qualifier							
Perfluorooctanesulfonic acid (PFOS)	17	J M	217	237	M	ng/L		102	70 - 130
Perfluorooctanoic acid (PFOA)	24		109	124		ng/L		92	70 - 130
Perfluorononanoic acid (PFNA)	20	U M	109	98.7		ng/L		91	70 - 130
Perfluorohexanesulfonic acid (PFHxS)	12	U M	166	177		ng/L		106	70 - 130
Perfluoroheptanoic acid (PFHpA)	8.1	J	53.5	59.8		ng/L		97	70 - 130
Perfluorobutanesulfonic acid (PFBS)	36	U	495	523		ng/L		105	70 - 130

Surrogate	MS	MS	Limits
	%Recovery	Qualifier	
13C2 PFHxA	96		70 - 130
13C2 PFDA	84		70 - 130

QC Sample Results

Client: Tetra Tech, Inc.
 Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-38382-1

Method: 537 - Perfluorinated Alkyl Acids (LC/MS) (Continued)

Lab Sample ID: 320-38382-1 MSD

Matrix: Water

Analysis Batch: 220845

Client Sample ID: NAWC-041918-RW-154

Prep Type: Total/NA

Prep Batch: 219896

Analyte	Sample	Sample	Spike	MSD	MSD	Unit	D	%Rec	%Rec.	RPD	RPD
	Result	Qualifier	Added	Result	Qualifier				Limits	RPD	Limit
Perfluorooctanesulfonic acid (PFOS)	17	J M	217	185	M	ng/L		78	70 - 130	25	30
Perfluorooctanoic acid (PFOA)	24		109	89.8	J1	ng/L		60	70 - 130	32	30
Perfluorononanoic acid (PFNA)	20	U M	109	77.7		ng/L		71	70 - 130	24	30
Perfluorohexanesulfonic acid (PFHxS)	12	U M	166	116	J1	ng/L		70	70 - 130	41	30
Perfluoroheptanoic acid (PFHpA)	8.1	J	53.4	41.1	J1	ng/L		62	70 - 130	37	30
Perfluorobutanesulfonic acid (PFBS)	36	U	495	347	J1	ng/L		70	70 - 130	40	30
		MSD	MSD								
Surrogate		%Recovery	Qualifier	Limits							
13C2 PFHxA		66	Q	70 - 130							
13C2 PFDA		74		70 - 130							

QC Association Summary

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-38382-1

LCMS

Prep Batch: 219896

Lab Sample ID	Client Sample ID	Prep Type	Matrix	Method	Prep Batch
320-38382-1	NAWC-041918-RW-154	Total/NA	Water	537	
320-38382-2	NAWC-041918-FRB-154	Total/NA	Water	537	
320-38382-3	NAWC-041918-RW-146	Total/NA	Water	537	
320-38382-4	NAWC-041918-FRB-146	Total/NA	Water	537	
320-38382-5	NAWC-041918-RW-258	Total/NA	Water	537	
320-38382-6	NAWC-041918-FRB-258	Total/NA	Water	537	
320-38382-7	WGNA-041918-RW-3571	Total/NA	Water	537	
320-38382-8	WGNA-041918-FRB-3571	Total/NA	Water	537	
MB 320-219896/1-A	Method Blank	Total/NA	Water	537	
LCS 320-219896/2-A	Lab Control Sample	Total/NA	Water	537	
320-38382-1 MS	NAWC-041918-RW-154	Total/NA	Water	537	
320-38382-1 MSD	NAWC-041918-RW-154	Total/NA	Water	537	

Analysis Batch: 220845

Lab Sample ID	Client Sample ID	Prep Type	Matrix	Method	Prep Batch
320-38382-1	NAWC-041918-RW-154	Total/NA	Water	537	219896
320-38382-2	NAWC-041918-FRB-154	Total/NA	Water	537	219896
320-38382-3	NAWC-041918-RW-146	Total/NA	Water	537	219896
320-38382-4	NAWC-041918-FRB-146	Total/NA	Water	537	219896
320-38382-5	NAWC-041918-RW-258	Total/NA	Water	537	219896
320-38382-6	NAWC-041918-FRB-258	Total/NA	Water	537	219896
MB 320-219896/1-A	Method Blank	Total/NA	Water	537	219896
LCS 320-219896/2-A	Lab Control Sample	Total/NA	Water	537	219896
320-38382-1 MS	NAWC-041918-RW-154	Total/NA	Water	537	219896
320-38382-1 MSD	NAWC-041918-RW-154	Total/NA	Water	537	219896

Analysis Batch: 220847

Lab Sample ID	Client Sample ID	Prep Type	Matrix	Method	Prep Batch
320-38382-7	WGNA-041918-RW-3571	Total/NA	Water	537	219896
320-38382-8	WGNA-041918-FRB-3571	Total/NA	Water	537	219896

Lab Chronicle

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-38382-1

Client Sample ID: NAWC-041918-RW-154

Date Collected: 04/19/18 09:10

Date Received: 04/20/18 09:20

Lab Sample ID: 320-38382-1

Matrix: Water

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			219896	04/26/18 09:35	TWL	TAL SAC
Total/NA	Analysis	537		1	220845	05/01/18 12:34	JRB	TAL SAC

Client Sample ID: NAWC-041918-FRB-154

Date Collected: 04/19/18 09:05

Date Received: 04/20/18 09:20

Lab Sample ID: 320-38382-2

Matrix: Water

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			219896	04/26/18 09:35	TWL	TAL SAC
Total/NA	Analysis	537		1	220845	05/01/18 12:48	JRB	TAL SAC

Client Sample ID: NAWC-041918-RW-146

Date Collected: 04/19/18 10:10

Date Received: 04/20/18 09:20

Lab Sample ID: 320-38382-3

Matrix: Water

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			219896	04/26/18 09:35	TWL	TAL SAC
Total/NA	Analysis	537		1	220845	05/01/18 12:52	JRB	TAL SAC

Client Sample ID: NAWC-041918-FRB-146

Date Collected: 04/19/18 10:05

Date Received: 04/20/18 09:20

Lab Sample ID: 320-38382-4

Matrix: Water

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			219896	04/26/18 09:35	TWL	TAL SAC
Total/NA	Analysis	537		1	220845	05/01/18 12:57	JRB	TAL SAC

Client Sample ID: NAWC-041918-RW-258

Date Collected: 04/19/18 10:40

Date Received: 04/20/18 09:20

Lab Sample ID: 320-38382-5

Matrix: Water

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			219896	04/26/18 09:35	TWL	TAL SAC
Total/NA	Analysis	537		1	220845	05/01/18 13:02	JRB	TAL SAC

Client Sample ID: NAWC-041918-FRB-258

Date Collected: 04/19/18 10:35

Date Received: 04/20/18 09:20

Lab Sample ID: 320-38382-6

Matrix: Water

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			219896	04/26/18 09:35	TWL	TAL SAC
Total/NA	Analysis	537		1	220845	05/01/18 13:06	JRB	TAL SAC

TestAmerica Sacramento

Lab Chronicle

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-38382-1

Client Sample ID: WGNA-041918-RW-3571

Lab Sample ID: 320-38382-7

Date Collected: 04/19/18 11:10

Matrix: Water

Date Received: 04/20/18 09:20

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			219896	04/26/18 09:35	TWL	TAL SAC
Total/NA	Analysis	537		1	220847	05/01/18 13:20	JRB	TAL SAC

Client Sample ID: WGNA-041918-FRB-3571

Lab Sample ID: 320-38382-8

Date Collected: 04/19/18 11:05

Matrix: Water

Date Received: 04/20/18 09:20

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Prepared or Analyzed	Analyst	Lab
Total/NA	Prep	537			219896	04/26/18 09:35	TWL	TAL SAC
Total/NA	Analysis	537		1	220847	05/01/18 13:25	JRB	TAL SAC

Laboratory References:

TAL SAC = TestAmerica Sacramento, 880 Riverside Parkway, West Sacramento, CA 95605, TEL (916)373-5600

Accreditation/Certification Summary

Client: Tetra Tech, Inc.
 Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-38382-1

Laboratory: TestAmerica Sacramento

All accreditations/certifications held by this laboratory are listed. Not all accreditations/certifications are applicable to this report.

Authority	Program	EPA Region	Identification Number	Expiration Date
Alaska (UST)	State Program	10	17-020	01-20-21
Arizona	State Program	9	AZ0708	08-11-18
Arkansas DEQ	State Program	6	88-0691	06-17-19
California	State Program	9	2897	01-31-19
Colorado	State Program	8	CA00044	08-31-18
Connecticut	State Program	1	PH-0691	06-30-19
Florida	NELAP	4	E87570	06-30-18
Georgia	State Program	4	N/A	01-28-19
Hawaii	State Program	9	N/A	01-29-19
Illinois	NELAP	5	200060	03-17-19
Kansas	NELAP	7	E-10375	10-31-18
L-A-B	DoD ELAP		L2468	01-20-21
Louisiana	NELAP	6	30612	06-30-18
Maine	State Program	1	CA0004	04-14-20
Michigan	State Program	5	9947	01-31-20
Nevada	State Program	9	CA00044	07-31-18
New Hampshire	NELAP	1	2997	04-18-19
New Jersey	NELAP	2	CA005	06-30-18
New York	NELAP	2	11666	03-31-19
Oregon	NELAP	10	4040	01-29-19
Pennsylvania	NELAP	3	68-01272	03-31-19
Texas	NELAP	6	T104704399	05-31-18
US Fish & Wildlife	Federal		LE148388-0	07-31-18
USDA	Federal		P330-11-00436	01-17-21
USEPA UCMR	Federal	1	CA00044	11-06-18
Utah	NELAP	8	CA00044	02-28-19
Virginia	NELAP	3	460278	03-14-19
Washington	State Program	10	C581	05-05-18
West Virginia (DW)	State Program	3	9930C	12-31-18
Wyoming	State Program	8	8TMS-L	01-28-19

Method Summary

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-38382-1

Method	Method Description	Protocol	Laboratory
537	Perfluorinated Alkyl Acids (LC/MS)	EPA	TAL SAC
537	Extraction of Perfluorinated Alkyl Acids	EPA	TAL SAC

Protocol References:

EPA = US Environmental Protection Agency

Laboratory References:

TAL SAC = TestAmerica Sacramento, 880 Riverside Parkway, West Sacramento, CA 95605, TEL (916)373-5600

Sample Summary

Client: Tetra Tech, Inc.

TestAmerica Job ID: 320-38382-1

Project/Site: Warminster: PFAS, NAS JRB Willow Grove

Lab Sample ID	Client Sample ID	Matrix	Collected	Received
320-38382-1	NAWC-041918-RW-154	Water	04/19/18 09:10	04/20/18 09:20
320-38382-2	NAWC-041918-FRB-154	Water	04/19/18 09:05	04/20/18 09:20
320-38382-3	NAWC-041918-RW-146	Water	04/19/18 10:10	04/20/18 09:20
320-38382-4	NAWC-041918-FRB-146	Water	04/19/18 10:05	04/20/18 09:20
320-38382-5	NAWC-041918-RW-258	Water	04/19/18 10:40	04/20/18 09:20
320-38382-6	NAWC-041918-FRB-258	Water	04/19/18 10:35	04/20/18 09:20
320-38382-7	WGNA-041918-RW-3571	Water	04/19/18 11:10	04/20/18 09:20
320-38382-8	WGNA-041918-FRB-3571	Water	04/19/18 11:05	04/20/18 09:20

LCMS MANUAL INTEGRATION SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1

SDG No.: _____

Instrument ID: A8_N Analysis Batch Number: 217453

Lab Sample ID: IC 320-217453/3 Client Sample ID: _____

Date Analyzed: 04/11/18 11:45 Lab File ID: 2018.04.11_537ICALB_004.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.10	Peak assignment corrected	westendor fc	04/11/18 12:31

Lab Sample ID: IC 320-217453/4 Client Sample ID: _____

Date Analyzed: 04/11/18 11:50 Lab File ID: 2018.04.11_537ICALB_005.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.10	Peak assignment corrected	westendor fc	04/11/18 12:31

Lab Sample ID: IC 320-217453/5 Client Sample ID: _____

Date Analyzed: 04/11/18 11:55 Lab File ID: 2018.04.11_537ICALB_006.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.11	Peak assignment corrected	westendor fc	04/11/18 12:31

Lab Sample ID: IC 320-217453/6 ICISAV Client Sample ID: _____

Date Analyzed: 04/11/18 11:59 Lab File ID: 2018.04.11_537ICALB_007.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.10	Peak assignment corrected	westendor fc	04/11/18 12:31

LCMS MANUAL INTEGRATION SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1

SDG No.: _____

Instrument ID: A8_N Analysis Batch Number: 217453

Lab Sample ID: IC 320-217453/7 Client Sample ID: _____

Date Analyzed: 04/11/18 12:04 Lab File ID: 2018.04.11_537ICALB_008.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.10	Peak assignment corrected	westendor fc	04/11/18 12:31

Lab Sample ID: IC 320-217453/8 Client Sample ID: _____

Date Analyzed: 04/11/18 12:09 Lab File ID: 2018.04.11_537ICALB_009.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.09	Peak assignment corrected	westendor fc	04/11/18 12:31

Lab Sample ID: CCVL 320-217453/10 Client Sample ID: _____

Date Analyzed: 04/11/18 12:18 Lab File ID: 2018.04.11_537ICALB_011.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.10	Peak assignment corrected	westendor fc	04/11/18 12:32

Lab Sample ID: ICV 320-217453/12 Client Sample ID: _____

Date Analyzed: 04/11/18 12:27 Lab File ID: 2018.04.11_537ICALB_013.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.10	Peak assignment corrected	westendor fc	04/11/18 12:35

LCMS MANUAL INTEGRATION SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1

SDG No.: _____

Instrument ID: A8_N Analysis Batch Number: 220842

Lab Sample ID: CCVL 320-220842/1 Client Sample ID: _____

Date Analyzed: 05/01/18 11:19 Lab File ID: 2018.05.01_537AA_003.d GC Column: GeminiC18 3x1 ID: 3 (mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.12	Peak assignment corrected	roycea	05/01/18 13:10

LCMS MANUAL INTEGRATION SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1

SDG No.: _____

Instrument ID: A8_N Analysis Batch Number: 220845

Lab Sample ID: CCV 320-220845/13 CCVIS Client Sample ID: _____

Date Analyzed: 05/01/18 12:15 Lab File ID: 2018.05.01_537AA_015.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.12	Peak assignment corrected	barnettj	05/02/18 10:39

Lab Sample ID: LCS 320-219896/2-A Client Sample ID: _____

Date Analyzed: 05/01/18 12:29 Lab File ID: 2018.05.01_537AA_018.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.12	Peak assignment corrected	roycea	05/01/18 13:58

Lab Sample ID: 320-38382-1 Client Sample ID: NAWC-041918-RW-154

Date Analyzed: 05/01/18 12:34 Lab File ID: 2018.05.01_537AA_019.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorohexanesulfonic acid (PFHxS)	1.69	Missed Peak	barnettj	05/01/18 17:12
Perfluorononanoic acid (PFNA)	2.12	Missed Peak	barnettj	05/01/18 17:13
Perfluorooctanesulfonic acid (PFOS)	2.12	Missed Peak	barnettj	05/01/18 17:12

Lab Sample ID: 320-38382-1 MS Client Sample ID: NAWC-041918-RW-154 MS

Date Analyzed: 05/01/18 12:38 Lab File ID: 2018.05.01_537AA_020.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.12	Peak assignment corrected	barnettj	05/01/18 17:13

LCMS MANUAL INTEGRATION SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1

SDG No.: _____

Instrument ID: A8_N Analysis Batch Number: 220845

Lab Sample ID: 320-38382-1 MSD Client Sample ID: NAWC-041918-RW-154 MSD

Date Analyzed: 05/01/18 12:43 Lab File ID: 2018.05.01_537AA_021.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.12	Peak assignment corrected	barnettj	05/01/18 17:13

Lab Sample ID: 320-38382-3 Client Sample ID: NAWC-041918-RW-146

Date Analyzed: 05/01/18 12:52 Lab File ID: 2018.05.01_537AA_023.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.12	Peak assignment corrected	barnettj	05/01/18 17:13

Lab Sample ID: 320-38382-5 Client Sample ID: NAWC-041918-RW-258

Date Analyzed: 05/01/18 13:02 Lab File ID: 2018.05.01_537AA_025.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorohexanesulfonic acid (PFHxS)	1.69	Missed Peak	barnettj	05/01/18 17:14
Perfluorooctanesulfonic acid (PFOS)	2.12	Missed Peak	barnettj	05/01/18 17:14

Lab Sample ID: CCV 320-220845/25 CCVIS Client Sample ID: _____

Date Analyzed: 05/01/18 13:11 Lab File ID: 2018.05.01_537AA_027.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.12	Peak assignment corrected	roycea	05/01/18 14:00

LCMS MANUAL INTEGRATION SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1

SDG No.: _____

Instrument ID: A8_N Analysis Batch Number: 220847

Lab Sample ID: CCV 320-220847/25 CCVIS Client Sample ID: _____

Date Analyzed: 05/01/18 13:11 Lab File ID: 2018.05.01_537AA_027.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.12	Peak assignment corrected	roycea	05/01/18 14:00

Lab Sample ID: 320-38382-7 Client Sample ID: WGNA-041918-RW-3571

Date Analyzed: 05/01/18 13:20 Lab File ID: 2018.05.01_537AA_029.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorobutanesulfonic acid (PFBS)	1.39	Missed Peak	barnettj	05/01/18 17:15
Perfluorohexanesulfonic acid (PFHxS)	1.68	Missed Peak	barnettj	05/01/18 17:15
Perfluorooctanesulfonic acid (PFOS)	2.11	Missed Peak	barnettj	05/01/18 17:15
Perfluorononanoic acid (PFNA)	2.12	Missed Peak	barnettj	05/01/18 17:15

Lab Sample ID: CCV 320-220847/29 CCVIS Client Sample ID: _____

Date Analyzed: 05/01/18 13:30 Lab File ID: 2018.05.01_537AA_031.d GC Column: GeminiC18 3x1 ID: 3(mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Perfluorooctanesulfonic acid (PFOS)	2.11	Peak assignment corrected	roycea	05/01/18 14:01

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-38382-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration					
					Reagent ID	Volume Added							
LC537-HSP_00029	10/06/18	04/06/18	Methanol, Lot 104453	30 mL	LCPFBSA_00002	849 uL	Perfluorobutanesulfonic acid (PFBS)	1250.86 ng/mL					
					LCPFHpA_00009	81 uL	Perfluoroheptanoic acid (PFHpA)	135 ng/mL					
					LCPFHxS-br_00005	277 uL	Perfluorohexane Sulfonate	420.117 ng/mL					
							Perfluorohexanesulfonic acid (PFHxS)	420.117 ng/mL					
					LCPFNA_00009	165 uL	Perfluorononanoic acid (PFNA)	275 ng/mL					
					LCPFOA_00010	165 uL	Perfluorooctanoic acid (PFOA)	275 ng/mL					
		LCPFOS-br_00005	355 uL	Perfluorooctanesulfonic acid (PFOS)	549.067 ng/mL								
.LCPFBSA_00002	12/02/21	Wellington Laboratories, Lot LPFBS1116		(Purchased Reagent)		Perfluorobutanesulfonic acid (PFBS)	44.2 ug/mL						
.LCPFHpA_00009	12/02/21	Wellington Laboratories, Lot PFHpA1216		(Purchased Reagent)		Perfluoroheptanoic acid (PFHpA)	50 ug/mL						
.LCPFHxS-br_00005	01/04/22	Wellington Laboratories, Lot brPFHxSK0117		(Purchased Reagent)		Perfluorohexane Sulfonate	45.5 ug/mL						
						Perfluorohexanesulfonic acid (PFHxS)	45.5 ug/mL						
.LCPFNA_00009	07/20/22	Wellington Laboratories, Lot PFNA0717		(Purchased Reagent)		Perfluorononanoic acid (PFNA)	50 ug/mL						
.LCPFOA_00010	09/27/22	Wellington Laboratories, Lot PFOA0917		(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	50 ug/mL						
.LCPFOS-br_00005	01/12/22	Wellington Laboratories, Lot brPFOSK0117		(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	46.4 ug/mL						
LC537-ICV_00030	07/30/18	02/15/18	MeOH/H2O, Lot 067374	10 mL	LC537-IS_00059	1000 uL	13C2-PFOA	10 ng/mL					
							13C4 PFOS	28.68 ng/mL					
					.LC537-IS_00059	07/30/18	01/30/18	Methanol, Lot 090285	30000 uL	LCM2PFOA_00007	60 uL	13C2-PFOA	0.1 ug/mL
									LCMPFOS_00021	180 uL	13C4 PFOS	0.2868 ug/mL	
						(Purchased Reagent)	13C2-PFOA	50 ug/mL					
						(Purchased Reagent)	13C4 PFOS	47.8 ug/mL					
LC537-ICV_00030	07/30/18	02/15/18	MeOH/H2O, Lot 067374	10 mL	LC537-SU_00059	1000 uL	13C2 PFDA	10 ng/mL					
							13C2 PFHxA	10 ng/mL					
							LC537ICIM2_00001	400 uL	Perfluorobutanesulfonic acid (PFBS)	100.092 ng/mL			
									Perfluoroheptanoic acid (PFHpA)	10 ng/mL			
									Perfluorohexanesulfonic acid (PFHxS)	20.1619 ng/mL			
									Perfluorononanoic acid (PFNA)	20.1641 ng/mL			
									Perfluorooctanoic acid (PFOA)	20.167 ng/mL			
									Perfluorooctanesulfonic acid (PFOS)	20.1702 ng/mL			
.LC537-SU_00059	07/30/18	01/30/18	Methanol, Lot 104453	30000 uL	LCMPFDA_00012	60 uL	13C2 PFDA	0.1 ug/mL					
					LCMPFHxA_00015	60 uL	13C2 PFHxA	0.1 ug/mL					
						(Purchased Reagent)	13C2 PFDA	50 ug/mL					
						(Purchased Reagent)	13C2 PFHxA	50 ug/mL					
.LCMPFDA_00012	09/30/21	Wellington Laboratories, Lot MPFDA0916		(Purchased Reagent)		13C2 PFDA	50 ug/mL						
.LCMPFHxA_00015	11/22/21	Wellington Laboratories, Lot MPFHxA1116		(Purchased Reagent)		13C2 PFHxA	50 ug/mL						
.LC537ICIM2_00001	08/15/18	02/15/18	Methanol, Lot 090285	10 mL	LC537ICIM_00020	0.5 mL	Perfluorobutanesulfonic acid (PFBS)	2.5023 ug/mL					
							Perfluoroheptanoic acid (PFHpA)	0.25 ug/mL					

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-38382-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
							Perfluorohexanesulfonic acid (PFHxS)	0.504047 ug/mL
							Perfluorononanoic acid (PFNA)	0.504103 ug/mL
							Perfluorooctanoic acid (PFOA)	0.504176 ug/mL
							Perfluorooctanesulfonic acid (PFOS)	0.504255 ug/mL
..LC537ICIM_00020	08/15/18	02/15/18	Methanol, Lot 090285	25 mL	LC537-PFBS2_00009	0.625 mL	Perfluorobutanesulfonic acid (PFBS)	50.0459 ug/mL
					LC537-PFHpa2_00012	0.0625 mL	Perfluoroheptanoic acid (PFHpA)	5 ug/mL
					LC537-PFHxS2_00009	0.126 mL	Perfluorohexanesulfonic acid (PFHxS)	10.0809 ug/mL
					LC537-PFNA2_00010	0.126 mL	Perfluorononanoic acid (PFNA)	10.0821 ug/mL
					LC537-PFOA2_00011	0.126 mL	Perfluorooctanoic acid (PFOA)	10.0835 ug/mL
					LC537-PFOS2_00011	0.126 mL	Perfluorooctanesulfonic acid (PFOS)	10.0851 ug/mL
...LC537-PFBS2_00009	08/15/18	02/15/18	Methanol, Lot 090285	17.1 mL	LC537_PFBS2_00002	0.0343 g	Perfluorobutanesulfonic acid (PFBS)	2001.84 ug/mL
....LC537_PFBS2_00002	09/08/22	Santa Cruz Biotechnology, Lot F0917			(Purchased Reagent)		Perfluorobutanesulfonic acid (PFBS)	0.998 g/g
..LC537-PFHpa2_00012	08/15/18	02/15/18	Methanol, Lot 09092	23.95 mL	LC537_PFHpa2_00002	0.0479 g	Perfluoroheptanoic acid (PFHpA)	2000 ug/mL
....LC537_PFHpa2_00002	06/13/22	Afla Aesar, Lot 10200390			(Purchased Reagent)		Perfluoroheptanoic acid (PFHpA)	1 g/g
..LC537-PFHxS2_00009	08/15/18	02/15/18	Methanol, Lot 090285	25.87 mL	LC537_PFHxS2_00002	0.0569 g	Perfluorohexanesulfonic acid (PFHxS)	2000.19 ug/mL
....LC537_PFHxS2_00002	06/08/22	Santa Cruz Biotechnology, Lot G2516			(Purchased Reagent)		Perfluorohexanesulfonic acid (PFHxS)	0.9094 g/g
..LC537-PFNA2_00010	08/15/18	02/15/18	Methanol, Lot 090285	16.58 mL	LC537 PFNA2_00002	0.0333 g	Perfluorononanoic acid (PFNA)	2000.41 ug/mL
...LC537 PFNA2_00002	06/14/22	Aldrich, Lot MKCC0699			(Purchased Reagent)		Perfluorononanoic acid (PFNA)	0.996 g/g
..LC537-PFOA2_00011	08/15/18	02/15/18	Methanol, Lot 090285	22.96 mL	LC537 PFOA2_00002	0.0464 g	Perfluorooctanoic acid (PFOA)	2000.7 ug/mL
...LC537 PFOA2_00002	06/09/22	Afla Aesar, Lot 10199078			(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	0.99 g/g
..LC537-PFOS2_00011	08/15/18	02/15/18	Methanol, Lot 090285	14.71 mL	LC537_PFOS2_00002	0.0378 g	Perfluorooctanesulfonic acid (PFOS)	2001.01 ug/mL
....LC537_PFOS2_00002	06/14/22	Sigma, Lot BCBQ0108V			(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	0.7787 g/g
LC537-IS_00068	12/26/18	04/26/18	Methanol, Lot 090285	30000 uL	LCM2PFOA_00010	60 uL	13C2-PFOA	0.1 ug/mL
					LCMPFOS_00024	180 uL	13C4 PFOS	0.2868 ug/mL
.LCM2PFOA_00010	02/12/21	Wellington Laboratories, Lot M2PFOA0216			(Purchased Reagent)		13C2-PFOA	50 ug/mL
.LCMPFOS_00024	05/19/22	Wellington Laboratories, Lot MPFOS517			(Purchased Reagent)		13C4 PFOS	47.8 ug/mL
LC537-L1_00022	09/30/18	04/02/18	MeOH/H2O, Lot 090285	5 mL	LC537-IS_00065	500 uL	13C2-PFOA	10 ng/mL
							13C4 PFOS	28.68 ng/mL
					LC537-MSP_00033	60 uL	Perfluorobutanesulfonic acid (PFBS)	8.99912 ng/mL
							Perfluoroheptanoic acid (PFHpA)	0.96 ng/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-38382-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
							Perfluorohexanesulfonic acid (PFHxS)	3.003 ng/mL
							Perfluorononanoic acid (PFNA)	1.98 ng/mL
							Perfluorooctanoic acid (PFOA)	1.98 ng/mL
							Perfluorooctanesulfonic acid (PFOS)	3.95328 ng/mL
					LC537-SU_00064	500 uL	13C2 PFDA	10 ng/mL
							13C2 PFHxA	10 ng/mL
.LC537-IS_00065	10/02/18	04/02/18	Methanol, Lot 090285	30000 uL	LCM2PFOA_00010	60 uL	13C2-PFOA	0.1 ug/mL
					LCMPFOS_00024	180 uL	13C4 PFOS	0.2868 ug/mL
..LCM2PFOA_00010	02/12/21	Wellington Laboratories, Lot M2PFOA0216			(Purchased Reagent)		13C2-PFOA	50 ug/mL
..LCMPFOS_00024	05/19/22	Wellington Laboratories, Lot MPFOS517			(Purchased Reagent)		13C4 PFOS	47.8 ug/mL
.LC537-MSP_00033	09/30/18	03/30/18	Methanol, Lot 104453	30 mL	LCPFBSA_00002	509 uL	Perfluorobutanesulfonic acid (PFBS)	749.927 ng/mL
					LCPFHpA_00009	48 uL	Perfluoroheptanoic acid (PFHpA)	80 ng/mL
					LCPFHxS-br_00005	165 uL	Perfluorohexanesulfonic acid (PFHxS)	250.25 ng/mL
					LCPFNA_00009	99 uL	Perfluorononanoic acid (PFNA)	165 ng/mL
					LCPFOA_00010	99 uL	Perfluorooctanoic acid (PFOA)	165 ng/mL
					LCPFOS-br_00005	213 uL	Perfluorooctanesulfonic acid (PFOS)	329.44 ng/mL
..LCPFBSA_00002	12/02/21	Wellington Laboratories, Lot LPFBS1116			(Purchased Reagent)		Perfluorobutanesulfonic acid (PFBS)	44.2 ug/mL
..LCPFHpA_00009	12/02/21	Wellington Laboratories, Lot PFHpA1216			(Purchased Reagent)		Perfluoroheptanoic acid (PFHpA)	50 ug/mL
..LCPFHxS-br_00005	01/04/22	Wellington Laboratories, Lot brPFHxSK0117			(Purchased Reagent)		Perfluorohexanesulfonic acid (PFHxS)	45.5 ug/mL
..LCPFNA_00009	07/20/22	Wellington Laboratories, Lot PFNA0717			(Purchased Reagent)		Perfluorononanoic acid (PFNA)	50 ug/mL
..LCPFOA_00010	09/27/22	Wellington Laboratories, Lot PFOA0917			(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	50 ug/mL
..LCPFOS-br_00005	01/12/22	Wellington Laboratories, Lot brPFOSK0117			(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	46.4 ug/mL
.LC537-SU_00064	10/02/18	04/02/18	Methanol, Lot 104453	30000 uL	LCMPFDA_00012	60 uL	13C2 PFDA	0.1 ug/mL
					LCMPFHxA_00015	60 uL	13C2 PFHxA	0.1 ug/mL
..LCMPFDA_00012	09/30/21	Wellington Laboratories, Lot MPFDA0916			(Purchased Reagent)		13C2 PFDA	50 ug/mL
..LCMPFHxA_00015	11/22/21	Wellington Laboratories, Lot MPFHxA1116			(Purchased Reagent)		13C2 PFHxA	50 ug/mL
LC537-L2_00022	09/30/18	04/02/18	MeOH/H2O, Lot 090285	20 mL	LC537-HSP_00028	320 uL	Perfluorobutanesulfonic acid (PFBS)	20.0138 ng/mL
							Perfluoroheptanoic acid (PFHpA)	2.16 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	6.72187 ng/mL
							Perfluorononanoic acid (PFNA)	4.4 ng/mL
							Perfluorooctanoic acid (PFOA)	4.4 ng/mL
							Perfluorooctanesulfonic acid (PFOS)	8.78507 ng/mL
					LC537-IS_00065	2 mL	13C2-PFOA	10 ng/mL
							13C4 PFOS	28.68 ng/mL
					LC537-SU_00064	2 mL	13C2 PFDA	10 ng/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-38382-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
.LC537-HSP_00028	09/30/18	03/30/18	Methanol, Lot 104453	30 mL	LCPFBSA_00002	849 uL	13C2 PFHxA	10 ng/mL
					LCPFHpa_00009	81 uL	Perfluorobutanesulfonic acid (PFBS)	1250.86 ng/mL
					LCPFHxS-br_00005	277 uL	Perfluoroheptanoic acid (PFHpA)	135 ng/mL
					LCPFNA_00009	165 uL	Perfluorohexanesulfonic acid (PFHxS)	420.117 ng/mL
					LCPFOA_00010	165 uL	Perfluorononanoic acid (PFNA)	275 ng/mL
LCPFOS-br_00005	355 uL	Perfluorooctanoic acid (PFOA)	275 ng/mL					
..LCPFBSA_00002	12/02/21	Wellington Laboratories, Lot LPFBS1116			(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	549.067 ng/mL
..LCPFHpa_00009	12/02/21	Wellington Laboratories, Lot PFHpA1216			(Purchased Reagent)		Perfluorobutanesulfonic acid (PFBS)	44.2 ug/mL
..LCPFHxS-br_00005	01/04/22	Wellington Laboratories, Lot brPFHxSK0117			(Purchased Reagent)		Perfluoroheptanoic acid (PFHpA)	50 ug/mL
..LCPFNA_00009	07/20/22	Wellington Laboratories, Lot PFNA0717			(Purchased Reagent)		Perfluorohexanesulfonic acid (PFHxS)	45.5 ug/mL
..LCPFOA_00010	09/27/22	Wellington Laboratories, Lot PFOA0917			(Purchased Reagent)		Perfluorononanoic acid (PFNA)	50 ug/mL
..LCPFOS-br_00005	01/12/22	Wellington Laboratories, Lot brPFOSK0117			(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	50 ug/mL
.LC537-IS_00065	10/02/18	04/02/18	Methanol, Lot 090285	30000 uL	LCM2PFOA_00010	60 uL	13C2-PFOA	0.1 ug/mL
					LCMPFOS_00024	180 uL	13C4 PFOS	0.2868 ug/mL
..LCM2PFOA_00010	02/12/21	Wellington Laboratories, Lot M2PFOA0216			(Purchased Reagent)		13C2-PFOA	50 ug/mL
..LCMPFOS_00024	05/19/22	Wellington Laboratories, Lot MPFOS517			(Purchased Reagent)		13C4 PFOS	47.8 ug/mL
.LC537-SU_00064	10/02/18	04/02/18	Methanol, Lot 104453	30000 uL	LCMPFDA_00012	60 uL	13C2 PFDA	0.1 ug/mL
					LCMPFHxA_00015	60 uL	13C2 PFHxA	0.1 ug/mL
..LCMPFDA_00012	09/30/21	Wellington Laboratories, Lot MPFDA0916			(Purchased Reagent)		13C2 PFDA	50 ug/mL
..LCMPFHxA_00015	11/22/21	Wellington Laboratories, Lot MPFHxA1116			(Purchased Reagent)		13C2 PFHxA	50 ug/mL
LC537-L3_00025	09/30/18	04/02/18	MeOH/H2O, Lot 090285	20 mL	LC537-HSP_00028	720 uL	Perfluorobutanesulfonic acid (PFBS)	45.031 ng/mL
							Perfluoroheptanoic acid (PFHpA)	4.86 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	15.1242 ng/mL
							Perfluorononanoic acid (PFNA)	9.9 ng/mL
							Perfluorooctanoic acid (PFOA)	9.9 ng/mL
							Perfluorooctanesulfonic acid (PFOS)	19.7664 ng/mL
					LC537-IS_00065	2 mL	13C2-PFOA	10 ng/mL
LC537-SU_00064	2 mL	13C4 PFOS	28.68 ng/mL					
.LC537-HSP_00028	09/30/18	03/30/18	Methanol, Lot 104453	30 mL	LCPFBSA_00002	849 uL	13C2 PFDA	10 ng/mL
					LCPFHpa_00009	81 uL	13C2 PFHxA	10 ng/mL
					LCPFHxS-br_00005	277 uL	13C2 PFHxA	10 ng/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-38382-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
					LCPFNA_00009	165 uL	Perfluorononanoic acid (PFNA)	275 ng/mL
					LCPFOA_00010	165 uL	Perfluorooctanoic acid (PFOA)	275 ng/mL
					LCPFOS-br_00005	355 uL	Perfluorooctanesulfonic acid (PFOS)	549.067 ng/mL
..LCPFBSA_00002	12/02/21	Wellington Laboratories, Lot LPFBS1116			(Purchased Reagent)		Perfluorobutanesulfonic acid (PFBS)	44.2 ug/mL
..LCPFHpA_00009	12/02/21	Wellington Laboratories, Lot PFHpA1216			(Purchased Reagent)		Perfluoroheptanoic acid (PFHpA)	50 ug/mL
..LCPFHxS-br_00005	01/04/22	Wellington Laboratories, Lot brPFHxSK0117			(Purchased Reagent)		Perfluorohexanesulfonic acid (PFHxS)	45.5 ug/mL
..LCPFNA_00009	07/20/22	Wellington Laboratories, Lot PFNA0717			(Purchased Reagent)		Perfluorononanoic acid (PFNA)	50 ug/mL
..LCPFOA_00010	09/27/22	Wellington Laboratories, Lot PFOA0917			(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	50 ug/mL
..LCPFOS-br_00005	01/12/22	Wellington Laboratories, Lot brPFOSK0117			(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	46.4 ug/mL
.LC537-IS_00065	10/02/18	04/02/18	Methanol, Lot 090285	30000 uL	LCM2PFOA_00010	60 uL	13C2-PFOA	0.1 ug/mL
					LCMPFOS_00024	180 uL	13C4 PFOS	0.2868 ug/mL
..LCM2PFOA_00010	02/12/21	Wellington Laboratories, Lot M2PFOA0216			(Purchased Reagent)		13C2-PFOA	50 ug/mL
..LCMPFOS_00024	05/19/22	Wellington Laboratories, Lot MPFOS517			(Purchased Reagent)		13C4 PFOS	47.8 ug/mL
.LC537-SU_00064	10/02/18	04/02/18	Methanol, Lot 104453	30000 uL	LCMPFDA_00012	60 uL	13C2 PFDA	0.1 ug/mL
					LCMPFHxA_00015	60 uL	13C2 PFHxA	0.1 ug/mL
..LCMPFDA_00012	09/30/21	Wellington Laboratories, Lot MPFDA0916			(Purchased Reagent)		13C2 PFDA	50 ug/mL
..LCMPFHxA_00015	11/22/21	Wellington Laboratories, Lot MPFHxA1116			(Purchased Reagent)		13C2 PFHxA	50 ug/mL
LC537-L4_00022	09/30/18	04/02/18	MeOH/H2O, Lot 090285	5 mL	LC537-HSP_00028	360 uL	Perfluorobutanesulfonic acid (PFBS)	90.0619 ng/mL
							Perfluoroheptanoic acid (PFHpA)	9.72 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	30.2484 ng/mL
							Perfluorononanoic acid (PFNA)	19.8 ng/mL
							Perfluorooctanoic acid (PFOA)	19.8 ng/mL
							Perfluorooctanesulfonic acid (PFOS)	39.5328 ng/mL
					LC537-IS_00065	500 uL	13C2-PFOA	10 ng/mL
							13C4 PFOS	28.68 ng/mL
					LC537-SU_00064	500 uL	13C2 PFDA	10 ng/mL
							13C2 PFHxA	10 ng/mL
.LC537-HSP_00028	09/30/18	03/30/18	Methanol, Lot 104453	30 mL	LCPFBSA_00002	849 uL	Perfluorobutanesulfonic acid (PFBS)	1250.86 ng/mL
					LCPFHpA_00009	81 uL	Perfluoroheptanoic acid (PFHpA)	135 ng/mL
					LCPFHxS-br_00005	277 uL	Perfluorohexanesulfonic acid (PFHxS)	420.117 ng/mL
					LCPFNA_00009	165 uL	Perfluorononanoic acid (PFNA)	275 ng/mL
					LCPFOA_00010	165 uL	Perfluorooctanoic acid (PFOA)	275 ng/mL
					LCPFOS-br_00005	355 uL	Perfluorooctanesulfonic acid (PFOS)	549.067 ng/mL
..LCPFBSA_00002	12/02/21	Wellington Laboratories, Lot LPFBS1116			(Purchased Reagent)		Perfluorobutanesulfonic acid (PFBS)	44.2 ug/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-38382-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
..LCPFHpA_00009	12/02/21	Wellington Laboratories, Lot PFHpA1216			(Purchased Reagent)		Perfluoroheptanoic acid (PFHpA)	50 ug/mL
..LCPFHxS-br_00005	01/04/22	Wellington Laboratories, Lot brPFHxSK0117			(Purchased Reagent)		Perfluorohexanesulfonic acid (PFHxS)	45.5 ug/mL
..LCPFNA 00009	07/20/22	Wellington Laboratories, Lot PFNA0717			(Purchased Reagent)		Perfluorononanoic acid (PFNA)	50 ug/mL
..LCPFOA 00010	09/27/22	Wellington Laboratories, Lot PFOA0917			(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	50 ug/mL
..LCPFOS-br_00005	01/12/22	Wellington Laboratories, Lot brPFOSK0117			(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	46.4 ug/mL
..LC537-IS_00065	10/02/18	04/02/18	Methanol, Lot 090285	30000 uL	LCM2PFOA 00010	60 uL	13C2-PFOA	0.1 ug/mL
					LCMPFOS 00024	180 uL	13C4 PFOS	0.2868 ug/mL
..LCM2PFOA 00010	02/12/21	Wellington Laboratories, Lot M2PFOA0216			(Purchased Reagent)		13C2-PFOA	50 ug/mL
..LCMPFOS 00024	05/19/22	Wellington Laboratories, Lot MPFOS517			(Purchased Reagent)		13C4 PFOS	47.8 ug/mL
..LC537-SU_00064	10/02/18	04/02/18	Methanol, Lot 104453	30000 uL	LCMPFDA 00012	60 uL	13C2 PFDA	0.1 ug/mL
					LCMPFHxA 00015	60 uL	13C2 PFHxA	0.1 ug/mL
..LCMPFDA 00012	09/30/21	Wellington Laboratories, Lot MPFDA0916			(Purchased Reagent)		13C2 PFDA	50 ug/mL
..LCMPFHxA 00015	11/22/21	Wellington Laboratories, Lot MPFHxA1116			(Purchased Reagent)		13C2 PFHxA	50 ug/mL
LC537-L5_00026	09/30/18	04/02/18	MeOH/H2O, Lot 090285	20 mL	LC537-HSP_00028	2160 uL	Perfluorobutanesulfonic acid (PFBS)	135.093 ng/mL
							Perfluoroheptanoic acid (PFHpA)	14.58 ng/mL
							Perfluorohexanesulfonic acid (PFHxS)	45.3726 ng/mL
							Perfluorononanoic acid (PFNA)	29.7 ng/mL
							Perfluorooctanoic acid (PFOA)	29.7 ng/mL
							Perfluorooctanesulfonic acid (PFOS)	59.2992 ng/mL
					LC537-IS_00065	2 mL	13C2-PFOA	10 ng/mL
							13C4 PFOS	28.68 ng/mL
					LC537-SU_00064	2 mL	13C2 PFDA	10 ng/mL
							13C2 PFHxA	10 ng/mL
..LC537-HSP_00028	09/30/18	03/30/18	Methanol, Lot 104453	30 mL	LCPFBSA_00002	849 uL	Perfluorobutanesulfonic acid (PFBS)	1250.86 ng/mL
					LCPFHpA_00009	81 uL	Perfluoroheptanoic acid (PFHpA)	135 ng/mL
					LCPFHxS-br_00005	277 uL	Perfluorohexanesulfonic acid (PFHxS)	420.117 ng/mL
					LCPFNA 00009	165 uL	Perfluorononanoic acid (PFNA)	275 ng/mL
					LCPFOA 00010	165 uL	Perfluorooctanoic acid (PFOA)	275 ng/mL
					LCPFOS-br_00005	355 uL	Perfluorooctanesulfonic acid (PFOS)	549.067 ng/mL
..LCPFBSA_00002	12/02/21	Wellington Laboratories, Lot LPFBS1116			(Purchased Reagent)		Perfluorobutanesulfonic acid (PFBS)	44.2 ug/mL
..LCPFHpA_00009	12/02/21	Wellington Laboratories, Lot PFHpA1216			(Purchased Reagent)		Perfluoroheptanoic acid (PFHpA)	50 ug/mL
..LCPFHxS-br_00005	01/04/22	Wellington Laboratories, Lot brPFHxSK0117			(Purchased Reagent)		Perfluorohexanesulfonic acid (PFHxS)	45.5 ug/mL
..LCPFNA 00009	07/20/22	Wellington Laboratories, Lot PFNA0717			(Purchased Reagent)		Perfluorononanoic acid (PFNA)	50 ug/mL
..LCPFOA 00010	09/27/22	Wellington Laboratories, Lot PFOA0917			(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	50 ug/mL

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento

Job No.: 320-38382-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration		
					Reagent ID	Volume Added				
..LCPFOS-br_00005	01/12/22	Wellington Laboratories, Lot brPFOSK0117			(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	46.4 ug/mL		
.LC537-IS_00065	10/02/18	04/02/18	Methanol, Lot 090285	30000 uL	LCM2PFOA_00010	60 uL	13C2-PFOA	0.1 ug/mL		
					LCMPFOS_00024	180 uL	13C4 PFOS	0.2868 ug/mL		
..LCM2PFOA_00010	02/12/21	Wellington Laboratories, Lot M2PFOA0216			(Purchased Reagent)		13C2-PFOA	50 ug/mL		
..LCMPFOS_00024	05/19/22	Wellington Laboratories, Lot MPFOS517			(Purchased Reagent)		13C4 PFOS	47.8 ug/mL		
.LC537-SU_00064	10/02/18	04/02/18	Methanol, Lot 104453	30000 uL	LCMPFDA_00012	60 uL	13C2 PFDA	0.1 ug/mL		
					LCMPFHxA_00015	60 uL	13C2 PFHxA	0.1 ug/mL		
..LCMPFDA_00012	09/30/21	Wellington Laboratories, Lot MPFDA0916			(Purchased Reagent)		13C2 PFDA	50 ug/mL		
..LCMPFHxA_00015	11/22/21	Wellington Laboratories, Lot MPFHxA1116			(Purchased Reagent)		13C2 PFHxA	50 ug/mL		
LC537-L6_00022	09/30/18	04/02/18	MeOH/H2O, Lot 090285	5 mL	LC537-HSP_00028	720 uL	Perfluorobutanesulfonic acid (PFBS)	180.124 ng/mL		
							Perfluoroheptanoic acid (PFHpA)	19.44 ng/mL		
							Perfluorohexanesulfonic acid (PFHxS)	60.4968 ng/mL		
							Perfluorononanoic acid (PFNA)	39.6 ng/mL		
							Perfluorooctanoic acid (PFOA)	39.6 ng/mL		
							Perfluorooctanesulfonic acid (PFOS)	79.0656 ng/mL		
					LC537-IS_00065	500 uL	13C2-PFOA	10 ng/mL		
							13C4 PFOS	28.68 ng/mL		
					LC537-SU_00064	500 uL	13C2 PFDA	10 ng/mL		
							13C2 PFHxA	10 ng/mL		
.LC537-HSP_00028	09/30/18	03/30/18	Methanol, Lot 104453	30 mL	LCPFBSA_00002	849 uL	Perfluorobutanesulfonic acid (PFBS)	1250.86 ng/mL		
							LCPFHpA_00009	81 uL	Perfluoroheptanoic acid (PFHpA)	135 ng/mL
							LCPFHxS-br_00005	277 uL	Perfluorohexanesulfonic acid (PFHxS)	420.117 ng/mL
							LCPFNA_00009	165 uL	Perfluorononanoic acid (PFNA)	275 ng/mL
							LCPFOA_00010	165 uL	Perfluorooctanoic acid (PFOA)	275 ng/mL
					LCPFOS-br_00005	355 uL	Perfluorooctanesulfonic acid (PFOS)	549.067 ng/mL		
..LCPFBSA_00002	12/02/21	Wellington Laboratories, Lot LPFBS1116			(Purchased Reagent)		Perfluorobutanesulfonic acid (PFBS)	44.2 ug/mL		
..LCPFHpA_00009	12/02/21	Wellington Laboratories, Lot PFHpA1216			(Purchased Reagent)		Perfluoroheptanoic acid (PFHpA)	50 ug/mL		
..LCPFHxS-br_00005	01/04/22	Wellington Laboratories, Lot brPFHxSK0117			(Purchased Reagent)		Perfluorohexanesulfonic acid (PFHxS)	45.5 ug/mL		
..LCPFNA_00009	07/20/22	Wellington Laboratories, Lot PFNA0717			(Purchased Reagent)		Perfluorononanoic acid (PFNA)	50 ug/mL		
..LCPFOA_00010	09/27/22	Wellington Laboratories, Lot PFOA0917			(Purchased Reagent)		Perfluorooctanoic acid (PFOA)	50 ug/mL		
..LCPFOS-br_00005	01/12/22	Wellington Laboratories, Lot brPFOSK0117			(Purchased Reagent)		Perfluorooctanesulfonic acid (PFOS)	46.4 ug/mL		
.LC537-IS_00065	10/02/18	04/02/18	Methanol, Lot 090285	30000 uL	LCM2PFOA_00010	60 uL	13C2-PFOA	0.1 ug/mL		
					LCMPFOS_00024	180 uL	13C4 PFOS	0.2868 ug/mL		
..LCM2PFOA_00010	02/12/21	Wellington Laboratories, Lot M2PFOA0216			(Purchased Reagent)		13C2-PFOA	50 ug/mL		
..LCMPFOS_00024	05/19/22	Wellington Laboratories, Lot MPFOS517			(Purchased Reagent)		13C4 PFOS	47.8 ug/mL		
.LC537-SU_00064	10/02/18	04/02/18	Methanol, Lot 104453	30000 uL	LCMPFDA_00012	60 uL	13C2 PFDA	0.1 ug/mL		

REAGENT TRACEABILITY SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1


SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
					LCMPFHxA_00015	60 uL	13C2 PFHxA	0.1 ug/mL
..LCMPFDA_00012	09/30/21		Wellington Laboratories, Lot MPFDA0916		(Purchased Reagent)		13C2 PFDA	50 ug/mL
..LCMPFHxA_00015	11/22/21		Wellington Laboratories, Lot MPFHxA1116		(Purchased Reagent)		13C2 PFHxA	50 ug/mL
LC537-SU_00066	10/10/18	04/10/18	Methanol, Lot 104453	30000 uL	LCMPFDA_00012	60 uL	13C2 PFDA	0.1 ug/mL
					LCMPFHxA_00015	60 uL	13C2 PFHxA	0.1 ug/mL
.LCMPFDA_00012	09/30/21		Wellington Laboratories, Lot MPFDA0916		(Purchased Reagent)		13C2 PFDA	50 ug/mL
.LCMPFHxA_00015	11/22/21		Wellington Laboratories, Lot MPFHxA1116		(Purchased Reagent)		13C2 PFHxA	50 ug/mL

Reagent

LC537_PFB2_00002

P: 6.8.17 SW



CERTIFICATE OF ANALYSIS

The Power to Question

Catalog Number: sc-236187
Lot Number: F0917
Product Name: Nonafluorobutane-1-sulfonic acid
CAS Number: 375-73-5
Molecular Formula: $C_4HF_9O_3S$
Molecular Weight: 300.10

Test	Specification	Result
Appearance	Colorless liquid	Complies
Identification (19F-NMR)	Conforms to structure	Complies
Purity (Sodium Hydroxide Titration)	$\geq 97\%$	101.3%
Infrared Spectrum	Conforms to structure	Complies

Reagent

LC537_PFHpA2_00002

Certificate of analysis

R:6.13.17 SW

Product No.: A12092
Product: Perfluoroheptanoic acid, 98+%
Lot No.: 10200390

PFHpA

Appearance: White fused solid
Water Content (Karl-Fischer): 0.30%
Melting Point: 32.0-34.3°C
Assay (Aqueous acid-base titration): 99.7%
Identification (FTIR): Conforms

This document has been electronically generated and does not require a signature.

Order our products online www.alfa.com

ThermoFisher
SCIENTIFIC

Reagent

LC537_PFHxS2_00002

n: 6-E-17SKV




The Future is Custom

CERTIFICATE OF ANALYSIS

Catalog Number: sc-237289
 Lot Number: G2516
 Product Name: Tridecafluorohexane-1-sulfonic acid potassium salt
 CAS Number: 3871-99-6
 Molecular Formula: $C_6F_{13}KO_3S$
 Molecular Weight: 438.20

Test	Specification	Result
Appearance	White to faint beige powder or crystals	White powder
Identification (Infrared Spectrum)	Consistent with structure	Complies
Purity (Titration, Ion Exchange)	≥ 98.0%	100.4%

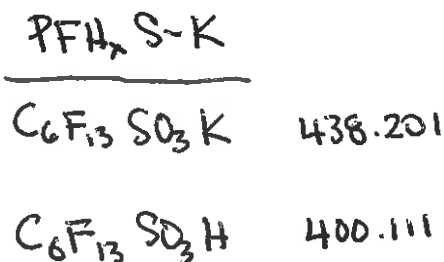

MW correction = $\frac{400.11}{438.201} = 0.91307$ PFH₂S
 cas# 355-46-4

Purity $\frac{1}{MW}$ correction = 90.9%

This document was produced electronically and is valid without a signature.

Reagent

LC537_PFN2_00002

17-6.14.17 SKW

3050 Spruce Street, Saint Louis, MO 63103, USA
Website: www.sigmaaldrich.com
Email USA: techserv@sial.com
Outside USA: eurtechserv@sial.com

Certificate of Analysis

Product Name:
Perfluorononanoic acid - 97%

Product Number: 394459
Batch Number: MKCC0699
Brand: ALDRICH
CAS Number: 375-95-1
MDL Number: MFCD00039605
Formula: C₉HF₁₇O₂
Formula Weight: 464.08 g/mol
Quality Release Date: 07 DEC 2016



Test	Specification	Result
Appearance (Color)	White to Off-White	White
Appearance (Form)	Powder or Crystals or Crystalline Chunk(s) or Granule or Flakes or Solid	Powder
Infrared Spectrum	Conforms to Structure	Conforms
GC (area %)	> 96.5 %	98.2 %

Michael Grady, Manager
Quality Control
Milwaukee, WI US

PFNA

Sigma-Aldrich warrants, that at the time of the quality release or subsequent retest date this product conformed to the information contained in this publication. The current Specification sheet may be available at Sigma-Aldrich.com. For further inquiries, please contact Technical Service. Purchaser must determine the suitability of the product for its particular use. See reverse side of invoice or packing slip for additional terms and conditions of sale.

Reagent

LC537_PFOA2_00002

Certificate of analysis

P: 6/9/17 

Product No.: L08862
Product: Perfluorooctanoic acid, 95%
Lot No.: 10199078

PFOA

Appearance: White powder
Water Content (Karl-Fischer): 1.30%
Melting Point: 47.6-54.0°C
Assay (Aqueous acid-base titration): 98.4%
Assay (GC Silyl Deriv): 97.2%

This document has been electronically generated and does not require a signature.

Order our products online www.alfa.com

ThermoFisher
SCIENTIFIC

Reagent

LC537_PFO2_00002

N: 6.14.17 SKV

Certificate of Analysis

Product Name: HEPTADEC AFLUORO OCTANESULFONIC ACID TETRAETHYLAMMONIUM SALT
 98 %
Product Number: 365289
Batch Number: BCBQ0108V
Brand: Aldrich
CAS Number: 56773-42-3
Formula: $CF_3(CF_2)_6CF_2SO_3N(C_2H_5)_4$
Formula Weight: 629.37
Quality Release Date: 11 JUN 2015


TEST	SPECIFICATION	RESULT
APPEARANCE (COLOR)	WHITE TO OFF WHITE	OFF-WHITE
APPEARANCE (FORM)	POWDER OR POWDER WITH CHUNK(S)	POWDER
CARBON CONTENT	29.77 % - 31.29 %	29.97 %
INFRARED SPECTRUM	CONFORMS TO STRUCTURE	CONFORMS

Claudia Geitner

Dr. Claudia Geitner
 Manager Quality Control
 Buchs, Switzerland

MW correction: $\frac{500.125}{629.37} = 0.7946$

Purity & MW correction = 77.87%

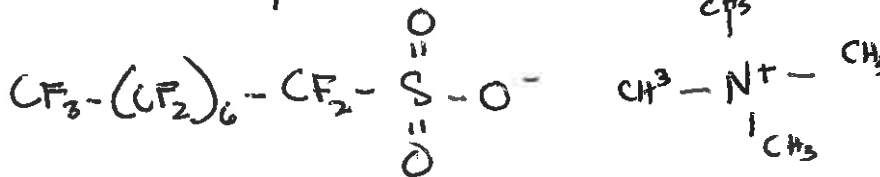

	$C_{17}F_{17}SO_3 + H$	$C_8H_{20}N$
C = 12.011	96.088	96.088
F = 18.998	322.966	—
S = 32.066	32.066	—
O = 16.999	47.997	—
H = 1.008	1.008	20.160
N = 14.007	—	14.007
	<hr/>	<hr/>
	500.125	130.255

Reagent

LCM2PFOA_00007




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: M2PFOA **LOT NUMBER:** M2PFOA0216
COMPOUND: Perfluoro-n-[1,2-¹³C₂]octanoic acid

STRUCTURE: **CAS #:** Not available

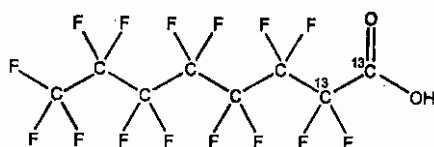

MOLECULAR FORMULA:	¹³ C ₂ ¹² C ₆ HF ₁₆ O ₂	MOLECULAR WEIGHT:	416.05
CONCENTRATION:	50 ± 2.5 µg/ml	SOLVENT(S):	Methanol Water (<1%)
CHEMICAL PURITY:	>98%	ISOTOPIC PURITY:	≥99% ¹³ C (1,2- ¹³ C ₂)
LAST TESTED: (mm/dd/yyyy)	02/12/2016		
EXPIRY DATE: (mm/dd/yyyy)	02/12/2021		
RECOMMENDED STORAGE:	Store ampoule in a cool, dark place		

DOCUMENTATION/ DATA ATTACHED:

Figure 1: LC/MS Data (TIC and Mass Spectrum)
 Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent conversion of the carboxylic acid to the methyl ester.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: 
 B.G. Chittim **Date:** 02/24/2016
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
 519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters

x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:


Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: M2PFOA; LC/MS Data (TIC and Mass Spectrum)

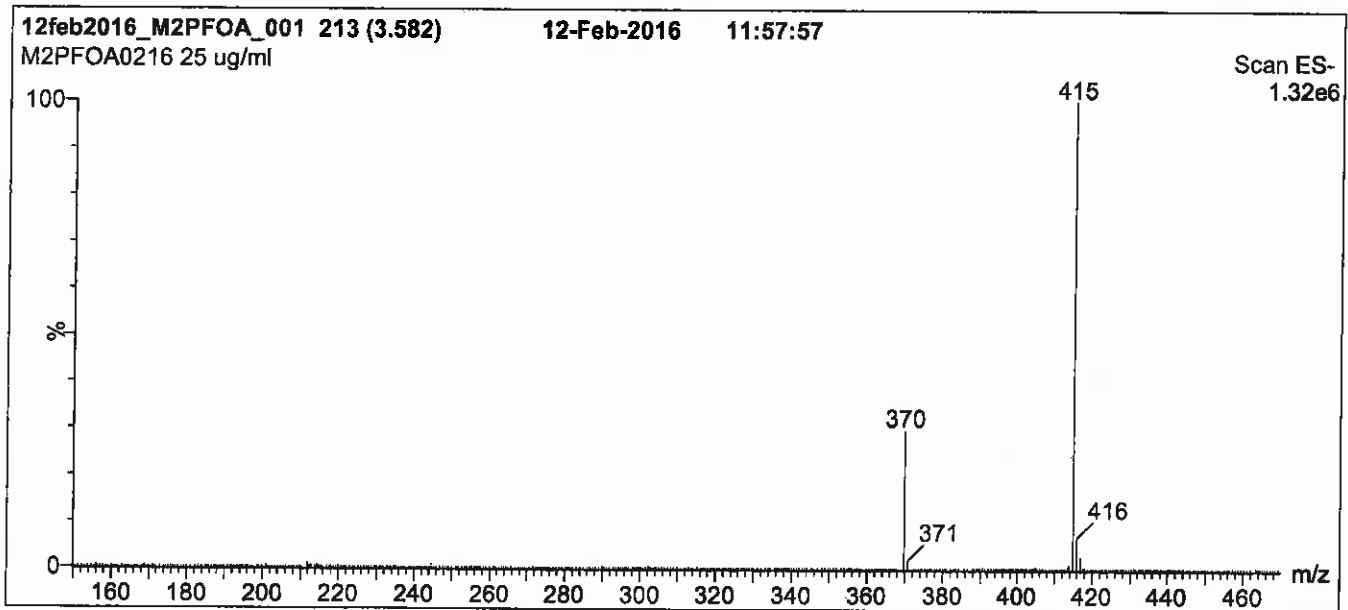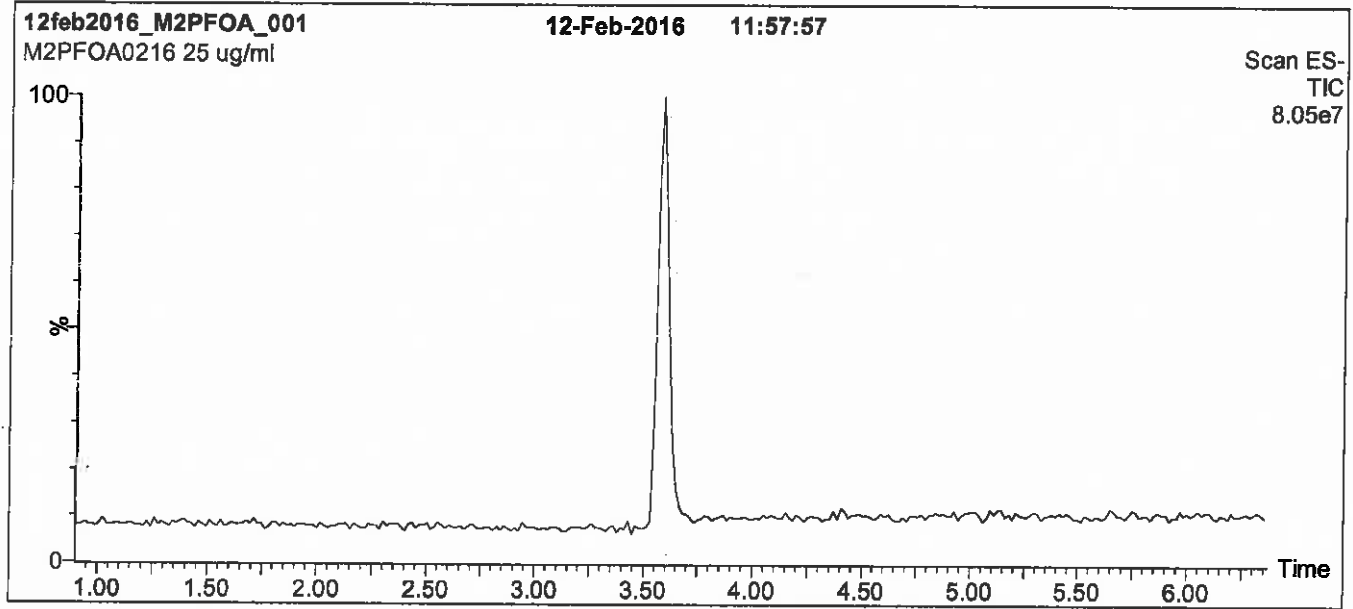

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
 1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
 Start: 50% (80:20 MeOH:ACN) / 50% H₂O
 (both with 10 mM NH₄OAc buffer)
 Ramp to 90% organic over 7.5 min and hold for 1.5 min
 before returning to initial conditions in 0.5 min.
 Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (150 - 850 amu)

Source: Electrospray (negative)
 Capillary Voltage (kV) = 3.00
 Cone Voltage (V) = 15.00
 Cone Gas Flow (l/hr) = 100
 Desolvation Gas Flow (l/hr) = 750

Figure 2: M2PFOA; LC/MS/MS Data (Selected MRM Transitions)

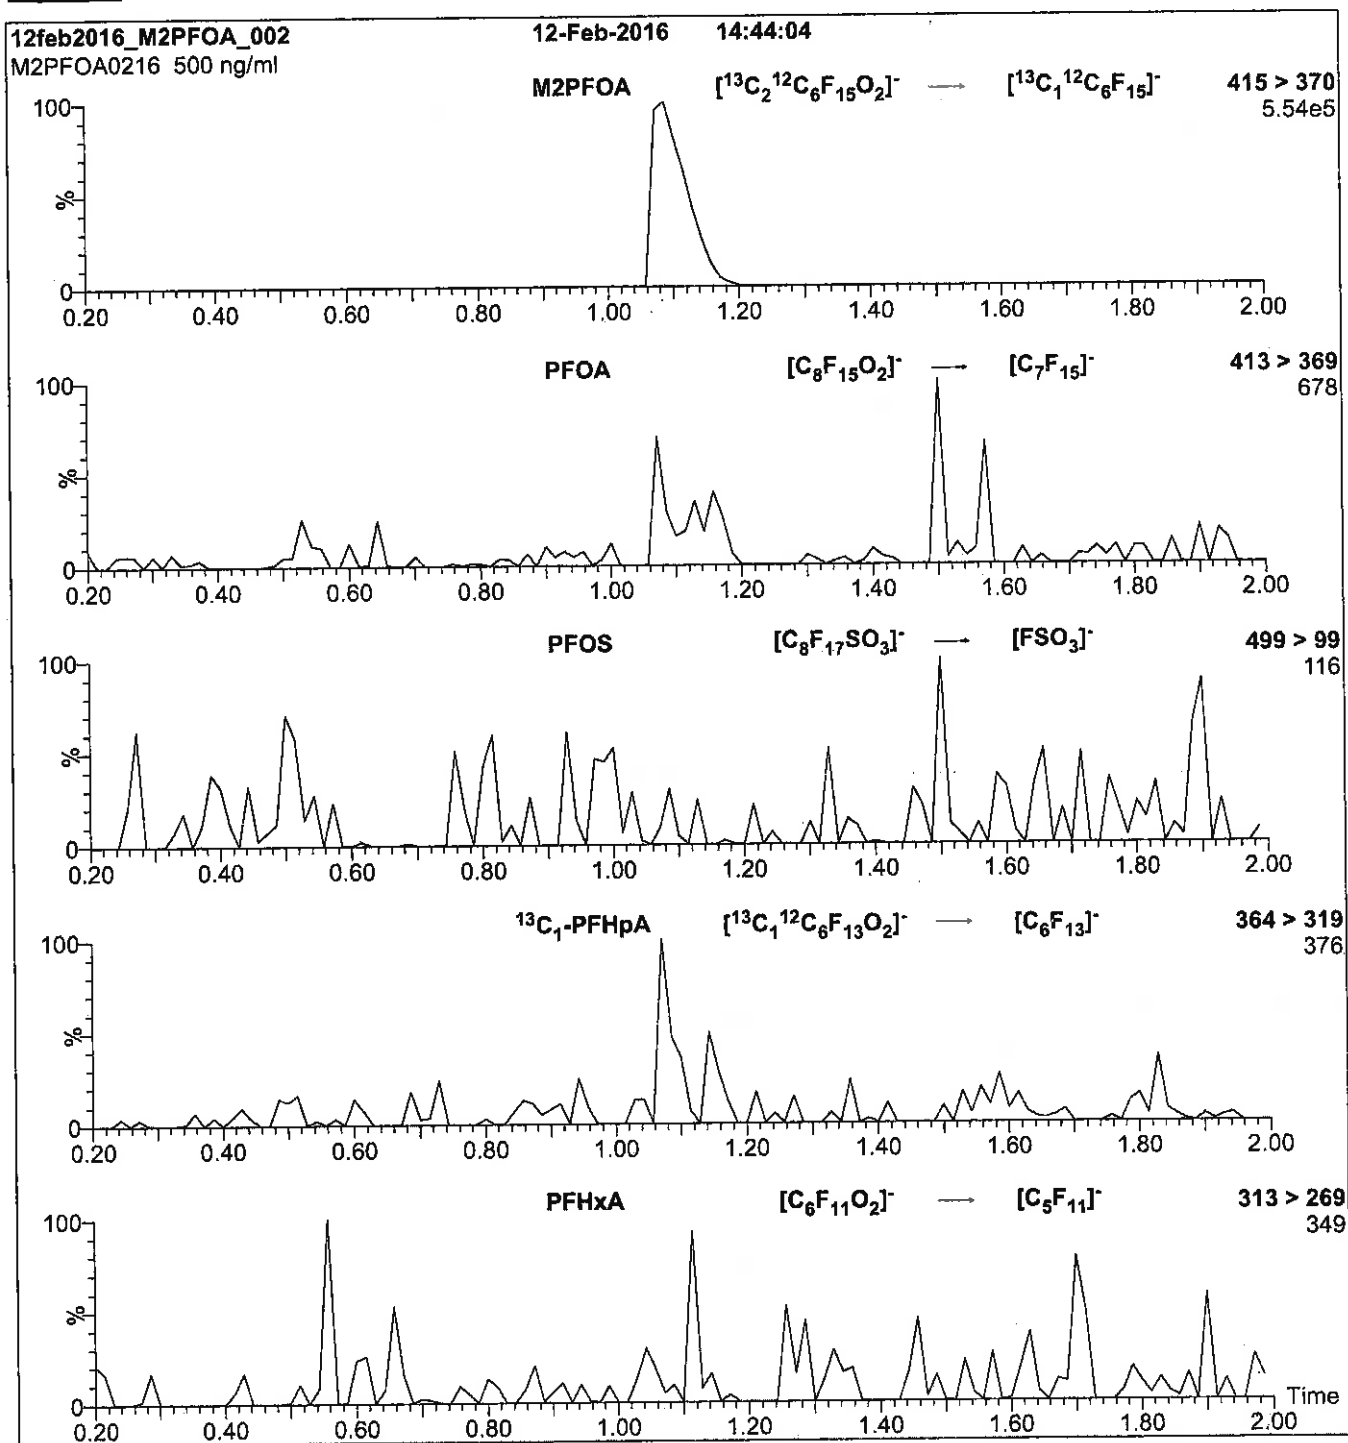

Conditions for Figure 2:

Injection: Direct loop injection
10 μl (500 ng/ml M2PFOA)

Mobile phase: Isocratic 80% MeOH / 20% H_2O

Flow: 300 $\mu\text{l}/\text{min}$

MS Parameters

Collision Gas (mbar) = 3.39e-3
Collision Energy (eV) = 10

Reagent

LCM2PFOA_00010




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: M2PFOA **LOT NUMBER:** M2PFOA0216
COMPOUND: Perfluoro-n-[1,2-¹³C₂]octanoic acid

STRUCTURE: **CAS #:** Not available

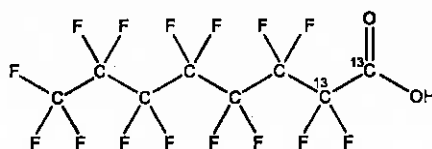

MOLECULAR FORMULA: ¹³C₂¹²C₈HF₁₆O₂
CONCENTRATION: 50 ± 2.5 µg/ml

MOLECULAR WEIGHT: 416.05
SOLVENT(S): Methanol
 Water (<1%)

CHEMICAL PURITY: >98%

ISOTOPIC PURITY: ≥99%¹³C
 (1,2-¹³C₂)

LAST TESTED: (mm/dd/yyyy) 02/12/2016

EXPIRY DATE: (mm/dd/yyyy) 02/12/2021

RECOMMENDED STORAGE: Store ampoule in a cool, dark place

DOCUMENTATION/ DATA ATTACHED:


Figure 1: LC/MS Data (TIC and Mass Spectrum)

Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent conversion of the carboxylic acid to the methyl ester.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: 
 B.G. Chittim **Date:** 02/24/2016
 (mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
 519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:


Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: M2PFOA; LC/MS Data (TIC and Mass Spectrum)

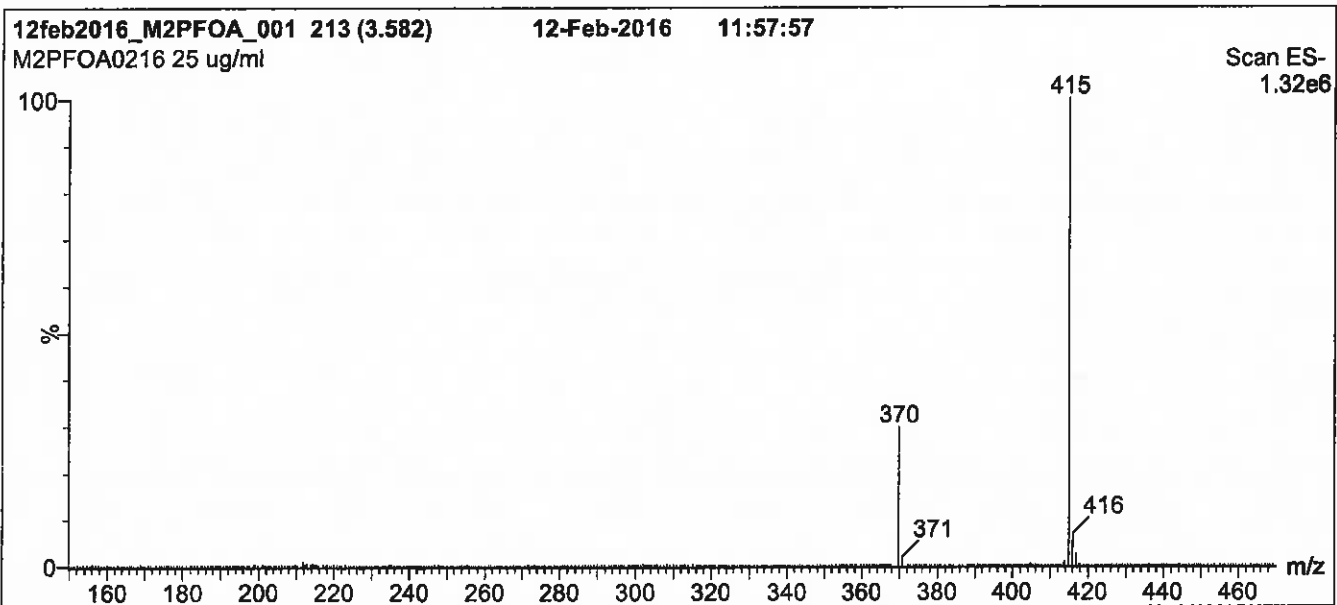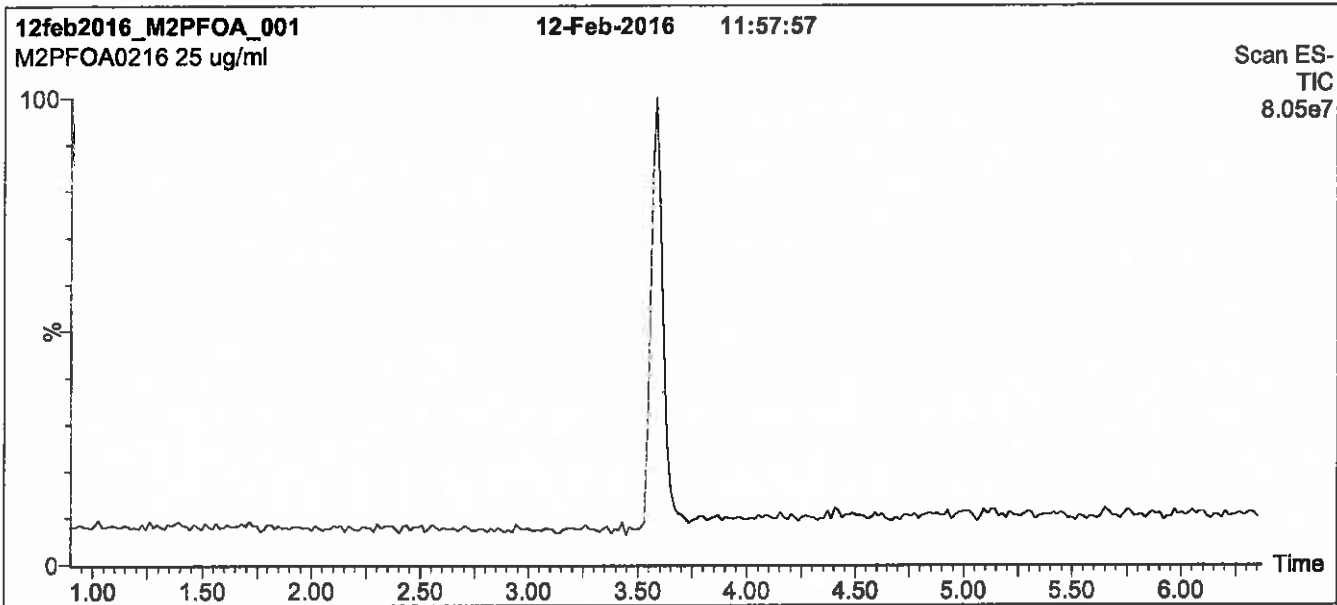

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
 1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
 Start: 50% (80:20 MeOH:ACN) / 50% H₂O
 (both with 10 mM NH₄OAc buffer)
 Ramp to 90% organic over 7.5 min and hold for 1.5 min
 before returning to initial conditions in 0.5 min.
 Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (150 - 850 amu)

Source: Electrospray (negative)
 Capillary Voltage (kV) = 3.00
 Cone Voltage (V) = 15.00
 Cone Gas Flow (l/hr) = 100
 Desolvation Gas Flow (l/hr) = 750

Figure 2: M2PFOA; LC/MS/MS Data (Selected MRM Transitions)

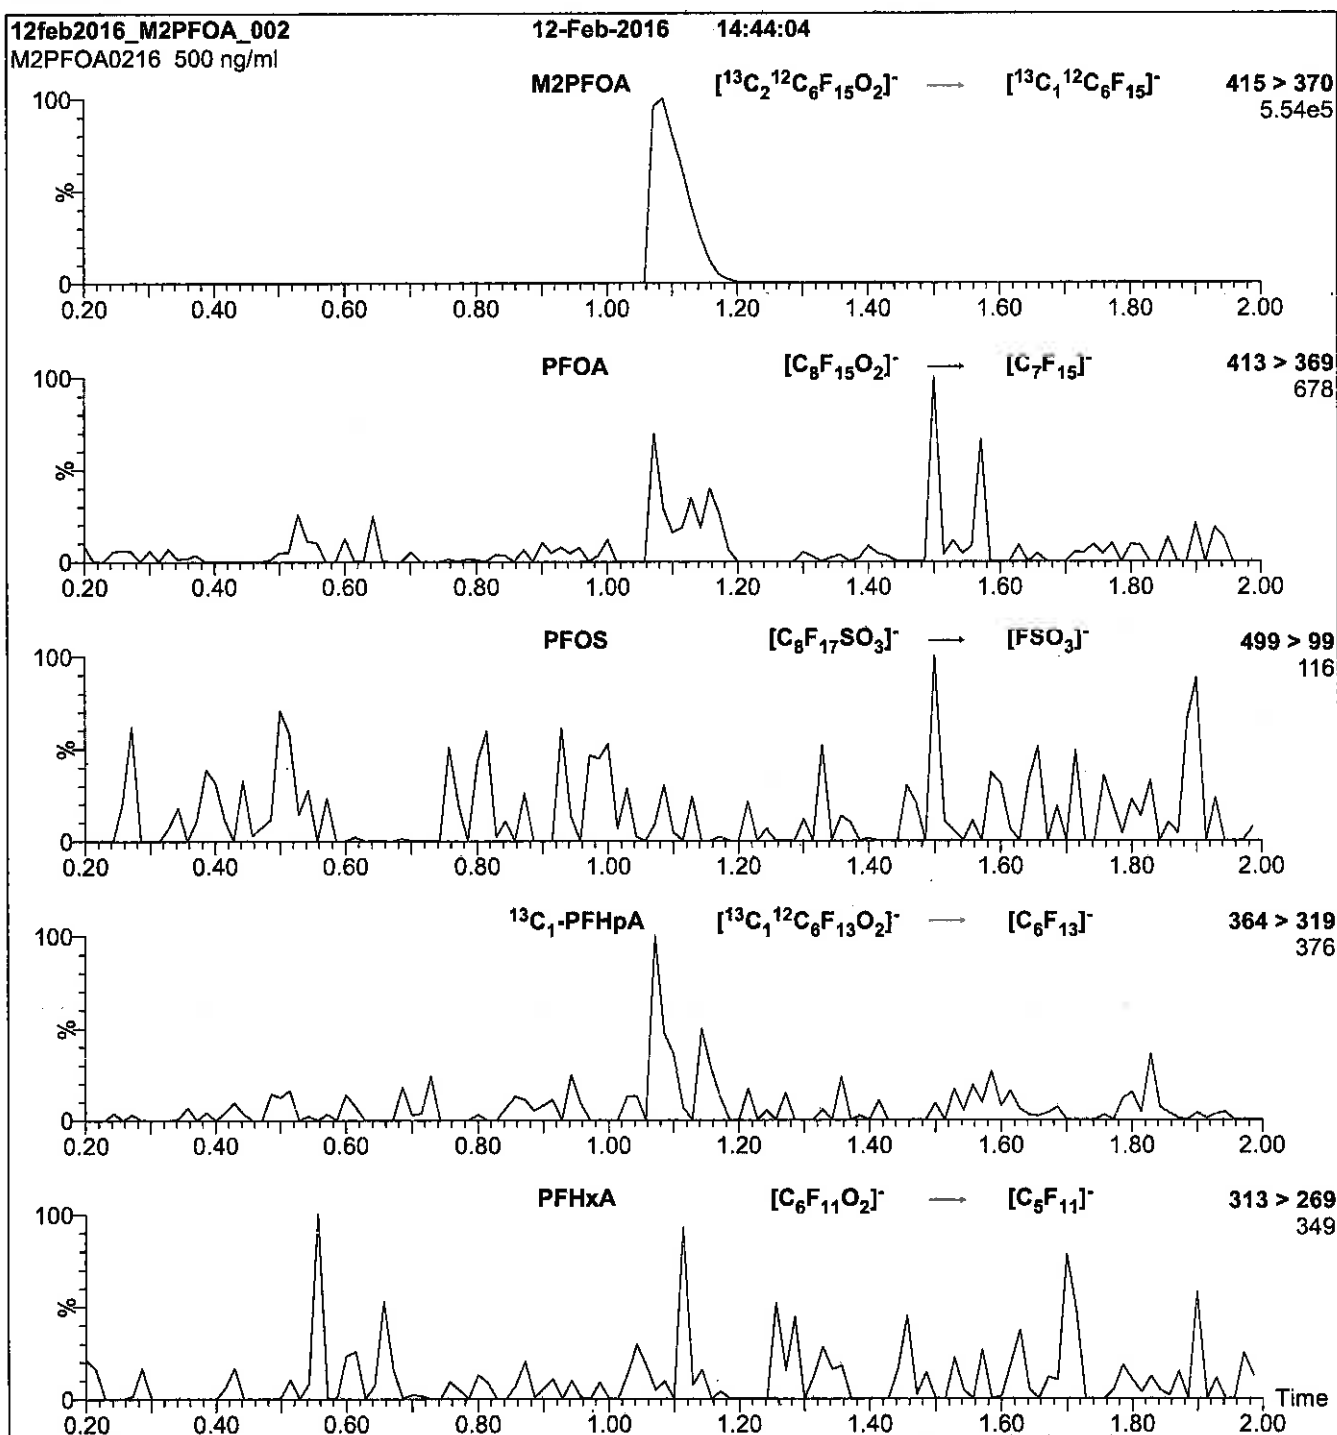

Conditions for Figure 2:

Injection: Direct loop injection
10 μl (500 ng/ml M2PFOA)

Mobile phase: Isocratic 80% MeOH / 20% H_2O

Flow: 300 $\mu\text{l}/\text{min}$

MS Parameters

Collision Gas (mbar) = 3.39e-3
Collision Energy (eV) = 10

Reagent

LCMPFDA_00012

R: SBC 12/21/16



814255

ID: LCMFDA_00012

Exp: 09/30/21 Prpd: SBC

13C2-Perfluorodecanoic a




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: MPFDA **LOT NUMBER:** MPFDA0916
COMPOUND: Perfluoro-n-[1,2-¹³C₂]decanoic acid

STRUCTURE: **CAS #:** Not available

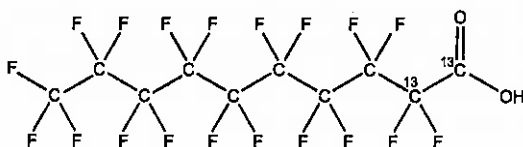

MOLECULAR FORMULA: ¹³C₂¹²C₈HF₁₉O₂
CONCENTRATION: 50 ± 2.5 µg/ml

MOLECULAR WEIGHT: 516.07
SOLVENT(S): Methanol
Water (<1%)

CHEMICAL PURITY: >98%

ISOTOPIC PURITY: ≥99% ¹³C
(1,2-¹³C₂)

LAST TESTED: (mm/dd/yyyy) 09/30/2016

EXPIRY DATE: (mm/dd/yyyy) 09/30/2021

RECOMMENDED STORAGE: Store ampoule in a cool, dark place

DOCUMENTATION/ DATA ATTACHED:

Figure 1: LC/MS Data (TIC and Mass Spectrum)

Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent conversion of the carboxylic acid to the methyl ester.
- Contains < 0.1% of ¹³C₁-PFNA.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By:
B.G. Chrftim

Date: 10/07/2016
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: MPFDA; LC/MS Data (TIC and Mass Spectrum)

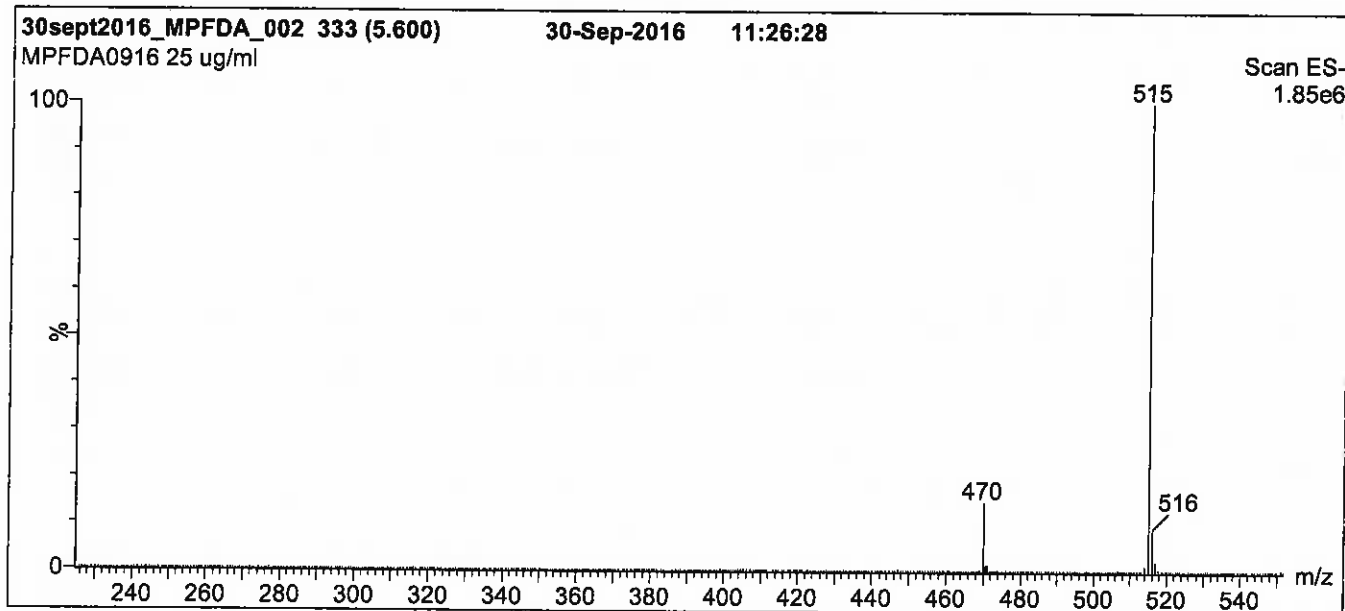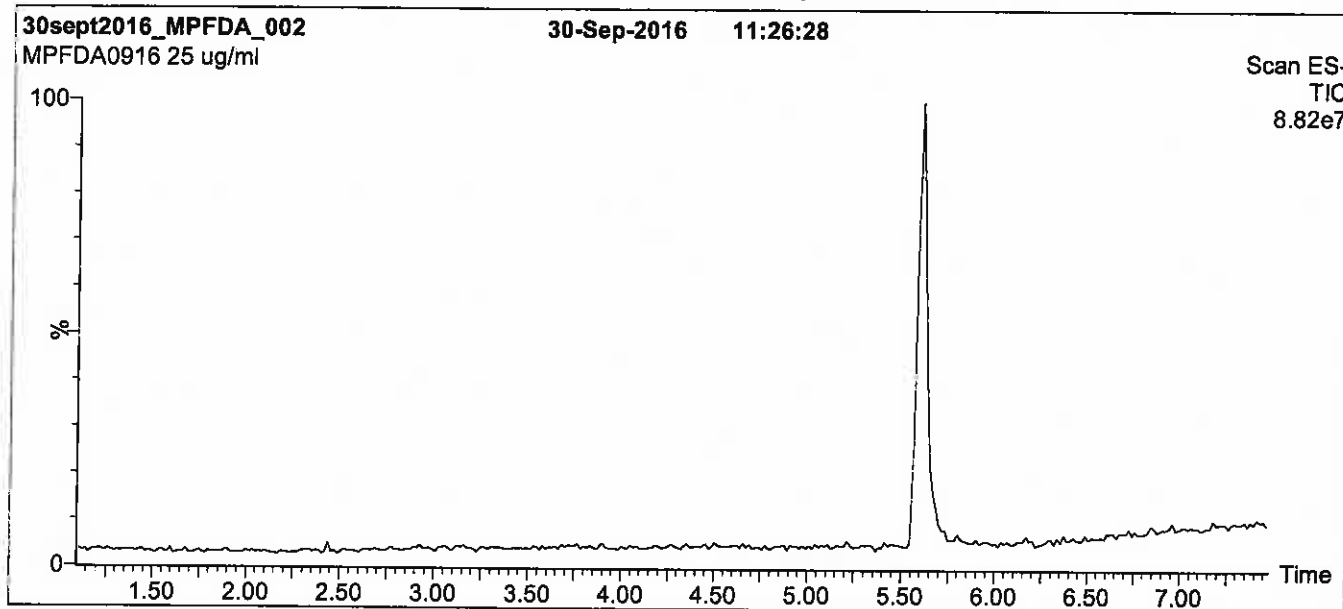

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm


Mobile phase: Gradient
Start: 50% (80:20 MeOH:ACN) / 50% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 90% organic over 7 min and hold for 1.5 min
before returning to initial conditions in 0.5 min.
Time: 10 min

Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (225 - 850 amu)
Source: Electrospray (negative)
Capillary Voltage (kV) = 2.00
Cone Voltage (V) = 15.00
Cone Gas Flow (l/hr) = 50
Desolvation Gas Flow (l/hr) = 750

Figure 2: MPFDA; LC/MS/MS Data (Selected MRM Transitions)

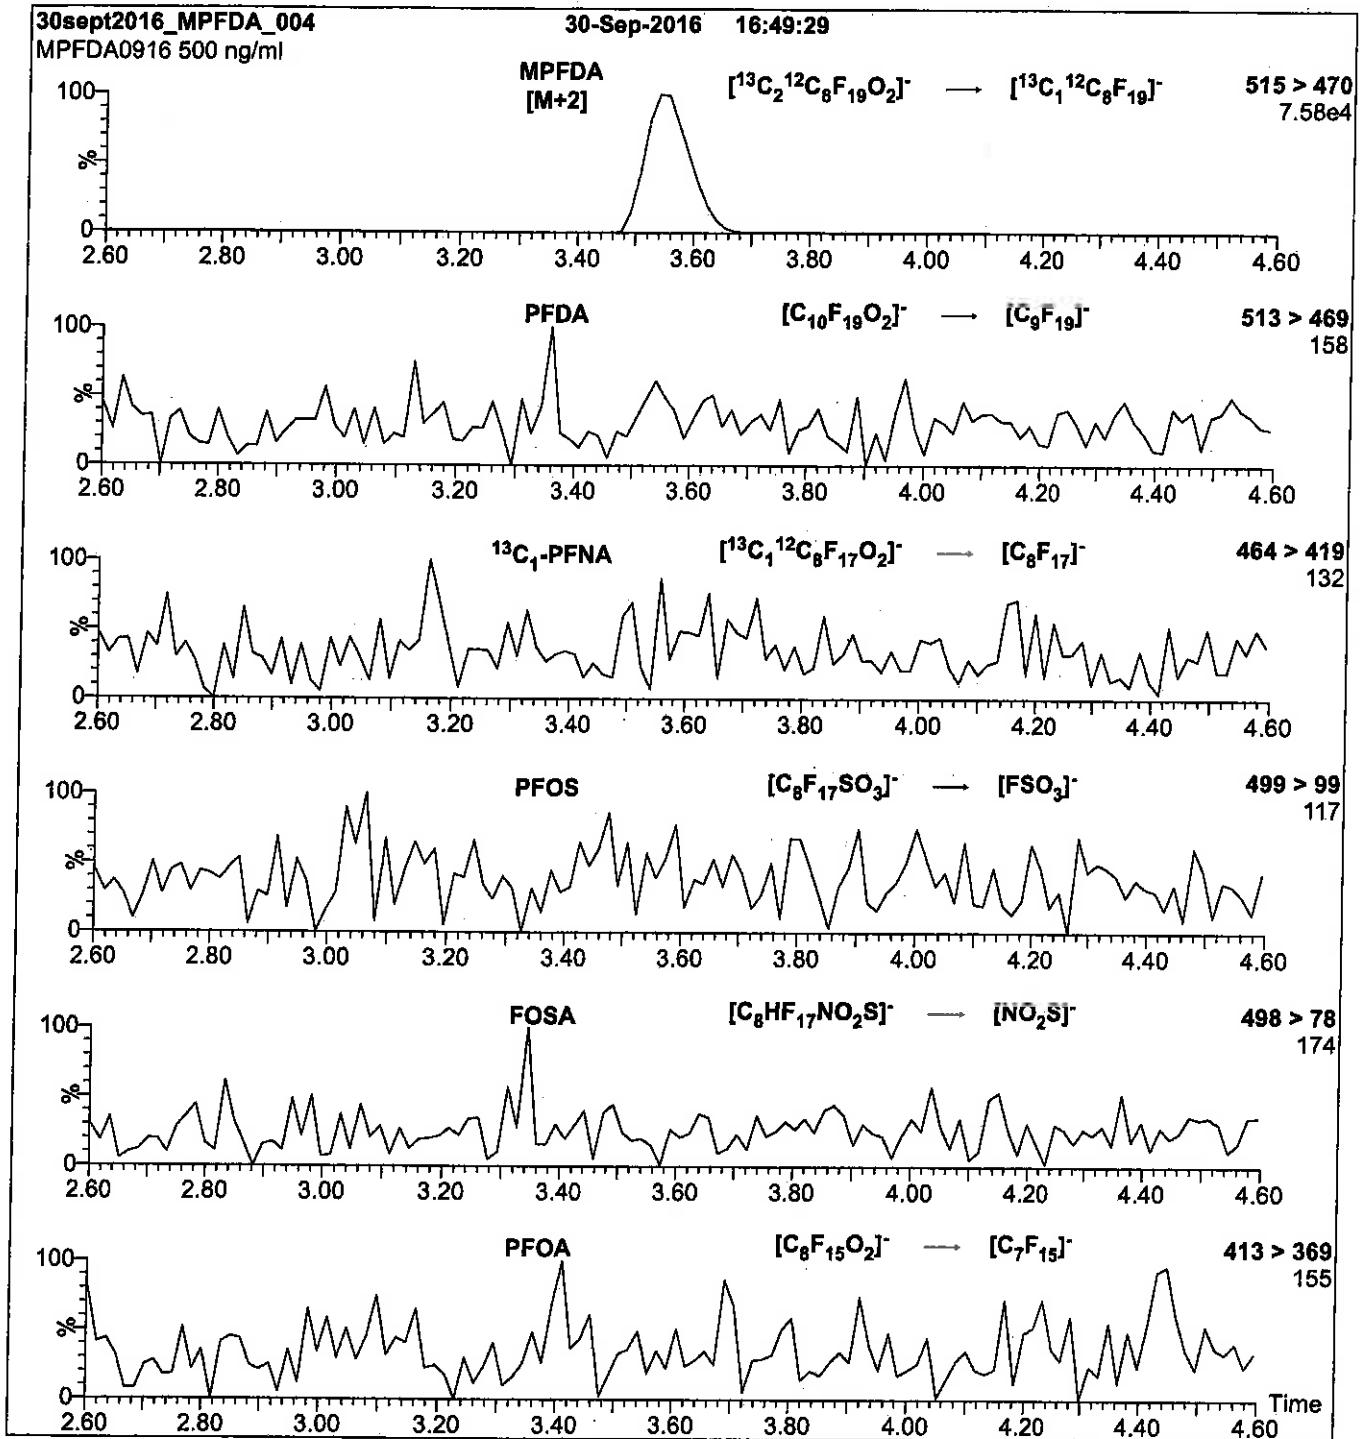

Conditions for Figure 2:

Injection: Direct loop injection
10 μ l (500 ng/ml MPFDA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
(both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.31e-3
Collision Energy (eV) = 13

Reagent

LCMPFHxA_00015


r: 5/15/17 SKJ



WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: MPFHxA **LOT NUMBER:** MPFHxA1116
COMPOUND: Perfluoro-n-[1,2-¹³C₂]hexanoic acid
STRUCTURE: **CAS #:** Not available

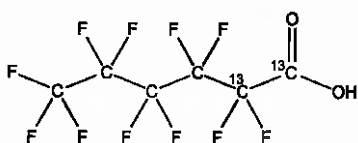

MOLECULAR FORMULA:	¹³ C ₂ ¹² C ₄ HF ₁₁ O ₂	MOLECULAR WEIGHT:	316.04
CONCENTRATION:	50 ± 2.5 µg/ml	SOLVENT(S):	Methanol Water (<1%)
CHEMICAL PURITY:	>98%	ISOTOPIC PURITY:	≥99% ¹³ C (1,2- ¹³ C ₂)
LAST TESTED: (mm/dd/yyyy)	11/22/2016		
EXPIRY DATE: (mm/dd/yyyy)	11/22/2021		
RECOMMENDED STORAGE:	Store ampoule in a cool, dark place		


DOCUMENTATION/ DATA ATTACHED:

Figure 1: LC/MS Data (TIC and Mass Spectrum)
 Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent conversion of the carboxylic acid to the methyl ester.
- Contains < 0.1% of perfluoro-n-hexanoic acid and ~ 0.3% of perfluoro-n-octanoic acid.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By:  **Date:** 12/13/2016
 B.G. Chittim (mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
 519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:


Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: MPFHxA; LC/MS Data (TIC and Mass Spectrum)

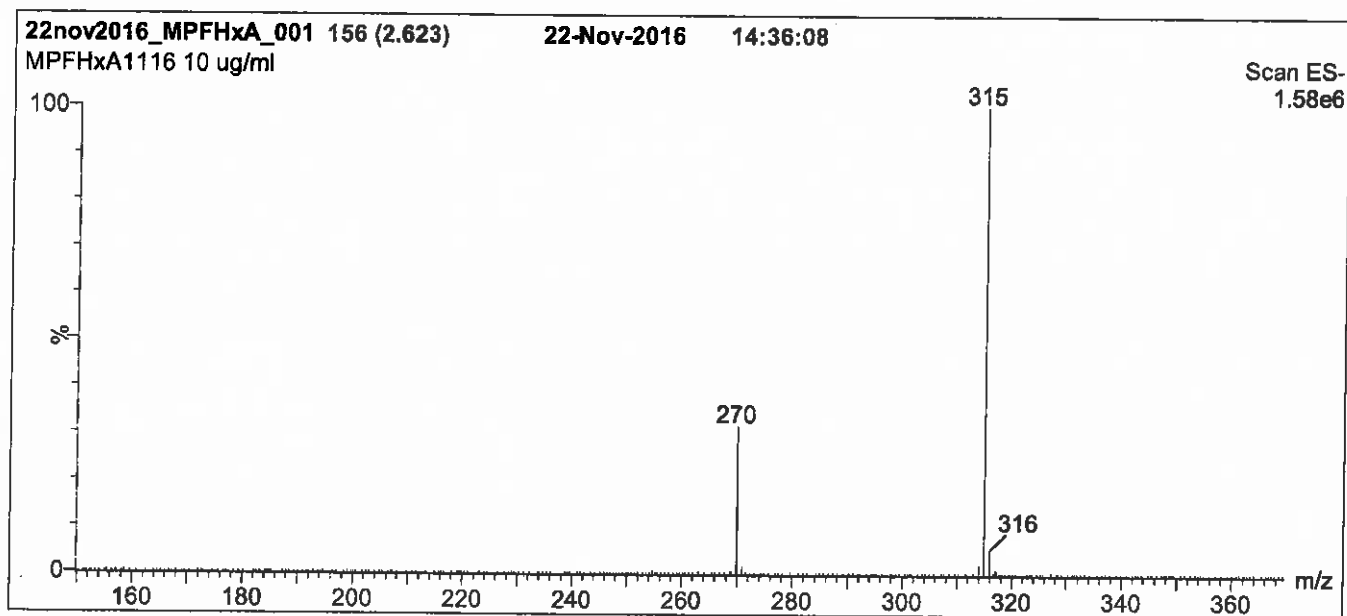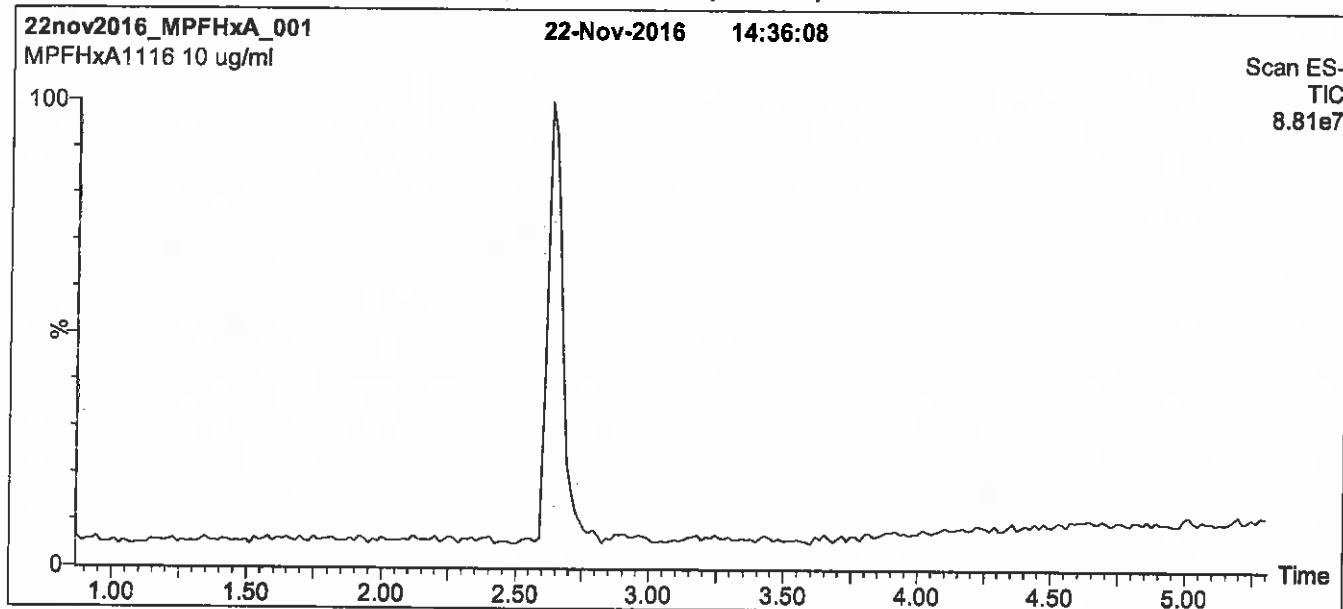

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm


Mobile phase: Gradient
Start: 40% (80:20 MeOH:ACN) / 60% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 90% organic over 7 min and hold for 2 min
before returning to initial conditions over 0.5 min.
Time: 10 min

Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (150 - 850 amu)
Source: Electrospray (negative)
Capillary Voltage (kV) = 2.00
Cone Voltage (V) = 15.00
Cone Gas Flow (l/hr) = 100
Desolvation Gas Flow (l/hr) = 750

Figure 2: MPFHxA; LC/MS/MS Data (Selected MRM Transitions)

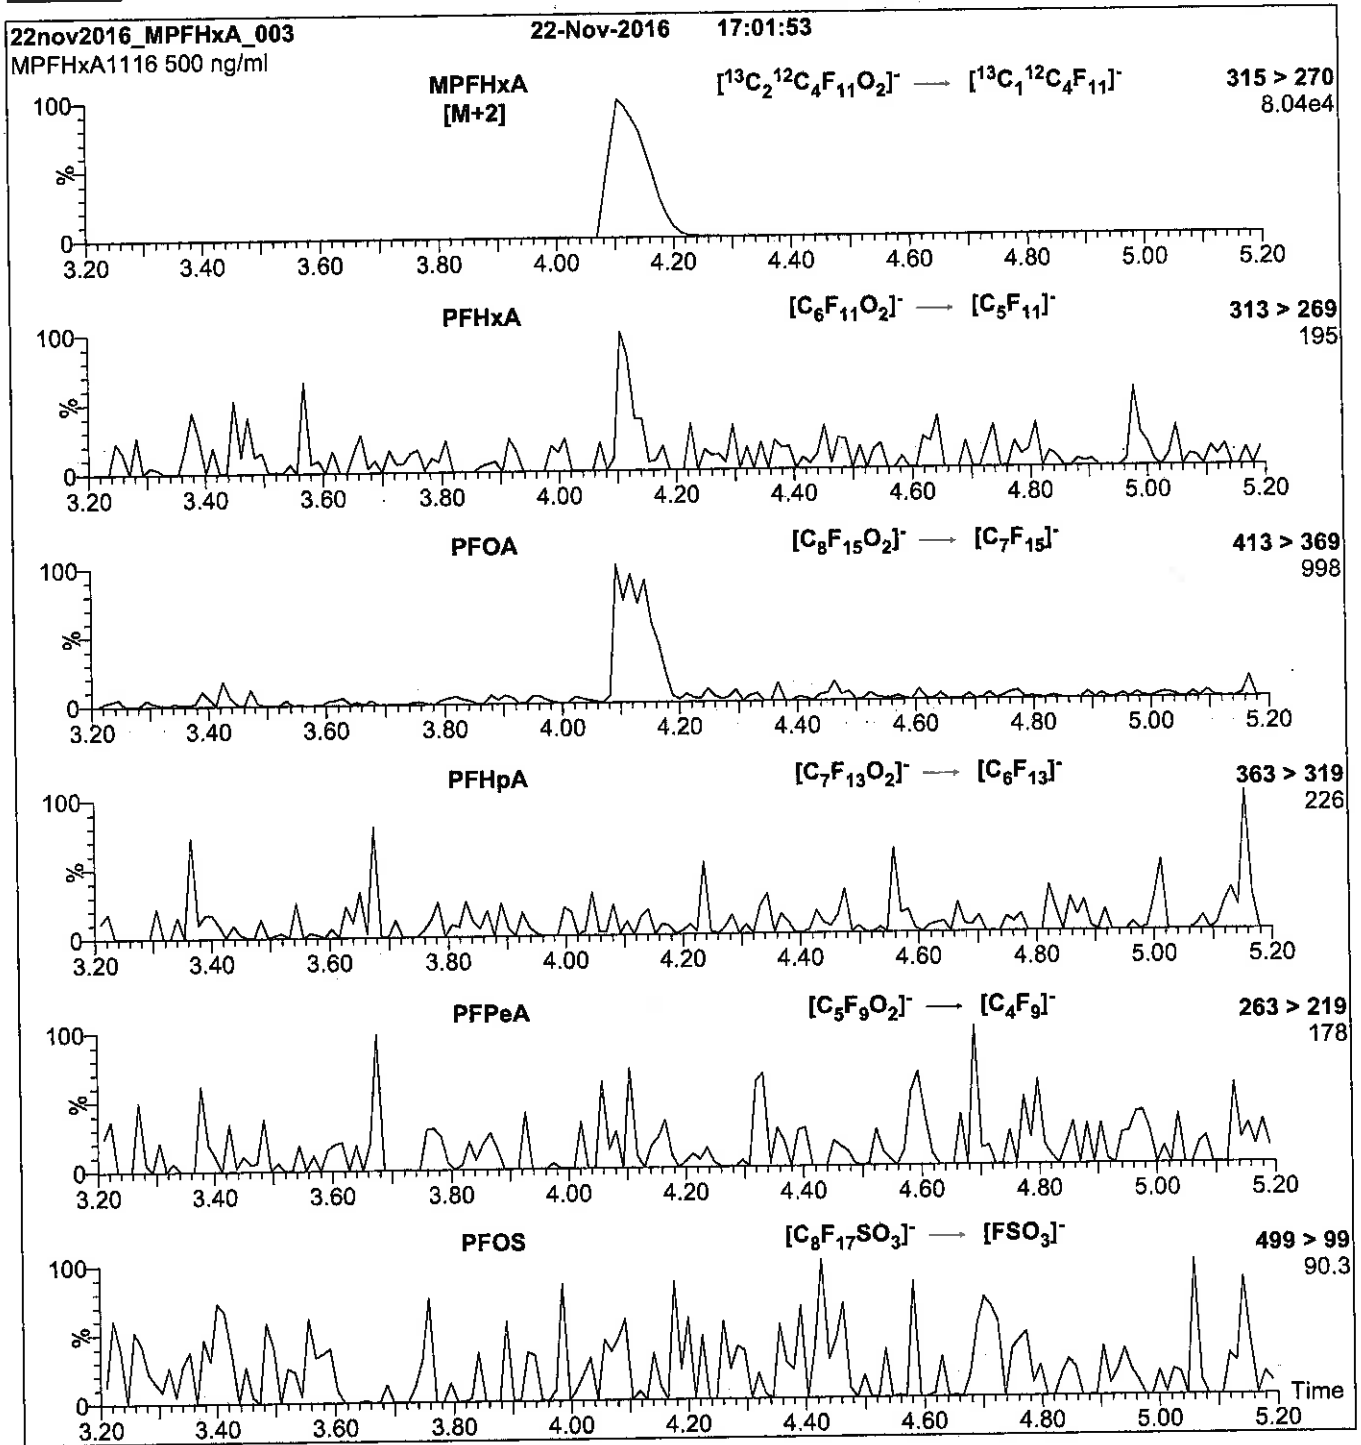

Conditions for Figure 2:

Injection: Direct loop injection
 10 μ l (500 ng/ml MPFHxA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
 (both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.46e-3
 Collision Energy (eV) = 10

Reagent

LCMPFOS_00021

r: 5/6/17 skv




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: MPFOS **LOT NUMBER:** MPFOS1216
COMPOUND: Sodium perfluoro-1-[1,2,3,4-¹³C₄]octanesulfonate

STRUCTURE: **CAS #:** Not available

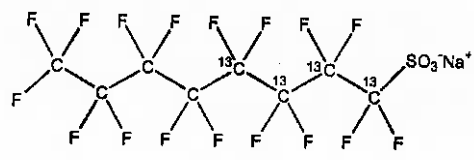

MOLECULAR FORMULA:	¹³ C ₄ ¹² C ₄ F ₁₇ SO ₃ Na	MOLECULAR WEIGHT:	526.08
CONCENTRATION:	50.0 ± 2.5 µg/ml (Na salt) 47.8 ± 2.4 µg/ml (MPFOS anion)	SOLVENT(S):	Methanol
CHEMICAL PURITY:	>98%	ISOTOPIC PURITY:	≥99% ¹³ C (1,2,3,4- ¹³ C ₄)
LAST TESTED: (mm/dd/yyyy)	12/12/2016		
EXPIRY DATE: (mm/dd/yyyy)	12/12/2021		
RECOMMENDED STORAGE:	Store ampoule in a cool, dark place		


DOCUMENTATION/ DATA ATTACHED:

- Figure 1: LC/MS Data (TIC and Mass Spectrum)
- Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains ~ 0.8% Sodium perfluoro-1-[1,2,3-¹³C₃]heptanesulfonate.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By:  **Date:** 12/14/2016
 B.G. Chrifim (mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
 519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: MPFOS; LC/MS Data (TIC and Mass Spectrum)

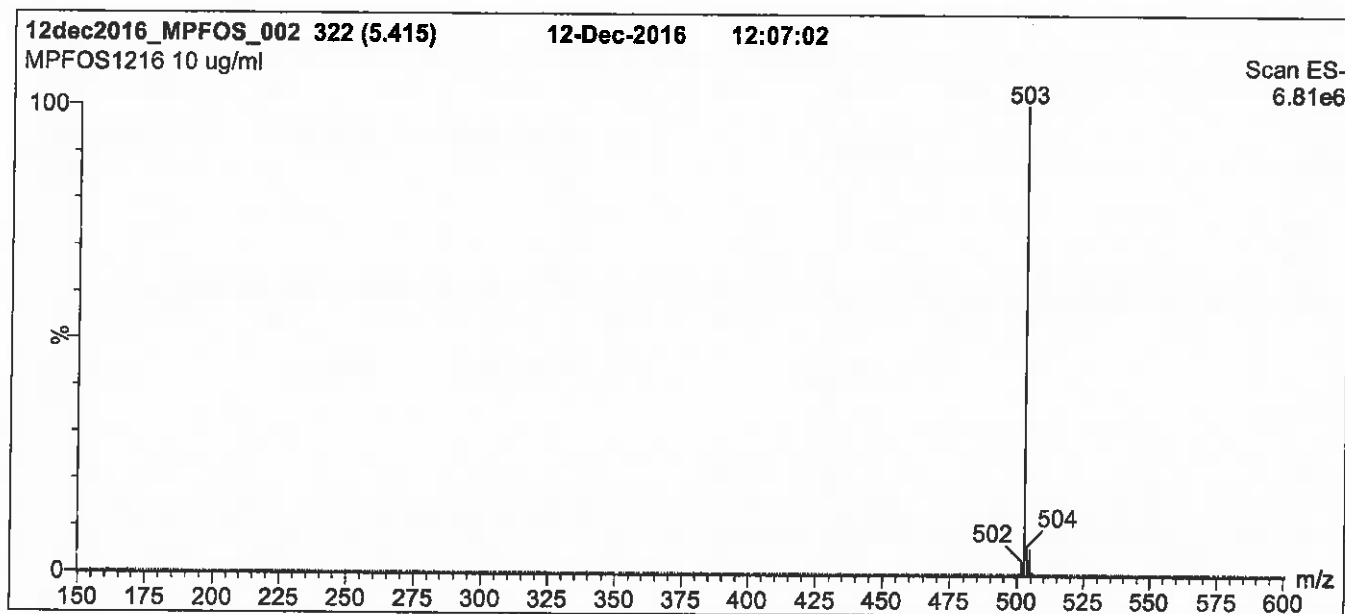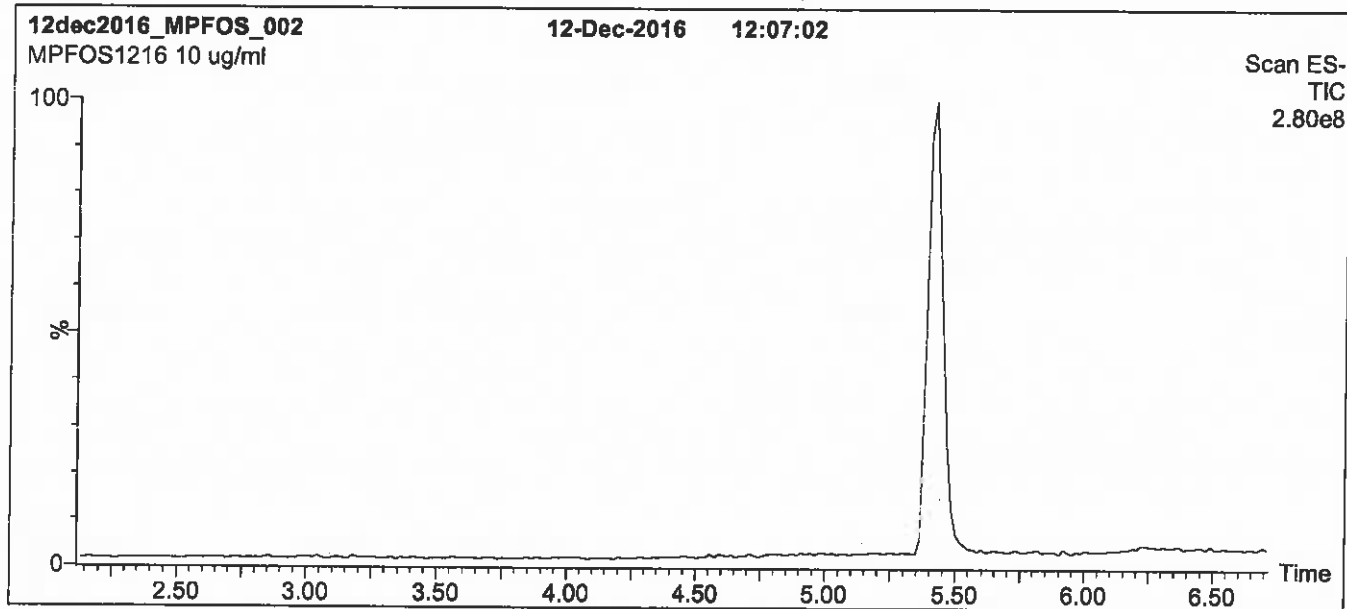

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
Start: 50% (80:20 MeOH:ACN) / 50% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 85% organic over 7.5 min and hold for 1.5 min
before returning to initial conditions in 0.5 min.
Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (150 - 850 amu)

Source: Electrospray (negative)
Capillary Voltage (kV) = 3.00
Cone Voltage (V) = 60.00
Cone Gas Flow (l/hr) = 50
Desolvation Gas Flow (l/hr) = 750

Figure 2: MPFOS; LC/MS/MS Data (Selected MRM Transitions)

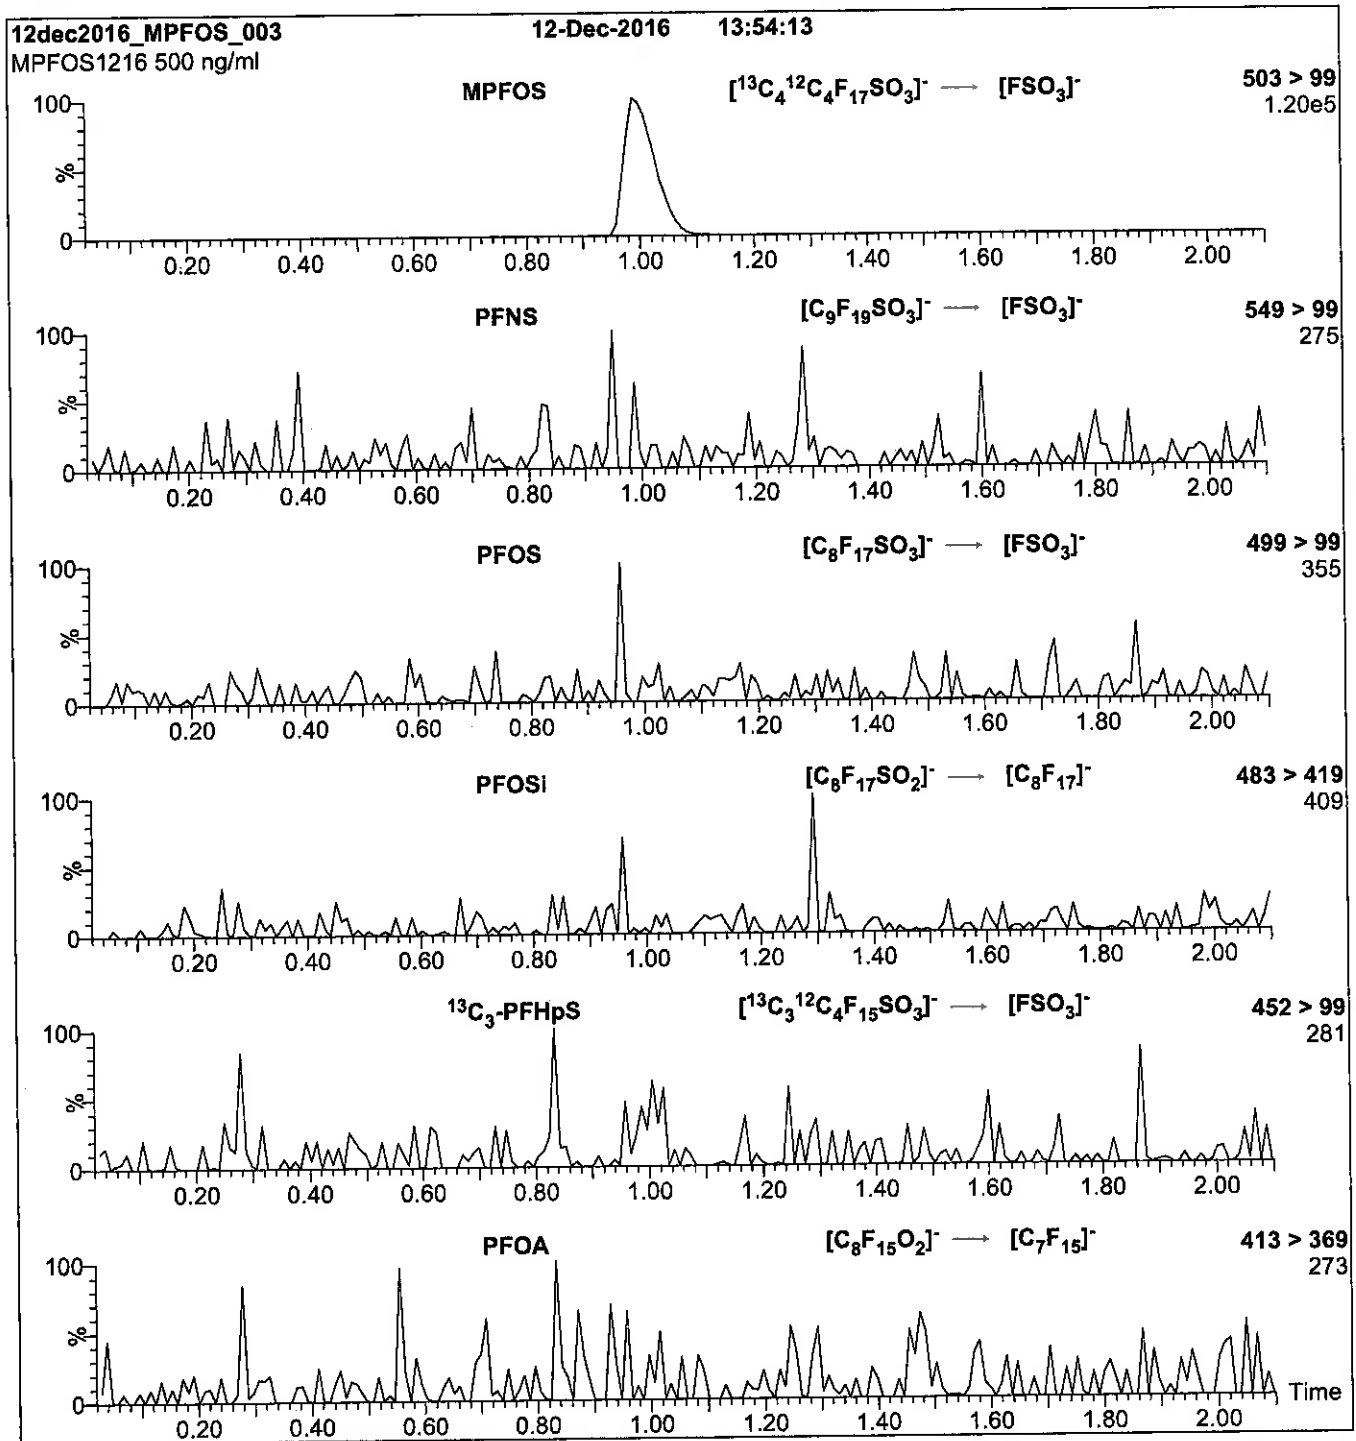

Conditions for Figure 2:

Injection: Direct loop injection
 10 μl (500 ng/ml MPFOS)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H_2O
 (both with 10 mM NH_4OAc buffer)

Flow: 300 $\mu\text{l}/\text{min}$

MS Parameters

Collision Gas (mbar) = 3.35e-3
 Collision Energy (eV) = 40

Reagent

LCMPFOS_00024

r: skln skj




**WELLINGTON
LABORATORIES**

**CERTIFICATE OF ANALYSIS
DOCUMENTATION**

PRODUCT CODE: MPFOS **LOT NUMBER:** MPFOS0517
COMPOUND: Sodium perfluoro-1-[1,2,3,4-¹³C₄]octanesulfonate

STRUCTURE: **CAS #:** Not available

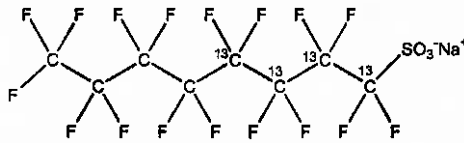

MOLECULAR FORMULA: ¹³C₄¹²C₄F₁₇SO₃Na **MOLECULAR WEIGHT:** 526.08
CONCENTRATION: 50.0 ± 2.5 µg/ml (Na salt) **SOLVENT(S):** Methanol
47.8 ± 2.4 µg/ml (MPFOS anion)
CHEMICAL PURITY: >98% **ISOTOPIC PURITY:** ≥99% ¹³C
LAST TESTED: (mm/dd/yyyy) 05/19/2017 (1,2,3,4-¹³C₄)
EXPIRY DATE: (mm/dd/yyyy) 05/19/2022
RECOMMENDED STORAGE: Store ampoule in a cool, dark place


DOCUMENTATION/ DATA ATTACHED:

Figure 1: LC/MS Data (TIC and Mass Spectrum)
Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains ~ 0.8% Sodium perfluoro-1-[1,2,3-¹³C₃]heptanesulfonate.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By:  **Date:** 05/30/2017
B.G. Chittim, General Manager (mm/dd/yyyy)

**Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com**

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers. In order to maintain the integrity of the assigned value(s), and associated uncertainty, the dilution or injection of a subsample of this product should be performed using calibrated measuring equipment.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using calibrated NIST and/or NRC traceable external weights. All volumetric glassware used is calibrated, of Class A tolerance, and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: MPFOS; LC/MS Data (TIC and Mass Spectrum)

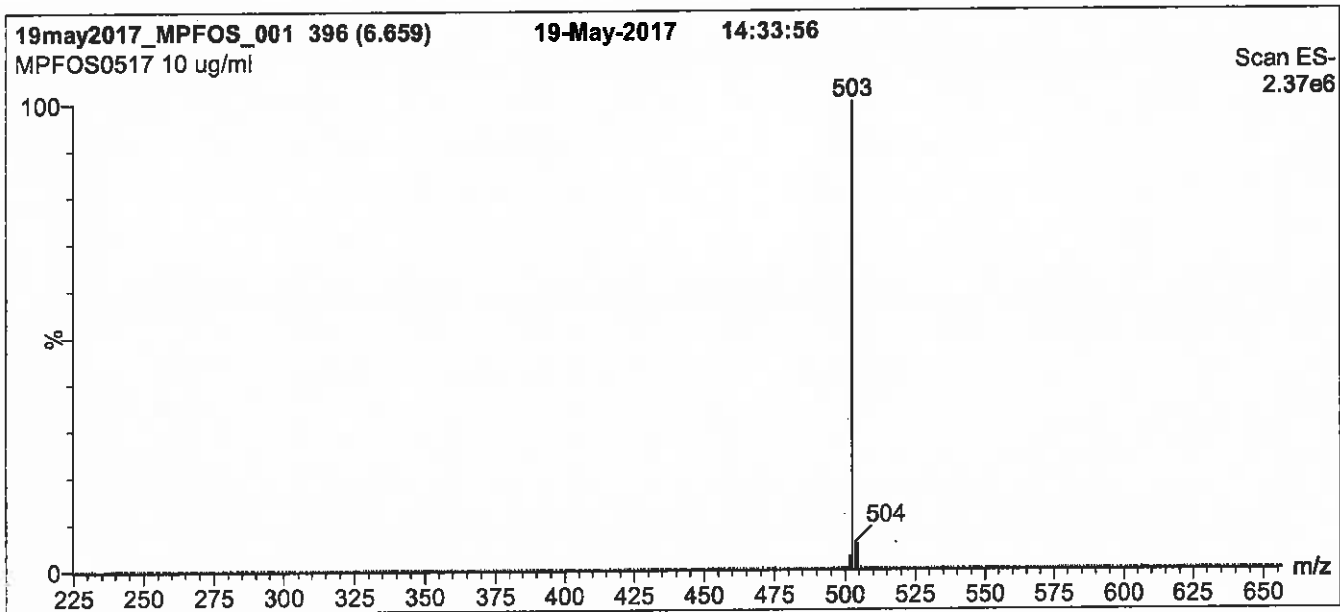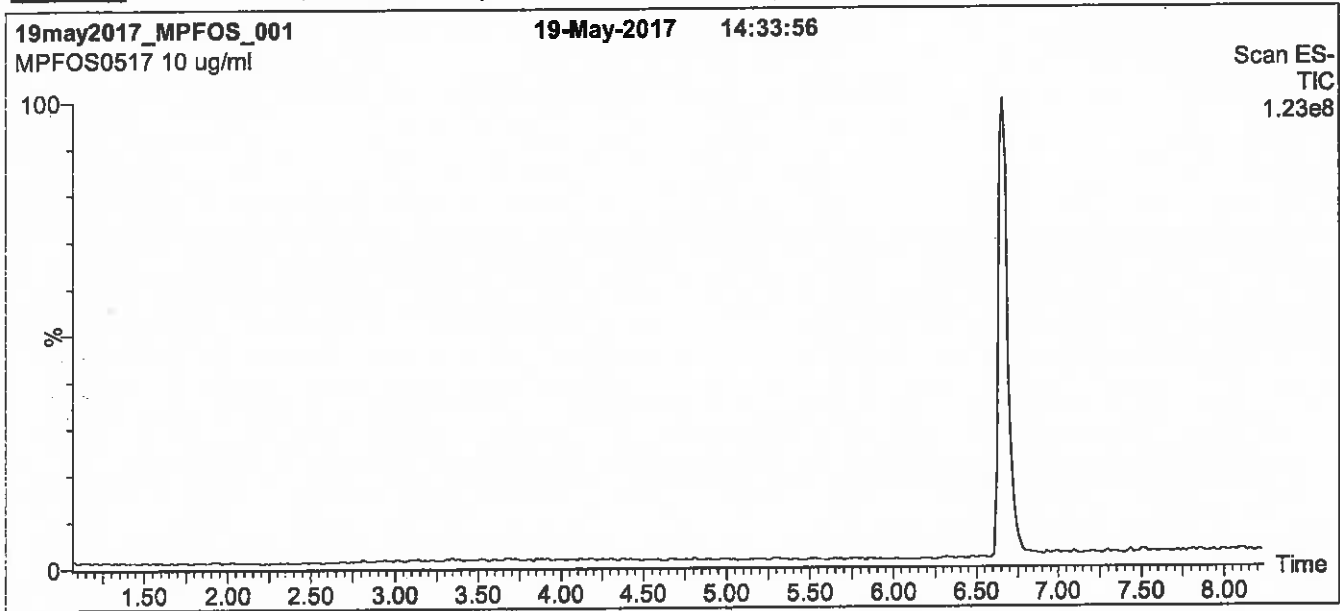

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
 1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
 Start: 50% (80:20 MeOH:ACN) / 50% H₂O
 (both with 10 mM NH₄OAc buffer)
 Ramp to 90% organic over 8 min and hold for 1 min
 before returning to initial conditions in 0.5 min.
 Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (225 - 850 amu)

Source: Electrospray (negative)
 Capillary Voltage (kV) = 3.00
 Cone Voltage (V) = 60.00
 Cone Gas Flow (l/hr) = 50
 Desolvation Gas Flow (l/hr) = 750

Figure 2: MPFOS; LC/MS/MS Data (Selected MRM Transitions)

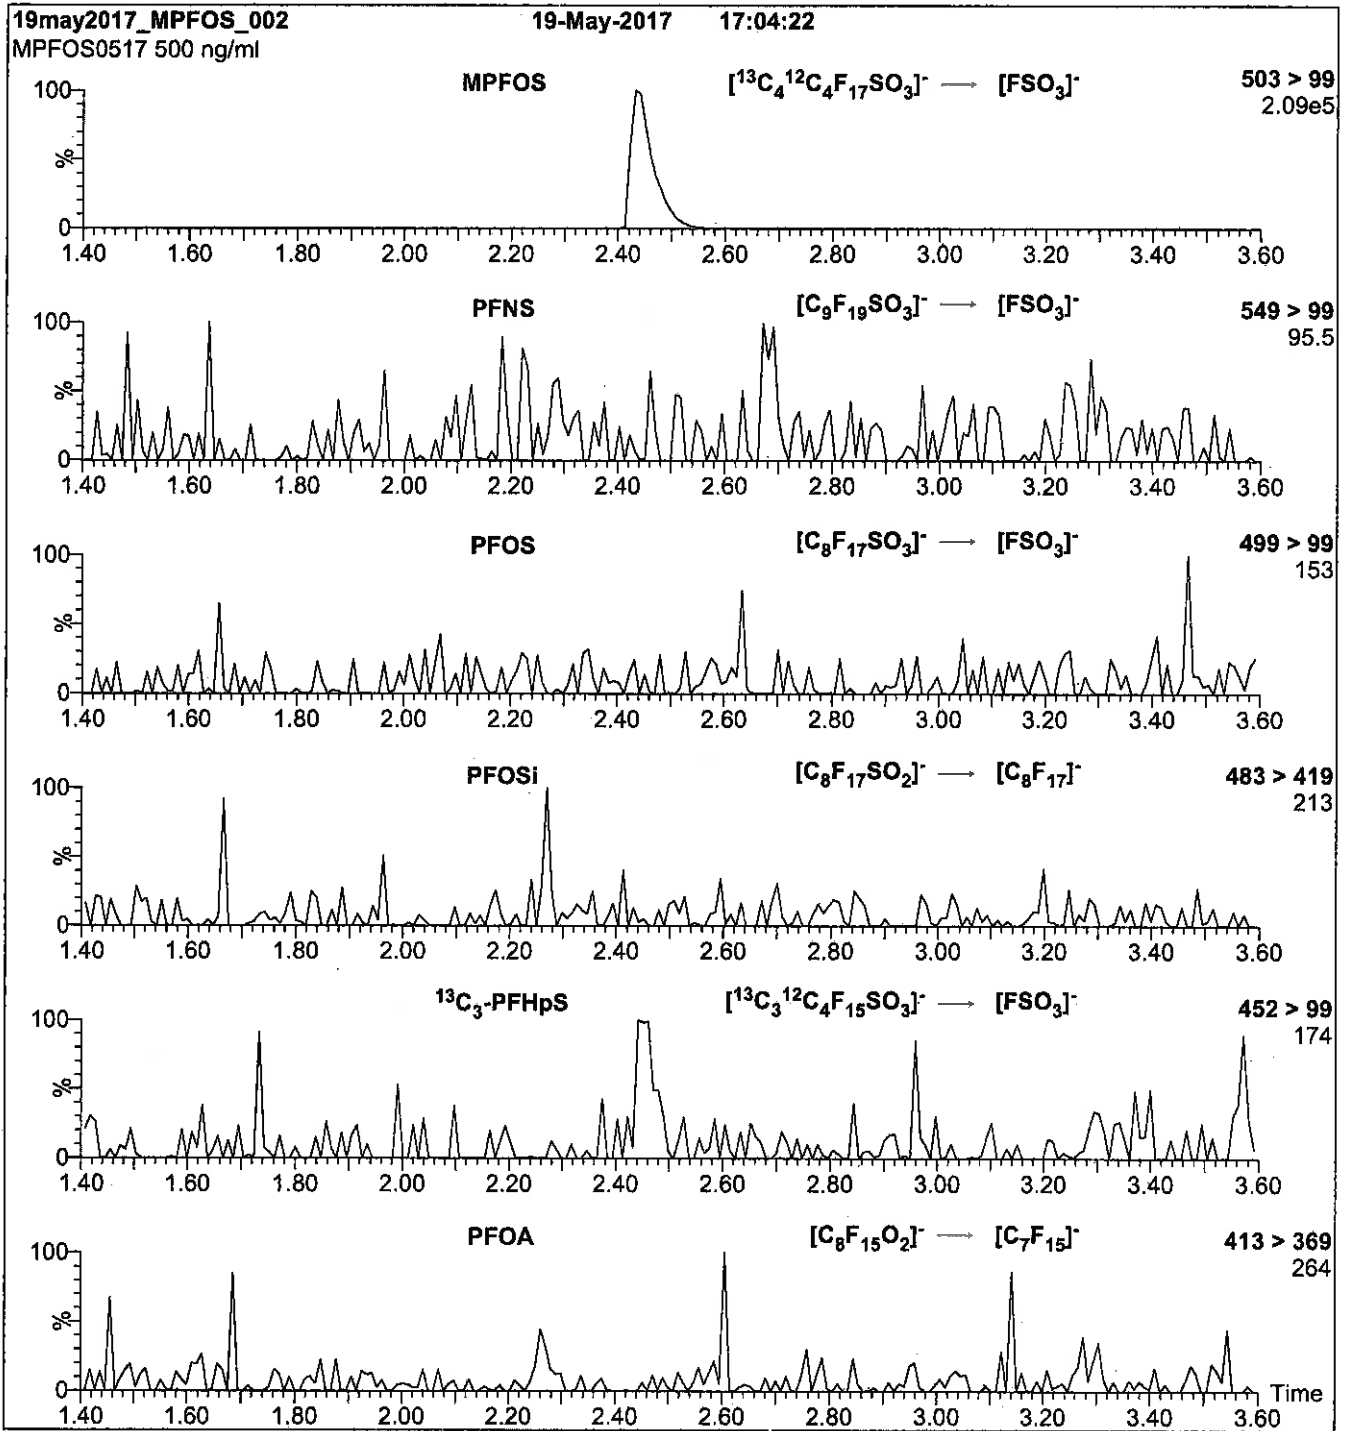

Conditions for Figure 2:

Injection: Direct loop injection
10 μl (500 ng/ml MPFOS)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H_2O
(both with 10 mM NH_4OAc buffer)

Flow: 300 $\mu\text{l}/\text{min}$

MS Parameters

Collision Gas (mbar) = 3.31e-3
Collision Energy (eV) = 40

Reagent

LCPFBSA_00002


n: 12/17 SKW



WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: L-PFBS **LOT NUMBER:** LPFBS1116
COMPOUND: Potassium perfluoro-1-butanesulfonate
STRUCTURE: **CAS #:** 29420-49-3



MOLECULAR FORMULA: C₄F₉SO₃K **MOLECULAR WEIGHT:** 338.19
CONCENTRATION: 50.0 ± 2.5 µg/ml (K salt) **SOLVENT(S):** Methanol
44.2 ± 2.2 µg/ml (PFBS anion)
CHEMICAL PURITY: >98%
LAST TESTED: (mm/dd/yyyy) 12/02/2016
EXPIRY DATE: (mm/dd/yyyy) 12/02/2021
RECOMMENDED STORAGE: Store ampoule in a cool, dark place

DOCUMENTATION/ DATA ATTACHED:

- Figure 1: LC/MS Data (TIC and Mass Spectrum)
- Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

• See page 2 for further details.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By:  **Date:** 12/05/2016
B.G. Chittim (mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at Info@well-labs.com

Figure 1: L-PFBS; LC/MS Data (TIC and Mass Spectrum)

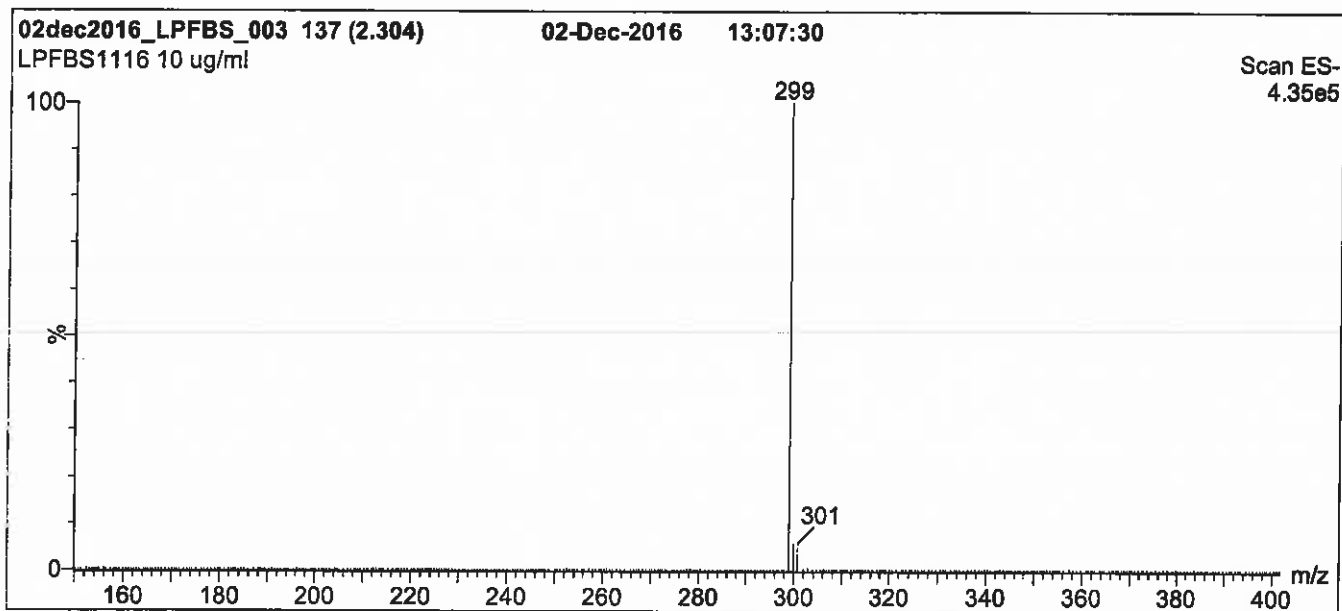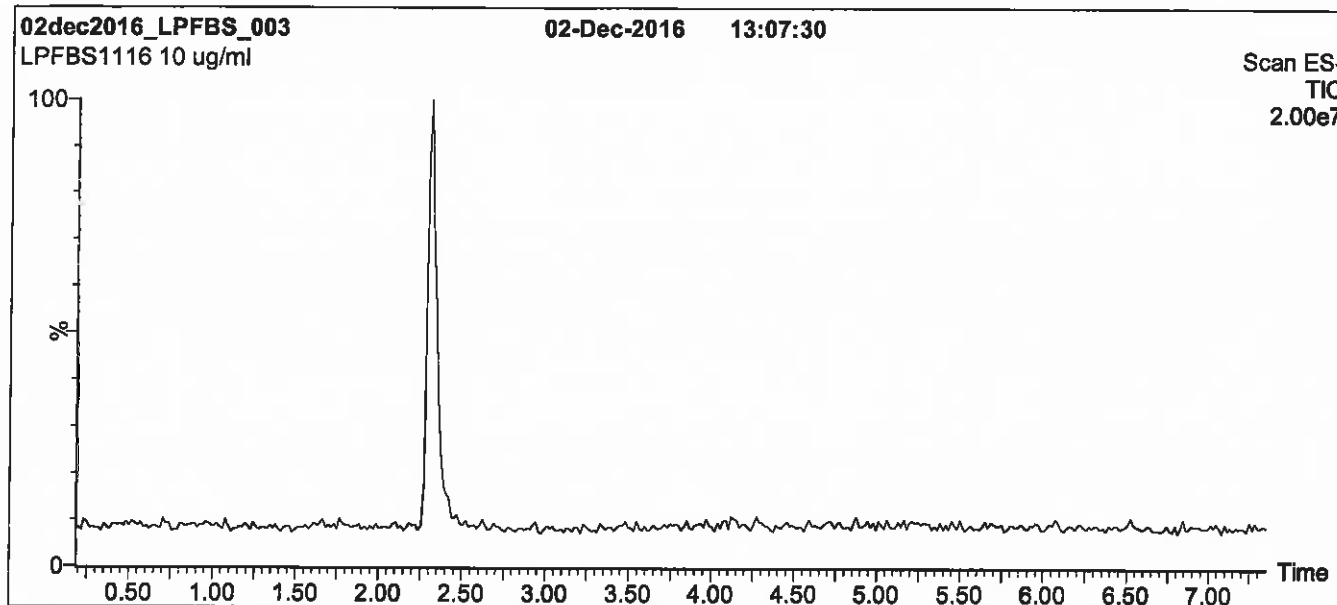

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈,
 1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
 Start: 40% (80:20 MeOH:ACN) / 60% H₂O
 (both with 10 mM NH₄OAc buffer)
 Ramp to 90% organic over 7 min and hold for 2 min
 before returning to initial conditions in 0.5 min.
 Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (150 - 850 amu)

Source: Electrospray (negative)
 Capillary Voltage (kV) = 2.00
 Cone Voltage (V) = 40.00
 Cone Gas Flow (l/hr) = 50
 Desolvation Gas Flow (l/hr) = 750

Figure 2: L-PFBS; LC/MS/MS Data (Selected MRM Transitions)

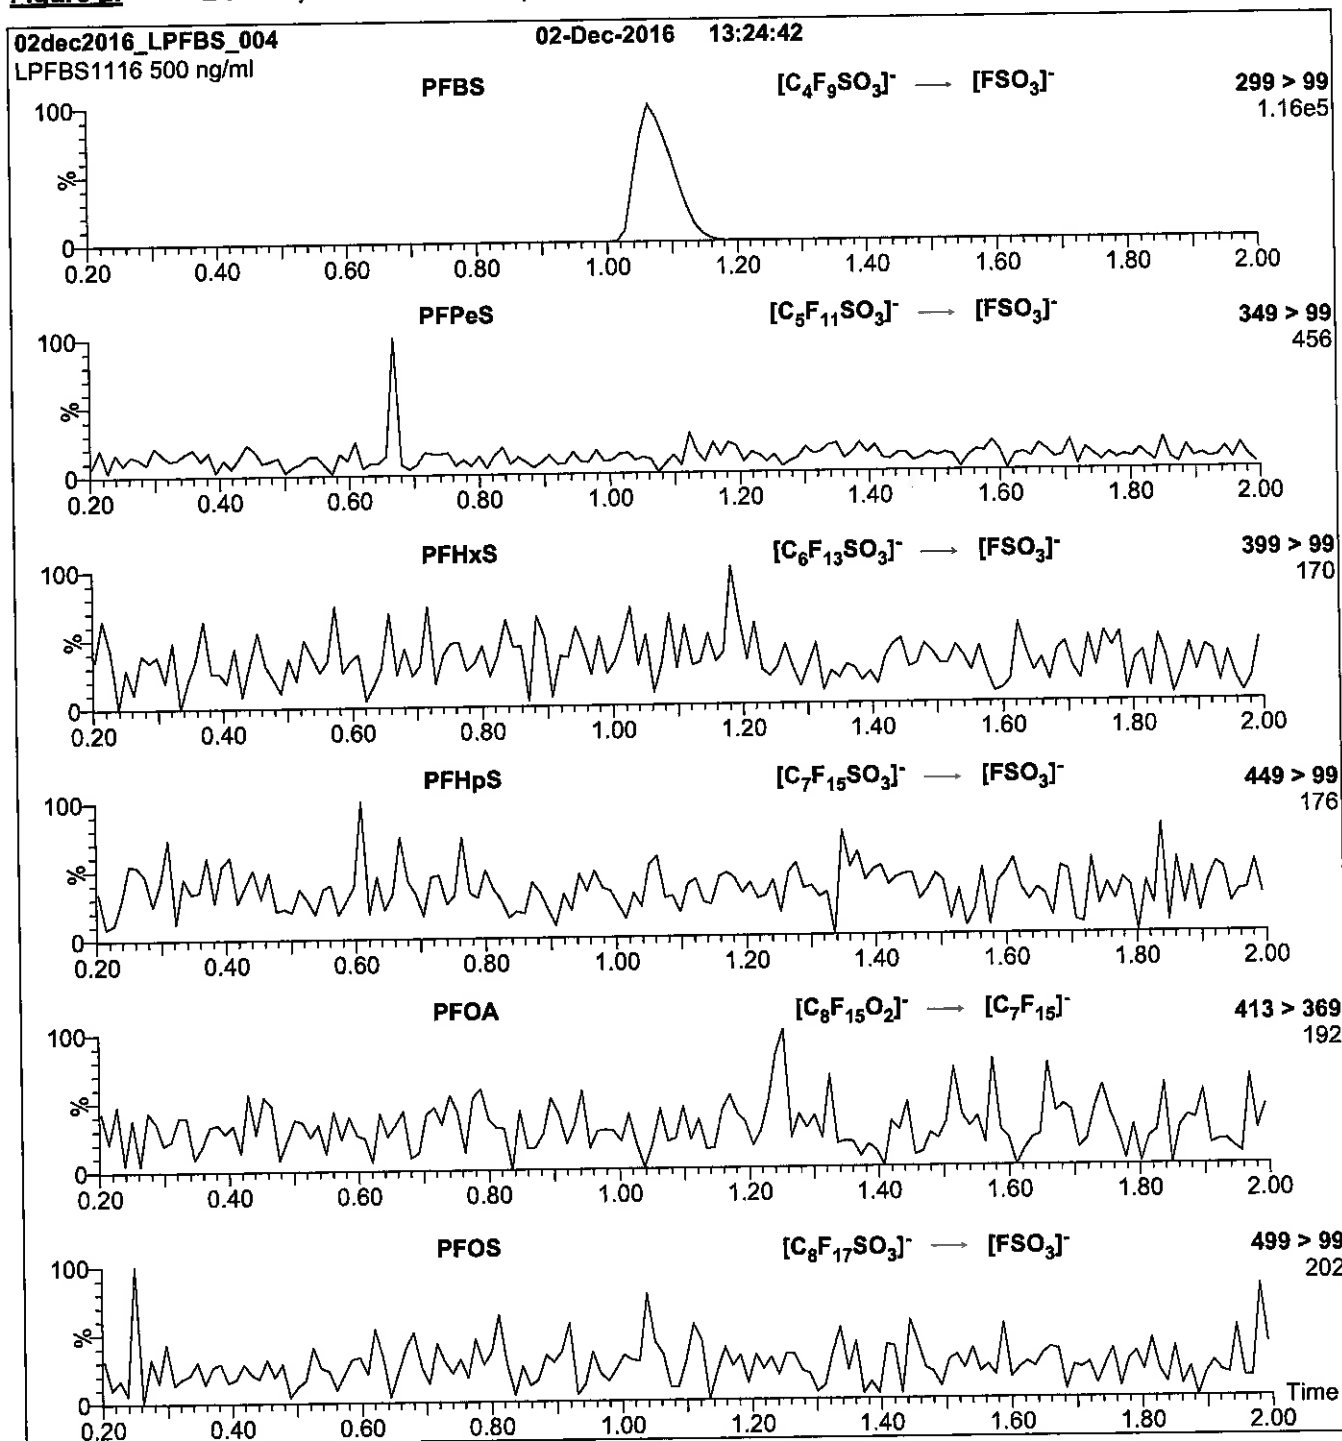

Conditions for Figure 2:

Injection: Direct loop injection
10 μ l (500 ng/ml L-PFBS)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
(both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.28e-3
Collision Energy (eV) = 25

Reagent

LCPFHpA_00009

P: 9/21/17 SKJ




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: PFHpA **LOT NUMBER:** PFHpA1216
COMPOUND: Perfluoro-n-heptanoic acid

STRUCTURE: **CAS #:** 375-85-9

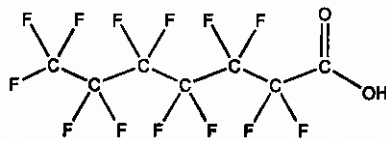

MOLECULAR FORMULA: $C_7HF_{13}O_2$ **MOLECULAR WEIGHT:** 364.06
CONCENTRATION: $50 \pm 2.5 \mu\text{g/ml}$ **SOLVENT(S):** Methanol
Water (<1%)
CHEMICAL PURITY: >98%
LAST TESTED: (mm/dd/yyyy) 12/02/2016
EXPIRY DATE: (mm/dd/yyyy) 12/02/2021
RECOMMENDED STORAGE: Store ampoule in a cool, dark place


DOCUMENTATION/ DATA ATTACHED:

Figure 1: LC/MS Data (TIC and Mass Spectrum)
Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent conversion of the carboxylic acid to the methyl ester.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: 
B.G. Chittim **Date:** 12/12/2016
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:


Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: PFHpA; LC/MS Data (TIC and Mass Spectrum)

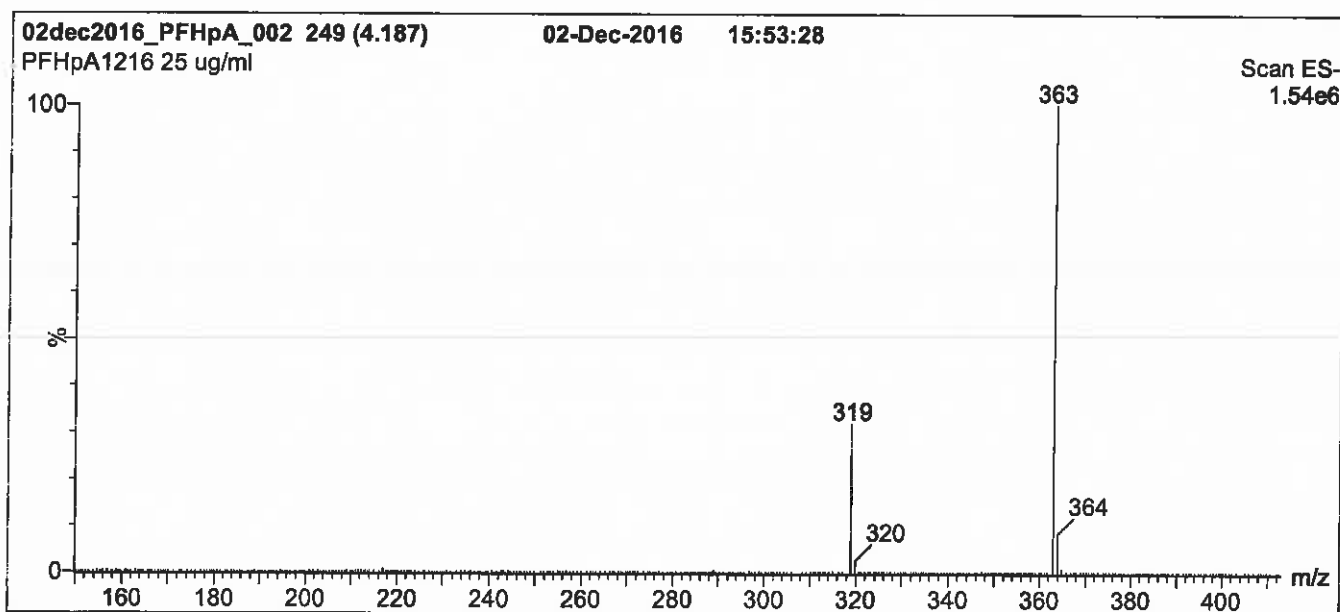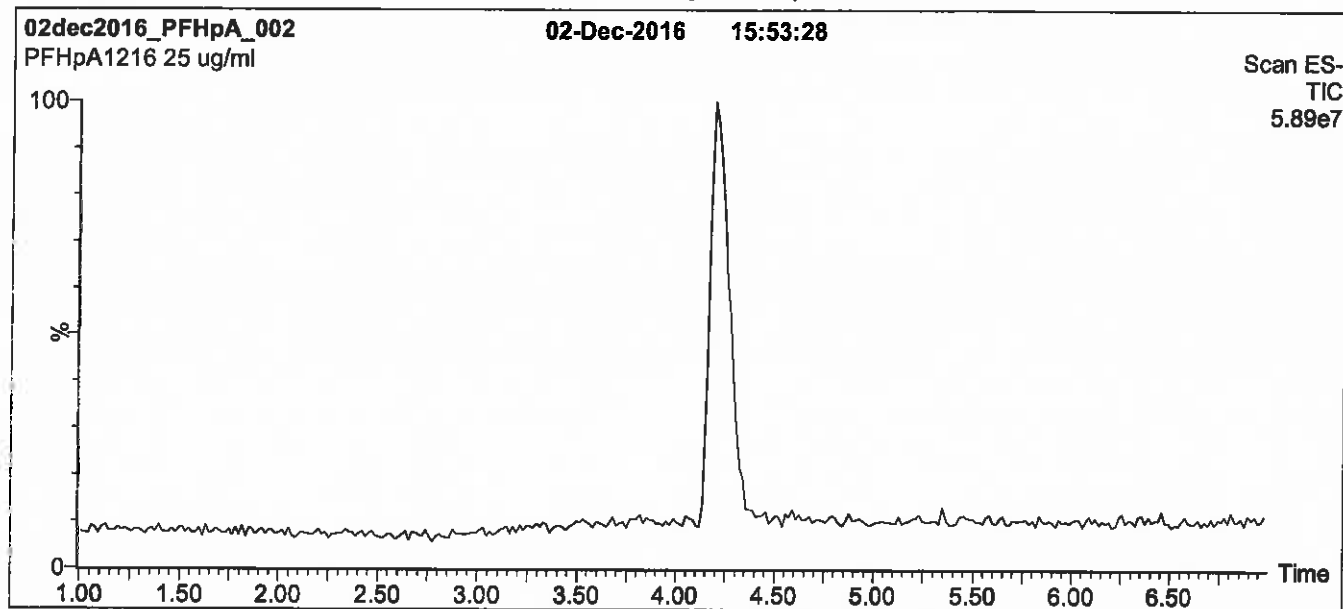

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro micro API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
Start: 50% (80:20 MeOH:ACN) / 50% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 90% organic over 7.5 min and hold for
1.5 min before returning to initial conditions in 0.5 min.
Time: 10 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (150 - 850 amu)

Source: Electrospray (negative)
Capillary Voltage (kV) = 2.00
Cone Voltage (V) = 15.00
Cone Gas Flow (l/hr) = 50
Desolvation Gas Flow (l/hr) = 750

Figure 2: PFHpA; LC/MS/MS Data (Selected MRM Transitions)

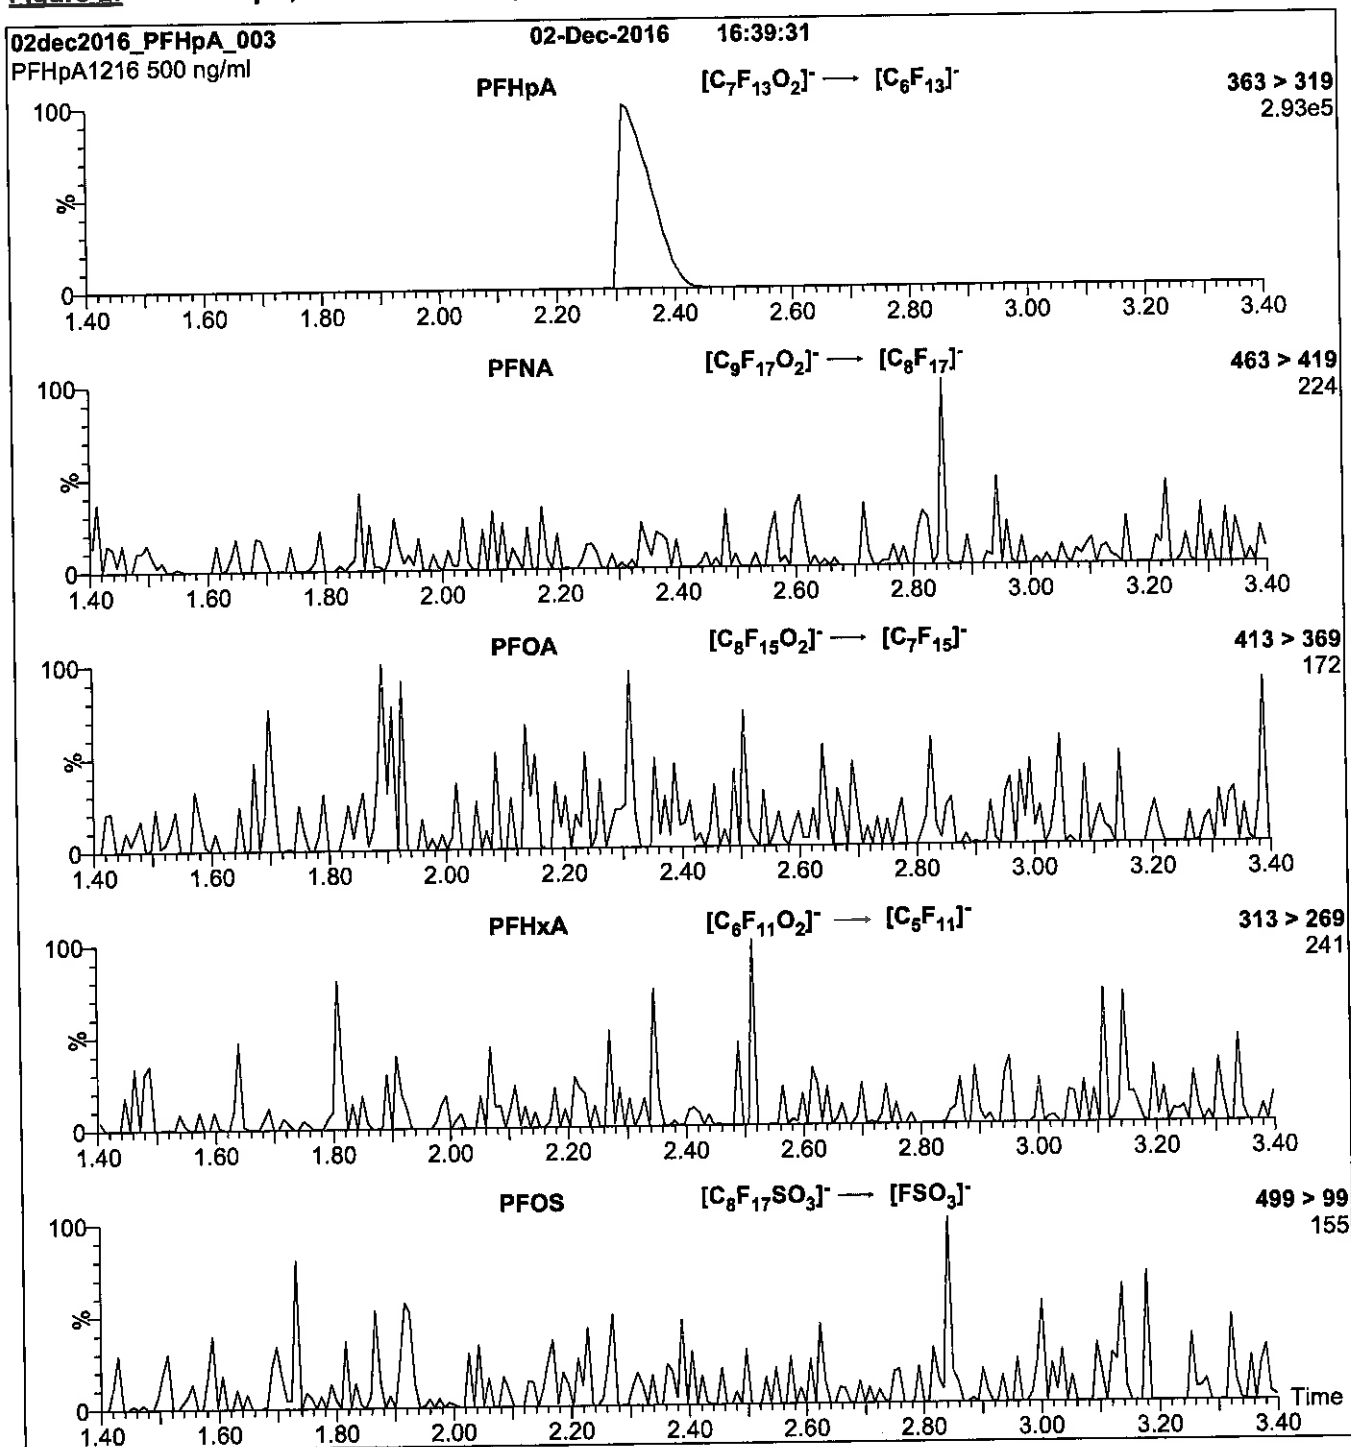

Conditions for Figure 2:

Injection: Direct loop injection
 10 μ l (500 ng/ml PFHpA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
 (both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.50e-3
 Collision Energy (eV) = 11

Reagent

LCPFHxS-br_00005

P: 10/2017 SKV



WELLINGTON
LABORATORIES

CERTIFICATE OF ANALYSIS
DOCUMENTATION

br-PFHxSK

Potassium Perfluorohexanesulfonate
Solution/Mixture of Linear and
Branched Isomers

PRODUCT CODE: br-PFHxSK
LOT NUMBER: brPFHxSK0117
CONCENTRATION: 50.0 ± 2.5 µg/ml (total potassium salt)
45.5 ± 2.3 µg/ml (total PFHxS anion)
SOLVENT(S): Methanol
DATE PREPARED: (mm/dd/yyyy) 01/03/2017
LAST TESTED: (mm/dd/yyyy) 01/04/2017
EXPIRY DATE: (mm/dd/yyyy) 01/04/2022
RECOMMENDED STORAGE: Store ampoule in a cool, dark place

DESCRIPTION:

The chemical purity has been determined to be ≥98% perfluorohexanesulfonate linear and branched isomers. The full name, structure and percent composition for each of the identified isomeric components are given in Table A.

DOCUMENTATION/ DATA ATTACHED:

Table A: Isomeric Components and Percent Composition by ¹⁹F-NMR
Figure 1: LC/MS Data (TIC and Mass Spectrum)
Figure 2: LC/MS Data (SIR)
Figure 3: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains ~ 0.5% of perfluoro-1-pentanesulfonate and ~ 0.2% of perfluoro-1-octanesulfonate.
- CAS#: 3871-99-6 (for linear isomer; potassium salt).

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compounds it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:


Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.

QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Table A: br-PFHxSK; Isomeric Components and Percent Composition (by ¹⁹F-NMR)*



Isomer	Name	Structure	Percent Composition by ¹⁹ F-NMR
1	Potassium perfluoro-1-hexanesulfonate	CF ₃ CF ₂ CF ₂ CF ₂ CF ₂ CF ₂ SO ₃ ⁻ K ⁺	81.1
2	Potassium 1-trifluoromethylperfluoropentanesulfonate**	$\begin{array}{c} \text{CF}_3\text{CF}_2\text{CF}_2\text{CF}_2\text{CF}(\text{SO}_3^-\text{K}^+) \\ \\ \text{CF}_3 \end{array}$	2.9
3	Potassium 2-trifluoromethylperfluoropentanesulfonate	$\begin{array}{c} \text{CF}_3\text{CF}_2\text{CF}_2\text{CF}(\text{CF}_3)\text{CF}_2\text{SO}_3^-\text{K}^+ \\ \\ \text{CF}_3 \end{array}$	1.4
4	Potassium 3-trifluoromethylperfluoropentanesulfonate	$\begin{array}{c} \text{CF}_3\text{CF}_2\text{CF}(\text{CF}_3)\text{CF}_2\text{CF}_2\text{SO}_3^-\text{K}^+ \\ \\ \text{CF}_3 \end{array}$	5.0
5	Potassium 4-trifluoromethylperfluoropentanesulfonate	$\begin{array}{c} \text{CF}_3\text{CF}(\text{CF}_3)\text{CF}_2\text{CF}_2\text{CF}_2\text{SO}_3^-\text{K}^+ \\ \\ \text{CF}_3 \end{array}$	8.9
6	Potassium 3,3-di(trifluoromethyl)perfluorobutanesulfonate	$\begin{array}{c} \text{CF}_3 \\ \\ \text{CF}_3\text{C}(\text{CF}_3)_2\text{CF}_2\text{SO}_3^-\text{K}^+ \\ \\ \text{CF}_3 \end{array}$	0.2
7	Other Unidentified Isomers		0.5

* Percent of total perfluorohexanesulfonate isomers only.
 ** Systematic Name: Potassium perfluorohexane-2-sulfonate.

Certified By: 
 B.G. Chittim

Date: 01/20/2017
(mm/dd/yyyy)

Figure 1: br-PFHxSK; LC/MS Data (TIC and Mass Spectrum)

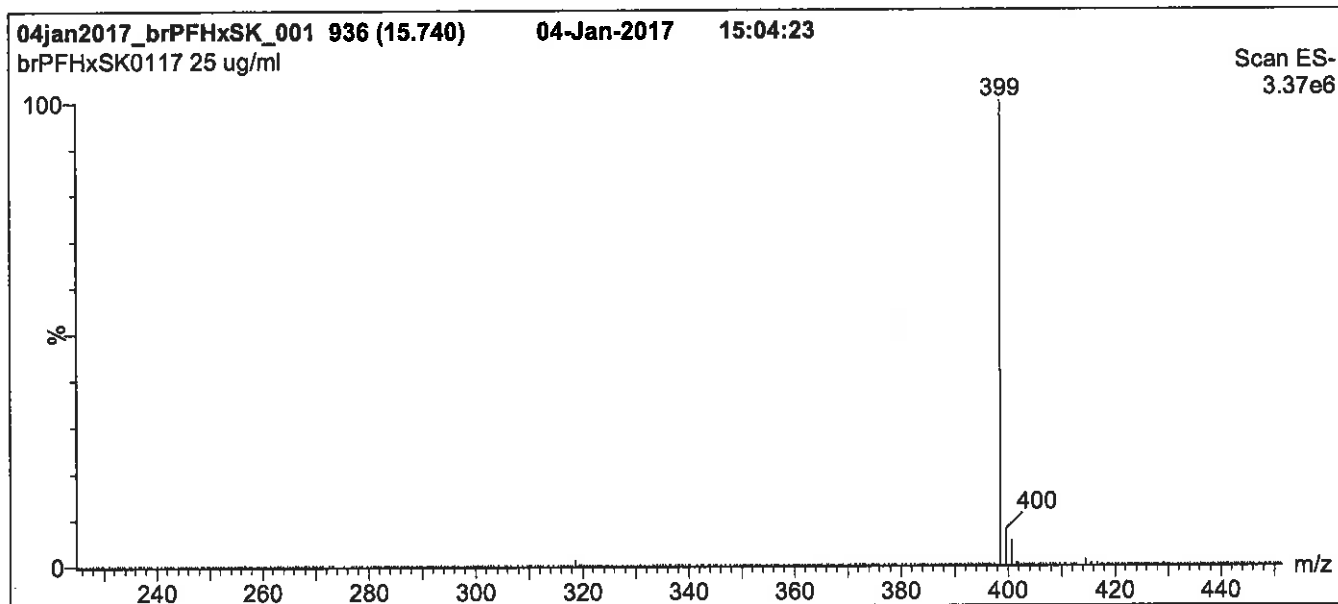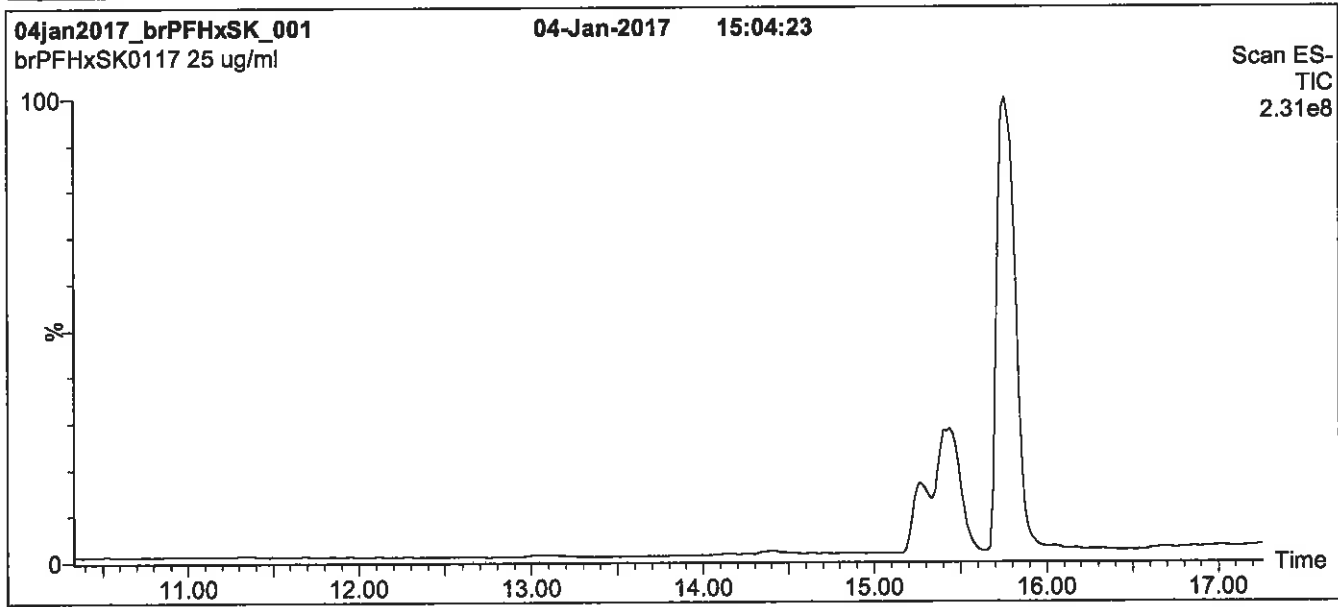

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro micro API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
1.7 μm, 2.1 x 100 mm

Mobile phase: Gradient
Start: 20% (80:20 MeOH:ACN) / 80% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 50% organic over 14 min. Ramp to
90% organic over 3 min and hold for 1.5 min
before returning to initial conditions in 0.5 min.
Time: 20 min


Flow: 300 μl/min

MS Parameters

Experiment: Full Scan (225 - 850 amu)

Source: Electrospray (negative)
Capillary Voltage (kV) = 3.00
Cone Voltage (V) = 50.00
Cone Gas Flow (l/hr) = 60
Desolvation Gas Flow (l/hr) = 750

Figure 2: br-PFHxSK; LC/MS Data (SIR)

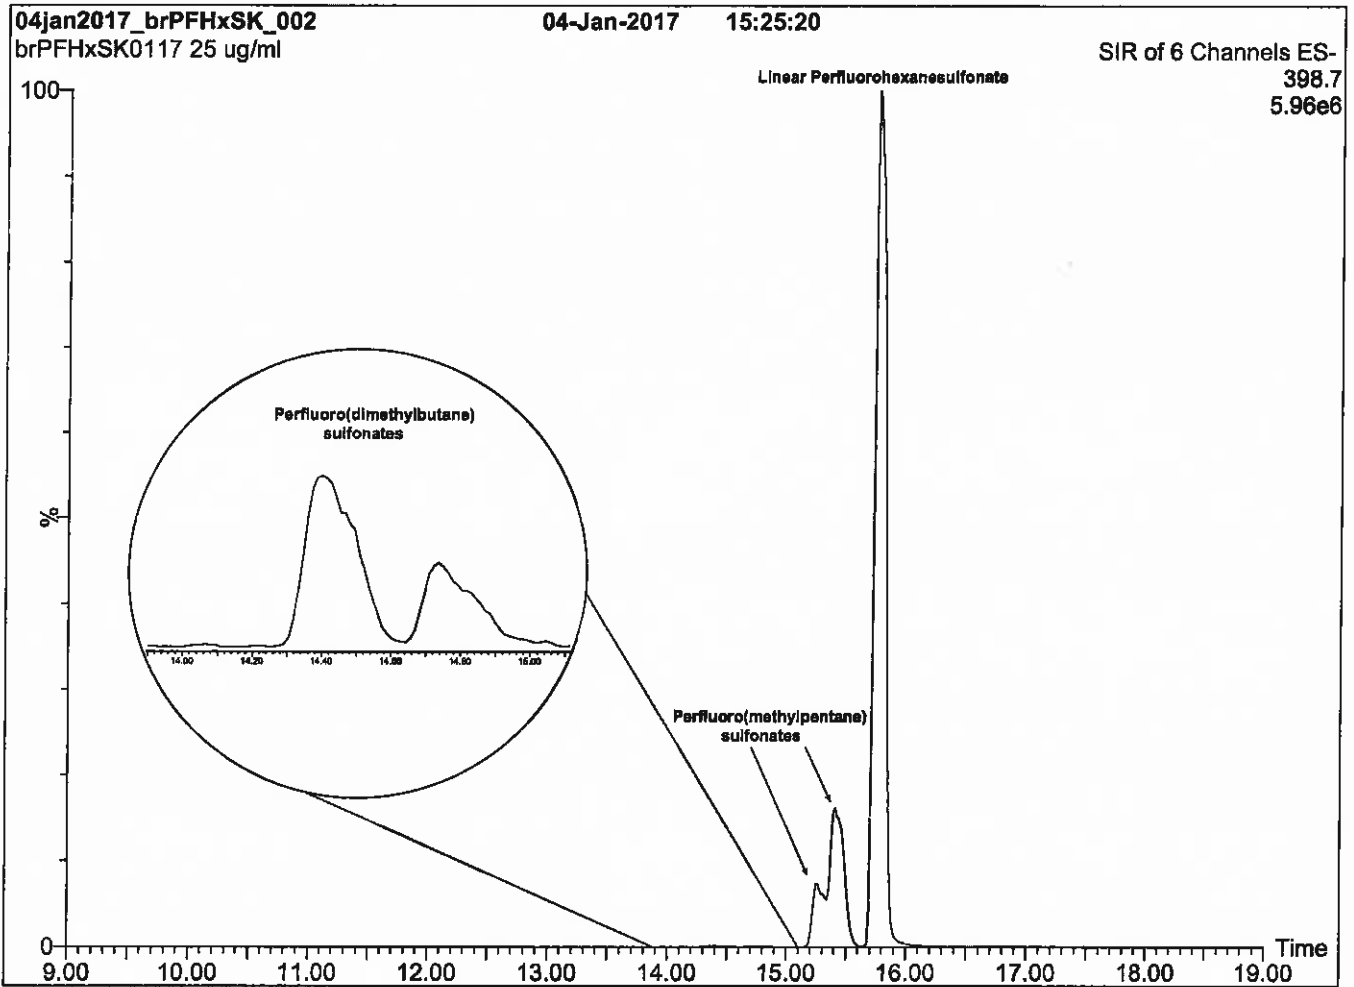

Conditions for Figure 2:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
Start: 20% (80:20 MeOH:ACN) / 80% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 50% organic over 14 min. Ramp to
90% organic over 3 min and hold for 1.5 min
before returning to initial conditions in 0.5 min.
Time: 20 min


Flow: 300 μ l/min

MS Parameters

Experiment: SIR (6 channels)

Source: Electrospray (negative)
Capillary Voltage (kV) = 3.00
Cone Voltage (V) = variable (15-62)
Cone Gas Flow (l/hr) = 60
Desolvation Gas Flow (l/hr) = 750

Figure 3: br-PFHxSK; LC/MS/MS Data (Selected MRM Transitions)

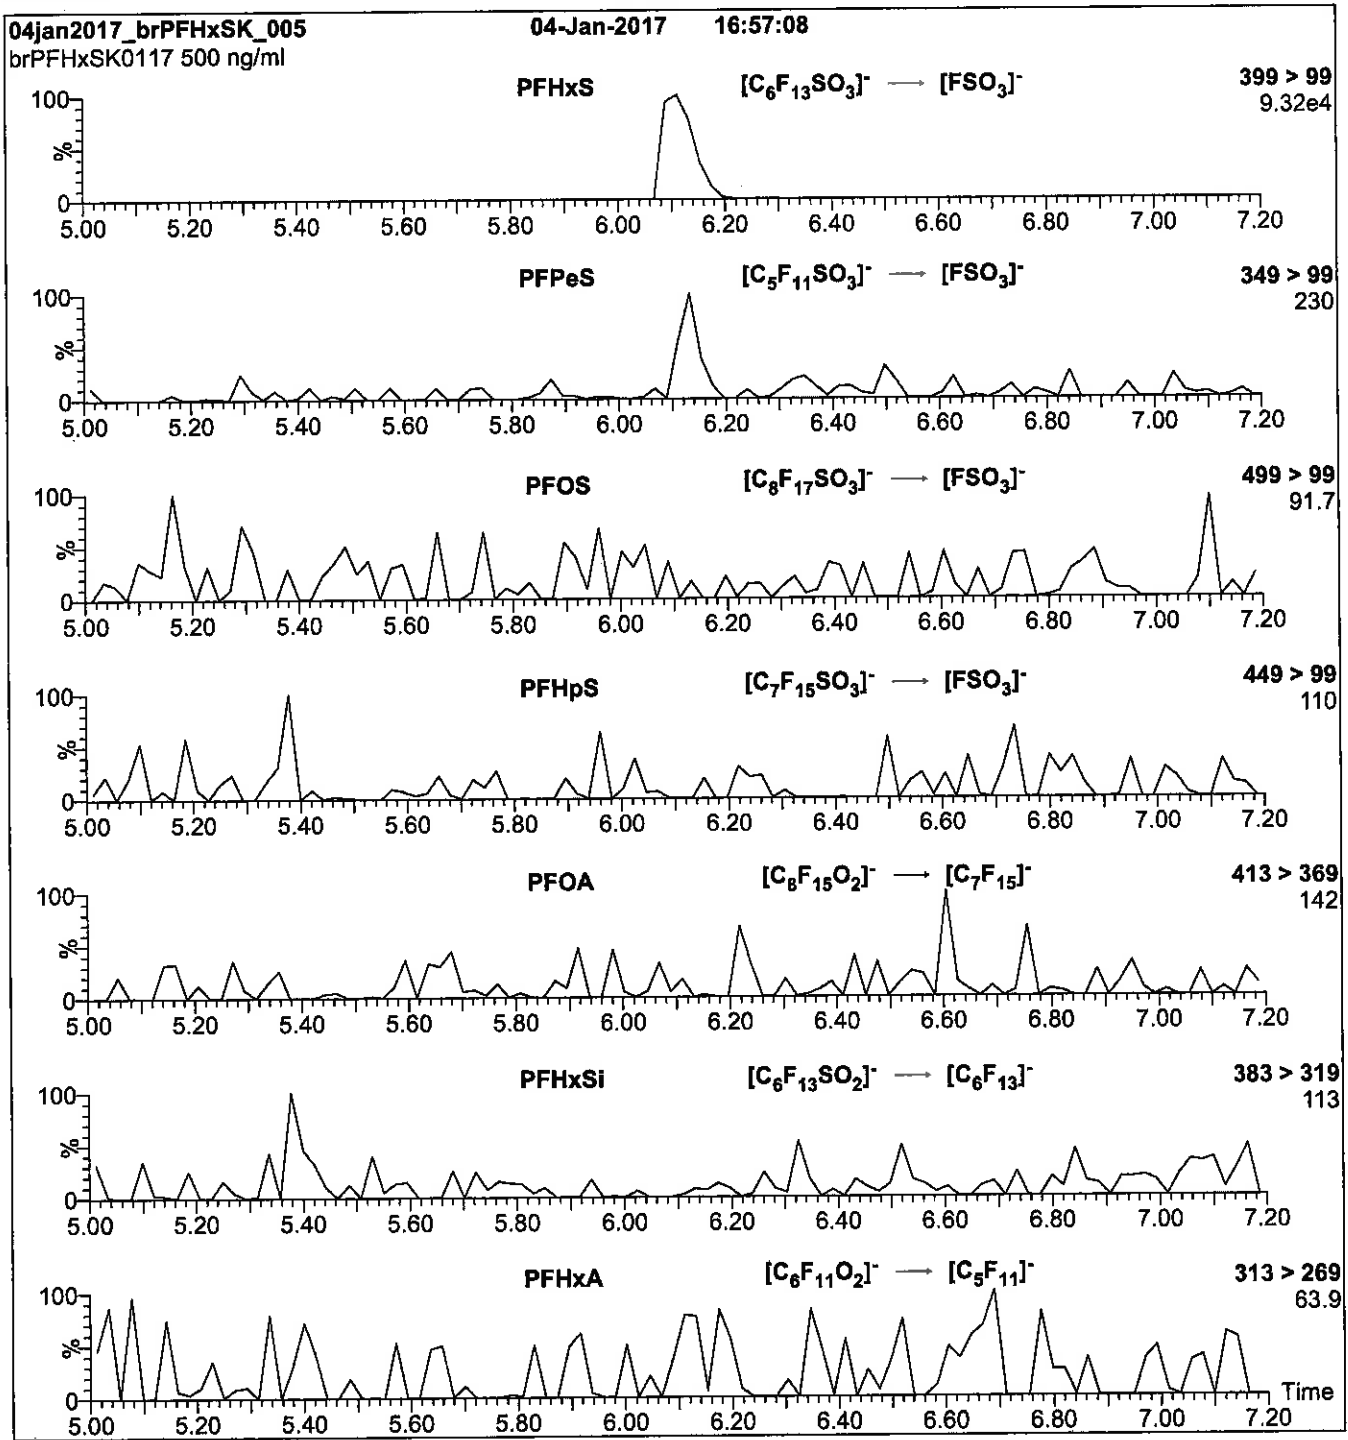

Conditions for Figure 3:

Injection: Direct loop injection
10 μ l (500 ng/ml br-PFHxSK)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
(both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.35e-3
Collision Energy (eV) = 30

Reagent

LCPFNA_00009

r: 9/2/17 skv




WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: PFNA **LOT NUMBER:** PFNA0717
COMPOUND: Perfluoro-n-nonanoic acid

STRUCTURE: **CAS #:** 375-95-1

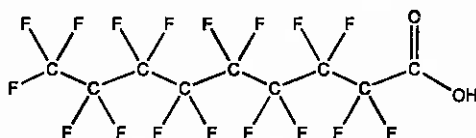

MOLECULAR FORMULA: $C_9HF_{17}O_2$ **MOLECULAR WEIGHT:** 464.08
CONCENTRATION: $50 \pm 2.5 \mu\text{g/ml}$ **SOLVENT(S):** Methanol
Water (<1%)
CHEMICAL PURITY: >98%
LAST TESTED: (mm/dd/yyyy) 07/20/2017
EXPIRY DATE: (mm/dd/yyyy) 07/20/2022
RECOMMENDED STORAGE: Store ampoule in a cool, dark place

DOCUMENTATION/ DATA ATTACHED:

Figure 1: LC/MS Data (TIC and Mass Spectrum)
Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent conversion of the carboxylic acid to the methyl ester.
- Contains ~ 0.1% of perfluoro-n-octanoic acid (PFOA), < 0.1% of perfluoro-n-heptanoic acid (PFHpA), and < 0.1% of perfluoro-n-undecanoic acid (PFUdA).

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: 
B.G. Chittim, General Manager **Date:** 07/24/2017
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers. In order to maintain the integrity of the assigned value(s), and associated uncertainty, the dilution or injection of a subsample of this product should be performed using calibrated measuring equipment.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters

x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using calibrated NIST and/or NRC traceable external weights. All volumetric glassware used is calibrated, of Class A tolerance, and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:

Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: PFNA; LC/MS Data (TIC and Mass Spectrum)

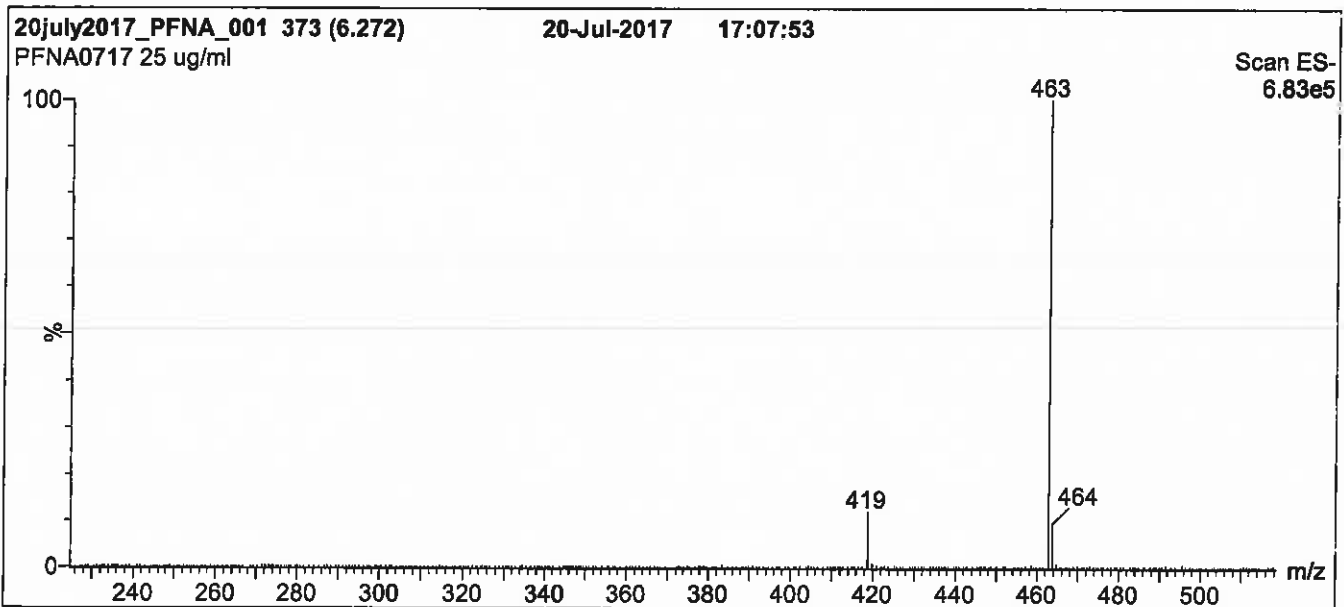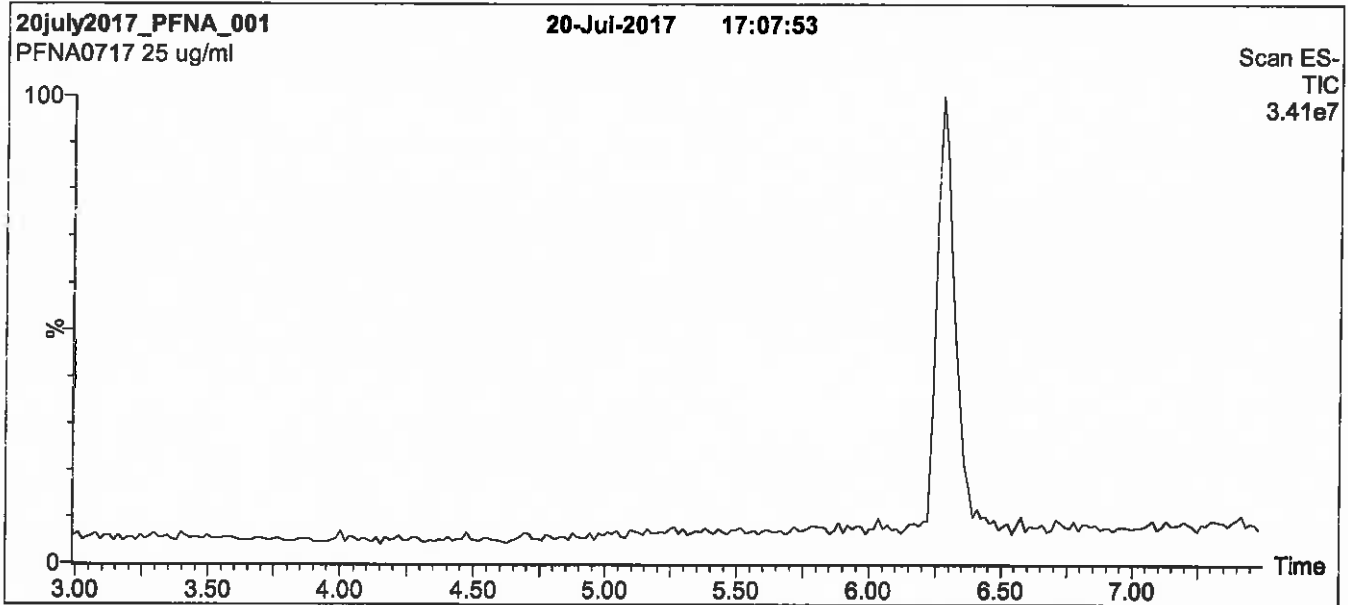

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm


Mobile phase: Gradient
Start: 50% (80:20 MeOH:ACN) / 50% H₂O
(both with 10 mM NH₄OAc buffer)
Hold for 1 min. Ramp to 90% organic over 7 min and hold
for 1 min before returning to initial conditions in 0.5 min.
Time: 10 min

Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (225 - 850 amu)
Source: Electrospray (negative)
Capillary Voltage (kV) = 2.00
Cone Voltage (V) = 15.00
Cone Gas Flow (l/hr) = 50
Desolvation Gas Flow (l/hr) = 750

Figure 2: PFNA; LC/MS/MS Data (Selected MRM Transitions)

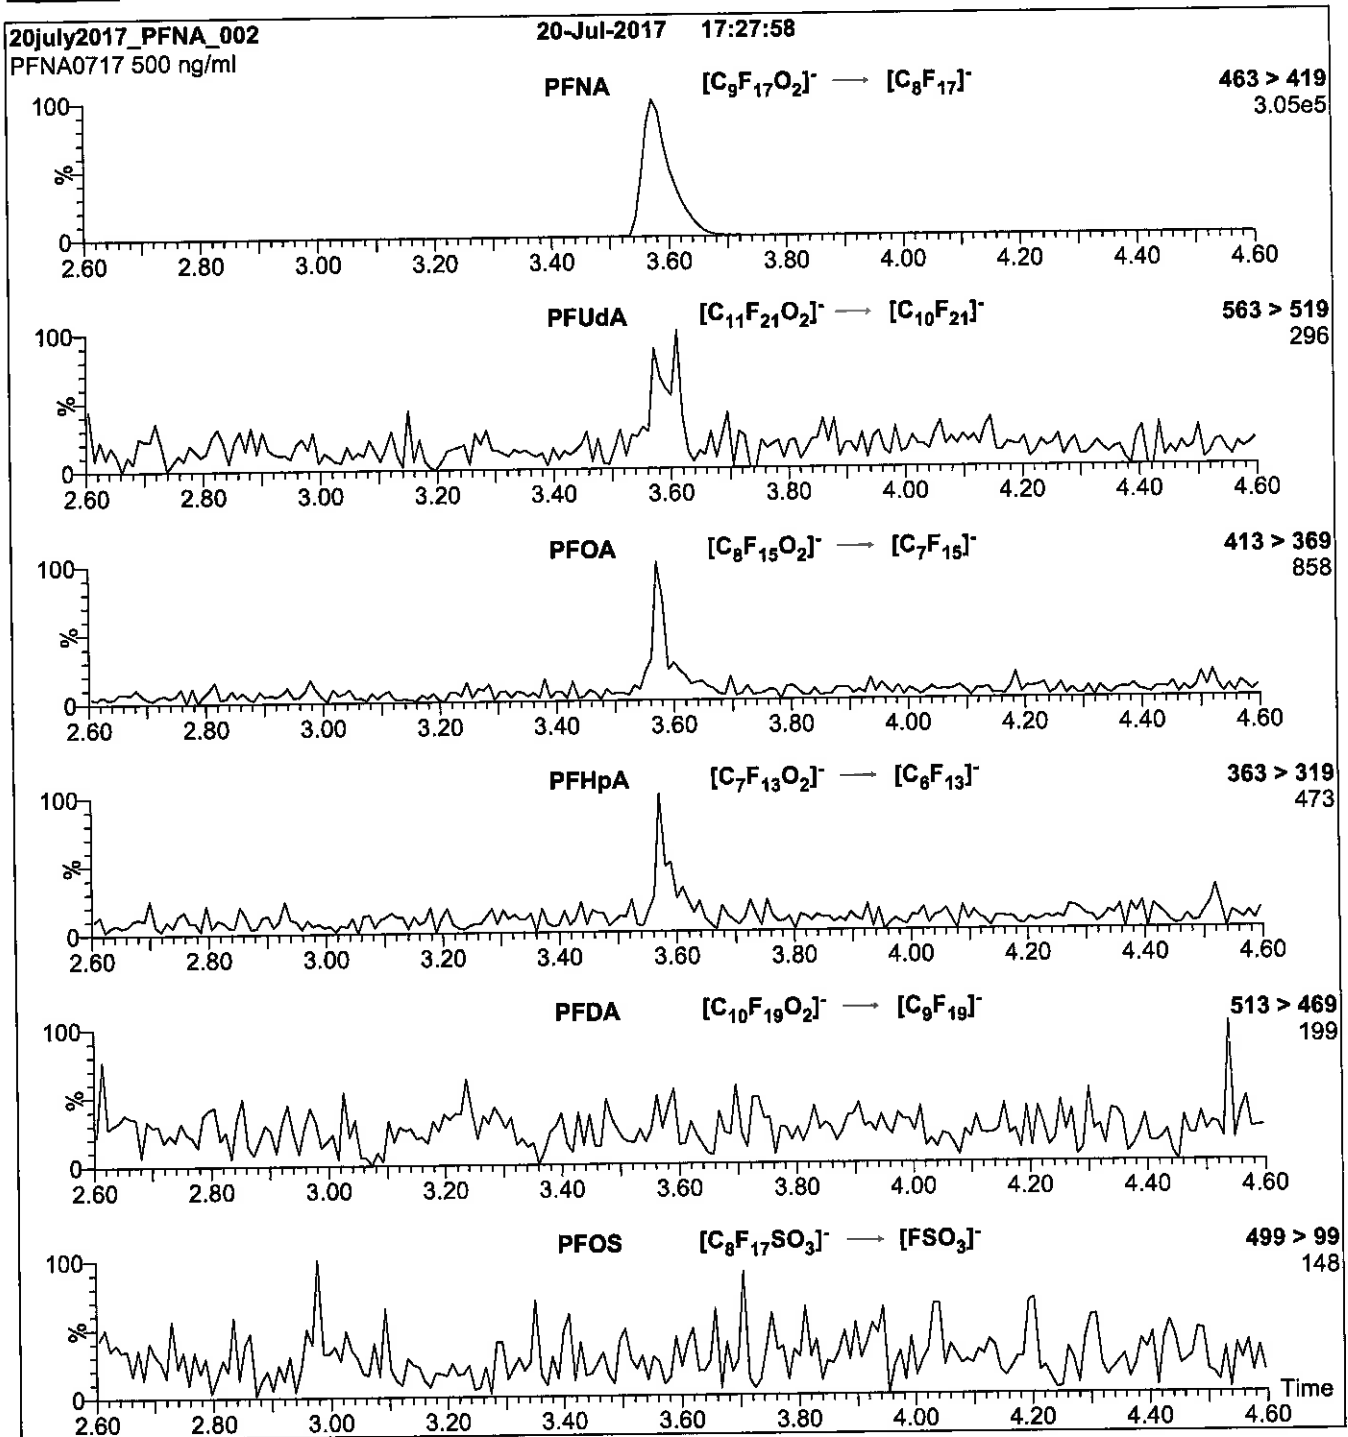

Conditions for Figure 2:

Injection: Direct loop injection
 10 μ l (500 ng/ml PFNA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
 (both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.50e-3
 Collision Energy (eV) = 11

Reagent

LCPFOA_00010

P: 10/2017 SKV



WELLINGTON LABORATORIES


CERTIFICATE OF ANALYSIS DOCUMENTATION

PRODUCT CODE: PFOA
COMPOUND: Perfluoro-n-octanoic acid

LOT NUMBER: PFOA0917

STRUCTURE:

CAS #: 335-67-1

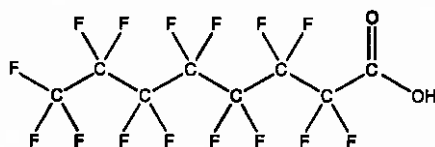

MOLECULAR FORMULA: C₈HF₁₅O₂
CONCENTRATION: 50 ± 2.5 µg/ml

MOLECULAR WEIGHT: 414.07
SOLVENT(S): Methanol
Water (<1%)

CHEMICAL PURITY: >98%
LAST TESTED: (mm/dd/yyyy) 09/27/2017
EXPIRY DATE: (mm/dd/yyyy) 09/27/2022
RECOMMENDED STORAGE: Store ampoule in a cool, dark place

DOCUMENTATION/ DATA ATTACHED:

Figure 1: LC/MS Data (TIC and Mass Spectrum)
Figure 2: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- Contains 4 mole eq. of NaOH to prevent conversion of the carboxylic acid to the methyl ester.

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Certified By: 
B.G. Chittim, General Manager

Date: 09/28/2017
(mm/dd/yyyy)

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compound it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers. In order to maintain the integrity of the assigned value(s), and associated uncertainty, the dilution or injection of a subsample of this product should be performed using calibrated measuring equipment.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using calibrated NIST and/or NRC traceable external weights. All volumetric glassware used is calibrated, of Class A tolerance, and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:


Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.



QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Figure 1: PFOA; LC/MS Data (TIC and Mass Spectrum)

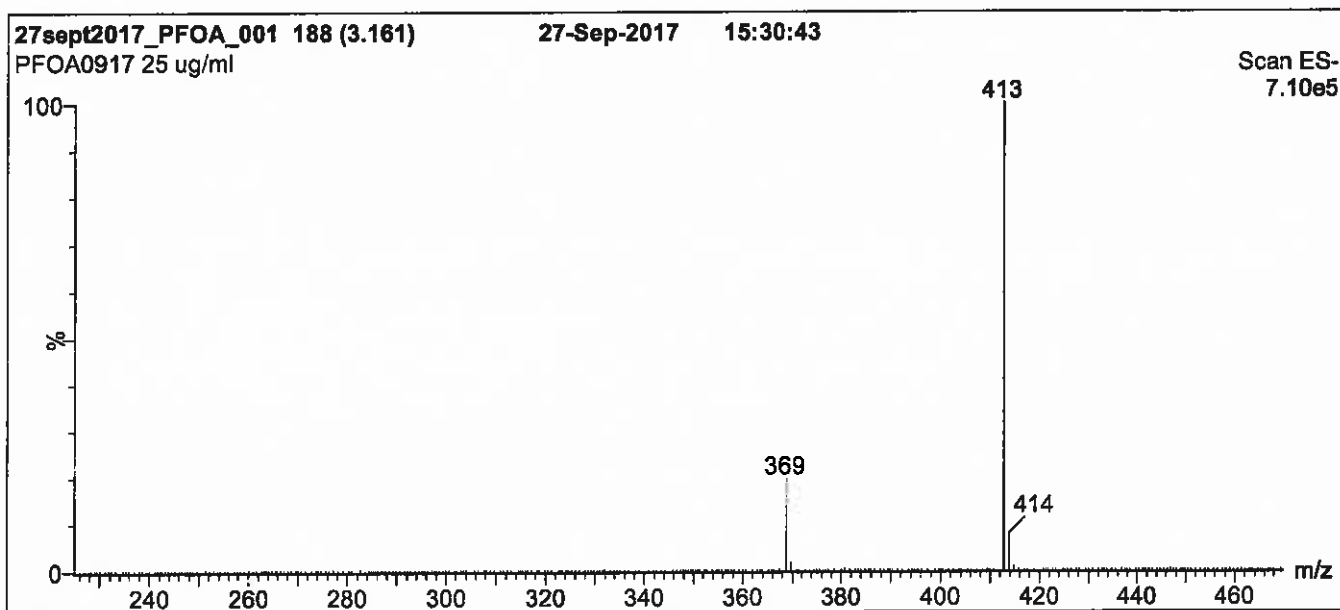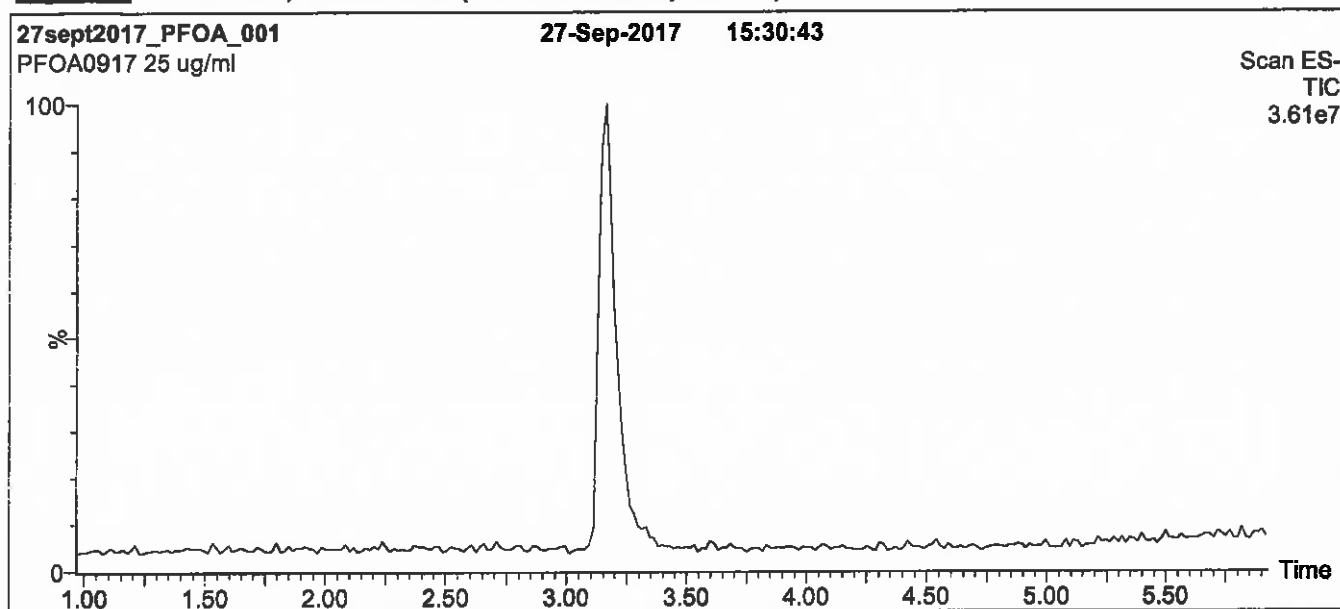

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions


Column: Acquity UPLC BEH Shield RP₁₈
1.7 μ m, 2.1 x 100 mm
Mobile phase: Gradient
Start: 50% (80:20 MeOH:ACN) / 50% H₂O
(both with 10 mM NH₄OAc buffer)
Ramp to 90% organic over 7 min and hold for
2 min before returning to initial conditions in 0.5 min.
Time: 10 min

Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (225 - 850 amu)
Source: Electrospray (negative)
Capillary Voltage (kV) = 3.00
Cone Voltage (V) = 15.00
Cone Gas Flow (l/hr) = 100
Desolvation Gas Flow (l/hr) = 750

Figure 2: PFOA; LC/MS/MS Data (Selected MRM Transitions)

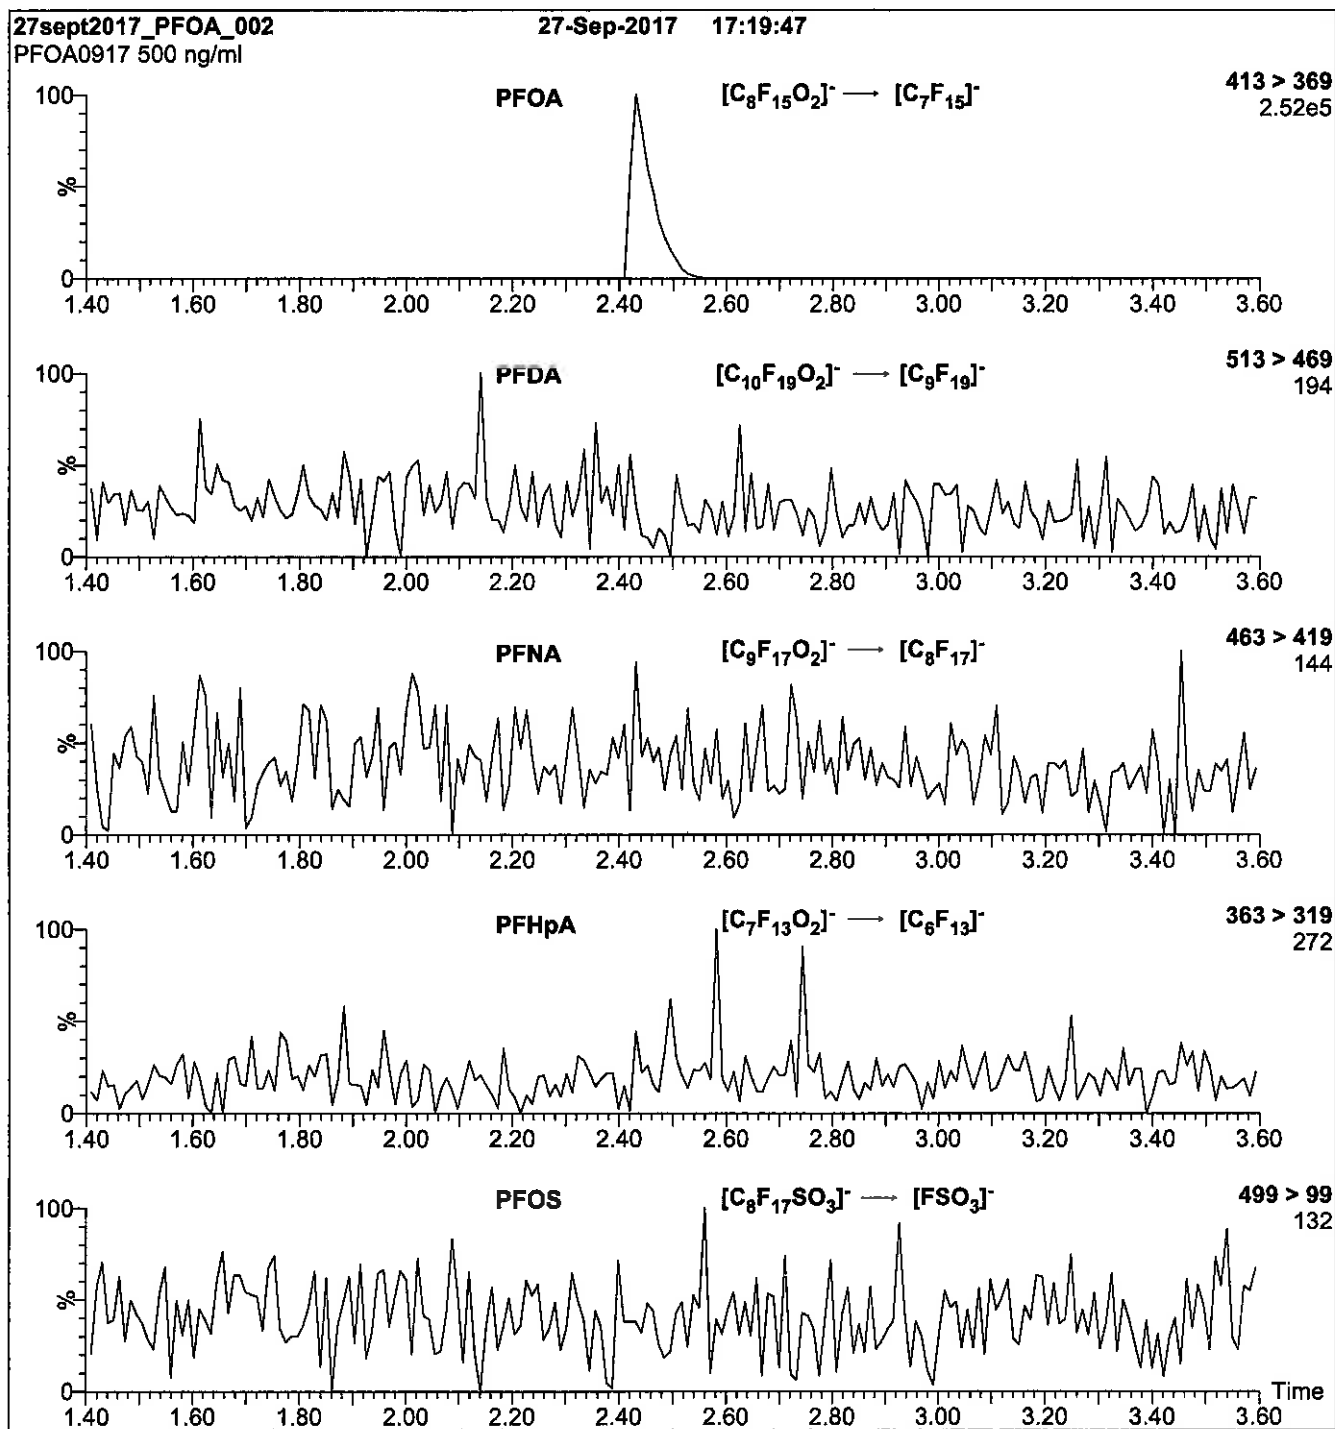

Conditions for Figure 2:

Injection: Direct loop injection
10 μ l (500 ng/ml PFOA)

Mobile phase: Isocratic 80% (80:20 MeOH:ACN) / 20% H₂O
(both with 10 mM NH₄OAc buffer)

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.46e-3
Collision Energy (eV) = 11

Reagent

LCPFOS-br_00005

P: 10/2017 SKV



WELLINGTON LABORATORIES

CERTIFICATE OF ANALYSIS DOCUMENTATION

br-PFOSK

Potassium Perfluorooctanesulfonate Solution/Mixture of Linear and Branched Isomers

<u>PRODUCT CODE:</u>	br-PFOSK
<u>LOT NUMBER:</u>	brPFOSK0117
<u>CONCENTRATION:</u>	50 ± 2.5 µg/ml (total potassium salt) 46.4 ± 2.3 µg/ml (total PFOS anion)
<u>SOLVENT(S):</u>	Methanol
<u>DATE PREPARED:</u> (mm/dd/yyyy)	01/09/2017
<u>LAST TESTED:</u> (mm/dd/yyyy)	01/12/2017
<u>EXPIRY DATE:</u> (mm/dd/yyyy)	01/12/2022
<u>RECOMMENDED STORAGE:</u>	Store ampoule in a cool, dark place

DESCRIPTION:

The chemical purity has been determined to be ≥98% perfluorooctanesulfonate linear and branched isomers. The full name, structure and percent composition for each of the isomeric components are given in Table A.

DOCUMENTATION/ DATA ATTACHED:

Table A: Isomeric Components and Percent Composition by ¹⁹F-NMR
Figure 1: LC/MS Data (TIC and Mass Spectrum)
Figure 2: LC/MS Data (SIR)
Figure 3: LC/MS/MS Data (Selected MRM Transitions)

ADDITIONAL INFORMATION:

- See page 2 for further details.
- A 5-point calibration curve was generated using linear PFOS (potassium salt) and mass-labelled PFOS as an internal standard to enable quantitation of br-PFOSK using isotopic dilution.
- CAS#: 2795-39-3 (for linear isomer; potassium salt).

FOR LABORATORY USE ONLY: NOT FOR HUMAN OR DRUG USE

Wellington Laboratories Inc., 345 Southgate Dr. Guelph ON N1G 3M5 CANADA
519-822-2436 • Fax: 519-822-2849 • info@well-labs.com

INTENDED USE:

The products prepared by Wellington Laboratories Inc. are for laboratory use only. This certified reference material (CRM) was designed to be used as a standard for the identification and/or quantification of the specific chemical compounds it contains.

HAZARDS:

This product should only be used by qualified personnel familiar with its potential hazards and trained in the handling of hazardous chemicals. Due care should be exercised to prevent unnecessary human contact or ingestion. All procedures should be carried out in a well-functioning fume hood and suitable gloves, eye protection, and clothing should be worn at all times. Waste should be disposed of according to national and regional regulations. Safety Data Sheets (SDSs) are available upon request.

SYNTHESIS / CHARACTERIZATION:

Where possible, all of our products are synthesized using single-product unambiguous routes. They are then characterized, and their structures and purities confirmed, using a combination of the most relevant techniques, such as NMR, GC/MS, LC/MS/MS, SFC/UV/MS/MS, x-ray crystallography, and melting point. Isotopic purities of mass-labelled compounds are also confirmed using HRGC/HRMS and/or LC/MS/MS.

HOMOGENEITY:

Prior to solution preparation, crystalline material is tested for homogeneity using a variety of techniques (as stated above) and its solubility in a given diluent is taken into consideration. Duplicate solutions of a new product are prepared from the same crystalline lot and, after the addition of an appropriate internal standard, they are compared by GC/MS, LC/MS/MS and/or SFC/UV/MS/MS. The relative response factors of the analyte of interest in each solution are required to be <5% RSD. New solution lots of existing products are compared to older lots in the same manner, which further confirms the homogeneity of the crystalline material as well as the stability and homogeneity of the solutions in the storage containers.

UNCERTAINTY:

The maximum combined relative standard uncertainty of our reference standard solutions is calculated using the following equation:

The combined relative standard uncertainty, $u_c(y)$, of a value y and the uncertainty of the independent parameters x_1, x_2, \dots, x_n on which it depends is:

$$u_c(y(x_1, x_2, \dots, x_n)) = \sqrt{\sum_{i=1}^n u(y, x_i)^2}$$

where x is expressed as a relative standard uncertainty of the individual parameter.

The individual uncertainties taken into account include those associated with weights (calibration of the balance) and volumes (calibration of the volumetric glassware). An expanded maximum combined percent relative uncertainty of $\pm 5\%$ (calculated with a coverage factor of 2 and a level of confidence of 95%) is stated on the Certificate of Analysis for all of our products.

TRACEABILITY:

All reference standard solutions are traceable to specific crystalline lots. The microbalances used for solution preparation are regularly tested by an external ISO/IEC 17025 accredited calibration company. In addition, their calibration is verified prior to each weighing using NIST and/or NRC traceable external weights. All volumetric glassware used is of Class A tolerance and has been tested according to the appropriate ASTM procedures, which are ultimately traceable to NIST. For certain products, traceability to international interlaboratory studies has also been established.

EXPIRY DATE / PERIOD OF VALIDITY:


Ongoing stability studies of this product have demonstrated stability in its composition and concentration, until the specified expiry date, in the unopened ampoule. Monitoring for any degradation or change in concentration of the listed analyte(s) is performed on a routine basis.

LIMITED WARRANTY:

At the time of shipment, all products are warranted to be free of defects in material and workmanship and to conform to the stated technical and purity specifications.

QUALITY MANAGEMENT:

This product was produced using a Quality Management System registered to the latest versions of ISO 9001 by SAI Global, ISO/IEC 17025 by the Canadian Association for Laboratory Accreditation Inc. (CALA; A 1226), and ISO GUIDE 34 by ANSI-ASQ National Accreditation Board (ANAB; AR-1523).



For additional information or assistance concerning this or any other products from Wellington Laboratories Inc., please visit our website at www.well-labs.com or contact us directly at info@well-labs.com

Table A: br-PFOSK; Isomeric Components and Percent Composition (by ¹⁹F-NMR)*



Isomer	Name	Structure	Percent Composition by ¹⁹ F-NMR
1	Potassium perfluoro-1-octanesulfonate	CF ₃ CF ₂ CF ₂ CF ₂ CF ₂ CF ₂ CF ₂ CF ₂ SO ₃ ⁻ K ⁺	78.8
2	Potassium 1-trifluoromethylperfluoroheptanesulfonate**	CF ₃ CF ₂ CF ₂ CF ₂ CF ₂ CF ₂ CF ₂ SO ₃ ⁻ K ⁺ CF ₃	1.2
3	Potassium 2-trifluoromethylperfluoroheptanesulfonate	CF ₃ CF ₂ CF ₂ CF ₂ CF ₂ CF ₂ CF ₂ SO ₃ ⁻ K ⁺ CF ₃	0.6
4	Potassium 3-trifluoromethylperfluoroheptanesulfonate	CF ₃ CF ₂ CF ₂ CF ₂ CF ₂ CF ₂ CF ₂ SO ₃ ⁻ K ⁺ CF ₃	1.9
5	Potassium 4-trifluoromethylperfluoroheptanesulfonate	CF ₃ CF ₂ CF ₂ CF ₂ CF ₂ CF ₂ CF ₂ SO ₃ ⁻ K ⁺ CF ₃	2.2
6	Potassium 5-trifluoromethylperfluoroheptanesulfonate	CF ₃ CF ₂ CF ₂ CF ₂ CF ₂ CF ₂ CF ₂ SO ₃ ⁻ K ⁺ CF ₃	4.5
7	Potassium 6-trifluoromethylperfluoroheptanesulfonate	CF ₃ CF ₂ CF ₂ CF ₂ CF ₂ CF ₂ CF ₂ SO ₃ ⁻ K ⁺ CF ₃	10.0
8	Potassium 5,5-di(trifluoromethyl)perfluorohexanesulfonate	CF ₃ CF ₂ CF ₂ CF ₂ CF ₂ CF ₂ SO ₃ ⁻ K ⁺ CF ₃ CF ₃	0.2
9	Potassium 4,4-di(trifluoromethyl)perfluorohexanesulfonate	CF ₃ CF ₂ CF ₂ CF ₂ CF ₂ CF ₂ SO ₃ ⁻ K ⁺ CF ₃ CF ₃	0.03
10	Potassium 4,5-di(trifluoromethyl)perfluorohexanesulfonate	CF ₃ CF ₂ CF ₂ CF ₂ CF ₂ CF ₂ SO ₃ ⁻ K ⁺ CF ₃ CF ₃	0.4
11	Potassium 3,5-di(trifluoromethyl)perfluorohexanesulfonate	CF ₃ CF ₂ CF ₂ CF ₂ CF ₂ CF ₂ SO ₃ ⁻ K ⁺ CF ₃ CF ₃	0.07

* Percent of total perfluorooctanesulfonate isomers only. Isomers are labelled in Figure 2.
 ** Systematic Name: Potassium perfluorooctane-2-sulfonate.

Certified By: 
 B.G. Chittim

Date: 01/20/2017
 (mm/dd/yyyy)

Figure 1: br-PFOSK; LC/MS Data (TIC and Mass Spectrum)

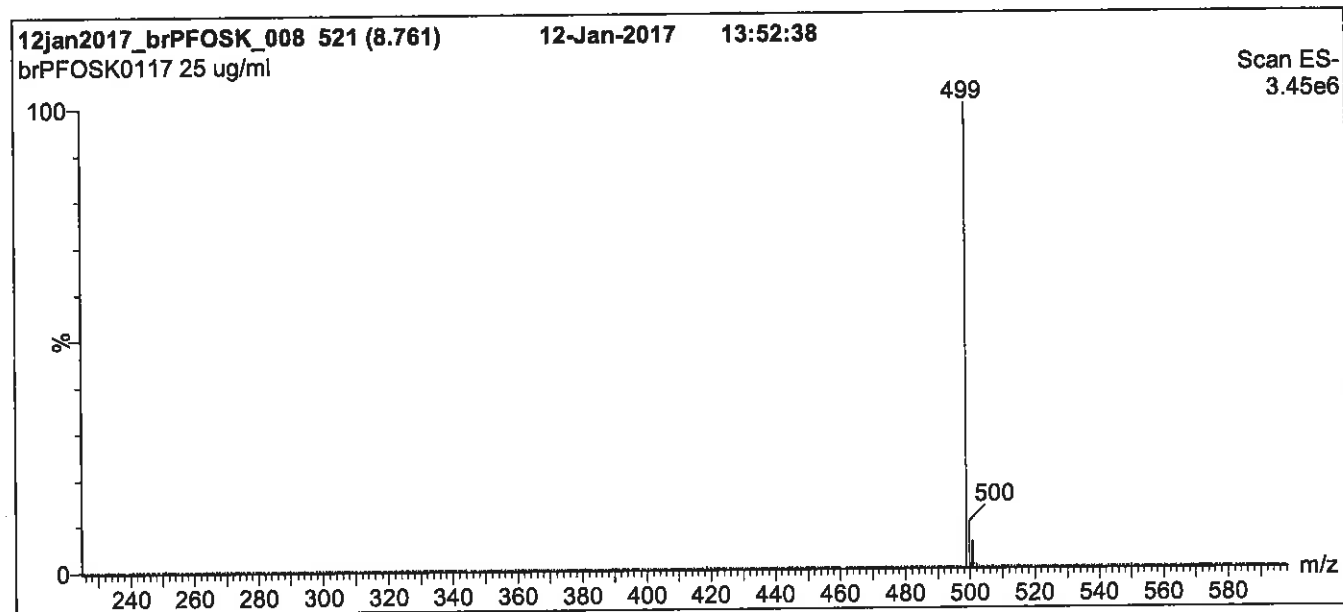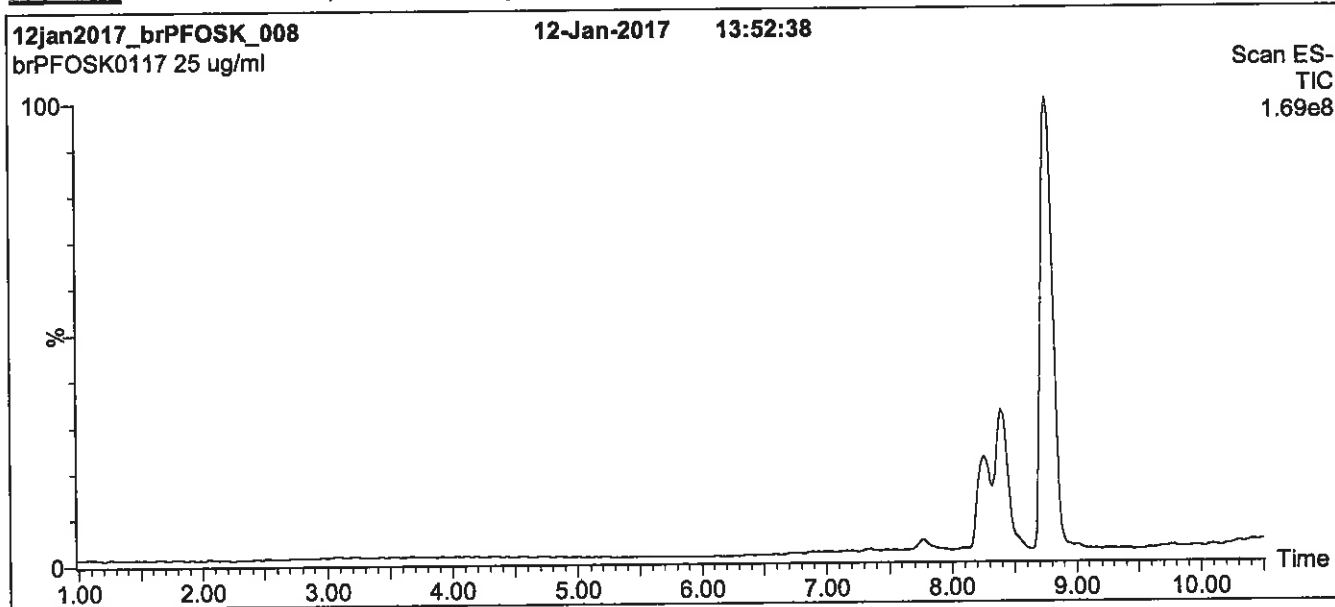

Conditions for Figure 1:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS

Chromatographic Conditions

Column: Acquity UPLC BEH Shield RP₁₈
 1.7 μ m, 2.1 x 100 mm

Mobile phase: Gradient
 Start: 45% (80:20 MeOH:ACN) / 55% H₂O
 (both with 10 mM NH₄OAc buffer)
 Ramp to 90% organic over 12 min and hold for 2 min.
 Return to initial conditions over 0.5 min.
 Time: 16 min


Flow: 300 μ l/min

MS Parameters

Experiment: Full Scan (225 - 850 amu)

Source: Electrospray (negative)
 Capillary Voltage (kV) = 3.00
 Cone Voltage (V) = 60.00
 Cone Gas Flow (l/hr) = 50
 Desolvation Gas Flow (l/hr) = 750

Figure 2: br-PFOSK; LC/MS Data (SIR)

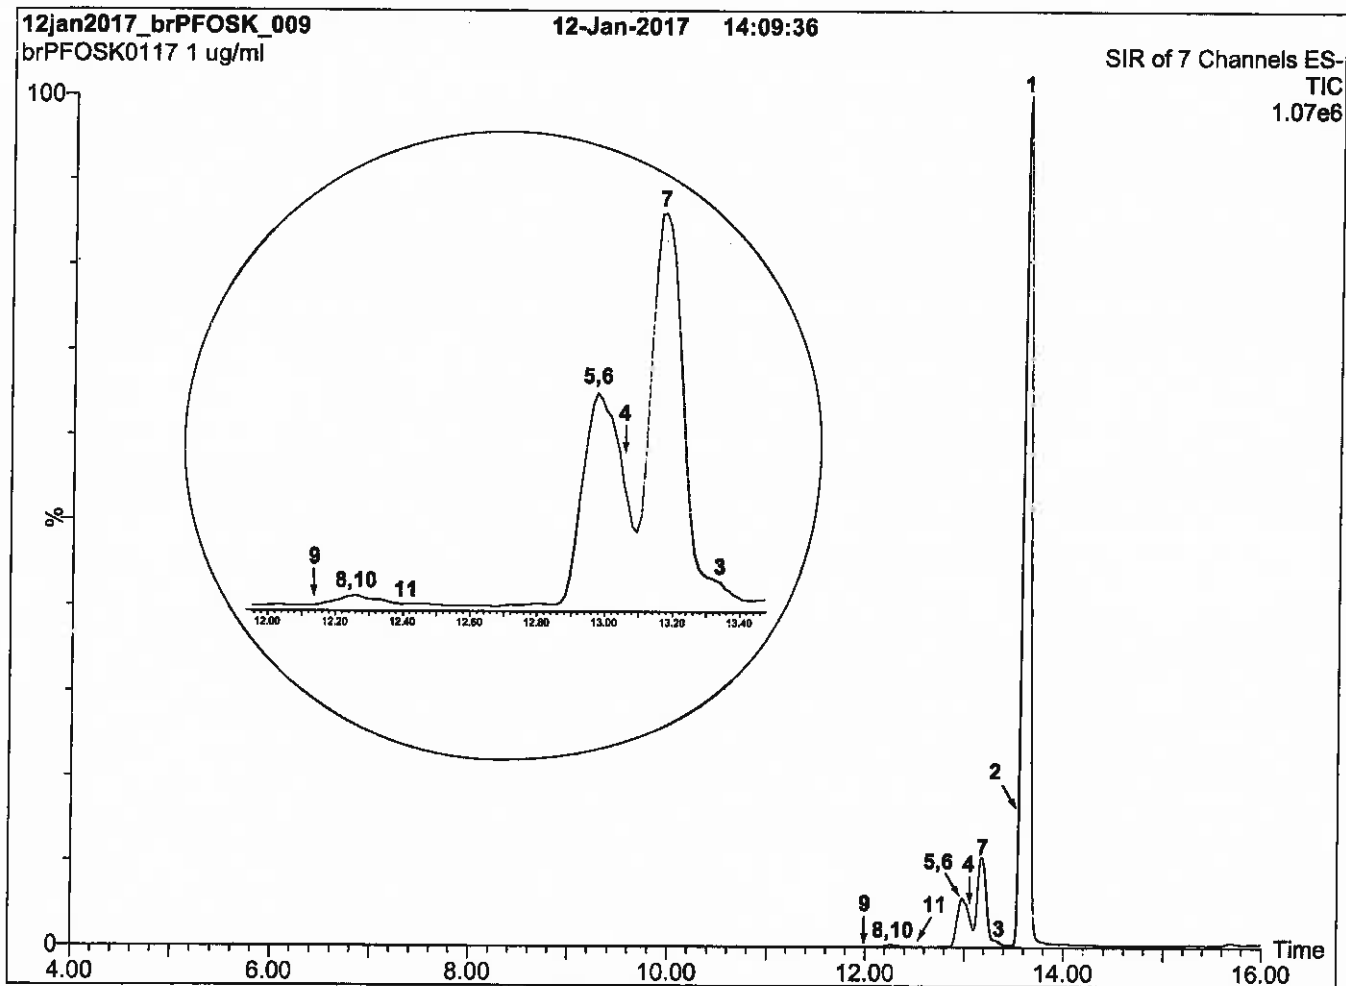

Conditions for Figure 2:

LC: Waters Acquity Ultra Performance LC
MS: Micromass Quattro *micro* API MS


Chromatographic Conditions:

Column: Acquity UPLC BEH Shield RP₁₈ (1.7 μ m, 2.1 x 100 mm)
Injection: 1.0 μ g/ml of br-PFOSK
Mobile Phase: Gradient
45% (80:20 MeOH:ACN) / 55% H₂O (both with 10 mM NH₄OAc buffer)
Ramp to 90% organic over 15 min and hold for 3 min.
Return to Initial conditions over 1 min.
Time: 20 min
Flow: 300 μ l/min

MS Conditions:

SIR (ES)
Source = 110 °C
Desolvation = 325 °C
Cone Voltage = 60V

Figure 3: br-PFOSK; LC/MS/MS Data (Selected MRM Transitions)

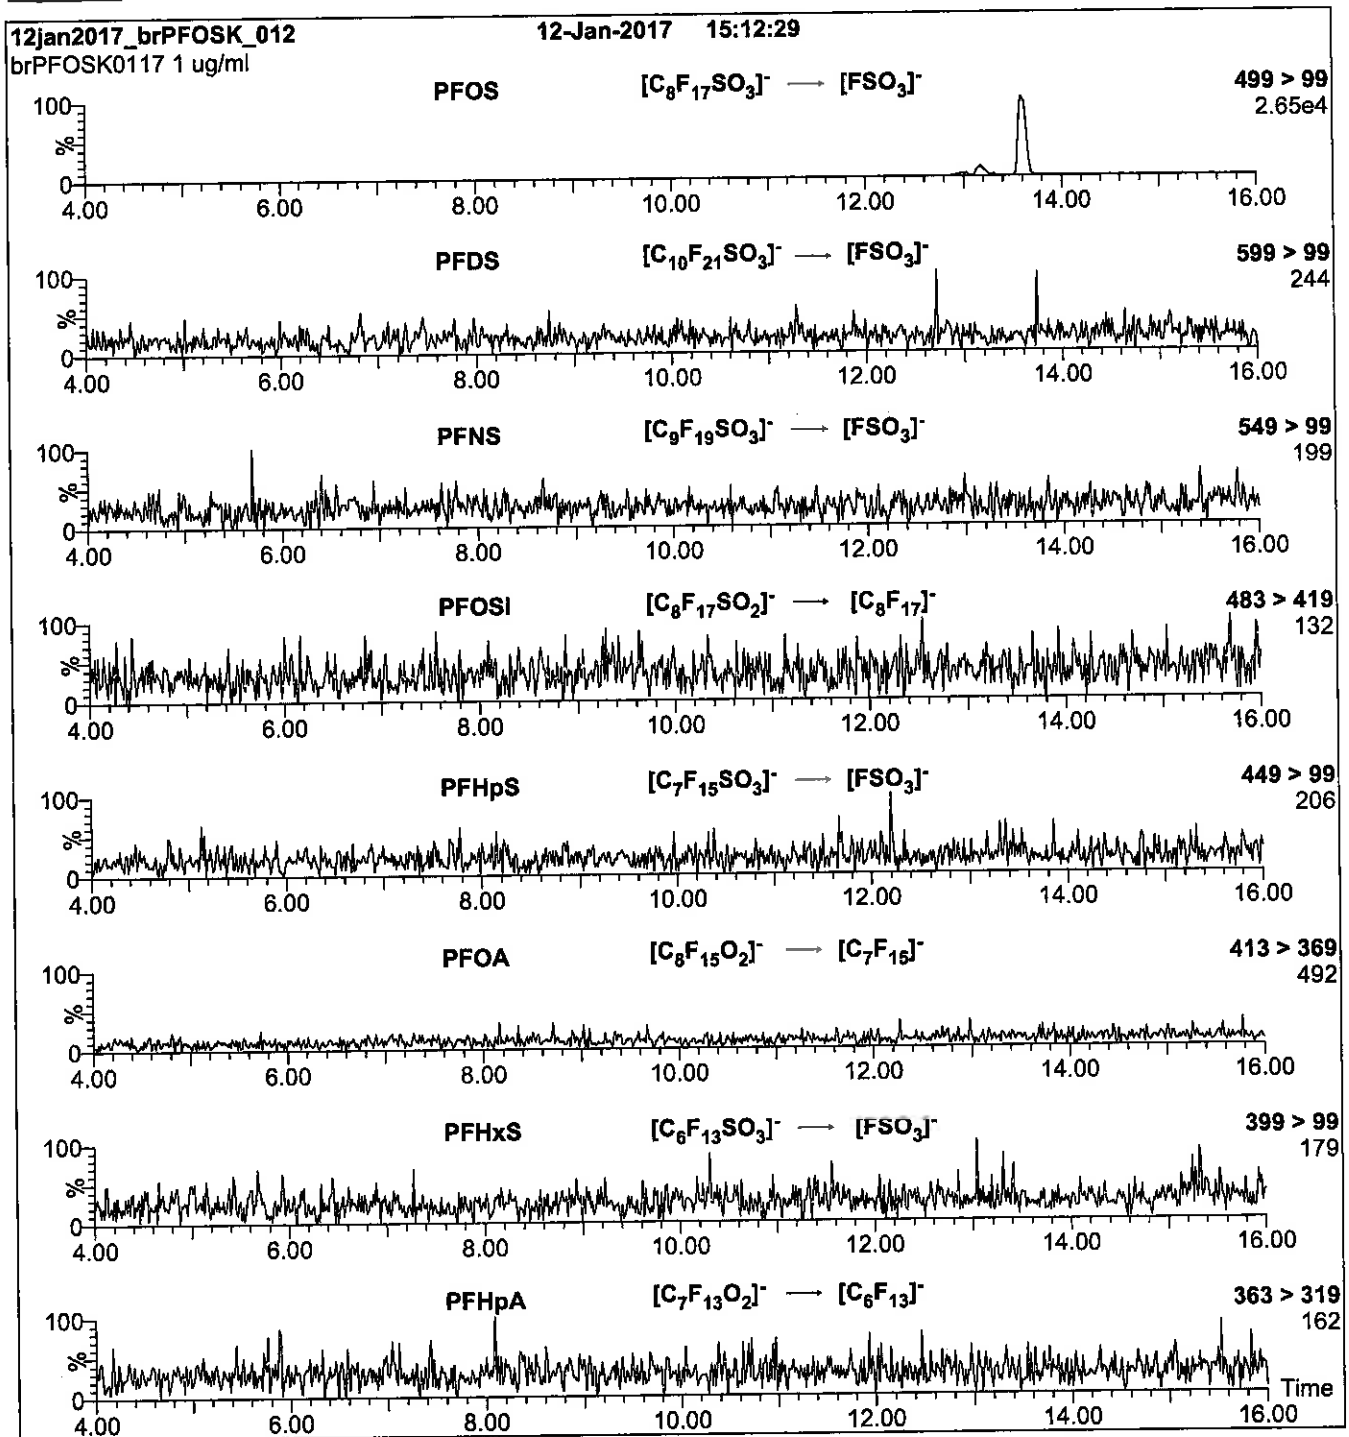

Conditions for Figure 3:

Injection: On-column

Mobile phase: Same as Figure 2

Flow: 300 μ l/min

MS Parameters

Collision Gas (mbar) = 3.31e-3

Collision Energy (eV) = 11-50 (variable)

Method 537 DOD

Perfluorinated Alkyl Acids (LC/MS)
by Method 537 DOD

FORM II
LCMS SURROGATE RECOVERY

Lab Name: TestAmerica Sacramento

Job No.: 320-38382-1

SDG No.: _____

Matrix: Water

Level: Low

GC Column (1): GeminiC18 3 ID: 3 (mm)

Client Sample ID	Lab Sample ID	PFHxA #	PFDA #
NAWC-041918-RW-154	320-38382-1	100	89
NAWC-041918-FRB-154	320-38382-2	106	85
NAWC-041918-RW-146	320-38382-3	100	83
NAWC-041918-FRB-146	320-38382-4	106	88
NAWC-041918-RW-258	320-38382-5	98	80
NAWC-041918-FRB-258	320-38382-6	106	85
WGNA-041918-RW-357	320-38382-7	99	79
WGNA-041918-FRB-357	320-38382-8	103	87
	MB 320-219896/1-A	107	90
	LCS 320-219896/2-A	108	91
NAWC-041918-RW-154 MS	320-38382-1 MS	96	84
NAWC-041918-RW-154 MSD	320-38382-1 MSD	66 Q	74

PFHxA = 13C2 PFHxA
PFDA = 13C2 PFDA

QC LIMITS
70-130
70-130

Column to be used to flag recovery values

FORM III
LCMS LAB CONTROL SAMPLE RECOVERY

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Matrix: Water Level: Low Lab File ID: 2018.05.01_537AA_018.d
 Lab ID: LCS 320-219896/2-A Client ID: _____

COMPOUND	SPIKE ADDED (ng/L)	LCS CONCENTRATION (ng/L)	LCS % REC	QC LIMITS REC	#
Perfluorooctanesulfonic acid (PFOS)	220	225	103	70-130	M
Perfluorooctanoic acid (PFOA)	110	110	100	70-130	
Perfluorononanoic acid (PFNA)	110	102	93	70-130	
Perfluorohexanesulfonic acid (PFHxS)	168	179	106	70-130	
Perfluoroheptanoic acid (PFHpA)	54.0	58.2	108	70-130	
Perfluorobutanesulfonic acid (PFBS)	500	519	104	70-130	

Column to be used to flag recovery and RPD values

FORM III
LCMS MATRIX SPIKE RECOVERY

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Matrix: Water Level: Low Lab File ID: 2018.05.01_537AA_020.d
 Lab ID: 320-38382-1 MS Client ID: NAWC-041918-RW-154 MS

COMPOUND	SPIKE ADDED (ng/L)	SAMPLE CONCENTRATION (ng/L)	MS CONCENTRATION (ng/L)	MS % REC	QC LIMITS REC	#
Perfluorooctanesulfonic acid (PFOS)	217	17 J	237	102	70-130	M
Perfluorooctanoic acid (PFOA)	109	24	124	92	70-130	
Perfluorononanoic acid (PFNA)	109	20 U	98.7	91	70-130	
Perfluorohexanesulfonic acid (PFHxS)	166	12 U	177	106	70-130	
Perfluoroheptanoic acid (PFHpA)	53.5	8.1 J	59.8	97	70-130	
Perfluorobutanesulfonic acid (PFBS)	495	36 U	523	105	70-130	

Column to be used to flag recovery and RPD values

FORM III
LCMS MATRIX SPIKE DUPLICATE RECOVERY

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Matrix: Water Level: Low Lab File ID: 2018.05.01_537AA_021.d
 Lab ID: 320-38382-1 MSD Client ID: NAWC-041918-RW-154 MSD

COMPOUND	SPIKE ADDED (ng/L)	MSD CONCENTRATION (ng/L)	MSD % REC	% RPD	QC LIMITS		#
					RPD	REC	
Perfluorooctanesulfonic acid (PFOS)	217	185	78	25	30	70-130	M
Perfluorooctanoic acid (PFOA)	109	89.8	60	32	30	70-130	J1
Perfluorononanoic acid (PFNA)	109	77.7	71	24	30	70-130	
Perfluorohexanesulfonic acid (PFHxS)	166	116	70	41	30	70-130	J1
Perfluoroheptanoic acid (PFHpA)	53.4	41.1	62	37	30	70-130	J1
Perfluorobutanesulfonic acid (PFBS)	495	347	70	40	30	70-130	J1

Column to be used to flag recovery and RPD values

FORM IV
LCMS METHOD BLANK SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Lab File ID: 2018.05.01_537AA_017.d Lab Sample ID: MB 320-219896/1-A
 Matrix: Water Date Extracted: 04/26/2018 09:35
 Instrument ID: A8_N Date Analyzed: 05/01/2018 12:24
 Level: (Low/Med) Low

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES:

CLIENT SAMPLE ID	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED
	LCS 320-219896/2-A	2018.05.01_537AA 018.d	05/01/2018 12:29
NAWC-041918-RW-154	320-38382-1	2018.05.01_537AA 019.d	05/01/2018 12:34
NAWC-041918-RW-154 MS	320-38382-1 MS	2018.05.01_537AA 020.d	05/01/2018 12:38
NAWC-041918-RW-154 MSD	320-38382-1 MSD	2018.05.01_537AA 021.d	05/01/2018 12:43
NAWC-041918-FRB-154	320-38382-2	2018.05.01_537AA 022.d	05/01/2018 12:48
NAWC-041918-RW-146	320-38382-3	2018.05.01_537AA 023.d	05/01/2018 12:52
NAWC-041918-FRB-146	320-38382-4	2018.05.01_537AA 024.d	05/01/2018 12:57
NAWC-041918-RW-258	320-38382-5	2018.05.01_537AA 025.d	05/01/2018 13:02
NAWC-041918-FRB-258	320-38382-6	2018.05.01_537AA 026.d	05/01/2018 13:06
WGNA-041918-RW-3571	320-38382-7	2018.05.01_537AA 029.d	05/01/2018 13:20
WGNA-041918-FRB-3571	320-38382-8	2018.05.01_537AA 030.d	05/01/2018 13:25

FORM VIII
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Instrument ID: A8_N Calibration Start Date: 04/11/2018 11:45
 GC Column: GeminiC18 3x100 ID: 3(mm) Calibration End Date: 04/11/2018 12:09
 Calibration ID: 38530

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
INITIAL CALIBRATION MEAN AREA AND MEAN RT	970041	1.86	2344935	2.10		
UPPER LIMIT	1455062	2.36	3517403	2.60		
LOWER LIMIT	485021	1.36	1172468	1.60		
LAB SAMPLE ID	CLIENT SAMPLE ID					
CCVL 320-217453/10	964533	1.87	2387973	2.10		
ICV 320-217453/12	1123391	1.86	2710764	2.10		
CCVL 320-220842/1	950434	1.90	2226982	2.12		
CCV 320-220845/13 CCVIS	1006734	1.88	2332599	2.12		
MB 320-219896/1-A	896308	1.89	2119146	2.12		
LCS 320-219896/2-A	885760	1.90	2152883	2.12		
320-38382-1	NAWC-041918-RW-154	918602	2172570	2.12		
320-38382-1 MS	NAWC-041918-RW-154 MS	873603	1979894	2.12		
320-38382-1 MSD	NAWC-041918-RW-154 MSD	927451	2186239	2.12		
320-38382-2	NAWC-041918-FRB-154	931565	2174288	2.12		
320-38382-3	NAWC-041918-RW-146	908929	2119366	2.12		
320-38382-4	NAWC-041918-FRB-146	907706	2174599	2.12		
320-38382-5	NAWC-041918-RW-258	877855	2070367	2.12		
320-38382-6	NAWC-041918-FRB-258	880431	2120366	2.11		
CCV 320-220845/25 CCVIS		848761	2054615	2.11		
CCV 320-220847/25 CCVIS		848761	2054615	2.11		
320-38382-7	WGNA-041918-RW-3571	849895	1937754	2.11		
320-38382-8	WGNA-041918-FRB-3571	836252	1978104	2.11		
CCV 320-220847/29 CCVIS		851622	2073725	2.11		

13PFOA = 13C2-PFOA

PFOS = 13C4 PFOS

Area Limit = 50%-150% of internal standard area
 RT Limit = ± 0.5 minutes of internal standard RT

Column used to flag values outside QC limits

FORM VIII
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Sample No.: CCV 320-220845/13 Date Analyzed: 05/01/2018 12:15
 Instrument ID: A8_N GC Column: GeminiC18 3x100 ID: 3 (mm)
 Lab File ID (Standard): 2018.05.01_537AA_01 Heated Purge: (Y/N) N
 Calibration ID: 38530

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	1006734	1.88	2332599	2.12		
UPPER LIMIT	1409428	2.38	3265639	2.62		
LOWER LIMIT	704714	1.38	1632819	1.62		
LAB SAMPLE ID	CLIENT SAMPLE ID					
MB 320-219896/1-A		896308	1.89	2119146	2.12	
LCS 320-219896/2-A		885760	1.90	2152883	2.12	
320-38382-1	NAWC-041918-RW-154	918602	1.89	2172570	2.12	
320-38382-1 MS	NAWC-041918-RW-154 MS	873603	1.89	1979894	2.12	
320-38382-1 MSD	NAWC-041918-RW-154 MSD	927451	1.89	2186239	2.12	
320-38382-2	NAWC-041918-FRB-154	931565	1.88	2174288	2.12	
320-38382-3	NAWC-041918-RW-146	908929	1.89	2119366	2.12	
320-38382-4	NAWC-041918-FRB-146	907706	1.89	2174599	2.12	
320-38382-5	NAWC-041918-RW-258	877855	1.89	2070367	2.12	
320-38382-6	NAWC-041918-FRB-258	880431	1.88	2120366	2.11	

13PFOA = 13C2-PFOA

PFOS = 13C4 PFOS

Area Limit = 70%-140% of internal standard area
 RT Limit = ± 0.5 minutes of internal standard RT

Column used to flag values outside QC limits

FORM VIII
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Sample No.: CCV 320-220845/25 Date Analyzed: 05/01/2018 13:11
 Instrument ID: A8_N GC Column: GeminiC18 3x100 ID: 3 (mm)
 Lab File ID (Standard): 2018.05.01_537AA_02 Heated Purge: (Y/N) N
 Calibration ID: 38530

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	848761	1.88	2054615	2.11		
UPPER LIMIT	1188265	2.38	2876461	2.61		
LOWER LIMIT	594133	1.38	1438231	1.61		
LAB SAMPLE ID	CLIENT SAMPLE ID					
MB 320-219896/1-A		896308	1.89	2119146	2.12	
LCS 320-219896/2-A		885760	1.90	2152883	2.12	
320-38382-1	NAWC-041918-RW-154	918602	1.89	2172570	2.12	
320-38382-1 MS	NAWC-041918-RW-154 MS	873603	1.89	1979894	2.12	
320-38382-1 MSD	NAWC-041918-RW-154 MSD	927451	1.89	2186239	2.12	
320-38382-2	NAWC-041918-FRB-154	931565	1.88	2174288	2.12	
320-38382-3	NAWC-041918-RW-146	908929	1.89	2119366	2.12	
320-38382-4	NAWC-041918-FRB-146	907706	1.89	2174599	2.12	
320-38382-5	NAWC-041918-RW-258	877855	1.89	2070367	2.12	
320-38382-6	NAWC-041918-FRB-258	880431	1.88	2120366	2.11	

13PFOA = 13C2-PFOA
 PFOS = 13C4 PFOS

Area Limit = 70%-140% of internal standard area
 RT Limit = ± 0.5 minutes of internal standard RT

Column used to flag values outside QC limits

FORM VIII
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Sample No.: CCV 320-220847/25 Date Analyzed: 05/01/2018 13:11
 Instrument ID: A8_N GC Column: GeminiC18 3x100 ID: 3 (mm)
 Lab File ID (Standard): 2018.05.01_537AA_02 Heated Purge: (Y/N) N
 Calibration ID: 38530

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	848761	1.88	2054615	2.11		
UPPER LIMIT	1188265	2.38	2876461	2.61		
LOWER LIMIT	594133	1.38	1438231	1.61		
LAB SAMPLE ID	CLIENT SAMPLE ID					
320-38382-7	WGNA-041918-RW-3571	849895	1.87	1937754	2.11	
320-38382-8	WGNA-041918-FRB-3571	836252	1.88	1978104	2.11	

13PFOA = 13C2-PFOA
 PFOS = 13C4 PFOS

Area Limit = 70%-140% of internal standard area
 RT Limit = ± 0.5 minutes of internal standard RT

Column used to flag values outside QC limits

FORM VIII
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Sample No.: CCV 320-220847/29 Date Analyzed: 05/01/2018 13:30
 Instrument ID: A8_N GC Column: GeminiC18 3x100 ID: 3 (mm)
 Lab File ID (Standard): 2018.05.01_537AA_03 Heated Purge: (Y/N) N
 Calibration ID: 38530

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	851622	1.88	2073725	2.11		
UPPER LIMIT	1192271	2.38	2903215	2.61		
LOWER LIMIT	596135	1.38	1451608	1.61		
LAB SAMPLE ID	CLIENT SAMPLE ID					
320-38382-7	WGNA-041918-RW-3571		849895	1.87	1937754	2.11
320-38382-8	WGNA-041918-FRB-3571		836252	1.88	1978104	2.11

13PFOA = 13C2-PFOA
 PFOS = 13C4 PFOS

Area Limit = 70%-140% of internal standard area
 RT Limit = ± 0.5 minutes of internal standard RT

Column used to flag values outside QC limits

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Client Sample ID: NAWC-041918-RW-154 Lab Sample ID: 320-38382-1
 Matrix: Water Lab File ID: 2018.05.01_537AA_019.d
 Analysis Method: 537 Date Collected: 04/19/2018 09:10
 Extraction Method: 537 Date Extracted: 04/26/2018 09:35
 Sample wt/vol: 252.2 (mL) Date Analyzed: 05/01/2018 12:34
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 220845 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	17	J M	40	16	6.7
335-67-1	Perfluorooctanoic acid (PFOA)	24		20	7.9	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U M	24	20	7.9
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U M	30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	8.1	J	9.9	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	89	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	100		70-130
STL00996	13C2 PFDA	89		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_019.d
 Lims ID: 320-38382-A-1-A
 Client ID: NAWC-041918-RW-154
 Sample Type: Client
 Inject. Date: 01-May-2018 12:34:02 ALS Bottle#: 12 Worklist Smp#: 17
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-38382-a-1-a
 Misc. Info.: Plate: 1 Rack: 6
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 02-May-2018 10:24:00 Calib Date: 11-Apr-2018 12:09:09
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK005

First Level Reviewer: barnettj Date: 01-May-2018 17:13:10

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.396	1.388	0.008	1.000	165732	2.08		114	
298.90 > 99.00	1.396	1.388	0.008	1.000	131238		1.26(0.00-0.00)	128	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.533	1.533	0.0	1.000	971950	9.95		8114	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.692	1.692	0.0	1.000	145593	1.17		41.2	M
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.692	1.692	0.0	1.000	201963	2.05		16.1	
* 6 13C2-PFOA									
415.00 > 370.00	1.889	1.882	0.007		918602	10.0		5122	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.889	1.889	0.0	1.000	594807	6.10		66.3	
413.00 > 169.00	1.889	1.889	0.0	1.000	349708		1.70(0.00-0.00)	268	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.117	2.117	0.0	1.000	336940	4.17		62.9	a
499.00 > 99.00	2.117	2.117	0.0	1.000	57468		5.86(0.00-0.00)	72.8	a
* 7 13C4 PFOS									
503.00 > 80.00	2.117	2.117	0.0		2172570	28.7		1121	
9 Perfluorononanoic acid									
463.00 > 419.00	2.124	2.124	0.0	1.000	45868	0.5927		6.1	M
\$ 10 13C2 PFDA									
515.00 > 470.00	2.269	2.269	0.0	1.000	692506	8.86		5722	

QC Flag Legend


Review Flags

M - Manually Integrated


a - User Assigned ID

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_019.d
Injection Date: 01-May-2018 12:34:02 Instrument ID: A8_N
Lims ID: 320-38382-A-1-A Lab Sample ID: 320-38382-1
Client ID: NAWC-041918-RW-154
Operator ID: SACINSTLCMS01 ALS Bottle#: 12 Worklist Smp#: 17
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL

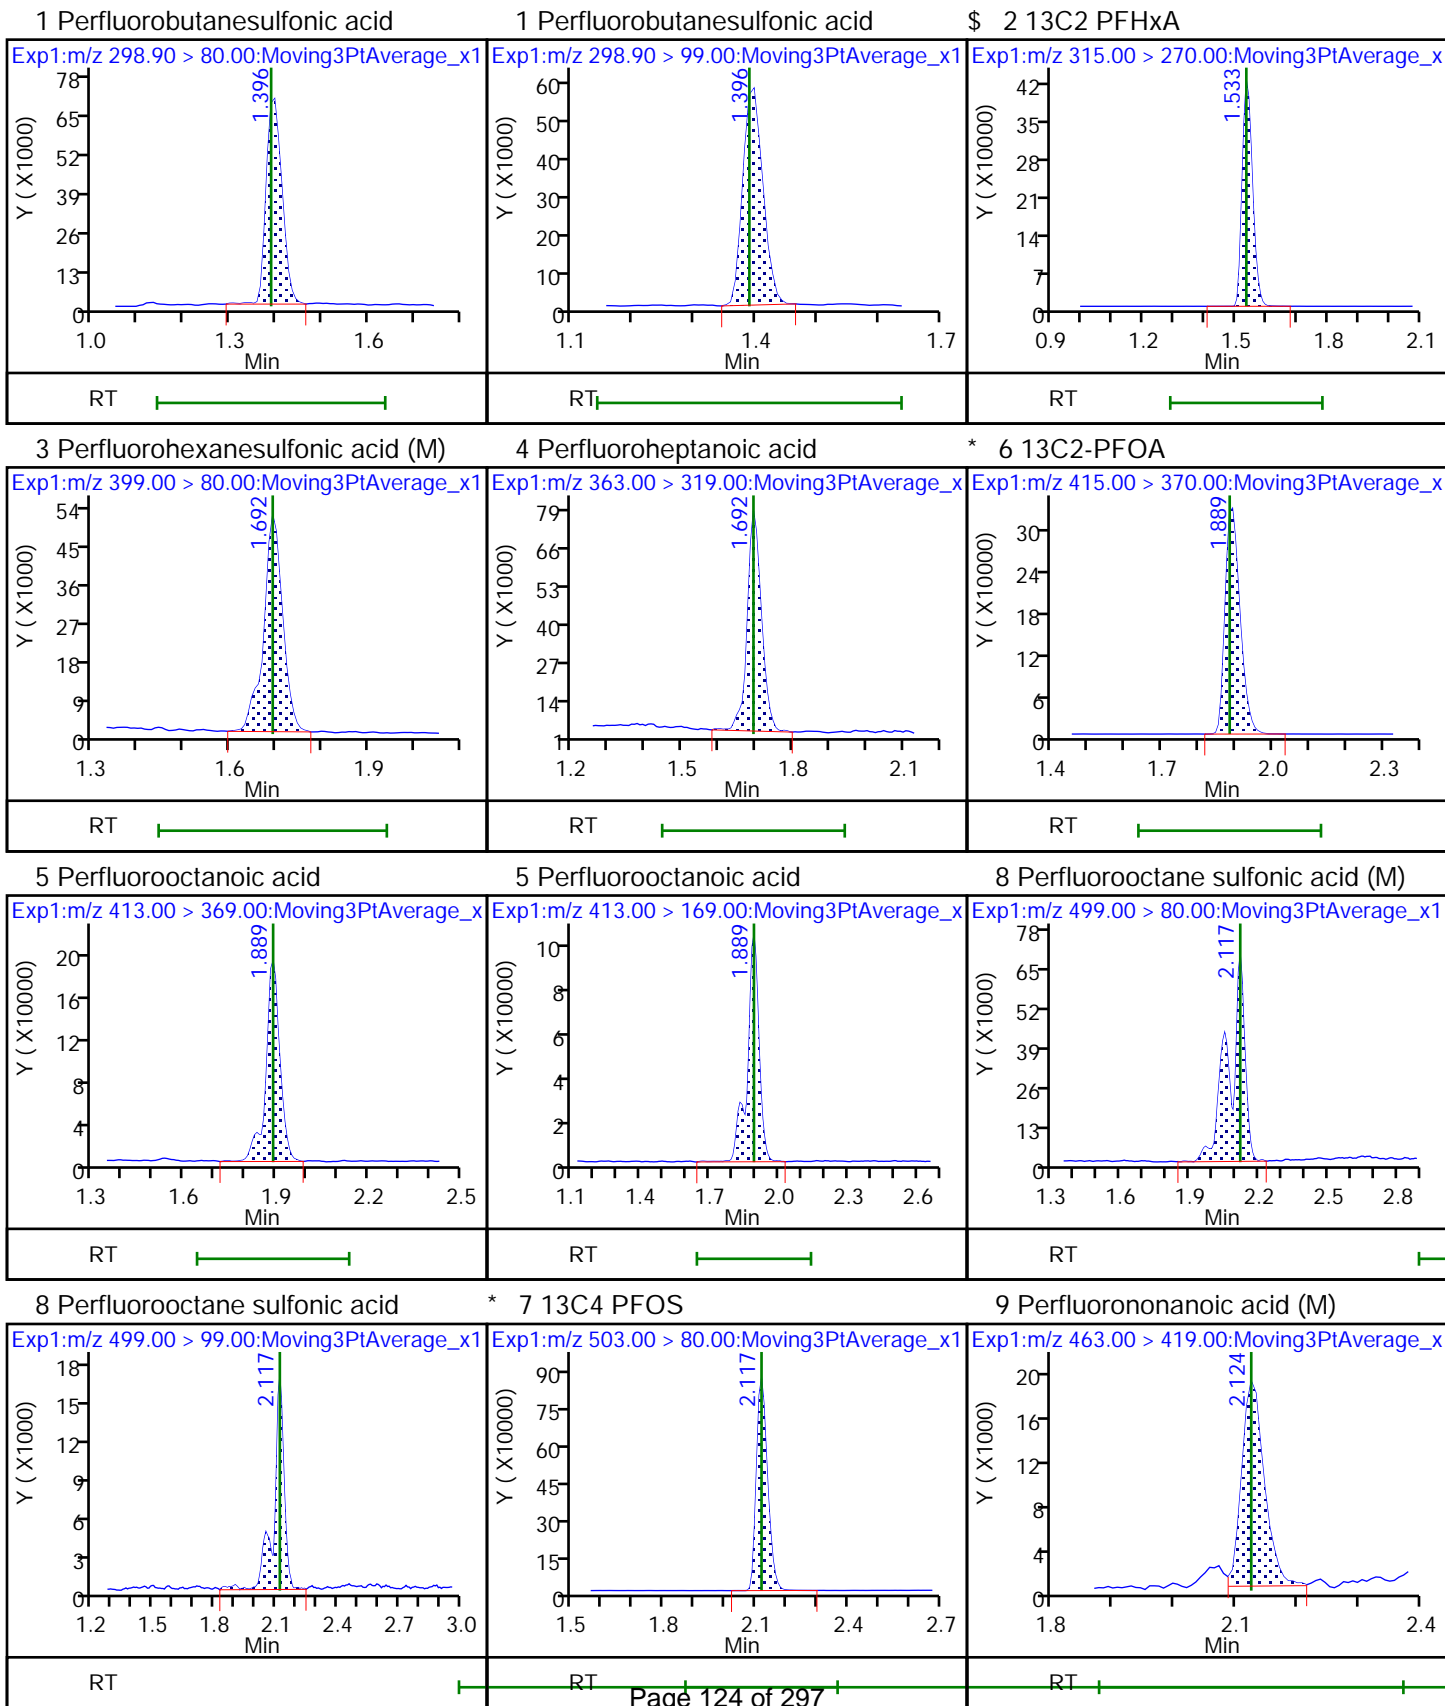

\$ 10 13C2 PFDA

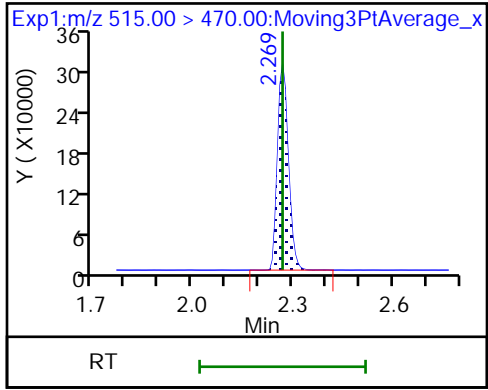

TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_019.d
 Lims ID: 320-38382-A-1-A
 Client ID: NAWC-041918-RW-154
 Sample Type: Client
 Inject. Date: 01-May-2018 12:34:02 ALS Bottle#: 12 Worklist Smp#: 17
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-38382-a-1-a
 Misc. Info.: Plate: 1 Rack: 6
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 02-May-2018 10:24:00 Calib Date: 11-Apr-2018 12:09:09
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK005

First Level Reviewer: barnettj Date: 01-May-2018 17:13:10

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	9.95	99.52
\$ 10 13C2 PFDA	10.0	8.86	88.64

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_019.d
Injection Date: 01-May-2018 12:34:02 Instrument ID: A8_N
Lims ID: 320-38382-A-1-A Lab Sample ID: 320-38382-1
Client ID: NAWC-041918-RW-154
Operator ID: SACINSTLCMS01 ALS Bottle#: 12 Worklist Smp#: 17
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1


Signal: 1

Not Detected
Expected RT: 2.12

Processing Integration Results

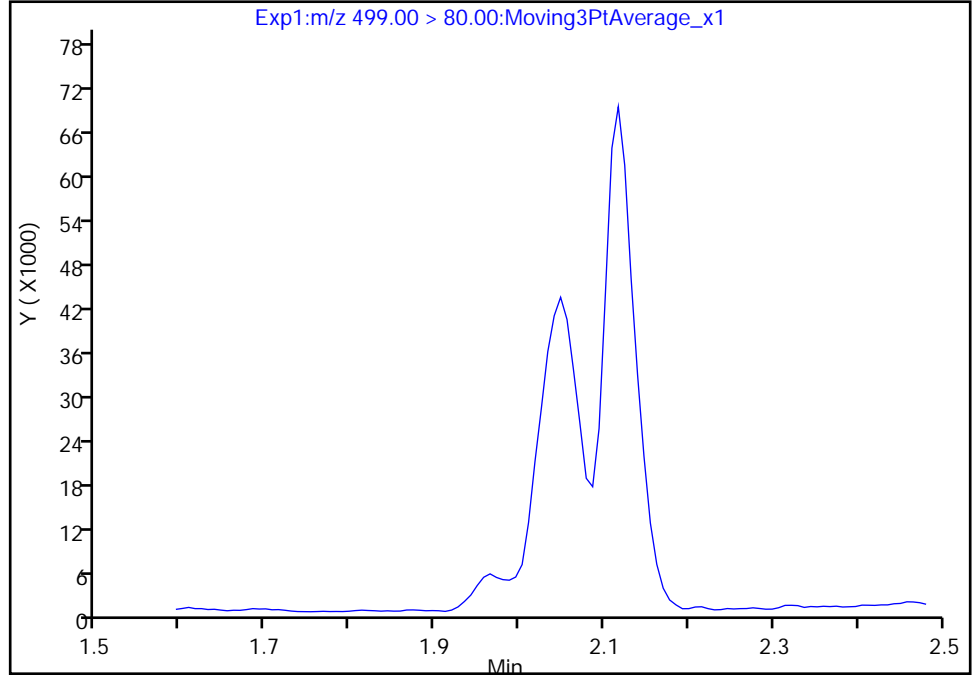

Manual Integration Results

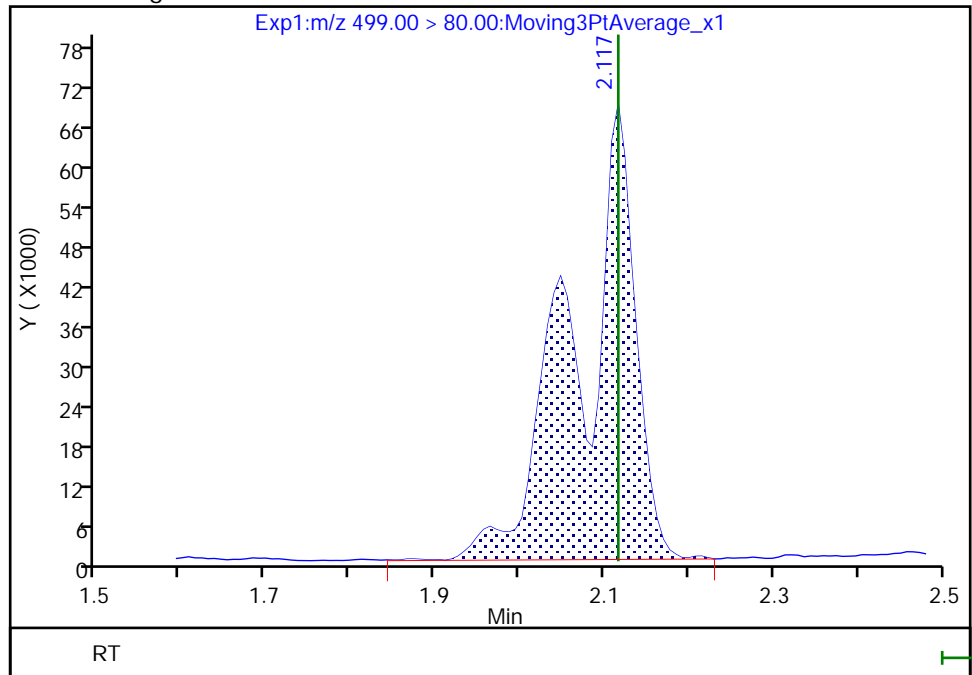

RT: 2.12
Area: 336940
Amount: 4.172257
Amount Units: ng/ml

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_019.d
Injection Date: 01-May-2018 12:34:02 Instrument ID: A8_N
Lims ID: 320-38382-A-1-A Lab Sample ID: 320-38382-1
Client ID: NAWC-041918-RW-154
Operator ID: SACINSTLCMS01 ALS Bottle#: 12 Worklist Smp#: 17
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

9 Perfluorononanoic acid, CAS: 375-95-1


Signal: 1

Not Detected
Expected RT: 2.12

Processing Integration Results

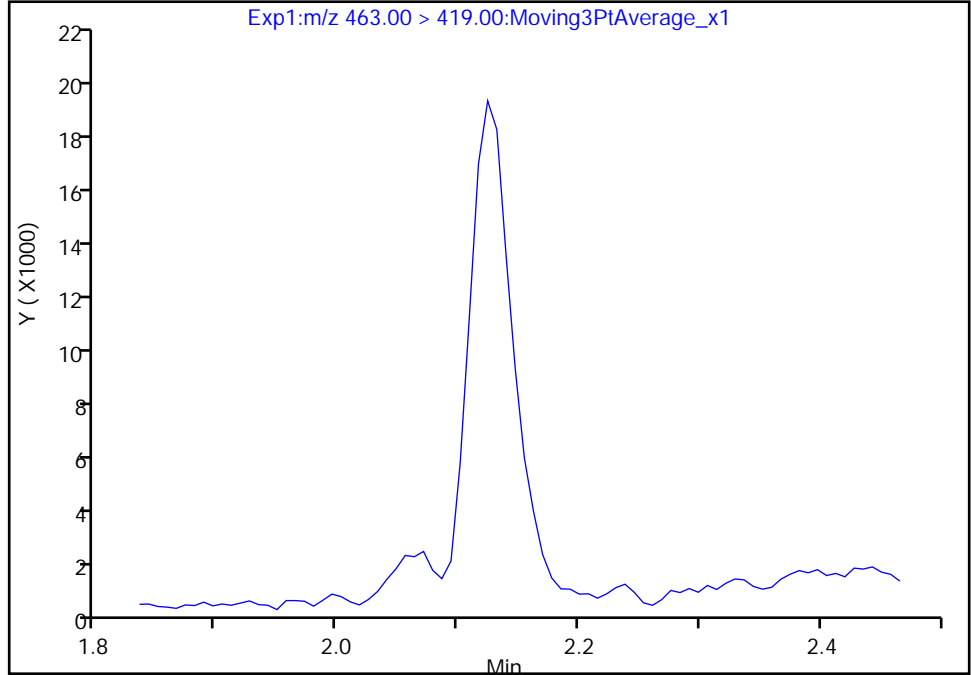

Manual Integration Results

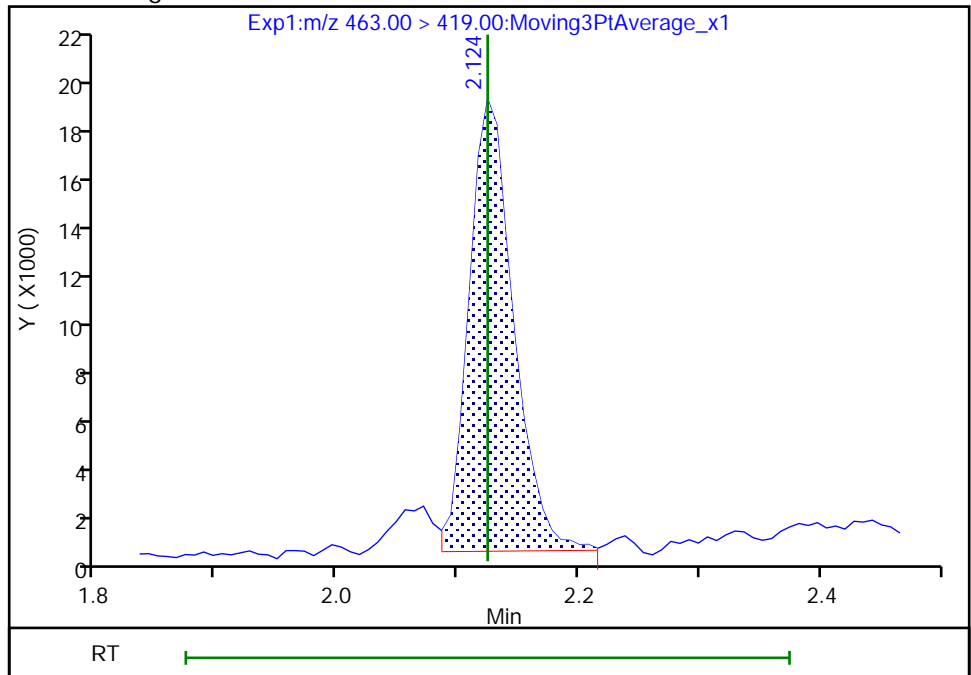

RT: 2.12
Area: 45868
Amount: 0.592746
Amount Units: ng/ml

Reviewer: barnettj, 01-May-2018 17:13:04
Audit Action: Manually Integrated

Audit Reason: Missed Peak
Page 128 of 297

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_019.d
Injection Date: 01-May-2018 12:34:02 Instrument ID: A8_N
Lims ID: 320-38382-A-1-A Lab Sample ID: 320-38382-1
Client ID: NAWC-041918-RW-154
Operator ID: SACINSTLCMS01 ALS Bottle#: 12 Worklist Smp#: 17
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

3 Perfluorohexanesulfonic acid, CAS: 355-46-4


Signal: 1

Not Detected
Expected RT: 1.69

Processing Integration Results

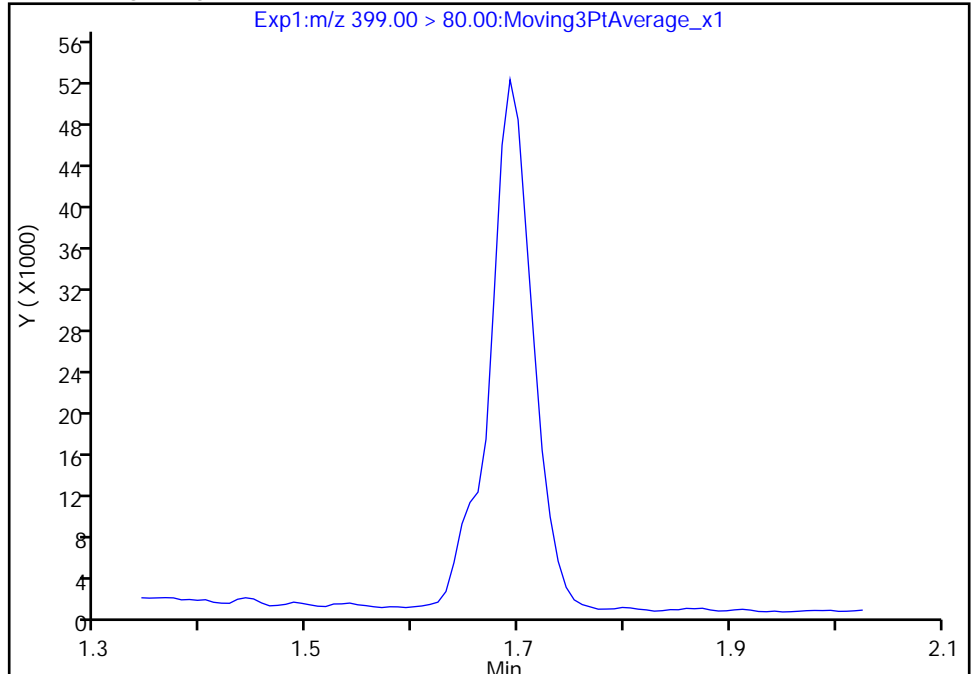

Manual Integration Results

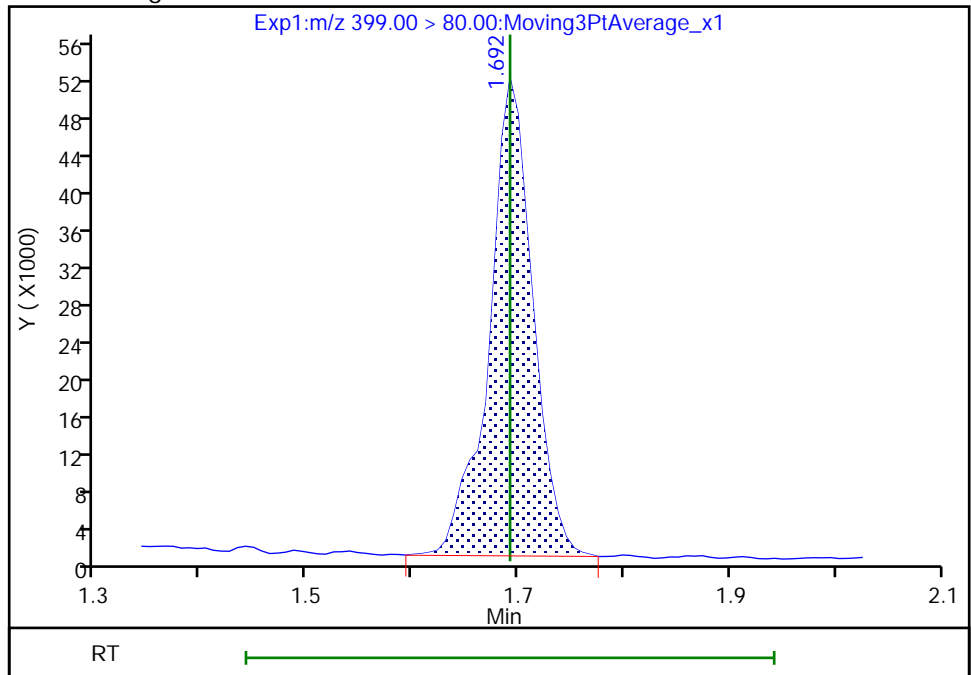

RT: 1.69
Area: 145593
Amount: 1.170339
Amount Units: ng/ml

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Client Sample ID: NAWC-041918-FRB-154 Lab Sample ID: 320-38382-2
 Matrix: Water Lab File ID: 2018.05.01_537AA_022.d
 Analysis Method: 537 Date Collected: 04/19/2018 09:05
 Extraction Method: 537 Date Extracted: 04/26/2018 09:35
 Sample wt/vol: 266.7(mL) Date Analyzed: 05/01/2018 12:48
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 220845 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	37	15	6.4
335-67-1	Perfluorooctanoic acid (PFOA)	7.5	U	19	7.5	2.6
375-95-1	Perfluorononanoic acid (PFNA)	19	U	22	19	7.5
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.7	U	9.4	3.7	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	84	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	106		70-130
STL00996	13C2 PFDA	85		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_022.d
 Lims ID: 320-38382-A-2-A
 Client ID: NAWC-041918-FRB-154
 Sample Type: Client
 Inject. Date: 01-May-2018 12:48:06 ALS Bottle#: 15 Worklist Smp#: 20
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-38382-a-2-a
 Misc. Info.: Plate: 1 Rack: 6
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 02-May-2018 10:24:00 Calib Date: 11-Apr-2018 12:09:09
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_009.d


Column 1 : Det: EXP1
 Process Host: XAWRK005

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
\$ 2 13C2 PFHxA	315.00 > 270.00	1.533	1.533	0.0	1.000	1048020	10.6	8131	
* 6 13C2-PFOA	415.00 > 370.00	1.882	1.882	0.0		931565	10.0	5469	
* 7 13C4 PFOS	503.00 > 80.00	2.117	2.117	0.0		2174288	28.7	1203	
\$ 10 13C2 PFDA	515.00 > 470.00	2.269	2.269	0.0	1.000	674585	8.51	5653	


TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_022.d
Injection Date: 01-May-2018 12:48:06 Instrument ID: A8_N
Lims ID: 320-38382-A-2-A Lab Sample ID: 320-38382-2
Client ID: NAWC-041918-FRB-154
Operator ID: SACINSTLCMS01 ALS Bottle#: 15 Worklist Smp#: 20
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL


1 Perfluorobutanesulfonic acid (ND) 1 Perfluorobutanesulfonic acid (ND) \$ 2 13C2 PFHxA

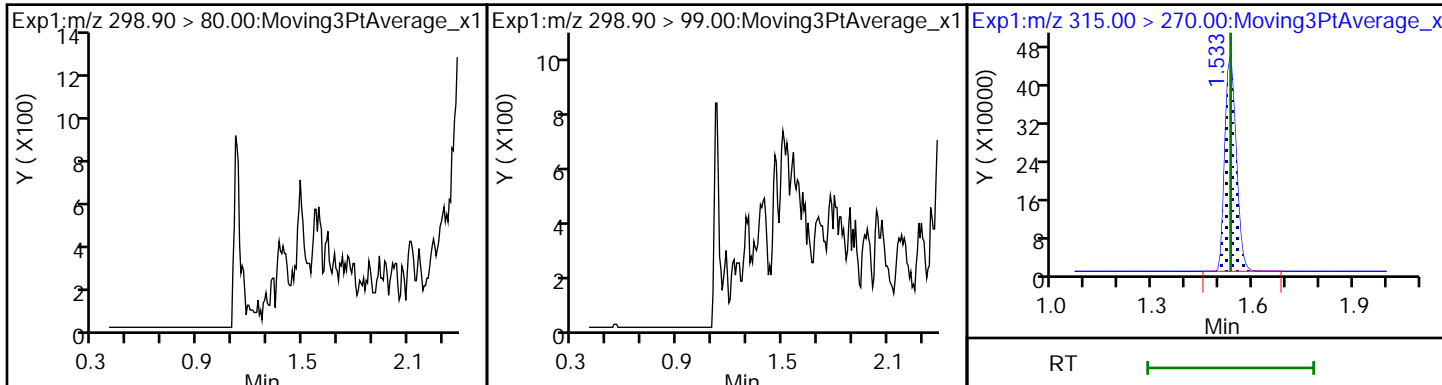


3 Perfluorohexanesulfonic acid (ND) 4 Perfluoroheptanoic acid (ND) * 6 13C2-PFOA

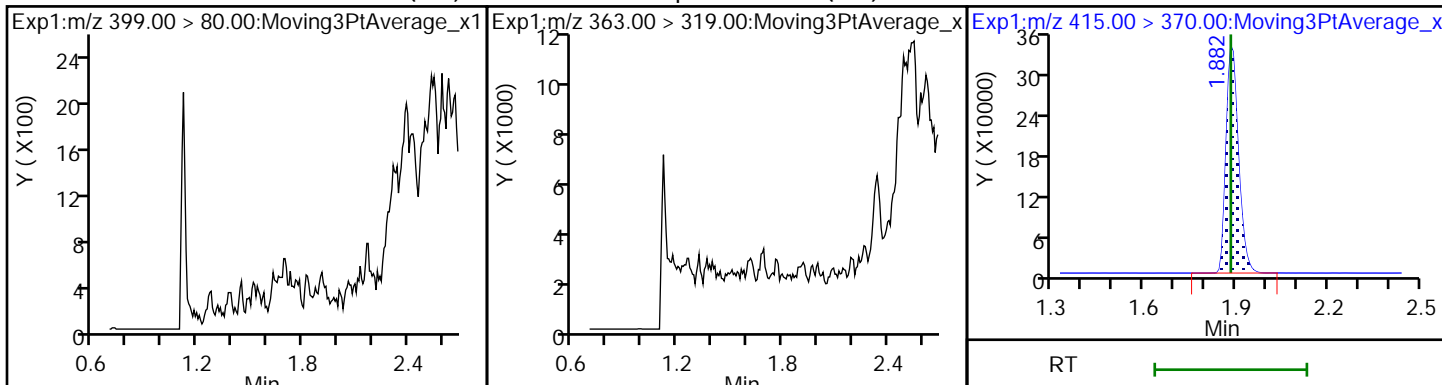


5 Perfluorooctanoic acid (ND) 5 Perfluorooctanoic acid (ND) 8 Perfluorooctane sulfonic acid (ND)

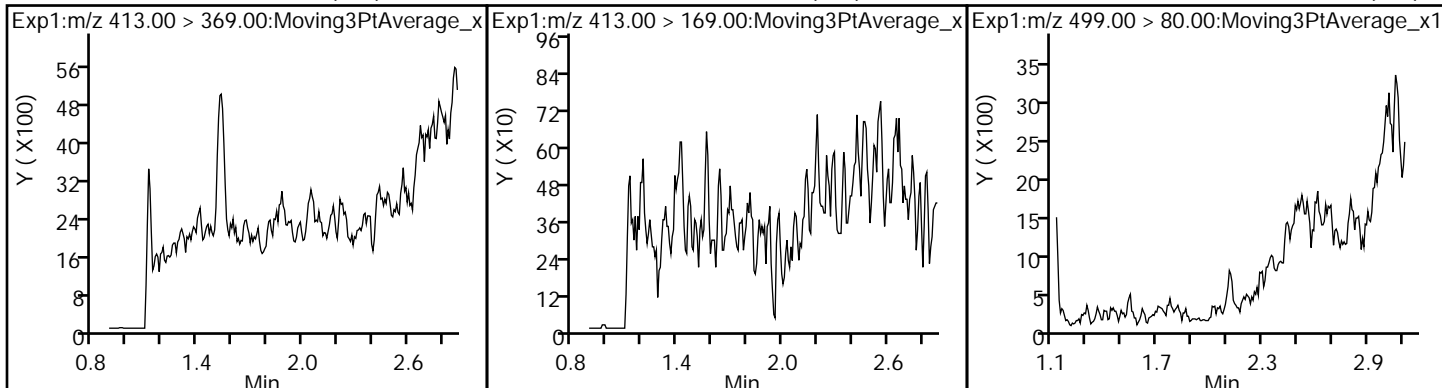

8 Perfluorooctane sulfonic acid (ND) * 7 13C4 PFOS 9 Perfluorononanoic acid (ND)

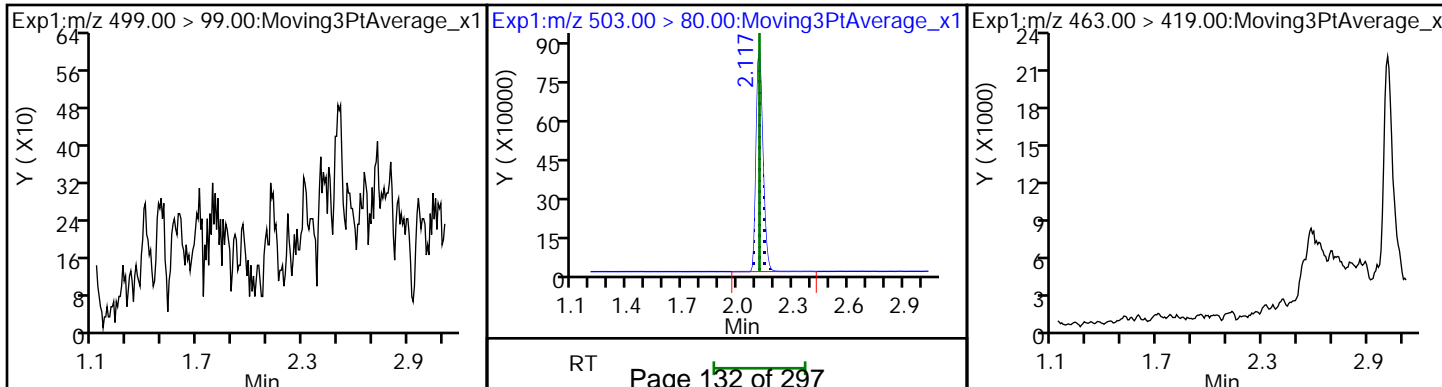

\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_022.d
 Lims ID: 320-38382-A-2-A
 Client ID: NAWC-041918-FRB-154
 Sample Type: Client
 Inject. Date: 01-May-2018 12:48:06 ALS Bottle#: 15 Worklist Smp#: 20
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-38382-a-2-a
 Misc. Info.: Plate: 1 Rack: 6
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 02-May-2018 10:24:00 Calib Date: 11-Apr-2018 12:09:09
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK005

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	10.6	105.82
\$ 10 13C2 PFDA	10.0	8.51	85.15

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Client Sample ID: NAWC-041918-RW-146 Lab Sample ID: 320-38382-3
 Matrix: Water Lab File ID: 2018.05.01_537AA_023.d
 Analysis Method: 537 Date Collected: 04/19/2018 10:10
 Extraction Method: 537 Date Extracted: 04/26/2018 09:35
 Sample wt/vol: 204.8(mL) Date Analyzed: 05/01/2018 12:52
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 220845 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	14	J M	49	20	8.3
335-67-1	Perfluorooctanoic acid (PFOA)	27		24	9.8	3.4
375-95-1	Perfluorononanoic acid (PFNA)	24	U	29	24	9.8
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	15	U	37	15	6.7
375-85-9	Perfluoroheptanoic acid (PFHpA)	7.0	J	12	4.9	2.3
375-73-5	Perfluorobutanesulfonic acid (PFBS)	44	U	110	44	20

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	100		70-130
STL00996	13C2 PFDA	83		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_023.d
 Lims ID: 320-38382-A-3-A
 Client ID: NAWC-041918-RW-146
 Sample Type: Client
 Inject. Date: 01-May-2018 12:52:47 ALS Bottle#: 16 Worklist Smp#: 21
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-38382-a-3-a
 Misc. Info.: Plate: 1 Rack: 6
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 02-May-2018 10:24:00 Calib Date: 11-Apr-2018 12:09:09
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK005

First Level Reviewer: barnettj Date: 01-May-2018 17:13:59

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.396	1.388	0.008	1.000	80173	1.03		49.8	
298.90 > 99.00	1.396	1.388	0.008	1.000	57719		1.39(0.00-0.00)	56.4	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.540	1.533	0.007	1.000	962995	9.97		6666	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.699	1.692	0.007	1.000	79396	0.6542		18.7	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.699	1.692	0.007	1.000	139156	1.43		10.4	
* 6 13C2-PFOA									
415.00 > 370.00	1.889	1.882	0.007		908929	10.0		6364	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.889	1.889	0.0	1.000	528490	5.47		59.8	
413.00 > 169.00	1.889	1.889	0.0	1.000	296871		1.78(0.00-0.00)	251	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.124	2.117	0.007	1.000	218628	2.78		37.6	a
499.00 > 99.00	2.124	2.117	0.007	1.000	40349		5.42(0.00-0.00)	47.2	a
* 7 13C4 PFOS									
503.00 > 80.00	2.124	2.117	0.007		2119366	28.7		999	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.269	2.269	0.0	1.000	642288	8.31		5074	


QC Flag Legend

Review Flags


a - User Assigned ID

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_023.d
Injection Date: 01-May-2018 12:52:47 Instrument ID: A8_N
Lims ID: 320-38382-A-3-A Lab Sample ID: 320-38382-3
Client ID: NAWC-041918-RW-146
Operator ID: SACINSTLCMS01 ALS Bottle#: 16 Worklist Smp#: 21
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL

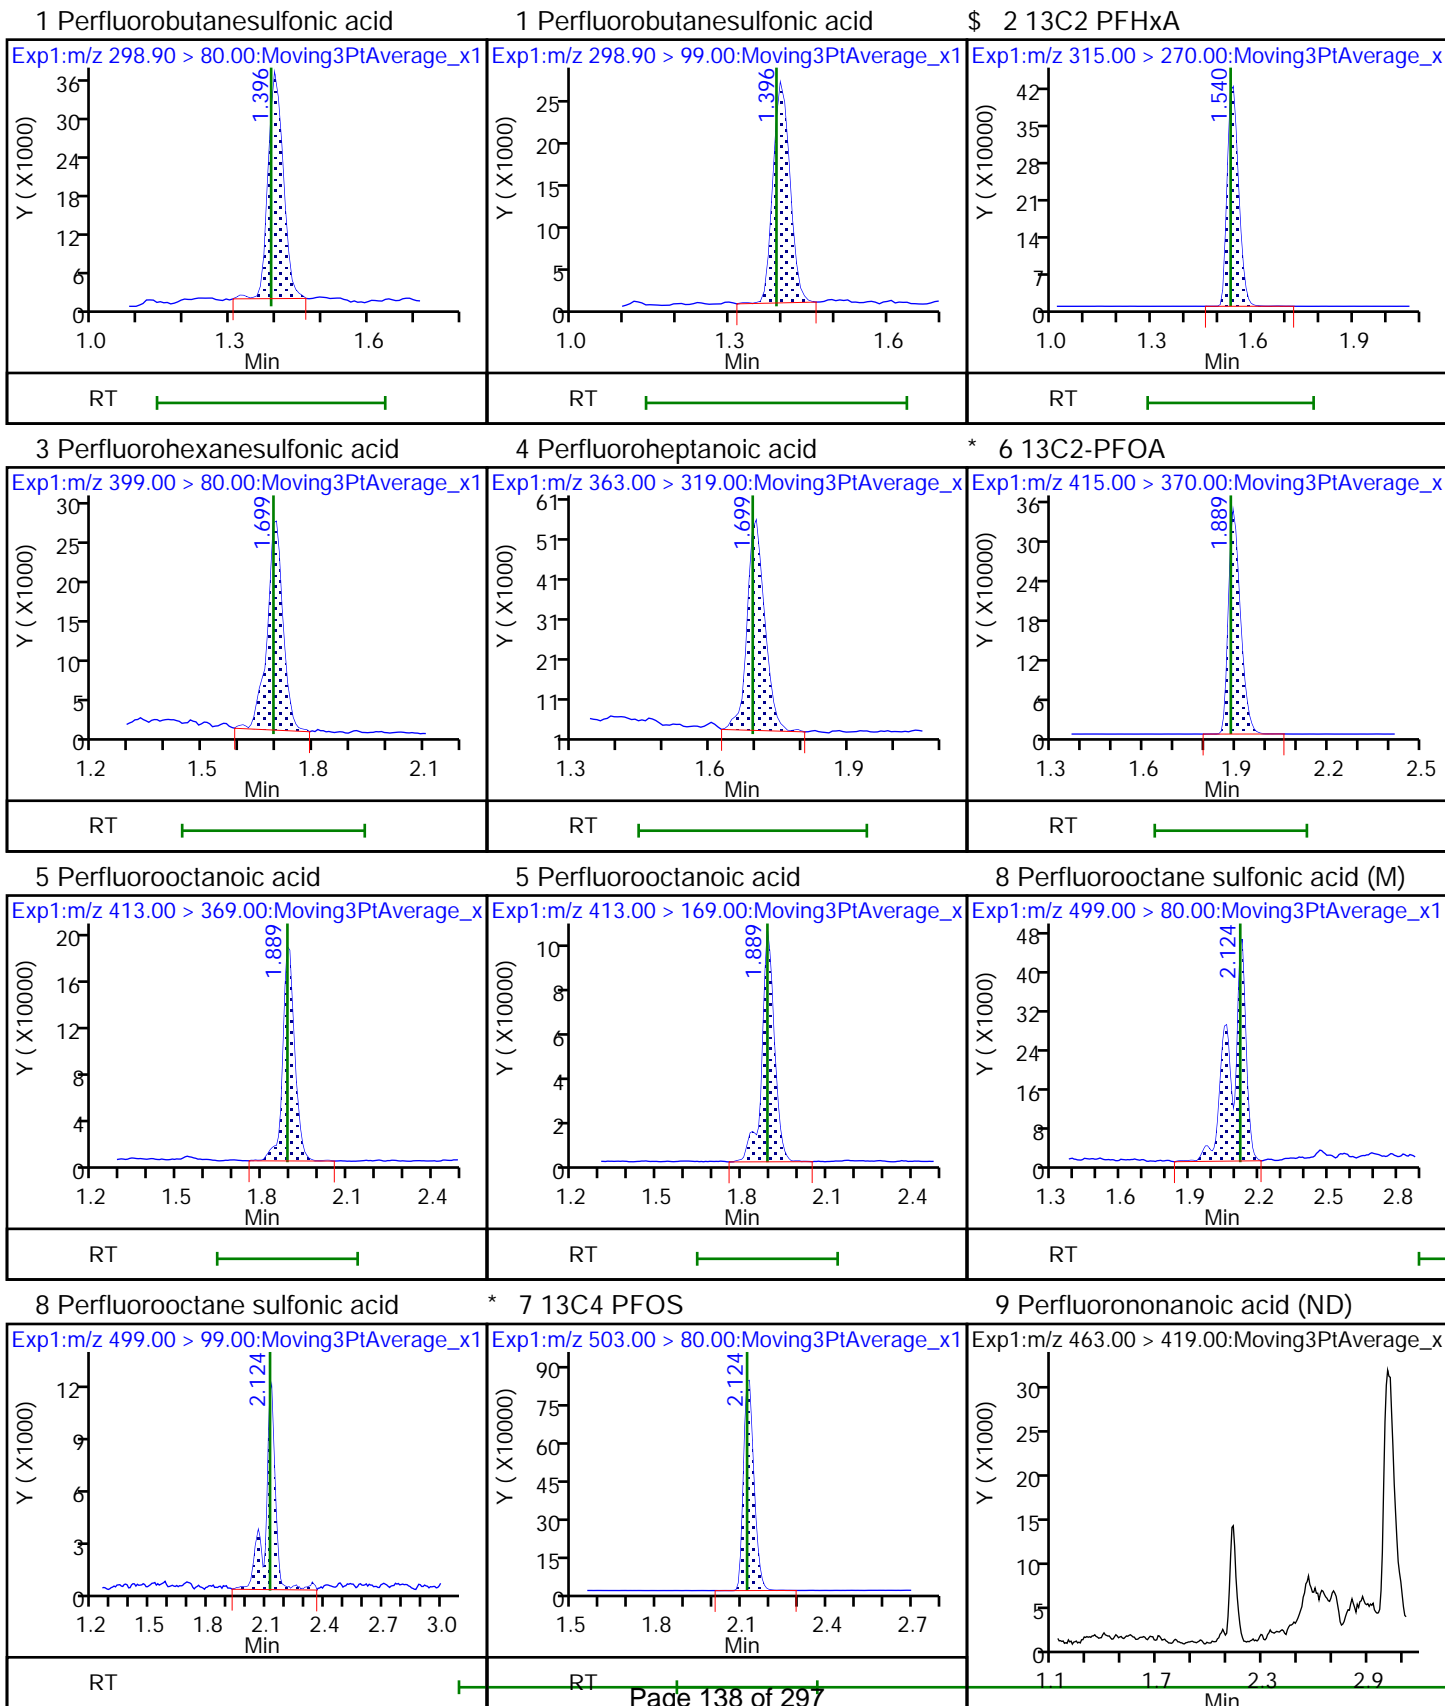

\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_023.d
 Lims ID: 320-38382-A-3-A
 Client ID: NAWC-041918-RW-146
 Sample Type: Client
 Inject. Date: 01-May-2018 12:52:47 ALS Bottle#: 16 Worklist Smp#: 21
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-38382-a-3-a
 Misc. Info.: Plate: 1 Rack: 6
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 02-May-2018 10:24:00 Calib Date: 11-Apr-2018 12:09:09
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK005

First Level Reviewer: barnettj Date: 01-May-2018 17:13:59

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	9.97	99.65
\$ 10 13C2 PFDA	10.0	8.31	83.09

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_023.d
Injection Date: 01-May-2018 12:52:47 Instrument ID: A8_N
Lims ID: 320-38382-A-3-A Lab Sample ID: 320-38382-3
Client ID: NAWC-041918-RW-146
Operator ID: SACINSTLCMS01 ALS Bottle#: 16 Worklist Smp#: 21
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.12

Processing Integration Results

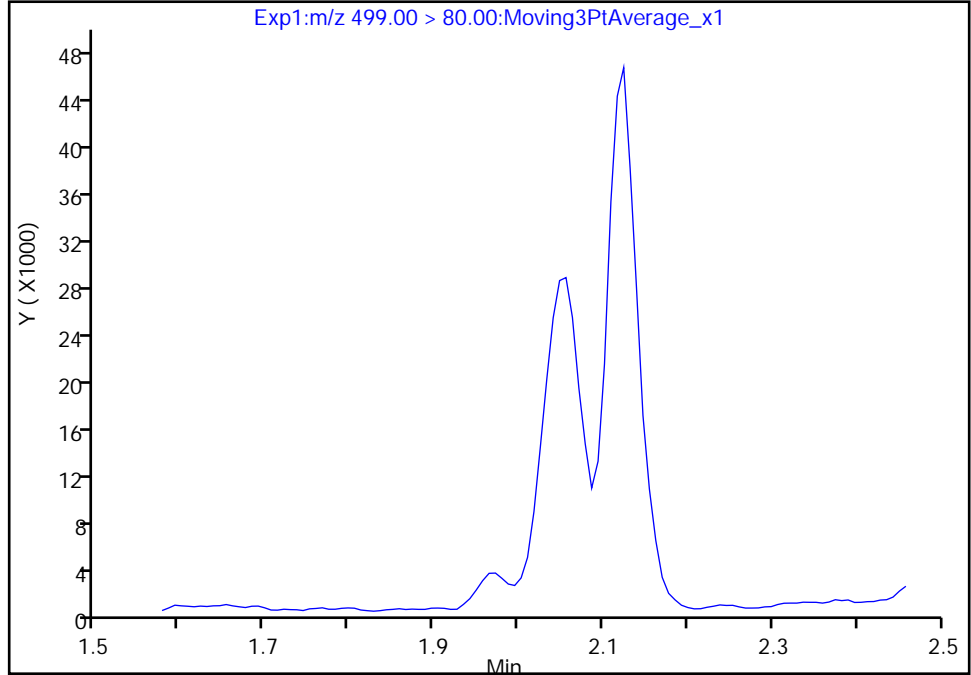

Manual Integration Results

RT: 2.12
Area: 218628
Amount: 2.775186
Amount Units: ng/ml

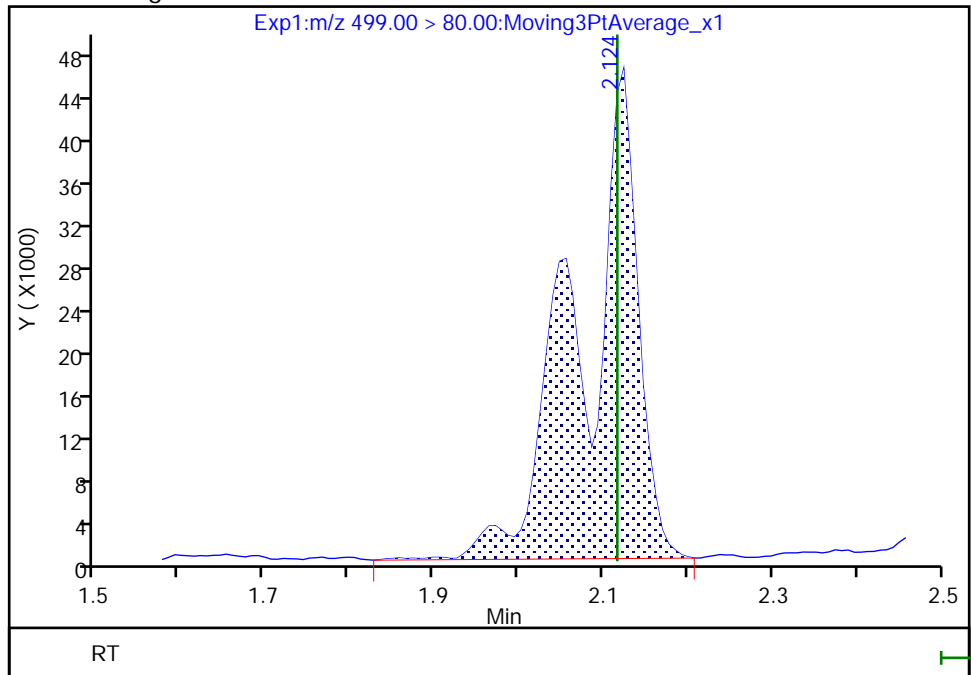

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Client Sample ID: NAWC-041918-FRB-146 Lab Sample ID: 320-38382-4
 Matrix: Water Lab File ID: 2018.05.01_537AA_024.d
 Analysis Method: 537 Date Collected: 04/19/2018 10:05
 Extraction Method: 537 Date Extracted: 04/26/2018 09:35
 Sample wt/vol: 263.6(mL) Date Analyzed: 05/01/2018 12:57
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 220845 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	38	15	6.4
335-67-1	Perfluorooctanoic acid (PFOA)	7.6	U	19	7.6	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	U	9.5	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	85	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	106		70-130
STL00996	13C2 PFDA	88		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_024.d
 Lims ID: 320-38382-A-4-A
 Client ID: NAWC-041918-FRB-146
 Sample Type: Client
 Inject. Date: 01-May-2018 12:57:29 ALS Bottle#: 17 Worklist Smp#: 22
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-38382-a-4-a
 Misc. Info.: Plate: 1 Rack: 6
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 02-May-2018 10:24:00 Calib Date: 11-Apr-2018 12:09:09
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_009.d


Column 1 : Det: EXP1
 Process Host: XAWRK005

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
\$ 2 13C2 PFHxA	315.00 > 270.00	1.540	1.533	0.007	1.000	1026175	10.6	7540	
* 6 13C2-PFOA	415.00 > 370.00	1.889	1.882	0.007		907706	10.0	5908	
* 7 13C4 PFOS	503.00 > 80.00	2.124	2.117	0.007		2174599	28.7	1353	
\$ 10 13C2 PFDA	515.00 > 470.00	2.276	2.269	0.008	1.000	680042	8.81	6137	


TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_024.d
Injection Date: 01-May-2018 12:57:29 Instrument ID: A8_N
Lims ID: 320-38382-A-4-A Lab Sample ID: 320-38382-4
Client ID: NAWC-041918-FRB-146
Operator ID: SACINSTLCMS01 ALS Bottle#: 17 Worklist Smp#: 22
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL


1 Perfluorobutanesulfonic acid (ND) 1 Perfluorobutanesulfonic acid (ND) \$ 2 13C2 PFHxA

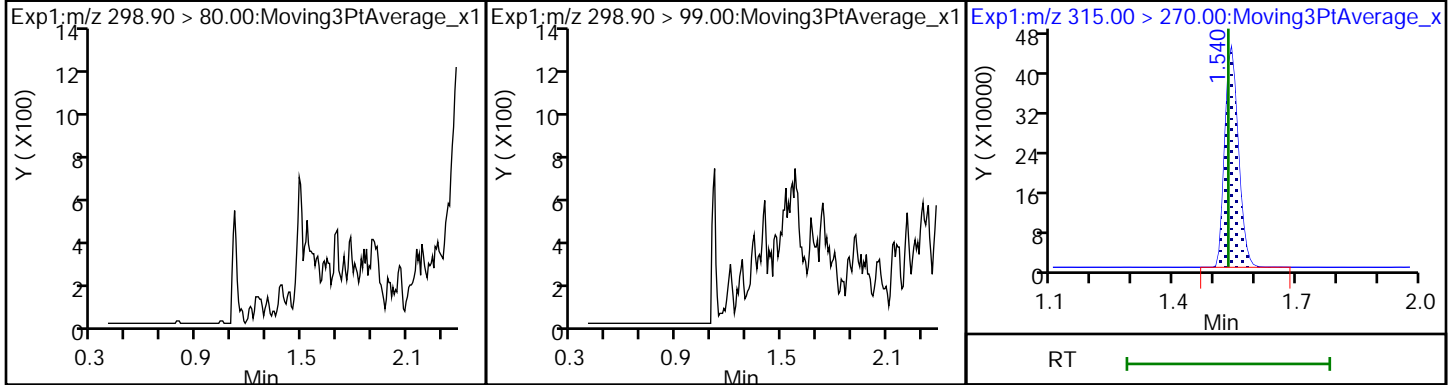


3 Perfluorohexanesulfonic acid (ND) 4 Perfluoroheptanoic acid (ND) * 6 13C2-PFOA

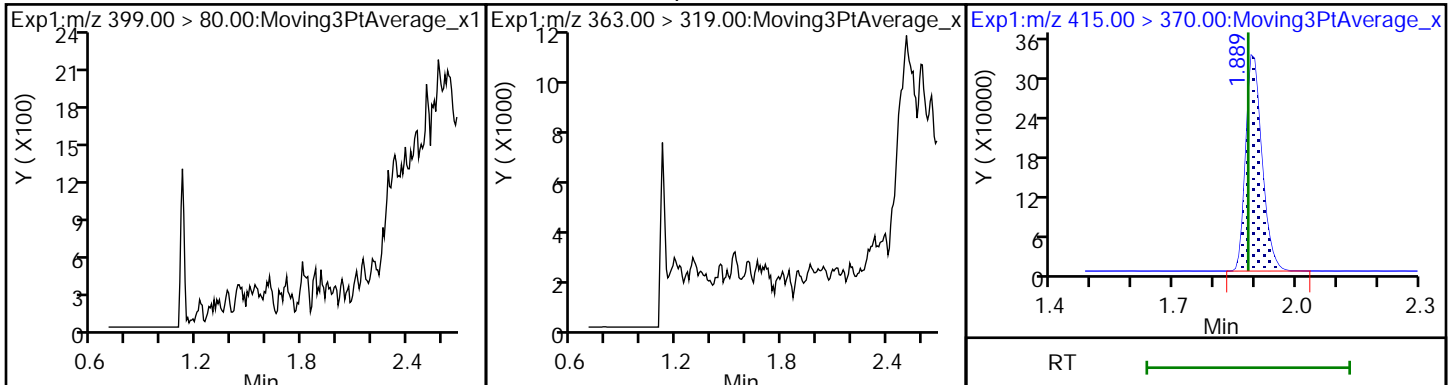


5 Perfluorooctanoic acid (ND) 5 Perfluorooctanoic acid (ND) 8 Perfluorooctane sulfonic acid (ND)

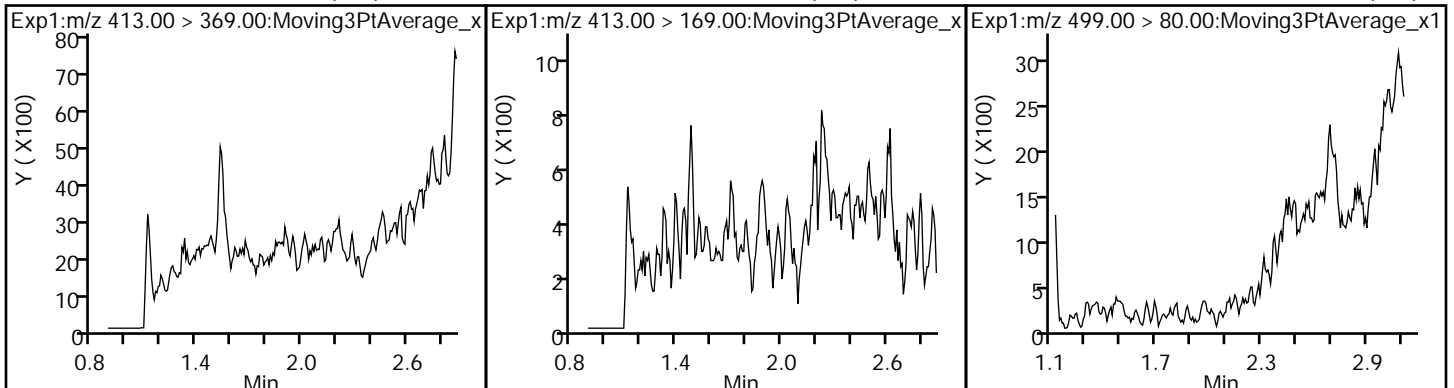

8 Perfluorooctane sulfonic acid (ND) * 7 13C4 PFOS 9 Perfluorononanoic acid (ND)

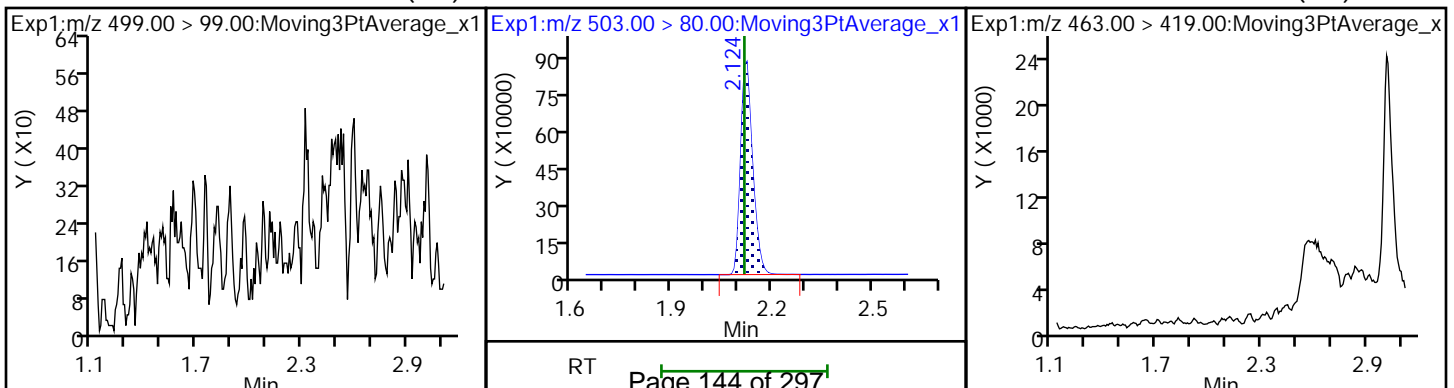

\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_024.d
 Lims ID: 320-38382-A-4-A
 Client ID: NAWC-041918-FRB-146
 Sample Type: Client
 Inject. Date: 01-May-2018 12:57:29 ALS Bottle#: 17 Worklist Smp#: 22
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-38382-a-4-a
 Misc. Info.: Plate: 1 Rack: 6
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 02-May-2018 10:24:00 Calib Date: 11-Apr-2018 12:09:09
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK005

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	10.6	106.33
\$ 10 13C2 PFDA	10.0	8.81	88.09

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Client Sample ID: NAWC-041918-RW-258 Lab Sample ID: 320-38382-5
 Matrix: Water Lab File ID: 2018.05.01_537AA_025.d
 Analysis Method: 537 Date Collected: 04/19/2018 10:40
 Extraction Method: 537 Date Extracted: 04/26/2018 09:35
 Sample wt/vol: 260.9(mL) Date Analyzed: 05/01/2018 13:02
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 220845 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	J M	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	20		19	7.7	2.7
375-95-1	Perfluorononanoic acid (PFNA)	10	J	23	19	7.7
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U M	29	11	5.3
375-85-9	Perfluoroheptanoic acid (PFHpA)	8.3	J	9.6	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	86	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	98		70-130
STL00996	13C2 PFDA	80		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_025.d
 Lims ID: 320-38382-A-5-A
 Client ID: NAWC-041918-RW-258
 Sample Type: Client
 Inject. Date: 01-May-2018 13:02:10 ALS Bottle#: 18 Worklist Smp#: 23
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-38382-a-5-a
 Misc. Info.: Plate: 1 Rack: 6
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 02-May-2018 10:24:00 Calib Date: 11-Apr-2018 12:09:09
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK005

First Level Reviewer: barnettj Date: 01-May-2018 17:14:35

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.396	1.388	0.008	1.000	171503	2.26		64.8	
298.90 > 99.00	1.396	1.388	0.008	1.000	132324		1.30(0.00-0.00)	126	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.540	1.533	0.007	1.000	917939	9.84		6441	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.692	1.692	0.0	1.000	62851	0.5302		11.0	M
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.692	1.692	0.0	1.000	203357	2.16		14.4	
* 6 13C2-PFOA									
415.00 > 370.00	1.889	1.882	0.007		877855	10.0		5254	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.889	1.889	0.0	1.000	491910	5.27		44.8	
413.00 > 169.00	1.889	1.889	0.0	1.000	286201		1.72(0.00-0.00)	246	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.117	2.117	0.0	1.000	330626	4.30		55.1	a
499.00 > 99.00	2.117	2.117	0.0	1.000	64804		5.10(0.00-0.00)	80.3	a
* 7 13C4 PFOS									
503.00 > 80.00	2.117	2.117	0.0		2070367	28.7		723	
9 Perfluorononanoic acid									
463.00 > 419.00	2.124	2.124	0.0	1.000	193817	2.62		18.7	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.269	2.269	0.0	1.000	600367	8.04		5020	

QC Flag Legend


Review Flags

M - Manually Integrated


a - User Assigned ID

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_025.d
Injection Date: 01-May-2018 13:02:10 Instrument ID: A8_N
Lims ID: 320-38382-A-5-A Lab Sample ID: 320-38382-5
Client ID: NAWC-041918-RW-258
Operator ID: SACINSTLCMS01 ALS Bottle#: 18 Worklist Smp#: 23
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL

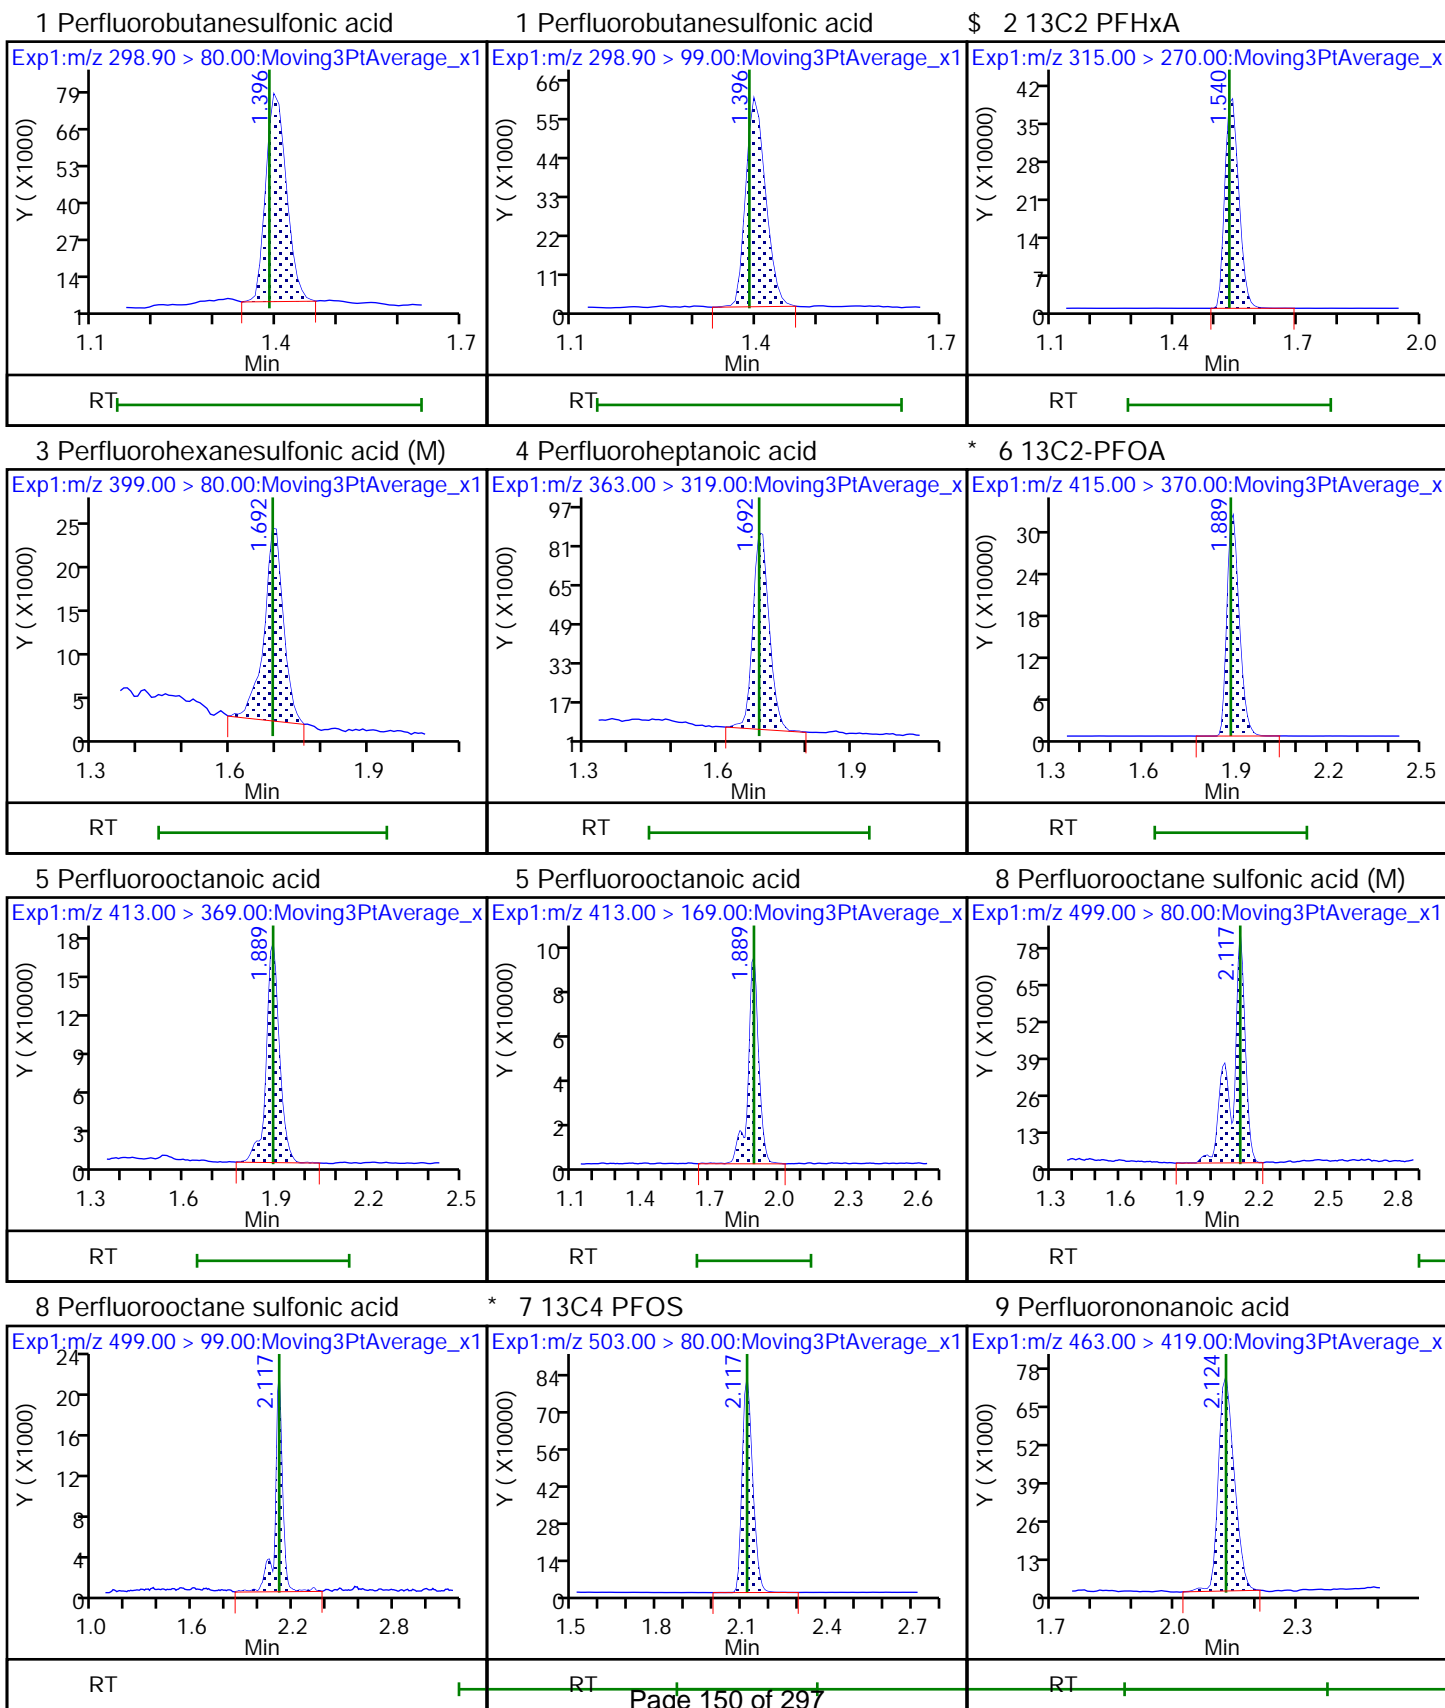

\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_025.d
 Lims ID: 320-38382-A-5-A
 Client ID: NAWC-041918-RW-258
 Sample Type: Client
 Inject. Date: 01-May-2018 13:02:10 ALS Bottle#: 18 Worklist Smp#: 23
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-38382-a-5-a
 Misc. Info.: Plate: 1 Rack: 6
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 02-May-2018 10:24:00 Calib Date: 11-Apr-2018 12:09:09
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK005

First Level Reviewer: barnettj Date: 01-May-2018 17:14:35

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	9.84	98.35
\$ 10 13C2 PFDA	10.0	8.04	80.41

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_025.d
Injection Date: 01-May-2018 13:02:10 Instrument ID: A8_N
Lims ID: 320-38382-A-5-A Lab Sample ID: 320-38382-5
Client ID: NAWC-041918-RW-258
Operator ID: SACINSTLCMS01 ALS Bottle#: 18 Worklist Smp#: 23
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.12

Processing Integration Results

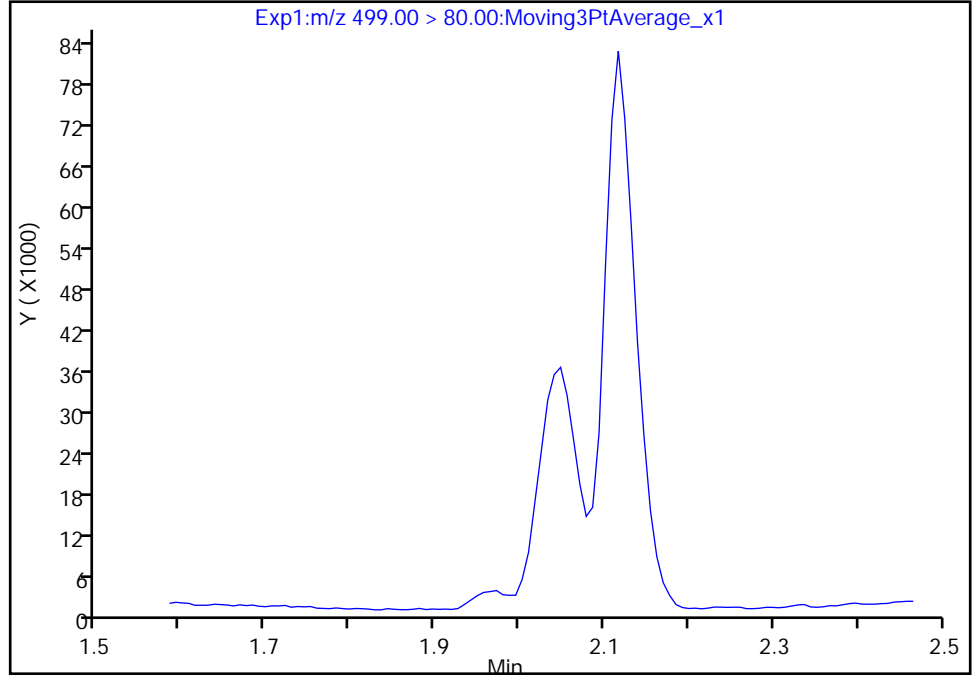

Manual Integration Results

RT: 2.12
Area: 330626
Amount: 4.296175
Amount Units: ng/ml

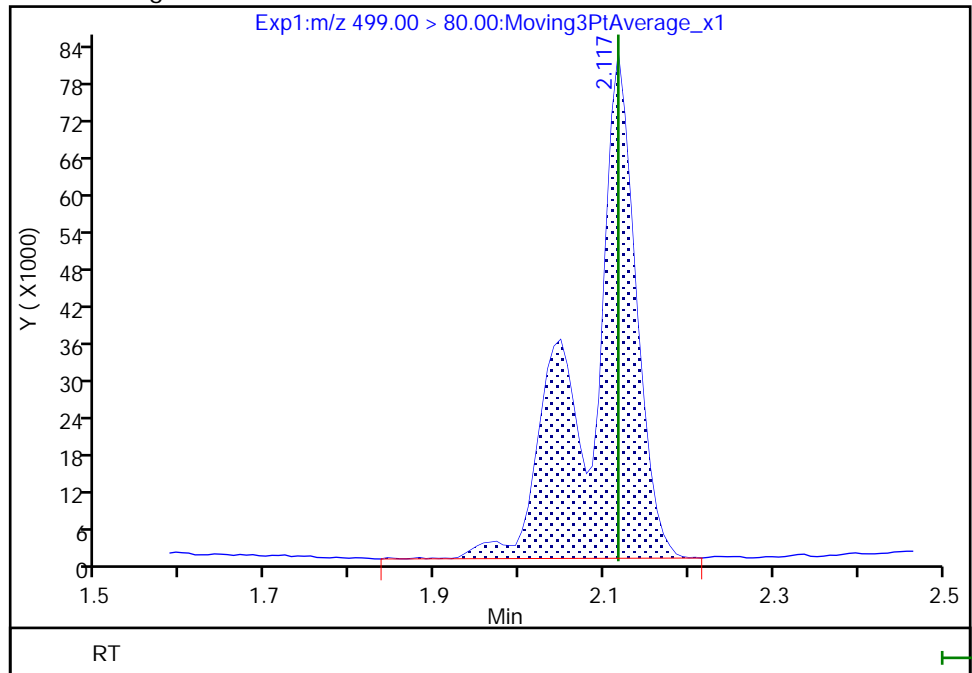

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_025.d
Injection Date: 01-May-2018 13:02:10 Instrument ID: A8_N
Lims ID: 320-38382-A-5-A Lab Sample ID: 320-38382-5
Client ID: NAWC-041918-RW-258
Operator ID: SACINSTLCMS01 ALS Bottle#: 18 Worklist Smp#: 23
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

3 Perfluorohexanesulfonic acid, CAS: 355-46-4


Signal: 1

Not Detected
Expected RT: 1.69

Processing Integration Results

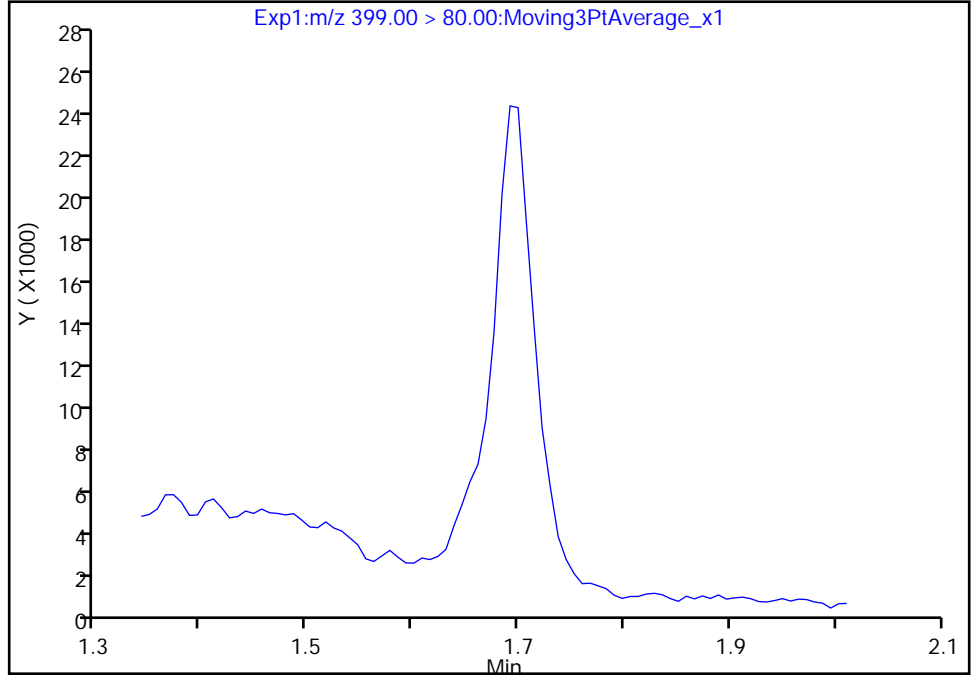

Manual Integration Results

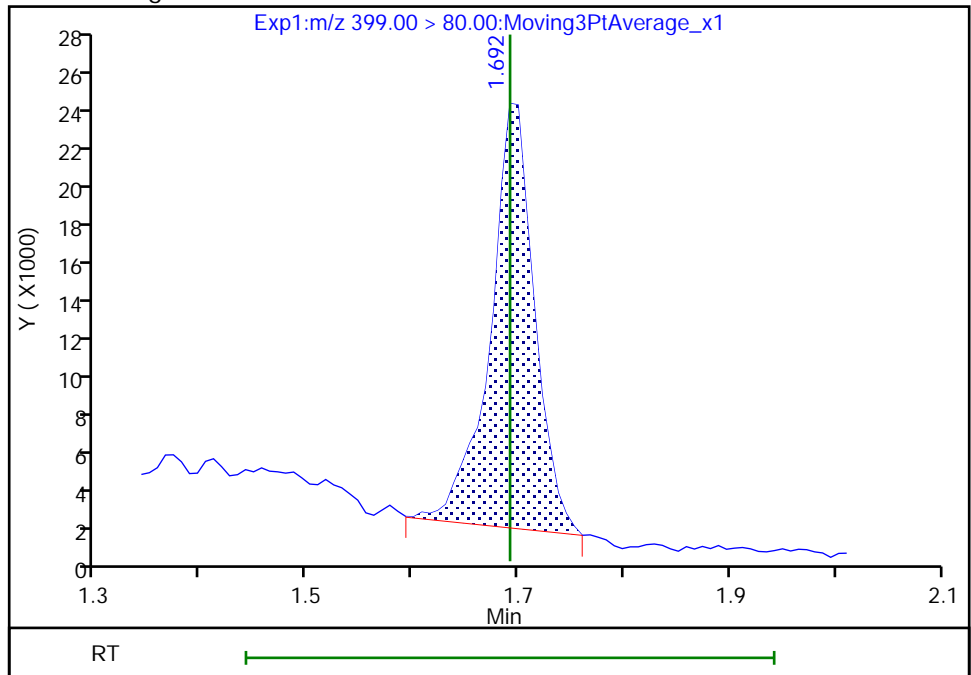

RT: 1.69
Area: 62851
Amount: 0.530164
Amount Units: ng/ml

Reviewer: barnettj, 01-May-2018 17:14:18
Audit Action: Manually Integrated

Audit Reason: Missed Peak
Page 154 of 297

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Client Sample ID: NAWC-041918-FRB-258 Lab Sample ID: 320-38382-6
 Matrix: Water Lab File ID: 2018.05.01_537AA_026.d
 Analysis Method: 537 Date Collected: 04/19/2018 10:35
 Extraction Method: 537 Date Extracted: 04/26/2018 09:35
 Sample wt/vol: 267.6(mL) Date Analyzed: 05/01/2018 13:06
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 220845 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	37	15	6.4
335-67-1	Perfluorooctanoic acid (PFOA)	7.5	U	19	7.5	2.6
375-95-1	Perfluorononanoic acid (PFNA)	19	U	22	19	7.5
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.1
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.7	U	9.3	3.7	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	84	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	106		70-130
STL00996	13C2 PFDA	85		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_026.d
 Lims ID: 320-38382-A-6-A
 Client ID: NAWC-041918-FRB-258
 Sample Type: Client
 Inject. Date: 01-May-2018 13:06:50 ALS Bottle#: 19 Worklist Smp#: 24
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-38382-a-6-a
 Misc. Info.: Plate: 1 Rack: 6
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 02-May-2018 10:24:00 Calib Date: 11-Apr-2018 12:09:09
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_009.d


Column 1 : Det: EXP1
 Process Host: XAWRK005

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
\$ 2 13C2 PFHxA	315.00 > 270.00	1.533	1.533	0.0	1.000	989770	10.6	7401	
* 6 13C2-PFOA	415.00 > 370.00	1.882	1.882	0.0		880431	10.0	5711	
* 7 13C4 PFOS	503.00 > 80.00	2.109	2.117	-0.008		2120366	28.7	1214	
\$ 10 13C2 PFDA	515.00 > 470.00	2.269	2.269	0.0	1.000	634565	8.47	5983	


TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_026.d
Injection Date: 01-May-2018 13:06:50 Instrument ID: A8_N
Lims ID: 320-38382-A-6-A Lab Sample ID: 320-38382-6
Client ID: NAWC-041918-FRB-258
Operator ID: SACINSTLCMS01 ALS Bottle#: 19 Worklist Smp#: 24
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL


1 Perfluorobutanesulfonic acid (ND) 1 Perfluorobutanesulfonic acid (ND) \$ 2 13C2 PFHxA

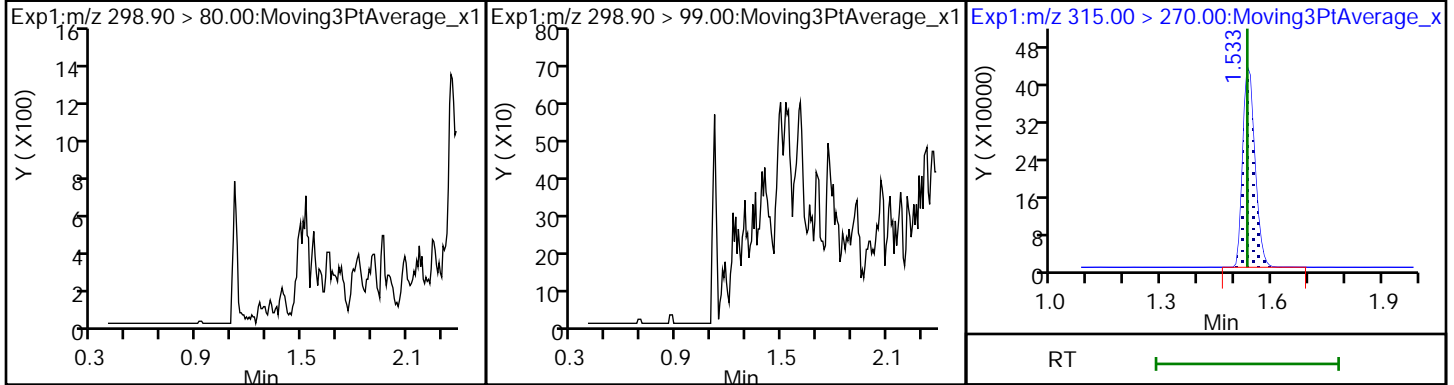


3 Perfluorohexanesulfonic acid (ND) 4 Perfluoroheptanoic acid (ND) * 6 13C2-PFOA

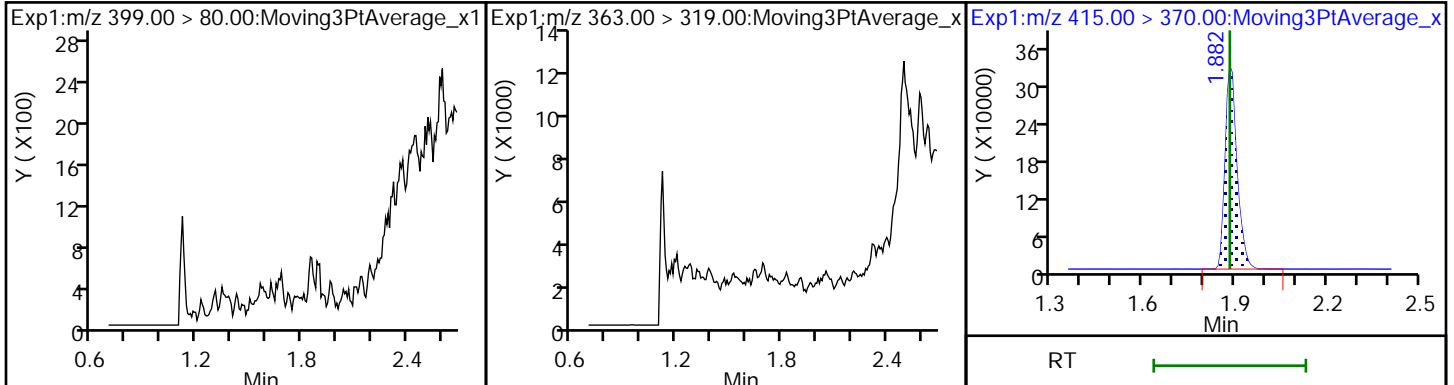


5 Perfluorooctanoic acid (ND) 5 Perfluorooctanoic acid (ND) 8 Perfluorooctane sulfonic acid (ND)

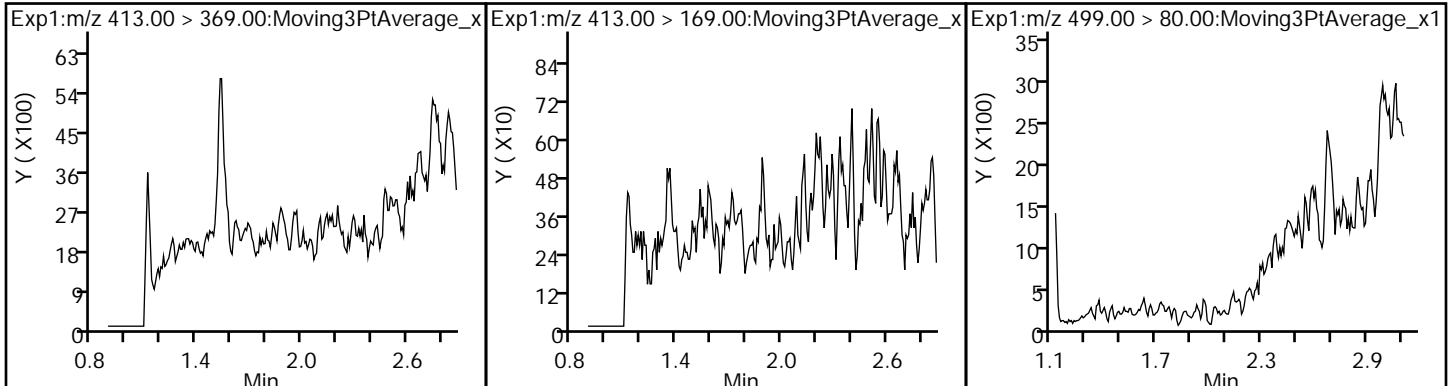

8 Perfluorooctane sulfonic acid (ND) * 7 13C4 PFOS 9 Perfluorononanoic acid (ND)

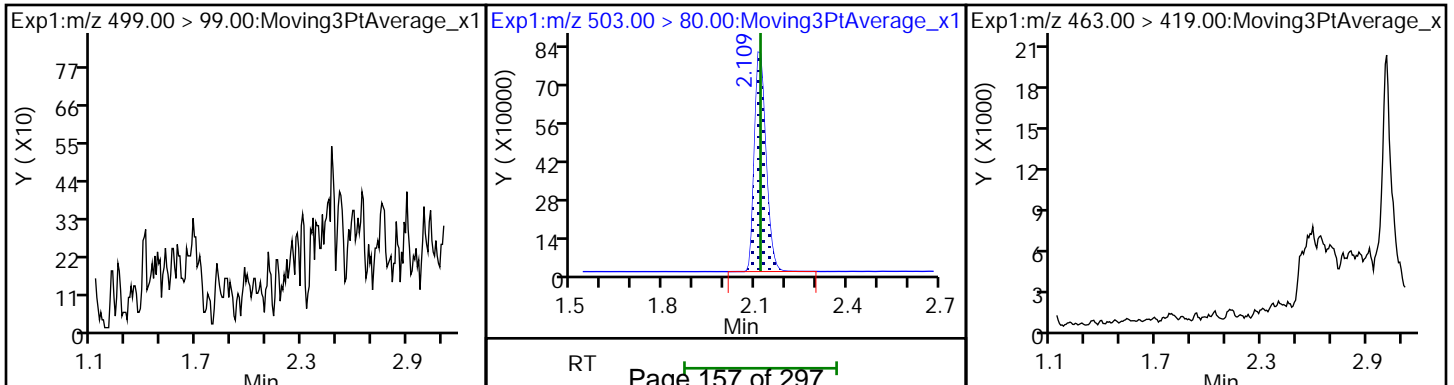

\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_026.d
 Lims ID: 320-38382-A-6-A
 Client ID: NAWC-041918-FRB-258
 Sample Type: Client
 Inject. Date: 01-May-2018 13:06:50 ALS Bottle#: 19 Worklist Smp#: 24
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-38382-a-6-a
 Misc. Info.: Plate: 1 Rack: 6
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 02-May-2018 10:24:00 Calib Date: 11-Apr-2018 12:09:09
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK005

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	10.6	105.74
\$ 10 13C2 PFDA	10.0	8.47	84.75

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Client Sample ID: WGNA-041918-RW-3571 Lab Sample ID: 320-38382-7
 Matrix: Water Lab File ID: 2018.05.01_537AA_029.d
 Analysis Method: 537 Date Collected: 04/19/2018 11:10
 Extraction Method: 537 Date Extracted: 04/26/2018 09:35
 Sample wt/vol: 277.2 (mL) Date Analyzed: 05/01/2018 13:20
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 220847 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	8.0	J M	36	14	6.1
335-67-1	Perfluorooctanoic acid (PFOA)	10	J	18	7.2	2.5
375-95-1	Perfluorononanoic acid (PFNA)	18	U M	22	18	7.2
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U M	27	11	5.0
375-85-9	Perfluoroheptanoic acid (PFHpA)	12		9.0	3.6	1.7
375-73-5	Perfluorobutanesulfonic acid (PFBS)	32	U M	81	32	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	99		70-130
STL00996	13C2 PFDA	79		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_029.d
 Lims ID: 320-38382-A-7-A
 Client ID: WGNA-041918-RW-3571
 Sample Type: Client
 Inject. Date: 01-May-2018 13:20:51 ALS Bottle#: 20 Worklist Smp#: 27
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-38382-a-7-a
 Misc. Info.: Plate: 1 Rack: 6
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 02-May-2018 10:27:59 Calib Date: 11-Apr-2018 12:09:09
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK005

First Level Reviewer: barnettj Date: 01-May-2018 17:15:50

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.388	1.396	-0.008	1.000	55022	0.7742		38.3	M
298.90 > 99.00	1.388	1.396	-0.008	1.000	46305		1.19(0.00-0.00)	46.5	M
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.525	1.533	-0.008	1.000	890055	9.85		7049	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.684	1.692	-0.008	1.000	117546	1.06		35.0	M
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.684	1.692	-0.008	1.000	296880	3.25		25.1	
* 6 13C2-PFOA									
415.00 > 370.00	1.874	1.882	-0.008		849895	10.0		5433	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.882	1.882	0.0	1.000	259108	2.87		32.6	
413.00 > 169.00	1.882	1.882	0.0	1.000	149728		1.73(0.00-0.00)	132	
* 7 13C4 PFOS									
503.00 > 80.00	2.109	2.109	0.0		1937754	28.7		1047	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.109	2.117	-0.008	1.000	159706	2.22		30.2	a
499.00 > 99.00	2.109	2.117	-0.008	1.000	30133		5.30(0.00-0.00)	35.9	a
9 Perfluorononanoic acid									
463.00 > 419.00	2.117	2.124	-0.007	1.000	65928	0.9209		7.7	M
\$ 10 13C2 PFDA									
515.00 > 470.00	2.261	2.269	-0.007	1.000	570890	7.90		4713	

QC Flag Legend

Review Flags


M - Manually Integrated

a - User Assigned ID


TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_029.d
Injection Date: 01-May-2018 13:20:51 Instrument ID: A8_N
Lims ID: 320-38382-A-7-A Lab Sample ID: 320-38382-7
Client ID: WGNA-041918-RW-3571
Operator ID: SACINSTLCMS01 ALS Bottle#: 20 Worklist Smp#: 27
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL


1 Perfluorobutanesulfonic acid (M) 1 Perfluorobutanesulfonic acid (M) \$ 2 13C2 PFHxA

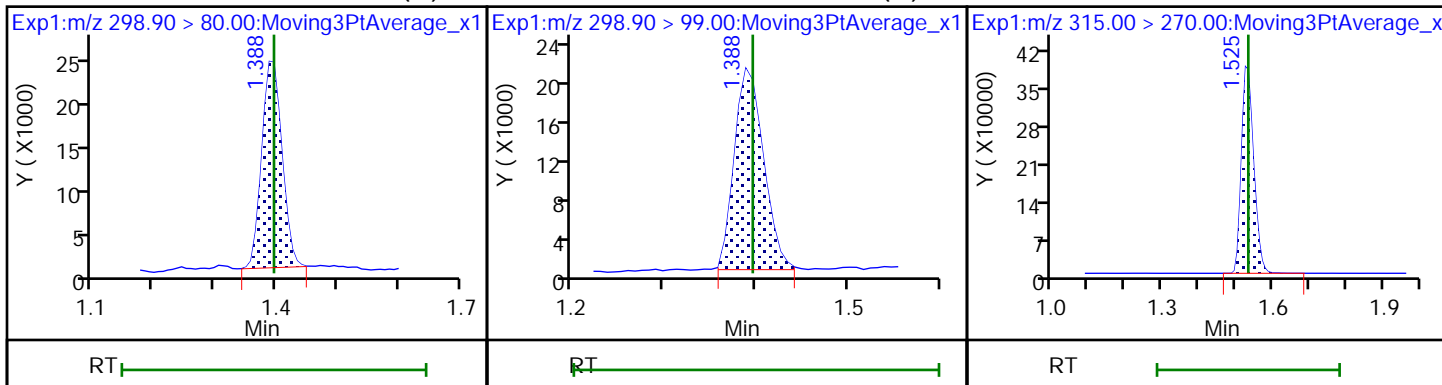


3 Perfluorohexanesulfonic acid (M) 4 Perfluoroheptanoic acid * 6 13C2-PFOA

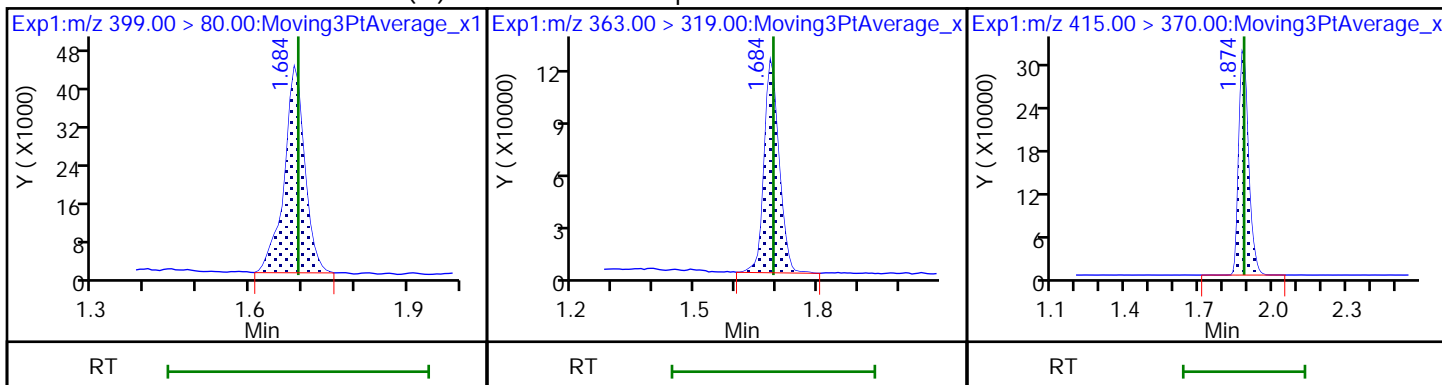


5 Perfluorooctanoic acid 5 Perfluorooctanoic acid * 7 13C4 PFOS

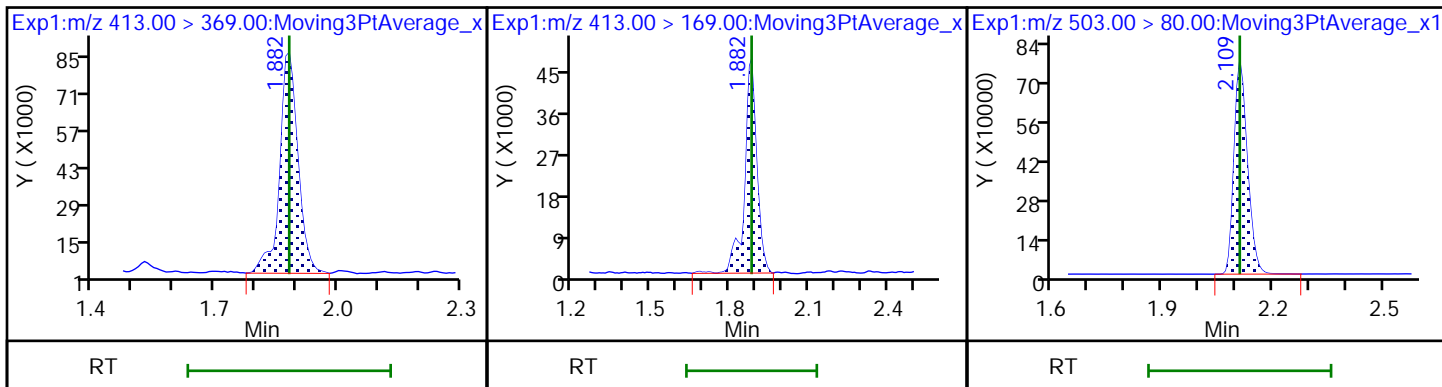

8 Perfluorooctane sulfonic acid (M) 8 Perfluorooctane sulfonic acid 9 Perfluorononanoic acid (M)

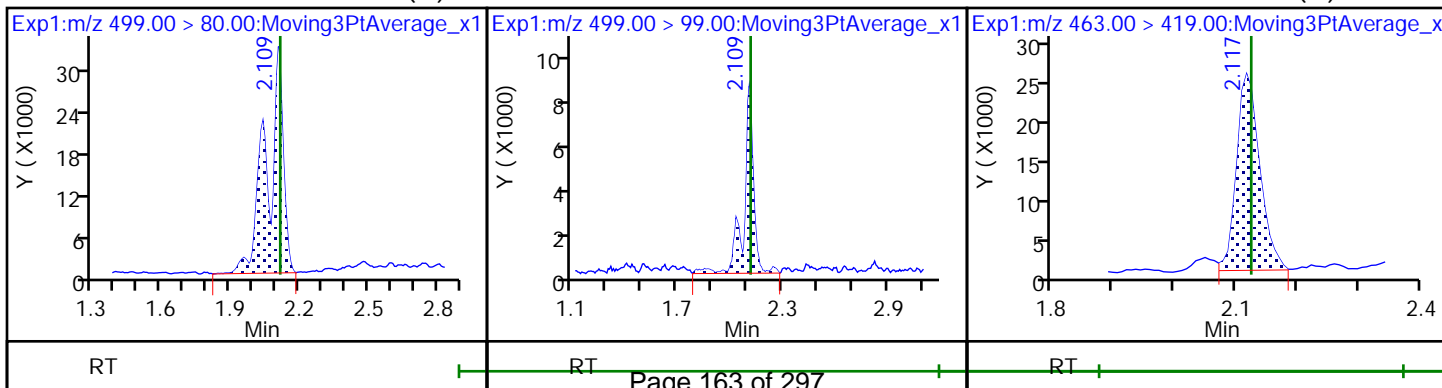

\$ 10 13C2 PFDA

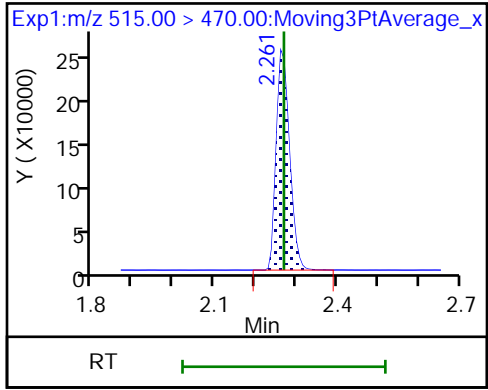

TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_029.d
 Lims ID: 320-38382-A-7-A
 Client ID: WGNA-041918-RW-3571
 Sample Type: Client
 Inject. Date: 01-May-2018 13:20:51 ALS Bottle#: 20 Worklist Smp#: 27
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-38382-a-7-a
 Misc. Info.: Plate: 1 Rack: 6
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 02-May-2018 10:27:59 Calib Date: 11-Apr-2018 12:09:09
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK005

First Level Reviewer: barnettj Date: 01-May-2018 17:15:50

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	9.85	98.50
\$ 10 13C2 PFDA	10.0	7.90	78.98

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_029.d
Injection Date: 01-May-2018 13:20:51 Instrument ID: A8_N
Lims ID: 320-38382-A-7-A Lab Sample ID: 320-38382-7
Client ID: WGNA-041918-RW-3571
Operator ID: SACINSTLCMS01 ALS Bottle#: 20 Worklist Smp#: 27
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.12

Processing Integration Results

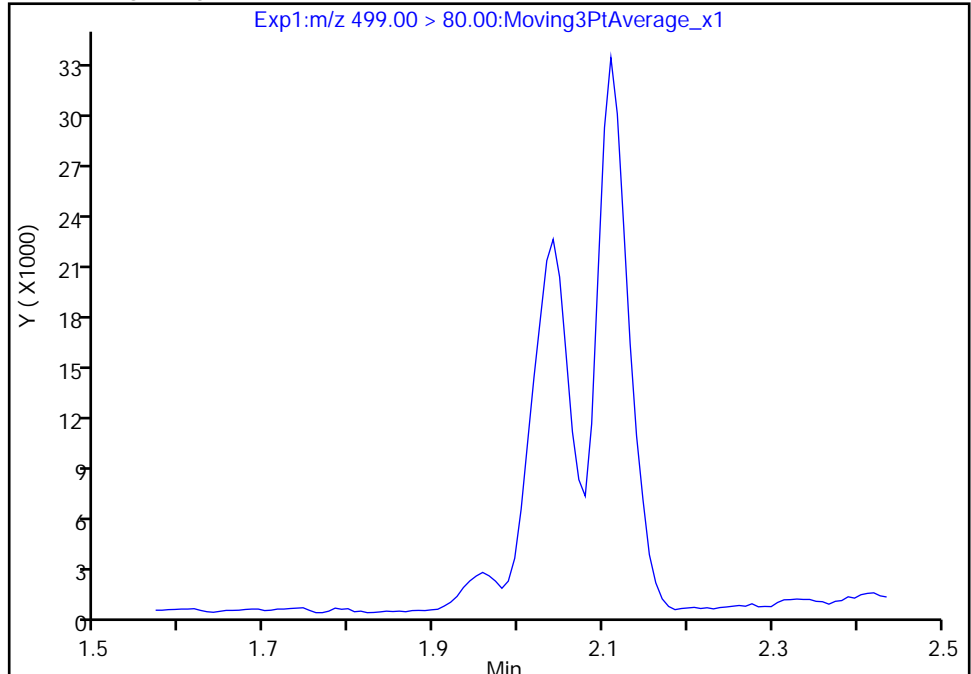

Manual Integration Results

RT: 2.11
Area: 159706
Amount: 2.217251
Amount Units: ng/ml

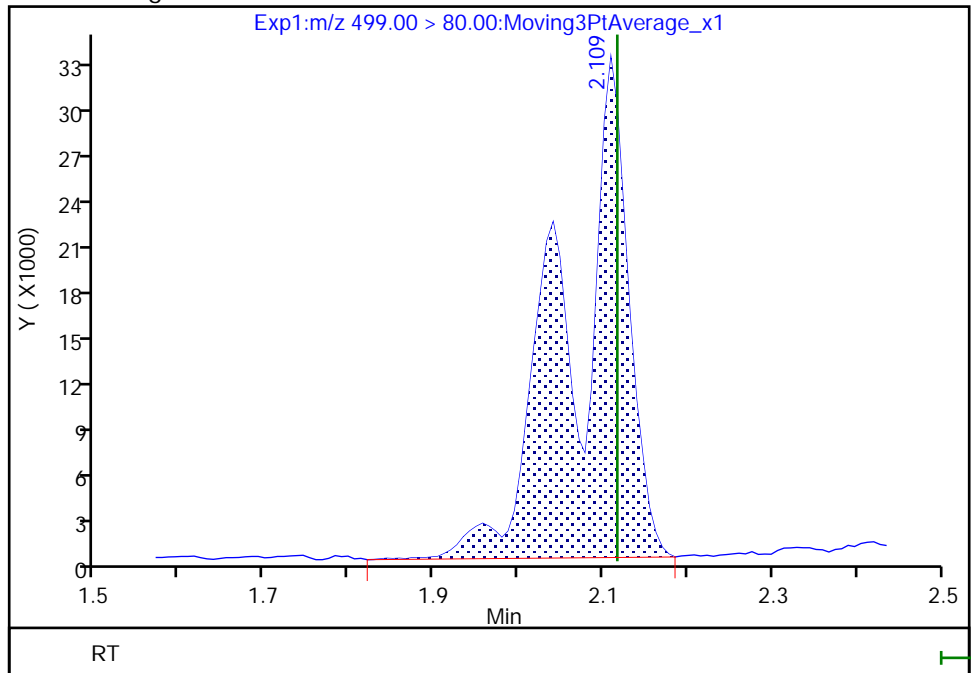

Reviewer: barnettj, 01-May-2018 17:15:31
Audit Action: Assigned Compound ID

Audit Reason: Missed Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_029.d
Injection Date: 01-May-2018 13:20:51 Instrument ID: A8_N
Lims ID: 320-38382-A-7-A Lab Sample ID: 320-38382-7
Client ID: WGNA-041918-RW-3571
Operator ID: SACINSTLCMS01 ALS Bottle#: 20 Worklist Smp#: 27
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

9 Perfluorononanoic acid, CAS: 375-95-1

Signal: 1


Not Detected
Expected RT: 2.12

Processing Integration Results

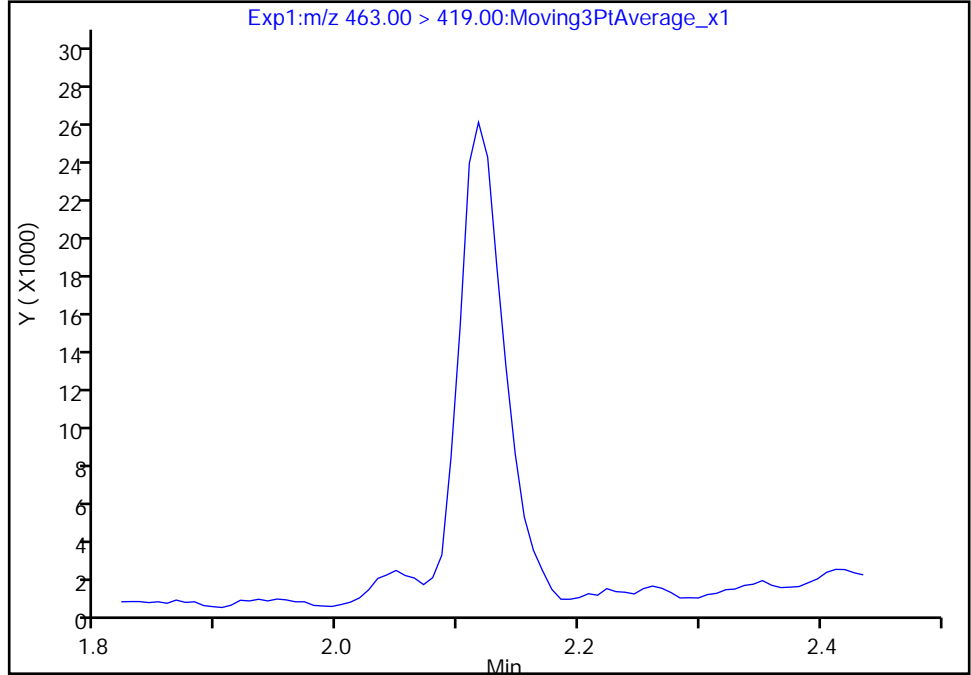

Manual Integration Results

RT: 2.12
Area: 65928
Amount: 0.920854
Amount Units: ng/ml

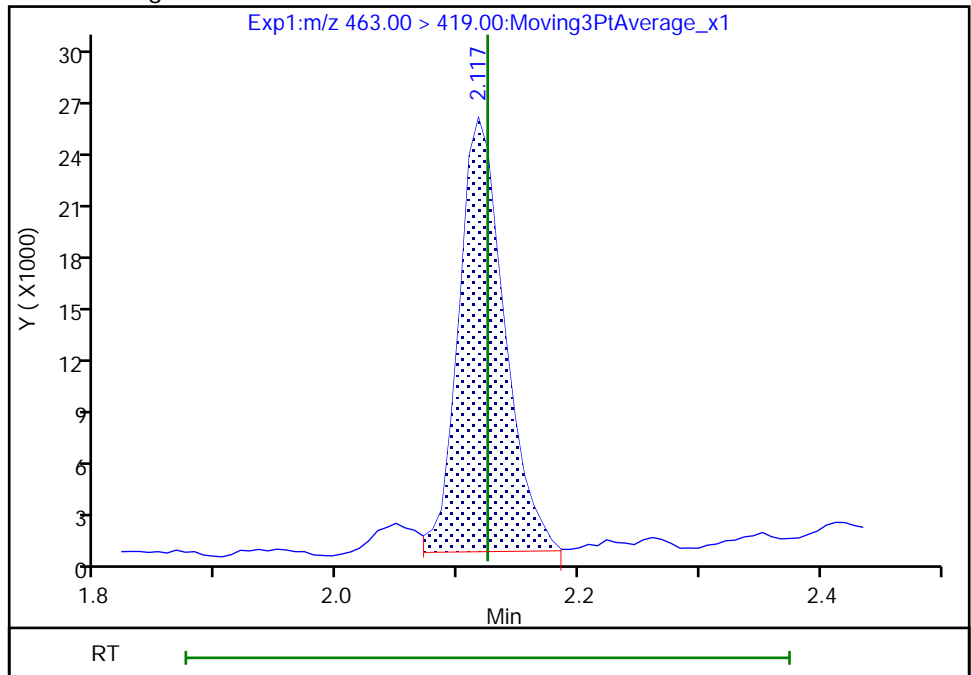

Reviewer: barnettj, 01-May-2018 17:15:43
Audit Action: Manually Integrated

Audit Reason: Missed Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_029.d
Injection Date: 01-May-2018 13:20:51 Instrument ID: A8_N
Lims ID: 320-38382-A-7-A Lab Sample ID: 320-38382-7
Client ID: WGNA-041918-RW-3571
Operator ID: SACINSTLCMS01 ALS Bottle#: 20 Worklist Smp#: 27
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

3 Perfluorohexanesulfonic acid, CAS: 355-46-4


Signal: 1

Not Detected
Expected RT: 1.69

Processing Integration Results

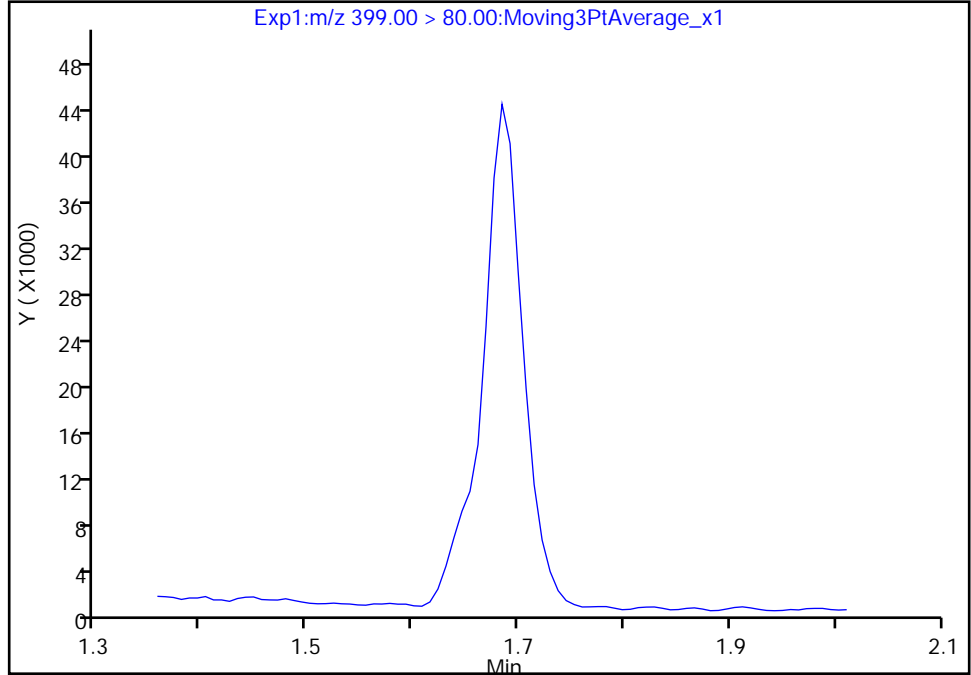

Manual Integration Results

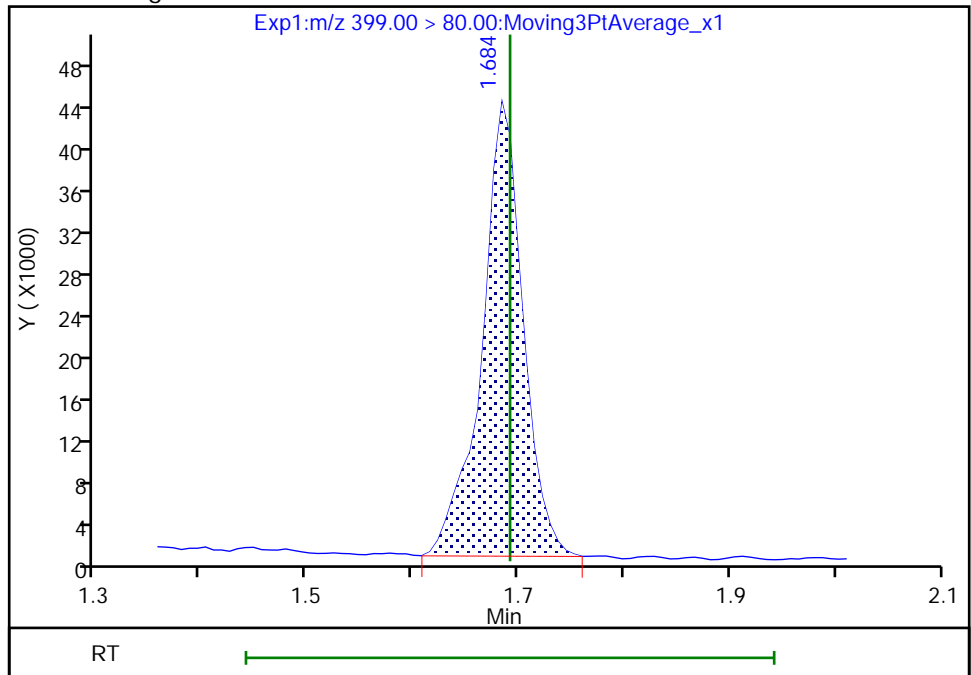

RT: 1.68
Area: 117546
Amount: 1.059386
Amount Units: ng/ml

Reviewer: barnettj, 01-May-2018 17:15:23
Audit Action: Manually Integrated

Audit Reason: Missed Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_029.d
Injection Date: 01-May-2018 13:20:51 Instrument ID: A8_N
Lims ID: 320-38382-A-7-A Lab Sample ID: 320-38382-7
Client ID: WGNA-041918-RW-3571
Operator ID: SACINSTLCMS01 ALS Bottle#: 20 Worklist Smp#: 27
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

1 Perfluorobutanesulfonic acid, CAS: 375-73-5

Signal: 1


Not Detected
Expected RT: 1.40

Processing Integration Results

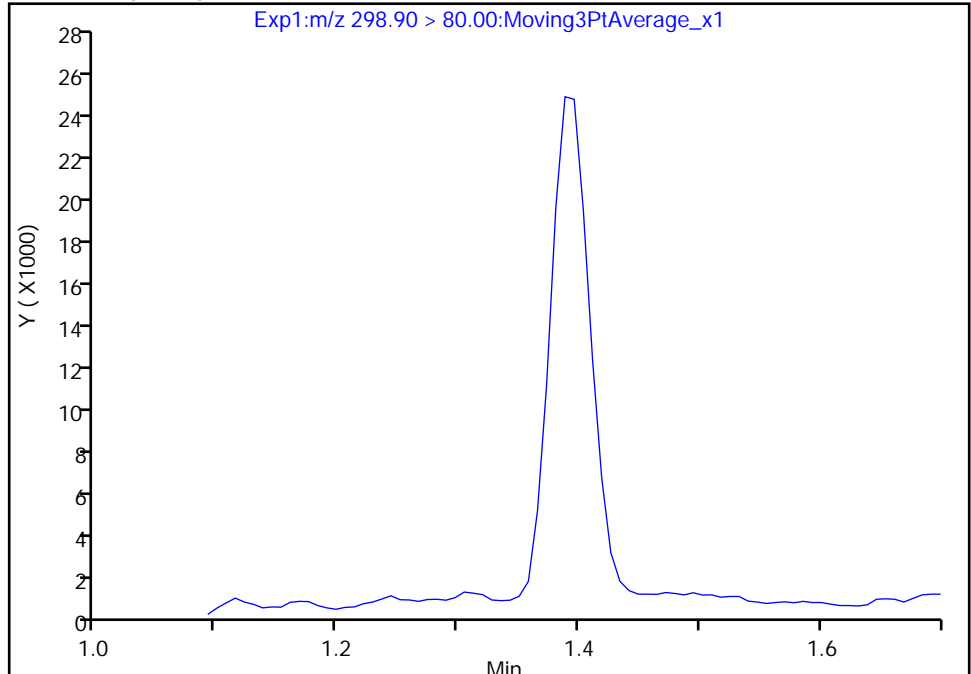

Manual Integration Results

RT: 1.39
Area: 55022
Amount: 0.774159
Amount Units: ng/ml

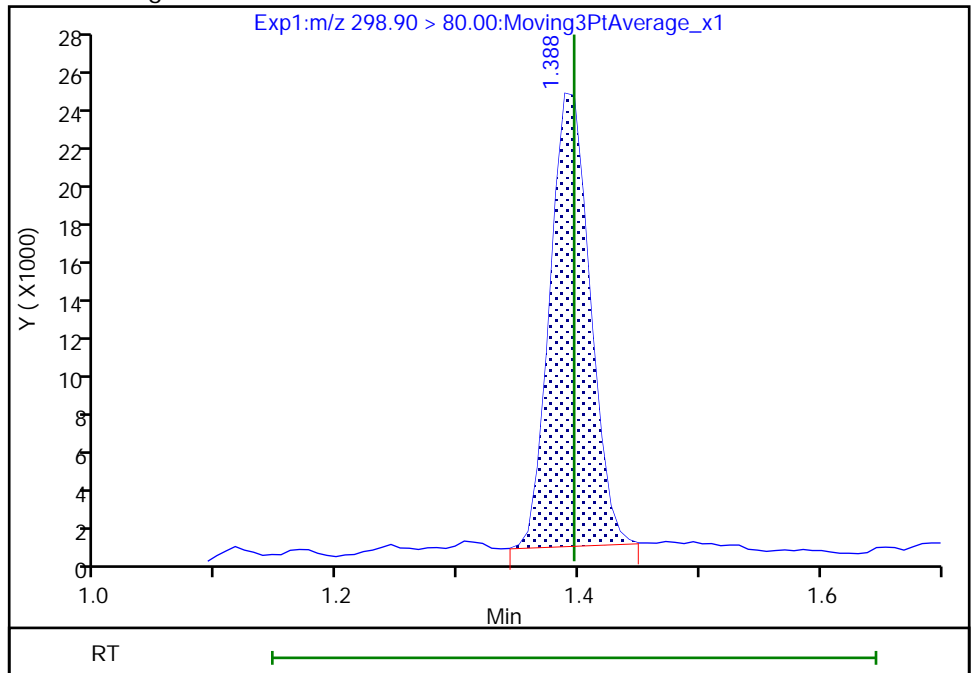

Reviewer: barnettj, 01-May-2018 17:15:08
Audit Action: Manually Integrated

Audit Reason: Missed Peak

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_029.d
Injection Date: 01-May-2018 13:20:51 Instrument ID: A8_N
Lims ID: 320-38382-A-7-A Lab Sample ID: 320-38382-7
Client ID: WGNA-041918-RW-3571
Operator ID: SACINSTLCMS01 ALS Bottle#: 20 Worklist Smp#: 27
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

1 Perfluorobutanesulfonic acid, CAS: 375-73-5

Signal: 2


Not Detected
Expected RT: 1.40

Processing Integration Results

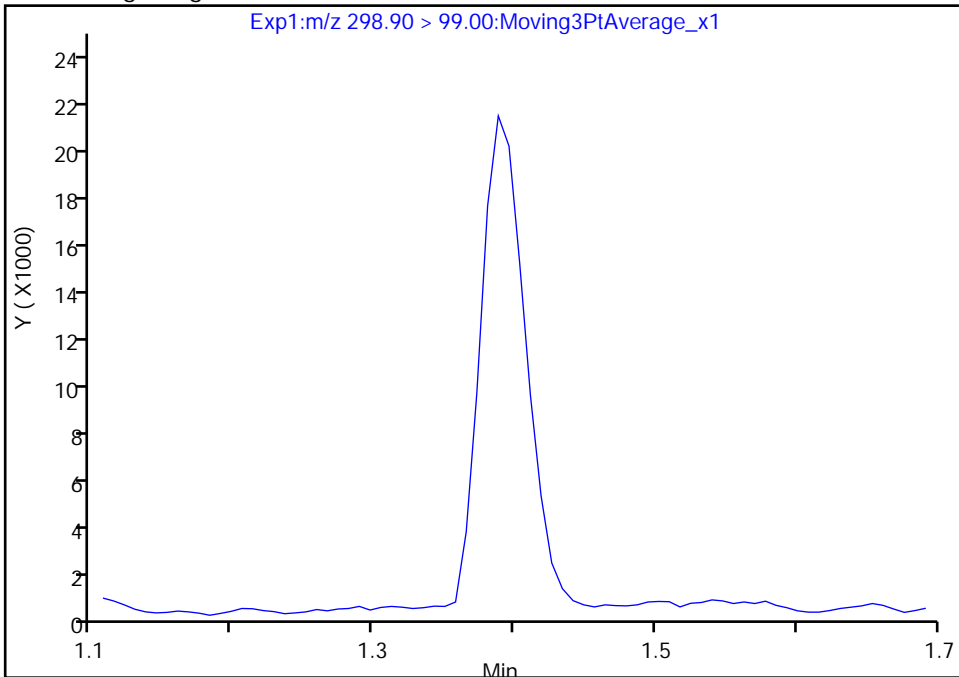

Manual Integration Results

RT: 1.39
Area: 46305
Amount: 0.774159
Amount Units: ng/ml

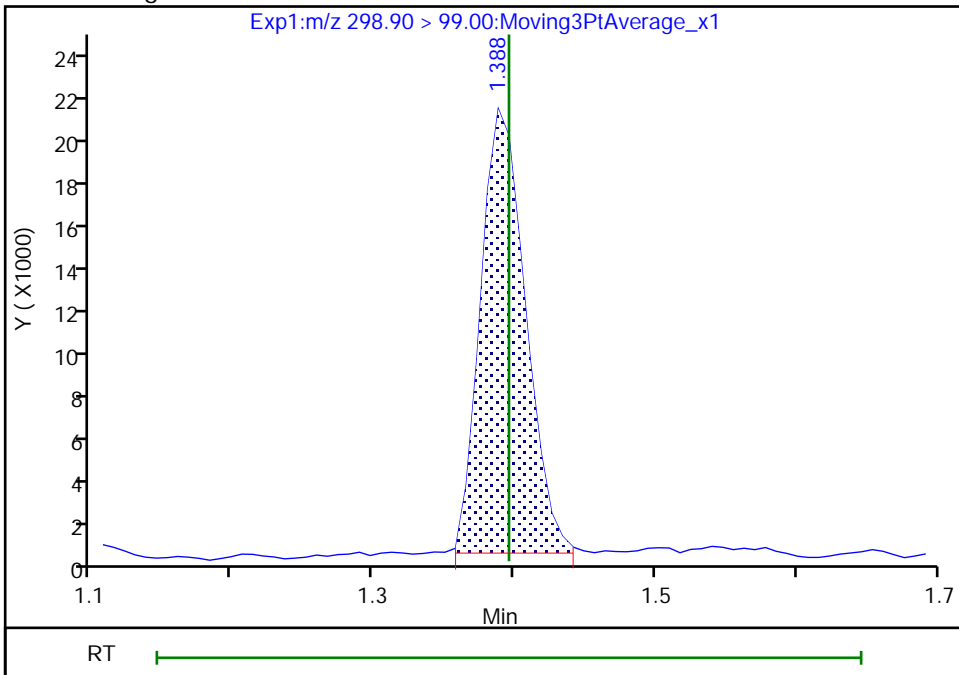

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Client Sample ID: WGNA-041918-FRB-3571 Lab Sample ID: 320-38382-8
 Matrix: Water Lab File ID: 2018.05.01_537AA_030.d
 Analysis Method: 537 Date Collected: 04/19/2018 11:05
 Extraction Method: 537 Date Extracted: 04/26/2018 09:35
 Sample wt/vol: 234.5 (mL) Date Analyzed: 05/01/2018 13:25
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 220847 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	17	U	43	17	7.2
335-67-1	Perfluorooctanoic acid (PFOA)	8.5	U	21	8.5	3.0
375-95-1	Perfluorononanoic acid (PFNA)	21	U	26	21	8.5
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	13	U	32	13	5.9
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.3	U	11	4.3	2.0
375-73-5	Perfluorobutanesulfonic acid (PFBS)	38	U	96	38	17

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	103		70-130
STL00996	13C2 PFDA	87		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_030.d
 Lims ID: 320-38382-A-8-A
 Client ID: WGNA-041918-FRB-3571
 Sample Type: Client
 Inject. Date: 01-May-2018 13:25:32 ALS Bottle#: 21 Worklist Smp#: 28
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-38382-a-8-a
 Misc. Info.: Plate: 1 Rack: 6
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 02-May-2018 10:27:59 Calib Date: 11-Apr-2018 12:09:09
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_009.d


Column 1 : Det: EXP1
 Process Host: XAWRK005

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
\$ 2 13C2 PFHxA	315.00 > 270.00	1.533	1.533	0.0	1.000	912513	10.3	7786	
* 6 13C2-PFOA	415.00 > 370.00	1.882	1.882	0.0		836252	10.0	5178	
* 7 13C4 PFOS	503.00 > 80.00	2.109	2.109	0.0		1978104	28.7	1156	
\$ 10 13C2 PFDA	515.00 > 470.00	2.269	2.269	0.0	1.000	618672	8.70	5984	


TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_030.d
Injection Date: 01-May-2018 13:25:32 Instrument ID: A8_N
Lims ID: 320-38382-A-8-A Lab Sample ID: 320-38382-8
Client ID: WGNA-041918-FRB-3571
Operator ID: SACINSTLCMS01 ALS Bottle#: 21 Worklist Smp#: 28
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL


1 Perfluorobutanesulfonic acid (ND) 1 Perfluorobutanesulfonic acid (ND) \$ 2 13C2 PFHxA

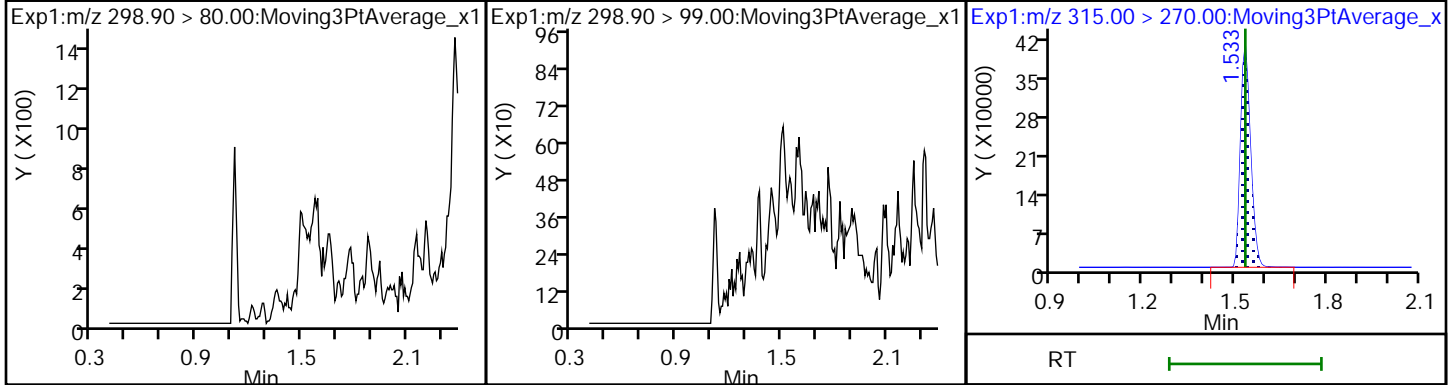


3 Perfluorohexanesulfonic acid (ND) 4 Perfluoroheptanoic acid (ND) * 6 13C2-PFOA

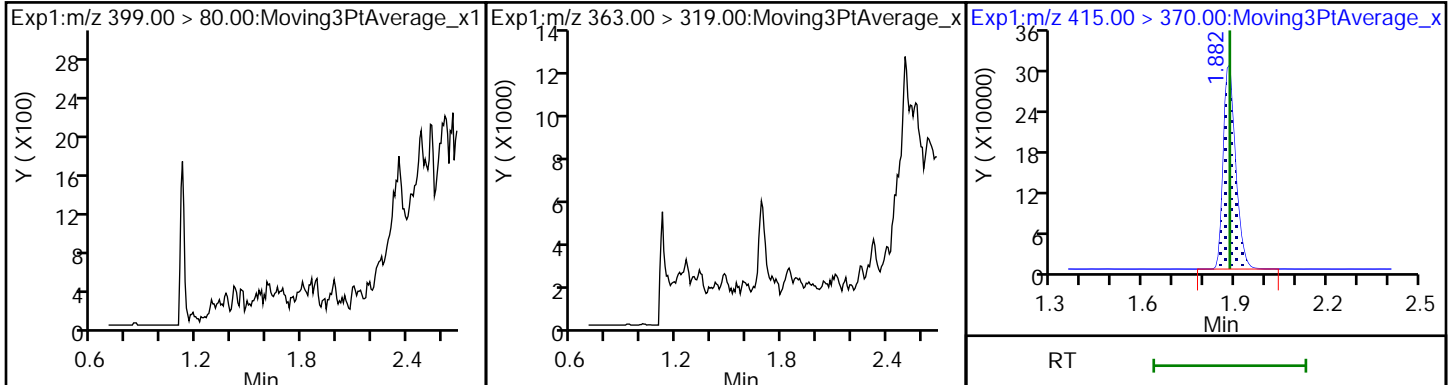


5 Perfluorooctanoic acid (ND) 5 Perfluorooctanoic acid (ND) * 7 13C4 PFOS

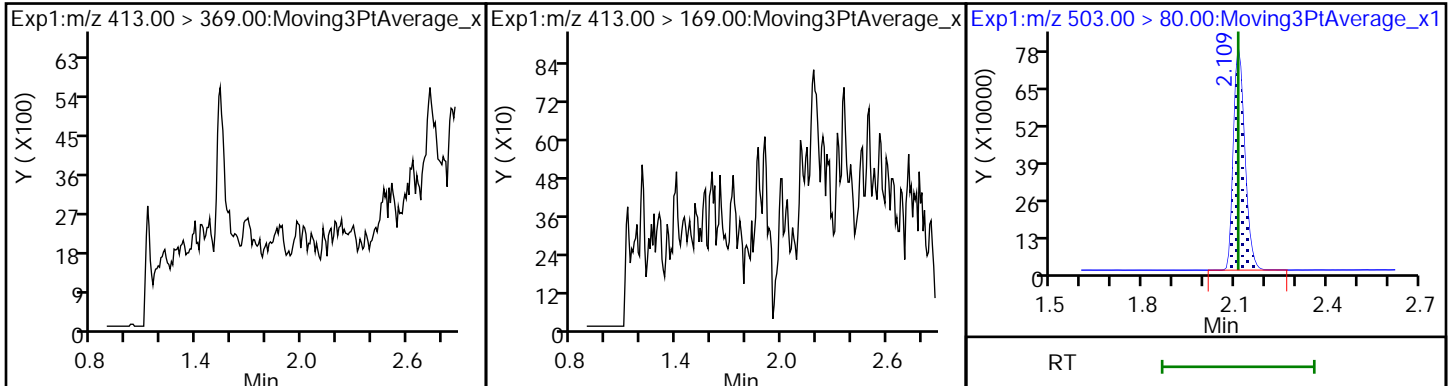

8 Perfluorooctane sulfonic acid (ND) 8 Perfluorooctane sulfonic acid (ND) 9 Perfluorononanoic acid (ND)

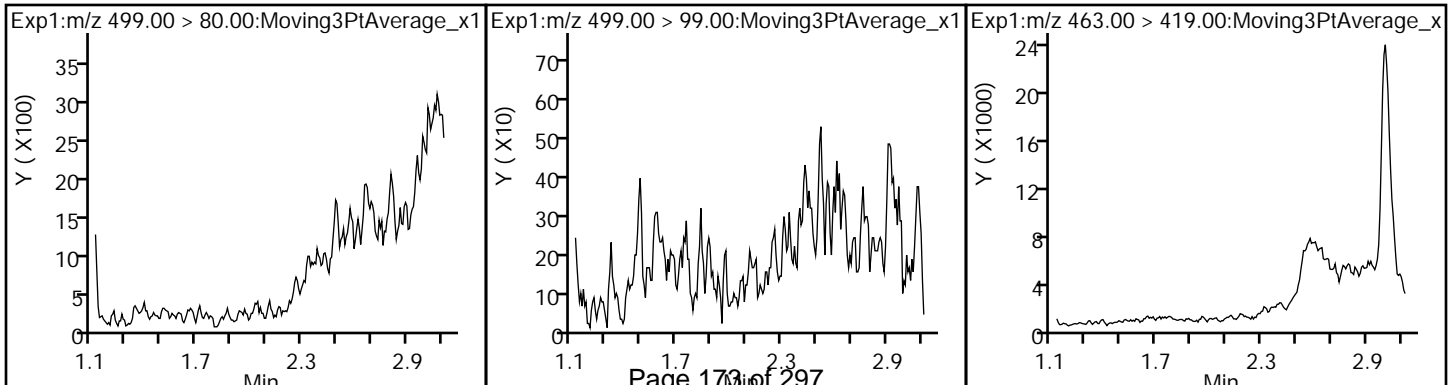

\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_030.d
 Lims ID: 320-38382-A-8-A
 Client ID: WGNA-041918-FRB-3571
 Sample Type: Client
 Inject. Date: 01-May-2018 13:25:32 ALS Bottle#: 21 Worklist Smp#: 28
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-38382-a-8-a
 Misc. Info.: Plate: 1 Rack: 6
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 02-May-2018 10:27:59 Calib Date: 11-Apr-2018 12:09:09
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK005

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	10.3	102.64
\$ 10 13C2 PFDA	10.0	8.70	86.99

FORM VI
LCMS BY INTERNAL STANDARD - INITIAL CALIBRATION DATA
CURVE EVALUATION

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1 Analy Batch No.: 217453

SDG No.: _____

Instrument ID: A8_N GC Column: GeminiC18 3 ID: 3(mm) Heated Purge: (Y/N) N

Calibration Start Date: 04/11/2018 11:45 Calibration End Date: 04/11/2018 12:09 Calibration ID: 38530

Calibration Files:

LEVEL:	LAB SAMPLE ID:	LAB FILE ID:
Level 1	IC 320-217453/3	2018.04.11_537ICALB_004.d
Level 2	IC 320-217453/4	2018.04.11_537ICALB_005.d
Level 3	IC 320-217453/5	2018.04.11_537ICALB_006.d
Level 4	IC 320-217453/6	2018.04.11_537ICALB_007.d
Level 5	IC 320-217453/7	2018.04.11_537ICALB_008.d
Level 6	IC 320-217453/8	2018.04.11_537ICALB_009.d

ANALYTE	RRF					CURVE TYPE	COEFFICIENT			#	MIN RRF	%RSD	#	MAX %RSD	R^2 OR COD	#	MIN R^2 OR COD
	LVL 1 LVL 6	LVL 2	LVL 3	LVL 4	LVL 5		B	M1	M2								
Perfluorobutanesulfonic acid (PFBS)	1.1422 0.9535	1.0952	1.0744	1.0454	1.0008	Ave		1.0519			6.4		30.0				
Perfluoroheptanoic acid (PFHpA)	1.0850 1.0447	1.0991	1.0649	1.0783	1.0702	Ave		1.0737			1.7		30.0				
Perfluorohexanesulfonic acid (PFHxS)	1.6457 1.6837	1.5988	1.6030	1.6384	1.6838	Ave		1.6422			2.3		30.0				
Perfluorooctanoic acid (PFOA)	1.0599 1.0325	1.0296	1.0703	1.0516	1.1300	Ave		1.0623			3.5		30.0				
Perfluorooctanesulfonic acid (PFOS)	1.0432 1.0989	1.0519	1.0326	1.0935	1.0764	Ave		1.0661			2.6		30.0				
Perfluorononanoic acid (PFNA)	0.8261 0.8363	0.8133	0.8488	0.8818	0.8480	Ave		0.8424			2.8		30.0				
13C2 PFHxA	1.0447 1.0648	1.0532	1.0875	1.0687	1.0602	Ave		1.0632			1.4		30.0				
13C2 PFDA	0.8513 0.8262	0.8714	0.8533	0.8487	0.8519	Ave		0.8505			1.7		30.0				

Note: The M1 coefficient is the same as Ave RRF for an Ave curve type.

FORM VI
LCMS BY INTERNAL STANDARD - INITIAL CALIBRATION DATA
RESPONSE AND CONCENTRATION

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1 Analy Batch No.: 217453

SDG No.: _____

Instrument ID: A8_N GC Column: GeminiC18 3 ID: 3(mm) Heated Purge: (Y/N) N

Calibration Start Date: 04/11/2018 11:45 Calibration End Date: 04/11/2018 12:09 Calibration ID: 38530

Calibration Files:

LEVEL:	LAB SAMPLE ID:	LAB FILE ID:
Level 1	IC 320-217453/3	2018.04.11_537ICALB_004.d
Level 2	IC 320-217453/4	2018.04.11_537ICALB_005.d
Level 3	IC 320-217453/5	2018.04.11_537ICALB_006.d
Level 4	IC 320-217453/6	2018.04.11_537ICALB_007.d
Level 5	IC 320-217453/7	2018.04.11_537ICALB_008.d
Level 6	IC 320-217453/8	2018.04.11_537ICALB_009.d

ANALYTE	IS REF	CURVE TYPE	RESPONSE					CONCENTRATION (NG/ML)				
			LVL 1 LVL 6	LVL 2	LVL 3	LVL 4	LVL 5	LVL 1 LVL 6	LVL 2	LVL 3	LVL 4	LVL 5
Perfluorobutanesulfonic acid (PFBS)	PFOS	Ave	870696 13871852	1696932	4015148	8010147	10764182	9.00 180	20.0	45.0	90.1	135
Perfluoroheptanoic acid (PFHpA)	13PF OA	Ave	108741 1996261	218860	489075	1044752	1450463	0.960 19.4	2.16	4.86	9.72	14.6
Perfluorohexanesulfonic acid (PFHxS)	PFOS	Ave	418640 8226588	831963	2012030	4216387	6082352	3.00 60.5	6.72	15.1	30.2	45.4
Perfluorooctanoic acid (PFOA)	13PF OA	Ave	219100 4019004	417632	1001316	2075568	3119787	1.98 39.6	4.40	9.90	19.8	29.7
Perfluorooctanesulfonic acid (PFOS)	PFOS	Ave	349354 7016962	715378	1693810	3678059	5081660	3.95 79.1	8.79	19.8	39.5	59.3
Perfluorononanoic acid (PFNA)	13PF OA	Ave	170770 3255374	329904	794076	1740422	2341235	1.98 39.6	4.40	9.90	19.8	29.7
13C2 PFHxA	13PF OA	Ave	1090690 1046576	970942	1027706	1065262	985534	10.0 10.0	10.0	10.0	10.0	10.0
13C2 PFDA	13PF OA	Ave	888742 812112	803402	806360	845990	791901	10.0 10.0	10.0	10.0	10.0	10.0

Curve Type Legend:

Ave = Average ISTD

FORM VI
 LCMS BY INTERNAL STANDARD - INITIAL CALIBRATION DATA
 READBACK PERCENT ERROR

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1 Analy Batch No.: 217453

SDG No.: _____


Instrument ID: A8_N GC Column: GeminiC18 3 ID: 3(mm) Heated Purge: (Y/N) N


Calibration Start Date: 04/11/2018 11:45 Calibration End Date: 04/11/2018 12:09 Calibration ID: 38530

Calibration Files:

LEVEL:	LAB SAMPLE ID:	LAB FILE ID:
Level 1	IC 320-217453/3	2018.04.11_537ICALB_004.d
Level 2	IC 320-217453/4	2018.04.11_537ICALB_005.d
Level 3	IC 320-217453/5	2018.04.11_537ICALB_006.d
Level 4	IC 320-217453/6	2018.04.11_537ICALB_007.d
Level 5	IC 320-217453/7	2018.04.11_537ICALB_008.d
Level 6	IC 320-217453/8	2018.04.11_537ICALB_009.d

ANALYTE	PERCENT ERROR						PERCENT ERROR LIMIT					
	LVL 1 #	LVL 2 #	LVL 3 #	LVL 4 #	LVL 5 #	LVL 6 #	LVL 1	LVL 2	LVL 3	LVL 4	LVL 5	LVL 6
Perfluorobutanesulfonic acid (PFBS)	8.6	4.1	2.1	-0.6	-4.9	-9.4	50	30	30	30	30	30
Perfluoroheptanoic acid (PFHpA)	1.0	2.4	-0.8	0.4	-0.3	-2.7	50	30	30	30	30	30
Perfluorohexanesulfonic acid (PFHxS)	0.2	-2.6	-2.4	-0.2	2.5	2.5	50	30	30	30	30	30
Perfluorooctanoic acid (PFOA)	-0.2	-3.1	0.7	-1.0	6.4	-2.8	50	30	30	30	30	30
Perfluorooctanesulfonic acid (PFOS)	-2.1	-1.3	-3.1	2.6	1.0	3.1	50	30	30	30	30	30
Perfluorononanoic acid (PFNA)	-1.9	-3.5	0.8	4.7	0.7	-0.7	50	30	30	30	30	30
13C2 PFHxA	-1.7	-0.9	2.3	0.5	-0.3	0.1	30	30	30	30	30	30
13C2 PFDA	0.1	2.5	0.3	-0.2	0.2	-2.9	30	30	30	30	30	30

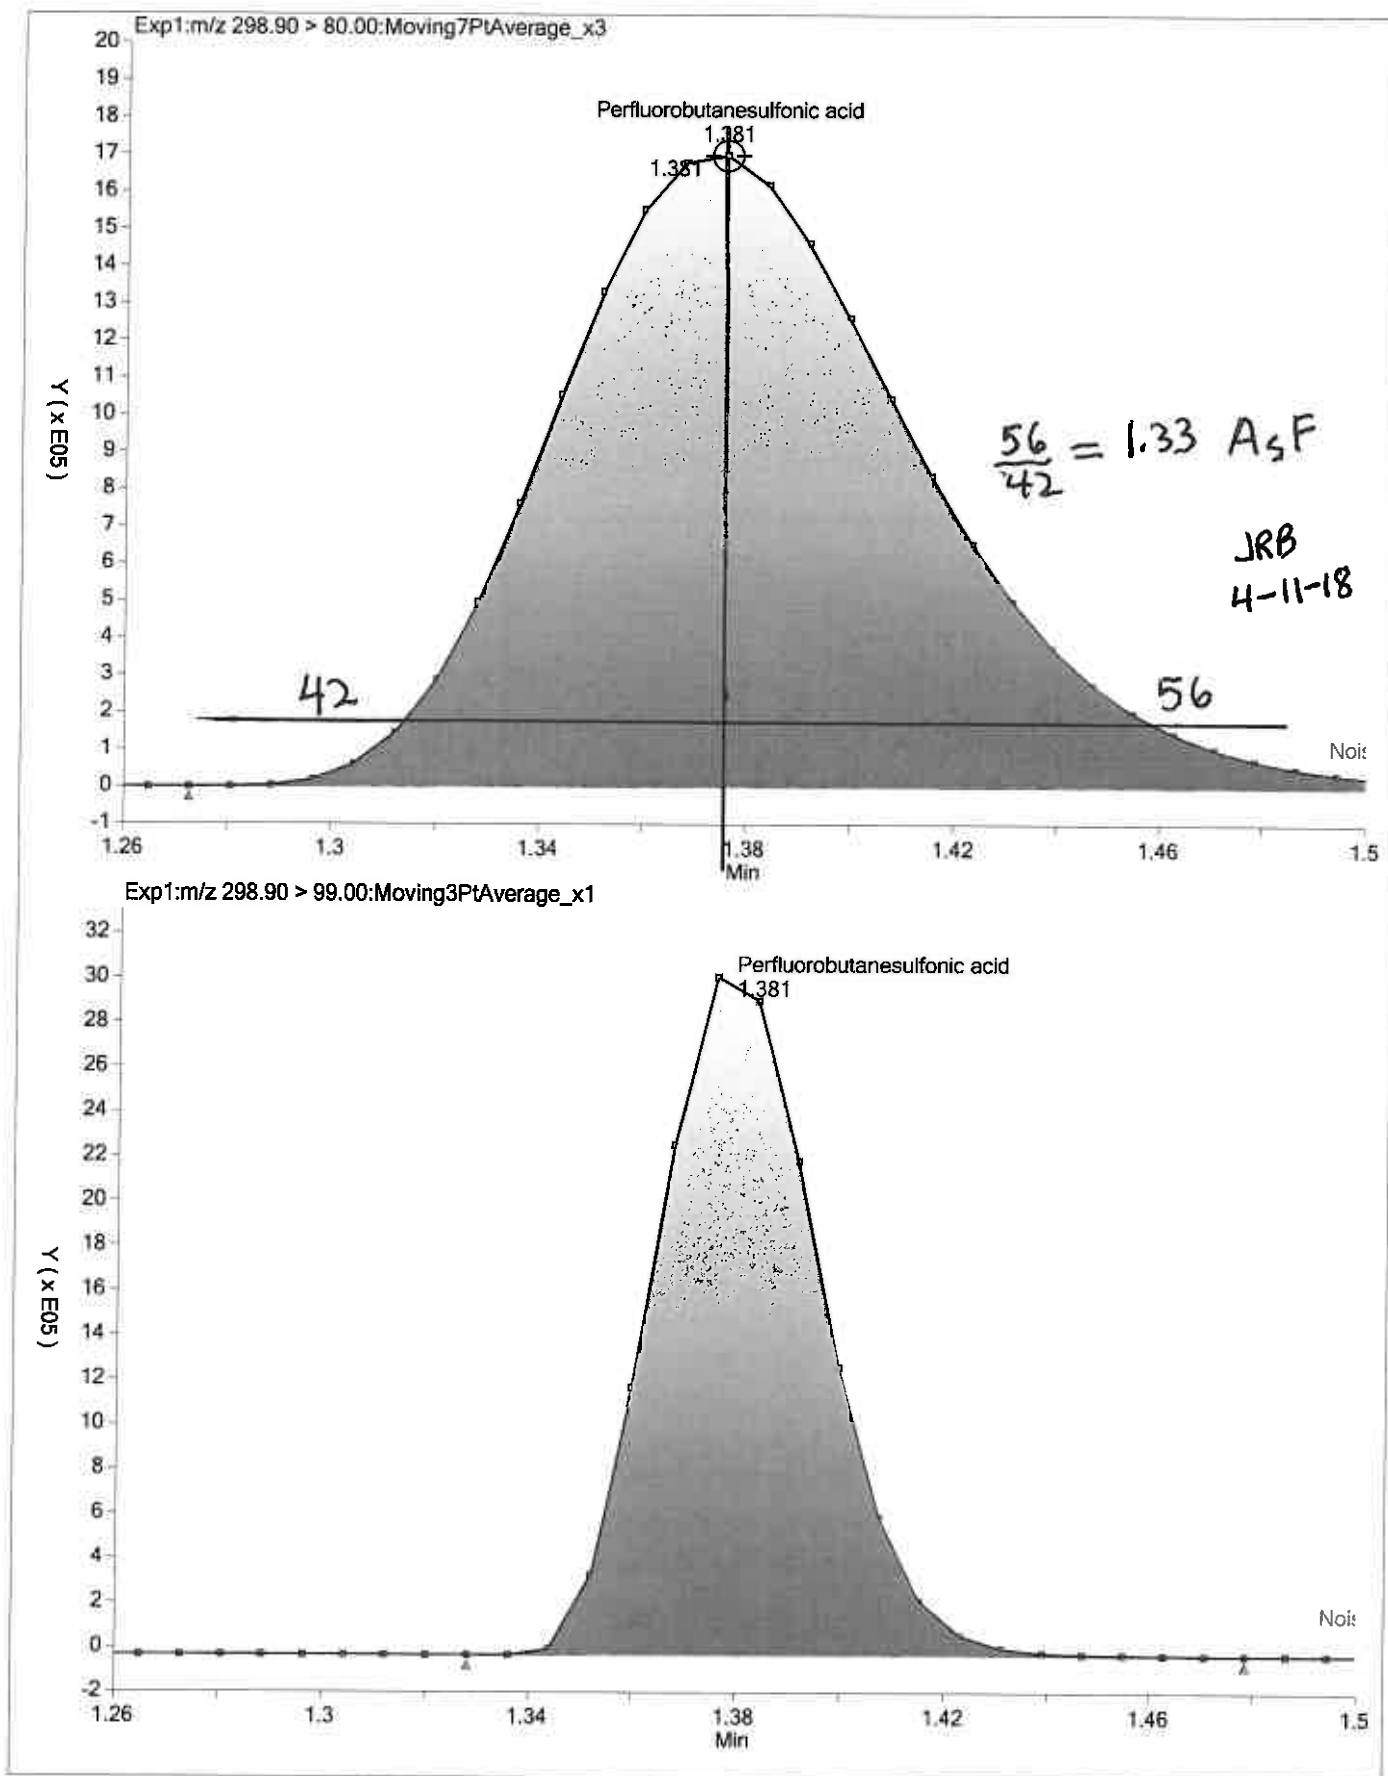

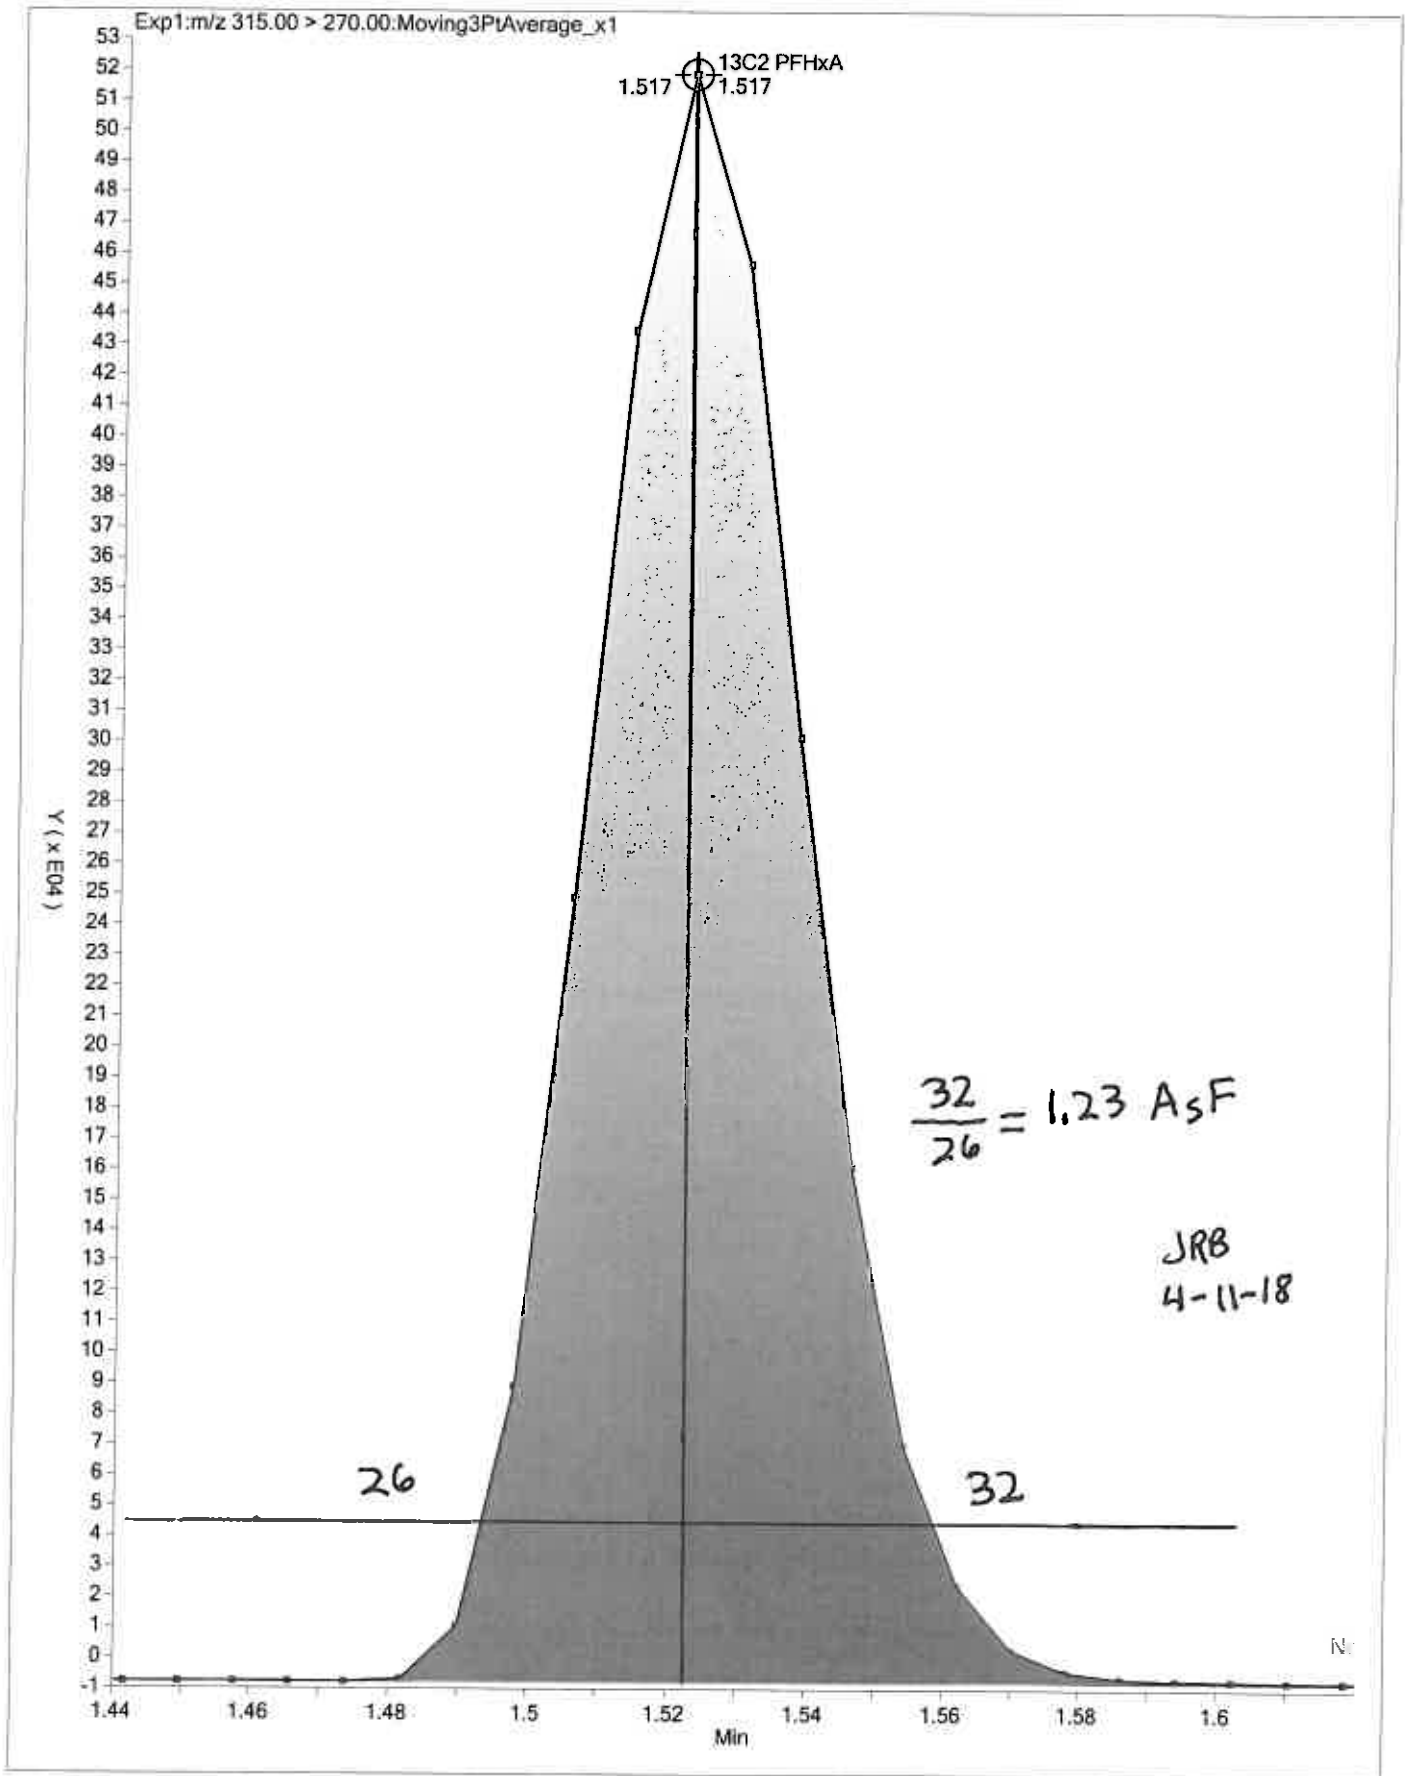

TestAmerica Laboratories
Istd/Surrogate Recovery Report

Worklist Name: 11APR2018A_537B_ICAL Worklist Num: 56557
 Instrument: A8_N Method: 537_A8_N
 Batch Directory: \\ChromNa\Sacramento\ChromData\A8_N\20180411-56557.b
 Limit Group: LC 537 ICAL
 Analysis Type: SemiVOA
 Inj Volume: 2.00 Inj Vol Units: ul

Lims Batch: 217453
 CCV IS Mode: Select Ical Level, Cal Level: 3
 Non-Cal IS Mode: Last Ccal Sample

\$ 2 13C2 PFHxA
 \$ 10 13C2 PFDA

Lab ID	Inj Date	\$ 2	\$ 10	* 6 13C2-PFOA	* 7 13C4 PFOS
IS Std					
# 1 RB	11-Apr-2018 11:36:27			1027183 1.87	2580682 2.11
# 2 RB	11-Apr-2018 11:41:06			957389 93.2	2343443 90.8
IS Std					
# 3 IC L1	11-Apr-2018 11:45:47	1.52 98.26	2.26 100.10	1044020> 100.0*	2429483> 100.0*
# 4 IC L2	11-Apr-2018 11:50:27	1.51 99.06	2.26 102.50	921915> 88.3*	2220259> 91.4*
# 5 IC L3	11-Apr-2018 11:55:08	1.52 102.30	2.26 100.30	945031> 90.5*	2380125> 98.0*
# 6 IC L4	11-Apr-2018 11:59:48	1.52 100.50	2.26 99.79	996809> 95.5*	2440107> 100.4*
# 7 IC L5	11-Apr-2018 12:04:29	1.52 99.72	2.26 100.20	929546> 89.0*	2283311> 94.0*
# 8 IC L6	11-Apr-2018 12:09:09	1.51 100.10	2.25 97.15	982926> 94.1*	2316327> 95.3*
IS Std					
# 9 RB	11-Apr-2018 12:13:50			945031 1.87	2380125 2.11
IS Std					
# 10 CCVL	11-Apr-2018 12:18:29	1.52 97.44	2.26 103.40	964533 96.8	2387973 97.9
IS Std					
# 11 ICB	11-Apr-2018 12:23:10			964533 1.87	2387973 2.10
IS Std					
# 12 ICV	11-Apr-2018 12:27:50	1.51 92.99	2.25 91.91	1123391 112.7	2710764 111.1

13C2-PFOA

$$RPD = \frac{1044020 - 921915}{\frac{1044020 + 921915}{2}} \times 100 = 12.4$$

13C4-PFOS

$$RPD = \frac{2440107 - 2220259}{\frac{2440107 + 2220259}{2}} \times 100 = 9.43$$

JRB
4-11-18

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_004.d
 Lims ID: IC L1
 Client ID:
 Sample Type: IC Calib Level: 1
 Inject. Date: 11-Apr-2018 11:45:47 ALS Bottle#: 1 Worklist Smp#: 3
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: L1_537
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub9

Method: \\ChromNa\Sacramento\ChromData\A8_N\20180411-56557.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 11-Apr-2018 12:35:27 Calib Date: 11-Apr-2018 12:09:09
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last Ical File: \\ChromNA\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK015

First Level Reviewer: westendorfc Date: 11-Apr-2018 12:31:32

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.381	1.382	-0.001	1.000	870696	9.77		690	
298.90 > 99.00	1.381	1.382	-0.001	1.000	638403		1.36(0.00-0.00)	875	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.517	1.515	0.002	1.000	1090690	9.83		11391	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.669	1.669	0.0	1.000	418640	3.01		133	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.669	1.669	0.0	1.000	108741	0.9701		13.9	
* 6 13C2-PFOA									
415.00 > 370.00	1.866	1.865	0.001		1044020	10.0		6295	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.866	1.866	0.0	1.000	219100	1.98		35.1	
413.00 > 169.00	1.866	1.866	0.0	1.000	116014		1.89(0.00-0.00)	128	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.102	2.094	0.008	1.000	349354	3.87		105	a
499.00 > 99.00	2.102	2.094	0.008	1.000	79188		4.41(0.00-0.00)	237	a
* 7 13C4 PFOS									
503.00 > 80.00	2.102	2.102	0.0		2429483	28.7		1437	
9 Perfluorononanoic acid									
463.00 > 419.00	2.109	2.109	0.0	1.000	170770	1.94		31.2	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.261	2.260	0.001	1.000	888742	10.0		8004	

QC Flag Legend

Review Flags

a - User Assigned ID

Reagents:

LC537-L1_00022

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_004.d

Injection Date: 11-Apr-2018 11:45:47

Instrument ID: A8_N

Lims ID: IC L1

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 1

Worklist Smp#: 3

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA

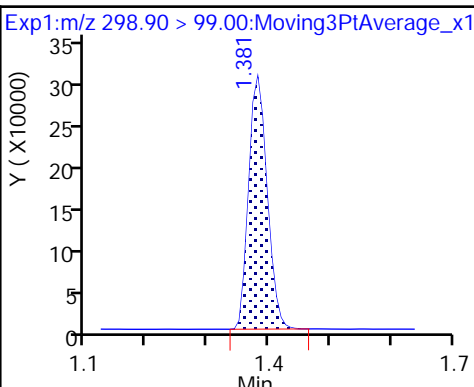

3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA

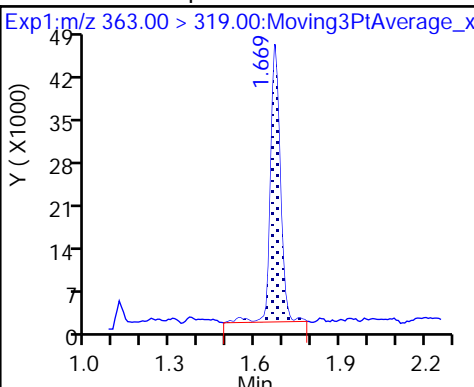

5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)

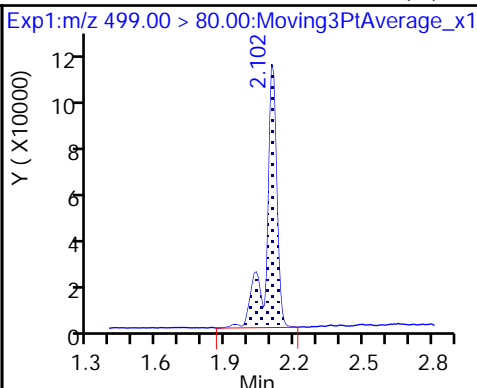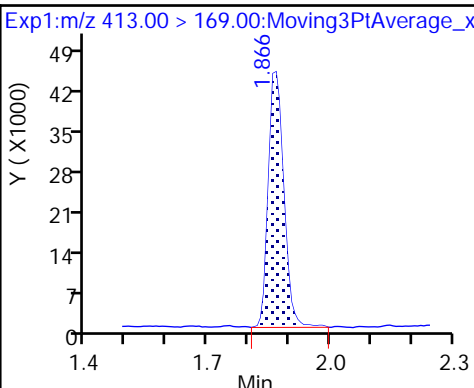


8 Perfluorooctane sulfonic acid

* 7 13C4 PFOS

9 Perfluorononanoic acid

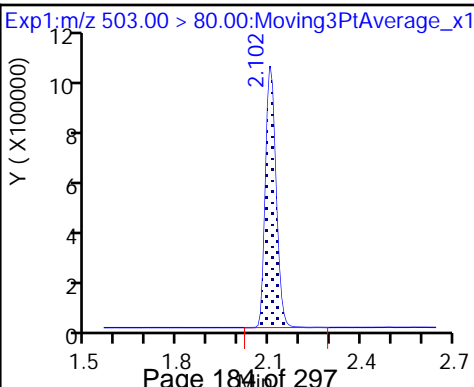

\$ 10 13C2 PFDA

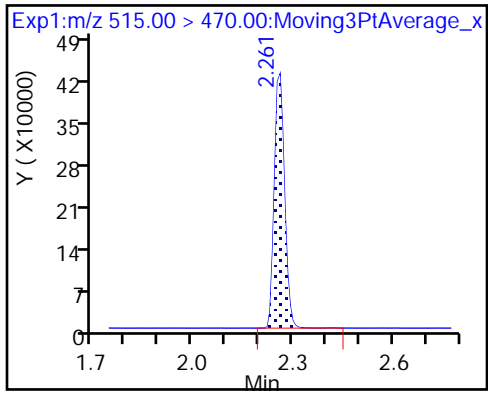

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_004.d
Injection Date: 11-Apr-2018 11:45:47 Instrument ID: A8_N
Lims ID: IC L1
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 1 Worklist Smp#: 3
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.09

Processing Integration Results

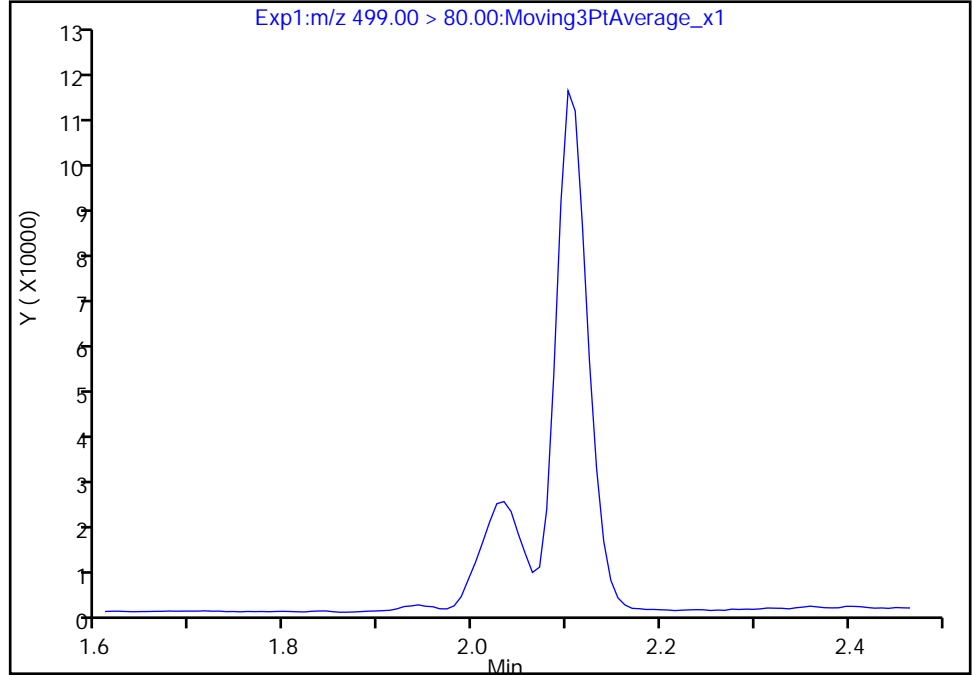

RT: 2.10
Area: 349354
Amount: 3.868513
Amount Units: ng/ml

Manual Integration Results

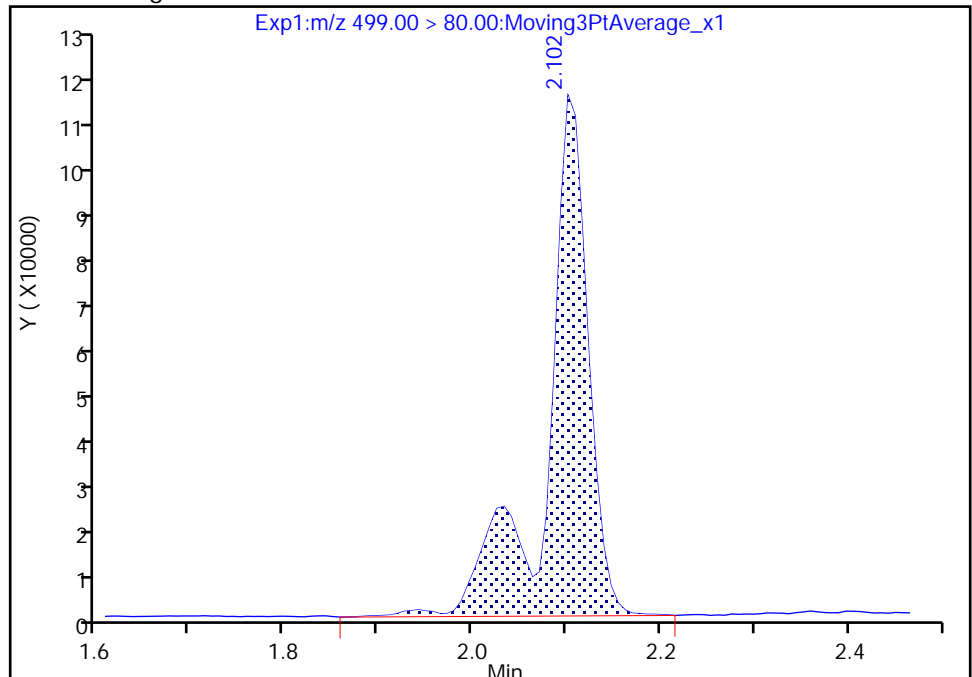

Reviewer: westendorfc, 11-Apr-2018 12:31:29
Audit Action: Assigned Compound ID

Audit Reason: Peak assignment corrected

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_005.d
 Lims ID: IC L2
 Client ID:
 Sample Type: IC Calib Level: 2
 Inject. Date: 11-Apr-2018 11:50:27 ALS Bottle#: 2 Worklist Smp#: 4
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: L2_537
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub9

Method: \\ChromNa\Sacramento\ChromData\A8_N\20180411-56557.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 11-Apr-2018 12:35:28 Calib Date: 11-Apr-2018 12:09:09
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last Ical File: \\ChromNA\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK015

First Level Reviewer: westendorfc Date: 11-Apr-2018 12:31:37

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.381	1.382	-0.001	1.000	1696932	20.8		1370	
298.90 > 99.00	1.381	1.382	-0.001	1.000	1238814		1.37(0.00-0.00)	1448	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.510	1.515	-0.005	1.000	970942	9.91		9056	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.669	1.669	0.0	1.000	218860	2.21		24.5	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.669	1.669	0.0	1.000	831963	6.54		251	
* 6 13C2-PFOA									
415.00 > 370.00	1.866	1.865	0.001		921915	10.0		5396	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.866	1.866	0.0	1.000	417632	4.26		64.6	
413.00 > 169.00	1.866	1.866	0.0	1.000	226435		1.84(0.00-0.00)	235	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.102	2.094	0.008	1.000	715378	8.67		193	a
499.00 > 99.00	2.102	2.094	0.008	1.000	153149		4.67(0.00-0.00)	389	a
* 7 13C4 PFOS									
503.00 > 80.00	2.102	2.102	0.0		2220259	28.7		1258	
9 Perfluorononanoic acid									
463.00 > 419.00	2.109	2.109	0.0	1.000	329904	4.25		54.3	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.261	2.260	0.001	1.000	803402	10.2		7224	

QC Flag Legend

Review Flags

a - User Assigned ID

Reagents:

LC537-L2_00022

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_005.d

Injection Date: 11-Apr-2018 11:50:27

Instrument ID: A8_N

Lims ID: IC L2

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 2

Worklist Smp#: 4

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



4 Perfluoroheptanoic acid

3 Perfluorohexanesulfonic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)

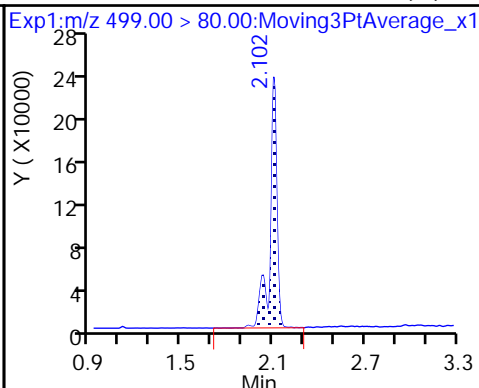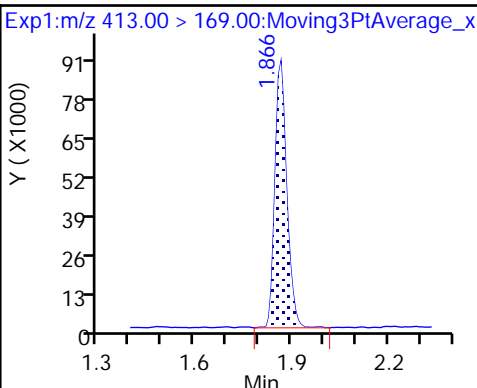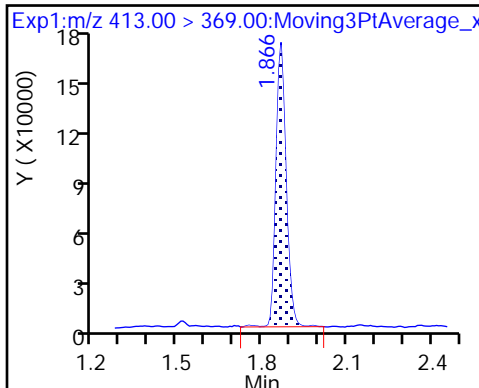


8 Perfluorooctane sulfonic acid

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA

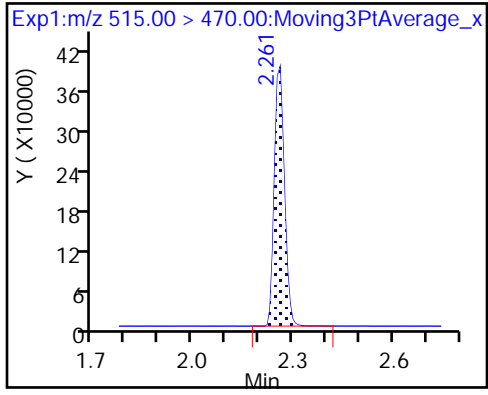

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_005.d
Injection Date: 11-Apr-2018 11:50:27 Instrument ID: A8_N
Lims ID: IC L2
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 2 Worklist Smp#: 4
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.09

Processing Integration Results

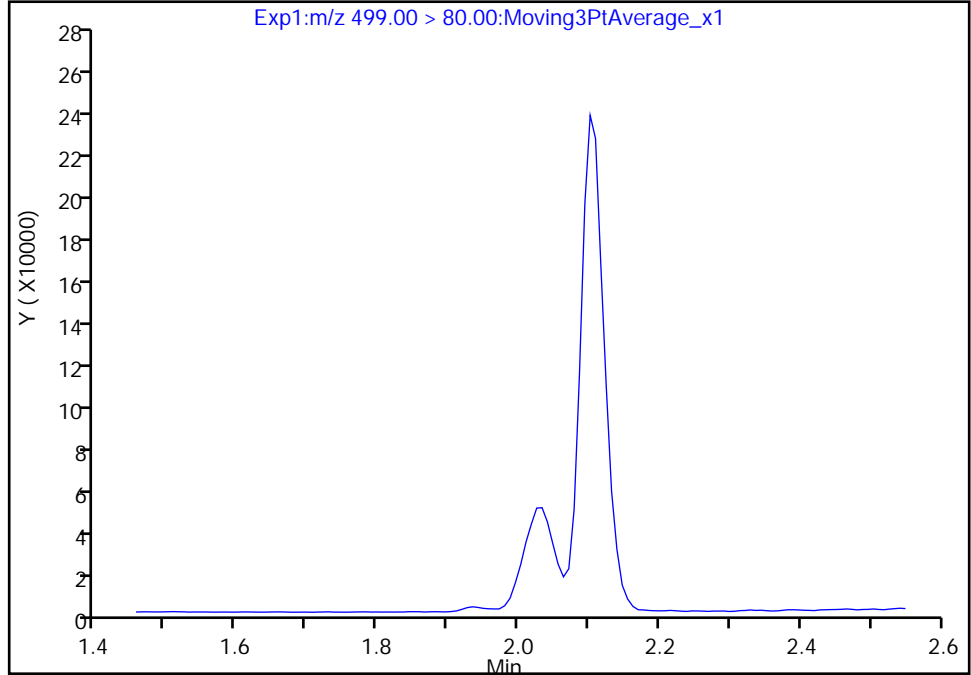

Manual Integration Results

RT: 2.10
Area: 715378
Amount: 8.668106
Amount Units: ng/ml

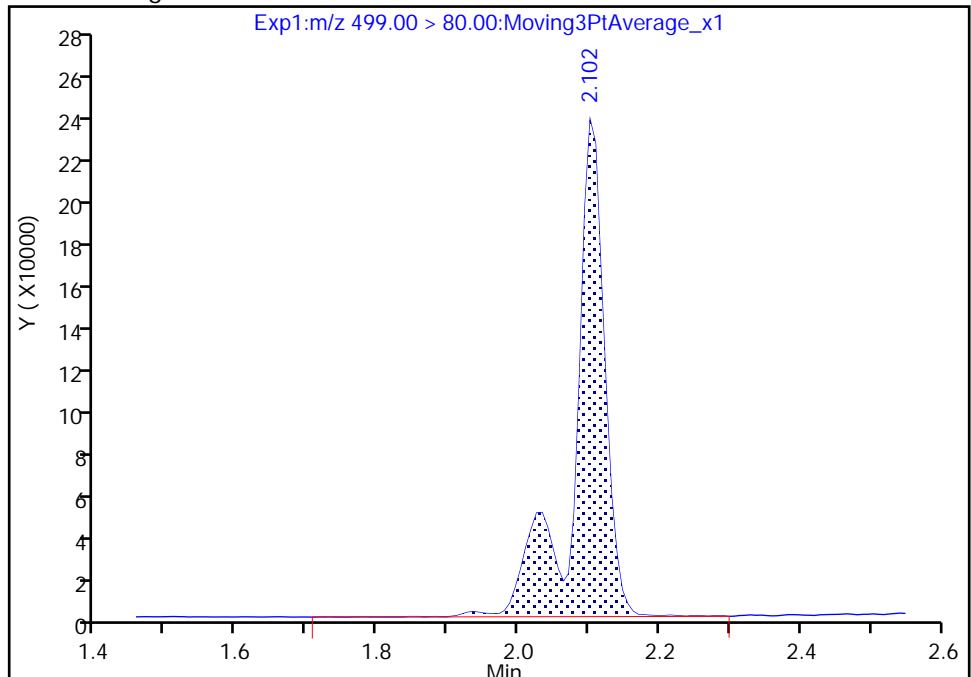

Reviewer: westendorfc, 11-Apr-2018 12:31:35
Audit Action: Assigned Compound ID

Audit Reason: Peak assignment corrected

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_006.d
 Lims ID: IC L3
 Client ID:
 Sample Type: IC Calib Level: 3
 Inject. Date: 11-Apr-2018 11:55:08 ALS Bottle#: 3 Worklist Smp#: 5
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: L3_537
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub9

Method: \\ChromNa\Sacramento\ChromData\A8_N\20180411-56557.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 11-Apr-2018 12:35:29 Calib Date: 11-Apr-2018 12:09:09
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last Ical File: \\ChromNA\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK015

First Level Reviewer: westendorfc Date: 11-Apr-2018 12:31:41

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.388	1.382	0.006	1.000	4015148	46.0		3087	
298.90 > 99.00	1.388	1.382	0.006	1.000	3101910		1.29(0.00-0.00)	3481	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.517	1.515	0.002	1.000	1027706	10.2		8913	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.677	1.669	0.008	1.000	2012030	14.8		618	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.677	1.669	0.008	1.000	489075	4.82		58.8	
* 6 13C2-PFOA									
415.00 > 370.00	1.866	1.865	0.001		945031	10.0		5639	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.874	1.866	0.008	1.000	1001316	9.97		149	
413.00 > 169.00	1.866	1.866	0.0	0.996	522184		1.92(0.00-0.00)	570	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.109	2.094	0.015	1.000	1693810	19.1		469	a
499.00 > 99.00	2.109	2.094	0.015	1.000	359496		4.71(0.00-0.00)	862	a
* 7 13C4 PFOS									
503.00 > 80.00	2.109	2.102	0.007		2380125	28.7		1348	
9 Perfluorononanoic acid									
463.00 > 419.00	2.117	2.109	0.008	1.000	794076	9.97		123	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.261	2.260	0.001	1.000	806360	10.0		7204	

QC Flag Legend

Review Flags

a - User Assigned ID

Reagents:

LC537-L3_00025

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_006.d

Injection Date: 11-Apr-2018 11:55:08

Instrument ID: A8_N

Lims ID: IC L3

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 3

Worklist Smp#: 5

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA

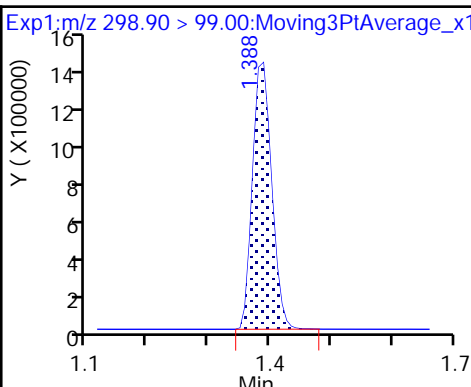

3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA

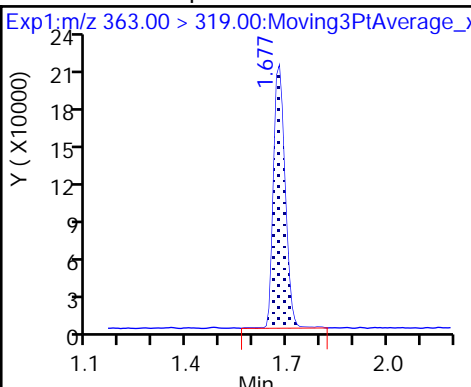

5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)

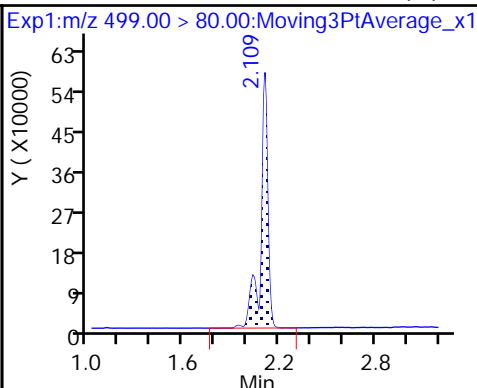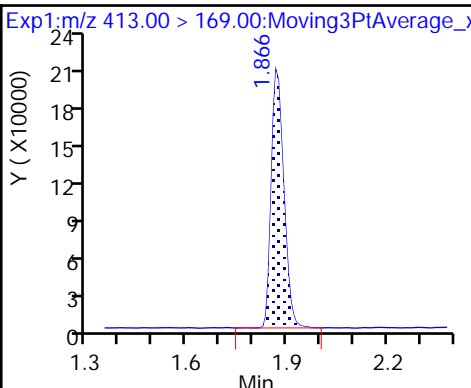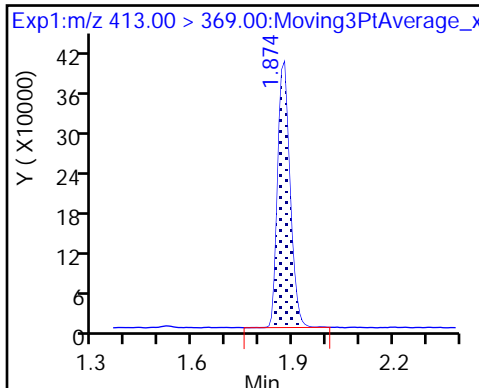


8 Perfluorooctane sulfonic acid

* 7 13C4 PFOS

9 Perfluorononanoic acid

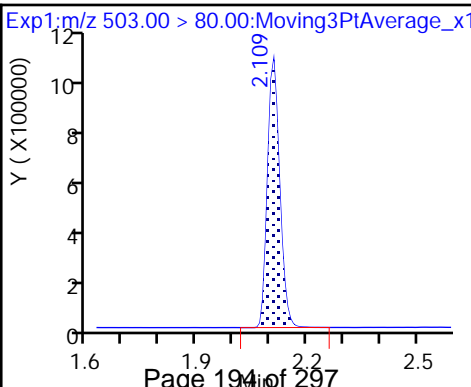

\$ 10 13C2 PFDA

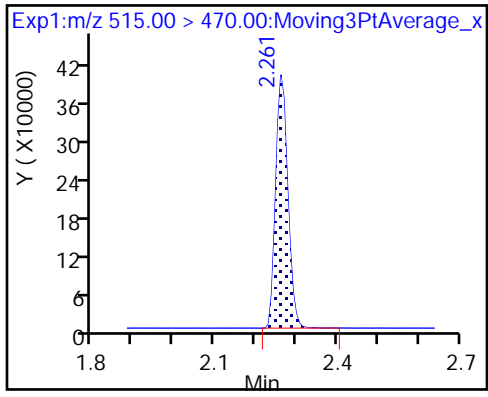

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_006.d
Injection Date: 11-Apr-2018 11:55:08 Instrument ID: A8_N
Lims ID: IC L3
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 3 Worklist Smp#: 5
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.09

Processing Integration Results

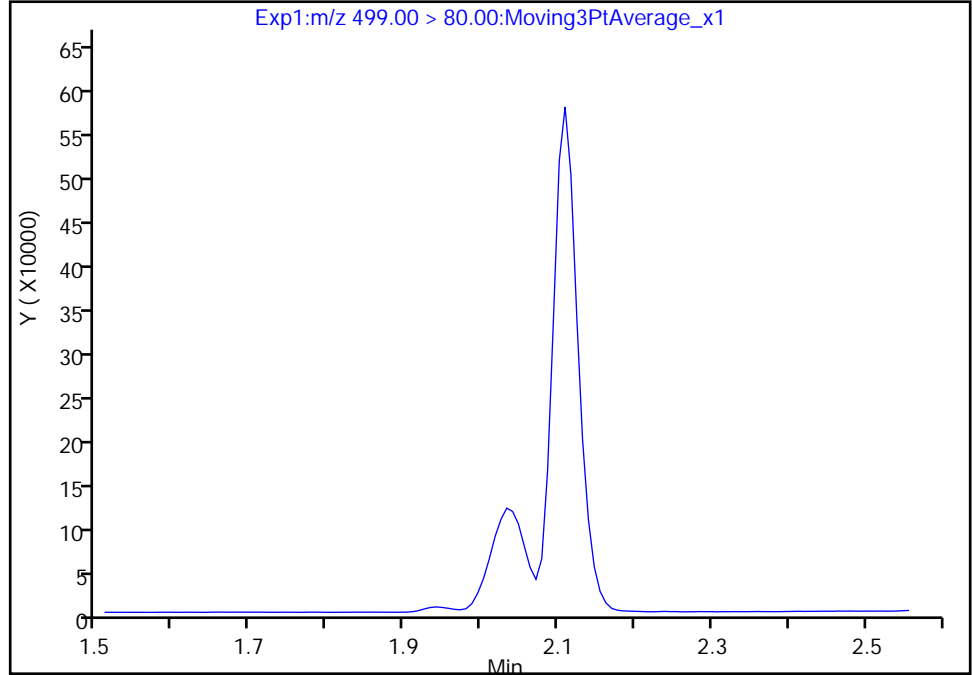

RT: 2.11
Area: 1693810
Amount: 19.145080
Amount Units: ng/ml

Manual Integration Results

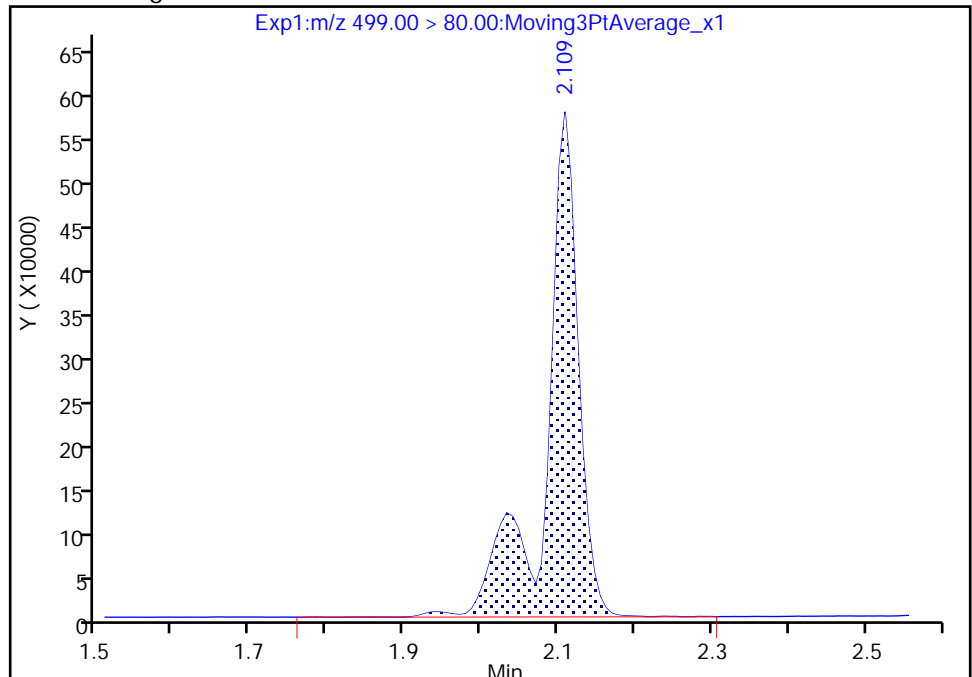

Reviewer: westendorfc, 11-Apr-2018 12:31:39
Audit Action: Assigned Compound ID

Audit Reason: Peak assignment corrected

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_007.d
 Lims ID: IC L4
 Client ID:
 Sample Type: ICISAV Calib Level: 4
 Inject. Date: 11-Apr-2018 11:59:48 ALS Bottle#: 4 Worklist Smp#: 6
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: L4_537
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub9

Method: \\ChromNa\Sacramento\ChromData\A8_N\20180411-56557.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 11-Apr-2018 12:35:30 Calib Date: 11-Apr-2018 12:09:09
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last Ical File: \\ChromNA\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK015

First Level Reviewer: westendorfc Date: 11-Apr-2018 12:31:47

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.381	1.382	-0.001	1.000	8010147	89.5		5376	
298.90 > 99.00	1.381	1.382	-0.001	1.000	6369602		1.26(0.00-0.00)	6440	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.517	1.515	0.002	1.000	1065262	10.1		8514	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.669	1.669	0.0	1.000	1044752	9.76		122	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.669	1.669	0.0	1.000	4216387	30.2		1268	
* 6 13C2-PFOA									
415.00 > 370.00	1.866	1.865	0.001		996809	10.0		6544	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.866	1.866	0.0	1.000	2075568	19.6		309	
413.00 > 169.00	1.866	1.866	0.0	1.000	1142250		1.82(0.00-0.00)	1229	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.102	2.094	0.008	1.000	3678059	40.6		1000	a
499.00 > 99.00	2.102	2.094	0.008	1.000	748966		4.91(0.00-0.00)	1731	a
* 7 13C4 PFOS									
503.00 > 80.00	2.102	2.102	0.0		2440107	28.7		1331	
9 Perfluorononanoic acid									
463.00 > 419.00	2.109	2.109	0.0	1.000	1740422	20.7		274	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.261	2.260	0.001	1.000	845990	9.98		7531	

QC Flag Legend

Review Flags

a - User Assigned ID

Reagents:

LC537-L4_00022

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_007.d

Injection Date: 11-Apr-2018 11:59:48

Instrument ID: A8_N

Lims ID: IC L4

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 4

Worklist Smp#: 6

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA

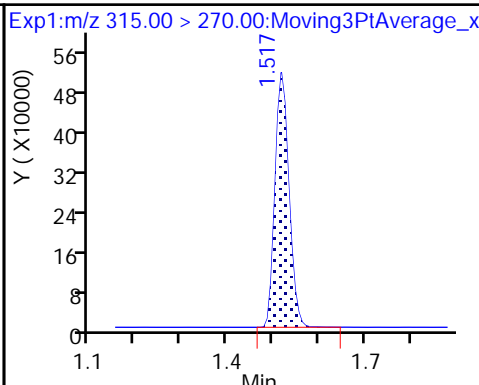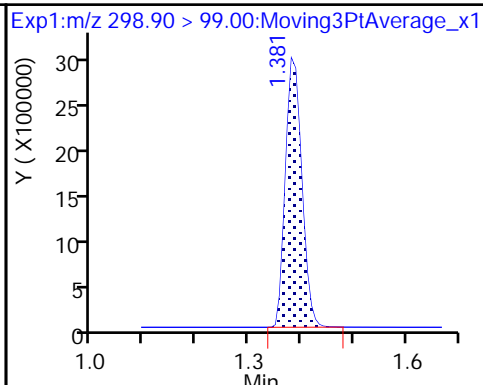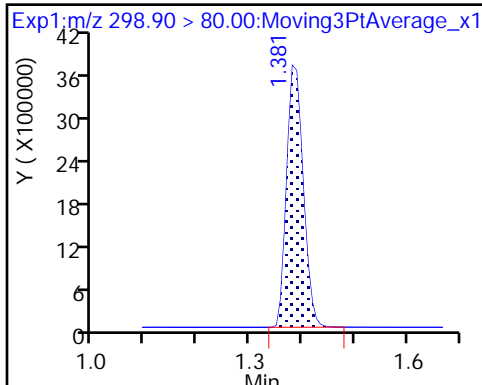

4 Perfluoroheptanoic acid

3 Perfluorohexanesulfonic acid




* 6 13C2-PFOA

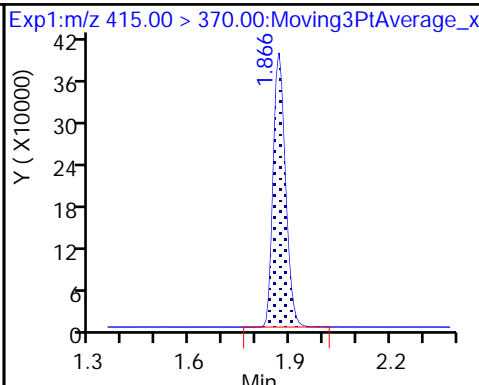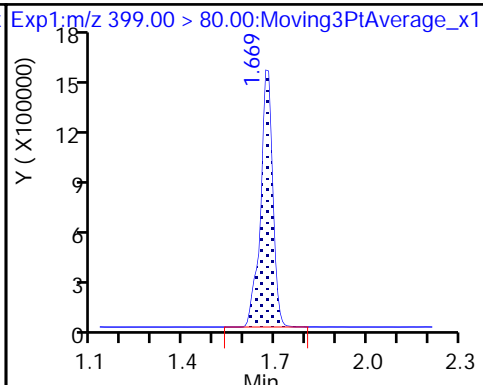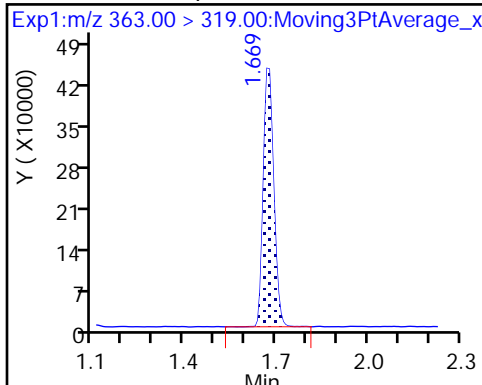

5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)

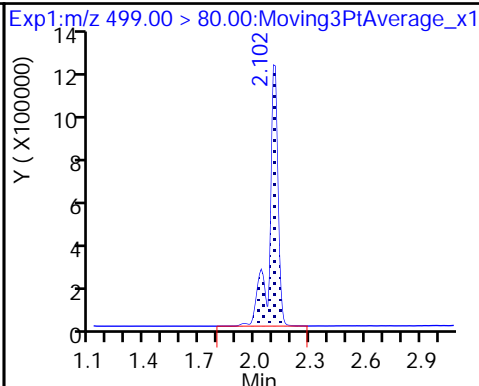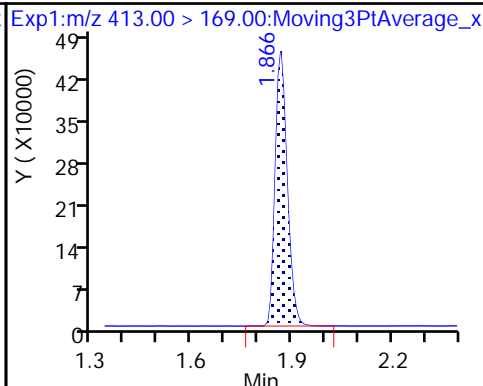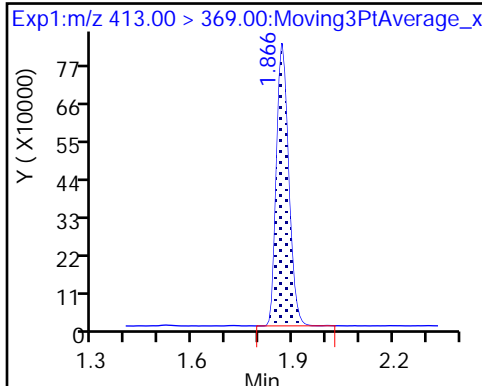


8 Perfluorooctane sulfonic acid

* 7 13C4 PFOS

9 Perfluorononanoic acid

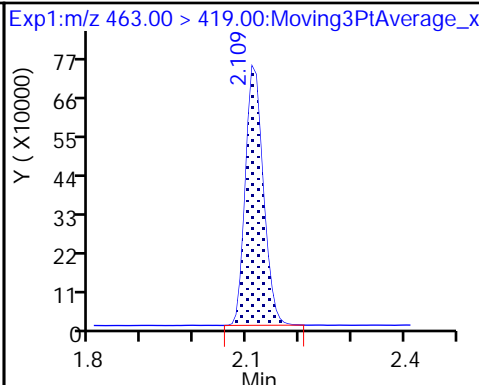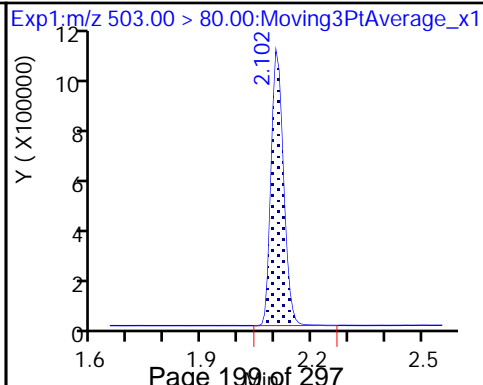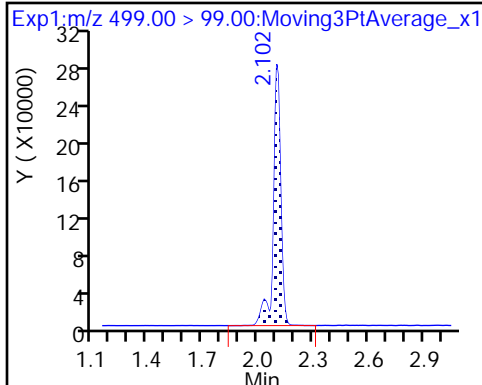

\$ 10 13C2 PFDA

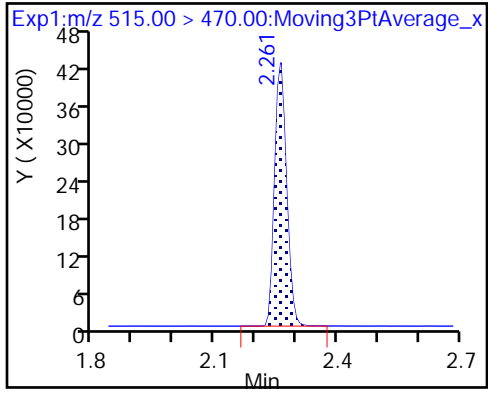

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_007.d
Injection Date: 11-Apr-2018 11:59:48 Instrument ID: A8_N
Lims ID: IC L4
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 4 Worklist Smp#: 6
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.09

Processing Integration Results

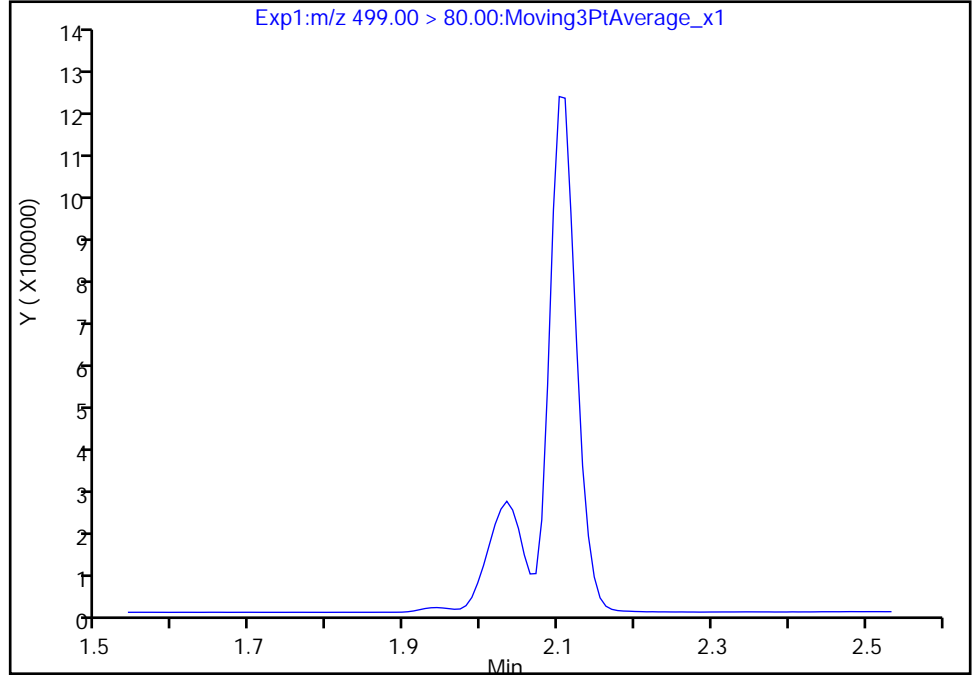

RT: 2.10
Area: 3678059
Amount: 40.551047
Amount Units: ng/ml

Manual Integration Results

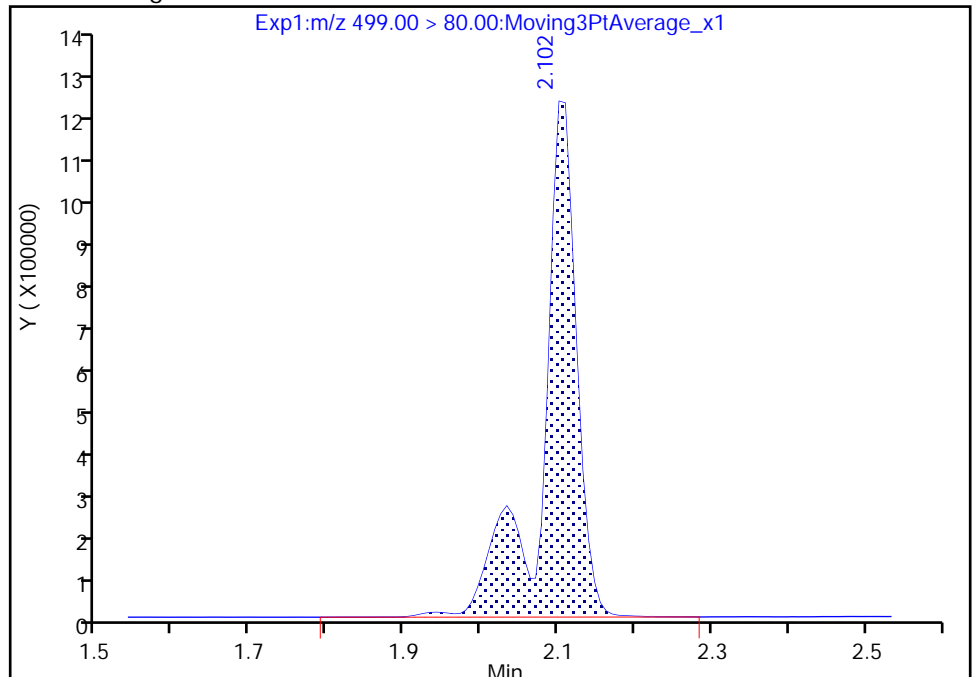

Reviewer: westendorfc, 11-Apr-2018 12:31:45
Audit Action: Assigned Compound ID

Audit Reason: Peak assignment corrected

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_008.d
 Lims ID: IC L5
 Client ID:
 Sample Type: IC Calib Level: 5
 Inject. Date: 11-Apr-2018 12:04:29 ALS Bottle#: 5 Worklist Smp#: 7
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: L5_537
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub9

Method: \\ChromNa\Sacramento\ChromData\A8_N\20180411-56557.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 11-Apr-2018 12:35:32 Calib Date: 11-Apr-2018 12:09:09
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last Ical File: \\ChromNA\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK015

First Level Reviewer: westendorfc Date: 11-Apr-2018 12:31:52

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.381	1.382	-0.001	1.000	10764182	128.5		6999	
298.90 > 99.00	1.381	1.382	-0.001	1.000	8269613		1.30(0.00-0.00)	7836	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.517	1.515	0.002	1.000	985534	9.97		7814	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.669	1.669	0.0	1.000	6082352	46.5		1721	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.669	1.669	0.0	1.000	1450463	14.5		171	
* 6 13C2-PFOA									
415.00 > 370.00	1.866	1.865	0.001		929546	10.0		5174	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.866	1.866	0.0	1.000	3119787	31.6		475	
413.00 > 169.00	1.866	1.866	0.0	1.000	1555272		2.01(0.00-0.00)	1662	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.102	2.094	0.008	1.000	5081660	59.9		1317	a
499.00 > 99.00	2.102	2.094	0.008	1.000	1106855		4.59(0.00-0.00)	2490	a
* 7 13C4 PFOS									
503.00 > 80.00	2.102	2.102	0.0		2283311	28.7		1206	
9 Perfluorononanoic acid									
463.00 > 419.00	2.109	2.109	0.0	1.000	2341235	29.9		363	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.261	2.260	0.001	1.000	791901	10.0		6104	

QC Flag Legend

Review Flags

a - User Assigned ID

Reagents:

LC537-L5_00026

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_008.d

Injection Date: 11-Apr-2018 12:04:29

Instrument ID: A8_N

Lims ID: IC L5

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 5

Worklist Smp#: 7

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA

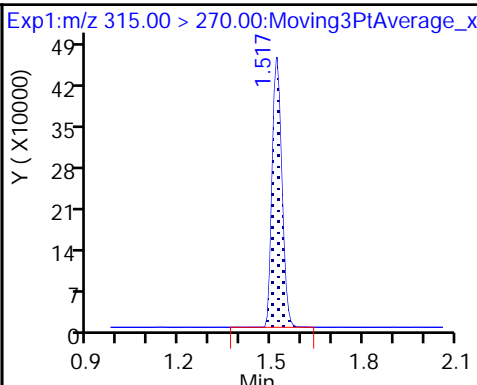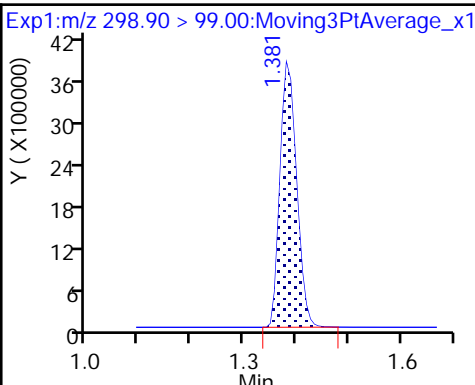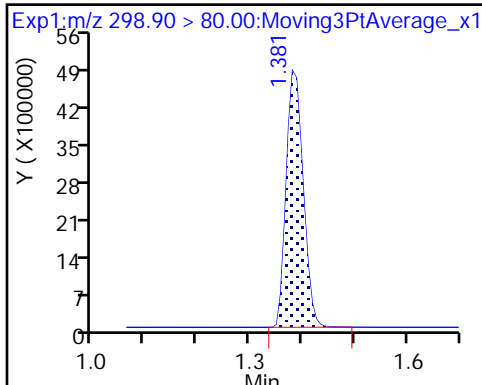

3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA

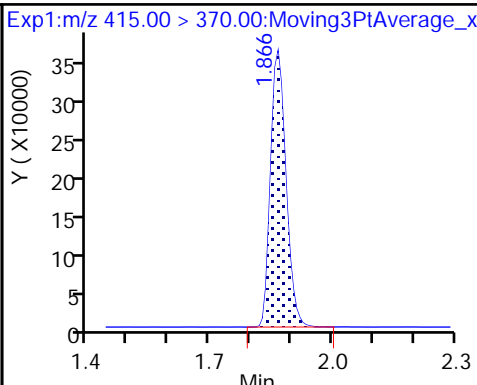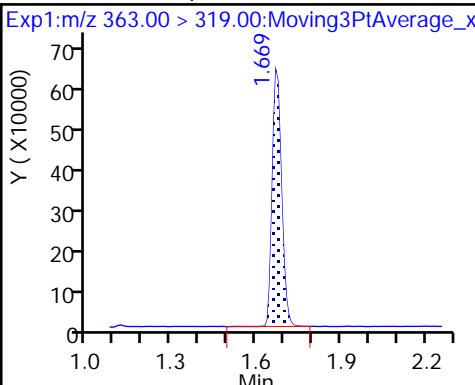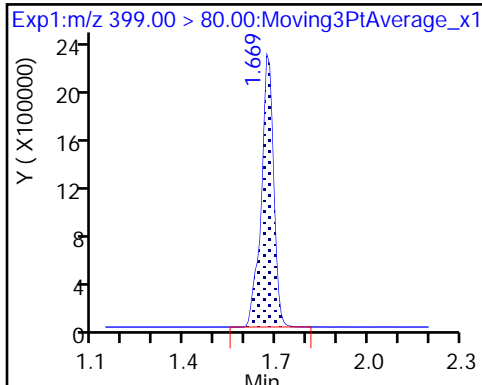

5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)

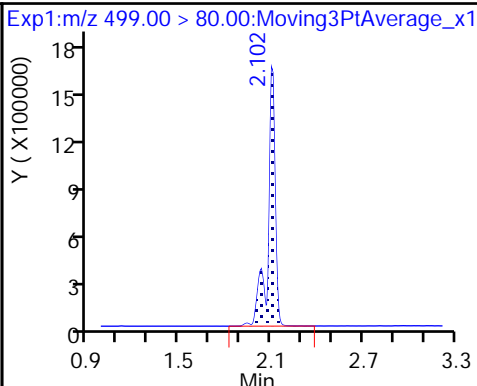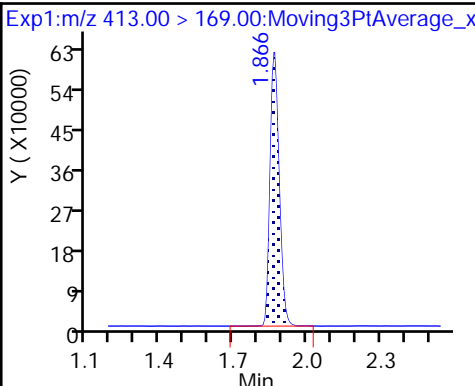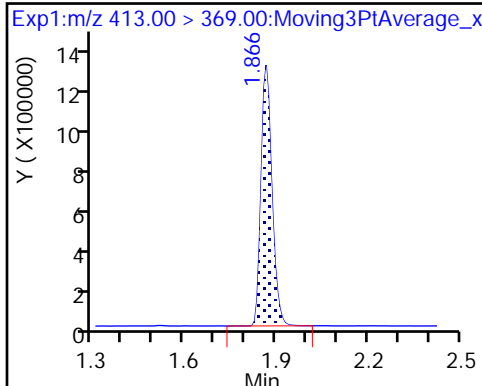


8 Perfluorooctane sulfonic acid

* 7 13C4 PFOS

9 Perfluorononanoic acid

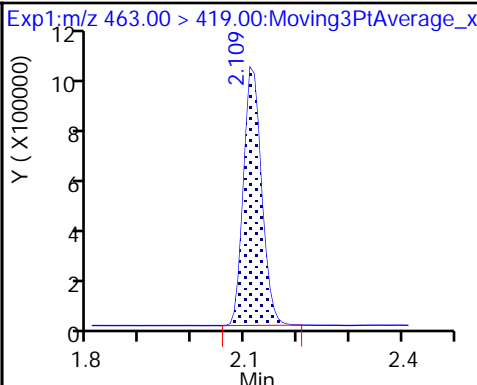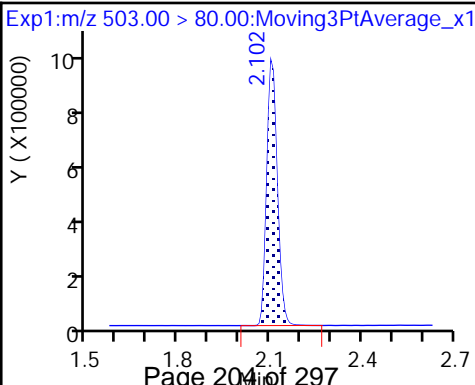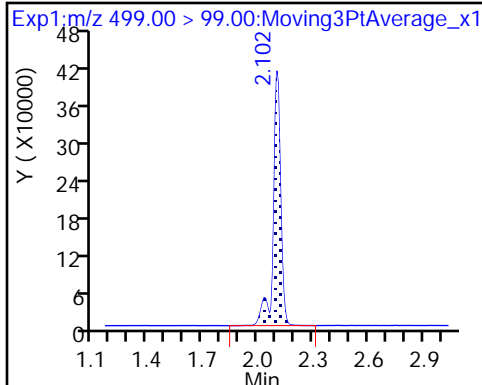

\$ 10 13C2 PFDA

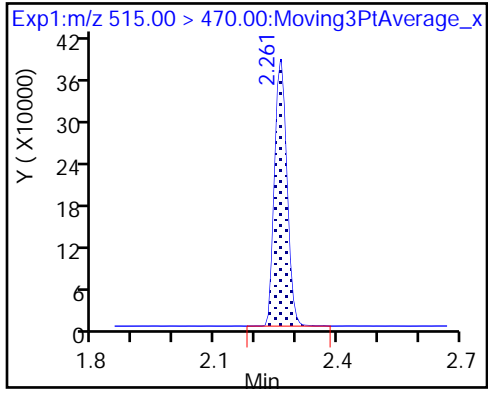

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_008.d
Injection Date: 11-Apr-2018 12:04:29 Instrument ID: A8_N
Lims ID: IC L5
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 5 Worklist Smp#: 7
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.09

Processing Integration Results

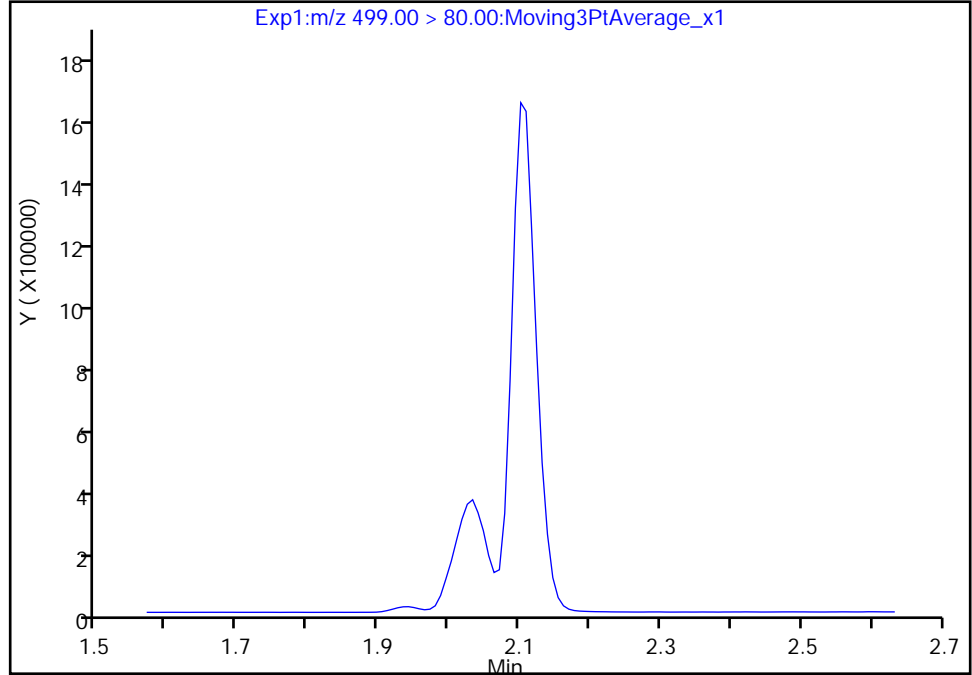

RT: 2.10
Area: 5081660
Amount: 59.873244
Amount Units: ng/ml

Manual Integration Results

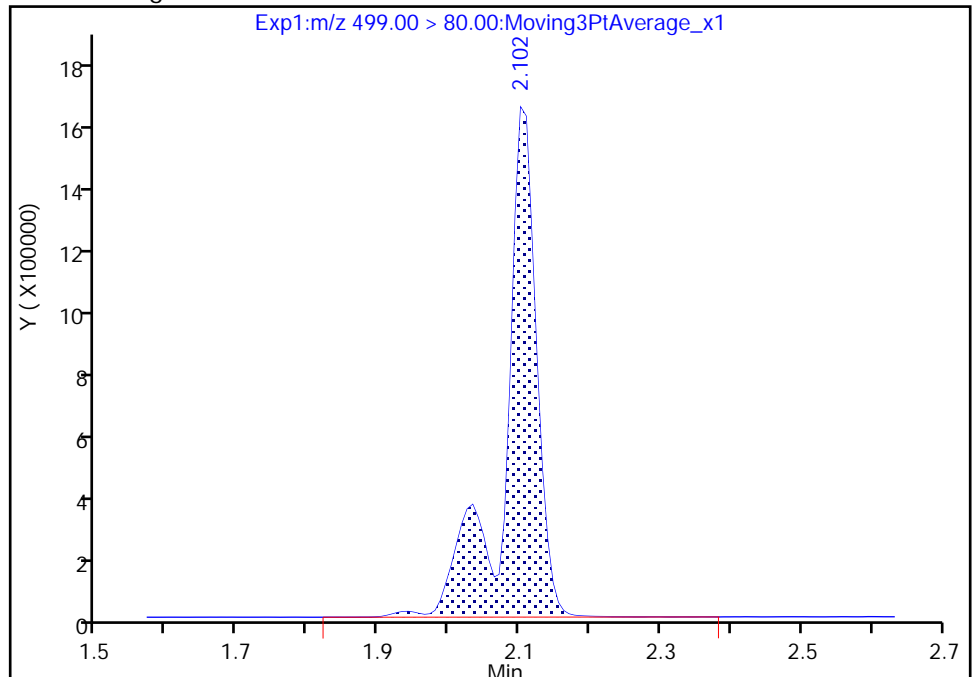

Reviewer: westendorfc, 11-Apr-2018 12:31:49
Audit Action: Assigned Compound ID

Audit Reason: Peak assignment corrected

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_009.d
 Lims ID: IC L6
 Client ID:
 Sample Type: IC Calib Level: 6
 Inject. Date: 11-Apr-2018 12:09:09 ALS Bottle#: 6 Worklist Smp#: 8
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: L6_537
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub9

Method: \\ChromNa\Sacramento\ChromData\A8_N\20180411-56557.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 11-Apr-2018 12:35:33 Calib Date: 11-Apr-2018 12:09:09
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last Ical File: \\ChromNA\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK015

First Level Reviewer: westendorfc Date: 11-Apr-2018 12:31:59

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.381	1.382	-0.001	1.000	13871852	163.3		8258	
298.90 > 99.00	1.381	1.382	-0.001	1.000	10985181		1.26(0.00-0.00)	9440	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.510	1.515	-0.005	1.000	1046576	10.0		9565	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.662	1.669	-0.007	1.000	1996261	18.9		234	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.662	1.669	-0.007	1.000	8226588	62.0		2319	
* 6 13C2-PFOA									
415.00 > 370.00	1.859	1.865	-0.006		982926	10.0		5616	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.859	1.866	-0.007	1.000	4019004	38.5		570	
413.00 > 169.00	1.859	1.866	-0.007	1.000	2217251		1.81(0.00-0.00)	2465	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.094	2.094	0.0	1.000	7016962	81.5		1855	a
499.00 > 99.00	2.094	2.094	0.0	1.000	1468337		4.78(0.00-0.00)	3642	a
* 7 13C4 PFOS									
503.00 > 80.00	2.094	2.102	-0.008		2316327	28.7		1268	
9 Perfluorononanoic acid									
463.00 > 419.00	2.102	2.109	-0.007	1.000	3255374	39.3		485	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.253	2.260	-0.007	1.000	812112	9.71		7134	

QC Flag Legend

Review Flags

a - User Assigned ID

Reagents:

LC537-L6_00022

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_009.d

Injection Date: 11-Apr-2018 12:09:09

Instrument ID: A8_N

Lims ID: IC L6

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 6

Worklist Smp#: 8

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA

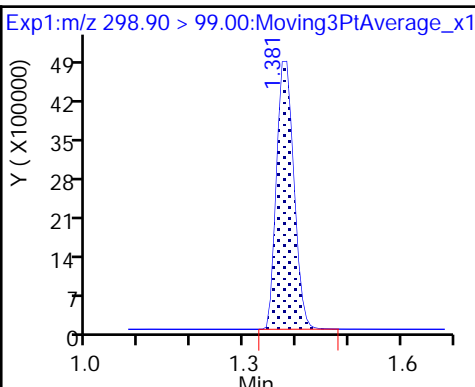

4 Perfluoroheptanoic acid

3 Perfluorohexanesulfonic acid




* 6 13C2-PFOA

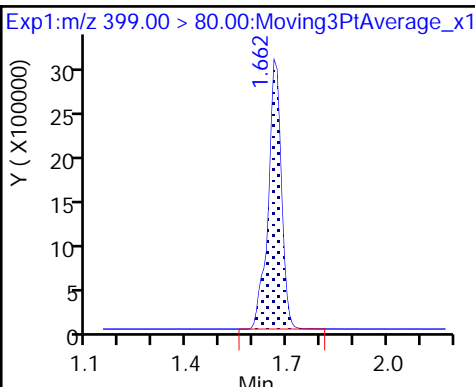

5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)

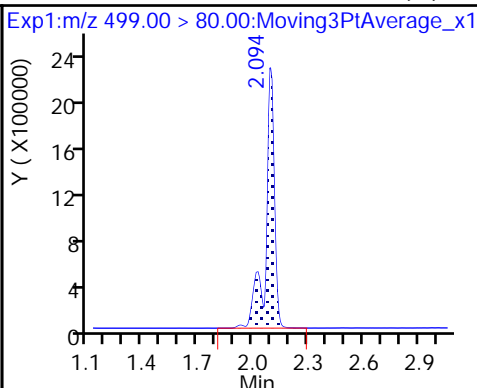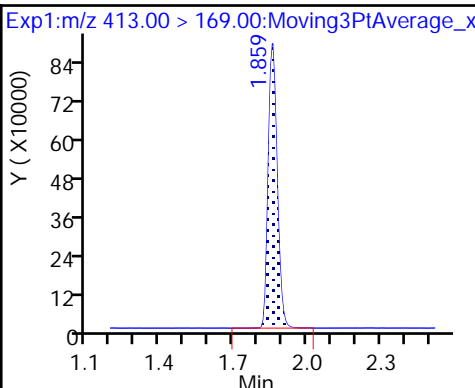


8 Perfluorooctane sulfonic acid

* 7 13C4 PFOS

9 Perfluorononanoic acid

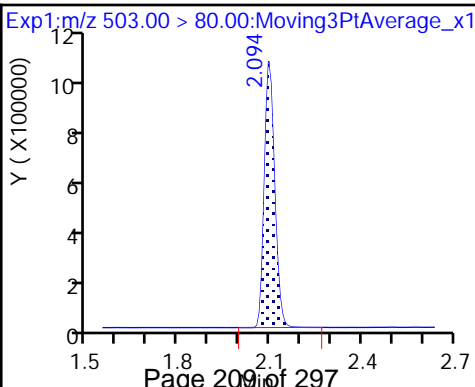

\$ 10 13C2 PFDA

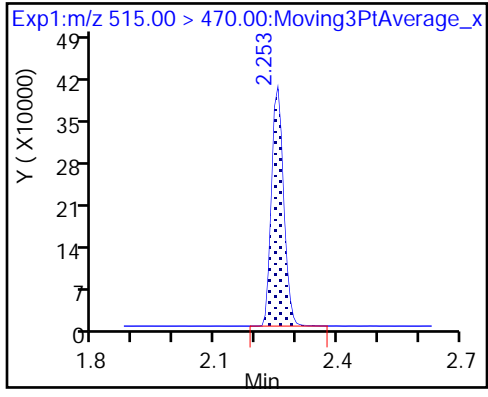

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_009.d
Injection Date: 11-Apr-2018 12:09:09 Instrument ID: A8_N
Lims ID: IC L6
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 6 Worklist Smp#: 8
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.09

Processing Integration Results

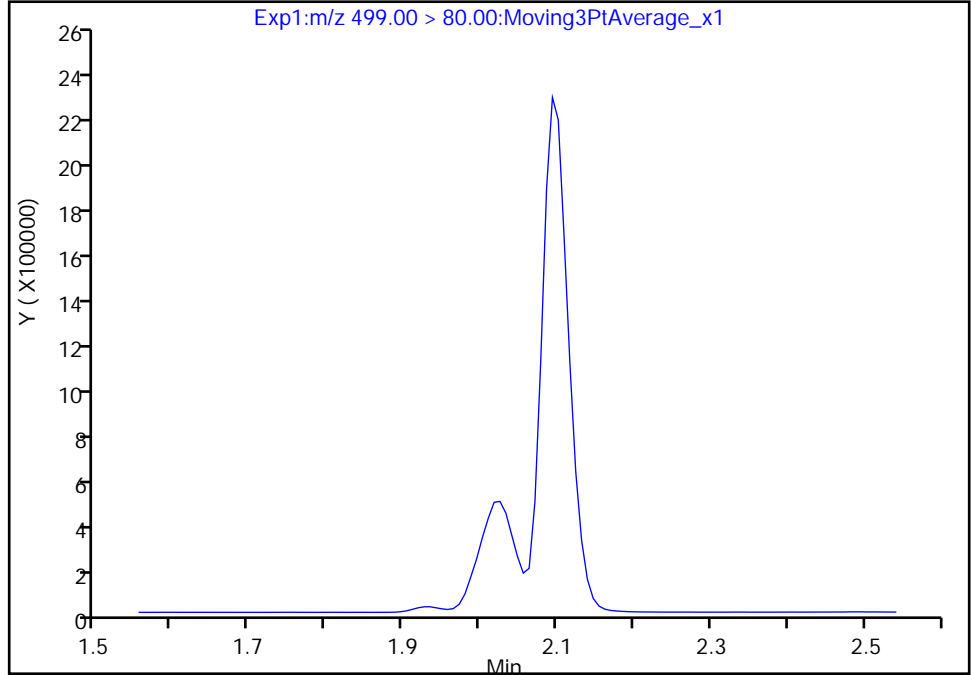

Manual Integration Results

RT: 2.09
Area: 7016962
Amount: 81.496978
Amount Units: ng/ml

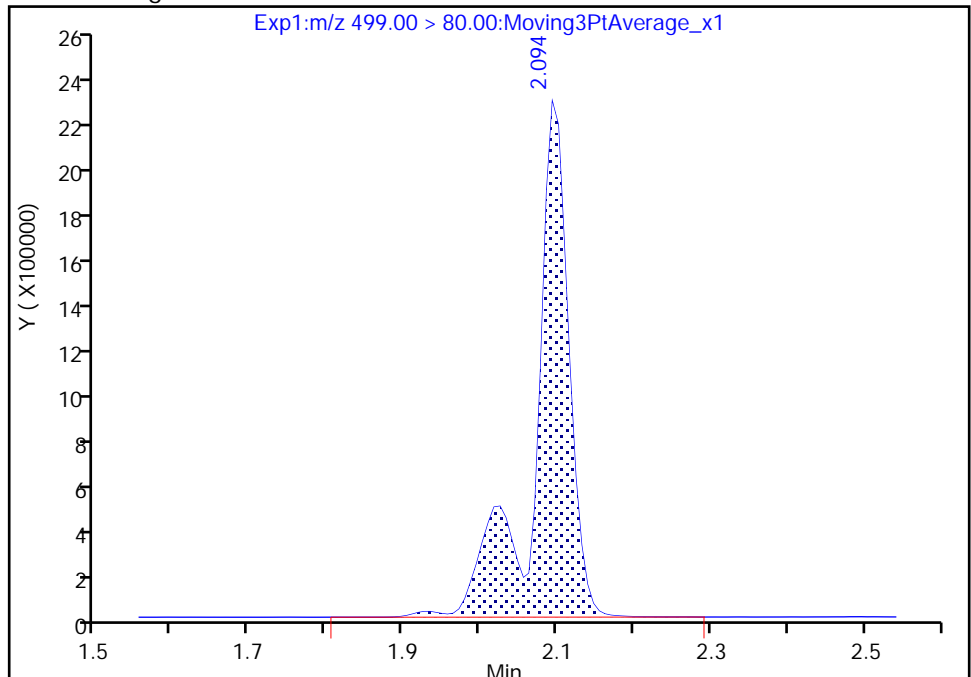

Calibration


/ Perfluorobutanesulfonic acid

Curve Type: Average
 Weighting: Conc_Sq
 Origin: Force
 Dependency: Response
 Calib Mode: ISTD
 Response Base:
 RF Rounding: 0

Curve Coefficients	
Intercept:	0
Slope:	1.052

Error Coefficients	
Standard Error:	8860000
Relative Standard Error:	6.4
Correlation Coefficient:	0.995
Coefficient of Determination (Adjusted):	0.993

ID	Level	Concentration	Rel. Resp.	IS Amount	IS Response	RRF	Used
1	IC 320-217453/3	8.99912	10.27855	28.68	2429483.0	1.142173	Y
2	IC 320-217453/4	20.01376	21.91997	28.68	2220259.0	1.095245	Y
3	IC 320-217453/5	45.03096	48.381679	28.68	2380125.0	1.074409	Y
4	IC 320-217453/6	90.06192	94.147927	28.68	2440107.0	1.045369	Y
5	IC 320-217453/7	135.09288	135.205734	28.68	2283311.0	1.000835	Y
6	IC 320-217453/8	180.12384	171.756715	28.68	2316327.0	0.953548	Y

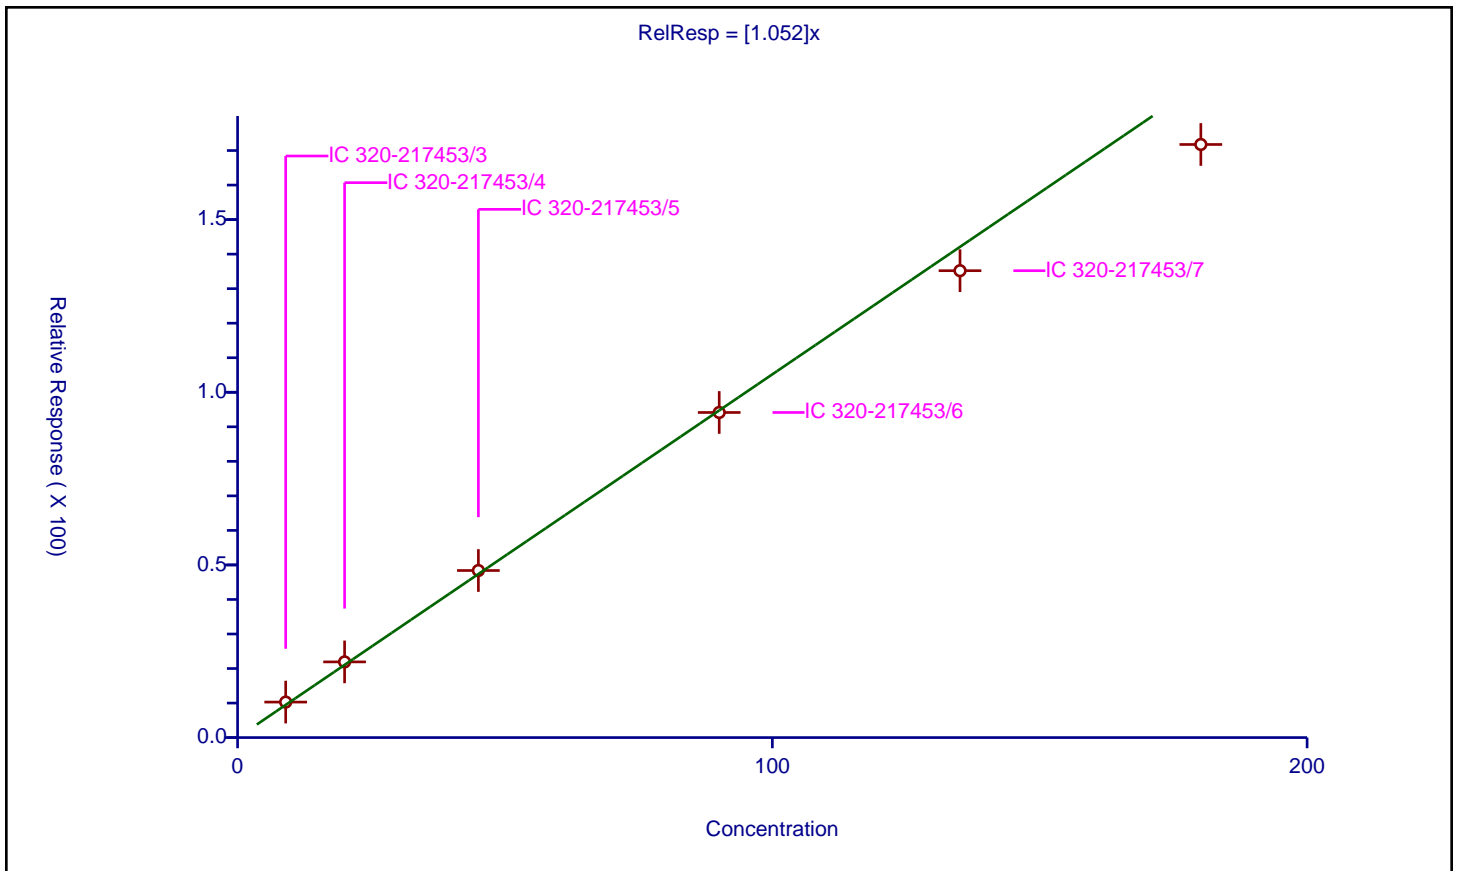

Calibration


/ 13C2 PFHxA

Curve Type: Average
Weighting: Conc_Sq
Origin: Force
Dependency: Response
Calib Mode: ISTD
Response Base:
RF Rounding: 0

Curve Coefficients	
Intercept:	0
Slope:	1.063

Error Coefficients	
Standard Error:	1130000
Relative Standard Error:	1.4
Correlation Coefficient:	NA
Coefficient of Determination (Adjusted):	0

ID	Level	Concentration	Rel. Resp.	IS Amount	IS Response	RRF	Used
1	IC 320-217453/3	10.0	10.447022	10.0	1044020.0	1.044702	Y
2	IC 320-217453/4	10.0	10.531795	10.0	921915.0	1.05318	Y
3	IC 320-217453/5	10.0	10.874839	10.0	945031.0	1.087484	Y
4	IC 320-217453/6	10.0	10.686721	10.0	996809.0	1.068672	Y
5	IC 320-217453/7	10.0	10.602316	10.0	929546.0	1.060232	Y
6	IC 320-217453/8	10.0	10.647556	10.0	982926.0	1.064756	Y

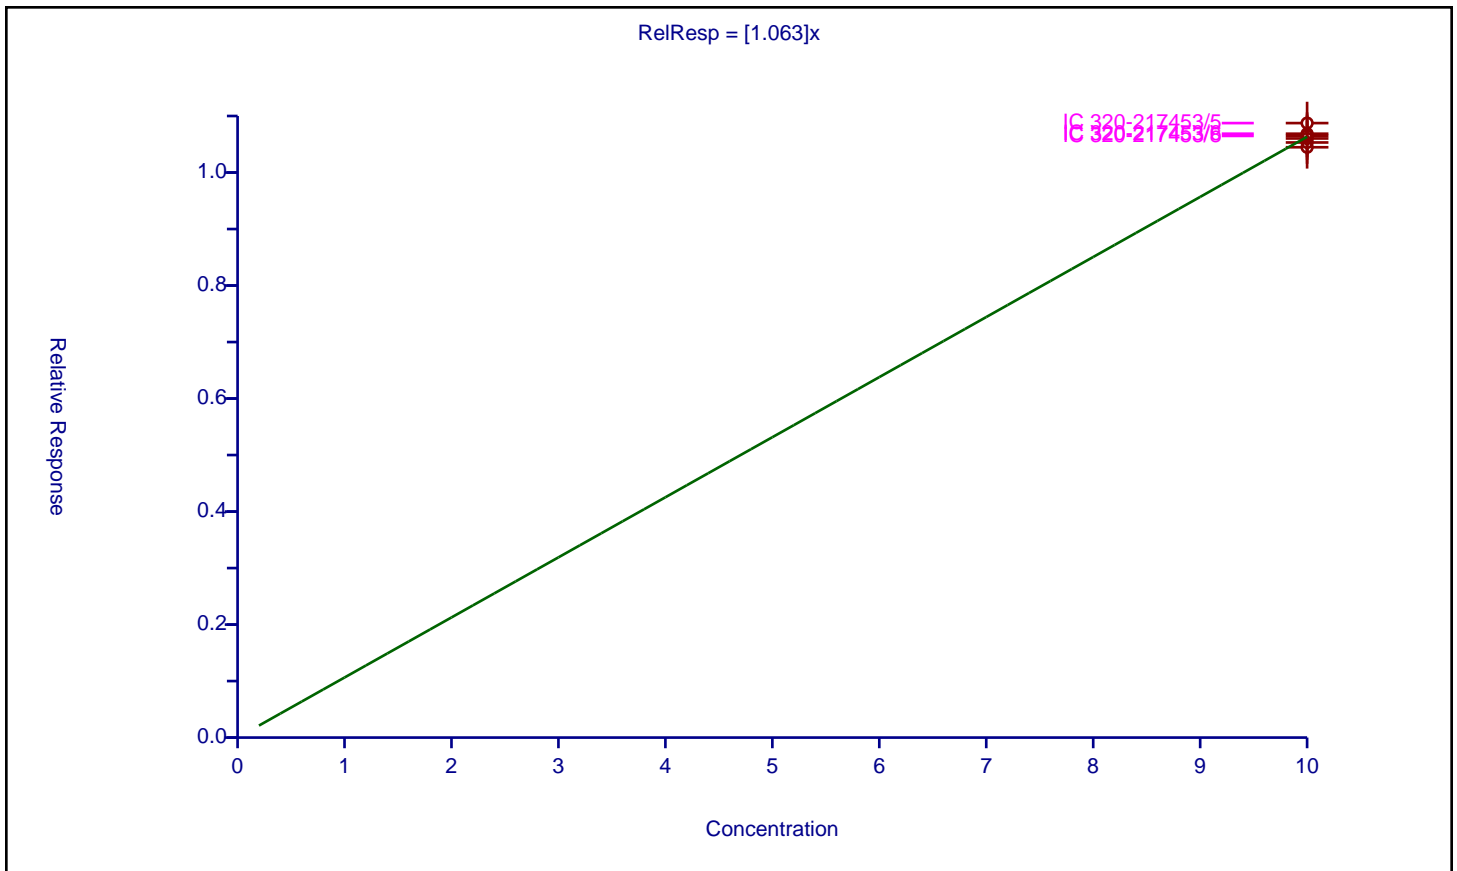

Calibration


/ Perfluorohexanesulfonic acid

Curve Type: Average
 Weighting: Conc_Sq
 Origin: Force
 Dependency: Response
 Calib Mode: ISTD
 Response Base:
 RF Rounding: 0

Curve Coefficients	
Intercept:	0
Slope:	1.642

Error Coefficients	
Standard Error:	5050000
Relative Standard Error:	2.3
Correlation Coefficient:	0.999
Coefficient of Determination (Adjusted):	0.999

ID	Level	Concentration	Rel. Resp.	IS Amount	IS Response	RRF	Used
1	IC 320-217453/3	3.003	4.942037	28.68	2429483.0	1.6457	Y
2	IC 320-217453/4	6.721867	10.746809	28.68	2220259.0	1.598783	Y
3	IC 320-217453/5	15.1242	24.244534	28.68	2380125.0	1.603029	Y
4	IC 320-217453/6	30.2484	49.557654	28.68	2440107.0	1.638356	Y
5	IC 320-217453/7	45.3726	76.39864	28.68	2283311.0	1.683806	Y
6	IC 320-217453/8	60.4968	101.85891	28.68	2316327.0	1.683707	Y

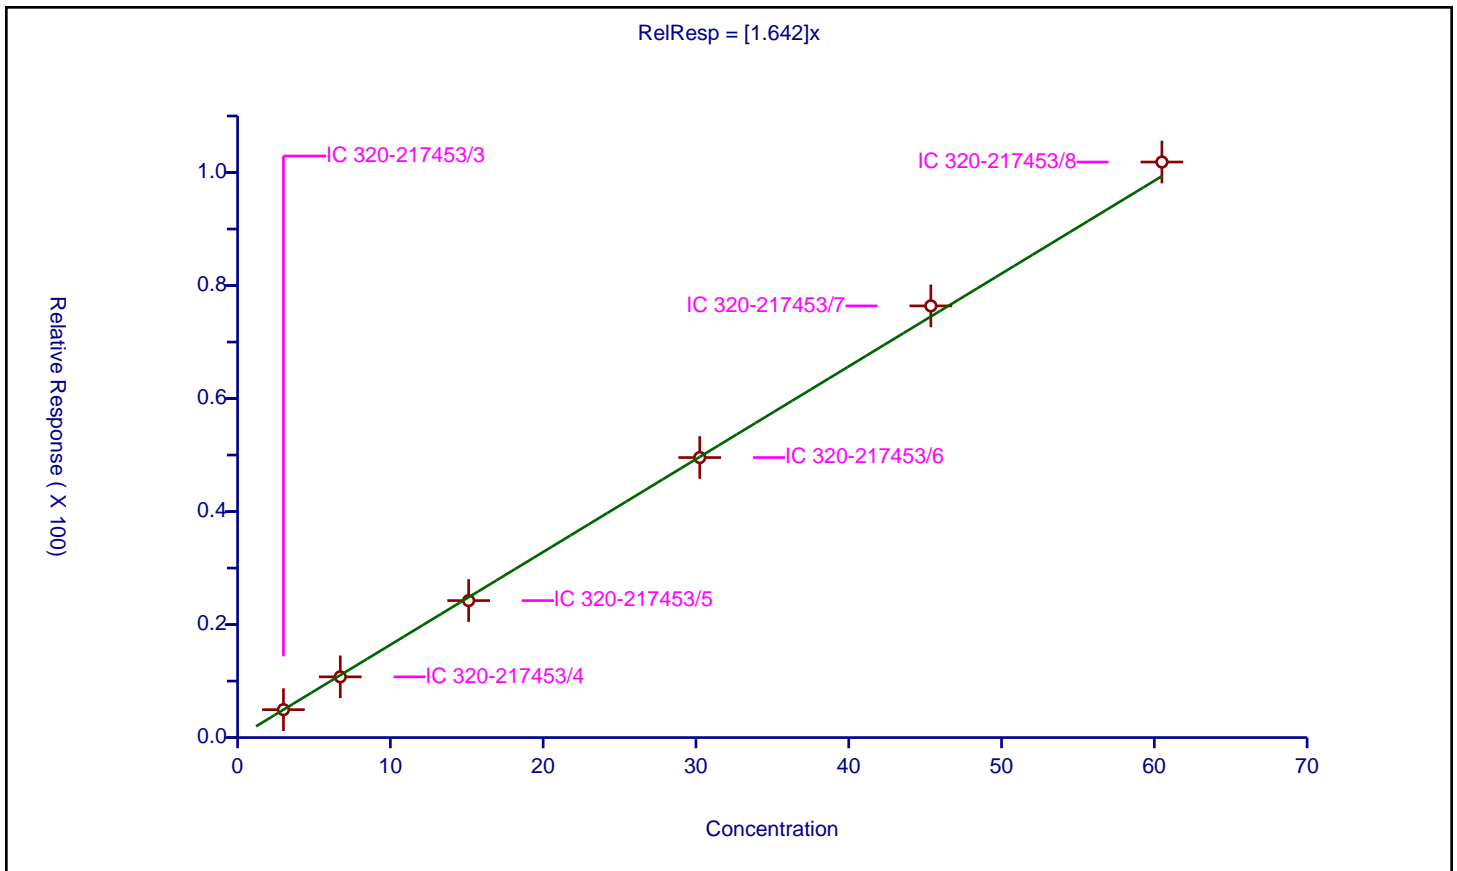

Calibration


/ Perfluoroheptanoic acid

Curve Type: Average
 Weighting: Conc_Sq
 Origin: Force
 Dependency: Response
 Calib Mode: ISTD
 Response Base:
 RF Rounding: 0

Curve Coefficients	
Intercept:	0
Slope:	1.074

Error Coefficients	
Standard Error:	1220000
Relative Standard Error:	1.7
Correlation Coefficient:	0.998
Coefficient of Determination (Adjusted):	1.000

ID	Level	Concentration	Rel. Resp.	IS Amount	IS Response	RRF	Used
1	IC 320-217453/3	0.96	1.041561	10.0	1044020.0	1.084959	Y
2	IC 320-217453/4	2.16	2.373972	10.0	921915.0	1.099061	Y
3	IC 320-217453/5	4.86	5.175227	10.0	945031.0	1.064862	Y
4	IC 320-217453/6	9.72	10.480965	10.0	996809.0	1.078289	Y
5	IC 320-217453/7	14.58	15.603994	10.0	929546.0	1.070233	Y
6	IC 320-217453/8	19.44	20.309372	10.0	982926.0	1.044721	Y

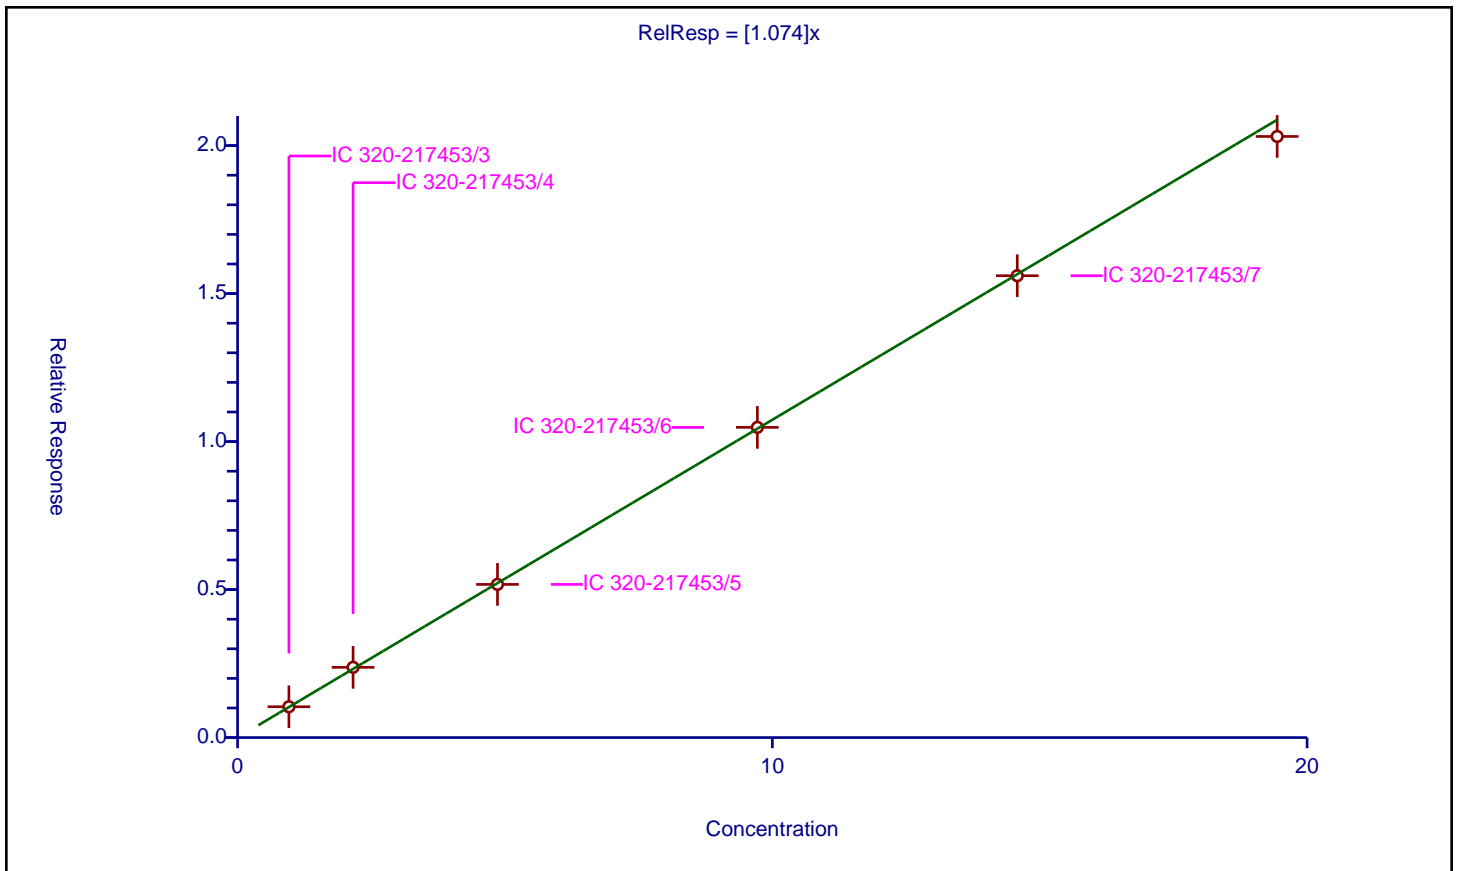

Calibration


/ Perfluorooctanoic acid

Curve Type: Average
 Weighting: Conc_Sq
 Origin: Force
 Dependency: Response
 Calib Mode: ISTD
 Response Base:
 RF Rounding: 0

Curve Coefficients	
Intercept:	0
Slope:	1.062

Error Coefficients	
Standard Error:	2510000
Relative Standard Error:	3.5
Correlation Coefficient:	0.999
Coefficient of Determination (Adjusted):	0.998

ID	Level	Concentration	Rel. Resp.	IS Amount	IS Response	RRF	Used
1	IC 320-217453/3	1.98	2.098619	10.0	1044020.0	1.059908	Y
2	IC 320-217453/4	4.4	4.530049	10.0	921915.0	1.029557	Y
3	IC 320-217453/5	9.9	10.595589	10.0	945031.0	1.070262	Y
4	IC 320-217453/6	19.8	20.822123	10.0	996809.0	1.051622	Y
5	IC 320-217453/7	29.7	33.562481	10.0	929546.0	1.13005	Y
6	IC 320-217453/8	39.6	40.888165	10.0	982926.0	1.032529	Y

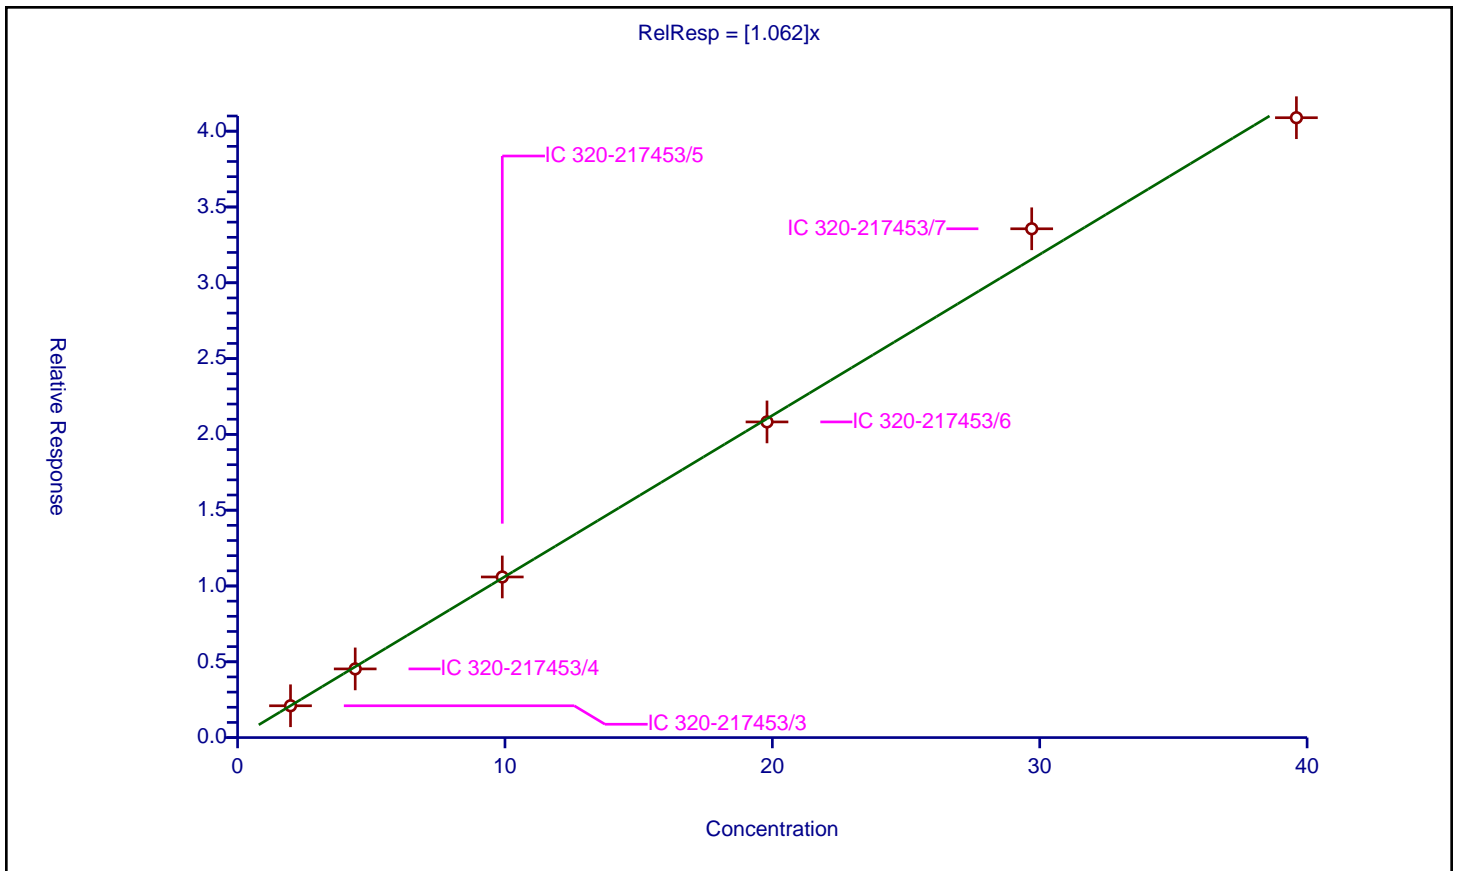

Calibration


/ Perfluorooctane sulfonic acid

Curve Type: Average
 Weighting: Conc_Sq
 Origin: Force
 Dependency: Response
 Calib Mode: ISTD
 Response Base:
 RF Rounding: 0

Curve Coefficients	
Intercept:	0
Slope:	1.066

Error Coefficients	
Standard Error:	4290000
Relative Standard Error:	2.6
Correlation Coefficient:	0.998
Coefficient of Determination (Adjusted):	0.999

ID	Level	Concentration	Rel. Resp.	IS Amount	IS Response	RRF	Used
1	IC 320-217453/3	3.95328	4.124117	28.68	2429483.0	1.043214	Y
2	IC 320-217453/4	8.785067	9.240832	28.68	2220259.0	1.05188	Y
3	IC 320-217453/5	19.7664	20.41005	28.68	2380125.0	1.032563	Y
4	IC 320-217453/6	39.5328	43.230372	28.68	2440107.0	1.093532	Y
5	IC 320-217453/7	59.2992	63.829241	28.68	2283311.0	1.076393	Y
6	IC 320-217453/8	79.0656	86.881718	28.68	2316327.0	1.098856	Y

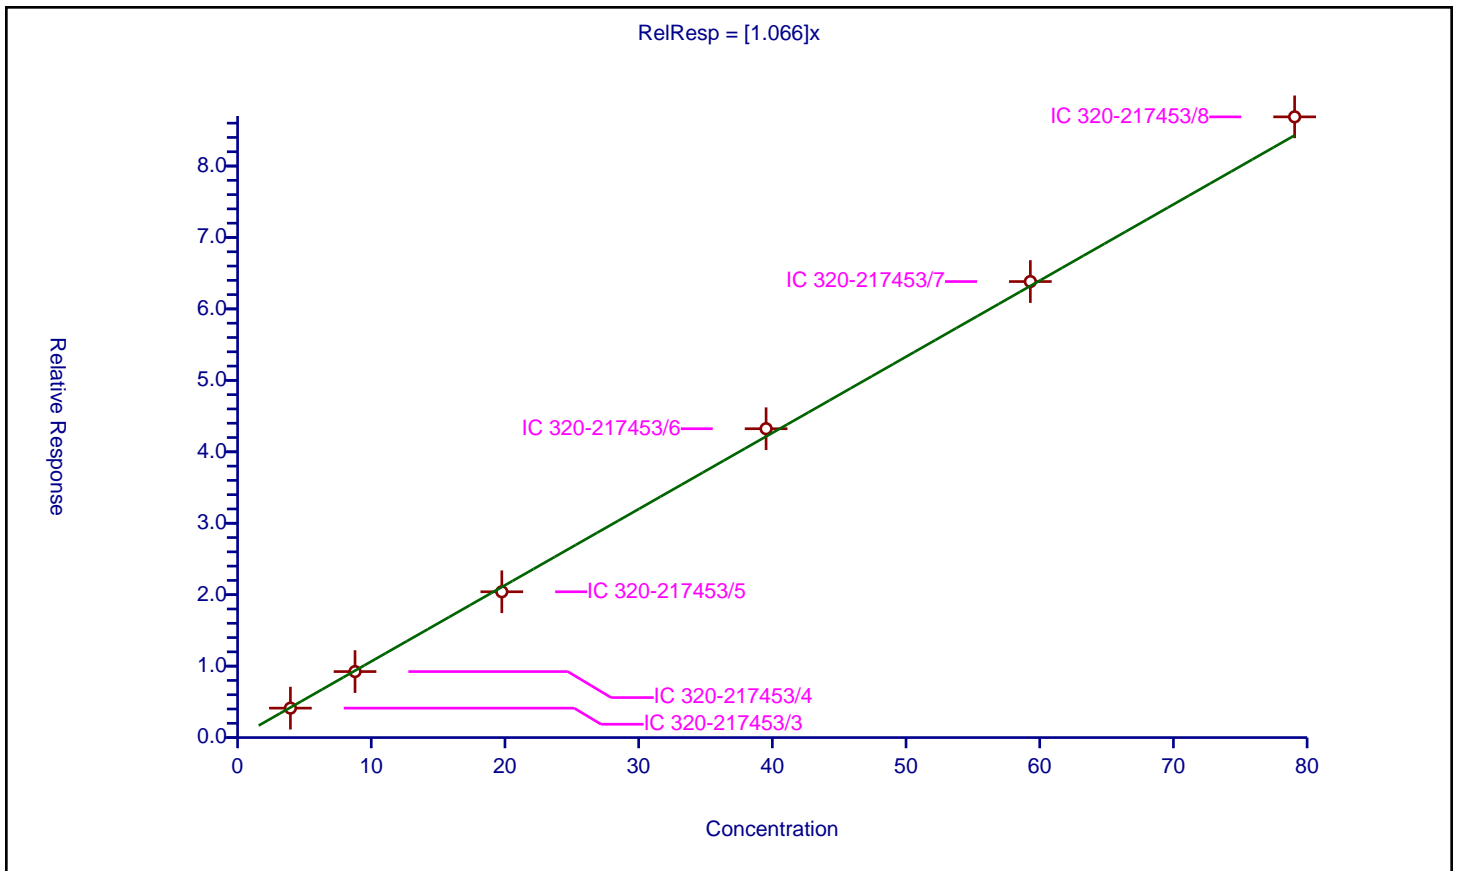

Calibration


/ Perfluorononanoic acid

Curve Type: Average
 Weighting: Conc_Sq
 Origin: Force
 Dependency: Response
 Calib Mode: ISTD
 Response Base:
 RF Rounding: 0

Curve Coefficients	
Intercept:	0
Slope:	0.8424

Error Coefficients	
Standard Error:	1990000
Relative Standard Error:	2.8
Correlation Coefficient:	0.997
Coefficient of Determination (Adjusted):	0.999

ID	Level	Concentration	Rel. Resp.	IS Amount	IS Response	RRF	Used
1	IC 320-217453/3	1.98	1.635697	10.0	1044020.0	0.826109	Y
2	IC 320-217453/4	4.4	3.578464	10.0	921915.0	0.813287	Y
3	IC 320-217453/5	9.9	8.402645	10.0	945031.0	0.848752	Y
4	IC 320-217453/6	19.8	17.459935	10.0	996809.0	0.881815	Y
5	IC 320-217453/7	29.7	25.186865	10.0	929546.0	0.848043	Y
6	IC 320-217453/8	39.6	33.119218	10.0	982926.0	0.836344	Y

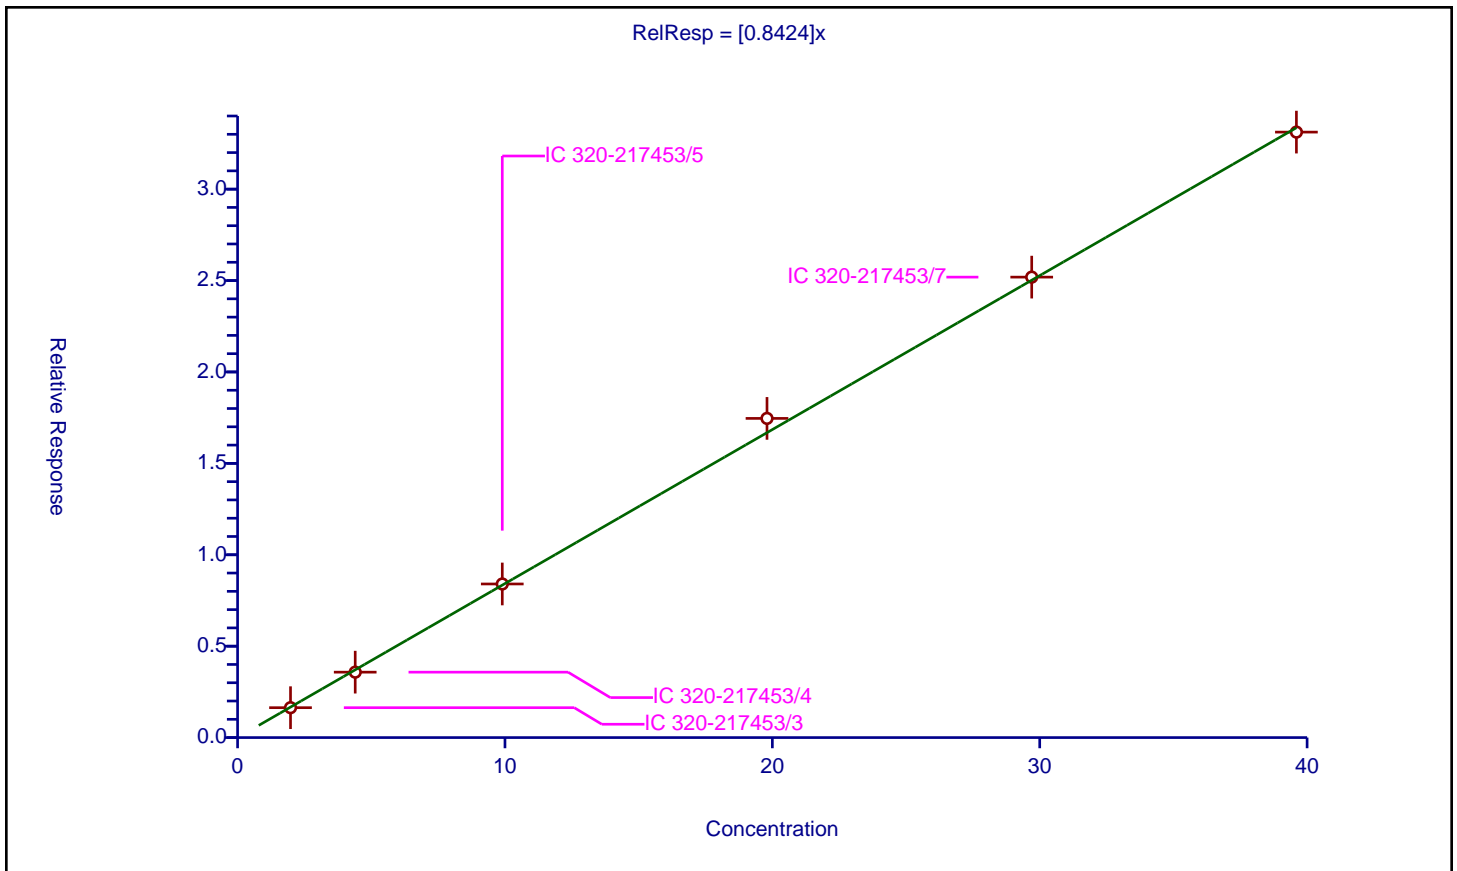

Calibration


/ 13C2 PFDA

Curve Type: Average
 Weighting: Conc_Sq
 Origin: Force
 Dependency: Response
 Calib Mode: ISTD
 Response Base:
 RF Rounding: 0

Curve Coefficients	
Intercept:	0
Slope:	0.8505

Error Coefficients	
Standard Error:	904000
Relative Standard Error:	1.7
Correlation Coefficient:	NA
Coefficient of Determination (Adjusted):	0

ID	Level	Concentration	Rel. Resp.	IS Amount	IS Response	RRF	Used
1	IC 320-217453/3	10.0	8.512691	10.0	1044020.0	0.851269	Y
2	IC 320-217453/4	10.0	8.714491	10.0	921915.0	0.871449	Y
3	IC 320-217453/5	10.0	8.53263	10.0	945031.0	0.853263	Y
4	IC 320-217453/6	10.0	8.486982	10.0	996809.0	0.848698	Y
5	IC 320-217453/7	10.0	8.519223	10.0	929546.0	0.851922	Y
6	IC 320-217453/8	10.0	8.262189	10.0	982926.0	0.826219	Y

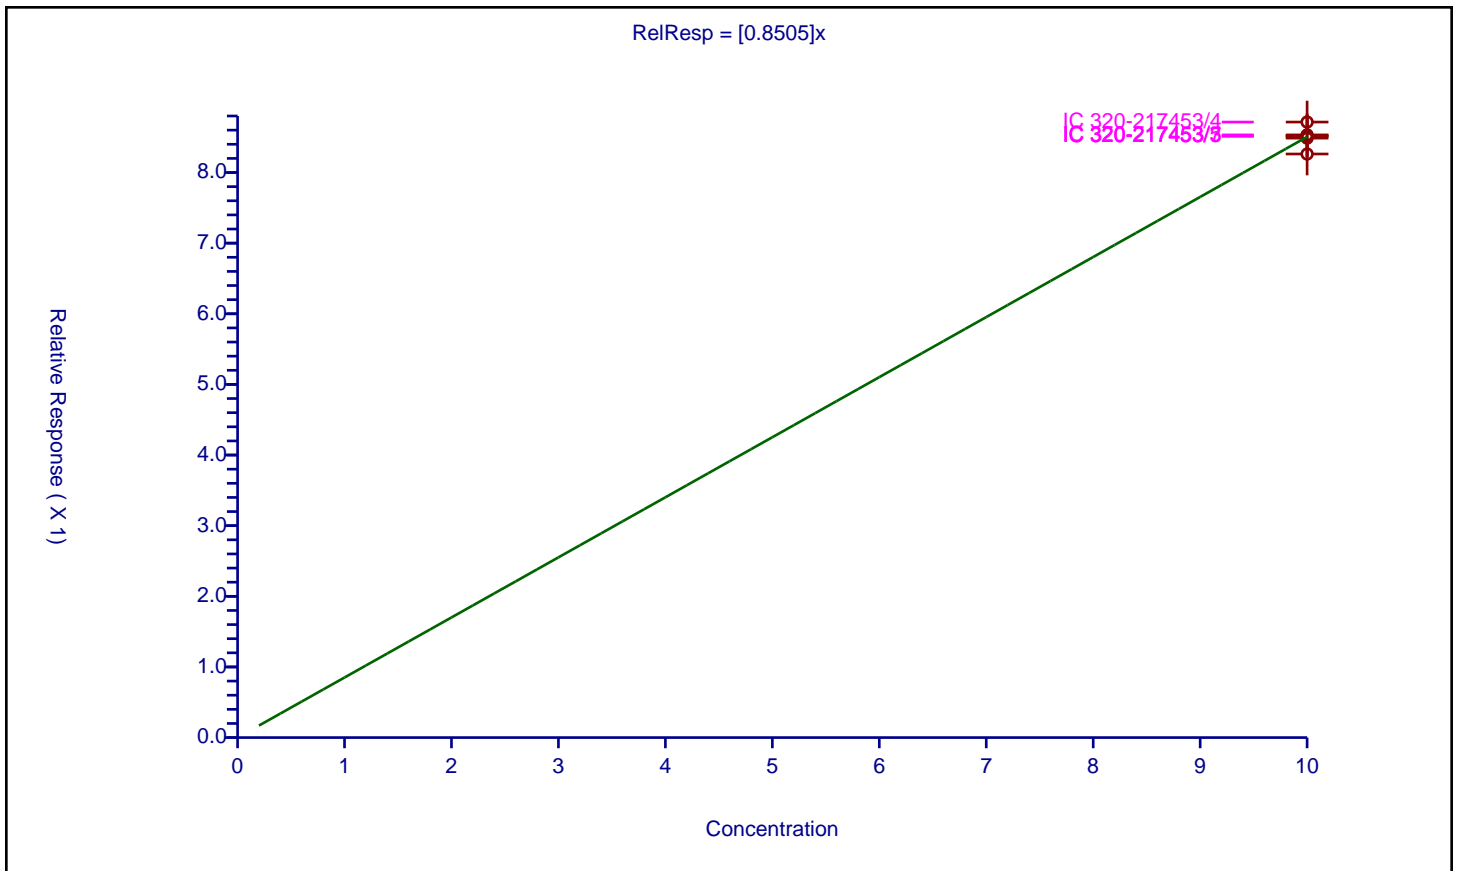

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Lab Sample ID: CCVL 320-217453/10 Calibration Date: 04/11/2018 12:18
 Instrument ID: A8_N Calib Start Date: 04/11/2018 11:45
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 04/11/2018 12:09
 Lab File ID: 2018.04.11_537ICALB_011.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	Ave	1.052	1.078		20.5	20.0	2.5	50.0
Perfluoroheptanoic acid (PFHpA)	Ave	1.074	1.079		2.17	2.16	0.5	50.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.642	1.583		6.48	6.72	-3.6	50.0
Perfluorooctanoic acid (PFOA)	Ave	1.062	1.067		4.42	4.40	0.4	50.0
Perfluorooctanesulfonic acid (PFOS)	Ave	1.066	1.026		8.45	8.79	-3.8	50.0
Perfluorononanoic acid (PFNA)	Ave	0.8424	0.8056		4.21	4.40	-4.4	50.0
13C2 PFHxA	Ave	1.063	1.036		9.74	10.0	-2.6	30.0
13C2 PFDA	Ave	0.8505	0.8798		10.3	10.0	3.4	30.0

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_011.d
 Lims ID: CCVL
 Client ID:
 Sample Type: CCVL
 Inject. Date: 11-Apr-2018 12:18:29 ALS Bottle#: 2 Worklist Smp#: 10
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: CCV L2
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub9
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180411-56557.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 11-Apr-2018 12:35:34 Calib Date: 11-Apr-2018 12:09:09
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last Ical File: \\ChromNA\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK015

First Level Reviewer: westendorfc Date: 11-Apr-2018 12:32:05

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.381	1.382	-0.001	1.000	1796973	20.5		1419	
298.90 > 99.00	1.381	1.382	-0.001	1.000	1315166		1.37(0.00-0.00)	1507	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.517	1.515	0.002	1.000	999202	9.74		8081	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.669	1.669	0.0	1.000	886015	6.48		254	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.669	1.669	0.0	1.000	224797	2.17		28.4	
* 6 13C2-PFOA									
415.00 > 370.00	1.866	1.865	0.001		964533	10.0		6486	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.866	1.866	0.0	1.000	452711	4.42		66.1	
413.00 > 169.00	1.859	1.866	-0.007	0.996	238029		1.90(0.00-0.00)	253	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.102	2.094	0.008	1.000	750245	8.45		211	a
499.00 > 99.00	2.102	2.094	0.008	1.000	160618		4.67(0.00-0.00)	405	a
* 7 13C4 PFOS									
503.00 > 80.00	2.102	2.102	0.0		2387973	28.7		1256	
9 Perfluorononanoic acid									
463.00 > 419.00	2.109	2.109	0.0	1.000	341890	4.21		51.1	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.261	2.260	0.001	1.000	848574	10.3		7810	

QC Flag Legend

Review Flags

a - User Assigned ID

Reagents:

LC537-L2_00022

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_011.d

Injection Date: 11-Apr-2018 12:18:29

Instrument ID: A8_N

Lims ID: CCVL

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 2

Worklist Smp#: 10

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)

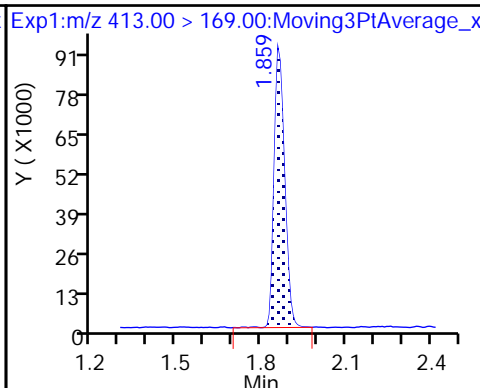


8 Perfluorooctane sulfonic acid

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA

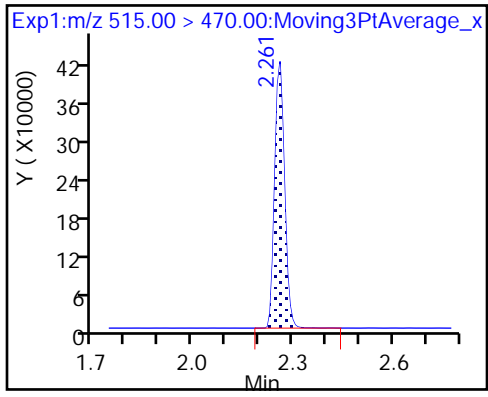

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_011.d
Injection Date: 11-Apr-2018 12:18:29 Instrument ID: A8_N
Lims ID: CCVL
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 2 Worklist Smp#: 10
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.09

Processing Integration Results

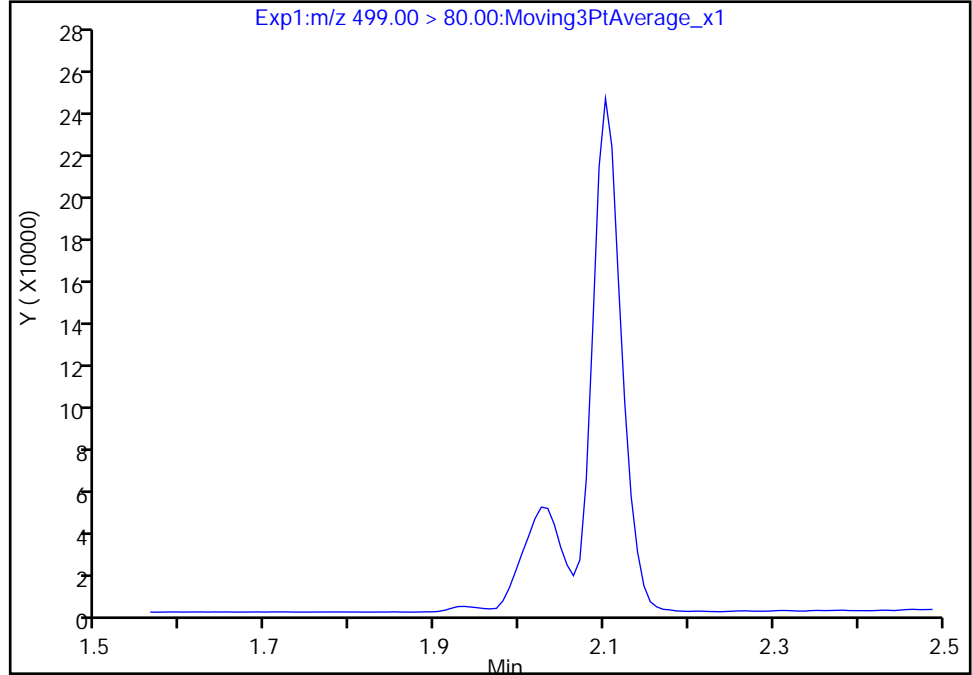

Manual Integration Results

RT: 2.10
Area: 750245
Amount: 8.452126
Amount Units: ng/ml

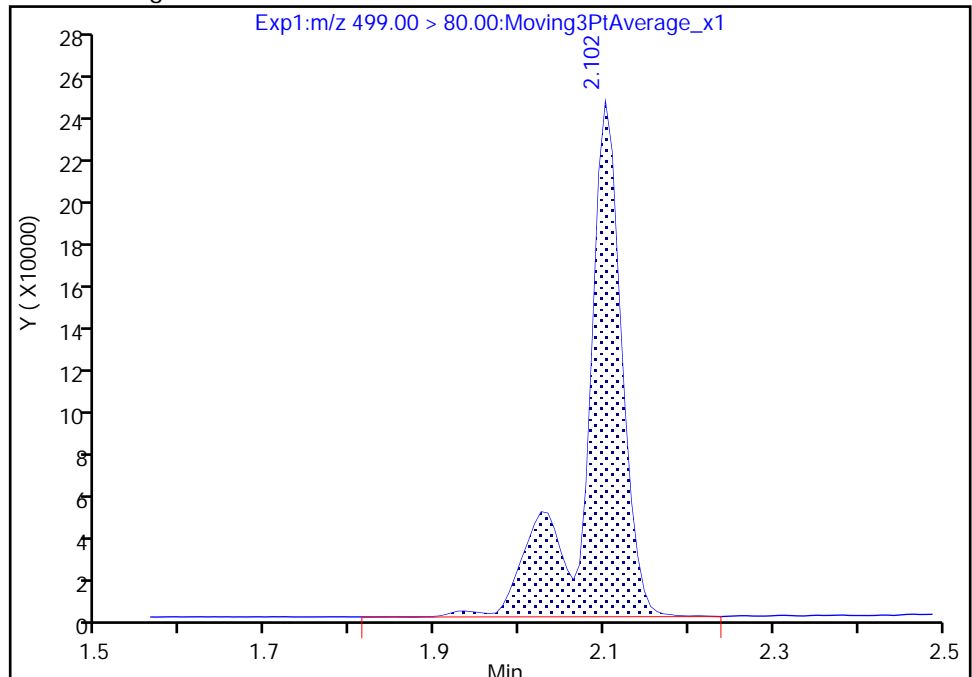

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Lab Sample ID: ICV 320-217453/12 Calibration Date: 04/11/2018 12:27
 Instrument ID: A8_N Calib Start Date: 04/11/2018 11:45
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 04/11/2018 12:09
 Lab File ID: 2018.04.11_537ICALB_013.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	Ave	1.052	0.9079		86.4	100	-13.7	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	1.074	0.9453		8.80	10.0	-12.0	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.642	1.546		19.0	20.2	-5.8	30.0
Perfluorooctanoic acid (PFOA)	Ave	1.062	0.8947		17.0	20.2	-15.8	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	1.066	0.9451		17.9	20.2	-11.3	30.0
Perfluorononanoic acid (PFNA)	Ave	0.8424	0.7643		18.3	20.2	-9.3	30.0
13C2 PFHxA	Ave	1.063	0.9887		9.30	10.0	-7.0	30.0
13C2 PFDA	Ave	0.8505	0.7817		9.19	10.0	-8.1	30.0

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_013.d
 Lims ID: ICV
 Client ID:
 Sample Type: ICV
 Inject. Date: 11-Apr-2018 12:27:50 ALS Bottle#: 7 Worklist Smp#: 12
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: ICV
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist:

Method: \\ChromNa\Sacramento\ChromData\A8_N\20180411-56557.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 11-Apr-2018 12:35:36 Calib Date: 11-Apr-2018 12:09:09
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last Ical File: \\ChromNA\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK015

First Level Reviewer: westendorfc Date: 11-Apr-2018 12:35:17

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.381	1.382	-0.001	1.000	8588615	86.4		6016	
298.90 > 99.00	1.381	1.382	-0.001	1.000	6638954		1.29(0.00-0.00)	7031	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.510	1.515	-0.005	1.000	1110636	9.30		10046	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.669	1.669	0.0	1.000	2946450	19.0		915	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.669	1.669	0.0	1.000	1061944	8.80		129	
* 6 13C2-PFOA									
415.00 > 370.00	1.859	1.865	-0.006		1123391	10.0		7104	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.859	1.866	-0.007	1.000	2026973	17.0		297	
413.00 > 169.00	1.859	1.866	-0.007	1.000	1039561		1.95(0.00-0.00)	1075	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.102	2.094	0.008	1.000	1801850	17.9		451	a
499.00 > 99.00	2.102	2.094	0.008	1.000	352970		5.10(0.00-0.00)	761	a
* 7 13C4 PFOS									
503.00 > 80.00	2.102	2.102	0.0		2710764	28.7		1406	
9 Perfluorononanoic acid									
463.00 > 419.00	2.109	2.109	0.0	1.000	1731220	18.3		262	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.253	2.260	-0.007	1.000	878101	9.19		8492	

QC Flag Legend

Review Flags

a - User Assigned ID

Reagents:

LC537-ICV_00030

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_013.d

Injection Date: 11-Apr-2018 12:27:50

Instrument ID: A8_N

Lims ID: ICV

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 7

Worklist Smp#: 12

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)

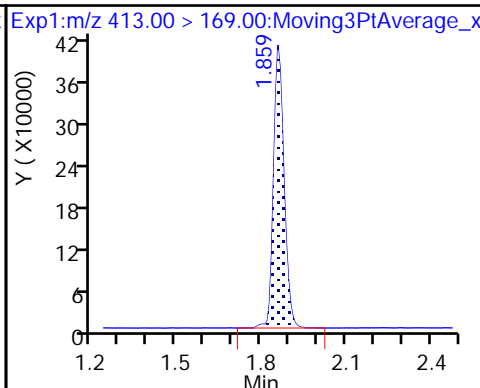


8 Perfluorooctane sulfonic acid

* 7 13C4 PFOS

9 Perfluorononanoic acid



\$ 10 13C2 PFDA

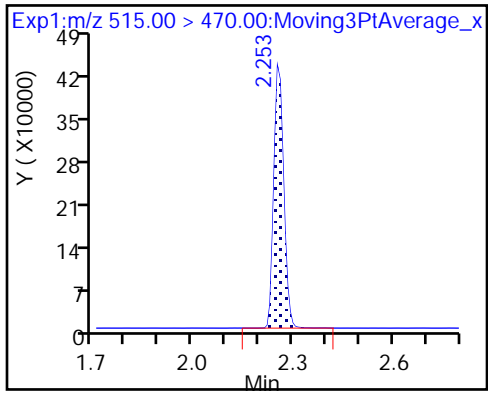

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_013.d
Injection Date: 11-Apr-2018 12:27:50 Instrument ID: A8_N
Lims ID: ICV
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 7 Worklist Smp#: 12
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.09

Processing Integration Results

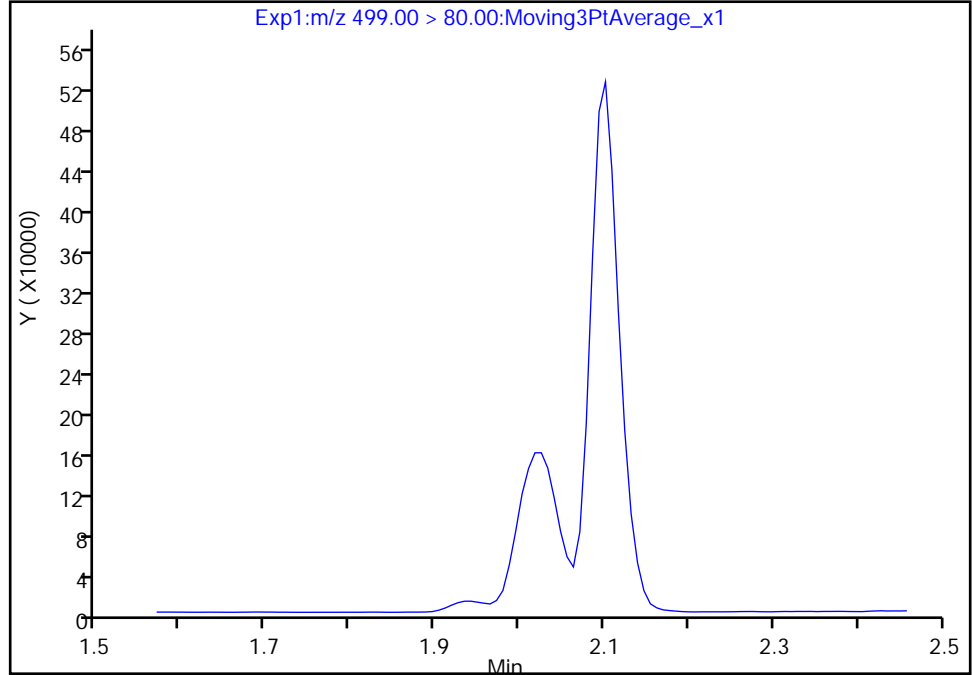

RT: 2.10
Area: 1801850
Amount: 17.882127
Amount Units: ng/ml

Manual Integration Results

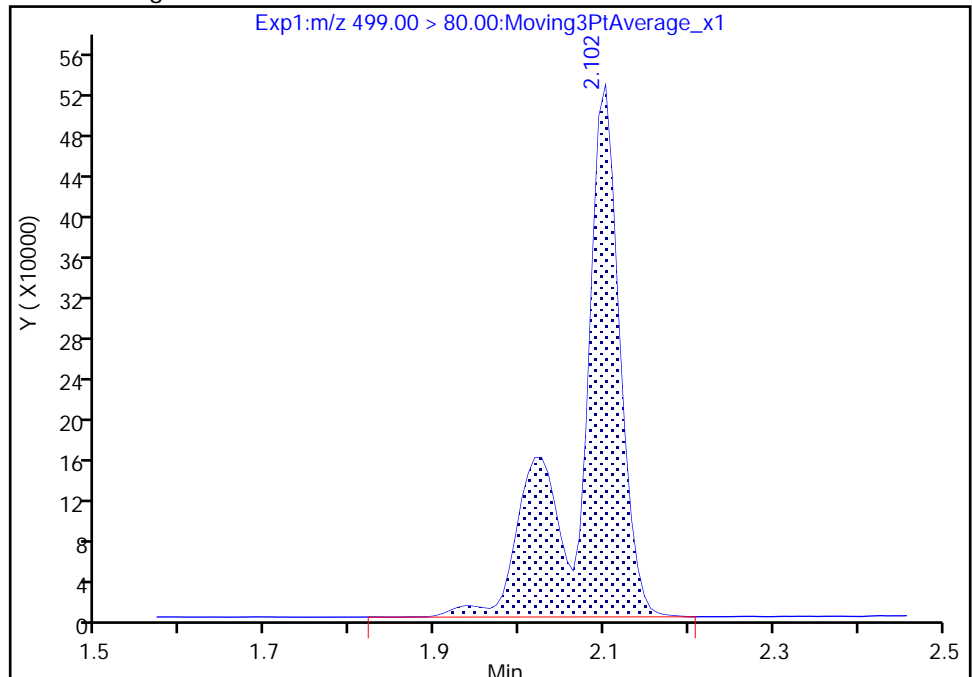

Reviewer: westendorfc, 11-Apr-2018 12:35:10
Audit Action: Assigned Compound ID

Audit Reason: Peak assignment corrected

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Lab Sample ID: CCVL 320-220842/1 Calibration Date: 05/01/2018 11:19
 Instrument ID: A8_N Calib Start Date: 04/11/2018 11:45
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 04/11/2018 12:09
 Lab File ID: 2018.05.01_537AA_003.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	Ave	1.052	1.092		20.8	20.0	3.8	50.0
Perfluoroheptanoic acid (PFHpA)	Ave	1.074	1.039		2.09	2.16	-3.2	50.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.642	1.575		6.45	6.72	-4.1	50.0
Perfluorooctanoic acid (PFOA)	Ave	1.062	1.007		4.17	4.40	-5.2	50.0
Perfluorooctanesulfonic acid (PFOS)	Ave	1.066	1.017		8.38	8.79	-4.6	50.0
Perfluorononanoic acid (PFNA)	Ave	0.8424	0.7780		4.06	4.40	-7.6	50.0
13C2 PFHxA	Ave	1.063	1.073		10.1	10.0	0.9	30.0
13C2 PFDA	Ave	0.8505	0.7541		8.87	10.0	-11.3	30.0

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_003.d
 Lims ID: CCVL
 Client ID:
 Sample Type: CCVL
 Inject. Date: 01-May-2018 11:19:07 ALS Bottle#: 2 Worklist Smp#: 1
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: CCVL
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub9
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 02-May-2018 10:23:02 Calib Date: 11-Apr-2018 12:09:09
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK005

First Level Reviewer: roycea Date: 01-May-2018 13:11:08

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.388	1.396	-0.008	1.000	1697132	20.8		1483	
298.90 > 99.00	1.388	1.396	-0.008	1.000	1286945		1.32(0.00-0.00)	1335	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.533	1.533	0.0	1.000	1019694	10.1		7846	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.699	1.684	0.015	1.000	822008	6.45		284	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.699	1.684	0.015	1.000	213378	2.09		19.4	
* 6 13C2-PFOA									
415.00 > 370.00	1.897	1.874	0.023		950434	10.0		6777	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.897	1.874	0.023	1.000	421252	4.17		60.0	
413.00 > 169.00	1.897	1.874	0.023	1.000	228126		1.85(0.00-0.00)	228	
* 7 13C4 PFOS									
503.00 > 80.00	2.124	2.109	0.015		2226982	28.7		1363	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.124	2.117	0.007	1.000	693620	8.38		221	a
499.00 > 99.00	2.124	2.117	0.007	1.000	158362		4.38(0.00-0.00)	292	a
9 Perfluorononanoic acid									
463.00 > 419.00	2.132	2.124	0.008	1.000	325352	4.06		55.4	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.261	2.269	-0.007	1.000	716744	8.87		5468	

QC Flag Legend

Review Flags

a - User Assigned ID

Reagents:

LC537-L2_00022

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_003.d

Injection Date: 01-May-2018 11:19:07

Instrument ID: A8_N

Lims ID: CCVL

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 2

Worklist Smp#: 1

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA

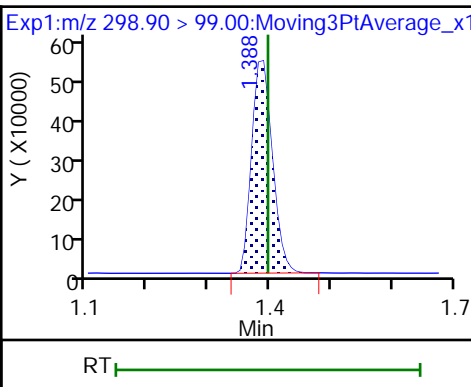

3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA

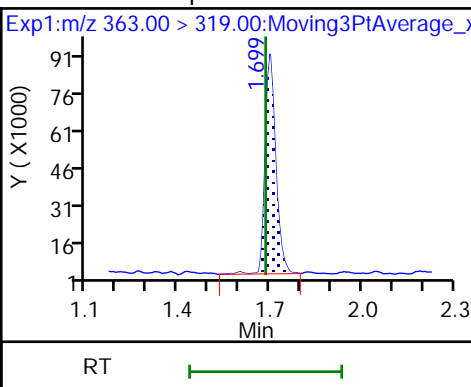

5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




* 7 13C4 PFOS

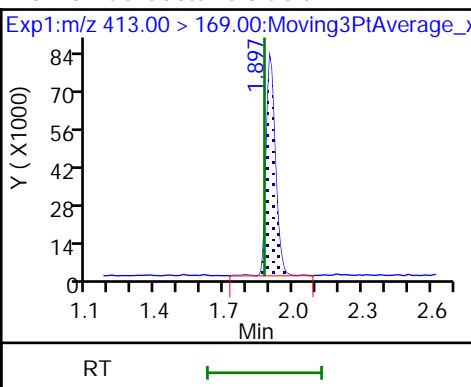


8 Perfluorooctane sulfonic acid (M)

8 Perfluorooctane sulfonic acid

9 Perfluorononanoic acid

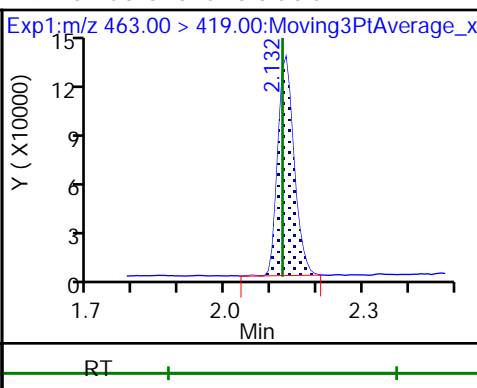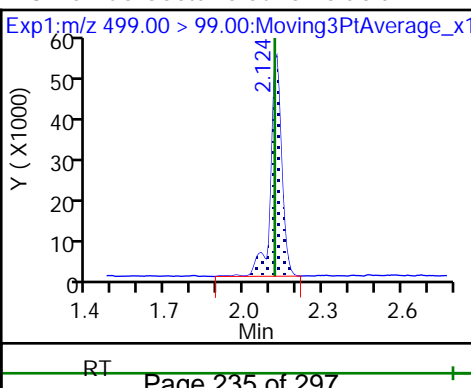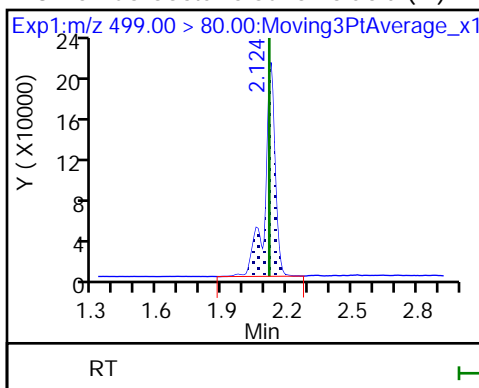

\$ 10 13C2 PFDA



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_003.d
Injection Date: 01-May-2018 11:19:07 Instrument ID: A8_N
Lims ID: CCVL
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 2 Worklist Smp#: 1
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.12

Processing Integration Results

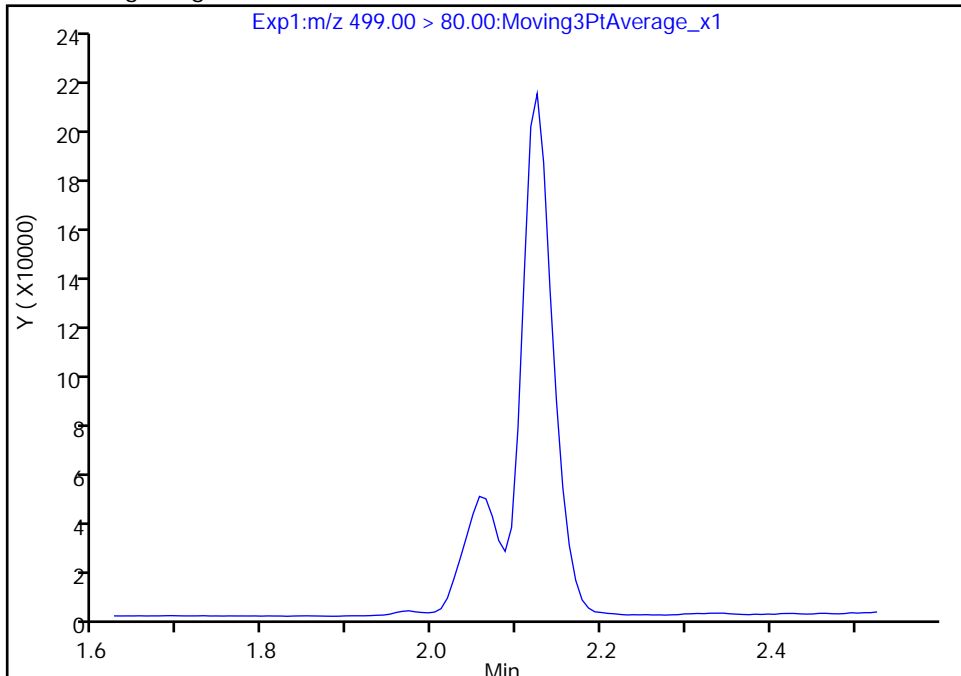

RT: 2.12
Area: 693620
Amount: 8.379096
Amount Units: ng/ml

Manual Integration Results

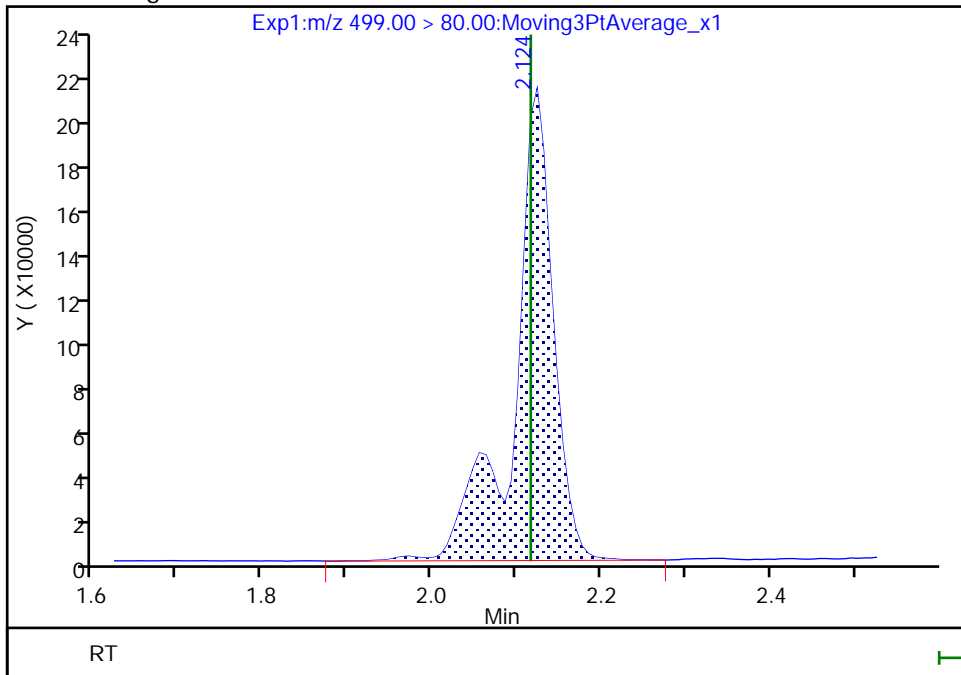

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Lab Sample ID: CCV 320-220845/13 Calibration Date: 05/01/2018 12:15
 Instrument ID: A8_N Calib Start Date: 04/11/2018 11:45
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 04/11/2018 12:09
 Lab File ID: 2018.05.01_537AA_015.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	Ave	1.052	1.055		135	135	0.3	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	1.074	1.021		13.9	14.6	-4.9	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.642	1.688		46.6	45.4	2.8	30.0
Perfluorooctanoic acid (PFOA)	Ave	1.062	1.053		29.4	29.7	-0.9	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	1.066	1.119		62.2	59.3	4.9	30.0
Perfluorononanoic acid (PFNA)	Ave	0.8424	0.7703		27.2	29.7	-8.6	30.0
13C2 PFHxA	Ave	1.063	1.046		9.84	10.0	-1.6	30.0
13C2 PFDA	Ave	0.8505	0.7549		8.88	10.0	-11.2	30.0

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_015.d
 Lims ID: CCV L5
 Client ID:
 Sample Type: CCVIS
 Inject. Date: 01-May-2018 12:15:21 ALS Bottle#: 5 Worklist Smp#: 13
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: CCV L5
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub9
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 02-May-2018 10:40:23 Calib Date: 11-Apr-2018 12:09:09
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK005

First Level Reviewer: barnettj Date: 02-May-2018 10:39:52

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.388	1.388	0.0	1.000	11587254	135.4		8673	
298.90 > 99.00	1.388	1.388	0.0	1.000	9055143		1.28(0.00-0.00)	7968	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.533	1.533	0.0	1.000	1053511	9.84		7355	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.692	1.692	0.0	1.000	6227383	46.6		1970	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.692	1.692	0.0	1.000	1498414	13.9		144	
* 6 13C2-PFOA									
415.00 > 370.00	1.882	1.882	0.0		1006734	10.0		5843	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.889	1.889	0.0	1.000	3148324	29.4		444	
413.00 > 169.00	1.882	1.889	-0.007	0.996	1649818		1.91(0.00-0.00)	1670	
* 7 13C4 PFOS									
503.00 > 80.00	2.117	2.117	0.0		2332599	28.7		1322	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.117	2.117	0.0	1.000	5394512	62.2		1598	a
499.00 > 99.00	2.117	2.117	0.0	1.000	1131486		4.77(0.00-0.00)	2087	a
9 Perfluorononanoic acid									
463.00 > 419.00	2.124	2.124	0.0	1.000	2303243	27.2		369	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.269	2.269	0.0	1.000	759932	8.88		5736	

QC Flag Legend

Review Flags

a - User Assigned ID

Reagents:

LC537-L5_00026

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_015.d

Injection Date: 01-May-2018 12:15:21

Instrument ID: A8_N

Lims ID: CCV L5

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 5

Worklist Smp#: 13

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




* 7 13C4 PFOS

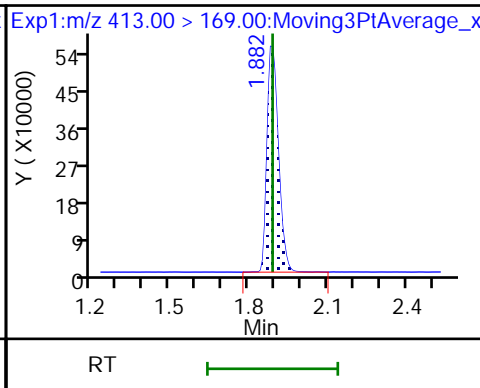


8 Perfluorooctane sulfonic acid (M)

8 Perfluorooctane sulfonic acid

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_015.d
Injection Date: 01-May-2018 12:15:21 Instrument ID: A8_N
Lims ID: CCV L5
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 5 Worklist Smp#: 13
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.12

Processing Integration Results

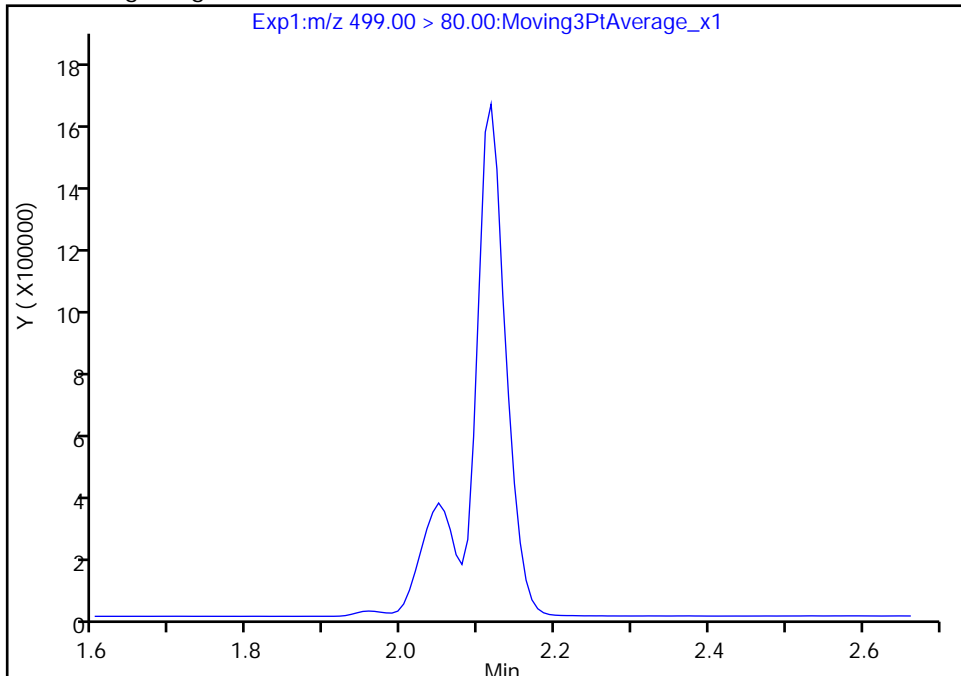

Manual Integration Results

RT: 2.12
Area: 5394512
Amount: 62.216321
Amount Units: ng/ml

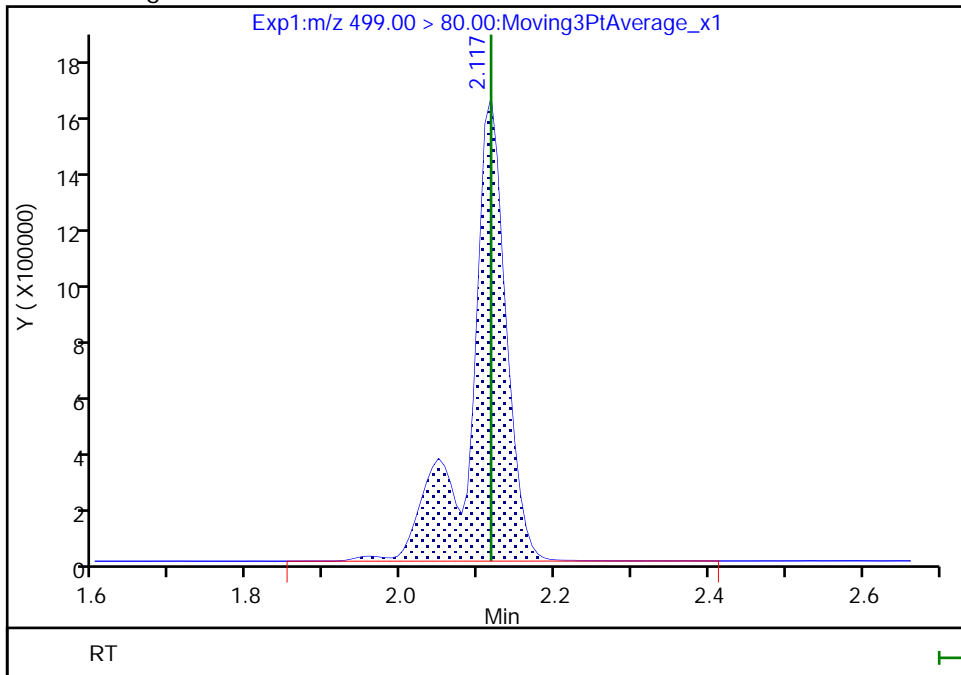

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Lab Sample ID: CCV 320-220845/25 Calibration Date: 05/01/2018 13:11
 Instrument ID: A8_N Calib Start Date: 04/11/2018 11:45
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 04/11/2018 12:09
 Lab File ID: 2018.05.01_537AA_027.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	Ave	1.052	1.108		47.4	45.0	5.3	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	1.074	1.096		4.96	4.86	2.1	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.642	1.664		15.3	15.1	1.3	30.0
Perfluorooctanoic acid (PFOA)	Ave	1.062	1.050		9.79	9.90	-1.1	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	1.066	1.050		19.5	19.8	-1.5	30.0
Perfluorononanoic acid (PFNA)	Ave	0.8424	0.8166		9.60	9.90	-3.1	30.0
13C2 PFHxA	Ave	1.063	1.066		10.0	10.0	0.3	30.0
13C2 PFDA	Ave	0.8505	0.7446		8.75	10.0	-12.5	30.0

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Lab Sample ID: CCV 320-220847/25 Calibration Date: 05/01/2018 13:11
 Instrument ID: A8_N Calib Start Date: 04/11/2018 11:45
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 04/11/2018 12:09
 Lab File ID: 2018.05.01_537AA_027.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	Ave	1.052	1.108		47.4	45.0	5.3	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	1.074	1.096		4.96	4.86	2.1	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.642	1.664		15.3	15.1	1.3	30.0
Perfluorooctanoic acid (PFOA)	Ave	1.062	1.050		9.79	9.90	-1.1	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	1.066	1.050		19.5	19.8	-1.5	30.0
Perfluorononanoic acid (PFNA)	Ave	0.8424	0.8166		9.60	9.90	-3.1	30.0
13C2 PFHxA	Ave	1.063	1.066		10.0	10.0	0.3	30.0
13C2 PFDA	Ave	0.8505	0.7446		8.75	10.0	-12.5	30.0

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_027.d
 Lims ID: CCV L3
 Client ID:
 Sample Type: CCVIS
 Inject. Date: 01-May-2018 13:11:31 ALS Bottle#: 3 Worklist Smp#: 25
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: CCV L3
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub9
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 02-May-2018 10:27:59 Calib Date: 11-Apr-2018 12:09:09
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last Ical File: \\ChromNA\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK005

First Level Reviewer: roycea Date: 01-May-2018 14:00:50

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.396	1.396	0.0	1.000	3573483	47.4		2929	
298.90 > 99.00	1.396	1.396	0.0	1.000	2839021		1.26(0.00-0.00)	2865	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.533	1.533	0.0	1.000	904809	10.0		6943	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.692	1.692	0.0	1.000	1803133	15.3		577	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.692	1.692	0.0	1.000	452175	4.96		42.6	
* 6 13C2-PFOA									
415.00 > 370.00	1.882	1.882	0.0		848761	10.0		5151	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.882	1.882	0.0	1.000	882443	9.79		131	
413.00 > 169.00	1.882	1.882	0.0	1.000	469054		1.88(0.00-0.00)	470	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.117	2.117	0.0	1.000	1486529	19.5		447	a
499.00 > 99.00	2.117	2.117	0.0	1.000	324920		4.58(0.00-0.00)	615	a
* 7 13C4 PFOS									
503.00 > 80.00	2.109	2.109	0.0		2054615	28.7		1202	
9 Perfluorononanoic acid									
463.00 > 419.00	2.124	2.124	0.0	1.000	686122	9.60		106	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.269	2.269	0.0	1.000	631959	8.75		4654	

QC Flag Legend

Review Flags

a - User Assigned ID

Reagents:

LC537-L3_00025

Amount Added: 1.00

Units: mL

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_027.d
 Lims ID: CCV L3
 Client ID:
 Sample Type: CCVIS
 Inject. Date: 01-May-2018 13:11:31 ALS Bottle#: 3 Worklist Smp#: 25
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: CCV L3
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub9
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 02-May-2018 10:27:59 Calib Date: 11-Apr-2018 12:09:09
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK005

First Level Reviewer: roycea Date: 01-May-2018 14:00:50

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.396	1.396	0.0	1.000	3573483	47.4		2929	
298.90 > 99.00	1.396	1.396	0.0	1.000	2839021		1.26(0.00-0.00)	2865	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.533	1.533	0.0	1.000	904809	10.0		6943	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.692	1.692	0.0	1.000	1803133	15.3		577	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.692	1.692	0.0	1.000	452175	4.96		42.6	
* 6 13C2-PFOA									
415.00 > 370.00	1.882	1.882	0.0		848761	10.0		5151	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.882	1.882	0.0	1.000	882443	9.79		131	
413.00 > 169.00	1.882	1.882	0.0	1.000	469054		1.88(0.00-0.00)	470	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.117	2.117	0.0	1.000	1486529	19.5		447	a
499.00 > 99.00	2.117	2.117	0.0	1.000	324920		4.58(0.00-0.00)	615	a
* 7 13C4 PFOS									
503.00 > 80.00	2.109	2.109	0.0		2054615	28.7		1202	
9 Perfluorononanoic acid									
463.00 > 419.00	2.124	2.124	0.0	1.000	686122	9.60		106	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.269	2.269	0.0	1.000	631959	8.75		4654	

QC Flag Legend

Review Flags

a - User Assigned ID

Reagents:

LC537-L3_00025

Amount Added: 1.00

Units: mL

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_027.d

Injection Date: 01-May-2018 13:11:31

Instrument ID: A8_N

Lims ID: CCV L3

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 3

Worklist Smp#: 25

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA

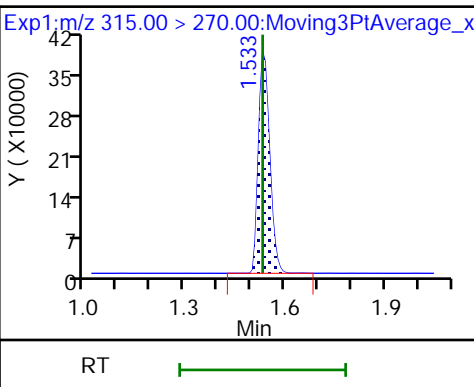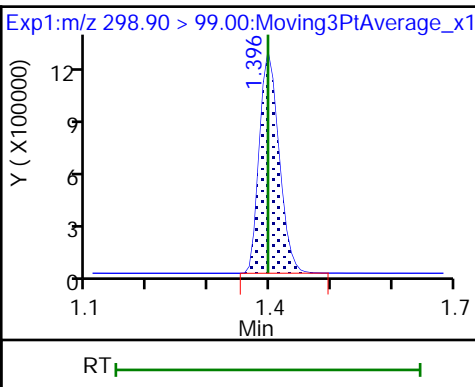

3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA

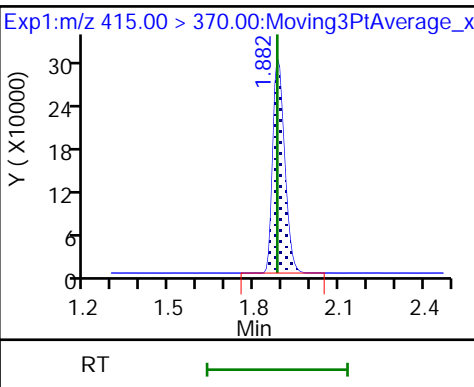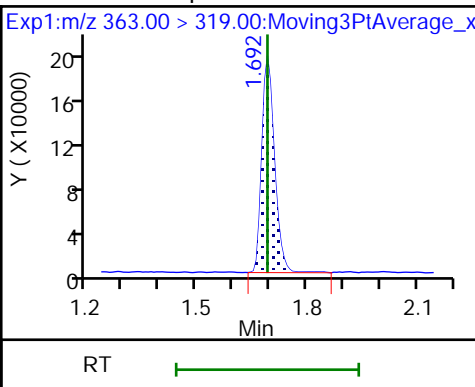

5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)

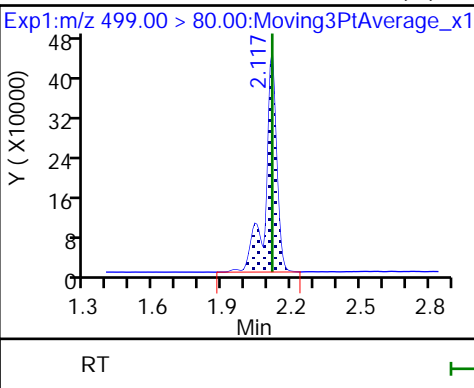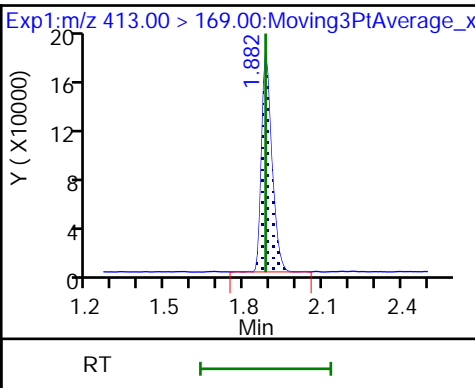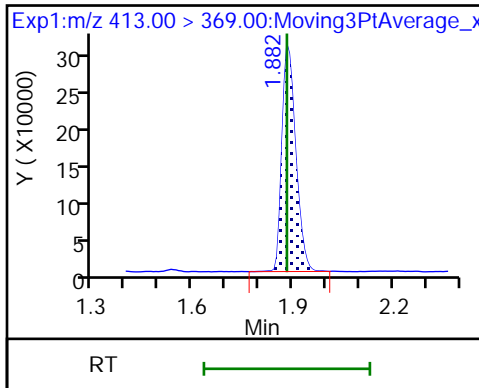


8 Perfluorooctane sulfonic acid

* 7 13C4 PFOS

9 Perfluorononanoic acid

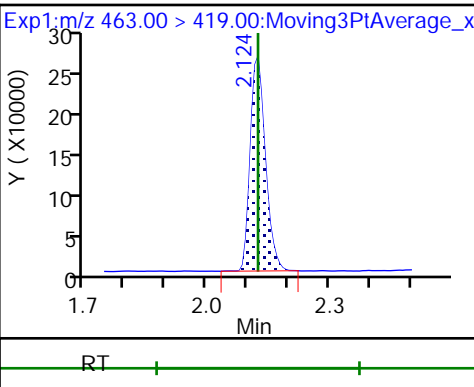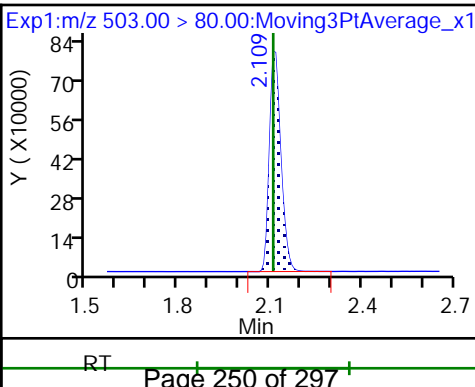

\$ 10 13C2 PFDA



TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_027.d

Injection Date: 01-May-2018 13:11:31

Instrument ID: A8_N

Lims ID: CCV L3

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 3

Worklist Smp#: 25

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA

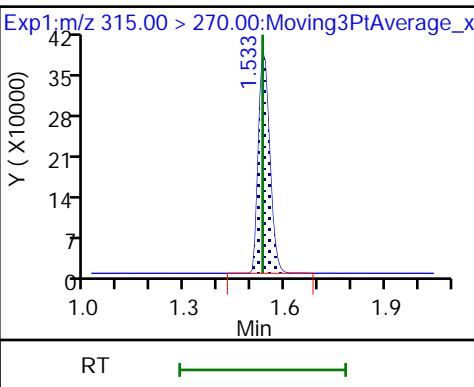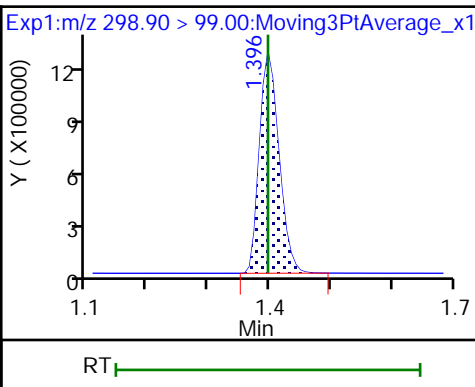

3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA

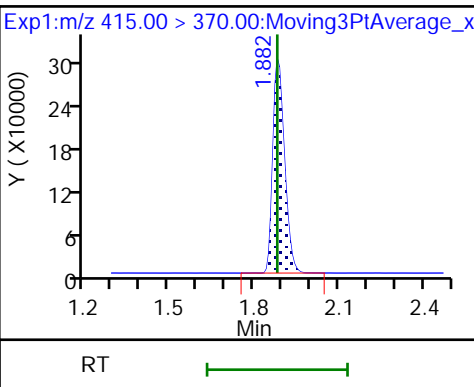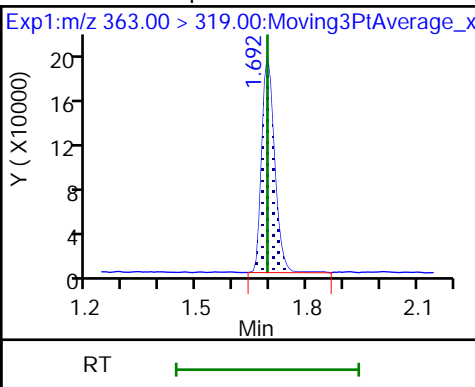

5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)

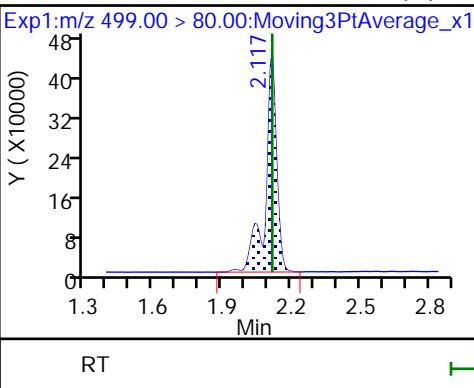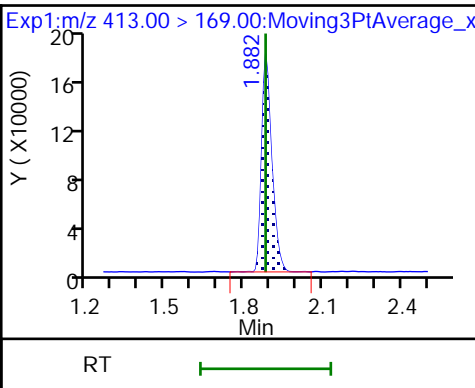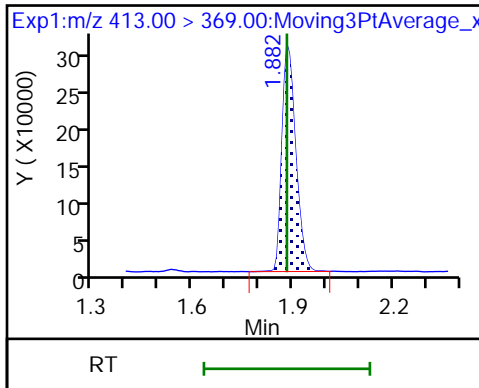


8 Perfluorooctane sulfonic acid

* 7 13C4 PFOS

9 Perfluorononanoic acid

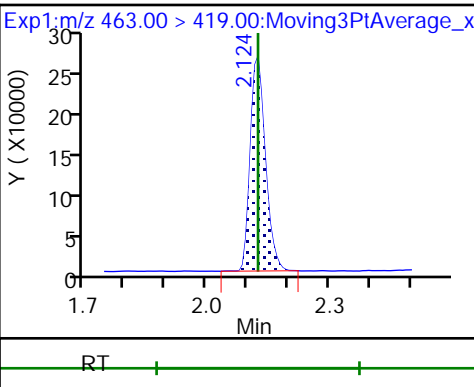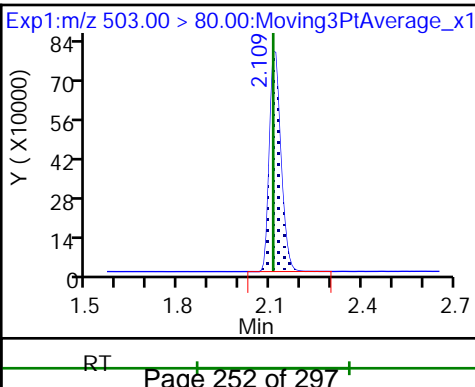

\$ 10 13C2 PFDA



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_027.d
Injection Date: 01-May-2018 13:11:31 Instrument ID: A8_N
Lims ID: CCV L3
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 3 Worklist Smp#: 25
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.12

Processing Integration Results

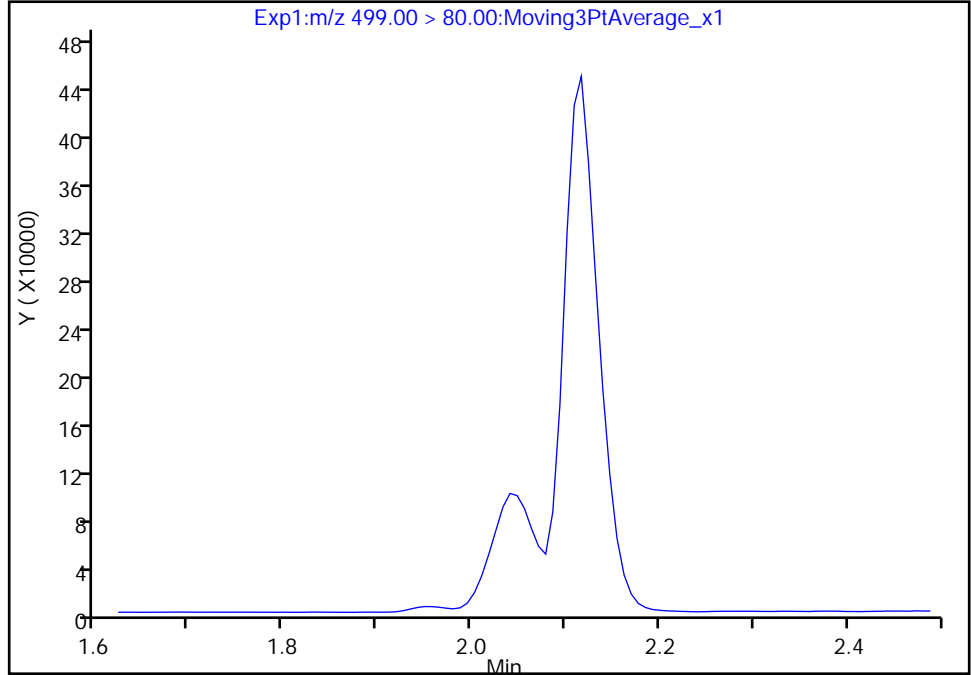

RT: 2.12
Area: 1486529
Amount: 19.464138
Amount Units: ng/ml

Manual Integration Results

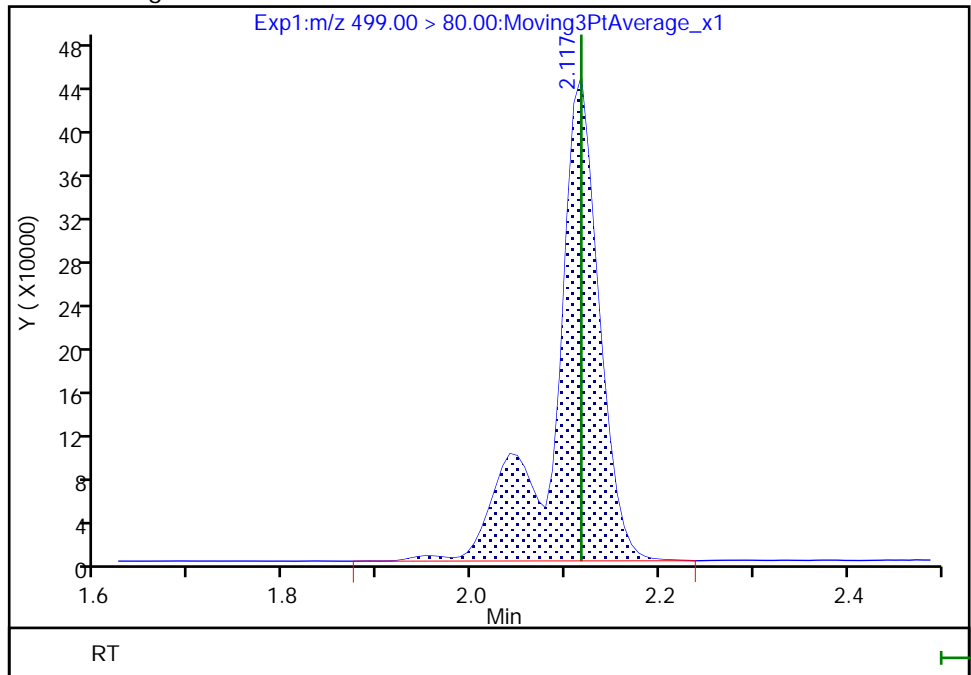

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_027.d
Injection Date: 01-May-2018 13:11:31 Instrument ID: A8_N
Lims ID: CCV L3
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 3 Worklist Smp#: 25
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.12

Processing Integration Results

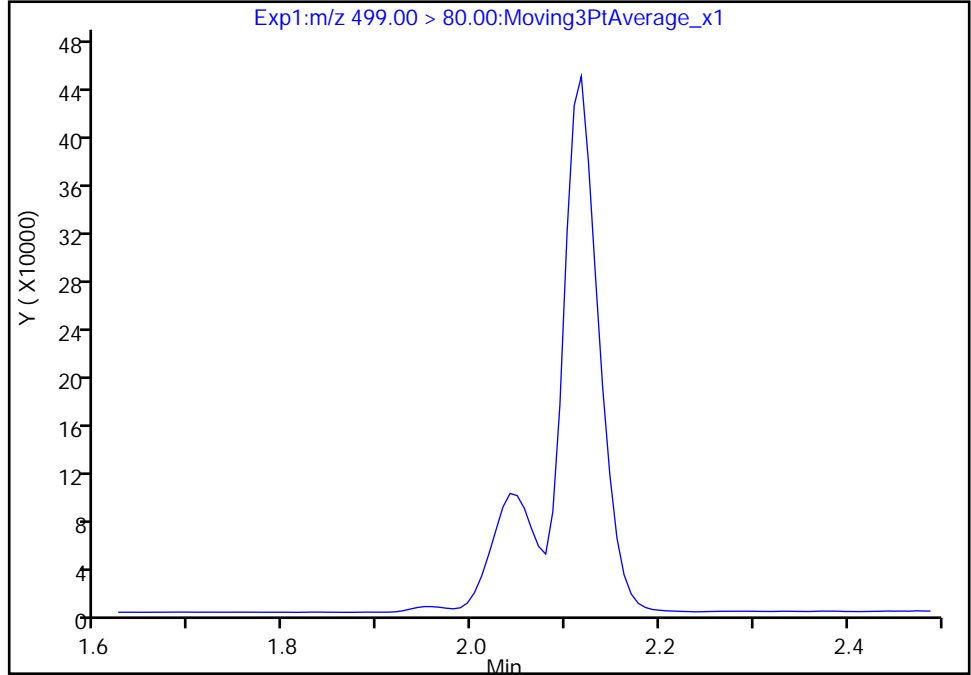

RT: 2.12
Area: 1486529
Amount: 19.464138
Amount Units: ng/ml

Manual Integration Results

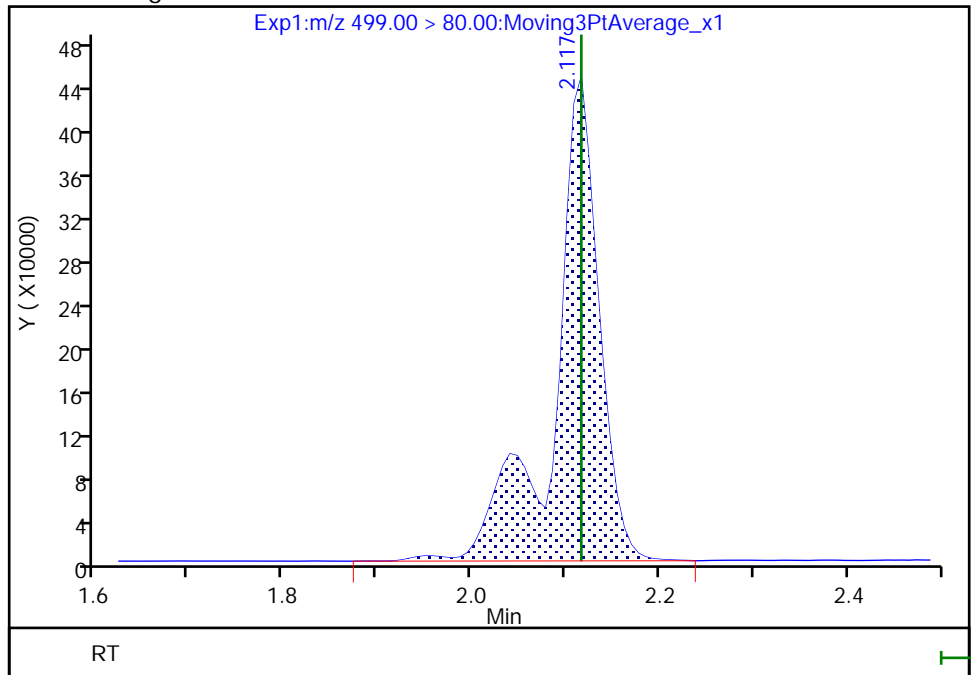

Reviewer: roycea, 01-May-2018 14:00:30
Audit Action: Assigned Compound ID

Audit Reason: Peak assignment corrected
Page 255 of 297

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Lab Sample ID: CCV 320-220847/29 Calibration Date: 05/01/2018 13:30
 Instrument ID: A8_N Calib Start Date: 04/11/2018 11:45
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 04/11/2018 12:09
 Lab File ID: 2018.05.01_537AA_031.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	Ave	1.052	1.053		135	135	0.1	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	1.074	1.077		14.6	14.6	0.3	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.642	1.641		45.3	45.4	-0.0	30.0
Perfluorooctanoic acid (PFOA)	Ave	1.062	1.096		30.6	29.7	3.1	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	1.066	1.095		60.9	59.3	2.7	30.0
Perfluorononanoic acid (PFNA)	Ave	0.8424	0.8000		28.2	29.7	-5.0	30.0
13C2 PFHxA	Ave	1.063	1.068		10.0	10.0	0.5	30.0
13C2 PFDA	Ave	0.8505	0.7823		9.20	10.0	-8.0	30.0

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_031.d
 Lims ID: CCV L5
 Client ID:
 Sample Type: CCVIS
 Inject. Date: 01-May-2018 13:30:13 ALS Bottle#: 5 Worklist Smp#: 29
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: CCV L5
 Misc. Info.: Plate: 1 Rack: 1
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Sublist: chrom-537_A8_N*sub9
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 02-May-2018 10:28:16 Calib Date: 11-Apr-2018 12:09:09
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK005

First Level Reviewer: roycea Date: 01-May-2018 14:01:19

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.396	1.396	0.0	1.000	10287368	135.3		7508	
298.90 > 99.00	1.396	1.396	0.0	1.000	8112695		1.27(0.00-0.00)	7693	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.533	1.533	0.0	1.000	909589	10.0		7509	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.684	1.684	0.0	1.000	5383819	45.3		1664	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.684	1.684	0.0	1.000	1337101	14.6		116	
* 6 13C2-PFOA									
415.00 > 370.00	1.882	1.882	0.0		851622	10.0		5475	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.882	1.882	0.0	1.000	2771226	30.6		410	
413.00 > 169.00	1.874	1.882	-0.008	0.996	1456013		1.90(0.00-0.00)	1396	
* 7 13C4 PFOS									
503.00 > 80.00	2.109	2.109	0.0		2073725	28.7		1180	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.109	2.117	-0.008	1.000	4695343	60.9		1374	a
499.00 > 99.00	2.109	2.117	-0.008	1.000	979932		4.79(0.00-0.00)	1858	a
9 Perfluorononanoic acid									
463.00 > 419.00	2.117	2.117	0.0	1.000	2023553	28.2		317	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.269	2.269	0.0	1.000	666188	9.20		5014	

QC Flag Legend

Review Flags

a - User Assigned ID

Reagents:

LC537-L5_00026

Amount Added: 1.00

Units: mL

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_031.d

Injection Date: 01-May-2018 13:30:13

Instrument ID: A8_N

Lims ID: CCV L5

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 5

Worklist Smp#: 29

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA



3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA



5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




* 7 13C4 PFOS

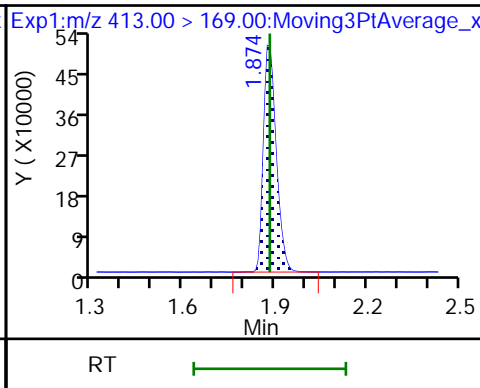


8 Perfluorooctane sulfonic acid (M)

8 Perfluorooctane sulfonic acid

9 Perfluorononanoic acid



\$ 10 13C2 PFDA



TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_031.d
Injection Date: 01-May-2018 13:30:13 Instrument ID: A8_N
Lims ID: CCV L5
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 5 Worklist Smp#: 29
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.12

Processing Integration Results

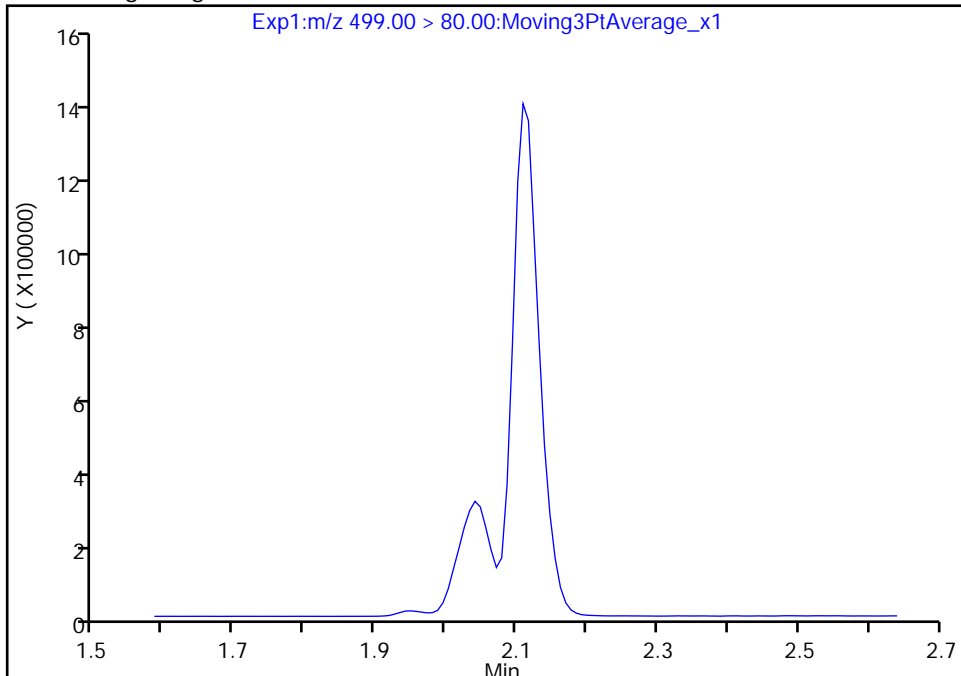

Manual Integration Results

RT: 2.11
Area: 4695343
Amount: 60.912779
Amount Units: ng/ml

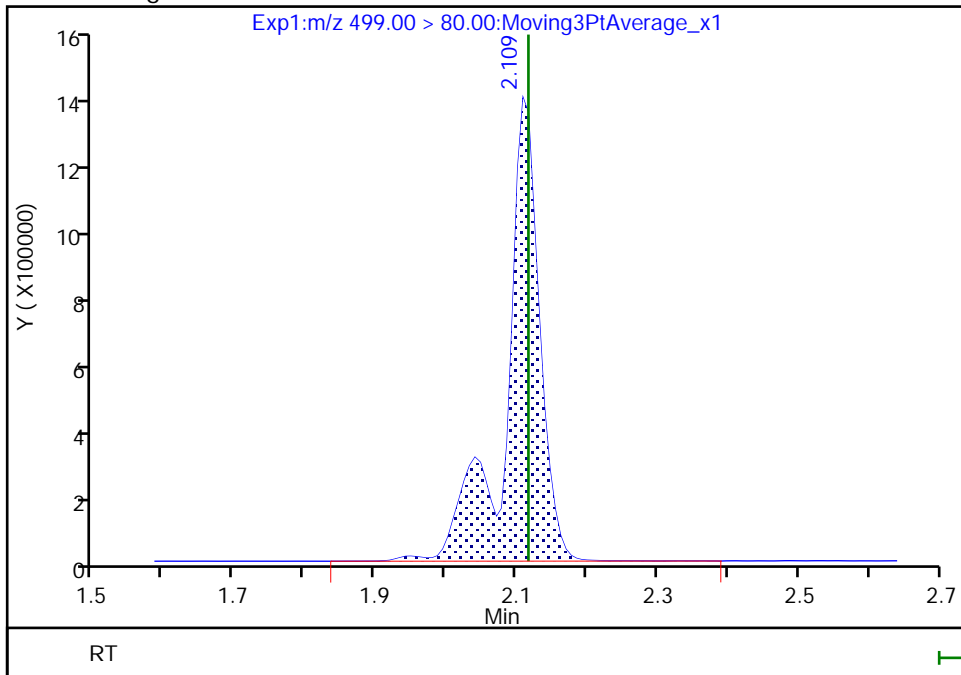

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Client Sample ID: _____ Lab Sample ID: MB 320-219896/1-A
 Matrix: Water Lab File ID: 2018.05.01_537AA_017.d
 Analysis Method: 537 Date Collected: _____
 Extraction Method: 537 Date Extracted: 04/26/2018 09:35
 Sample wt/vol: 250 (mL) Date Analyzed: 05/01/2018 12:24
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 220845 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	8.0	U	20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.0	U	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	107		70-130
STL00996	13C2 PFDA	90		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_017.d
 Lims ID: MB 320-219896/1-A
 Client ID:
 Sample Type: MB
 Inject. Date: 01-May-2018 12:24:40 ALS Bottle#: 10 Worklist Smp#: 15
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: mb 320-219896/1-a
 Misc. Info.: Plate: 1 Rack: 6
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 02-May-2018 10:24:00 Calib Date: 11-Apr-2018 12:09:09
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_009.d

Column 1 : Det: EXP1
 Process Host: XAWRK005

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
\$ 2 13C2 PFHxA	315.00 > 270.00	1.540	1.533	0.007	1.000	1022227	10.7	7972	
* 6 13C2-PFOA	415.00 > 370.00	1.889	1.882	0.007		896308	10.0	6233	
* 7 13C4 PFOS	503.00 > 80.00	2.117	2.117	0.0		2119146	28.7	1339	
\$ 10 13C2 PFDA	515.00 > 470.00	2.269	2.269	0.0	1.000	684019	8.97	5676	

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_017.d

Injection Date: 01-May-2018 12:24:40

Instrument ID: A8_N

Lims ID: MB 320-219896/1-A

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 10

Worklist Smp#: 15

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid (ND)

1 Perfluorobutanesulfonic acid (ND)




\$ 2 13C2 PFHxA

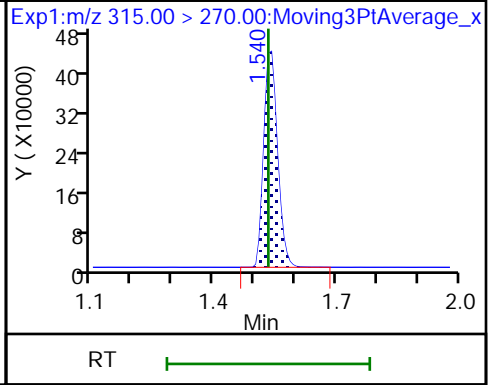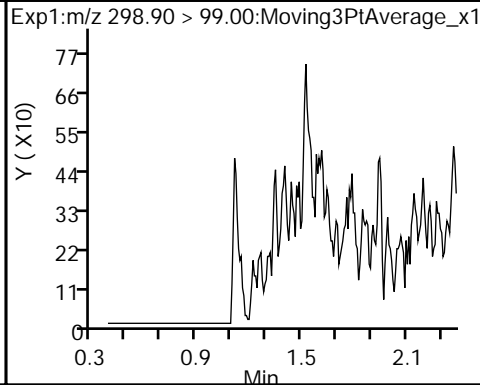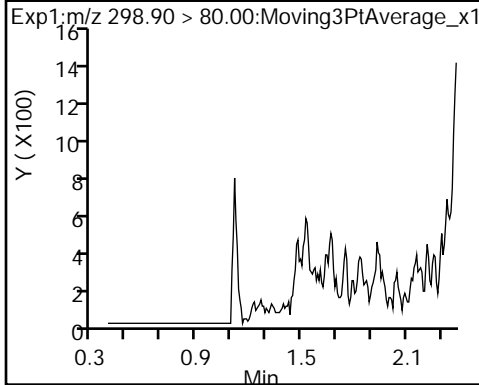

3 Perfluorohexanesulfonic acid (ND)

4 Perfluoroheptanoic acid (ND)




* 6 13C2-PFOA

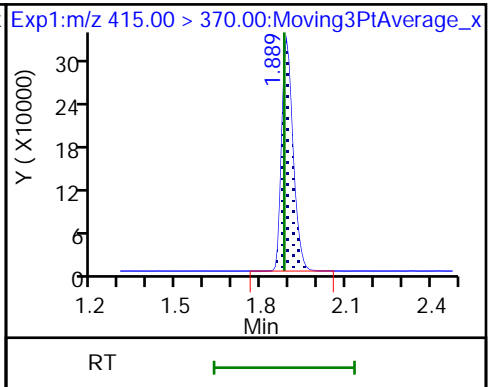

5 Perfluorooctanoic acid (ND)

5 Perfluorooctanoic acid (ND)




8 Perfluorooctane sulfonic acid (ND)

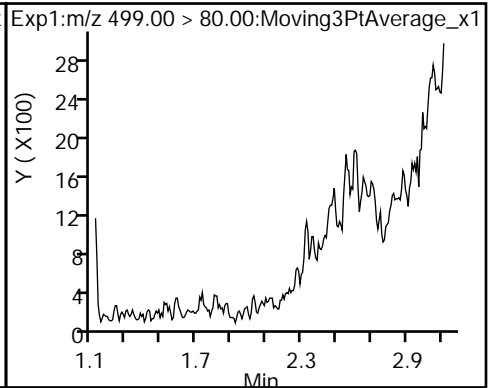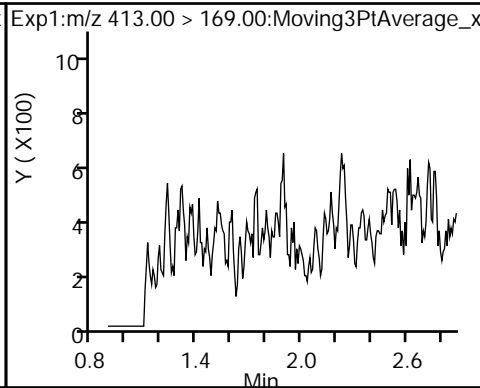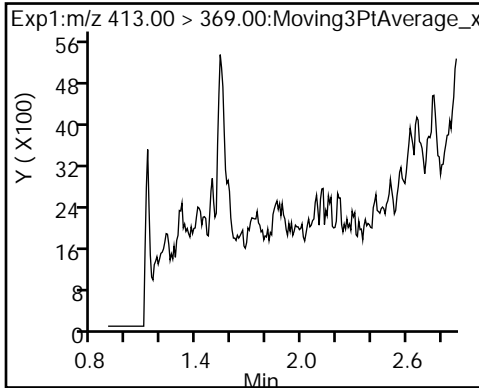


8 Perfluorooctane sulfonic acid (ND)

* 7 13C4 PFOS

9 Perfluorononanoic acid (ND)

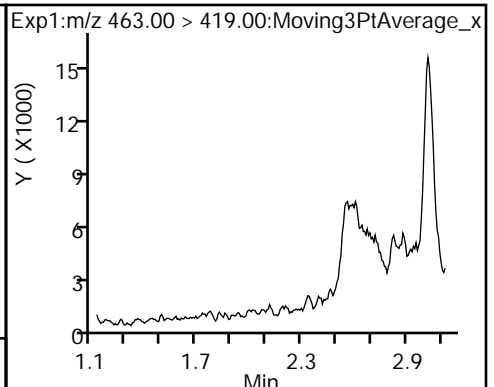

\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_017.d
 Lims ID: MB 320-219896/1-A
 Client ID:
 Sample Type: MB
 Inject. Date: 01-May-2018 12:24:40 ALS Bottle#: 10 Worklist Smp#: 15
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: mb 320-219896/1-a
 Misc. Info.: Plate: 1 Rack: 6
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 02-May-2018 10:24:00 Calib Date: 11-Apr-2018 12:09:09
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK005

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	10.7	107.27
\$ 10 13C2 PFDA	10.0	8.97	89.73

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Client Sample ID: _____ Lab Sample ID: LCS 320-219896/2-A
 Matrix: Water Lab File ID: 2018.05.01_537AA_018.d
 Analysis Method: 537 Date Collected: _____
 Extraction Method: 537 Date Extracted: 04/26/2018 09:35
 Sample wt/vol: 250 (mL) Date Analyzed: 05/01/2018 12:29
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 220845 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	225	M	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	110		20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	102		24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	179		30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	58.2		10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	519		90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	108		70-130
STL00996	13C2 PFDA	91		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_018.d
 Lims ID: LCS 320-219896/2-A
 Client ID:
 Sample Type: LCS
 Inject. Date: 01-May-2018 12:29:21 ALS Bottle#: 11 Worklist Smp#: 16
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: lcs 320-219896/2-a
 Misc. Info.: Plate: 1 Rack: 6
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 02-May-2018 10:24:00 Calib Date: 11-Apr-2018 12:09:09
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK005

First Level Reviewer: roycea Date: 01-May-2018 13:59:02

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.396	1.388	0.008	1.000	10254311	129.9		7920	
298.90 > 99.00	1.396	1.388	0.008	1.000	7947753		1.29(0.00-0.00)	7309	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.540	1.533	0.007	1.000	1020854	10.8		8106	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.699	1.692	0.007	1.000	5514720	44.7		1793	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.699	1.692	0.007	1.000	1383663	14.5		133	
* 6 13C2-PFOA									
415.00 > 370.00	1.897	1.882	0.015		885760	10.0		6150	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.897	1.889	0.008	1.000	2578388	27.4		373	
413.00 > 169.00	1.897	1.889	0.008	1.000	1499455		1.72(0.00-0.00)	1572	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.124	2.117	0.007	1.000	4508152	56.3		1355	a
499.00 > 99.00	2.124	2.117	0.007	1.000	964858		4.67(0.00-0.00)	1702	a
* 7 13C4 PFOS									
503.00 > 80.00	2.117	2.117	0.0		2152883	28.7		1357	
9 Perfluorononanoic acid									
463.00 > 419.00	2.132	2.124	0.008	1.000	1910486	25.6		260	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.269	2.269	0.0	1.000	686008	9.11		5460	

QC Flag Legend

Review Flags

a - User Assigned ID

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_018.d

Injection Date: 01-May-2018 12:29:21

Instrument ID: A8_N

Lims ID: LCS 320-219896/2-A

Client ID:

Operator ID: SACINSTLCMS01

ALS Bottle#: 11

Worklist Smp#: 16

Injection Vol: 2.0 ul

Dil. Factor: 1.0000




Method: 537_A8_N

Limit Group: LC 537 ICAL

1 Perfluorobutanesulfonic acid

1 Perfluorobutanesulfonic acid




\$ 2 13C2 PFHxA

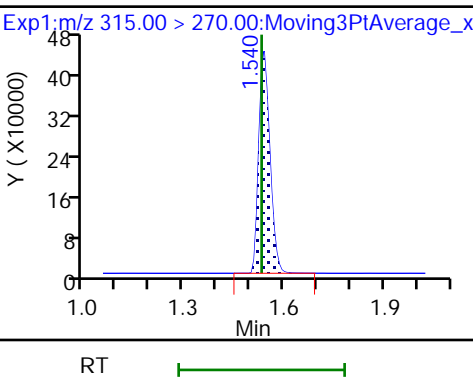

3 Perfluorohexanesulfonic acid

4 Perfluoroheptanoic acid




* 6 13C2-PFOA

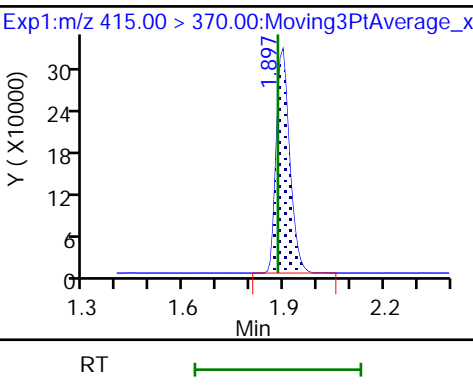

5 Perfluorooctanoic acid

5 Perfluorooctanoic acid




8 Perfluorooctane sulfonic acid (M)

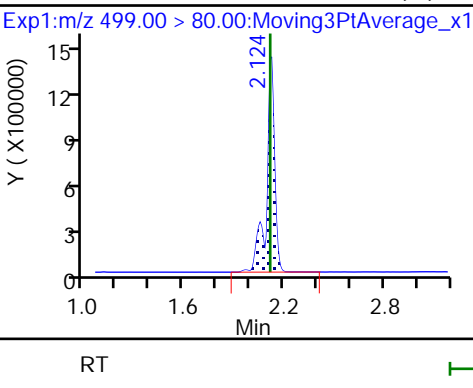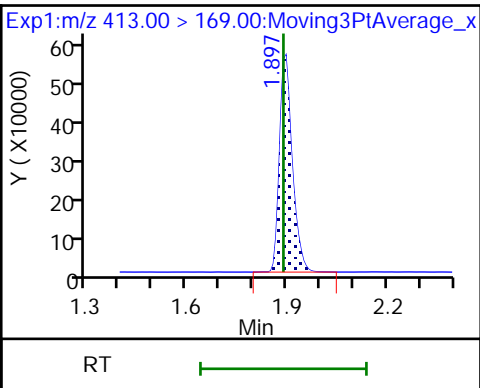


8 Perfluorooctane sulfonic acid

* 7 13C4 PFOS

9 Perfluorononanoic acid

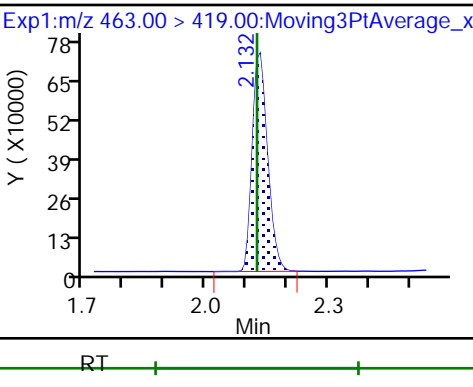

\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_018.d
 Lims ID: LCS 320-219896/2-A
 Client ID:
 Sample Type: LCS
 Inject. Date: 01-May-2018 12:29:21 ALS Bottle#: 11 Worklist Smp#: 16
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: lcs 320-219896/2-a
 Misc. Info.: Plate: 1 Rack: 6
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 02-May-2018 10:24:00 Calib Date: 11-Apr-2018 12:09:09
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK005

First Level Reviewer: roycea Date: 01-May-2018 13:59:02

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	10.8	108.40
\$ 10 13C2 PFDA	10.0	9.11	91.07

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_018.d
Injection Date: 01-May-2018 12:29:21 Instrument ID: A8_N
Lims ID: LCS 320-219896/2-A
Client ID:
Operator ID: SACINSTLCMS01 ALS Bottle#: 11 Worklist Smp#: 16
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.12

Processing Integration Results

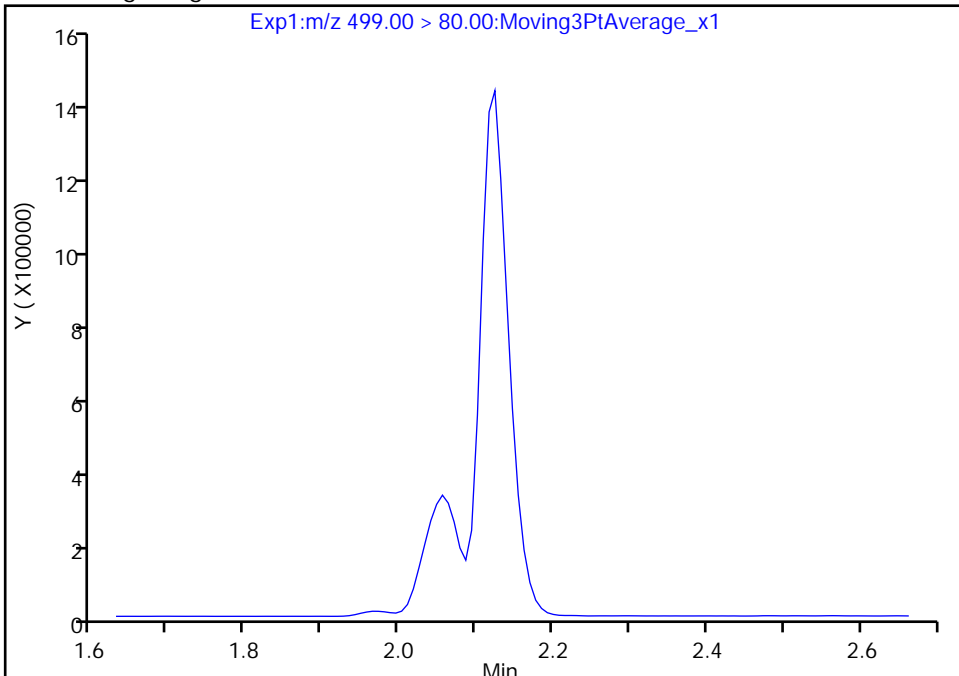

Manual Integration Results

RT: 2.12
Area: 4508152
Amount: 56.333972
Amount Units: ng/ml

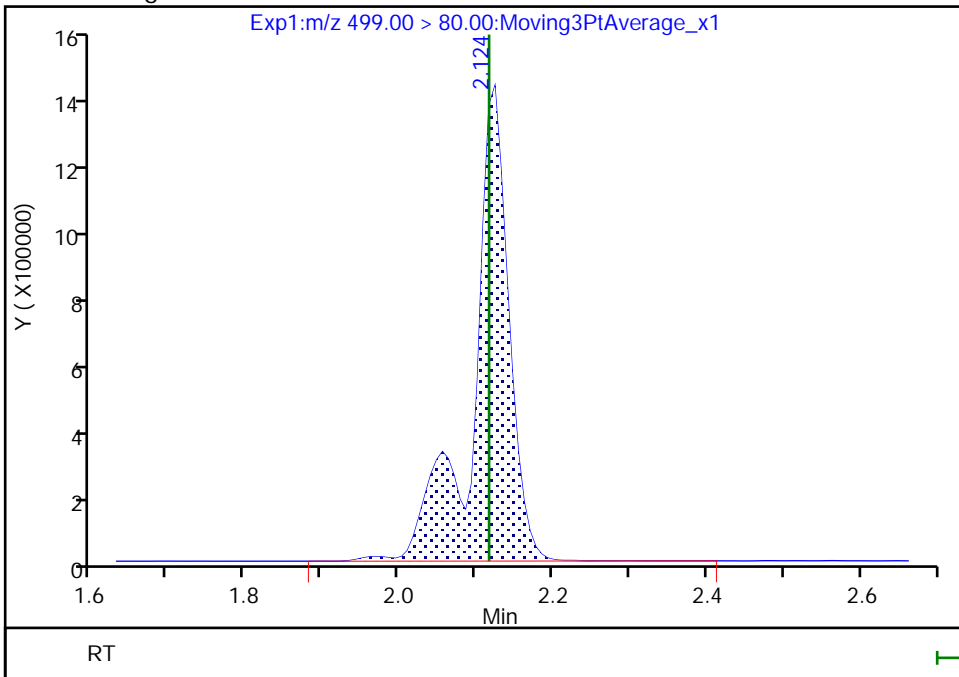

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Client Sample ID: NAWC-041918-RW-154 MS Lab Sample ID: 320-38382-1 MS
 Matrix: Water Lab File ID: 2018.05.01_537AA_020.d
 Analysis Method: 537 Date Collected: 04/19/2018 09:10
 Extraction Method: 537 Date Extracted: 04/26/2018 09:35
 Sample wt/vol: 252.5 (mL) Date Analyzed: 05/01/2018 12:38
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 220845 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	237	M	40	16	6.7
335-67-1	Perfluorooctanoic acid (PFOA)	124		20	7.9	2.8
375-95-1	Perfluorononanoic acid (PFNA)	98.7		24	20	7.9
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	177		30	12	5.4
375-85-9	Perfluoroheptanoic acid (PFHpA)	59.8		9.9	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	523		89	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	96		70-130
STL00996	13C2 PFDA	84		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_020.d
 Lims ID: 320-38382-A-1-B MS
 Client ID: NAWC-041918-RW-154
 Sample Type: MS
 Inject. Date: 01-May-2018 12:38:43 ALS Bottle#: 13 Worklist Smp#: 18
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-38382-a-1-b ms
 Misc. Info.: Plate: 1 Rack: 6
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 02-May-2018 10:24:00 Calib Date: 11-Apr-2018 12:09:09
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK005

First Level Reviewer: barnettj Date: 01-May-2018 17:13:21

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.396	1.388	0.008	1.000	9581866	131.9		6312	
298.90 > 99.00	1.396	1.388	0.008	1.000	7489678		1.28(0.00-0.00)	6743	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.533	1.533	0.0	1.000	891287	9.60		8014	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.692	1.692	0.0	1.000	5054176	44.6		1424	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.692	1.692	0.0	1.000	1415309	15.1		118	
* 6 13C2-PFOA									
415.00 > 370.00	1.889	1.882	0.007		873603	10.0		5766	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.889	1.889	0.0	1.000	2911362	31.4		377	
413.00 > 169.00	1.889	1.889	0.0	1.000	1627227		1.79(0.00-0.00)	1565	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.117	2.117	0.0	1.000	4411041	59.9		1159	a
499.00 > 99.00	2.117	2.117	0.0	1.000	893545		4.94(0.00-0.00)	1473	a
* 7 13C4 PFOS									
503.00 > 80.00	2.117	2.117	0.0		1979894	28.7		1110	
9 Perfluorononanoic acid									
463.00 > 419.00	2.124	2.124	0.0	1.000	1834502	24.9		231	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.269	2.269	0.0	1.000	622291	8.38		5941	


QC Flag Legend

Review Flags


a - User Assigned ID

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_020.d
Injection Date: 01-May-2018 12:38:43 Instrument ID: A8_N
Lims ID: 320-38382-A-1-B MS
Client ID: NAWC-041918-RW-154
Operator ID: SACINSTLCMS01 ALS Bottle#: 13 Worklist Smp#: 18
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL

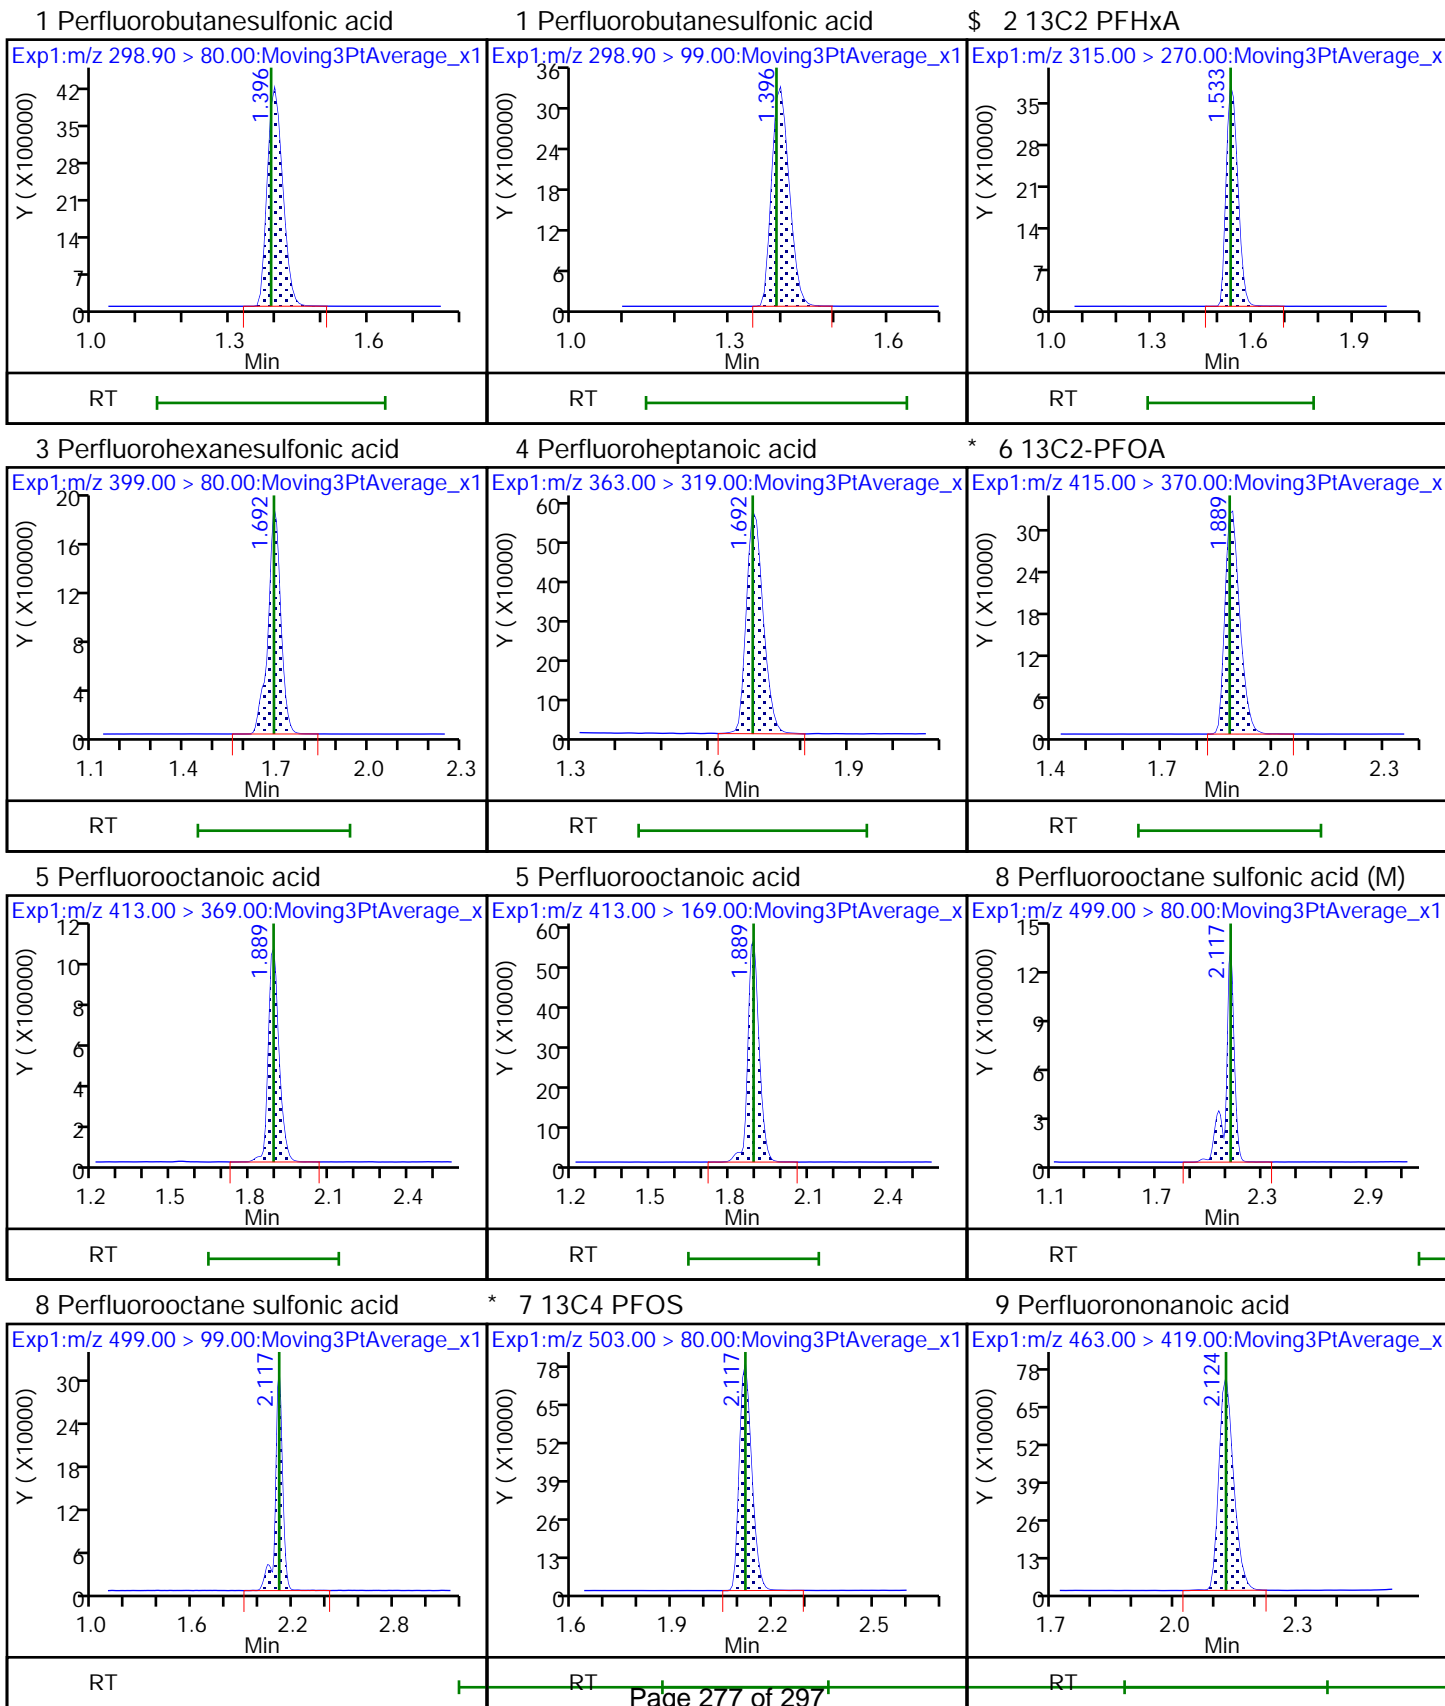

\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_020.d
 Lims ID: 320-38382-A-1-B MS
 Client ID: NAWC-041918-RW-154
 Sample Type: MS
 Inject. Date: 01-May-2018 12:38:43 ALS Bottle#: 13 Worklist Smp#: 18
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-38382-a-1-b ms
 Misc. Info.: Plate: 1 Rack: 6
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 02-May-2018 10:24:00 Calib Date: 11-Apr-2018 12:09:09
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK005

First Level Reviewer: barnettj Date: 01-May-2018 17:13:21

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	9.60	95.96
\$ 10 13C2 PFDA	10.0	8.38	83.76

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_020.d
Injection Date: 01-May-2018 12:38:43 Instrument ID: A8_N
Lims ID: 320-38382-A-1-B MS
Client ID: NAWC-041918-RW-154
Operator ID: SACINSTLCMS01 ALS Bottle#: 13 Worklist Smp#: 18
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.12

Processing Integration Results

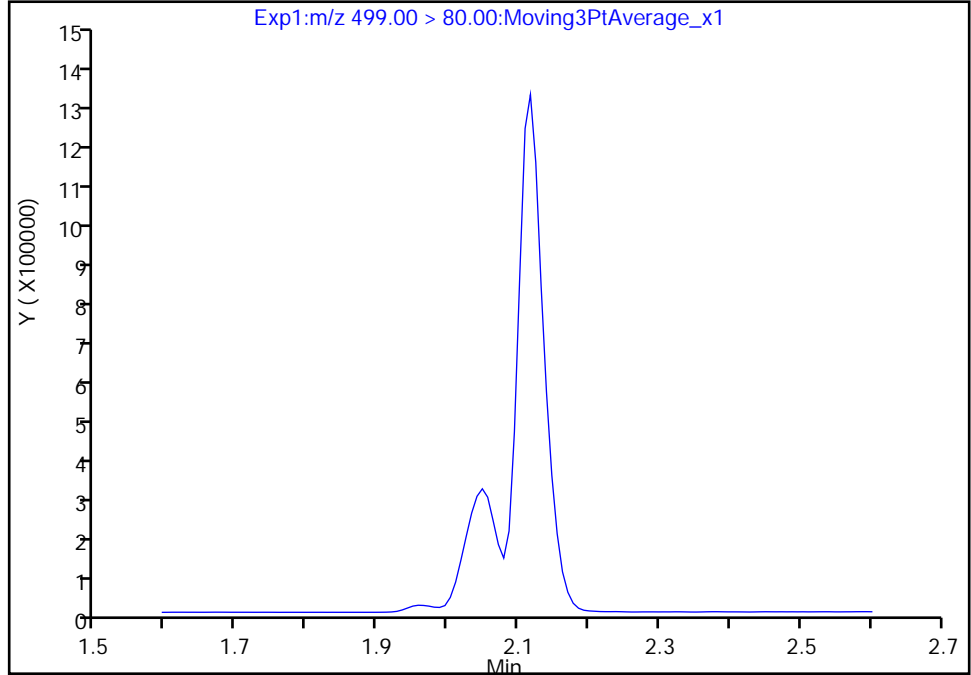

RT: 2.12
Area: 4411041
Amount: 59.936504
Amount Units: ng/ml

Manual Integration Results

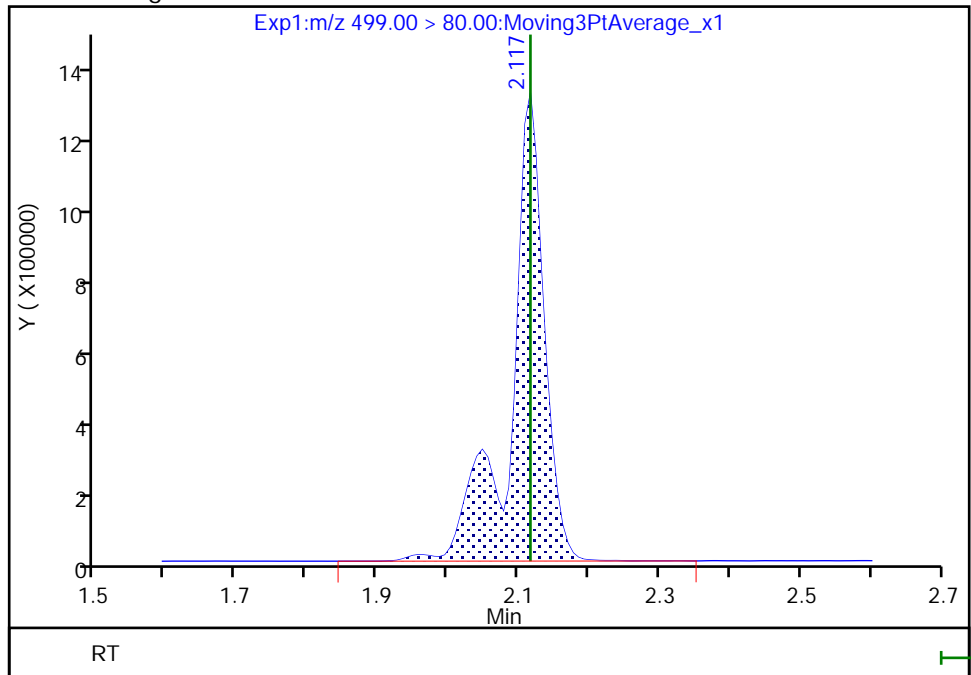

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Client Sample ID: NAWC-041918-RW-154 MSD Lab Sample ID: 320-38382-1 MSD
 Matrix: Water Lab File ID: 2018.05.01_537AA_021.d
 Analysis Method: 537 Date Collected: 04/19/2018 09:10
 Extraction Method: 537 Date Extracted: 04/26/2018 09:35
 Sample wt/vol: 252.6(mL) Date Analyzed: 05/01/2018 12:43
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 220845 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	185	M	40	16	6.7
335-67-1	Perfluorooctanoic acid (PFOA)	89.8	J1	20	7.9	2.8
375-95-1	Perfluorononanoic acid (PFNA)	77.7		24	20	7.9
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	116	J1	30	12	5.4
375-85-9	Perfluoroheptanoic acid (PFHpA)	41.1	J1	9.9	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	347	J1	89	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	66	Q	70-130
STL00996	13C2 PFDA	74		70-130

TestAmerica Sacramento
Target Compound Quantitation Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_021.d
 Lims ID: 320-38382-A-1-C MSD
 Client ID: NAWC-041918-RW-154
 Sample Type: MSD
 Inject. Date: 01-May-2018 12:43:24 ALS Bottle#: 14 Worklist Smp#: 19
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-38382-a-1-c msd
 Misc. Info.: Plate: 1 Rack: 6
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 02-May-2018 10:24:00 Calib Date: 11-Apr-2018 12:09:09
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK005

First Level Reviewer: barnettj Date: 01-May-2018 17:13:31

Signal	RT	EXP RT	DLT RT	REL RT	Response	Amount ng/ml	Ratio(Limits)	S/N	Flags
1 Perfluorobutanesulfonic acid									
298.90 > 80.00	1.396	1.388	0.008	1.000	7034097	87.7		4895	
298.90 > 99.00	1.396	1.388	0.008	1.000	5263368		1.34(0.00-0.00)	4905	
\$ 2 13C2 PFHxA									
315.00 > 270.00	1.540	1.533	0.007	1.000	650324	6.60		5325	
3 Perfluorohexanesulfonic acid									
399.00 > 80.00	1.699	1.692	0.007	1.000	3671426	29.3		1099	
4 Perfluoroheptanoic acid									
363.00 > 319.00	1.699	1.692	0.007	1.000	1033952	10.4		88.3	
* 6 13C2-PFOA									
415.00 > 370.00	1.889	1.882	0.007		927451	10.0		6387	
5 Perfluorooctanoic acid									
413.00 > 369.00	1.889	1.889	0.0	1.000	2235765	22.7		295	
413.00 > 169.00	1.889	1.889	0.0	1.000	1199634		1.86(0.00-0.00)	1222	
8 Perfluorooctane sulfonic acid									
499.00 > 80.00	2.117	2.117	0.0	1.000	3802069	46.8		993	a
499.00 > 99.00	2.117	2.117	0.0	1.000	797111		4.77(0.00-0.00)	1309	a
* 7 13C4 PFOS									
503.00 > 80.00	2.117	2.117	0.0		2186239	28.7		1195	
9 Perfluorononanoic acid									
463.00 > 419.00	2.124	2.124	0.0	1.000	1533567	19.6		207	
\$ 10 13C2 PFDA									
515.00 > 470.00	2.269	2.269	0.0	1.000	587015	7.44		5328	





QC Flag Legend

Review Flags


a - User Assigned ID

TestAmerica Sacramento

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_021.d
Injection Date: 01-May-2018 12:43:24 Instrument ID: A8_N
Lims ID: 320-38382-A-1-C MSD
Client ID: NAWC-041918-RW-154
Operator ID: SACINSTLCMS01 ALS Bottle#: 14 Worklist Smp#: 19
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL

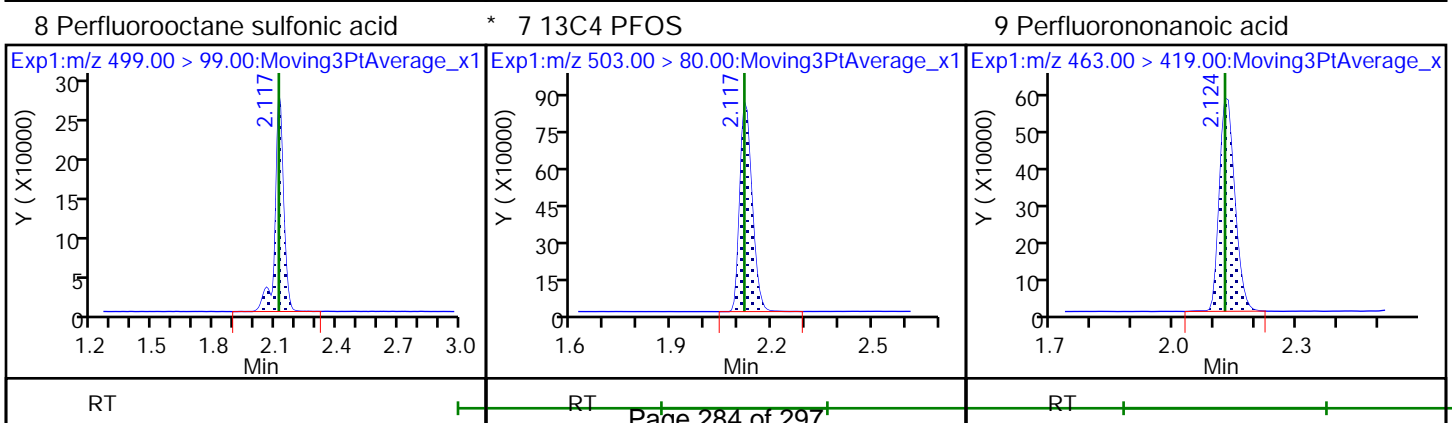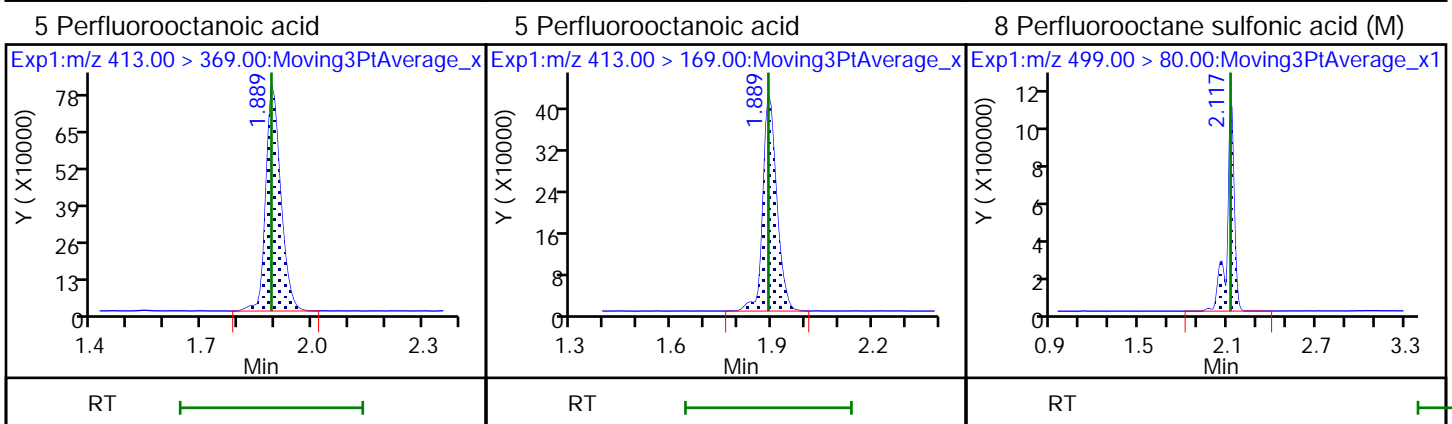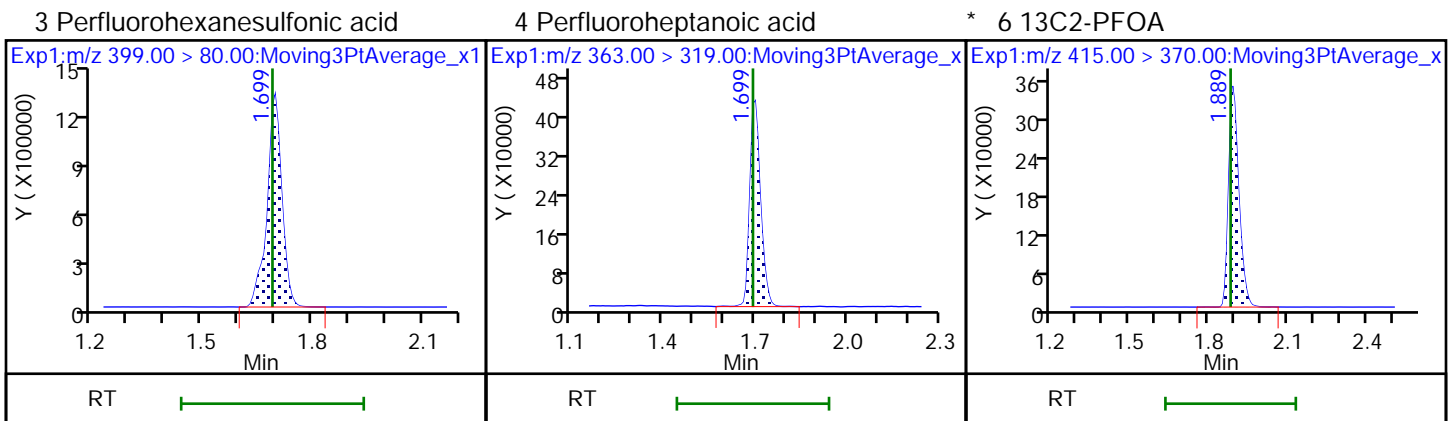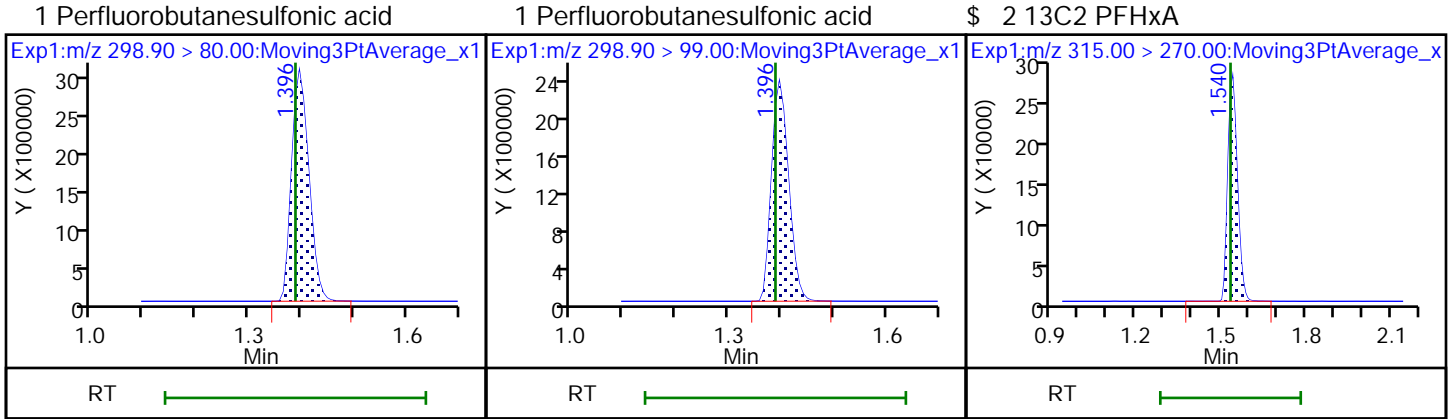

\$ 10 13C2 PFDA



TestAmerica Sacramento
Recovery Report

Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_021.d
 Lims ID: 320-38382-A-1-C MSD
 Client ID: NAWC-041918-RW-154
 Sample Type: MSD
 Inject. Date: 01-May-2018 12:43:24 ALS Bottle#: 14 Worklist Smp#: 19
 Injection Vol: 2.0 ul Dil. Factor: 1.0000
 Sample Info: 320-38382-a-1-c msd
 Misc. Info.: Plate: 1 Rack: 6
 Operator ID: SACINSTLCMS01 Instrument ID: A8_N
 Method: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\537_A8_N.m
 Limit Group: LC 537 ICAL
 Last Update: 02-May-2018 10:24:00 Calib Date: 11-Apr-2018 12:09:09
 Integrator: Picker
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\ChromNA\Sacramento\ChromData\A8_N\20180411-56557.b\2018.04.11_537ICALB_009.d
 Column 1 : Det: EXP1
 Process Host: XAWRK005

First Level Reviewer: barnettj Date: 01-May-2018 17:13:31

Compound	Amount Added	Amount Recovered	% Rec.
\$ 2 13C2 PFHxA	10.0	6.60	65.95
\$ 10 13C2 PFDA	10.0	7.44	74.42

TestAmerica Sacramento


Data File: \\ChromNa\Sacramento\ChromData\A8_N\20180501-57508.b\2018.05.01_537AA_021.d
Injection Date: 01-May-2018 12:43:24 Instrument ID: A8_N
Lims ID: 320-38382-A-1-C MSD
Client ID: NAWC-041918-RW-154
Operator ID: SACINSTLCMS01 ALS Bottle#: 14 Worklist Smp#: 19
Injection Vol: 2.0 ul Dil. Factor: 1.0000
Method: 537_A8_N Limit Group: LC 537 ICAL
Column: Detector EXP1

8 Perfluorooctane sulfonic acid, CAS: 1763-23-1

Signal: 1


Not Detected
Expected RT: 2.12

Processing Integration Results

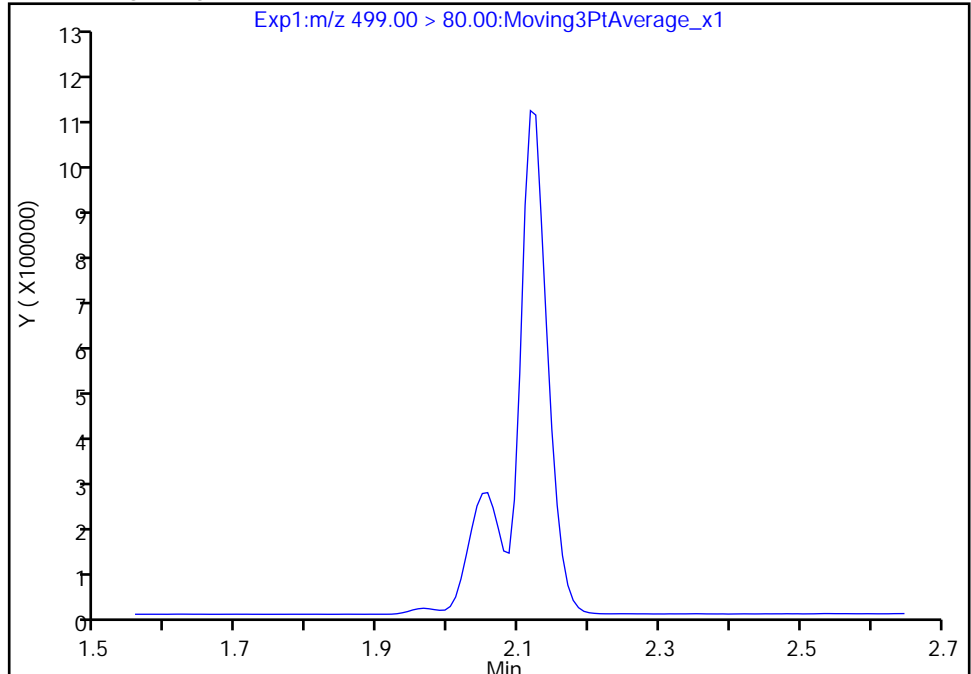

RT: 2.12
Area: 3802069
Amount: 46.785859
Amount Units: ng/ml

Manual Integration Results

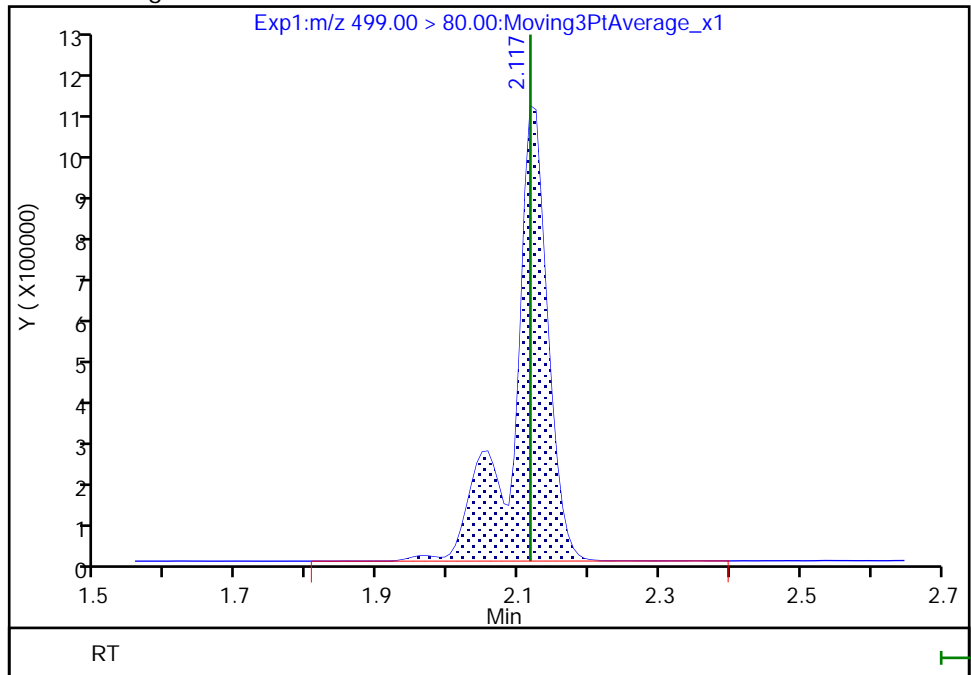

LCMS ANALYSIS RUN LOG

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1

SDG No.: _____

Instrument ID: A8_N Start Date: 04/11/2018 11:45

Analysis Batch Number: 217453 End Date: 04/11/2018 12:27

LAB SAMPLE ID	CLIENT SAMPLE ID	DATE ANALYZED	DILUTION FACTOR	LAB FILE ID	COLUMN ID
IC 320-217453/3		04/11/2018 11:45	1	2018.04.11_537I CALB 004.d	GeminiC18 3x100 3(mm)
IC 320-217453/4		04/11/2018 11:50	1	2018.04.11_537I CALB 005.d	GeminiC18 3x100 3(mm)
IC 320-217453/5		04/11/2018 11:55	1	2018.04.11_537I CALB 006.d	GeminiC18 3x100 3(mm)
IC 320-217453/6 ICISAV		04/11/2018 11:59	1	2018.04.11_537I CALB 007.d	GeminiC18 3x100 3(mm)
IC 320-217453/7		04/11/2018 12:04	1	2018.04.11_537I CALB 008.d	GeminiC18 3x100 3(mm)
IC 320-217453/8		04/11/2018 12:09	1	2018.04.11_537I CALB 009.d	GeminiC18 3x100 3(mm)
ZZZZZ		04/11/2018 12:13	1		GeminiC18 3x100 3(mm)
CCVL 320-217453/10		04/11/2018 12:18	1	2018.04.11_537I CALB 011.d	GeminiC18 3x100 3(mm)
ICB 320-217453/11		04/11/2018 12:23	1		GeminiC18 3x100 3(mm)
ICV 320-217453/12		04/11/2018 12:27	1	2018.04.11_537I CALB 013.d	GeminiC18 3x100 3(mm)

LCMS ANALYSIS RUN LOG

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1

SDG No.: _____

Instrument ID: A8_N Start Date: 05/01/2018 11:19

Analysis Batch Number: 220842 End Date: 05/01/2018 12:15

LAB SAMPLE ID	CLIENT SAMPLE ID	DATE ANALYZED	DILUTION FACTOR	LAB FILE ID	COLUMN ID
CCVL 320-220842/1		05/01/2018 11:19	1	2018.05.01_537A A 003.d	GeminiC18 3x100 3(mm)
CCV 320-220842/13 CCVIS		05/01/2018 12:15	1		GeminiC18 3x100 3(mm)

LCMS ANALYSIS RUN LOG

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1

SDG No.: _____

Instrument ID: A8_N Start Date: 05/01/2018 12:15

Analysis Batch Number: 220845 End Date: 05/01/2018 13:11

LAB SAMPLE ID	CLIENT SAMPLE ID	DATE ANALYZED	DILUTION FACTOR	LAB FILE ID	COLUMN ID
CCV 320-220845/13 CCVIS		05/01/2018 12:15	1	2018.05.01_537A A 015.d	GeminiC18 3x100 3(mm)
MB 320-219896/1-A		05/01/2018 12:24	1	2018.05.01_537A A 017.d	GeminiC18 3x100 3(mm)
LCS 320-219896/2-A		05/01/2018 12:29	1	2018.05.01_537A A 018.d	GeminiC18 3x100 3(mm)
320-38382-1		05/01/2018 12:34	1	2018.05.01_537A A 019.d	GeminiC18 3x100 3(mm)
320-38382-1 MS		05/01/2018 12:38	1	2018.05.01_537A A 020.d	GeminiC18 3x100 3(mm)
320-38382-1 MSD		05/01/2018 12:43	1	2018.05.01_537A A 021.d	GeminiC18 3x100 3(mm)
320-38382-2		05/01/2018 12:48	1	2018.05.01_537A A 022.d	GeminiC18 3x100 3(mm)
320-38382-3		05/01/2018 12:52	1	2018.05.01_537A A 023.d	GeminiC18 3x100 3(mm)
320-38382-4		05/01/2018 12:57	1	2018.05.01_537A A 024.d	GeminiC18 3x100 3(mm)
320-38382-5		05/01/2018 13:02	1	2018.05.01_537A A 025.d	GeminiC18 3x100 3(mm)
320-38382-6		05/01/2018 13:06	1	2018.05.01_537A A 026.d	GeminiC18 3x100 3(mm)
CCV 320-220845/25 CCVIS		05/01/2018 13:11	1	2018.05.01_537A A 027.d	GeminiC18 3x100 3(mm)

LCMS ANALYSIS RUN LOG

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1

SDG No.: _____

Instrument ID: A8_N Start Date: 05/01/2018 13:11

Analysis Batch Number: 220847 End Date: 05/01/2018 13:30

LAB SAMPLE ID	CLIENT SAMPLE ID	DATE ANALYZED	DILUTION FACTOR	LAB FILE ID	COLUMN ID
CCV 320-220847/25 CCVIS		05/01/2018 13:11	1	2018.05.01_537A A 027.d	GeminiC18 3x100 3(mm)
320-38382-7		05/01/2018 13:20	1	2018.05.01_537A A 029.d	GeminiC18 3x100 3(mm)
320-38382-8		05/01/2018 13:25	1	2018.05.01_537A A 030.d	GeminiC18 3x100 3(mm)
CCV 320-220847/29 CCVIS		05/01/2018 13:30	1	2018.05.01_537A A 031.d	GeminiC18 3x100 3(mm)

LCMS BATCH WORKSHEET

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1

SDG No.: _____

Batch Number: 219896 Batch Start Date: 04/26/18 09:25 Batch Analyst: Long, Tyrel W

Batch Method: 537 Batch End Date: 04/30/18 11:05

Lab Sample ID	Client Sample ID	Method Chain	Basis	GrossWeight	TareWeight	InitialAmount	FinalAmount	ReceivedpH	LC537-HSP 00029
MB 320-219896/1		537, 537				250 mL	1.00 mL	7 SU	
LCS 320-219896/2		537, 537				250 mL	1.00 mL	7 SU	100 uL
320-38382-A-1	NAWC-041918-RW-154	537, 537	T	281.45 g	29.28 g	252.2 mL	1.00 mL	7 SU	
320-38382-A-1	NAWC-041918-RW-154	537, 537	T	281.43 g	28.91 g	252.5 mL	1.00 mL	7 SU	100 uL
320-38382-A-1	NAWC-041918-RW-154	537, 537	T	281.19 g	28.59 g	252.6 mL	1.00 mL	7 SU	100 uL
320-38382-A-2	NAWC-041918-FRB-154	537, 537	T	296.44 g	29.79 g	266.7 mL	1.00 mL	7 SU	
320-38382-A-3	NAWC-041918-RW-146	537, 537	T	233.47 g	28.65 g	204.8 mL	1.00 mL	7 SU	
320-38382-A-4	NAWC-041918-FRB-146	537, 537	T	293.49 g	29.87 g	263.6 mL	1.00 mL	7 SU	
320-38382-A-5	NAWC-041918-RW-258	537, 537	T	290.55 g	29.67 g	260.9 mL	1.00 mL	7 SU	
320-38382-A-6	NAWC-041918-FRB-258	537, 537	T	295.41 g	27.84 g	267.6 mL	1.00 mL	7 SU	
320-38382-A-7	WGNA-041918-RW-3571	537, 537	T	306.16 g	28.97 g	277.2 mL	1.00 mL	7 SU	
320-38382-A-8	WGNA-041918-FRB-3571	537, 537	T	262.80 g	28.26 g	234.5 mL	1.00 mL	7 SU	

Lab Sample ID	Client Sample ID	Method Chain	Basis	LC537-IS 00068	LC537-SU 00066	AnalysisComment			
MB 320-219896/1		537, 537		100 uL	100 uL	Chlorine ND			
LCS 320-219896/2		537, 537		100 uL	100 uL	Chlorine ND			
320-38382-A-1	NAWC-041918-RW-154	537, 537	T	100 uL	100 uL	Chlorine ND			
320-38382-A-1	NAWC-041918-RW-154	537, 537	T	100 uL	100 uL	Chlorine ND			

The pound sign (#) in the amount added field denotes that the reagent was used undiluted. All calculations are performed using the stated concentration for this reagent.

LCMS BATCH WORKSHEET

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1

SDG No.: _____

Batch Number: 219896 Batch Start Date: 04/26/18 09:25 Batch Analyst: Long, Tyrel W

Batch Method: 537 Batch End Date: 04/30/18 11:05

Lab Sample ID	Client Sample ID	Method Chain	Basis	LC537-IS 00068	LC537-SU 00066	AnalysisComment			
320-38382-A-1 MSD	NAWC-041918-RW-1 54	537, 537	T	100 uL	100 uL	Chlorine ND The following sample was observed to have some opaque residue on the bottom of the centrifuge tube after extraction when the sample were brought to final volume.			
320-38382-A-2	NAWC-041918-FRB- 154	537, 537	T	100 uL	100 uL	Chlorine ND			
320-38382-A-3	NAWC-041918-RW-1 46	537, 537	T	100 uL	100 uL	Chlorine ND			
320-38382-A-4	NAWC-041918-FRB- 146	537, 537	T	100 uL	100 uL	Chlorine ND			
320-38382-A-5	NAWC-041918-RW-2 58	537, 537	T	100 uL	100 uL	Chlorine ND			
320-38382-A-6	NAWC-041918-FRB- 258	537, 537	T	100 uL	100 uL	Chlorine ND			
320-38382-A-7	WGNA-041918-RW-3 571	537, 537	T	100 uL	100 uL	Chlorine ND			
320-38382-A-8	WGNA-041918-FRB- 3571	537, 537	T	100 uL	100 uL	Chlorine ND			

The pound sign (#) in the amount added field denotes that the reagent was used undiluted. All calculations are performed using the stated concentration for this reagent.

LCMS BATCH WORKSHEET

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1

SDG No.: _____

Batch Number: 219896 Batch Start Date: 04/26/18 09:25 Batch Analyst: Long, Tyrel W

Batch Method: 537 Batch End Date: 04/30/18 11:05

Batch Notes	
Analyst ID - Aliquot Step	VPM
Analyst ID - Concentration	SKD/VPM
Analyst ID - Final Volume Step	VPM
Internal Standard ID#	1223393
Manifold ID	4
Methanol ID	1217927
pH Indicator ID	3817
Pipette ID	R40536G
Analyst ID - IS Reagent Drop	VPM
Analyst ID - IS Reagent Drop Witness	TWL
Analyst ID - SU Reagent Drop	TWL
Analyst ID - SU Reagent Drop Witness	HJA
Analyst ID - TA Reagent Drop	TWL
Analyst ID - TA Reagent Drop Witness	HJA
SPE Cartridge Lot ID	6369499-12
Trizma ID	SLBR5241V
Reagent Water ID	04/21/18

Basis	Basis Description
T	Total/NA

The pound sign (#) in the amount added field denotes that the reagent was used undiluted. All calculations are performed using the stated concentration for this reagent.

Shipping and Receiving Documents

Chain of Custody Record

TestAmerica Sacramento
 880 Riverside Parkway
 West Sacramento, CA 95605-1500
 phone 916.373.5600 fax 303.467.7248

TestAmerica
 THE LEADER IN ENVIRONMENTAL TESTING
 TestAmerica Laboratories, Inc.

Client Contact
 TetraTech
 234 Mall Boulevard Suite 260
 King of Prussia, PA 19406
 610-382-1174
 610-491-9688
 Project Name: WEO4
 Site: WEO4
 P.O # 1132358 (through EarthToxics)

Regulatory Program: DW IMPDES RCRA Other: _____
 Regulatory Manager: Andy Frebowitz
 Tel/Fax: 610.382.1170
 Analysis Turnaround Time
 CALENDAR DAYS WORKING DAYS
 TAT if different from Below 21
 2 weeks
 1 week
 2 days
 1 day

Site Contact: Mary Kay Bond Lab Contact: Dave Alllucker
 Date: 4/19/2018 Carrier: FedEx
 COC No: 1 of 1 COCs
 Sampler: Mary Kay Bond
 For Lab Use Only:
 Walk-in Client: _____
 Lab Sampling: _____
 Job / SDG No.: _____

Sample Identification	Sample Date	Sample Time	Sample Type (C=Comp, G=Grab)	Matrix	# of Cont.	Filtered Sample (Y/N)	Perform MS / MSD (Y/N)	EPA 537 UCMR3	Sample Specific Notes:
NAWC-041918-RW-154	4/19/2018	9:10	G	DW	6	N	N	Y	MS/MSD
NAWC-041918-FRB-154	4/19/2018	9:05	G	DW	2	N	N	Y	Field Reagent Blank
NAWC-041918-RW-146	4/19/2018	10:10	G	DW	2	N	N	Y	Field Reagent Blank
NAWC-041918-FRB-146	4/19/2018	10:05	G	DW	2	N	N	Y	Field Reagent Blank
NAWC-041918-RW-258	4/19/2018	10:40	G	DW	2	N	N	Y	Field Reagent Blank
NAWC-041918-FRB-258	4/19/2018	10:35	G	DW	2	N	N	Y	Field Reagent Blank
WGNA-041918-RW-3571	4/19/2018	11:10	G	DW	2	N	N	Y	Field Reagent Blank
WGNA-041918-FRB-3571	4/19/2018	11:05	G	DW	2	N	N	Y	Field Reagent Blank
Preservation Used: 1= Ice, 2= HCl; 3= H2SO4; 4=HNO3; 5=NaOH; 6= Other: Trizma						6			

Possible Hazard Identification:
 Are any samples from a listed EPA Hazardous Waste? Please List any EPA Waste Codes for the sample in the
 Non-Hazard Flammable Skin Irritant Poison B Unknown
 Fed Ex Tracking: 7720 4058 7199

Sample Disposal (A fee may be assessed if samples are retained longer than 1 month)
 Return to Client Disposal by Lab Archive for _____ Months

Custody Seal No.: _____
 Company: Tetra Tech
 Date/Time: 4/19/2018 16:00
 Relinquished by: *Mary Kay Bond*
 Date/Time: 4/20/18 0920
 Relinquished by: _____
 Date/Time: _____
 Relinquished by: _____
 Date/Time: _____

Therm ID No.: *AK-5* *ice*
 Cooler Temp. (°C): Obs'd: *0.0* Corr'd: _____
 Company: *PA-SAC*
 Company: _____
 Company: _____



320-36382 Chain of Custody

Login Sample Receipt Checklist

Client: Tetra Tech, Inc.

Job Number: 320-38382-1

Login Number: 38382
List Number: 1
Creator: Turpen, Troy

List Source: TestAmerica Sacramento

Question	Answer	Comment
Radioactivity wasn't checked or is \leq background as measured by a survey meter.	True	
The cooler's custody seal, if present, is intact.	True	094866, 094865
Sample custody seals, if present, are intact.	N/A	
The cooler or samples do not appear to have been compromised or tampered with.	True	
Samples were received on ice.	True	
Cooler Temperature is acceptable.	True	
Cooler Temperature is recorded.	True	
COC is present.	True	
COC is filled out in ink and legible.	True	
COC is filled out with all pertinent information.	True	
Is the Field Sampler's name present on COC?	True	
There are no discrepancies between the containers received and the COC.	True	
Samples are received within Holding Time (excluding tests with immediate HTs)	True	
Sample containers have legible labels.	True	
Containers are not broken or leaking.	True	
Sample collection date/times are provided.	True	
Appropriate sample containers are used.	True	
Sample bottles are completely filled.	True	
Sample Preservation Verified.	N/A	
There is sufficient vol. for all requested analyses, incl. any requested MS/MSDs	True	
Containers requiring zero headspace have no headspace or bubble is $<6\text{mm}$ (1/4").	True	
Multiphasic samples are not present.	True	
Samples do not require splitting or compositing.	True	
Residual Chlorine Checked.	N/A	

"NAWC-041918-RW-154", "537", "RES", "320-38382-1", "TALSAC", "1763-23-1", "Perfluorooctanesulfonic acid (PFOS)", "17", "ng/L", "J M", "6.7", "DL", "", "TRG", "", "", "40", "LOQ", "YES", "-99", "", "252.2", "1.00", "16", ""

"NAWC-041918-RW-154", "537", "RES", "320-38382-1", "TALSAC", "335-67-1", "Perfluorooctanoic acid (PFOA)", "24", "ng/L", "", "2.8", "DL", "", "TRG", "", "", "20", "LOQ", "YES", "-99", "", "252.2", "1.00", "7.9", ""

"NAWC-041918-RW-154", "537", "RES", "320-38382-1", "TALSAC", "355-46-4", "Perfluorohexanesulfonic acid (PFHxS)", "12", "ng/L", "U M", "5.5", "DL", "", "TRG", "", "", "30", "LOQ", "YES", "-99", "", "252.2", "1.00", "12", ""

"NAWC-041918-RW-154", "537", "RES", "320-38382-1", "TALSAC", "375-73-5", "Perfluorobutanesulfonic acid (PFBS)", "36", "ng/L", "U", "16", "DL", "", "TRG", "", "", "89", "LOQ", "YES", "-99", "", "252.2", "1.00", "36", ""

"NAWC-041918-RW-154", "537", "RES", "320-38382-1", "TALSAC", "375-85-9", "Perfluoroheptanoic acid (PFHpA)", "8.1", "ng/L", "J", "1.9", "DL", "", "TRG", "", "", "9.9", "LOQ", "YES", "-99", "", "252.2", "1.00", "4.0", ""

"NAWC-041918-RW-154", "537", "RES", "320-38382-1", "TALSAC", "375-95-1", "Perfluorononanoic acid (PFNA)", "20", "ng/L", "U M", "7.9", "DL", "", "TRG", "", "", "24", "LOQ", "YES", "-99", "", "252.2", "1.00", "20", ""

"NAWC-041918-RW-154", "537", "RES", "320-38382-1", "TALSAC", "STL00993", "13C2 PFHxA", "39", "ng/L", "", "-99", "DL", "", "SURR", "100", "", "-99", "LOQ", "YES", "39.7", "", "252.2", "1.00", "0", ""

"NAWC-041918-RW-154", "537", "RES", "320-38382-1", "TALSAC", "STL00996", "13C2 PFDA", "35", "ng/L", "", "-99", "DL", "", "SURR", "89", "", "-99", "LOQ", "YES", "39.7", "", "252.2", "1.00", "0", ""

"NAWC-041918-RW-154MS", "537", "RES", "320-38382-1MS", "TALSAC", "1763-23-1", "Perfluorooctanesulfonic acid (PFOS)", "237", "ng/L", "M", "6.7", "DL", "", "SPK", "102", "", "40", "LOQ", "YES", "217", "NAWC-041918-RW-154", "252.5", "1.00", "16", ""

"NAWC-041918-RW-154MS", "537", "RES", "320-38382-1MS", "TALSAC", "335-67-1", "Perfluorooctanoic acid (PFOA)", "124", "ng/L", "", "2.8", "DL", "", "SPK", "92", "", "20", "LOQ", "YES", "109", "NAWC-041918-RW-154", "252.5", "1.00", "7.9", ""

"NAWC-041918-RW-154MS", "537", "RES", "320-38382-1MS", "TALSAC", "355-46-4", "Perfluorohexanesulfonic acid (PFHxS)", "177", "ng/L", "", "5.4", "DL", "", "SPK", "106", "", "30", "LOQ", "YES", "166", "NAWC-041918-RW-154", "252.5", "1.00", "12", ""

"NAWC-041918-RW-154MS", "537", "RES", "320-38382-1MS", "TALSAC", "375-73-5", "Perfluorobutanesulfonic acid (PFBS)", "523", "ng/L", "", "16", "DL", "", "SPK", "105", "", "89", "LOQ", "YES", "495", "NAWC-041918-RW-154", "252.5", "1.00", "36", ""

"NAWC-041918-RW-154MS", "537", "RES", "320-38382-1MS", "TALSAC", "375-85-9", "Perfluoroheptanoic acid (PFHpA)", "59.8", "ng/L", "", "1.9", "DL", "", "SPK", "97", "", "9.9", "LOQ", "YES", "53.5", "NAWC-041918-RW-154", "252.5", "1.00", "4.0", ""

"NAWC-041918-RW-154MS", "537", "RES", "320-38382-1MS", "TALSAC", "375-95-1", "Perfluorononanoic acid (PFNA)", "98.7", "ng/L", "", "7.9", "DL", "", "SPK", "91", "", "24", "LOQ", "YES", "109", "NAWC-041918-RW-154", "252.5", "1.00", "20", ""

"NAWC-041918-RW-154MS", "537", "RES", "320-38382-1MS", "TALSAC", "STL00993", "13C2 PFHxA", "38.0", "ng/L", "", "-99", "DL", "", "SURR", "96", "", "-99", "LOQ", "YES", "39.6", "NAWC-041918-RW-154", "252.5", "1.00", "0", ""

"NAWC-041918-RW-154MS", "537", "RES", "320-38382-1MS", "TALSAC", "STL00996", "13C2 PFDA", "33.2", "ng/L", "", "-99", "DL", "", "SURR", "84", "", "-99", "LOQ", "YES", "39.6", "NAWC-041918-RW-154", "252.5", "1.00", "0", ""

"NAWC-041918-RW-154MSD", "537", "RES", "320-38382-1MSD", "TALSAC", "1763-23-1", "Perfluorooctanesulfonic acid (PFOS)", "185", "ng/L", "M", "6.7", "DL", "", "SPK", "78", "25", "40", "LOQ", "YES", "217", "NAWC-041918-RW-154", "252.6", "1.00", "16", ""

"NAWC-041918-RW-154MSD", "537", "RES", "320-38382-1MSD", "TALSAC", "335-67-1", "Perfluorooctanoic acid (PFOA)", "89.8", "ng/L", "J1", "2.8", "DL", "", "SPK", "60", "32", "20", "LOQ", "YES", "109", "NAWC-041918-RW-154", "252.6", "1.00", "7.9", ""

"NAWC-041918-RW-154MSD", "537", "RES", "320-38382-1MSD", "TALSAC", "355-46-4", "Perfluorohexanesulfonic acid (PFHxS)", "116", "ng/L", "J1", "5.4", "DL", "", "SPK", "70", "41", "30", "LOQ", "YES", "166", "NAWC-041918-RW-154", "252.6", "1.00", "12", ""

"NAWC-041918-RW-154MSD", "537", "RES", "320-38382-1MSD", "TALSAC", "375-73-5", "Perfluorobutanesulfonic acid (PFBS)", "347", "ng/L", "J1", "16", "DL", "", "SPK", "70", "40", "89", "LOQ", "YES", "495", "NAWC-041918-RW-154", "252.6", "1.00", "36", ""

"NAWC-041918-RW-154MSD", "537", "RES", "320-38382-1MSD", "TALSAC", "375-85-9", "Perfluoroheptanoic acid

(PFHpA),"41.1","ng/L","J1","1.9","DL","","SPK","62","37","9.9","LOQ","YES","53.4","NAWC-041918-RW-154","252.6","1.00","4.0",""
"NAWC-041918-RW-154MSD","537","RES","320-38382-1MSD","TALSAC","375-95-1","Perfluorononanoic acid (PFNA)","77.7","ng/L","","7.9","DL","","SPK","71","24","24","LOQ","YES","109","NAWC-041918-RW-154","252.6","1.00","20",""
"NAWC-041918-RW-154MSD","537","RES","320-38382-1MSD","TALSAC","STL00993","13C2 PFHxA","26.1","ng/L","Q","-99","DL","","SURR","66","","-99","LOQ","YES","39.6","NAWC-041918-RW-154","252.6","1.00","0",""
"NAWC-041918-RW-154MSD","537","RES","320-38382-1MSD","TALSAC","STL00996","13C2 PFDA","29.5","ng/L","","-99","DL","","SURR","74","","-99","LOQ","YES","39.6","NAWC-041918-RW-154","252.6","1.00","0",""
"NAWC-041918-FRB-154","537","RES","320-38382-2","TALSAC","1763-23-1","Perfluorooctanesulfonic acid (PFOS)","15","ng/L","U","6.4","DL","","TRG","","","37","LOQ","YES","-99","","266.7","1.00","15",""
"NAWC-041918-FRB-154","537","RES","320-38382-2","TALSAC","335-67-1","Perfluorooctanoic acid (PFOA)","7.5","ng/L","U","2.6","DL","","TRG","","","19","LOQ","YES","-99","","266.7","1.00","7.5",""
"NAWC-041918-FRB-154","537","RES","320-38382-2","TALSAC","355-46-4","Perfluorohexanesulfonic acid (PFHxS)","11","ng/L","U","5.2","DL","","TRG","","","28","LOQ","YES","-99","","266.7","1.00","11",""
"NAWC-041918-FRB-154","537","RES","320-38382-2","TALSAC","375-73-5","Perfluorobutanesulfonic acid (PFBS)","34","ng/L","U","15","DL","","TRG","","","84","LOQ","YES","-99","","266.7","1.00","34",""
"NAWC-041918-FRB-154","537","RES","320-38382-2","TALSAC","375-85-9","Perfluoroheptanoic acid (PFHpA)","3.7","ng/L","U","1.8","DL","","TRG","","","9.4","LOQ","YES","-99","","266.7","1.00","3.7",""
"NAWC-041918-FRB-154","537","RES","320-38382-2","TALSAC","375-95-1","Perfluorononanoic acid (PFNA)","19","ng/L","U","7.5","DL","","TRG","","","22","LOQ","YES","-99","","266.7","1.00","19",""
"NAWC-041918-FRB-154","537","RES","320-38382-2","TALSAC","STL00993","13C2 PFHxA","40","ng/L","","-99","DL","","SURR","106","","-99","LOQ","YES","37.5","","266.7","1.00","0",""
"NAWC-041918-FRB-154","537","RES","320-38382-2","TALSAC","STL00996","13C2 PFDA","32","ng/L","","-99","DL","","SURR","85","","-99","LOQ","YES","37.5","","266.7","1.00","0",""
"NAWC-041918-RW-146","537","RES","320-38382-3","TALSAC","1763-23-1","Perfluorooctanesulfonic acid (PFOS)","14","ng/L","J M","8.3","DL","","TRG","","","49","LOQ","YES","-99","","204.8","1.00","20",""
"NAWC-041918-RW-146","537","RES","320-38382-3","TALSAC","335-67-1","Perfluorooctanoic acid (PFOA)","27","ng/L","","3.4","DL","","TRG","","","24","LOQ","YES","-99","","204.8","1.00","9.8",""
"NAWC-041918-RW-146","537","RES","320-38382-3","TALSAC","355-46-4","Perfluorohexanesulfonic acid (PFHxS)","15","ng/L","U","6.7","DL","","TRG","","","37","LOQ","YES","-99","","204.8","1.00","15",""
"NAWC-041918-RW-146","537","RES","320-38382-3","TALSAC","375-73-5","Perfluorobutanesulfonic acid (PFBS)","44","ng/L","U","20","DL","","TRG","","","110","LOQ","YES","-99","","204.8","1.00","44",""
"NAWC-041918-RW-146","537","RES","320-38382-3","TALSAC","375-85-9","Perfluoroheptanoic acid (PFHpA)","7.0","ng/L","J","2.3","DL","","TRG","","","12","LOQ","YES","-99","","204.8","1.00","4.9",""
"NAWC-041918-RW-146","537","RES","320-38382-3","TALSAC","375-95-1","Perfluorononanoic acid (PFNA)","24","ng/L","U","9.8","DL","","TRG","","","29","LOQ","YES","-99","","204.8","1.00","24",""
"NAWC-041918-RW-146","537","RES","320-38382-3","TALSAC","STL00993","13C2 PFHxA","49","ng/L","","-99","DL","","SURR","100","","-99","LOQ","YES","48.8","","204.8","1.00","0",""
"NAWC-041918-RW-146","537","RES","320-38382-3","TALSAC","STL00996","13C2 PFDA","41","ng/L","","-99","DL","","SURR","83","","-99","LOQ","YES","48.8","","204.8","1.00","0",""
"NAWC-041918-FRB-146","537","RES","320-38382-4","TALSAC","1763-23-1","Perfluorooctanesulfonic acid (PFOS)","15","ng/L","U","6.4","DL","","TRG","","","38","LOQ","YES","-99","","263.6","1.00","15",""
"NAWC-041918-FRB-146","537","RES","320-38382-4","TALSAC","335-67-1","Perfluorooctanoic acid (PFOA)","7.6","ng/L","U","2.7","DL","","TRG","","","19","LOQ","YES","-99","","263.6","1.00","7.6",""
"NAWC-041918-FRB-146","537","RES","320-38382-4","TALSAC","355-46-4","Perfluorohexanesulfonic acid (PFHxS)","11","ng/L","U","5.2","DL","","TRG","","","28","LOQ","YES","-99","","263.6","1.00","11",""
"NAWC-041918-FRB-146","537","RES","320-38382-4","TALSAC","375-73-5","Perfluorobutanesulfonic acid (PFBS)","34","ng/L","U","15","DL","","TRG","","","85","LOQ","YES","-99","","263.6","1.00","34",""
"NAWC-041918-FRB-146","537","RES","320-38382-4","TALSAC","375-85-9","Perfluoroheptanoic acid (PFHpA)","3.8","ng/L","U","1.8","DL","","TRG","","","9.5","LOQ","YES","-99","","263.6","1.00","3.8",""
"NAWC-041918-FRB-146","537","RES","320-38382-4","TALSAC","375-95-1","Perfluorononanoic acid

(PFNA),"19","ng/L","U","7.6","DL","","TRG","","","23","LOQ","YES","-99","","263.6","1.00","19","","
"NAWC-041918-FRB-146","537","RES","320-38382-4","TALSAC","STL00993","13C2
PFHxA","40","ng/L","","-99","DL","","SURR","106","","-99","LOQ","YES","37.9","","263.6","1.00","0","","
"NAWC-041918-FRB-146","537","RES","320-38382-4","TALSAC","STL00996","13C2
PFDA","33","ng/L","","-99","DL","","SURR","88","","-99","LOQ","YES","37.9","","263.6","1.00","0","","
"NAWC-041918-RW-258","537","RES","320-38382-5","TALSAC","1763-23-1","Perfluorooctanesulfonic acid
(PFOS)","16","ng/L","J M","6.5","DL","","TRG","","","38","LOQ","YES","-99","","260.9","1.00","15","","
"NAWC-041918-RW-258","537","RES","320-38382-5","TALSAC","335-67-1","Perfluorooctanoic acid
(PFOA)","20","ng/L","","2.7","DL","","TRG","","","19","LOQ","YES","-99","","260.9","1.00","7.7","","
"NAWC-041918-RW-258","537","RES","320-38382-5","TALSAC","355-46-4","Perfluorohexanesulfonic acid
(PFHxS)","11","ng/L","U M","5.3","DL","","TRG","","","29","LOQ","YES","-99","","260.9","1.00","11","","
"NAWC-041918-RW-258","537","RES","320-38382-5","TALSAC","375-73-5","Perfluorobutanesulfonic acid
(PFBS)","34","ng/L","U","15","DL","","TRG","","","86","LOQ","YES","-99","","260.9","1.00","34","","
"NAWC-041918-RW-258","537","RES","320-38382-5","TALSAC","375-85-9","Perfluoroheptanoic acid
(PFHpA)","8.3","ng/L","J","1.8","DL","","TRG","","","9.6","LOQ","YES","-99","","260.9","1.00","3.8","","
"NAWC-041918-RW-258","537","RES","320-38382-5","TALSAC","375-95-1","Perfluorononanoic acid
(PFNA)","10","ng/L","J","7.7","DL","","TRG","","","23","LOQ","YES","-99","","260.9","1.00","19","","
"NAWC-041918-RW-258","537","RES","320-38382-5","TALSAC","STL00993","13C2
PFHxA","38","ng/L","","-99","DL","","SURR","98","","-99","LOQ","YES","38.3","","260.9","1.00","0","","
"NAWC-041918-RW-258","537","RES","320-38382-5","TALSAC","STL00996","13C2
PFDA","31","ng/L","","-99","DL","","SURR","80","","-99","LOQ","YES","38.3","","260.9","1.00","0","","
"NAWC-041918-FRB-258","537","RES","320-38382-6","TALSAC","1763-23-1","Perfluorooctanesulfonic acid
(PFOS)","15","ng/L","U","6.4","DL","","TRG","","","37","LOQ","YES","-99","","267.6","1.00","15","","
"NAWC-041918-FRB-258","537","RES","320-38382-6","TALSAC","335-67-1","Perfluorooctanoic acid
(PFOA)","7.5","ng/L","U","2.6","DL","","TRG","","","19","LOQ","YES","-99","","267.6","1.00","7.5","","
"NAWC-041918-FRB-258","537","RES","320-38382-6","TALSAC","355-46-4","Perfluorohexanesulfonic acid
(PFHxS)","11","ng/L","U","5.1","DL","","TRG","","","28","LOQ","YES","-99","","267.6","1.00","11","","
"NAWC-041918-FRB-258","537","RES","320-38382-6","TALSAC","375-73-5","Perfluorobutanesulfonic acid
(PFBS)","34","ng/L","U","15","DL","","TRG","","","84","LOQ","YES","-99","","267.6","1.00","34","","
"NAWC-041918-FRB-258","537","RES","320-38382-6","TALSAC","375-85-9","Perfluoroheptanoic acid
(PFHpA)","3.7","ng/L","U","1.8","DL","","TRG","","","9.3","LOQ","YES","-99","","267.6","1.00","3.7","","
"NAWC-041918-FRB-258","537","RES","320-38382-6","TALSAC","375-95-1","Perfluorononanoic acid
(PFNA)","19","ng/L","U","7.5","DL","","TRG","","","22","LOQ","YES","-99","","267.6","1.00","19","","
"NAWC-041918-FRB-258","537","RES","320-38382-6","TALSAC","STL00993","13C2
PFHxA","40","ng/L","","-99","DL","","SURR","106","","-99","LOQ","YES","37.4","","267.6","1.00","0","","
"NAWC-041918-FRB-258","537","RES","320-38382-6","TALSAC","STL00996","13C2
PFDA","32","ng/L","","-99","DL","","SURR","85","","-99","LOQ","YES","37.4","","267.6","1.00","0","","
"WGNA-041918-RW-3571","537","RES","320-38382-7","TALSAC","1763-23-1","Perfluorooctanesulfonic acid
(PFOS)","8.0","ng/L","J M","6.1","DL","","TRG","","","36","LOQ","YES","-99","","277.2","1.00","14","","
"WGNA-041918-RW-3571","537","RES","320-38382-7","TALSAC","335-67-1","Perfluorooctanoic acid
(PFOA)","10","ng/L","J","2.5","DL","","TRG","","","18","LOQ","YES","-99","","277.2","1.00","7.2","","
"WGNA-041918-RW-3571","537","RES","320-38382-7","TALSAC","355-46-4","Perfluorohexanesulfonic acid
(PFHxS)","11","ng/L","U M","5.0","DL","","TRG","","","27","LOQ","YES","-99","","277.2","1.00","11","","
"WGNA-041918-RW-3571","537","RES","320-38382-7","TALSAC","375-73-5","Perfluorobutanesulfonic acid
(PFBS)","32","ng/L","U M","15","DL","","TRG","","","81","LOQ","YES","-99","","277.2","1.00","32","","
"WGNA-041918-RW-3571","537","RES","320-38382-7","TALSAC","375-85-9","Perfluoroheptanoic acid
(PFHpA)","12","ng/L","","1.7","DL","","TRG","","","9.0","LOQ","YES","-99","","277.2","1.00","3.6","","
"WGNA-041918-RW-3571","537","RES","320-38382-7","TALSAC","375-95-1","Perfluorononanoic acid
(PFNA)","18","ng/L","U M","7.2","DL","","TRG","","","22","LOQ","YES","-99","","277.2","1.00","18","","
"WGNA-041918-RW-3571","537","RES","320-38382-7","TALSAC","STL00993","13C2
PFHxA","36","ng/L","","-99","DL","","SURR","99","","-99","LOQ","YES","36.1","","277.2","1.00","0","","
"WGNA-041918-RW-3571","537","RES","320-38382-7","TALSAC","STL00996","13C2
PFDA","28","ng/L","","-99","DL","","SURR","79","","-99","LOQ","YES","36.1","","277.2","1.00","0","","
"WGNA-041918-FRB-3571","537","RES","320-38382-8","TALSAC","1763-23-1","Perfluorooctanesulfonic acid

(PFOS),"17","ng/L","U","7.2","DL","","TRG","","","43","LOQ","YES","-99","","234.5","1.00","17",""
"WGNA-041918-FRB-3571","537","RES","320-38382-8","TALSAC","335-67-1","Perfluorooctanoic acid
(PFOA),"8.5","ng/L","U","3.0","DL","","TRG","","","21","LOQ","YES","-99","","234.5","1.00","8.5",""
"WGNA-041918-FRB-3571","537","RES","320-38382-8","TALSAC","355-46-4","Perfluorohexanesulfonic acid
(PFHxS),"13","ng/L","U","5.9","DL","","TRG","","","32","LOQ","YES","-99","","234.5","1.00","13",""
"WGNA-041918-FRB-3571","537","RES","320-38382-8","TALSAC","375-73-5","Perfluorobutanesulfonic acid
(PFBS),"38","ng/L","U","17","DL","","TRG","","","96","LOQ","YES","-99","","234.5","1.00","38",""
"WGNA-041918-FRB-3571","537","RES","320-38382-8","TALSAC","375-85-9","Perfluoroheptanoic acid
(PFHpA),"4.3","ng/L","U","2.0","DL","","TRG","","","11","LOQ","YES","-99","","234.5","1.00","4.3",""
"WGNA-041918-FRB-3571","537","RES","320-38382-8","TALSAC","375-95-1","Perfluorononanoic acid
(PFNA),"21","ng/L","U","8.5","DL","","TRG","","","26","LOQ","YES","-99","","234.5","1.00","21",""
"WGNA-041918-FRB-3571","537","RES","320-38382-8","TALSAC","STL00993","13C2
PFHxA","44","ng/L","","-99","DL","","SURR","103","","-99","LOQ","YES","42.6","","234.5","1.00","0",""
"WGNA-041918-FRB-3571","537","RES","320-38382-8","TALSAC","STL00996","13C2
PFDA","37","ng/L","","-99","DL","","SURR","87","","-99","LOQ","YES","42.6","","234.5","1.00","0",""
"LCS 320-219896/2-A","537","RES","LCS 320-219896/2-A","TALSAC","1763-23-1","Perfluorooctanesulfonic acid
(PFOS),"225","ng/L","M","6.8","DL","","SPK","103","","40","LOQ","YES","220","","250","1.00","16",""
"LCS 320-219896/2-A","537","RES","LCS 320-219896/2-A","TALSAC","335-67-1","Perfluorooctanoic acid
(PFOA),"110","ng/L","","2.8","DL","","SPK","100","","20","LOQ","YES","110","","250","1.00","8.0",""
"LCS 320-219896/2-A","537","RES","LCS 320-219896/2-A","TALSAC","355-46-4","Perfluorohexanesulfonic acid
(PFHxS),"179","ng/L","","5.5","DL","","SPK","106","","30","LOQ","YES","168","","250","1.00","12",""
"LCS 320-219896/2-A","537","RES","LCS 320-219896/2-A","TALSAC","375-73-5","Perfluorobutanesulfonic acid
(PFBS),"519","ng/L","","16","DL","","SPK","104","","90","LOQ","YES","500","","250","1.00","36",""
"LCS 320-219896/2-A","537","RES","LCS 320-219896/2-A","TALSAC","375-85-9","Perfluoroheptanoic acid
(PFHpA),"58.2","ng/L","","1.9","DL","","SPK","108","","10","LOQ","YES","54.0","","250","1.00","4.0",""
"LCS 320-219896/2-A","537","RES","LCS 320-219896/2-A","TALSAC","375-95-1","Perfluorononanoic acid
(PFNA),"102","ng/L","","8.0","DL","","SPK","93","","24","LOQ","YES","110","","250","1.00","20",""
"LCS 320-219896/2-A","537","RES","LCS 320-219896/2-A","TALSAC","STL00993","13C2
PFHxA","43.4","ng/L","","-99","DL","","SURR","108","","-99","LOQ","YES","40.0","","250","1.00","0",""
"LCS 320-219896/2-A","537","RES","LCS 320-219896/2-A","TALSAC","STL00996","13C2
PFDA","36.4","ng/L","","-99","DL","","SURR","91","","-99","LOQ","YES","40.0","","250","1.00","0",""
"MB 320-219896/1-A","537","RES","MB 320-219896/1-A","TALSAC","1763-23-1","Perfluorooctanesulfonic acid
(PFOS),"16","ng/L","U","6.8","DL","","TRG","","","40","LOQ","YES","-99","","250","1.00","16",""
"MB 320-219896/1-A","537","RES","MB 320-219896/1-A","TALSAC","335-67-1","Perfluorooctanoic acid
(PFOA),"8.0","ng/L","U","2.8","DL","","TRG","","","20","LOQ","YES","-99","","250","1.00","8.0",""
"MB 320-219896/1-A","537","RES","MB 320-219896/1-A","TALSAC","355-46-4","Perfluorohexanesulfonic acid
(PFHxS),"12","ng/L","U","5.5","DL","","TRG","","","30","LOQ","YES","-99","","250","1.00","12",""
"MB 320-219896/1-A","537","RES","MB 320-219896/1-A","TALSAC","375-73-5","Perfluorobutanesulfonic acid
(PFBS),"36","ng/L","U","16","DL","","TRG","","","90","LOQ","YES","-99","","250","1.00","36",""
"MB 320-219896/1-A","537","RES","MB 320-219896/1-A","TALSAC","375-85-9","Perfluoroheptanoic acid
(PFHpA),"4.0","ng/L","U","1.9","DL","","TRG","","","10","LOQ","YES","-99","","250","1.00","4.0",""
"MB 320-219896/1-A","537","RES","MB 320-219896/1-A","TALSAC","375-95-1","Perfluorononanoic acid
(PFNA),"20","ng/L","U","8.0","DL","","TRG","","","24","LOQ","YES","-99","","250","1.00","20",""
"MB 320-219896/1-A","537","RES","MB 320-219896/1-A","TALSAC","STL00993","13C2
PFHxA","42.9","ng/L","","-99","DL","","SURR","107","","-99","LOQ","YES","40.0","","250","1.00","0",""
"MB 320-219896/1-A","537","RES","MB 320-219896/1-A","TALSAC","STL00996","13C2
PFDA","35.9","ng/L","","-99","DL","","SURR","90","","-99","LOQ","YES","40.0","","250","1.00","0",""
"Unknown","Unknown","NAWC-041918-RW-154","04/19/2018 09:10","AQ","320-38382-
1","NM","","0.00","537","METHOD","RES","04/26/2018 09:35","05/01/2018
12:34","TALSAC","COA","WET","NA","1","NA","NA","","100","320-219896","320-219896","NA","320-
220845","320-38382-1","04/20/2018 09:20","04/23/2018 10:00",""
"Unknown","Unknown","NAWC-041918-RW-154MS","04/19/2018 09:10","AQ","320-38382-
1MS","MS","","0.00","537","METHOD","RES","04/26/2018 09:35","05/01/2018
12:38","TALSAC","COA","WET","NA","1","NA","NA","","100","320-219896","320-219896","NA","320-

220845","320-38382-1","04/20/2018 09:20","04/23/2018 10:00",""
"Unknown","Unknown","NAWC-041918-RW-154MSD","04/19/2018 09:10","AQ","320-38382-
1MSD","MSD","","0.00","537","METHOD","RES","04/26/2018 09:35","05/01/2018
12:43","TALSAC","COA","WET","NA","1","NA","NA","","100","320-219896","320-219896","NA","320-
220845","320-38382-1","04/20/2018 09:20","04/23/2018 10:00",""
"Unknown","Unknown","NAWC-041918-FRB-154","04/19/2018 09:05","AQ","320-38382-
2","FB","","0.00","537","METHOD","RES","04/26/2018 09:35","05/01/2018
12:48","TALSAC","COA","WET","NA","1","NA","NA","","100","320-219896","320-219896","NA","320-
220845","320-38382-1","04/20/2018 09:20","04/23/2018 10:00",""
"Unknown","Unknown","NAWC-041918-RW-146","04/19/2018 10:10","AQ","320-38382-
3","NM","","0.00","537","METHOD","RES","04/26/2018 09:35","05/01/2018
12:52","TALSAC","COA","WET","NA","1","NA","NA","","100","320-219896","320-219896","NA","320-
220845","320-38382-1","04/20/2018 09:20","04/23/2018 10:00",""
"Unknown","Unknown","NAWC-041918-FRB-146","04/19/2018 10:05","AQ","320-38382-
4","FB","","0.00","537","METHOD","RES","04/26/2018 09:35","05/01/2018
12:57","TALSAC","COA","WET","NA","1","NA","NA","","100","320-219896","320-219896","NA","320-
220845","320-38382-1","04/20/2018 09:20","04/23/2018 10:00",""
"Unknown","Unknown","NAWC-041918-RW-258","04/19/2018 10:40","AQ","320-38382-
5","NM","","0.00","537","METHOD","RES","04/26/2018 09:35","05/01/2018
13:02","TALSAC","COA","WET","NA","1","NA","NA","","100","320-219896","320-219896","NA","320-
220845","320-38382-1","04/20/2018 09:20","04/23/2018 10:00",""
"Unknown","Unknown","NAWC-041918-FRB-258","04/19/2018 10:35","AQ","320-38382-
6","FB","","0.00","537","METHOD","RES","04/26/2018 09:35","05/01/2018
13:06","TALSAC","COA","WET","NA","1","NA","NA","","100","320-219896","320-219896","NA","320-
220845","320-38382-1","04/20/2018 09:20","04/23/2018 10:00",""
"Unknown","Unknown","WGNA-041918-RW-3571","04/19/2018 11:10","AQ","320-38382-
7","NM","","0.00","537","METHOD","RES","04/26/2018 09:35","05/01/2018
13:20","TALSAC","COA","WET","NA","1","NA","NA","","100","320-219896","320-219896","NA","320-
220847","320-38382-1","04/20/2018 09:20","04/23/2018 10:00",""
"Unknown","Unknown","WGNA-041918-FRB-3571","04/19/2018 11:05","AQ","320-38382-
8","FB","","0.00","537","METHOD","RES","04/26/2018 09:35","05/01/2018
13:25","TALSAC","COA","WET","NA","1","NA","NA","","100","320-219896","320-219896","NA","320-
220847","320-38382-1","04/20/2018 09:20","04/23/2018 10:00",""
"Unknown","Unknown","LCS 320-219896/2-A","","AQ","LCS 320-219896/2-
A","LCS","","-99","537","METHOD","RES","04/26/2018 09:35","05/01/2018
12:29","TALSAC","COA","WET","NA","1","NA","NA","","100","320-219896","320-219896","NA","320-
220845","320-38382-1","04/26/2018 09:35","04/23/2018 10:00",""
"Unknown","Unknown","MB 320-219896/1-A","","AQ","MB 320-219896/1-
A","MB","","-99","537","METHOD","RES","04/26/2018 09:35","05/01/2018
12:24","TALSAC","COA","WET","NA","1","NA","NA","","100","320-219896","320-219896","NA","320-
220845","320-38382-1","04/26/2018 09:35","04/23/2018 10:00",""

TO: A. FREBOWITZ
SDG: 320-38382-1

PAGE 2

in the FRBs.

<u>Sample</u>	<u>Associated FRB</u>
NAWC-041918-RW-146	NAWC-041918-FRB-146
NAWC-041918-RW-154	NAWC-041918-FRB-154
NAWC-041918-RW-258	NAWC-041918-FRB-258
WGNA-041918-RW-3571	WGNA-041918-FRB-3571

Non-detected results were reported to the Limit of Detection (LOD).

The buffering agent Trizma was added to all drinking water samples.

Executive Summary


Laboratory Performance: The MSD %Rs and MS/MSD RPDs were outside the quality control limits for several compounds.

Other Factors Affecting Data Quality: Results below the RL were estimated.

The data for these analyses were reviewed with reference to the Environmental Protection Agency document EPA/600/R-08/092, Method 537, "Determination of Selected Perfluorinated Alkyl Acids in Drinking Water by Solid Phase Extraction and Liquid Chromatography/Tandem Mass Spectrometry (LC/MS/MS)", (September 2009), US EPA National Functional Guidelines for Organic Data Review (January 2017), and the Department of Defense (DoD) document entitled "Quality Systems Manual (QSM) for Environmental Laboratories" (July 2013) as applicable. The text of this report has been formulated to address only those areas affecting data quality.



Tetra Tech, Inc.
Terri L. Solomon
Chemist/Data Validator



Tetra Tech, Inc.
Joseph A. Samchuck
Data Validation Manager

Attachments:

Appendix A – Qualified Analytical Results
Appendix B – Results as Reported by the Laboratory
Appendix C – Support Documentation

Data Qualifier Definitions

The following definitions provide brief explanations of the validation qualifiers assigned to results in the data review process.

U	The analyte was analyzed for, but was not detected at a level greater than or equal to the level of the adjusted method detection limit for sample and method.
J	The analyte was positively identified and the associated numerical value is the approximate concentration of the analyte in the sample (due either to the quality of the data generated because certain quality control criteria were not met, or the concentration of the analyte was below the reporting limit).
J+	The result is an estimated quantity, but the result may be biased high.
J-	The result is an estimated quantity, but the result may be biased low.
UJ	The analyte was analyzed for, but was not detected. The reported detection limit is approximate and may be inaccurate or imprecise.
R	The sample result (detected) is unusable due to the quality of the data generated because certain criteria were not met. The analyte may or may not be present in the sample.
UR	The sample result (nondetected) is unusable due to the quality of the data generated because certain criteria were not met. The analyte may or may not be present in the sample.

Appendix A

Qualified Analytical Results

Qualifier Codes:

- A = Lab Blank Contamination
- B = Field Blank Contamination
- C = Calibration Noncompliance (i.e., % RSDs, %Ds, ICVs, CCVs, RRFs, etc.)
- C01 = GC/MS Tuning Noncompliance
- D = MS/MSD Recovery Noncompliance
- E = LCS/LCSD Recovery Noncompliance
- F = Lab Duplicate Imprecision
- G = Field Duplicate Imprecision
- H = Holding Time Exceedance
- I = ICP Serial Dilution Noncompliance
- J = ICP PDS Recovery Noncompliance; MSA's $r < 0.995$
- K = ICP Interference - includes ICS % R Noncompliance
- L = Instrument Calibration Range Exceedance
- M = Sample Preservation Noncompliance
- N = Internal Standard Noncompliance
- N01 = Internal Standard Recovery Noncompliance Dioxins
- N02 = Recovery Standard Noncompliance Dioxins
- N03 = Clean-up Standard Noncompliance Dioxins
- O = Poor Instrument Performance (i.e., base-time drifting)
- P = Uncertainty near detection limit ($< 2 \times$ IDL for inorganics and $<$ CRQL for organics)
- Q = Other problems (can encompass a number of issues; i.e.chromatography,interferences, etc.)
- R = Surrogates Recovery Noncompliance
- S = Pesticide/PCB Resolution
- T = % Breakdown Noncompliance for DDT and Endrin
- U = RPD between columns/detectors $>40\%$ for positive results determined via GC/HPLC
- V = Non-linear calibrations; correlation coefficient $r < 0.995$
- W = EMPC result
- X = Signal to noise response drop
- Y = Percent solids $<30\%$
- Z = Uncertainty at 2 standard deviations is greater than sample activity
- Z1 = Tentatively Identified Compound considered presumptively present
- Z2 = Tentatively Identified Compound column bleed
- Z3 = Tentatively Identified Compound aldol condensate
- Z4 = Sample activity is less than the at uncertainty at 3 standard deviations and greater than the MDC
- Z5 = Sample activity is less than the at uncertainty at 3 standard deviations and less than the MDC

PROJ_NO: 08005-WE04 SDG: 320-38382-1 FRACTION: PFAS MEDIA: WATER	NSAMPLE	NAWC-041918-FRB-146			NAWC-041918-FRB-154			NAWC-041918-FRB-258			NAWC-041918-RW-146		
	LAB_ID	320-38382-4			320-38382-2			320-38382-6			320-38382-3		
	SAMP_DATE	4/19/2018			4/19/2018			4/19/2018			4/19/2018		
	QC_TYPE	FB			FB			FB			NM		
	UNITS	NG/L			NG/L			NG/L			NG/L		
	PCT_SOLIDS	0.0			0.0			0.0			0.0		
	DUP_OF												
PARAMETER	RESULT	VQL	QLCD	RESULT	VQL	QLCD	RESULT	VQL	QLCD	RESULT	VQL	QLCD	
PENTADECAFLUOROOCTANOIC ACID (PFOA)	7.6	U		7.5	U		7.5	U		27			
PERFLUOROBUTANESULFONIC ACID (PFBS)	34	U		34	U		34	U		44	U		
PERFLUOROHEPTANOIC ACID (PFHPA)	3.8	U		3.7	U		3.7	U		7	J	P	
PERFLUOROHEXANESULFONIC ACID (PFHXS)	11	U		11	U		11	U		15	U		
PERFLUORONONANOIC ACID (PFNA)	19	U		19	U		19	U		24	U		
PERFLUOROOCTANESULFONIC ACID (PFOS)	15	U		15	U		15	U		14	J	P	

PROJ_NO: 08005-WE04 SDG: 320-38382-1 FRACTION: PFAS MEDIA: WATER	NSAMPLE	NAWC-041918-RW-154			NAWC-041918-RW-258			WGNA-041918-FRB-3571			WGNA-041918-RW-3571		
	LAB_ID	320-38382-1			320-38382-5			320-38382-8			320-38382-7		
	SAMP_DATE	4/19/2018			4/19/2018			4/19/2018			4/19/2018		
	QC_TYPE	NM			NM			FB			NM		
	UNITS	NG/L			NG/L			NG/L			NG/L		
	PCT_SOLIDS	0.0			0.0			0.0			0.0		
	DUP_OF												
PARAMETER	RESULT	VQL	QLCD	RESULT	VQL	QLCD	RESULT	VQL	QLCD	RESULT	VQL	QLCD	
PENTADECAFLUOROOCTANOIC ACID (PFOA)	24	J	D	20			8.5	U		10	J	P	
PERFLUOROBUTANESULFONIC ACID (PFBS)	36	UJ	D	34	U		38	U		32	U		
PERFLUOROHEPTANOIC ACID (PFHPA)	8.1	J	DP	8.3	J	P	4.3	U		12			
PERFLUOROHEXANESULFONIC ACID (PFHXS)	12	UJ	D	11	U		13	U		11	U		
PERFLUORONONANOIC ACID (PFNA)	20	U		10	J	P	21	U		18	U		
PERFLUOROOCTANESULFONIC ACID (PFOS)	17	J	P	16	J	P	17	U		8	J	P	

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Client Sample ID: NAWC-041918-RW-154 Lab Sample ID: 320-38382-1
 Matrix: Water Lab File ID: 2018.05.01_537AA_019.d
 Analysis Method: 537 Date Collected: 04/19/2018 09:10
 Extraction Method: 537 Date Extracted: 04/26/2018 09:35
 Sample wt/vol: 252.2 (mL) Date Analyzed: 05/01/2018 12:34
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 220845 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	17	J M	40	16	6.7
335-67-1	Perfluorooctanoic acid (PFOA)	24	J	20	7.9	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U M	24	20	7.9
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U M UJ	30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	8.1	J	9.9	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U UJ	89	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	100		70-130
STL00996	13C2 PFDA	89		70-130

Wesley L. Selman
05/29/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Client Sample ID: NAWC-041918-FRB-154 Lab Sample ID: 320-38382-2
 Matrix: Water Lab File ID: 2018.05.01_537AA_022.d
 Analysis Method: 537 Date Collected: 04/19/2018 09:05
 Extraction Method: 537 Date Extracted: 04/26/2018 09:35
 Sample wt/vol: 266.7(mL) Date Analyzed: 05/01/2018 12:48
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 220845 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	37	15	6.4
335-67-1	Perfluorooctanoic acid (PFOA)	7.5	U	19	7.5	2.6
375-95-1	Perfluorononanoic acid (PFNA)	19	U	22	19	7.5
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.7	U	9.4	3.7	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	84	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	106		70-130
STL00996	13C2 PFDA	85		70-130

Heidi L. Salomon
05/29/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Client Sample ID: NAWC-041918-RW-146 Lab Sample ID: 320-38382-3
 Matrix: Water Lab File ID: 2018.05.01_537AA_023.d
 Analysis Method: 537 Date Collected: 04/19/2018 10:10
 Extraction Method: 537 Date Extracted: 04/26/2018 09:35
 Sample wt/vol: 204.8(mL) Date Analyzed: 05/01/2018 12:52
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 220845 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	14	J M	49	20	8.3
335-67-1	Perfluorooctanoic acid (PFOA)	27		24	9.8	3.4
375-95-1	Perfluorononanoic acid (PFNA)	24	U	29	24	9.8
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	15	U	37	15	6.7
375-85-9	Perfluoroheptanoic acid (PFHpA)	7.0	J	12	4.9	2.3
375-73-5	Perfluorobutanesulfonic acid (PFBS)	44	U	110	44	20

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	100		70-130
STL00996	13C2 PFDA	83		70-130

Ali L. Selman
05/29/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Client Sample ID: NAWC-041918-FRB-146 Lab Sample ID: 320-38382-4
 Matrix: Water Lab File ID: 2018.05.01_537AA_024.d
 Analysis Method: 537 Date Collected: 04/19/2018 10:05
 Extraction Method: 537 Date Extracted: 04/26/2018 09:35
 Sample wt/vol: 263.6(mL) Date Analyzed: 05/01/2018 12:57
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 220845 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	38	15	6.4
335-67-1	Perfluorooctanoic acid (PFOA)	7.6	U	19	7.6	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	U	9.5	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	85	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	106		70-130
STL00996	13C2 PFDA	88		70-130

Atari L. Salaman
05/29/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Client Sample ID: NAWC-041918-RW-258 Lab Sample ID: 320-38382-5
 Matrix: Water Lab File ID: 2018.05.01_537AA_025.d
 Analysis Method: 537 Date Collected: 04/19/2018 10:40
 Extraction Method: 537 Date Extracted: 04/26/2018 09:35
 Sample wt/vol: 260.9(mL) Date Analyzed: 05/01/2018 13:02
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 220845 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	J M	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	20		19	7.7	2.7
375-95-1	Perfluorononanoic acid (PFNA)	10	J	23	19	7.7
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U M	29	11	5.3
375-85-9	Perfluoroheptanoic acid (PFHpA)	8.3	J	9.6	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	86	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	98		70-130
STL00996	13C2 PFDA	80		70-130

Ali J. Salem
05/29/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Client Sample ID: NAWC-041918-FRB-258 Lab Sample ID: 320-38382-6
 Matrix: Water Lab File ID: 2018.05.01_537AA_026.d
 Analysis Method: 537 Date Collected: 04/19/2018 10:35
 Extraction Method: 537 Date Extracted: 04/26/2018 09:35
 Sample wt/vol: 267.6(mL) Date Analyzed: 05/01/2018 13:06
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 220845 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	37	15	6.4
335-67-1	Perfluorooctanoic acid (PFOA)	7.5	U	19	7.5	2.6
375-95-1	Perfluorononanoic acid (PFNA)	19	U	22	19	7.5
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.1
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.7	U	9.3	3.7	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	84	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	106		70-130
STL00996	13C2 PFDA	85		70-130

Wesley L. Selman
05/29/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Client Sample ID: WGNA-041918-RW-3571 Lab Sample ID: 320-38382-7
 Matrix: Water Lab File ID: 2018.05.01_537AA_029.d
 Analysis Method: 537 Date Collected: 04/19/2018 11:10
 Extraction Method: 537 Date Extracted: 04/26/2018 09:35
 Sample wt/vol: 277.2 (mL) Date Analyzed: 05/01/2018 13:20
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 220847 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	8.0	J M	36	14	6.1
335-67-1	Perfluorooctanoic acid (PFOA)	10	J	18	7.2	2.5
375-95-1	Perfluorononanoic acid (PFNA)	18	U M	22	18	7.2
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U M	27	11	5.0
375-85-9	Perfluoroheptanoic acid (PFHpA)	12		9.0	3.6	1.7
375-73-5	Perfluorobutanesulfonic acid (PFBS)	32	U M	81	32	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	99		70-130
STL00996	13C2 PFDA	79		70-130

Wesley L. Selman
05/29/2018

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Client Sample ID: WGNA-041918-FRB-3571 Lab Sample ID: 320-38382-8
 Matrix: Water Lab File ID: 2018.05.01_537AA_030.d
 Analysis Method: 537 Date Collected: 04/19/2018 11:05
 Extraction Method: 537 Date Extracted: 04/26/2018 09:35
 Sample wt/vol: 234.5 (mL) Date Analyzed: 05/01/2018 13:25
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 220847 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	17	U	43	17	7.2
335-67-1	Perfluorooctanoic acid (PFOA)	8.5	U	21	8.5	3.0
375-95-1	Perfluorononanoic acid (PFNA)	21	U	26	21	8.5
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	13	U	32	13	5.9
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.3	U	11	4.3	2.0
375-73-5	Perfluorobutanesulfonic acid (PFBS)	38	U	96	38	17

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	103		70-130
STL00996	13C2 PFDA	87		70-130

Wesley L. Selman
05/29/2018

Appendix B

Results as Reported by the Laboratory

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Client Sample ID: NAWC-041918-RW-154 Lab Sample ID: 320-38382-1
 Matrix: Water Lab File ID: 2018.05.01_537AA_019.d
 Analysis Method: 537 Date Collected: 04/19/2018 09:10
 Extraction Method: 537 Date Extracted: 04/26/2018 09:35
 Sample wt/vol: 252.2 (mL) Date Analyzed: 05/01/2018 12:34
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 220845 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	17	J M	40	16	6.7
335-67-1	Perfluorooctanoic acid (PFOA)	24		20	7.9	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U M	24	20	7.9
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U M	30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	8.1	J	9.9	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	89	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	100		70-130
STL00996	13C2 PFDA	89		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Client Sample ID: NAWC-041918-FRB-154 Lab Sample ID: 320-38382-2
 Matrix: Water Lab File ID: 2018.05.01_537AA_022.d
 Analysis Method: 537 Date Collected: 04/19/2018 09:05
 Extraction Method: 537 Date Extracted: 04/26/2018 09:35
 Sample wt/vol: 266.7(mL) Date Analyzed: 05/01/2018 12:48
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 220845 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	37	15	6.4
335-67-1	Perfluorooctanoic acid (PFOA)	7.5	U	19	7.5	2.6
375-95-1	Perfluorononanoic acid (PFNA)	19	U	22	19	7.5
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.7	U	9.4	3.7	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	84	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	106		70-130
STL00996	13C2 PFDA	85		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Client Sample ID: NAWC-041918-RW-146 Lab Sample ID: 320-38382-3
 Matrix: Water Lab File ID: 2018.05.01_537AA_023.d
 Analysis Method: 537 Date Collected: 04/19/2018 10:10
 Extraction Method: 537 Date Extracted: 04/26/2018 09:35
 Sample wt/vol: 204.8(mL) Date Analyzed: 05/01/2018 12:52
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 220845 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	14	J M	49	20	8.3
335-67-1	Perfluorooctanoic acid (PFOA)	27		24	9.8	3.4
375-95-1	Perfluorononanoic acid (PFNA)	24	U	29	24	9.8
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	15	U	37	15	6.7
375-85-9	Perfluoroheptanoic acid (PFHpA)	7.0	J	12	4.9	2.3
375-73-5	Perfluorobutanesulfonic acid (PFBS)	44	U	110	44	20

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	100		70-130
STL00996	13C2 PFDA	83		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Client Sample ID: NAWC-041918-FRB-146 Lab Sample ID: 320-38382-4
 Matrix: Water Lab File ID: 2018.05.01_537AA_024.d
 Analysis Method: 537 Date Collected: 04/19/2018 10:05
 Extraction Method: 537 Date Extracted: 04/26/2018 09:35
 Sample wt/vol: 263.6(mL) Date Analyzed: 05/01/2018 12:57
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 220845 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	38	15	6.4
335-67-1	Perfluorooctanoic acid (PFOA)	7.6	U	19	7.6	2.7
375-95-1	Perfluorononanoic acid (PFNA)	19	U	23	19	7.6
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.2
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.8	U	9.5	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	85	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	106		70-130
STL00996	13C2 PFDA	88		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Client Sample ID: NAWC-041918-RW-258 Lab Sample ID: 320-38382-5
 Matrix: Water Lab File ID: 2018.05.01_537AA_025.d
 Analysis Method: 537 Date Collected: 04/19/2018 10:40
 Extraction Method: 537 Date Extracted: 04/26/2018 09:35
 Sample wt/vol: 260.9(mL) Date Analyzed: 05/01/2018 13:02
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 220845 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	J M	38	15	6.5
335-67-1	Perfluorooctanoic acid (PFOA)	20		19	7.7	2.7
375-95-1	Perfluorononanoic acid (PFNA)	10	J	23	19	7.7
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U M	29	11	5.3
375-85-9	Perfluoroheptanoic acid (PFHpA)	8.3	J	9.6	3.8	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	86	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	98		70-130
STL00996	13C2 PFDA	80		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Client Sample ID: NAWC-041918-FRB-258 Lab Sample ID: 320-38382-6
 Matrix: Water Lab File ID: 2018.05.01_537AA_026.d
 Analysis Method: 537 Date Collected: 04/19/2018 10:35
 Extraction Method: 537 Date Extracted: 04/26/2018 09:35
 Sample wt/vol: 267.6(mL) Date Analyzed: 05/01/2018 13:06
 Con. Extract Vol.: 1.00(mL) Dilution Factor: 1
 Injection Volume: 2(uL) GC Column: GeminiC18 3x100 ID: 3(mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 220845 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	15	U	37	15	6.4
335-67-1	Perfluorooctanoic acid (PFOA)	7.5	U	19	7.5	2.6
375-95-1	Perfluorononanoic acid (PFNA)	19	U	22	19	7.5
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U	28	11	5.1
375-85-9	Perfluoroheptanoic acid (PFHpA)	3.7	U	9.3	3.7	1.8
375-73-5	Perfluorobutanesulfonic acid (PFBS)	34	U	84	34	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	106		70-130
STL00996	13C2 PFDA	85		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Client Sample ID: WGNA-041918-RW-3571 Lab Sample ID: 320-38382-7
 Matrix: Water Lab File ID: 2018.05.01_537AA_029.d
 Analysis Method: 537 Date Collected: 04/19/2018 11:10
 Extraction Method: 537 Date Extracted: 04/26/2018 09:35
 Sample wt/vol: 277.2 (mL) Date Analyzed: 05/01/2018 13:20
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 220847 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	8.0	J M	36	14	6.1
335-67-1	Perfluorooctanoic acid (PFOA)	10	J	18	7.2	2.5
375-95-1	Perfluorononanoic acid (PFNA)	18	U M	22	18	7.2
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	11	U M	27	11	5.0
375-85-9	Perfluoroheptanoic acid (PFHpA)	12		9.0	3.6	1.7
375-73-5	Perfluorobutanesulfonic acid (PFBS)	32	U M	81	32	15

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	99		70-130
STL00996	13C2 PFDA	79		70-130

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Client Sample ID: WGNA-041918-FRB-3571 Lab Sample ID: 320-38382-8
 Matrix: Water Lab File ID: 2018.05.01_537AA_030.d
 Analysis Method: 537 Date Collected: 04/19/2018 11:05
 Extraction Method: 537 Date Extracted: 04/26/2018 09:35
 Sample wt/vol: 234.5 (mL) Date Analyzed: 05/01/2018 13:25
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 220847 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	17	U	43	17	7.2
335-67-1	Perfluorooctanoic acid (PFOA)	8.5	U	21	8.5	3.0
375-95-1	Perfluorononanoic acid (PFNA)	21	U	26	21	8.5
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	13	U	32	13	5.9
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.3	U	11	4.3	2.0
375-73-5	Perfluorobutanesulfonic acid (PFBS)	38	U	96	38	17

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	103		70-130
STL00996	13C2 PFDA	87		70-130

Appendix C

Support Documentation

TestAmerica Sacramento

880 Riverside Parkway
West Sacramento, CA 95605-1500
phone 916.373.5600 fax 303.467.7248

Chain of Custody Record



TestAmerica Laboratories, Inc.

Regulatory Program: DW NPDES RCRA Other:

Client Contact		Project Manager: Andy Frebowitz		Site Contact: Mary Kay Bond		Date: 4/19/2018		COC No.:			
TetraTech		Tel/Fax: 610.382.1170		Lab Contact: Dave Alltucker		Carrier: FedEx		1 of 1 COCs			
234 Mall Boulevard Suite 260		Analysis Turnaround Time								Sampler: Mary Kay Bond	
King of Prussia, PA 19406		<input type="checkbox"/> CALENDAR DAYS <input type="checkbox"/> WORKING DAYS								For Lab Use Only:	
610-382-1174		TAT if different from Below 21								Walk-in Client:	
610-491-9688		<input type="checkbox"/> 2 weeks								Lab Sampling:	
Project Name: WE04		<input type="checkbox"/> 1 week								Job / SDG No.:	
Site: WE04		<input type="checkbox"/> 2 days									
P O # 1132358 (through EarthToxics)		<input type="checkbox"/> 1 day									
Sample Identification		Sample Date	Sample Time	Sample Type (C=Comp, G=Grab)	Matrix	# of Cont.	Filtered Sample (Y/N)	Perform MS/MSD (Y/N)	EPA 537 UCMR3	Sample Specific Notes:	
NAWC-041918-RW-154		4/19/2018	9:10	G	DW	6	N	N	Y	MS/MSD	
NAWC-041918-FRB-154		4/19/2018	9:05	G	DW	2	N	N	Y	Field Reagent Blank	
NAWC-041918-RW-146		4/19/2018	10:10	G	DW	2	N	N	Y	Field Reagent Blank	
NAWC-041918-FRB-146		4/19/2018	10:05	G	DW	2	N	N	Y	Field Reagent Blank	
NAWC-041918-RW-258		4/19/2018	10:40	G	DW	2	N	N	Y	Field Reagent Blank	
NAWC-041918-FRB-258		4/19/2018	10:35	G	DW	2	N	N	Y	Field Reagent Blank	
WGNA-041918-RW-3571		4/19/2018	11:10	G	DW	2	N	N	Y	Field Reagent Blank	
WGNA-041918-FRB-3571		4/19/2018	11:05	G	DW	2	N	N	Y	Field Reagent Blank	
Preservation Used: 1= Ice, 2= HCl; 3= H2SO4; 4=HNO3; 5=NaOH; 6=Other: Trizma							6				
Possible Hazard Identification: Are any samples from a listed EPA Hazardous Waste? Please List any EPA Waste Codes for the sample in the							Sample Disposal (A fee may be assessed if samples are retained longer than 1 month)				
<input checked="" type="checkbox"/> Non-Hazard <input type="checkbox"/> Flammable <input type="checkbox"/> Skin Irritant <input type="checkbox"/> Poison B <input type="checkbox"/> Unknown							<input type="checkbox"/> Return to Client <input checked="" type="checkbox"/> Disposal by Lab <input type="checkbox"/> Archive for _____ Months				
Fed Ex Tracking: 7720 4058 7199											
Custody Seals Intact: <input type="checkbox"/> Yes <input type="checkbox"/> No		Custody Seal No.:		Cooler Temp. (°C): Obs'd: 0.0 Corr'd: 0.0		Therm ID No.: AK-5 ice					
Relinquished by: <i>Mary Kay Bond</i>		Company: Tetra Tech		Date/Time: 4/19/2018 16:00		Received by: <i>Ang D. [Signature]</i>		Company: <i>PA-SIAC</i>		Date/Time: 4/20/18 0920	
Relinquished by:		Company:		Date/Time:		Received by:		Company:		Date/Time:	
Relinquished by:		Company:		Date/Time:		Received in Laboratory by:		Company:		Date/Time:	

Page 296 of 297



320-38382 Chain of Custody

Job Narrative
320-38382-1

Receipt

The samples were received on 4/20/2018 9:20 AM; the samples arrived in good condition, properly preserved and, where required, on ice. The temperature of the cooler at receipt was 0.0° C.

LCMS

Method(s) 537: The first level standard from the initial calibration curve is used to evaluate the tune criteria. The instrument mass windows are set at +/- 0.5amu; therefore, detection of the analyte serves as verification that the assigned mass is within +/- 0.5amu of the true value, which meets the DoD/DOE QSM tune criterion.

Method(s) 537: The matrix spike duplicate (MS/MSD) recoveries and MS/MSD precision for preparation batch 320-219896 and analytical batch 320-220845 were outside control limits. Sample matrix interference and/or non-homogeneity are suspected because the associated laboratory control sample (LCS) was within acceptance limits.

Method(s) 537: Surrogate recovery for the following sample was outside control limits: NAWC-041918-RW-154 (320-38382-1[MSD]). Re-analysis was performed with concurring results. The original analysis has been reported.

No additional analytical or quality issues were noted, other than those described above or in the Definitions/Glossary page.

Organic Prep

No analytical or quality issues were noted, other than those described in the Definitions/Glossary page.

Method Summary

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-38382-1

Method	Method Description	Protocol	Laboratory
537	Perfluorinated Alkyl Acids (LC/MS)	EPA	TAL SAC
537	Extraction of Perfluorinated Alkyl Acids	EPA	TAL SAC

Protocol References:

EPA = US Environmental Protection Agency

Laboratory References:

TAL SAC = TestAmerica Sacramento, 880 Riverside Parkway, West Sacramento, CA 95605, TEL (916)373-5600

Sample Summary

Client: Tetra Tech, Inc.
Project/Site: Warminster: PFAS, NAS JRB Willow Grove

TestAmerica Job ID: 320-38382-1

Lab Sample ID	Client Sample ID	Matrix	Collected	Received
320-38382-1	NAWC-041918-RW-154	Water	04/19/18 09:10	04/20/18 09:20
320-38382-2	NAWC-041918-FRB-154	Water	04/19/18 09:05	04/20/18 09:20
320-38382-3	NAWC-041918-RW-146	Water	04/19/18 10:10	04/20/18 09:20
320-38382-4	NAWC-041918-FRB-146	Water	04/19/18 10:05	04/20/18 09:20
320-38382-5	NAWC-041918-RW-258	Water	04/19/18 10:40	04/20/18 09:20
320-38382-6	NAWC-041918-FRB-258	Water	04/19/18 10:35	04/20/18 09:20
320-38382-7	WGNA-041918-RW-3571	Water	04/19/18 11:10	04/20/18 09:20
320-38382-8	WGNA-041918-FRB-3571	Water	04/19/18 11:05	04/20/18 09:20

FORM II
LCMS SURROGATE RECOVERY

Lab Name: TestAmerica Sacramento

Job No.: 320-38382-1

SDG No.: _____

Matrix: Water

Level: Low

GC Column (1): GeminiC18 3 ID: 3 (mm)

Client Sample ID	Lab Sample ID	PFHxA #	PFDA #
NAWC-041918-RW-154	320-38382-1	100	89
NAWC-041918-FRB-154	320-38382-2	106	85
NAWC-041918-RW-146	320-38382-3	100	83
NAWC-041918-FRB-146	320-38382-4	106	88
NAWC-041918-RW-258	320-38382-5	98	80
NAWC-041918-FRB-258	320-38382-6	106	85
WGNA-041918-RW-357	320-38382-7	99	79
WGNA-041918-FRB-357	320-38382-8	103	87
	MB 320-219896/1-A	107	90
	LCS 320-219896/2-A	108	91
NAWC-041918-RW-154 MS	320-38382-1 MS	96	84
NAWC-041918-RW-154 MSD	320-38382-1 MSD	66 Q	74

PFHxA = 13C2 PFHxA
PFDA = 13C2 PFDA

QC LIMITS
70-130
70-130

Column to be used to flag recovery values

FORM III
LCMS LAB CONTROL SAMPLE RECOVERY

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Matrix: Water Level: Low Lab File ID: 2018.05.01_537AA_018.d
 Lab ID: LCS 320-219896/2-A Client ID: _____

COMPOUND	SPIKE ADDED (ng/L)	LCS CONCENTRATION (ng/L)	LCS % REC	QC LIMITS REC	#
Perfluorooctanesulfonic acid (PFOS)	220	225	103	70-130	M
Perfluorooctanoic acid (PFOA)	110	110	100	70-130	
Perfluorononanoic acid (PFNA)	110	102	93	70-130	
Perfluorohexanesulfonic acid (PFHxS)	168	179	106	70-130	
Perfluoroheptanoic acid (PFHpA)	54.0	58.2	108	70-130	
Perfluorobutanesulfonic acid (PFBS)	500	519	104	70-130	

Column to be used to flag recovery and RPD values

FORM III
LCMS MATRIX SPIKE RECOVERY

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Matrix: Water Level: Low Lab File ID: 2018.05.01_537AA_020.d
 Lab ID: 320-38382-1 MS Client ID: NAWC-041918-RW-154 MS

COMPOUND	SPIKE ADDED (ng/L)	SAMPLE CONCENTRATION (ng/L)	MS CONCENTRATION (ng/L)	MS % REC	QC LIMITS REC	#
Perfluorooctanesulfonic acid (PFOS)	217	17 J	237	102	70-130	M
Perfluorooctanoic acid (PFOA)	109	24	124	92	70-130	
Perfluorononanoic acid (PFNA)	109	20 U	98.7	91	70-130	
Perfluorohexanesulfonic acid (PFHxS)	166	12 U	177	106	70-130	
Perfluoroheptanoic acid (PFHpA)	53.5	8.1 J	59.8	97	70-130	
Perfluorobutanesulfonic acid (PFBS)	495	36 U	523	105	70-130	

Column to be used to flag recovery and RPD values

FORM III
LCMS MATRIX SPIKE DUPLICATE RECOVERY

Lab Name: TestAmerica Sacramento

Job No.: 320-38382-1

SDG No.: _____

Matrix: Water Level: Low

Lab File ID: 2018.05.01_537AA_021.d

Lab ID: 320-38382-1 MSD

Client ID: NAWC-041918-RW-154 MSD

COMPOUND	SPIKE ADDED (ng/L)	MSD CONCENTRATION (ng/L)	MSD % REC	% RPD	QC LIMITS		#
					RPD	REC	
Perfluorooctanesulfonic acid (PFOS)	217	185	78	25	30	70-130	M
Perfluorooctanoic acid (PFOA)	109	89.8	60	32	30	70-130	J1
Perfluorononanoic acid (PFNA)	109	77.7	71	24	30	70-130	
Perfluorohexanesulfonic acid (PFHxS)	166	116	70	41	30	70-130	J1
Perfluoroheptanoic acid (PFHpA)	53.4	41.1	62	37	30	70-130	J1
Perfluorobutanesulfonic acid (PFBS)	495	347	70	40	30	70-130	J1

Column to be used to flag recovery and RPD values

FORM IV
LCMS METHOD BLANK SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Lab File ID: 2018.05.01_537AA_017.d Lab Sample ID: MB 320-219896/1-A
 Matrix: Water Date Extracted: 04/26/2018 09:35
 Instrument ID: A8_N Date Analyzed: 05/01/2018 12:24
 Level: (Low/Med) Low

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES:

CLIENT SAMPLE ID	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED
	LCS 320-219896/2-A	2018.05.01_537AA 018.d	05/01/2018 12:29
NAWC-041918-RW-154	320-38382-1	2018.05.01_537AA 019.d	05/01/2018 12:34
NAWC-041918-RW-154 MS	320-38382-1 MS	2018.05.01_537AA 020.d	05/01/2018 12:38
NAWC-041918-RW-154 MSD	320-38382-1 MSD	2018.05.01_537AA 021.d	05/01/2018 12:43
NAWC-041918-FRB-154	320-38382-2	2018.05.01_537AA 022.d	05/01/2018 12:48
NAWC-041918-RW-146	320-38382-3	2018.05.01_537AA 023.d	05/01/2018 12:52
NAWC-041918-FRB-146	320-38382-4	2018.05.01_537AA 024.d	05/01/2018 12:57
NAWC-041918-RW-258	320-38382-5	2018.05.01_537AA 025.d	05/01/2018 13:02
NAWC-041918-FRB-258	320-38382-6	2018.05.01_537AA 026.d	05/01/2018 13:06
WGNA-041918-RW-3571	320-38382-7	2018.05.01_537AA 029.d	05/01/2018 13:20
WGNA-041918-FRB-3571	320-38382-8	2018.05.01_537AA 030.d	05/01/2018 13:25

FORM I
LCMS ORGANICS ANALYSIS DATA SHEET

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Client Sample ID: _____ Lab Sample ID: MB 320-219896/1-A
 Matrix: Water Lab File ID: 2018.05.01_537AA_017.d
 Analysis Method: 537 Date Collected: _____
 Extraction Method: 537 Date Extracted: 04/26/2018 09:35
 Sample wt/vol: 250 (mL) Date Analyzed: 05/01/2018 12:24
 Con. Extract Vol.: 1.00 (mL) Dilution Factor: 1
 Injection Volume: 2 (uL) GC Column: GeminiC18 3x100 ID: 3 (mm)
 % Moisture: _____ GPC Cleanup: (Y/N) N
 Analysis Batch No.: 220845 Units: ng/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
1763-23-1	Perfluorooctanesulfonic acid (PFOS)	16	U	40	16	6.8
335-67-1	Perfluorooctanoic acid (PFOA)	8.0	U	20	8.0	2.8
375-95-1	Perfluorononanoic acid (PFNA)	20	U	24	20	8.0
355-46-4	Perfluorohexanesulfonic acid (PFHxS)	12	U	30	12	5.5
375-85-9	Perfluoroheptanoic acid (PFHpA)	4.0	U	10	4.0	1.9
375-73-5	Perfluorobutanesulfonic acid (PFBS)	36	U	90	36	16

CAS NO.	SURROGATE	%REC	Q	LIMITS
STL00993	13C2 PFHxA	107		70-130
STL00996	13C2 PFDA	90		70-130

FORM VIII
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Instrument ID: A8_N Calibration Start Date: 04/11/2018 11:45
 GC Column: GeminiC18 3x100 ID: 3(mm) Calibration End Date: 04/11/2018 12:09
 Calibration ID: 38530

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
<u>INITIAL CALIBRATION MEAN AREA AND MEAN RT</u>	970041	1.86	2344935	2.10		
UPPER LIMIT	1455062	2.36	3517403	2.60		
LOWER LIMIT	485021	1.36	1172468	1.60		
LAB SAMPLE ID	CLIENT SAMPLE ID					
CCVL 320-217453/10		964533	1.87	2387973	2.10	
ICV 320-217453/12		1123391	1.86	2710764	2.10	
CCVL 320-220842/1		950434	1.90	2226982	2.12	
CCV 320-220845/13 CCVIS		1006734	1.88	2332599	2.12	
MB 320-219896/1-A		896308	1.89	2119146	2.12	
LCS 320-219896/2-A		885760	1.90	2152883	2.12	
320-38382-1	NAWC-041918-RW-154	918602	1.89	2172570	2.12	
320-38382-1 MS	NAWC-041918-RW-154 MS	873603	1.89	1979894	2.12	
320-38382-1 MSD	NAWC-041918-RW-154 MSD	927451	1.89	2186239	2.12	
320-38382-2	NAWC-041918-FRB-154	931565	1.88	2174288	2.12	
320-38382-3	NAWC-041918-RW-146	908929	1.89	2119366	2.12	
320-38382-4	NAWC-041918-FRB-146	907706	1.89	2174599	2.12	
320-38382-5	NAWC-041918-RW-258	877855	1.89	2070367	2.12	
320-38382-6	NAWC-041918-FRB-258	880431	1.88	2120366	2.11	
CCV 320-220845/25 CCVIS		848761	1.88	2054615	2.11	
CCV 320-220847/25 CCVIS		848761	1.88	2054615	2.11	
320-38382-7	WGNA-041918-RW-3571	849895	1.87	1937754	2.11	
320-38382-8	WGNA-041918-FRB-3571	836252	1.88	1978104	2.11	
CCV 320-220847/29 CCVIS		851622	1.88	2073725	2.11	

13PFOA = 13C2-PFOA

PFOS = 13C4 PFOS

Area Limit = 50%-150% of internal standard area

RT Limit = ± 0.5 minutes of internal standard RT

Column used to flag values outside QC limits

FORM VIII
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Sample No.: CCV 320-220845/13 Date Analyzed: 05/01/2018 12:15
 Instrument ID: A8_N GC Column: GeminiC18 3x100 ID: 3 (mm)
 Lab File ID (Standard): 2018.05.01_537AA_01 Heated Purge: (Y/N) N
 Calibration ID: 38530

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	1006734	1.88	2332599	2.12		
UPPER LIMIT	1409428	2.38	3265639	2.62		
LOWER LIMIT	704714	1.38	1632819	1.62		
LAB SAMPLE ID	CLIENT SAMPLE ID					
MB 320-219896/1-A		896308	1.89	2119146	2.12	
LCS 320-219896/2-A		885760	1.90	2152883	2.12	
320-38382-1	NAWC-041918-RW-154	918602	1.89	2172570	2.12	
320-38382-1 MS	NAWC-041918-RW-154 MS	873603	1.89	1979894	2.12	
320-38382-1 MSD	NAWC-041918-RW-154 MSD	927451	1.89	2186239	2.12	
320-38382-2	NAWC-041918-FRB-154	931565	1.88	2174288	2.12	
320-38382-3	NAWC-041918-RW-146	908929	1.89	2119366	2.12	
320-38382-4	NAWC-041918-FRB-146	907706	1.89	2174599	2.12	
320-38382-5	NAWC-041918-RW-258	877855	1.89	2070367	2.12	
320-38382-6	NAWC-041918-FRB-258	880431	1.88	2120366	2.11	

13PFOA = 13C2-PFOA

PFOS = 13C4 PFOS

Area Limit = 70%-140% of internal standard area

RT Limit = ± 0.5 minutes of internal standard RT

Column used to flag values outside QC limits

FORM VIII
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Sample No.: CCV 320-220845/25 Date Analyzed: 05/01/2018 13:11
 Instrument ID: A8_N GC Column: GeminiC18 3x100 ID: 3 (mm)
 Lab File ID (Standard): 2018.05.01_537AA_02 Heated Purge: (Y/N) N
 Calibration ID: 38530

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	848761	1.88	2054615	2.11		
UPPER LIMIT	1188265	2.38	2876461	2.61		
LOWER LIMIT	594133	1.38	1438231	1.61		
LAB SAMPLE ID	CLIENT SAMPLE ID					
MB 320-219896/1-A		896308	1.89	2119146	2.12	
LCS 320-219896/2-A		885760	1.90	2152883	2.12	
320-38382-1	NAWC-041918-RW-154	918602	1.89	2172570	2.12	
320-38382-1 MS	NAWC-041918-RW-154 MS	873603	1.89	1979894	2.12	
320-38382-1 MSD	NAWC-041918-RW-154 MSD	927451	1.89	2186239	2.12	
320-38382-2	NAWC-041918-FRB-154	931565	1.88	2174288	2.12	
320-38382-3	NAWC-041918-RW-146	908929	1.89	2119366	2.12	
320-38382-4	NAWC-041918-FRB-146	907706	1.89	2174599	2.12	
320-38382-5	NAWC-041918-RW-258	877855	1.89	2070367	2.12	
320-38382-6	NAWC-041918-FRB-258	880431	1.88	2120366	2.11	

13PFOA = 13C2-PFOA
 PFOS = 13C4 PFOS

Area Limit = 70%-140% of internal standard area
 RT Limit = ± 0.5 minutes of internal standard RT

Column used to flag values outside QC limits

FORM VIII
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Sample No.: CCV 320-220847/25 Date Analyzed: 05/01/2018 13:11
 Instrument ID: A8_N GC Column: GeminiC18 3x100 ID: 3 (mm)
 Lab File ID (Standard): 2018.05.01_537AA_02 Heated Purge: (Y/N) N
 Calibration ID: 38530

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	848761	1.88	2054615	2.11		
UPPER LIMIT	1188265	2.38	2876461	2.61		
LOWER LIMIT	594133	1.38	1438231	1.61		
LAB SAMPLE ID	CLIENT SAMPLE ID					
320-38382-7	WGNA-041918-RW-3571		849895	1.87	1937754	2.11
320-38382-8	WGNA-041918-FRB-3571		836252	1.88	1978104	2.11

13PFOA = 13C2-PFOA
 PFOS = 13C4 PFOS

Area Limit = 70%-140% of internal standard area
 RT Limit = ± 0.5 minutes of internal standard RT

Column used to flag values outside QC limits

FORM VIII
LCMS INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Sample No.: CCV 320-220847/29 Date Analyzed: 05/01/2018 13:30
 Instrument ID: A8_N GC Column: GeminiC18 3x100 ID: 3 (mm)
 Lab File ID (Standard): 2018.05.01_537AA_03 Heated Purge: (Y/N) N
 Calibration ID: 38530

	13PFOA		PFOS		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12/24 HOUR STD	851622	1.88	2073725	2.11		
UPPER LIMIT	1192271	2.38	2903215	2.61		
LOWER LIMIT	596135	1.38	1451608	1.61		
LAB SAMPLE ID	CLIENT SAMPLE ID					
320-38382-7	WGNA-041918-RW-3571		849895	1.87	1937754	2.11
320-38382-8	WGNA-041918-FRB-3571		836252	1.88	1978104	2.11

13PFOA = 13C2-PFOA
 PFOS = 13C4 PFOS

Area Limit = 70%-140% of internal standard area
 RT Limit = ± 0.5 minutes of internal standard RT

Column used to flag values outside QC limits

FORM VI
LCMS BY INTERNAL STANDARD - INITIAL CALIBRATION DATA
CURVE EVALUATION

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1 Analy Batch No.: 217453

SDG No.: _____

Instrument ID: A8_N GC Column: GeminiC18 3 ID: 3(mm) Heated Purge: (Y/N) N

Calibration Start Date: 04/11/2018 11:45 Calibration End Date: 04/11/2018 12:09 Calibration ID: 38530

Calibration Files:

LEVEL:	LAB SAMPLE ID:	LAB FILE ID:
Level 1	IC 320-217453/3	2018.04.11_537ICALB_004.d
Level 2	IC 320-217453/4	2018.04.11_537ICALB_005.d
Level 3	IC 320-217453/5	2018.04.11_537ICALB_006.d
Level 4	IC 320-217453/6	2018.04.11_537ICALB_007.d
Level 5	IC 320-217453/7	2018.04.11_537ICALB_008.d
Level 6	IC 320-217453/8	2018.04.11_537ICALB_009.d

ANALYTE	RRF					CURVE TYPE	COEFFICIENT			#	MIN RRF	%RSD	#	MAX %RSD	R ² OR COD	#	MIN R ² OR COD
	LVL 1 LVL 6	LVL 2	LVL 3	LVL 4	LVL 5		B	M1	M2								
Perfluorobutanesulfonic acid (PFBS)	1.1422 0.9535	1.0952	1.0744	1.0454	1.0008	Ave		1.0519			6.4		30.0				
Perfluoroheptanoic acid (PFHpA)	1.0850 1.0447	1.0991	1.0649	1.0783	1.0702	Ave		1.0737			1.7		30.0				
Perfluorohexanesulfonic acid (PFHxS)	1.6457 1.6837	1.5988	1.6030	1.6384	1.6838	Ave		1.6422			2.3		30.0				
Perfluorooctanoic acid (PFOA)	1.0599 1.0325	1.0296	1.0703	1.0516	1.1300	Ave		1.0623			3.5		30.0				
Perfluorooctanesulfonic acid (PFOS)	1.0432 1.0989	1.0519	1.0326	1.0935	1.0764	Ave		1.0661			2.6		30.0				
Perfluorononanoic acid (PFNA)	0.8261 0.8363	0.8133	0.8488	0.8818	0.8480	Ave		0.8424			2.8		30.0				
13C2 PFHxA	1.0447 1.0648	1.0532	1.0875	1.0687	1.0602	Ave		1.0632			1.4		30.0				
13C2 PFDA	0.8513 0.8262	0.8714	0.8533	0.8487	0.8519	Ave		0.8505			1.7		30.0				

Note: The M1 coefficient is the same as Ave RRF for an Ave curve type.

FORM VI
LCMS BY INTERNAL STANDARD - INITIAL CALIBRATION DATA
RESPONSE AND CONCENTRATION

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1 Analy Batch No.: 217453

SDG No.: _____

Instrument ID: A8_N GC Column: GeminiC18 3 ID: 3(mm) Heated Purge: (Y/N) N

Calibration Start Date: 04/11/2018 11:45 Calibration End Date: 04/11/2018 12:09 Calibration ID: 38530

Calibration Files:

LEVEL:	LAB SAMPLE ID:	LAB FILE ID:
Level 1	IC 320-217453/3	2018.04.11_537ICALB_004.d
Level 2	IC 320-217453/4	2018.04.11_537ICALB_005.d
Level 3	IC 320-217453/5	2018.04.11_537ICALB_006.d
Level 4	IC 320-217453/6	2018.04.11_537ICALB_007.d
Level 5	IC 320-217453/7	2018.04.11_537ICALB_008.d
Level 6	IC 320-217453/8	2018.04.11_537ICALB_009.d

ANALYTE	IS REF	CURVE TYPE	RESPONSE					CONCENTRATION (NG/ML)				
			LVL 1 LVL 6	LVL 2	LVL 3	LVL 4	LVL 5	LVL 1 LVL 6	LVL 2	LVL 3	LVL 4	LVL 5
Perfluorobutanesulfonic acid (PFBS)	PFOS	Ave	870696 13871852	1696932	4015148	8010147	10764182	9.00 180	20.0	45.0	90.1	135
Perfluoroheptanoic acid (PFHpA)	13PF OA	Ave	108741 1996261	218860	489075	1044752	1450463	0.960 19.4	2.16	4.86	9.72	14.6
Perfluorohexanesulfonic acid (PFHxS)	PFOS	Ave	418640 8226588	831963	2012030	4216387	6082352	3.00 60.5	6.72	15.1	30.2	45.4
Perfluorooctanoic acid (PFOA)	13PF OA	Ave	219100 4019004	417632	1001316	2075568	3119787	1.98 39.6	4.40	9.90	19.8	29.7
Perfluorooctanesulfonic acid (PFOS)	PFOS	Ave	349354 7016962	715378	1693810	3678059	5081660	3.95 79.1	8.79	19.8	39.5	59.3
Perfluorononanoic acid (PFNA)	13PF OA	Ave	170770 3255374	329904	794076	1740422	2341235	1.98 39.6	4.40	9.90	19.8	29.7
13C2 PFHxA	13PF OA	Ave	1090690 1046576	970942	1027706	1065262	985534	10.0 10.0	10.0	10.0	10.0	10.0
13C2 PFDA	13PF OA	Ave	888742 812112	803402	806360	845990	791901	10.0 10.0	10.0	10.0	10.0	10.0

Curve Type Legend:

Ave = Average ISTD

FORM VI
 LCMS BY INTERNAL STANDARD - INITIAL CALIBRATION DATA
 READBACK PERCENT ERROR

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1 Analy Batch No.: 217453

SDG No.: _____


Instrument ID: A8_N GC Column: GeminiC18 3 ID: 3(mm) Heated Purge: (Y/N) N


Calibration Start Date: 04/11/2018 11:45 Calibration End Date: 04/11/2018 12:09 Calibration ID: 38530

Calibration Files:

LEVEL:	LAB SAMPLE ID:	LAB FILE ID:
Level 1	IC 320-217453/3	2018.04.11_537ICALB_004.d
Level 2	IC 320-217453/4	2018.04.11_537ICALB_005.d
Level 3	IC 320-217453/5	2018.04.11_537ICALB_006.d
Level 4	IC 320-217453/6	2018.04.11_537ICALB_007.d
Level 5	IC 320-217453/7	2018.04.11_537ICALB_008.d
Level 6	IC 320-217453/8	2018.04.11_537ICALB_009.d

ANALYTE	PERCENT ERROR						PERCENT ERROR LIMIT					
	LVL 1 #	LVL 2 #	LVL 3 #	LVL 4 #	LVL 5 #	LVL 6 #	LVL 1	LVL 2	LVL 3	LVL 4	LVL 5	LVL 6
Perfluorobutanesulfonic acid (PFBS)	8.6	4.1	2.1	-0.6	-4.9	-9.4	50	30	30	30	30	30
Perfluoroheptanoic acid (PFHpA)	1.0	2.4	-0.8	0.4	-0.3	-2.7	50	30	30	30	30	30
Perfluorohexanesulfonic acid (PFHxS)	0.2	-2.6	-2.4	-0.2	2.5	2.5	50	30	30	30	30	30
Perfluorooctanoic acid (PFOA)	-0.2	-3.1	0.7	-1.0	6.4	-2.8	50	30	30	30	30	30
Perfluorooctanesulfonic acid (PFOS)	-2.1	-1.3	-3.1	2.6	1.0	3.1	50	30	30	30	30	30
Perfluorononanoic acid (PFNA)	-1.9	-3.5	0.8	4.7	0.7	-0.7	50	30	30	30	30	30
13C2 PFHxA	-1.7	-0.9	2.3	0.5	-0.3	0.1	30	30	30	30	30	30
13C2 PFDA	0.1	2.5	0.3	-0.2	0.2	-2.9	30	30	30	30	30	30

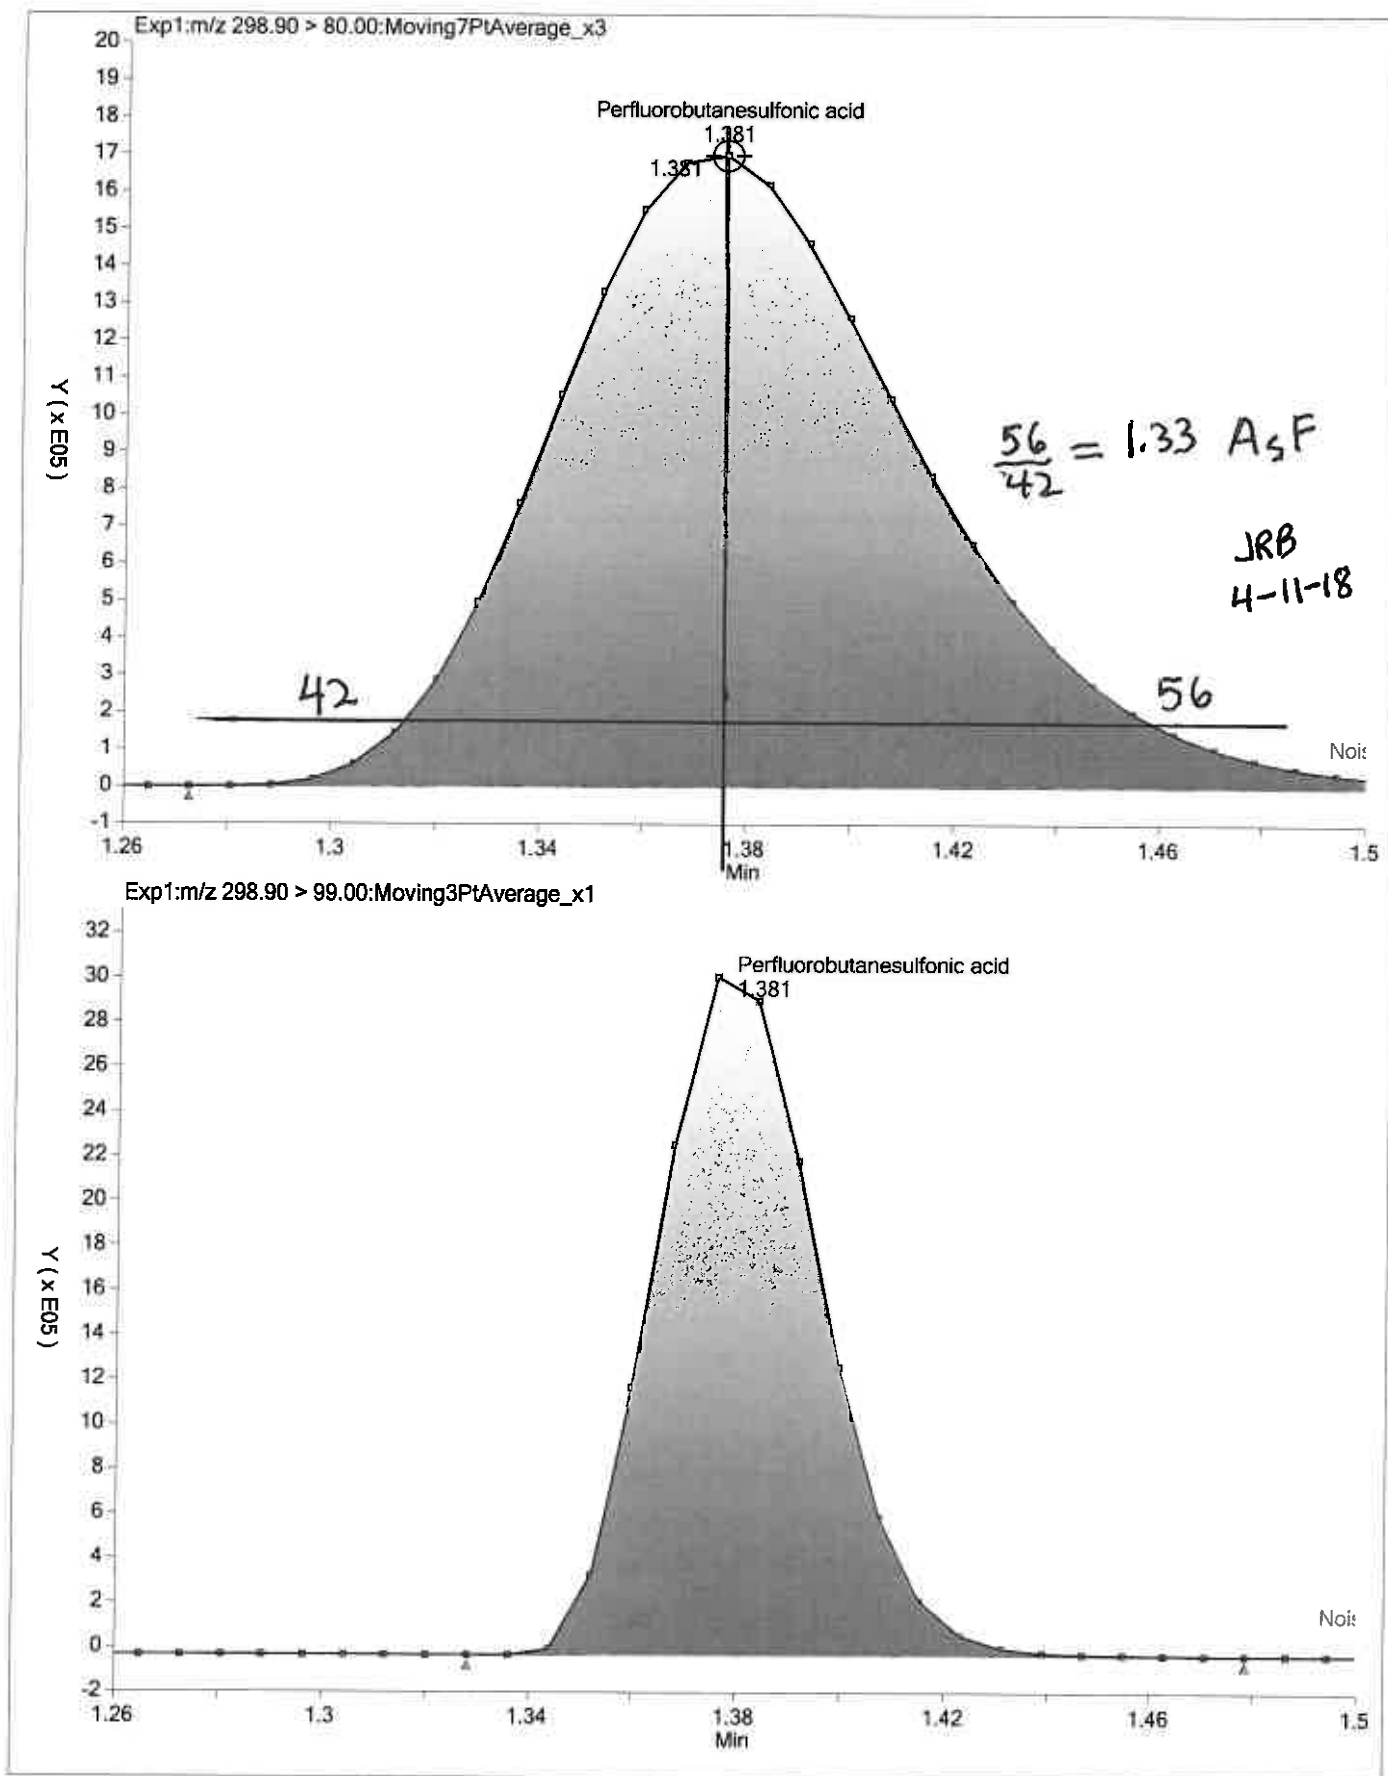

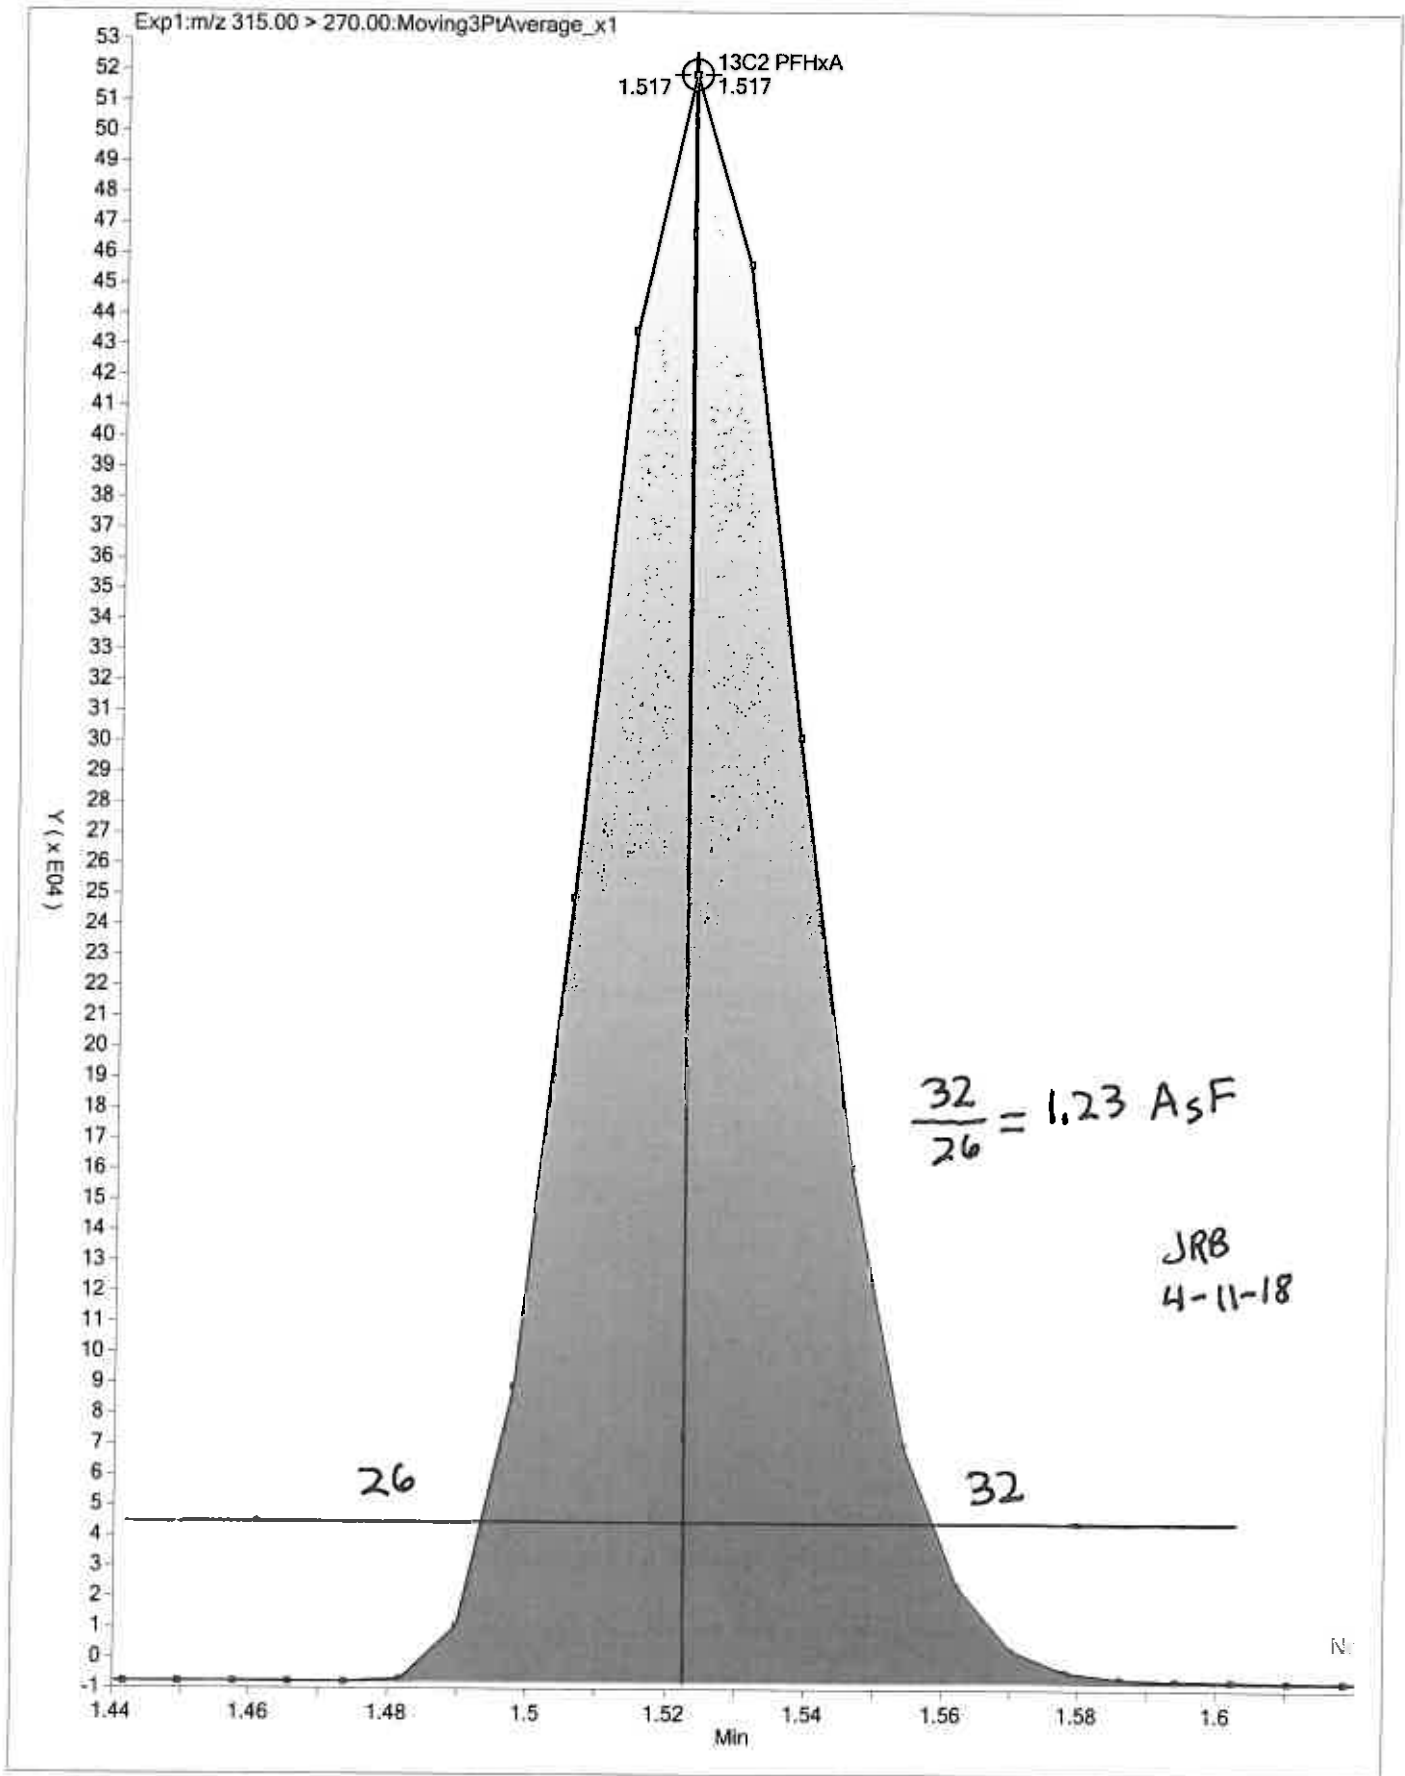

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Lab Sample ID: CCVL 320-217453/10 Calibration Date: 04/11/2018 12:18
 Instrument ID: A8_N Calib Start Date: 04/11/2018 11:45
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 04/11/2018 12:09
 Lab File ID: 2018.04.11_537ICALB_011.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	Ave	1.052	1.078		20.5	20.0	2.5	50.0
Perfluoroheptanoic acid (PFHpA)	Ave	1.074	1.079		2.17	2.16	0.5	50.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.642	1.583		6.48	6.72	-3.6	50.0
Perfluorooctanoic acid (PFOA)	Ave	1.062	1.067		4.42	4.40	0.4	50.0
Perfluorooctanesulfonic acid (PFOS)	Ave	1.066	1.026		8.45	8.79	-3.8	50.0
Perfluorononanoic acid (PFNA)	Ave	0.8424	0.8056		4.21	4.40	-4.4	50.0
13C2 PFHxA	Ave	1.063	1.036		9.74	10.0	-2.6	30.0
13C2 PFDA	Ave	0.8505	0.8798		10.3	10.0	3.4	30.0

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Lab Sample ID: ICV 320-217453/12 Calibration Date: 04/11/2018 12:27
 Instrument ID: A8_N Calib Start Date: 04/11/2018 11:45
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 04/11/2018 12:09
 Lab File ID: 2018.04.11_537ICALB_013.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	Ave	1.052	0.9079		86.4	100	-13.7	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	1.074	0.9453		8.80	10.0	-12.0	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.642	1.546		19.0	20.2	-5.8	30.0
Perfluorooctanoic acid (PFOA)	Ave	1.062	0.8947		17.0	20.2	-15.8	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	1.066	0.9451		17.9	20.2	-11.3	30.0
Perfluorononanoic acid (PFNA)	Ave	0.8424	0.7643		18.3	20.2	-9.3	30.0
13C2 PFHxA	Ave	1.063	0.9887		9.30	10.0	-7.0	30.0
13C2 PFDA	Ave	0.8505	0.7817		9.19	10.0	-8.1	30.0

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Lab Sample ID: CCVL 320-220842/1 Calibration Date: 05/01/2018 11:19
 Instrument ID: A8_N Calib Start Date: 04/11/2018 11:45
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 04/11/2018 12:09
 Lab File ID: 2018.05.01_537AA_003.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	Ave	1.052	1.092		20.8	20.0	3.8	50.0
Perfluoroheptanoic acid (PFHpA)	Ave	1.074	1.039		2.09	2.16	-3.2	50.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.642	1.575		6.45	6.72	-4.1	50.0
Perfluorooctanoic acid (PFOA)	Ave	1.062	1.007		4.17	4.40	-5.2	50.0
Perfluorooctanesulfonic acid (PFOS)	Ave	1.066	1.017		8.38	8.79	-4.6	50.0
Perfluorononanoic acid (PFNA)	Ave	0.8424	0.7780		4.06	4.40	-7.6	50.0
13C2 PFHxA	Ave	1.063	1.073		10.1	10.0	0.9	30.0
13C2 PFDA	Ave	0.8505	0.7541		8.87	10.0	-11.3	30.0

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Lab Sample ID: CCV 320-220845/13 Calibration Date: 05/01/2018 12:15
 Instrument ID: A8_N Calib Start Date: 04/11/2018 11:45
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 04/11/2018 12:09
 Lab File ID: 2018.05.01_537AA_015.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	Ave	1.052	1.055		135	135	0.3	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	1.074	1.021		13.9	14.6	-4.9	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.642	1.688		46.6	45.4	2.8	30.0
Perfluorooctanoic acid (PFOA)	Ave	1.062	1.053		29.4	29.7	-0.9	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	1.066	1.119		62.2	59.3	4.9	30.0
Perfluorononanoic acid (PFNA)	Ave	0.8424	0.7703		27.2	29.7	-8.6	30.0
13C2 PFHxA	Ave	1.063	1.046		9.84	10.0	-1.6	30.0
13C2 PFDA	Ave	0.8505	0.7549		8.88	10.0	-11.2	30.0

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Lab Sample ID: CCV 320-220845/25 Calibration Date: 05/01/2018 13:11
 Instrument ID: A8_N Calib Start Date: 04/11/2018 11:45
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 04/11/2018 12:09
 Lab File ID: 2018.05.01_537AA_027.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	Ave	1.052	1.108		47.4	45.0	5.3	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	1.074	1.096		4.96	4.86	2.1	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.642	1.664		15.3	15.1	1.3	30.0
Perfluorooctanoic acid (PFOA)	Ave	1.062	1.050		9.79	9.90	-1.1	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	1.066	1.050		19.5	19.8	-1.5	30.0
Perfluorononanoic acid (PFNA)	Ave	0.8424	0.8166		9.60	9.90	-3.1	30.0
13C2 PFHxA	Ave	1.063	1.066		10.0	10.0	0.3	30.0
13C2 PFDA	Ave	0.8505	0.7446		8.75	10.0	-12.5	30.0

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Lab Sample ID: CCV 320-220847/25 Calibration Date: 05/01/2018 13:11
 Instrument ID: A8_N Calib Start Date: 04/11/2018 11:45
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 04/11/2018 12:09
 Lab File ID: 2018.05.01_537AA_027.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	Ave	1.052	1.108		47.4	45.0	5.3	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	1.074	1.096		4.96	4.86	2.1	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.642	1.664		15.3	15.1	1.3	30.0
Perfluorooctanoic acid (PFOA)	Ave	1.062	1.050		9.79	9.90	-1.1	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	1.066	1.050		19.5	19.8	-1.5	30.0
Perfluorononanoic acid (PFNA)	Ave	0.8424	0.8166		9.60	9.90	-3.1	30.0
13C2 PFHxA	Ave	1.063	1.066		10.0	10.0	0.3	30.0
13C2 PFDA	Ave	0.8505	0.7446		8.75	10.0	-12.5	30.0

FORM VII
LCMS CONTINUING CALIBRATION DATA

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1
 SDG No.: _____
 Lab Sample ID: CCV 320-220847/29 Calibration Date: 05/01/2018 13:30
 Instrument ID: A8_N Calib Start Date: 04/11/2018 11:45
 GC Column: GeminiC18 3x100 ID: 3.00 (mm) Calib End Date: 04/11/2018 12:09
 Lab File ID: 2018.05.01_537AA_031.d Conc. Units: ng/mL

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Perfluorobutanesulfonic acid (PFBS)	Ave	1.052	1.053		135	135	0.1	30.0
Perfluoroheptanoic acid (PFHpA)	Ave	1.074	1.077		14.6	14.6	0.3	30.0
Perfluorohexanesulfonic acid (PFHxS)	Ave	1.642	1.641		45.3	45.4	-0.0	30.0
Perfluorooctanoic acid (PFOA)	Ave	1.062	1.096		30.6	29.7	3.1	30.0
Perfluorooctanesulfonic acid (PFOS)	Ave	1.066	1.095		60.9	59.3	2.7	30.0
Perfluorononanoic acid (PFNA)	Ave	0.8424	0.8000		28.2	29.7	-5.0	30.0
13C2 PFHxA	Ave	1.063	1.068		10.0	10.0	0.5	30.0
13C2 PFDA	Ave	0.8505	0.7823		9.20	10.0	-8.0	30.0

LCMS ANALYSIS RUN LOG

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1

SDG No.: _____

Instrument ID: A8_N Start Date: 04/11/2018 11:45

Analysis Batch Number: 217453 End Date: 04/11/2018 12:27

LAB SAMPLE ID	CLIENT SAMPLE ID	DATE ANALYZED	DILUTION FACTOR	LAB FILE ID	COLUMN ID
IC 320-217453/3		04/11/2018 11:45	1	2018.04.11_537I CALB 004.d	GeminiC18 3x100 3(mm)
IC 320-217453/4		04/11/2018 11:50	1	2018.04.11_537I CALB 005.d	GeminiC18 3x100 3(mm)
IC 320-217453/5		04/11/2018 11:55	1	2018.04.11_537I CALB 006.d	GeminiC18 3x100 3(mm)
IC 320-217453/6 ICISAV		04/11/2018 11:59	1	2018.04.11_537I CALB 007.d	GeminiC18 3x100 3(mm)
IC 320-217453/7		04/11/2018 12:04	1	2018.04.11_537I CALB 008.d	GeminiC18 3x100 3(mm)
IC 320-217453/8		04/11/2018 12:09	1	2018.04.11_537I CALB 009.d	GeminiC18 3x100 3(mm)
ZZZZZ		04/11/2018 12:13	1		GeminiC18 3x100 3(mm)
CCVL 320-217453/10		04/11/2018 12:18	1	2018.04.11_537I CALB 011.d	GeminiC18 3x100 3(mm)
ICB 320-217453/11		04/11/2018 12:23	1		GeminiC18 3x100 3(mm)
ICV 320-217453/12		04/11/2018 12:27	1	2018.04.11_537I CALB 013.d	GeminiC18 3x100 3(mm)

LCMS ANALYSIS RUN LOG

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1

SDG No.: _____

Instrument ID: A8_N Start Date: 05/01/2018 11:19

Analysis Batch Number: 220842 End Date: 05/01/2018 12:15

LAB SAMPLE ID	CLIENT SAMPLE ID	DATE ANALYZED	DILUTION FACTOR	LAB FILE ID	COLUMN ID
CCVL 320-220842/1		05/01/2018 11:19	1	2018.05.01_537A A 003.d	GeminiC18 3x100 3(mm)
CCV 320-220842/13 CCVIS		05/01/2018 12:15	1		GeminiC18 3x100 3(mm)

LCMS ANALYSIS RUN LOG

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1

SDG No.: _____

Instrument ID: A8_N Start Date: 05/01/2018 12:15

Analysis Batch Number: 220845 End Date: 05/01/2018 13:11

LAB SAMPLE ID	CLIENT SAMPLE ID	DATE ANALYZED	DILUTION FACTOR	LAB FILE ID	COLUMN ID
CCV 320-220845/13 CCVIS		05/01/2018 12:15	1	2018.05.01_537A A 015.d	GeminiC18 3x100 3(mm)
MB 320-219896/1-A		05/01/2018 12:24	1	2018.05.01_537A A 017.d	GeminiC18 3x100 3(mm)
LCS 320-219896/2-A		05/01/2018 12:29	1	2018.05.01_537A A 018.d	GeminiC18 3x100 3(mm)
320-38382-1		05/01/2018 12:34	1	2018.05.01_537A A 019.d	GeminiC18 3x100 3(mm)
320-38382-1 MS		05/01/2018 12:38	1	2018.05.01_537A A 020.d	GeminiC18 3x100 3(mm)
320-38382-1 MSD		05/01/2018 12:43	1	2018.05.01_537A A 021.d	GeminiC18 3x100 3(mm)
320-38382-2		05/01/2018 12:48	1	2018.05.01_537A A 022.d	GeminiC18 3x100 3(mm)
320-38382-3		05/01/2018 12:52	1	2018.05.01_537A A 023.d	GeminiC18 3x100 3(mm)
320-38382-4		05/01/2018 12:57	1	2018.05.01_537A A 024.d	GeminiC18 3x100 3(mm)
320-38382-5		05/01/2018 13:02	1	2018.05.01_537A A 025.d	GeminiC18 3x100 3(mm)
320-38382-6		05/01/2018 13:06	1	2018.05.01_537A A 026.d	GeminiC18 3x100 3(mm)
CCV 320-220845/25 CCVIS		05/01/2018 13:11	1	2018.05.01_537A A 027.d	GeminiC18 3x100 3(mm)

LCMS ANALYSIS RUN LOG

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1

SDG No.: _____

Instrument ID: A8_N Start Date: 05/01/2018 13:11

Analysis Batch Number: 220847 End Date: 05/01/2018 13:30

LAB SAMPLE ID	CLIENT SAMPLE ID	DATE ANALYZED	DILUTION FACTOR	LAB FILE ID	COLUMN ID
CCV 320-220847/25 CCVIS		05/01/2018 13:11	1	2018.05.01_537A A 027.d	GeminiC18 3x100 3(mm)
320-38382-7		05/01/2018 13:20	1	2018.05.01_537A A 029.d	GeminiC18 3x100 3(mm)
320-38382-8		05/01/2018 13:25	1	2018.05.01_537A A 030.d	GeminiC18 3x100 3(mm)
CCV 320-220847/29 CCVIS		05/01/2018 13:30	1	2018.05.01_537A A 031.d	GeminiC18 3x100 3(mm)

LCMS BATCH WORKSHEET

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1

SDG No.: _____

Batch Number: 219896 Batch Start Date: 04/26/18 09:25 Batch Analyst: Long, Tyrel W

Batch Method: 537 Batch End Date: 04/30/18 11:05

Lab Sample ID	Client Sample ID	Method Chain	Basis	GrossWeight	TareWeight	InitialAmount	FinalAmount	ReceivedpH	LC537-HSP 00029
MB 320-219896/1		537, 537				250 mL	1.00 mL	7 SU	
LCS 320-219896/2		537, 537				250 mL	1.00 mL	7 SU	100 uL
320-38382-A-1	NAWC-041918-RW-154	537, 537	T	281.45 g	29.28 g	252.2 mL	1.00 mL	7 SU	
320-38382-A-1	NAWC-041918-RW-154	537, 537	T	281.43 g	28.91 g	252.5 mL	1.00 mL	7 SU	100 uL
320-38382-A-1	NAWC-041918-RW-154	537, 537	T	281.19 g	28.59 g	252.6 mL	1.00 mL	7 SU	100 uL
320-38382-A-2	NAWC-041918-FRB-154	537, 537	T	296.44 g	29.79 g	266.7 mL	1.00 mL	7 SU	
320-38382-A-3	NAWC-041918-RW-146	537, 537	T	233.47 g	28.65 g	204.8 mL	1.00 mL	7 SU	
320-38382-A-4	NAWC-041918-FRB-146	537, 537	T	293.49 g	29.87 g	263.6 mL	1.00 mL	7 SU	
320-38382-A-5	NAWC-041918-RW-258	537, 537	T	290.55 g	29.67 g	260.9 mL	1.00 mL	7 SU	
320-38382-A-6	NAWC-041918-FRB-258	537, 537	T	295.41 g	27.84 g	267.6 mL	1.00 mL	7 SU	
320-38382-A-7	WGNA-041918-RW-3571	537, 537	T	306.16 g	28.97 g	277.2 mL	1.00 mL	7 SU	
320-38382-A-8	WGNA-041918-FRB-3571	537, 537	T	262.80 g	28.26 g	234.5 mL	1.00 mL	7 SU	

Lab Sample ID	Client Sample ID	Method Chain	Basis	LC537-IS 00068	LC537-SU 00066	AnalysisComment			
MB 320-219896/1		537, 537		100 uL	100 uL	Chlorine ND			
LCS 320-219896/2		537, 537		100 uL	100 uL	Chlorine ND			
320-38382-A-1	NAWC-041918-RW-154	537, 537	T	100 uL	100 uL	Chlorine ND			
320-38382-A-1	NAWC-041918-RW-154	537, 537	T	100 uL	100 uL	Chlorine ND			

The pound sign (#) in the amount added field denotes that the reagent was used undiluted. All calculations are performed using the stated concentration for this reagent.

LCMS BATCH WORKSHEET

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1

SDG No.: _____

Batch Number: 219896 Batch Start Date: 04/26/18 09:25 Batch Analyst: Long, Tyrel W

Batch Method: 537 Batch End Date: 04/30/18 11:05

Lab Sample ID	Client Sample ID	Method Chain	Basis	LC537-IS 00068	LC537-SU 00066	AnalysisComment			
320-38382-A-1 MSD	NAWC-041918-RW-1 54	537, 537	T	100 uL	100 uL	Chlorine ND The following sample was observed to have some opaque residue on the bottom of the centrifuge tube after extraction when the sample were brought to final volume.			
320-38382-A-2	NAWC-041918-FRB- 154	537, 537	T	100 uL	100 uL	Chlorine ND			
320-38382-A-3	NAWC-041918-RW-1 46	537, 537	T	100 uL	100 uL	Chlorine ND			
320-38382-A-4	NAWC-041918-FRB- 146	537, 537	T	100 uL	100 uL	Chlorine ND			
320-38382-A-5	NAWC-041918-RW-2 58	537, 537	T	100 uL	100 uL	Chlorine ND			
320-38382-A-6	NAWC-041918-FRB- 258	537, 537	T	100 uL	100 uL	Chlorine ND			
320-38382-A-7	WGNA-041918-RW-3 571	537, 537	T	100 uL	100 uL	Chlorine ND			
320-38382-A-8	WGNA-041918-FRB- 3571	537, 537	T	100 uL	100 uL	Chlorine ND			

The pound sign (#) in the amount added field denotes that the reagent was used undiluted. All calculations are performed using the stated concentration for this reagent.

LCMS BATCH WORKSHEET

Lab Name: TestAmerica Sacramento Job No.: 320-38382-1

SDG No.: _____

Batch Number: 219896 Batch Start Date: 04/26/18 09:25 Batch Analyst: Long, Tyrel W

Batch Method: 537 Batch End Date: 04/30/18 11:05

Batch Notes	
Analyst ID - Aliquot Step	VPM
Analyst ID - Concentration	SKD/VPM
Analyst ID - Final Volume Step	VPM
Internal Standard ID#	1223393
Manifold ID	4
Methanol ID	1217927
pH Indicator ID	3817
Pipette ID	R40536G
Analyst ID - IS Reagent Drop	VPM
Analyst ID - IS Reagent Drop Witness	TWL
Analyst ID - SU Reagent Drop	TWL
Analyst ID - SU Reagent Drop Witness	HJA
Analyst ID - TA Reagent Drop	TWL
Analyst ID - TA Reagent Drop Witness	HJA
SPE Cartridge Lot ID	6369499-12
Trizma ID	SLBR5241V
Reagent Water ID	04/21/18

Basis	Basis Description
T	Total/NA

The pound sign (#) in the amount added field denotes that the reagent was used undiluted. All calculations are performed using the stated concentration for this reagent.

PFAS Calibration Calculations:

Initial Calibration
Instrument A8_N

4/11/2018

PFOA

Analyte Concentration	Analyte Response	Internal Standard Response	Internal Standard Amount	RRF	Reported RRF
1.98	219100	1044020	10	1.05991	1.0599
4.4	417632	921915	10	1.02956	1.0296
9.9	1001316	945031	10	1.07026	1.0703
19.8	2075568	996809	10	1.05162	1.0516
29.7	3119787	929546	10	1.13005	1.13
39.6	4019004	982926	10	1.03253	1.0325
Average				1.06232	1.0623
Standard Deviation				0.0367	
RSD				0.0345	
%RSD				3.45396	3.5

Continuing Calibration

05/01/2018 @ 12:15

PFOA

Analyte Concentration	Analyte Response	Internal Standard Response	Internal Standard Amount	RRF	%D	Reported RRF	Reported %D
29.7	3148324	1006734	10	1.0530	-0.880055	1.053	-0.9

Sample Identification
Compound

NAWC-041918-RW-154
PFOA

Compound Area	594807	Average RRF	1.0623
Internal Standard Amount (ng)	10	Sample Volume(ml)	252.2
Dilution Factor	1	Volume Extract (ml)	1
Internal Standard Area	918602	Injection Volume (µl)	1

Concentration 24.1689 ng/L
Reported Result 24 ng/L

MA/MSD %R

NAWC-041918-RW-154			
PFOA MS %R	Spike amount	MS concentration	Sample Result
91.74	109	124	24
PFOA MSD %R	Spike amount	MSD concentration	Sample Result
60.37	109	89.8	24

MS/MSD RPD
31.99


Surrogate PFHxA

Compound Area	971950		
Internal Standard Amount (ng)	10		
Dilution Factor	1	Volume Extract (ml)	1
Internal Standard Area	918602	Injection Volume (µl)	1
Average RRF	1.0623		
Concentration	9.9602		
Surrogate %R	99.60	Spike amount	10

LCS %R


320-219896/2-A		
PFOA	Spike amount	LCS concentration
100.00	110	110

C:\AI\Projects\112008005\WE04\F.S.DR.03\NAWC_201901.mxd MKB 1/24/2019

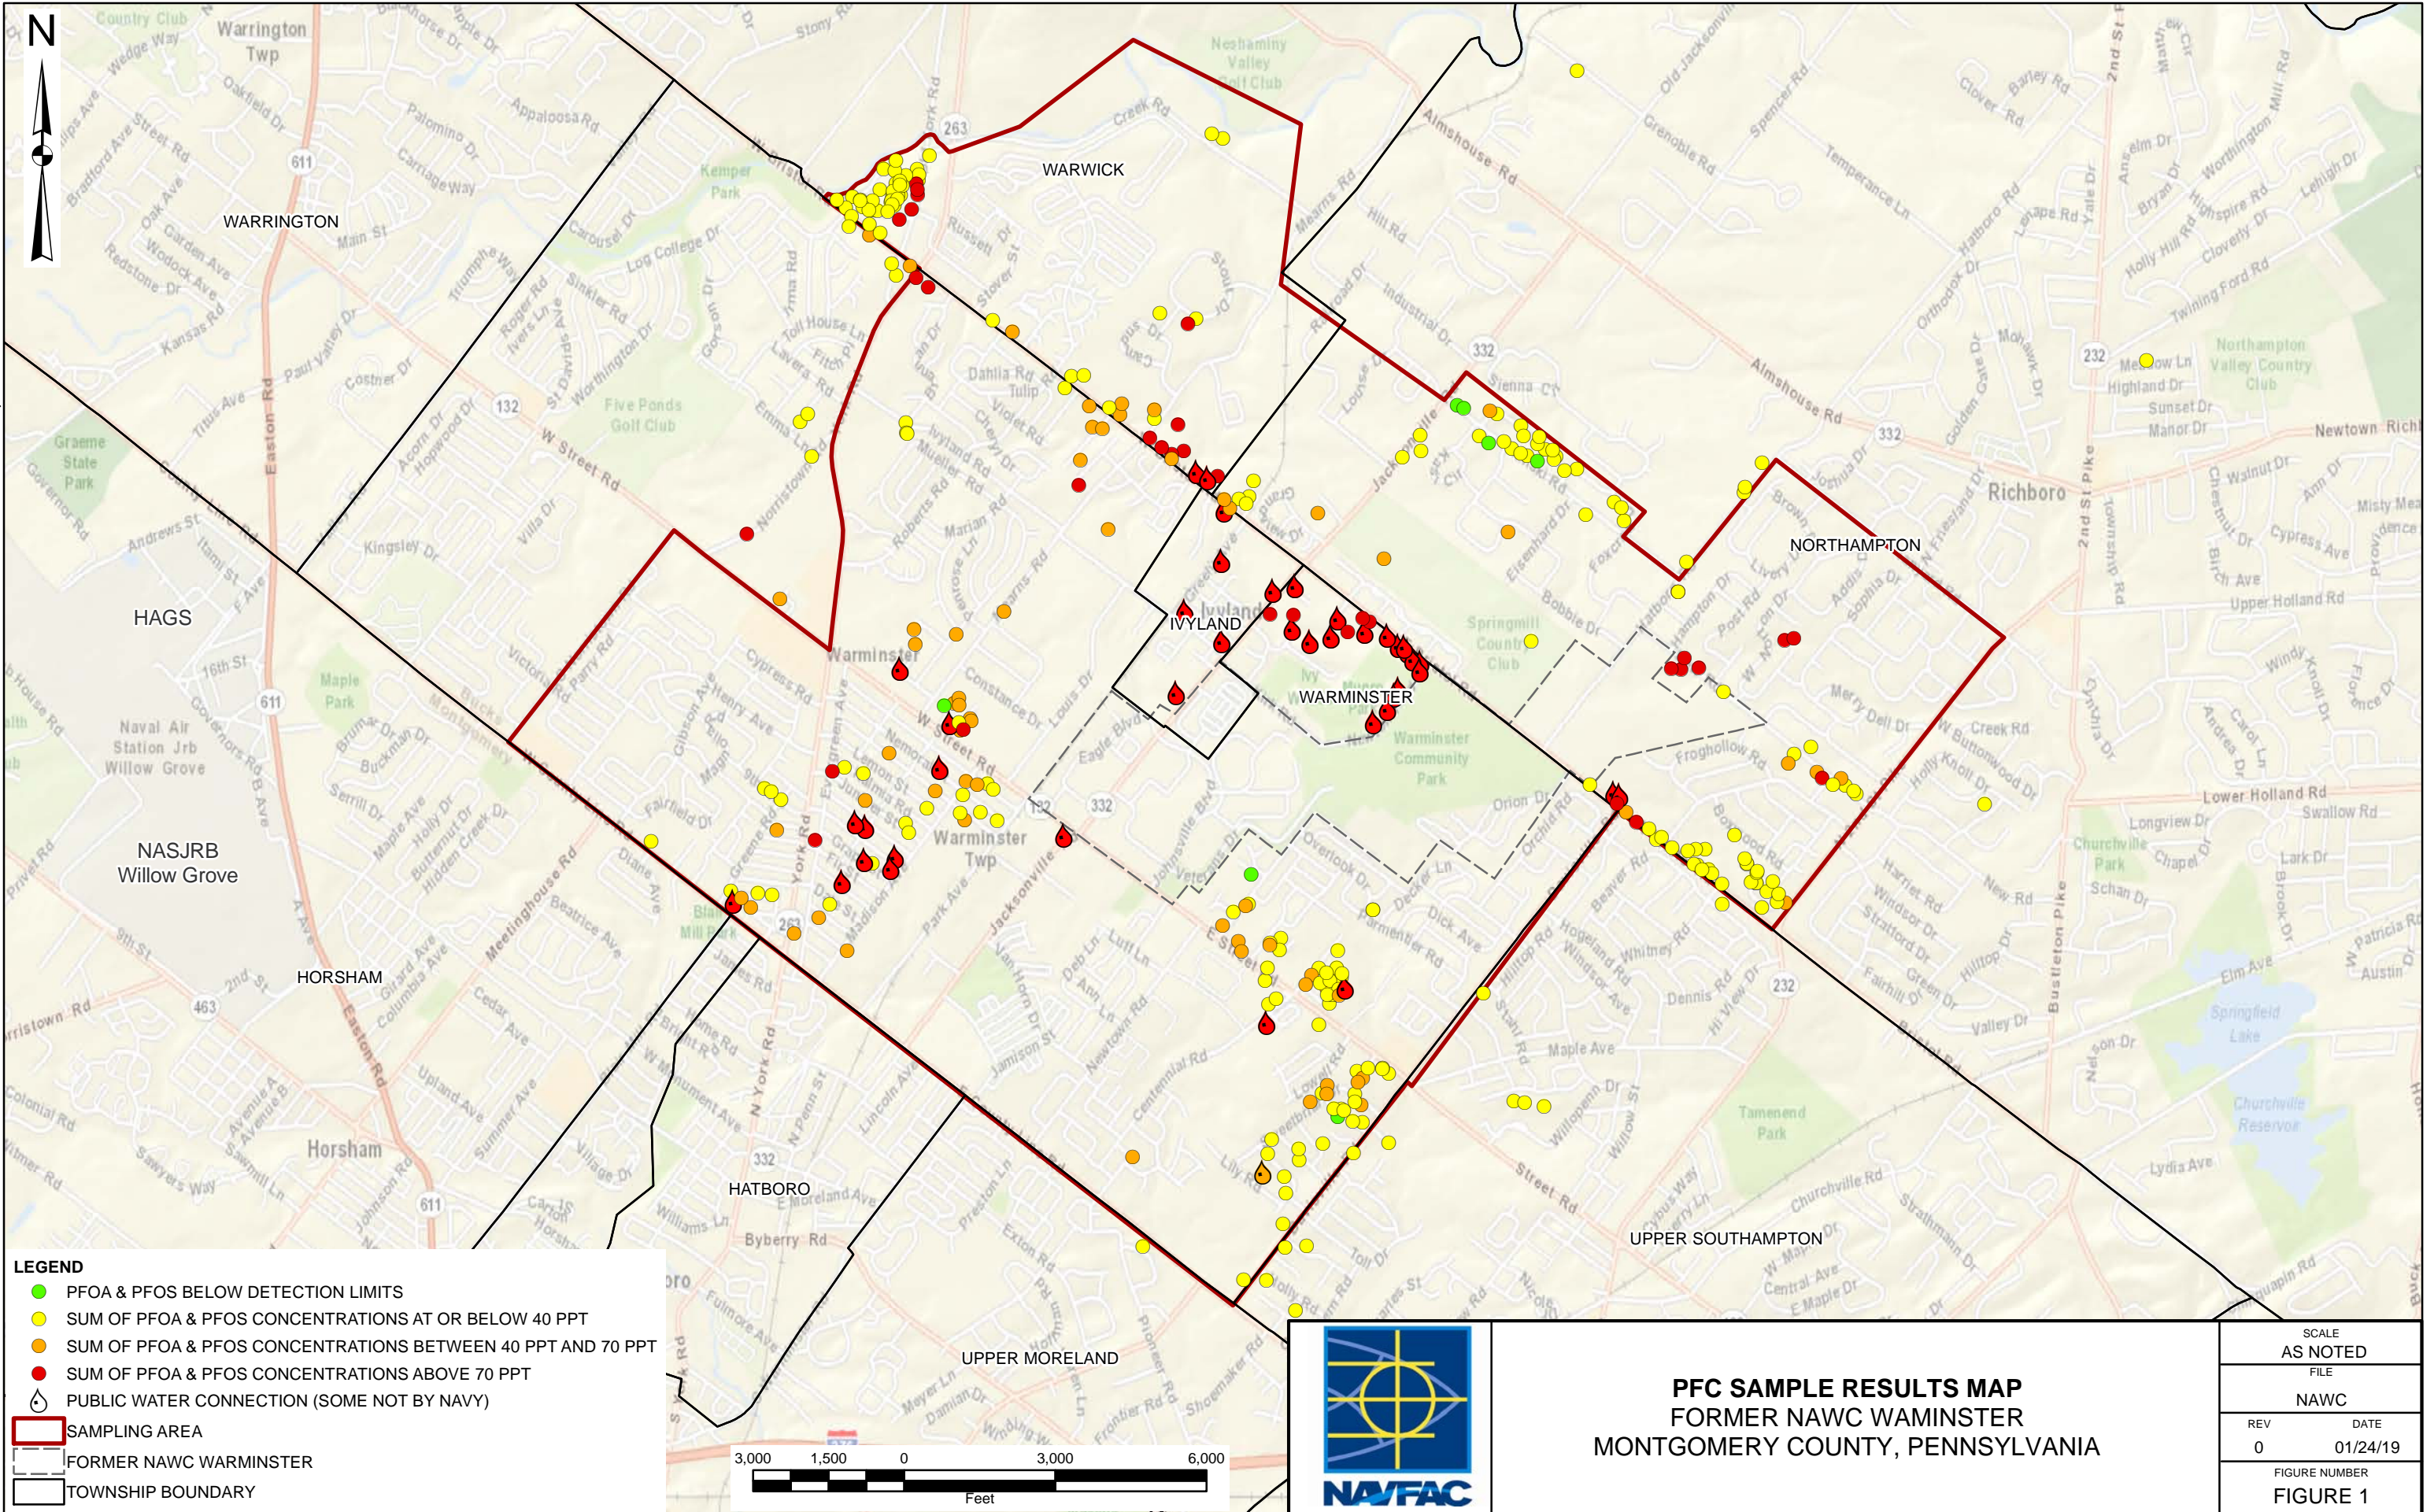

LEGEND

- PFOA & PFOS BELOW DETECTION LIMITS
- SUM OF PFOA & PFOS CONCENTRATIONS AT OR BELOW 40 PPT
- SUM OF PFOA & PFOS CONCENTRATIONS BETWEEN 40 PPT AND 70 PPT
- SUM OF PFOA & PFOS CONCENTRATIONS ABOVE 70 PPT
- 💧 PUBLIC WATER CONNECTION (SOME NOT BY NAVY)
- SAMPLING AREA
- FORMER NAWC WARRINSTER
- TOWNSHIP BOUNDARY



PFC SAMPLE RESULTS MAP
 FORMER NAWC WARRINSTER
 MONTGOMERY COUNTY, PENNSYLVANIA

SCALE AS NOTED	
FILE	
NAWC	
REV 0	DATE 01/24/19
FIGURE NUMBER	
FIGURE 1	